
Peak Find - Teste WL.jws

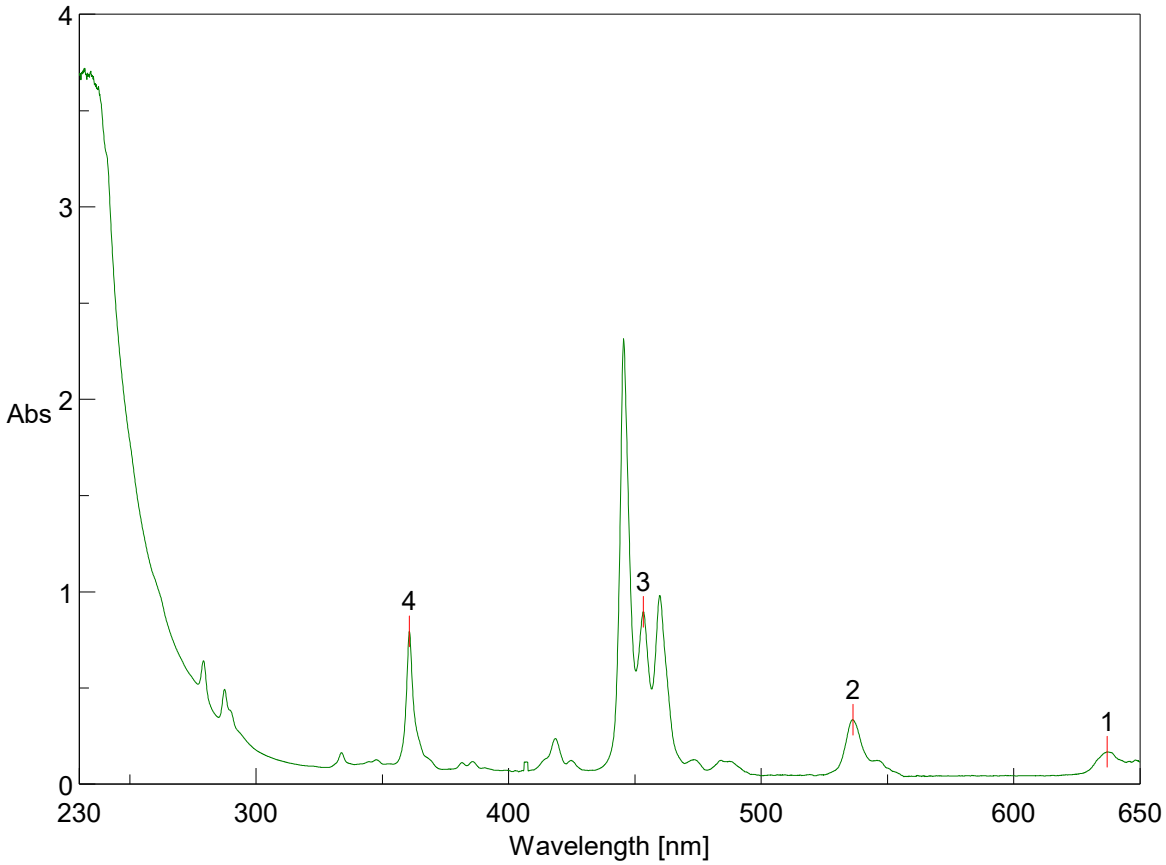

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	QPack
Division	Assistência Técnica
Company	Ortofarma Laboratório de Controle de Qualidade

[Detailed Information]

Creation date	24/07/2025 09:46
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201

[Measurement Information]

Instrument name	UV-07
Model name	V-730
Serial No.	D362561798
Accessory	USE-753
Accessory S/N	D362561798
Cell	
Ref. beam	
Measurement date	24/07/2025 09:41
Parameter file	C:\Workgroups\QPack\Teste WL.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.96 sec
Scan mode	Continuous
Scan speed	100 nm/min
Change source at	340 nm
Light source	D2
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	636.9	0.167495	2	536.3	0.333902
3	453.3	0.895349	4	360.7	0.792525

Creation QPackSA
Review
Approval