
Chromatogram

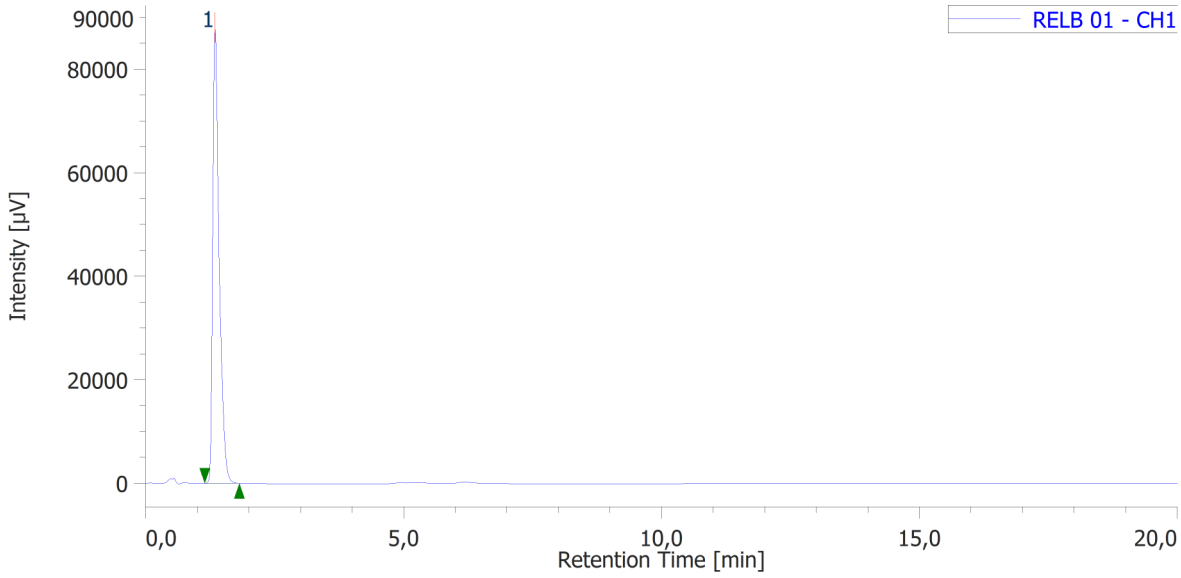


Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 14:50:40
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 14:30:37
Volume	20.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1.342	766351	87964	100.000	100.000	N/A	620	N/A	1.666		9639.2	N/A

Creator QPackSA
Reviewer
Approver

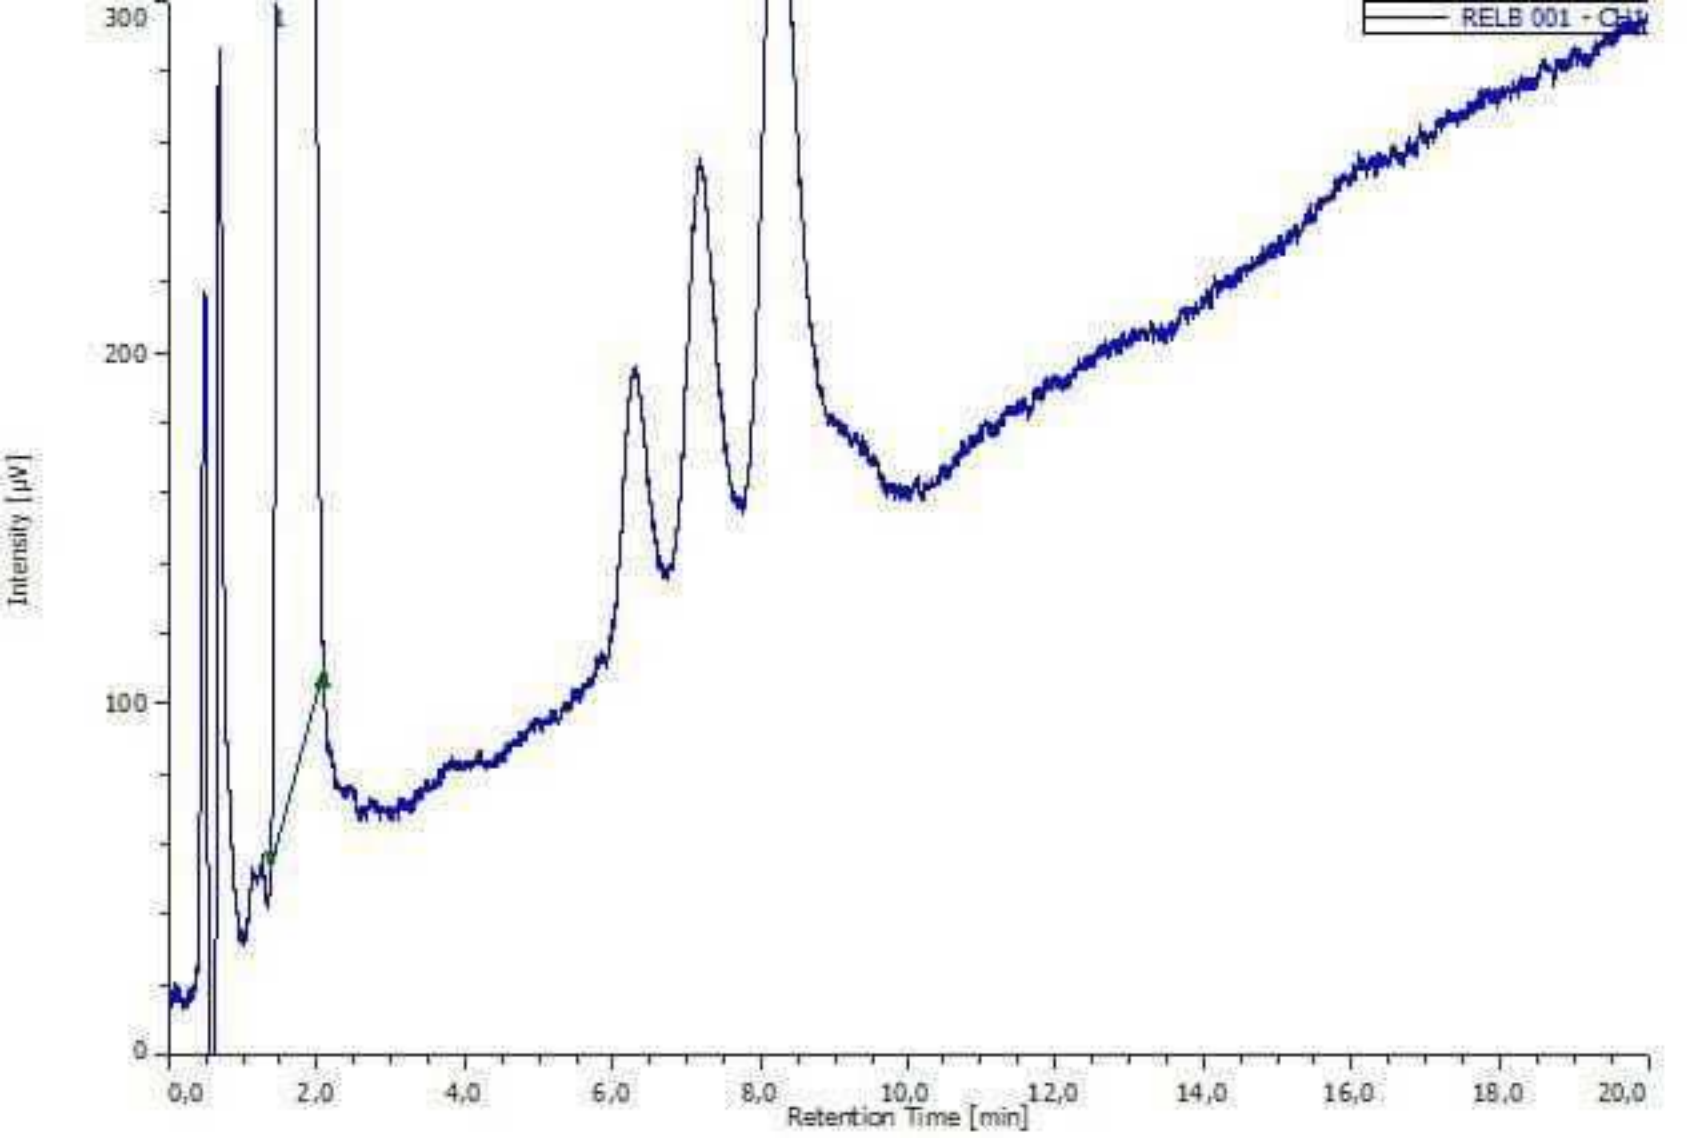
RELB 001 - CH1
300
200
100
0
Intensity [µV]
0,0
2,0
4,0
6,0
8,0
10,0
12,0
14,0
16,0
18,0
20,0
Retention Time [min]

Peak Find - EDUV HPLC-004 2023.jws

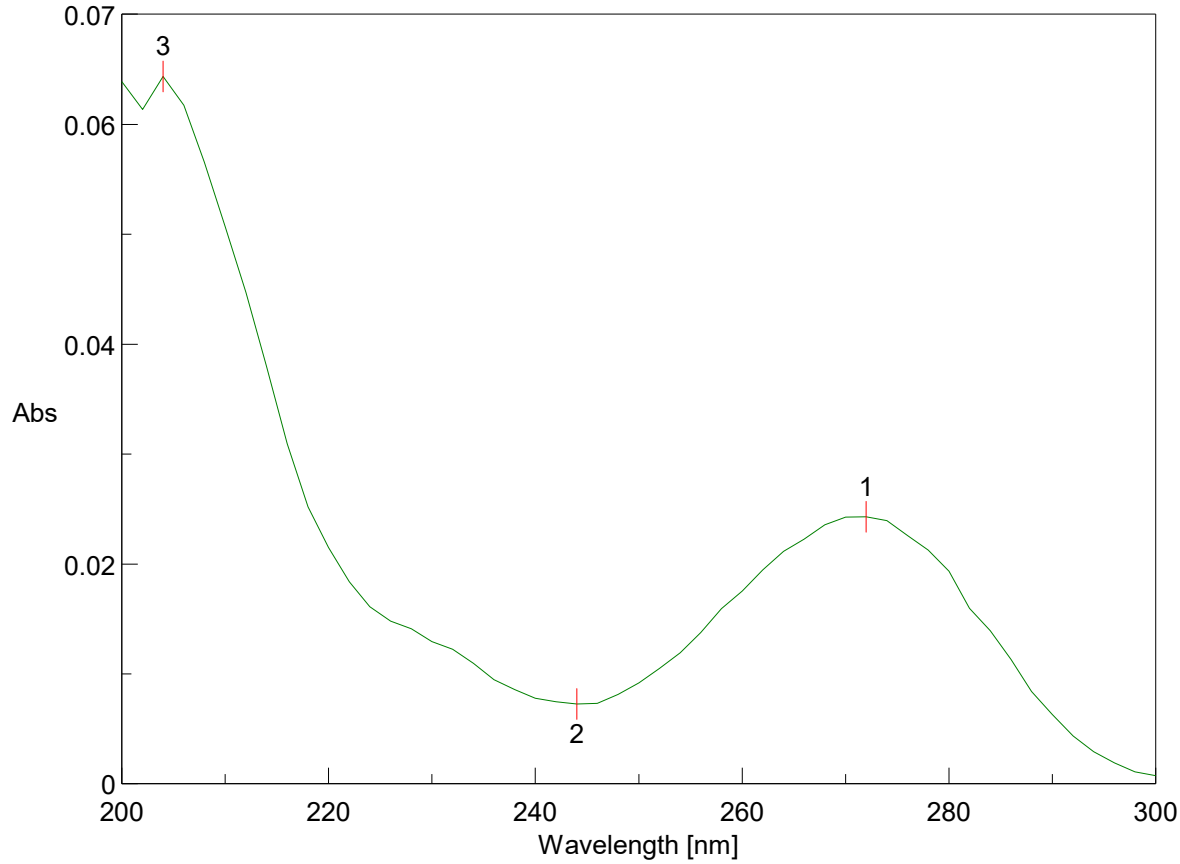

[Comments]

User	QPackSA
Workgroup	QPack
Division	Suporte Técnico
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	08/08/2023 14:26


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	600 nm	
Data interval	2 nm	
Data points	200	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0242864	2	244	0.00723946
3	204	0.0643139			

Creation	QPackSA
Review	
Approval	

Chromatogram

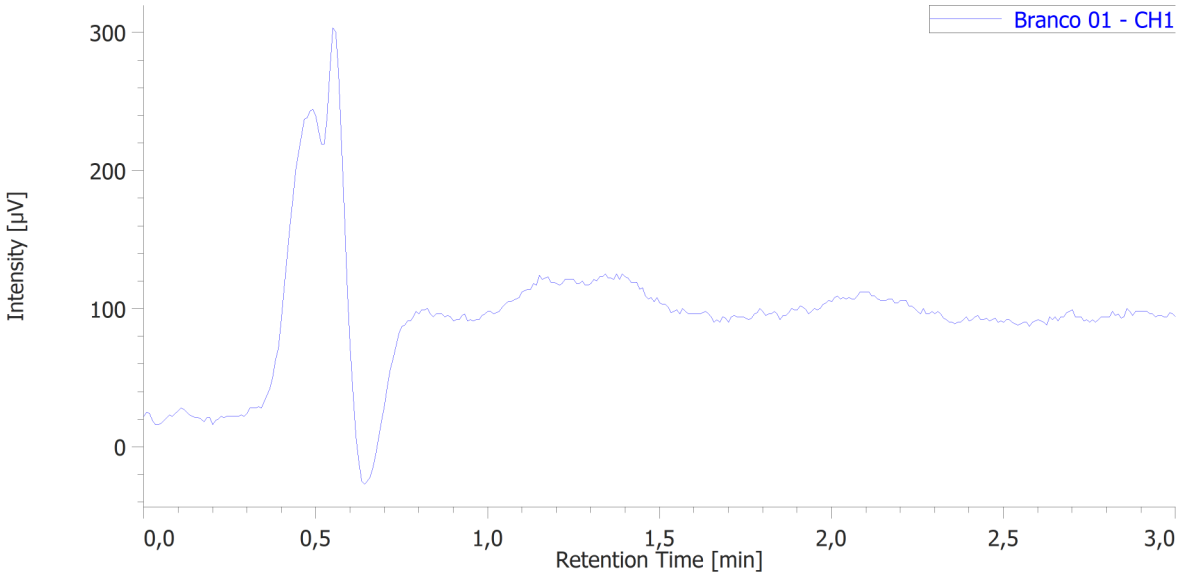


Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:24:28
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:21:25
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

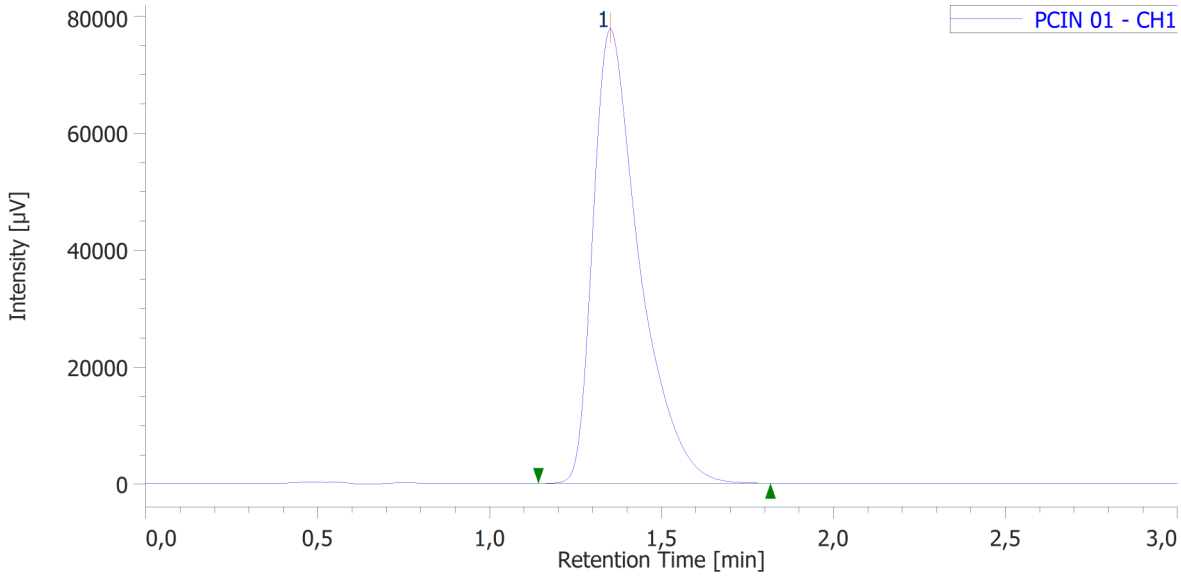

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:27:48
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:24:45
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,350	728124	77792	100,000	100,000	N/A	539	N/A	1,664		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

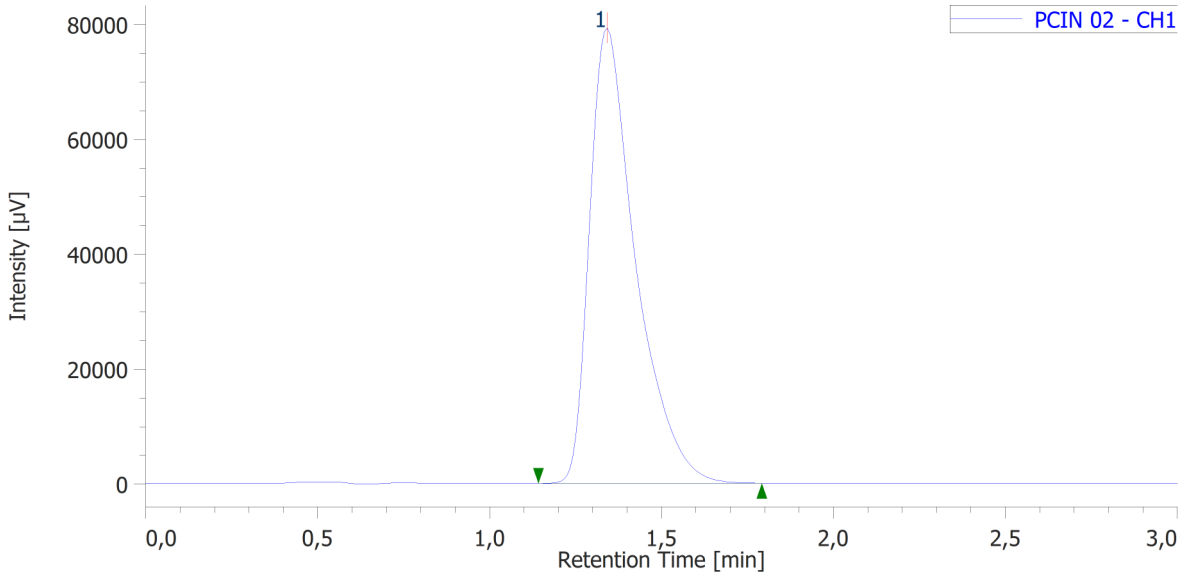

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:31:10
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:28:08
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,342	737954	79217	100,000	100,000	N/A	536	N/A	1,626		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

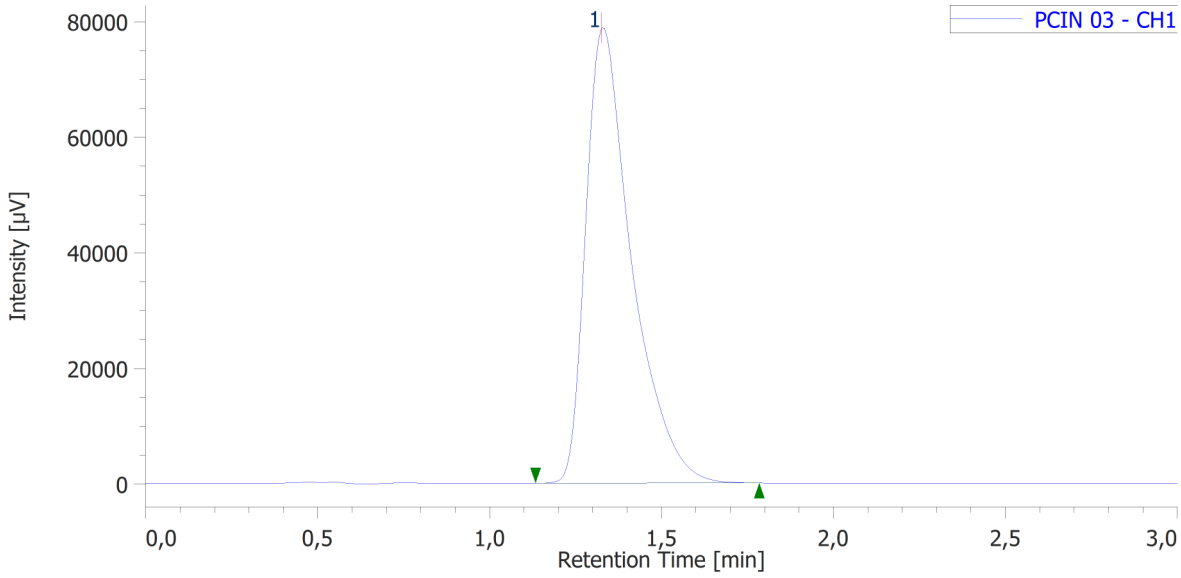

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:34:30
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:31:28
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,325	730693	78723	100,000	100,000	N/A	529	N/A	1,723		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

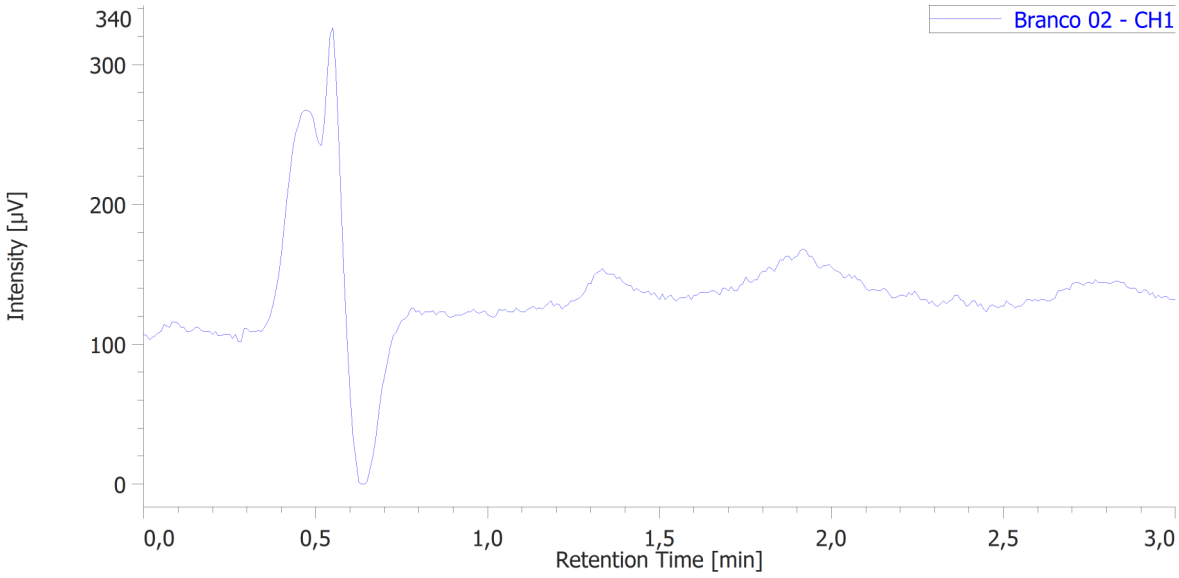


Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:37:50
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:34:48
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

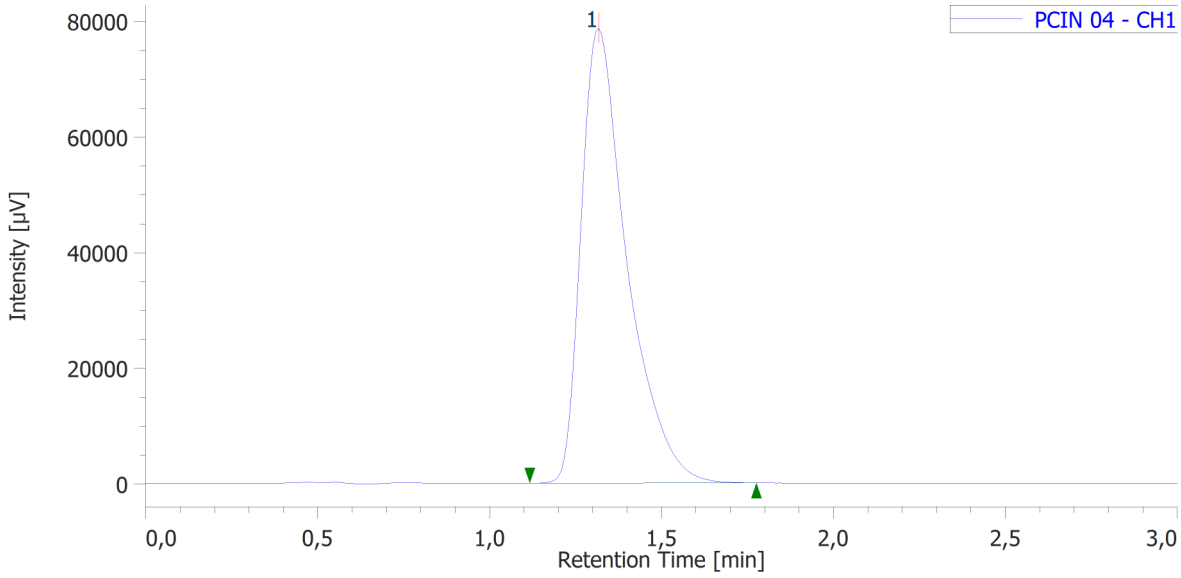

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:41:10
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:38:08
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,317	728704	78673	100,000	100,000	N/A	521	N/A	1,637		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

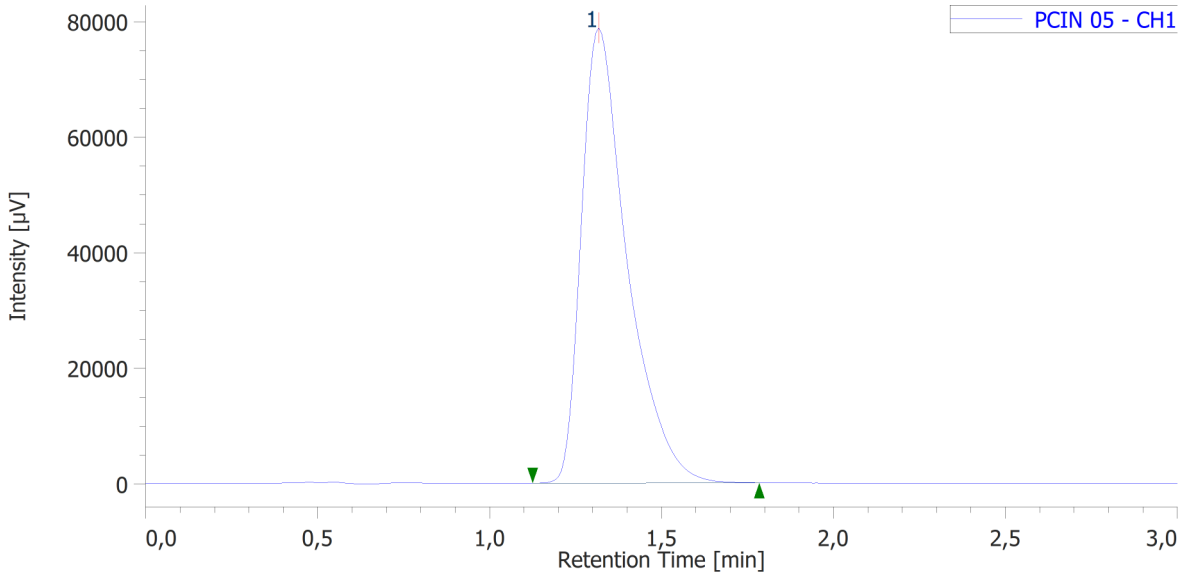

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:44:34
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:41:30
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,317	728461	78688	100,000	100,000	N/A	521	N/A	1,641		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

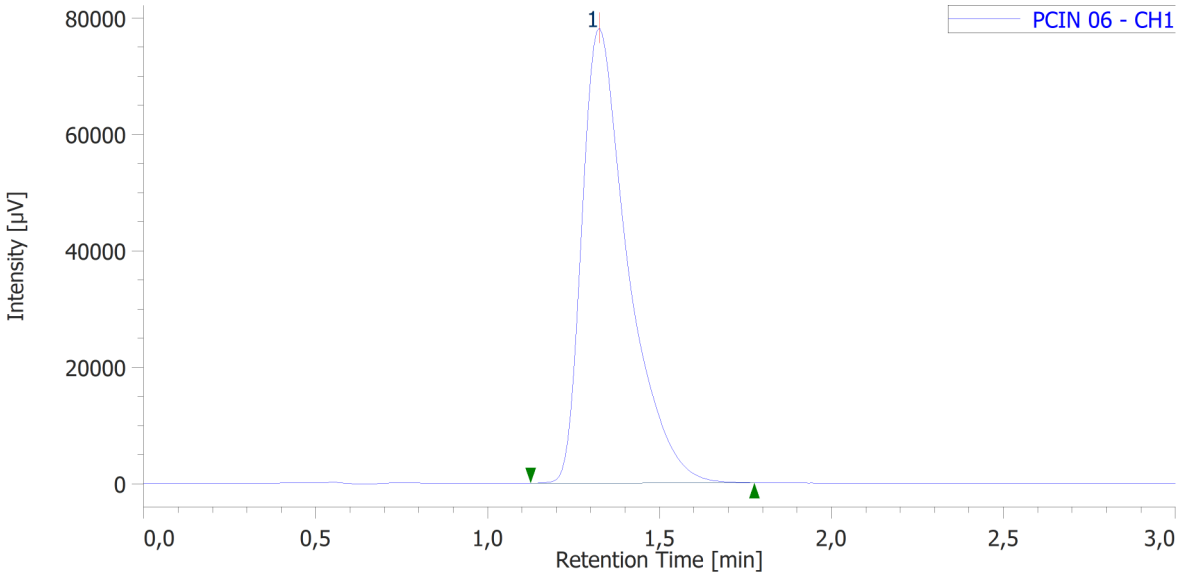

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:47:54
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:44:51
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,325	723066	78079	100,000	100,000	N/A	533	N/A	1,643		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

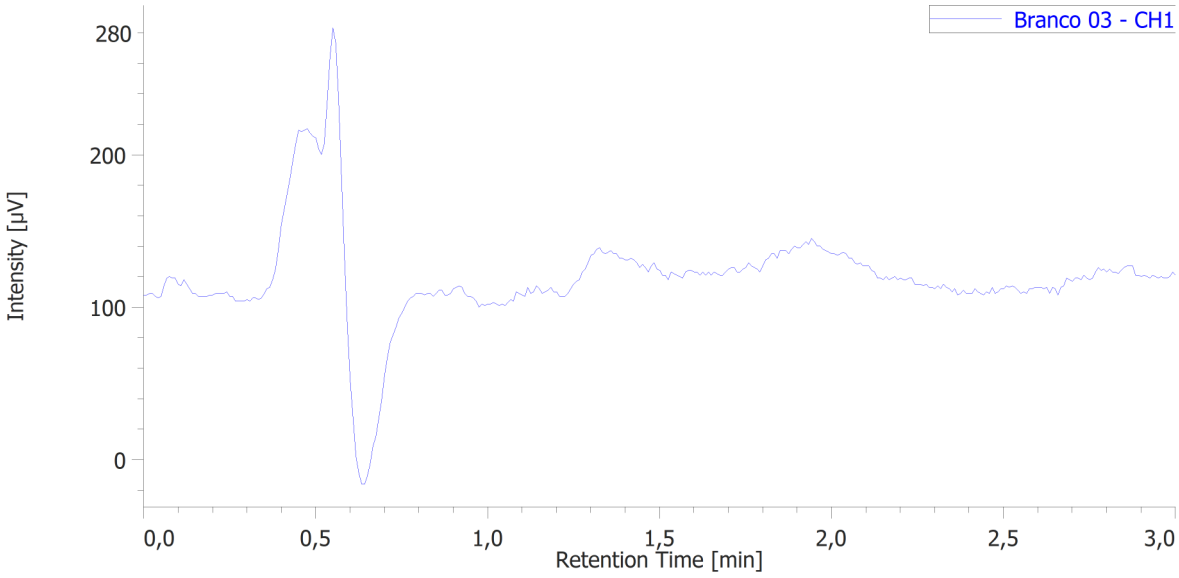


Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:51:14
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:48:11
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

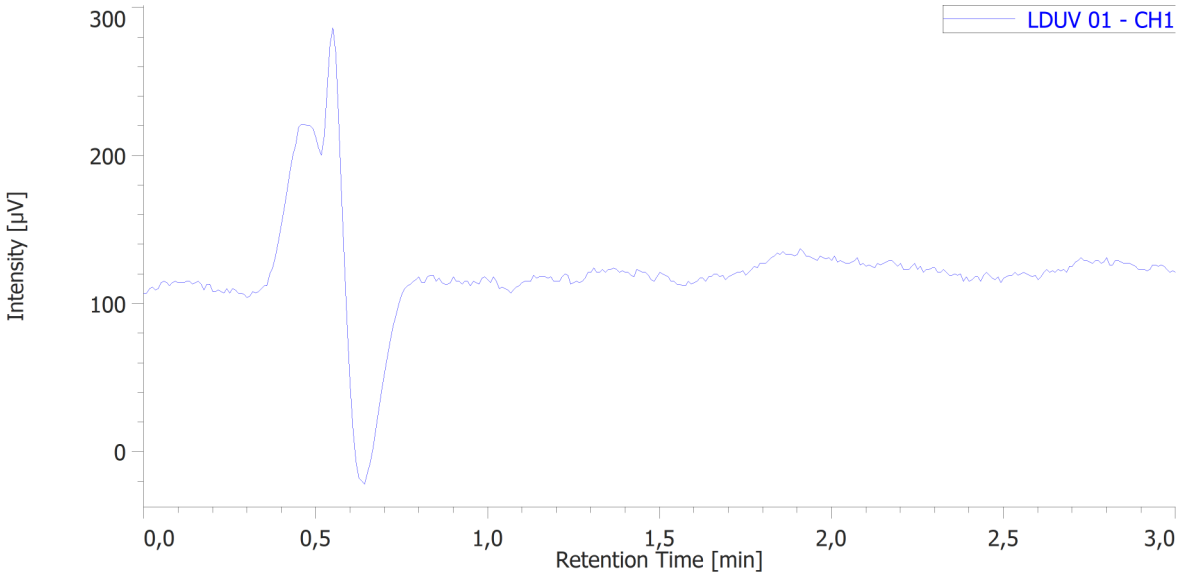


Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:54:36
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:51:33
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

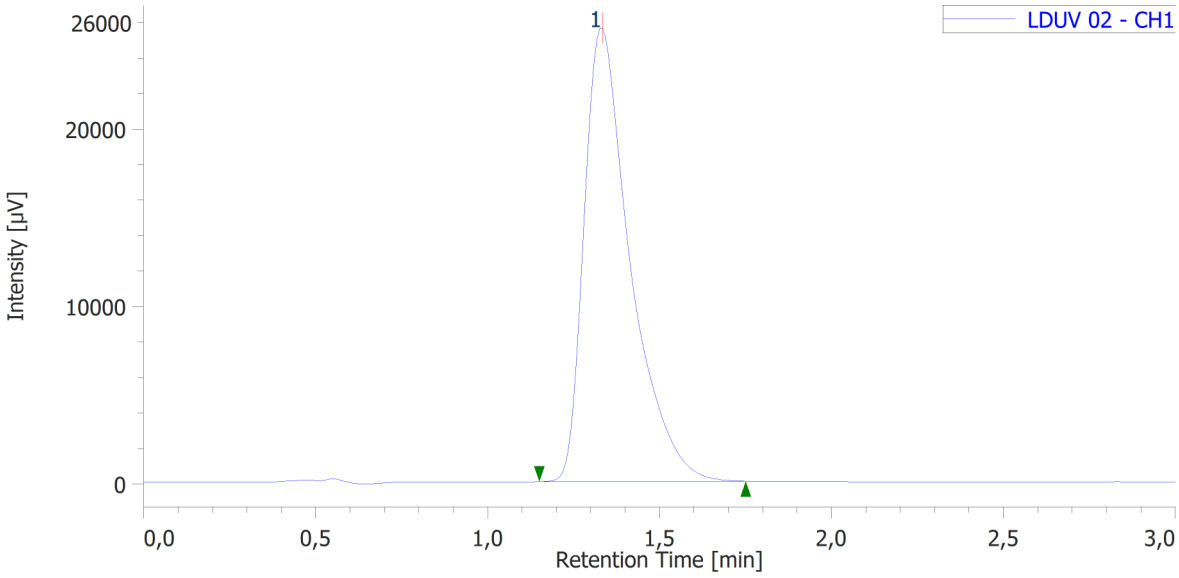

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 15:57:58
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:54:56
Volume	10.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,333	237675	25539	100,000	100,000	N/A	533	N/A	1,609		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

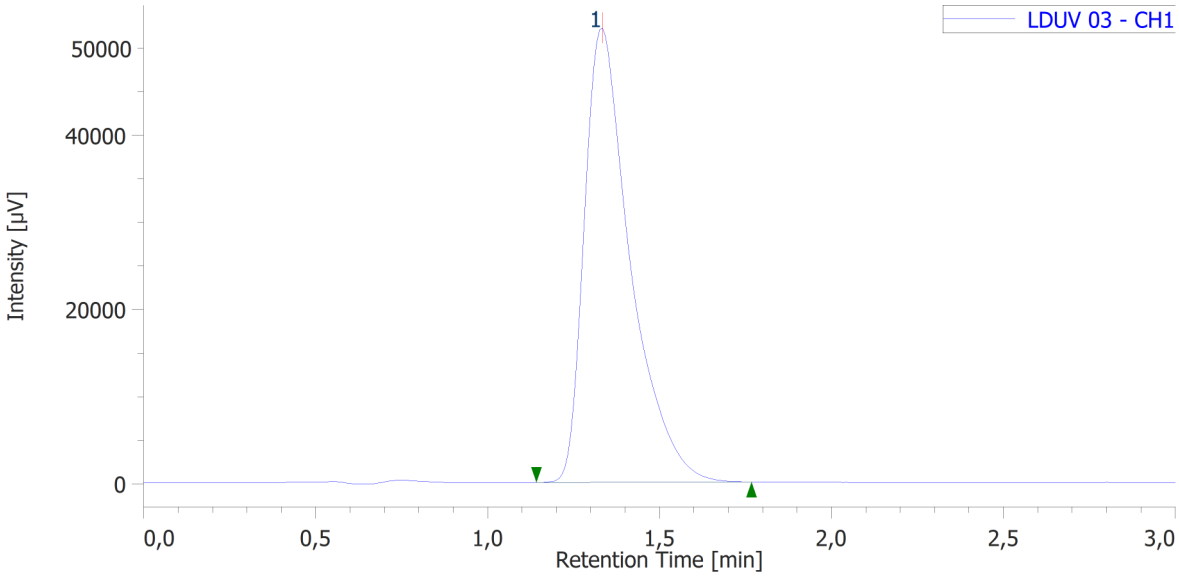

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:01:22
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 15:58:18
Volume	10.0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,333	485472	52148	100,000	100,000	N/A	534	N/A	1,621		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

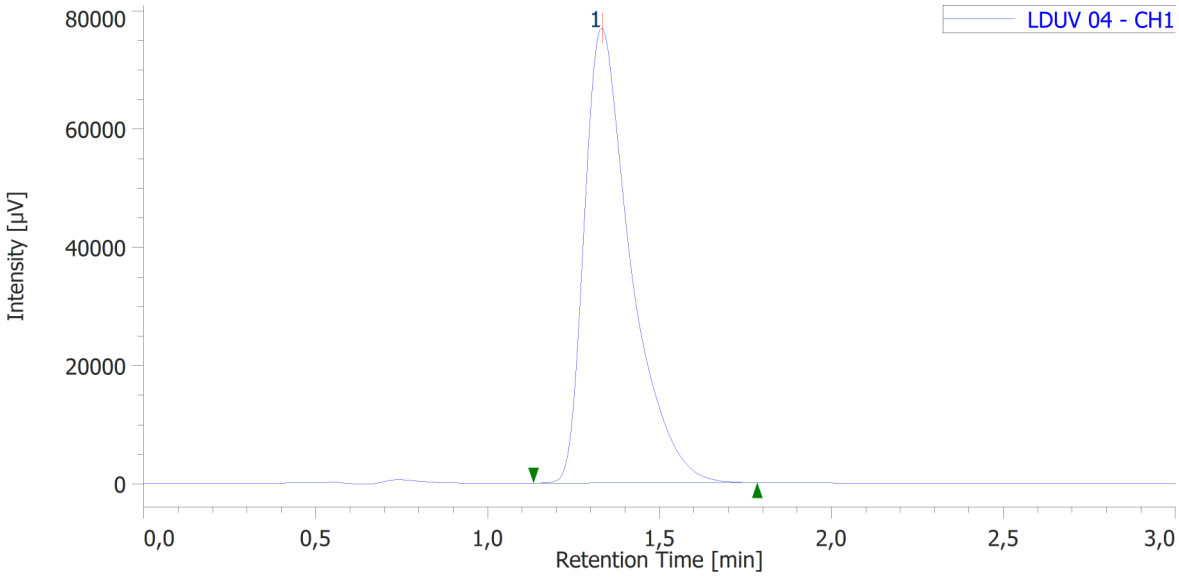

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:04:46
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:01:43
Volume	10.0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,333	720845	76903	100,000	100,000	N/A	527	N/A	1,630		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

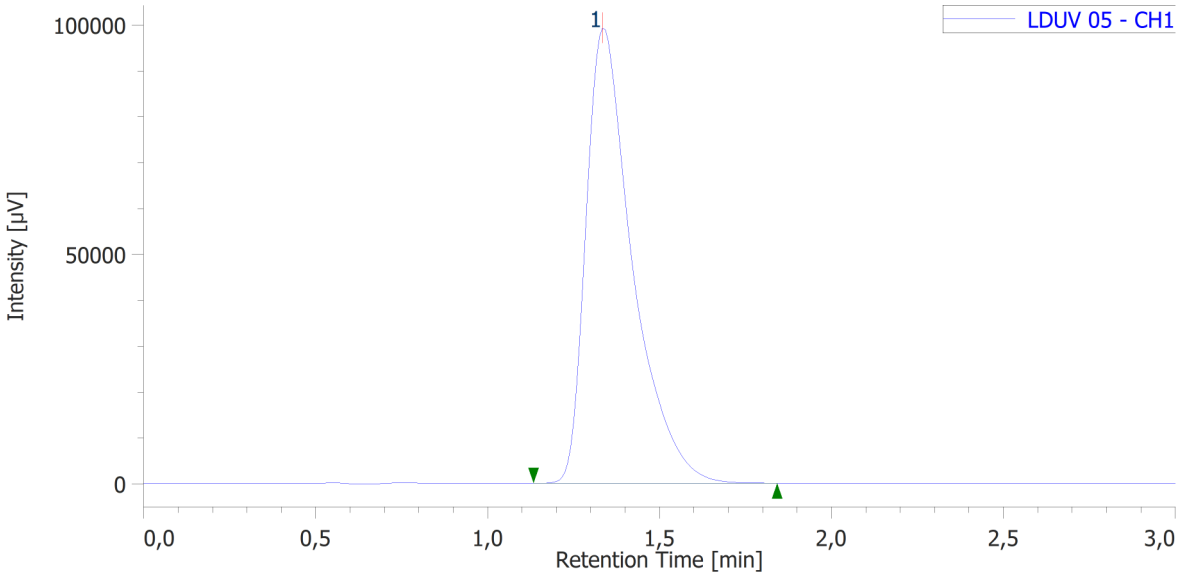

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:08:12
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:05:08
Volume	10.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,333	931178	99144	100,000	100,000	N/A	527	N/A	1,715		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

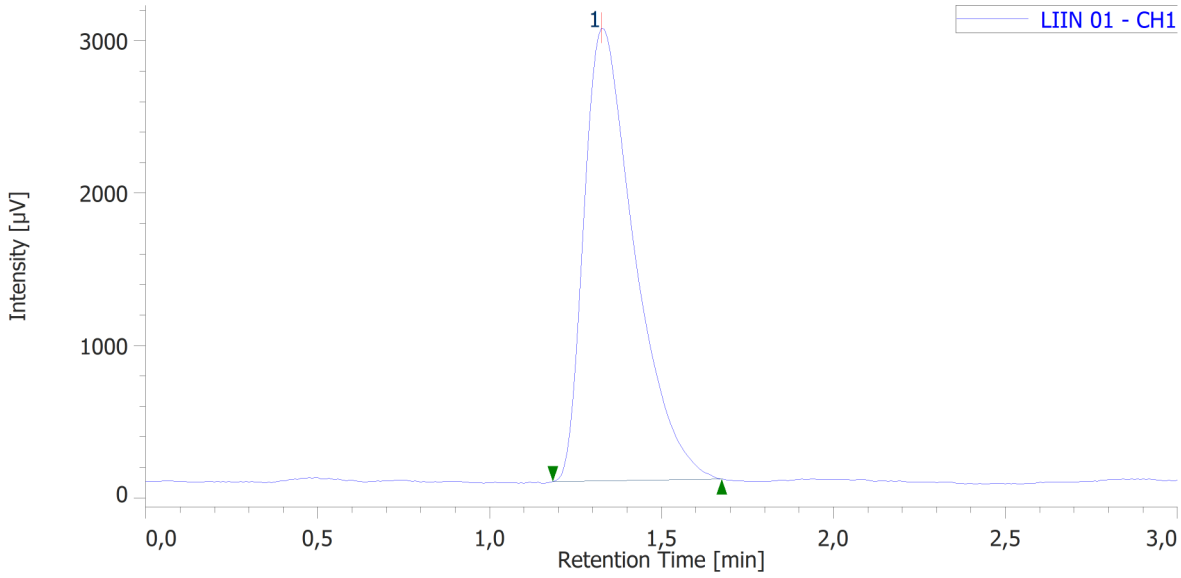

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:11:32
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:08:28
Volume	0.1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,325	30410	2971	100,000	100,000	N/A	408	N/A	1,722		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

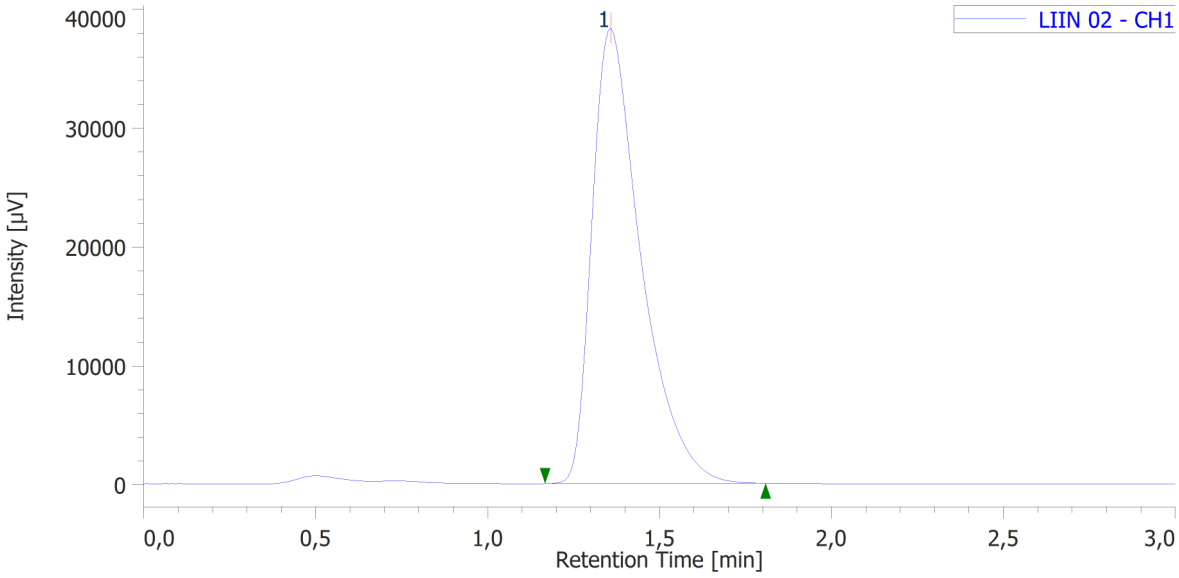

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:14:54
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:11:51
Volume	5.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,358	379245	38300	100,000	100,000	N/A	473	N/A	1,619		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

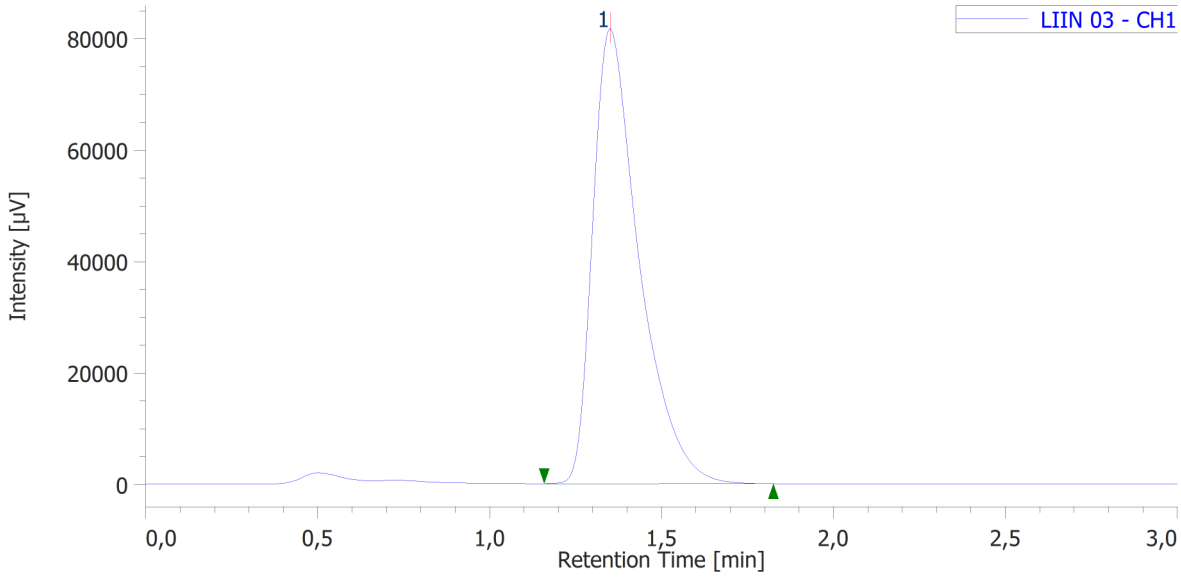

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:18:21
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:15:18
Volume	10.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,350	765395	81728	100,000	100,000	N/A	529	N/A	1,638		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

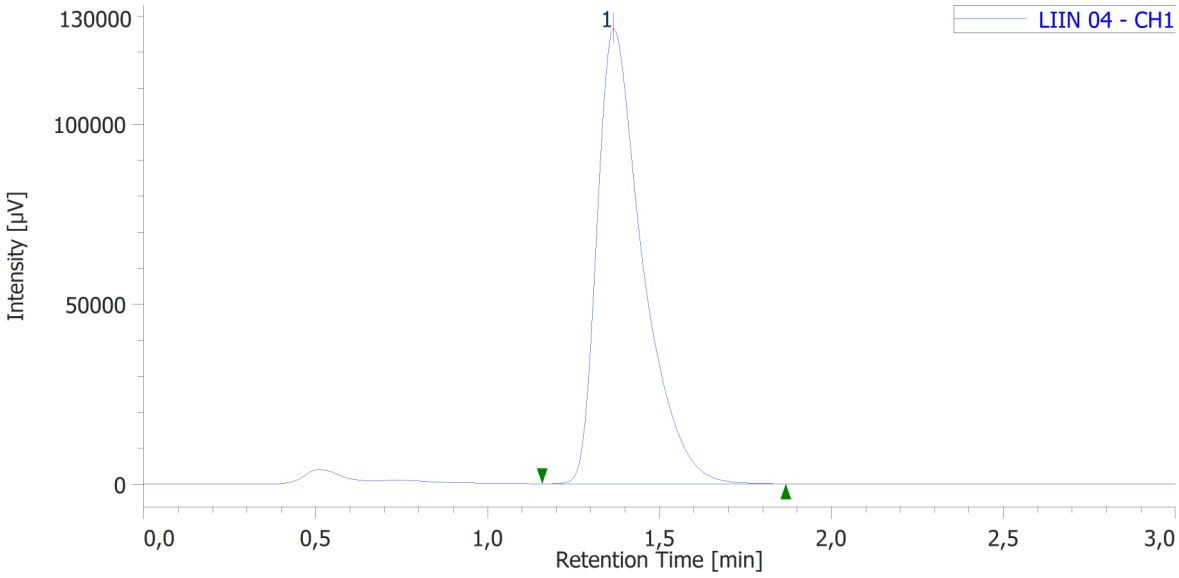

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:21:49
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:18:46
Volume	15.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1.367	1161110	126477	100.000	100.000	N/A	569	N/A	1.649		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

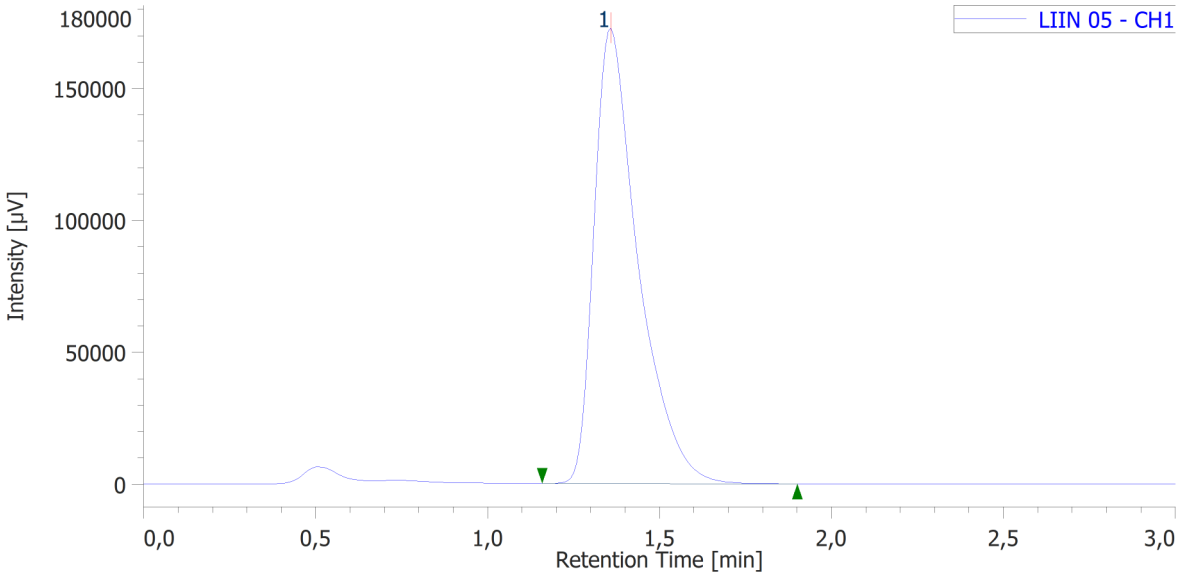

Chromatogram Information	
User Name	QPackSA
Date Modified	08/08/2023 16:25:19
Description	
HPLC System Name	HPLC-0004
Injection Date	08/08/2023 16:22:16
Volume	20.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeina	1	1,358	1539011	172548	100,000	100,000	N/A	604	N/A	1,625		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

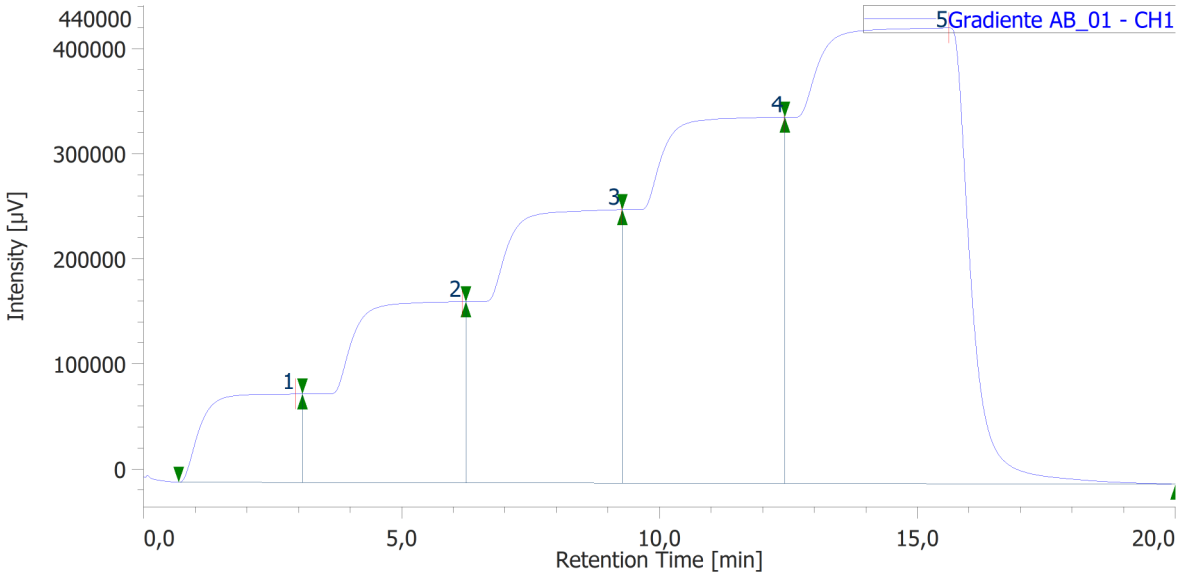

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 13:16:09
Description	
HPLC System Name	HPLC-0004
Injection Date	10/08/2023 11:58:43
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	GRAD
Control Method	Grad AB
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_01-CH1
Sample Name	Gradiente AB
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Unknown	1	2,942	10100910	84104	4,316	6,481	N/A	N/A	N/A	N/A		N/A	N/A
2	Unknown	1	6,167	27506748	172059	11,753	13,258	N/A	N/A	N/A	N/A		N/A	N/A
3	Unknown	1	9,250	42923297	260002	18,340	20,035	N/A	N/A	N/A	N/A		N/A	N/A
4	Unknown	1	12,417	61565900	348245	26,305	26,834	N/A	N/A	N/A	N/A		N/A	N/A
5	Unknown	1	15,600	91949853	433343	39,287	33,392	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

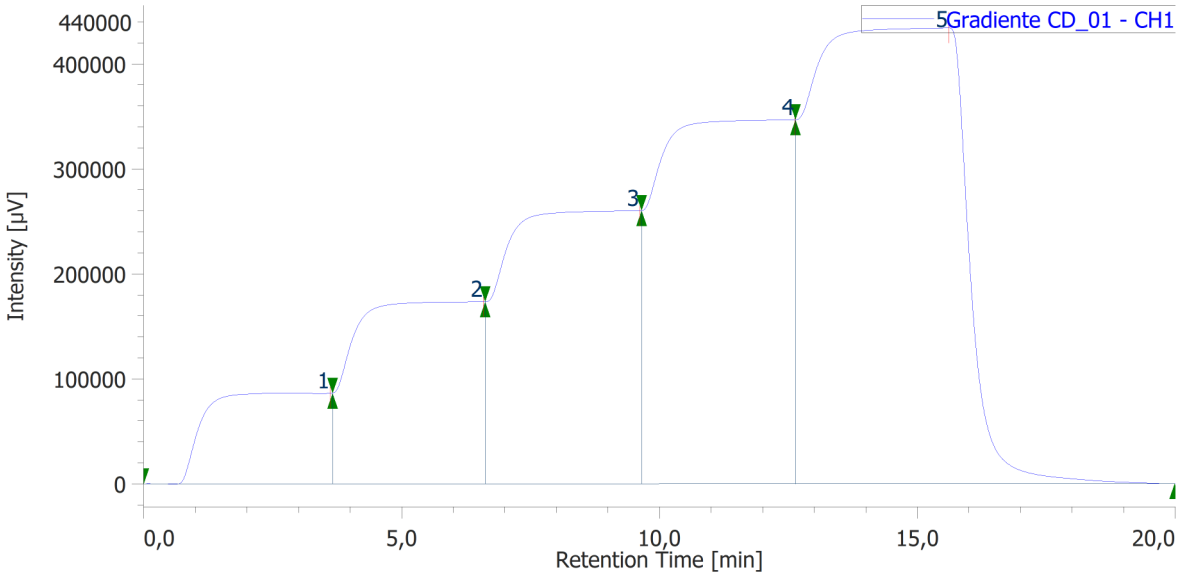

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 13:21:24
Description	
HPLC System Name	HPLC-0004
Injection Date	10/08/2023 12:18:59
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	GRAD
Control Method	Grad CD1
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_01-CH1
Sample Name	Gradiente CD
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Unknown	1	3,617	13471309	86039	5,742	6,621	N/A	N/A	N/A	N/A		N/A	N/A
2	Unknown	1	6,583	28634538	173258	12,206	13,334	N/A	N/A	N/A	N/A		N/A	N/A
3	Unknown	1	9,617	44977632	259776	19,172	19,992	N/A	N/A	N/A	N/A		N/A	N/A
4	Unknown	1	12,617	59855985	346408	25,514	26,659	N/A	N/A	N/A	N/A		N/A	N/A
5	Unknown	1	15,600	87657446	433906	37,365	33,393	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver