
Chromatogram

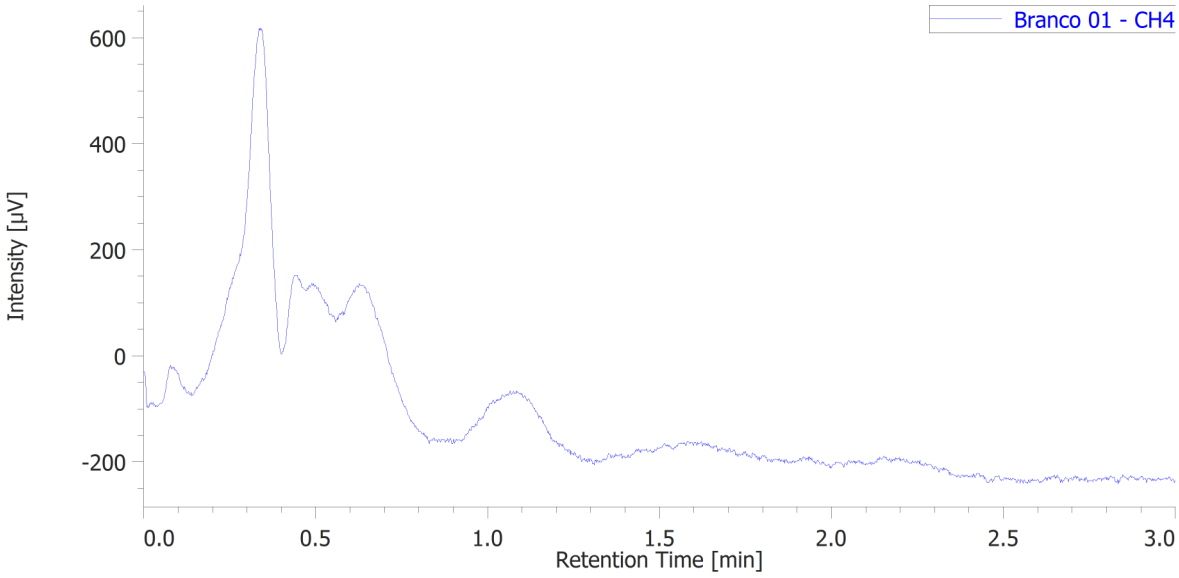


Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 12:47:25
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 12:44:21
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

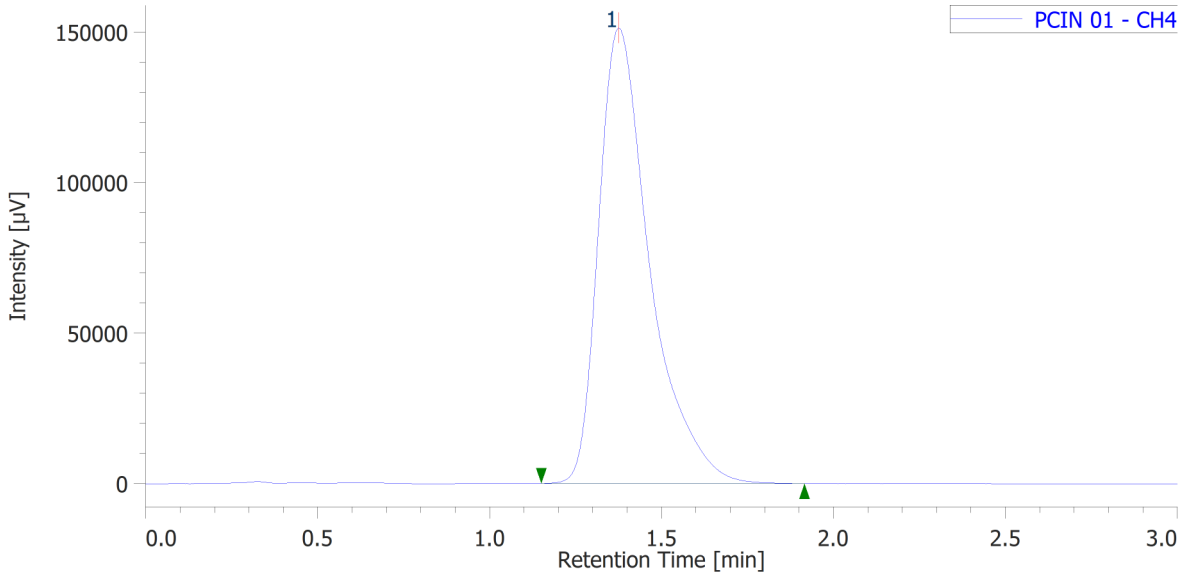

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:30:50
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 12:48:16
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.375	1566337	151263	100.000	100.000	N/A	465	N/A	1.583	

Creator QPackSA
Reviewer
Approver

Chromatogram

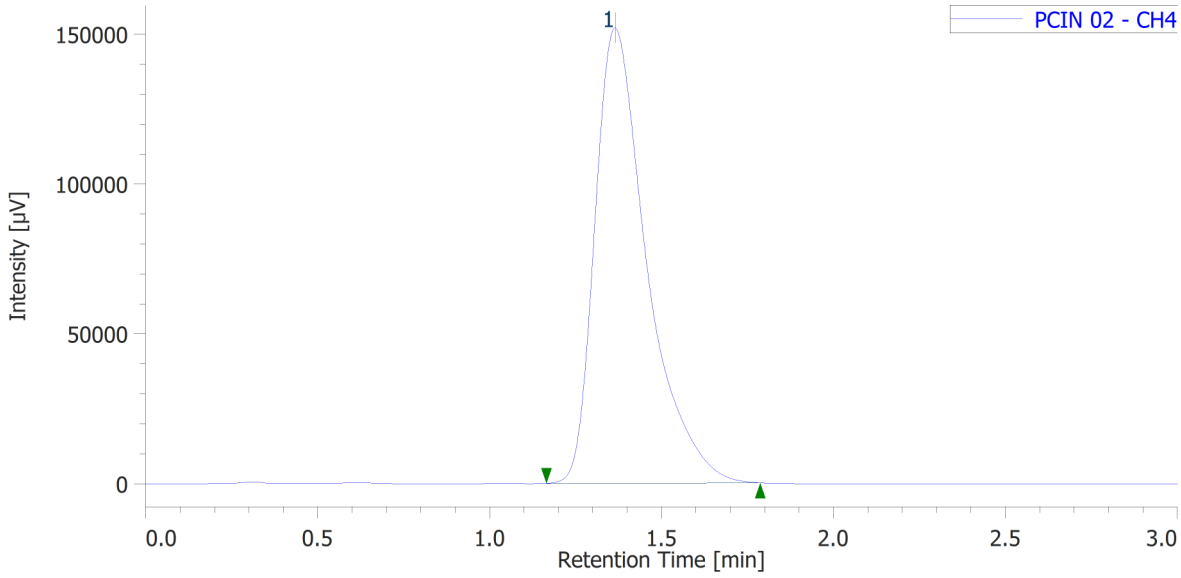

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 12:55:15
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 12:52:12
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.365	1594035	151827	100.000	100.000	N/A	438	N/A	1.574	

Creator QPackSA
Reviewer
Approver

Chromatogram

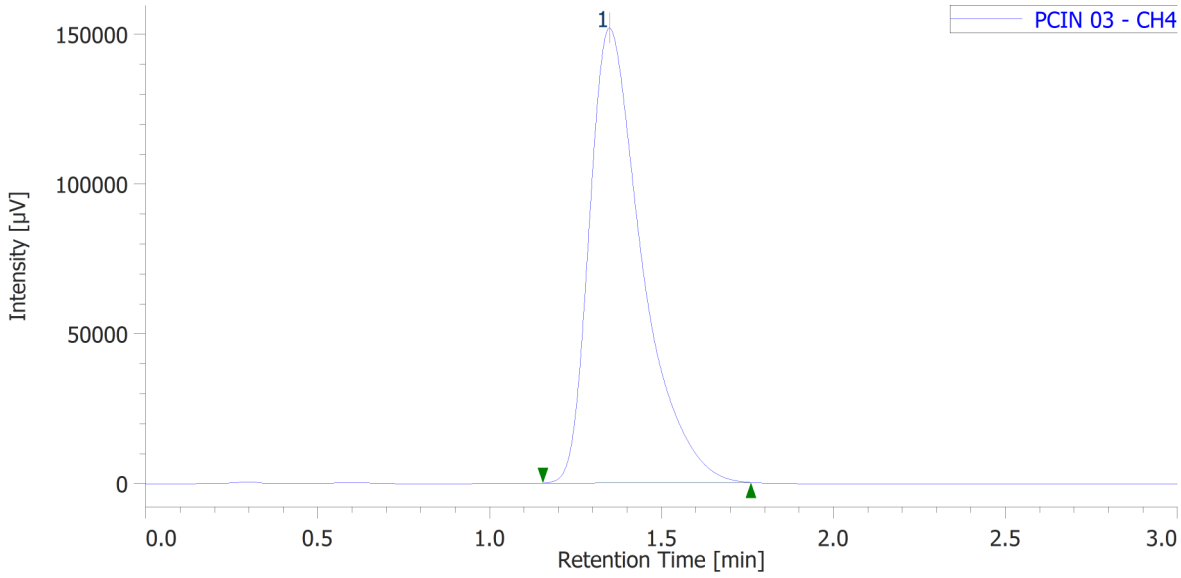

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:30:51
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 12:56:08
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.348	1614985	151835	100.000	100.000	N/A	412	N/A	1.594	

Creator QPackSA
Reviewer
Approver

Chromatogram

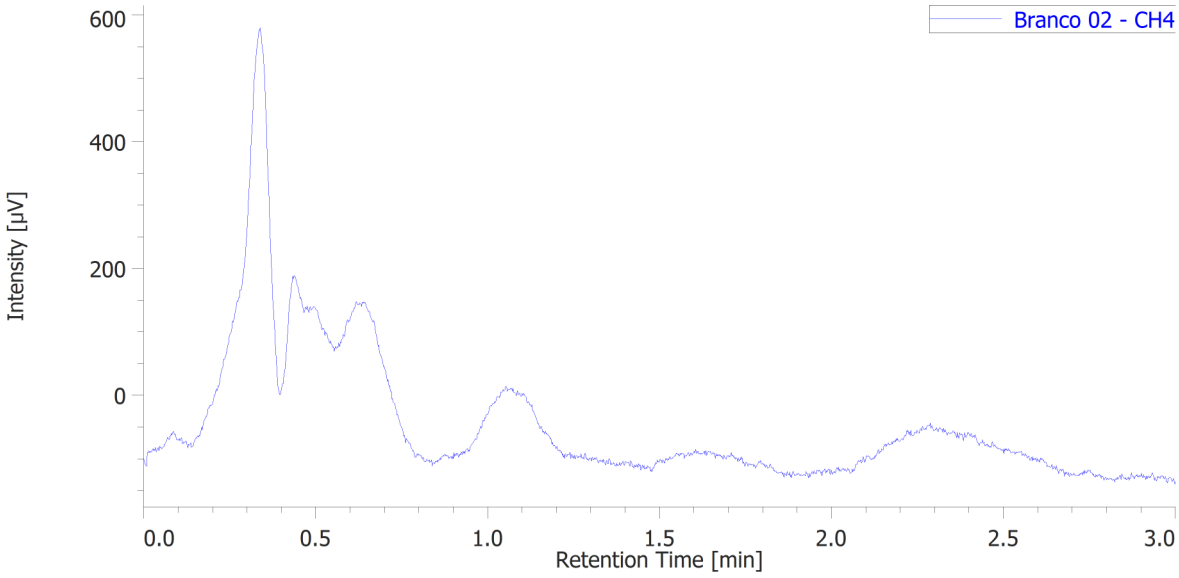


Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 13:03:05
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 13:00:01
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

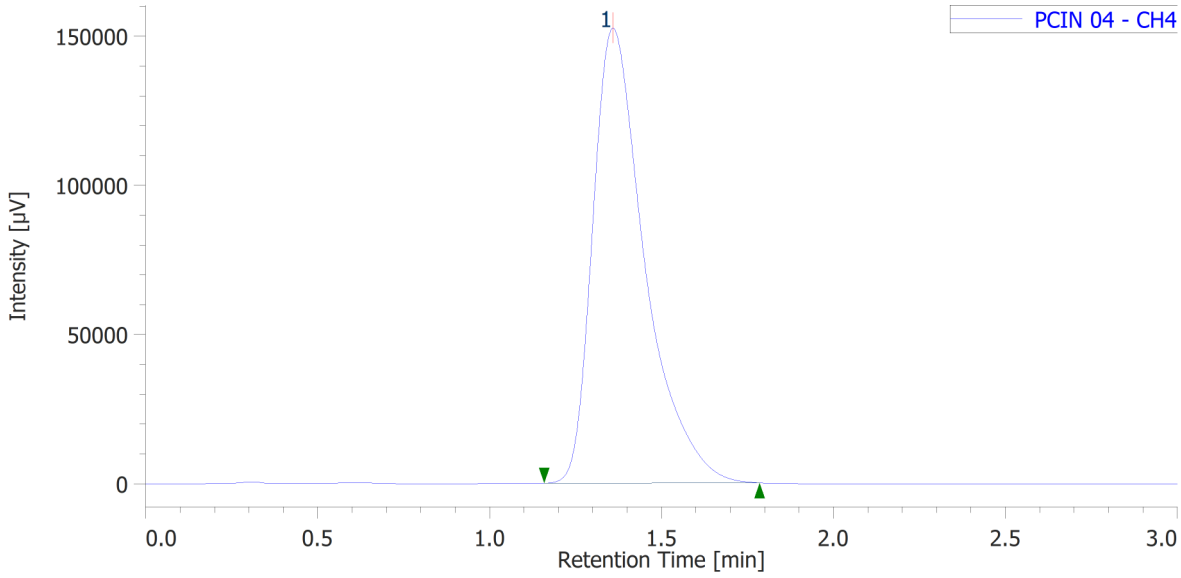

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 13:06:59
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 13:03:56
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.358	1604070	152532	100.000	100.000	N/A	431	N/A	1.584	

Creator QPackSA
Reviewer
Approver

Chromatogram

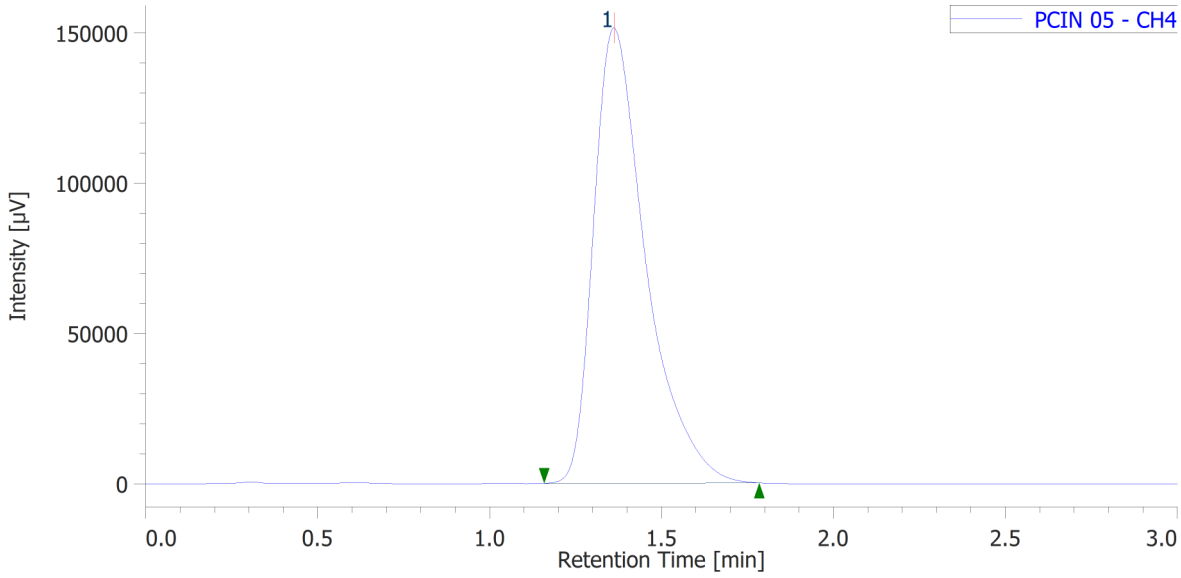

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 13:10:55
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 13:07:51
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.362	1600570	151381	100.000	100.000	N/A	427	N/A	1.577	

Creator QPackSA
Reviewer
Approver

Chromatogram

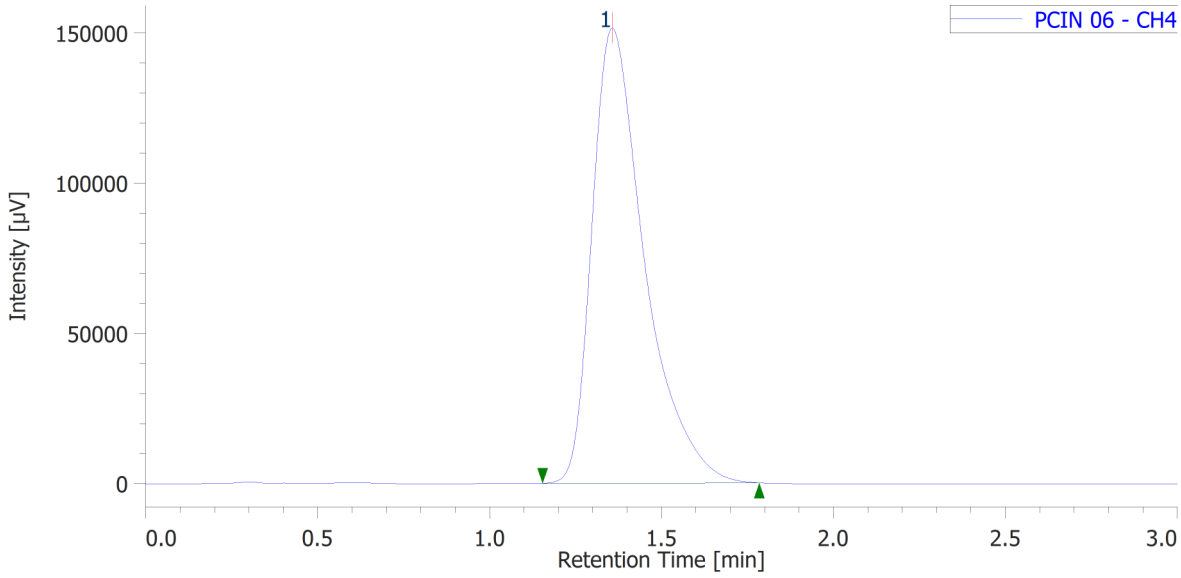

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 13:14:51
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 13:11:47
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.357	1608153	151436	100.000	100.000	N/A	420	N/A	1.590	

Creator QPackSA
Reviewer
Approver

Chromatogram

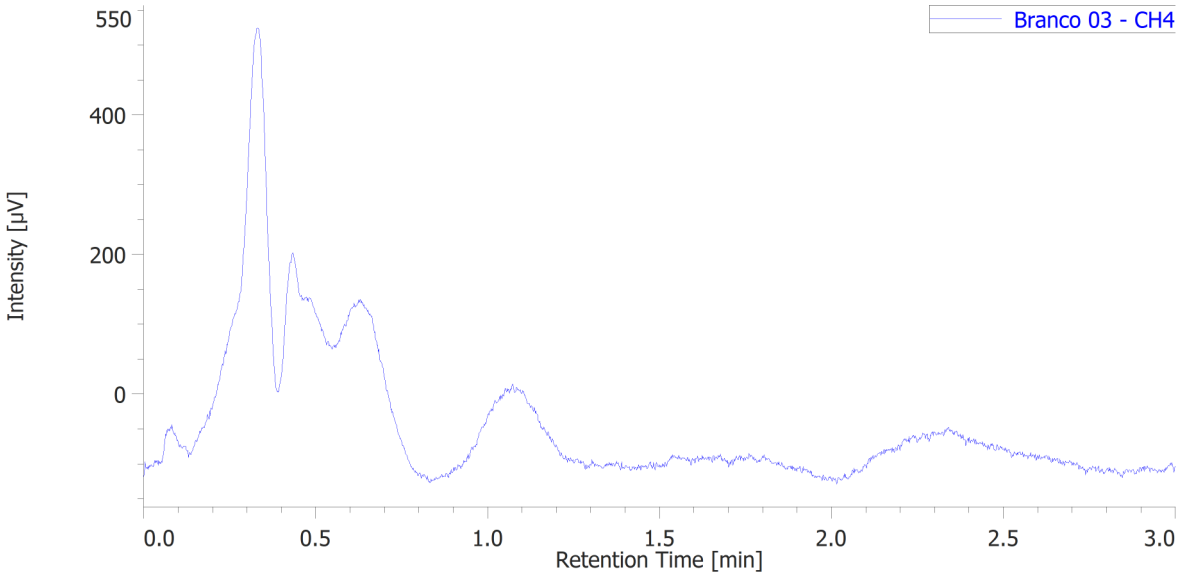


Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 13:18:43
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 13:15:40
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

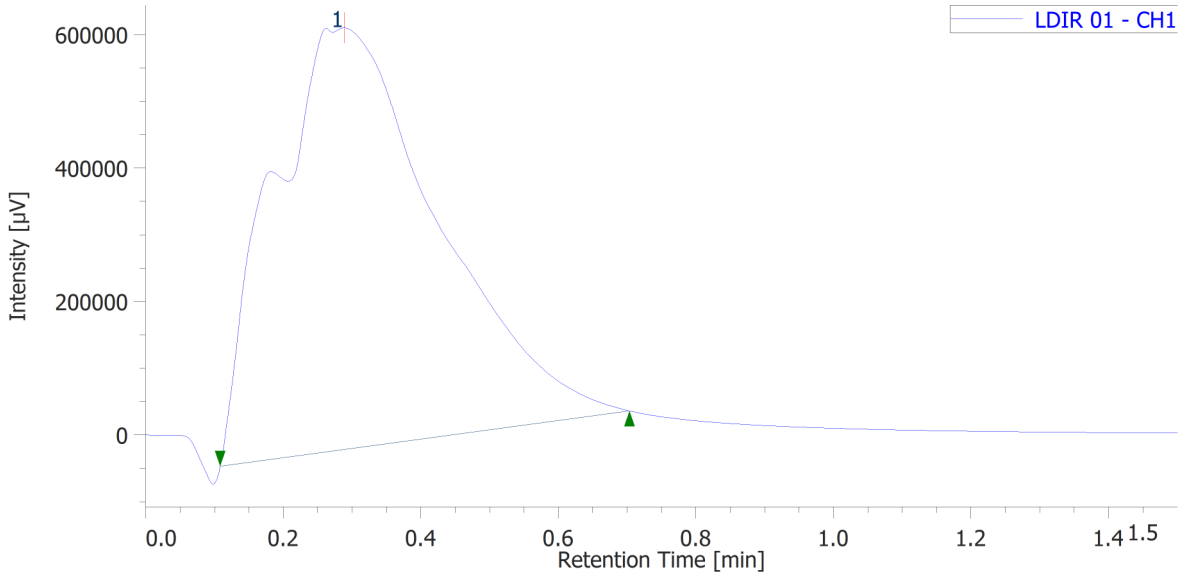

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 10:38:57
Description	
HPLC System Name	HPLC 002 RI
Injection Date	10/08/2023 10:06:58
Volume	0.1 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	1.5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH1
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.288	10550029	631284	100.000	100.000	N/A	6	N/A	1.500	

Creator
Reviewer
Approver

Chromatogram

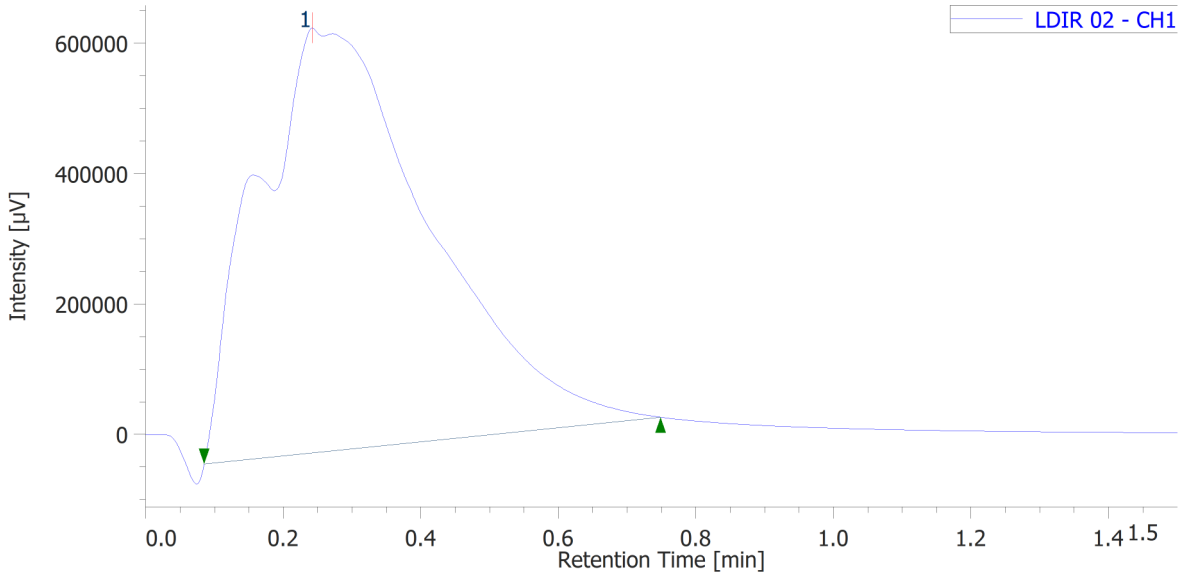

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 10:38:57
Description	
HPLC System Name	HPLC 002 RI
Injection Date	10/08/2023 10:09:39
Volume	2.0 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	1.5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH1
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.242	11300310	651640	100.000	100.000	N/A	4	N/A	1.859	

Creator
Reviewer
Approver

Chromatogram

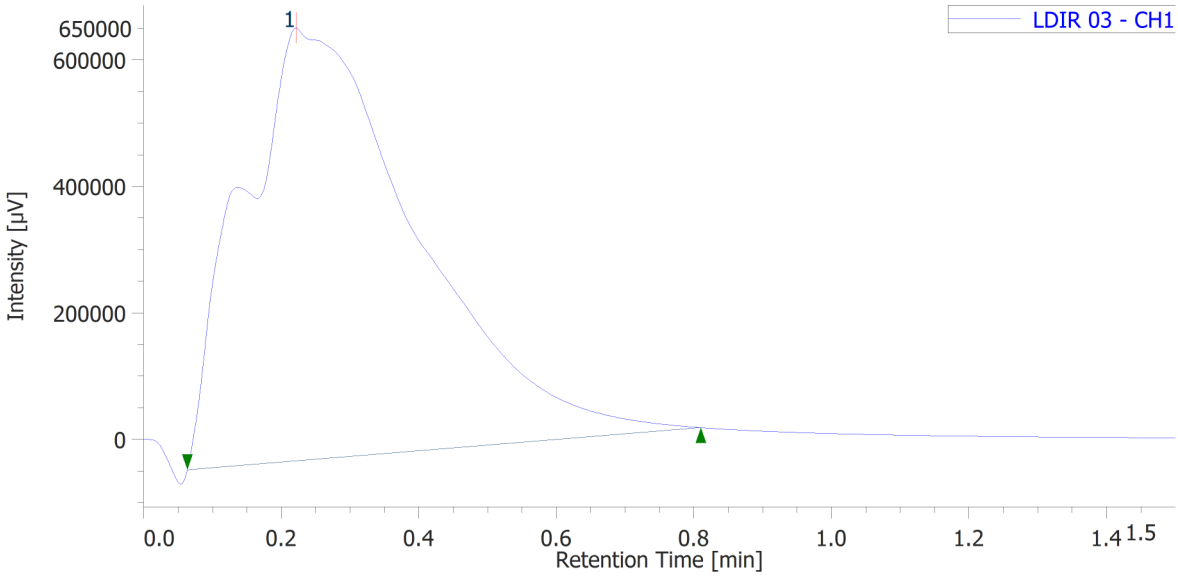

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 10:38:57
Description	
HPLC System Name	HPLC 002 RI
Injection Date	10/08/2023 10:12:22
Volume	4.0 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	1.5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH1
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.222	12099279	684104	100.000	100.000	N/A	3	N/A	1.964	

Creator
Reviewer
Approver

Chromatogram

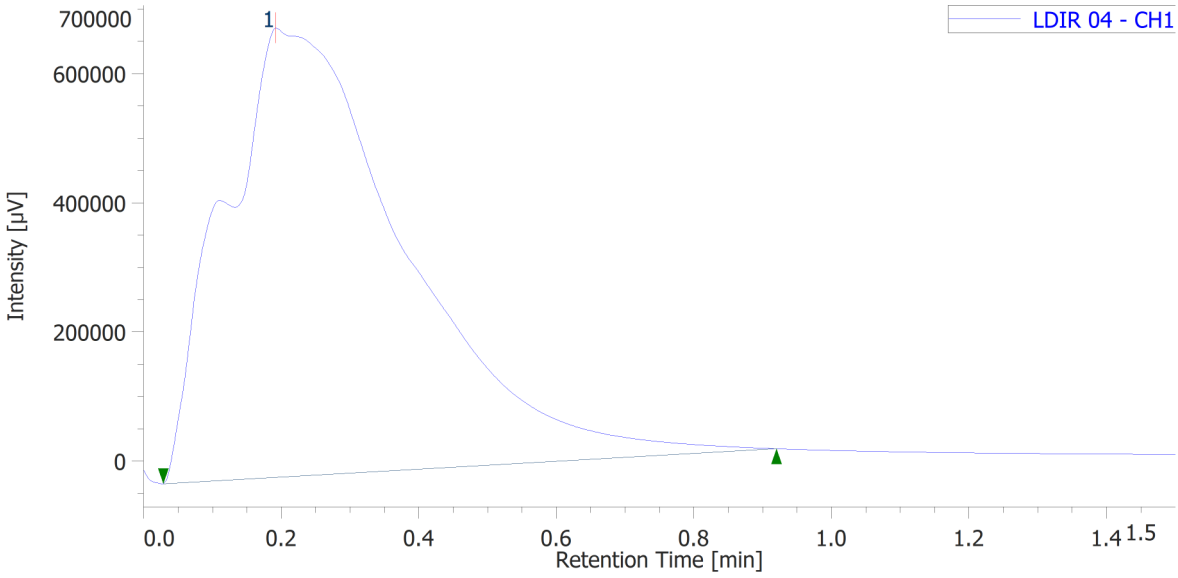

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 10:38:57
Description	
HPLC System Name	HPLC 002 RI
Injection Date	10/08/2023 10:15:08
Volume	6.0 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	1.5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH1
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.192	12797717	695646	100.000	100.000	N/A	2	N/A	2.117	

Creator
Reviewer
Approver

Chromatogram

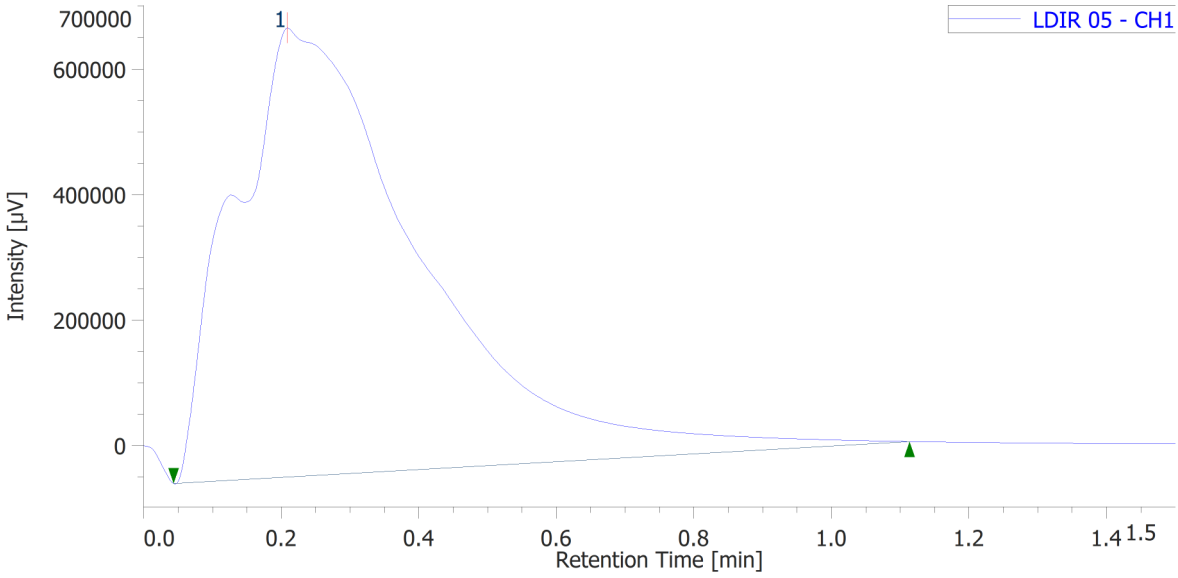

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 10:38:57
Description	
HPLC System Name	HPLC 002 RI
Injection Date	10/08/2023 10:17:54
Volume	8.0 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	1.5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH1
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0.208	13569652	715478	100.000	100.000	N/A	3	N/A	2.382	

Creator
Reviewer
Approver

Chromatogram

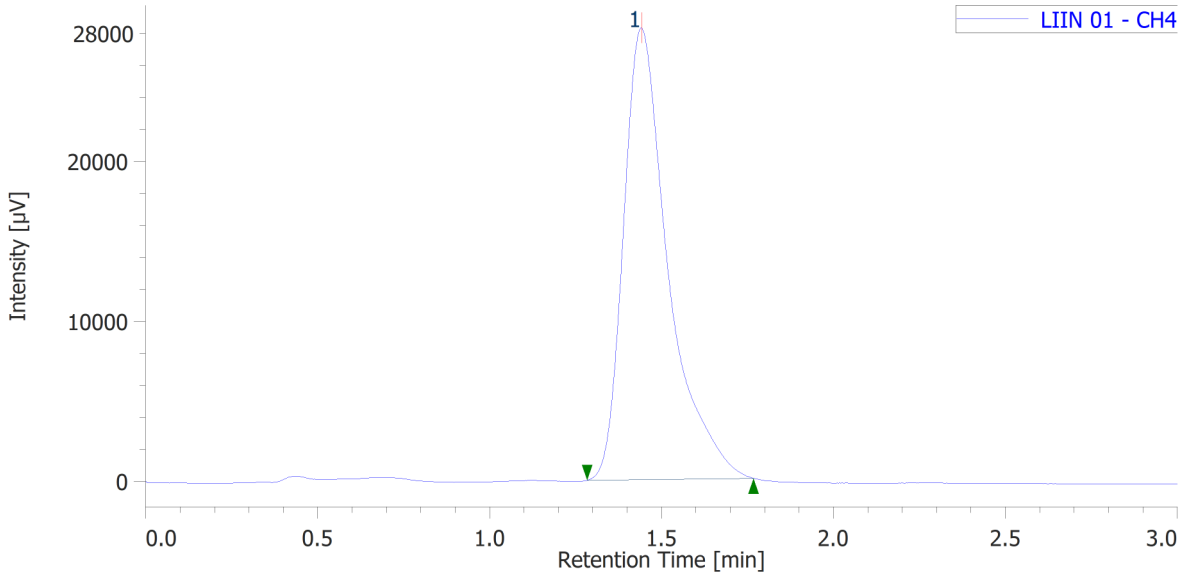

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:10:28
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:07:25
Volume	0.1 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.442	254310	28217	100.000	100.000	N/A	697	N/A	1.569	

Creator QPackSA
Reviewer
Approver

Chromatogram

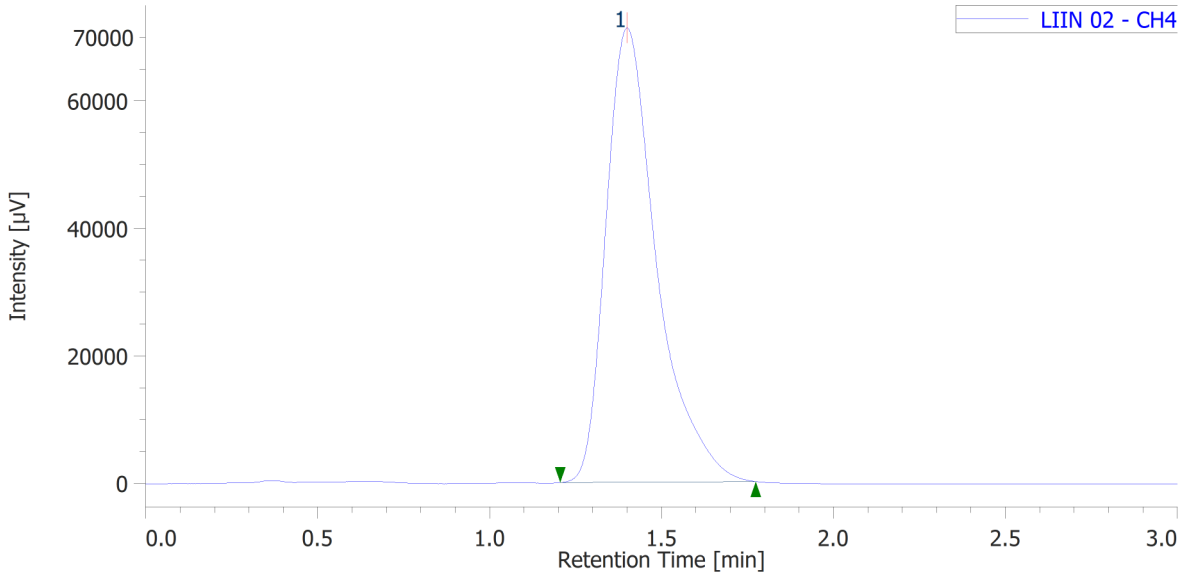

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:14:16
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:11:13
Volume	5.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.400	732335	71240	100.000	100.000	N/A	482	N/A	1.493	

Creator QPackSA
Reviewer
Approver

Chromatogram

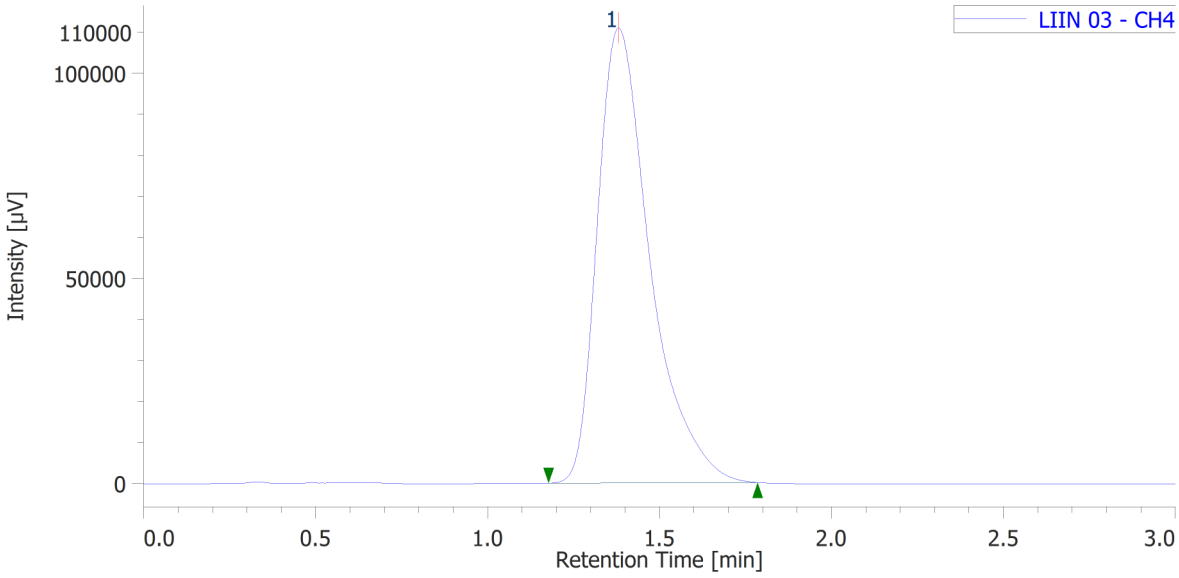

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:18:08
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:15:05
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.380	1181362	110862	100.000	100.000	N/A	427	N/A	1.540	

Creator QPackSA
Reviewer
Approver

Chromatogram

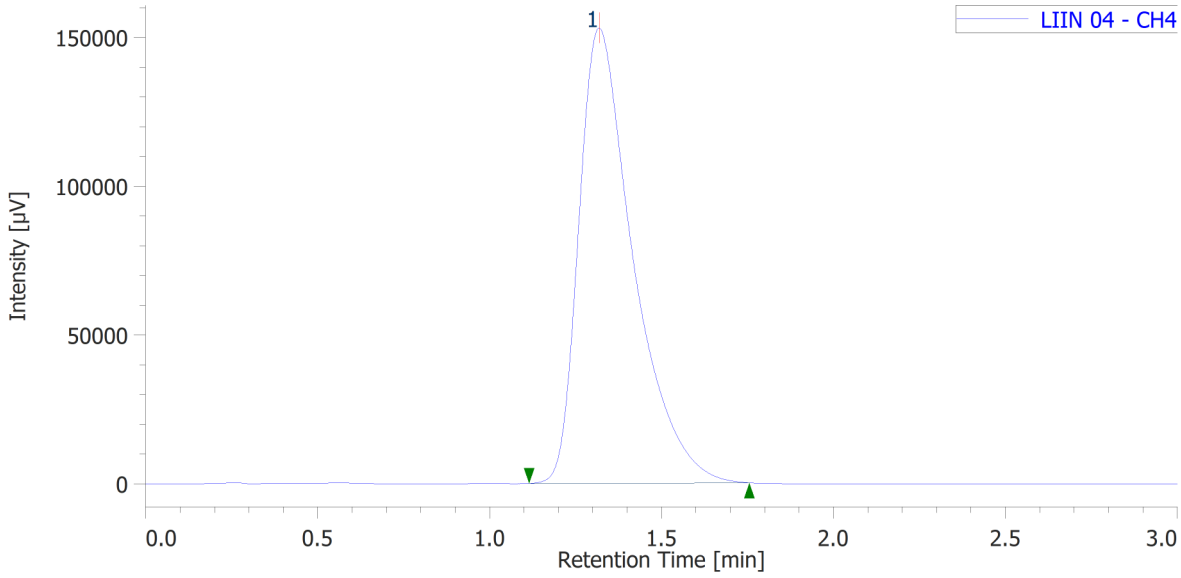

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:22:08
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:19:04
Volume	15.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.318	1679732	152899	100.000	100.000	N/A	366	N/A	1.621	

Creator QPackSA
Reviewer
Approver

Chromatogram

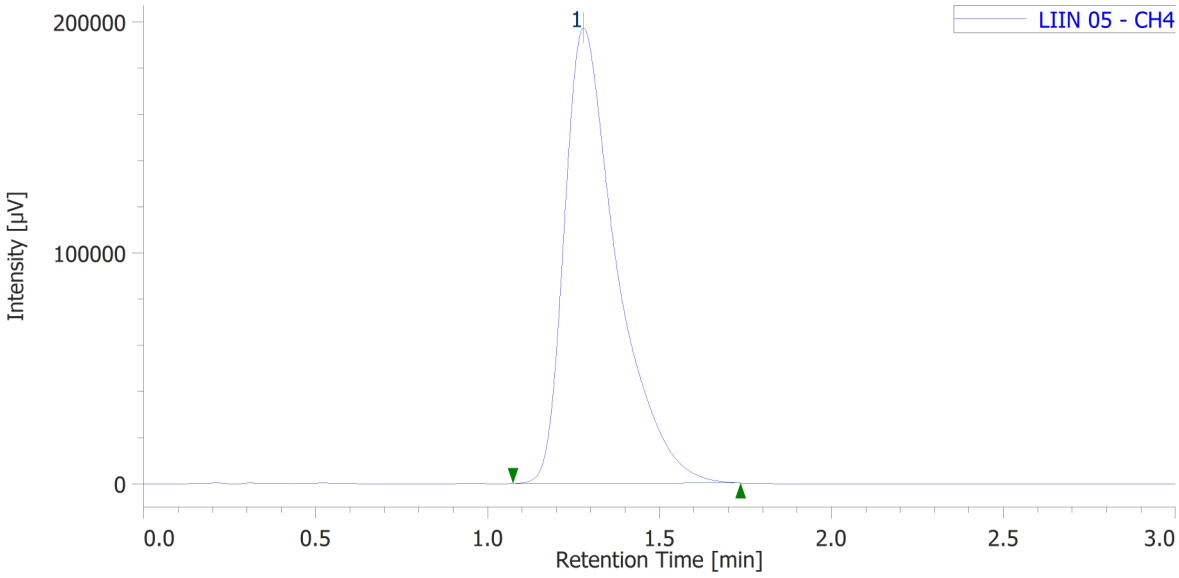

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 14:26:10
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:23:07
Volume	20.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1.278	2093812	197154	100.000	100.000	N/A	387	N/A	1.675	

Creator QPackSA
Reviewer
Approver

Chromatogram

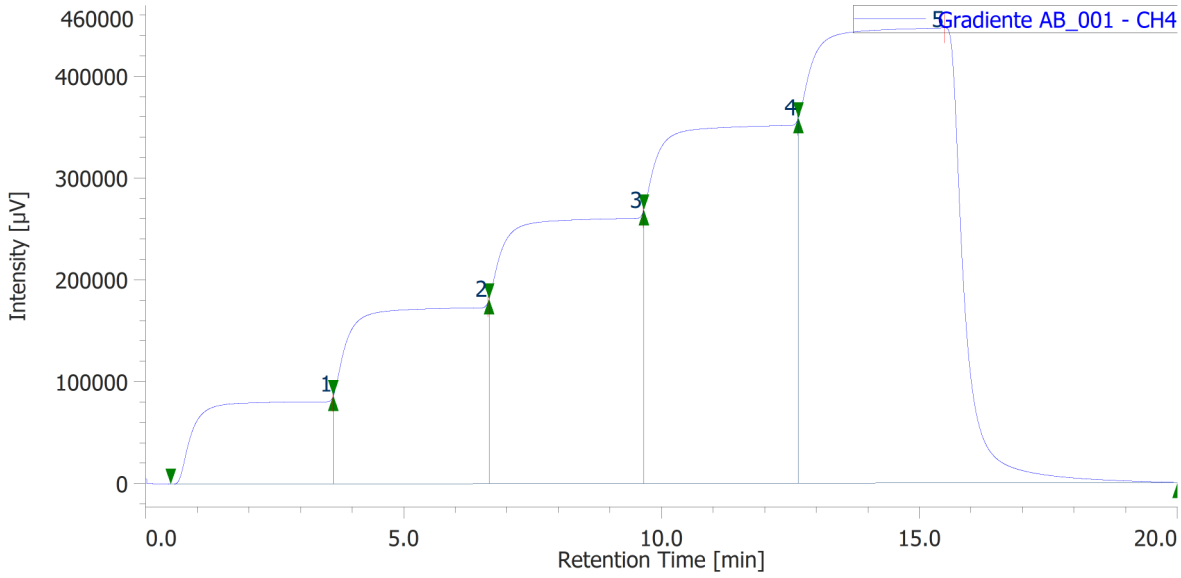

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 16:03:15
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 14:54:51
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	4	3.630	13216238	85646	5.597	6.430	N/A	N/A	N/A	N/A	
2	40%	4	6.635	29745552	178317	12.598	13.387	N/A	N/A	N/A	N/A	
3	60%	4	9.635	45405561	265574	19.230	19.938	N/A	N/A	N/A	N/A	
4	80%	4	12.633	61681228	356060	26.123	26.731	N/A	N/A	N/A	N/A	
5	100%	4	15.482	86072693	446424	36.453	33.515	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

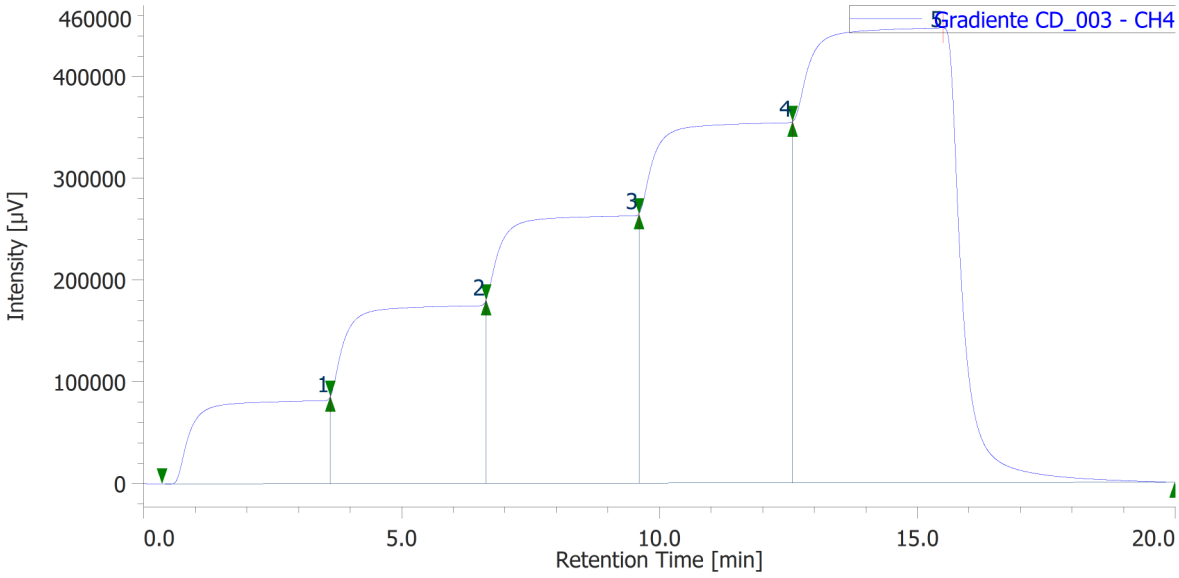

Chromatogram Information	
User Name	QPackSA
Date Modified	09/08/2023 16:03:15
Description	
HPLC System Name	HPLC 002 RI
Injection Date	09/08/2023 15:36:41
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_003-CH4
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	4	3.610	13163312	85014	5.540	6.391	N/A	N/A	N/A	N/A	
2	40%	4	6.630	29971554	179565	12.614	13.500	N/A	N/A	N/A	N/A	
3	60%	4	9.590	45164812	264167	19.008	19.860	N/A	N/A	N/A	N/A	
4	80%	4	12.570	61494141	354758	25.880	26.671	N/A	N/A	N/A	N/A	
5	100%	4	15.495	87817951	446619	36.959	33.577	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver