
Chromatogram

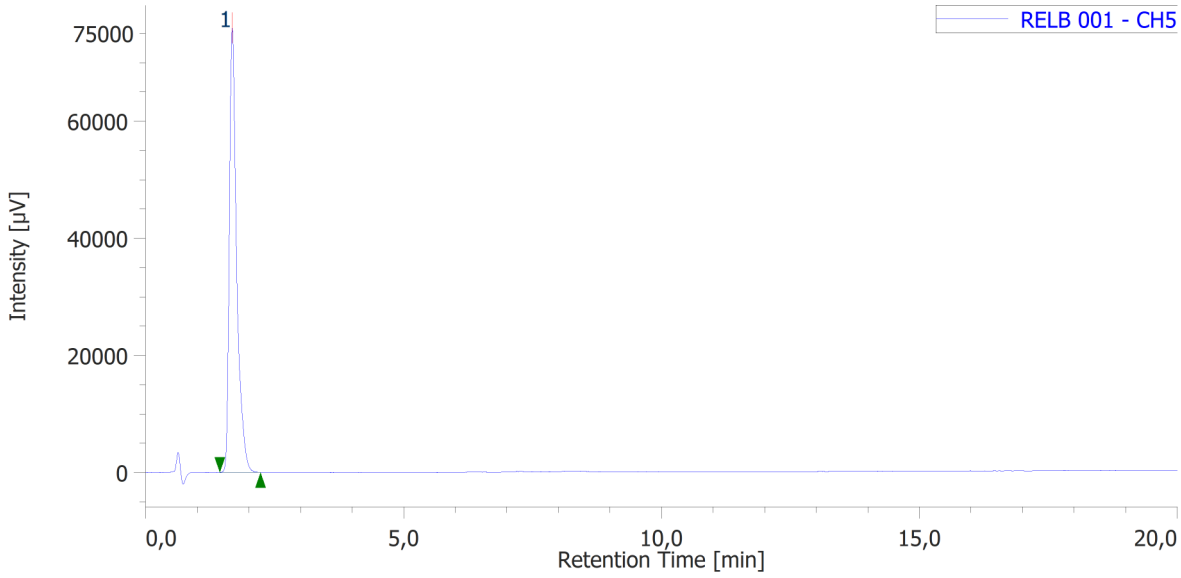


Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:44:55
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 17:50:18
Volume	20,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	RELB 001-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1,677	752680	75861	100,000	100,000	N/A	785	N/A	1,574		3488,6

Creator QPackSA
Reviewer
Approver

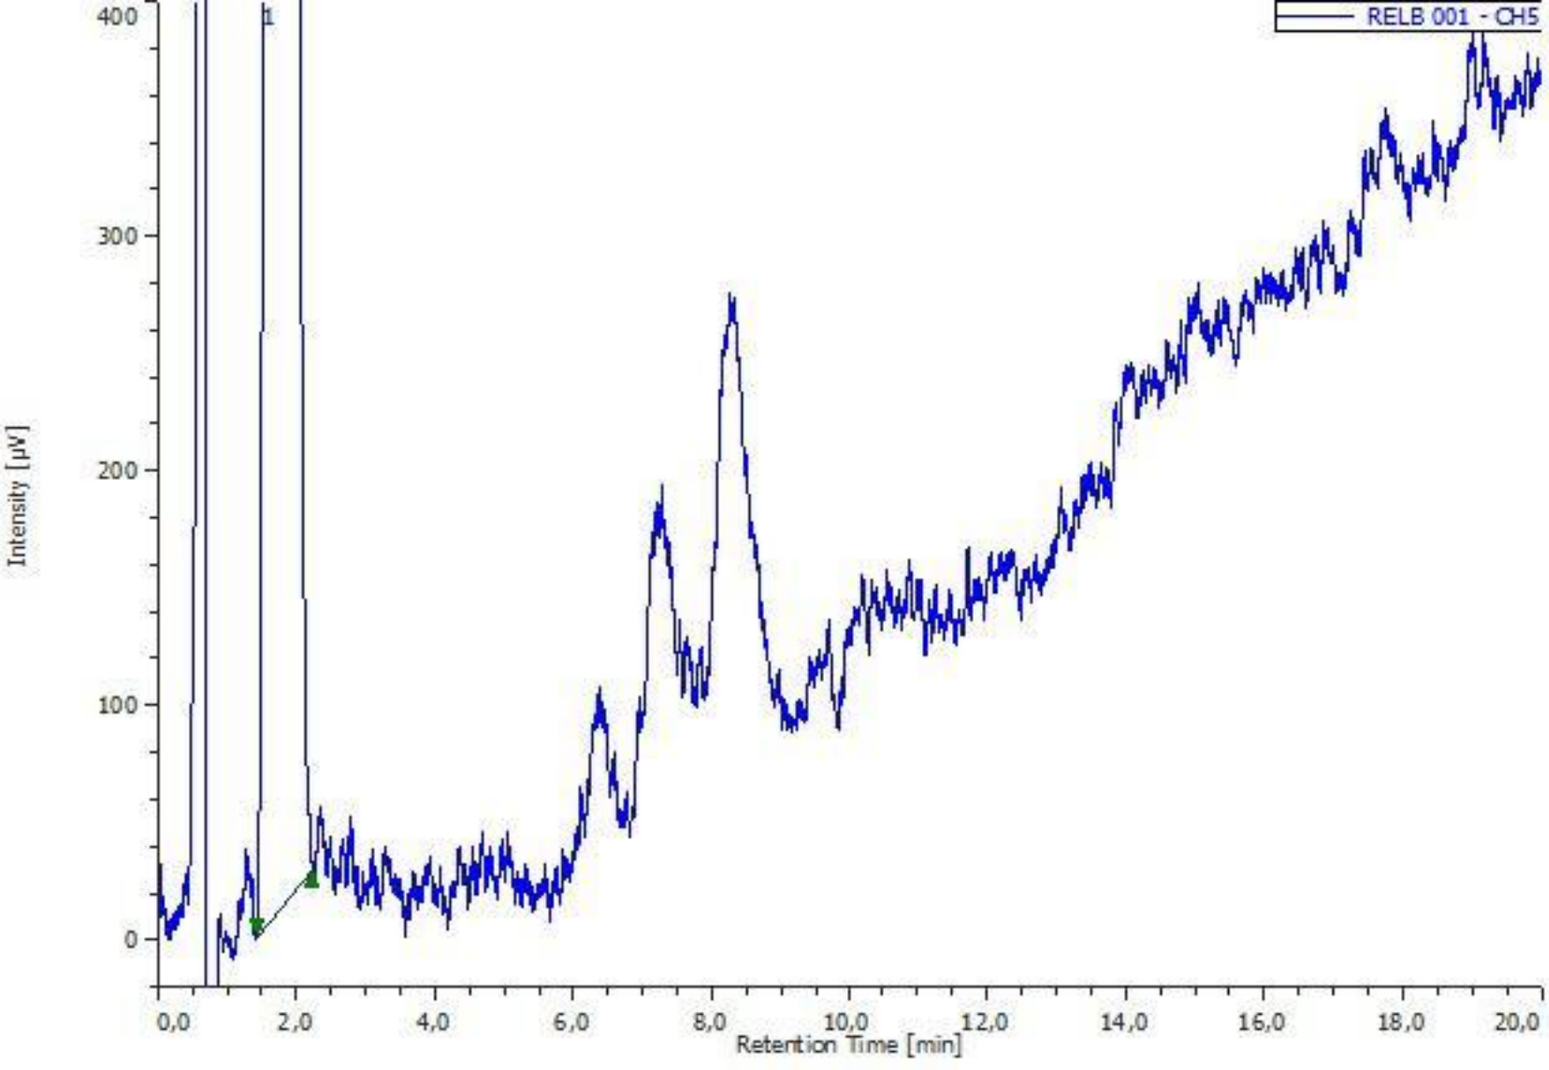
RELB 001 - CH5
1
400
300
200
100
0
Intensity [µV]
0,0
2,0
4,0
6,0
8,0
10,0
12,0
14,0
16,0
18,0
20,0
Retention Time [min]

Chromatogram

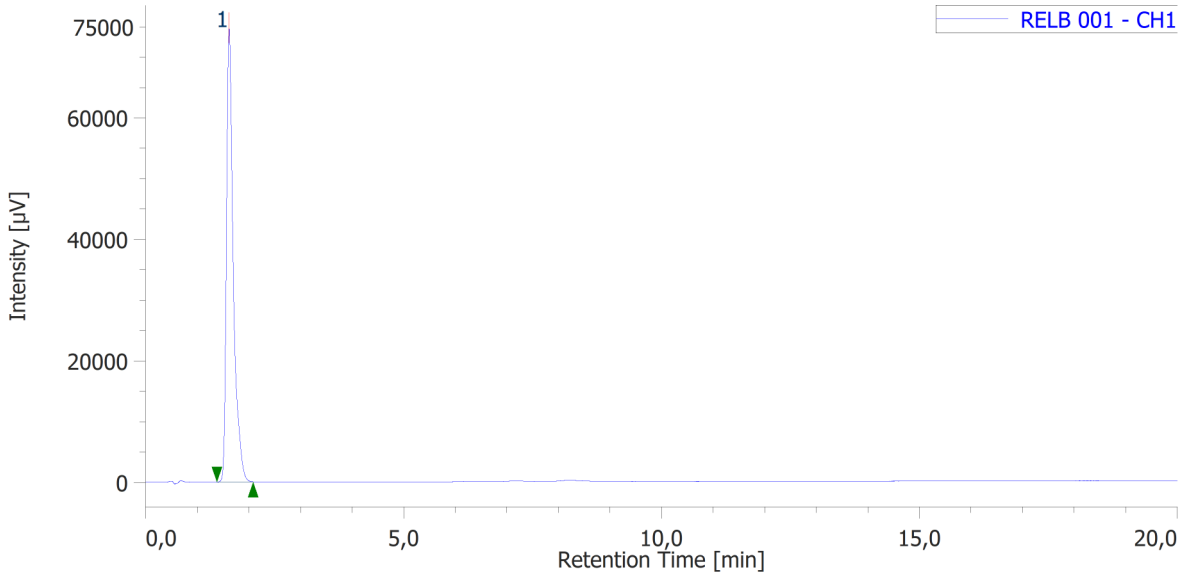


Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:44:55
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 17:50:18
Volume	20,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	RELB 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,615	689769	74687	100,000	100,000	N/A	851	N/A	1,640		10267,5

Creator QPackSA
Reviewer
Approver

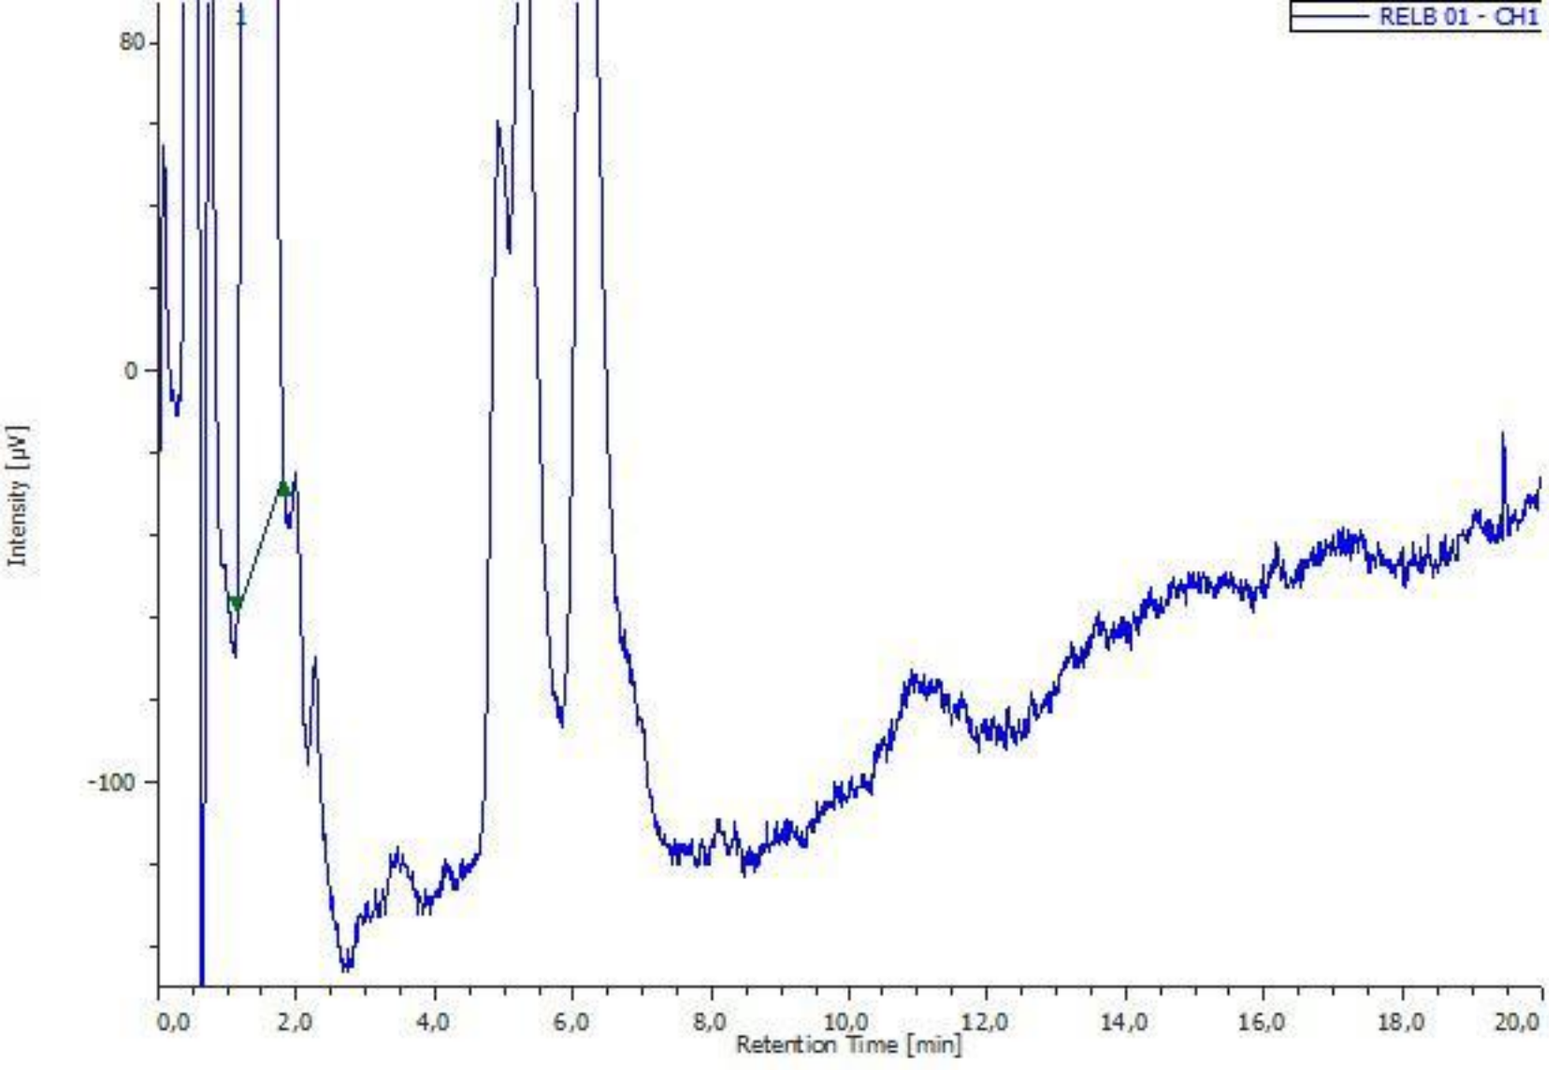
RELB 01 - CH1
1
80
0
-100
Intensity [µV]
0,0
2,0
4,0
6,0
8,0
10,0
12,0
14,0
16,0
18,0
20,0
Retention Time [min]

Peak Find - EDUV HPLC-0003 PDA 2023.jws

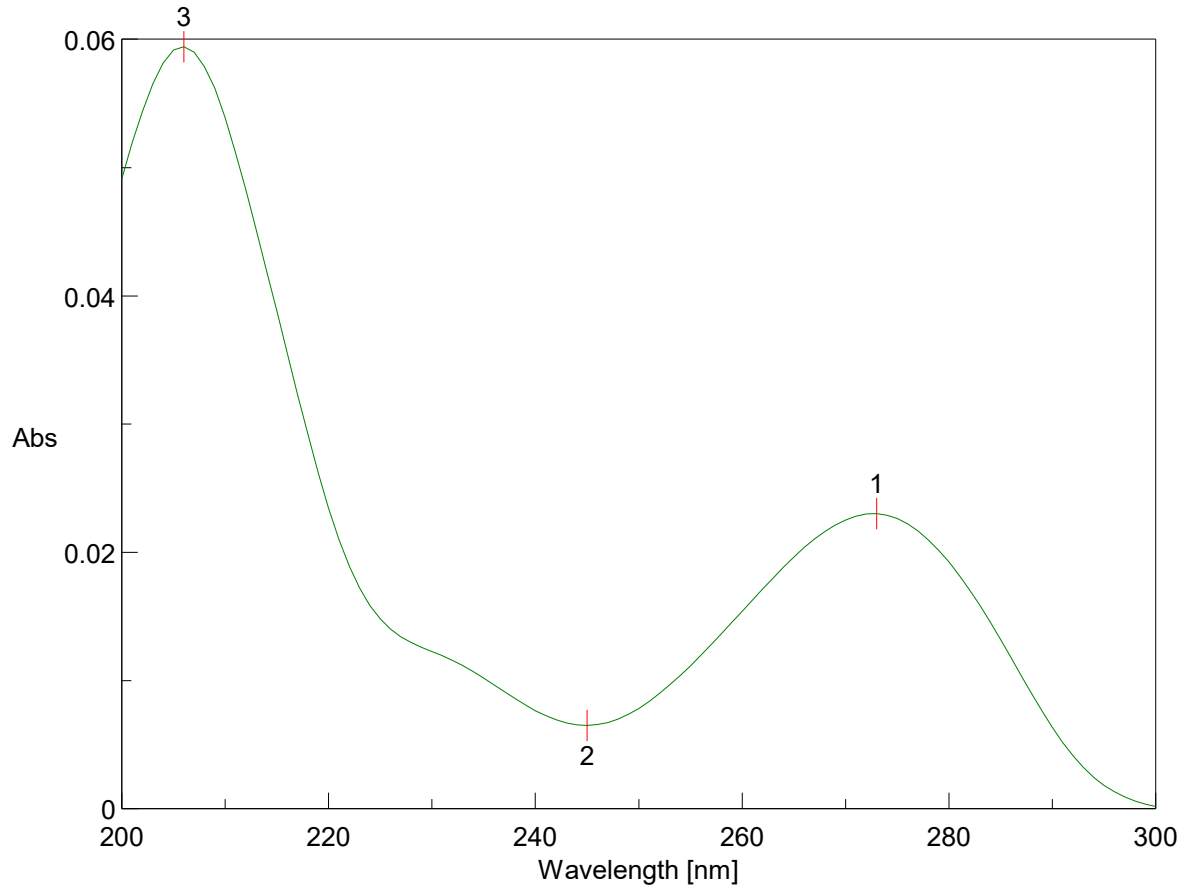

[Comments]

User	QPackSA
Workgroup	QPack
Division	Suporte Técnico
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	10/08/2023 15:14
Date modified	10/08/2023 15:14


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	300 nm	
Data interval	1 nm	
Data points	101	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.022999	2	245	0.006498
3	206	0.059409			

Creation	QPackSA
Review	
Approval	

Peak Find - EDUV HPLC-003 2023.jws

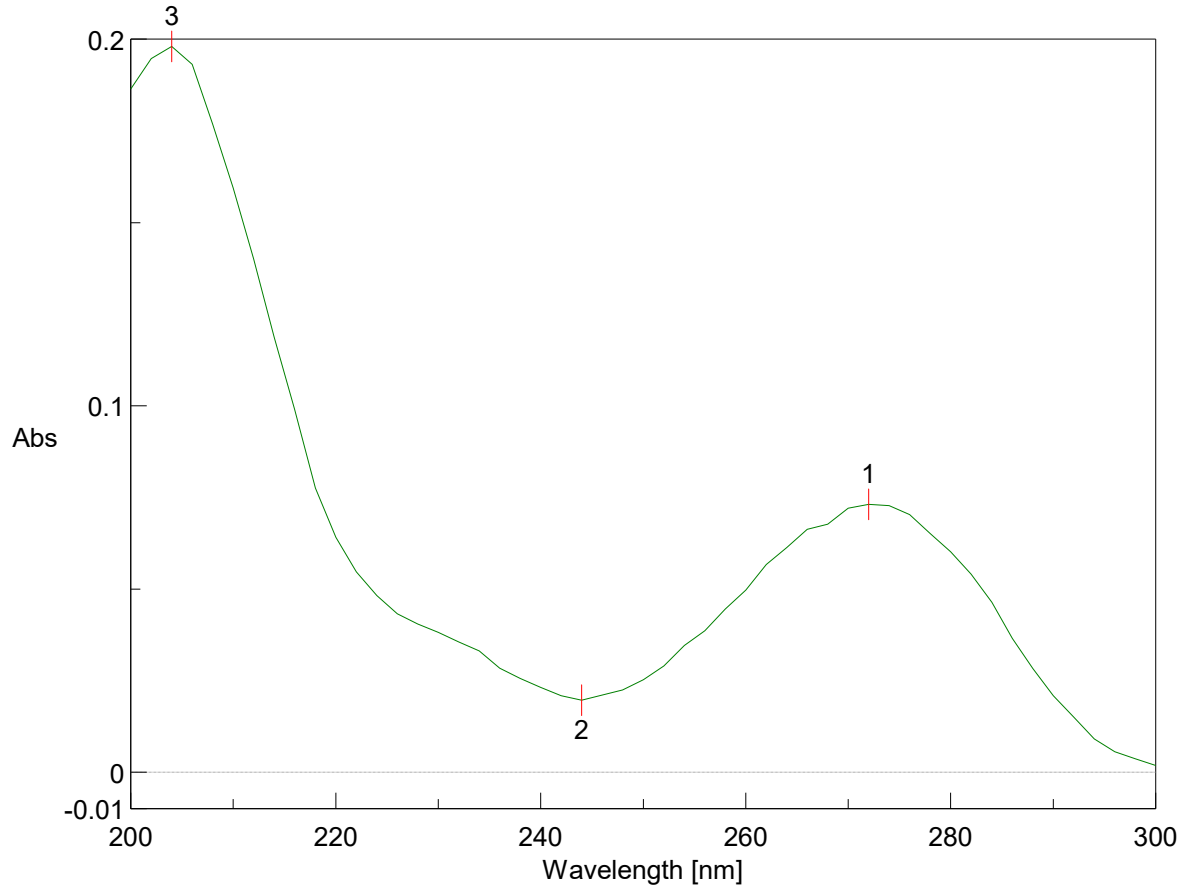

[Comments]

User	QPackSA
Workgroup	QPack
Division	Suporte Técnico
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	10/08/2023 15:09


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	370 nm	
Data interval	2 nm	
Data points	86	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0730077	2	244	0.0196176
3	204	0.197964			

Creation	QPackSA
Review	
Approval	

Chromatogram

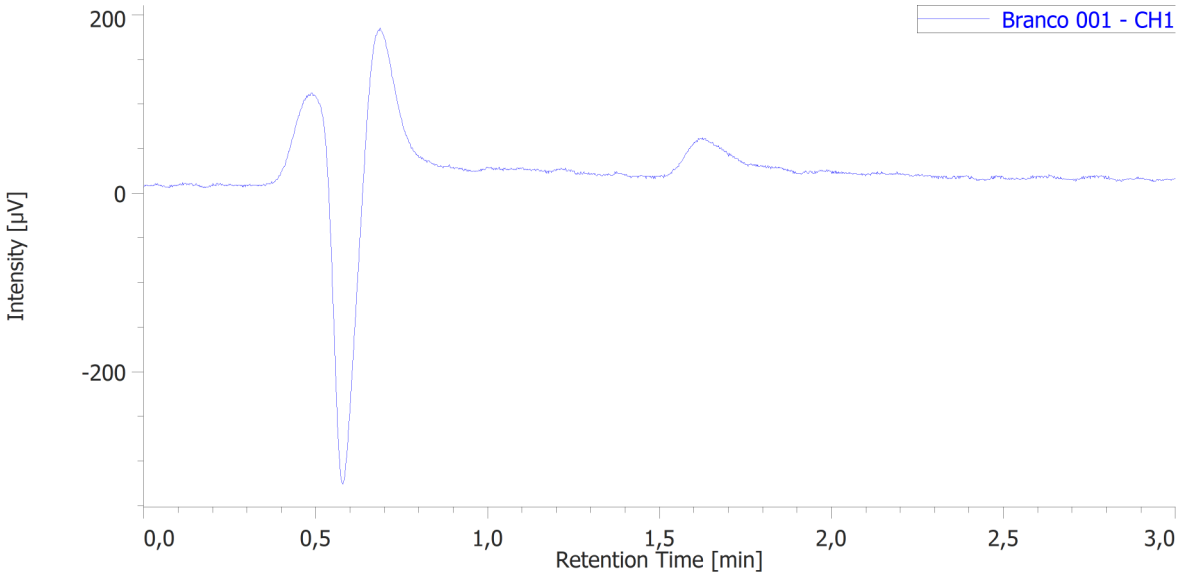


Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:42:22
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:39:20
Volume	10.0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

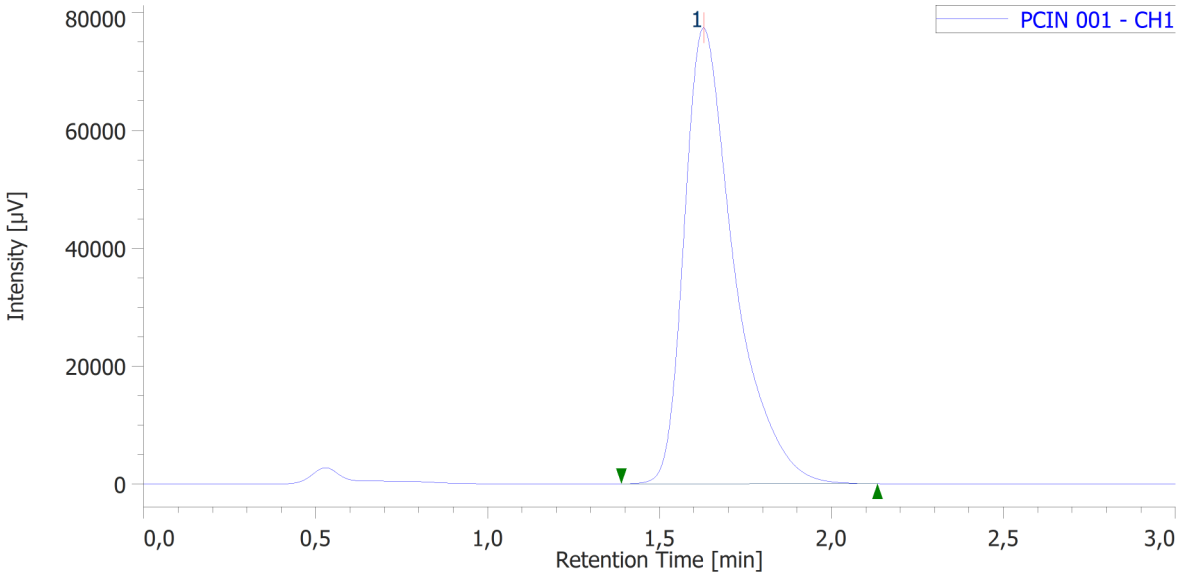

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:45:34
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:42:32
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.628	780488	77292	100.000	100.000	N/A	689	N/A	1.564		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

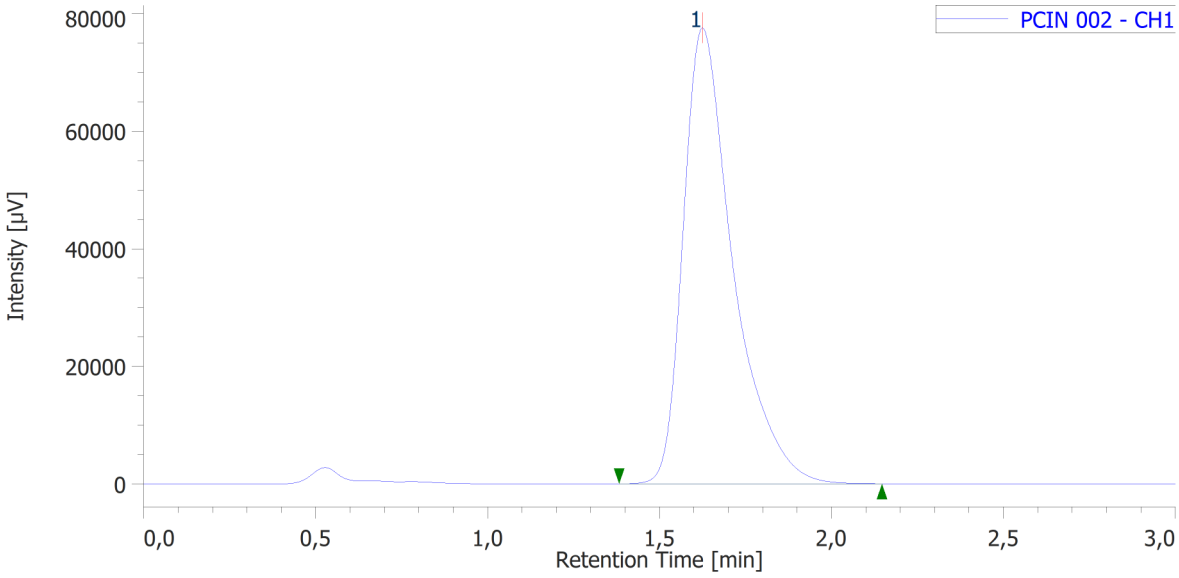

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:48:46
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:45:44
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.625	780831	77461	100.000	100.000	N/A	688	N/A	1.564		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

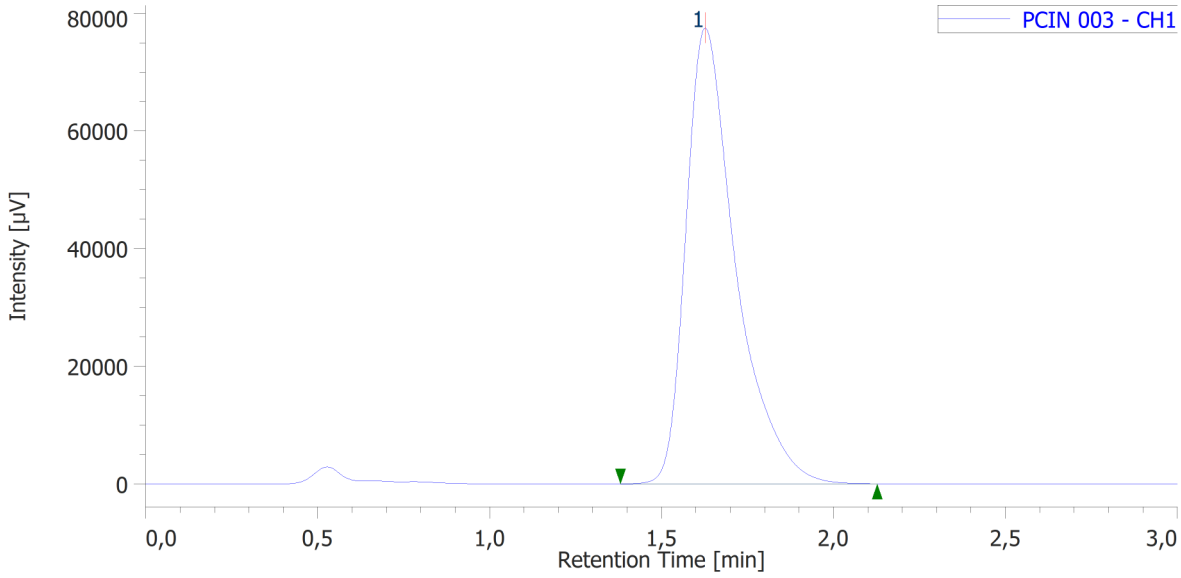

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:51:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:48:56
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.627	780065	77439	100.000	100.000	N/A	691	N/A	1.573		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

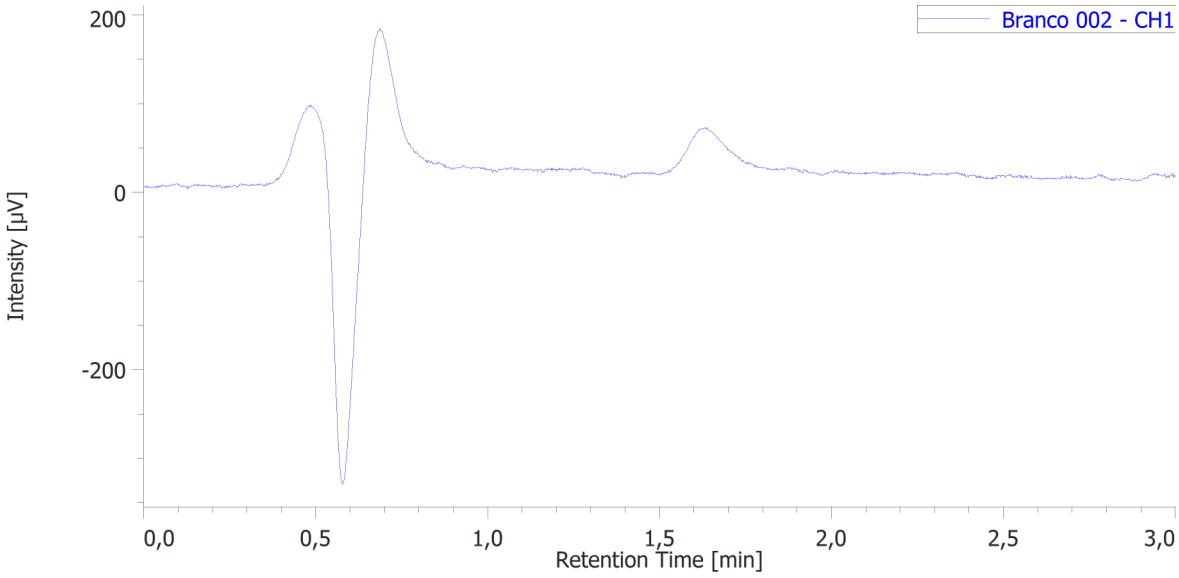


Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:55:10
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:52:08
Volume	10.0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

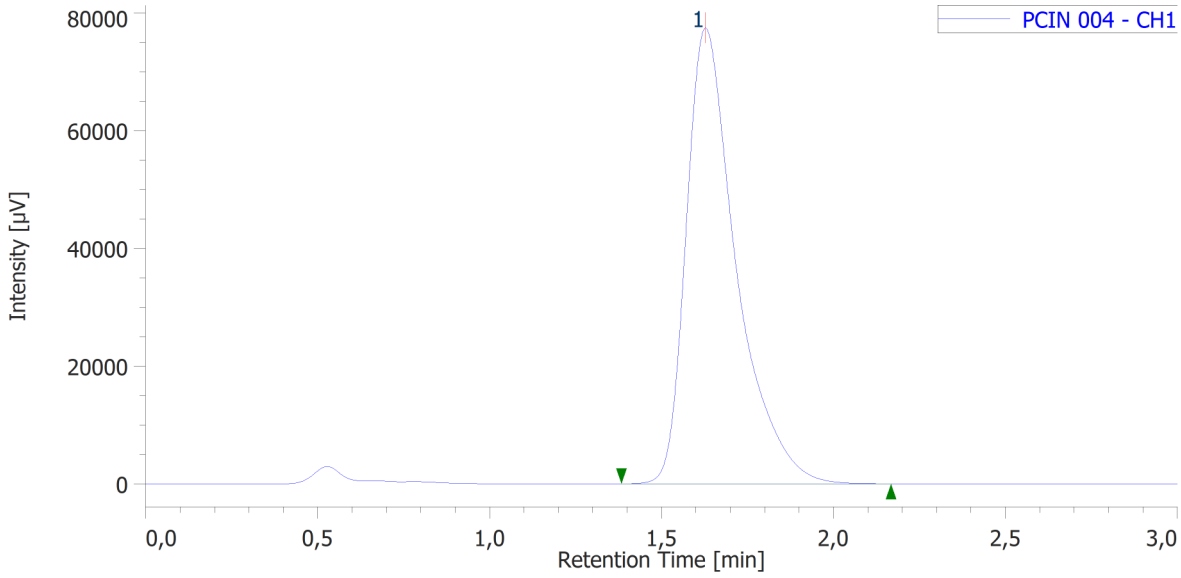

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 18:58:22
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:55:20
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.627	782635	77398	100.000	100.000	N/A	686	N/A	1.586		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

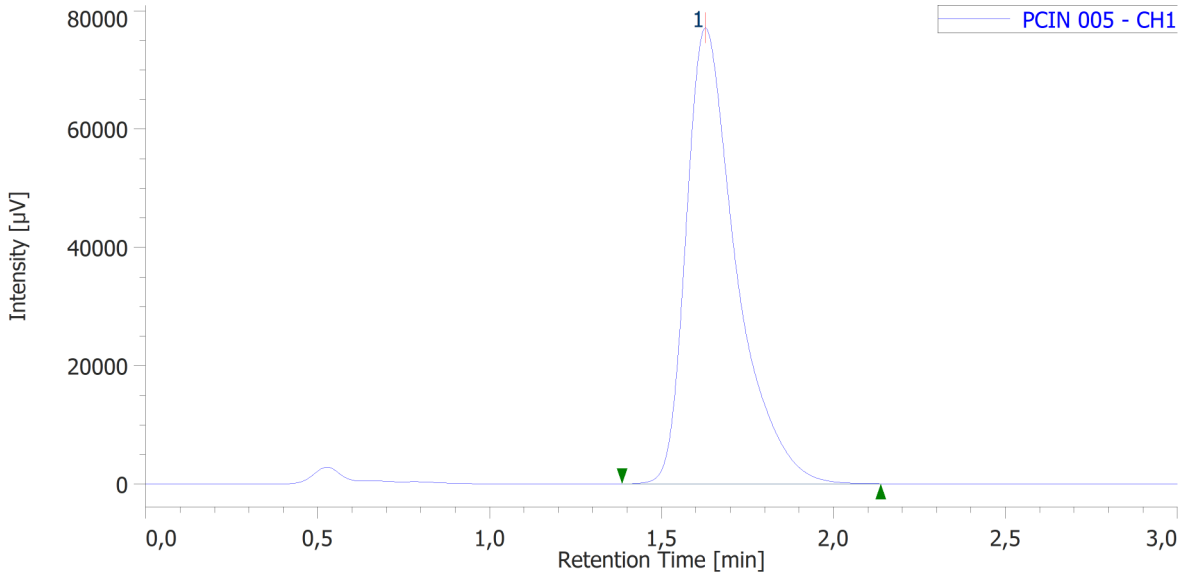

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 19:01:34
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 18:58:33
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.627	778579	76999	100.000	100.000	N/A	687	N/A	1.585		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

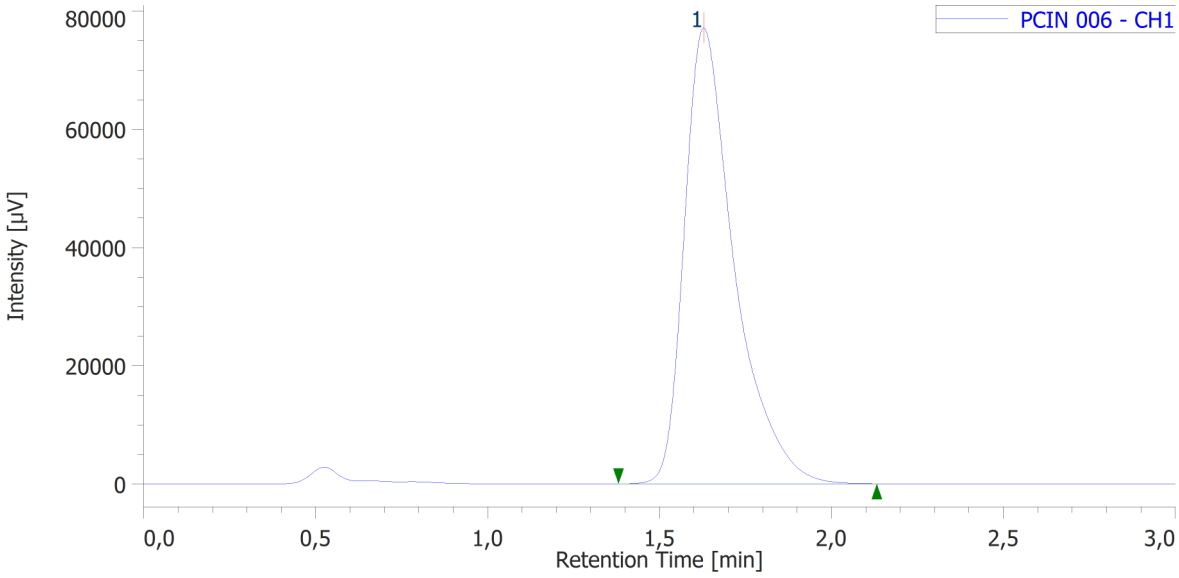

Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 19:04:46
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:01:45
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.628	779158	77073	100.000	100.000	N/A	688	N/A	1.573		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

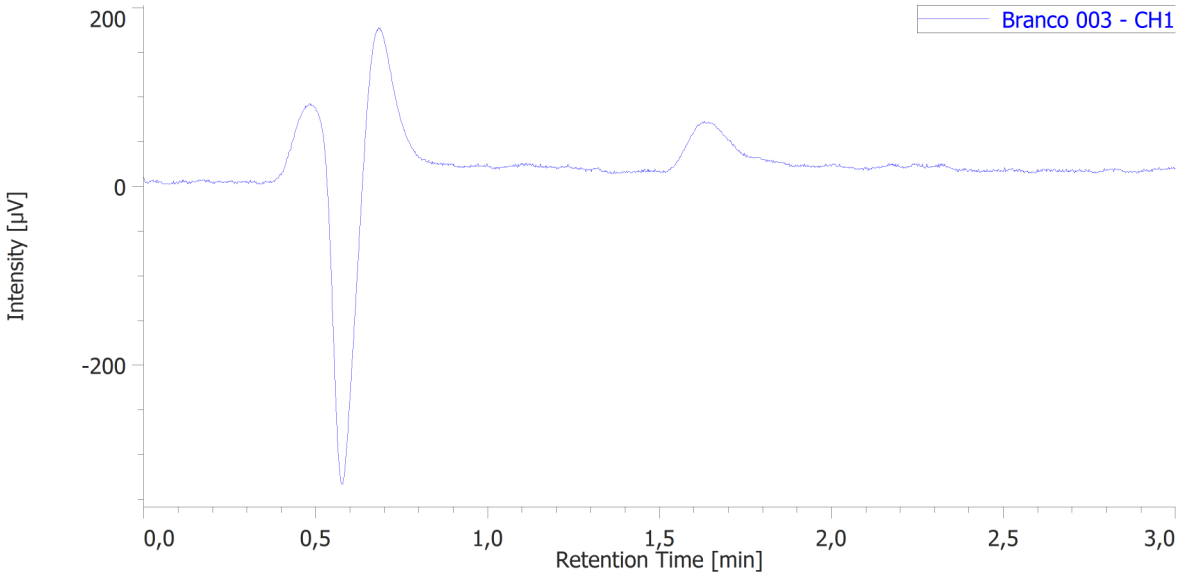


Chromatogram Information	
User Name	QPackSA
Date Modified	10/08/2023 19:08:00
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:04:57
Volume	10.0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

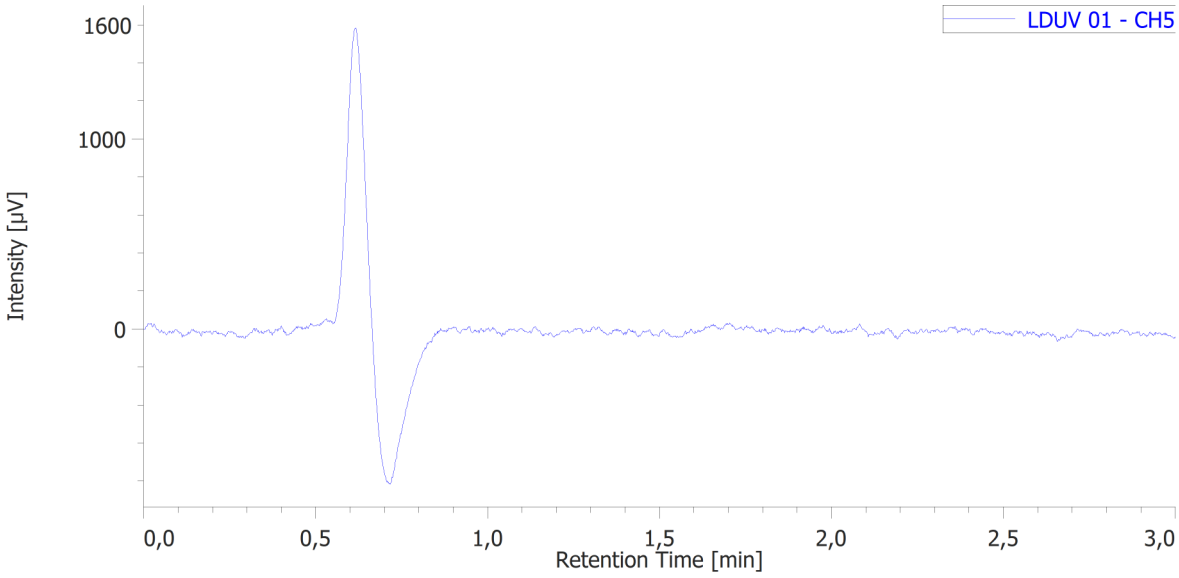


Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:23
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:08:09
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

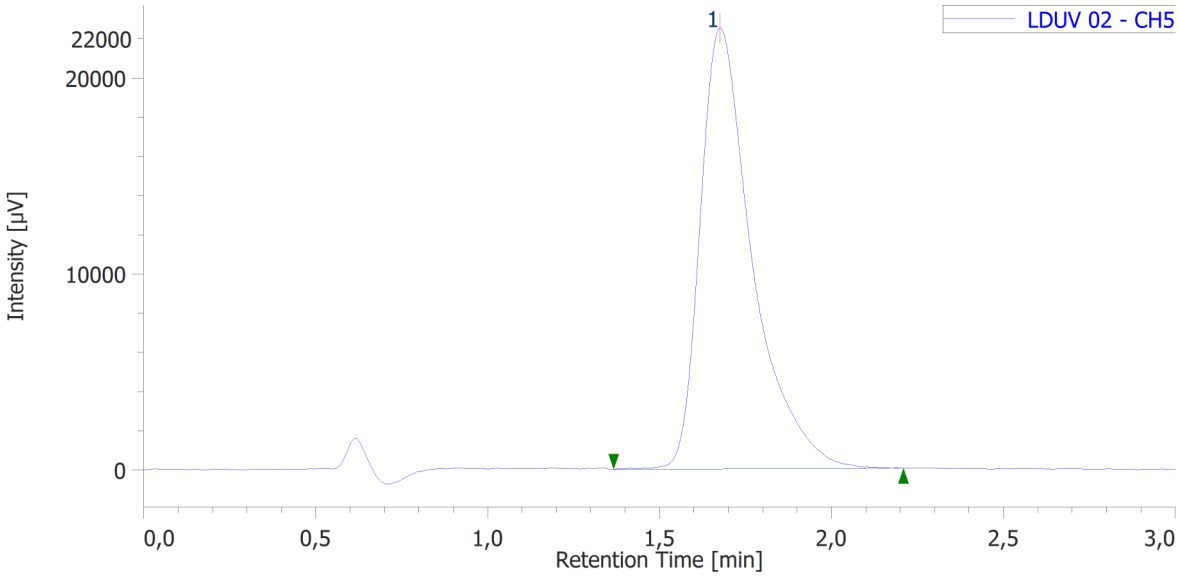

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:11:21
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:11:21
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.675	237657	22484	100.000	100.000	N/A	678	N/A	1.640		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

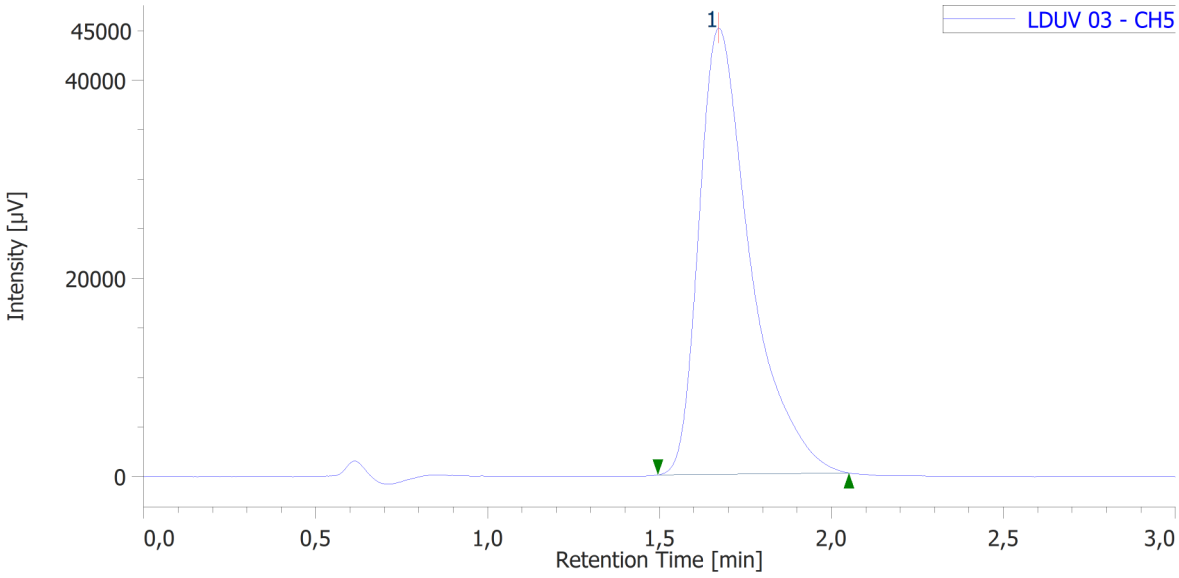

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:25
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:14:33
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.672	468205	45029	100.000	100.000	N/A	682	N/A	1.615		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

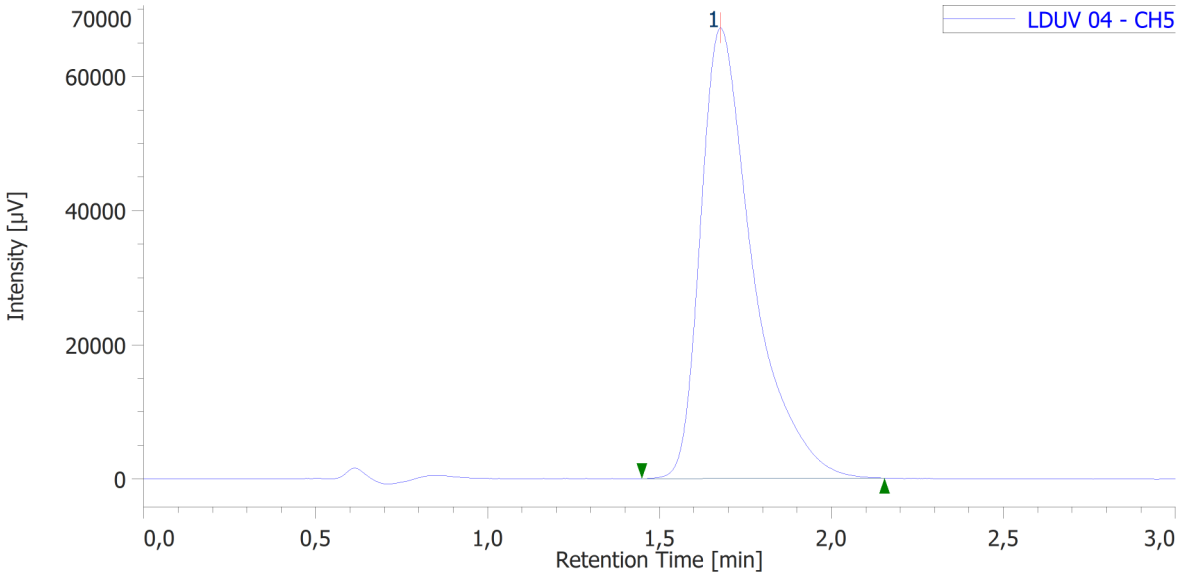

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:25
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:17:46
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.677	708659	67113	100.000	100.000	N/A	678	N/A	1.633		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

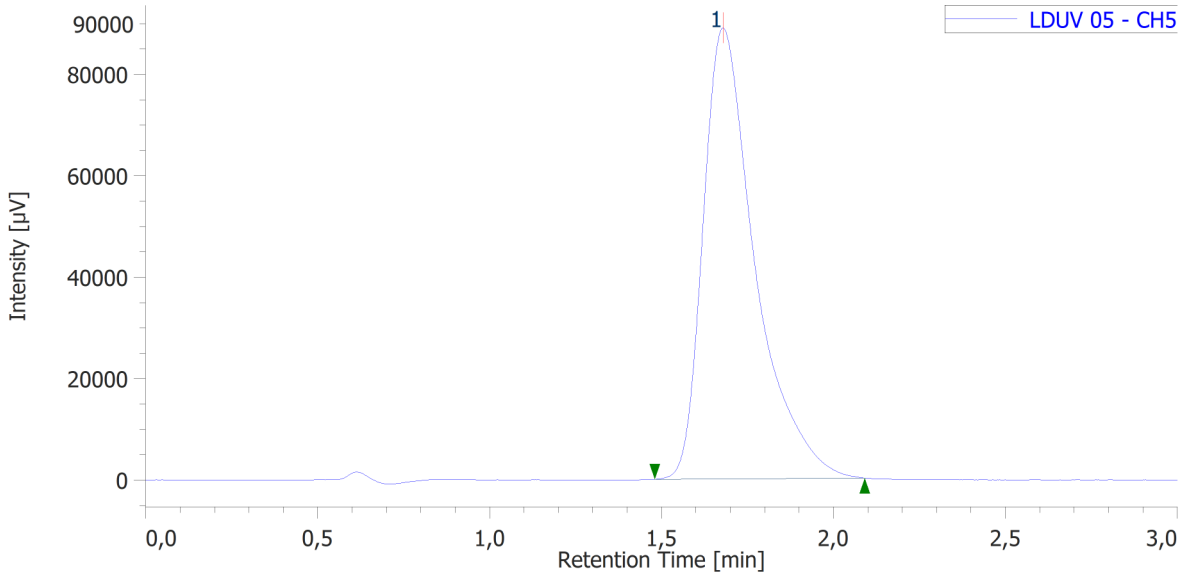

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:20:58
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.678	932660	88873	100.000	100.000	N/A	680	N/A	1.619		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

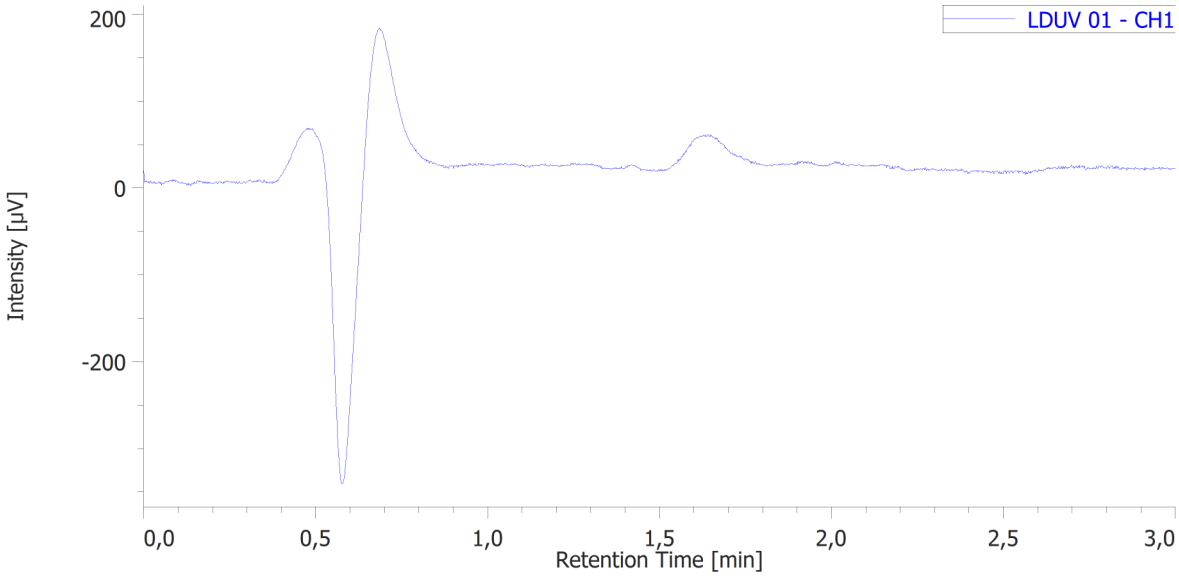


Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:23
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:08:09
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

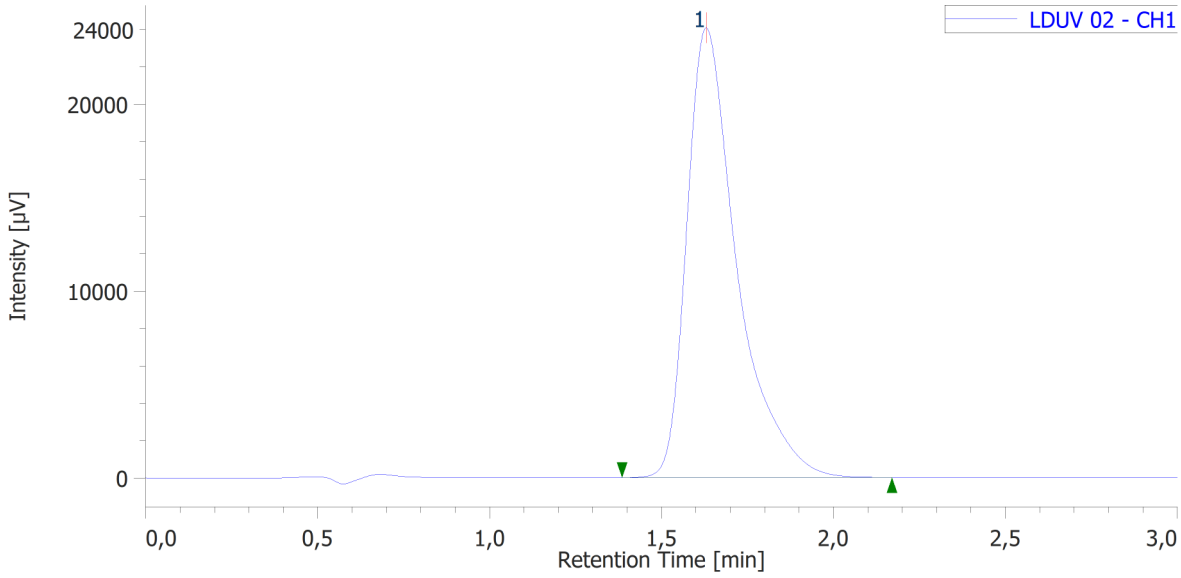

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:11:21
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:11:21
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,630	243611	24052	100,000	100,000	N/A	699	N/A	1,613		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

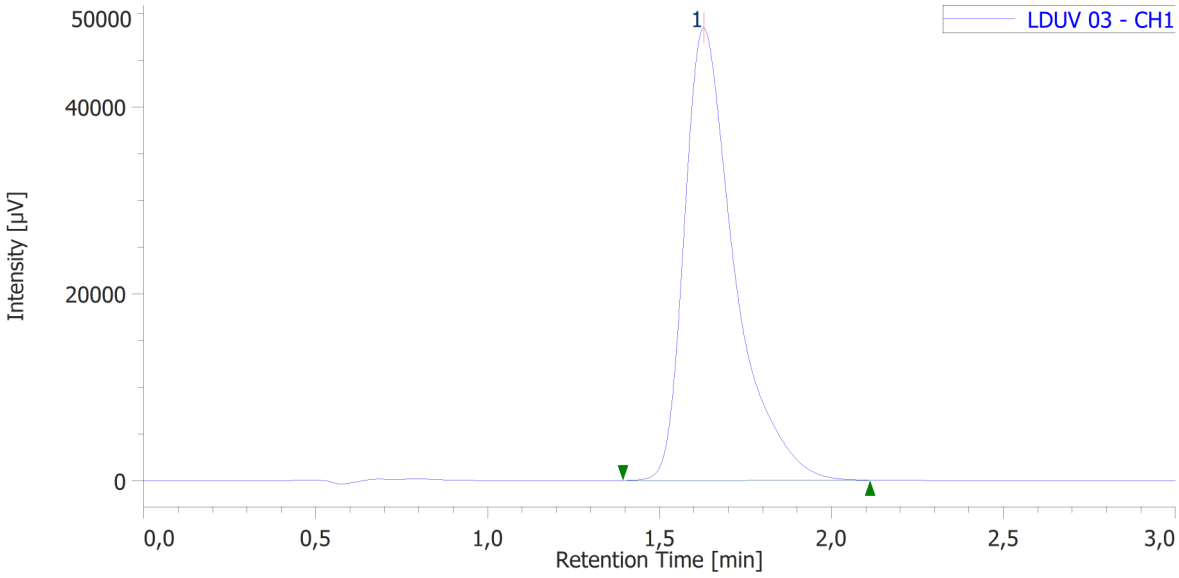

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:25
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:14:33
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.628	490031	48367	100.000	100.000	N/A	697	N/A	1.618		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

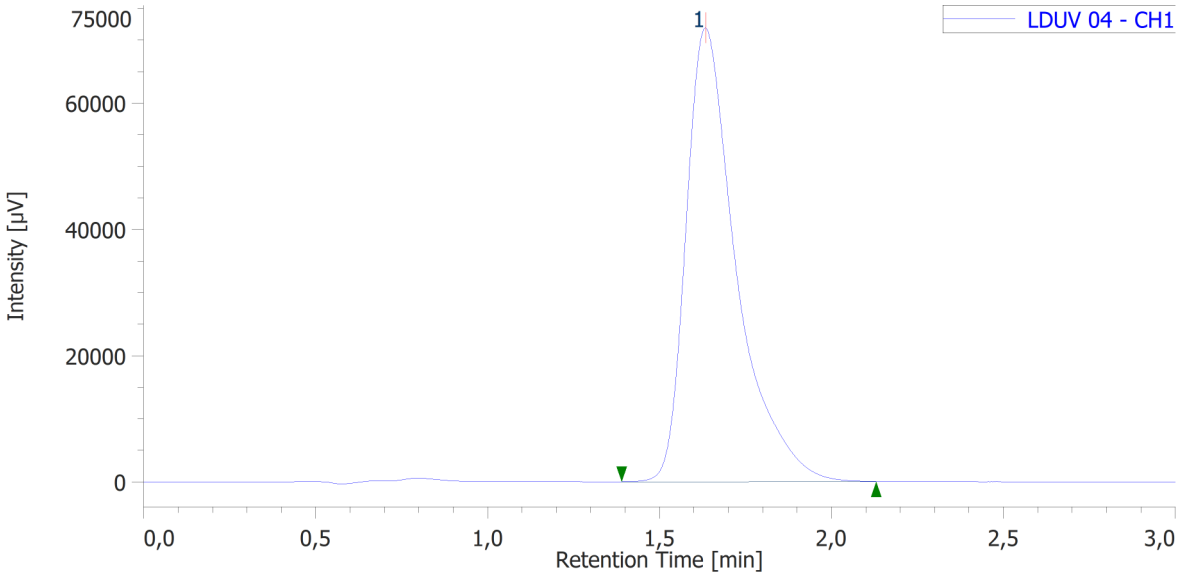

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 08:56:25
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:17:46
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,633	730103	71818	100,000	100,000	N/A	698	N/A	1,622		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

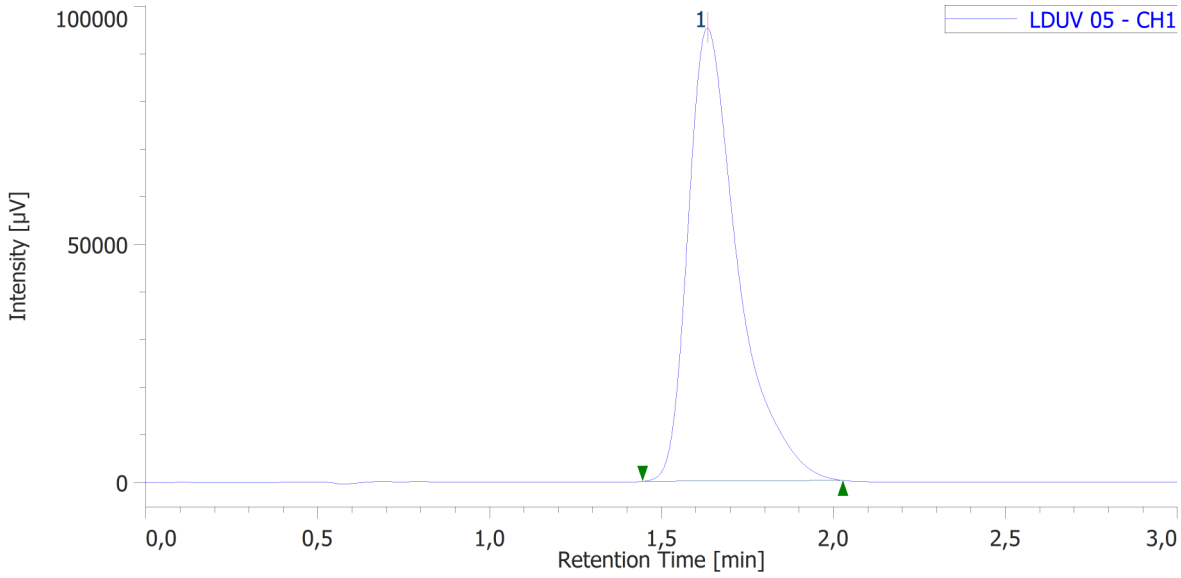

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:20:58
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.633	959056	95109	100.000	100.000	N/A	699	N/A	1.611		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

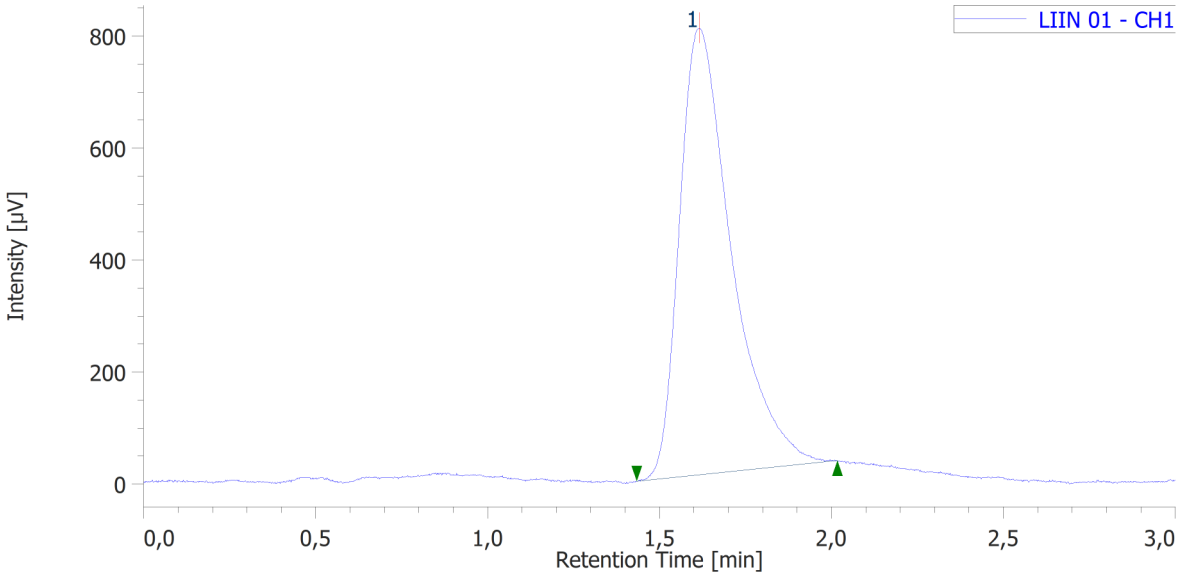

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:24:10
Volume	0.1 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.615	8395	797	100.000	100.000	N/A	602	N/A	1.622		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

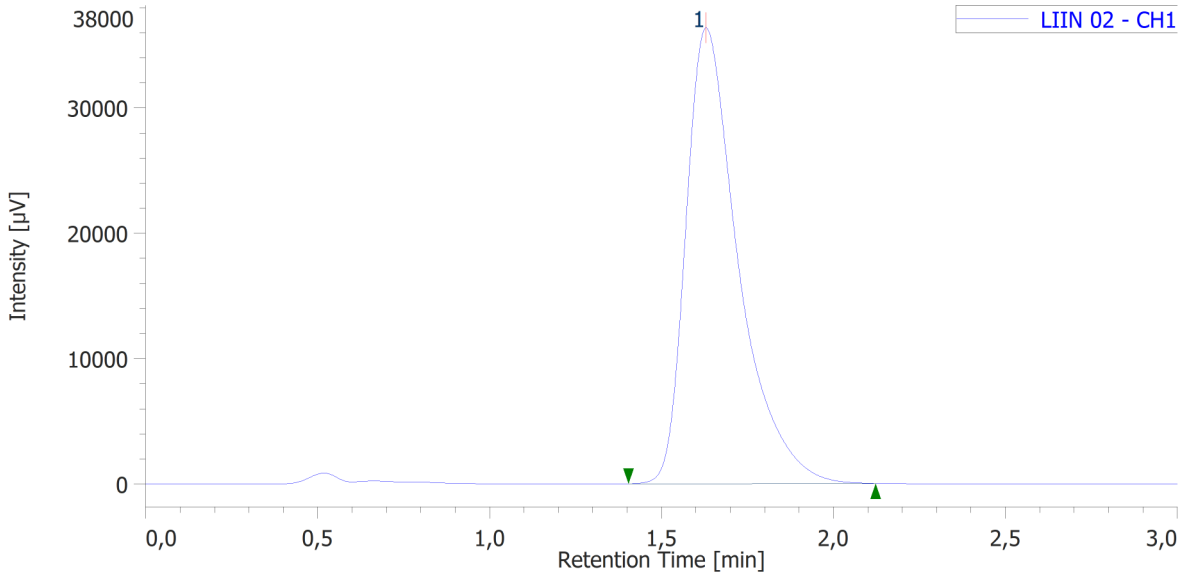

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:36
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:27:22
Volume	5.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.628	385591	36323	100.000	100.000	N/A	612	N/A	1.602		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

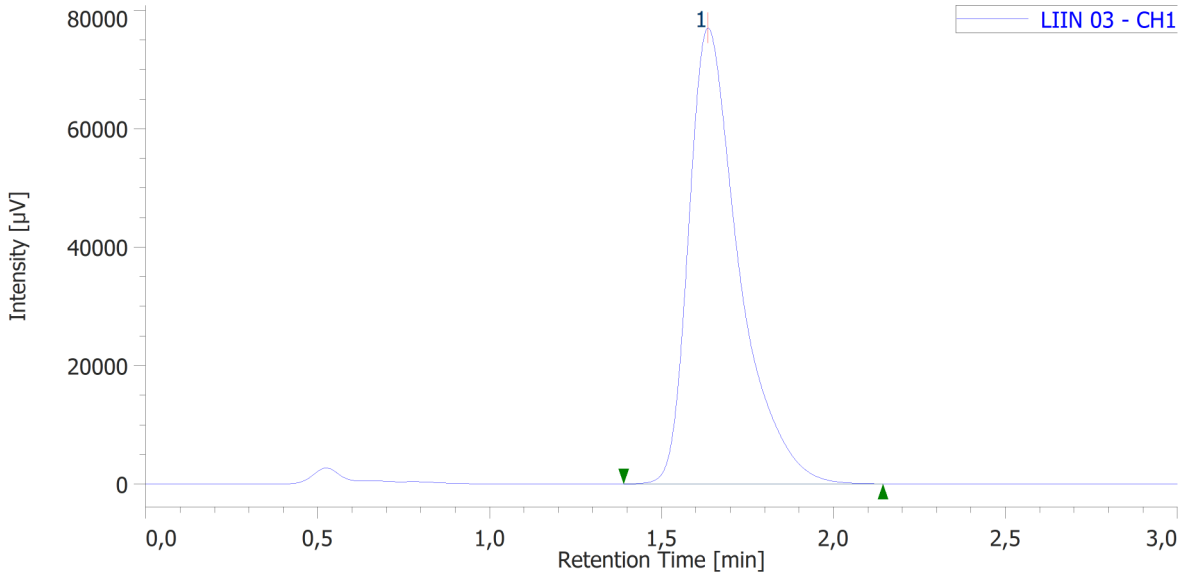

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:36
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:30:34
Volume	10.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,635	782178	76929	100,000	100,000	N/A	686	N/A	1,582		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

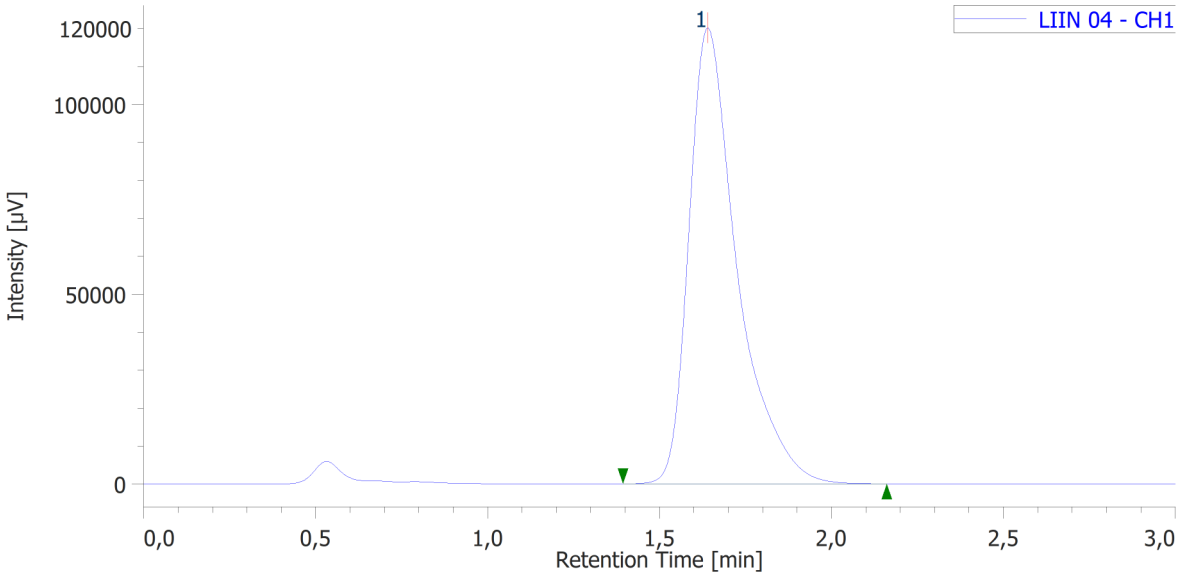

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:36
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:33:47
Volume	15,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,640	1171139	120056	100,000	100,000	N/A	764	N/A	1,575		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

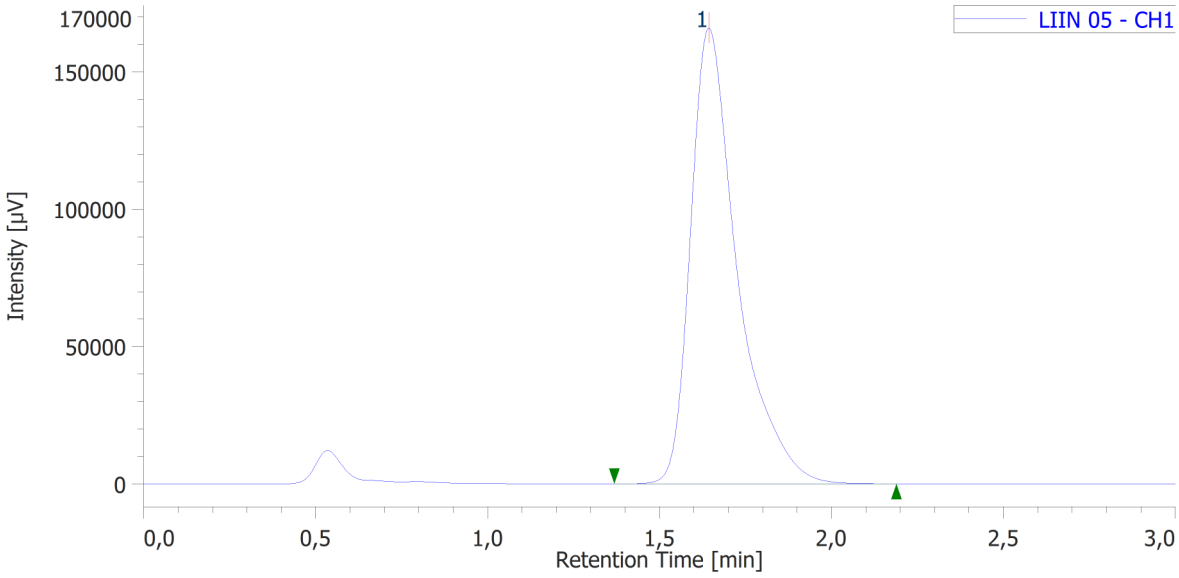

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 09:00:36
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	10/08/2023 19:37:00
Volume	20.0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.643	1566066	165830	100.000	100.000	N/A	829	N/A	1.577		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

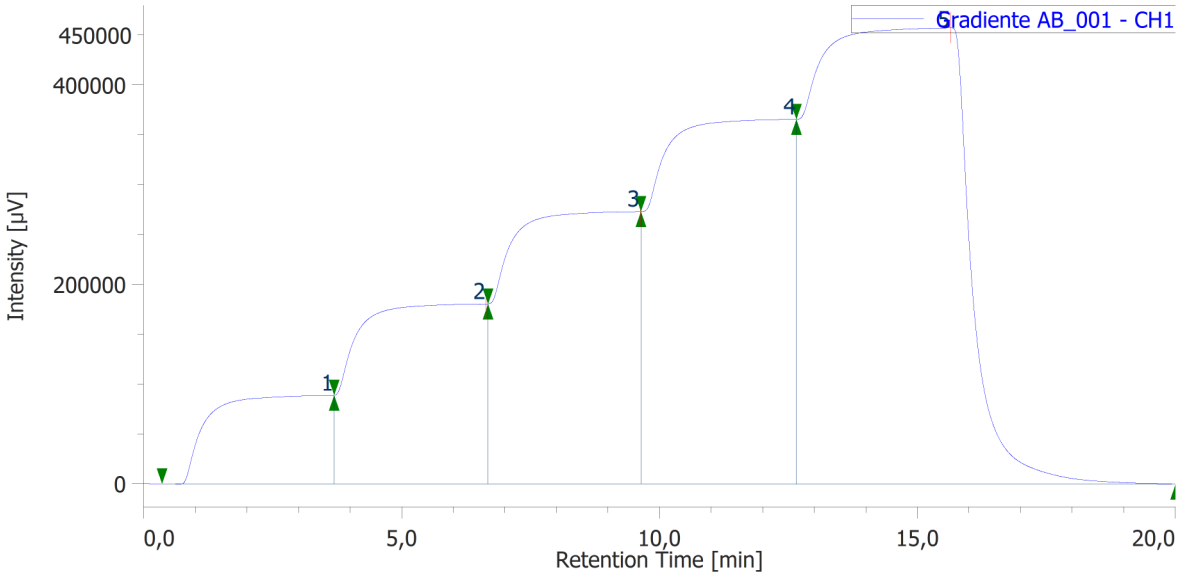

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 10:56:37
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	11/08/2023 09:43:05
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20 %	1	3,692	13526360	88719	5,497	6,501	N/A	N/A	N/A	N/A		N/A
2	40 %	1	6,635	29903141	180317	12,152	13,213	N/A	N/A	N/A	N/A		N/A
3	60 %	1	9,623	46018386	273032	18,701	20,007	N/A	N/A	N/A	N/A		N/A
4	80 %	1	12,650	63448042	365507	25,784	26,783	N/A	N/A	N/A	N/A		N/A
5	100 %	1	15,637	93178399	457102	37,866	33,495	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

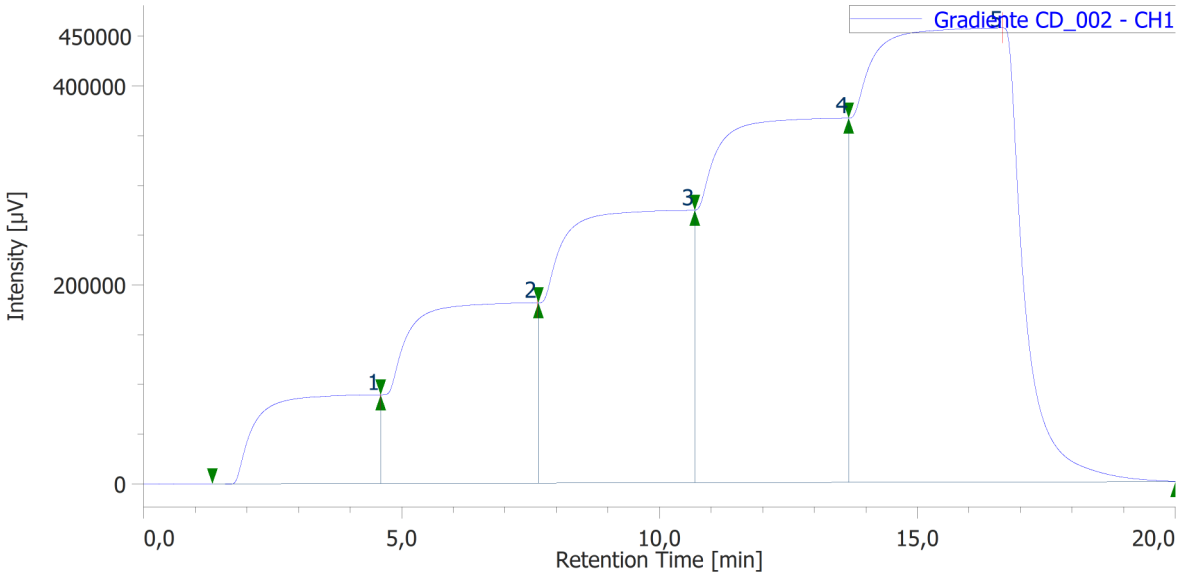

Chromatogram Information	
User Name	QPackSA
Date Modified	11/08/2023 10:56:38
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	11/08/2023 10:04:33
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	20 %	1	4,583	13148571	89051	5,344	6,522	N/A	N/A	N/A	N/A		N/A
2	40 %	1	7,628	30294005	181020	12,312	13,257	N/A	N/A	N/A	N/A		N/A
3	60 %	1	10,680	47200699	273687	19,183	20,044	N/A	N/A	N/A	N/A		N/A
4	80 %	1	13,660	63006920	365690	25,607	26,782	N/A	N/A	N/A	N/A		N/A
5	100 %	1	16,650	92399503	455979	37,553	33,395	N/A	N/A	N/A	N/A		N/A

Creator QPackSA
Reviewer
Approver