

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:10:22
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:09:20
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 200nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

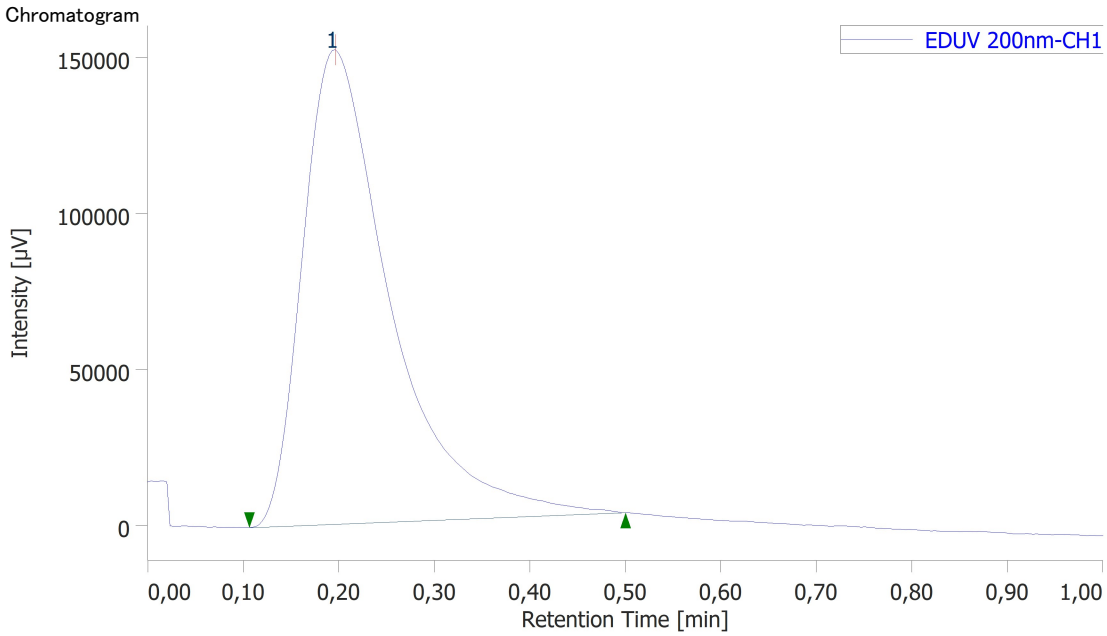

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	972602	151934	100,000	100,000	N/A	26	N/A	1,847	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:12:30
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:11:29
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 201nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

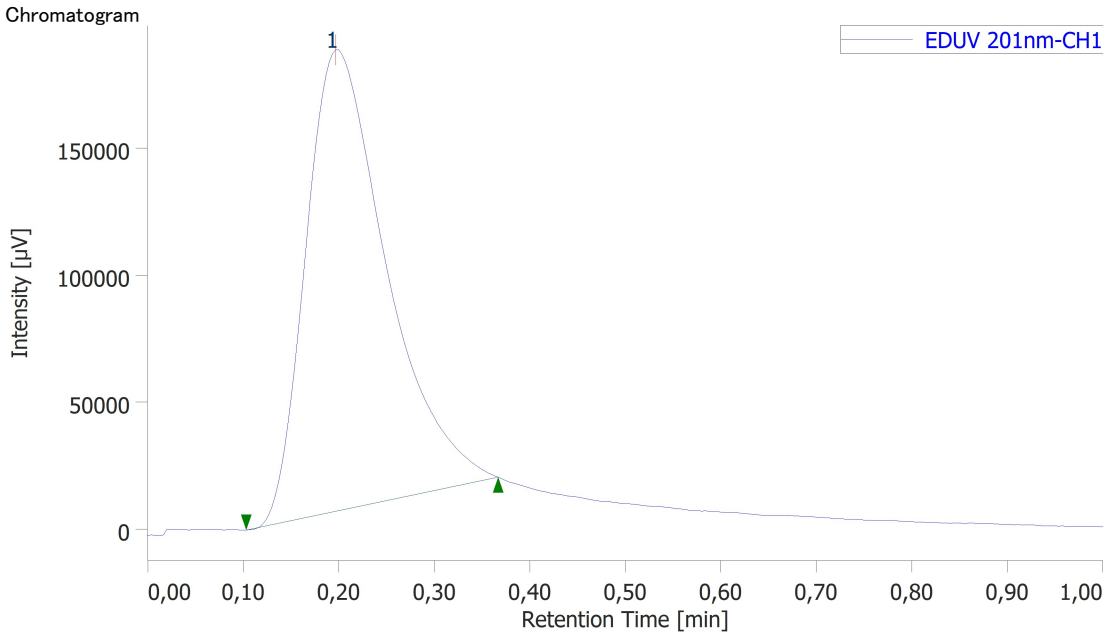

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1065652	181698	100,000	100,000	N/A	27	N/A	1,578	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:14:16
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:13:15
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 202nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

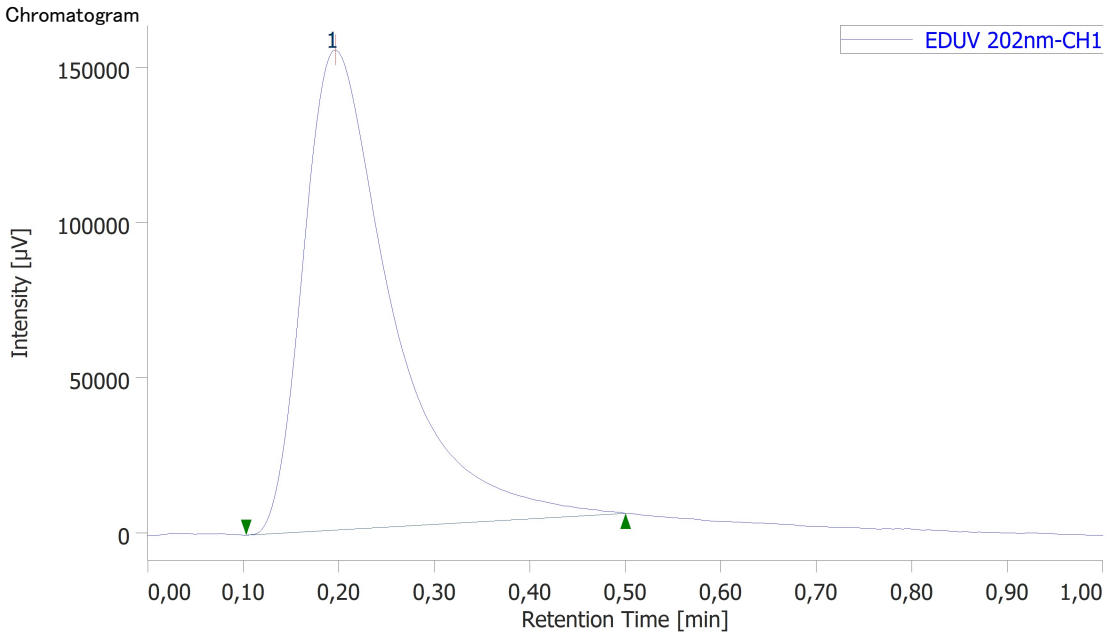

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1000590	154609	100,000	100,000	N/A	26	N/A	1,920	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:16:02
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:15:01
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 203nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

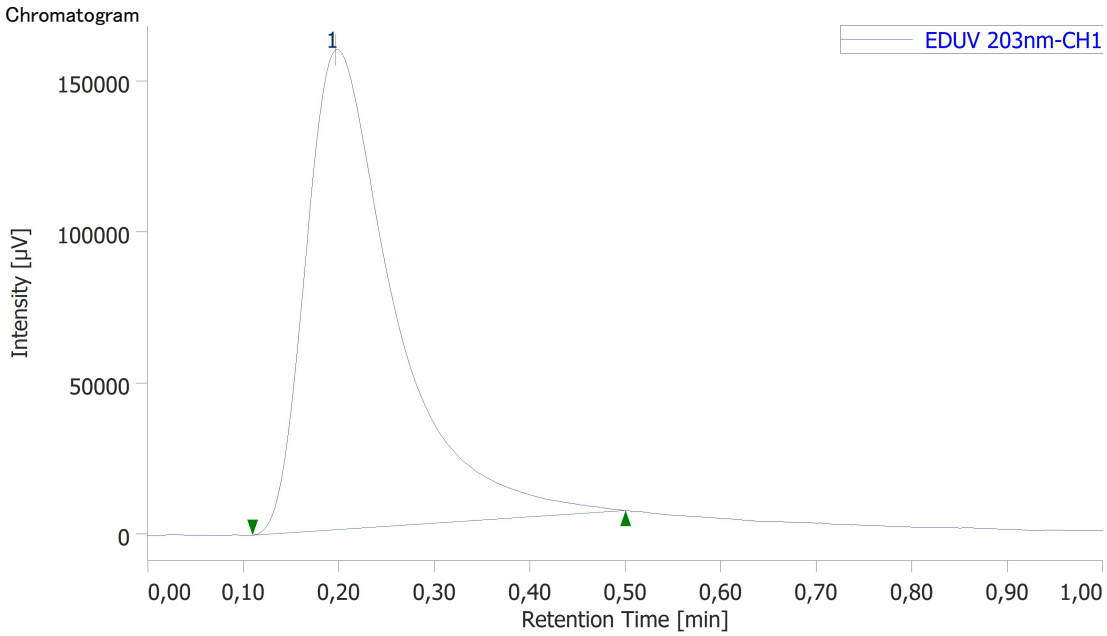

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1030759	158759	100,000	100,000	N/A	26	N/A	2,041	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:16:51
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 204nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

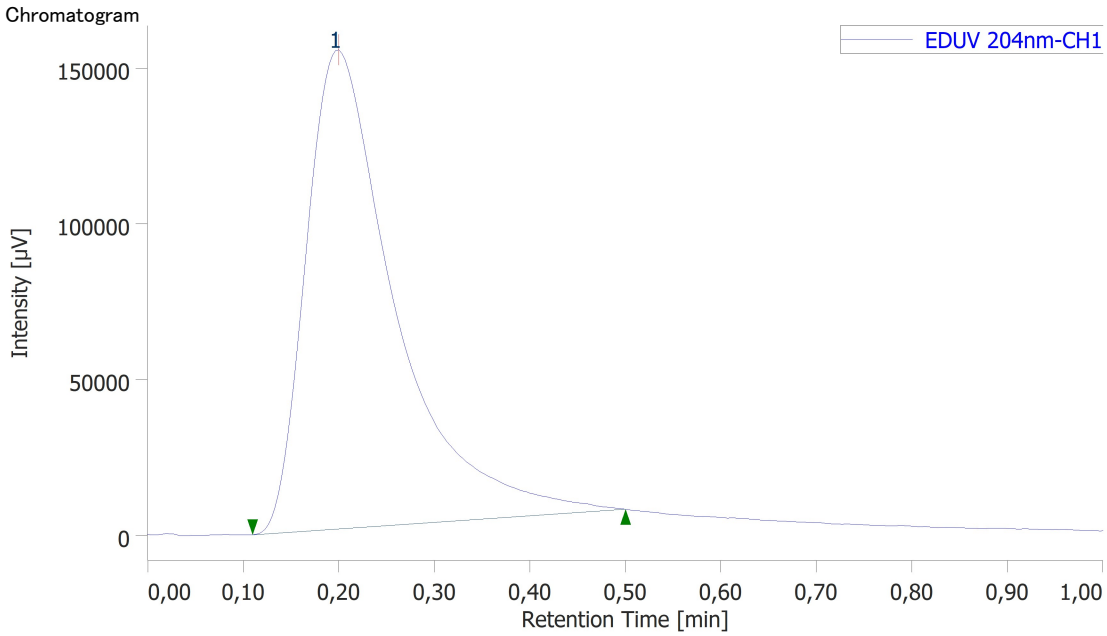

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1003853	153714	100,000	100,000	N/A	26	N/A	1,961	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:18:26
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 205nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

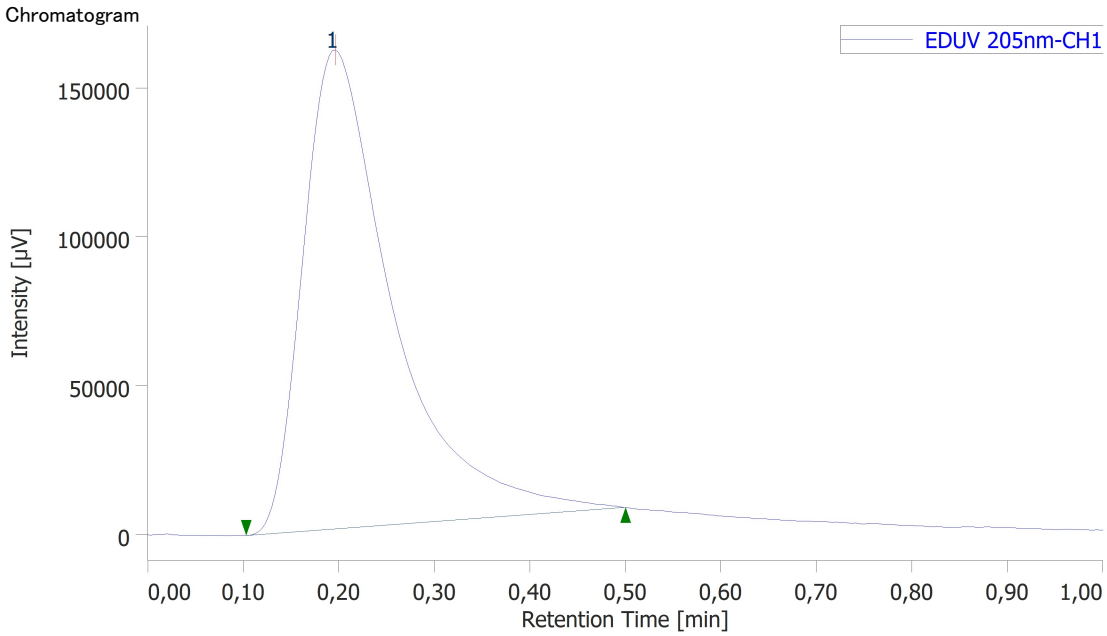

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1054507	160788	100,000	100,000	N/A	25	N/A	1,964	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:20:05
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 206nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

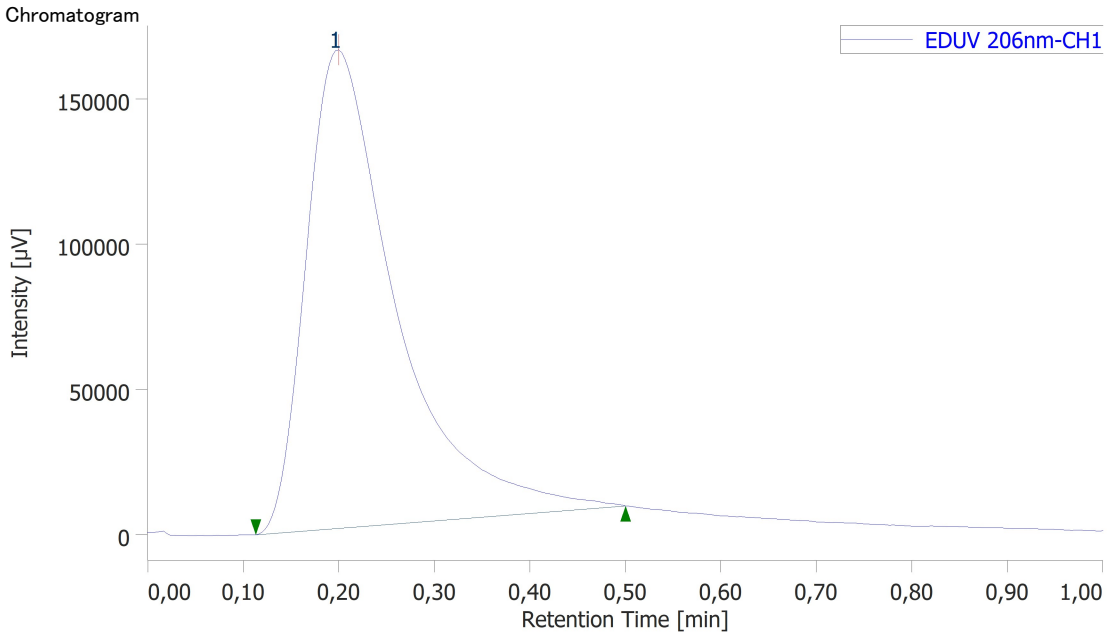

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1082115	164690	100,000	100,000	N/A	26	N/A	2,001	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:21:55
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 207nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

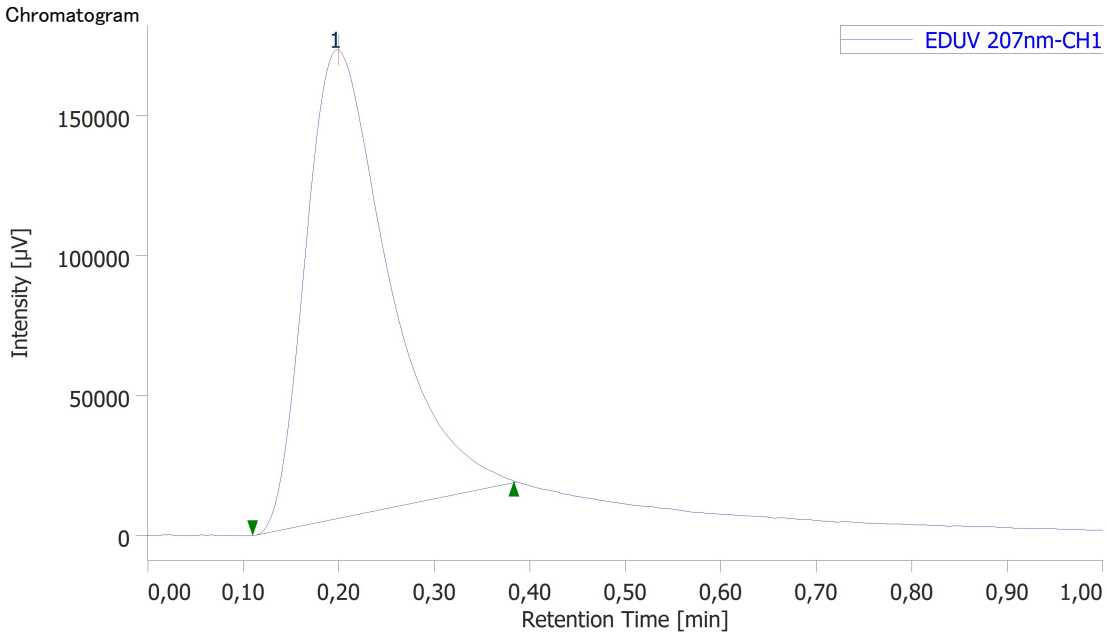

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1011750	167294	100,000	100,000	N/A	27	N/A	1,600	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:23:33
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 208nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

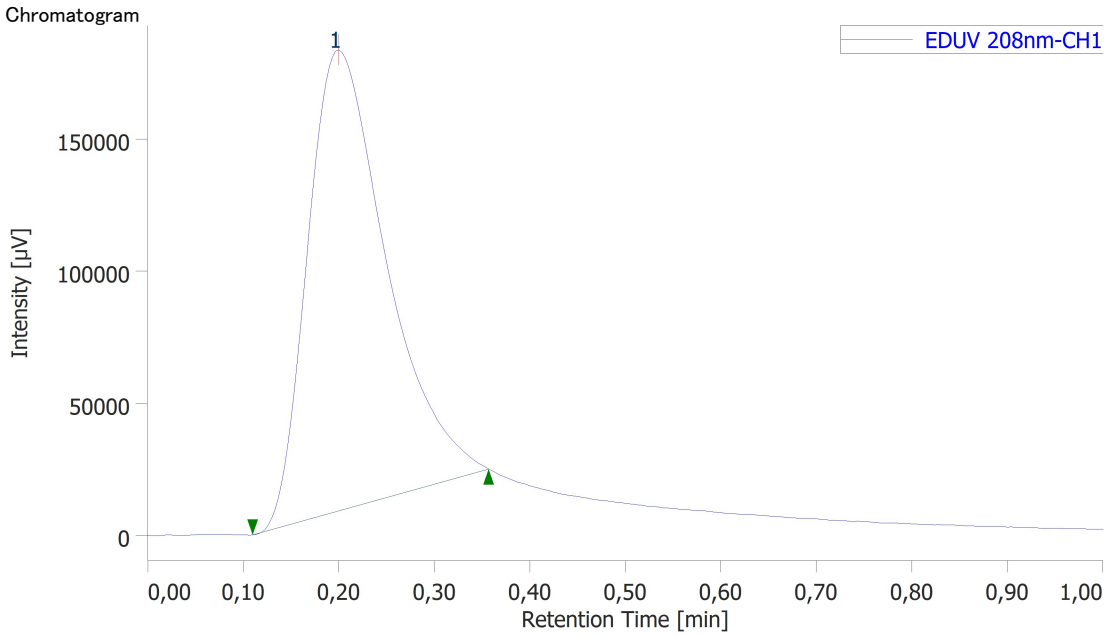

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1002462	174552	100,000	100,000	N/A	29	N/A	1,509	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:25:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 209nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

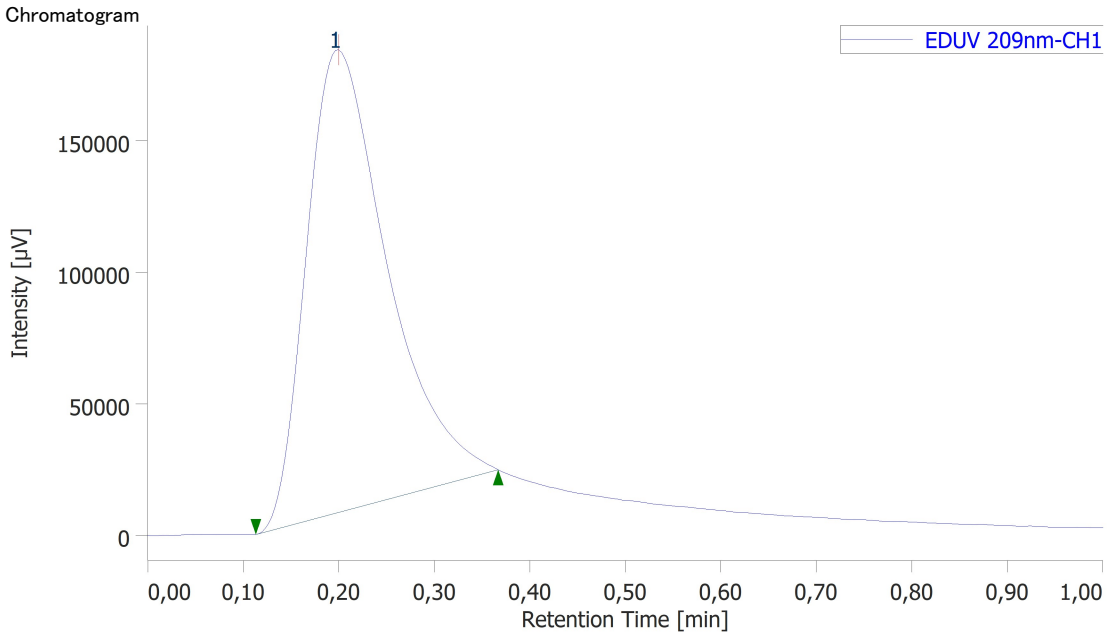


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1033255	175777	100,000	100,000	N/A	28	N/A	1,541	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:07:00
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:27:09
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 210nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	


Chromatogram

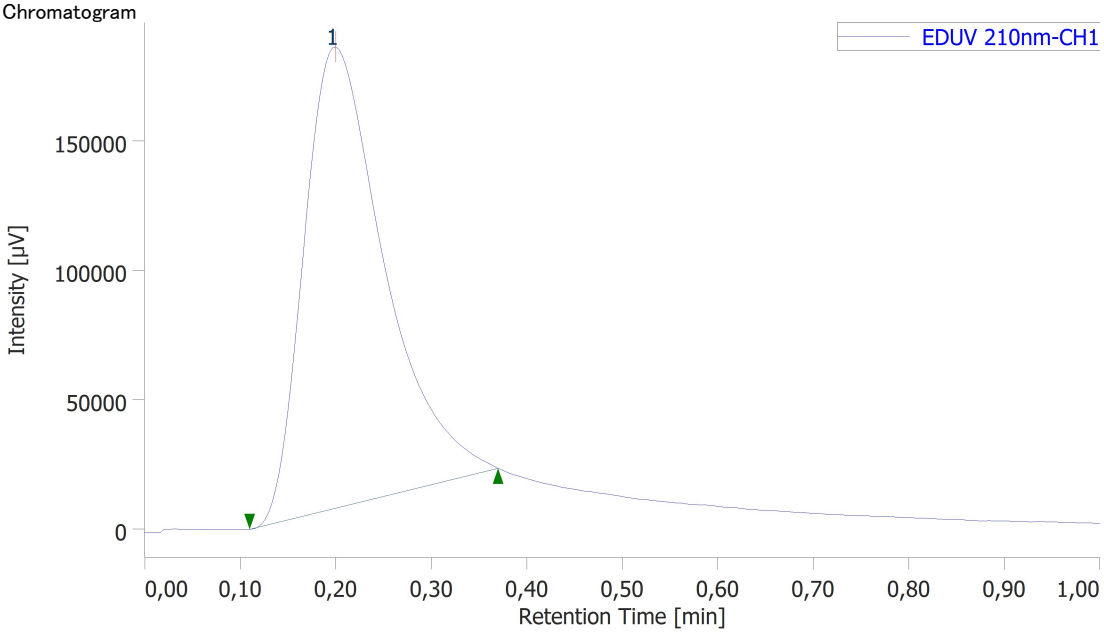

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1044848	178334	100,000	100,000	N/A	28	N/A	1,560	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:31:10
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:30:09
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 240nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

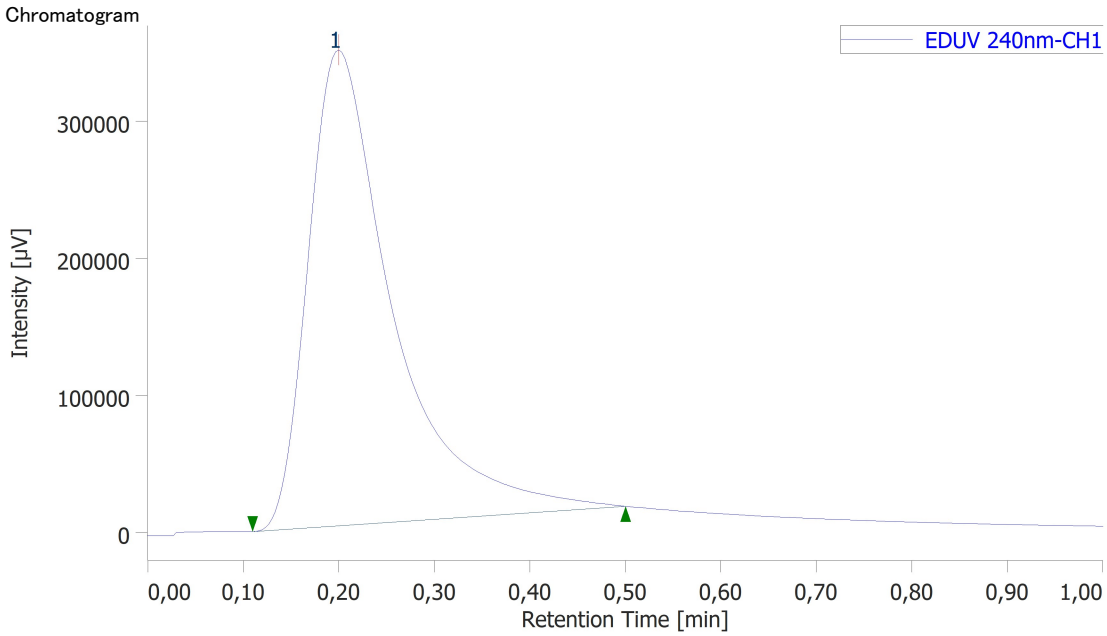

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	2139532	347061	100,000	100,000	N/A	30	N/A	1,980	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:33:12
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:32:11
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 241nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

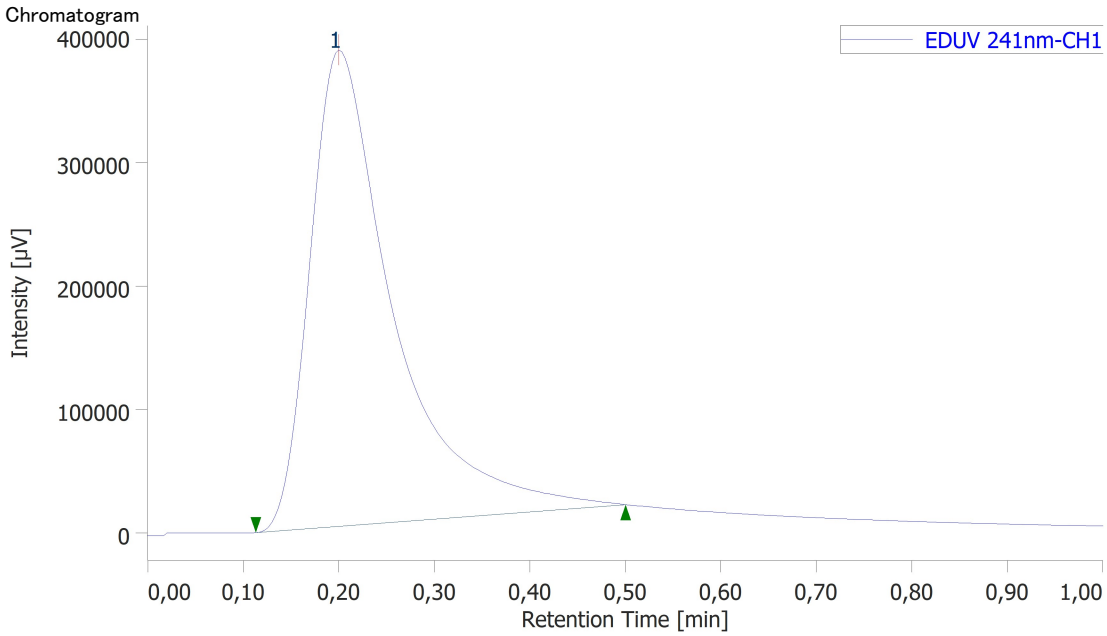


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	2348706	386019	100,000	100,000	N/A	32	N/A	2,041	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:35:02
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:34:02
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 242nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	


Chromatogram

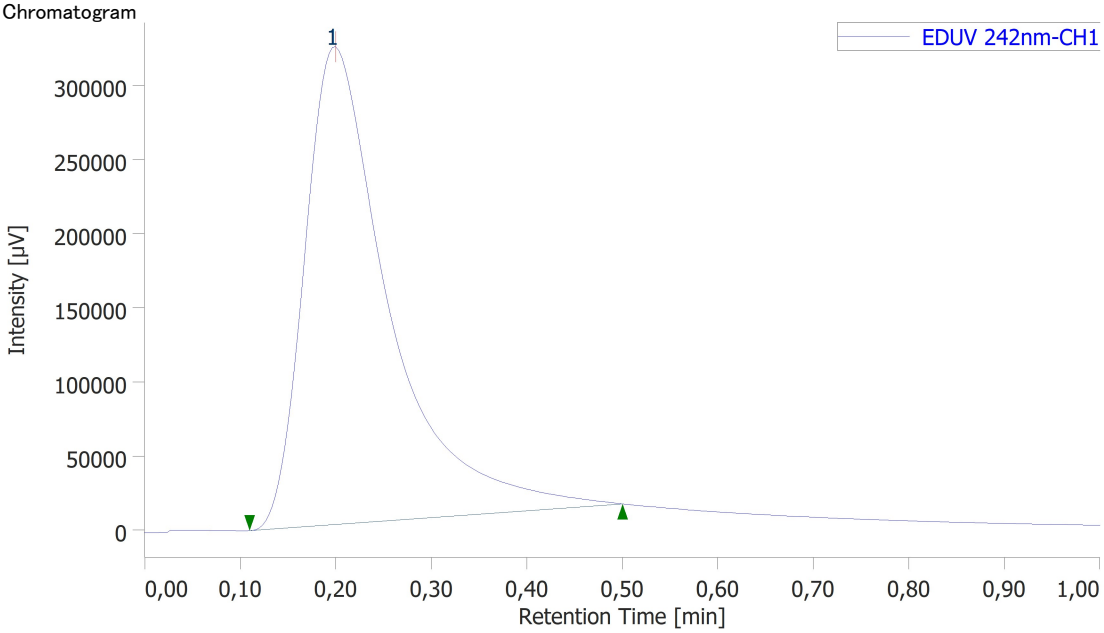

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1996084	322172	100,000	100,000	N/A	30	N/A	1,958	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:37:24
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:36:23
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 243nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

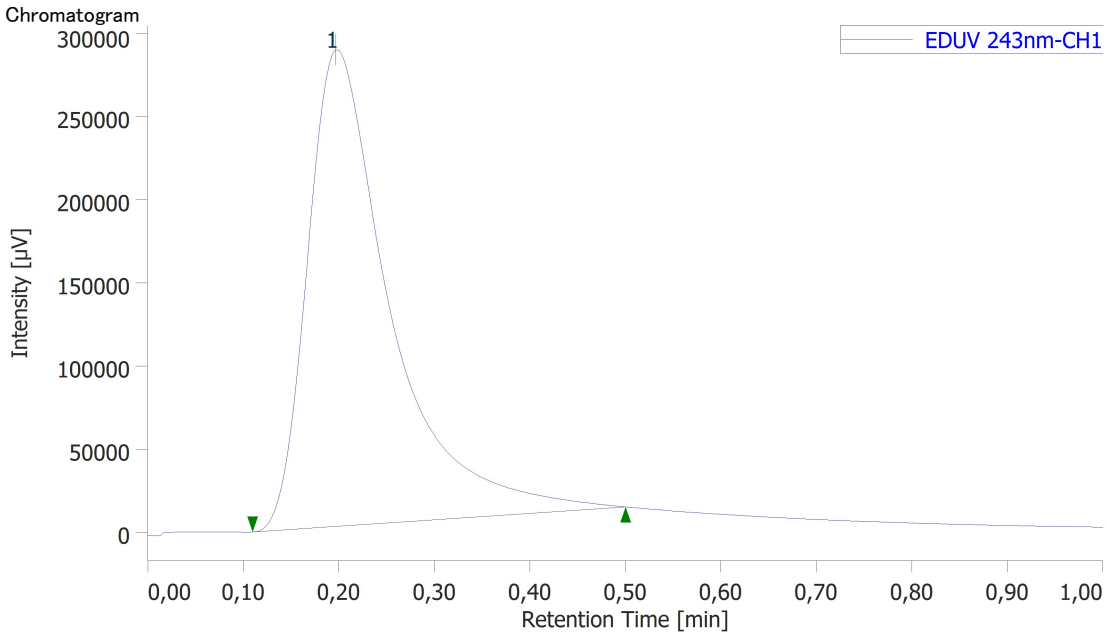

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1738764	286654	100,000	100,000	N/A	30	N/A	2,026	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:39:12
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:38:10
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 244nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

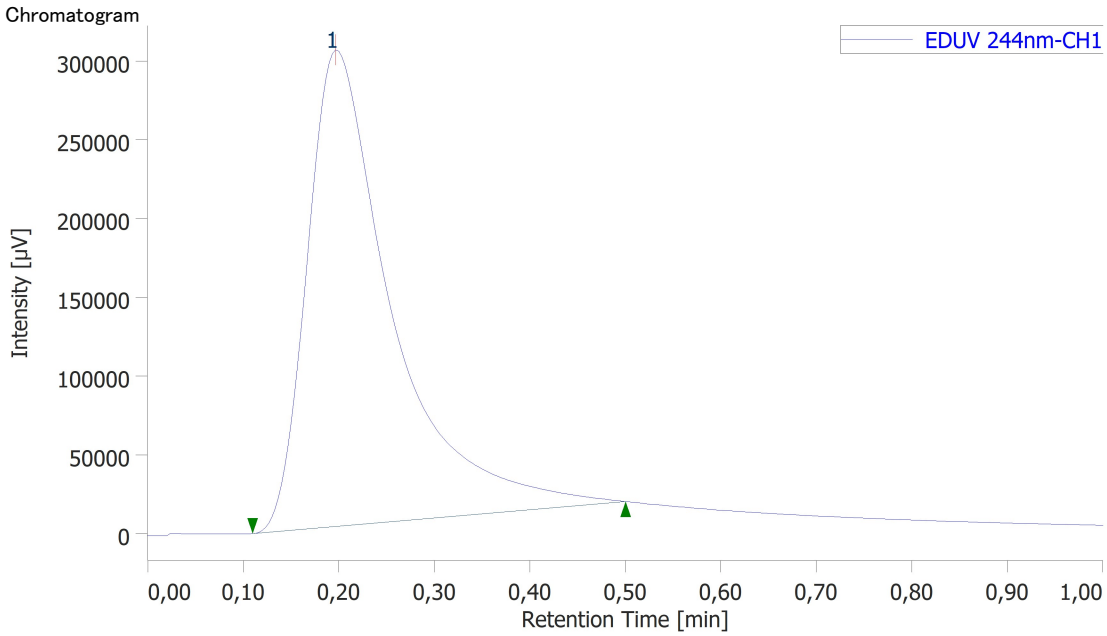

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1879324	302490	100,000	100,000	N/A	30	N/A	2,104	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:40:46
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:39:45
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 245nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

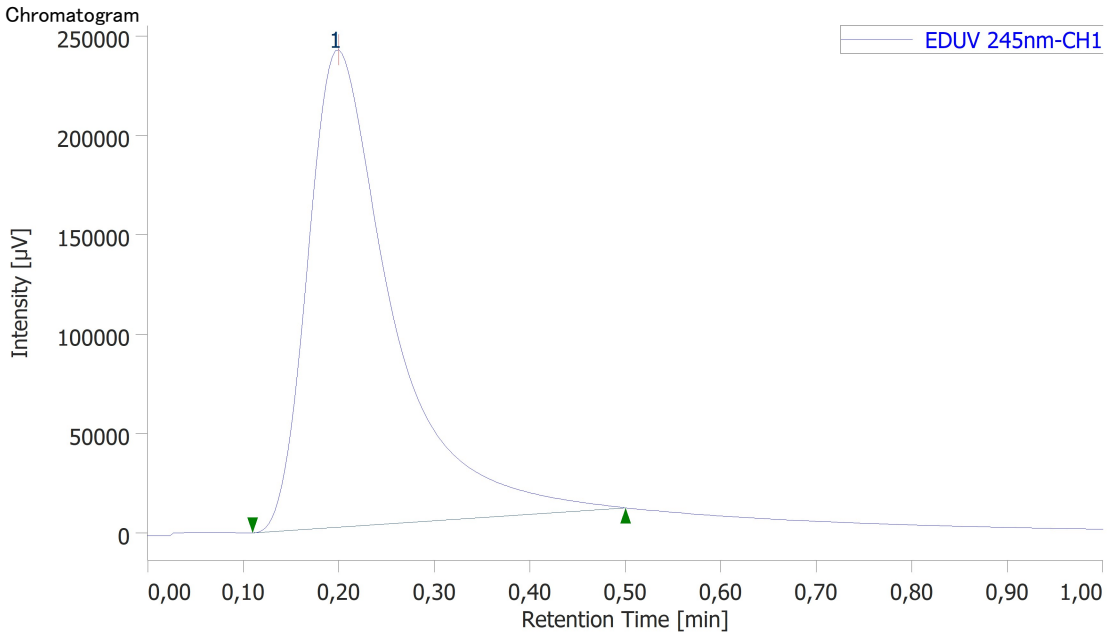

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1484796	240129	100,000	100,000	N/A	30	N/A	1,965	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:42:28
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:41:28
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 246nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

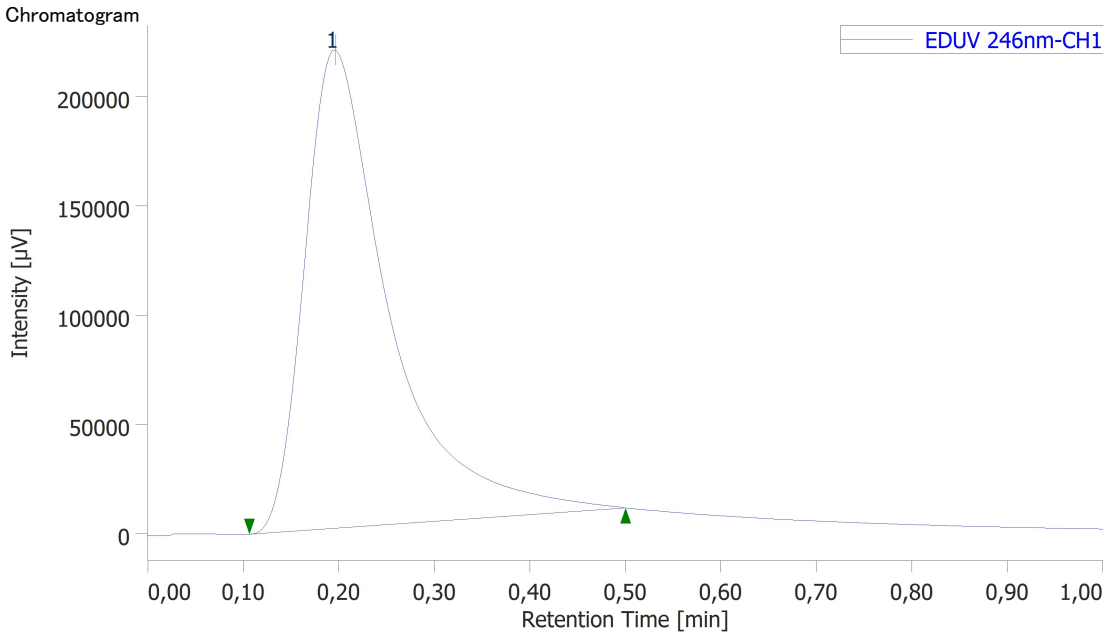

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1358061	218884	100,000	100,000	N/A	29	N/A	1,982	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:44:54
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:43:54
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 247nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

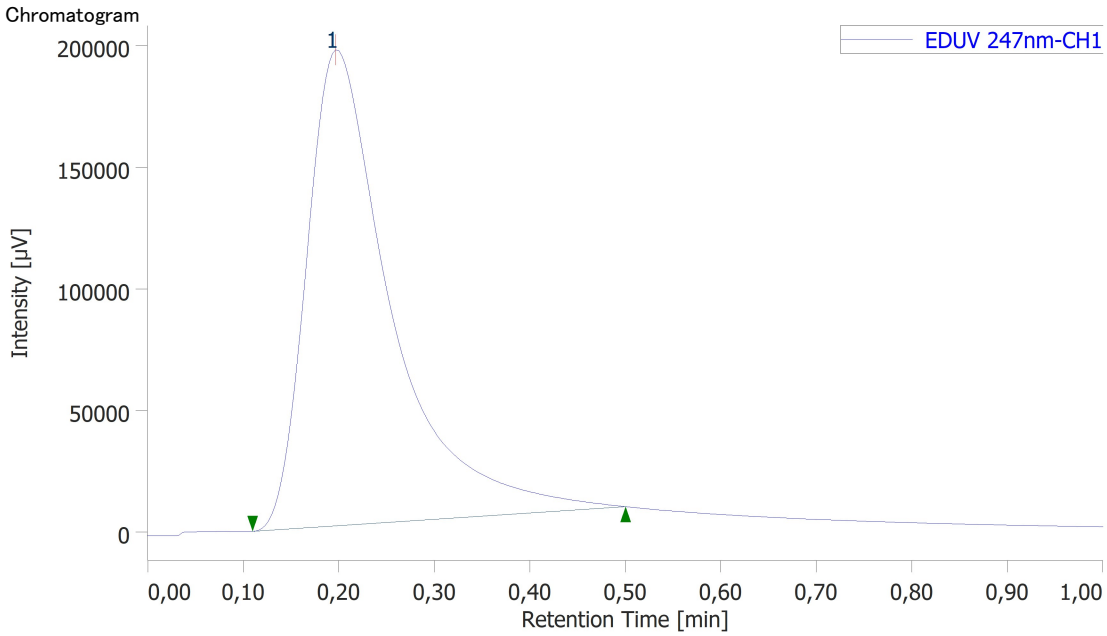

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1212858	195711	100,000	100,000	N/A	29	N/A	2,035	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:47:08
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:46:06
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 248nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

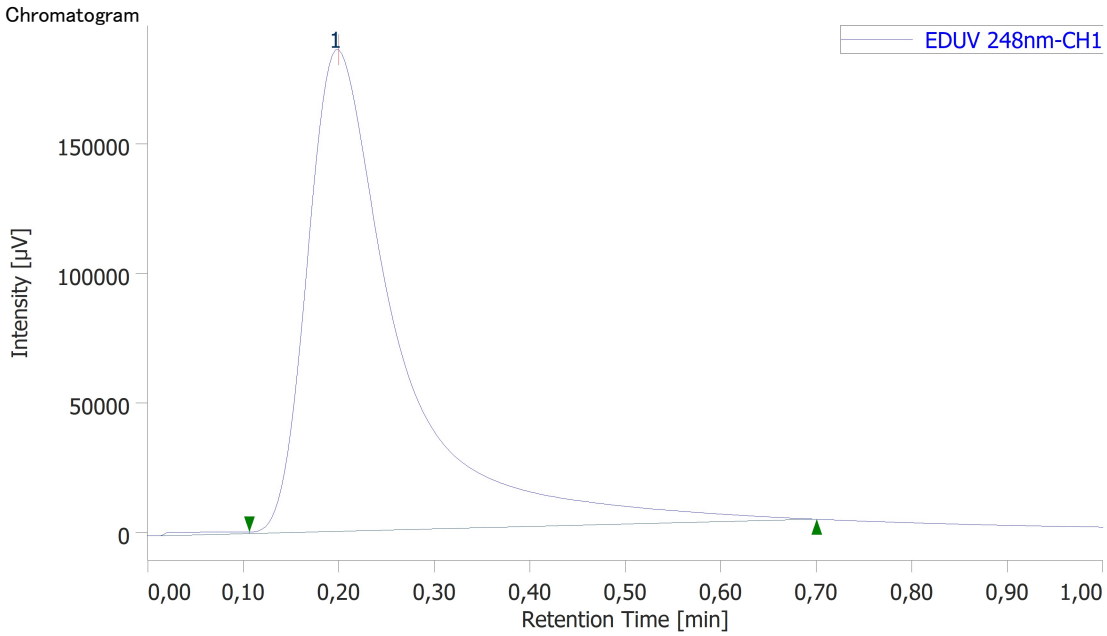

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	1251744	185789	100,000	100,000	N/A	30	N/A	2,417	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:48:48
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:47:47
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 249nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

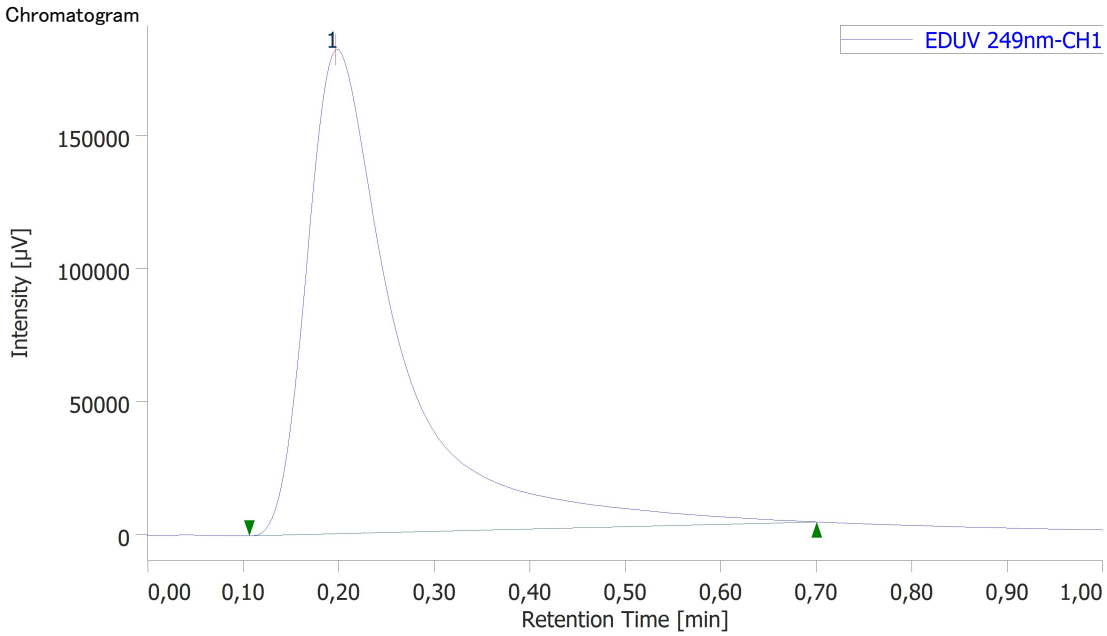

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1236128	181871	100,000	100,000	N/A	29	N/A	2,541	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:52:48
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:51:47
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVa
Control Method	EDUV 250nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

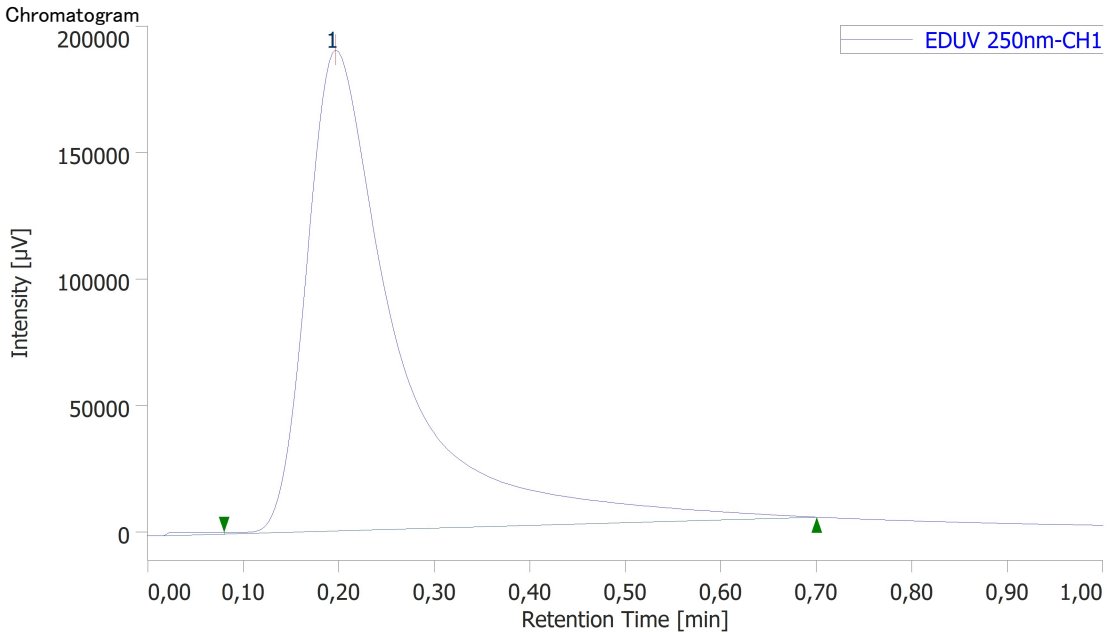


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1272942	190176	100,000	100,000	N/A	30	N/A	2,564	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:34:27
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:54:16
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 268nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	


Chromatogram

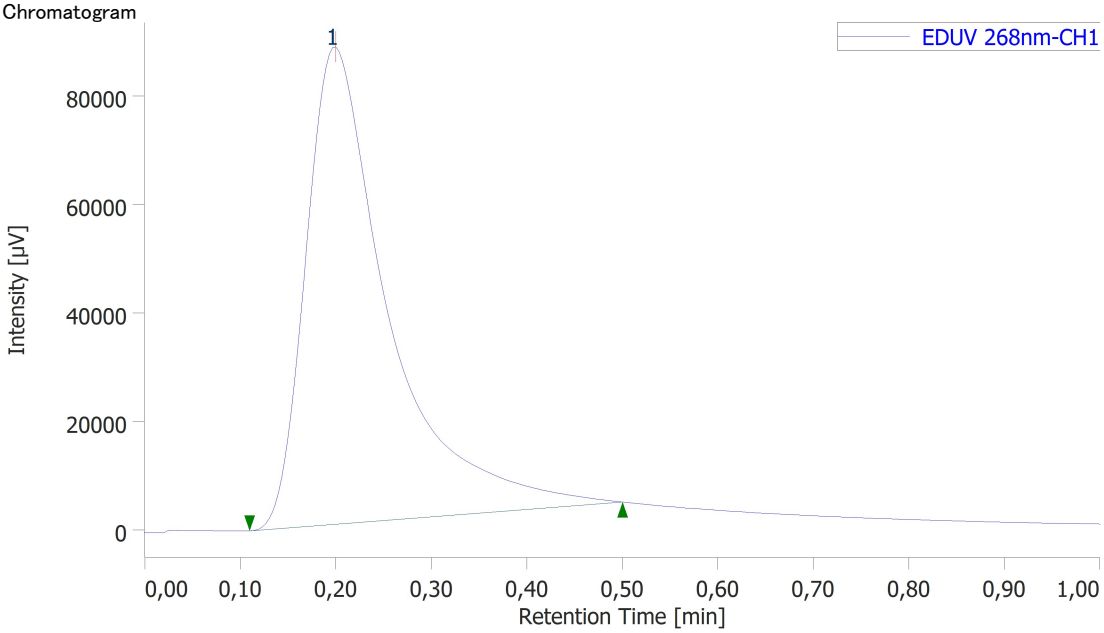

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	532294	87994	100,000	100,000	N/A	33	N/A	2,054	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 10:59:30
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 10:58:29
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 269nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

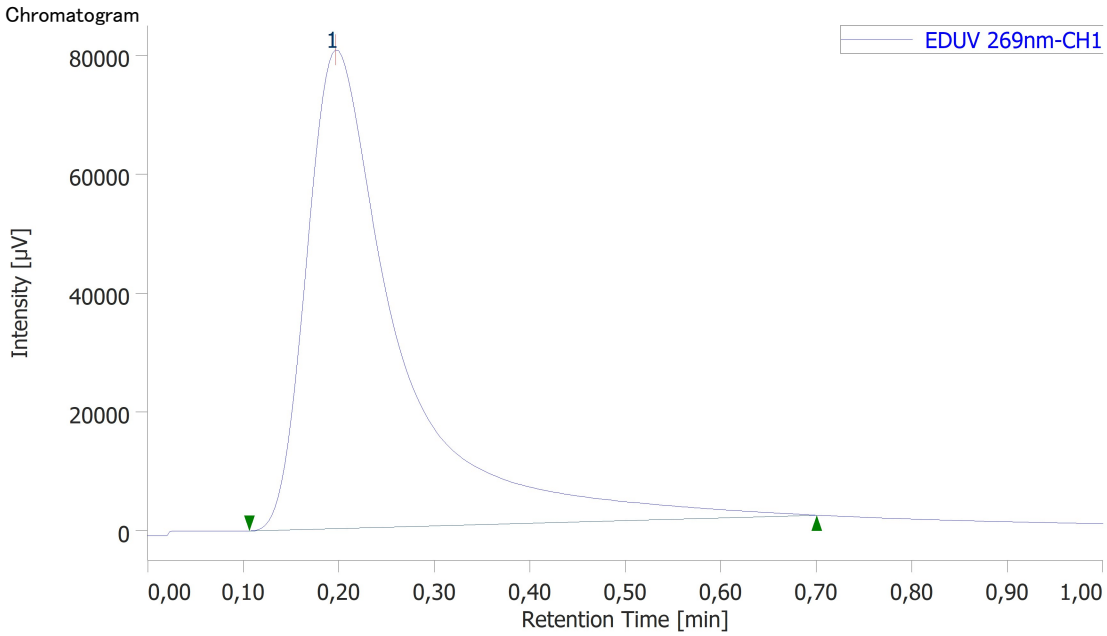

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	545473	80574	100,000	100,000	N/A	30	N/A	2,610	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:01:24
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:00:24
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 270nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

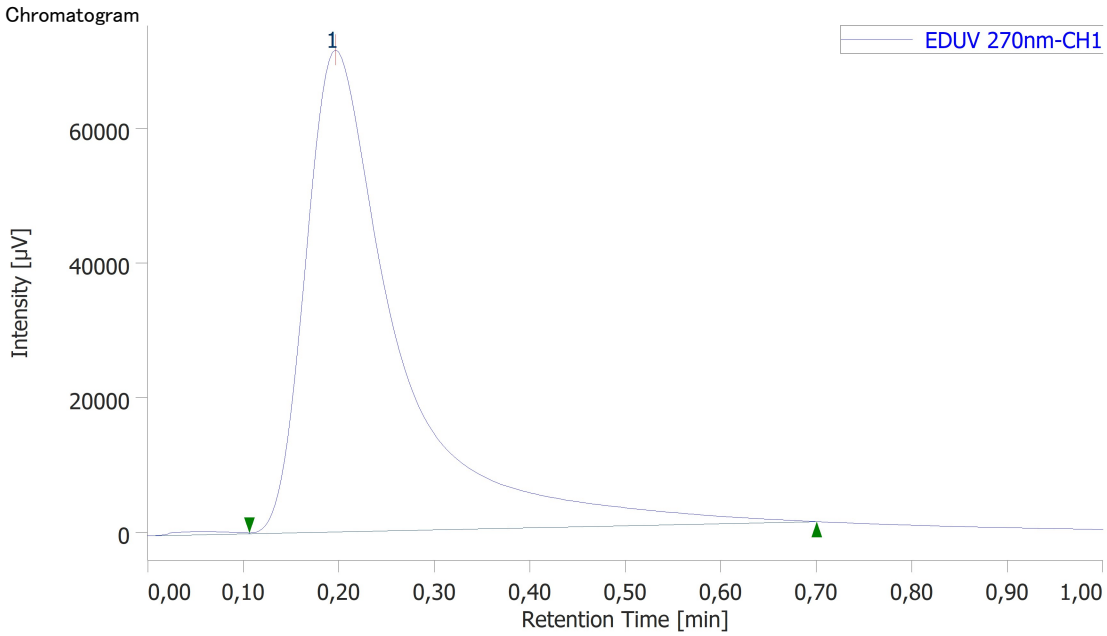

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	483690	71551	100,000	100,000	N/A	29	N/A	2,493	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:02:58
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:01:58
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 271nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

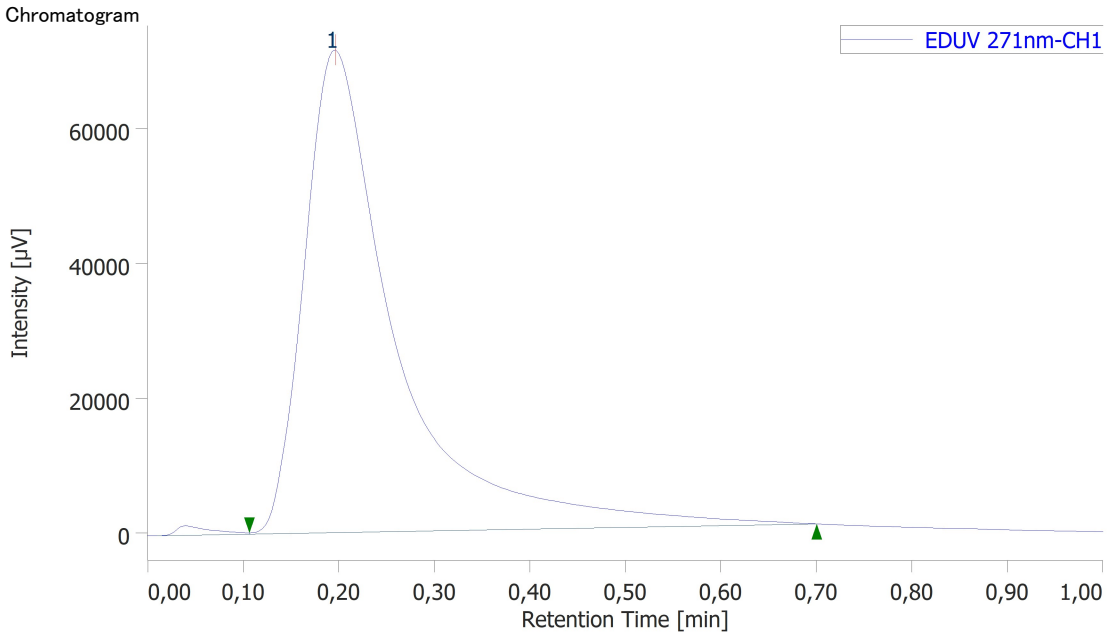

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	479672	71606	100,000	100,000	N/A	29	N/A	2,366	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:04:44
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:03:42
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 272nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

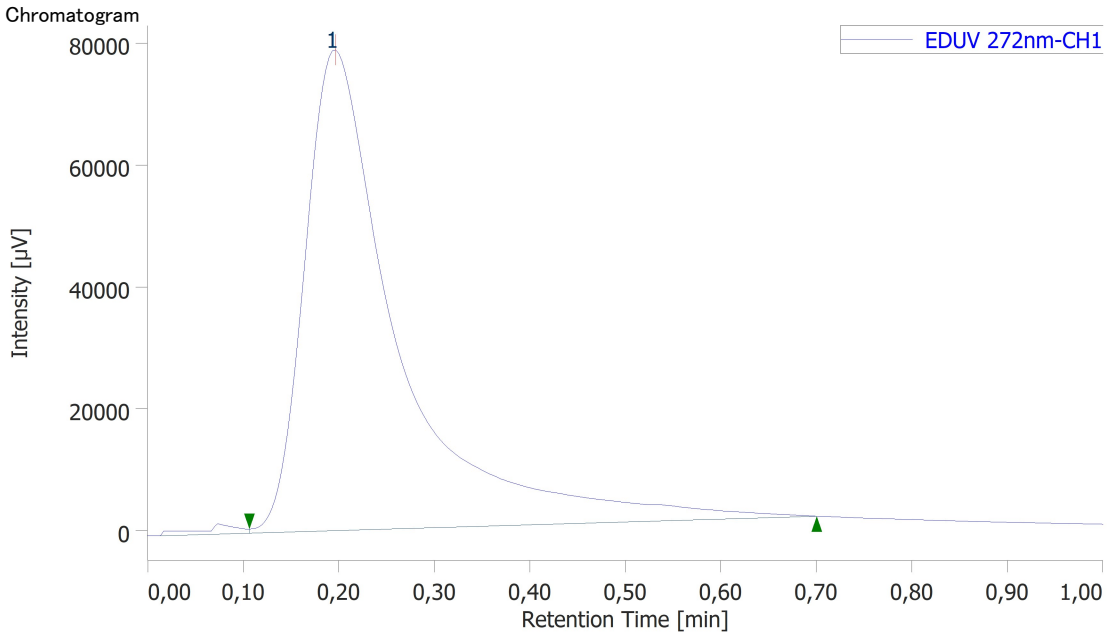

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	540454	78890	100,000	100,000	N/A	29	N/A	2,528	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:06:50
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:05:50
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 273nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

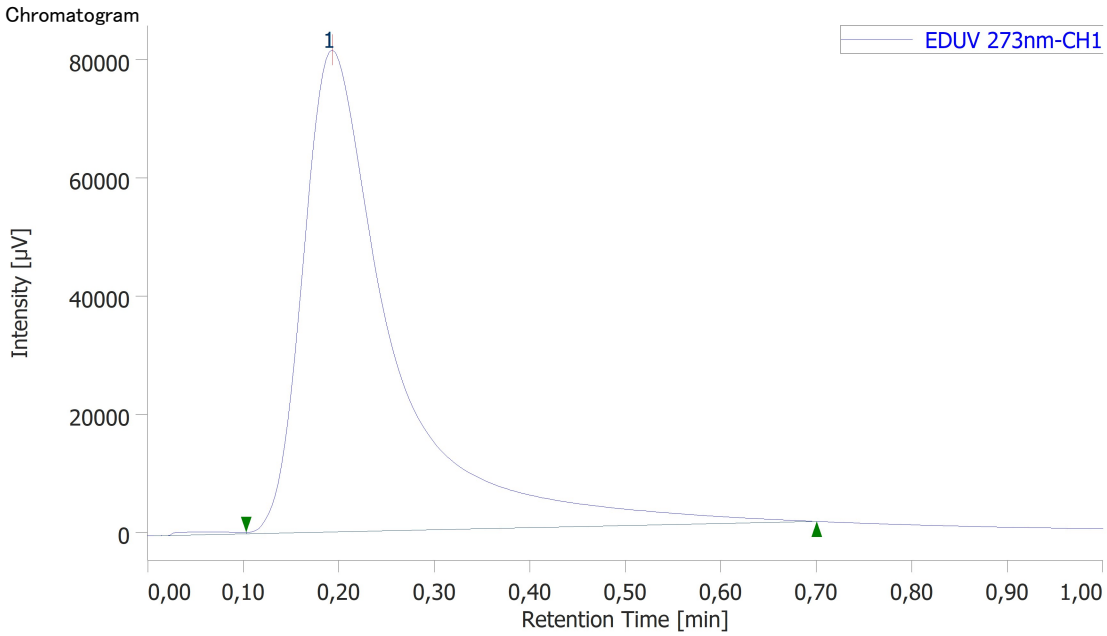

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,193	535846	81560	100,000	100,000	N/A	30	N/A	2,432	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:08:40
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:07:40
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 274nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

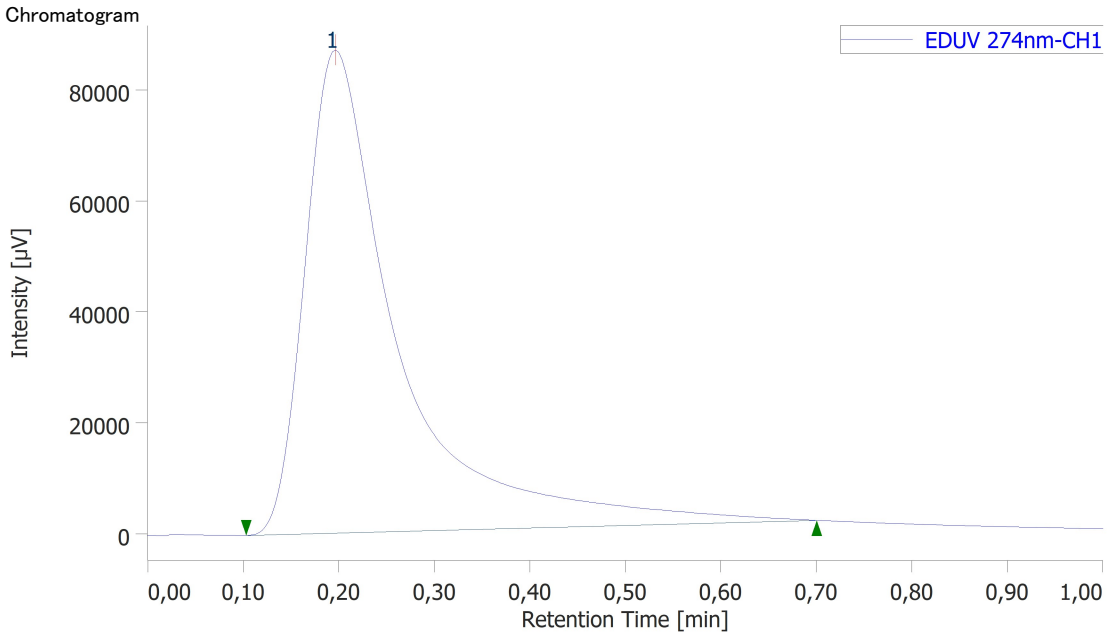


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	591567	87029	100,000	100,000	N/A	29	N/A	2,540	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:11:12
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:10:10
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 275nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	


Chromatogram

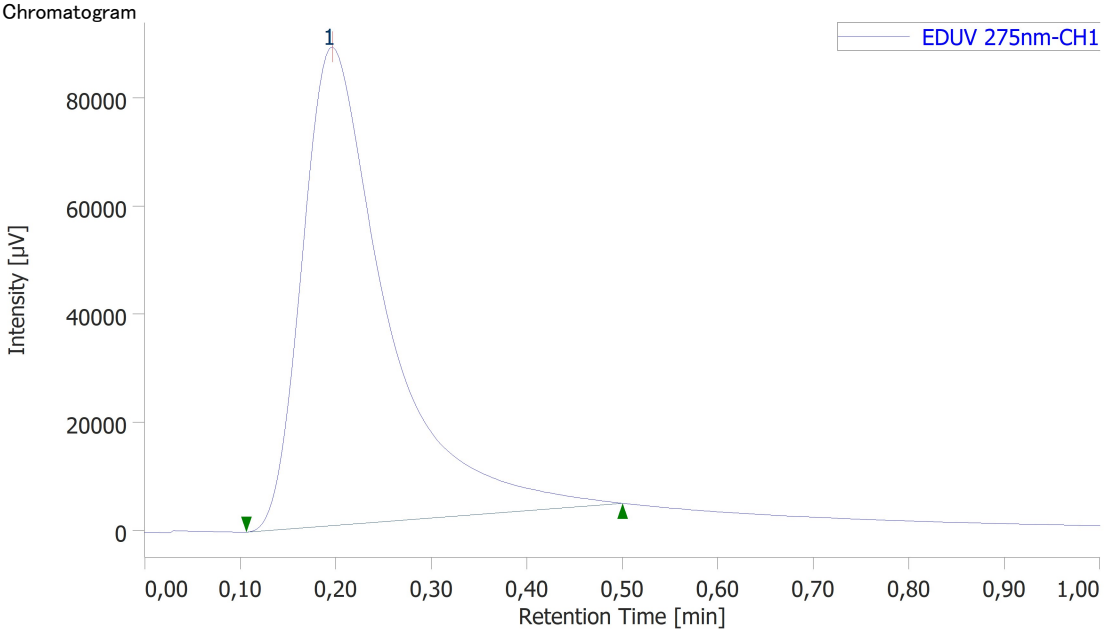

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	547044	88559	100,000	100,000	N/A	30	N/A	2,021	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:12:58
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:11:56
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 276nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

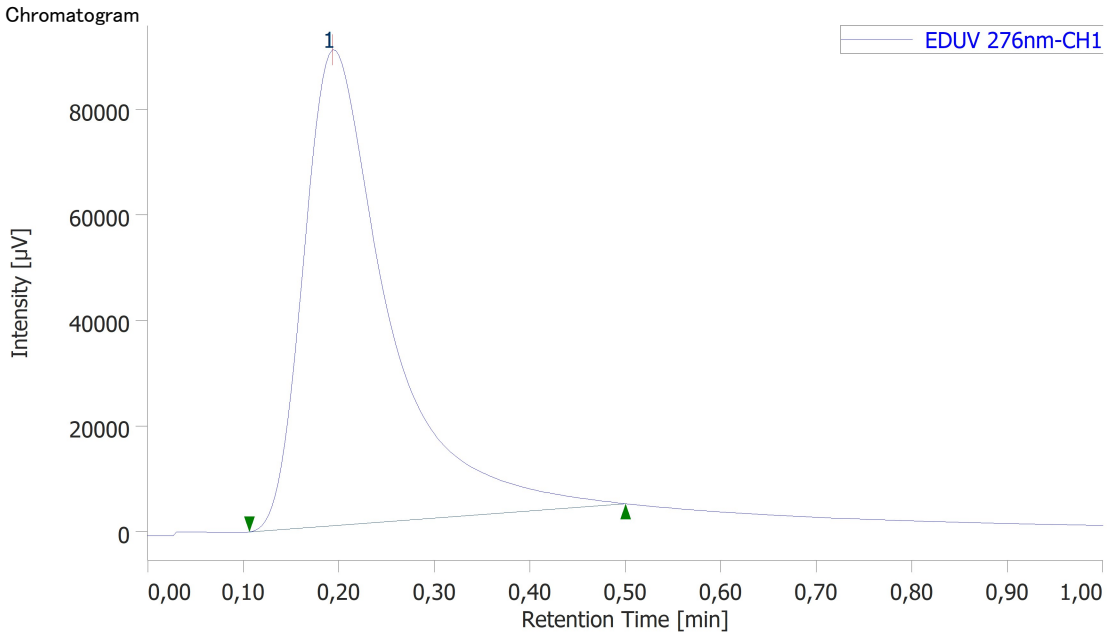

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,193	559468	90089	100,000	100,000	N/A	29	N/A	2,089	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:15:02
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:14:01
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 277nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

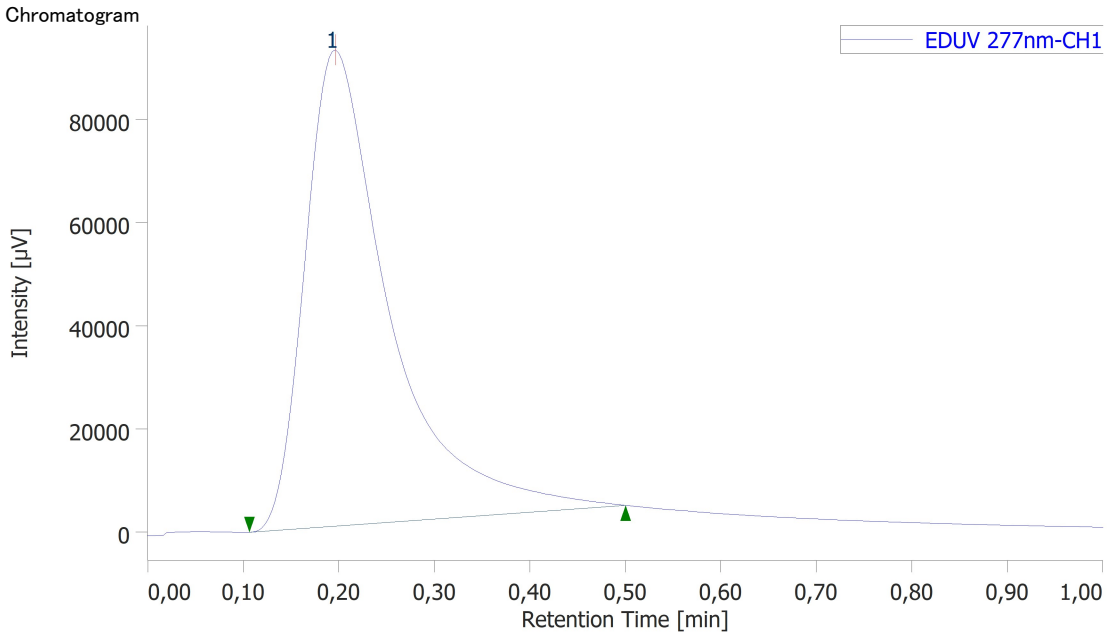


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	571248	92335	100,000	100,000	N/A	30	N/A	2,005	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 11:16:40
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 11:15:40
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUVb
Control Method	EDUV 278nm
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

Chromatogram

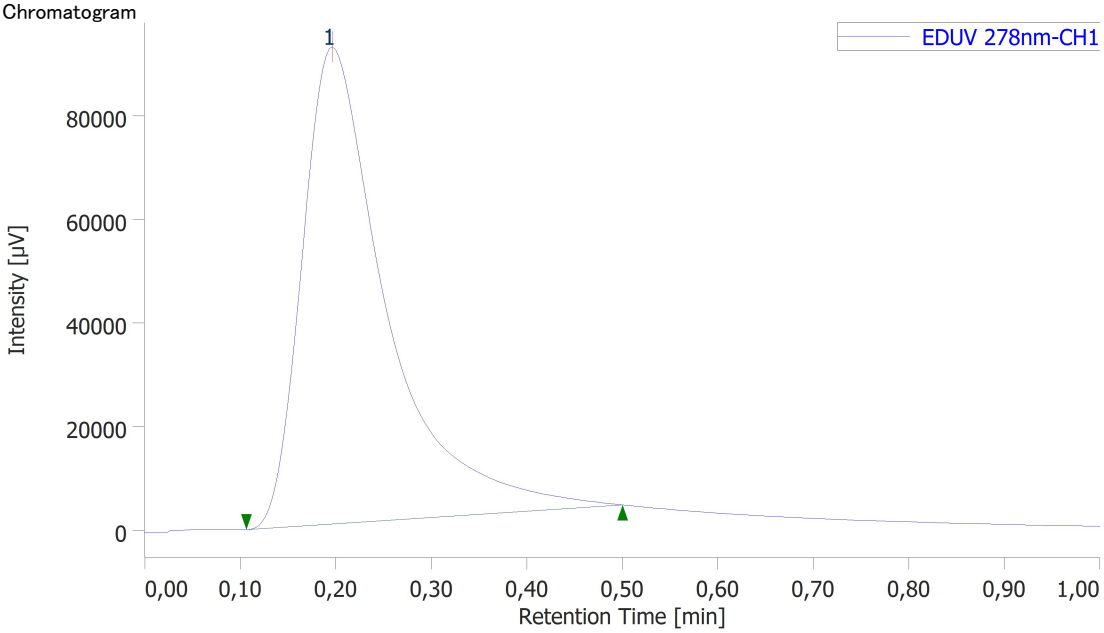


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	568722	92092	100,000	100,000	N/A	29	N/A	1,992	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 13:32:19
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:17:18
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	15,0 [min]
Acquisition Sequence	
Control Method	Ruído
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

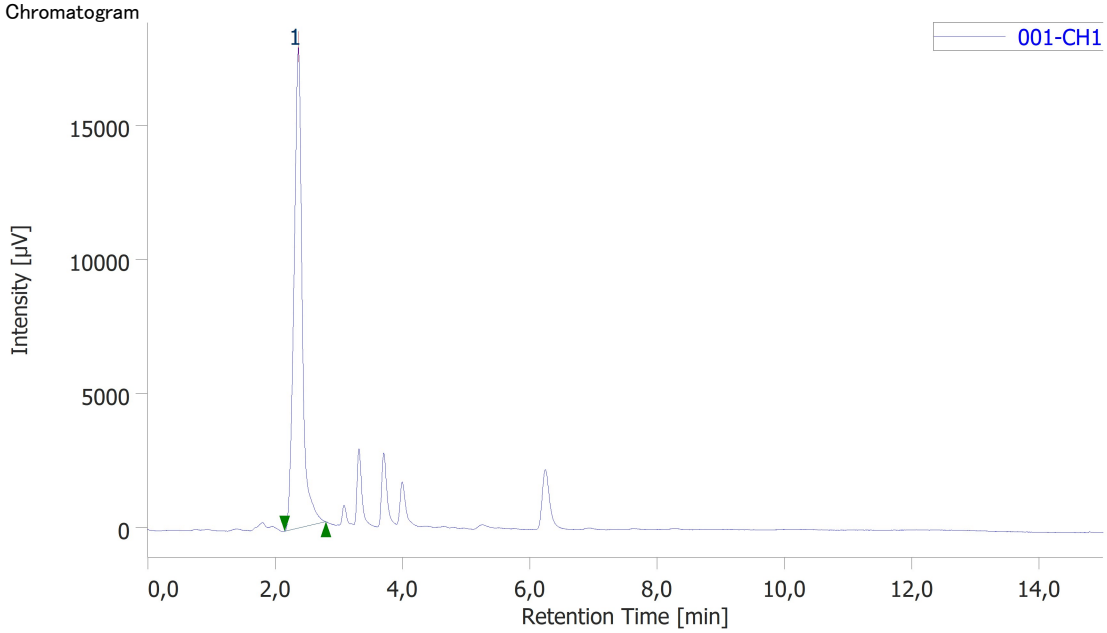

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,367	160169	17936	100,000	100,000	N/A	1702	N/A	1,168	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 13:37:23
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:33:53
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

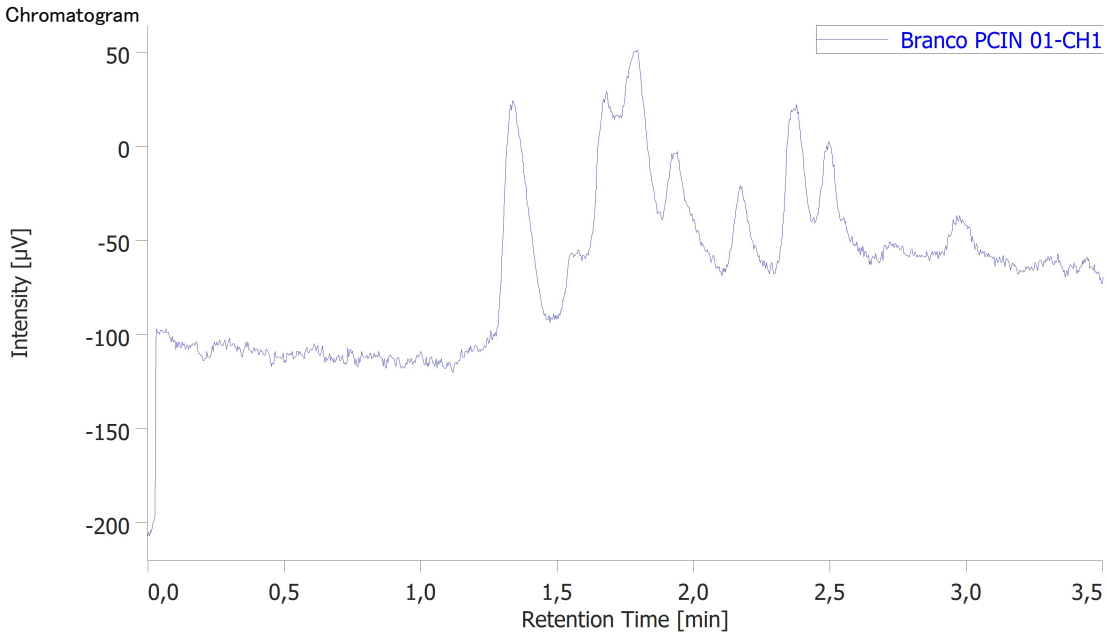

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 13:41:55
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:38:25
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

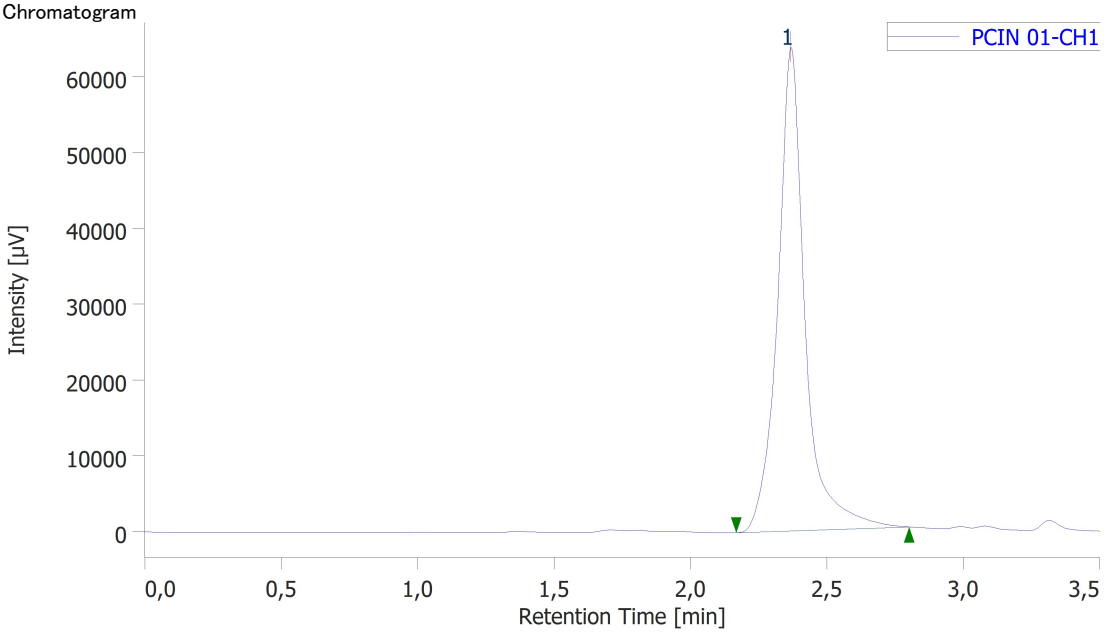


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,367	443129	63864	100,000	100,000	N/A	3664	N/A	1,191	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 13:46:05
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:42:35
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

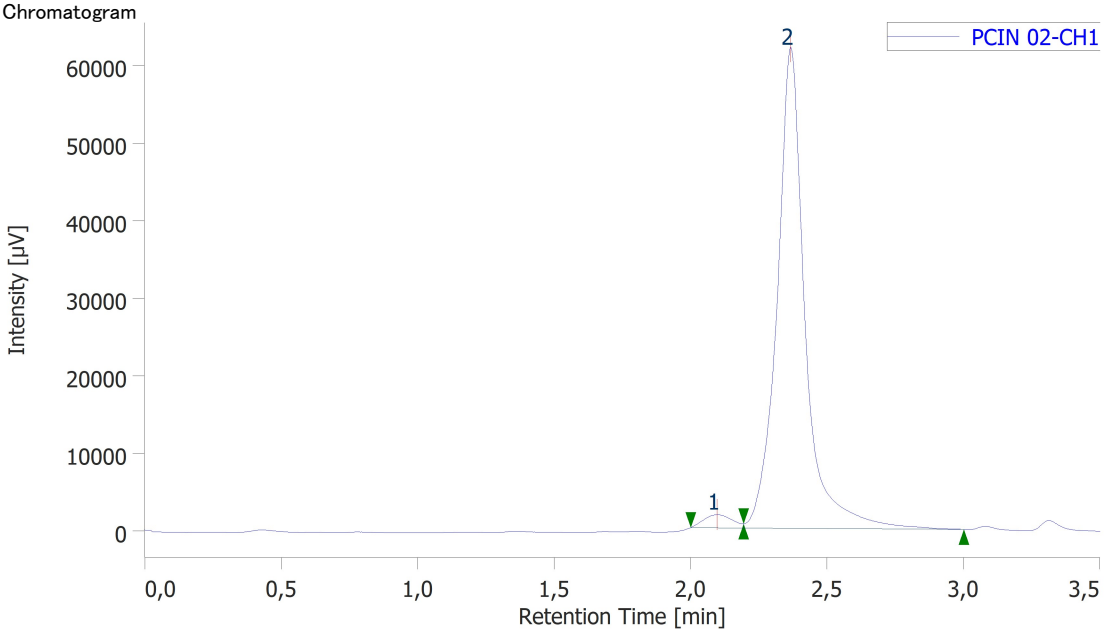


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,097	12131	1687	2,681	2,647	N/A	1641	1,479	N/A	
2	Cafeína	1	2,367	440296	62037	97,319	97,353	N/A	3538	N/A	1,165	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 13:51:39
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:48:07
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

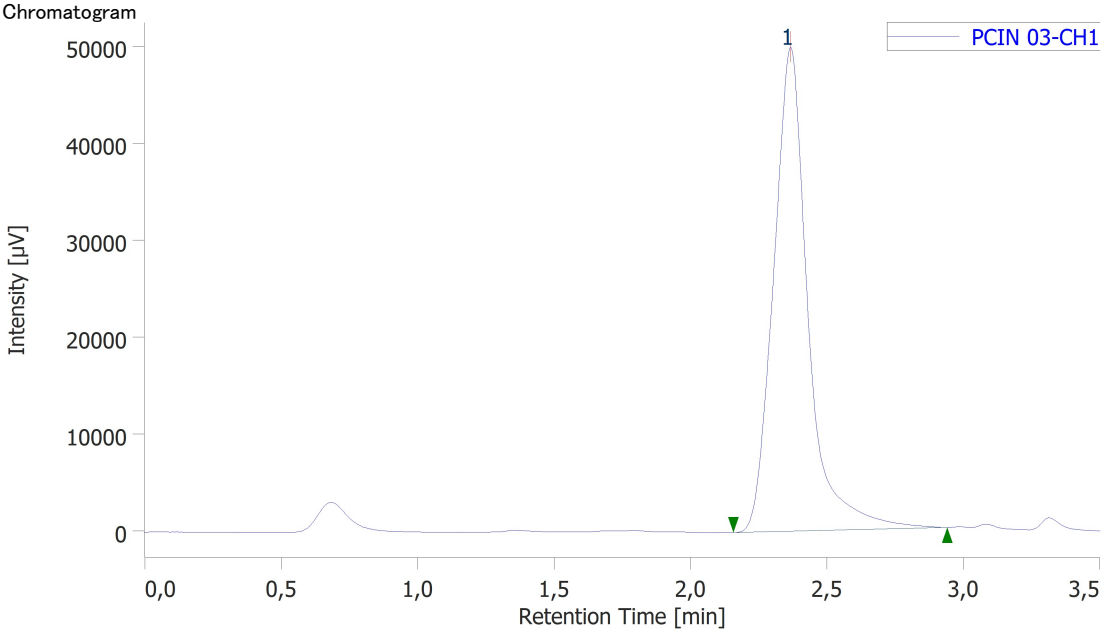


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,367	437225	49929	100,000	100,000	N/A	2003	N/A	1,278	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:00:09
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 13:56:38
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

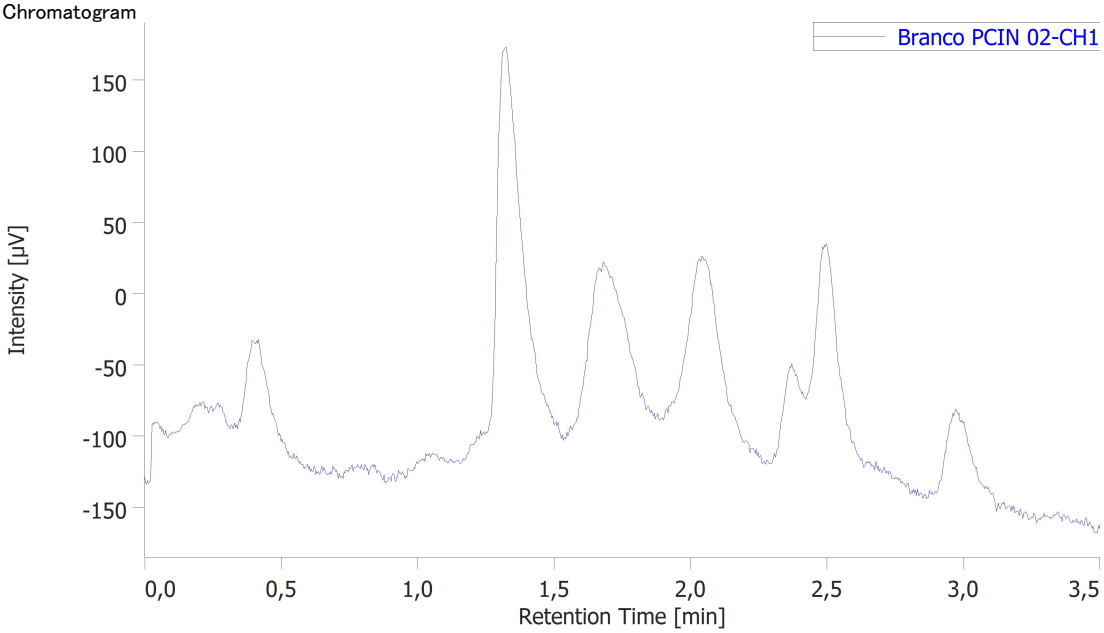

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:04:29
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:00:57
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

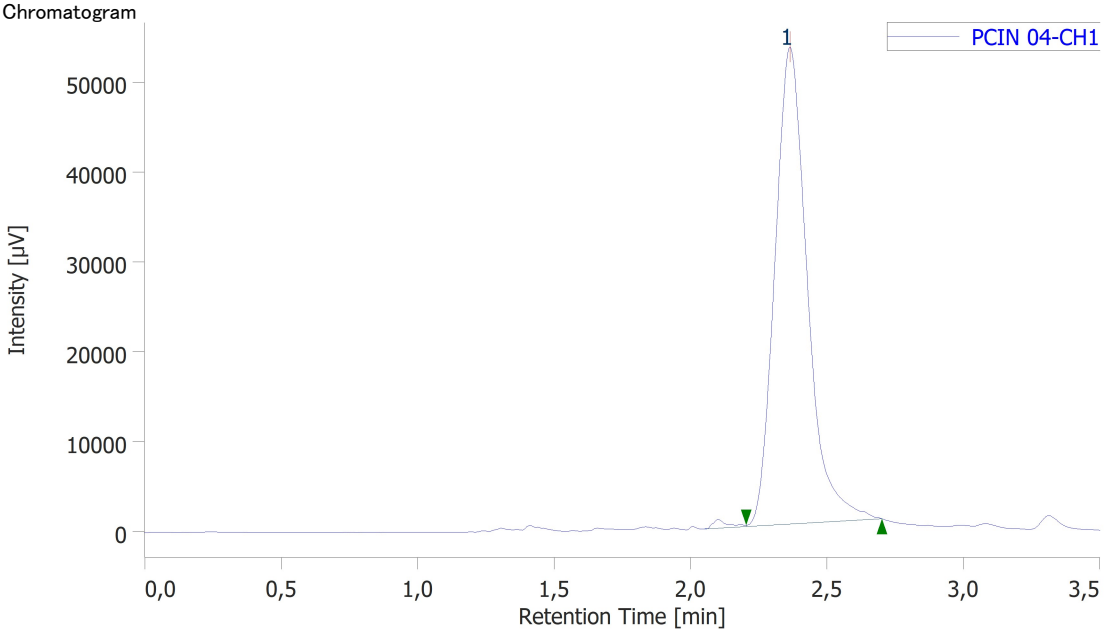


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,363	438025	53064	100,000	100,000	N/A	2007	N/A	1,274	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:08:49
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:05:19
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

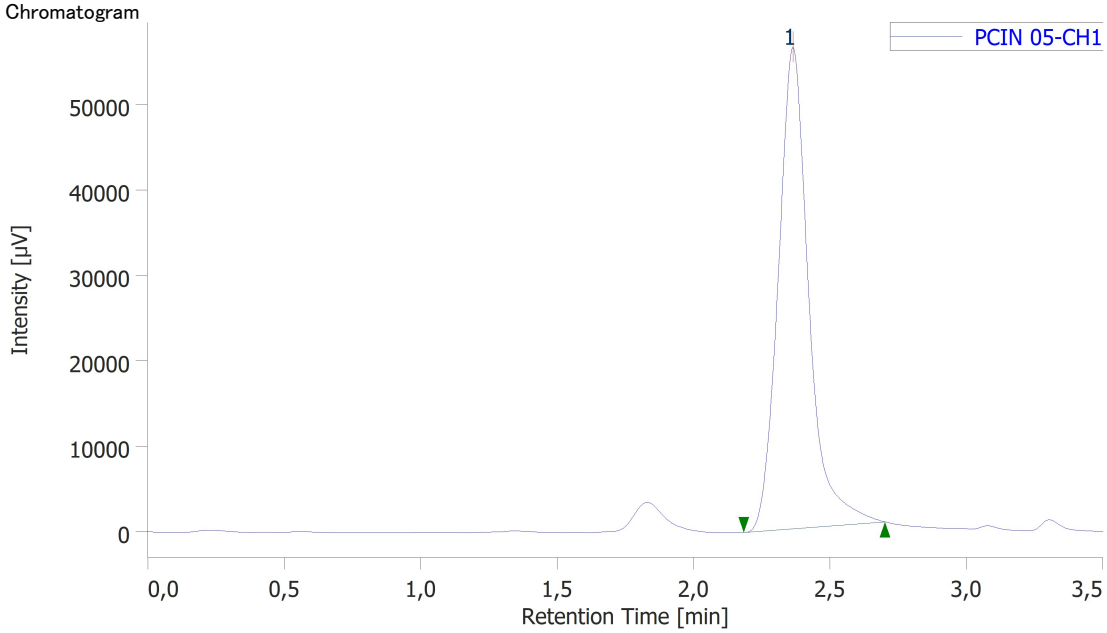


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,363	437002	56426	100,000	100,000	N/A	2452	N/A	1,251	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:13:09
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:09:39
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

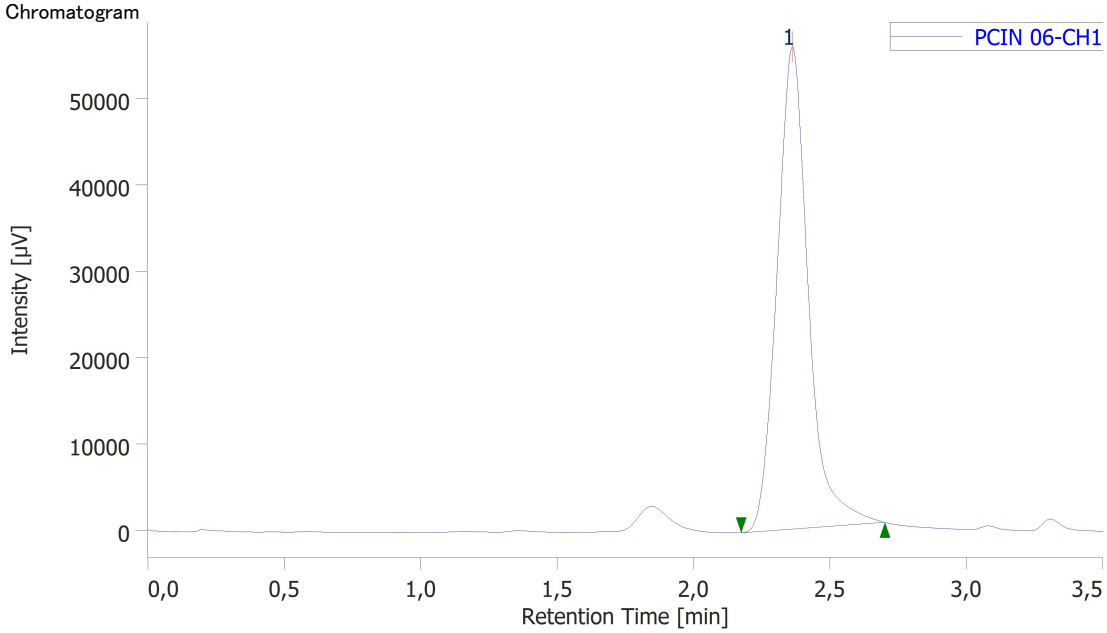


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,360	443650	55809	100,000	100,000	N/A	2267	N/A	1,230	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:17:17
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:13:47
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

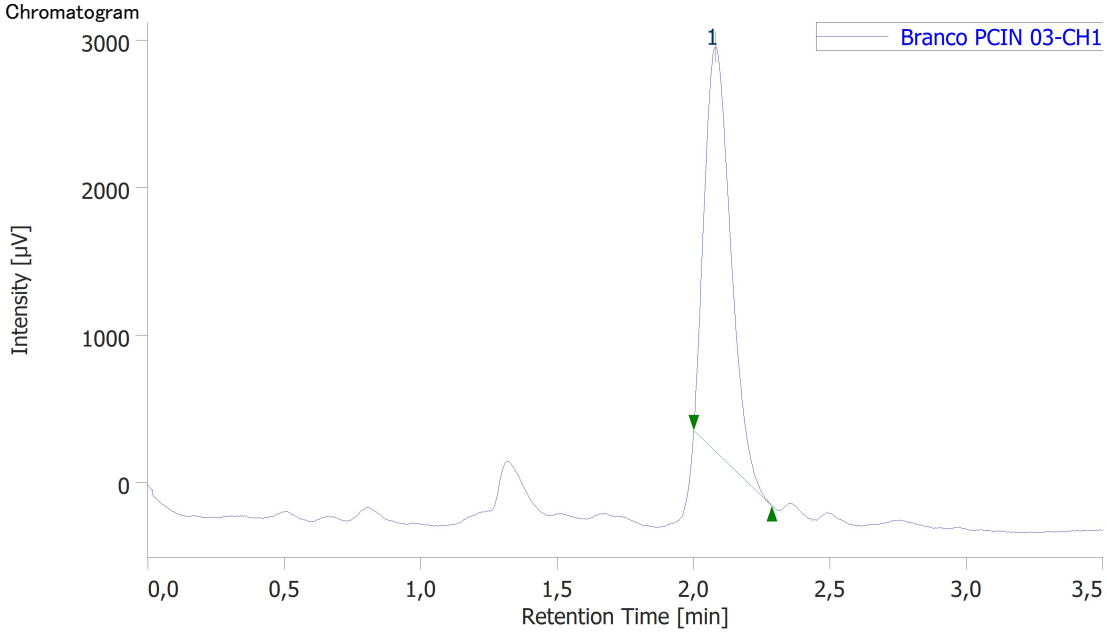

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,080	18295	2742	100,000	100,000	N/A	2130	N/A	1,395	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:23:45
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:20:14
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

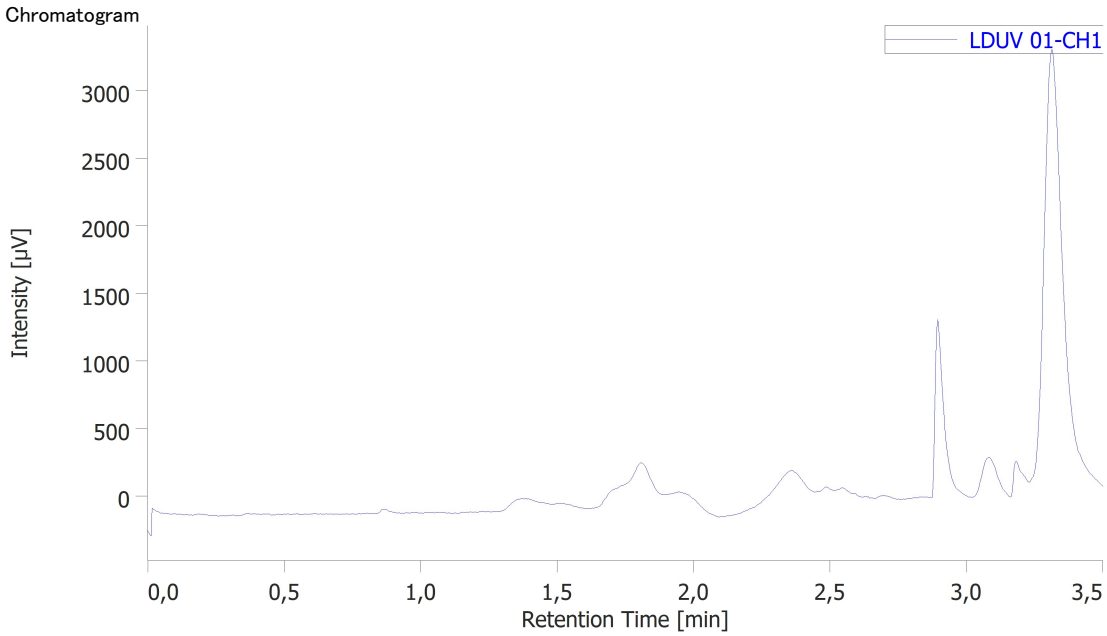

Peak Information – No data.


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:28:25
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:24:54
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

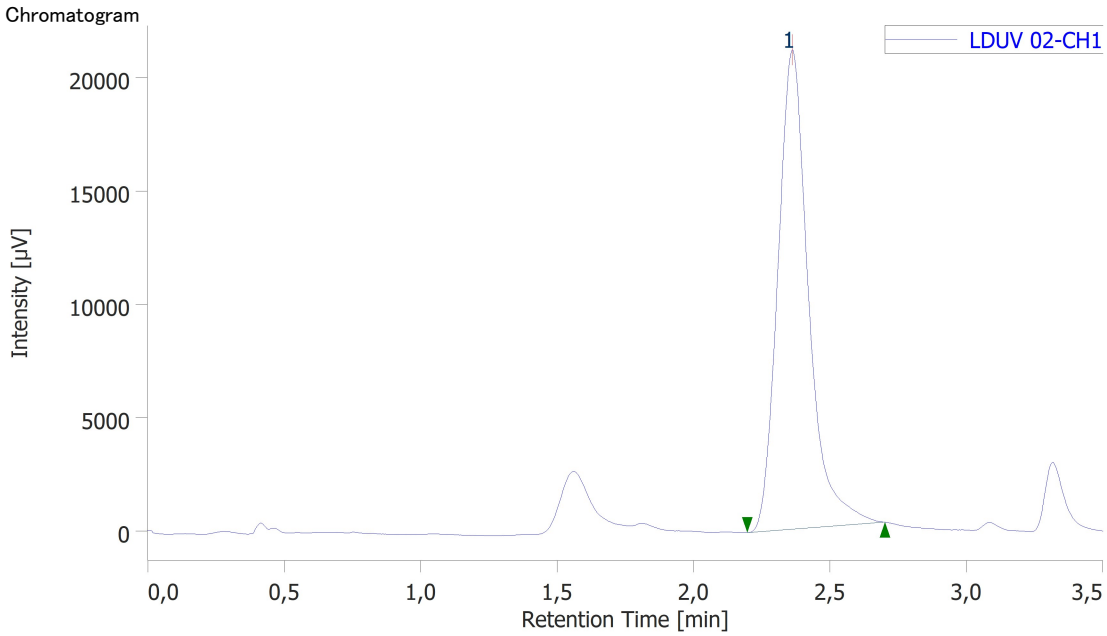

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,360	164905	21147	100,000	100,000	N/A	2361	N/A	1,311	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:33:01
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:29:30
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

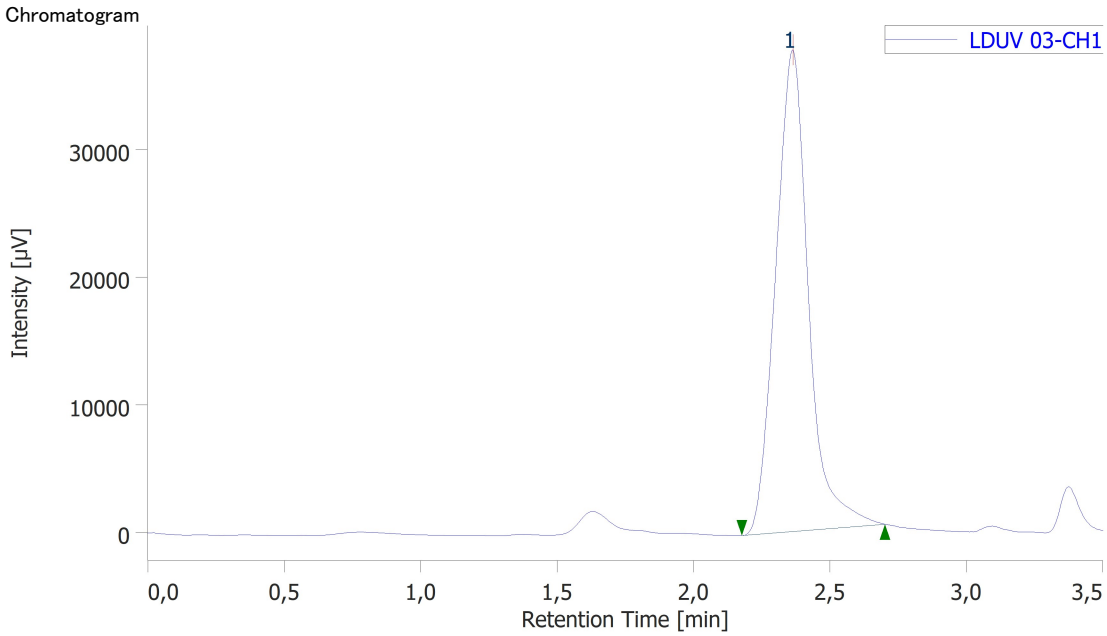

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,363	314683	37723	100,000	100,000	N/A	2020	N/A	1,173	


Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:37:47
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:34:15
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

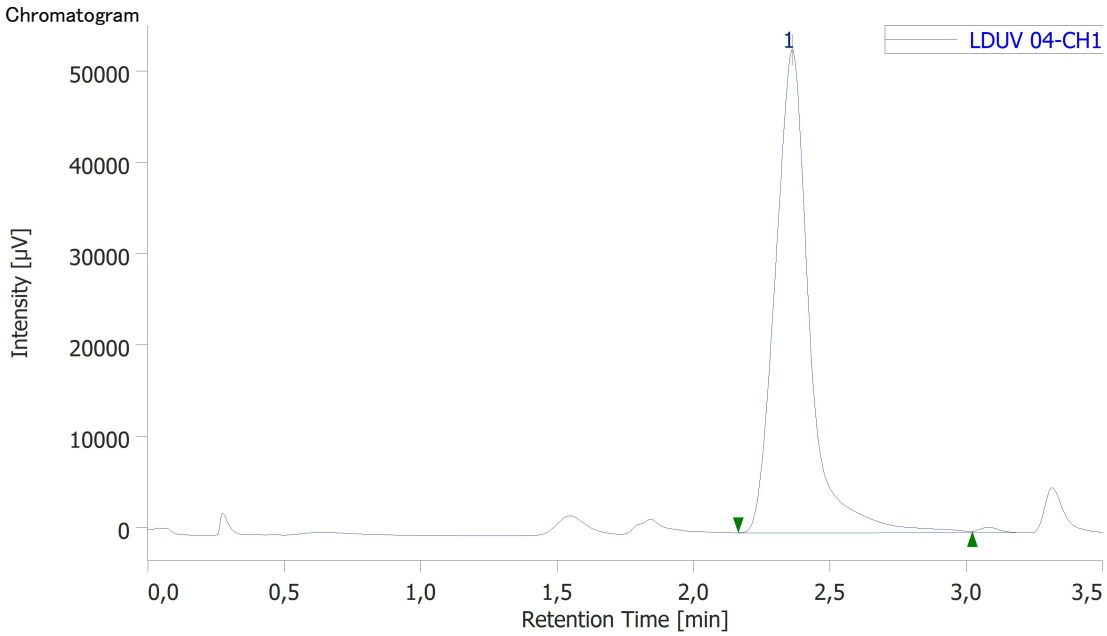

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,360	459324	52897	100,000	100,000	N/A	2034	N/A	1,296	

Chromatogram Information	
User Name	Administrator
Date Modified	30/09/2022 14:42:15
Description	
HPLC System Name	HPLC
Injection Date	30/09/2022 14:38:44
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

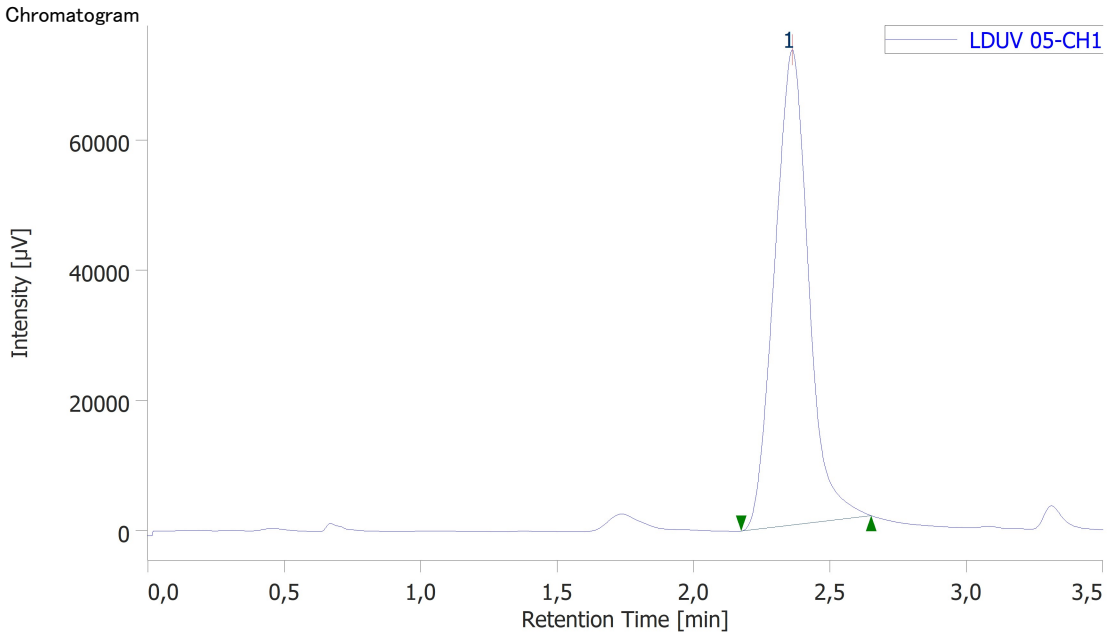

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2,360	632021	72965	100,000	100,000	N/A	1765	N/A	1,122	