
Peak Find - EDUV PDA_tR1,20 D.jws

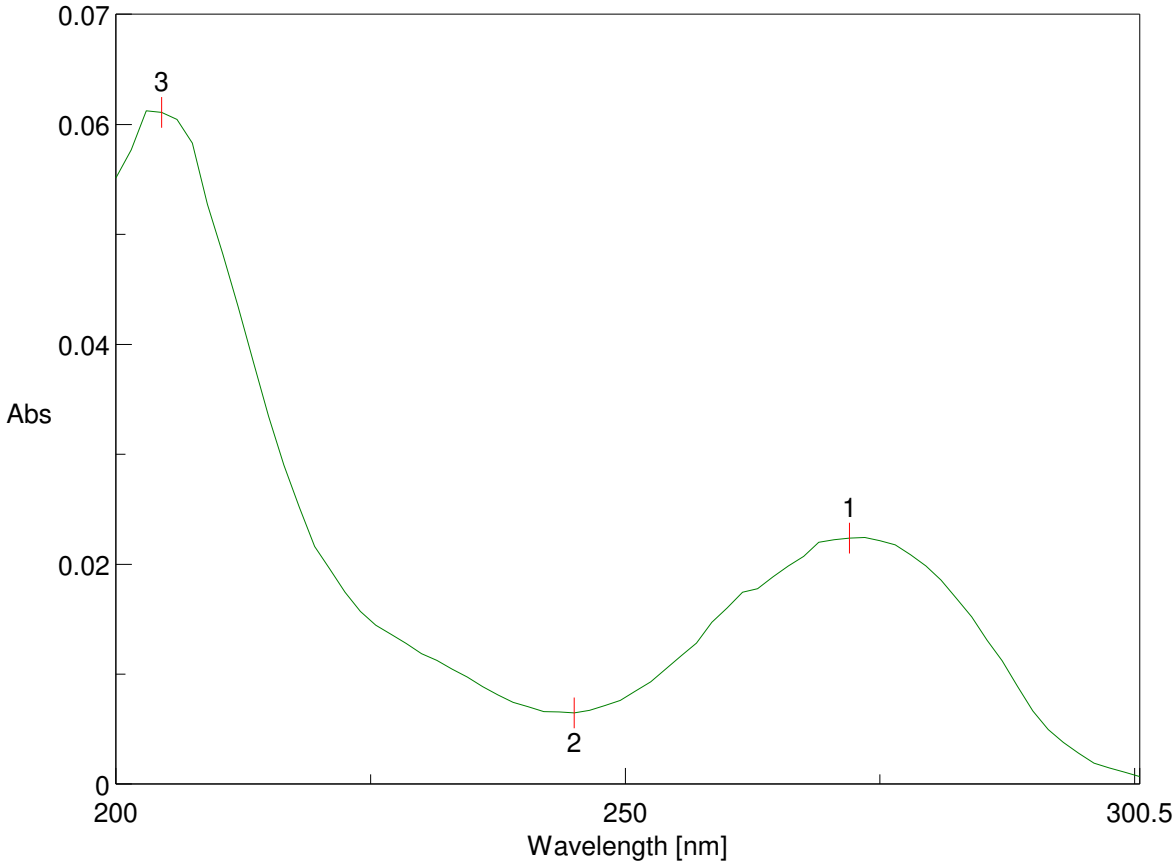

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	09/11/2022 09:01

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300.5 nm
Data interval	1.5 nm
Data points	68


[Measurement Information]

Instrument Name	MD-2015
Model Name	MD-2015
Serial No.	0000000000
ROM version	2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.022365	2	245	0.006464
3	204.5	0.061073			

Chromatogram

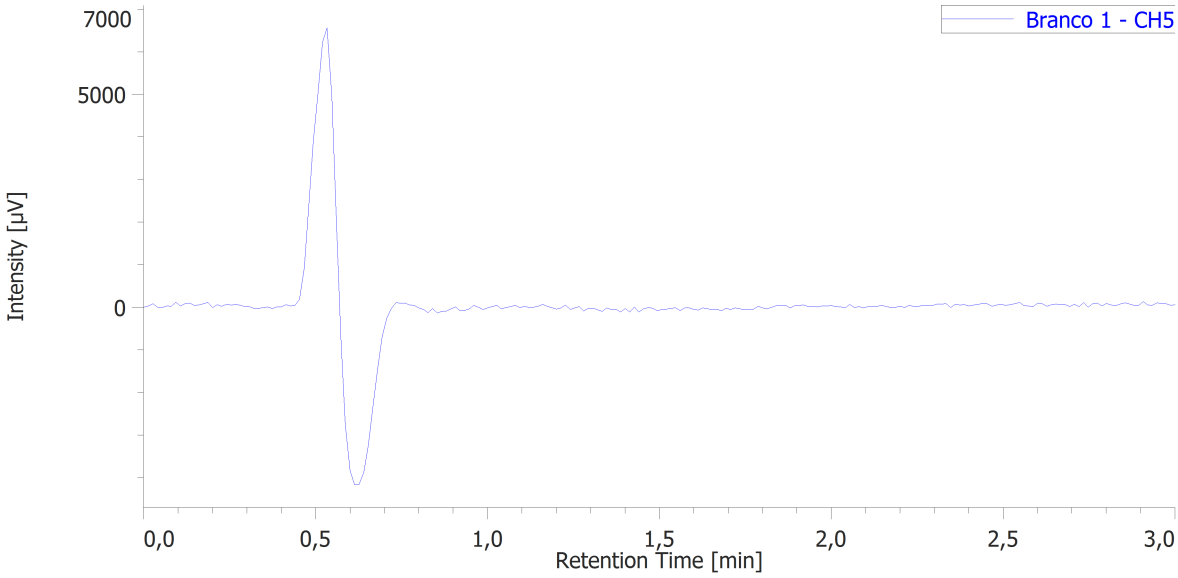


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:25
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:09:04
Volume	10,0 [µL]
Sample #	22
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

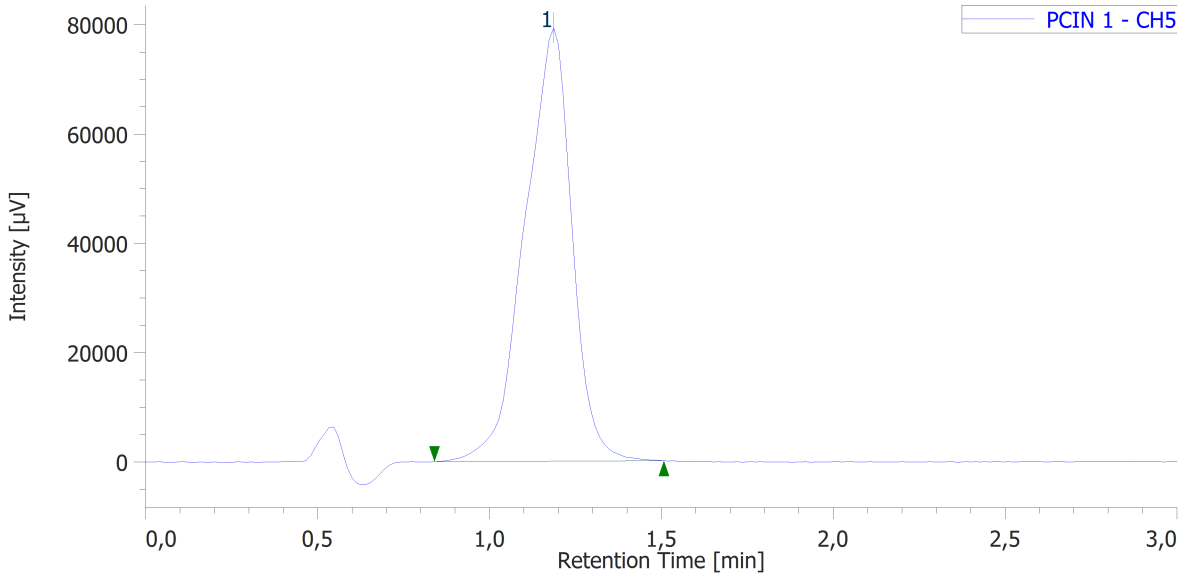

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:13:23
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	753334	79227	100,000	100,000	N/A	346	N/A	0,855	

Creator QPackSA
Reviewer
Approver

Chromatogram

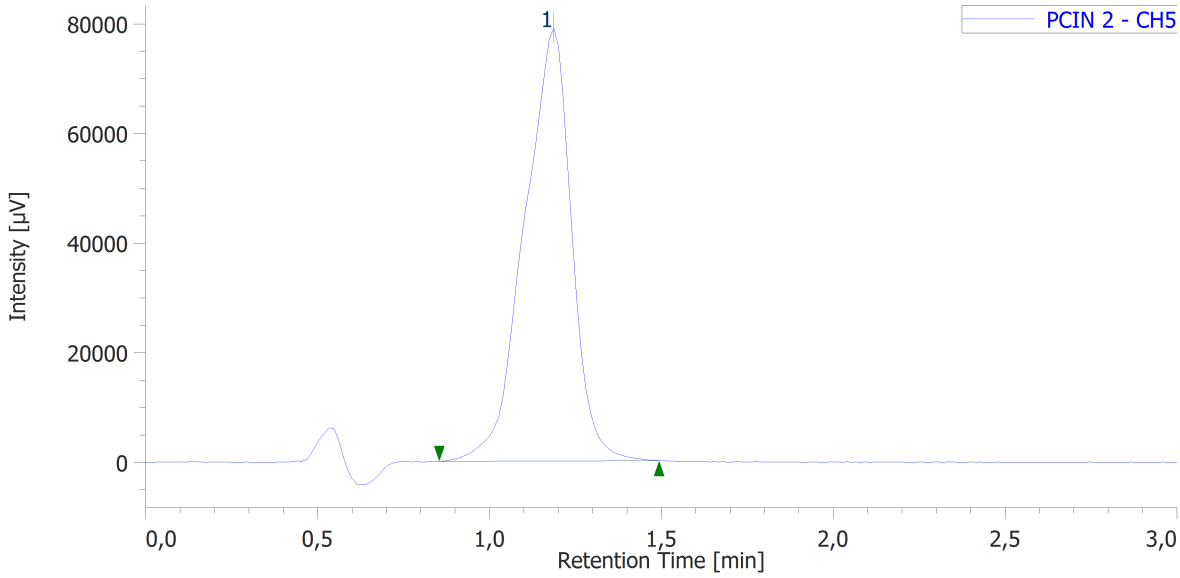

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:17:44
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	752062	78938	100,000	100,000	N/A	343	N/A	0,844	

Creator QPackSA
Reviewer
Approver

Chromatogram

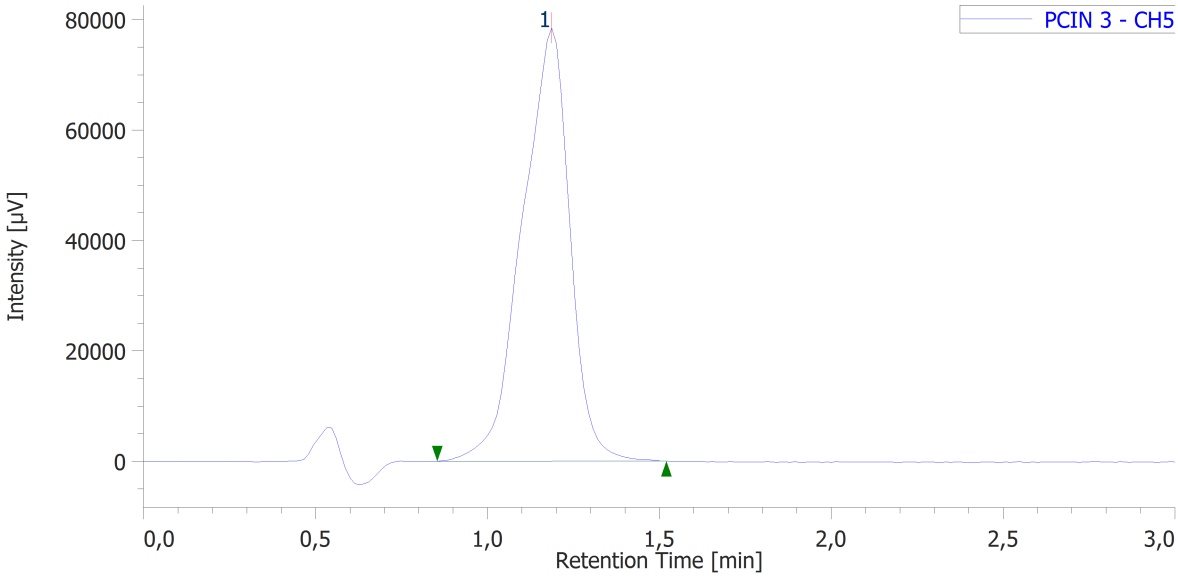

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:22:03
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	753432	78421	100,000	100,000	N/A	335	N/A	0,841	

Creator QPackSA
Reviewer
Approver

Chromatogram

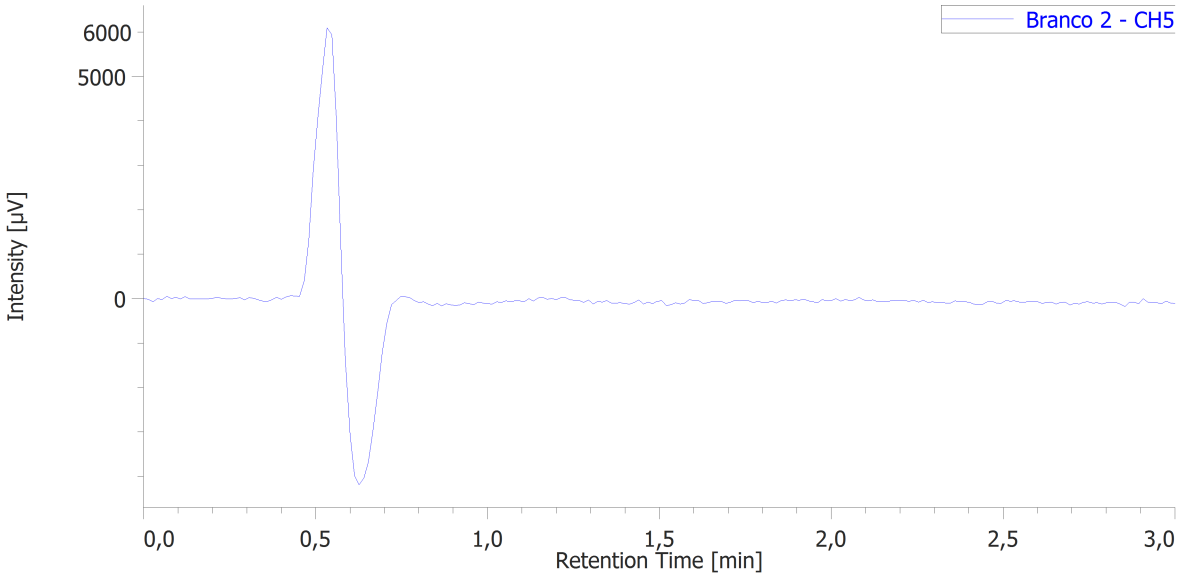


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:26:22
Volume	10,0 [µL]
Sample #	22
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

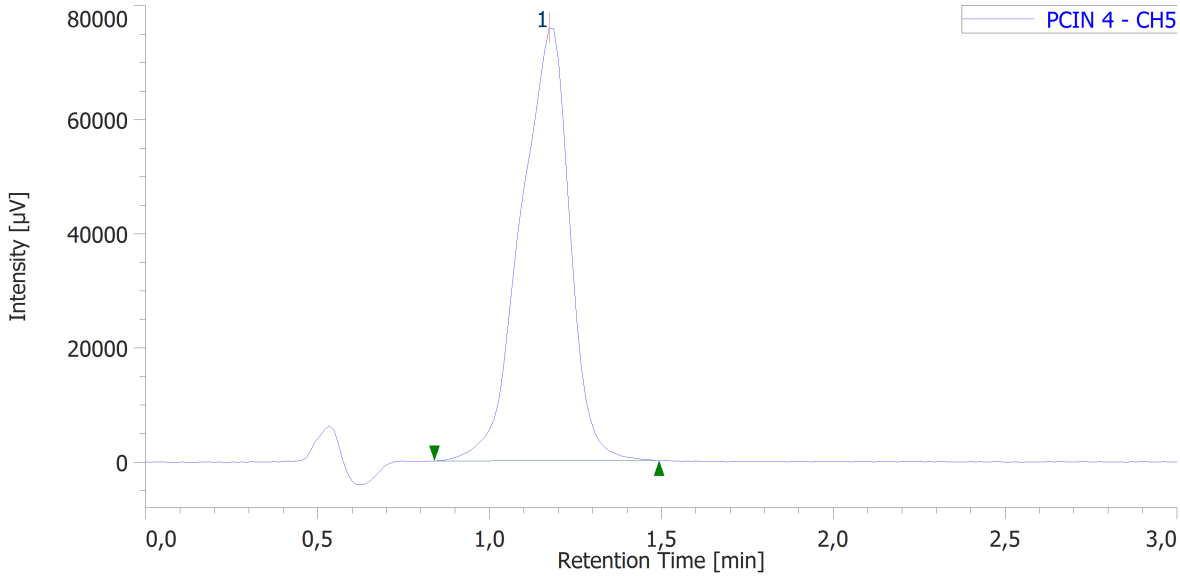

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:30:42
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,173	751909	75796	100,000	100,000	N/A	302	N/A	0,869	

Creator QPackSA
Reviewer
Approver

Chromatogram

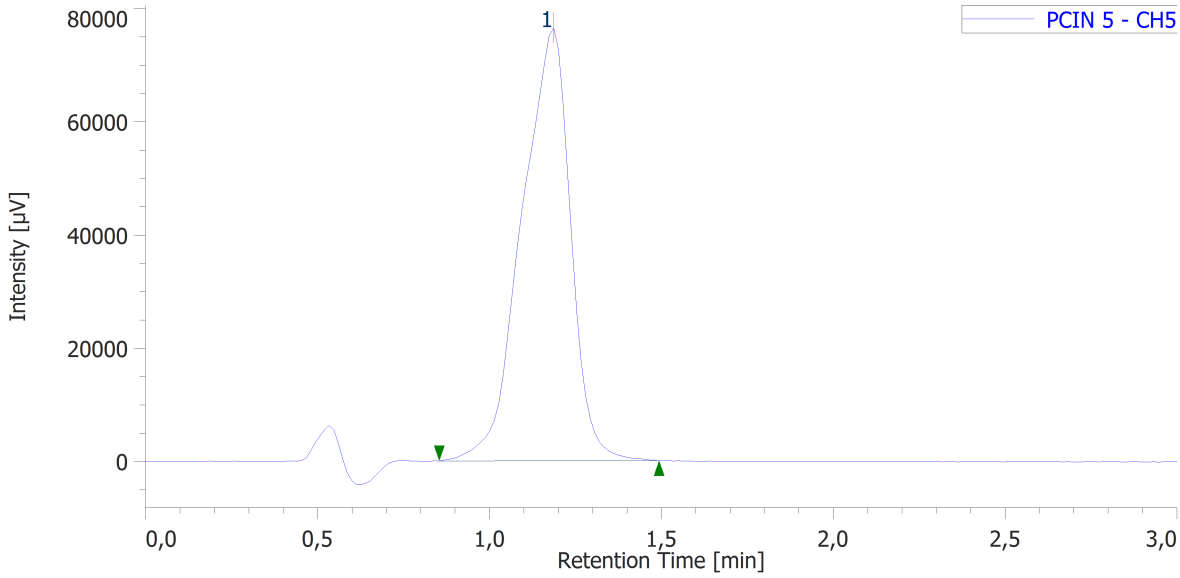

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:35:01
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	752508	76391	100,000	100,000	N/A	311	N/A	0,814	

Creator QPackSA
Reviewer
Approver

Chromatogram

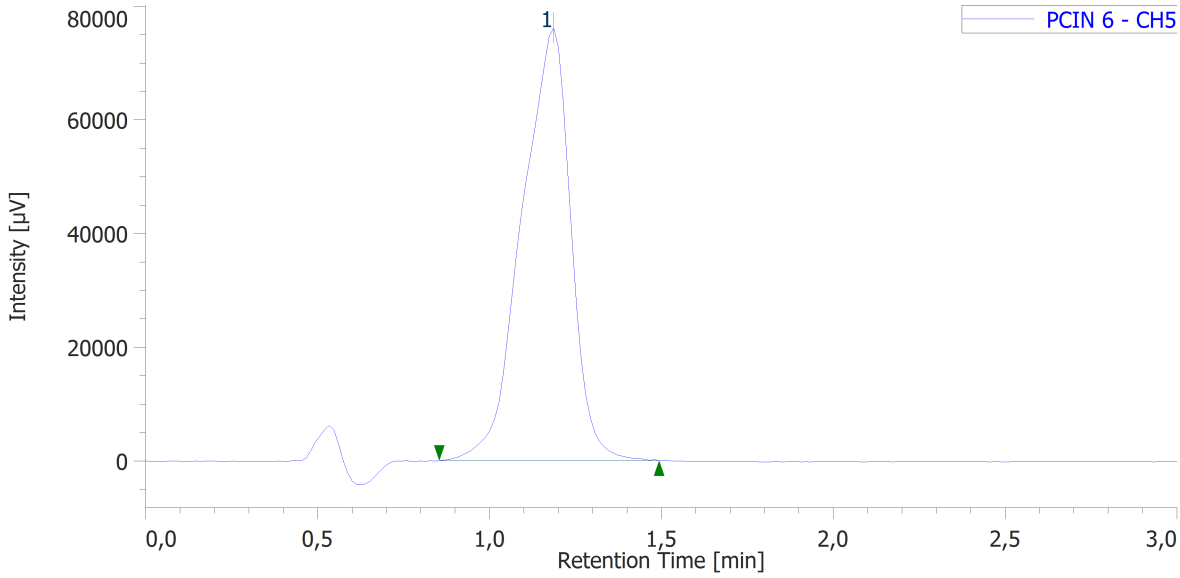

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:39:22
Volume	10,0 [µL]
Sample #	23
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	751905	76045	100,000	100,000	N/A	308	N/A	0,817	

Creator QPackSA
Reviewer
Approver

Chromatogram

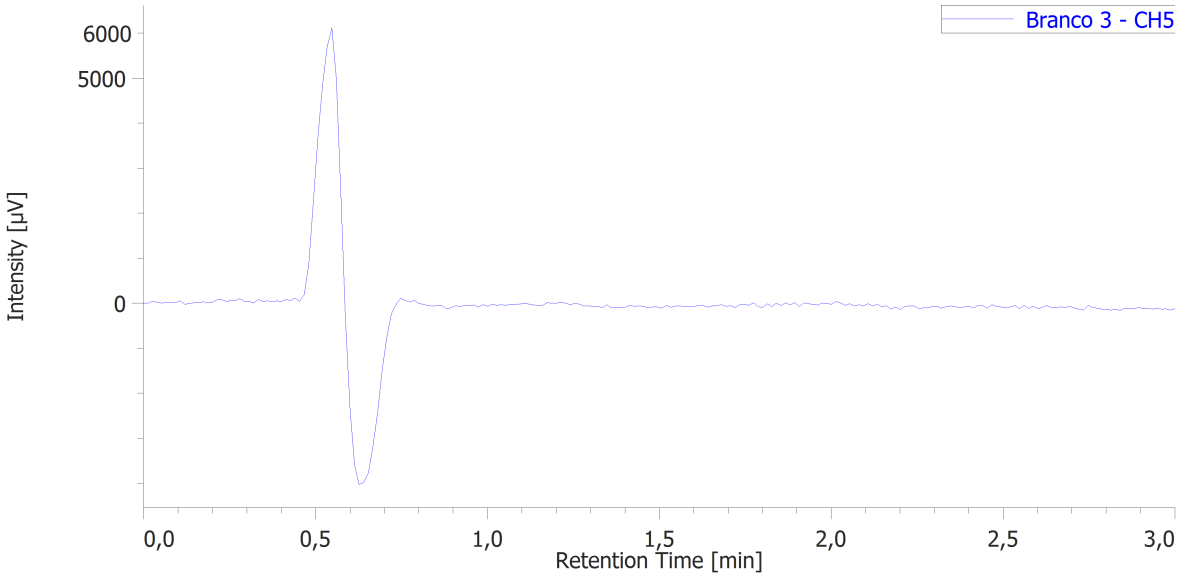


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:26
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:43:41
Volume	10,0 [µL]
Sample #	22
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

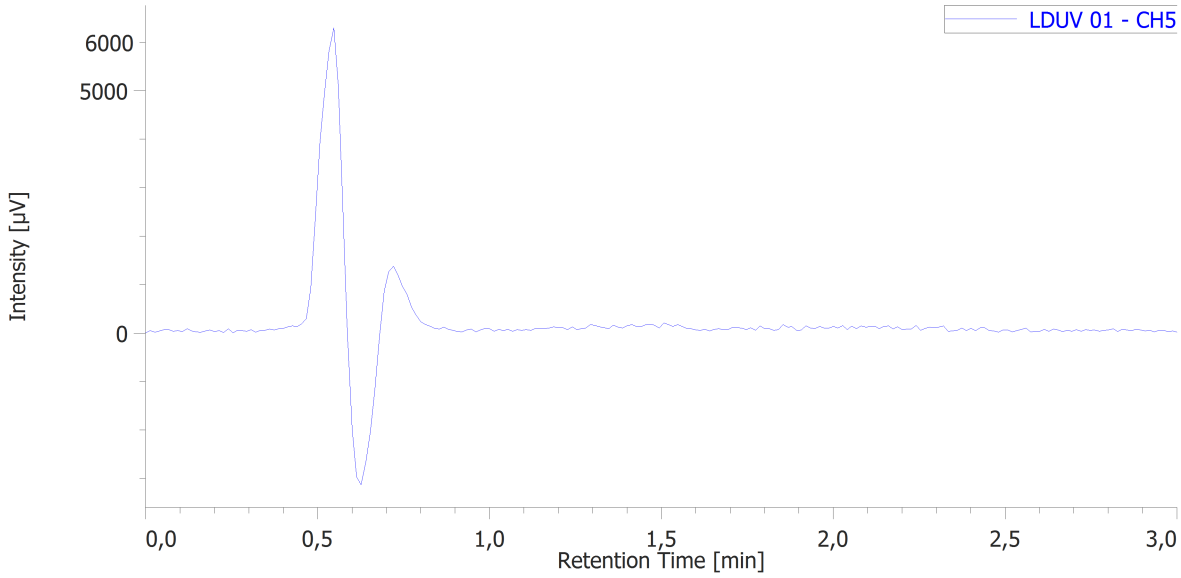


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:48:00
Volume	10,0 [µL]
Sample #	24
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

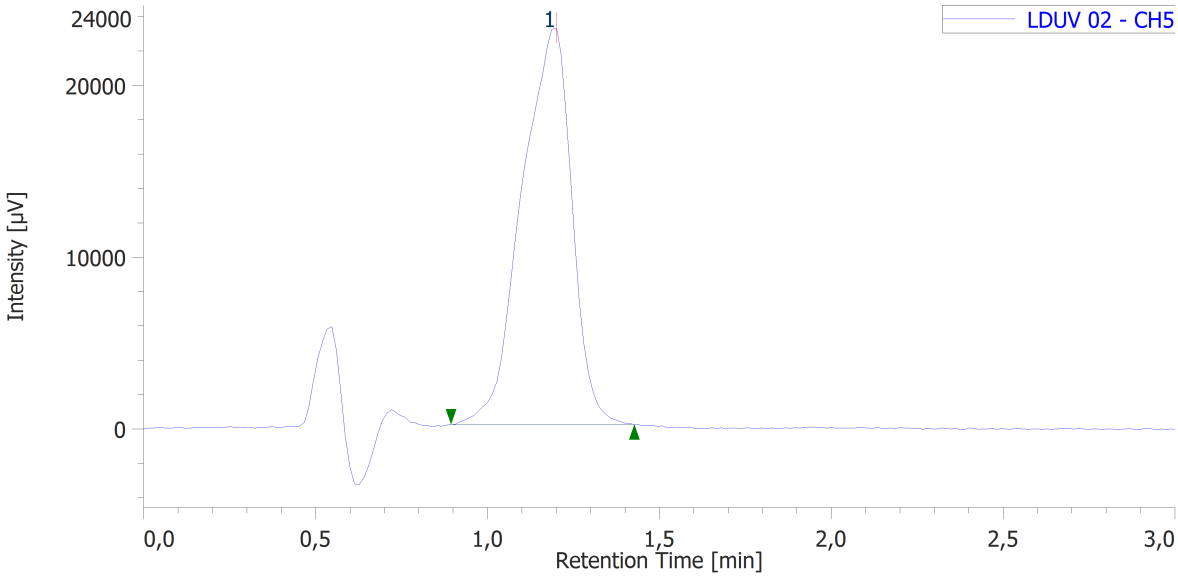

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:52:22
Volume	10,0 [µL]
Sample #	25
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,200	233566	23053	100,000	100,000	N/A	291	N/A	0,792	

Creator QPackSA
Reviewer
Approver

Chromatogram

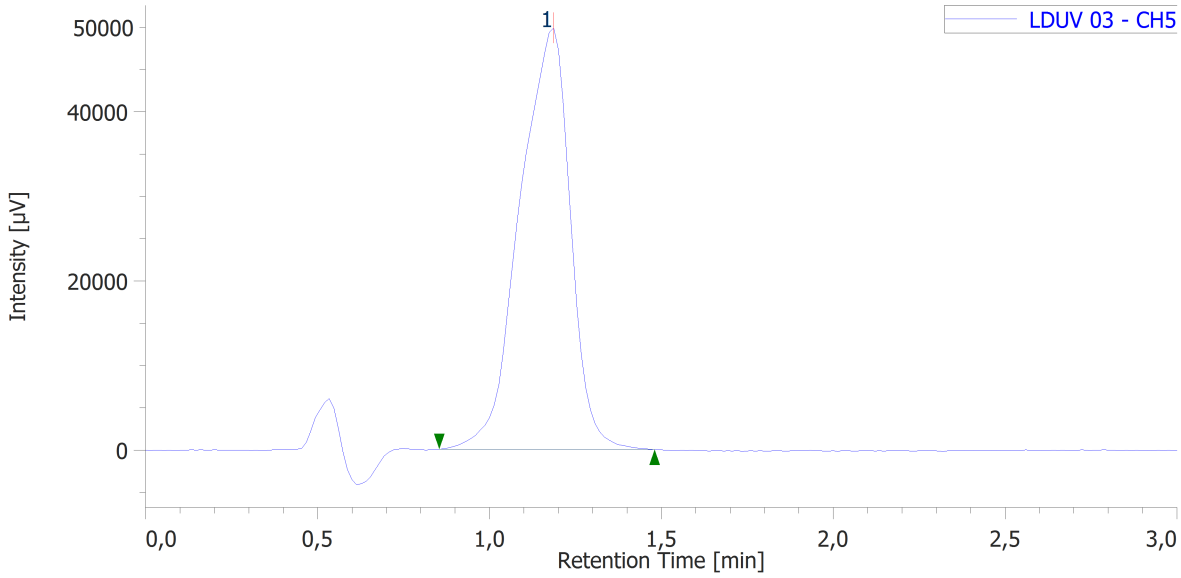

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 09:56:44
Volume	10,0 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	509314	49787	100,000	100,000	N/A	286	N/A	0,807	

Creator QPackSA
Reviewer
Approver

Chromatogram

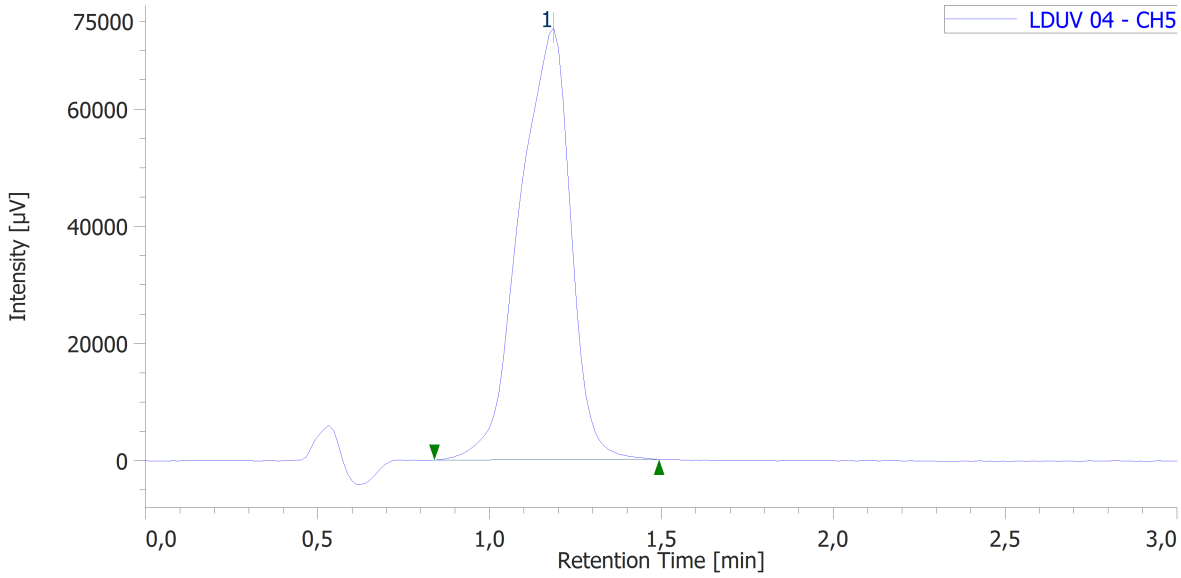

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:01:05
Volume	10,0 [µL]
Sample #	27
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	759367	73664	100,000	100,000	N/A	282	N/A	0,810	

Creator QPackSA
Reviewer
Approver

Chromatogram

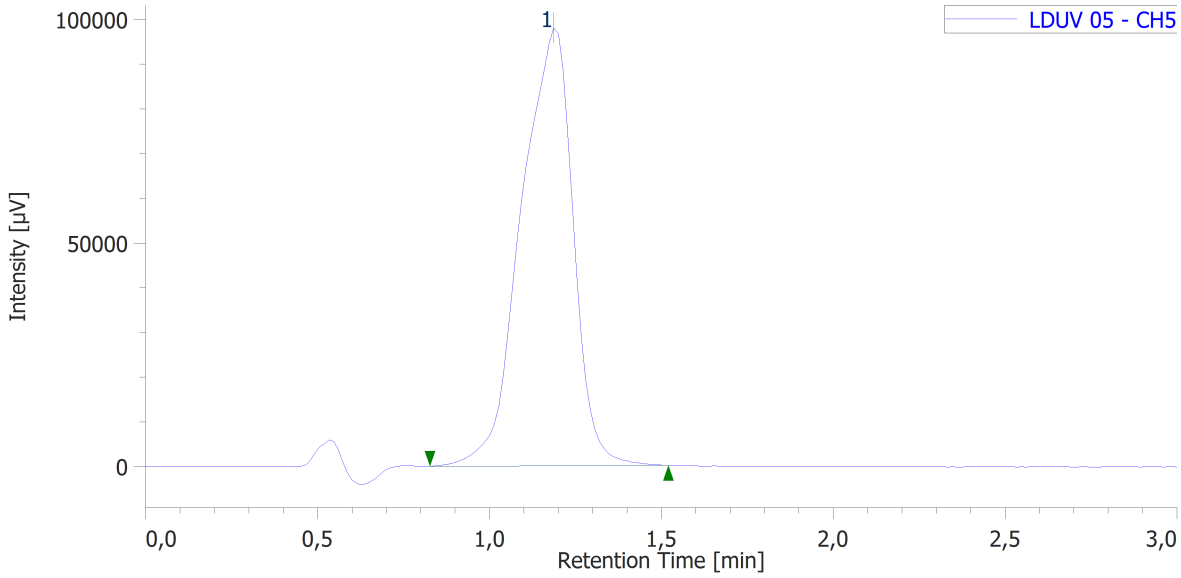

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:05:29
Volume	10,0 [µL]
Sample #	28
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	1027935	97867	100,000	100,000	N/A	270	N/A	0,832	

Creator QPackSA
Reviewer
Approver

Chromatogram

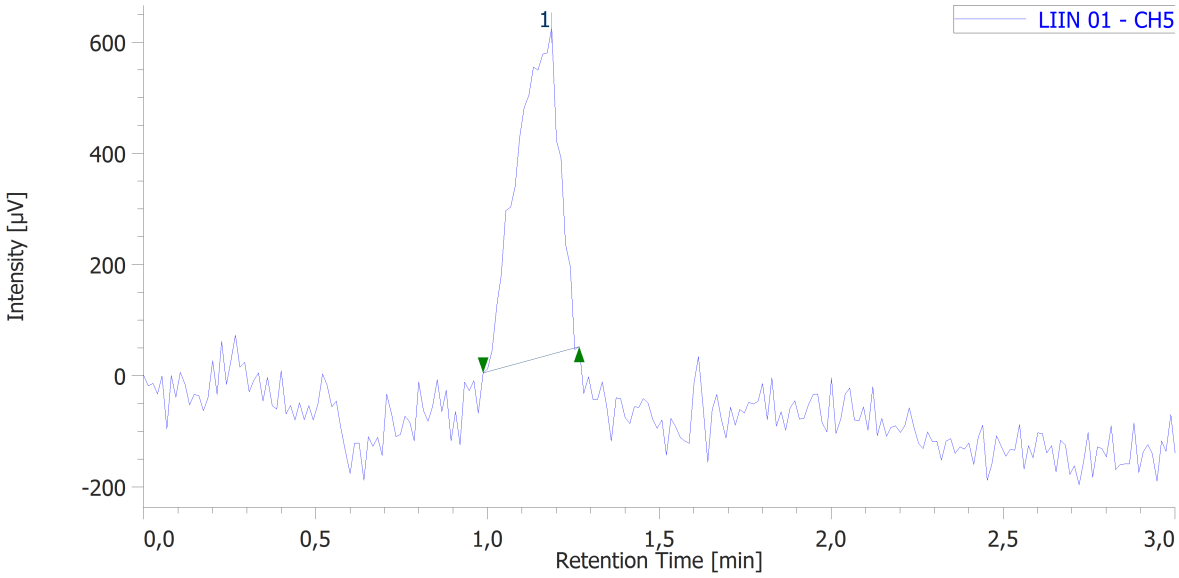

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:09:49
Volume	0,1 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	5068	586	100,000	100,000	N/A	356	N/A	0,681	

Creator QPackSA
Reviewer
Approver

Chromatogram

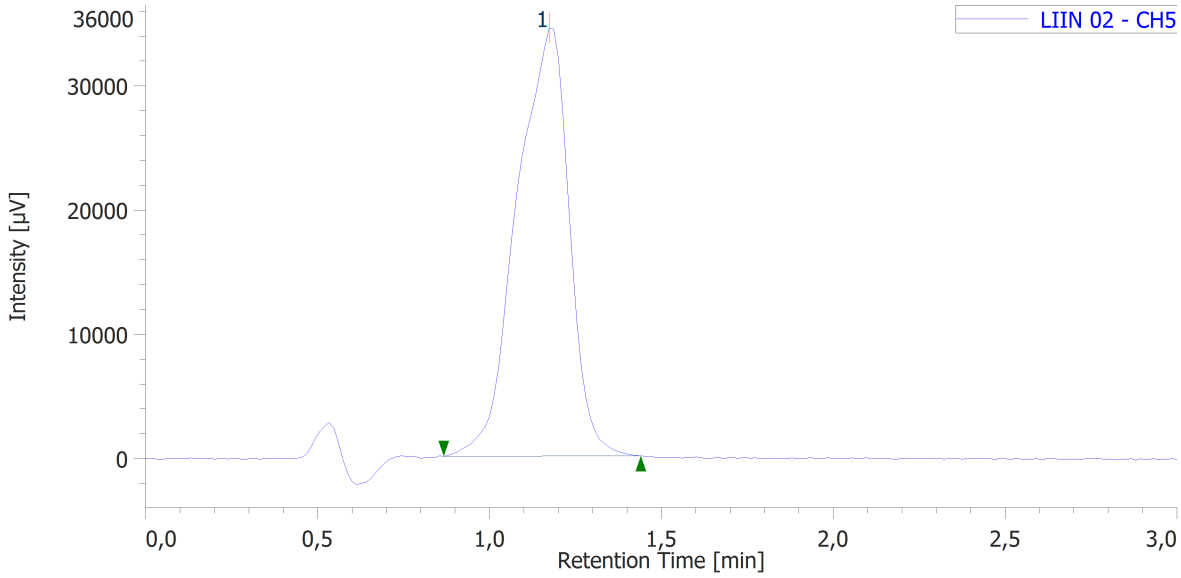

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:14:10
Volume	5,0 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,173	365192	34426	100,000	100,000	N/A	252	N/A	0,843	

Creator QPackSA
Reviewer
Approver

Chromatogram

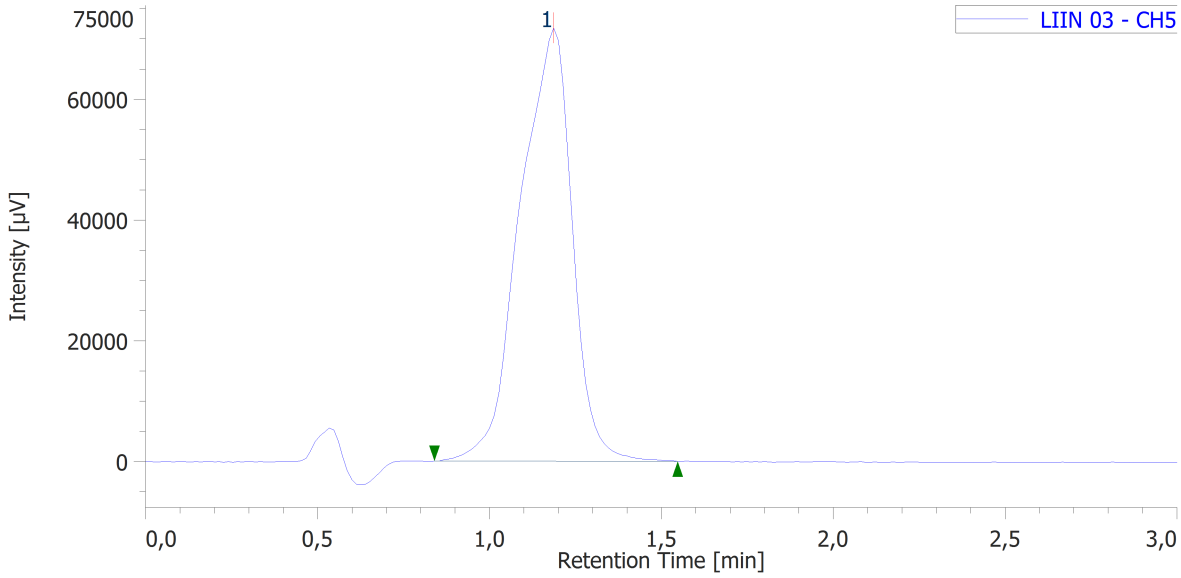

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:27
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:18:34
Volume	10,0 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,187	753987	71695	100,000	100,000	N/A	266	N/A	0,831	

Creator QPackSA
Reviewer
Approver

Chromatogram

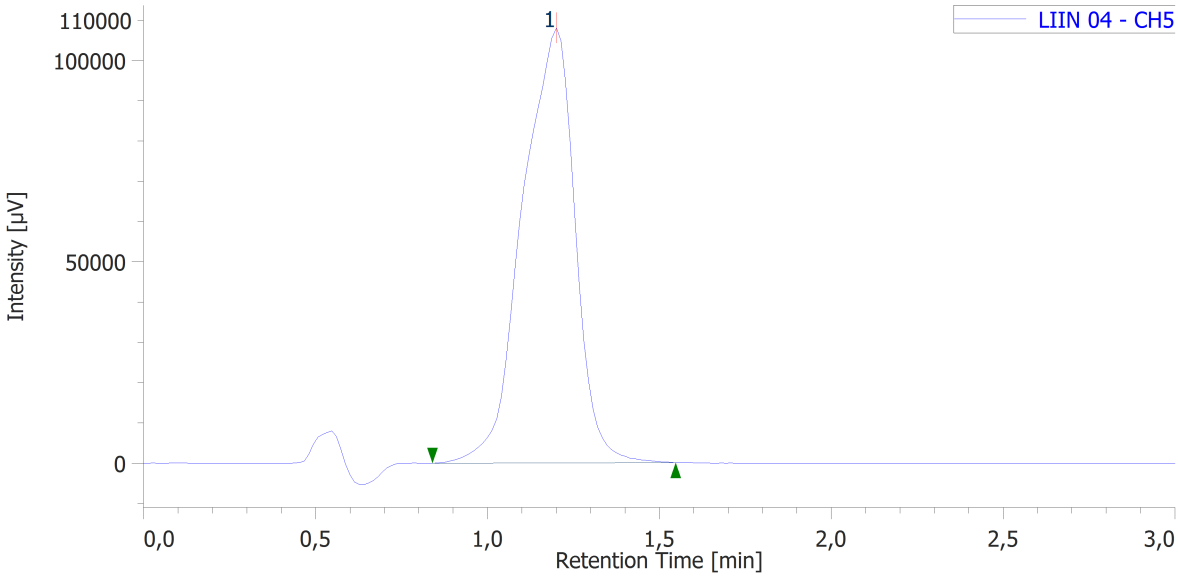

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:28
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:23:01
Volume	15,0 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,200	1148529	107915	100,000	100,000	N/A	267	N/A	0,832	

Creator QPackSA
Reviewer
Approver

Chromatogram

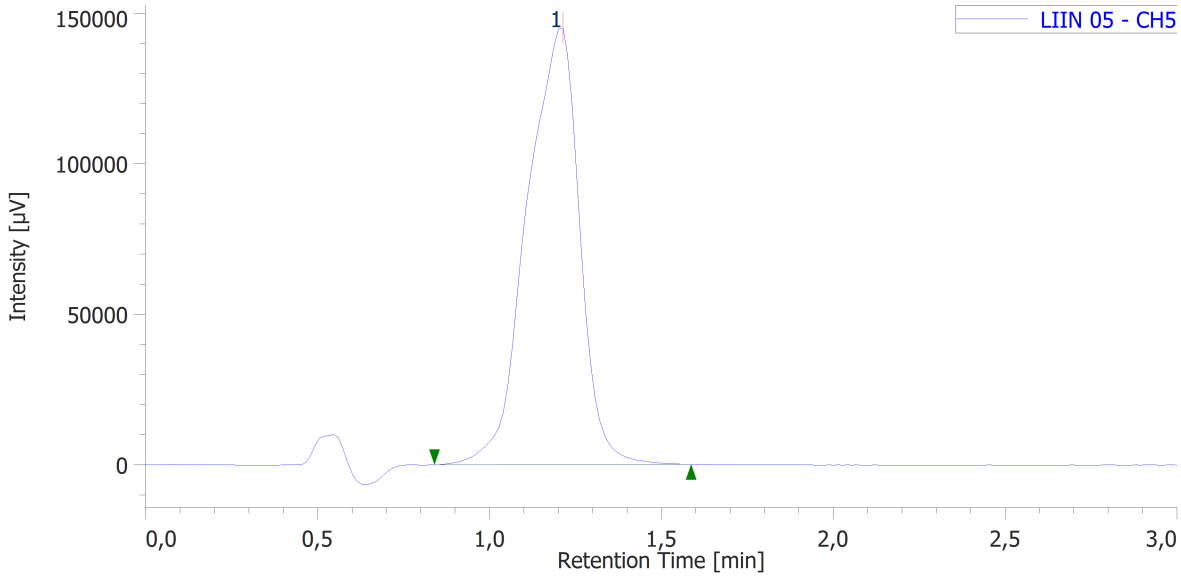

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2022 10:38:28
Description	
HPLC System Name	HPL 18 PDA
Injection Date	09/11/2022 10:27:30
Volume	20,0 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	QUALIFICAÇÃO_2022
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,213	1545393	144966	100,000	100,000	N/A	274	N/A	0,806	

Creator QPackSA
Reviewer
Approver

Chromatogram

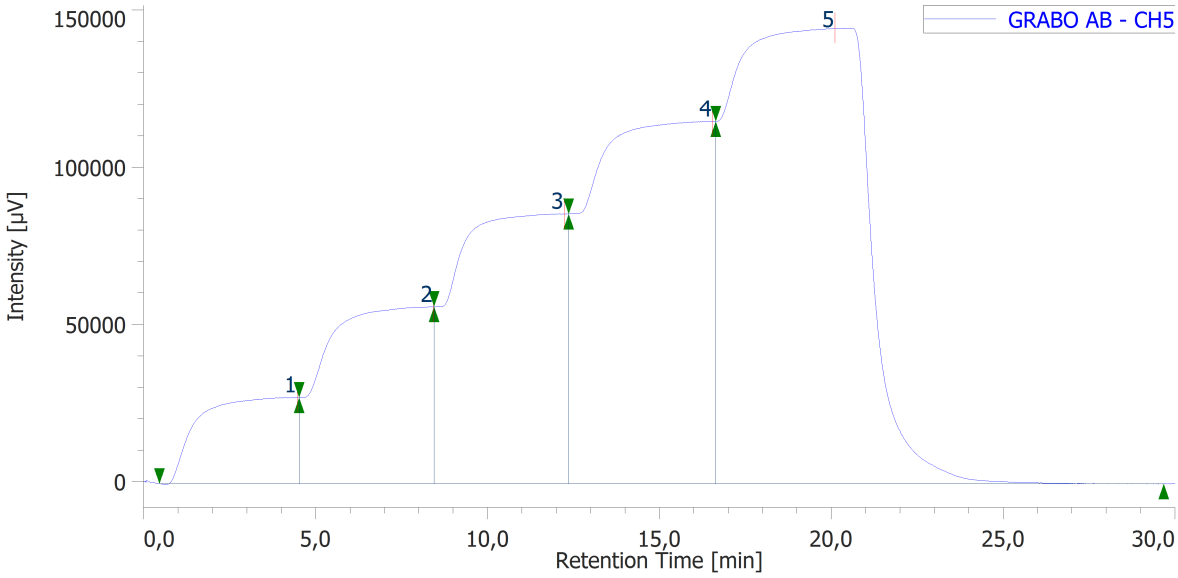

Chromatogram Information	
User Name	QPackSA
Date Modified	10/11/2022 11:02:14
Description	
HPLC System Name	HPL 18 PDA
Injection Date	10/11/2022 10:32:12
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	30,0 [min]
Acquisition Sequence	GRABO
Control Method	GRABO AB1
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRABO AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,467	5132442	27470	4,980	6,394	N/A	N/A	N/A	N/A	
2	Unknown	5	8,427	11656745	56252	11,310	13,093	N/A	N/A	N/A	N/A	
3	Unknown	5	12,227	18653545	85867	18,099	19,986	N/A	N/A	N/A	N/A	
4	Unknown	5	16,533	27757106	115179	26,933	26,809	N/A	N/A	N/A	N/A	
5	Unknown	5	20,107	39861898	144860	38,678	33,718	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

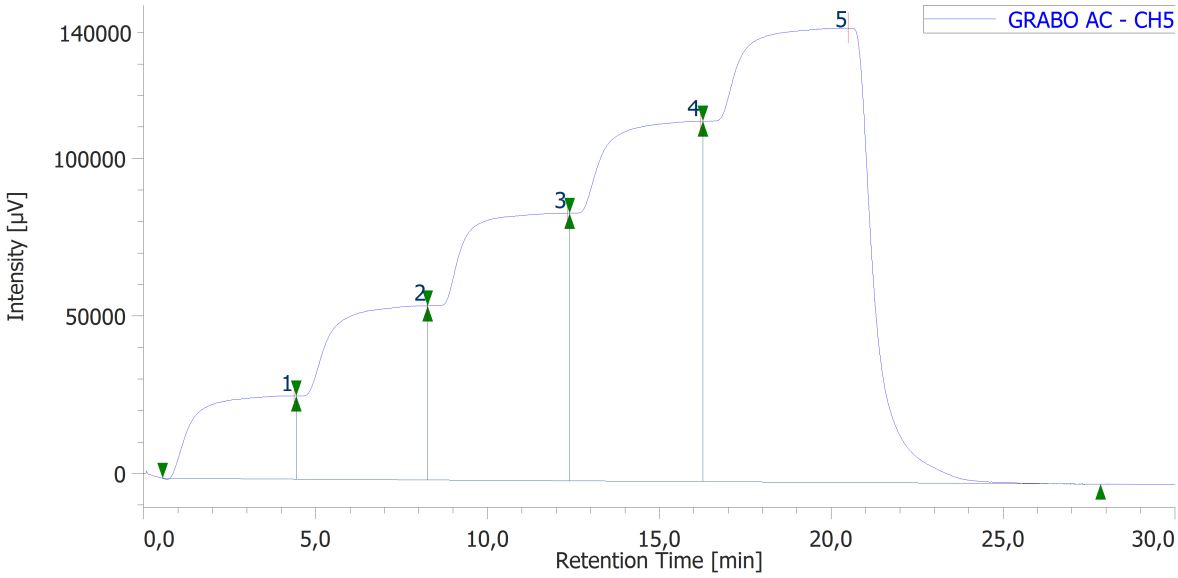

Chromatogram Information	
User Name	QPackSA
Date Modified	10/11/2022 13:54:41
Description	
HPLC System Name	HPL 18 PDA
Injection Date	10/11/2022 13:24:40
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	30,0 [min]
Acquisition Sequence	GRABO
Control Method	GRABO AC1
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRABO AC-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,373	4868623	26991	4,774	6,206	N/A	N/A	N/A	N/A	
2	Unknown	5	8,240	10995426	56266	10,781	12,996	N/A	N/A	N/A	N/A	
3	Unknown	5	12,320	19222842	84974	18,849	19,981	N/A	N/A	N/A	N/A	
4	Unknown	5	16,187	24886480	114418	24,402	26,905	N/A	N/A	N/A	N/A	
5	Unknown	5	20,480	42011421	144221	41,194	33,913	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver