
Peak Find - EDUV.jws

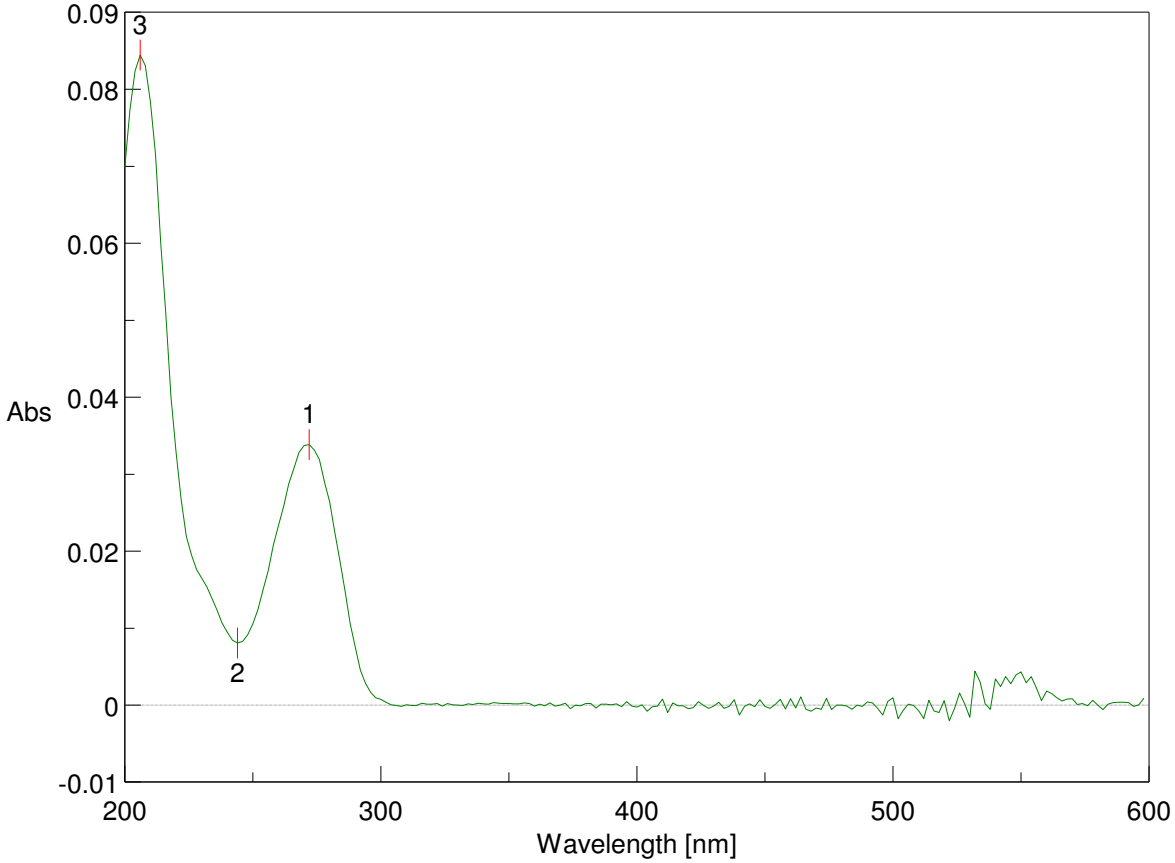

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	19/08/2025 11:51

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	X-LC 3075UV
Model Name	X-LC 3075UV
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.033811	2	244	0.00804698
3	206	0.084415			

Chromatogram

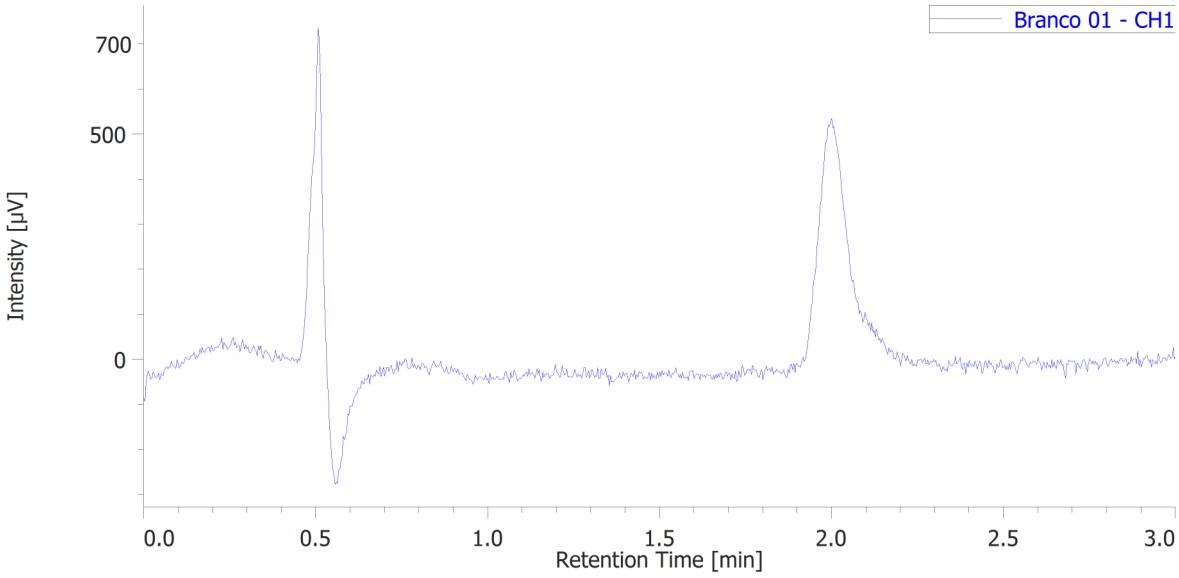


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:07:47
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 13:54:55
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

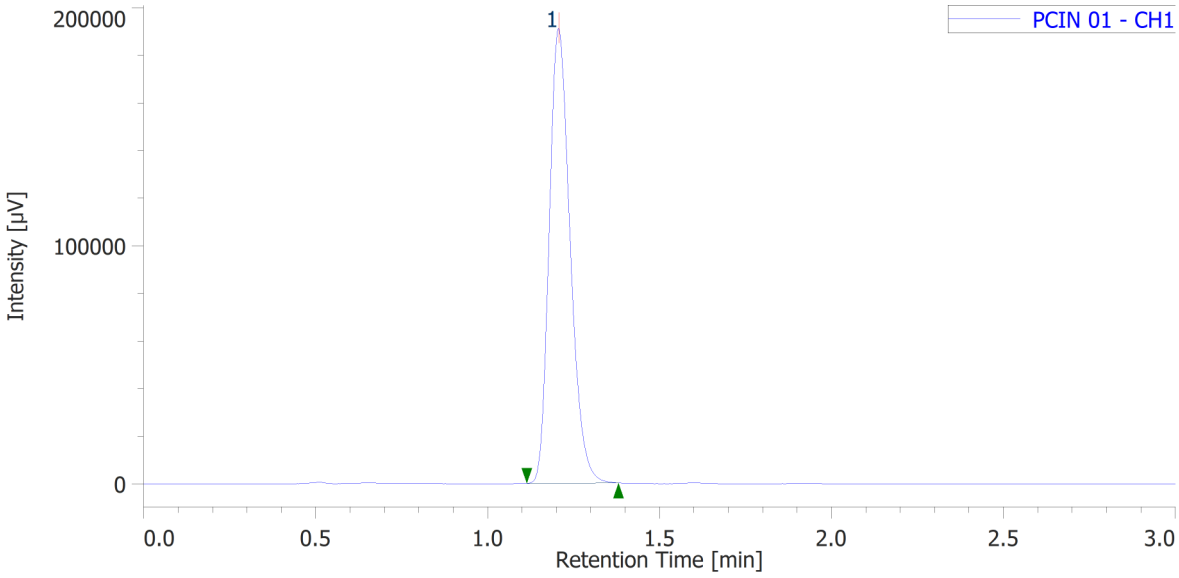

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:07:47
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 13:59:06
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	807746	191064	100.000	100.000	N/A	1909	N/A	1.234	

Creator Administrator
Reviewer
Approver

Chromatogram

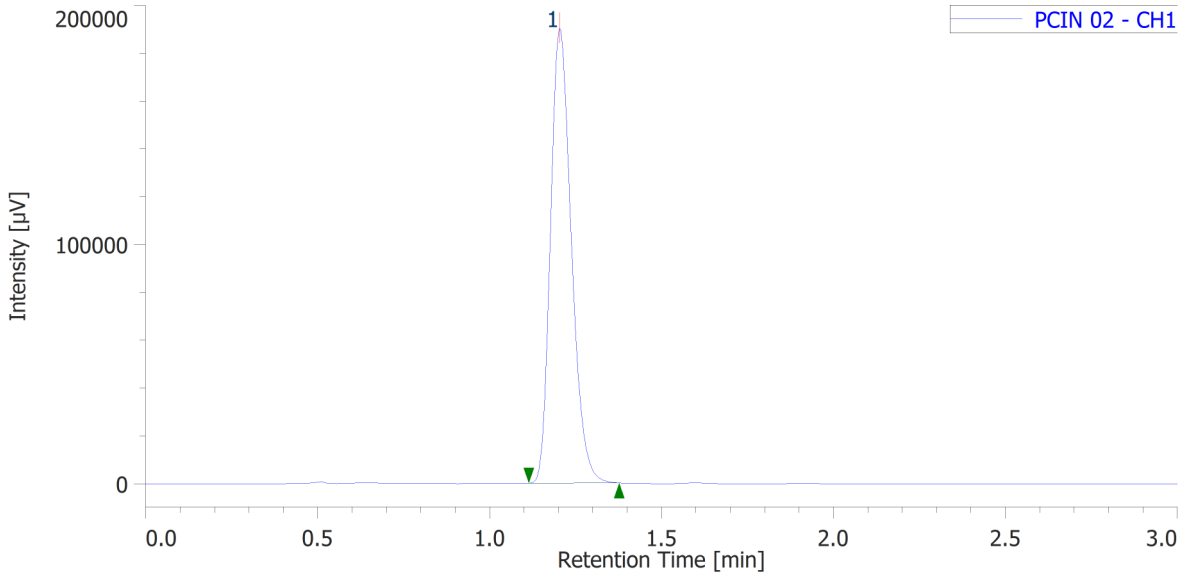

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:07:47
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:03:15
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.203	801013	190182	100.000	100.000	N/A	1912	N/A	1.259	

Creator Administrator
Reviewer
Approver

Chromatogram

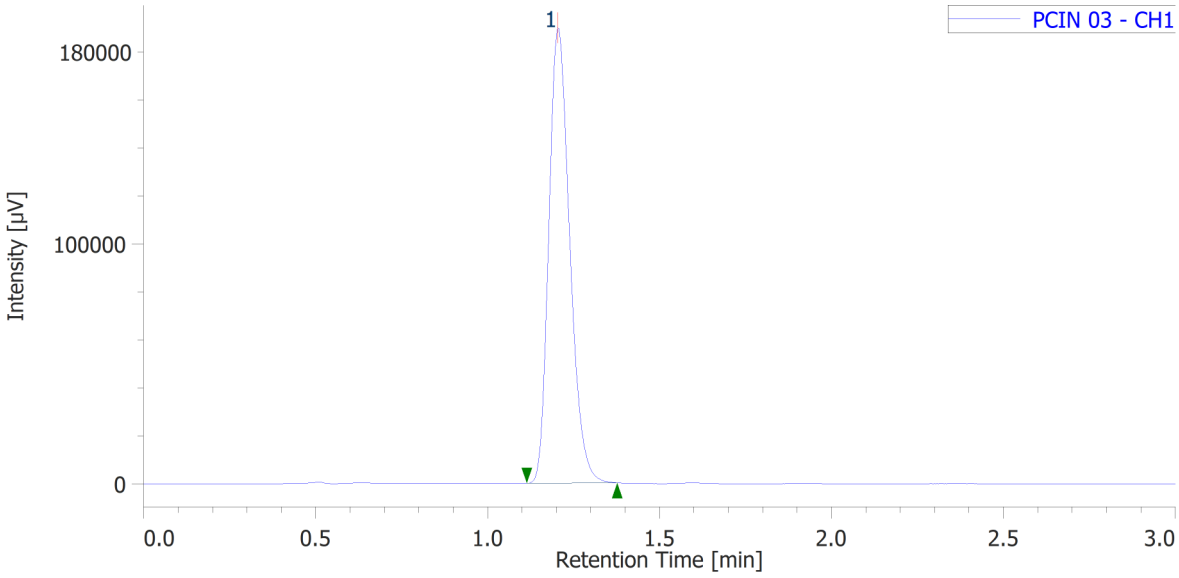

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:13:17
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:07:26
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.203	801982	189629	100.000	100.000	N/A	1899	N/A	1.282	

Creator Administrator
Reviewer
Approver

Chromatogram

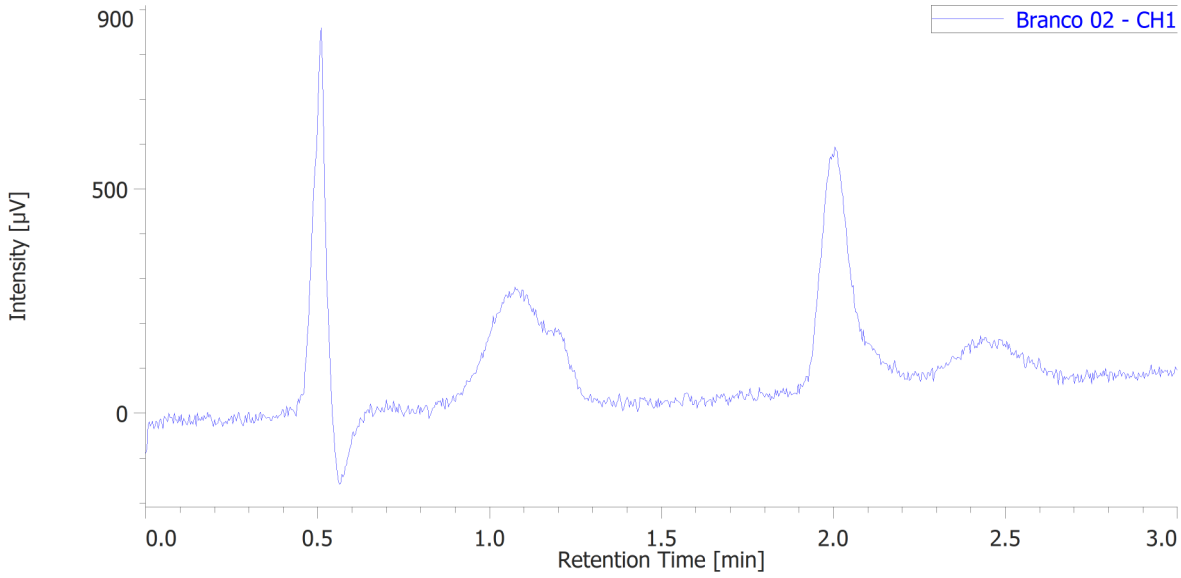


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:18:45
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:11:35
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

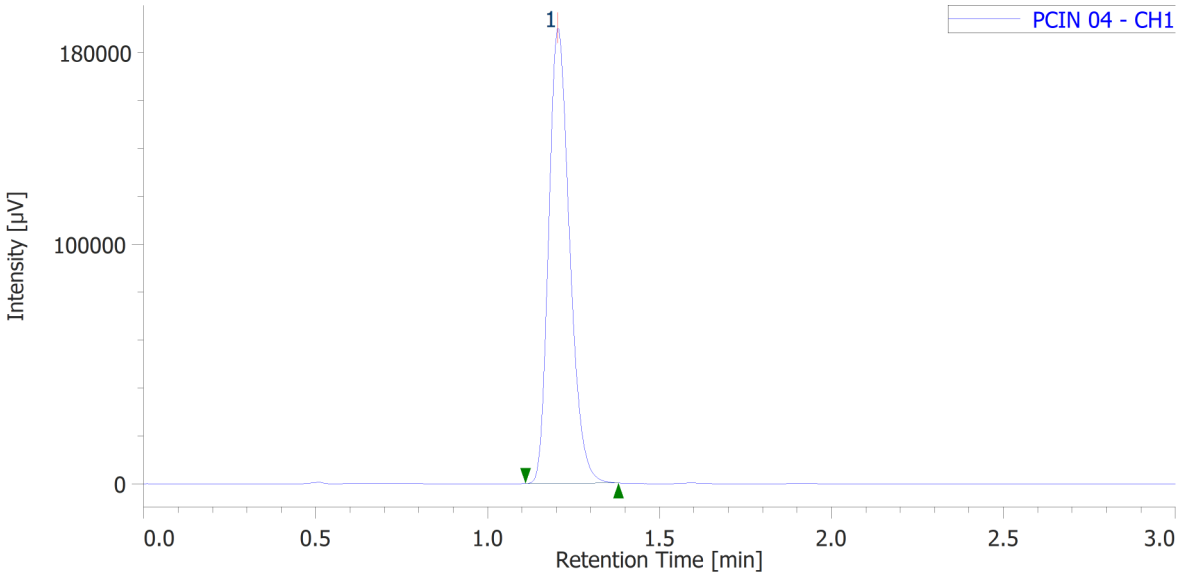

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:19:17
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:15:46
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.203	803584	189943	100.000	100.000	N/A	1902	N/A	1.276	

Creator Administrator
Reviewer
Approver

Chromatogram

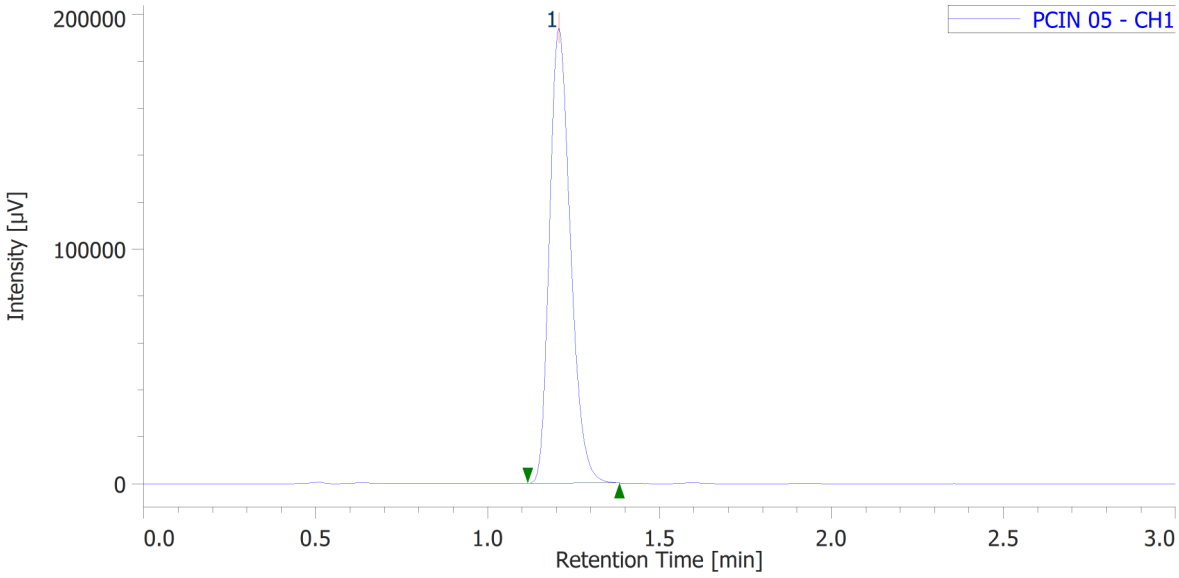

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:24:05
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:19:57
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	820950	193915	100.000	100.000	N/A	1908	N/A	1.261	

Creator Administrator
Reviewer
Approver

Chromatogram

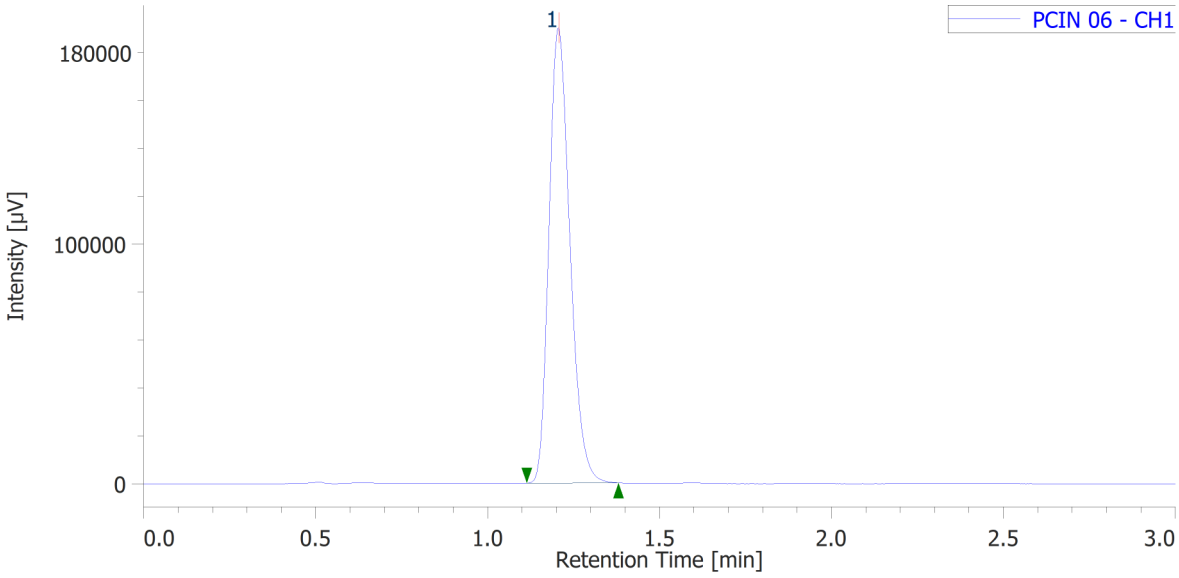

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:28:27
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:24:08
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	803665	189986	100.000	100.000	N/A	1911	N/A	1.221	

Creator Administrator
Reviewer
Approver

Chromatogram

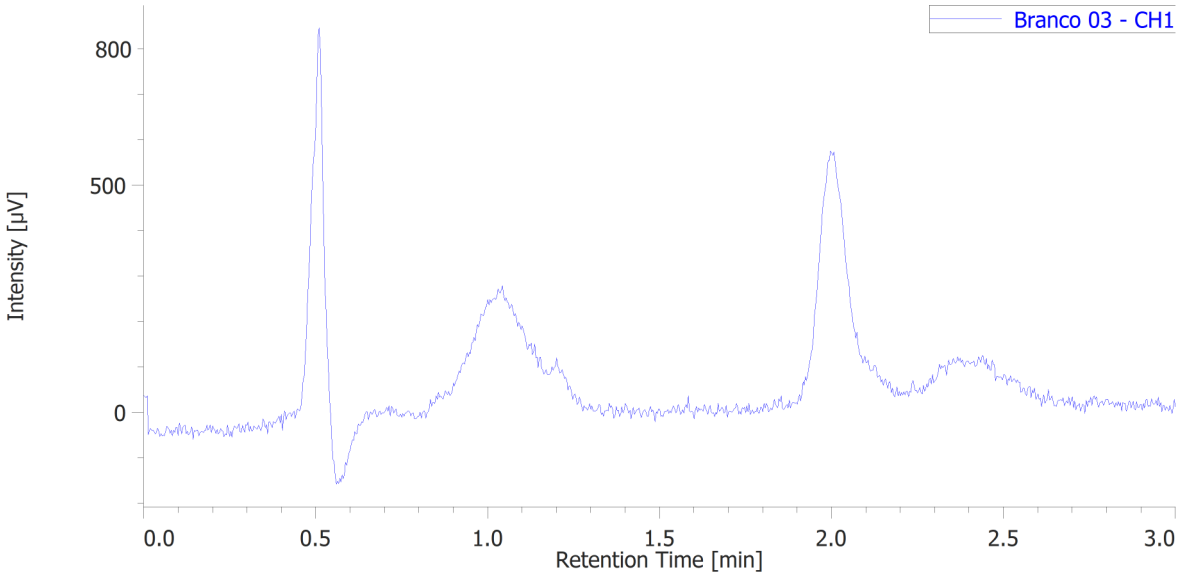


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2025 14:31:58
Description	
HPLC System Name	HPLC_0005
Injection Date	19/08/2025 14:28:19
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

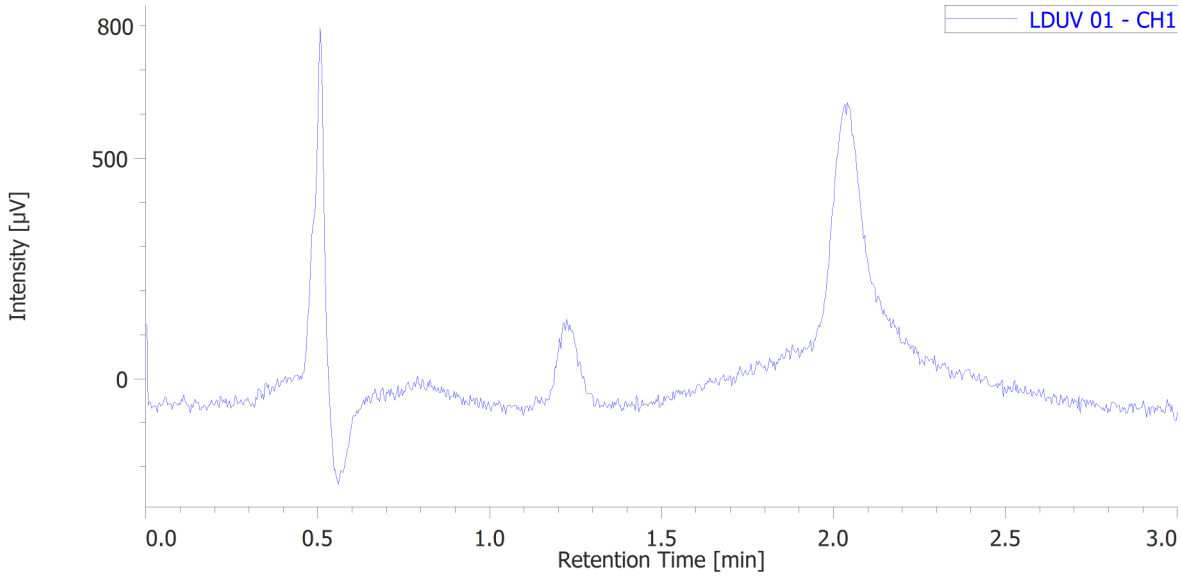


Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:55
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 08:39:31
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

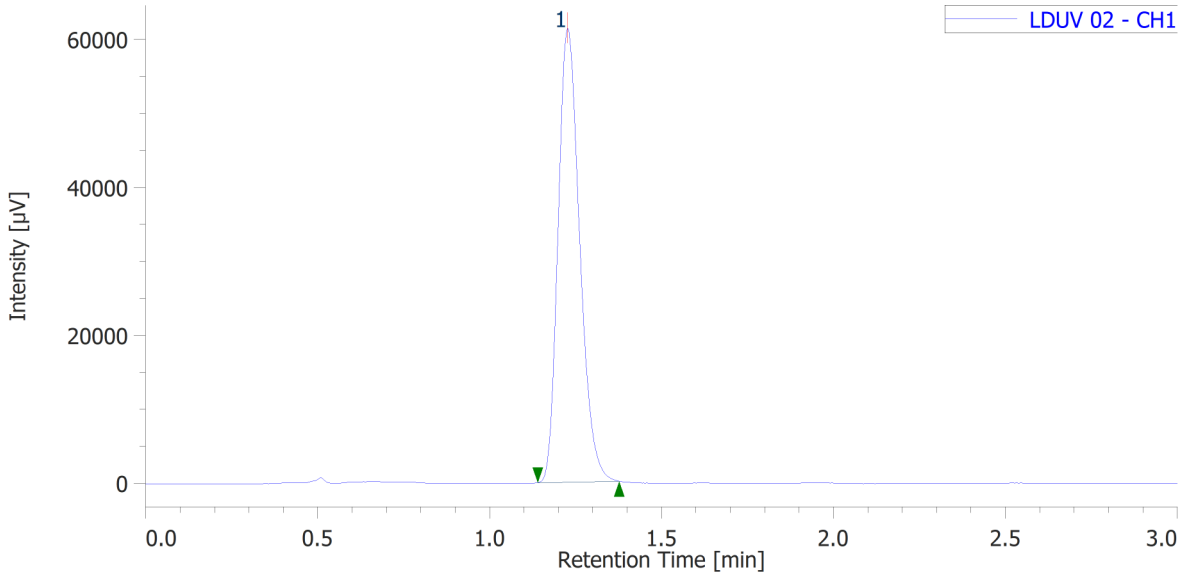

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:55
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 08:43:44
Volume	10.0 [µL]
Sample #	5
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.227	267600	61355	100.000	100.000	N/A	1847	N/A	1.253	

Creator Administrator
Reviewer
Approver

Chromatogram

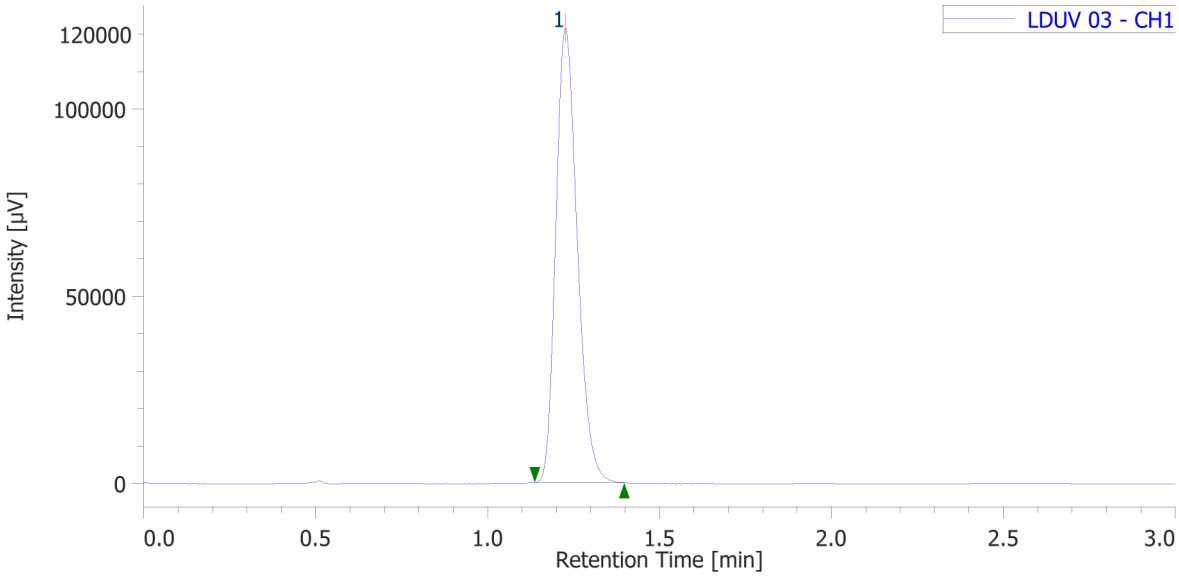

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:55
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 08:47:55
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.227	526584	121407	100.000	100.000	N/A	1870	N/A	1.232	

Creator Administrator
Reviewer
Approver

Chromatogram

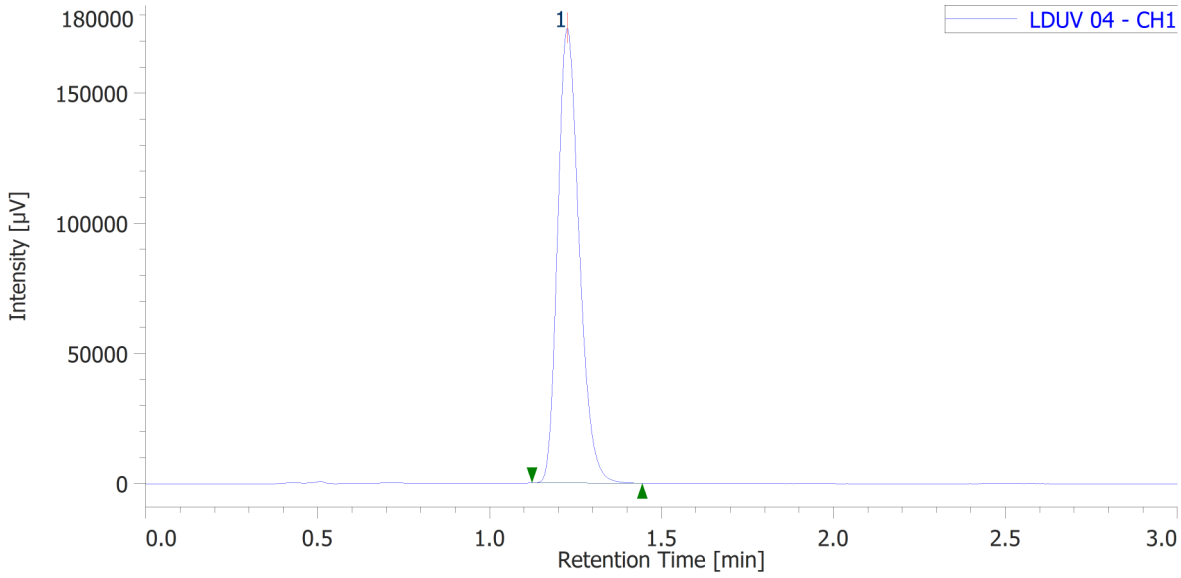

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:55
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 08:52:09
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.227	758950	174717	100.000	100.000	N/A	1876	N/A	1.227	

Creator Administrator
Reviewer
Approver

Chromatogram

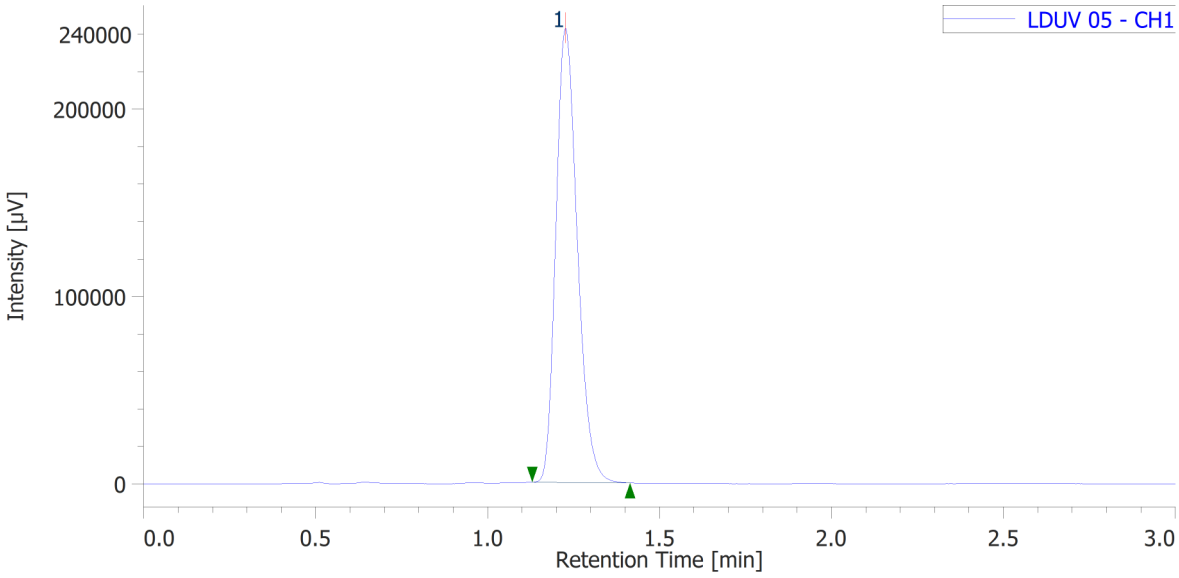

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 09:42:55
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 08:56:22
Volume	10.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.227	1051445	242518	100.000	100.000	N/A	1877	N/A	1.235	

Creator Administrator
Reviewer
Approver

Chromatogram

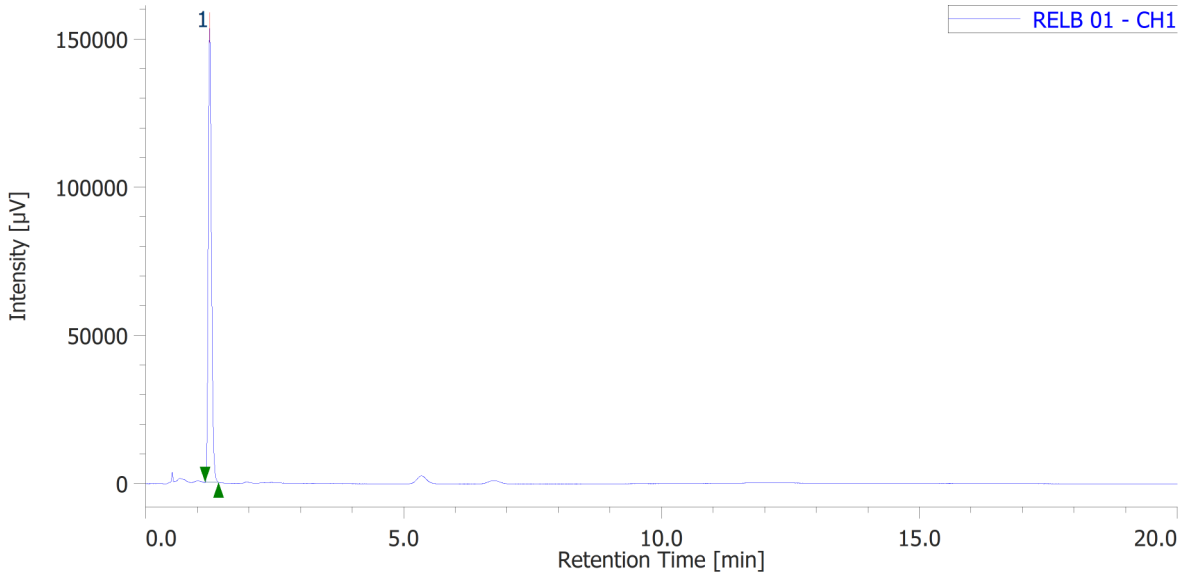

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 12:51:05
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:00:43
Volume	20.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.237	665171	153210	100.000	100.000	N/A	1901	N/A	1.296	

Creator Administrator
Reviewer
Approver

Chromatogram

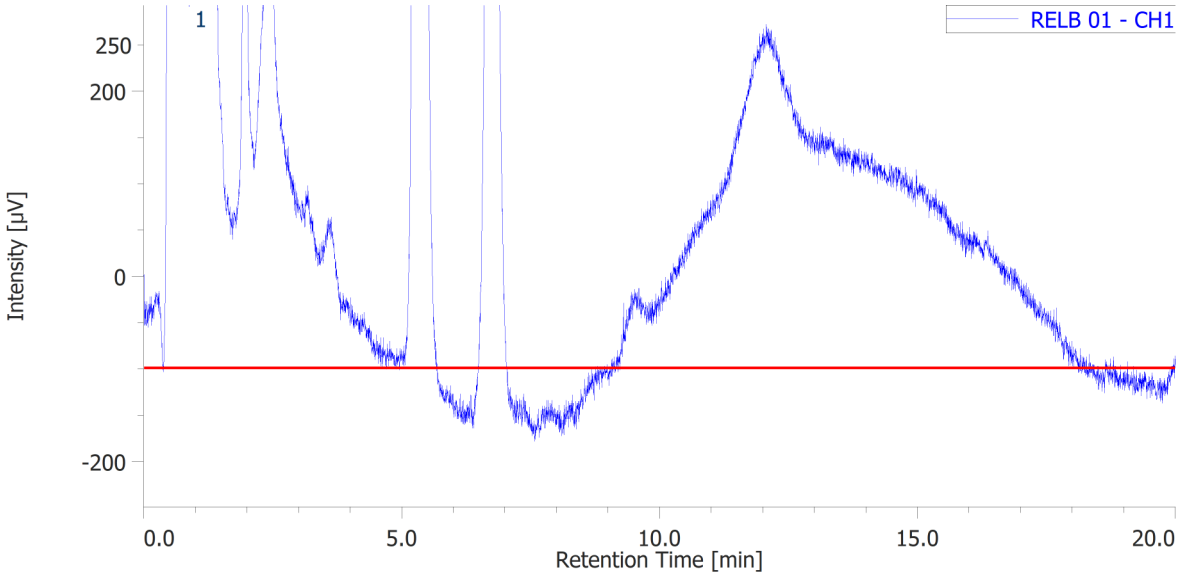


Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 12:51:05
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:00:43
Volume	20.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.237	665171	153210	100.000	100.000	N/A	1901	N/A	1.296	

Creator Administrator
Reviewer
Approver

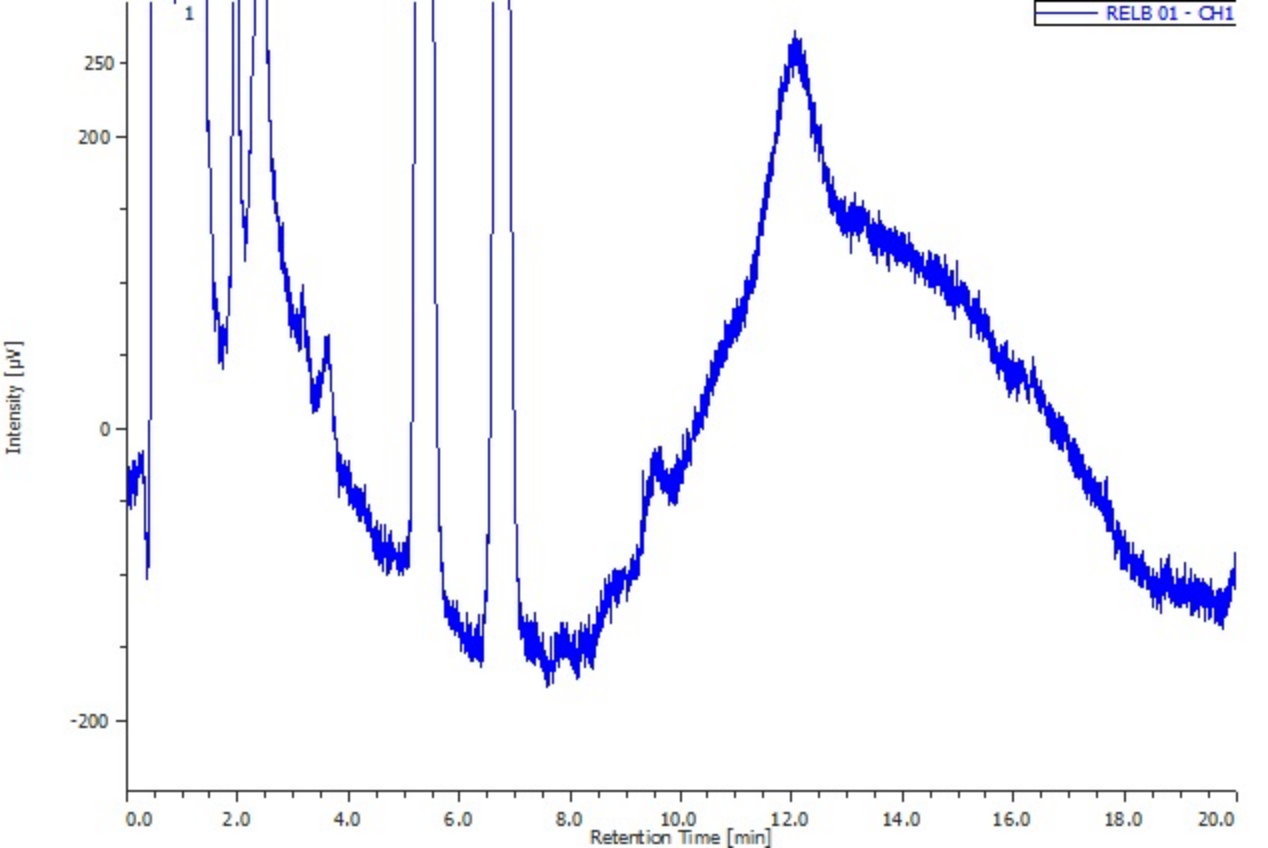
RELB 01 - CH1
1
250
200
0
-200
Intensity [µV]
0.0
2.0
4.0
6.0
8.0
10.0
12.0
14.0
16.0
18.0
20.0
Retention Time [min]

Chromatogram

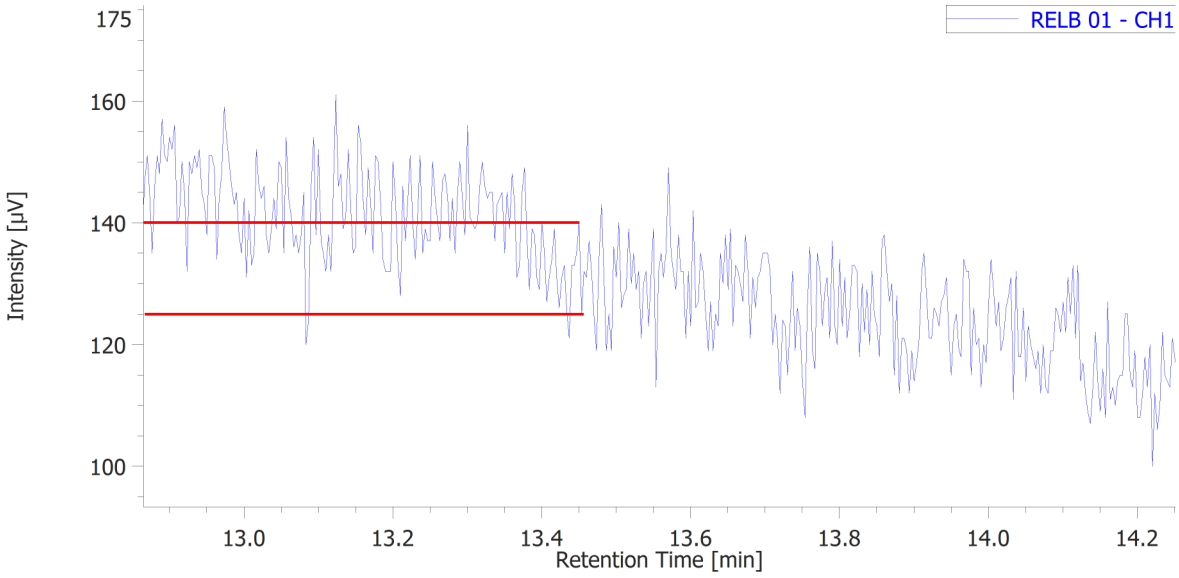


Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 12:51:05
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:00:43
Volume	20.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.237	665171	153210	100.000	100.000	N/A	1901	N/A	1.296	

Creator Administrator
Reviewer
Approver

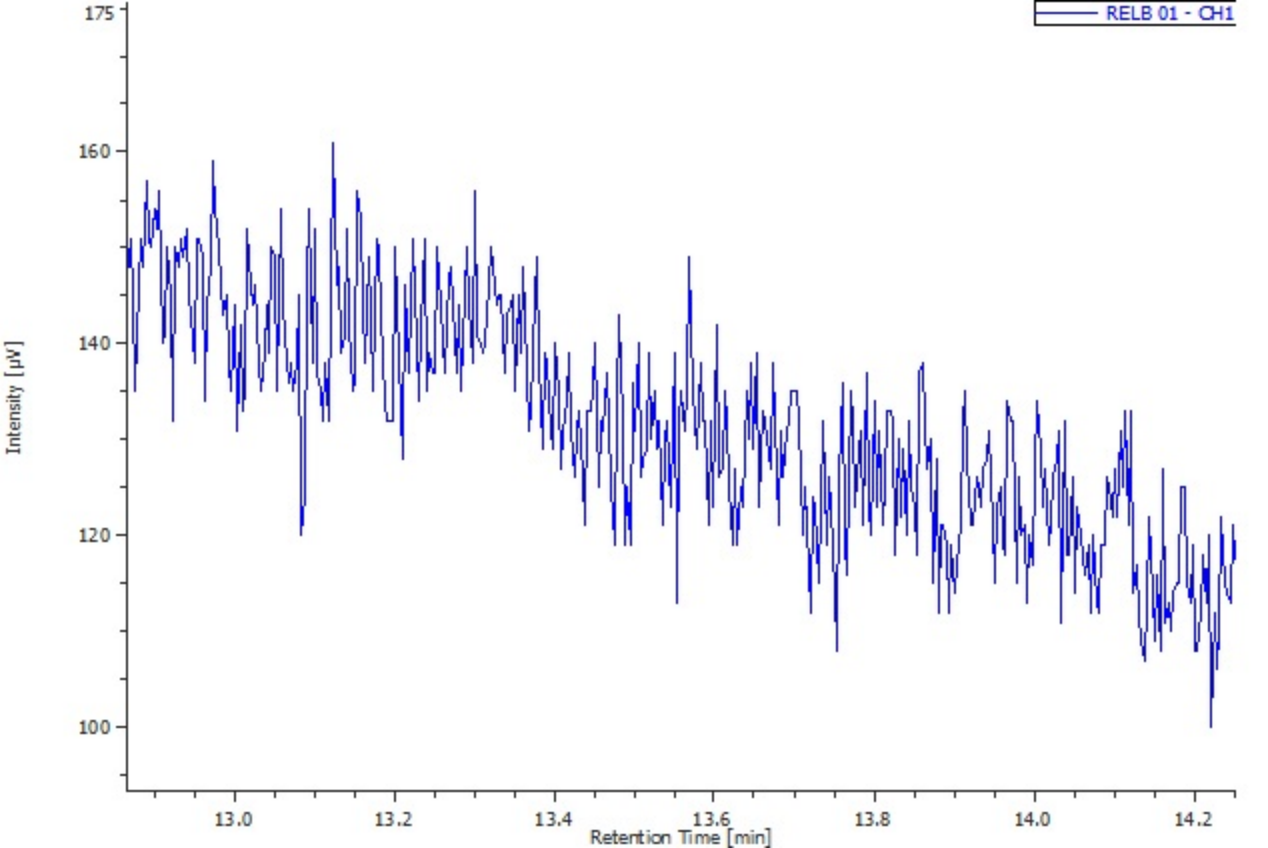
RELB 01 - CH1
175
160
140
120
100
Intensity [µV]
13.0
13.2
13.4
13.6
13.8
14.0
14.2
Retention Time [min]

Chromatogram

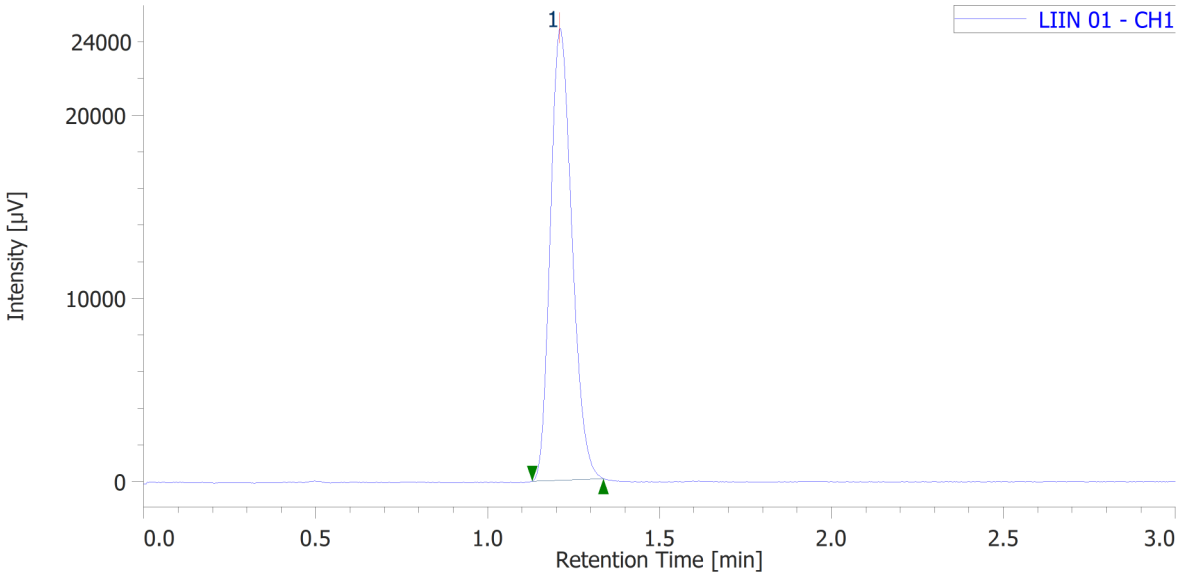

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 09:42:56
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:21:54
Volume	0.1 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.210	107439	24659	100.000	100.000	N/A	1765	N/A	1.225	

Creator Administrator
Reviewer
Approver

Chromatogram

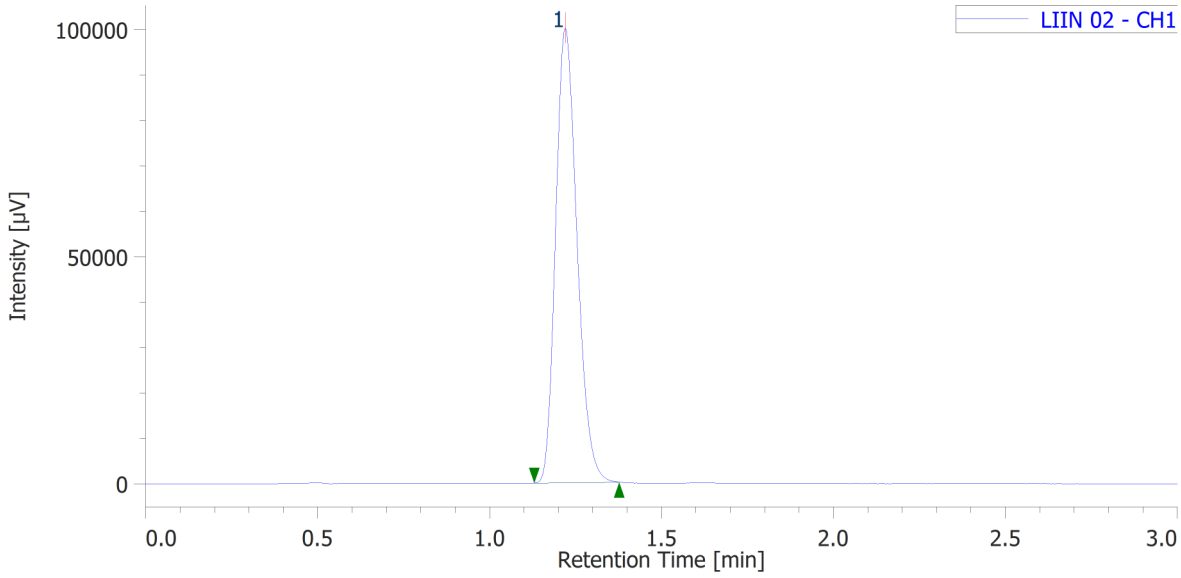

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:56
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:26:08
Volume	5.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.220	432354	100119	100.000	100.000	N/A	1850	N/A	1.224	

Creator Administrator
Reviewer
Approver

Chromatogram

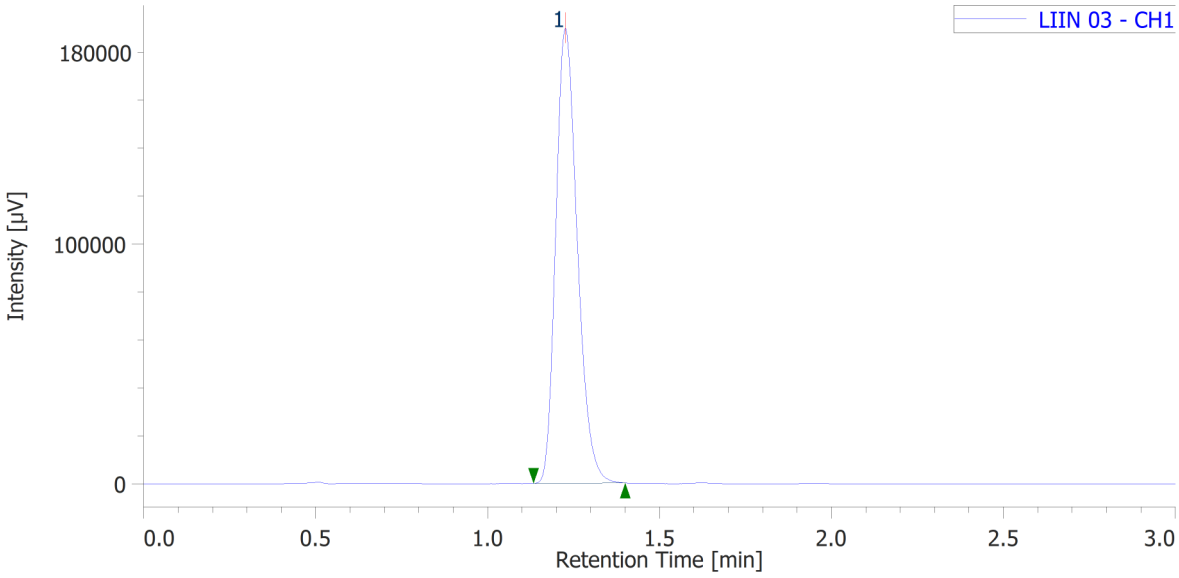

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:56
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:30:24
Volume	10.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.227	824677	189826	100.000	100.000	N/A	1868	N/A	1.235	

Creator Administrator
Reviewer
Approver

Chromatogram

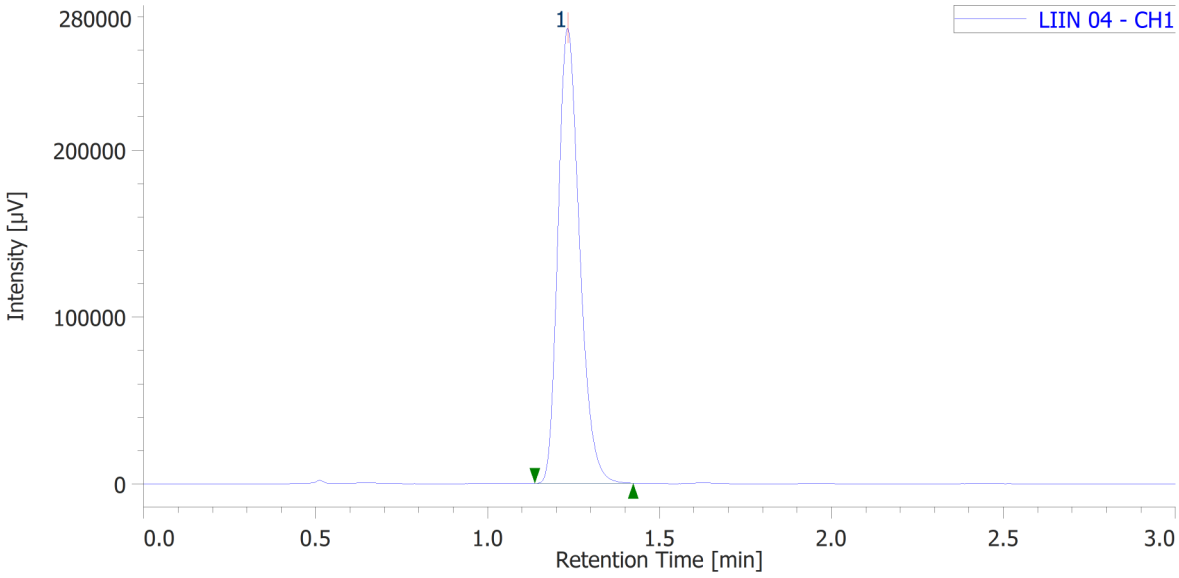

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:57
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:34:42
Volume	15.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.233	1185880	272743	100.000	100.000	N/A	1892	N/A	1.239	

Creator Administrator
Reviewer
Approver

Chromatogram

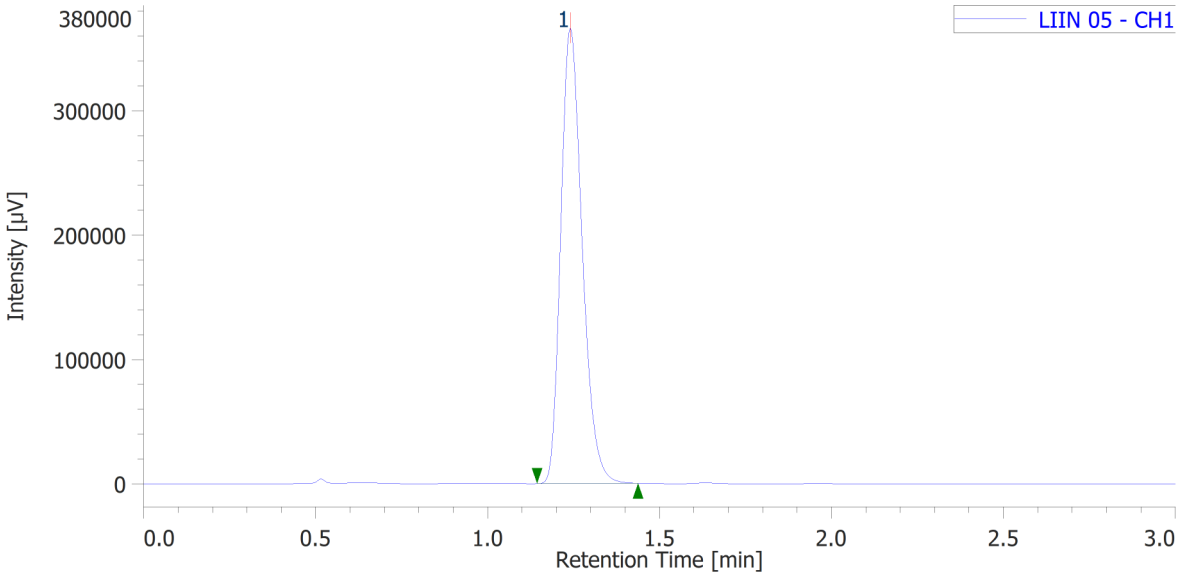

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 09:42:57
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 09:39:03
Volume	20.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação 05
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.240	1581607	366100	100.000	100.000	N/A	1945	N/A	1.267	

Creator Administrator
Reviewer
Approver

Chromatogram

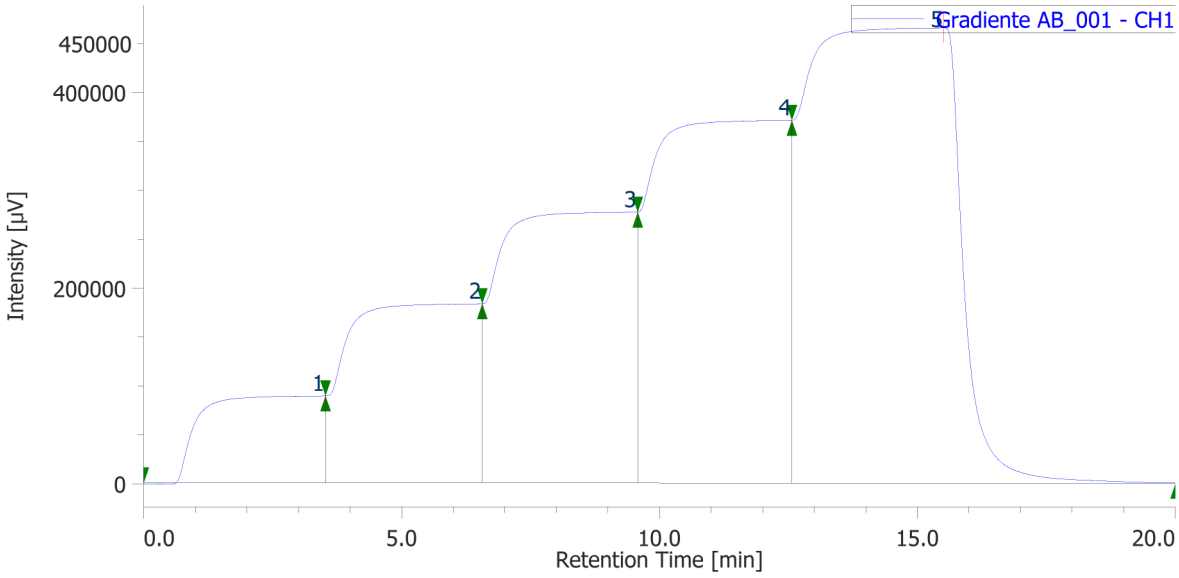

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 13:06:45
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 10:22:54
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.517	13610070	88769	5.464	6.418	N/A	N/A	N/A	N/A	
2	40%	1	6.553	30889689	182905	12.401	13.224	N/A	N/A	N/A	N/A	
3	60%	1	9.560	47817781	276499	19.197	19.991	N/A	N/A	N/A	N/A	
4	80%	1	12.557	64136469	370243	25.748	26.768	N/A	N/A	N/A	N/A	
5	100%	1	15.500	92641922	464731	37.191	33.600	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

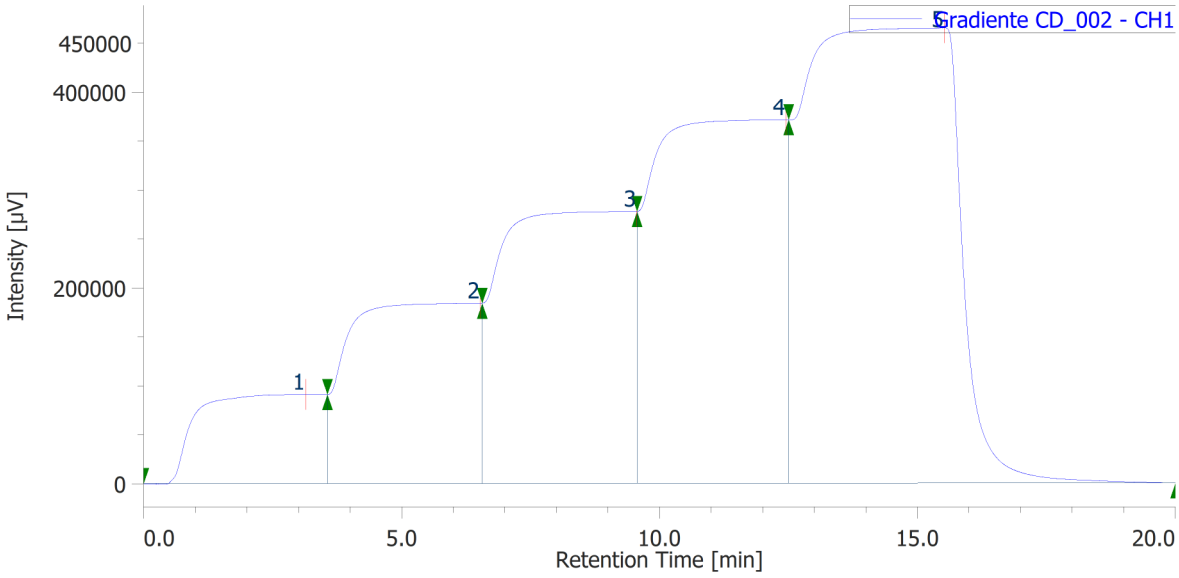

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 13:06:46
Description	
HPLC System Name	HPLC_0005
Injection Date	20/08/2025 10:43:58
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.140	14519937	90807	5.798	6.545	N/A	N/A	N/A	N/A	
2	40%	1	6.523	30894919	183772	12.338	13.246	N/A	N/A	N/A	N/A	
3	60%	1	9.557	47702832	277506	19.050	20.001	N/A	N/A	N/A	N/A	
4	80%	1	12.447	63305790	370800	25.281	26.726	N/A	N/A	N/A	N/A	
5	100%	1	15.523	93985850	464542	37.533	33.482	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver