
Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 15:55:39
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 15:26:31
Volume	10.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	LDIR
Control Method	Linearidade RI
Peak ID Table	Glicerol RI
Calibration Method	
Additional Information	
Column Info	

Chromatogram

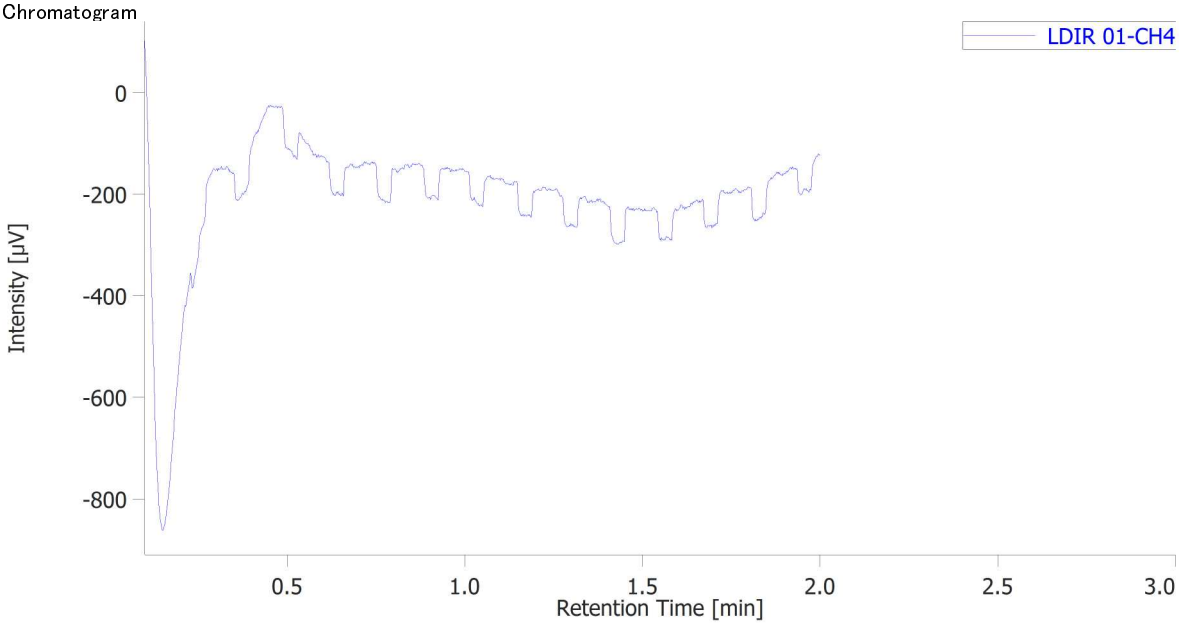


Peak Information - No data.

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 15:55:39
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 15:29:23
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	LDIR
Control Method	Linearidade RI
Peak ID Table	Glicerol RI
Calibration Method	
Additional Information	
Column Info	

Chromatogram

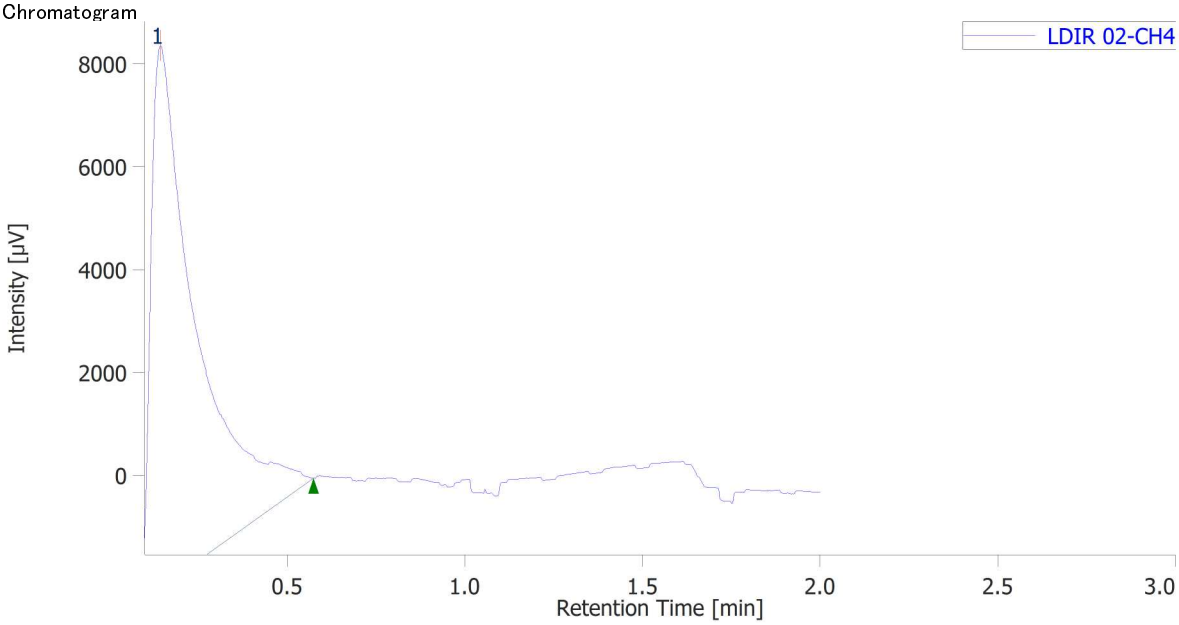

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.145	94153	10526	100.000	100.000	N/A	9	N/A	4.099	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 15:55:39
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 15:32:15
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	LDIR
Control Method	Linearidade RI
Peak ID Table	Glicerol RI
Calibration Method	
Additional Information	
Column Info	

Chromatogram

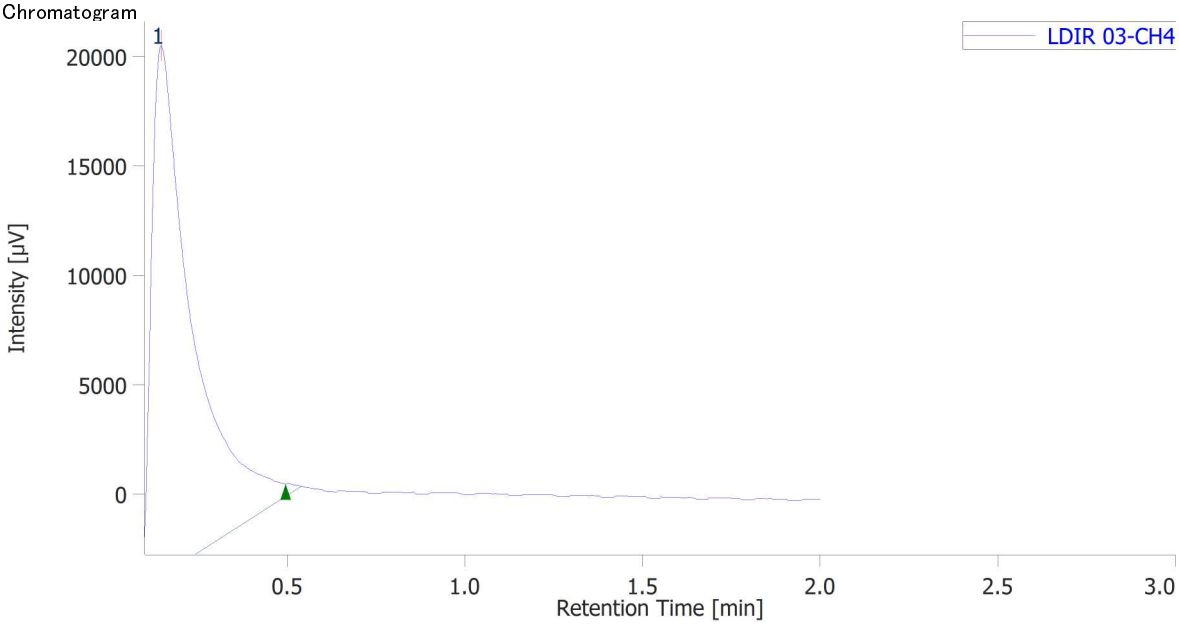

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.147	194582	24228	100.000	100.000	N/A	11	N/A	3.534	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 15:55:39
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 15:35:07
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	LDIR
Control Method	Linearidade RI
Peak ID Table	Glicerol RI
Calibration Method	
Additional Information	
Column Info	

Chromatogram

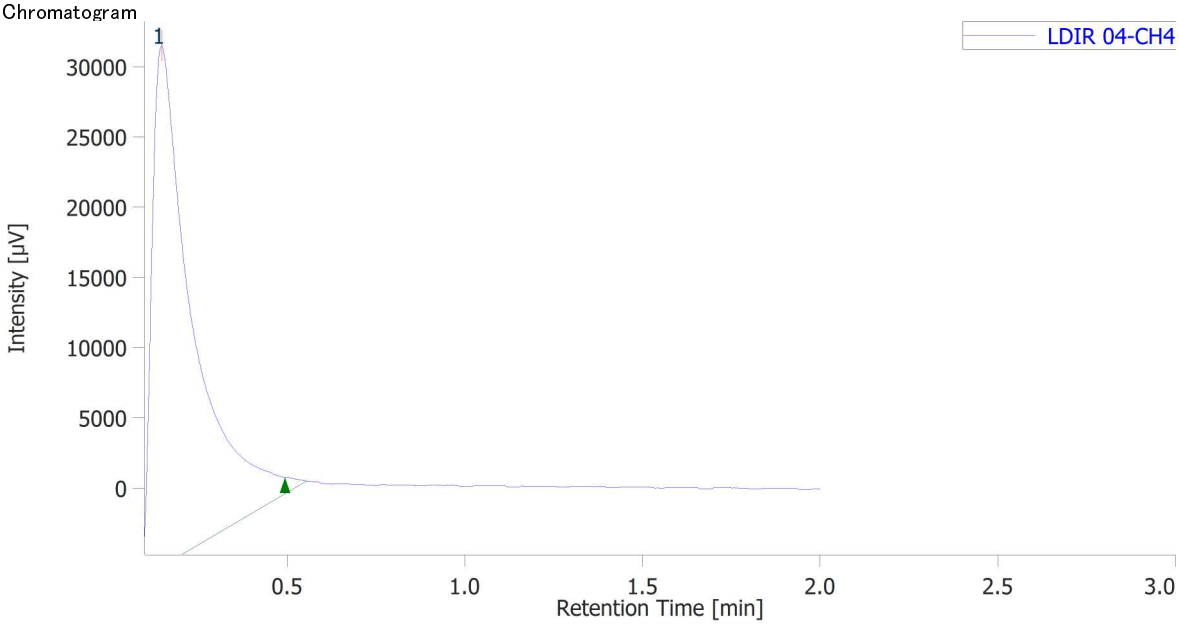

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.148	298297	37061	100.000	100.000	N/A	11	N/A	3.556	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 15:55:39
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 15:37:59
Volume	10.0 [µL]
Sample #	5
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	LDIR
Control Method	Linearidade RI
Peak ID Table	Glicerol RI
Calibration Method	
Additional Information	
Column Info	

Chromatogram

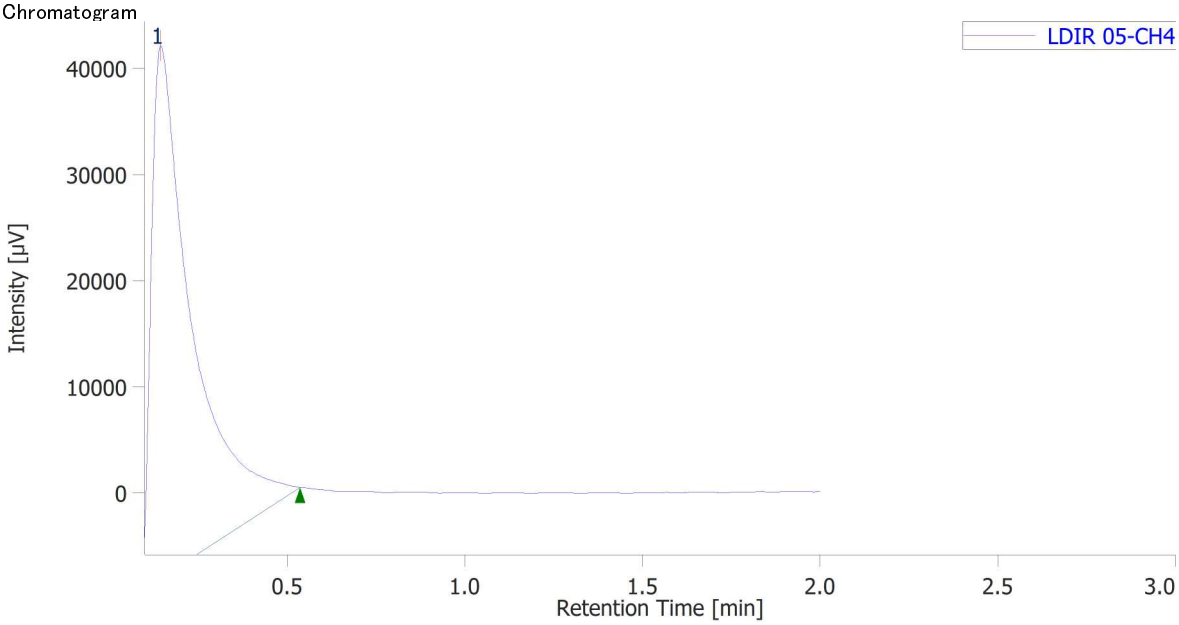

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	4	0.145	404496	50152	100.000	100.000	N/A	11	N/A	3.625	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 14:05:42
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 14:02:38
Volume	1.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

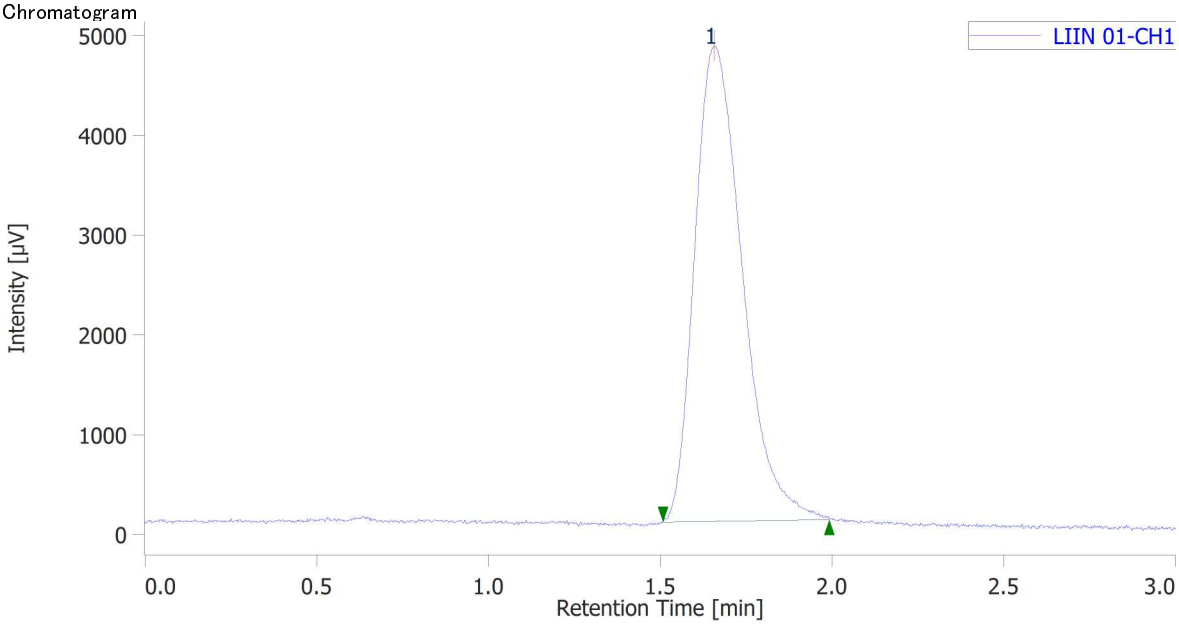


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.657	45839	4765	100.000	100.000	N/A	694	N/A	1.411	

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	21/08/2025 14:09:28
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 14:06:25
Volume	2.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

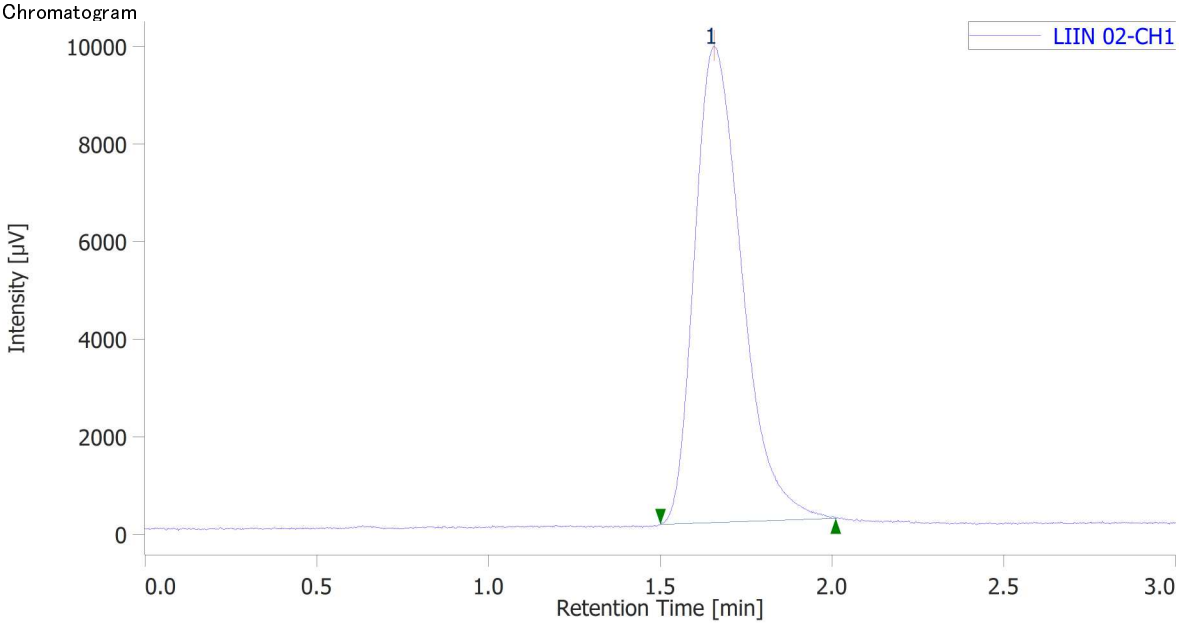

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.657	93364	9765	100.000	100.000	N/A	706	N/A	1.411	

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 14:13:22
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 14:10:18
Volume	4.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

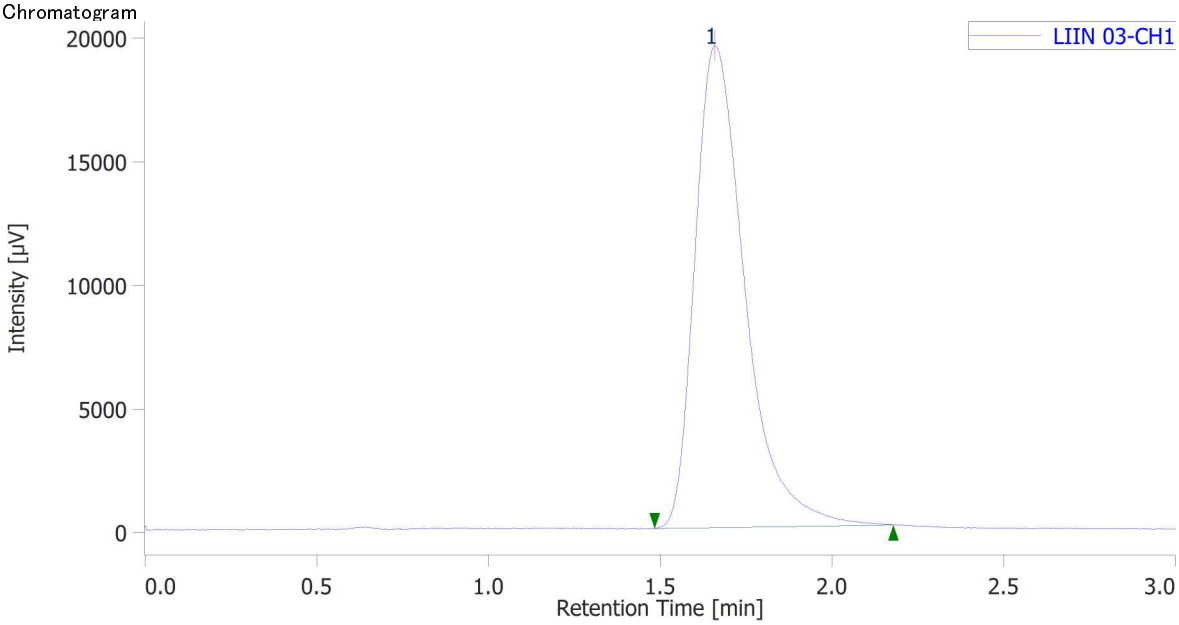


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.658	197185	19483	100.000	100.000	N/A	674	N/A	1.543	

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	21/08/2025 14:17:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 14:14:11
Volume	6.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

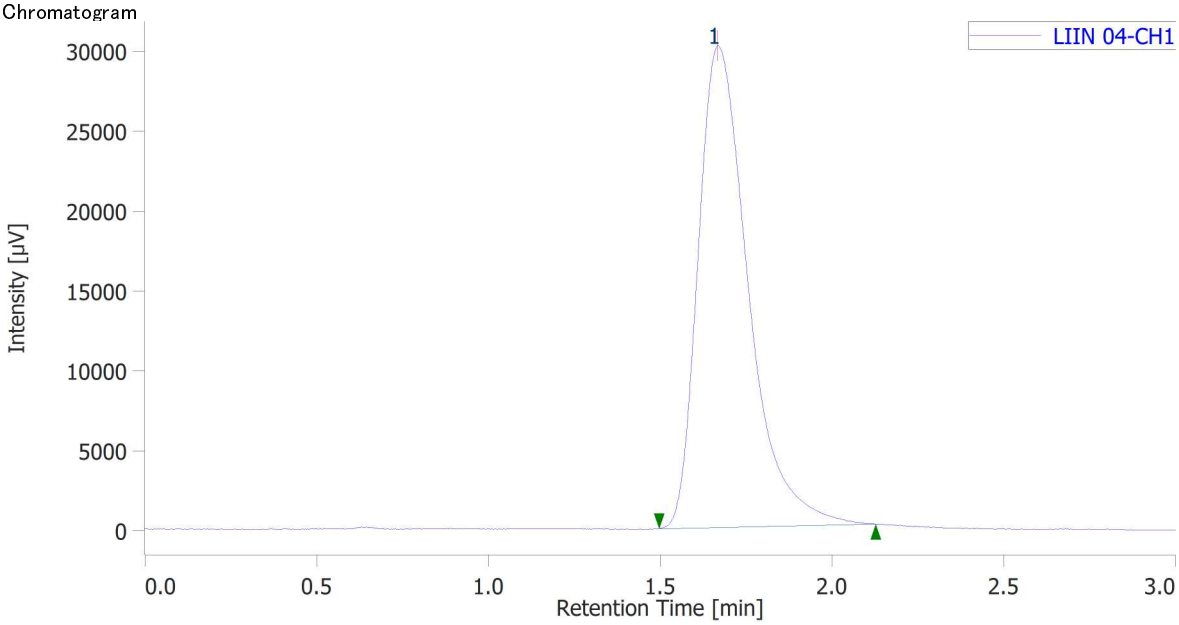

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.667	304881	30128	100.000	100.000	N/A	671	N/A	1.548	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	21/08/2025 14:23:00
Description	
HPLC System Name	HPLC 002 RI
Injection Date	21/08/2025 14:18:06
Volume	8.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

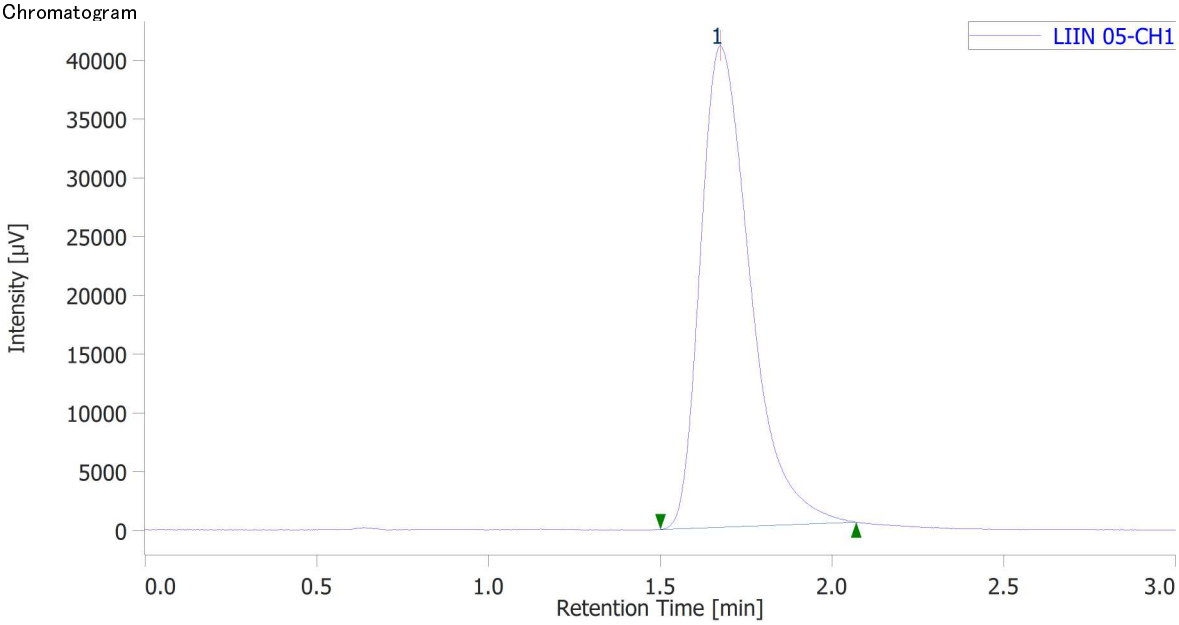


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.675	413160	40937	100.000	100.000	N/A	669	N/A	1.510	

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 14:49:42
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 14:46:38
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

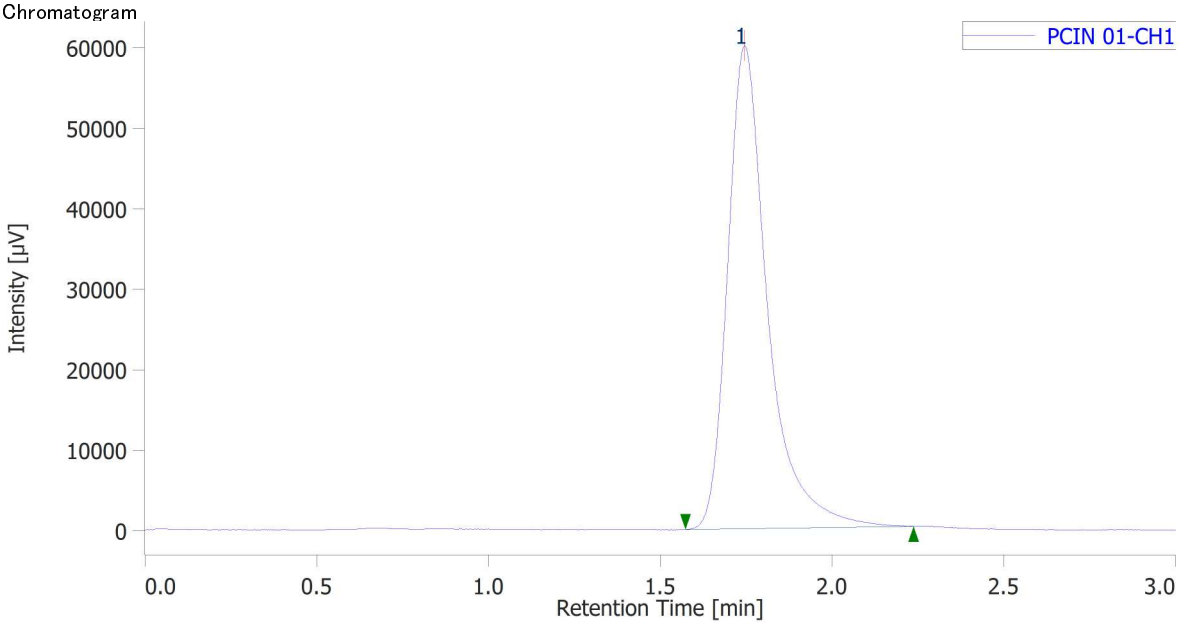


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.745	485983	59999	100.000	100.000	N/A	1282	N/A	1.484	

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 14:53:36
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 14:50:32
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

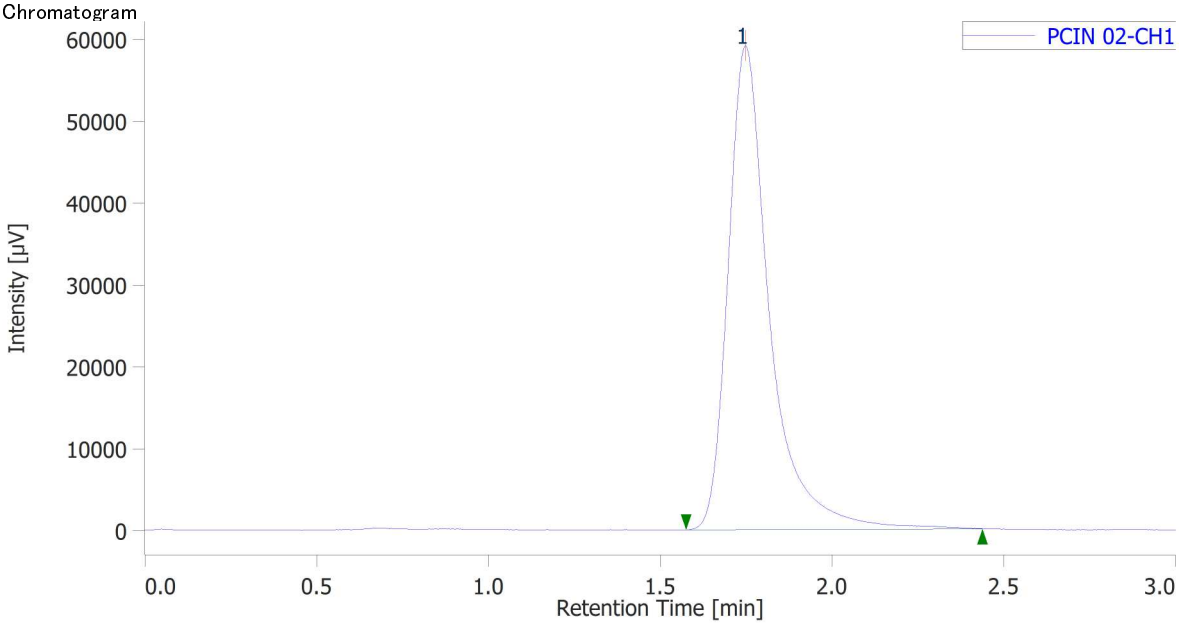


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.748	495335	59044	100.000	100.000	N/A	1244	N/A	1.516	

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 14:57:26
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 14:54:24
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

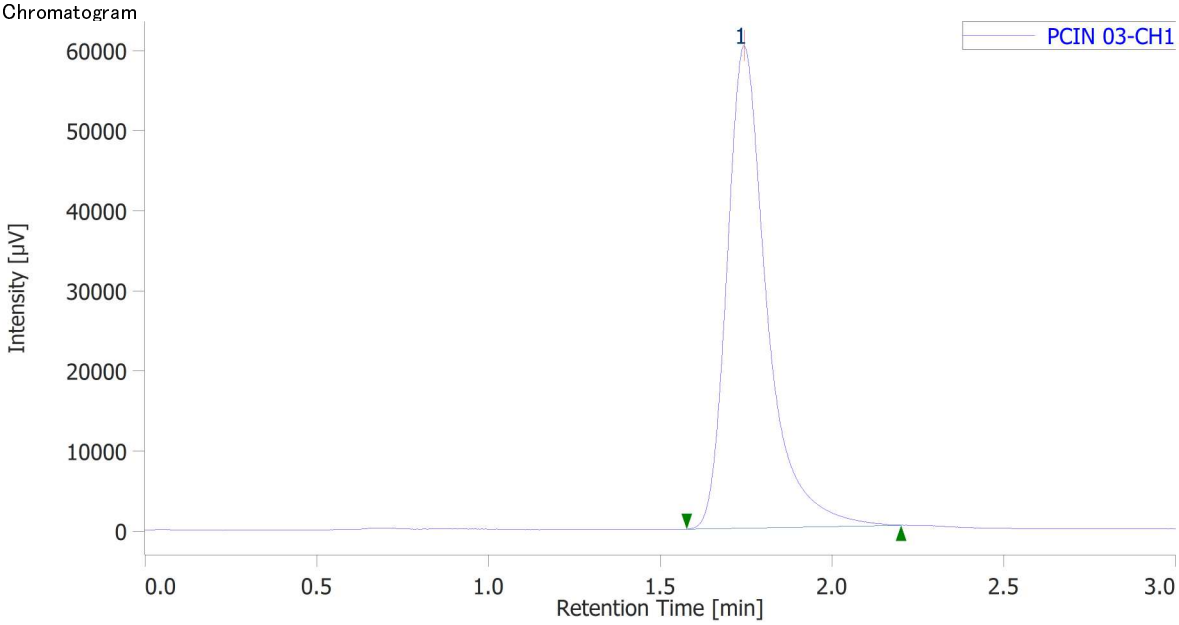

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.743	485949	60182	100.000	100.000	N/A	1276	N/A	1.474	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 15:05:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 15:02:10
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

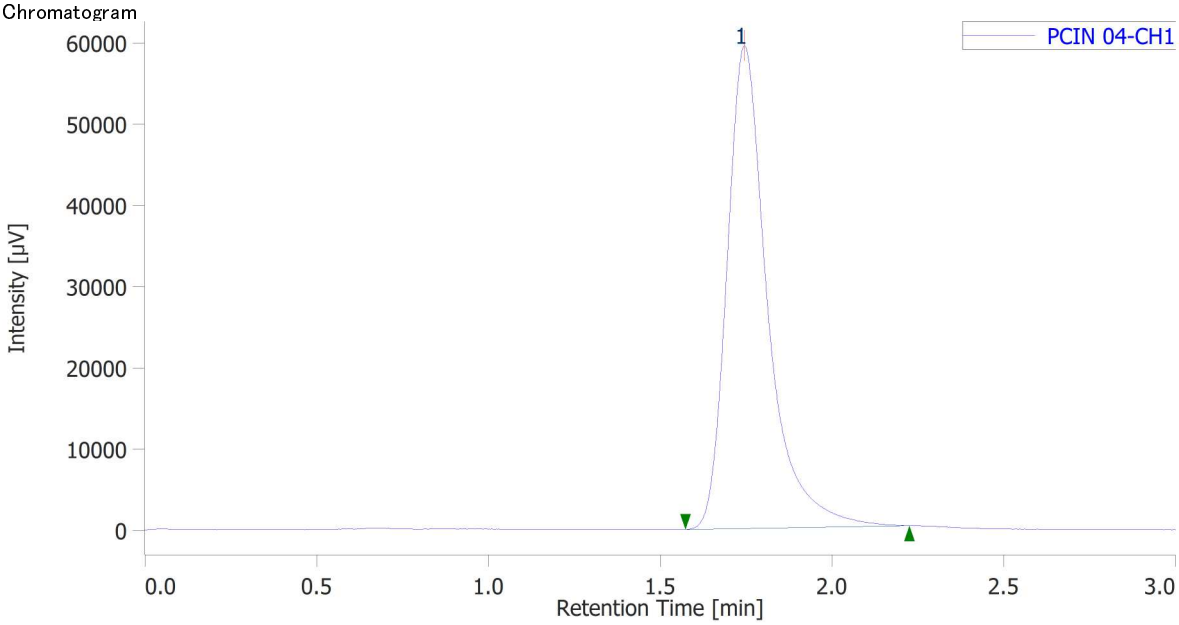

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.745	487849	59379	100.000	100.000	N/A	1229	N/A	1.459	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 15:09:08
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 15:06:04
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

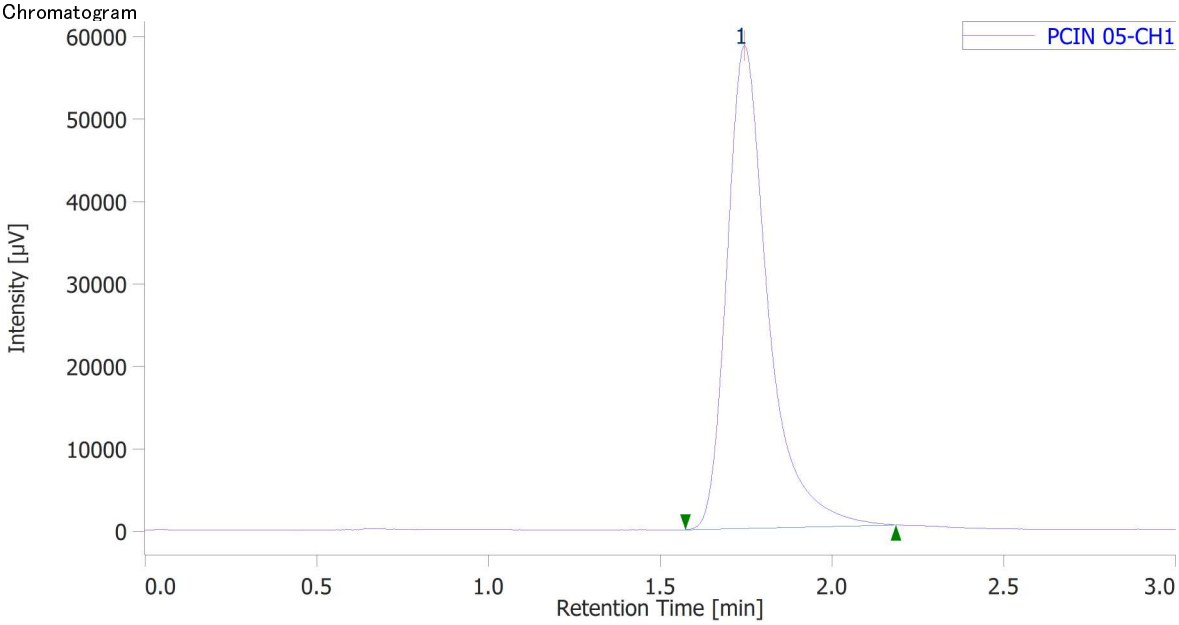


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.745	487961	58535	100.000	100.000	N/A	1197	N/A	1.482	

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 15:13:00
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 15:09:56
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

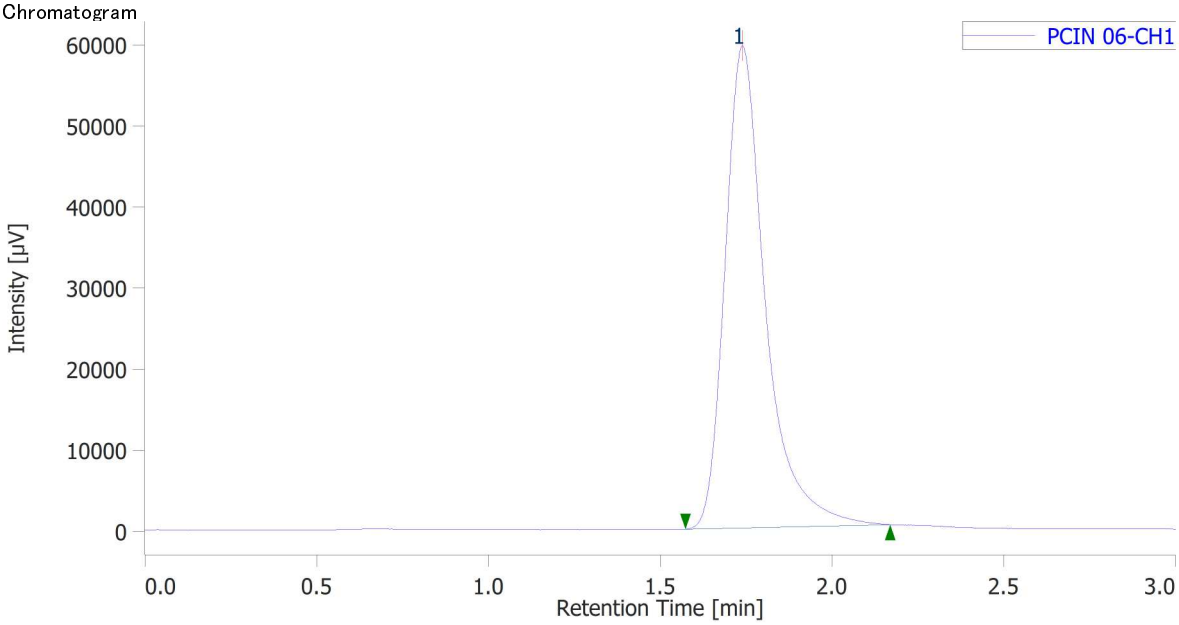

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.738	485993	59461	100.000	100.000	N/A	1225	N/A	1.466	

Creator Administrator
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 14:45:50
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 14:42:46
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

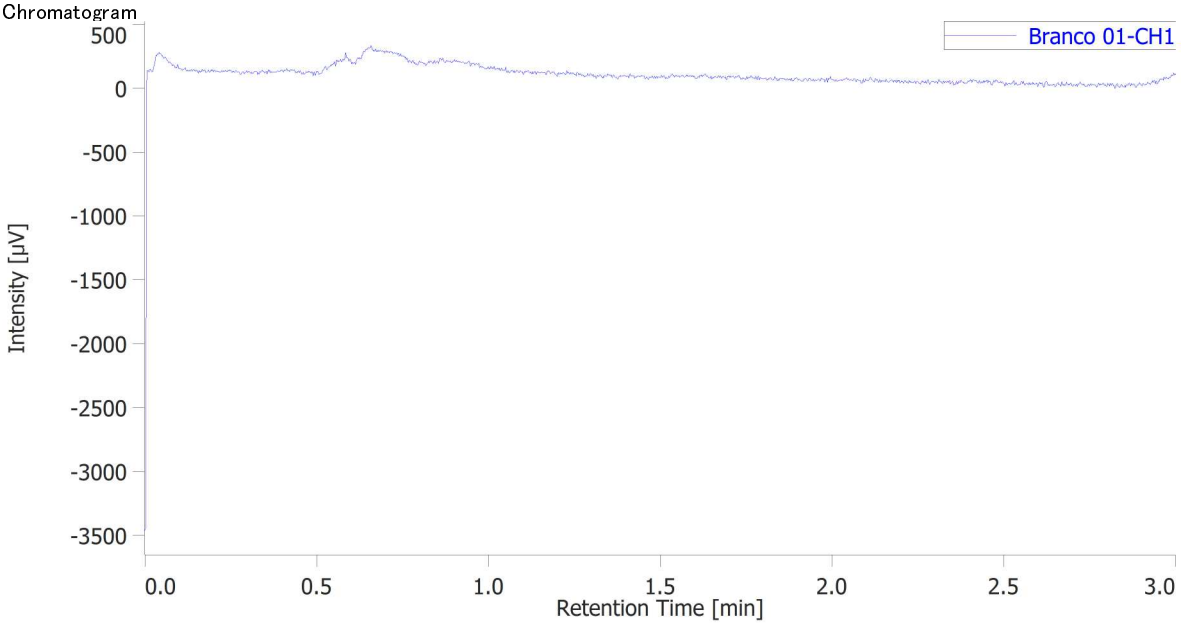


Peak Information - No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	20/08/2025 15:01:22
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 14:58:18
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

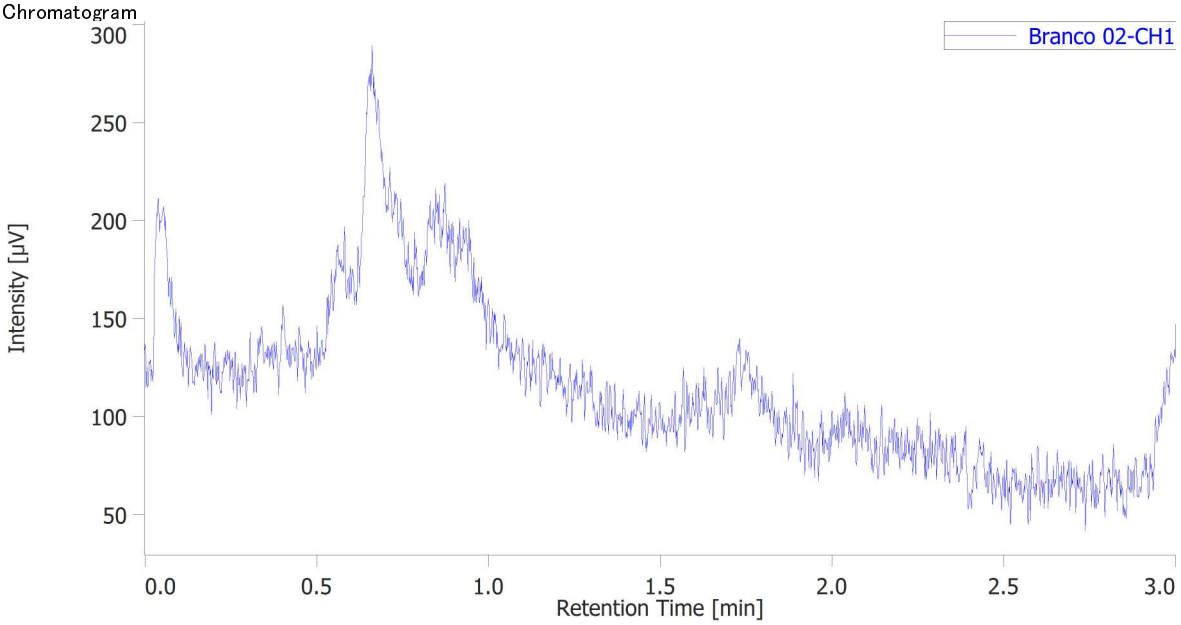


Peak Information - No data.

Creator Administrator
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	20/08/2025 15:16:52
Description	
HPLC System Name	HPLC 002 RI
Injection Date	20/08/2025 15:13:48
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

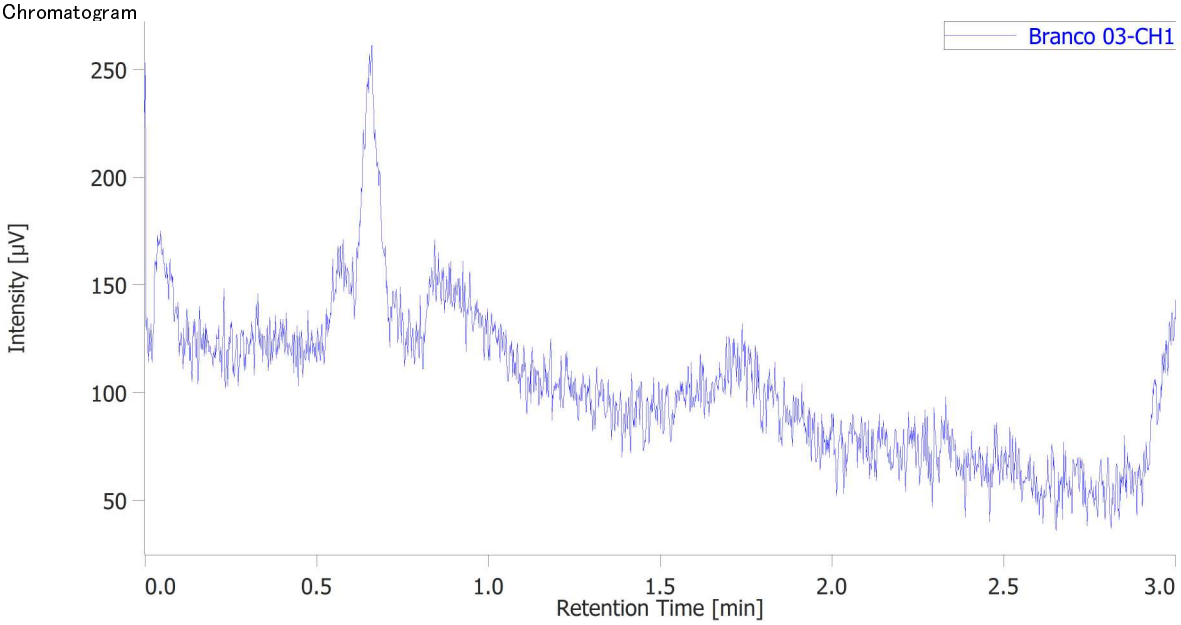

Peak Information - No data.

Creator Administrator
Reviewer
Approver