
Peak Find - EDUV HPLC-0005.jws

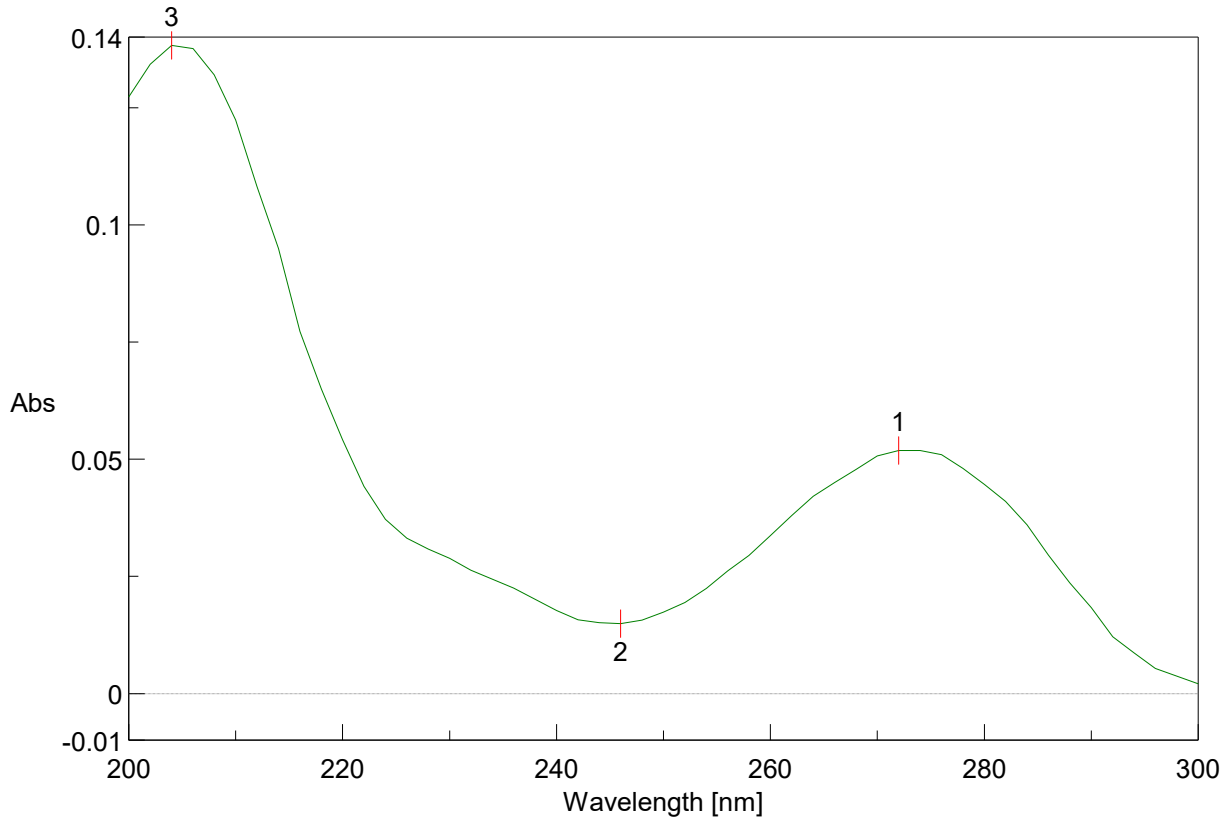

[Comments]

User	Administrator
Workgroup	
Division	
Company	QPack
Creation date	26/08/2024 16:41


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	600 nm	
Data interval	2 nm	
Data points	200	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.051802	2	246	0.014873
3	204	0.138212			

Creation	Administrator
Review	
Approval	

Chromatogram

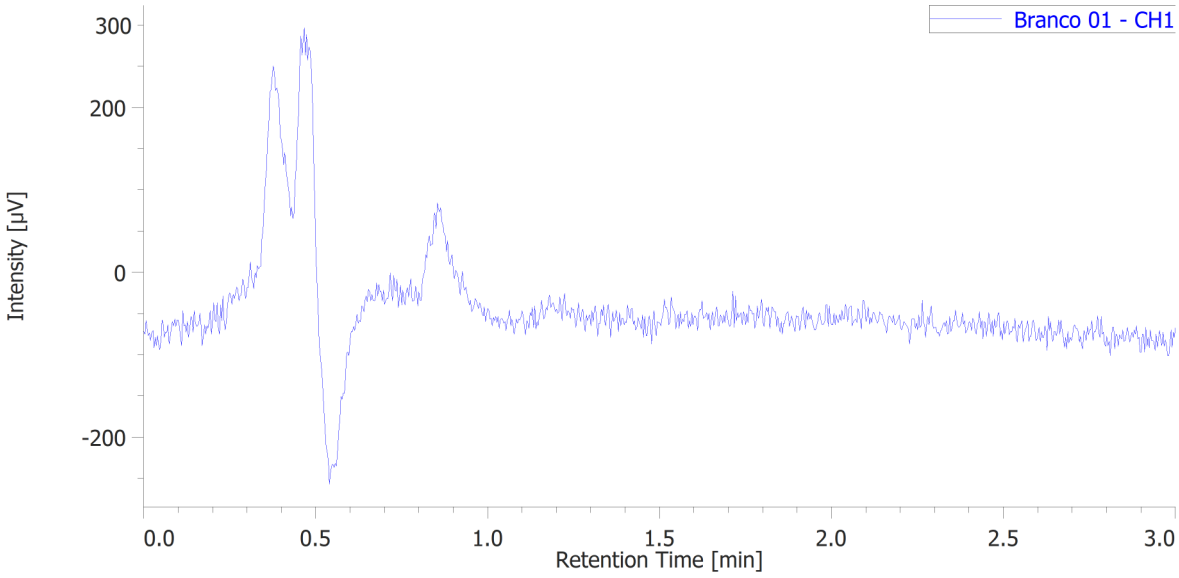


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:56
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 16:46:26
Volume	10.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator	Administrator
Reviewer	
Approver	

Chromatogram

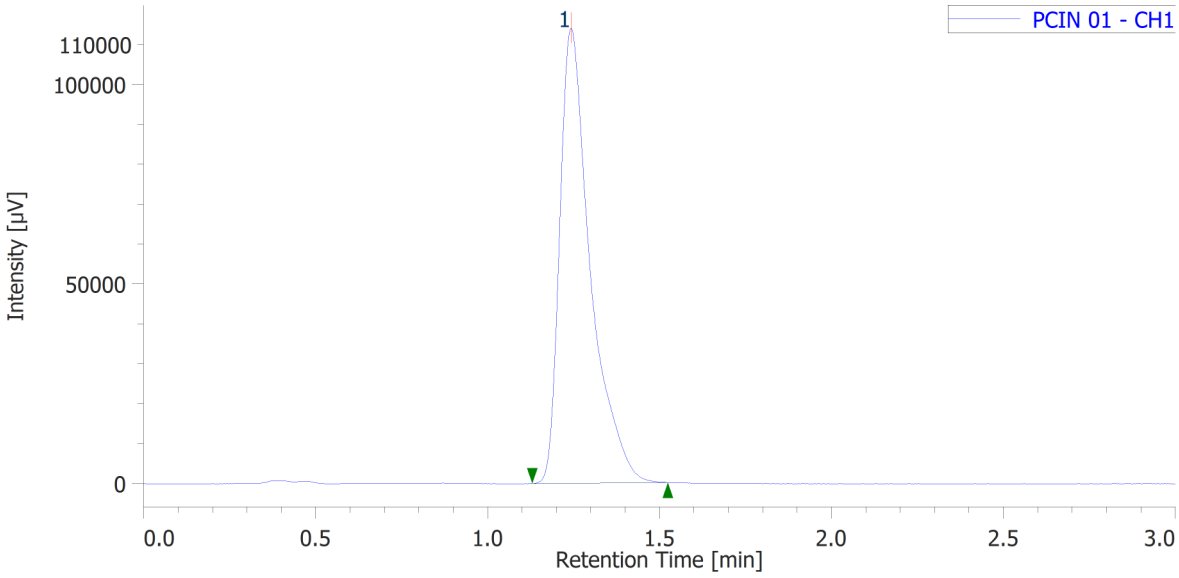

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:57
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 16:50:37
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.243	705176	114043	100.000	100.000	N/A	1105	N/A	1.676	

Creator Administrator
Reviewer
Approver

Chromatogram

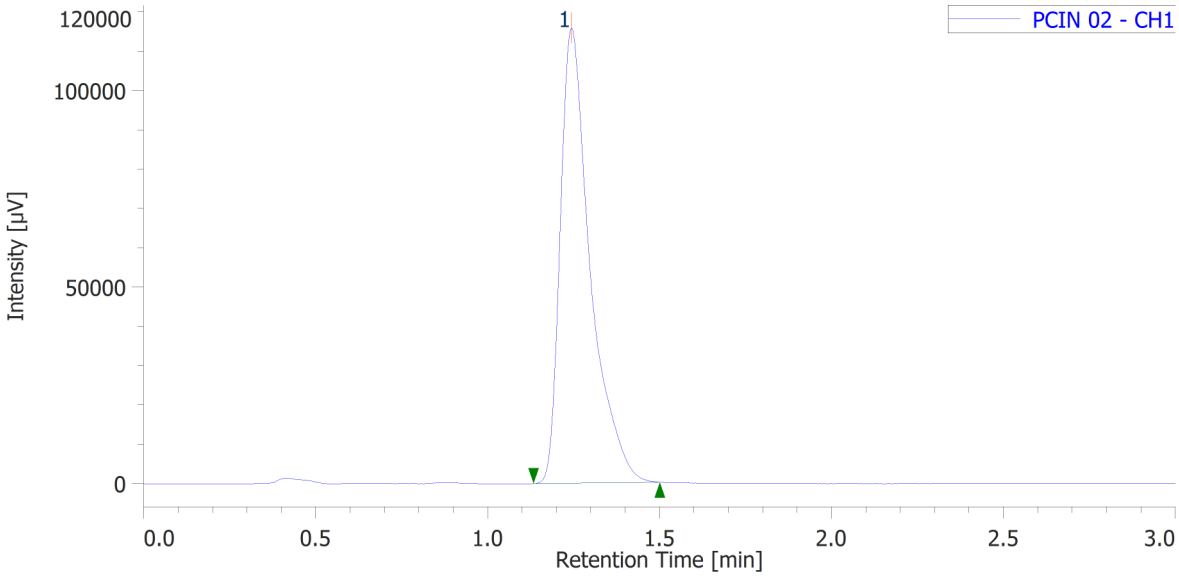

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:57
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 16:54:48
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.243	701048	115751	100.000	100.000	N/A	1146	N/A	1.683	

Creator Administrator
Reviewer
Approver

Chromatogram

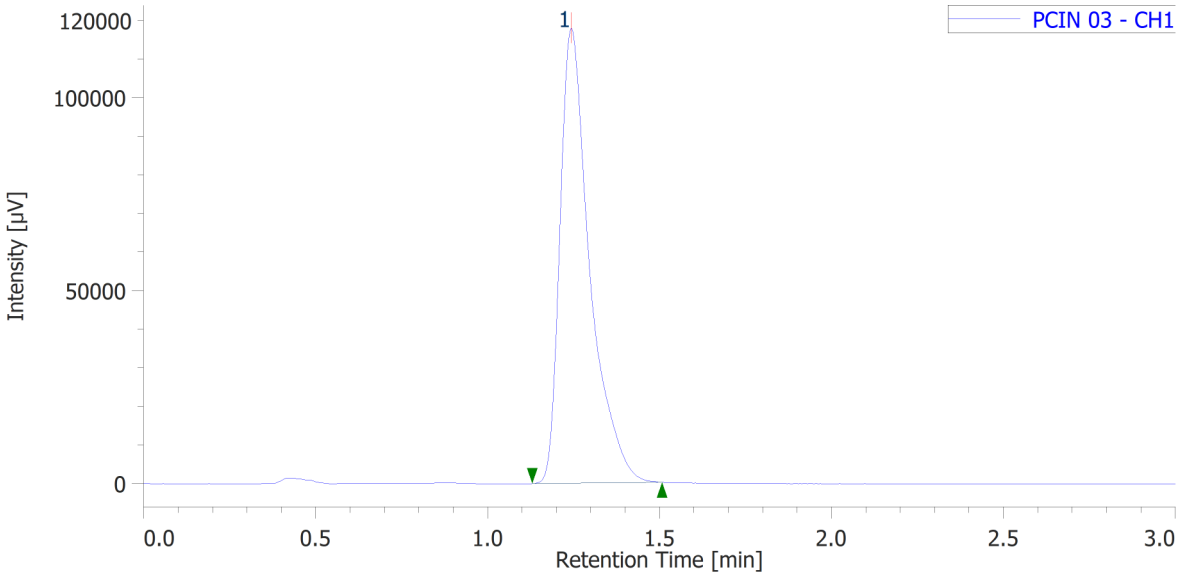

Chromatogram Information

User Name	Administrator
Date Modified	27/08/2024 08:08:58
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 16:58:59
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.243	709007	117931	100.000	100.000	N/A	1160	N/A	1.641	

Creator Administrator
Reviewer
Approver

Chromatogram

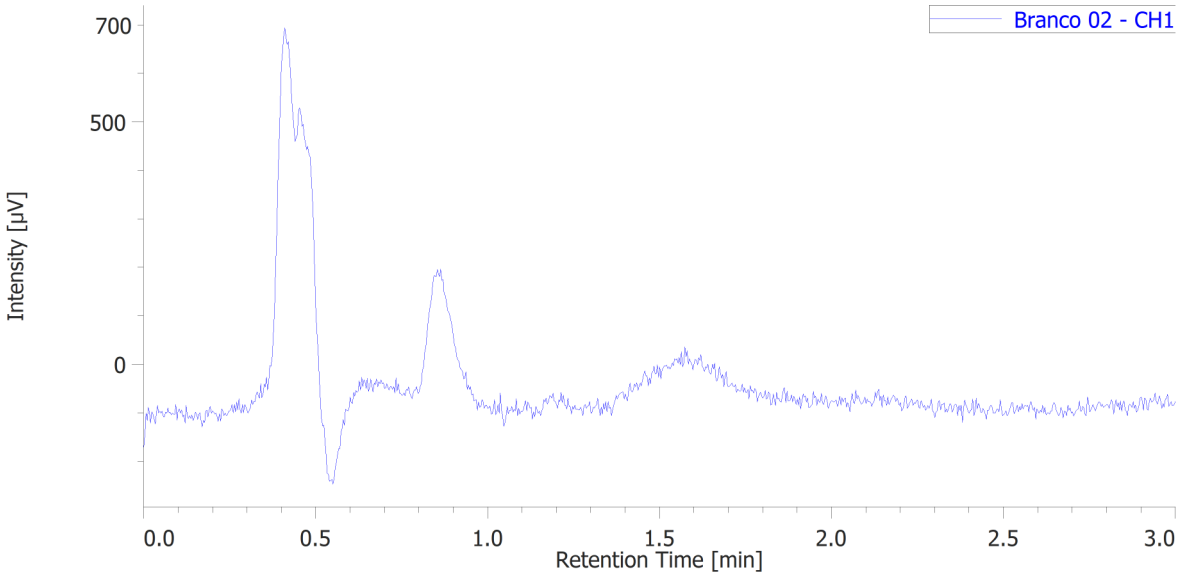


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:58
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 17:03:11
Volume	10.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator	Administrator
Reviewer	
Approver	

Chromatogram

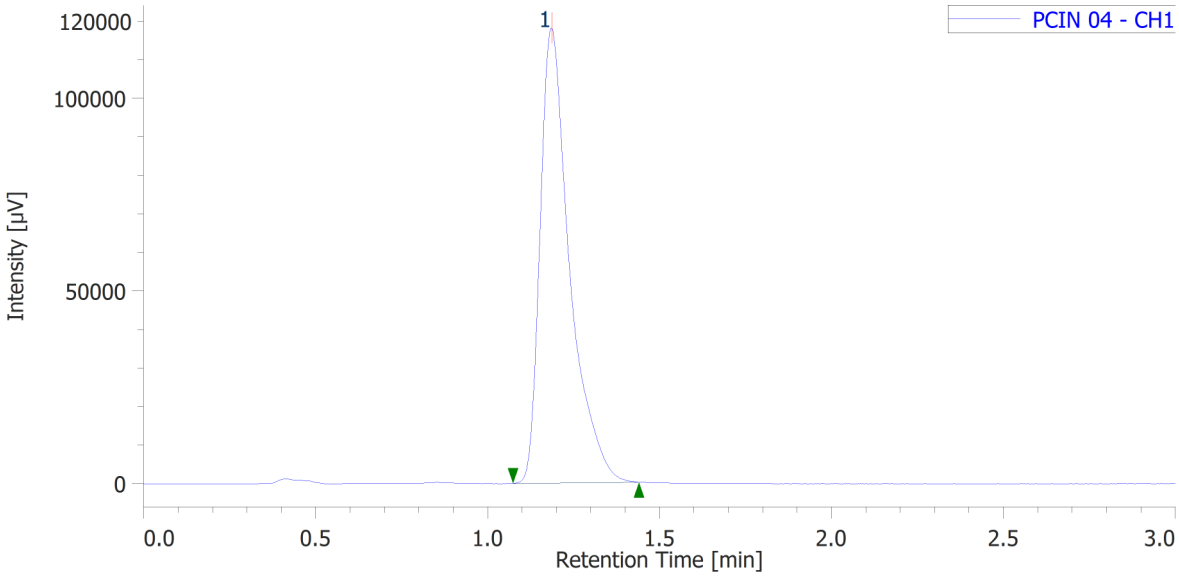

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:58
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 17:07:22
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.187	704246	118000	100.000	100.000	N/A	1068	N/A	1.611	

Creator Administrator
Reviewer
Approver

Chromatogram

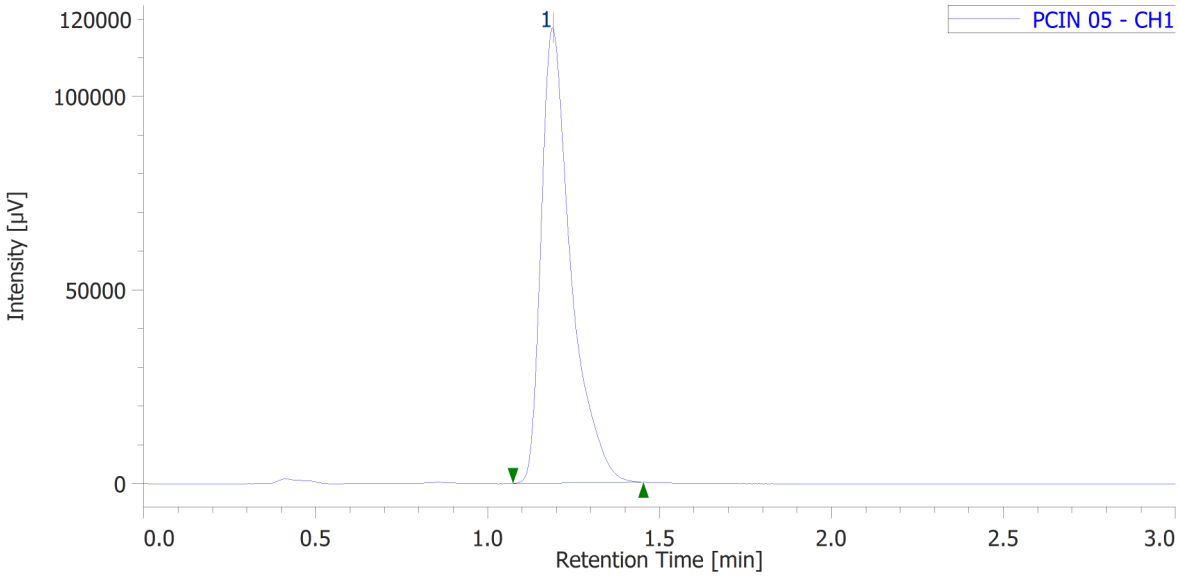

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:58
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 17:11:33
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.190	705213	117545	100.000	100.000	N/A	1064	N/A	1.613	

Creator Administrator
Reviewer
Approver

Chromatogram

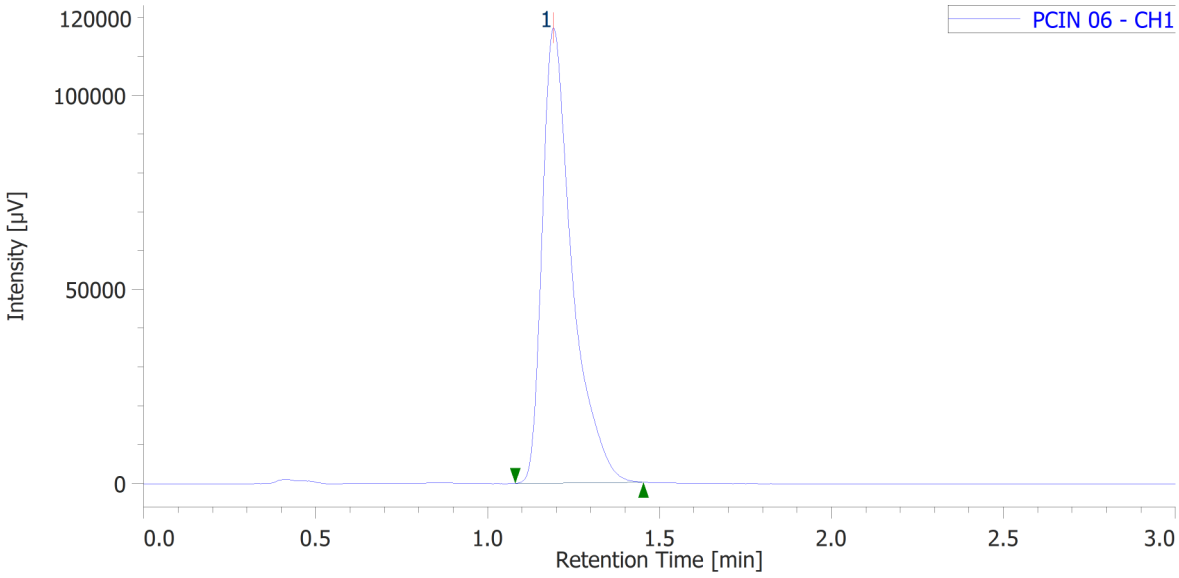

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:58
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 17:15:45
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.190	704983	117197	100.000	100.000	N/A	1060	N/A	1.693	

Creator Administrator
Reviewer
Approver

Chromatogram

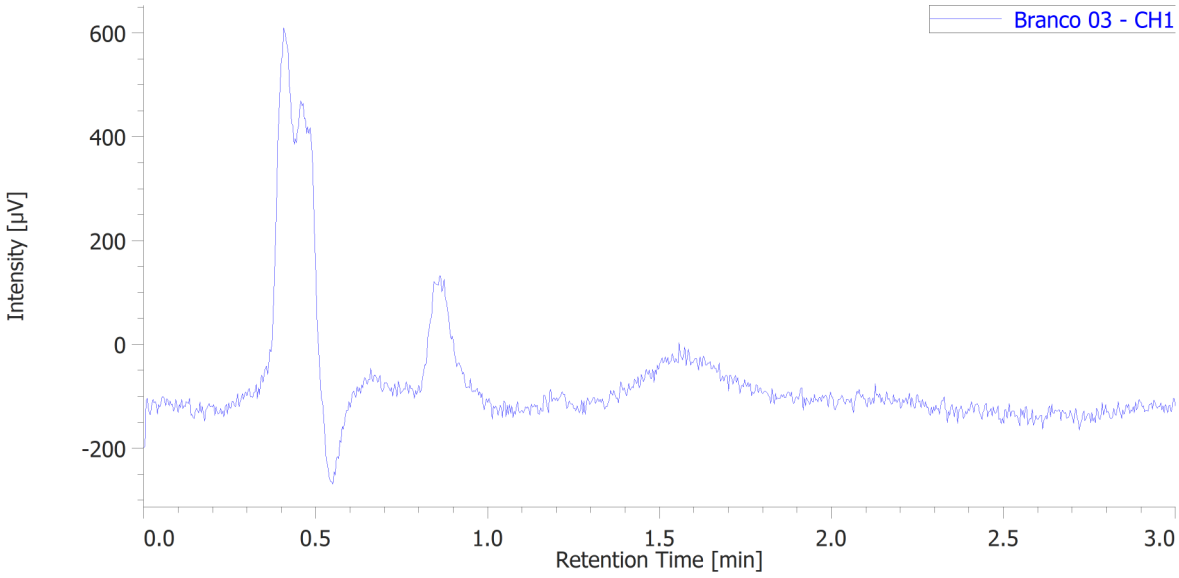


Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 08:08:59
Description	
HPLC System Name	HPLC_0005
Injection Date	26/08/2024 17:19:54
Volume	10.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator	Administrator
Reviewer	
Approver	

Chromatogram

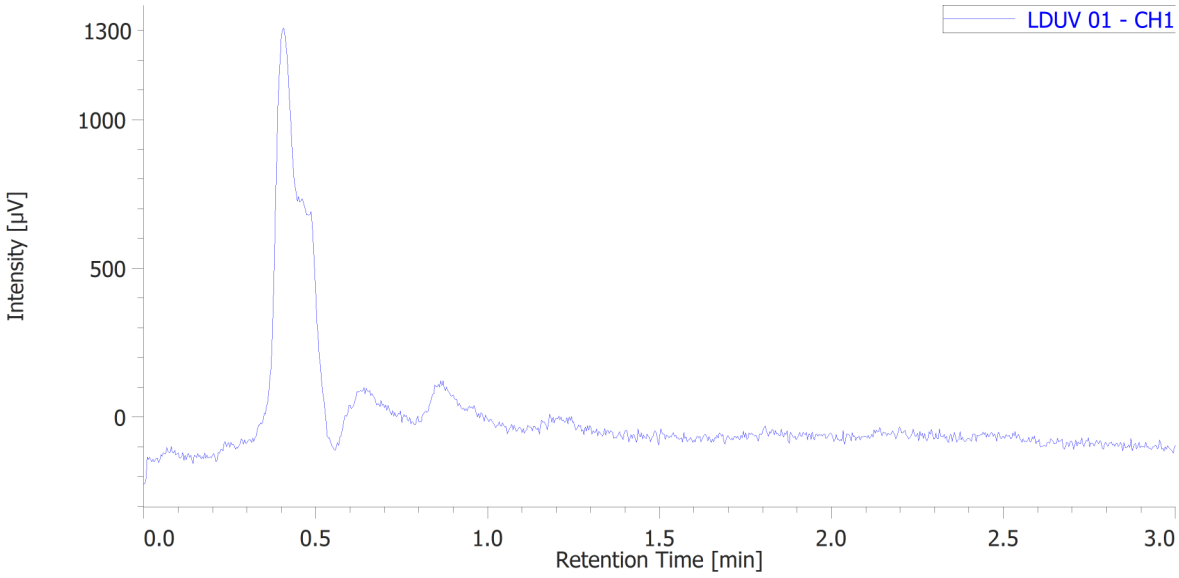


Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:18
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 08:43:50
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator Administrator
Reviewer
Approver

Chromatogram

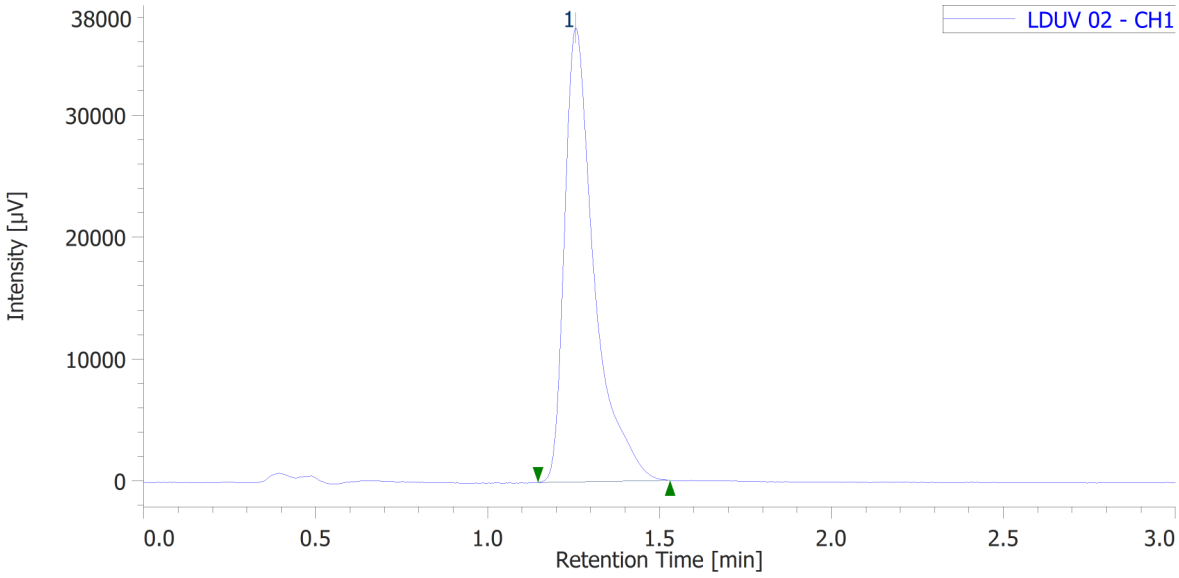

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:19
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 08:48:03
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.257	223404	37194	100.000	100.000	N/A	1236	N/A	1.776	

Creator Administrator
Reviewer
Approver

Chromatogram

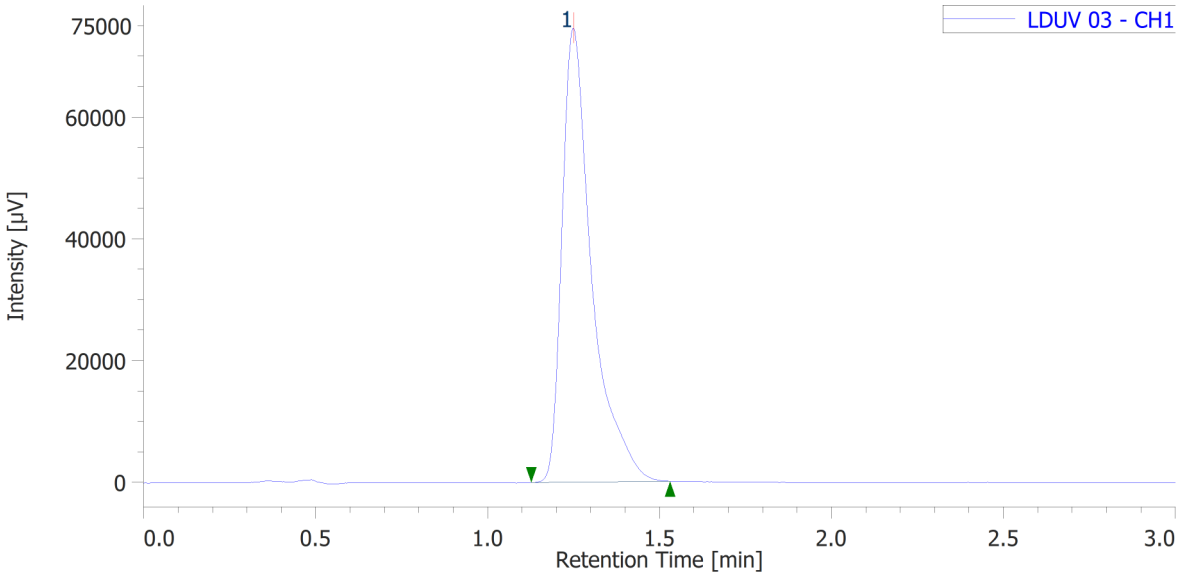

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:19
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 08:52:17
Volume	10.0 [µL]
Sample #	5
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.250	448661	74585	100.000	100.000	N/A	1219	N/A	1.741	

Creator Administrator
Reviewer
Approver

Chromatogram

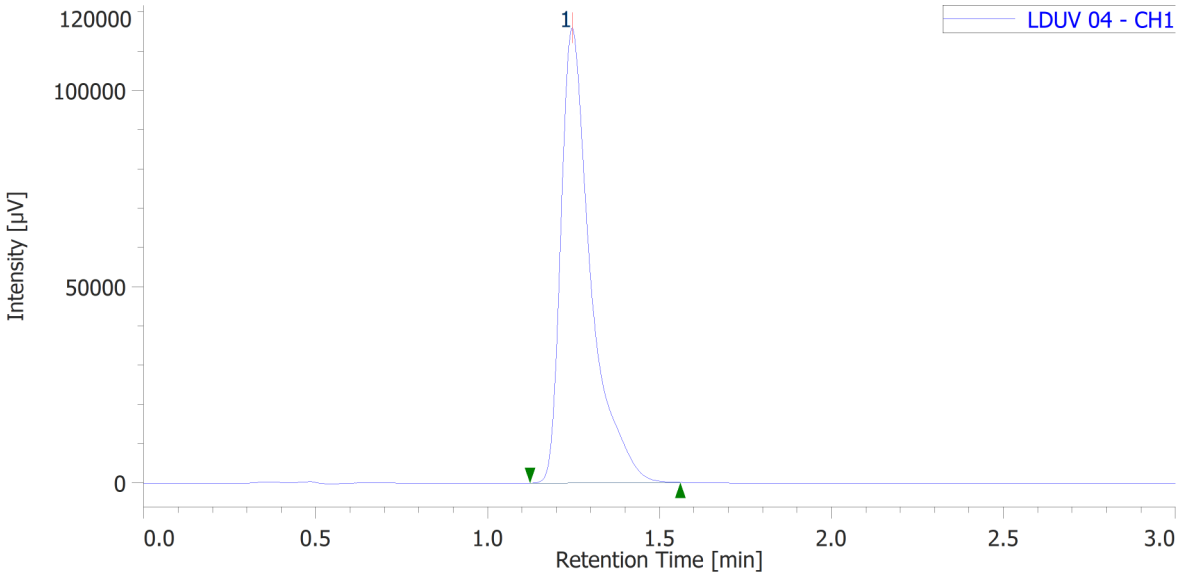

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:19
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 08:56:31
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.247	698884	115877	100.000	100.000	N/A	1212	N/A	1.747	

Creator Administrator
Reviewer
Approver

Chromatogram

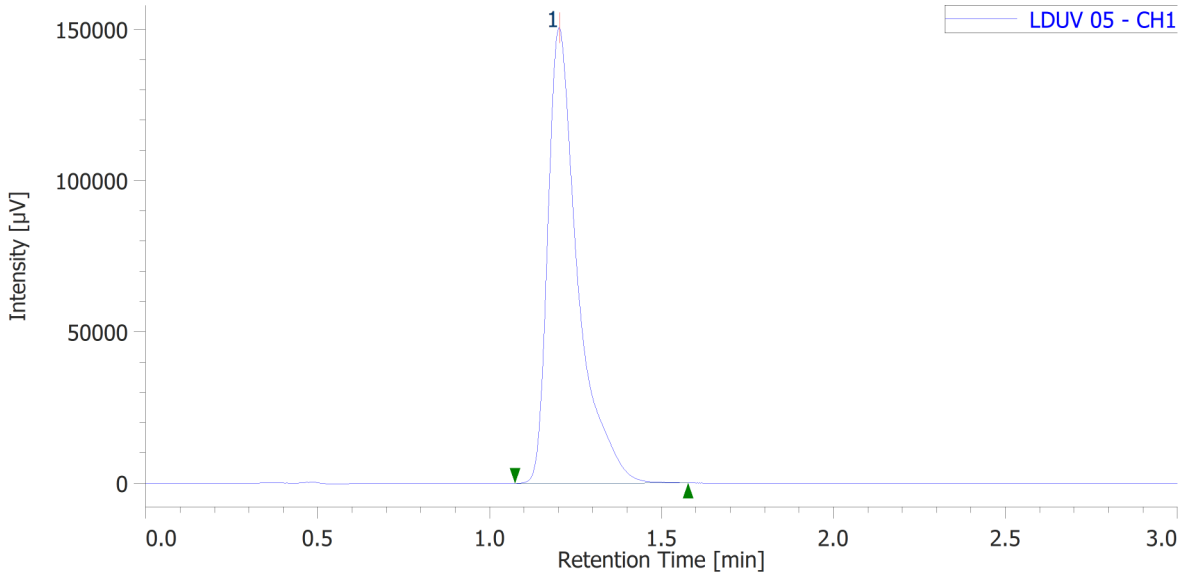

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:00:47
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.203	909181	150384	100.000	100.000	N/A	1125	N/A	1.731	

Creator Administrator
Reviewer
Approver

Chromatogram

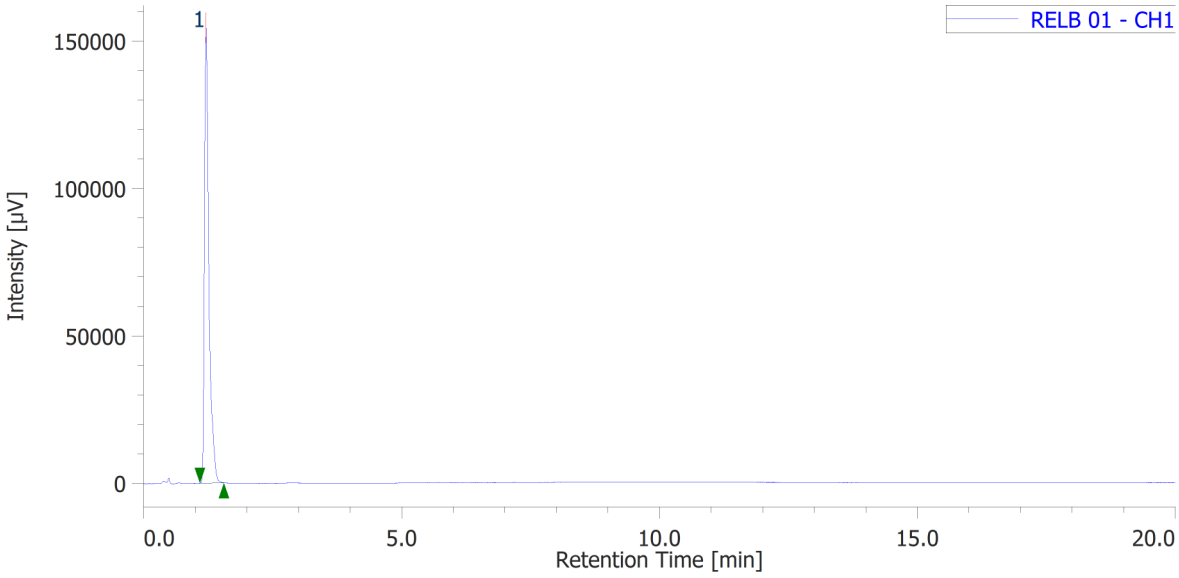

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:05:08
Volume	20.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	920787	154296	100.000	100.000	N/A	1167	N/A	1.832	

Creator Administrator
Reviewer
Approver

Chromatogram

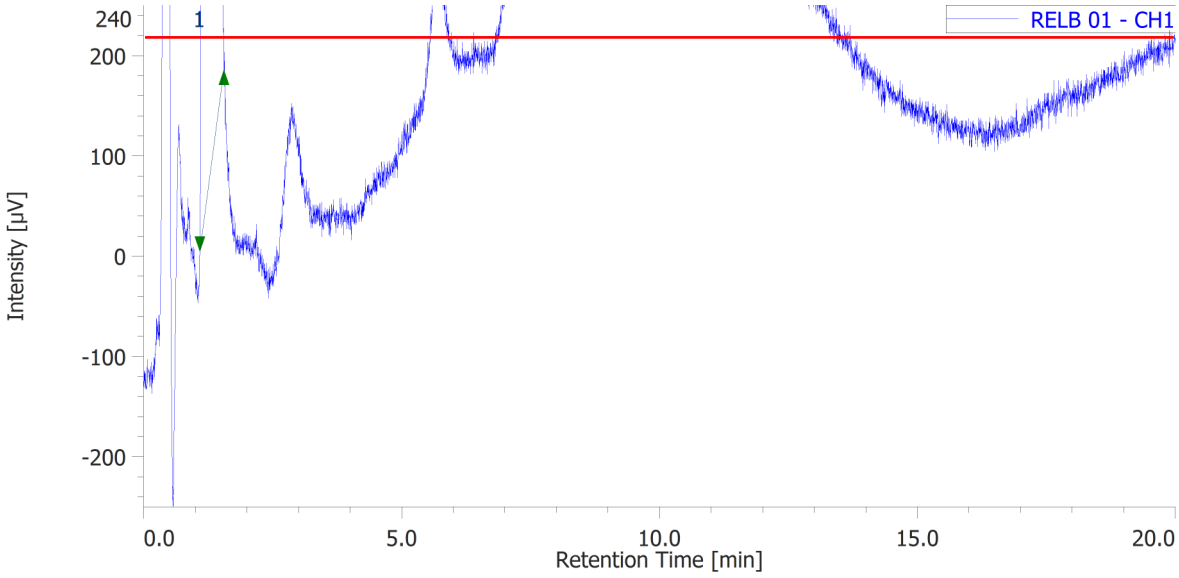

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:05:08
Volume	20.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	920787	154296	100.000	100.000	N/A	1167	N/A	1.832	

Creator Administrator
Reviewer
Approver

Chromatogram

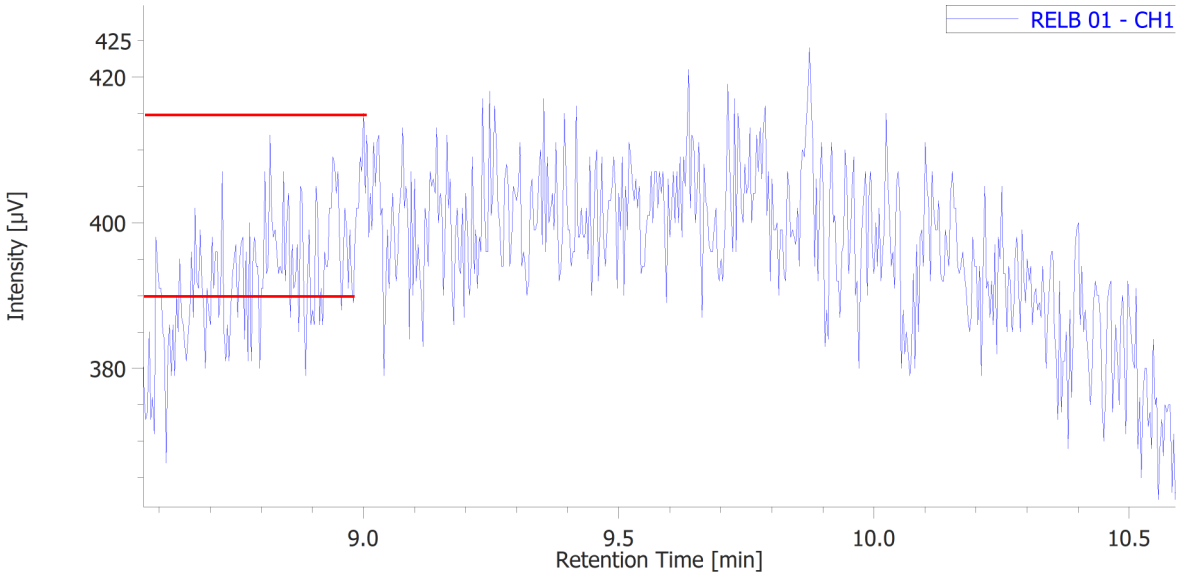

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:05:08
Volume	20.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.207	920787	154296	100.000	100.000	N/A	1167	N/A	1.832	

Creator Administrator
Reviewer
Approver

Chromatogram

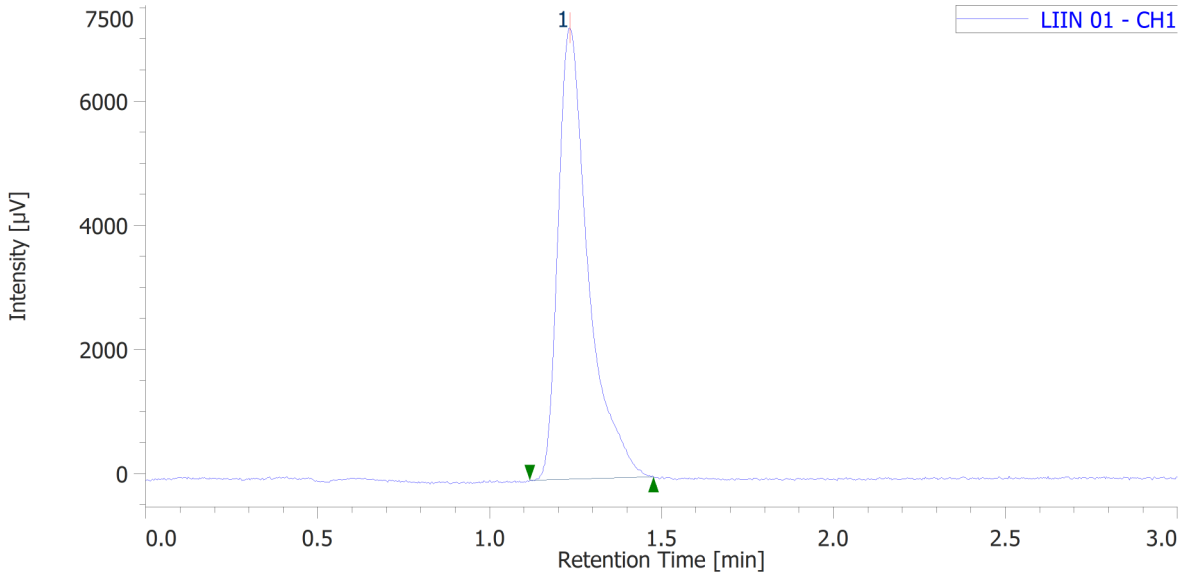

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:26:19
Volume	0.1 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.233	44277	7261	100.000	100.000	N/A	1130	N/A	1.696	

Creator Administrator
Reviewer
Approver

Chromatogram

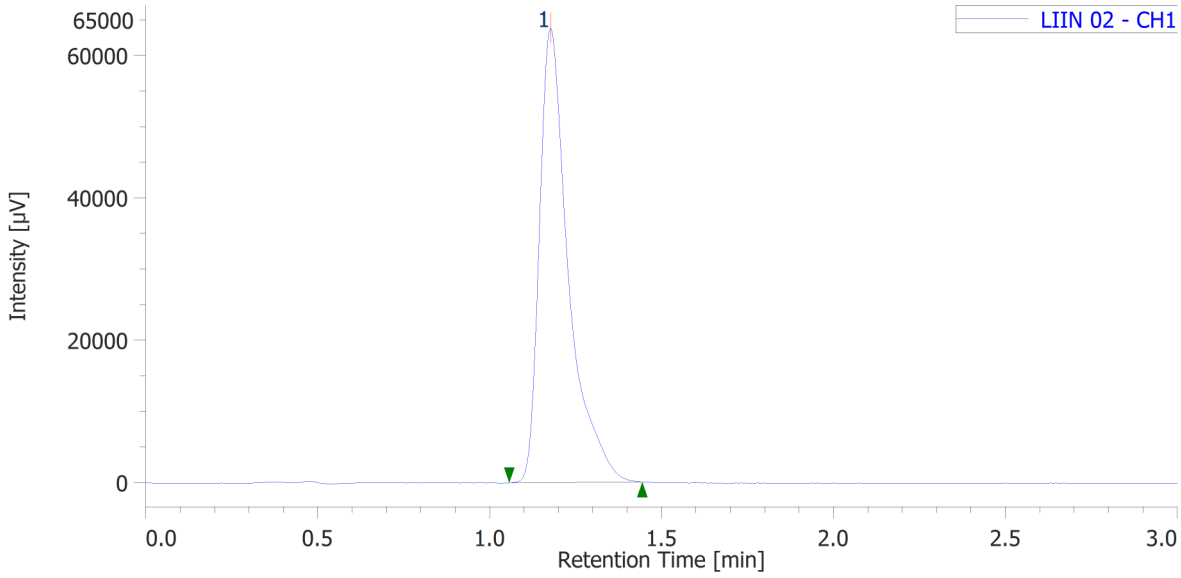

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:20
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:30:32
Volume	5.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.177	374531	63813	100.000	100.000	N/A	1124	N/A	1.740	

Creator Administrator
Reviewer
Approver

Chromatogram

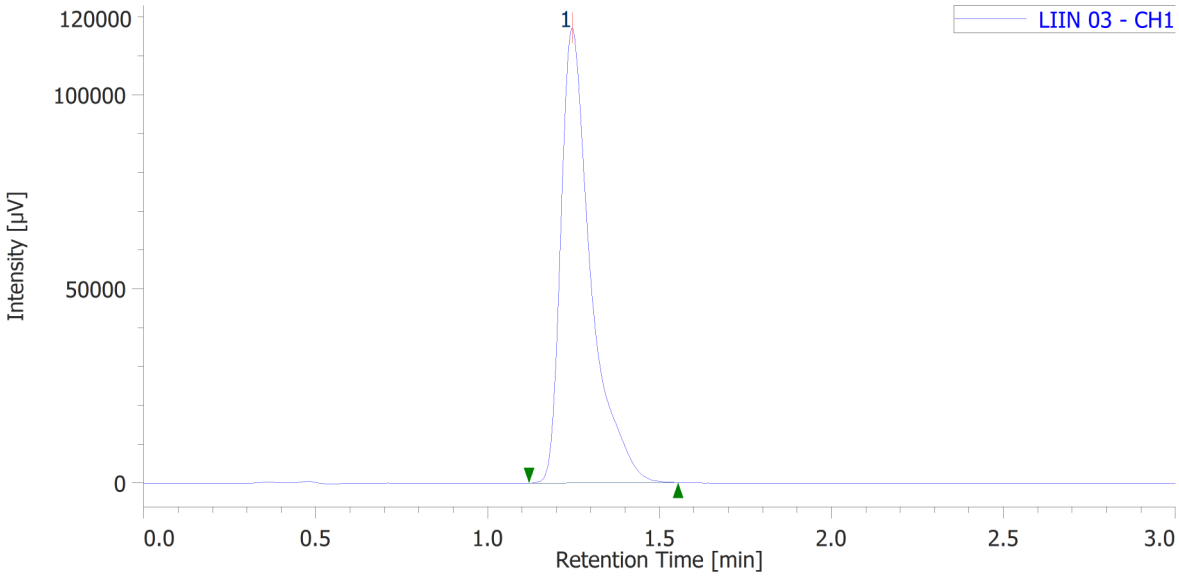

Chromatogram Information

User Name	Administrator
Date Modified	30/08/2024 11:07:21
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:34:49
Volume	10.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.247	710531	117170	100.000	100.000	N/A	1198	N/A	1.731	

Creator Administrator
Reviewer
Approver

Chromatogram

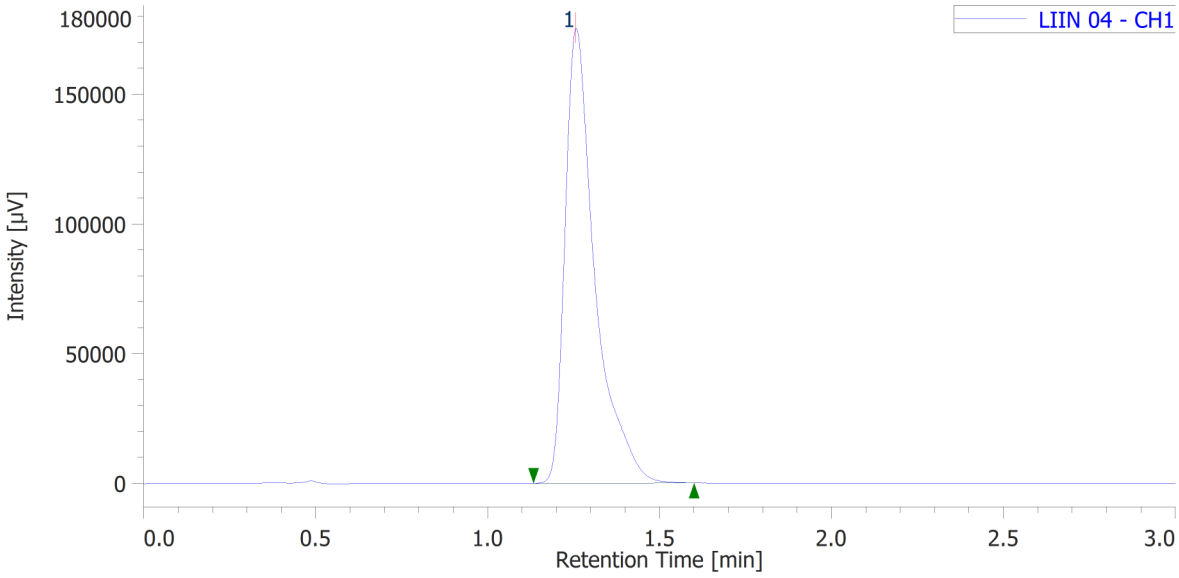

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:21
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:39:07
Volume	15.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.257	1057651	175416	100.000	100.000	N/A	1236	N/A	1.794	

Creator Administrator
Reviewer
Approver

Chromatogram

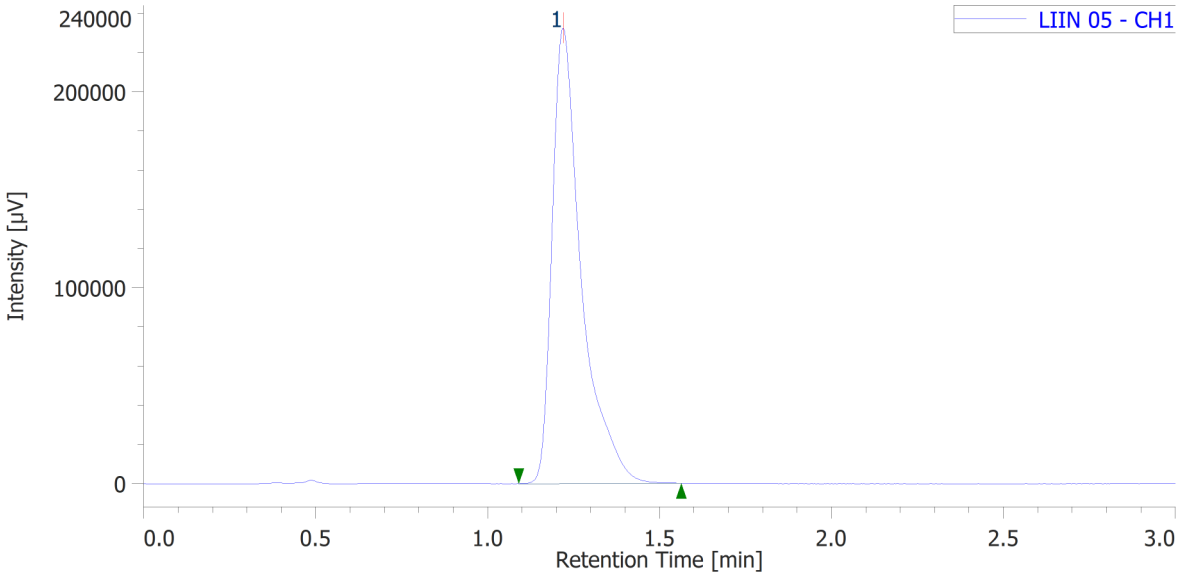

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2024 11:07:21
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 09:43:28
Volume	20.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.220	1371034	232450	100.000	100.000	N/A	1220	N/A	1.751	

Creator Administrator
Reviewer
Approver

Chromatogram

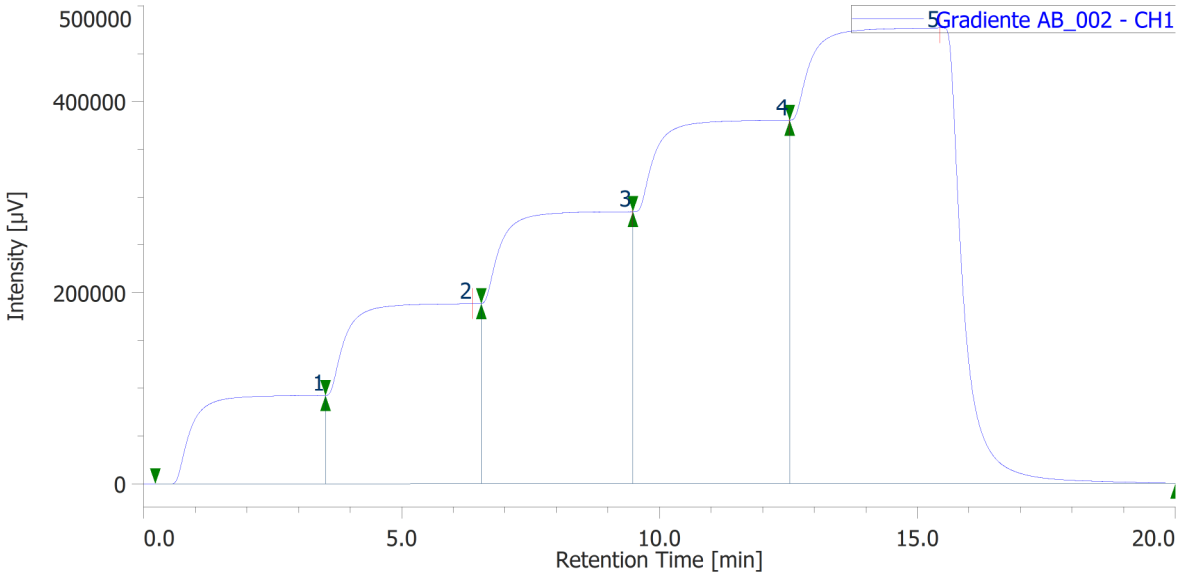

Chromatogram Information

User Name	Administrator
Date Modified	27/08/2024 11:09:56
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 10:24:35
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.520	14370921	92199	5.609	6.486	N/A	N/A	N/A	N/A	
2	40%	1	6.373	31847159	188324	12.431	13.248	N/A	N/A	N/A	N/A	
3	60%	1	9.470	47978533	284466	18.728	20.012	N/A	N/A	N/A	N/A	
4	80%	1	12.507	66718916	380023	26.043	26.734	N/A	N/A	N/A	N/A	
5	100%	1	15.433	95275435	476490	37.189	33.520	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

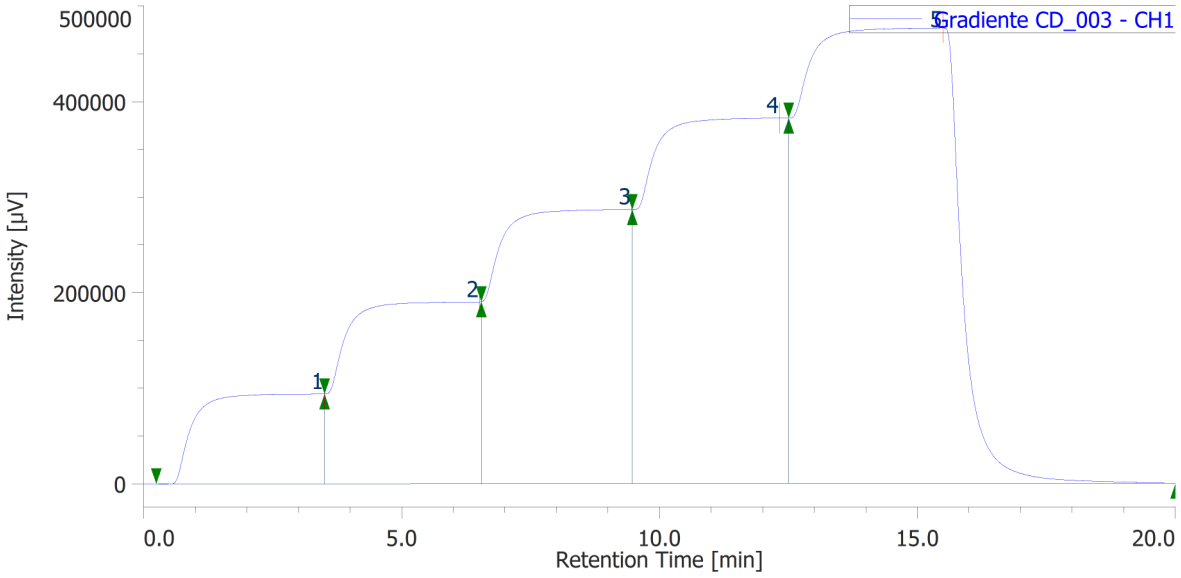

Chromatogram Information	
User Name	Administrator
Date Modified	27/08/2024 11:09:56
Description	
HPLC System Name	HPLC_0005
Injection Date	27/08/2024 10:45:32
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.500	14576041	94028	5.656	6.575	N/A	N/A	N/A	N/A	
2	40%	1	6.503	32269693	190170	12.523	13.298	N/A	N/A	N/A	N/A	
3	60%	1	9.453	48079370	286890	18.658	20.061	N/A	N/A	N/A	N/A	
4	80%	1	12.320	67065669	382468	26.026	26.744	N/A	N/A	N/A	N/A	
5	100%	1	15.490	95697327	476537	37.137	33.322	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver