


Software - 07.08.2026 - 1

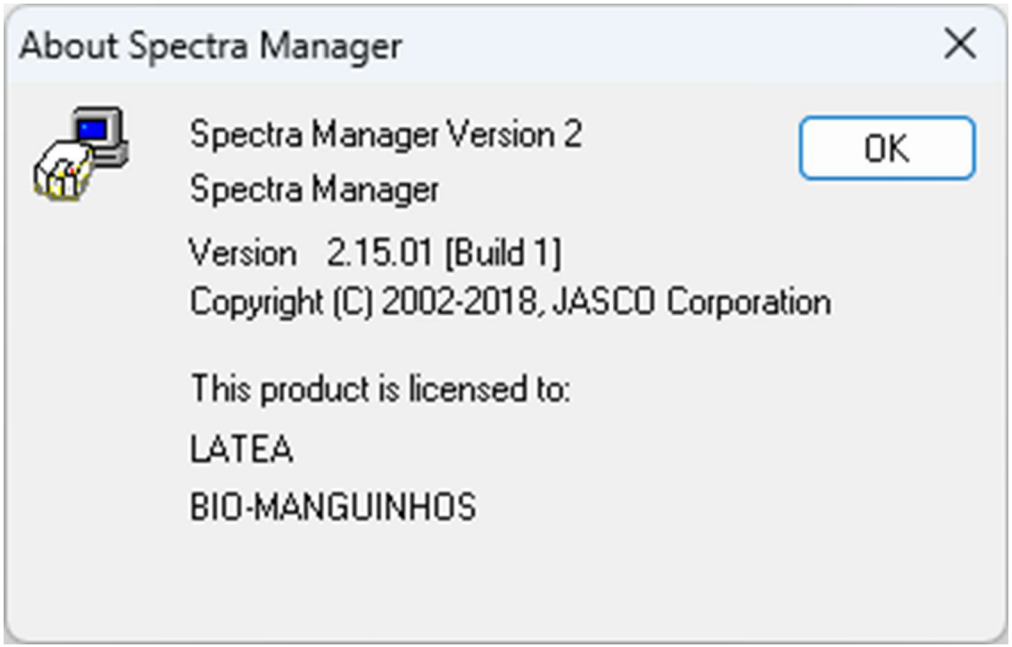


Software - 07.08.2026 - 2

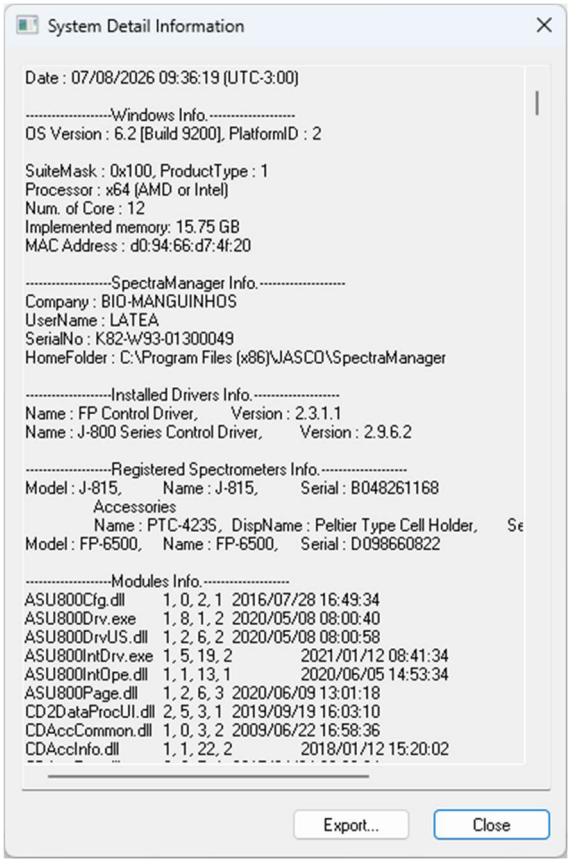


Software - 07.08.2026 - 3

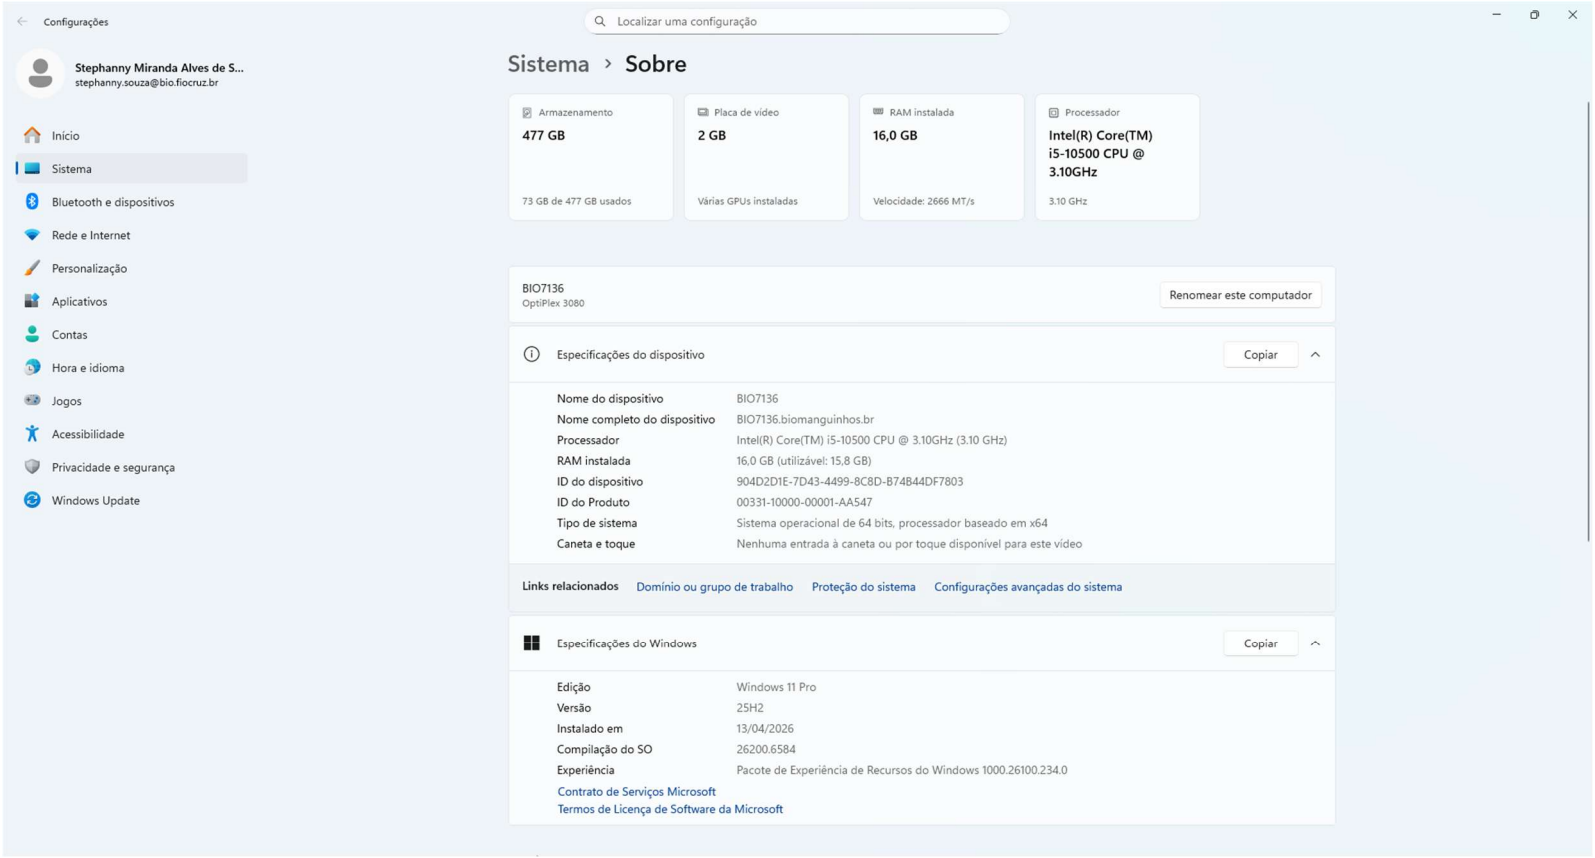


Software - 07.08.2026 - 4

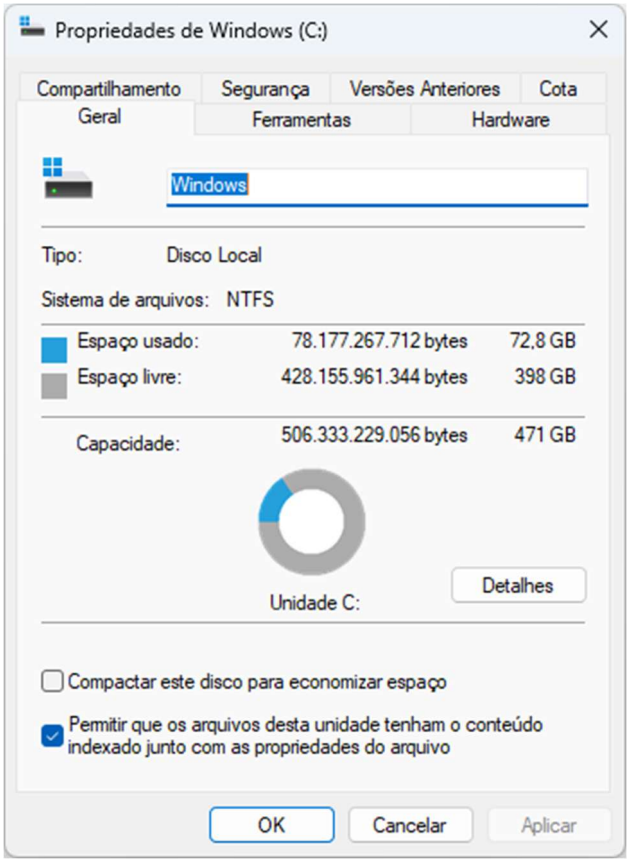


Software - 07.08.2026 - 5

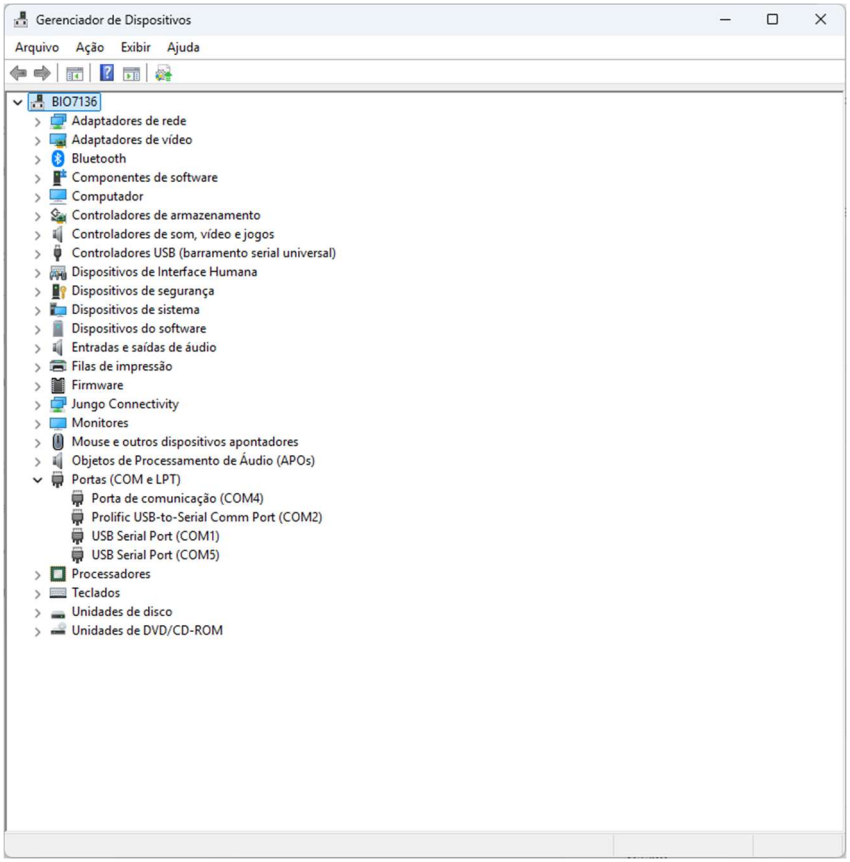


Software - 07.08.2026 - 6

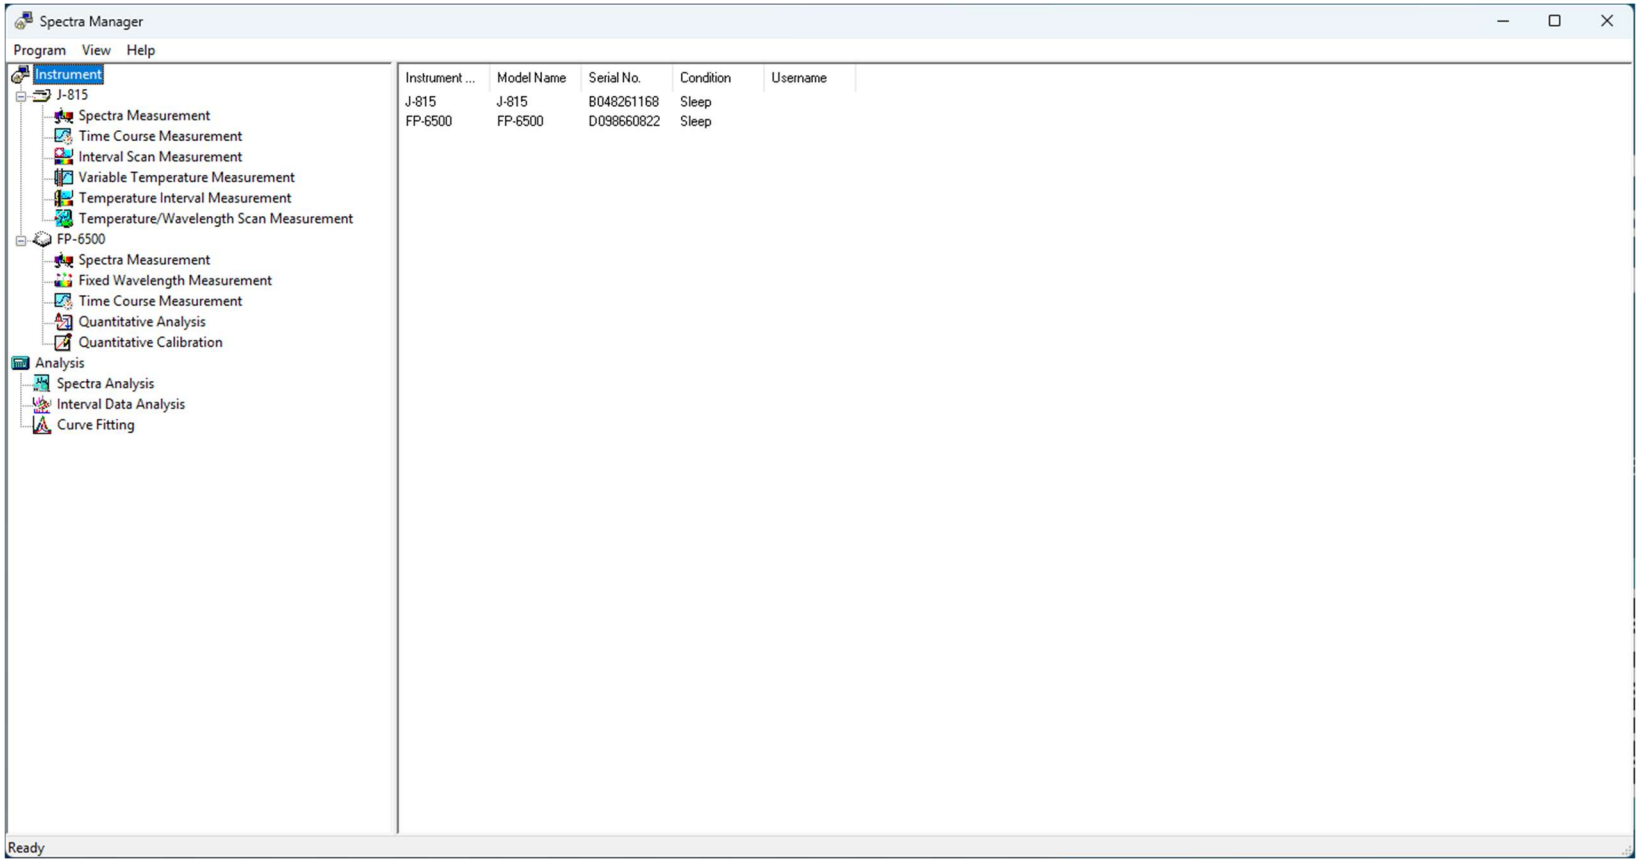


Software - 07.08.2026 - 7

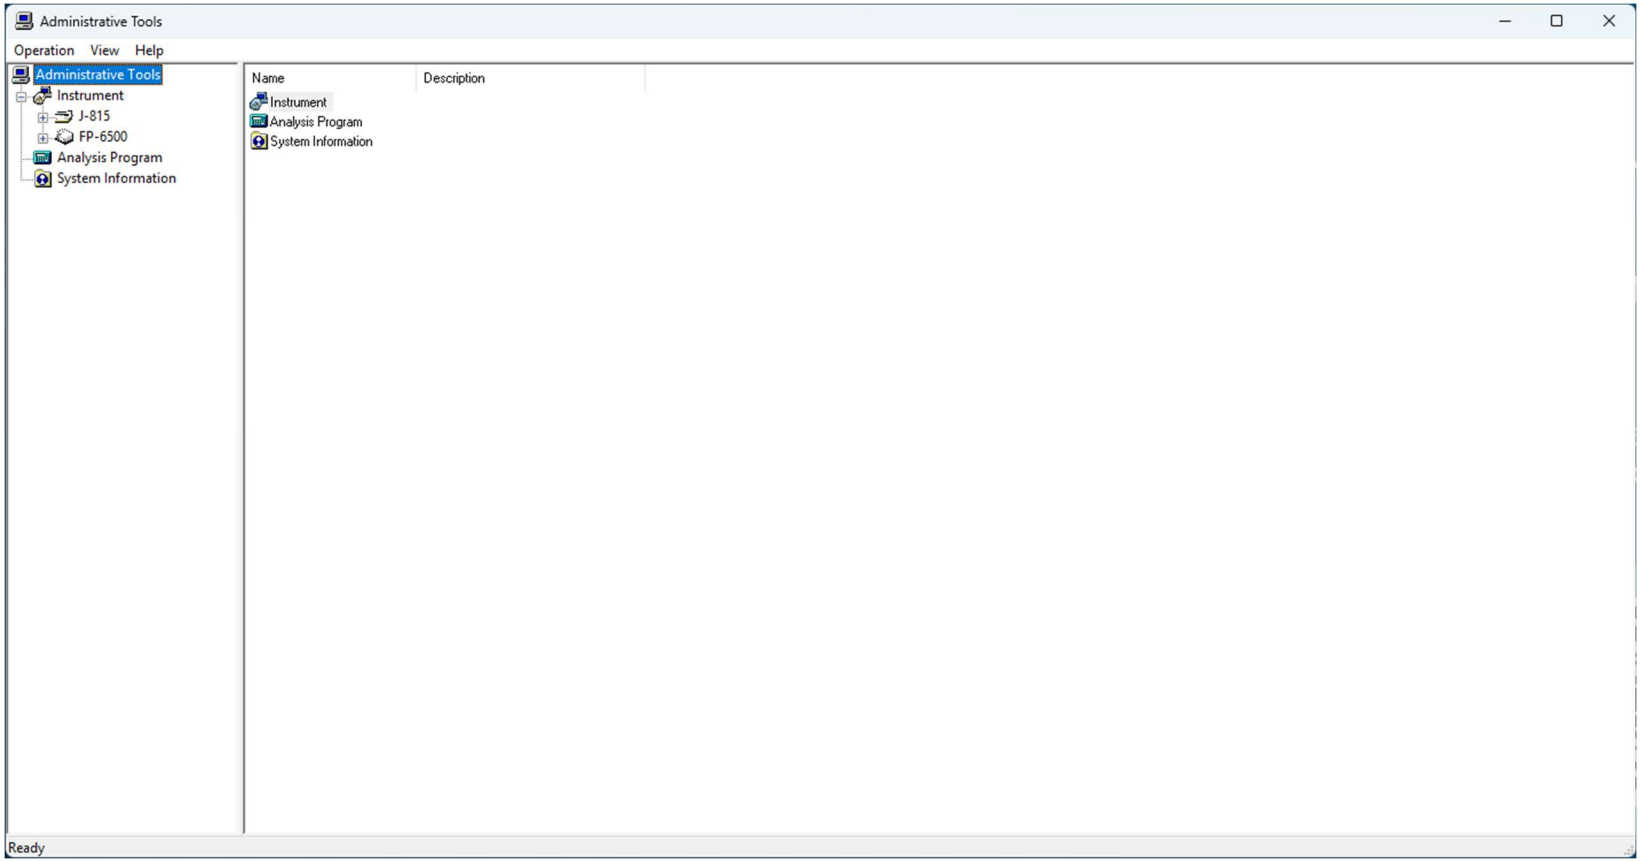


Software - 07.08.2026 - 8

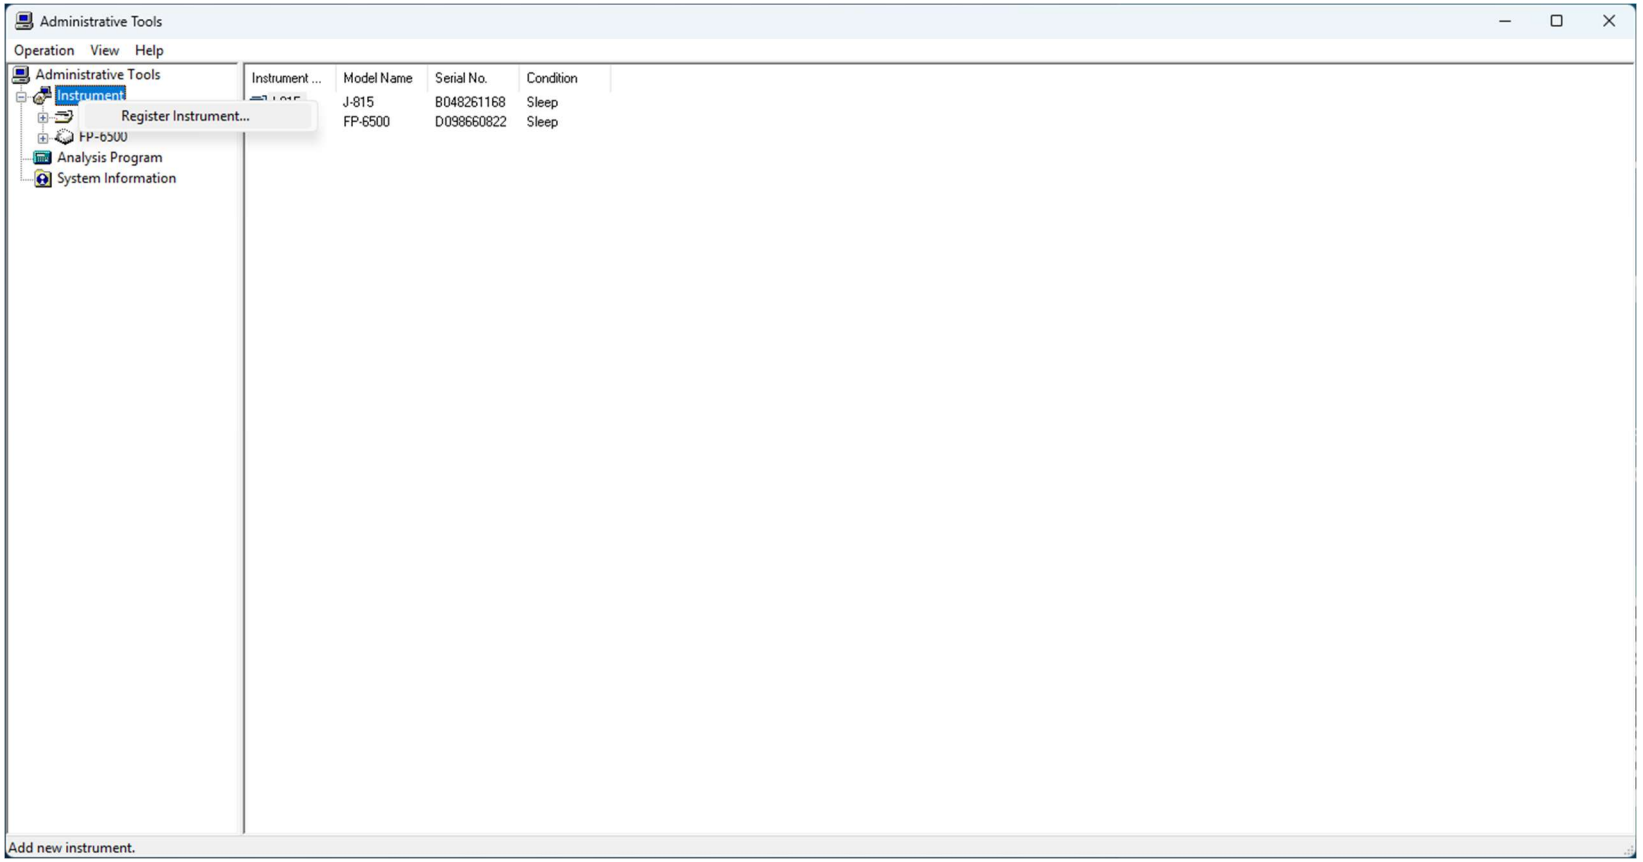


Software - 07.08.2026 - 9

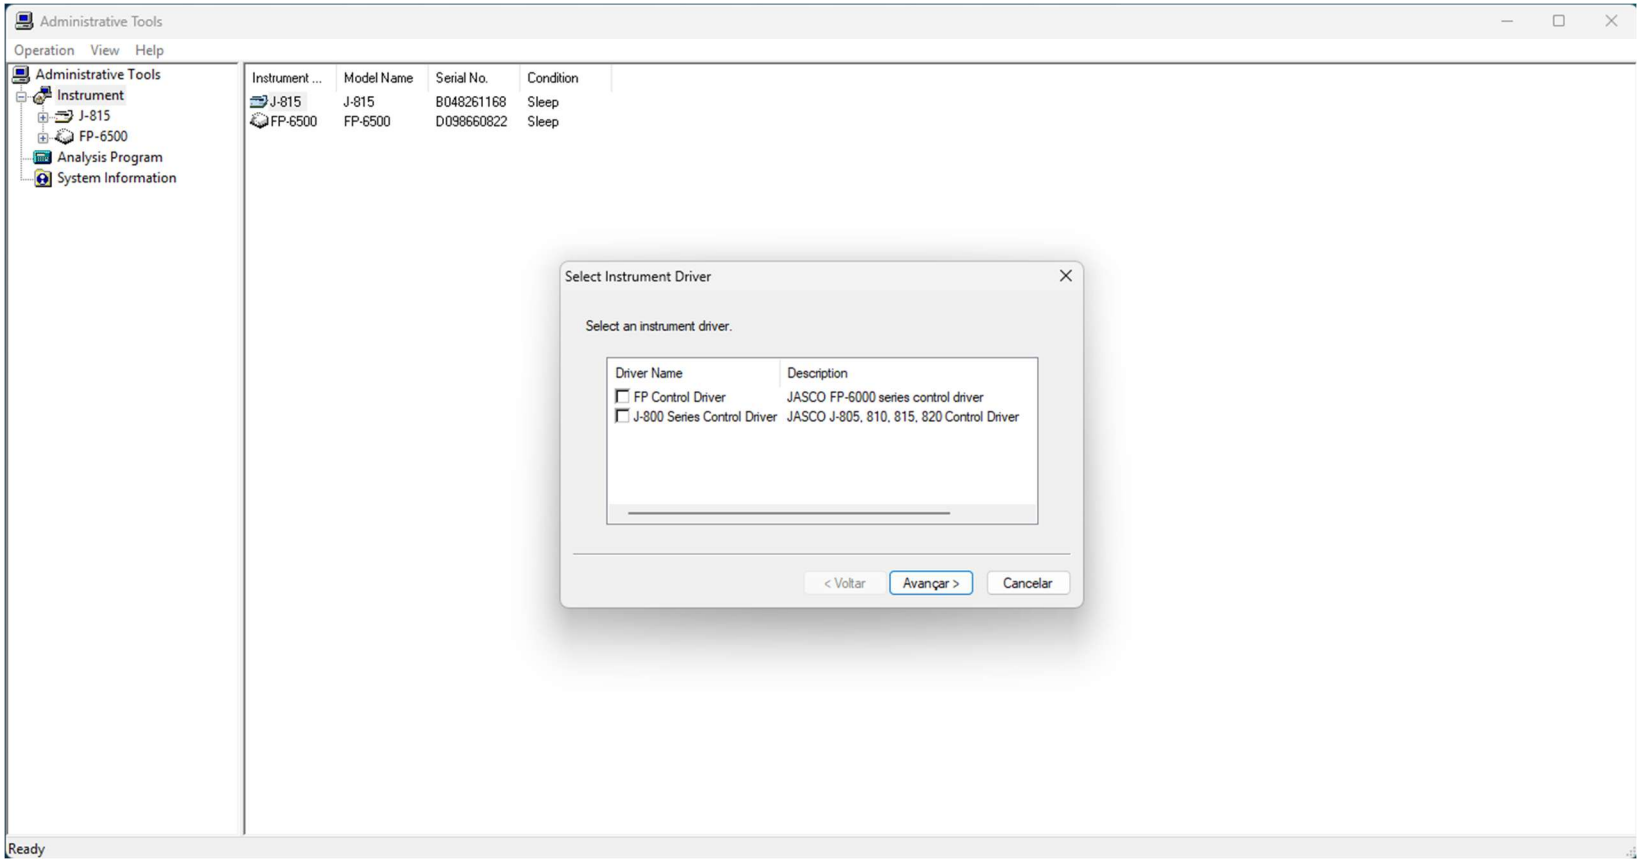


Software - 07.08.2026 - 10

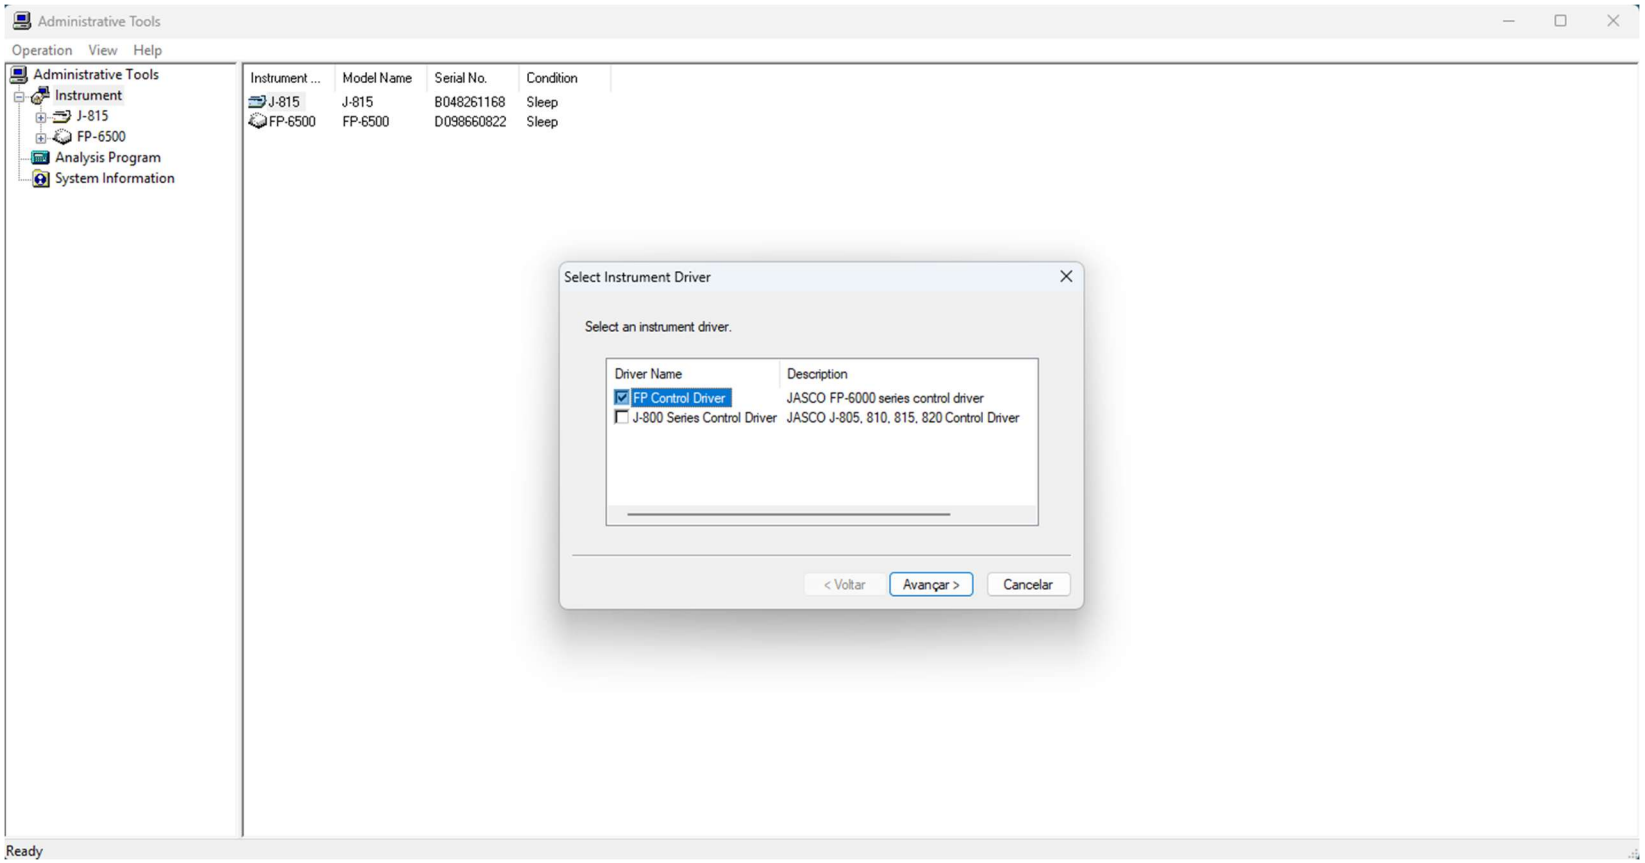


Software - 07.08.2026 - 11

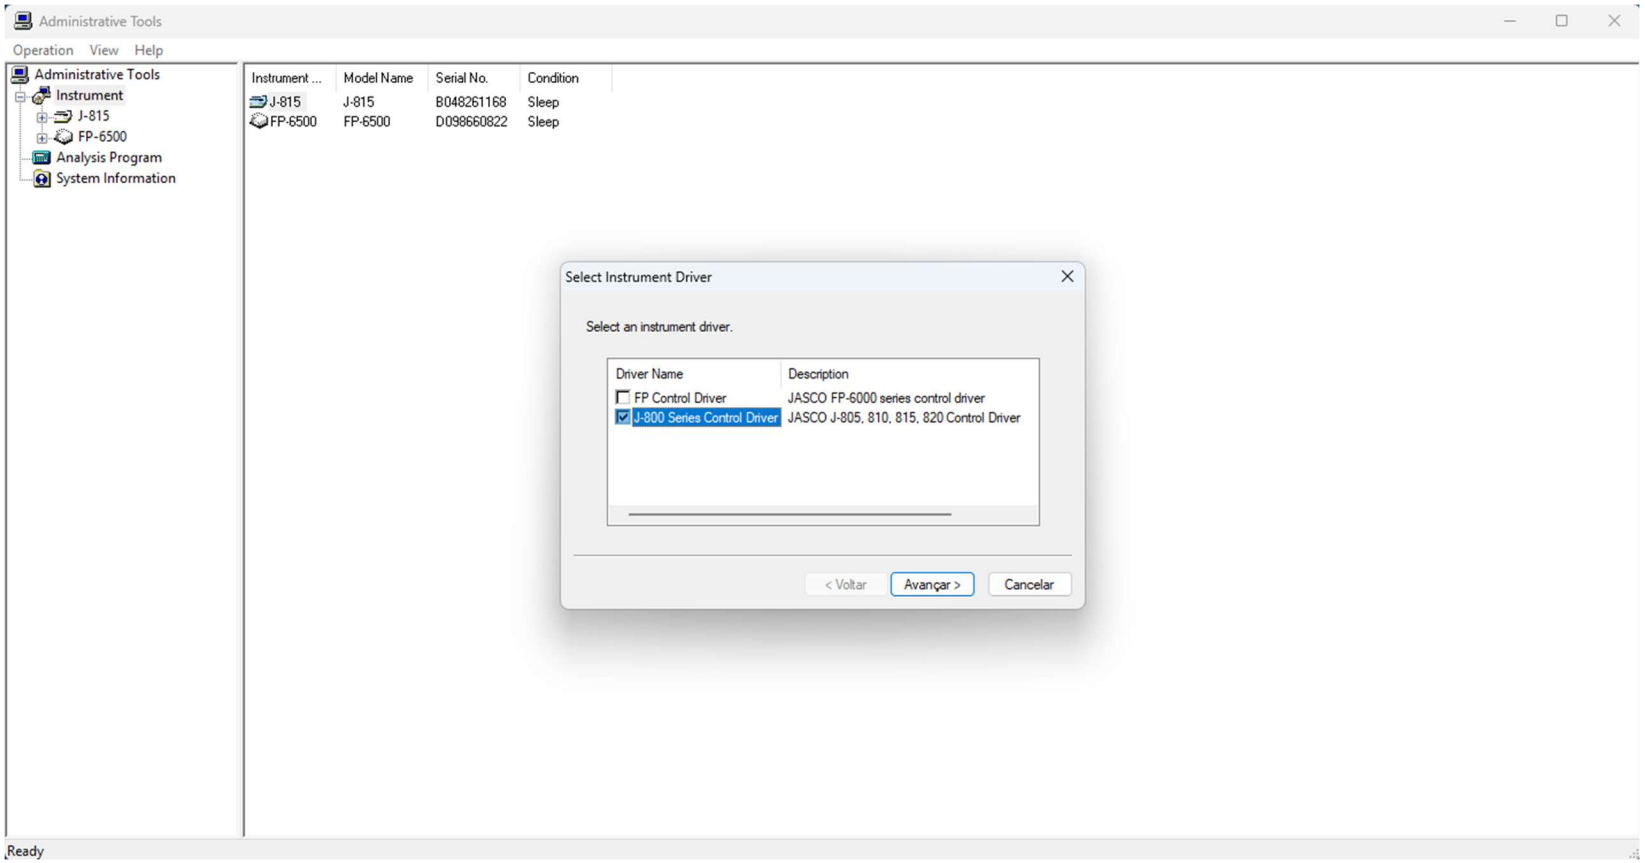


Software - 07.08.2026 - 12

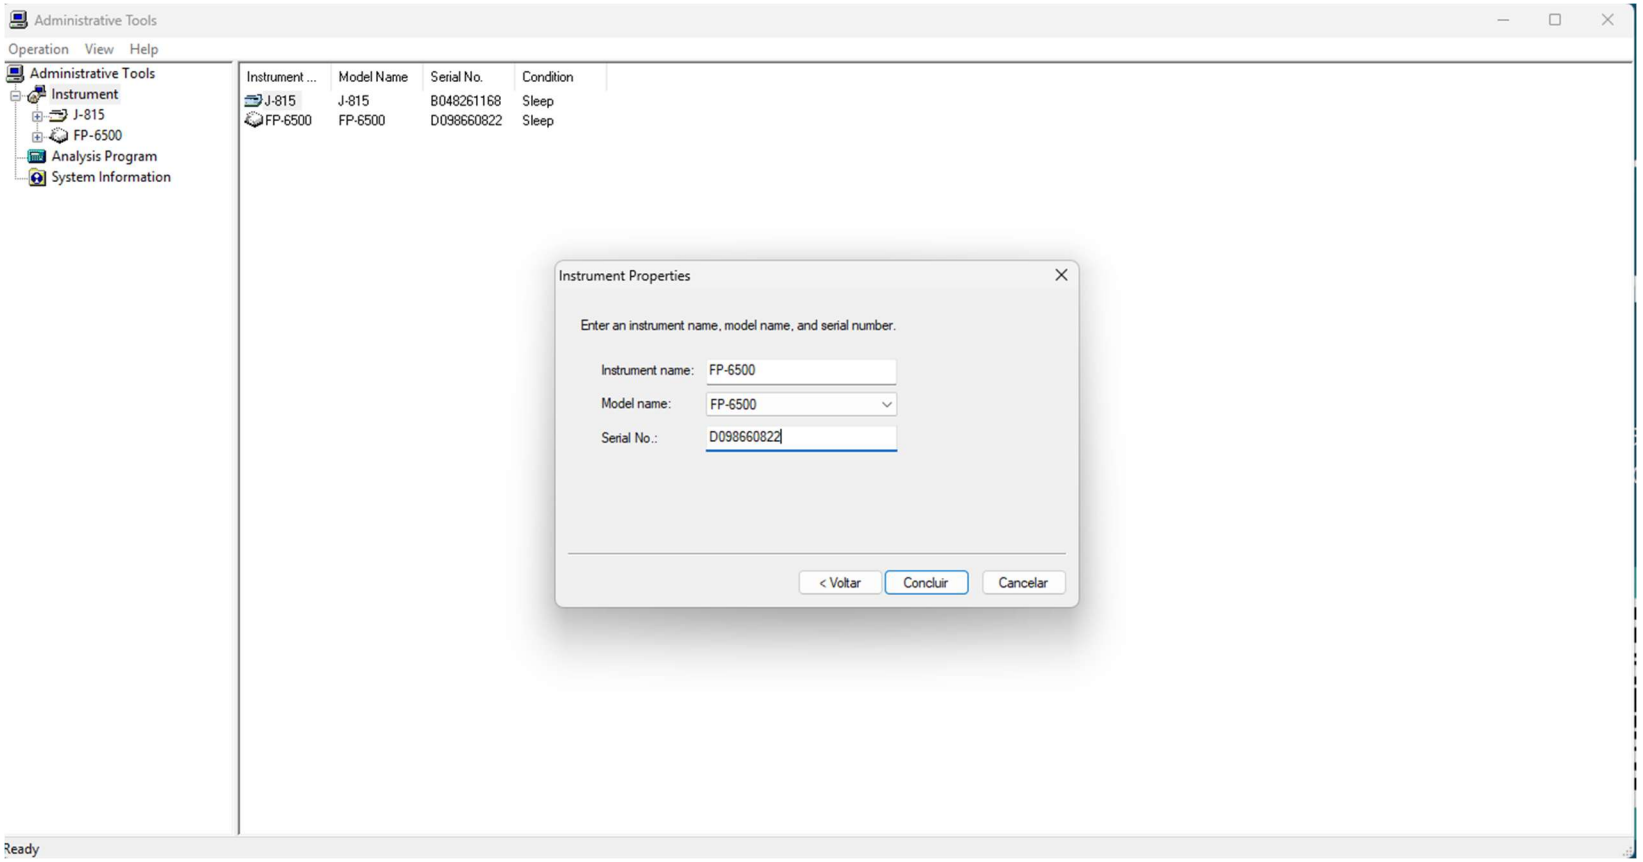


Software - 07.08.2026 - 13

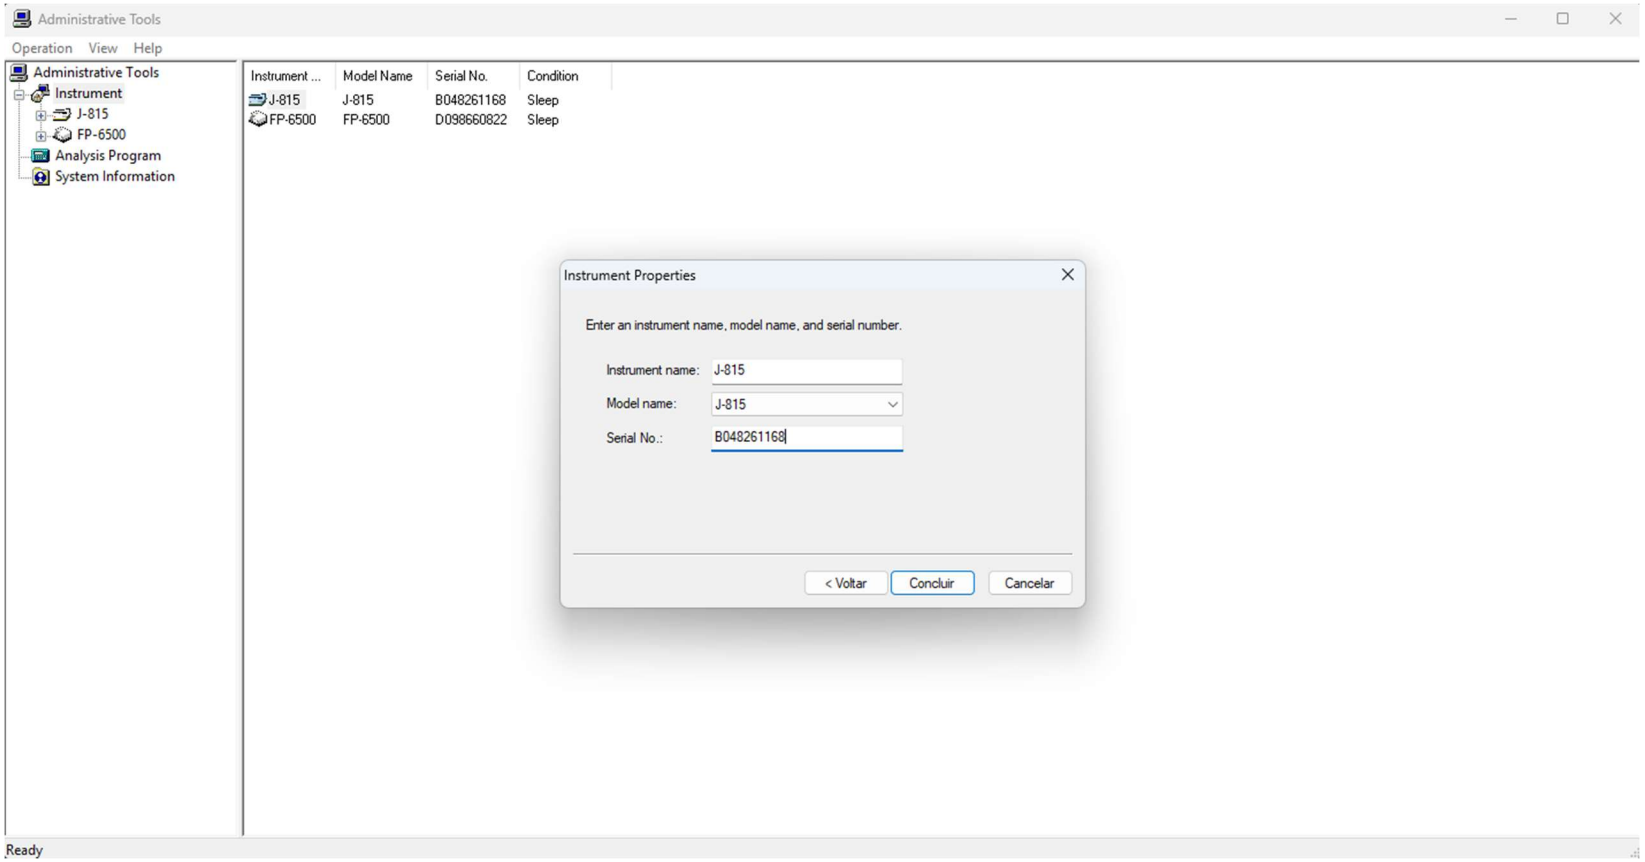


Software - 07.08.2026 - 14

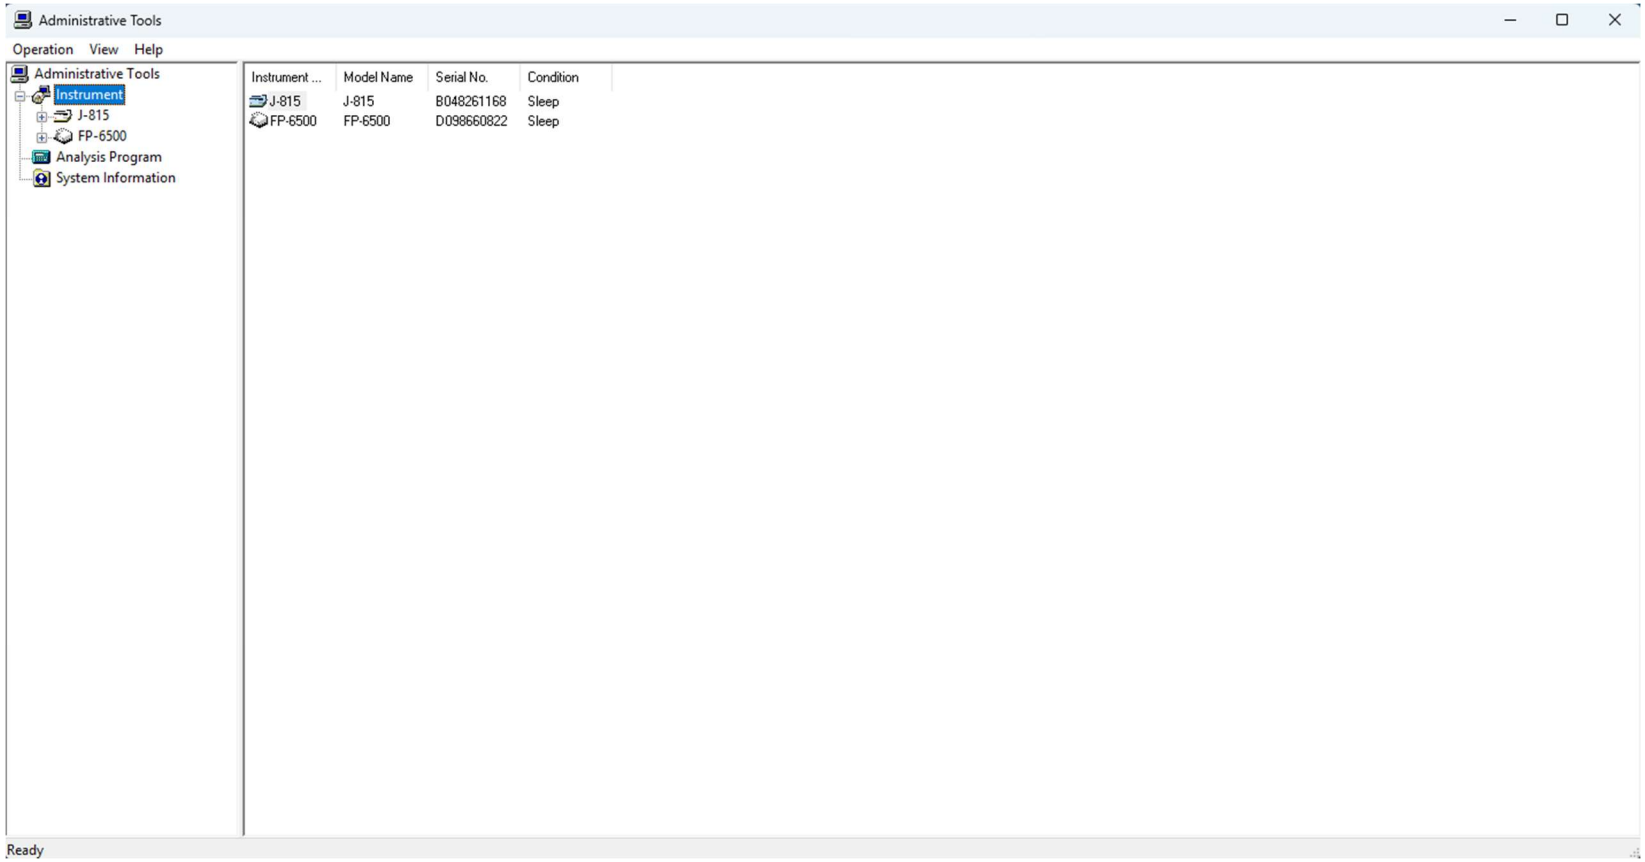


Software - 07.08.2026 - 15

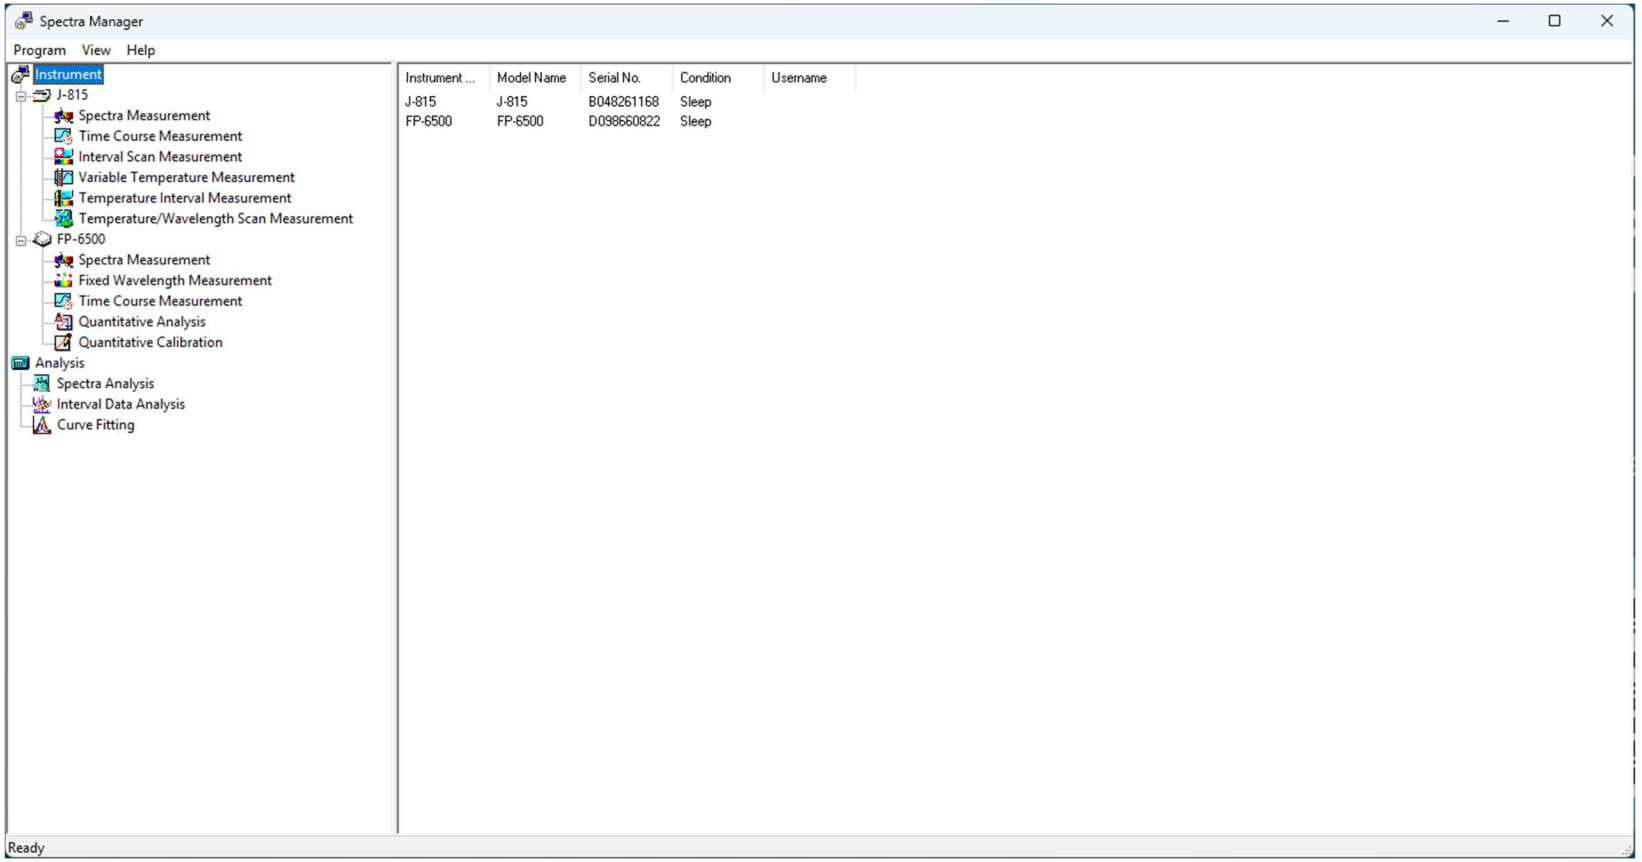


Software - 07.08.2026 - 16

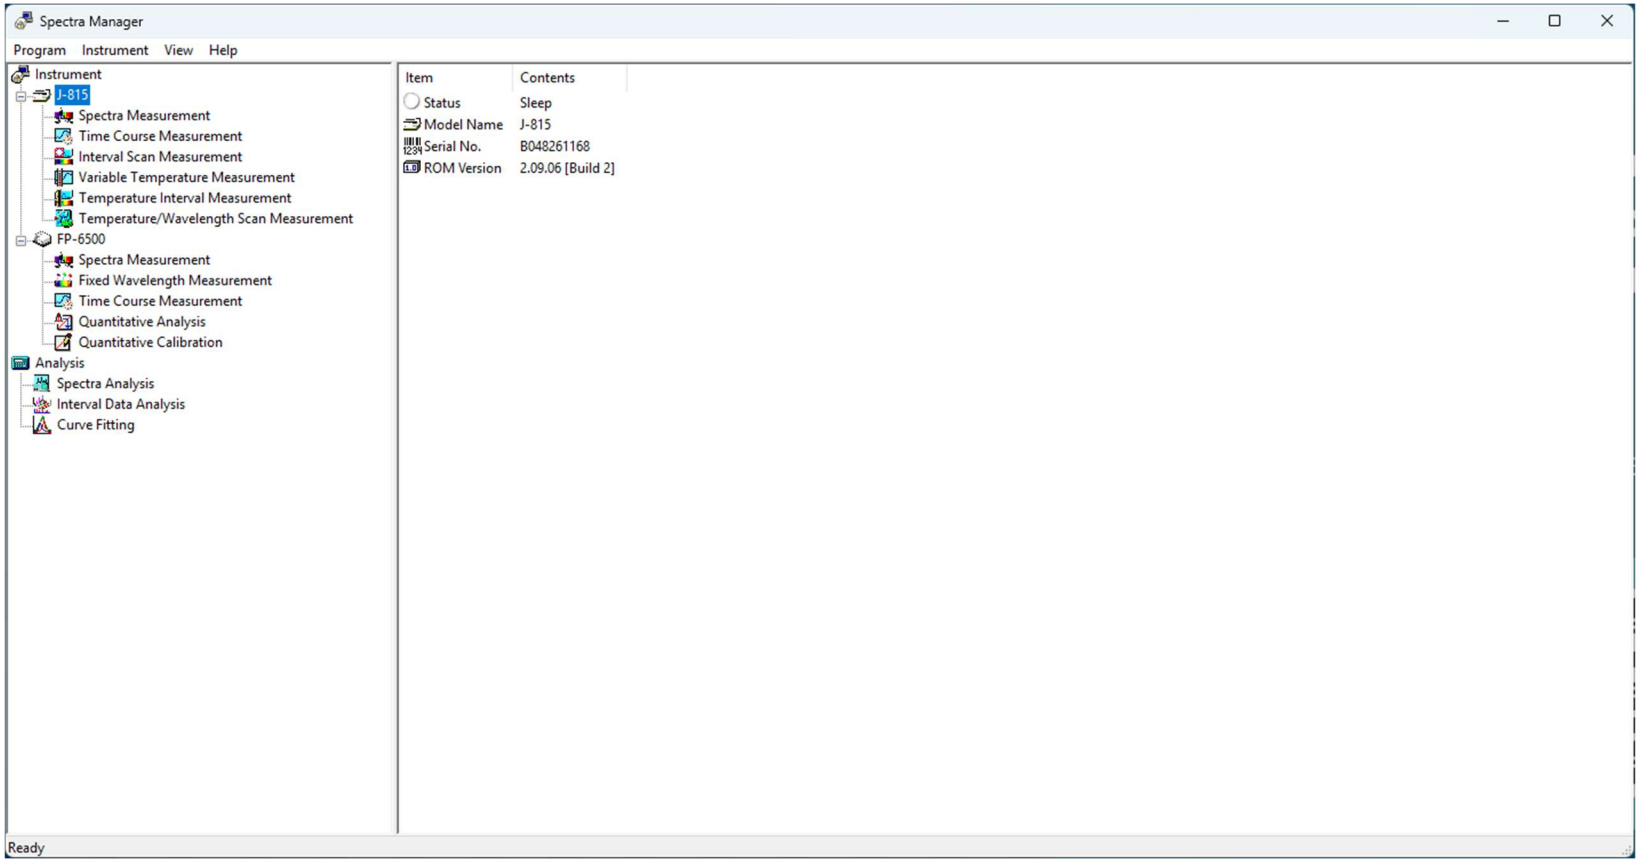


Software - 07.08.2026 - 17

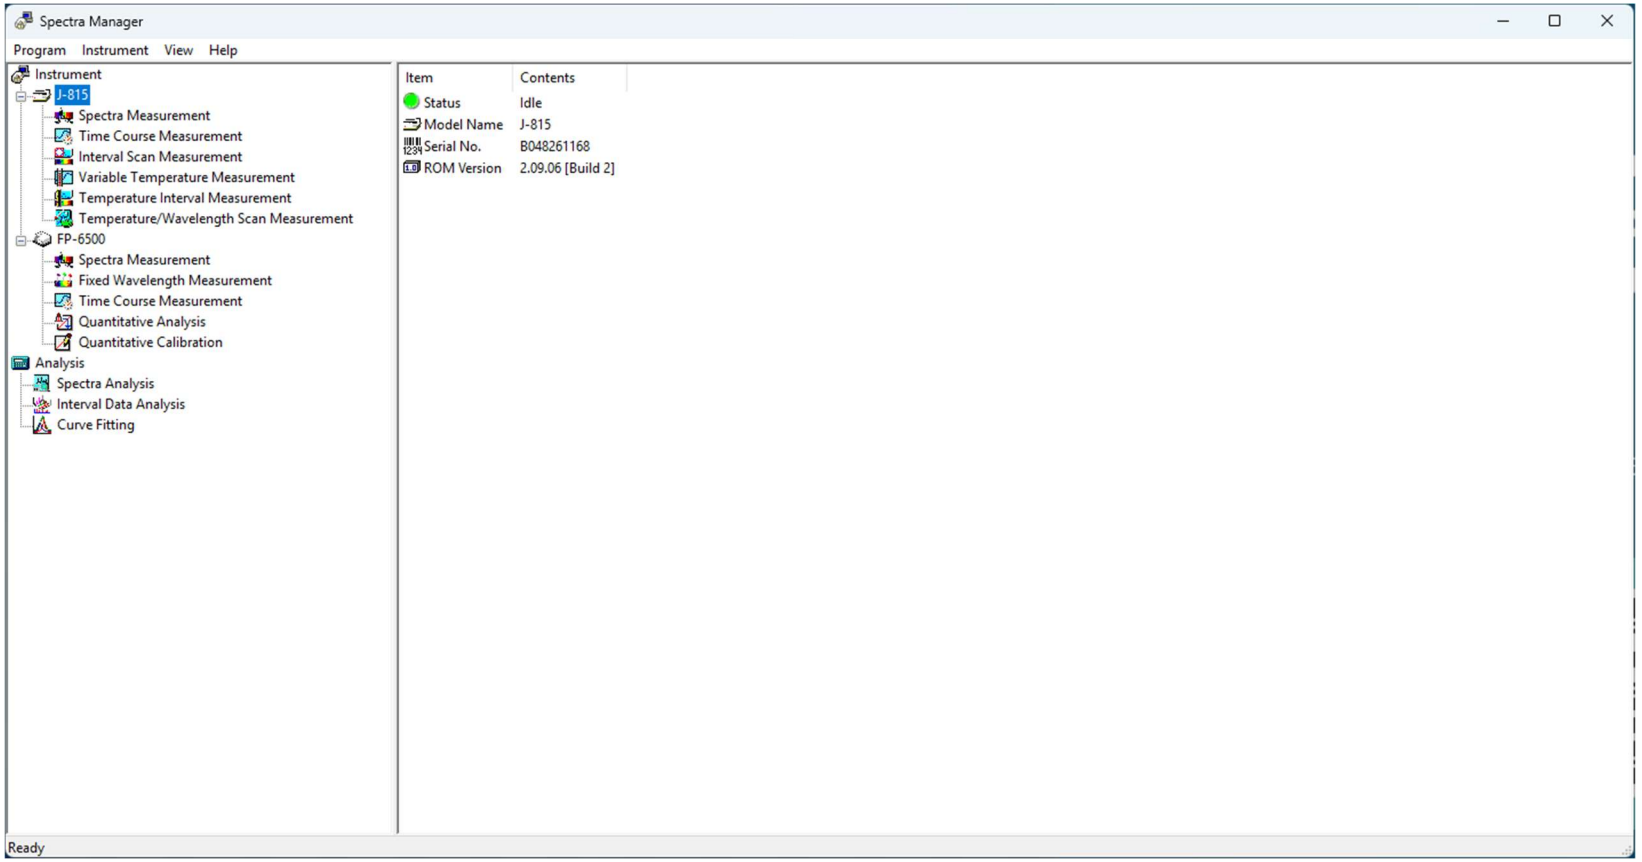


Software - 07.08.2026 - 18

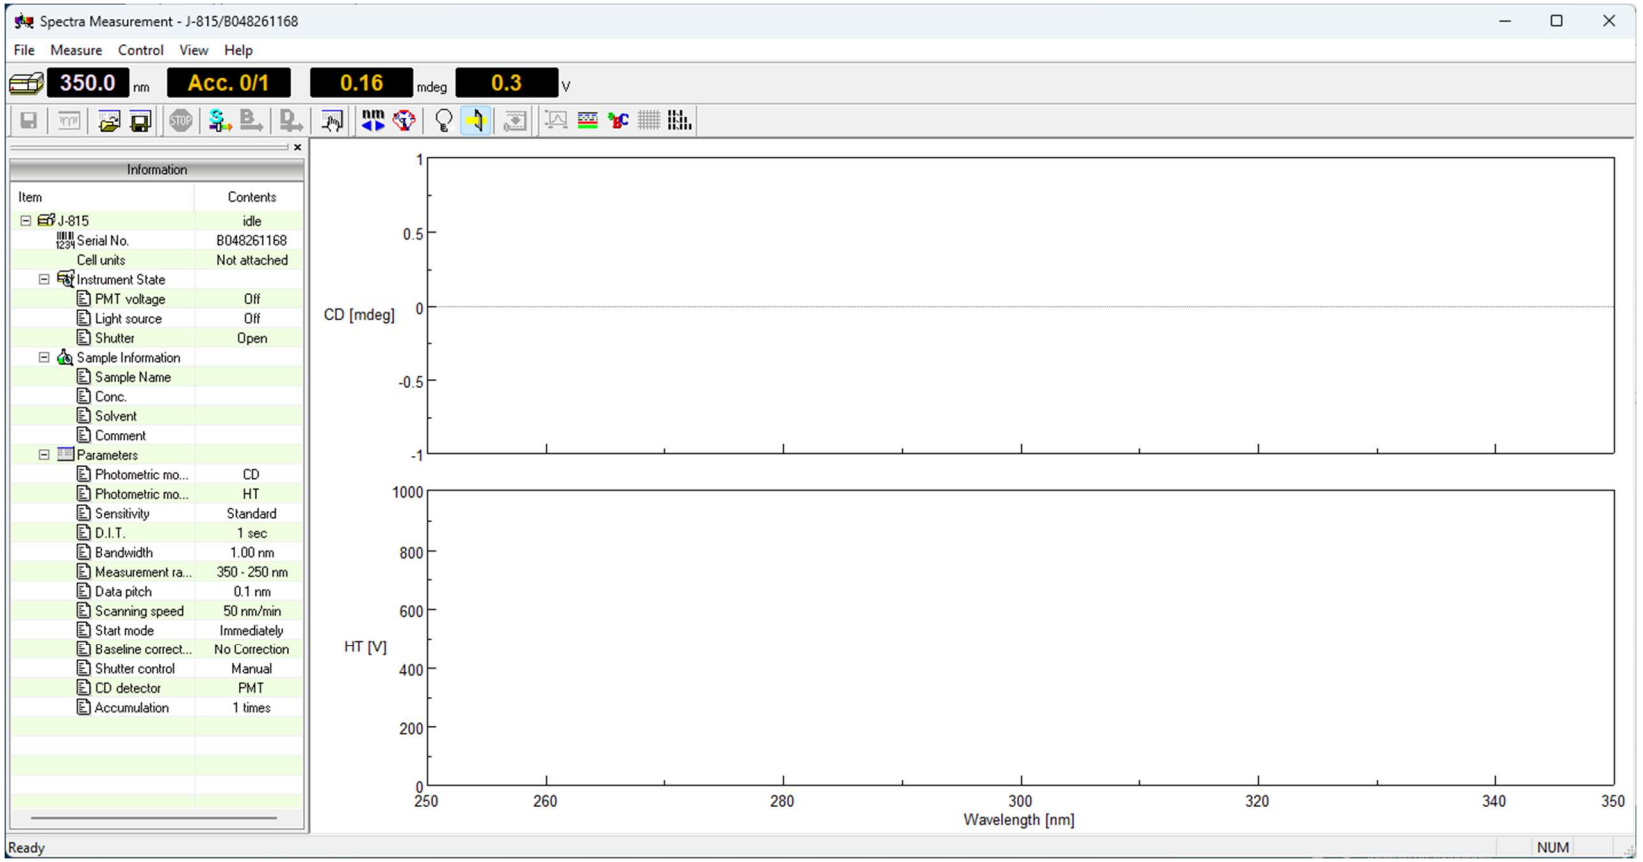


Software - 07.08.2026 - 19

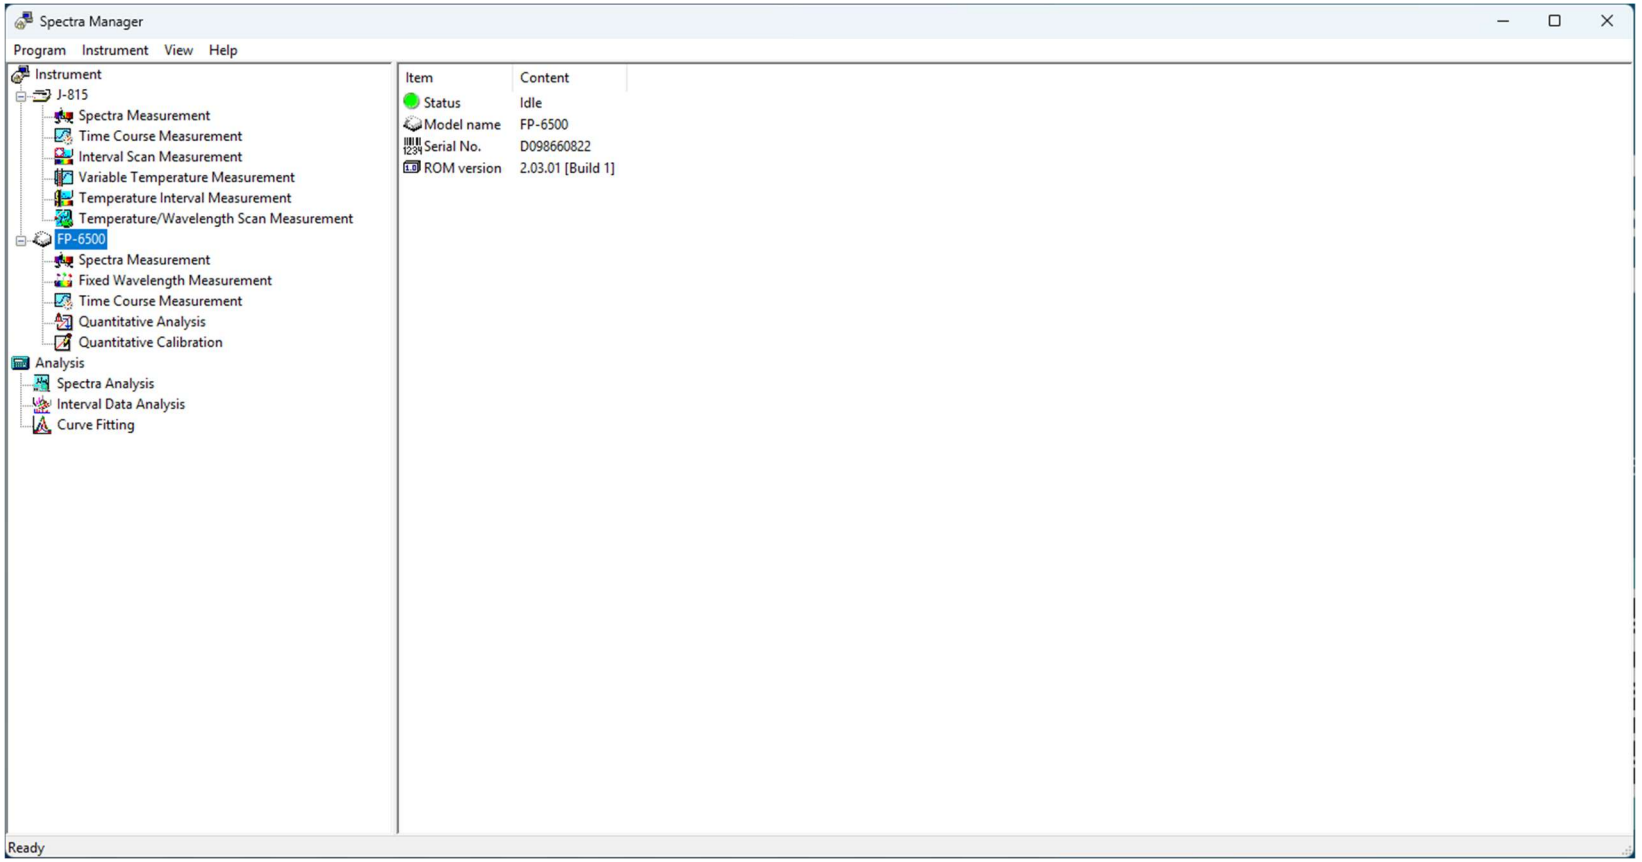


Software - 07.08.2026 - 20

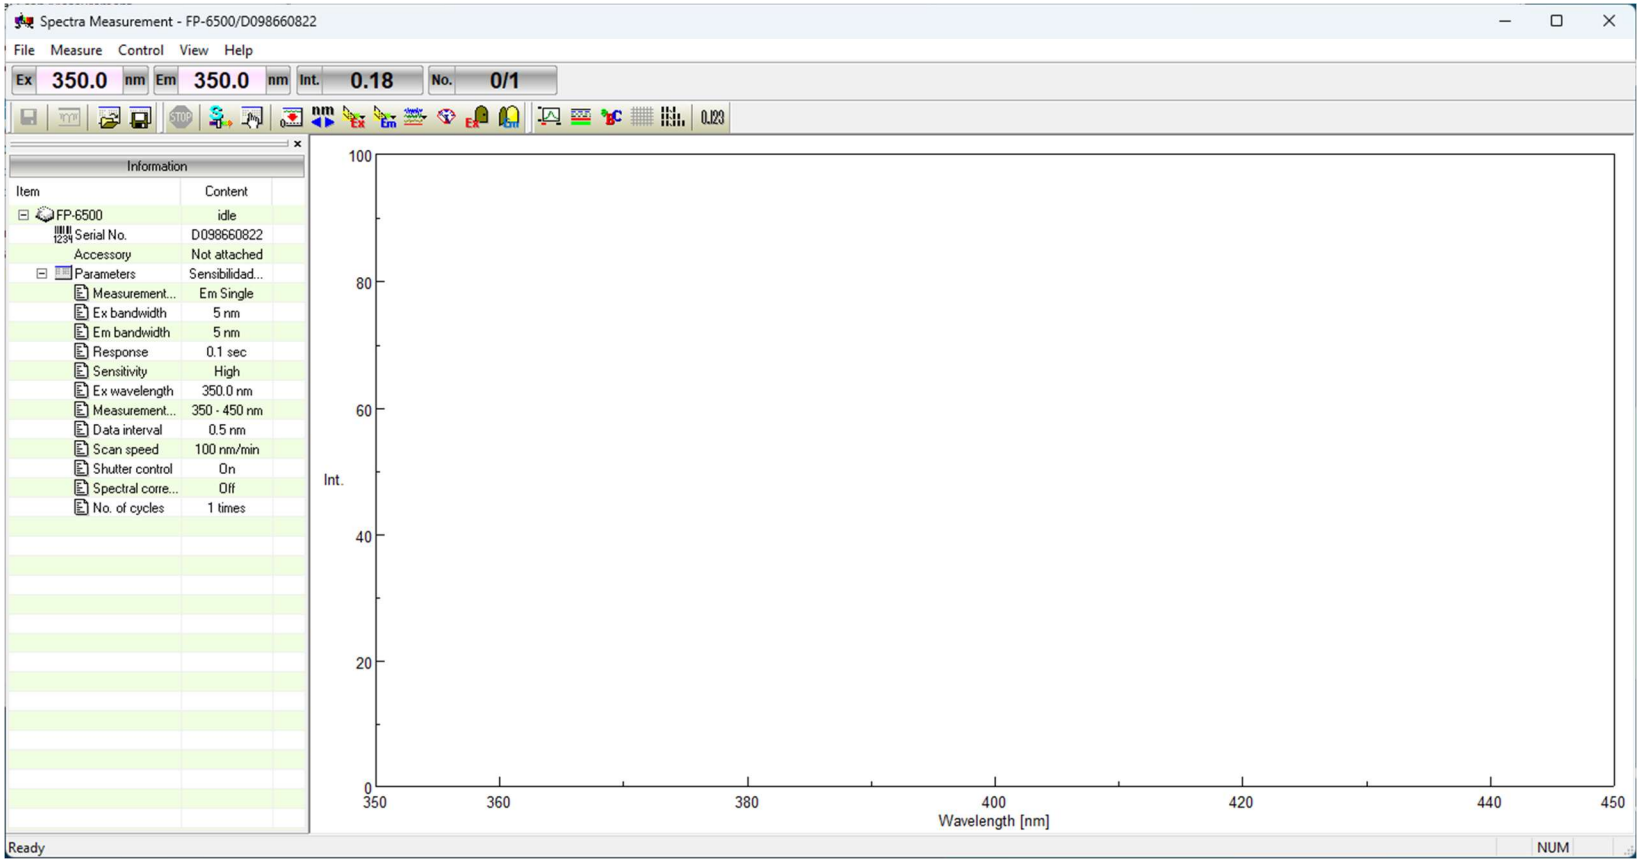


Software - 07.08.2026 - 21

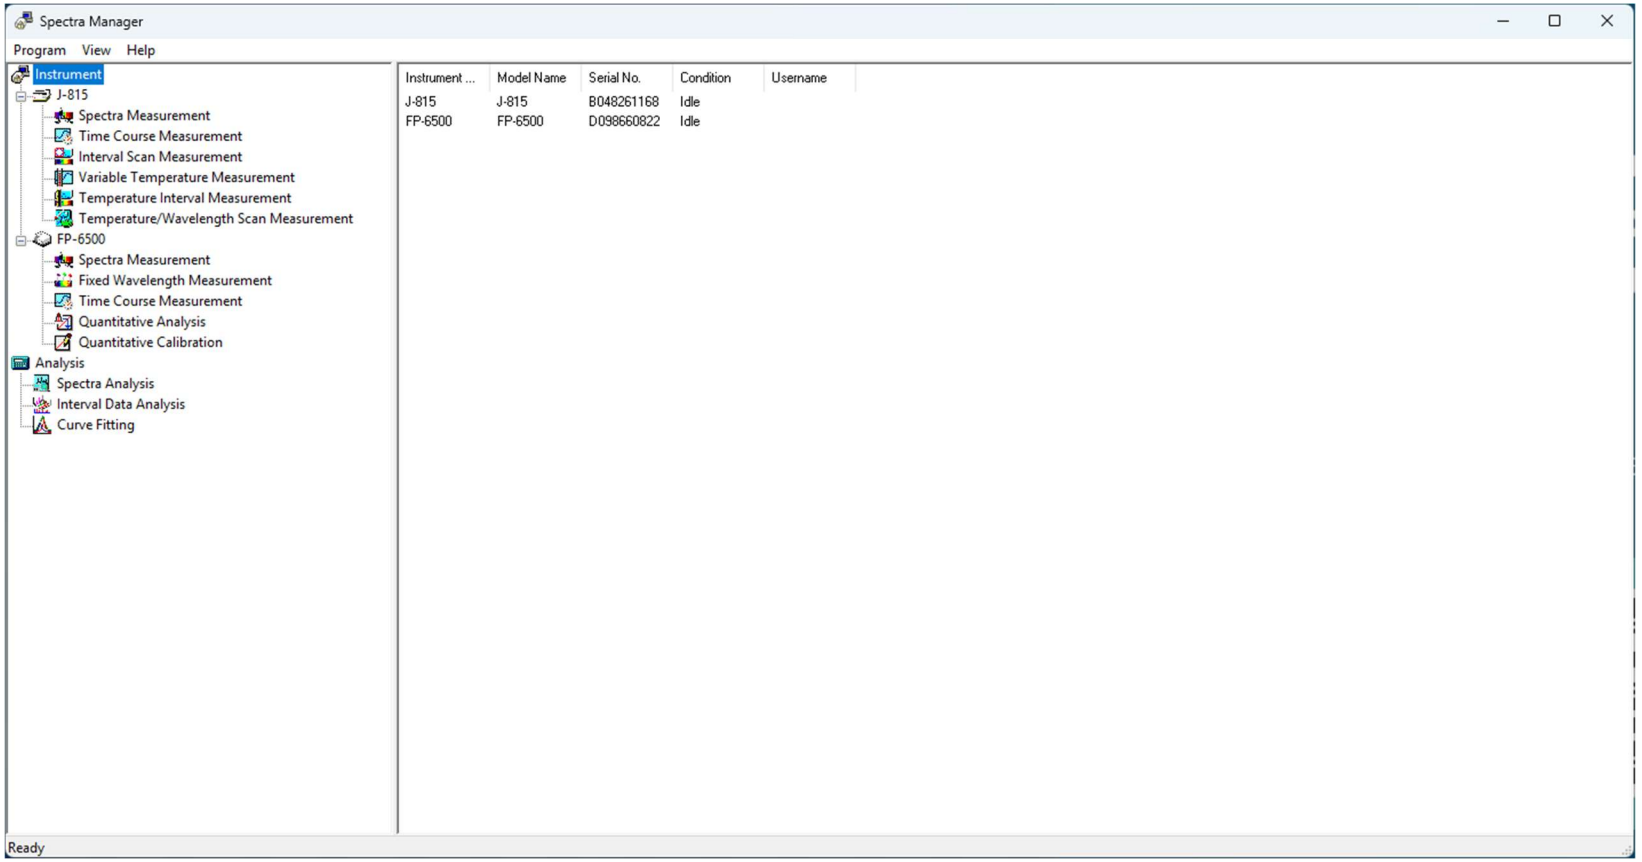


Software - 07.08.2026 - 22

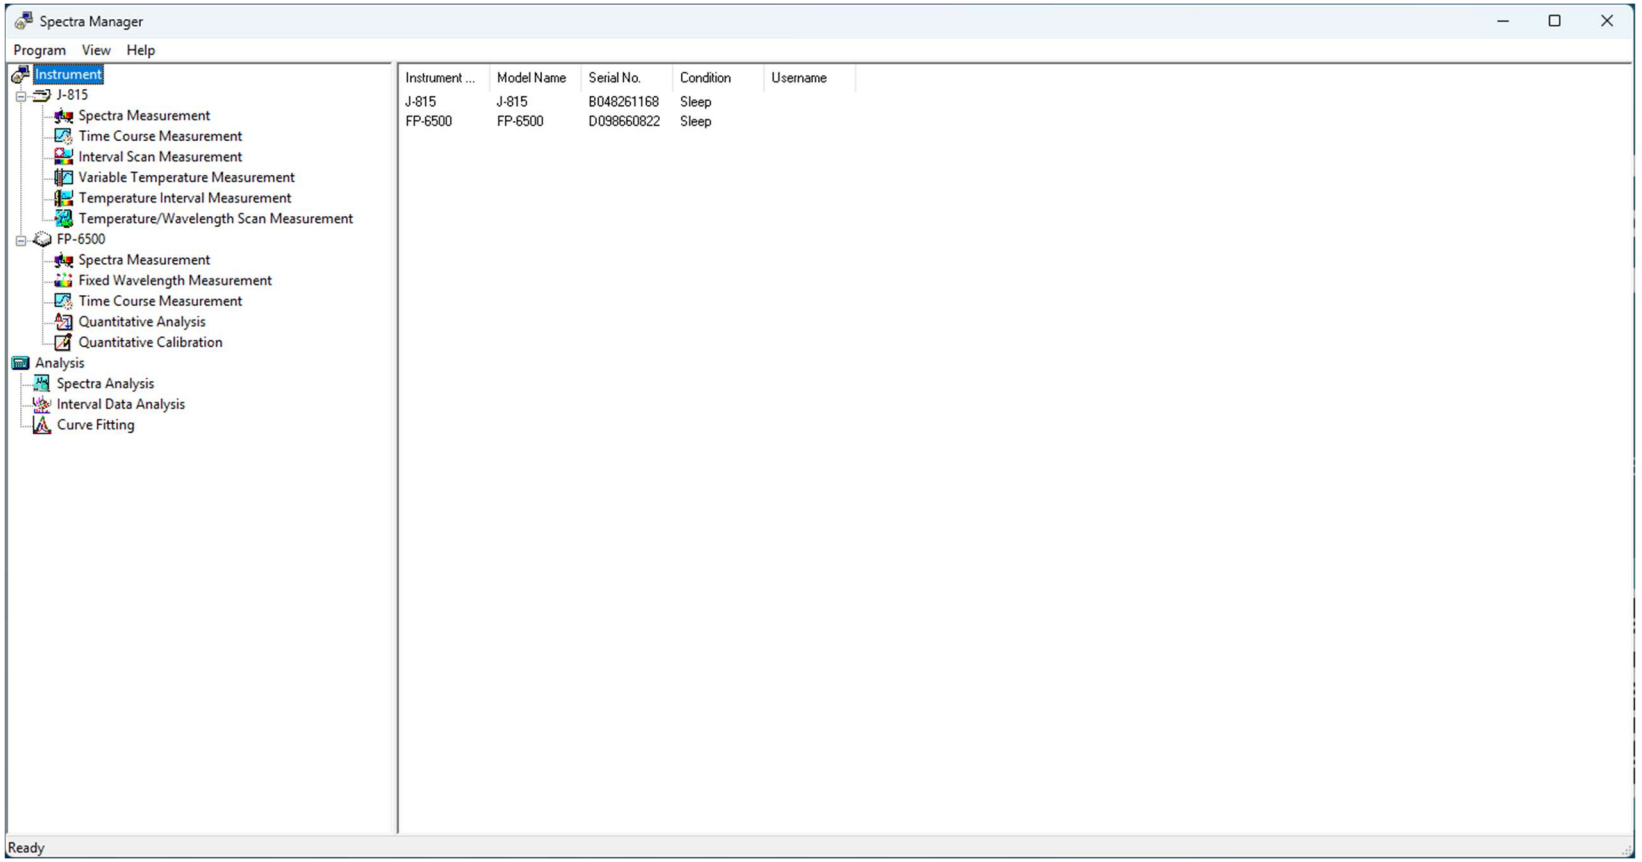


Software - 07.08.2026 - 23

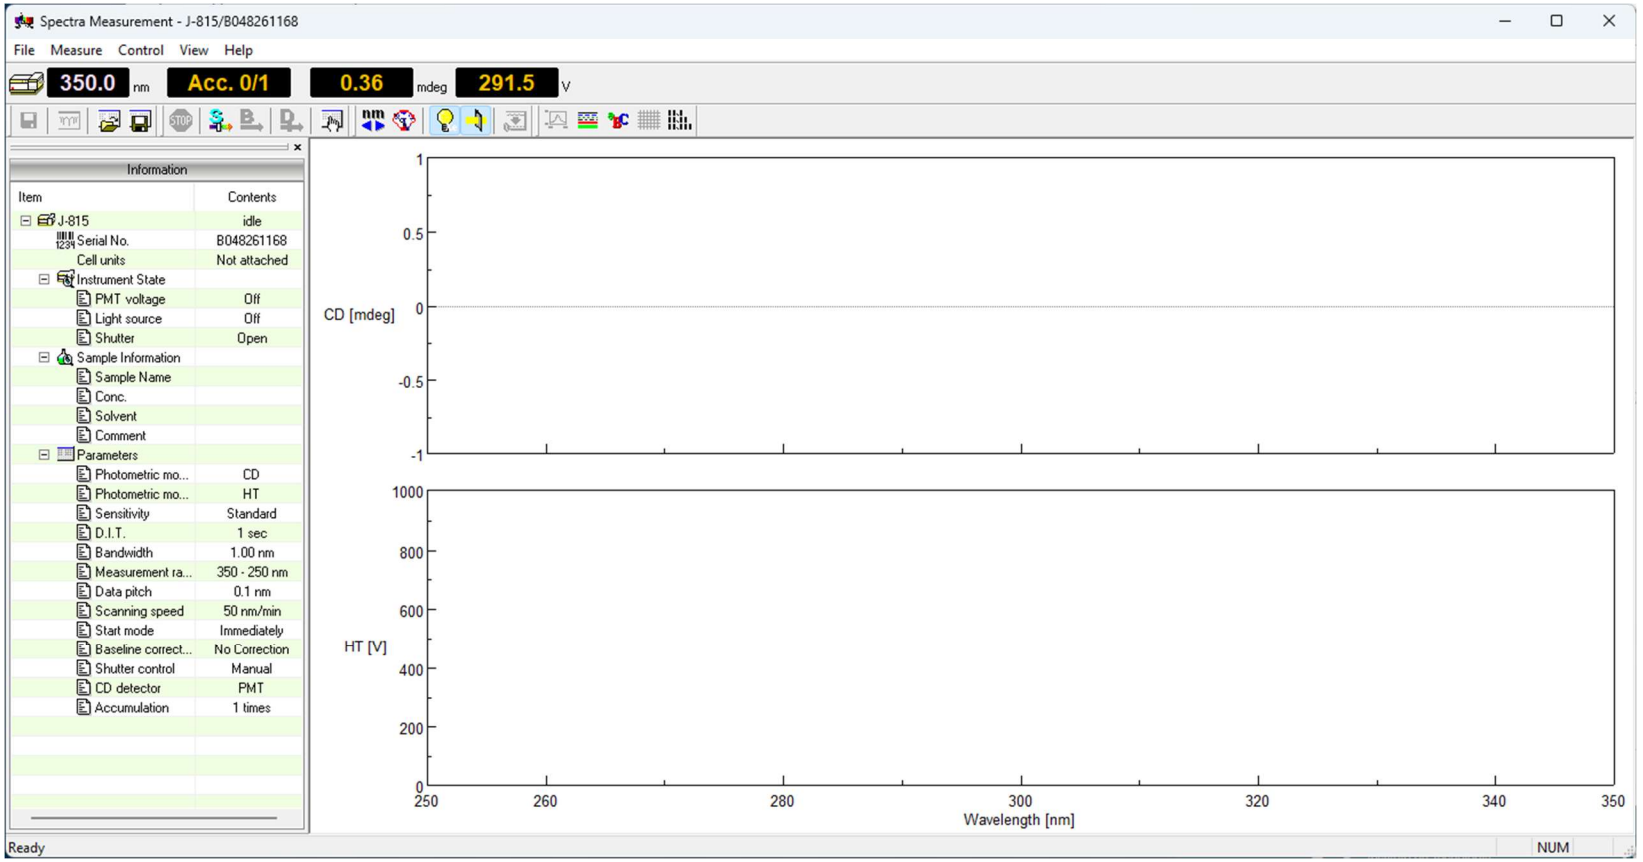


Software - 07.08.2026 - 24

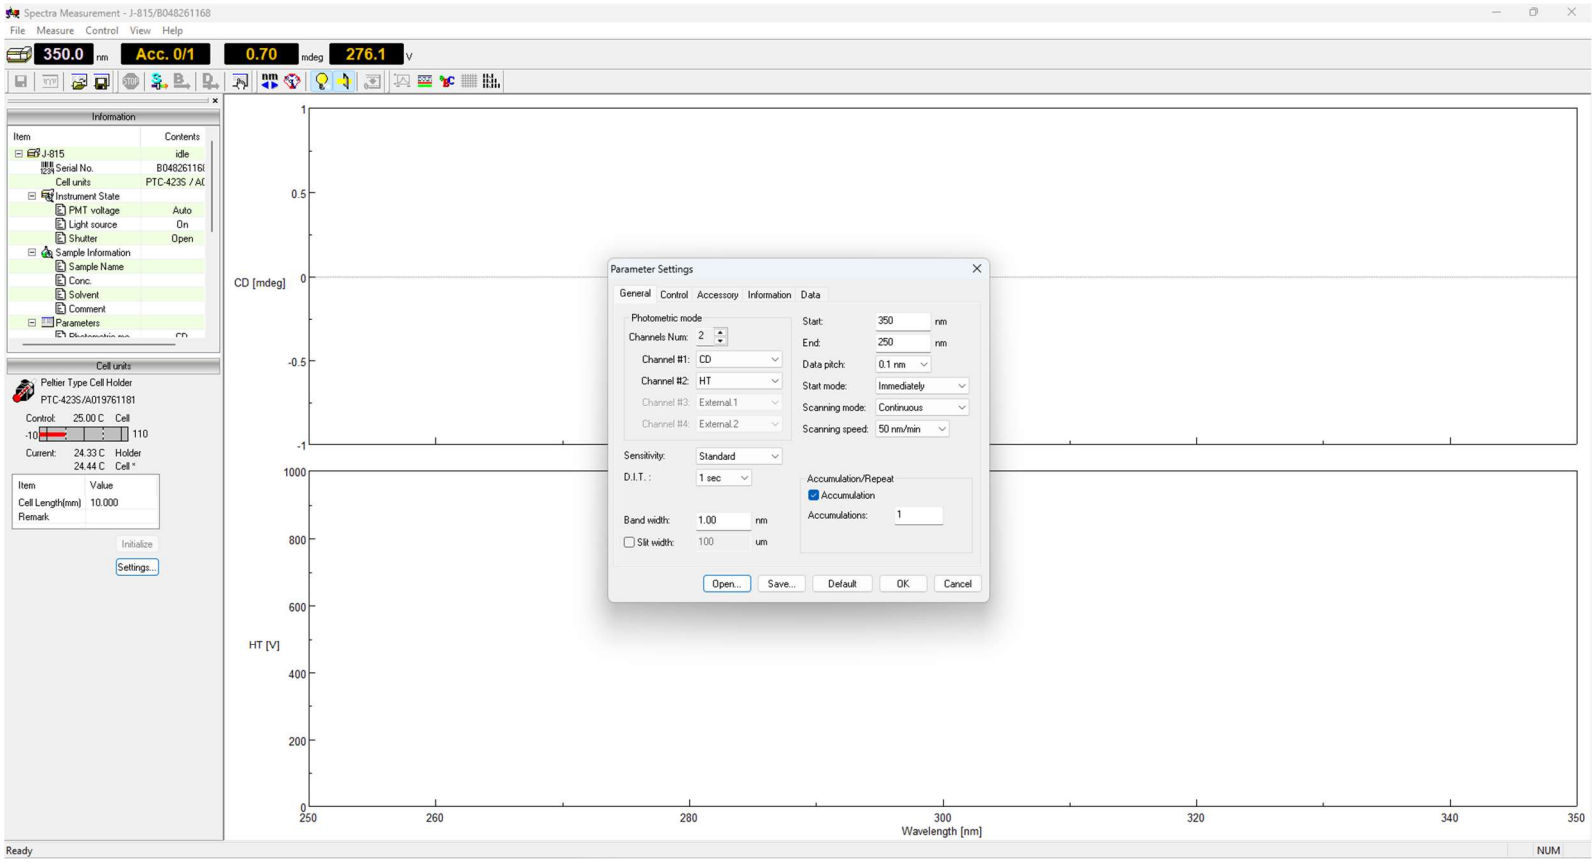


Software - 07.08.2026 - 25

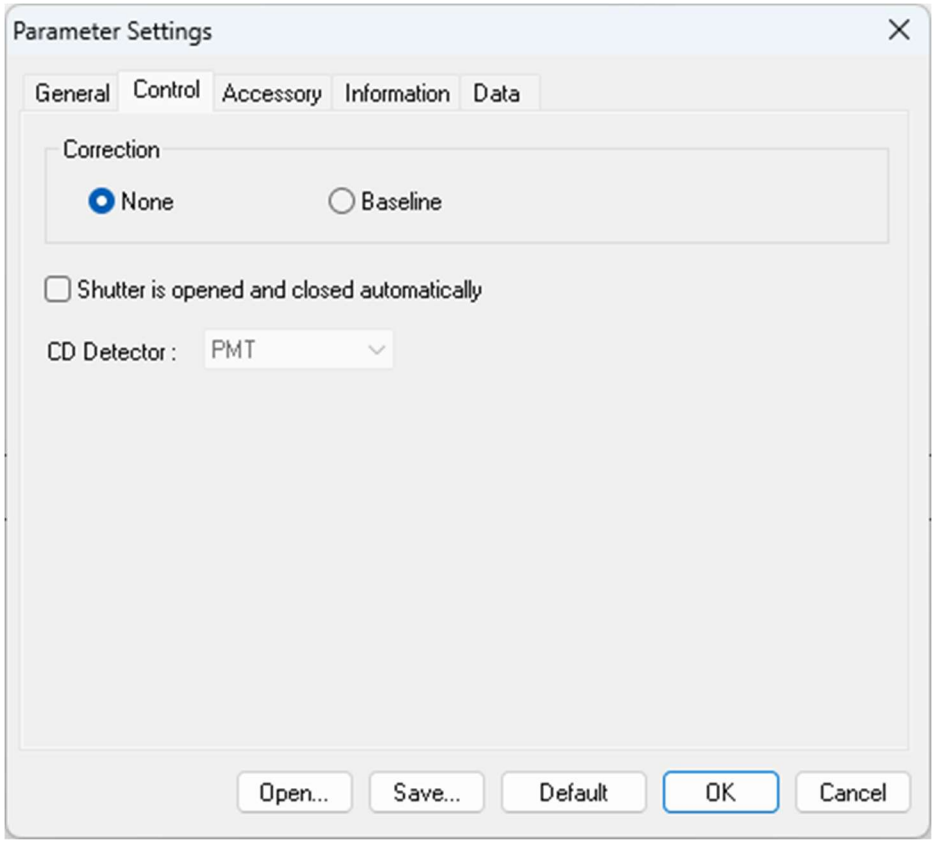


Software - 07.08.2026 - 26

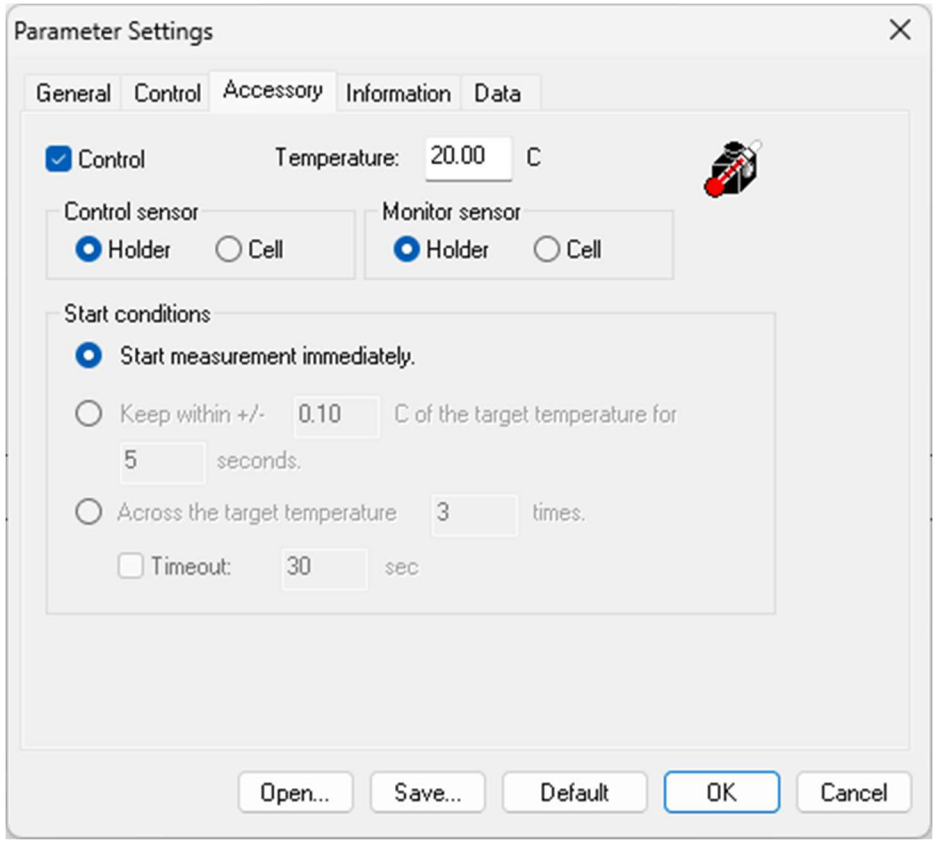


Software - 07.08.2026 - 27

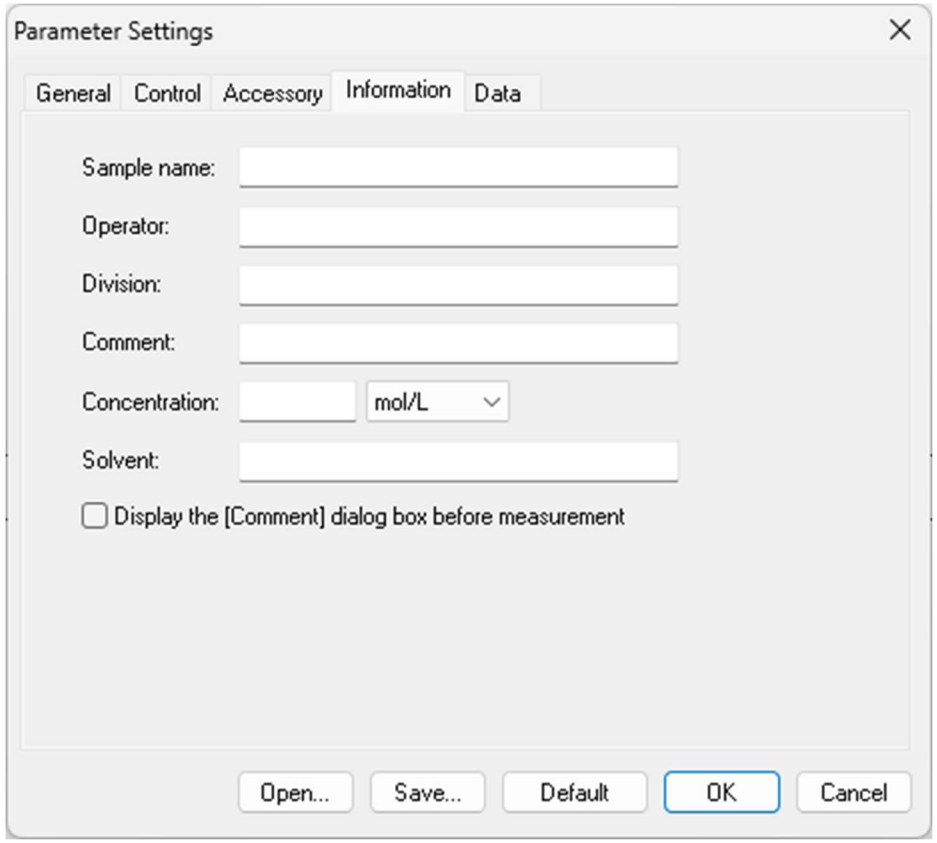


Software - 07.08.2026 - 28

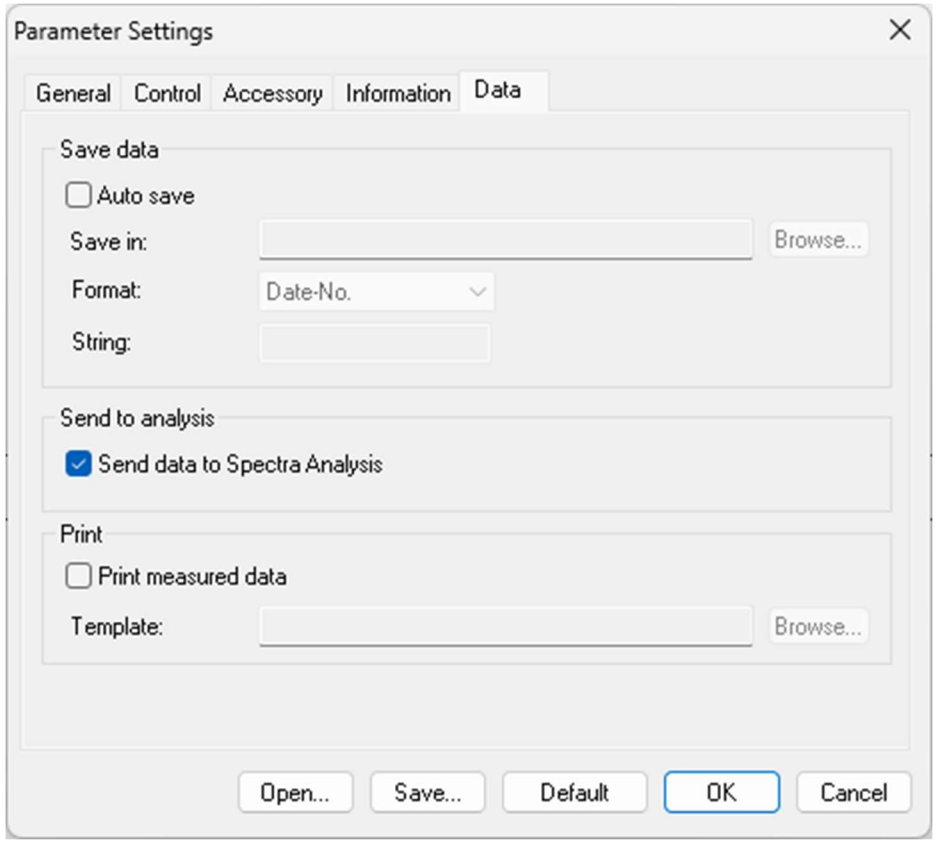


Software - 07.08.2026 - 29

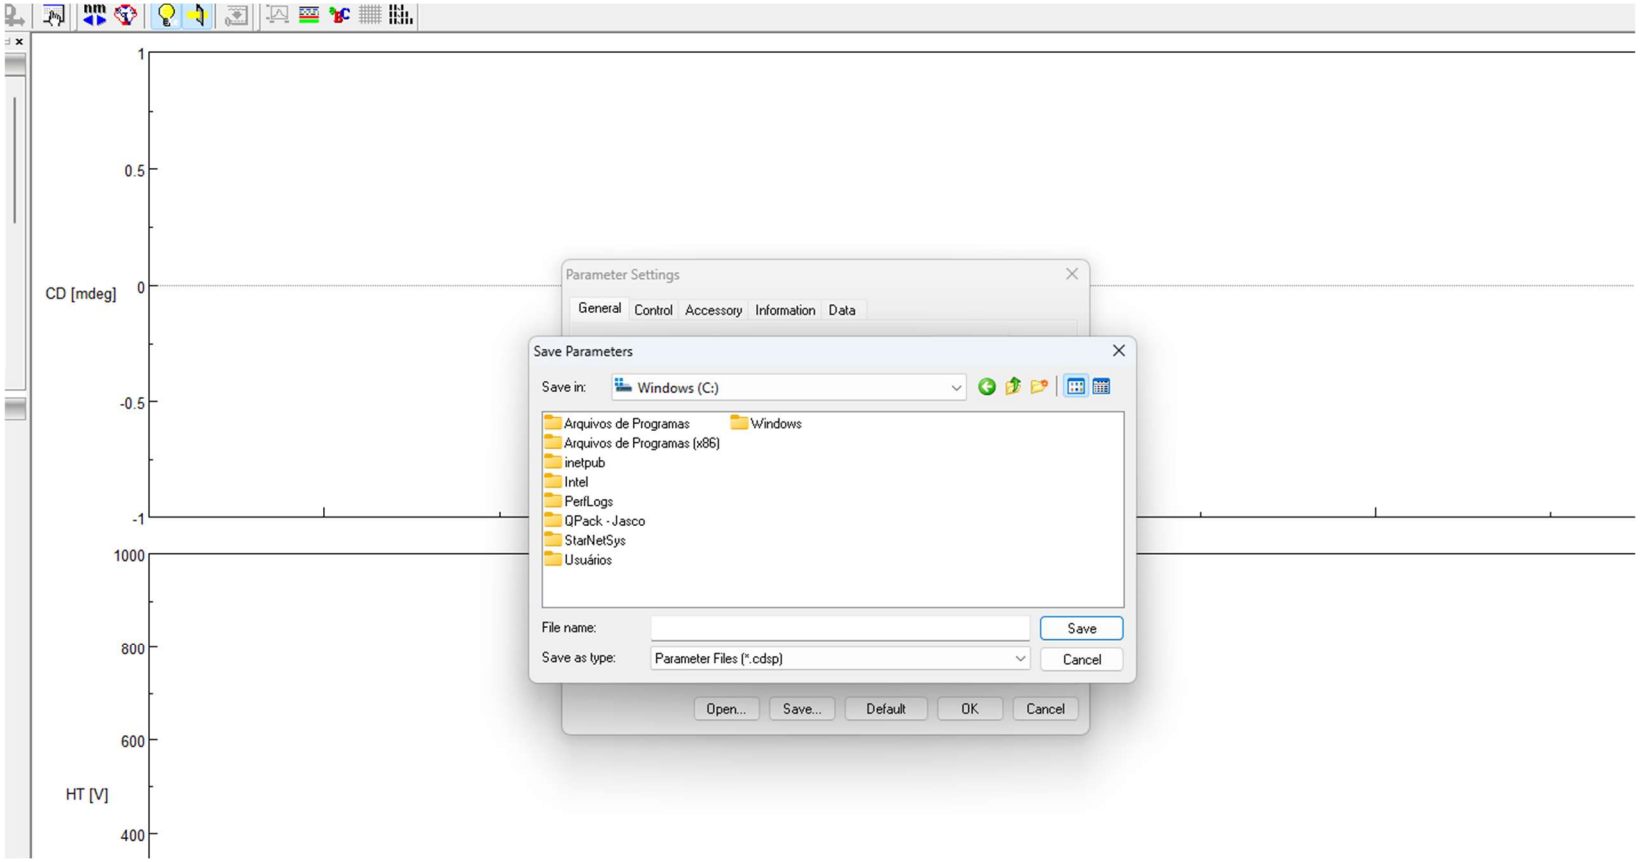


Software - 07.08.2026 - 30

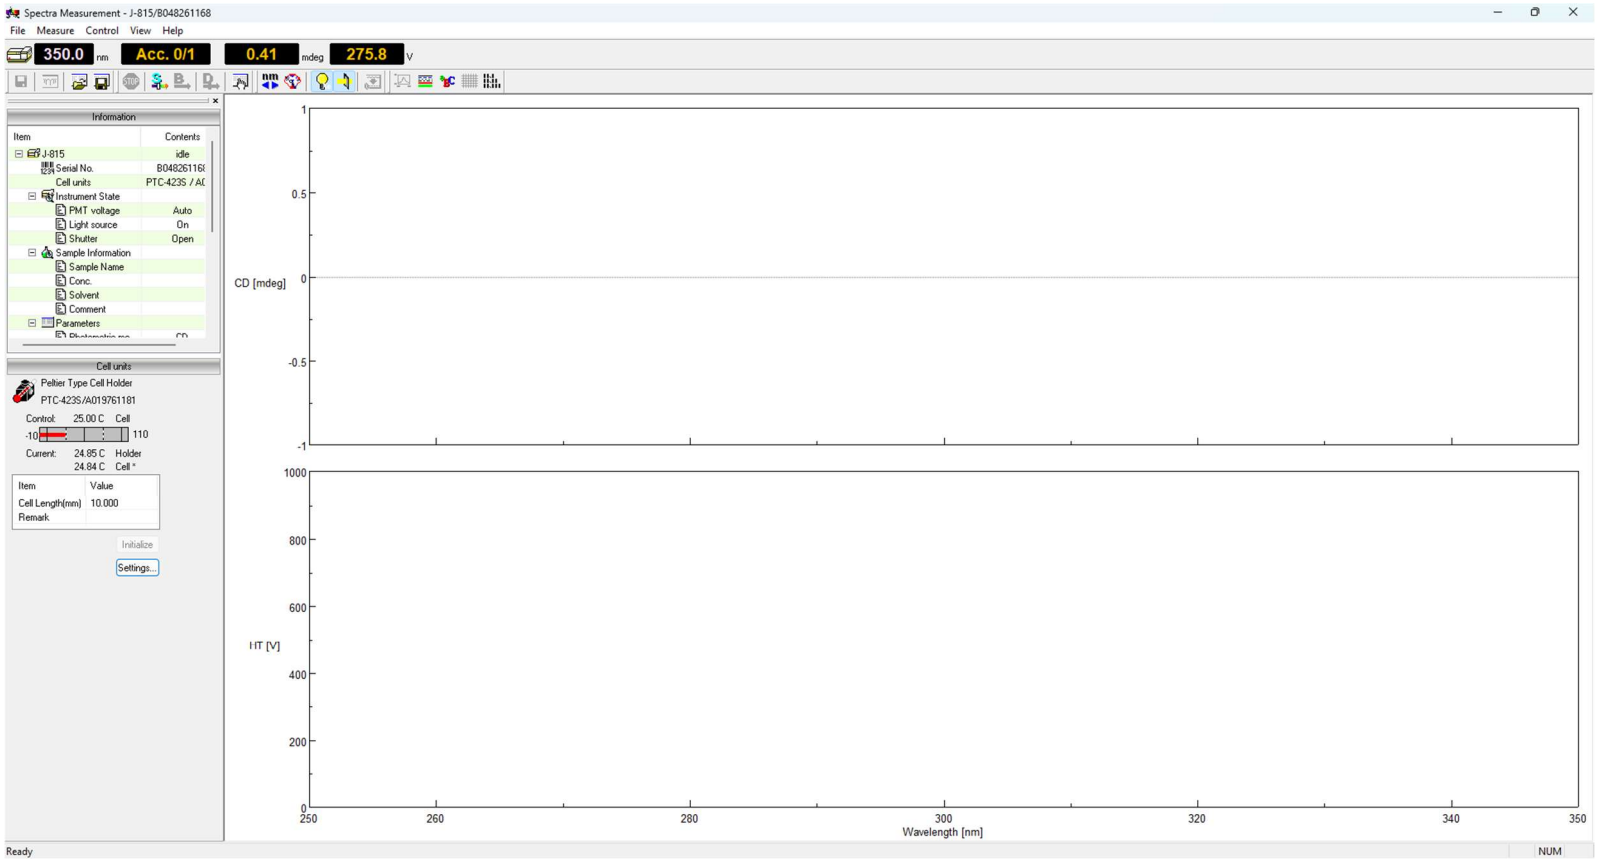


Software - 07.08.2026 - 31

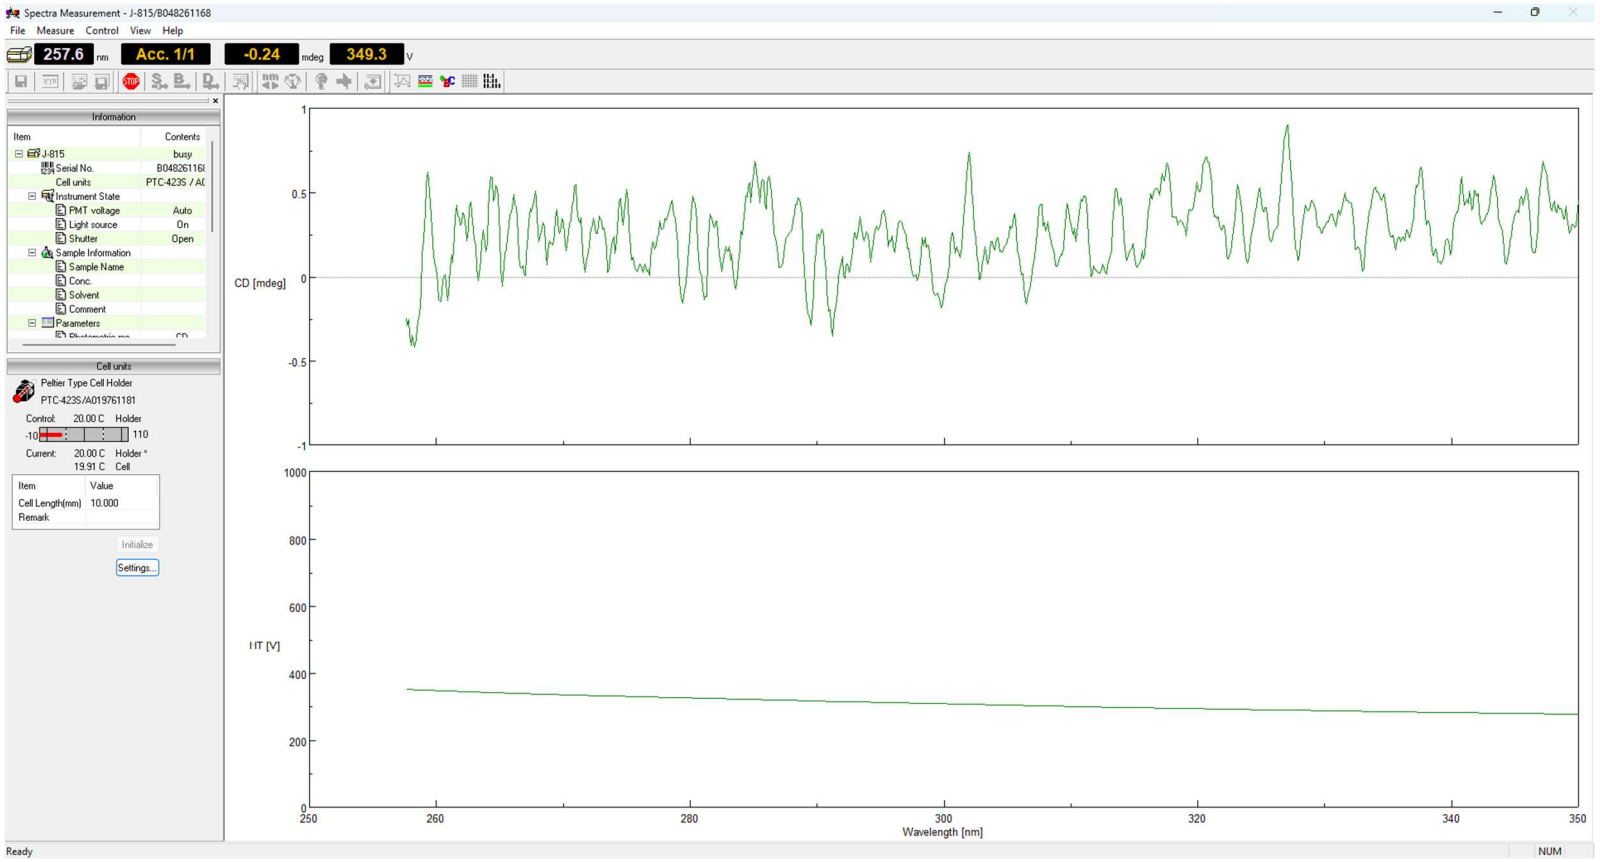


Software - 07.08.2026 - 32

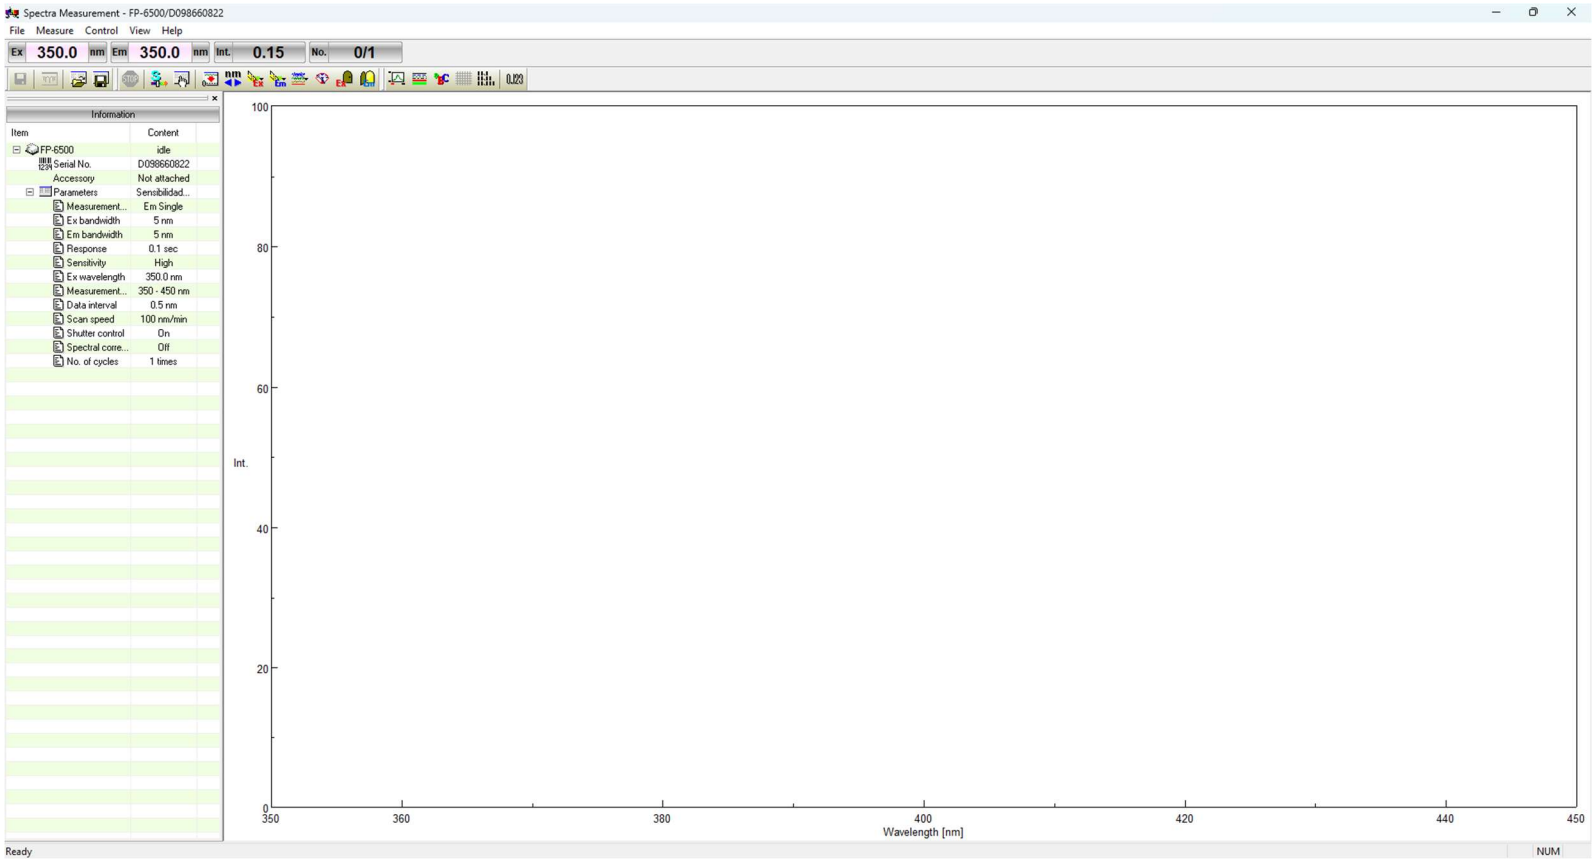


Software - 07.08.2026 - 33

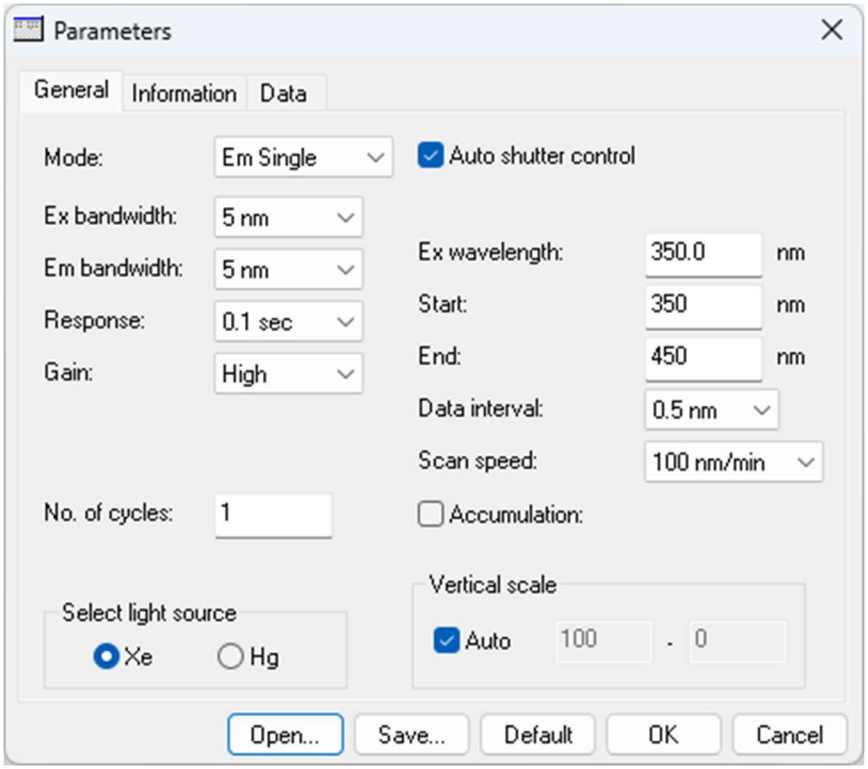


Software - 07.08.2026 - 34

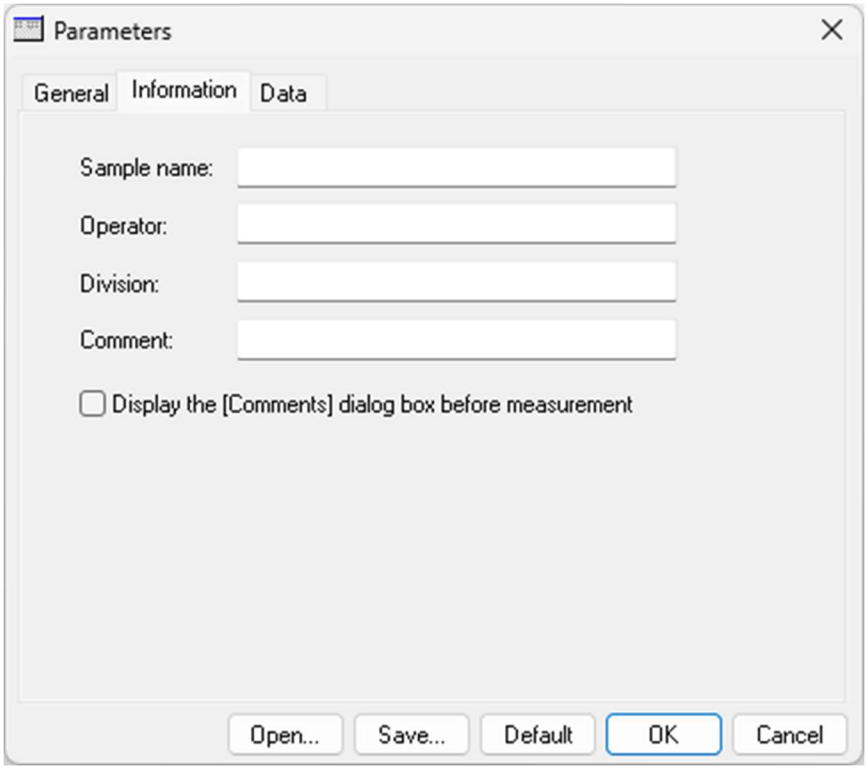


Software - 07.08.2026 - 35

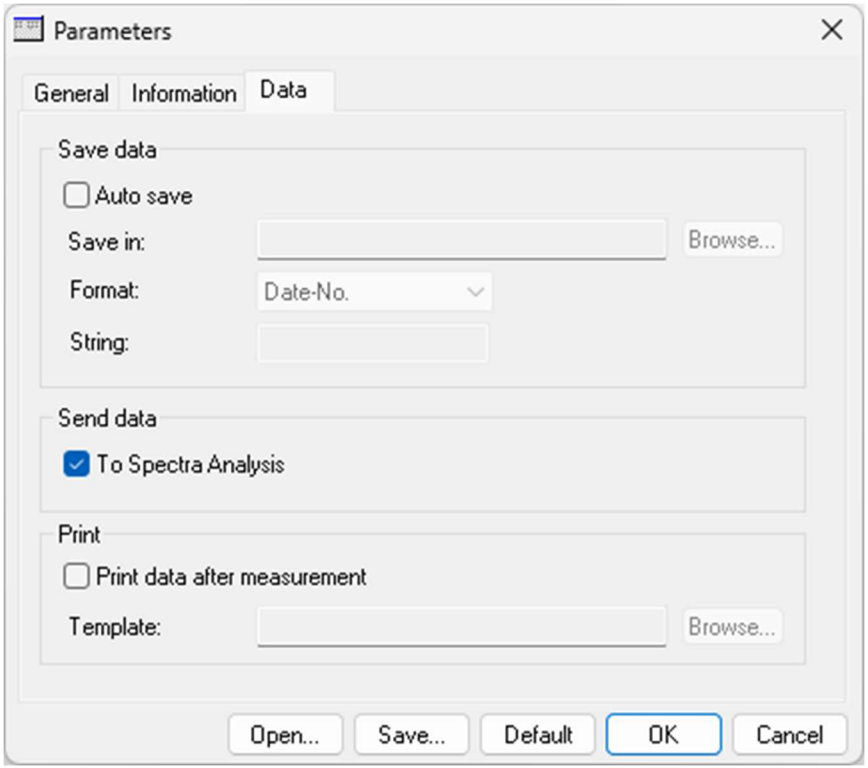


Software - 07.08.2026 - 36

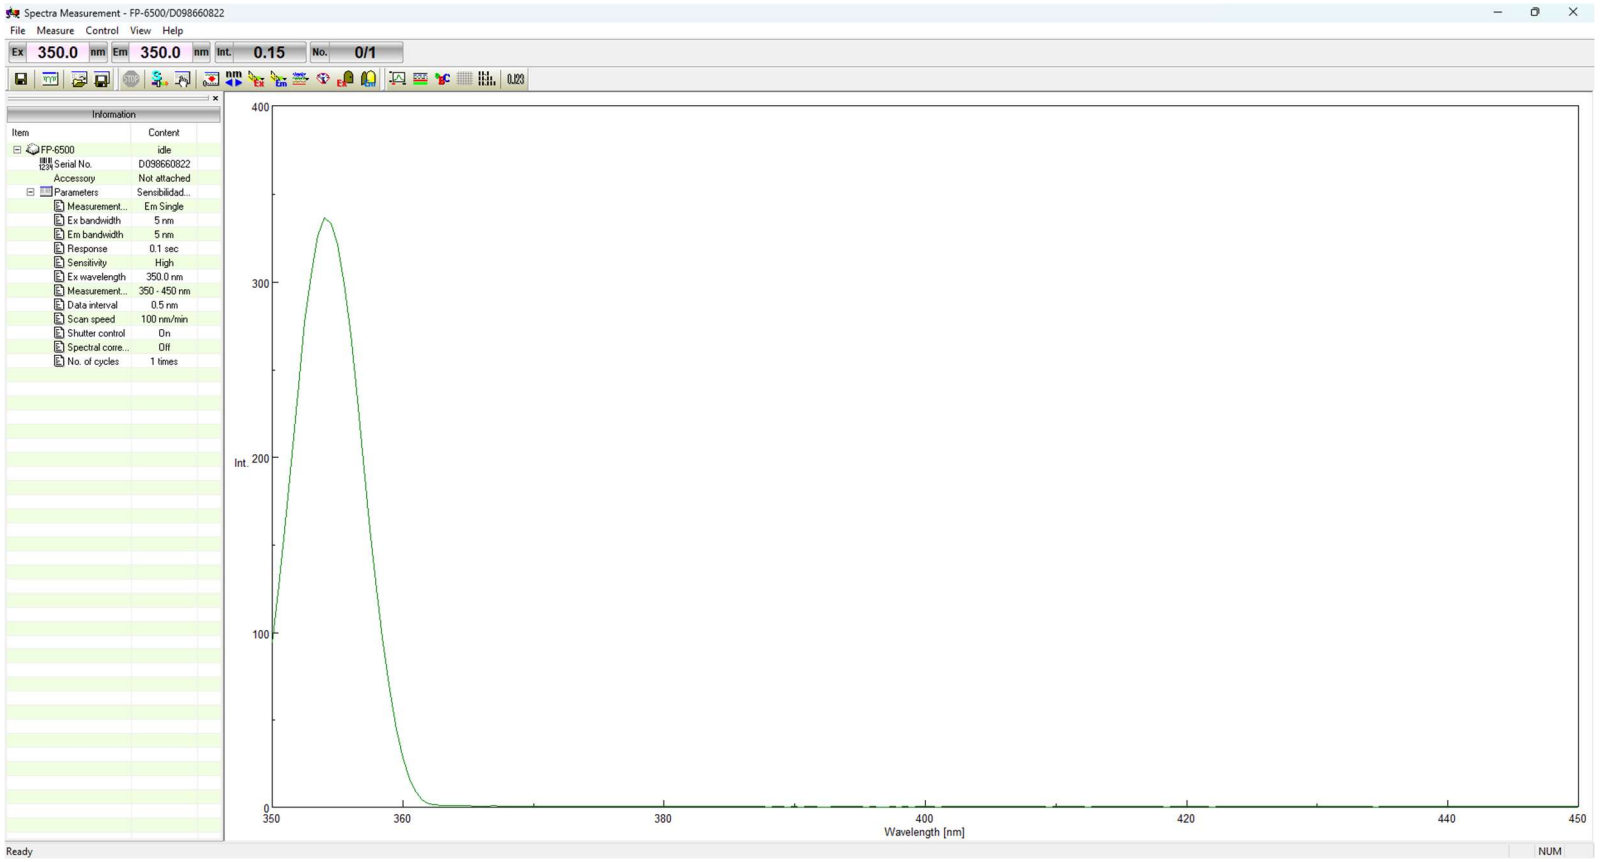


Software - 07.08.2026 - 37

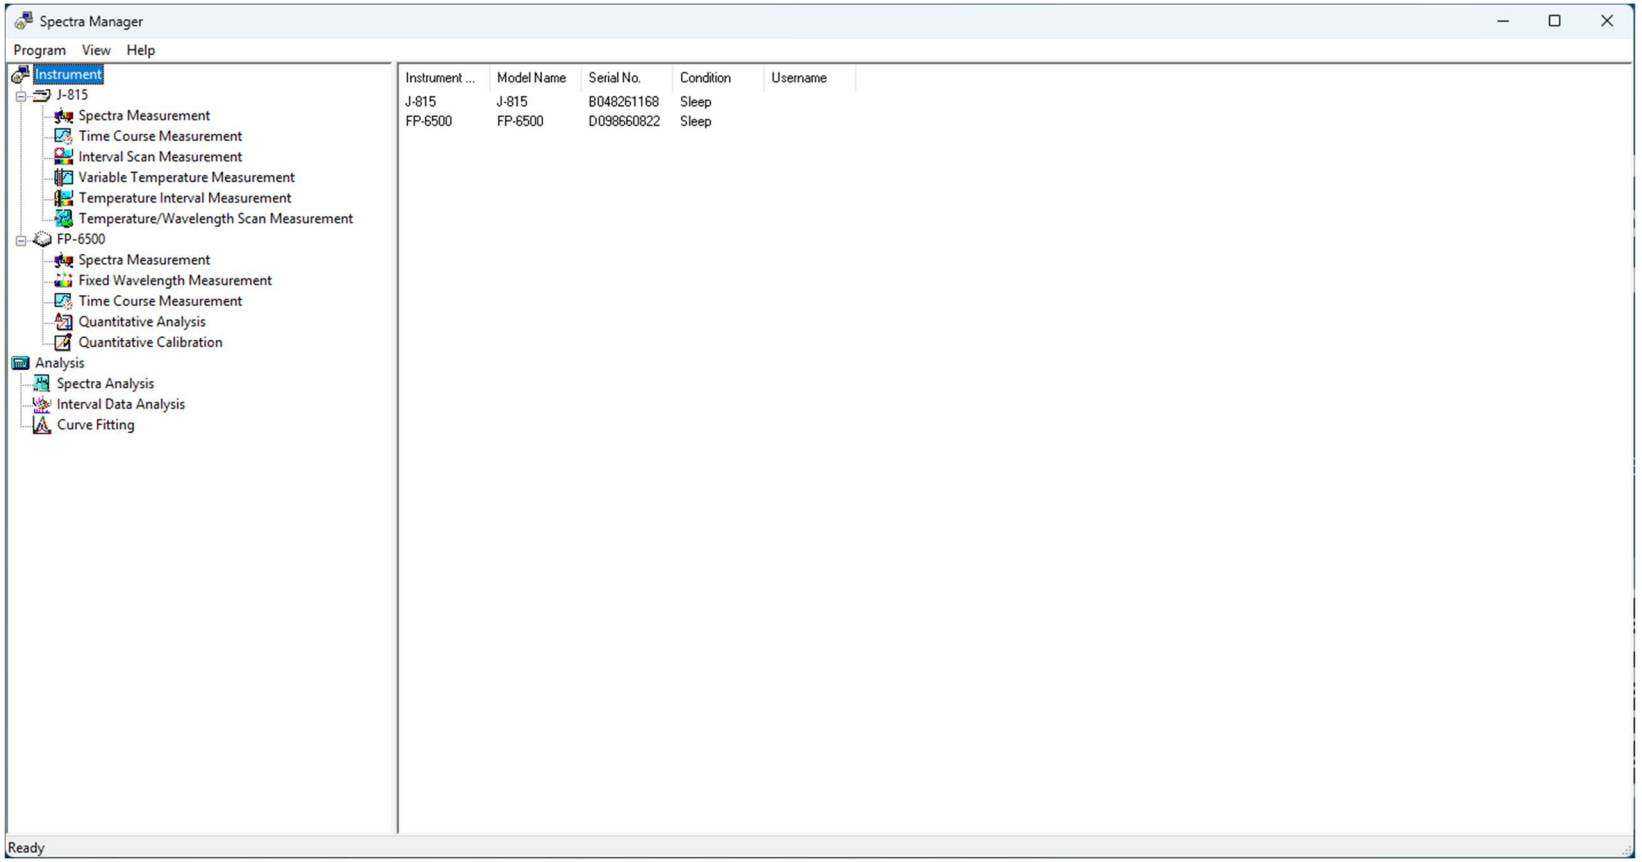


Software - 07.08.2026 - 38

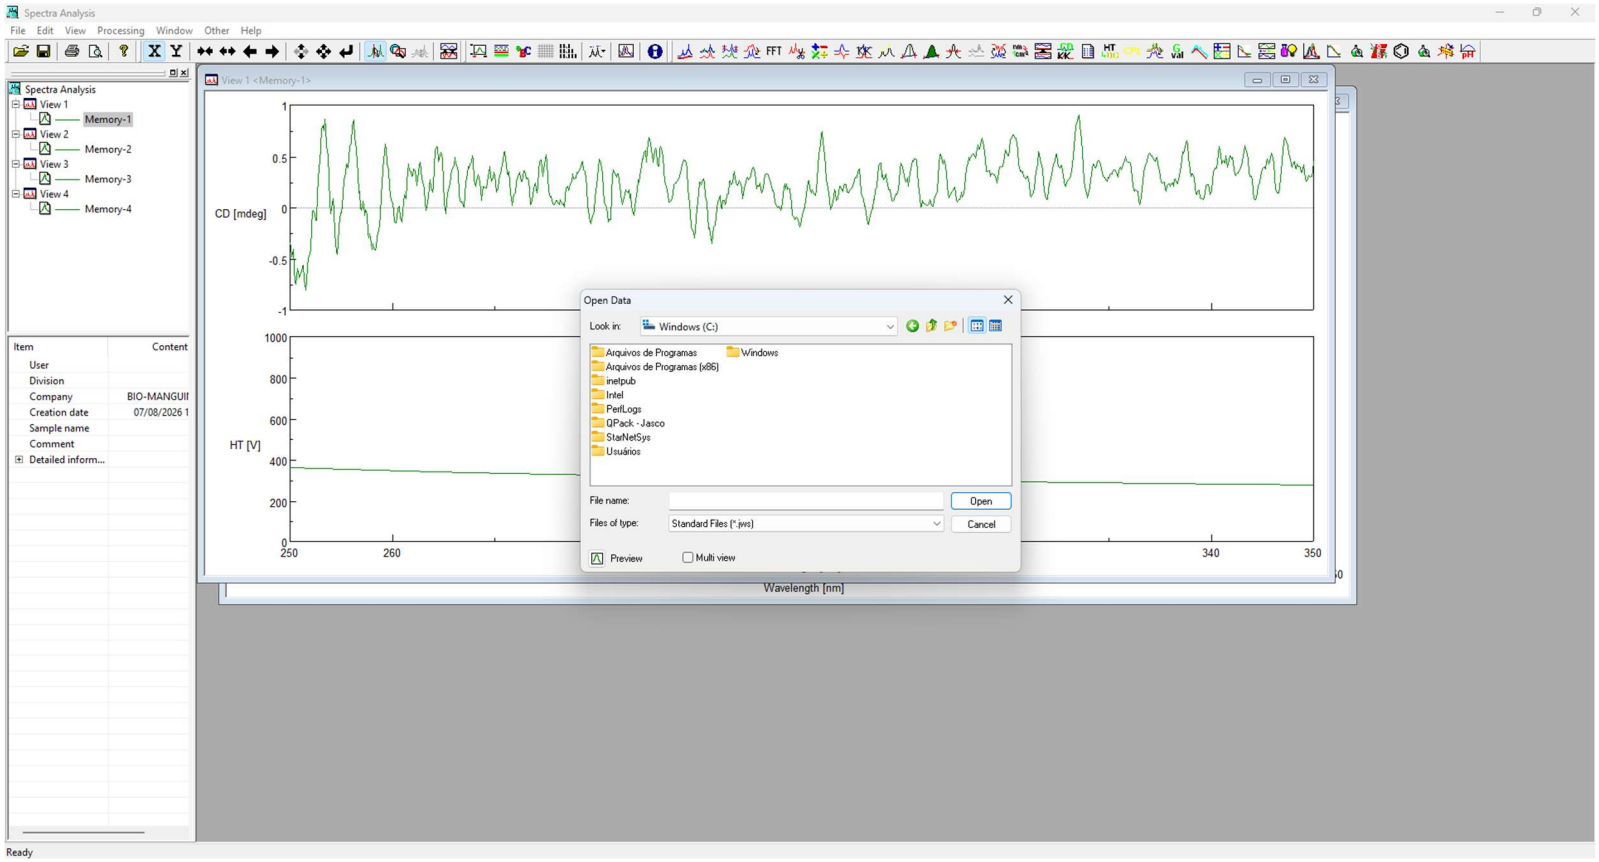


Software - 07.08.2026 - 39

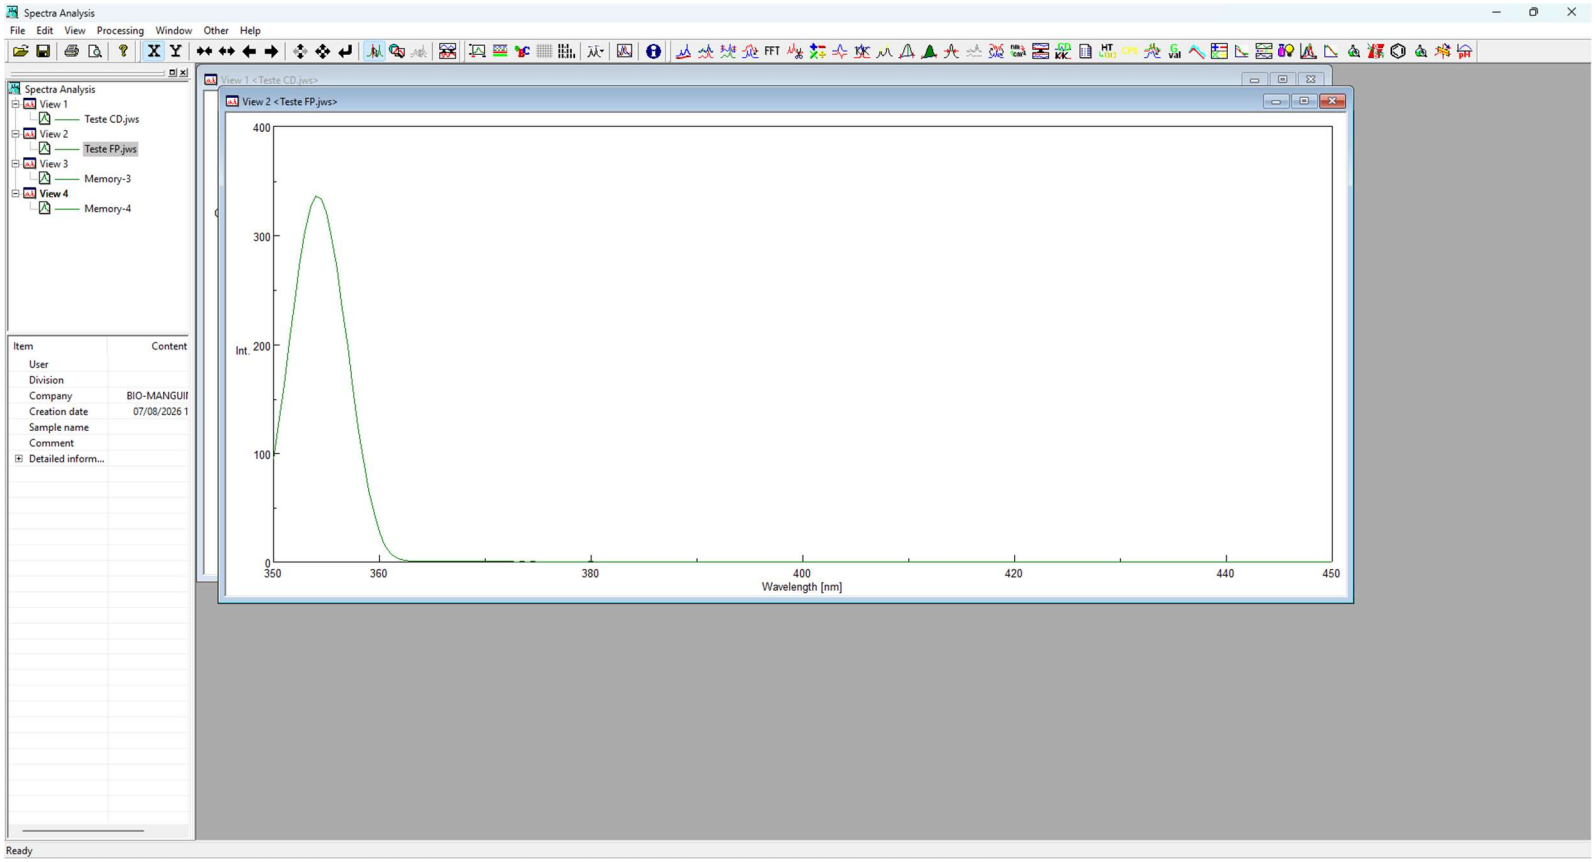


Software - 07.08.2026 - 40

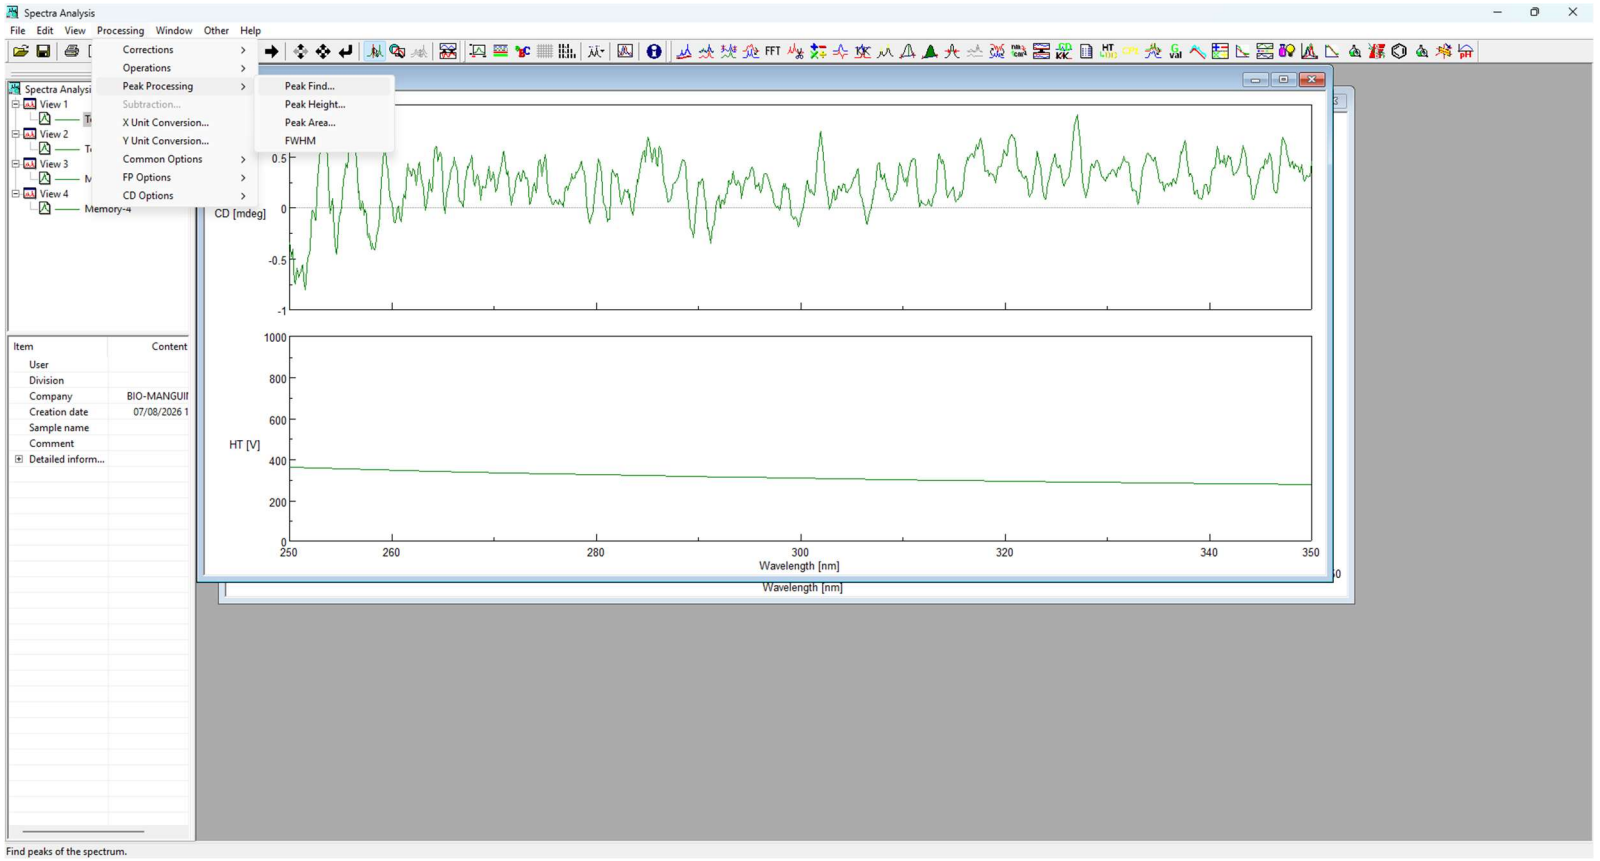


Software - 07.08.2026 - 41

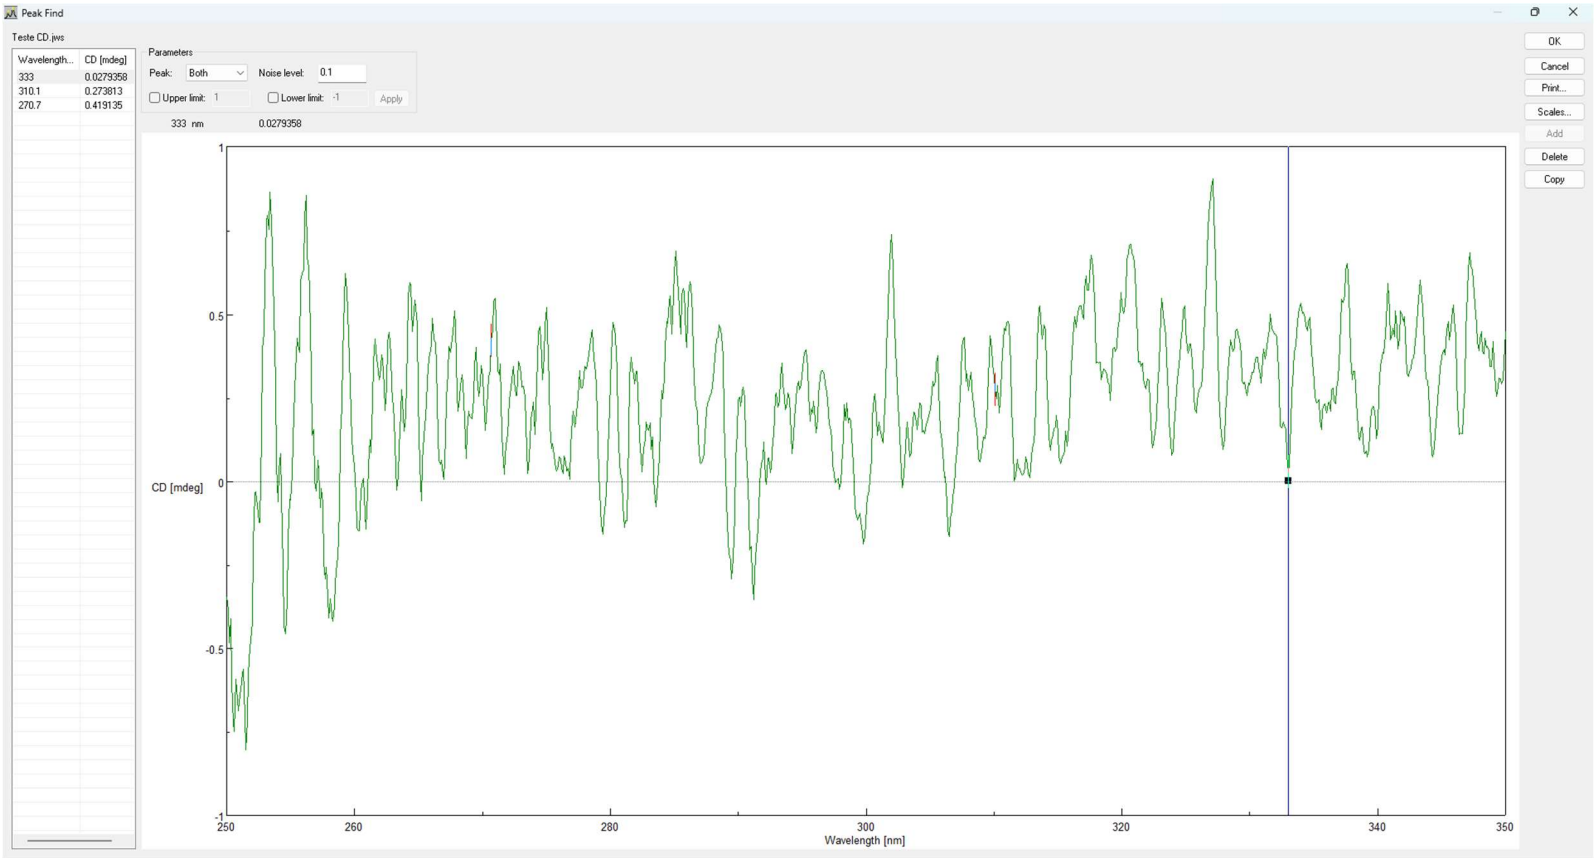


Software - 07.08.2026 - 42

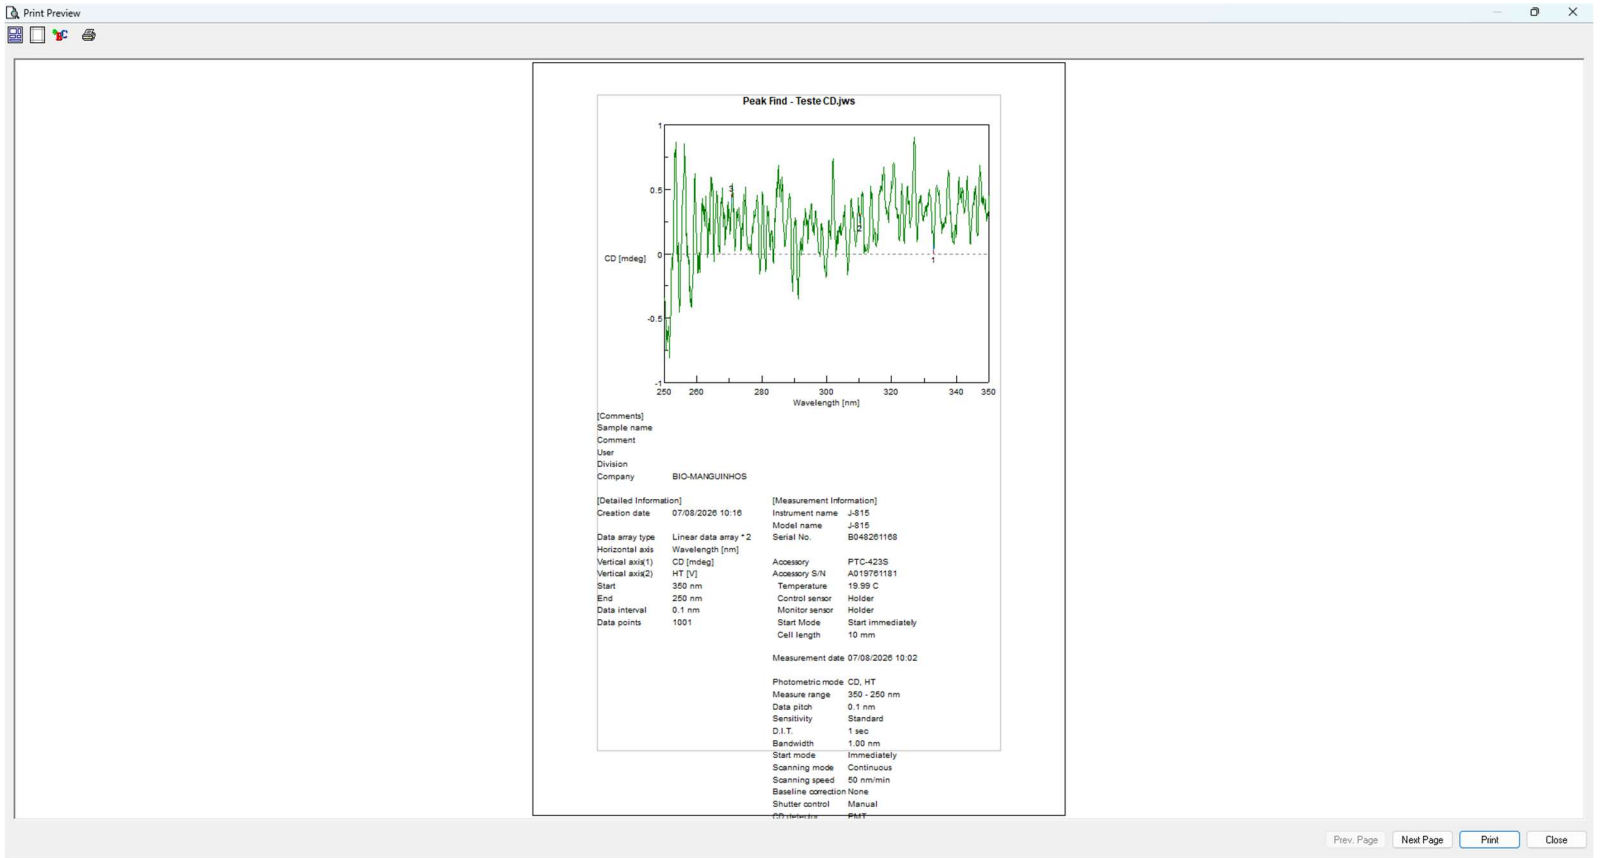


Software - 07.08.2026 - 43

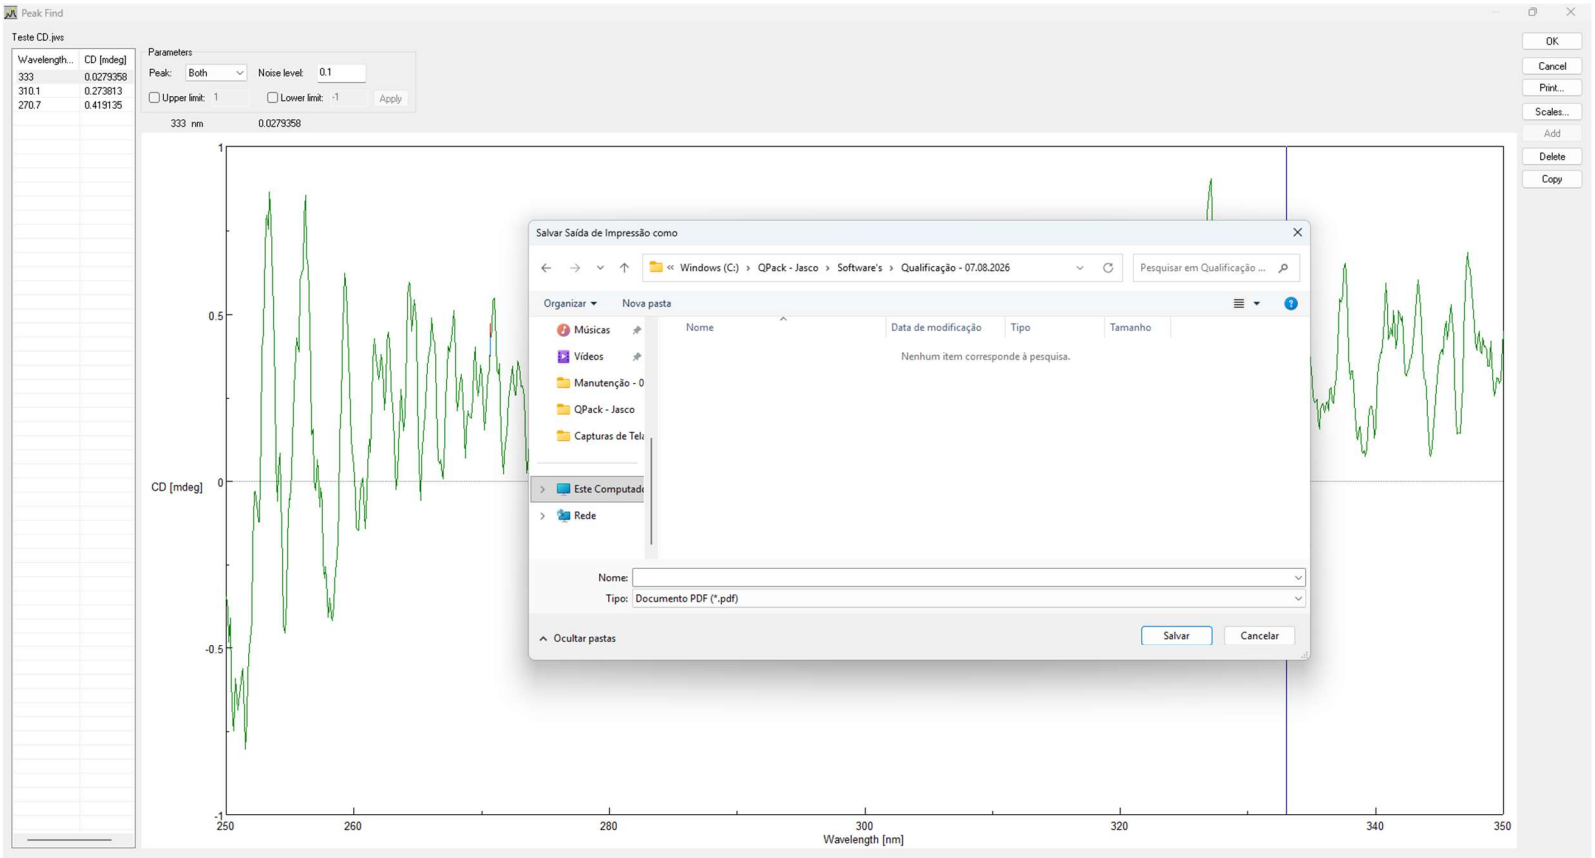


Software - 07.08.2026 - 44

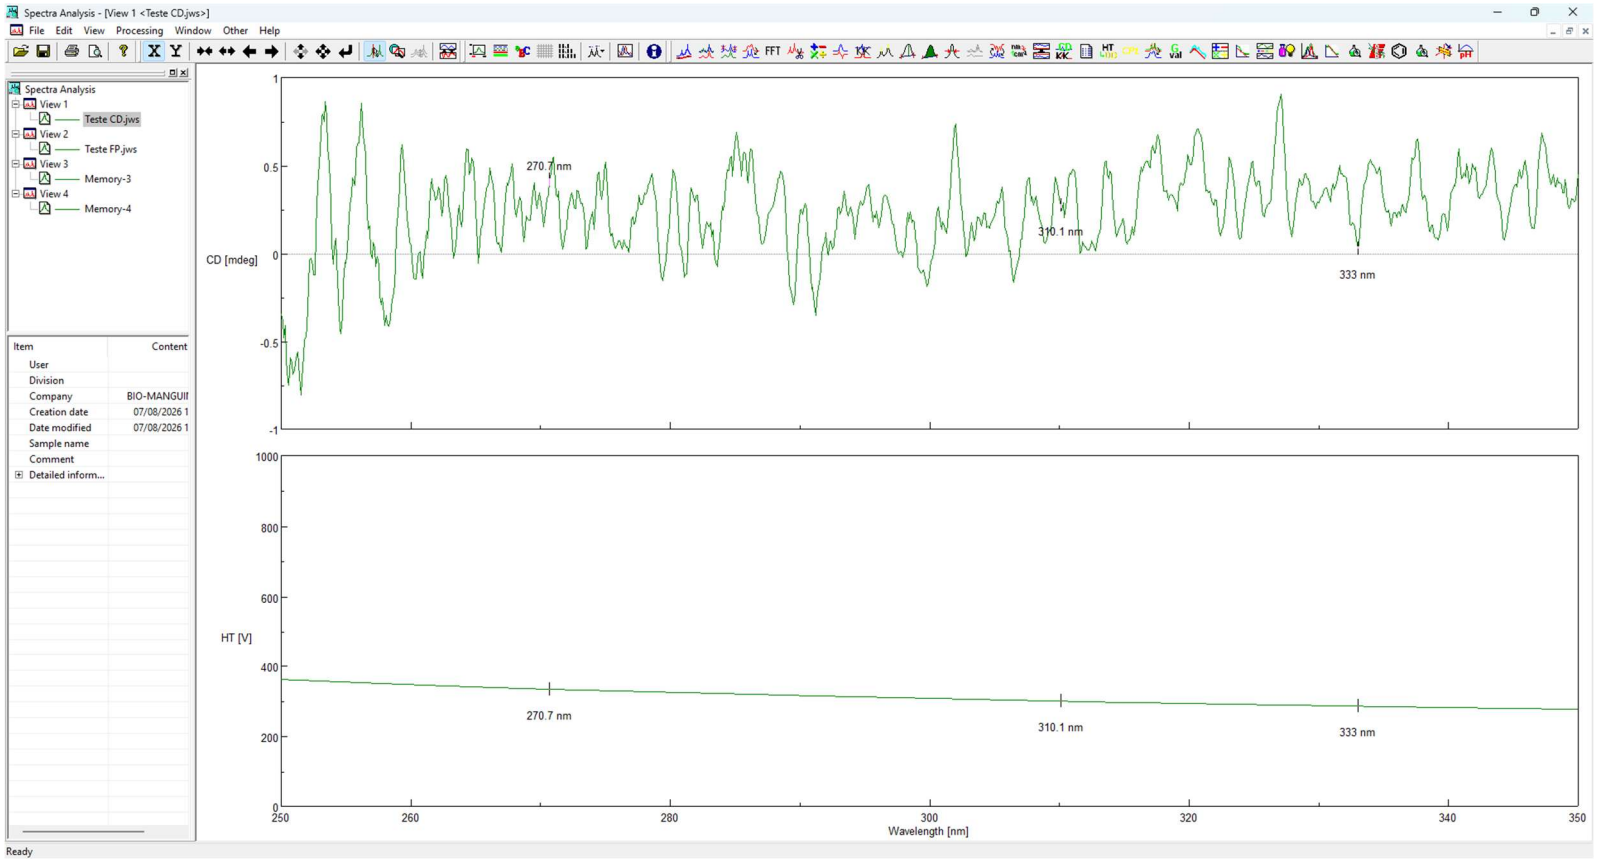


Software - 07.08.2026 - 45

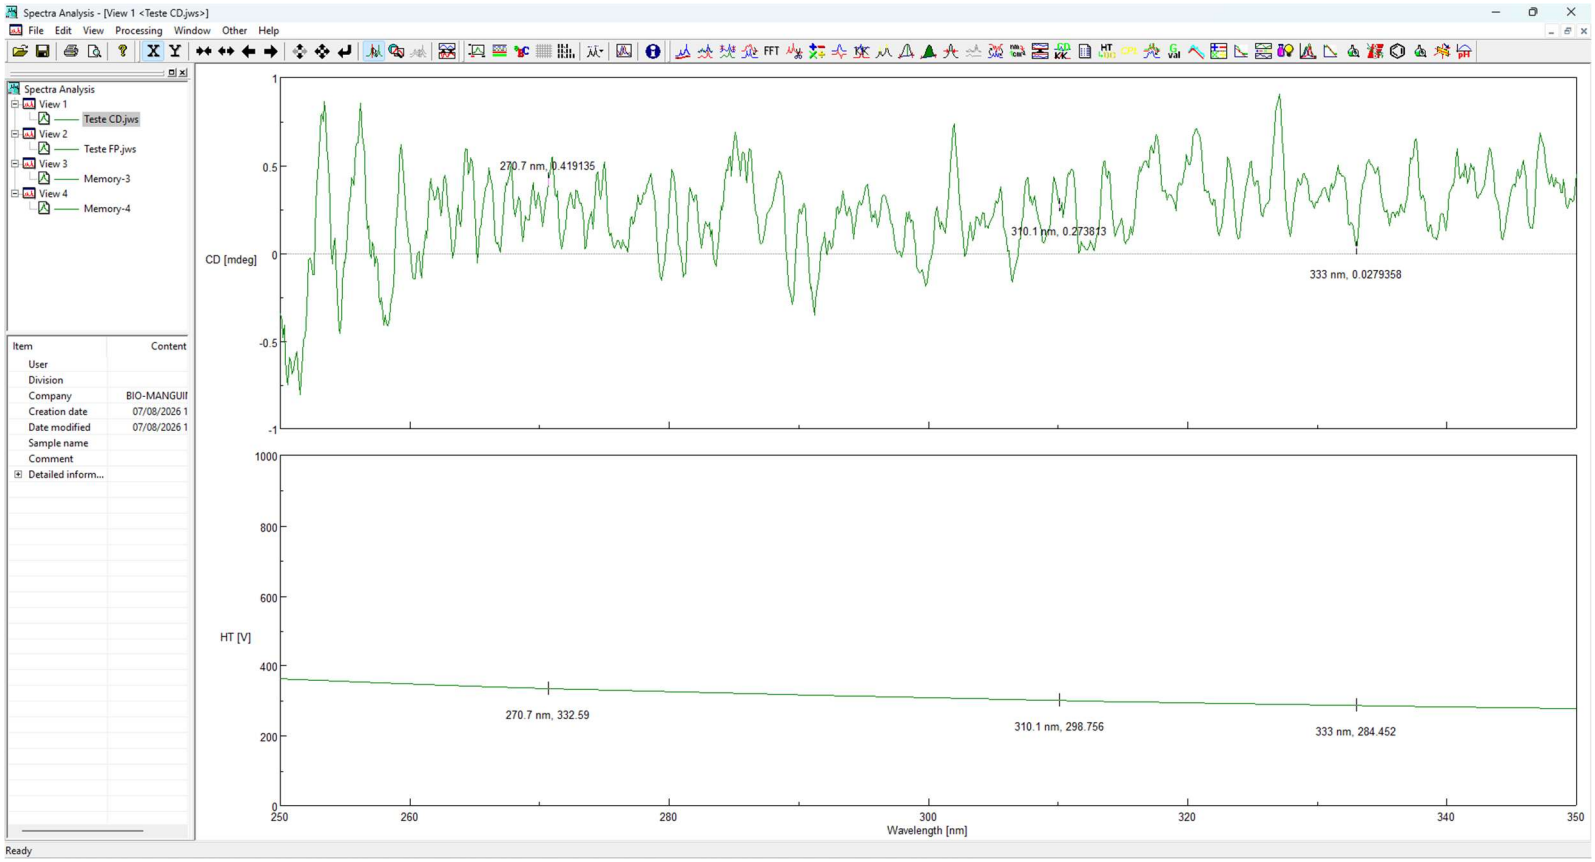


Software - 07.08.2026 - 46

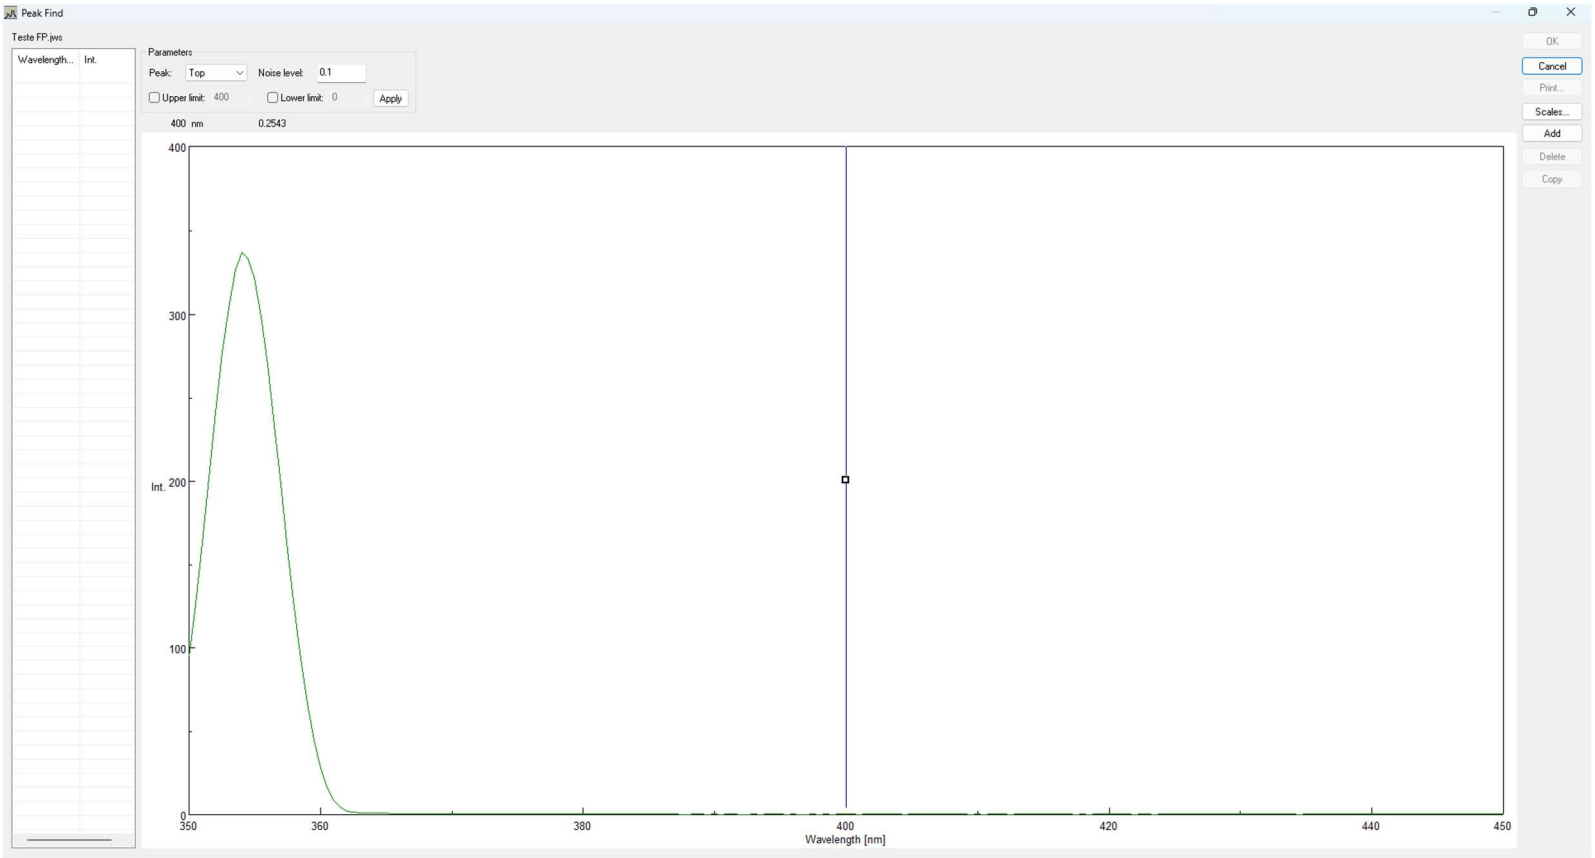


Software - 07.08.2026 - 47

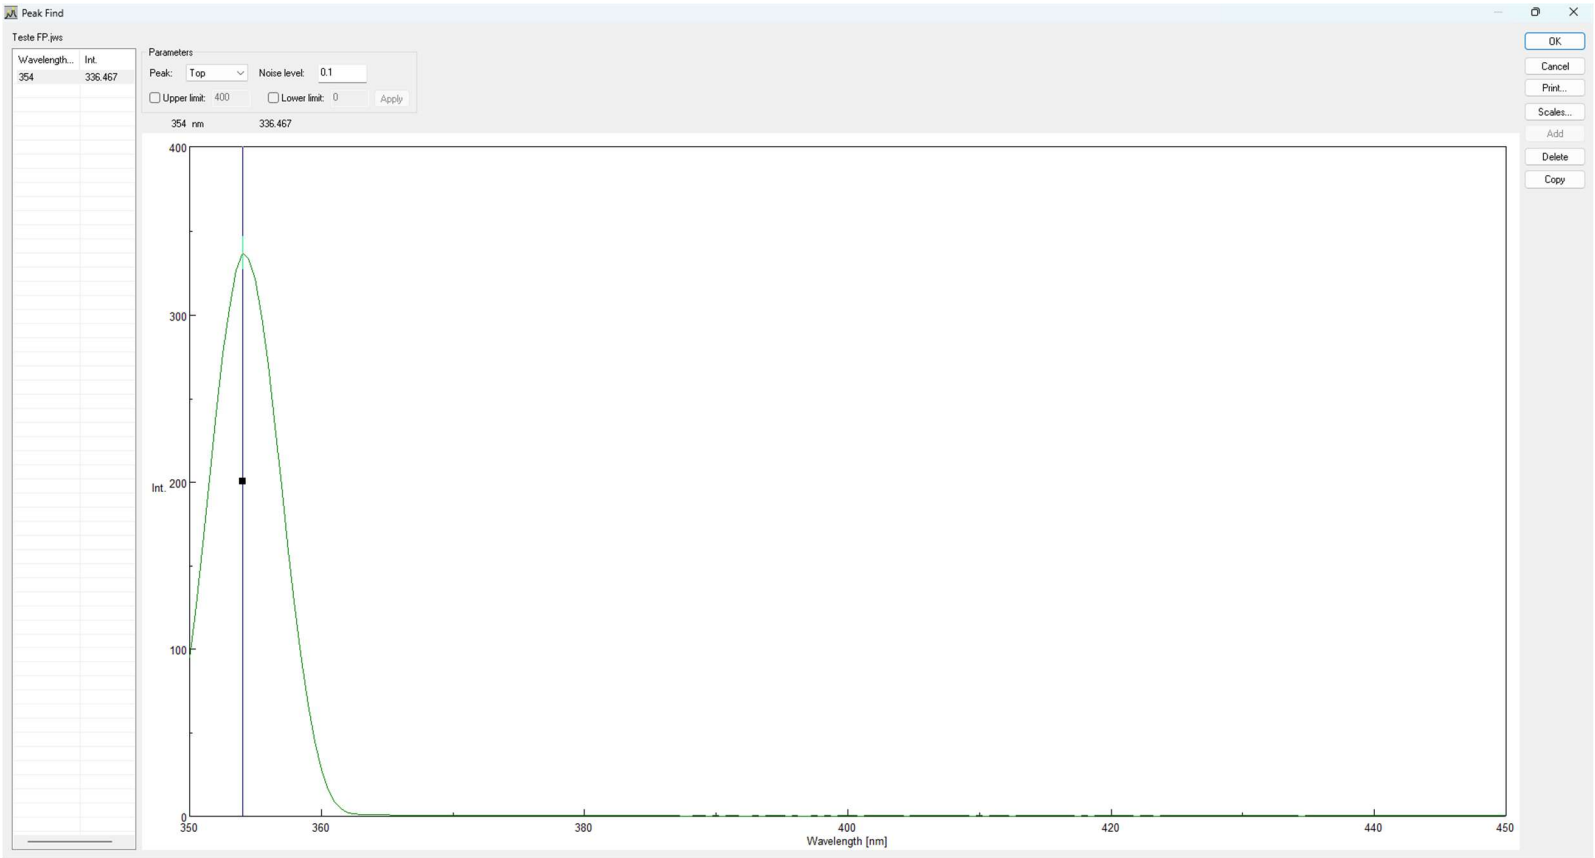


Software - 07.08.2026 - 48

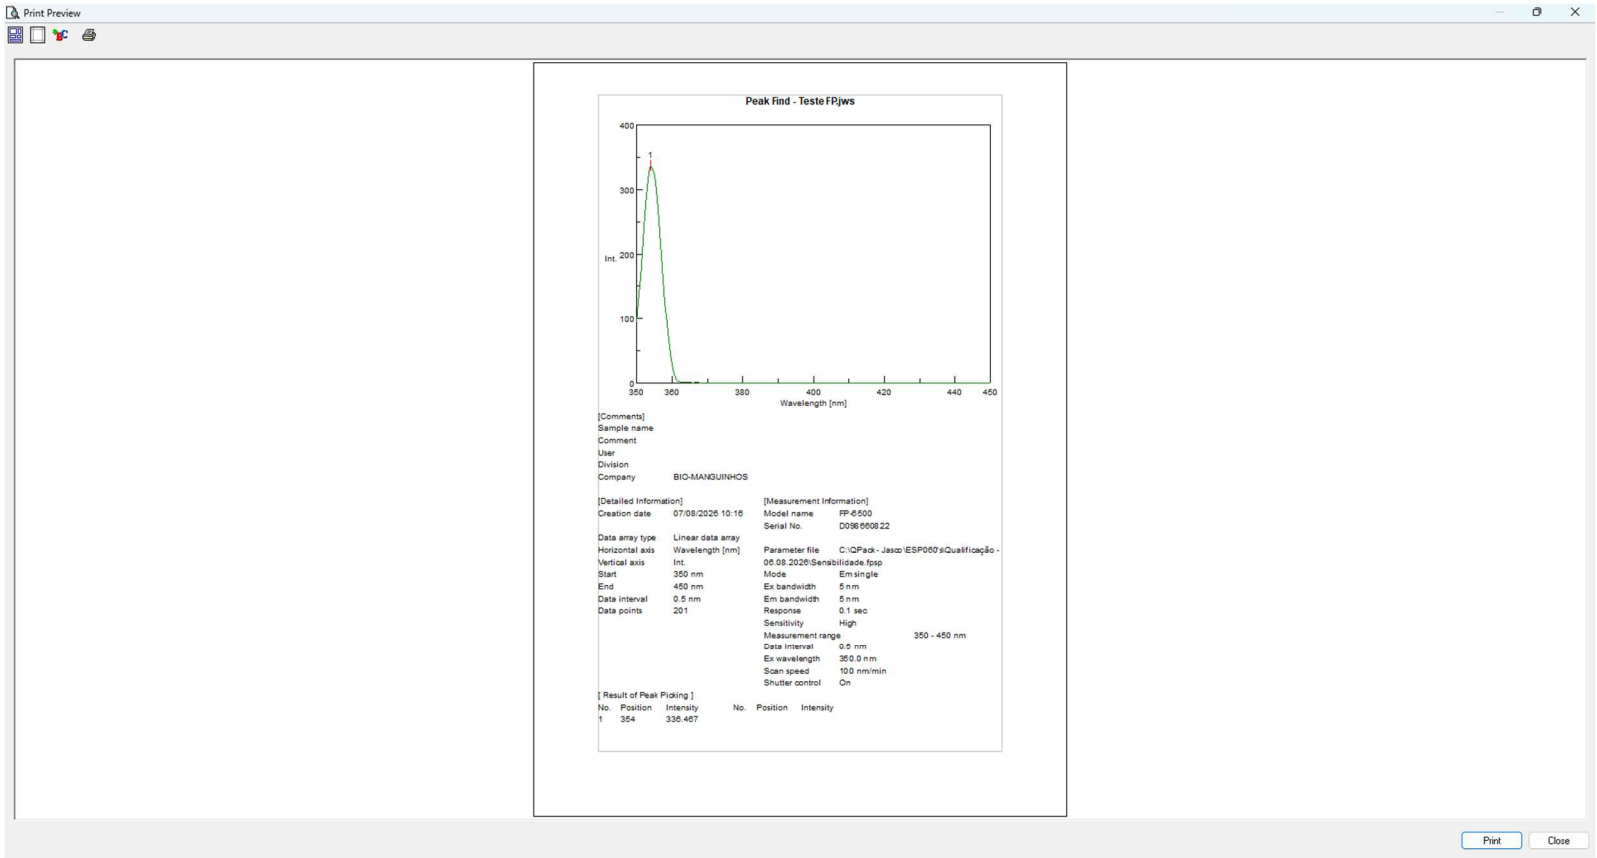


Software - 07.08.2026 - 49

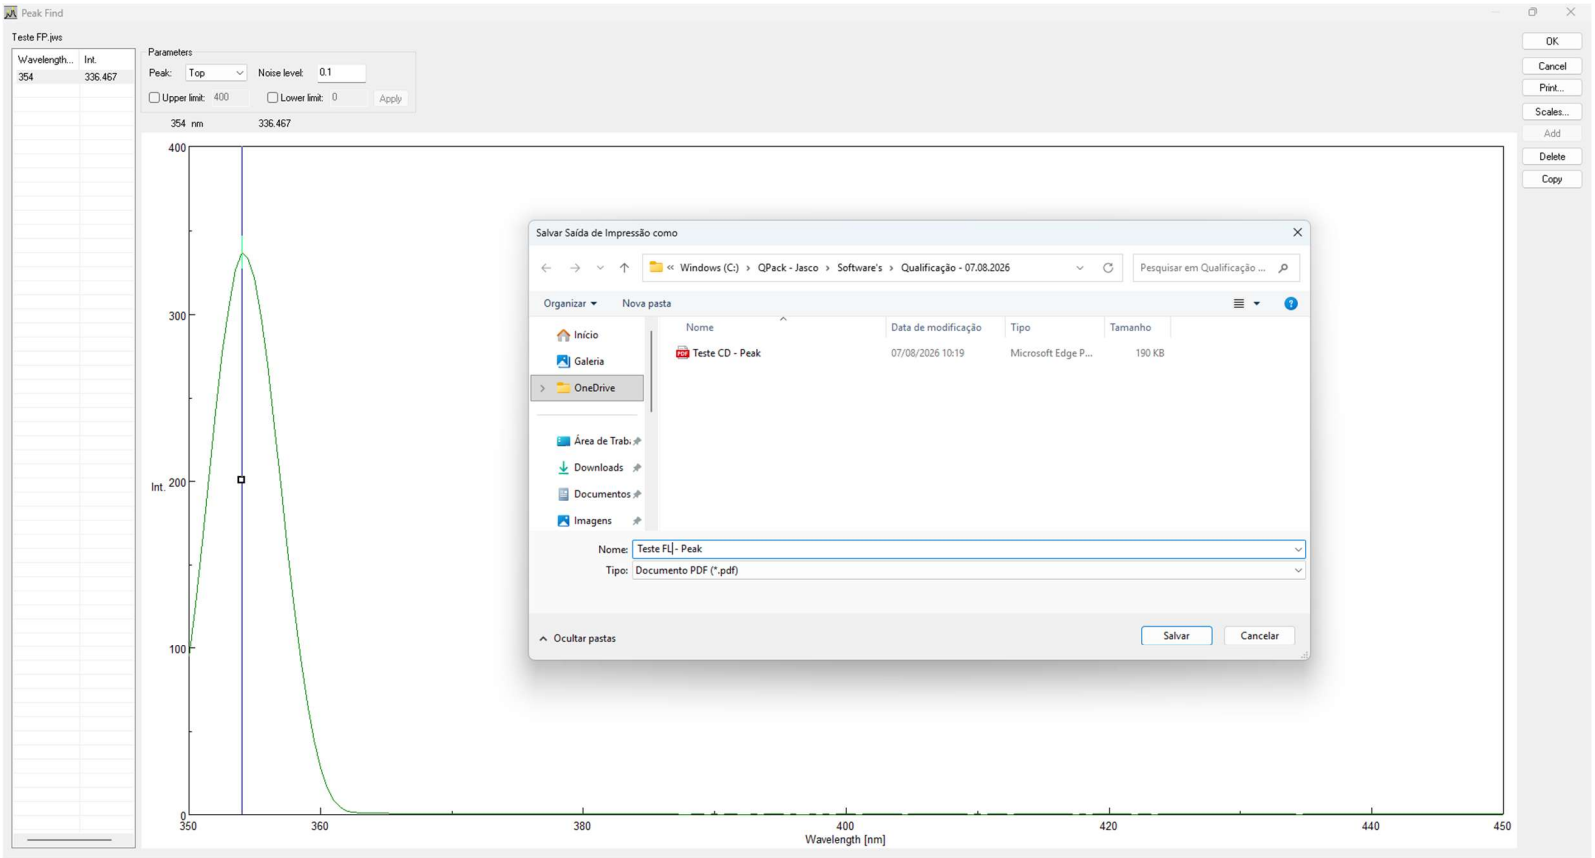


Software - 07.08.2026 - 50

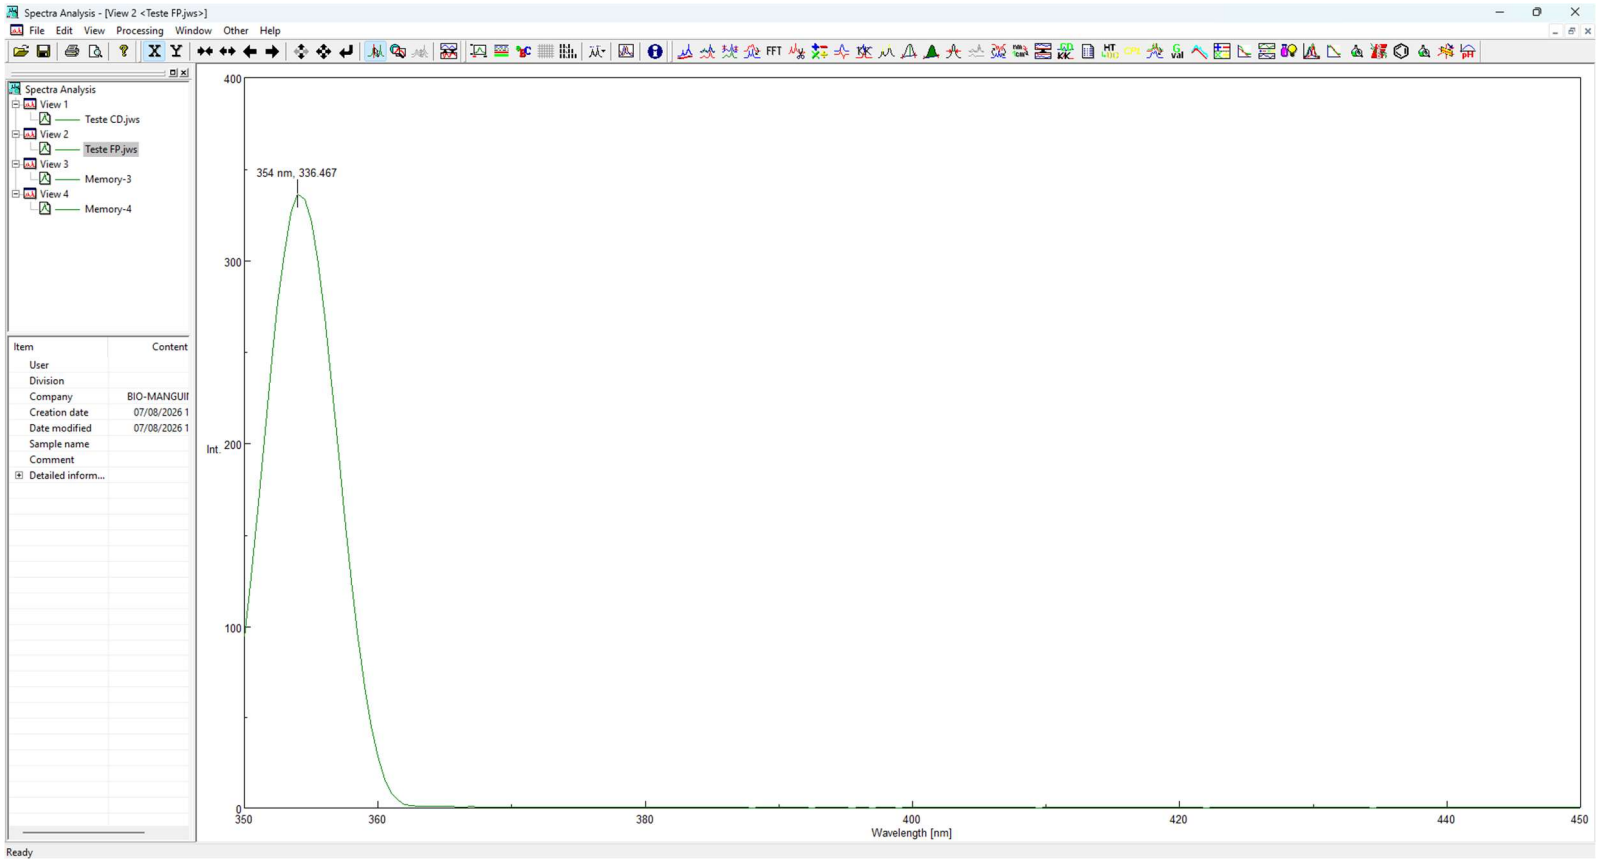

Software - 07.08.2026 - 51

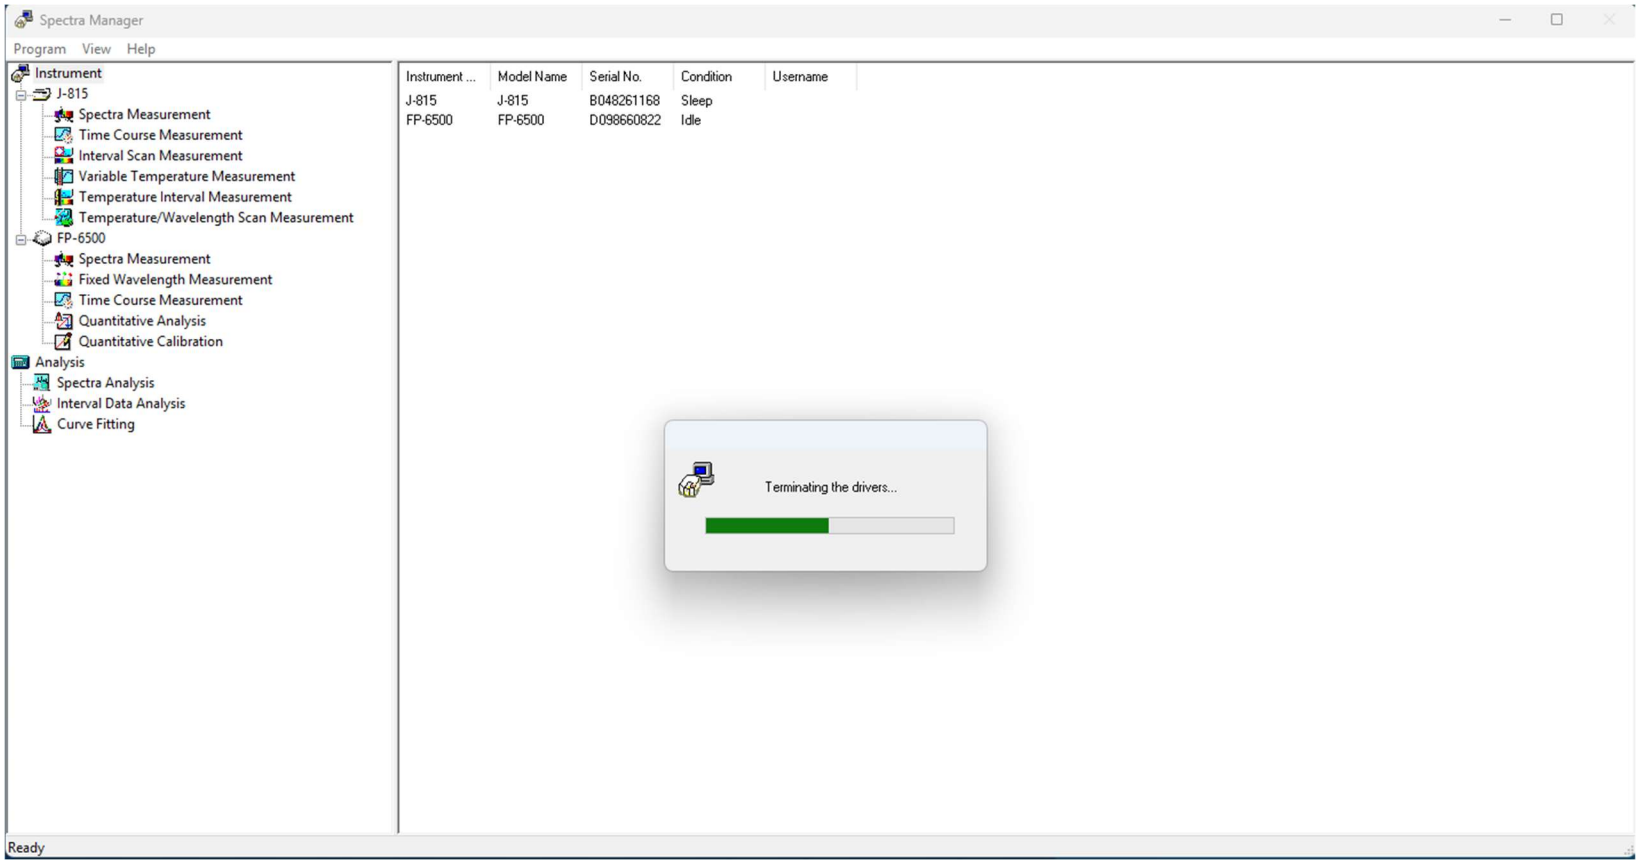

Software - 07.08.2026 - 52

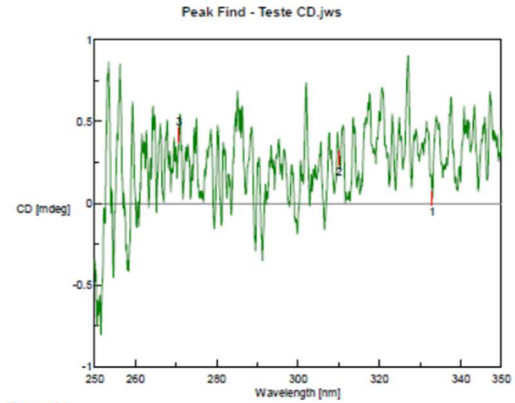


[Comments]	
Sample name	
Comment	
User	
Division	
Company	BIO-MANGUINHOS

[Detailed Information]	
Creation date	07/08/2026 10:16
Data array type	Linear data array * 2
Horizontal axis	Wavelength [nm]
Vertical axis(1)	CD [mdeg]
Vertical axis(2)	HT [V]
Start	350 nm
End	250 nm
Data interval	0.1 nm
Data points	1001

[Measurement Information]	
Instrument name	J-815
Model name	J-815
Serial No.	B048261168
Accessory	PTC-423S
Accessory S/N	A019761181
Temperature	19.99 C
Control sensor	Holder
Monitor sensor	Holder
Start Mode	Start immediately
Cell length	10 mm
Measurement date	07/08/2026 10:02
Photometric mode	CD, HT
Measure range	350 - 250 nm
Data pitch	0.1 nm
Sensitivity	Standard
D.I.T.	1 sec
Bandwidth	1.00 nm
Start mode	Immediately
Scanning mode	Continuous
Scanning speed	50 nm/min
Baseline correction	None
Shutter control	Manual
CD detector	PMT
PMT voltage	Auto
Accumulations	1

Software - 07.08.2026 - 53

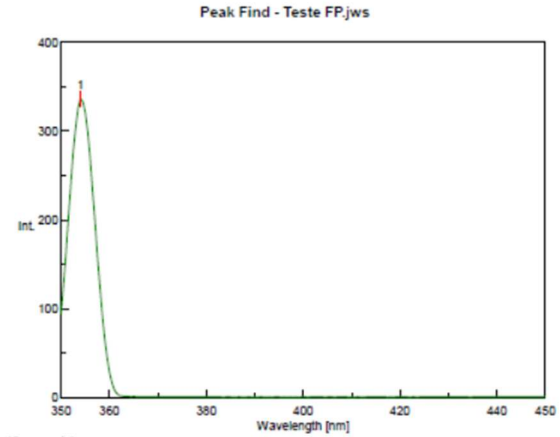

[Comments]
Sample name
Comment
User
Division
Company BIO-MANGUINHOS

[Detailed Information]
Creation date 07/08/2026 10:16

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Int.
Start 350 nm
End 450 nm
Data interval 0.5 nm
Data points 201

[Measurement Information]
Model name FP-6500
Serial No. D098660822

Parameter file C:\QPack - Jasco\ESP060's\Qualificação - 06.08.2026\Sensibilidade.fpsp
Mode Em single
Ex bandwidth 5 nm
Em bandwidth 5 nm
Response 0.1 sec
Sensitivity High
Measurement range 350 - 450 nm
Data interval 0.5 nm
Ex wavelength 350.0 nm
Scan speed 100 nm/min

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	354	336.467			