
Peak Find - HPLC-0003 EDUV 2024.jws

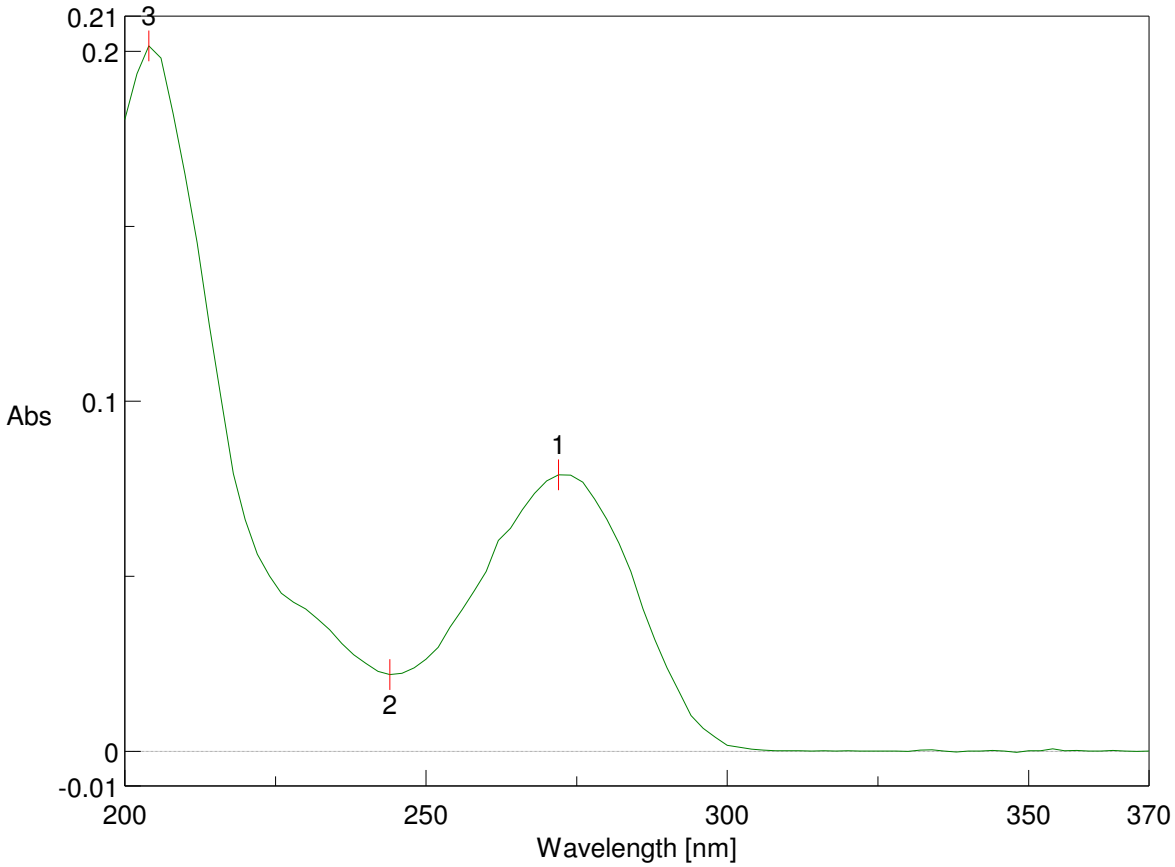

[Comments]

User	Administrator
Workgroup	Workgroup01
Division	
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	30/08/2024 10:42


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	370 nm	
Data interval	2 nm	
Data points	86	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.0789196	2	244	0.0217917
3	204	0.201504			

Creation	Administrator
Review	
Approval	

Peak Find - HPLC-0003 EDPDA 2024.jws

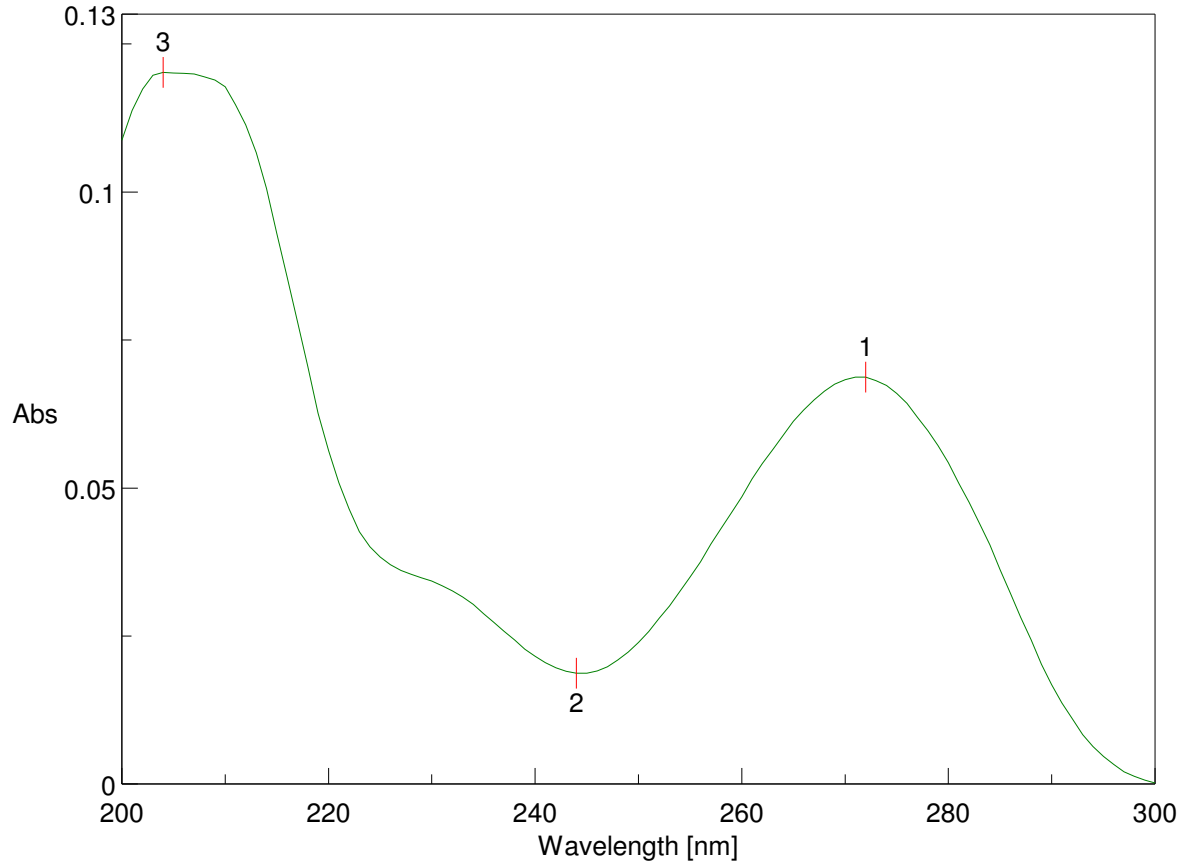

[Comments]

User	Administrator
Workgroup	Workgroup01
Division	
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	30/08/2024 10:54


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	300 nm	
Data interval	1 nm	
Data points	101	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.068688	2	244	0.018706
3	204	0.120182			

Creation	Administrator
Review	
Approval	

Chromatogram

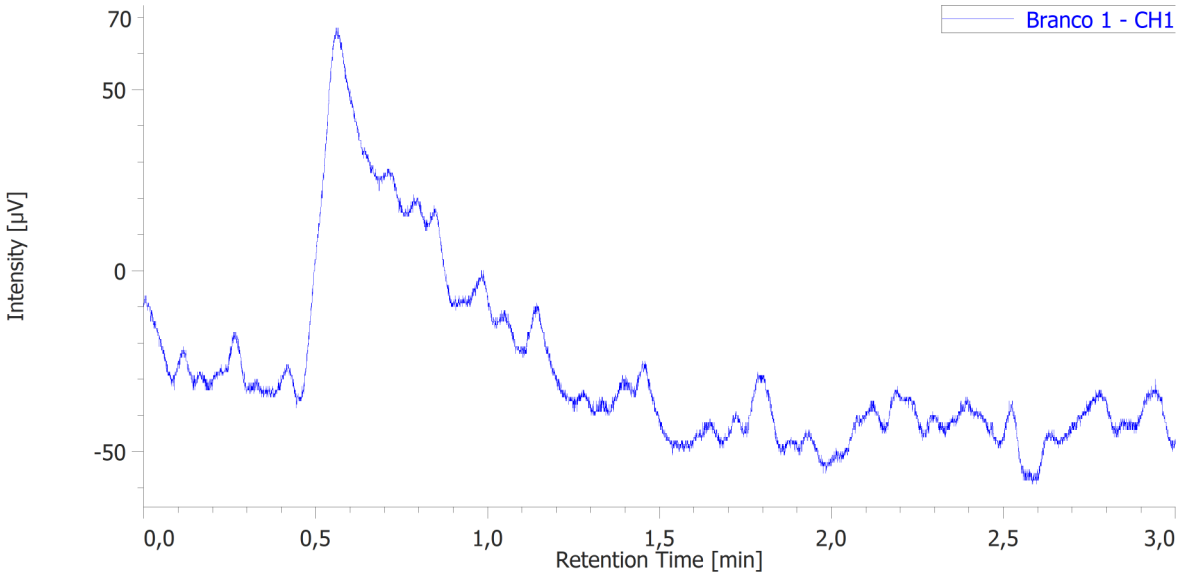


Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:10:15
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:07:12
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

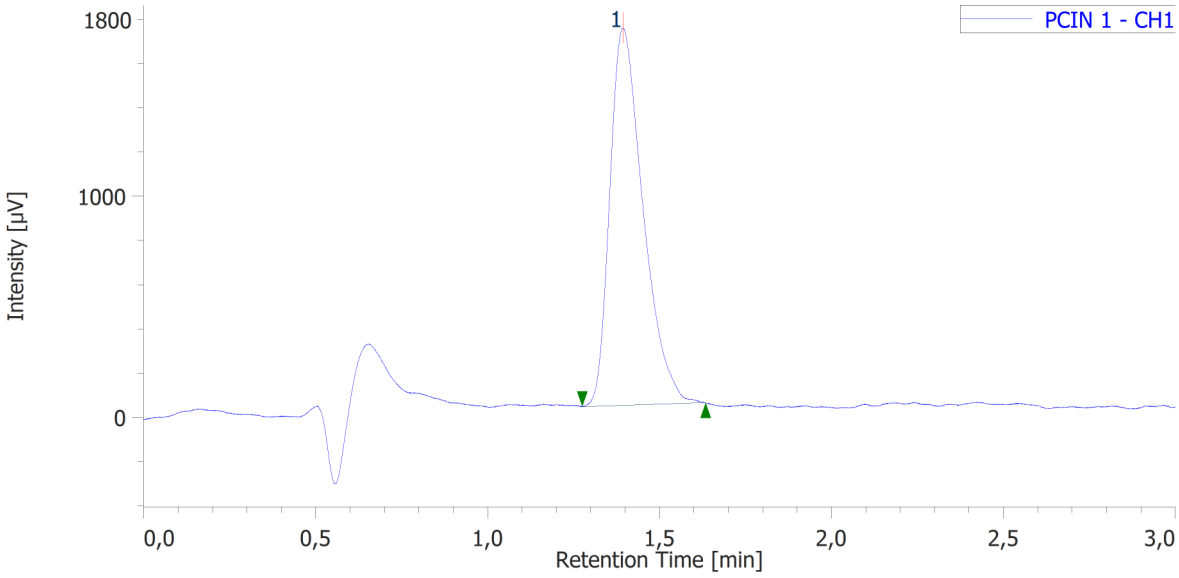

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:13:27
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:10:25
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.393	11478	1707	100.000	100.000	N/A	1022	N/A	1.459		N/A

Creator
Reviewer
Approver

Chromatogram

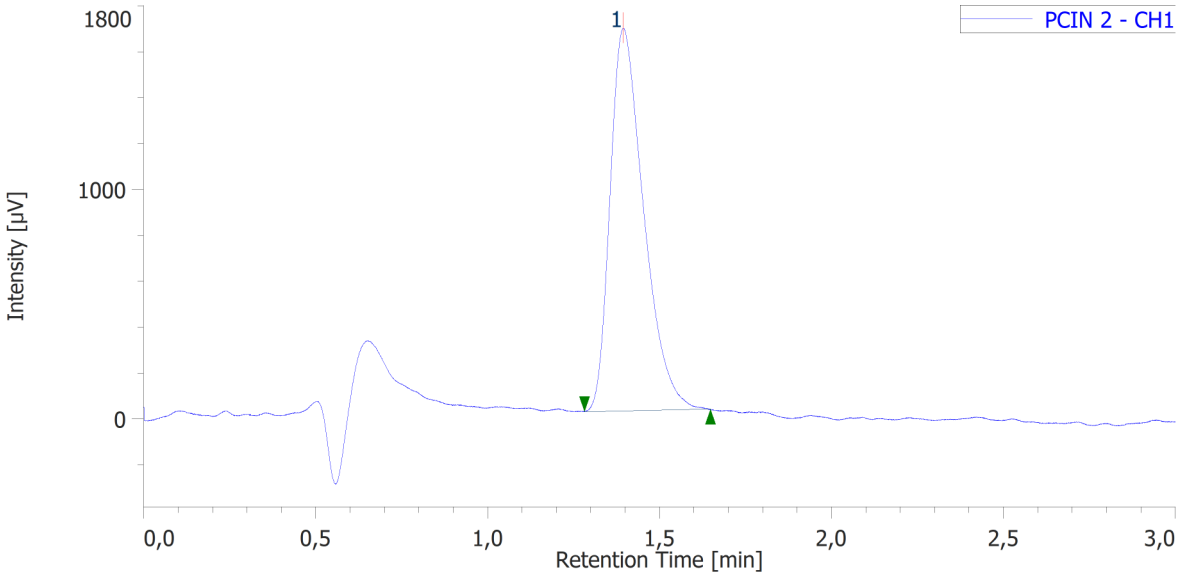

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:16:39
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:13:37
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.394	11342	1669	100.000	100.000	N/A	996	N/A	1.457		N/A

Creator
Reviewer
Approver

Chromatogram

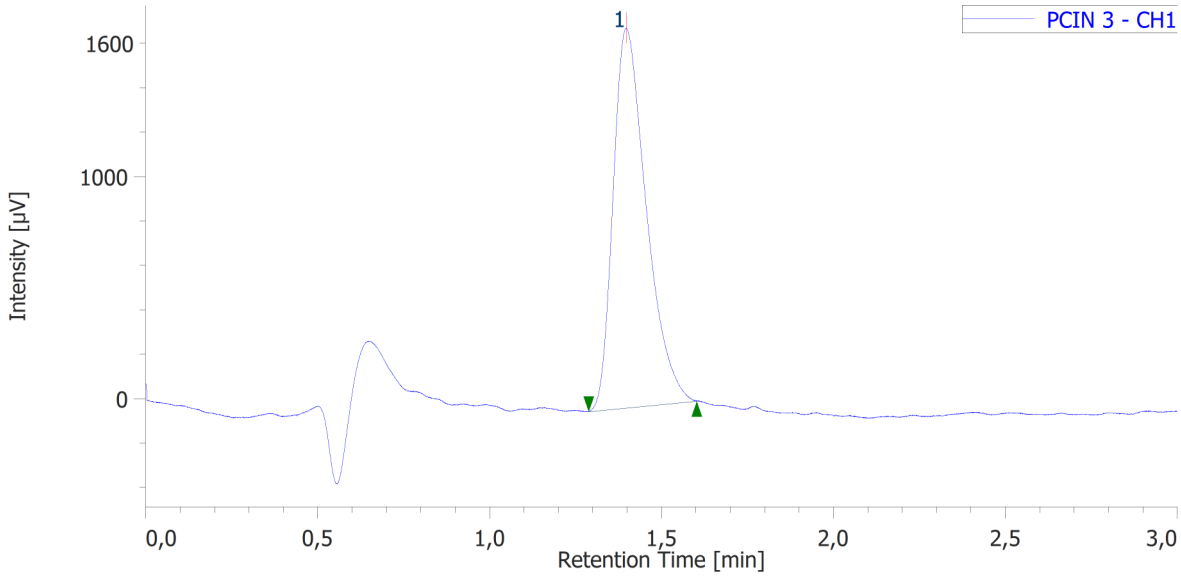

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:19:51
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:16:49
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.397	11498	1712	100.000	100.000	N/A	1030	N/A	1.459		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

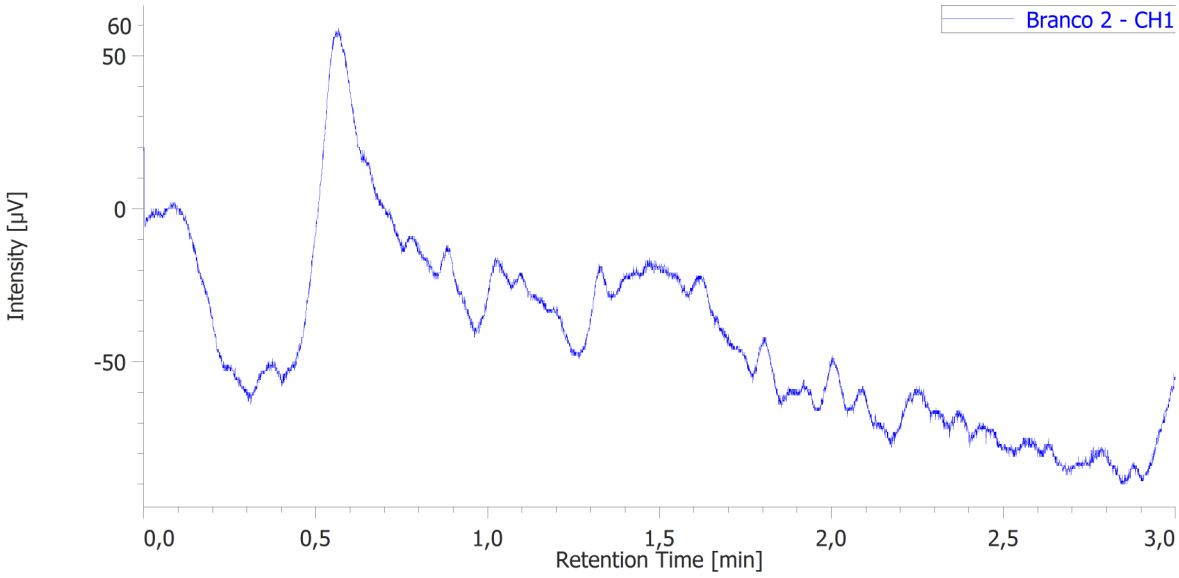


Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:23:03
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:20:01
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

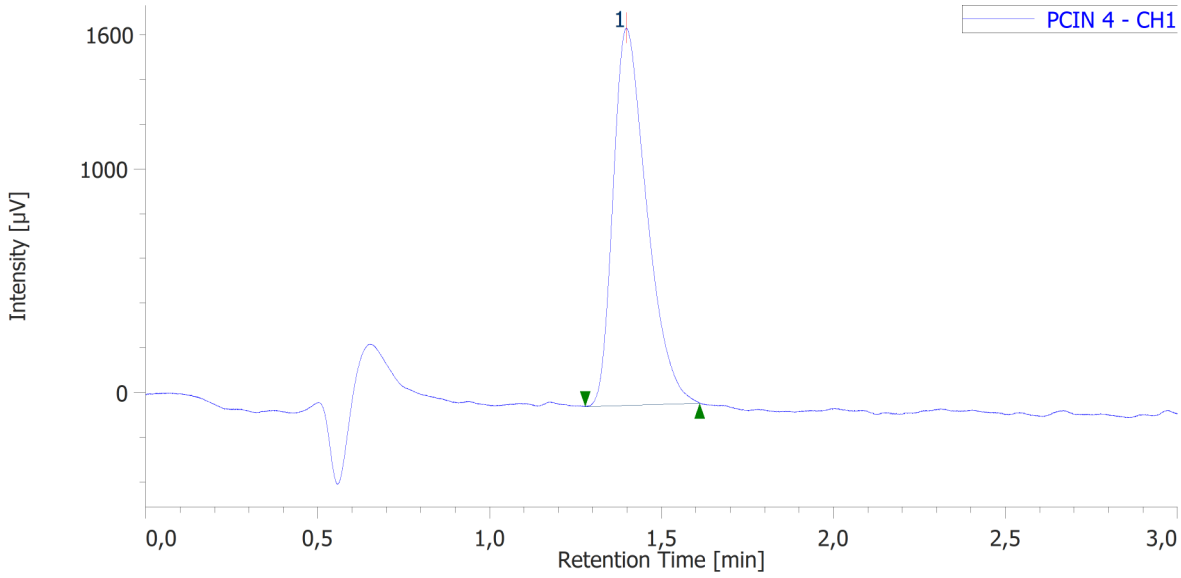

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:26:15
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:23:13
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.398	11466	1685	100.000	100.000	N/A	997	N/A	1.441		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

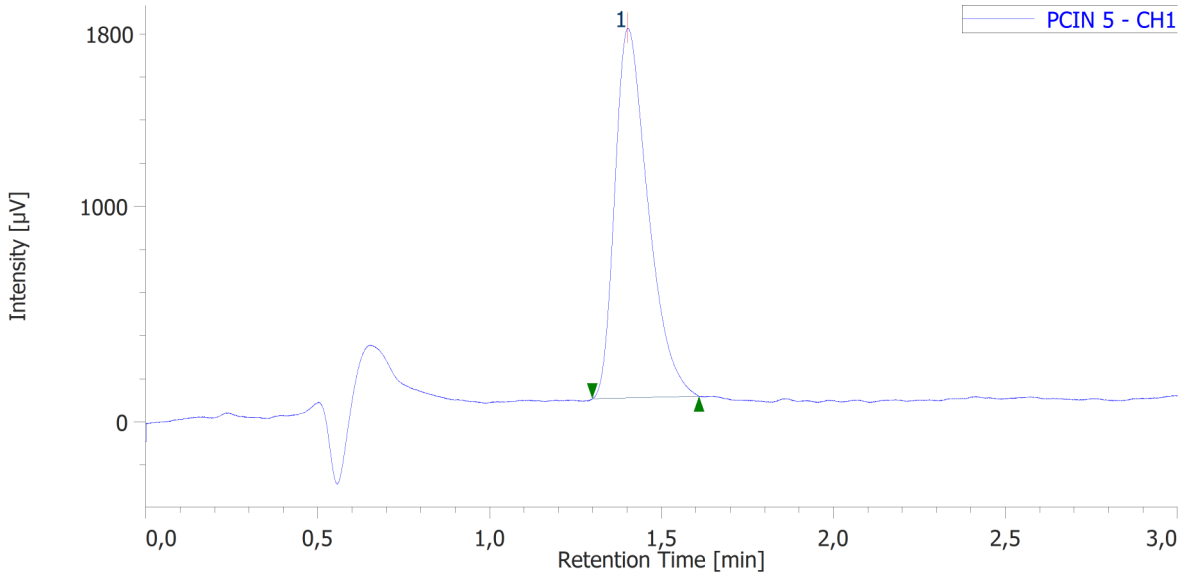

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:29:27
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:26:25
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.401	11498	1714	100.000	100.000	N/A	1039	N/A	1.485		N/A

Creator
Reviewer
Approver

Chromatogram

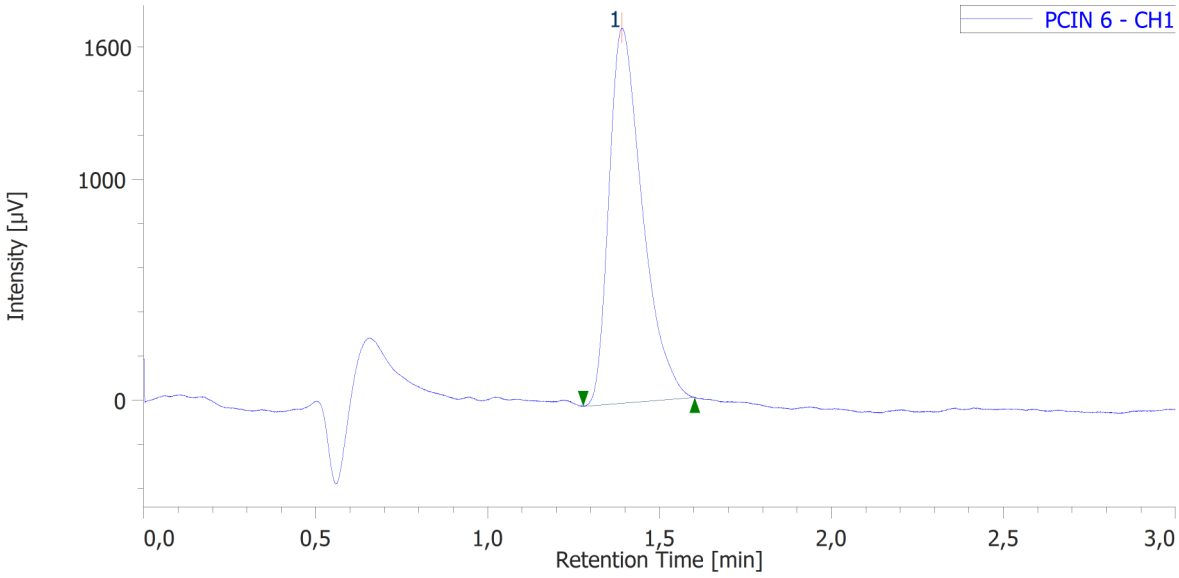

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:32:39
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:29:37
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.390	11467	1699	100.000	100.000	N/A	1017	N/A	1.506		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

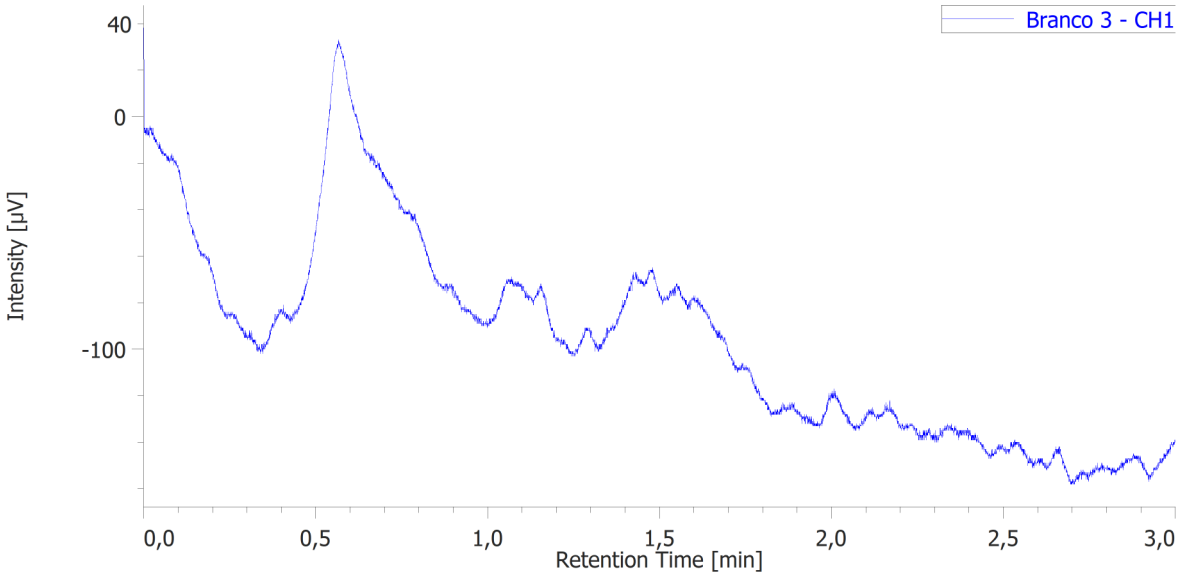

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 12:35:53
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:32:50
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Certificado Nº: 387/24 -RELB	Início da Qualificação: 29/08/2024	Página 1 de 3


Resultado obtido na altura do pico

	ALTURA DO PICO (mAU)
Resultado:	**101**

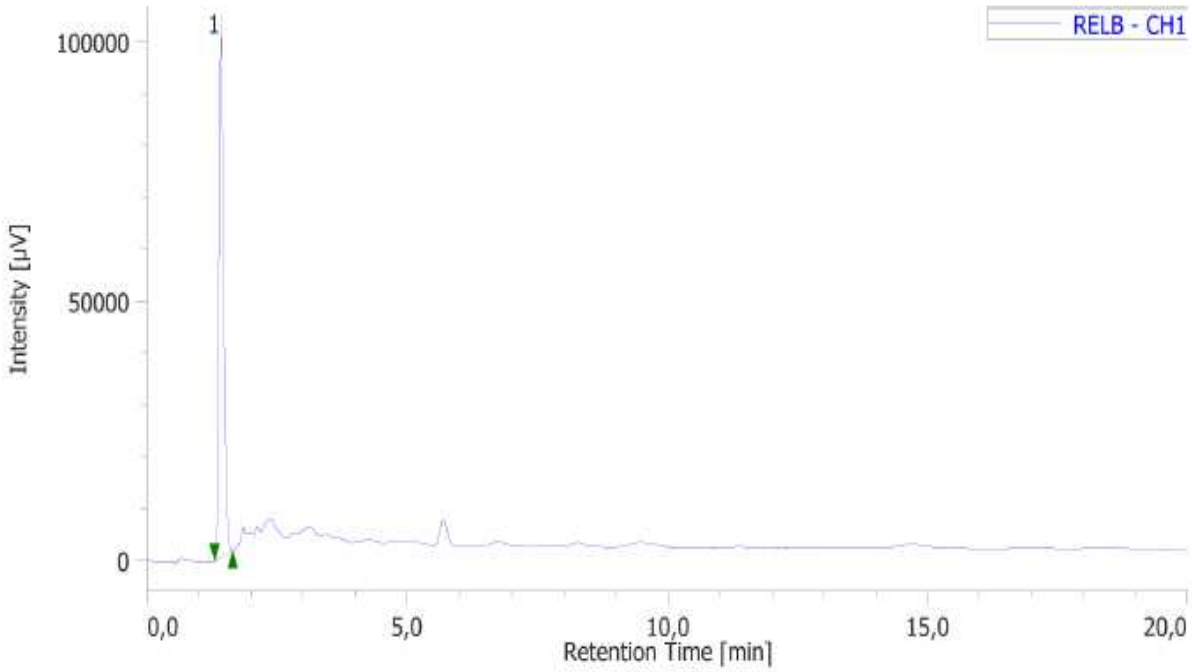

Resultado obtido no teste de sinal/ruído


Resultado:	Ruído (mAU)
VALOR MÁXIMO:	**2,4080**
VALOR MÍNIMO:	**2,3820**
	Ruído
	0,0260

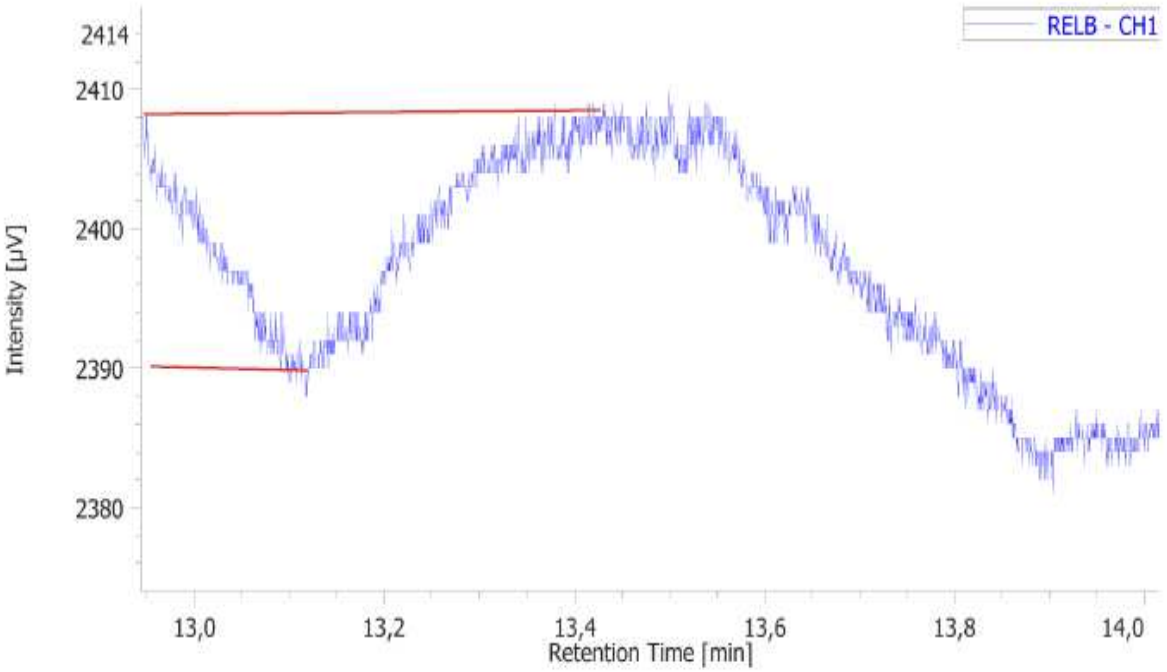


Certificado Nº: 000/00	Início da Qualificação:	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	**3,5000**	**3,0000**
VALOR MÍNIMO:	**2,5000**	
Resultado:	**1,0000**	

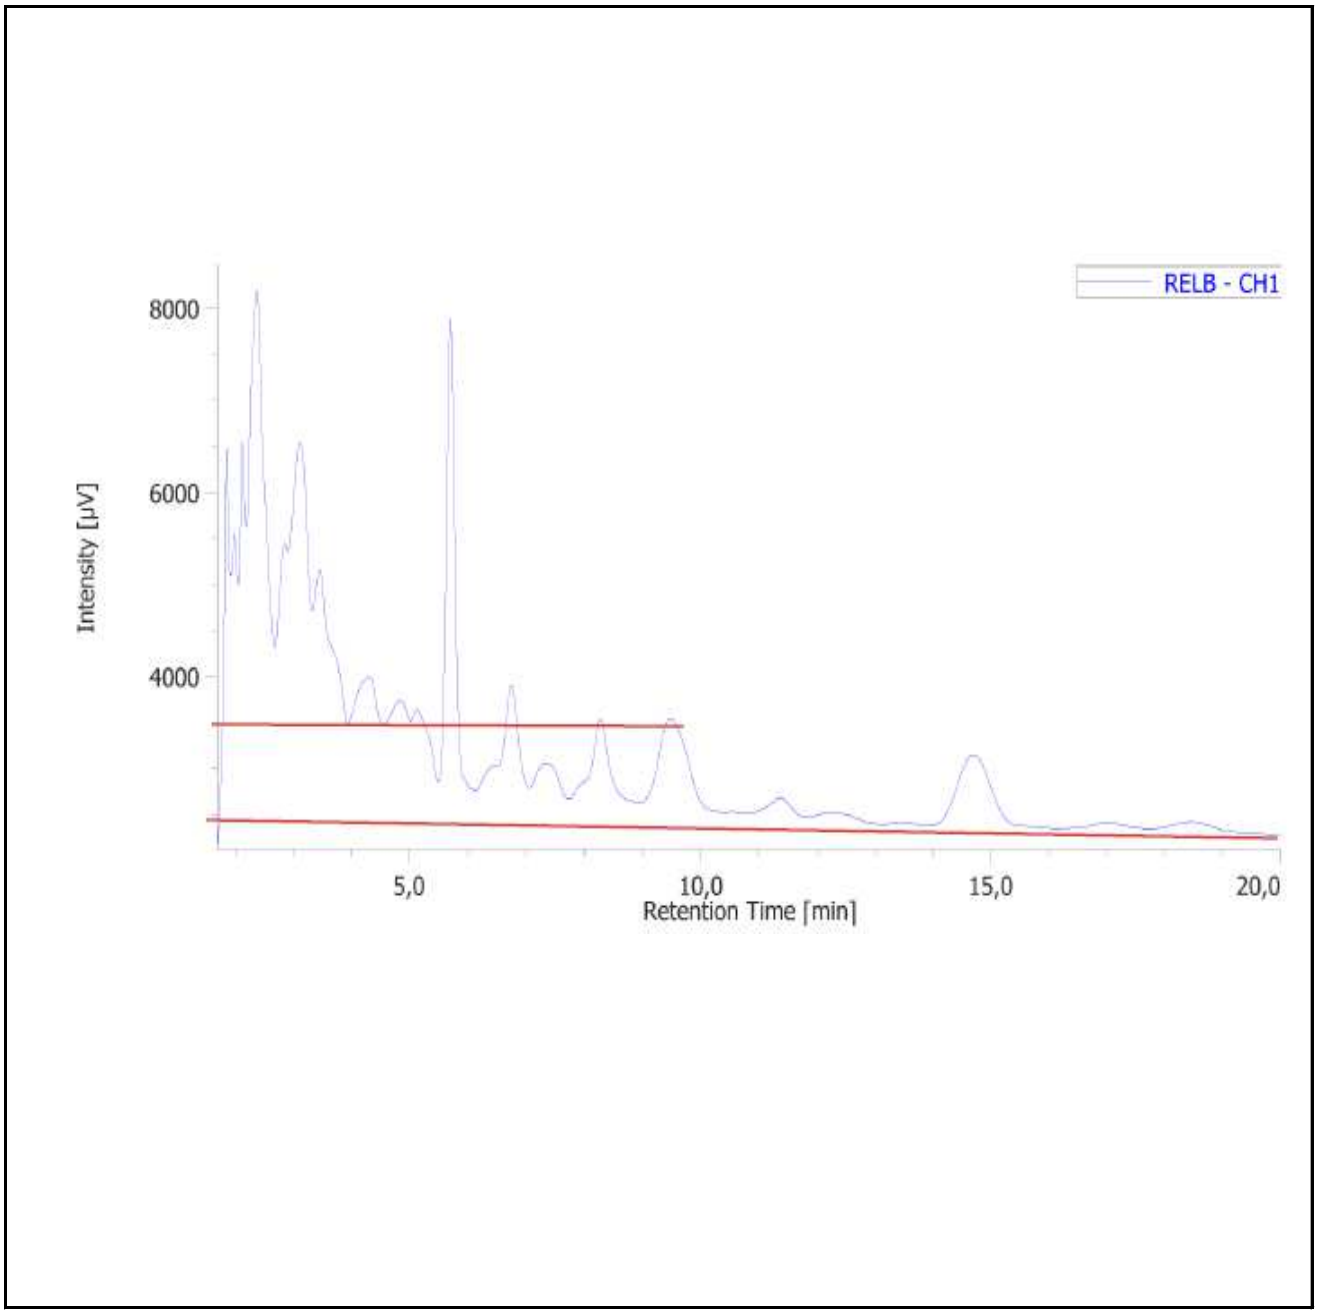

Chromatogram

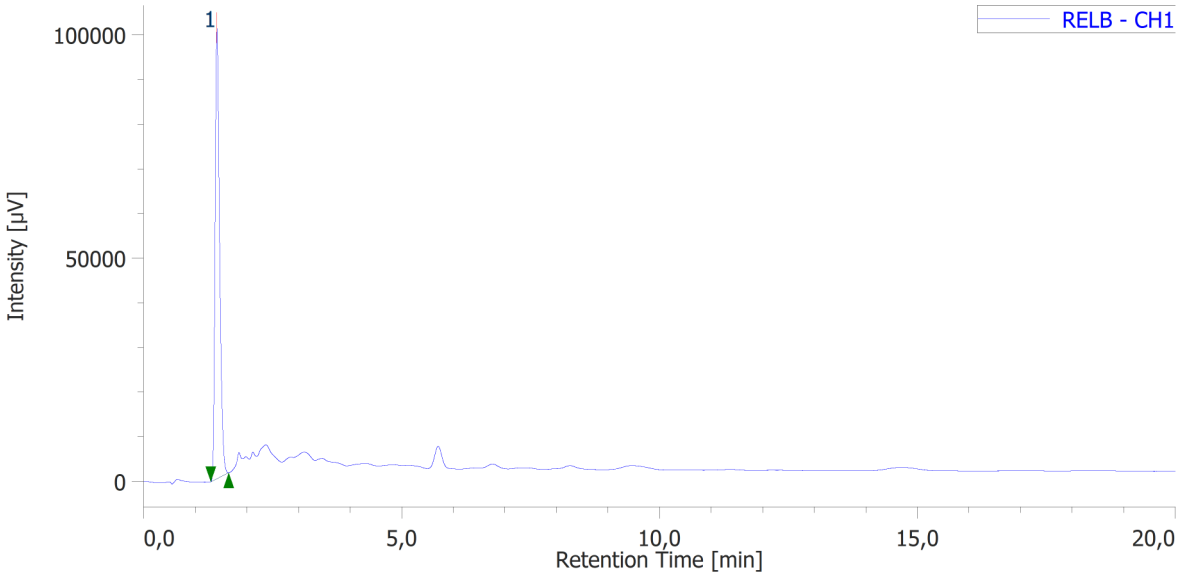

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.418	616015	100892	100.000	100.000	N/A	1299	N/A	1.372		2365.4

Creator
Reviewer
Approver

Chromatogram

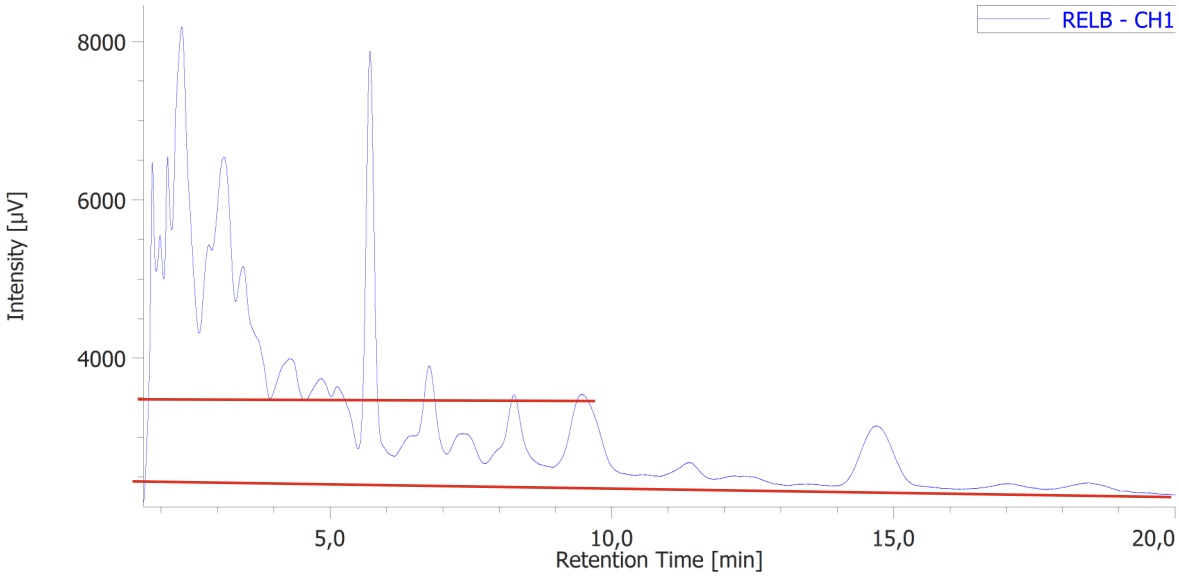

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,418	616015	100892	100,000	100,000	N/A	1299	N/A	1,372		2365,4

Creator
Reviewer
Approver

Chromatogram

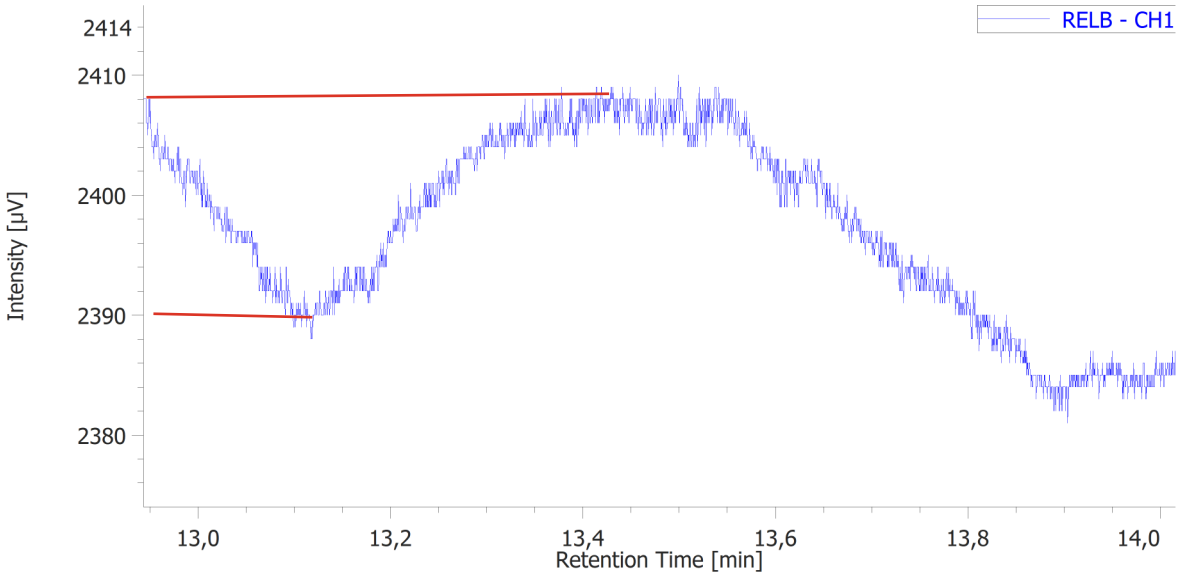

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação 03


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,418	616015	100892	100,000	100,000	N/A	1299	N/A	1,372		2365,4

Creator
Reviewer
Approver

Certificado Nº: 387/24 -RELB	Início da Qualificação: 29/08/2024	Página 1 de 3


Resultado obtido na altura do pico

	ALTURA DO PICO (mAU)
Resultado:	**96**

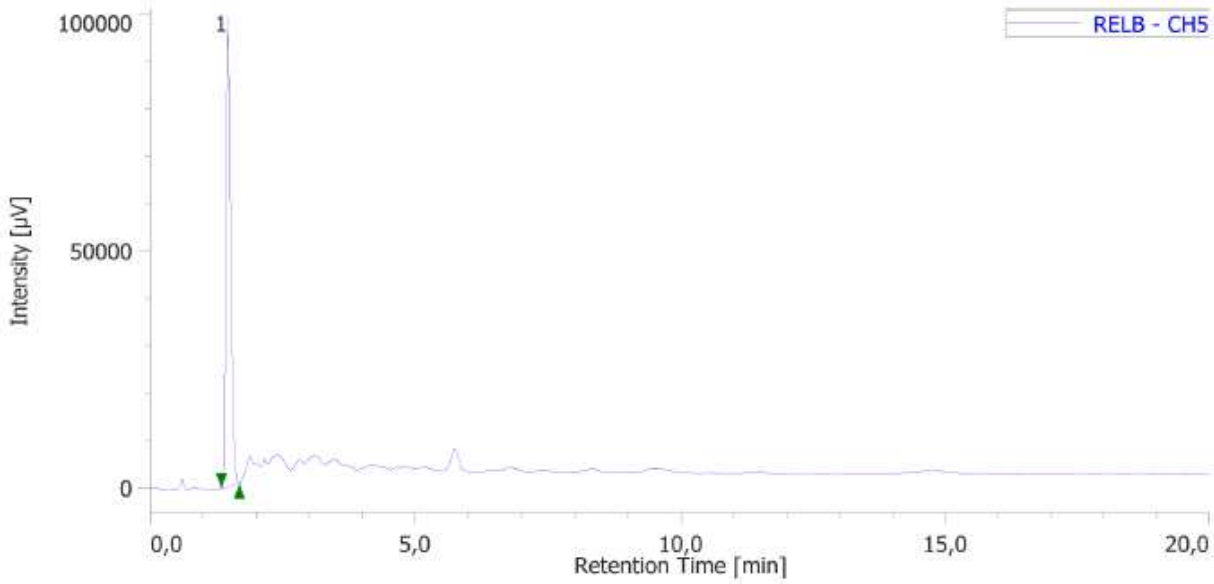

Resultado obtido no teste de sinal/ruído


Resultado:	Ruído (mAU)
VALOR MÁXIMO:	**2,8950**
VALOR MÍNIMO:	**2,8650**
	Ruído
	0,0300

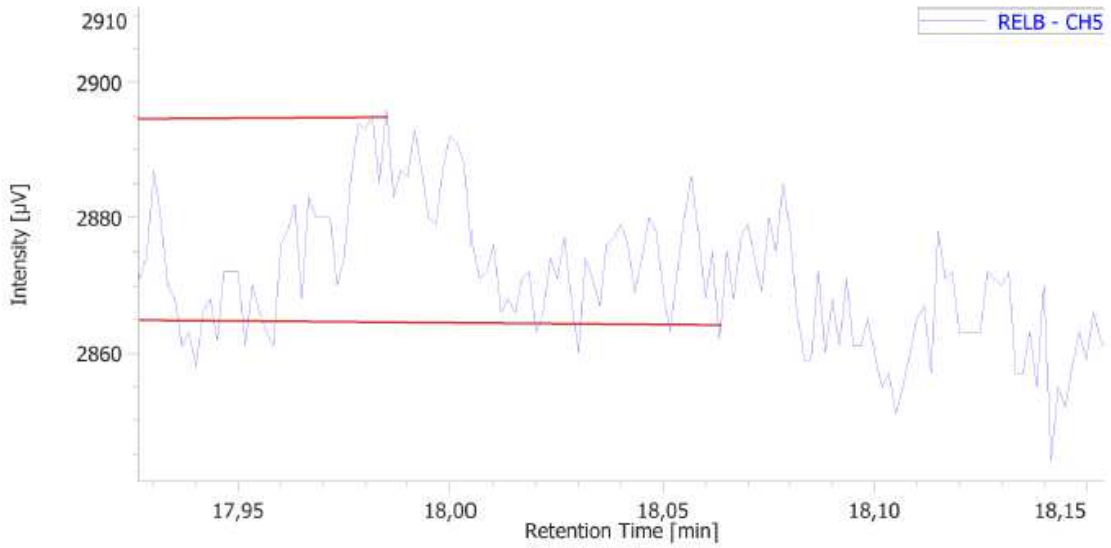


Certificado Nº: 000/00	Início da Qualificação:	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	**3,9000**	**3,0000**
VALOR MÍNIMO:	**2,9000**	
Resultado:	**1,0000**	

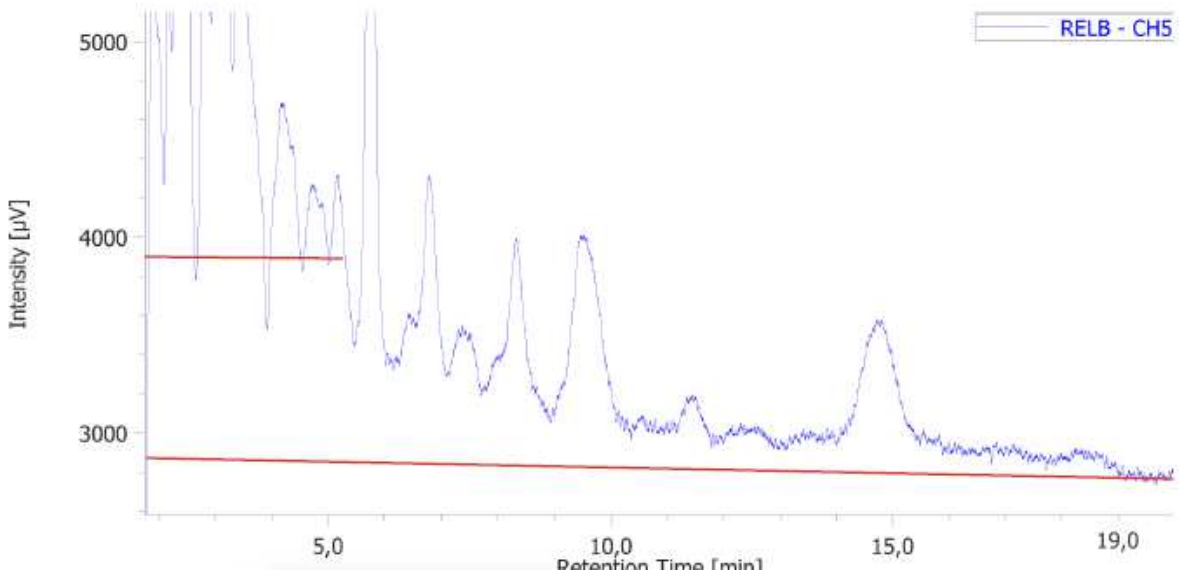

Chromatogram

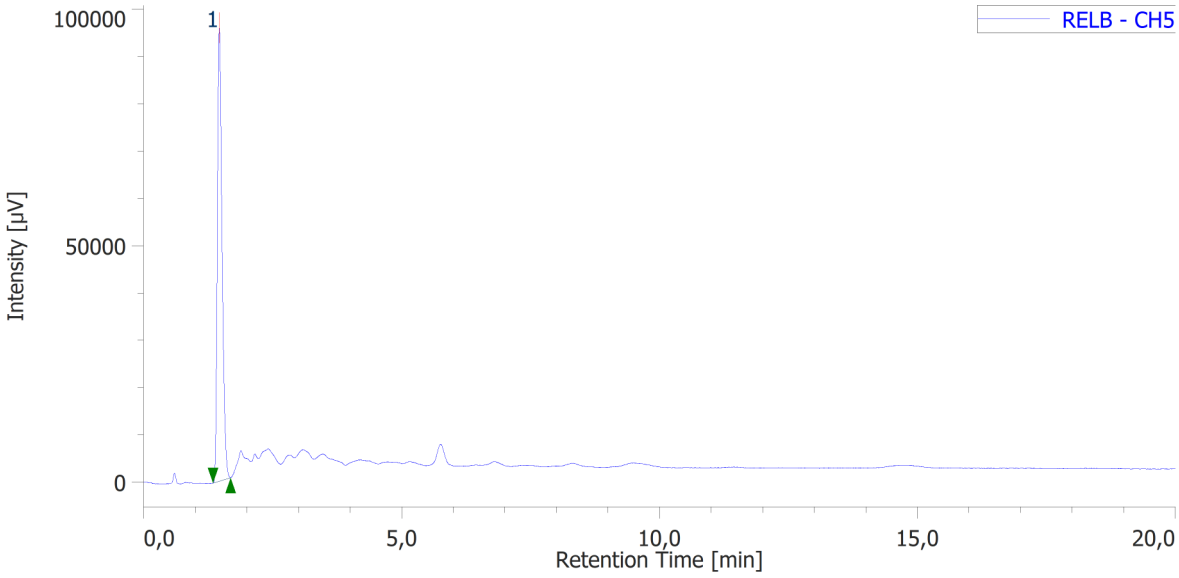

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1,463	608117	95812	100,000	100,000	N/A	1261	N/A	1,381		1180,5

Creator
Reviewer
Approver

Chromatogram

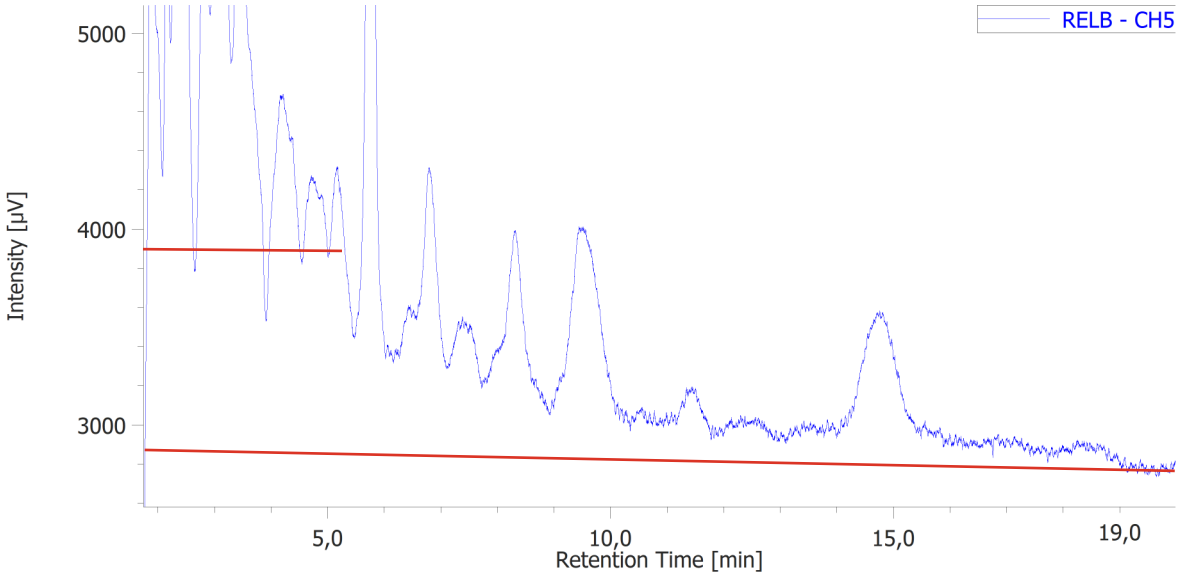

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1,463	608117	95812	100,000	100,000	N/A	1261	N/A	1,381		1180,5

Creator
Reviewer
Approver

Chromatogram

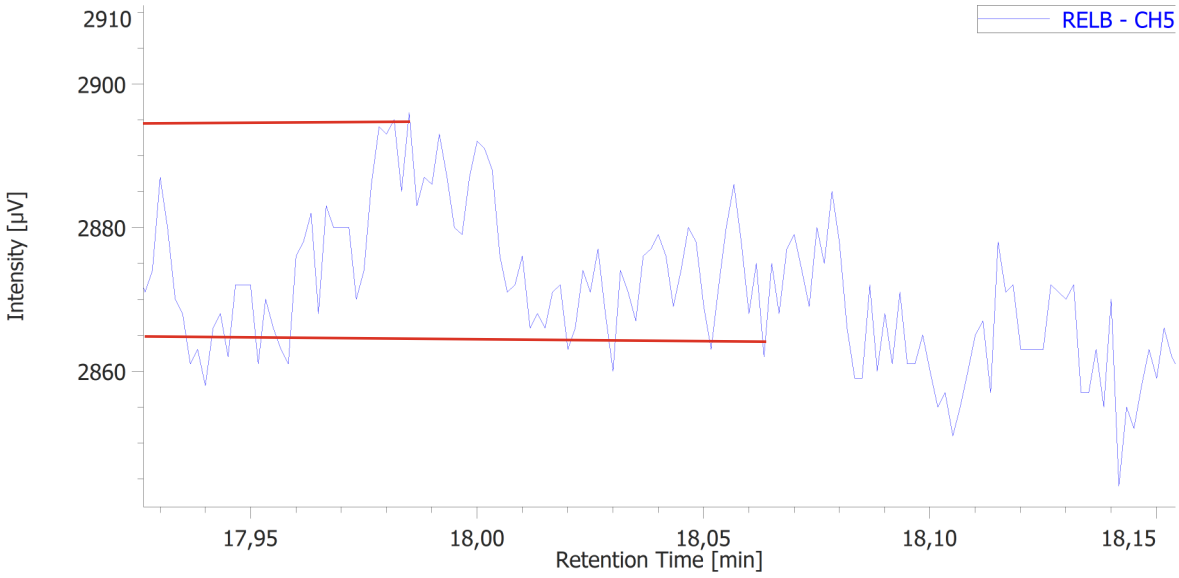

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 13:12:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 12:52:03
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	PCIN
Control Method	RELB HP03
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1,463	608117	95812	100,000	100,000	N/A	1261	N/A	1,381		1180,5

Creator
Reviewer
Approver

Chromatogram

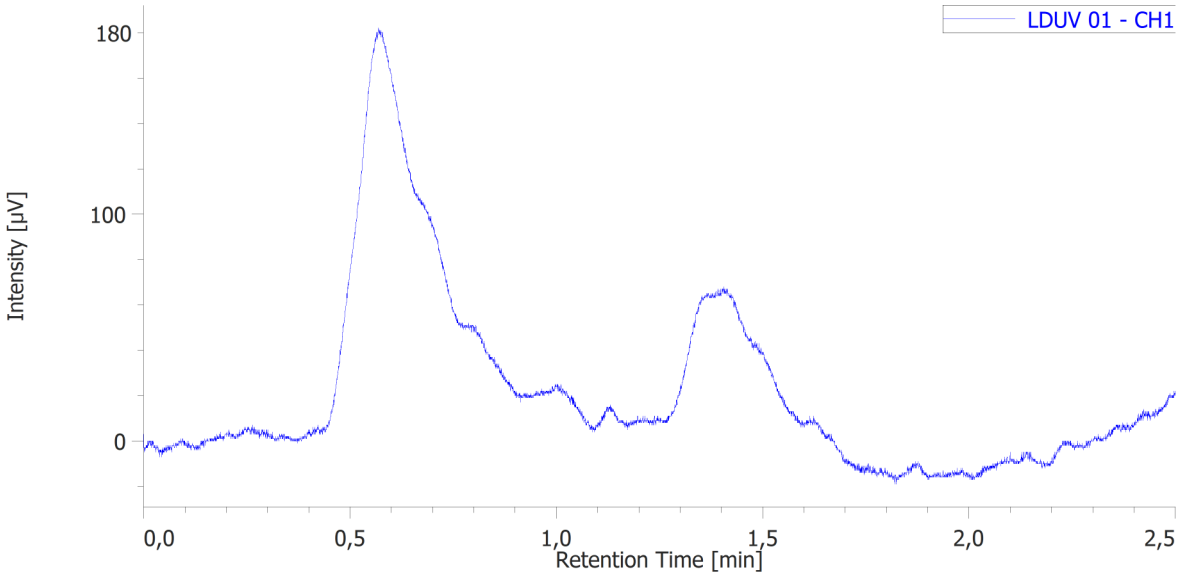


Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:47:23
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:44:51
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

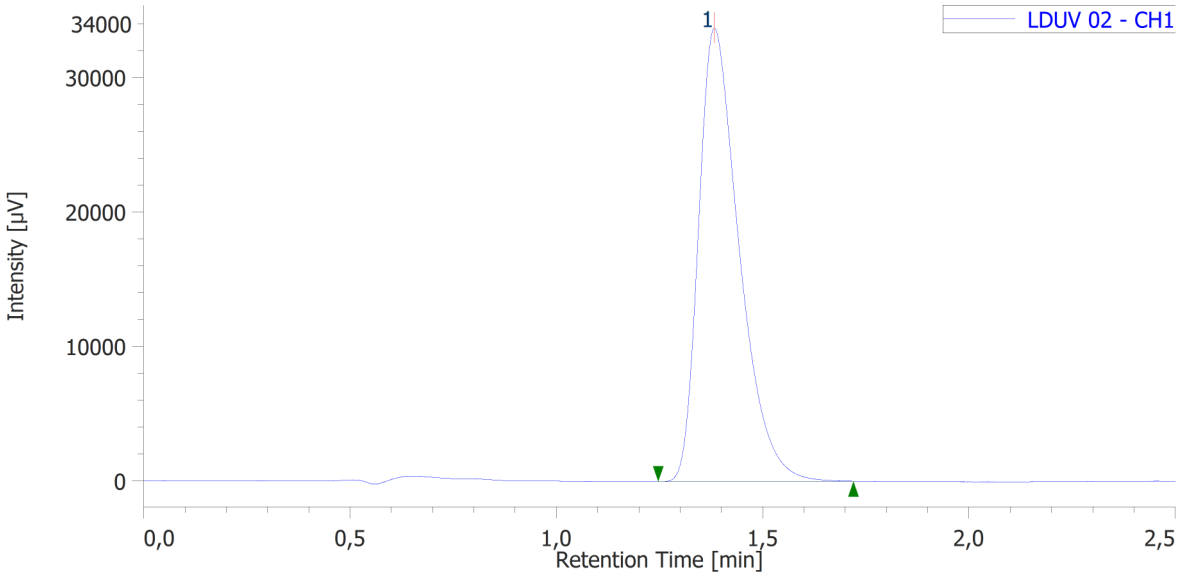

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:50:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:47:33
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.383	230275	33701	100.000	100.000	N/A	989	N/A	1.484		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

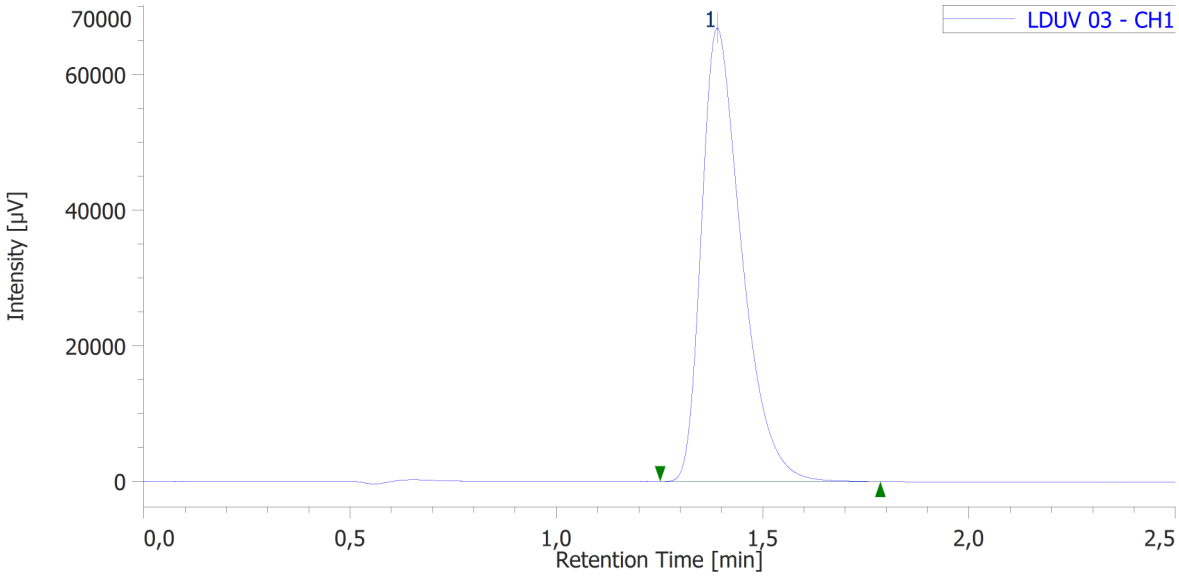

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:52:46
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:50:15
Volume	10.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.389	452132	66861	100.000	100.000	N/A	1026	N/A	1.483		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

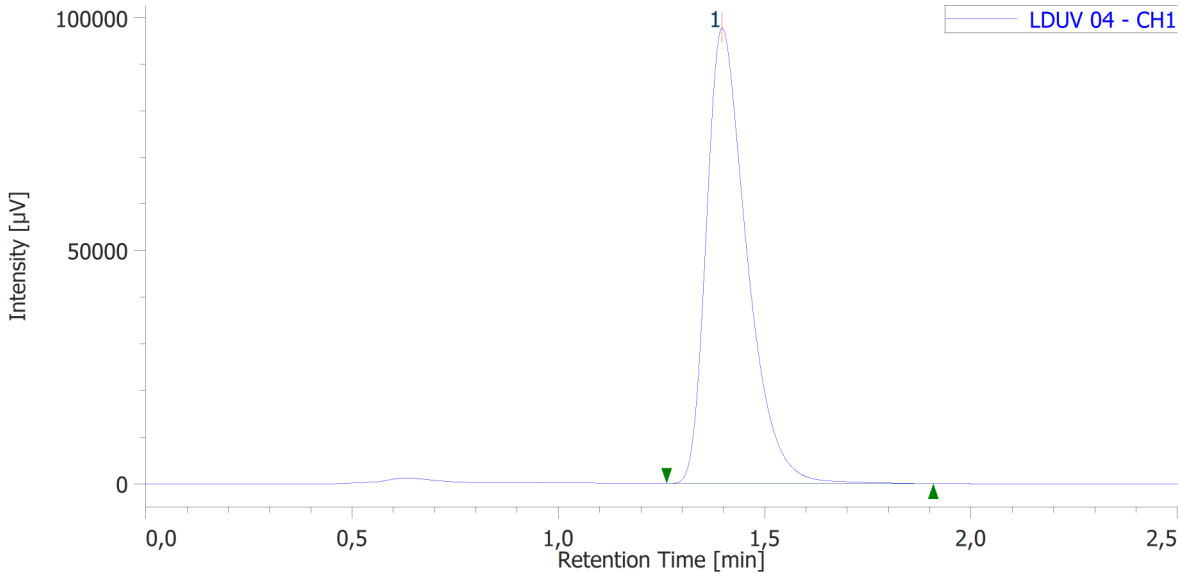

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:55:30
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:52:57
Volume	10.0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.397	665729	97660	100.000	100.000	N/A	1030	N/A	1.484		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

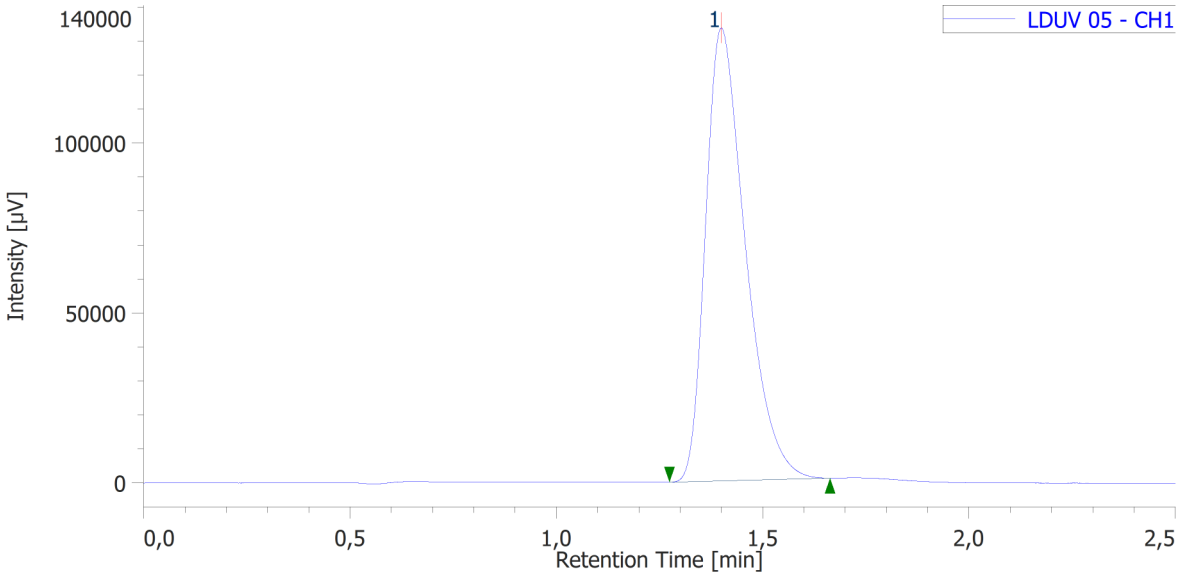

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:58:12
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:55:40
Volume	10.0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.399	893803	133171	100.000	100.000	N/A	1040	N/A	1.458		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

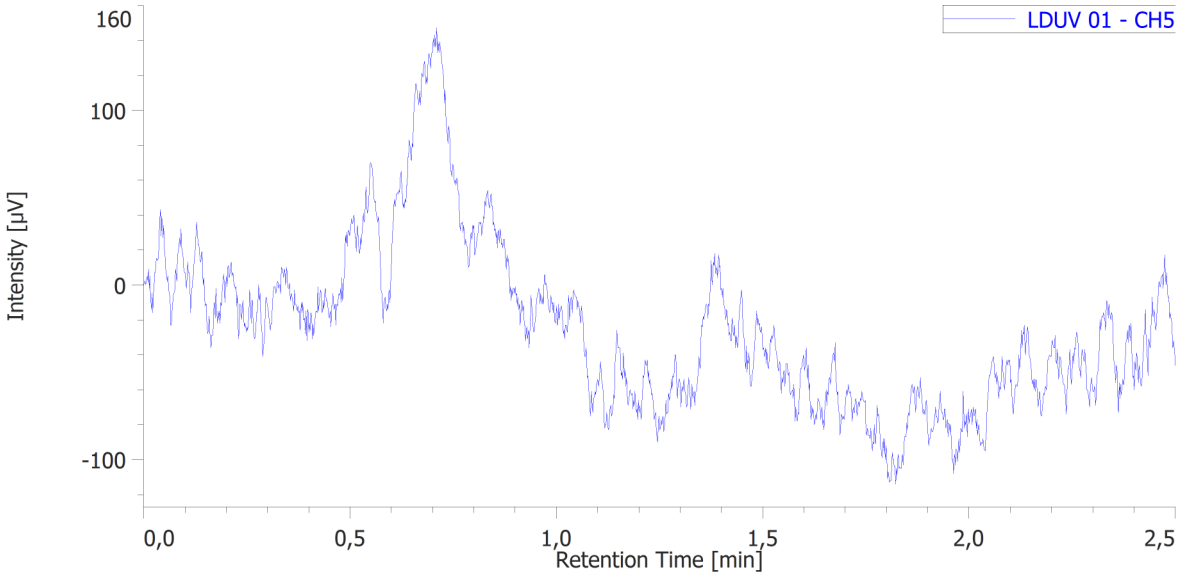


Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:47:23
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:44:51
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

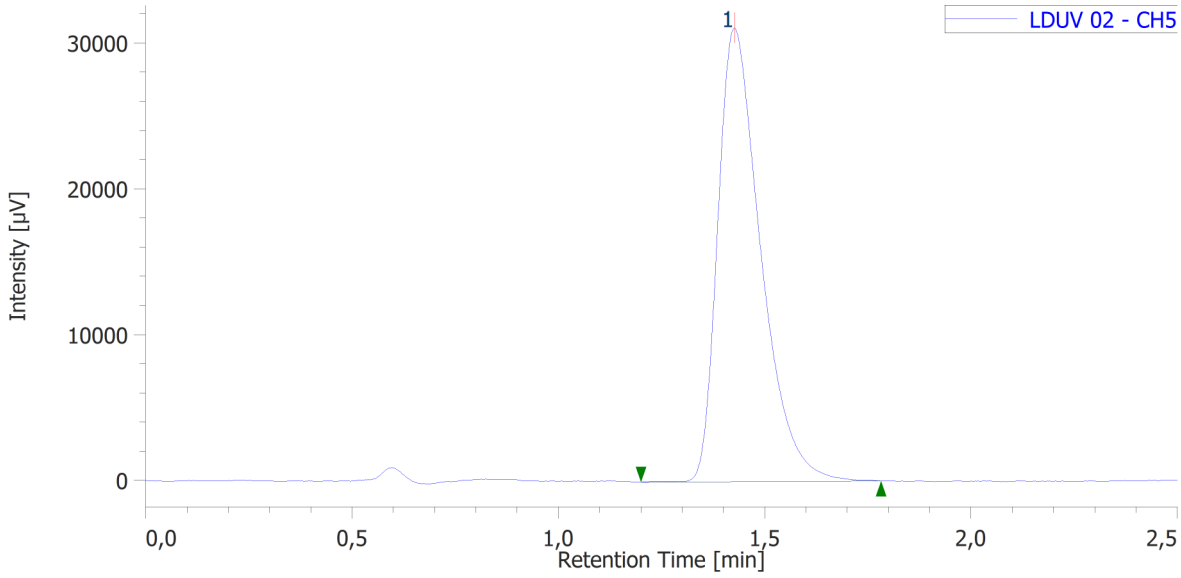

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:50:04
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:47:33
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.427	224711	31096	100.000	100.000	N/A	950	N/A	1.511		N/A

Creator
Reviewer
Approver

Chromatogram

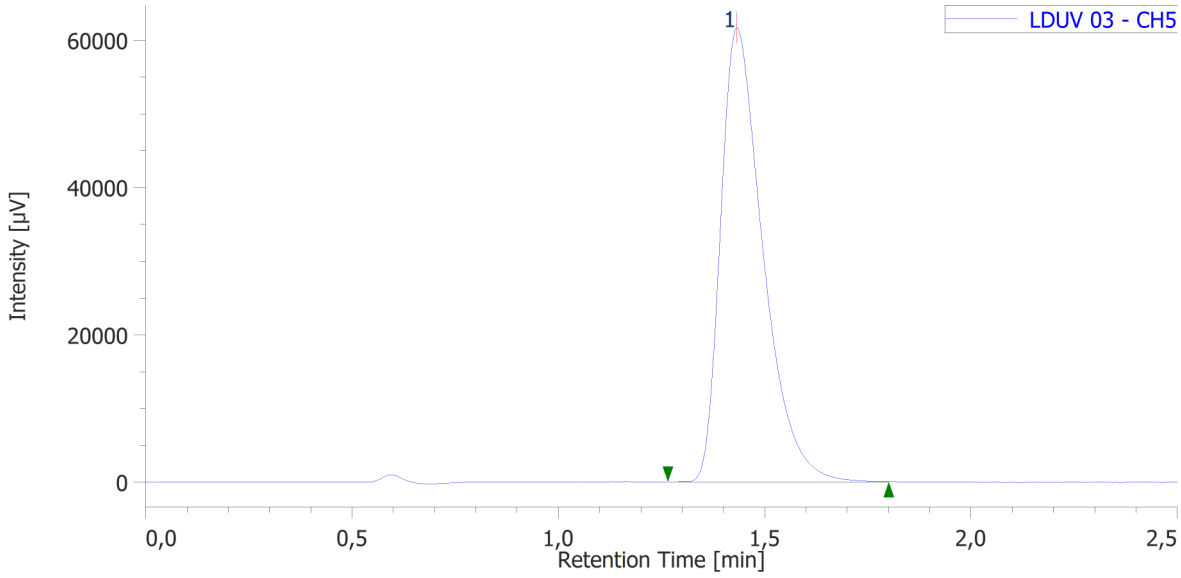

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:52:46
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:50:15
Volume	10.0 [μL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.432	439603	61590	100.000	100.000	N/A	980	N/A	1.541		N/A

Creator
Reviewer
Approver

Chromatogram

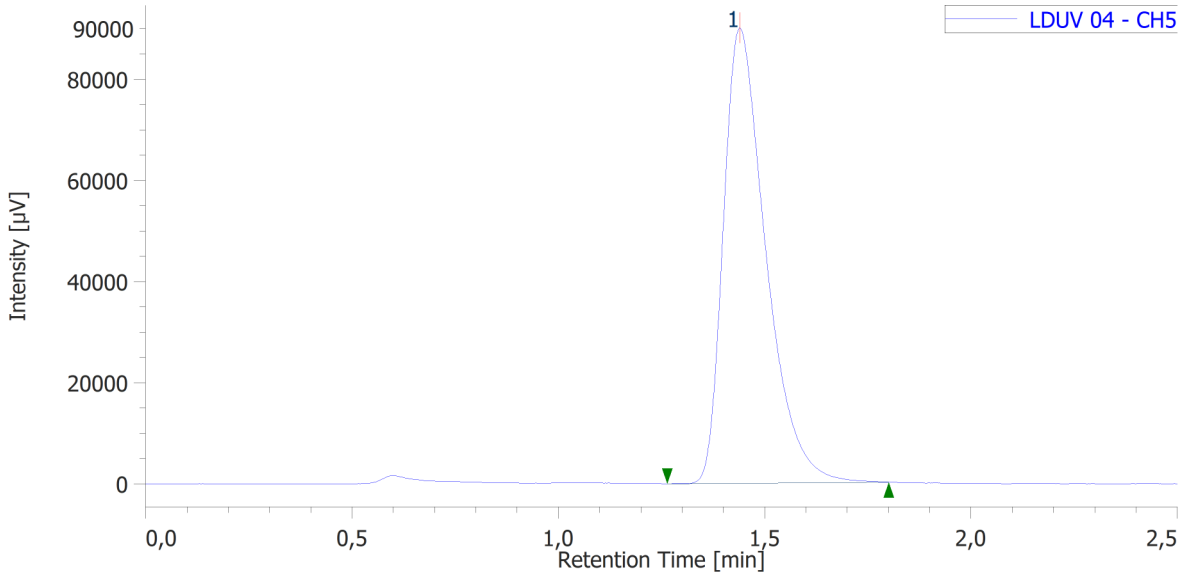

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:55:30
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:52:57
Volume	10.0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.440	643080	89933	100.000	100.000	N/A	990	N/A	1.512		N/A

Creator
Reviewer
Approver

Chromatogram

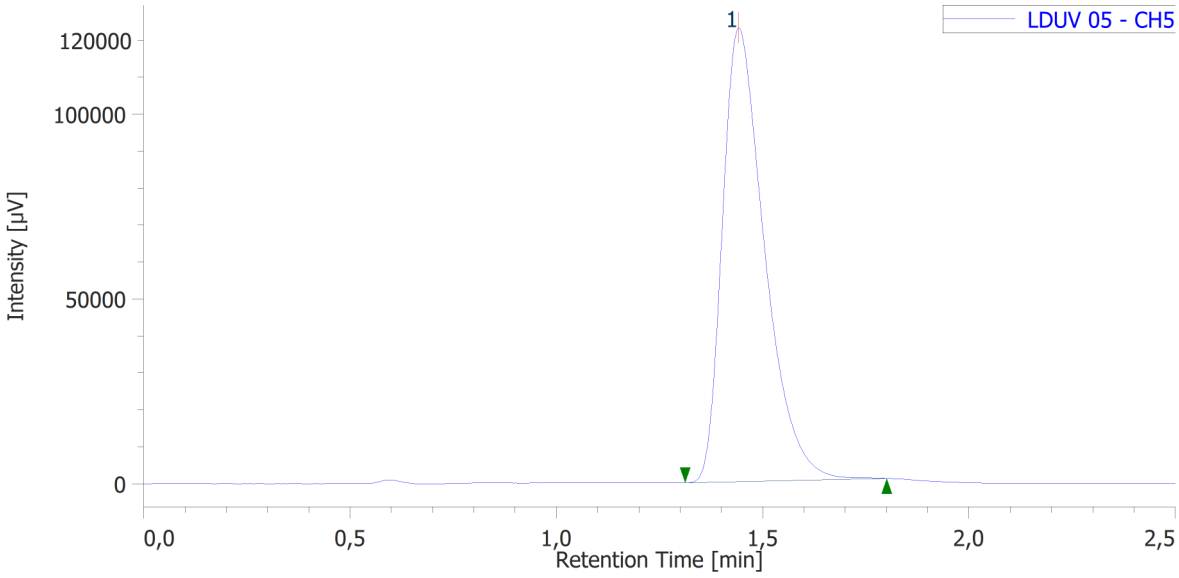

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 15:58:12
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:55:40
Volume	10.0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação 03

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	5	1.442	872121	122704	100.000	100.000	N/A	995	N/A	1.506		N/A

Creator
Reviewer
Approver

Chromatogram

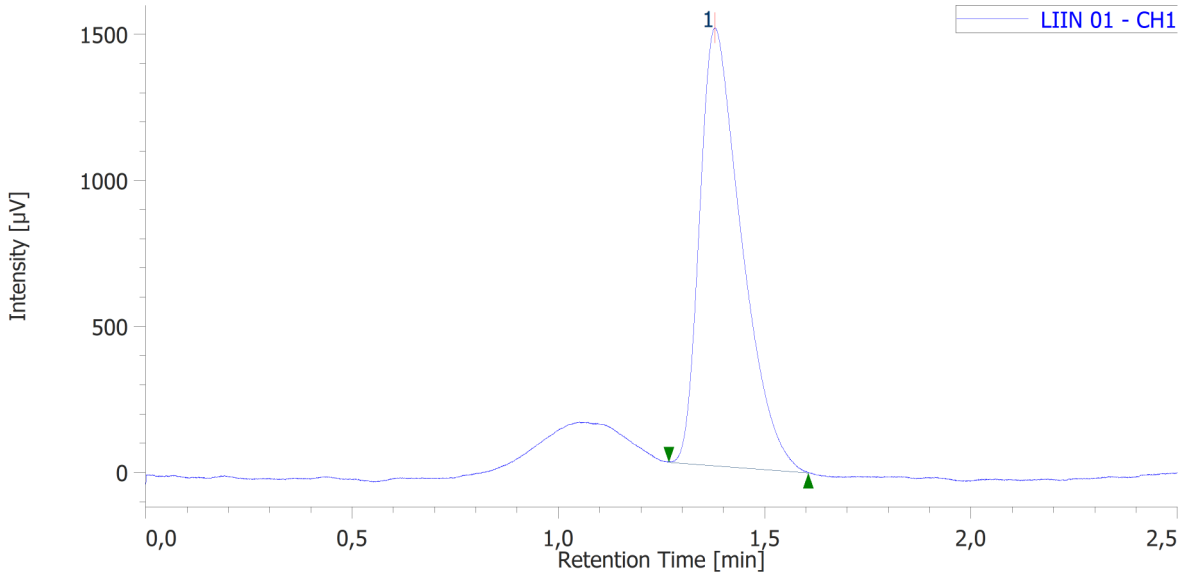

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 16:00:54
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 15:58:22
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1,379	10592	1499	100,000	100,000	N/A	899	N/A	1,578		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

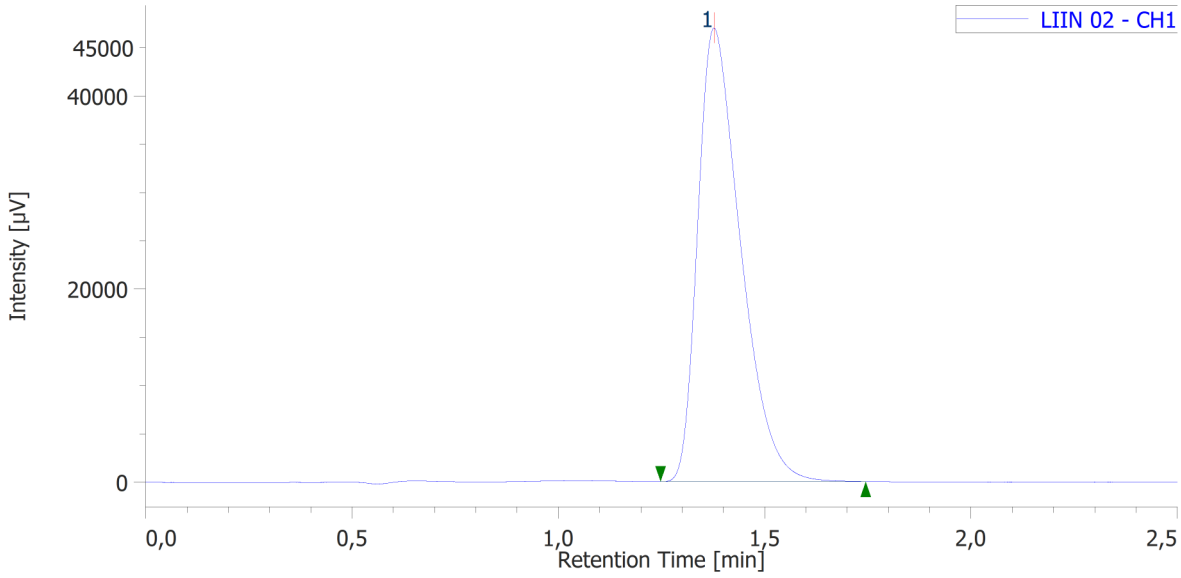

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 16:03:36
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 16:01:04
Volume	5.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.377	338071	46955	100.000	100.000	N/A	862	N/A	1.516		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

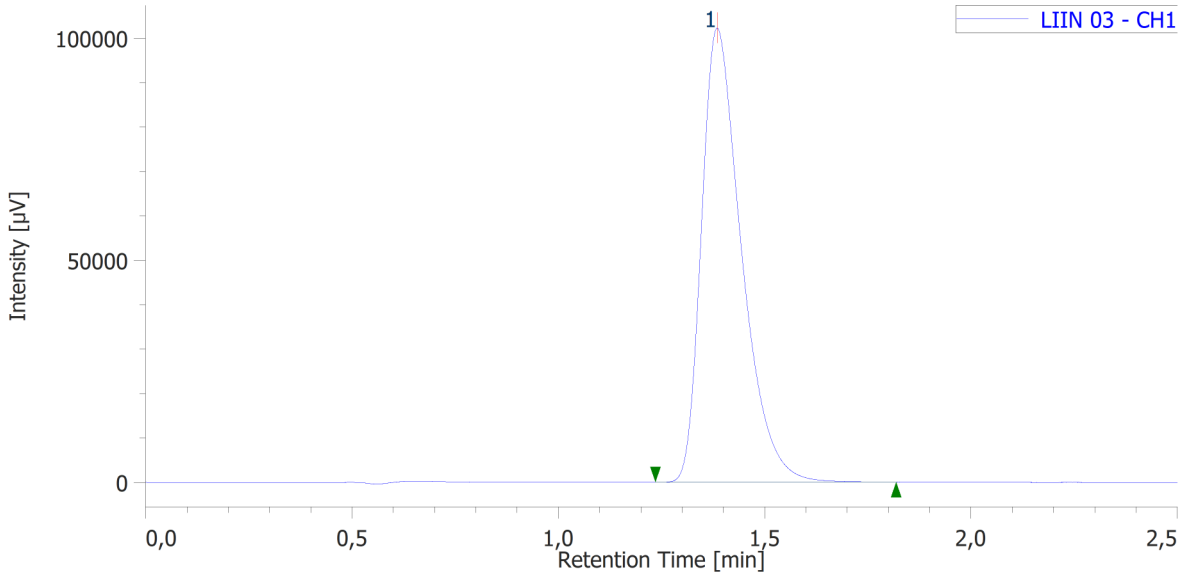

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 16:06:18
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 16:03:46
Volume	10.0 [μL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.385	687912	102229	100.000	100.000	N/A	1030	N/A	1.473		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

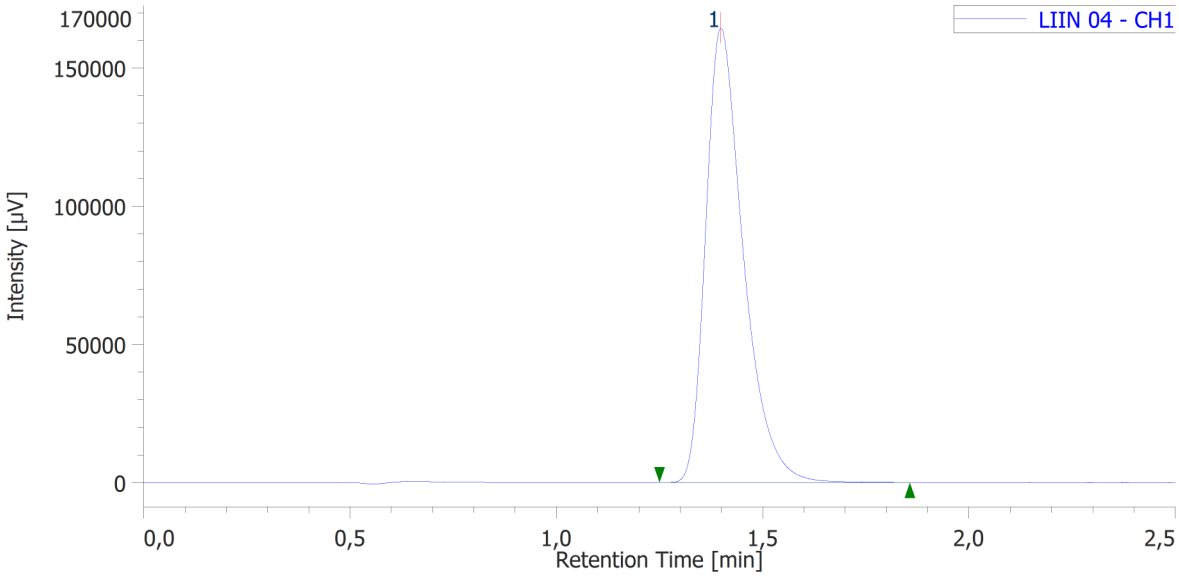

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 16:09:00
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 16:06:28
Volume	15.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.398	1043618	164332	100.000	100.000	N/A	1207	N/A	1.446		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

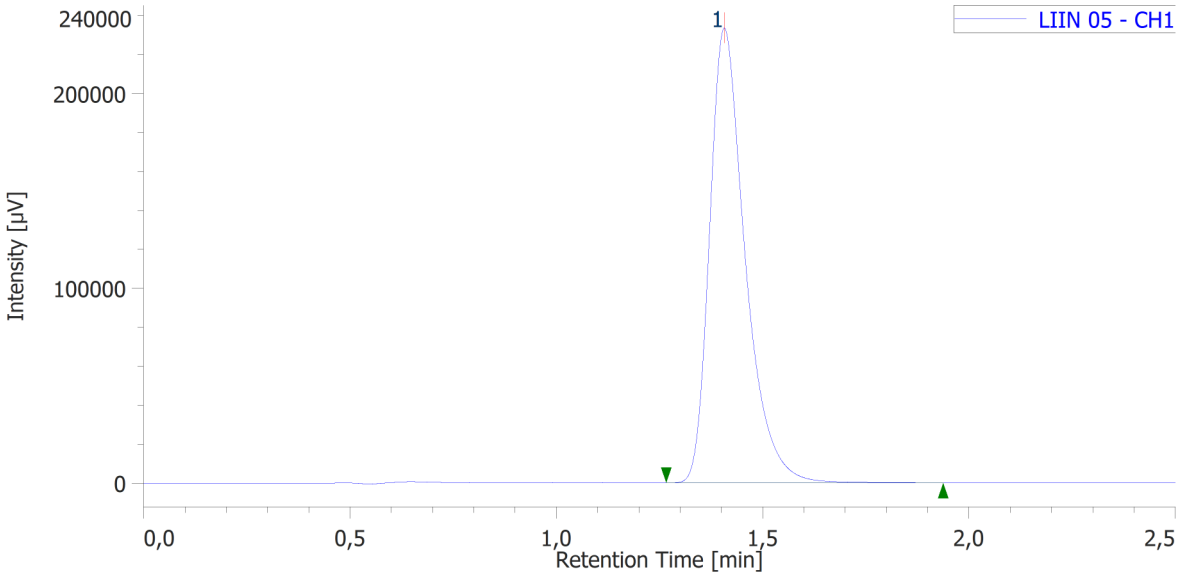

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 16:11:42
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 16:09:11
Volume	20.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2.5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HP03a
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeina	1	1.406	1399345	233477	100.000	100.000	N/A	1391	N/A	1.422		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

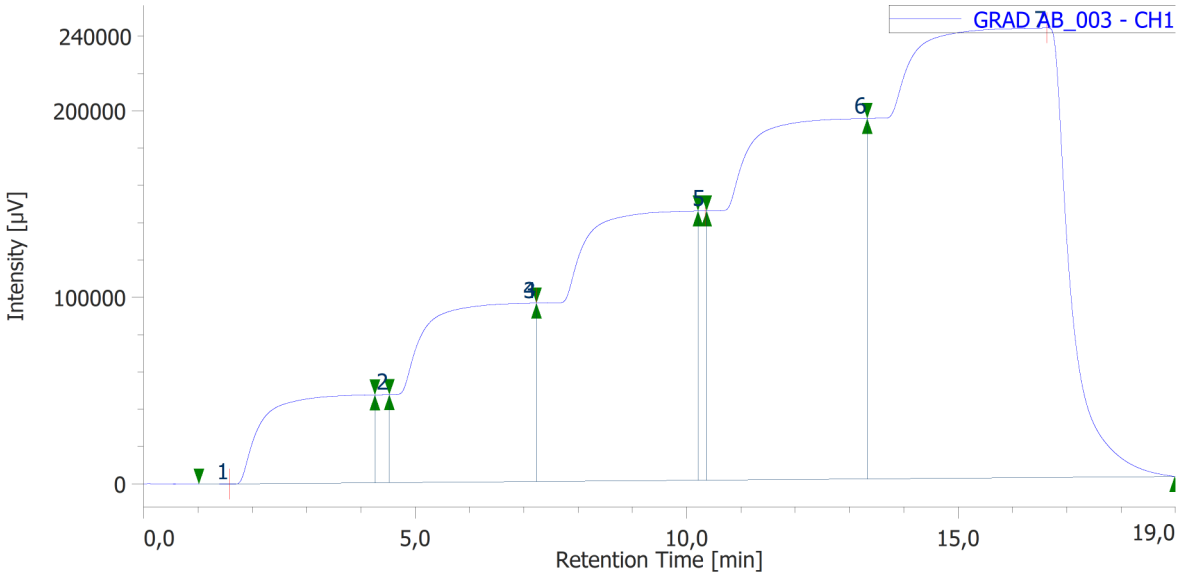

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 17:30:11
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 17:11:09
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB HP03
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	1	1,580	3065	146	0,002	0,018	N/A	90	N/A	0,634		N/A
2	20 %	1	4,519	754250	47144	0,609	5,774	N/A	N/A	N/A	N/A		N/A
3	Unknown	1	7,228	13802971	95511	11,152	11,698	N/A	N/A	N/A	N/A		N/A
4	40 %	1	7,231	23161171	95510	18,713	11,698	N/A	N/A	N/A	N/A		N/A
5	60 %	1	10,338	1387945	144292	1,121	17,672	N/A	N/A	N/A	N/A		N/A
6	80 %	1	13,319	32029998	193063	25,878	23,646	N/A	N/A	N/A	N/A		N/A
7	100 %	1	16,634	52631551	240810	42,523	29,494	N/A	N/A	N/A	N/A		N/A

Creator
Reviewer
Approver

Chromatogram

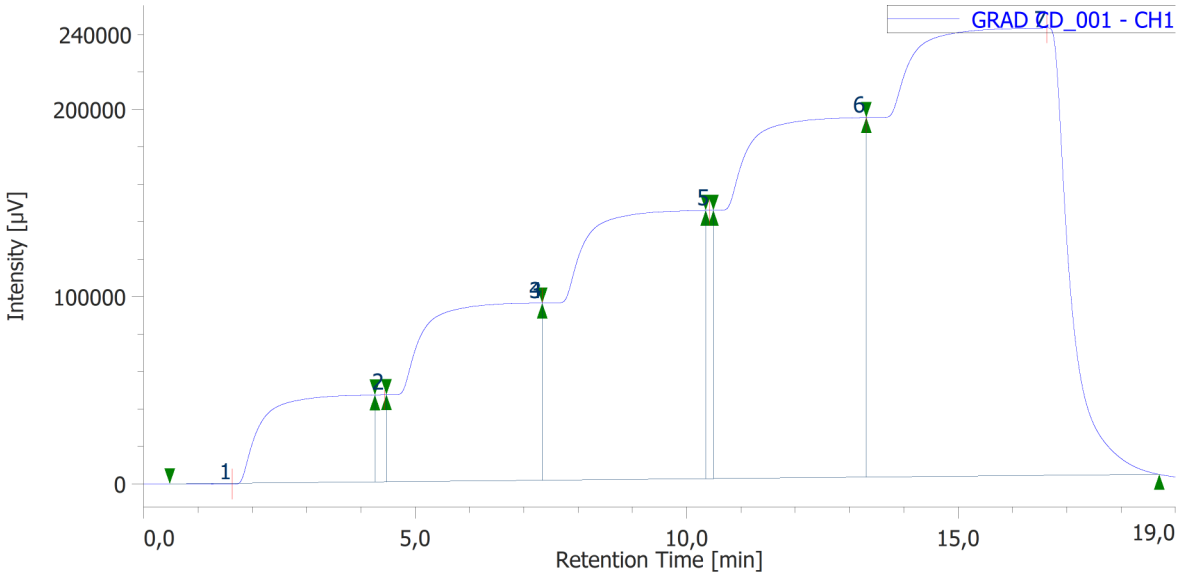

Chromatogram Information	
User Name	QPackSA
Date Modified	05/09/2024 17:56:05
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	05/09/2024 17:37:04
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad CD HP03
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD CD_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	1	1,628	16493	421	0,013	0,052	N/A	33	N/A	0,556		N/A
2	20 %	1	4,441	596416	46561	0,486	5,742	N/A	N/A	N/A	N/A		N/A
3	Unknown	1	7,334	14450874	94738	11,766	11,683	N/A	N/A	N/A	N/A		N/A
4	40 %	1	7,337	23613610	94736	19,227	11,683	N/A	N/A	N/A	N/A		N/A
5	60 %	1	10,423	1227257	143391	0,999	17,684	N/A	N/A	N/A	N/A		N/A
6	80 %	1	13,298	30595292	192049	24,912	23,684	N/A	N/A	N/A	N/A		N/A
7	100 %	1	16,632	52315695	238978	42,597	29,472	N/A	N/A	N/A	N/A		N/A

Creator
Reviewer
Approver