
Peak Find - HPLC_0005 UV_20230830T092751-0300.jws

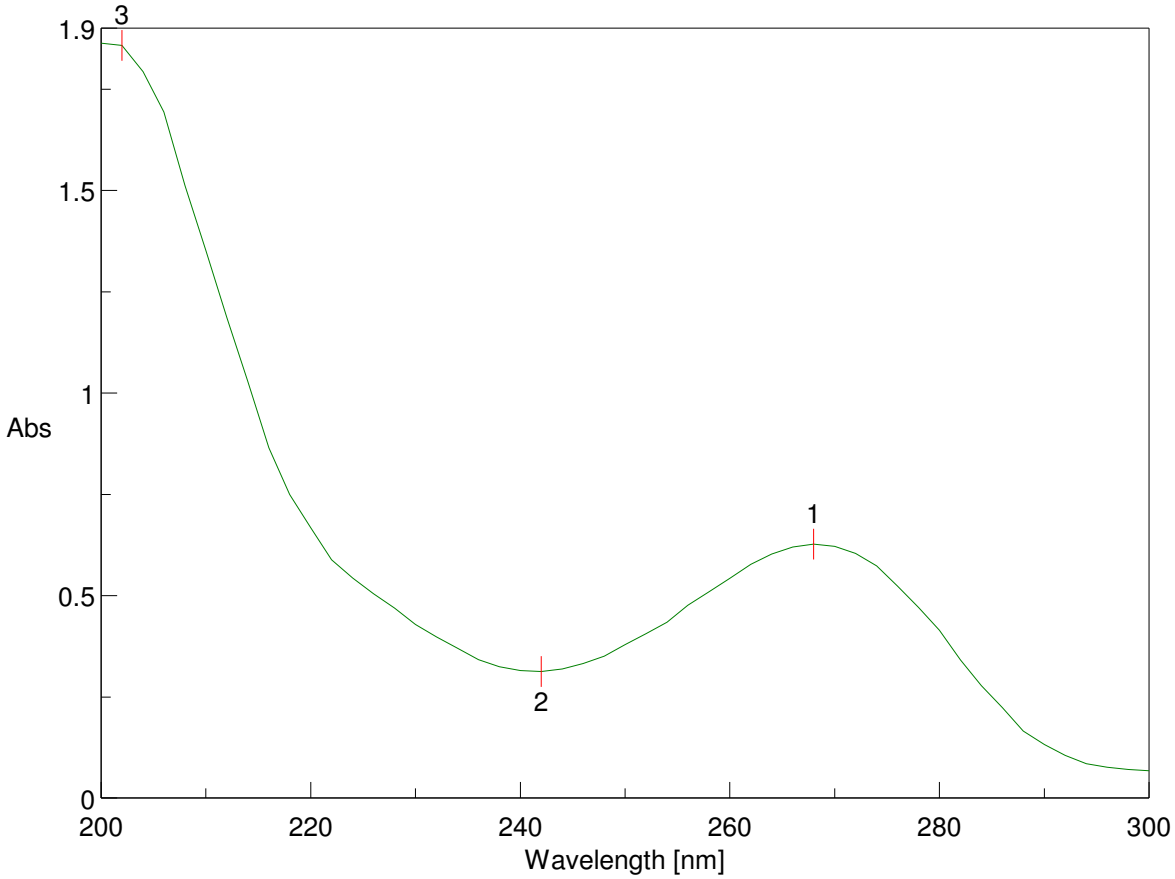

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	30/08/2023 09:27

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200

[Measurement Information]

Instrument Name	X-LC 3075UV
Model Name	X-LC 3075UV
Serial No.	0000000000
ROM version	V6.45


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	271	0.62632	2	243	0.312114
3	203	1.85742			

Chromatogram Information

User Name	Administrator
Date Modified	29/08/2023 17:01:37
Description	
HPLC System Name	HPLC_0005
Injection Date	29/08/2023 16:41:34
Volume	20.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação 05
Control Method	RELB
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	
Column Info	

Chromatogram

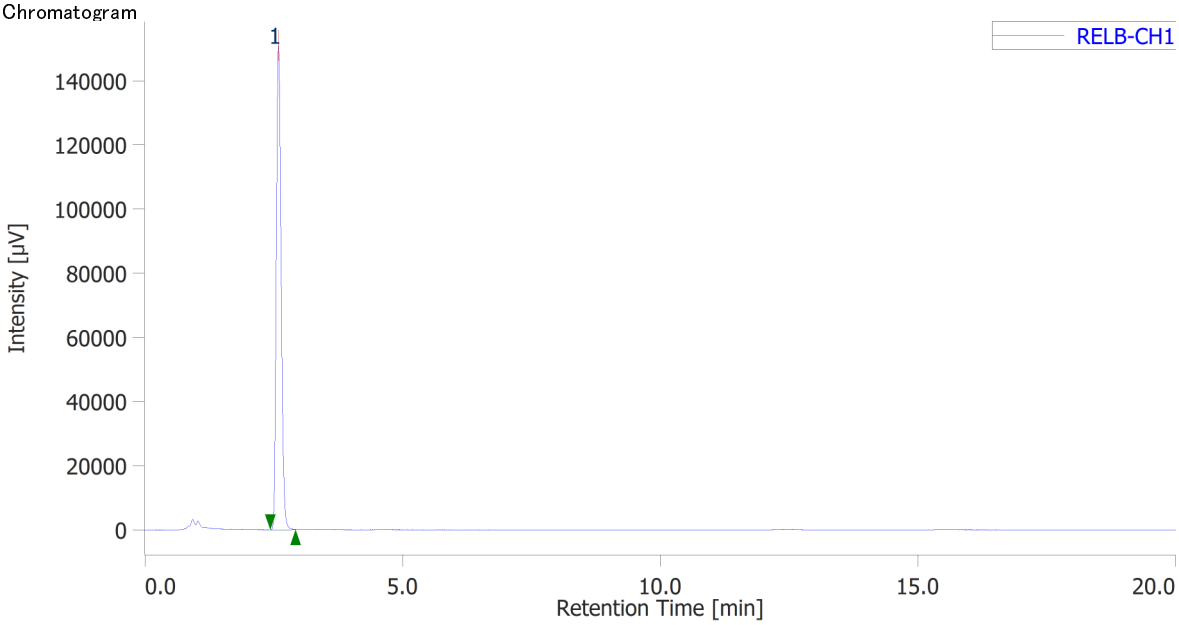


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.593	979313	150811	100.000	100.000	N/A	3692	N/A	1.221	

Creator
Reviewer
Approver

Chromatogram

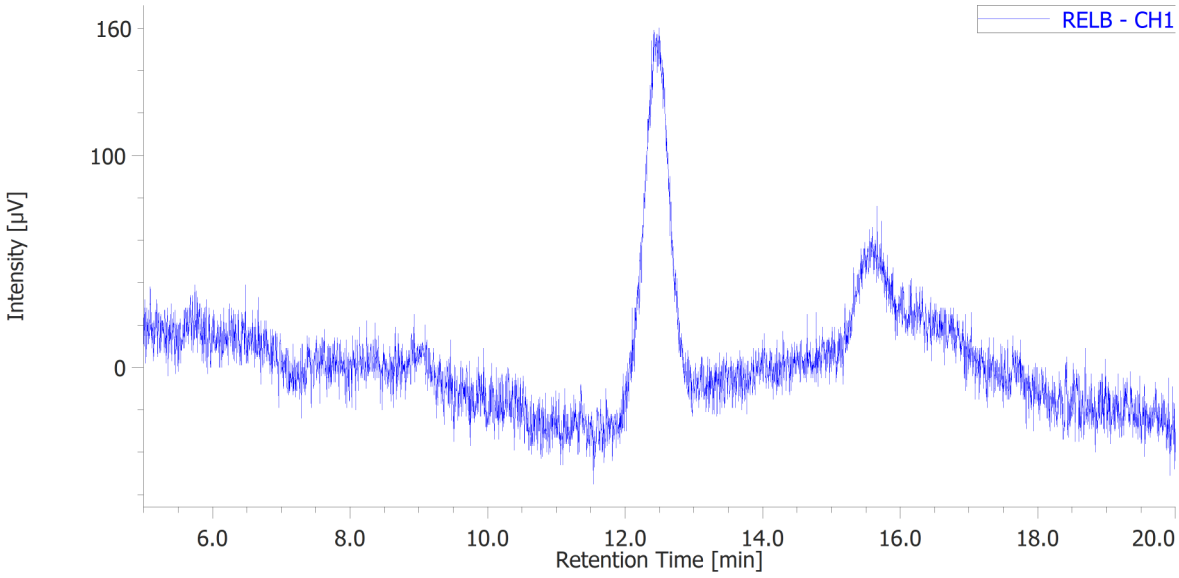

Chromatogram Information	
User Name	Administrator
Date Modified	29/08/2023 17:01:37
Description	
HPLC System Name	HPLC_0005
Injection Date	29/08/2023 16:41:34
Volume	20.0 [µL]
Sample #	1
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação 05
Control Method	RELB
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.593	979313	150811	100.000	100.000	N/A	3692	N/A	1.221	

Creator
Reviewer
Approver

Chromatogram

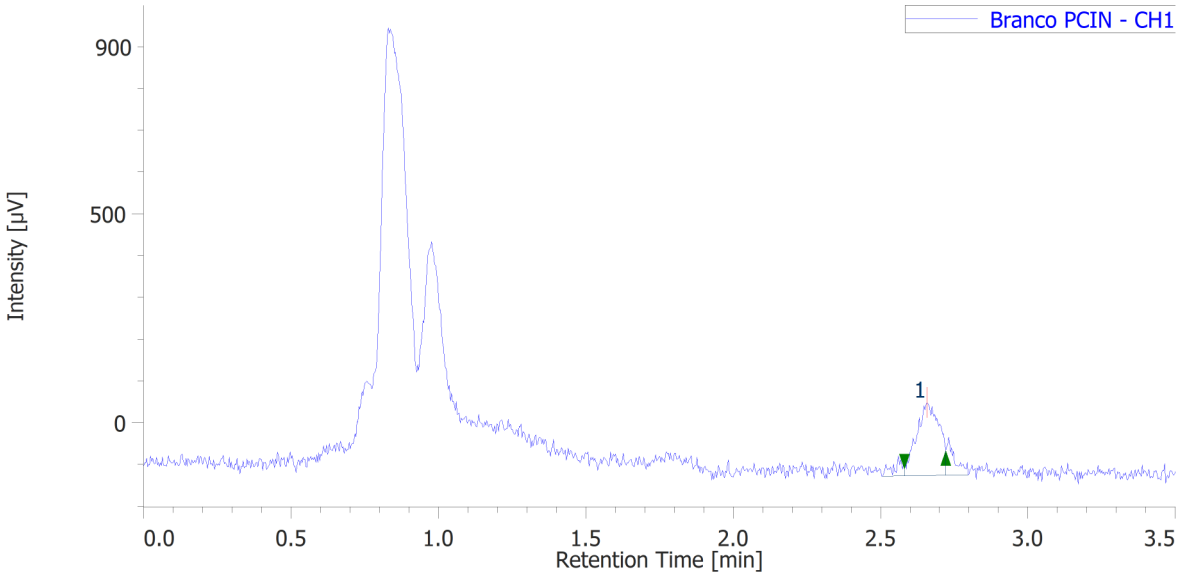

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:06:04
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:02:31
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco PCIN-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.657	924	174	100.000	100.000	N/A	3510	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

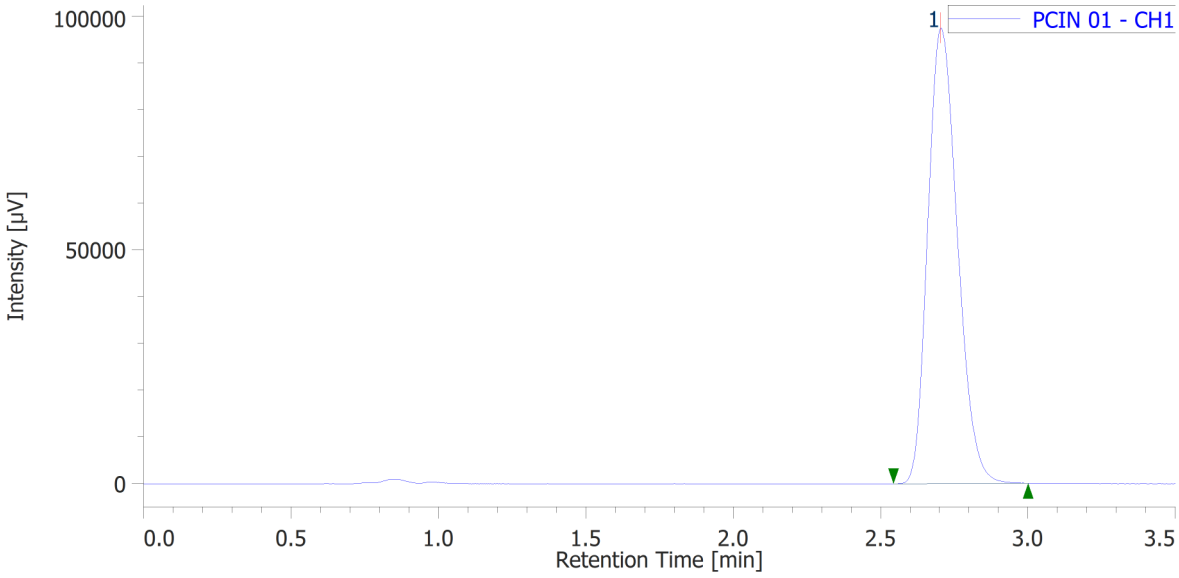

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:10:48
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:07:15
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.703	680304	97420	100.000	100.000	N/A	3407	N/A	1.238	

Creator
Reviewer
Approver

Chromatogram

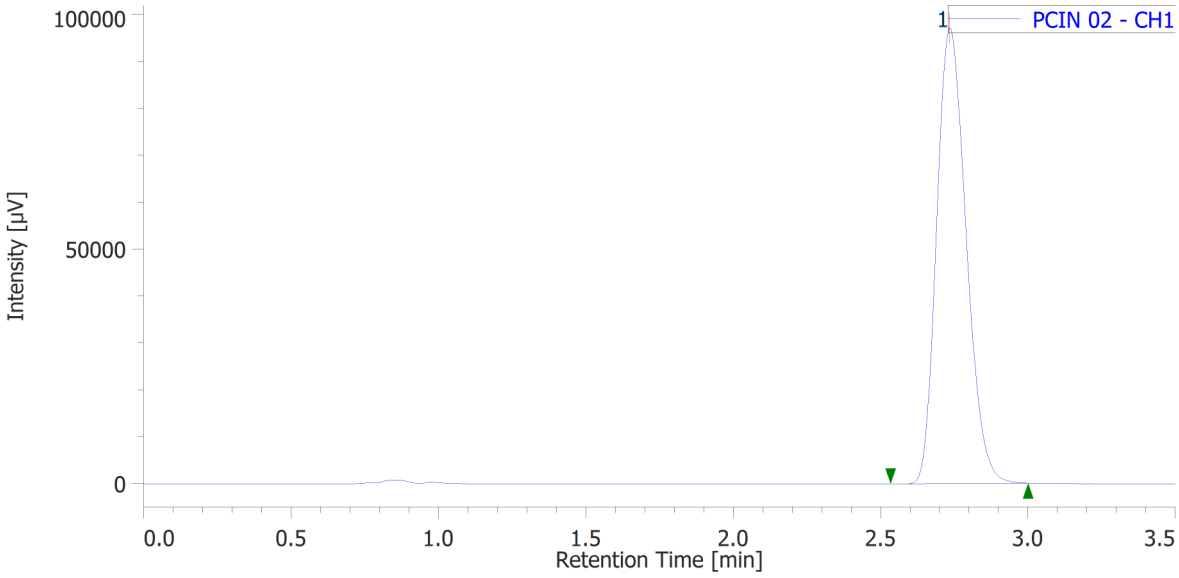

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:15:30
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:11:59
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.733	675924	97118	100.000	100.000	N/A	3500	N/A	1.235	

Creator
Reviewer
Approver

Chromatogram

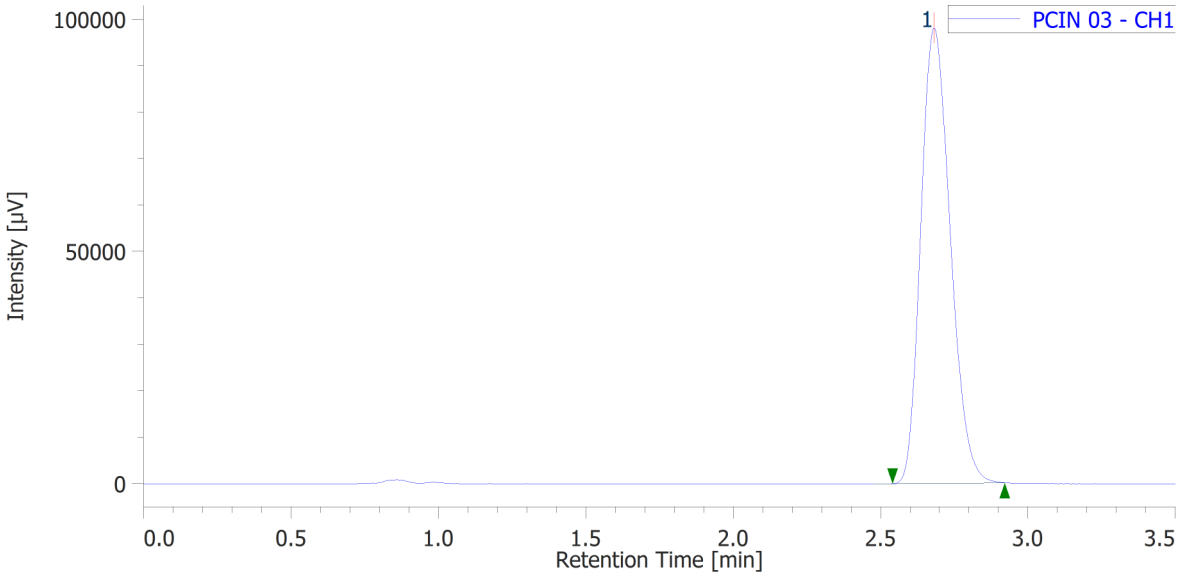

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:20:14
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:16:42
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.680	680969	98026	100.000	100.000	N/A	3377	N/A	1.230	

Creator
Reviewer
Approver

Chromatogram

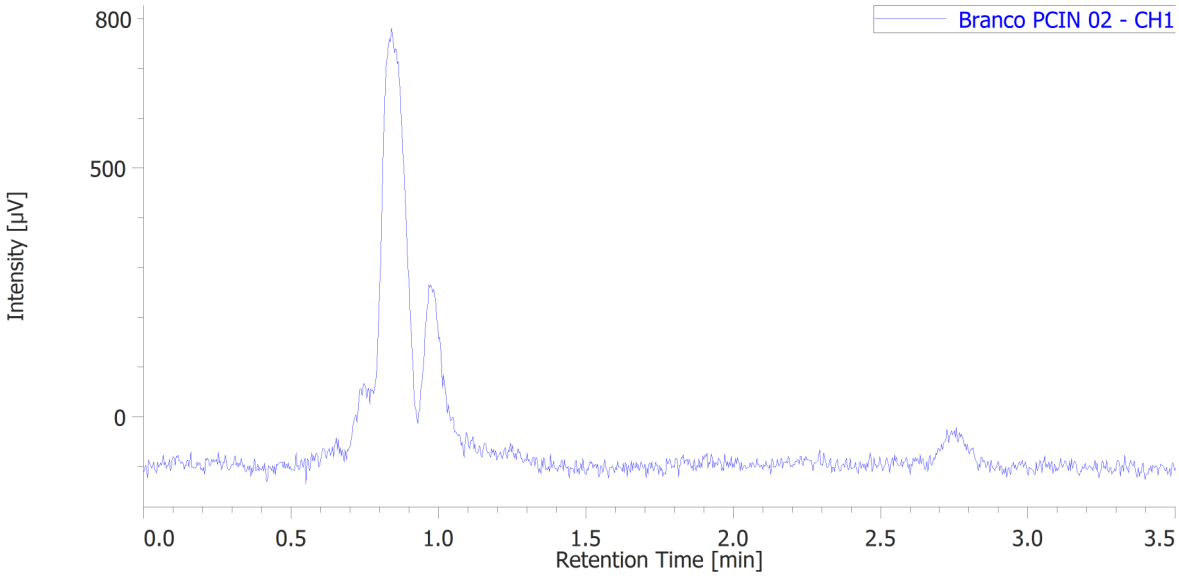


Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:24:56
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:21:23
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

Creator
Reviewer
Approver

Chromatogram

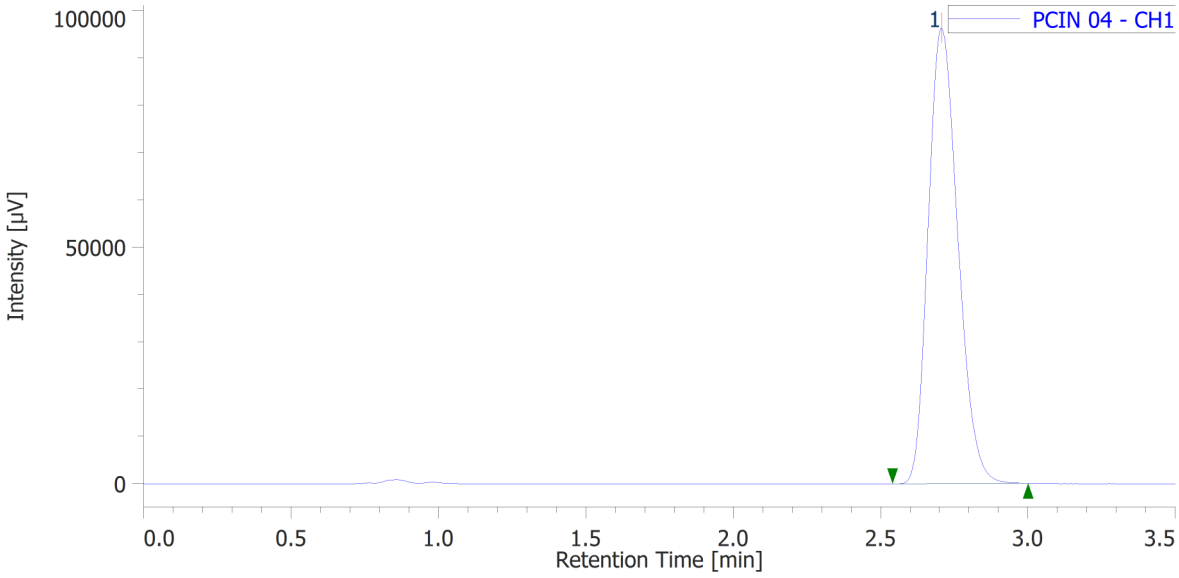

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:29:40
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:26:07
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.707	673066	96340	100.000	100.000	N/A	3414	N/A	1.213	

Creator
Reviewer
Approver

Chromatogram

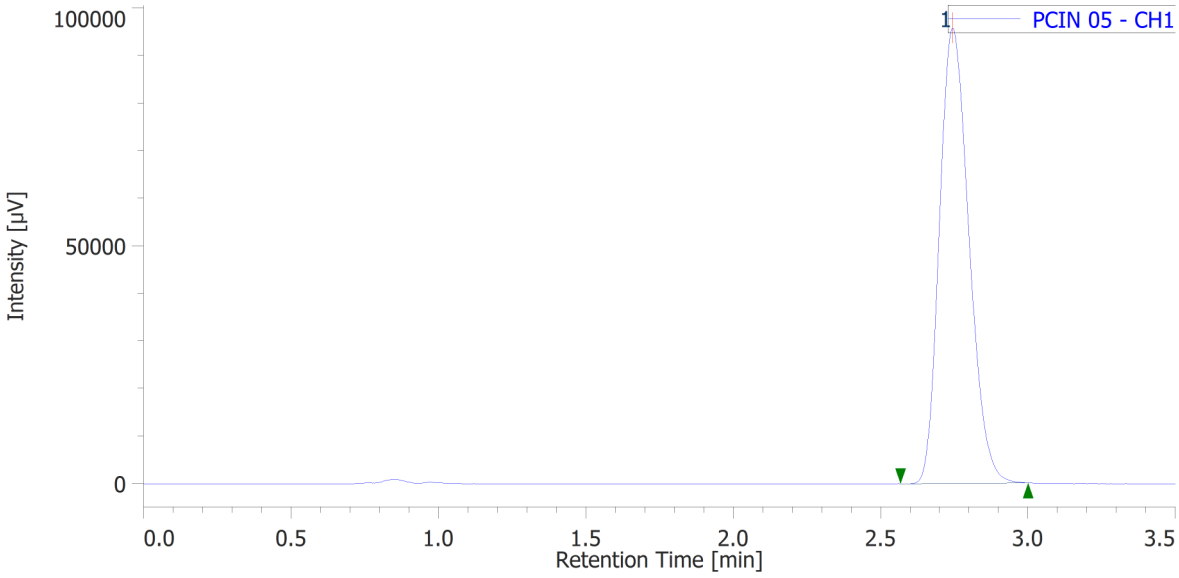

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:34:20
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:30:48
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.743	665791	95740	100.000	100.000	N/A	3529	N/A	1.227	

Creator
Reviewer
Approver

Chromatogram

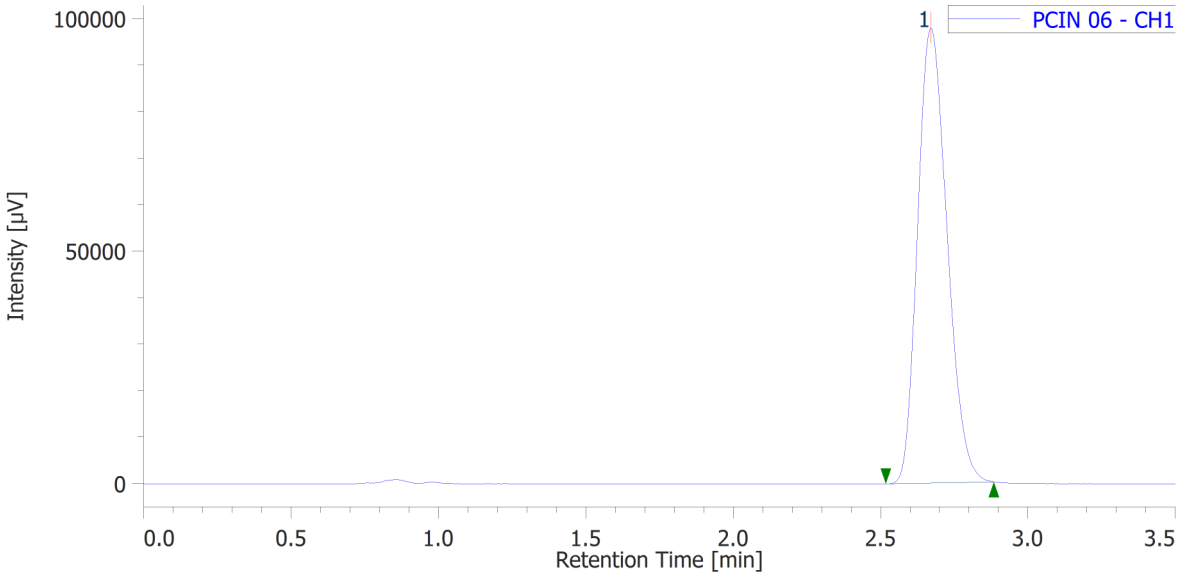

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:39:04
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:35:32
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.670	679480	97814	100.000	100.000	N/A	3335	N/A	1.217	

Creator
Reviewer
Approver

Chromatogram

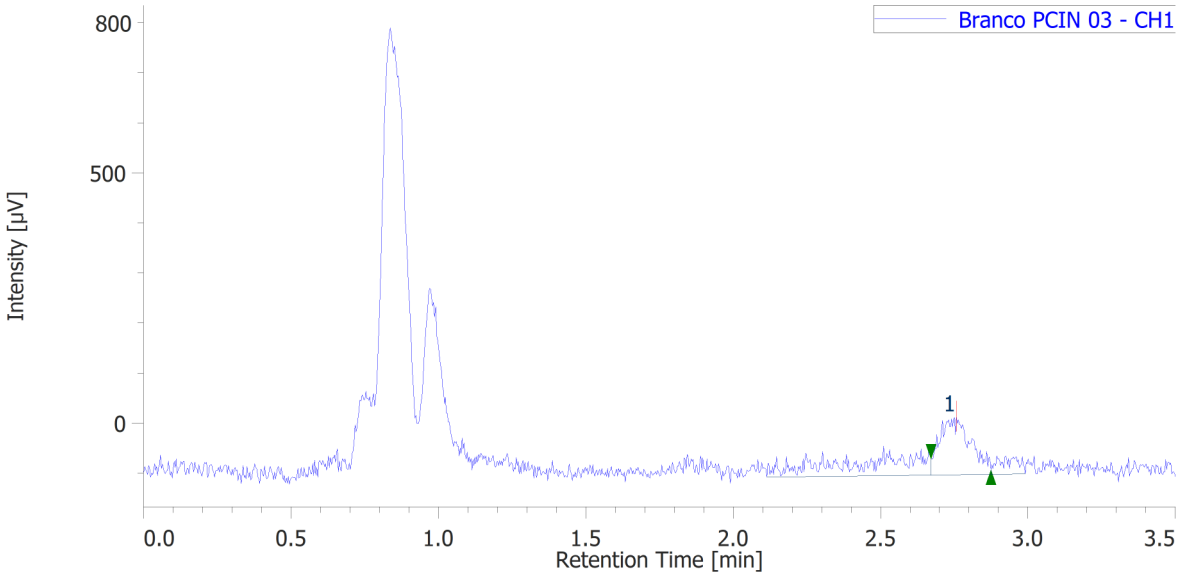

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:43:46
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:40:14
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.757	831	117	100.000	100.000	N/A	2456	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

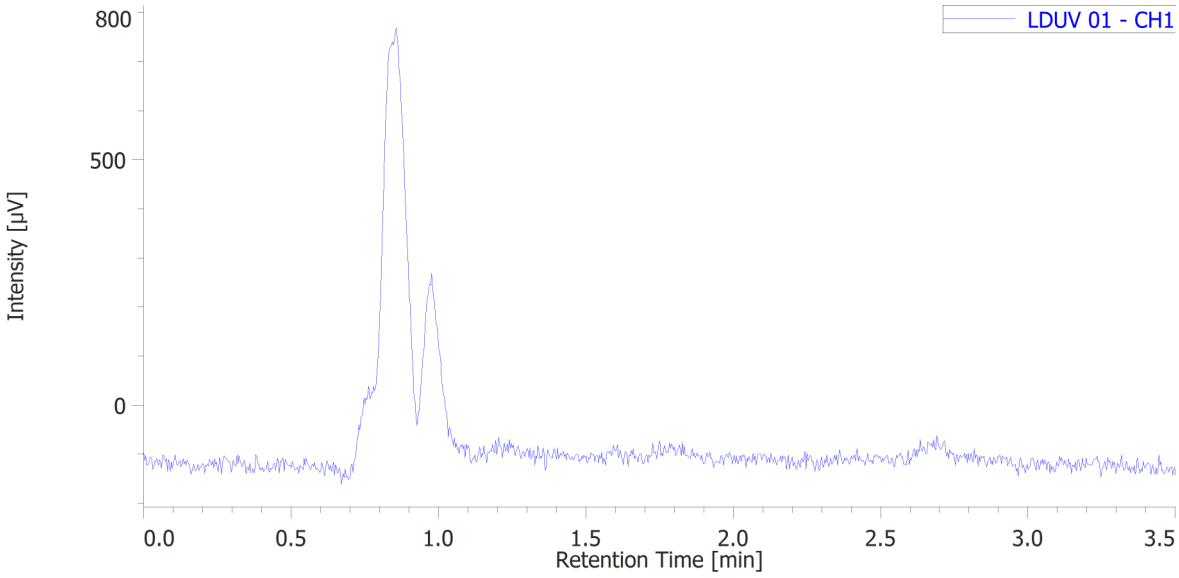


Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:48:30
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:44:57
Volume	10.0 [µL]
Sample #	5
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

Creator
Reviewer
Approver

Chromatogram

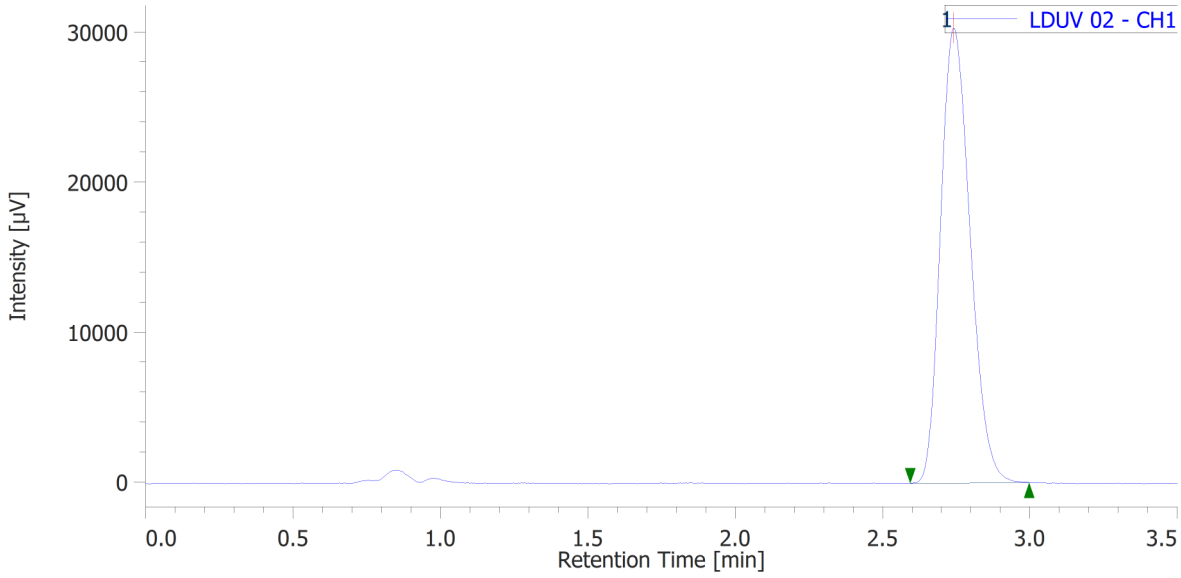

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:53:14
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:49:41
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.740	211868	30316	100.000	100.000	N/A	3488	N/A	1.234	

Creator
Reviewer
Approver

Chromatogram

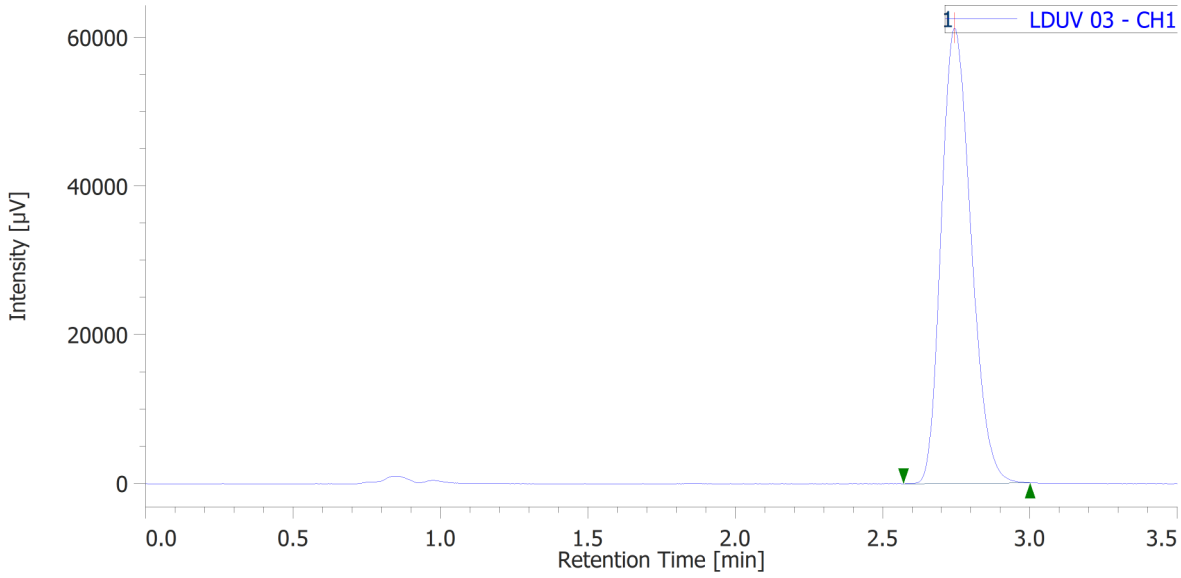

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 11:57:58
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:54:25
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.743	429848	61249	100.000	100.000	N/A	3461	N/A	1.228	

Creator
Reviewer
Approver

Chromatogram

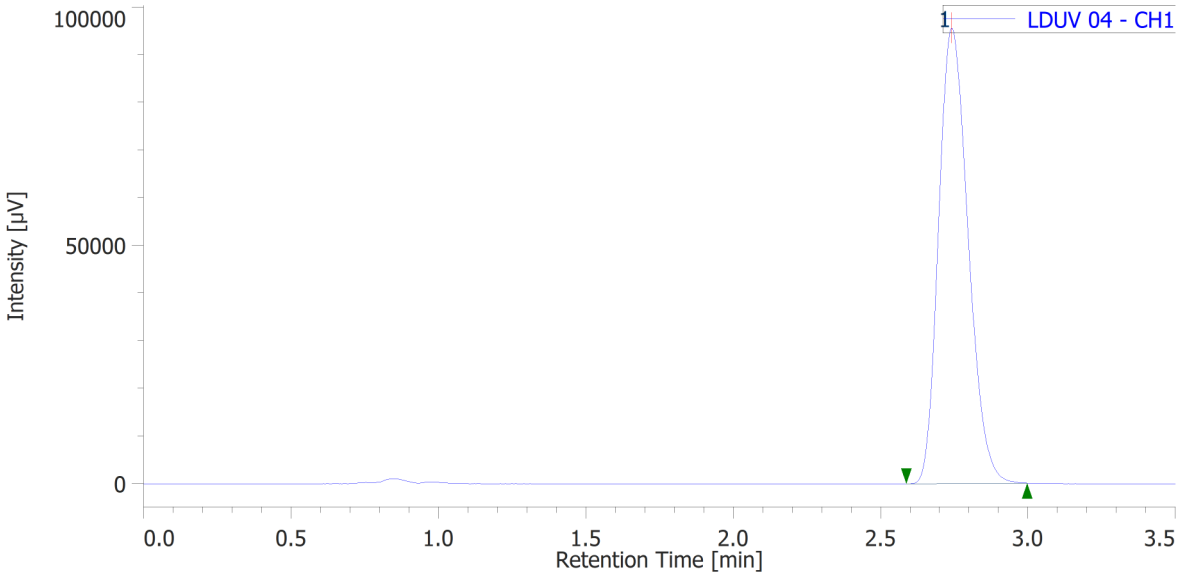

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:02:44
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 11:59:12
Volume	10.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.740	665160	95546	100.000	100.000	N/A	3513	N/A	1.236	

Creator
Reviewer
Approver

Chromatogram

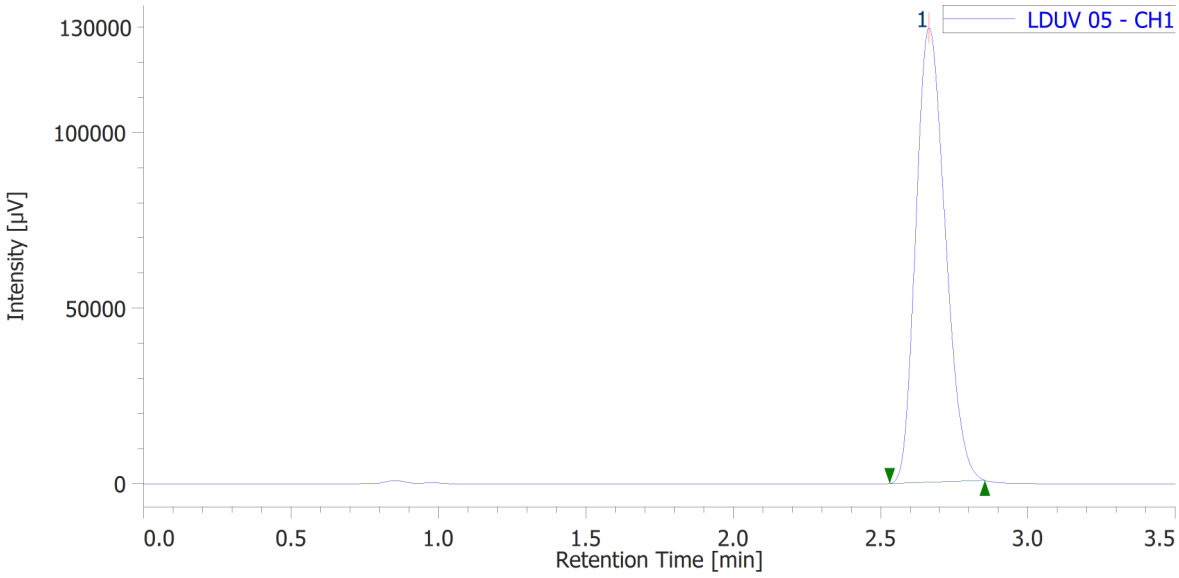

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:07:30
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:03:58
Volume	10.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.663	896331	129314	100.000	100.000	N/A	3309	N/A	1.219	

Creator
Reviewer
Approver

Chromatogram

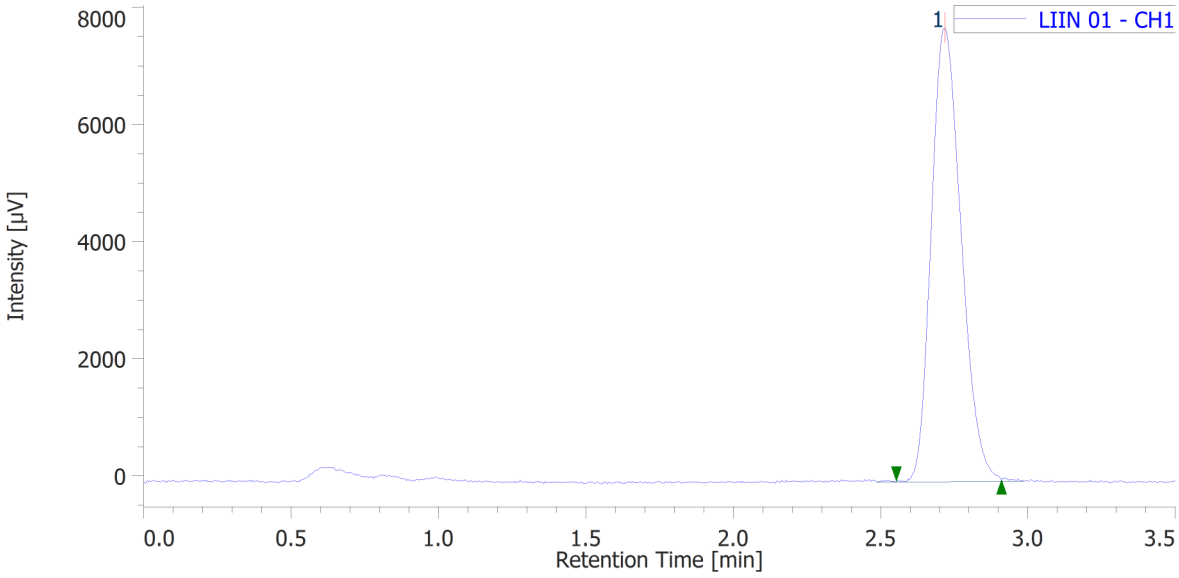

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:12:14
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:08:41
Volume	0.1 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.717	54631	7744	100.000	100.000	N/A	3373	N/A	1.228	

Creator
Reviewer
Approver

Chromatogram

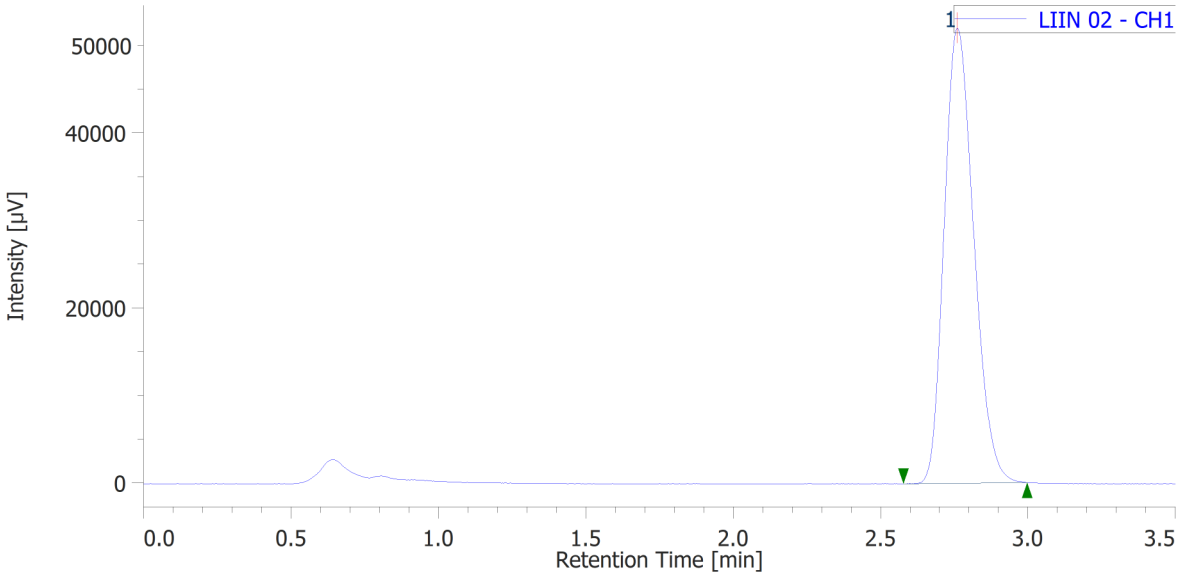

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:17:00
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:13:27
Volume	5.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.760	362854	52021	100.000	100.000	N/A	3568	N/A	1.227	

Creator
Reviewer
Approver

Chromatogram

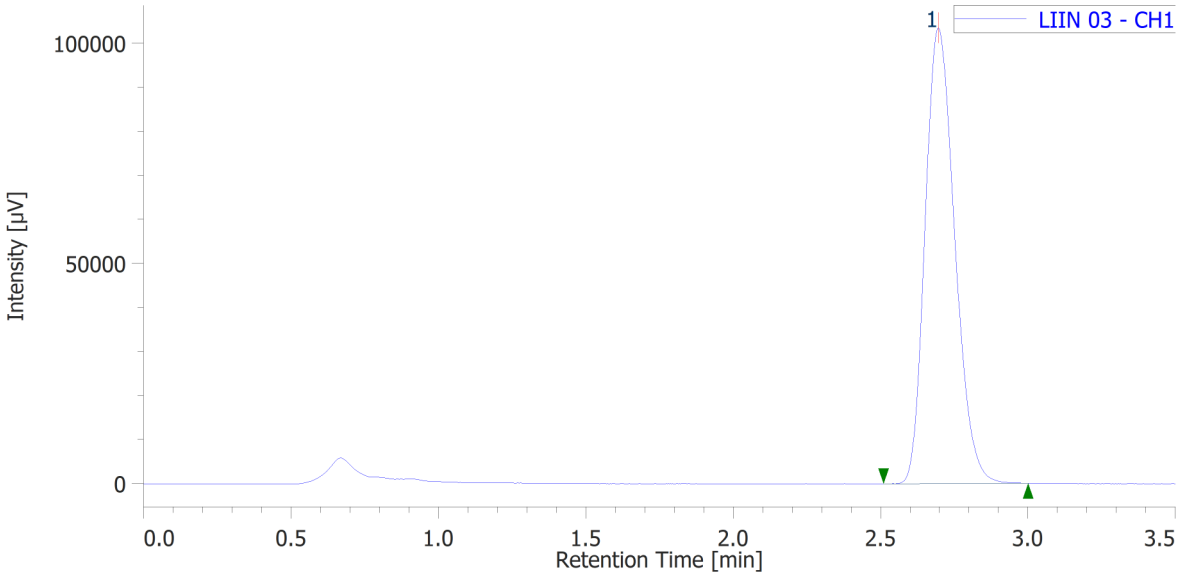

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:21:46
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:18:14
Volume	10.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.697	723070	103408	100.000	100.000	N/A	3398	N/A	1.208	

Creator
Reviewer
Approver

Chromatogram

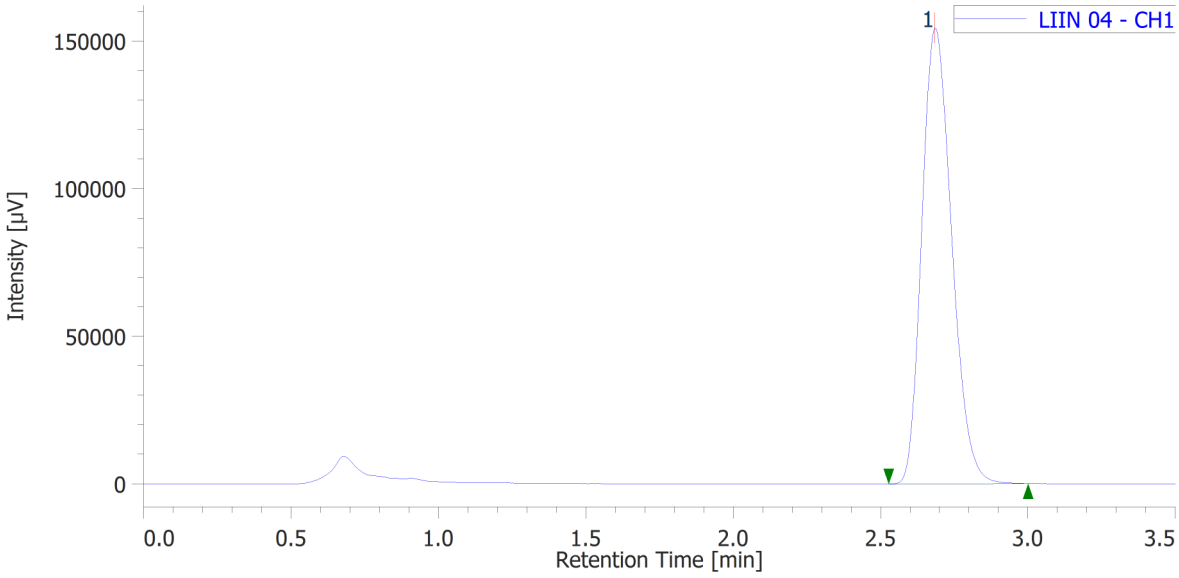

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:26:34
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:23:02
Volume	15.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.683	1086331	154394	100.000	100.000	N/A	3318	N/A	1.243	

Creator
Reviewer
Approver

Chromatogram

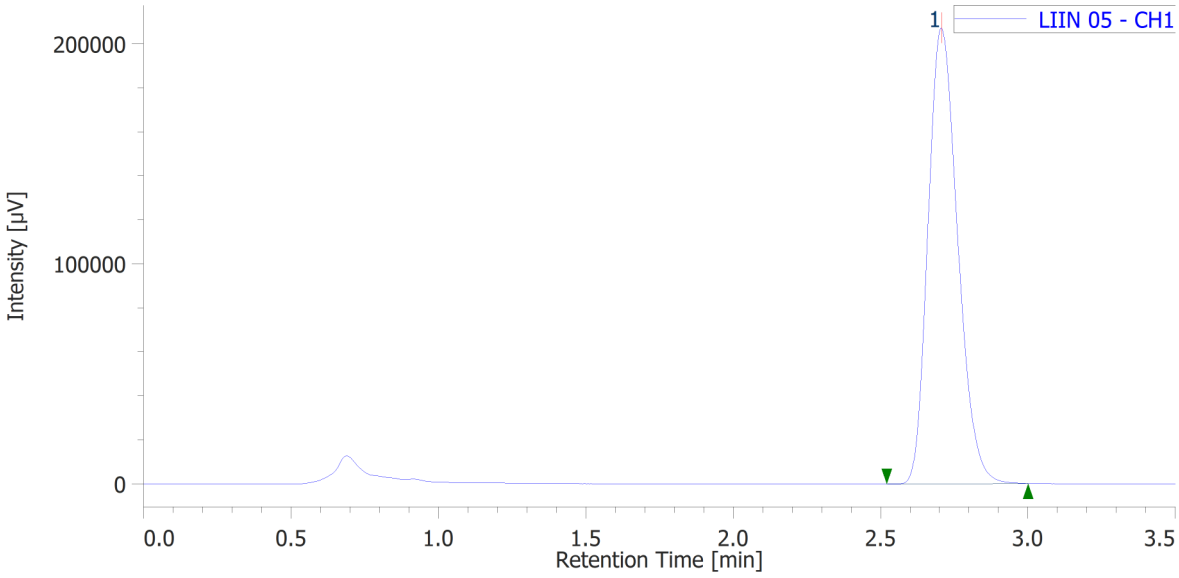

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 12:31:28
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 12:27:55
Volume	20.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.5 [min]
Acquisition Sequence	Qualificação 05
Control Method	Qualificação 05
Peak ID Table	Qualificação 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação 05

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	2.707	1449053	207074	100.000	100.000	N/A	3429	N/A	1.212	

Creator
Reviewer
Approver

Chromatogram

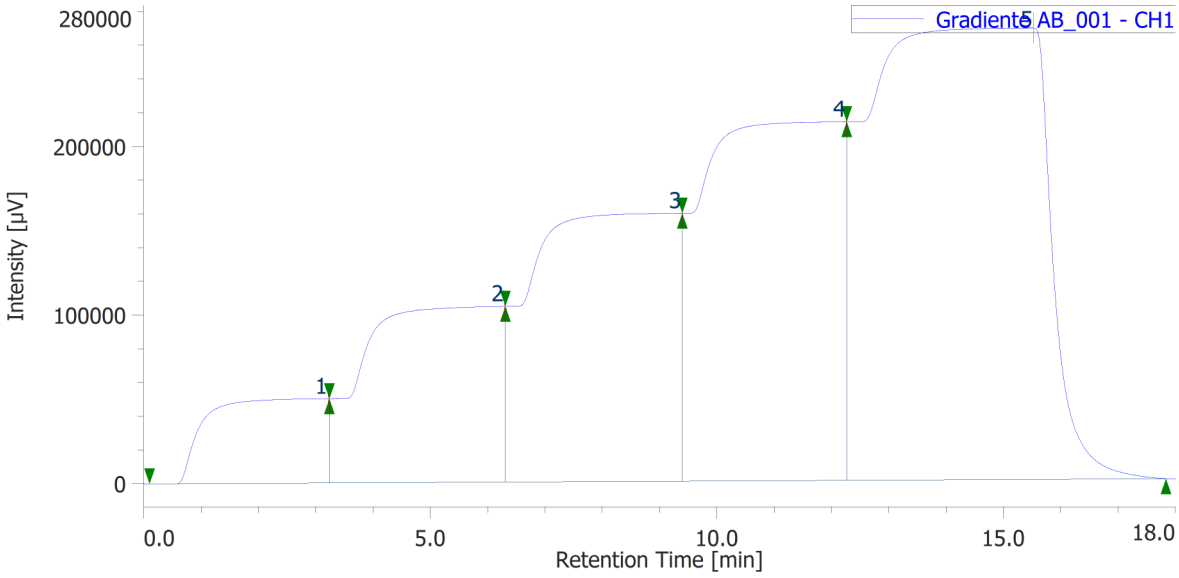

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 13:28:01
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 13:09:59
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	18.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.217	6846620	49984	4.804	6.303	N/A	N/A	N/A	N/A	
2	40%	1	6.293	16854796	104164	11.827	13.136	N/A	N/A	N/A	N/A	
3	60%	1	9.387	27329697	158774	19.178	20.022	N/A	N/A	N/A	N/A	
4	80%	1	12.250	34828174	212525	24.440	26.801	N/A	N/A	N/A	N/A	
5	100%	1	15.520	56646726	267541	39.750	33.738	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

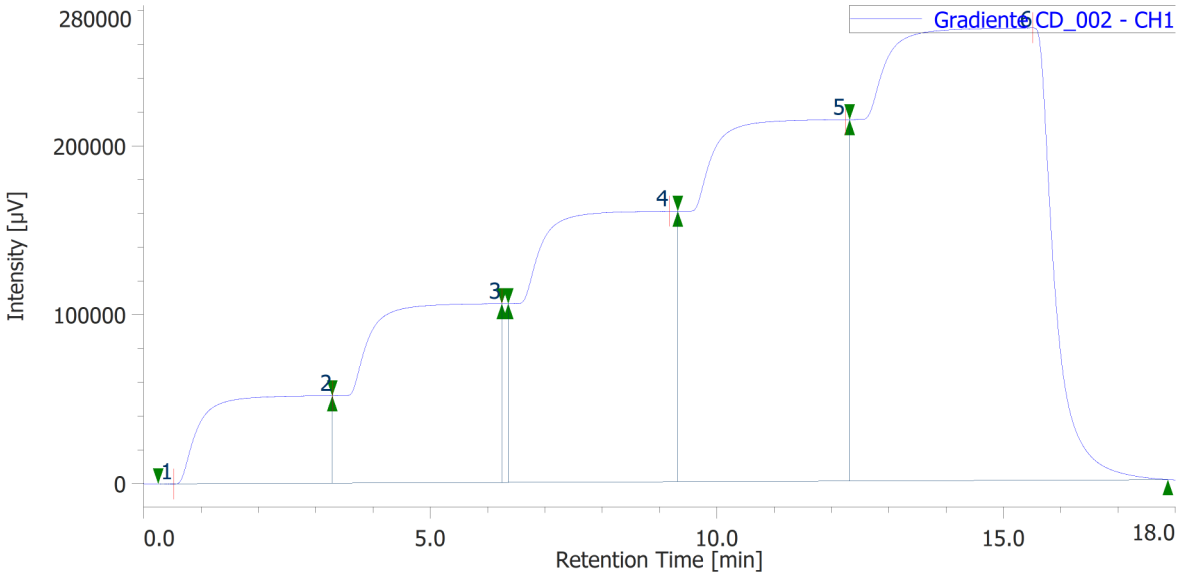

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 14:04:09
Description	
HPLC System Name	HPLC_0005
Injection Date	30/08/2023 13:46:06
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	18.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente 05
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0.520	-4386	99	N/A	0.012	N/A	47	N/A	0.602	
2	20%	1	3.297	16659782	51749	12.210	6.476	N/A	N/A	N/A	N/A	
3	40%	1	6.247	740549	105771	0.543	13.237	N/A	N/A	N/A	N/A	
4	60%	1	9.163	26477043	160064	19.404	20.032	N/A	N/A	N/A	N/A	
5	80%	1	12.247	36475015	213804	26.732	26.758	N/A	N/A	N/A	N/A	
6	100%	1	15.510	56100060	267553	41.115	33.484	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

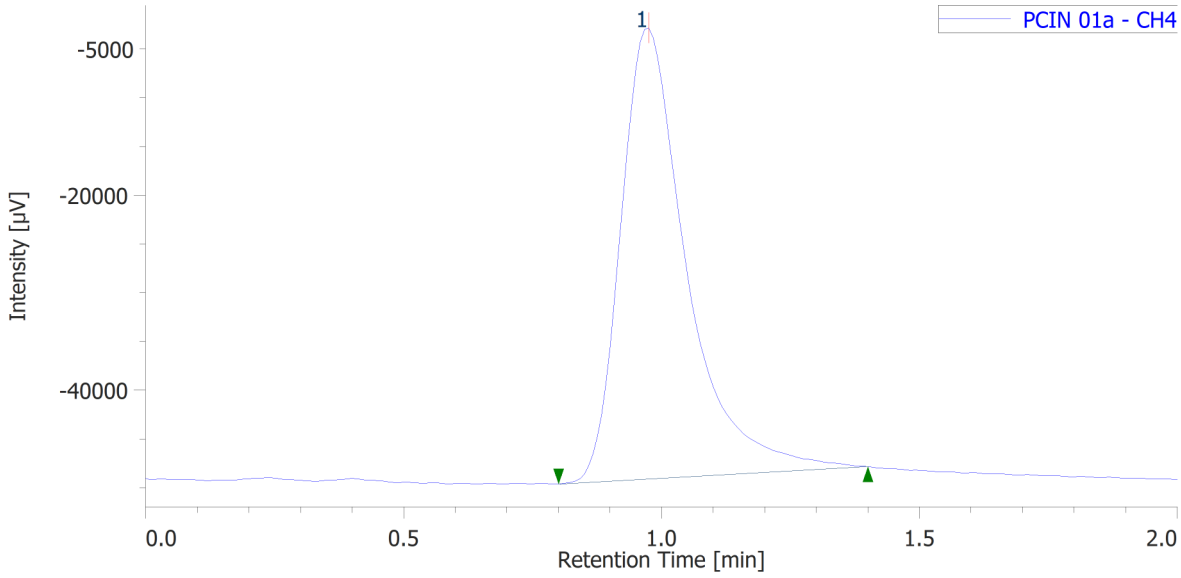

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:01:46
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 16:59:44
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.975	411627	46223	100.000	100.000	N/A	324	N/A	1.556	

Creator
Reviewer
Approver

Chromatogram

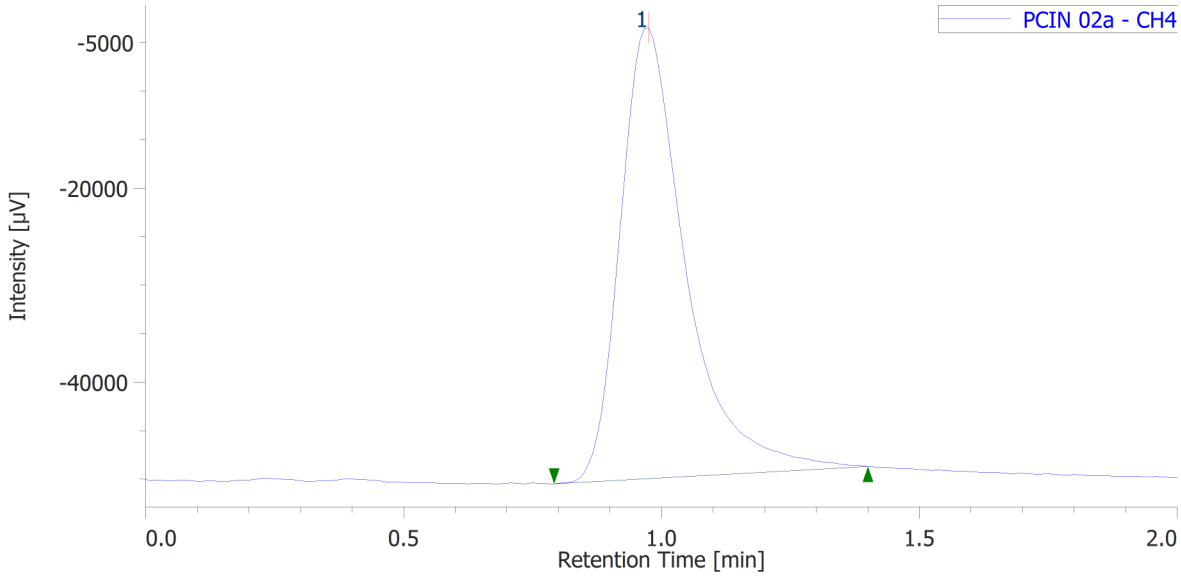

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:04:58
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:02:56
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.975	411675	46414	100.000	100.000	N/A	328	N/A	1.533	

Creator
Reviewer
Approver

Chromatogram

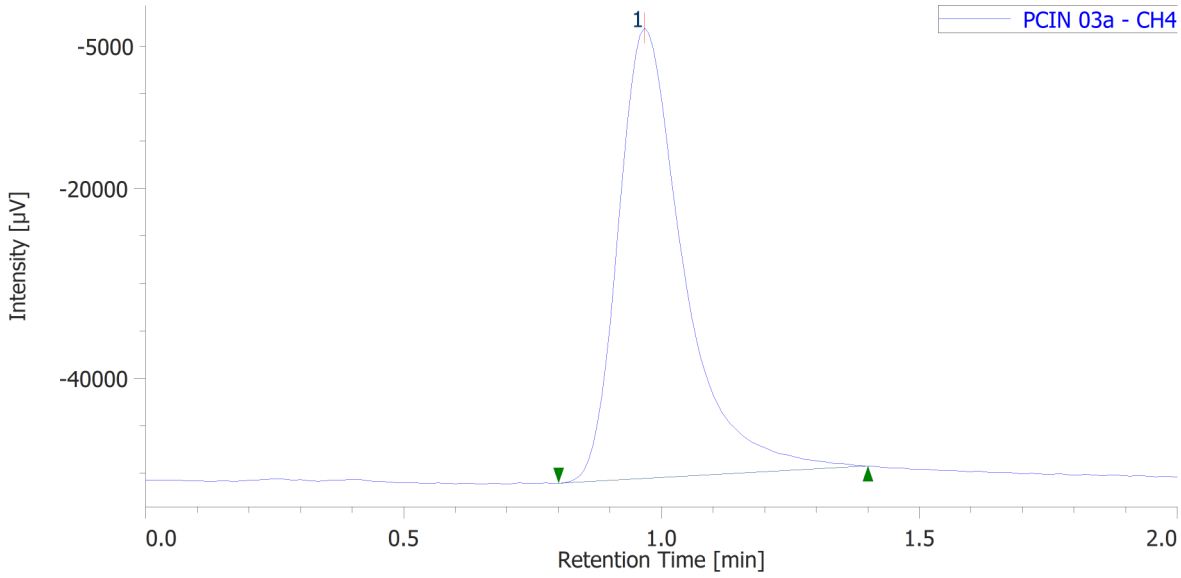

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:08:10
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:06:06
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	418181	47413	100.000	100.000	N/A	325	N/A	1.608	

Creator
Reviewer
Approver

Chromatogram

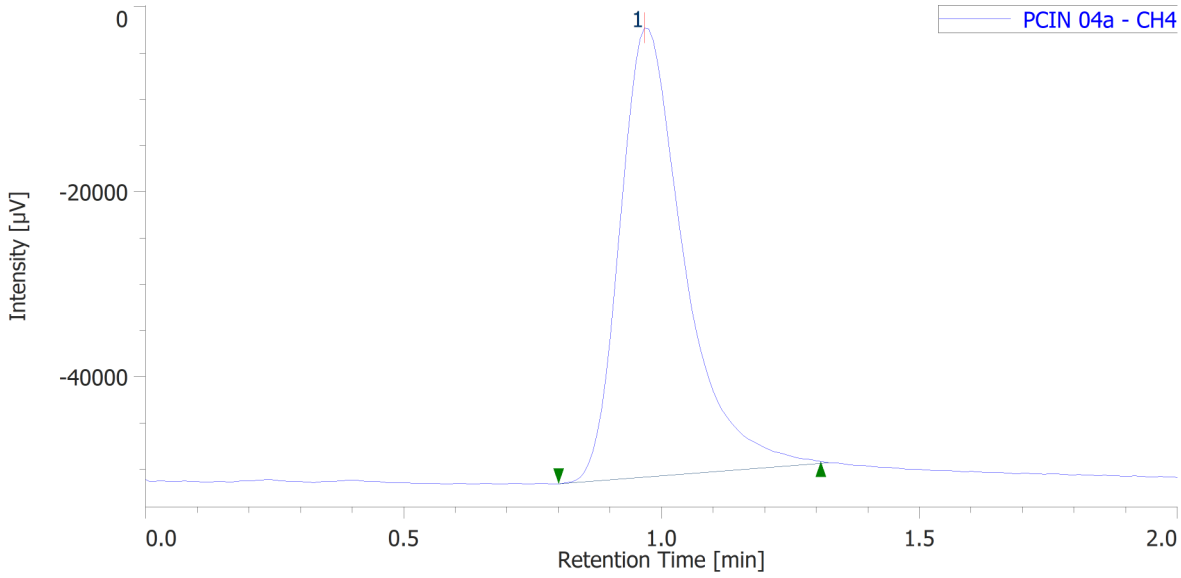

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:11:22
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:09:19
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	419703	48518	100.000	100.000	N/A	325	N/A	1.570	

Creator
Reviewer
Approver

Chromatogram

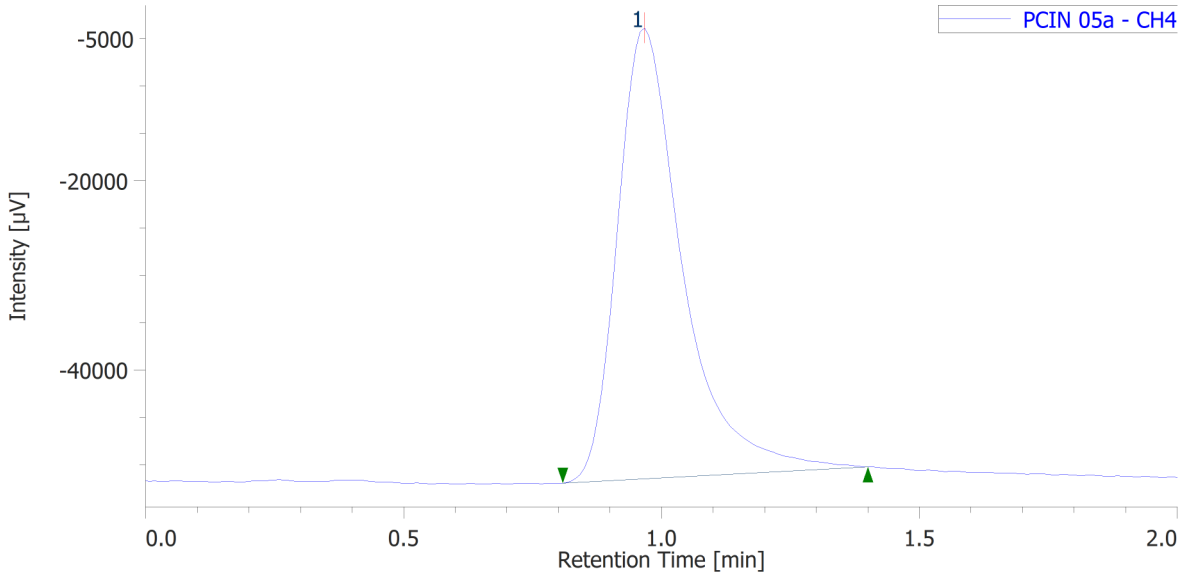

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:14:32
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:12:29
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	419098	47606	100.000	100.000	N/A	330	N/A	1.584	

Creator
Reviewer
Approver

Chromatogram

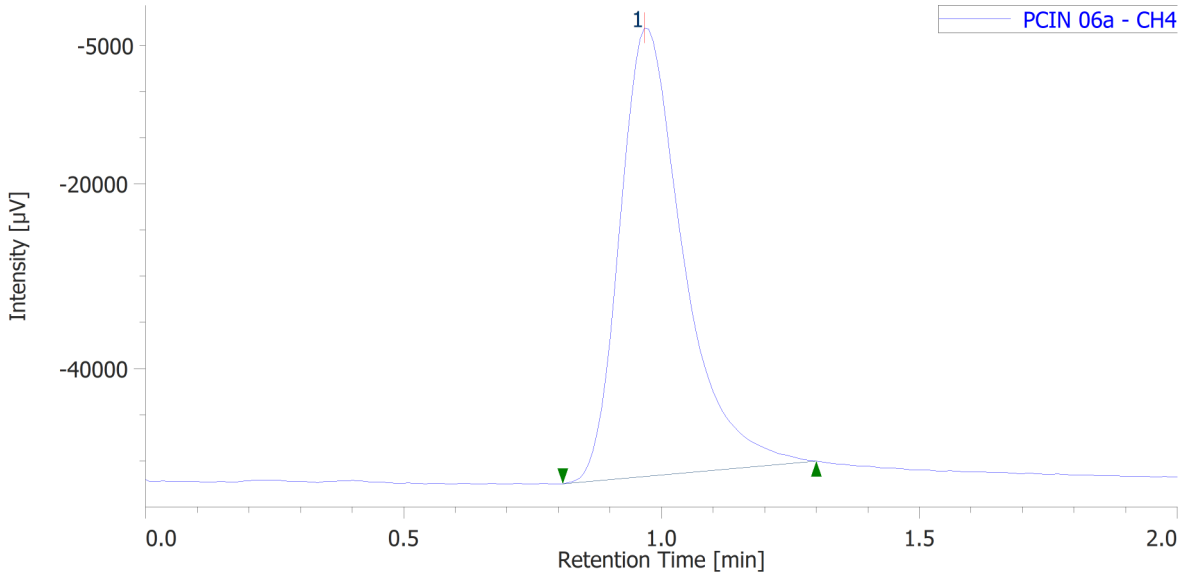

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:17:44
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:15:42
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	415397	48539	100.000	100.000	N/A	328	N/A	1.529	

Creator
Reviewer
Approver

Chromatogram

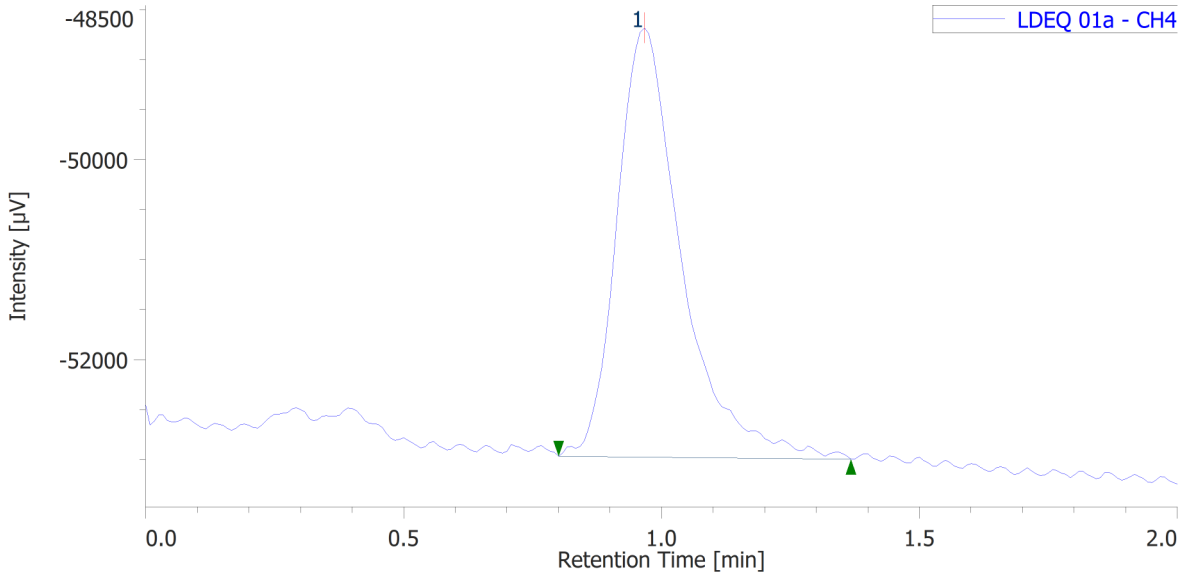

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:20:50
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:18:48
Volume	0.1 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDEQ 01a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	37444	4293	100.000	100.000	N/A	335	N/A	1.520	

Creator
Reviewer
Approver

Chromatogram

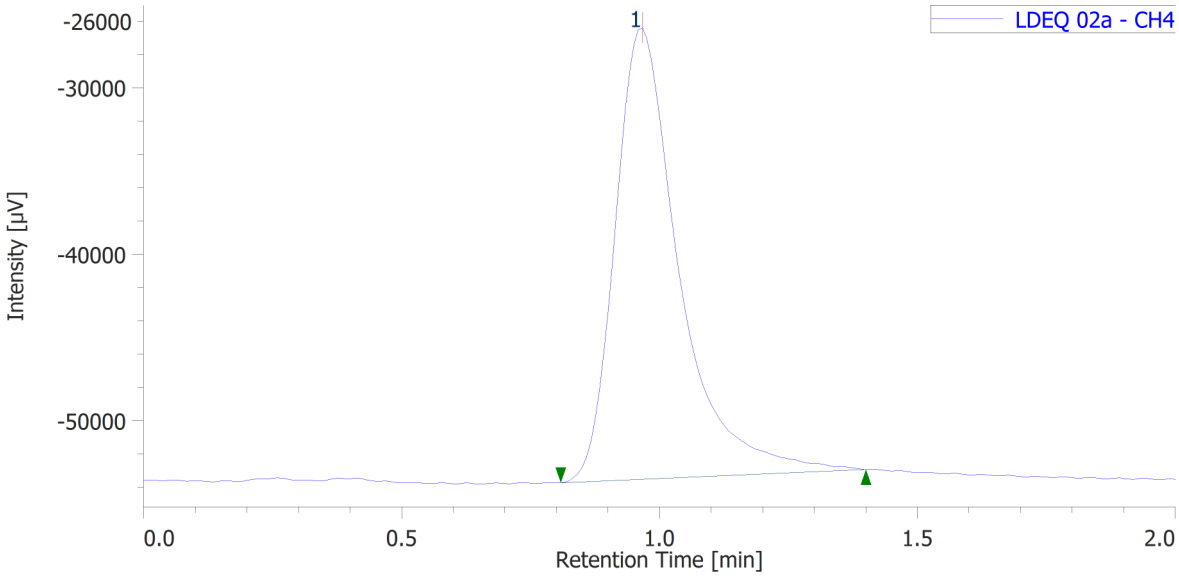

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:24:02
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:21:58
Volume	5.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDEQ 02a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	234309	27089	100.000	100.000	N/A	348	N/A	1.569	

Creator
Reviewer
Approver

Chromatogram

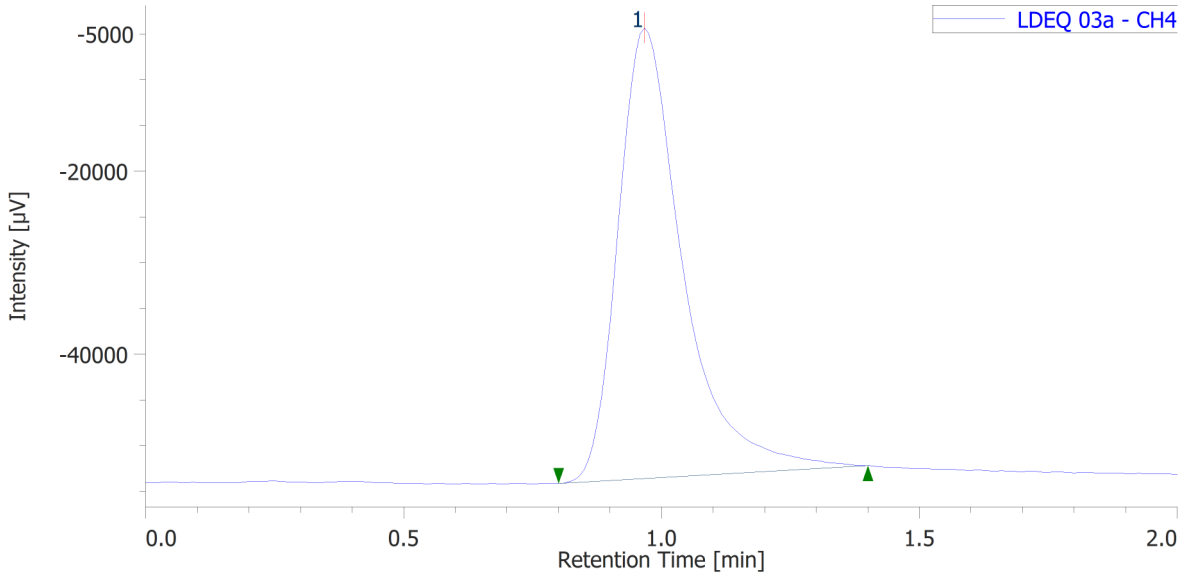

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:27:14
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:25:11
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDEQ 03a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	431483	49214	100.000	100.000	N/A	330	N/A	1.594	

Creator
Reviewer
Approver

Chromatogram

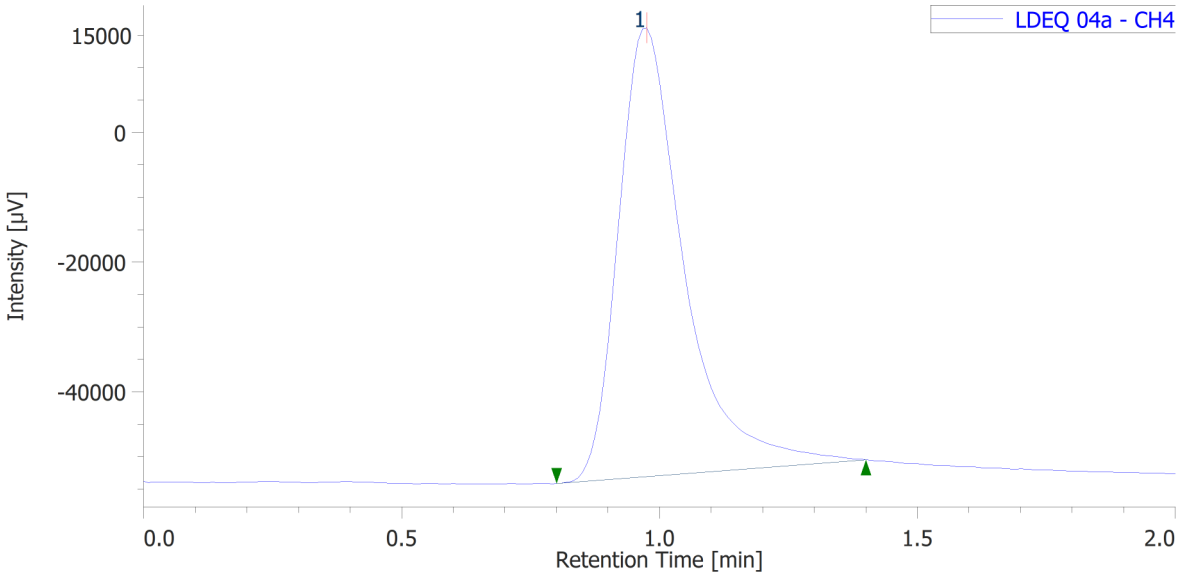

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:30:26
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:28:24
Volume	15.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDEQ 04a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.975	614733	69147	100.000	100.000	N/A	327	N/A	1.569	

Creator
Reviewer
Approver

Chromatogram

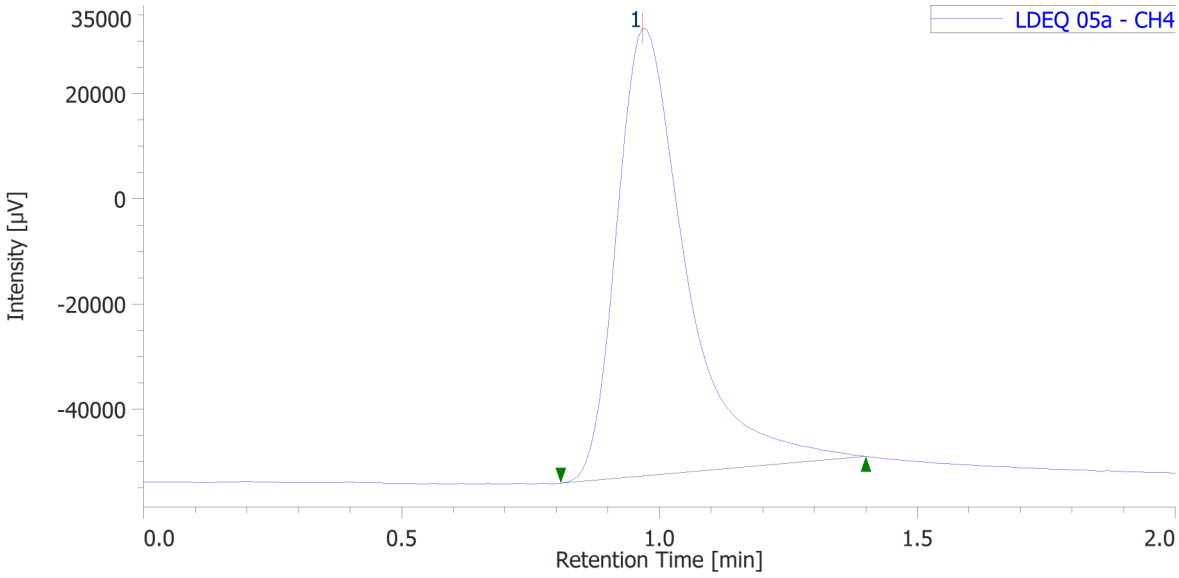

Chromatogram Information	
User Name	Administrator
Date Modified	30/08/2023 17:33:43
Description	
HPLC System Name	HPLC_0005 Iônico
Injection Date	30/08/2023 17:31:41
Volume	20.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação 05 Iônico
Control Method	Qualificação Iônico
Peak ID Table	L-Treonina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDEQ 05a-CH4
Sample Name	
Channel Name	CH4
Sampling Interval	500 [msec]
Peak Method	Qualificação Iônico

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	L-Treonina	4	0.967	793498	85174	100.000	100.000	N/A	294	N/A	1.773	

Creator
Reviewer
Approver