Single Injection Report

Agilent Technologies


Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\EDUV 001.sirslt\EDUV 001.dx		
Sample name:	EDUV 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A1
Injection date:	2025-08-27 12:09:40-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação - Spectro.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 12:17:23-03:00		

TR:

1.649

Nome do Composto:

Cafeína

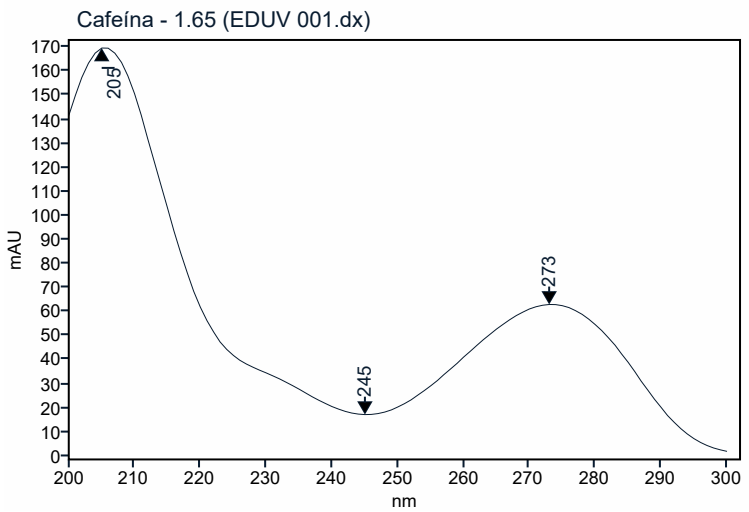


Name	RT [min]	Area	Peak Height
Cafeína	1.649	268.5460	62.645

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\RELB -001.sirslt\RELB -001.dx		
Sample name:	RELB <001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A2
Injection date:	2025-08-27 12:13:42-03:00	**Injection:**	1 of 1
Acq. method:	Sinal-Ruido.amx	**Injection volume:**	20.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 13:43:02-03:00		

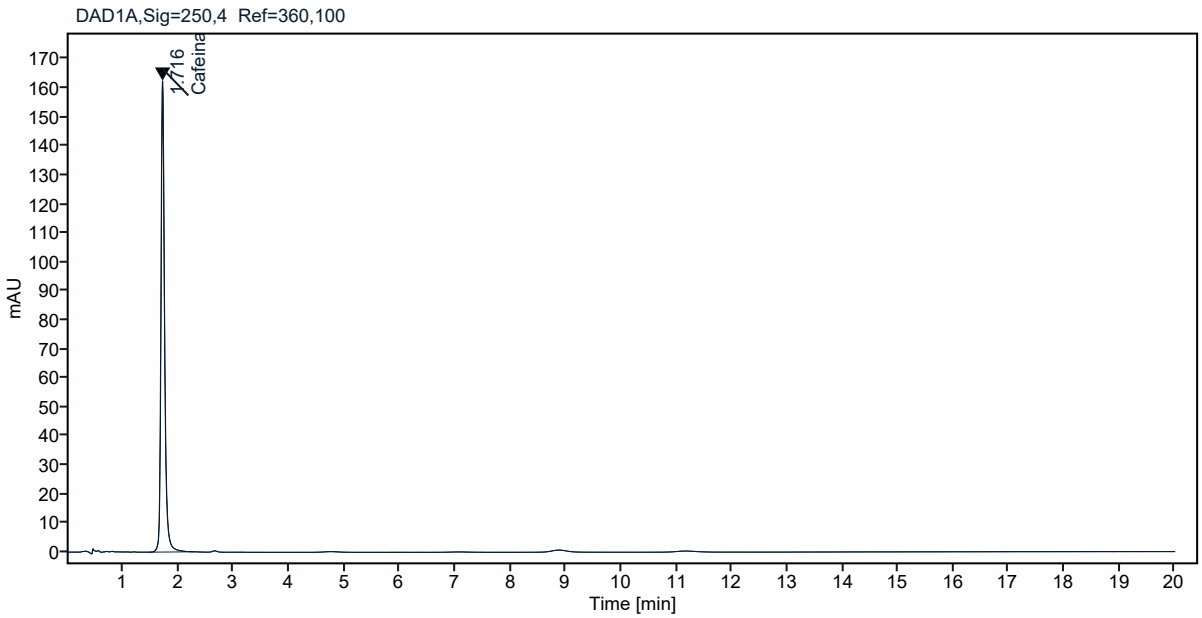


Name	RT [min]	Area	Peak Height
Cafeina	1.716	747.4751	162.641

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\RELB -001.sirslt\RELB -001.dx		
Sample name:	RELB <001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A2
Injection date:	2025-08-27 12:13:42-03:00	**Injection:**	1 of 1
Acq. method:	Sinal-Ruido.amx	**Injection volume:**	20.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 13:43:02-03:00		

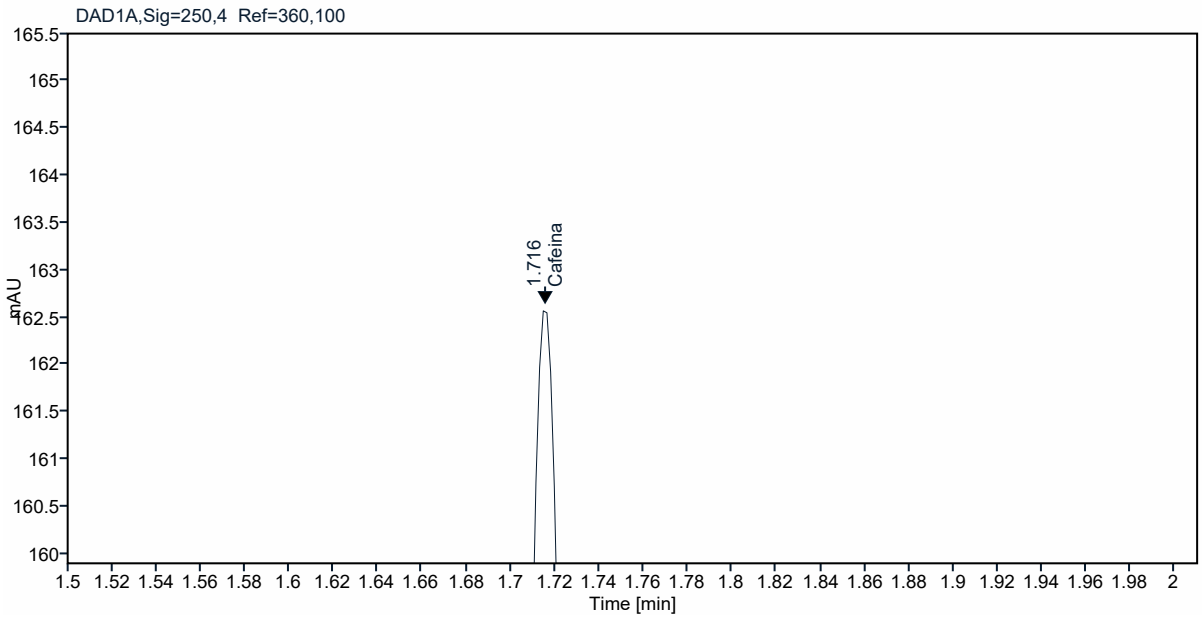


Name	RT [min]	Area	Peak Height
Cafeina	1.716	747.4751	162.641

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\RELB -001.sirslt\RELB -001.dx		
Sample name:	RELB <001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A2
Injection date:	2025-08-27 12:13:42-03:00	**Injection:**	1 of 1
Acq. method:	Sinal-Ruido.amx	**Injection volume:**	20.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 13:43:02-03:00		

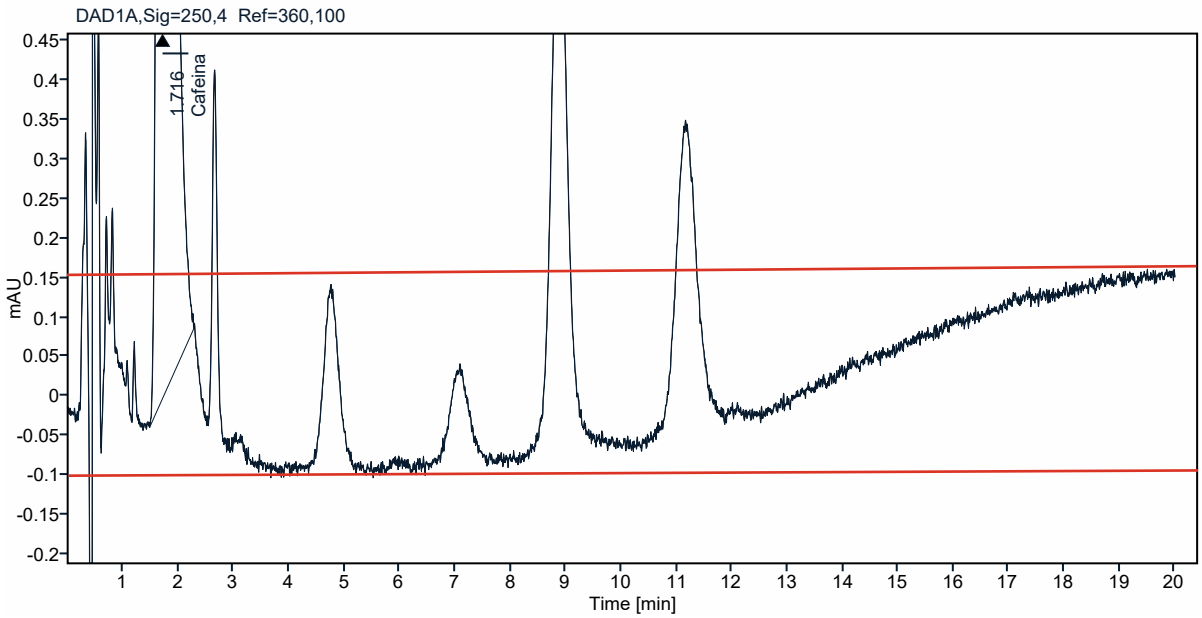


Name	RT [min]	Area	Peak Height
Cafeina	1.716	747.4751	162.641

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\RELB -001.sirslt\RELB -001.dx		
Sample name:	RELB <001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A2
Injection date:	2025-08-27 12:13:42-03:00	**Injection:**	1 of 1
Acq. method:	Sinal-Ruido.amx	**Injection volume:**	20.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 13:43:02-03:00		

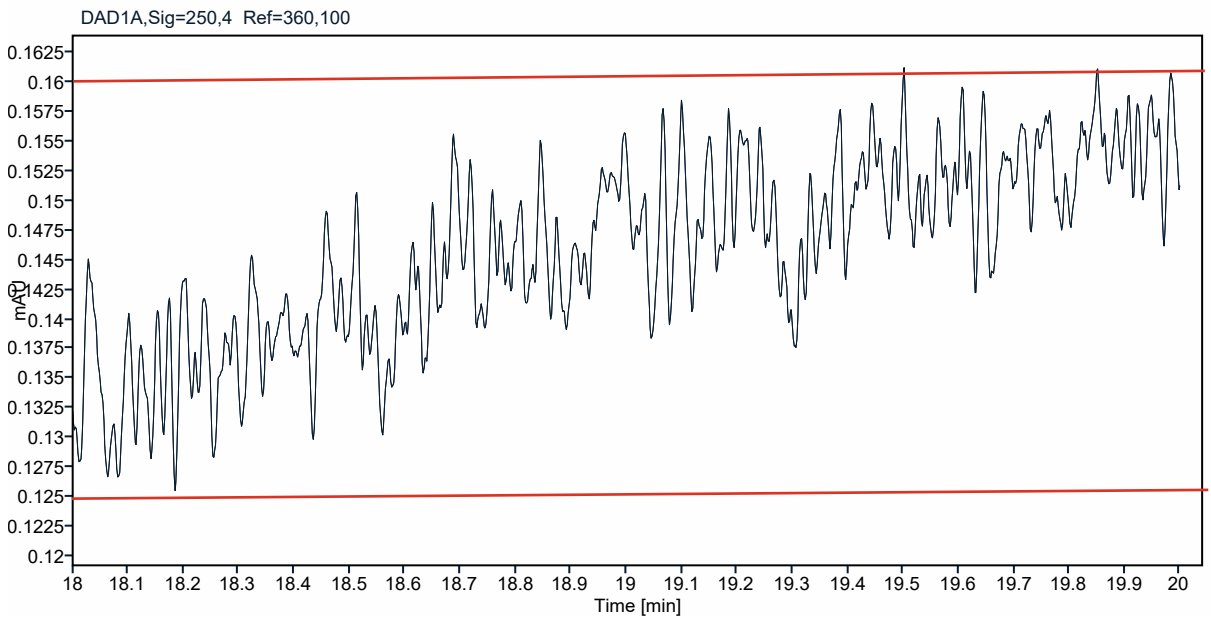


Name	RT [min]	Area	Peak Height
Cafeina	1.716	747.4751	162.641

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\Branco PCIN 01.dx		
Sample name:	Branco PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A3
Injection date:	2025-08-27 12:34:37-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

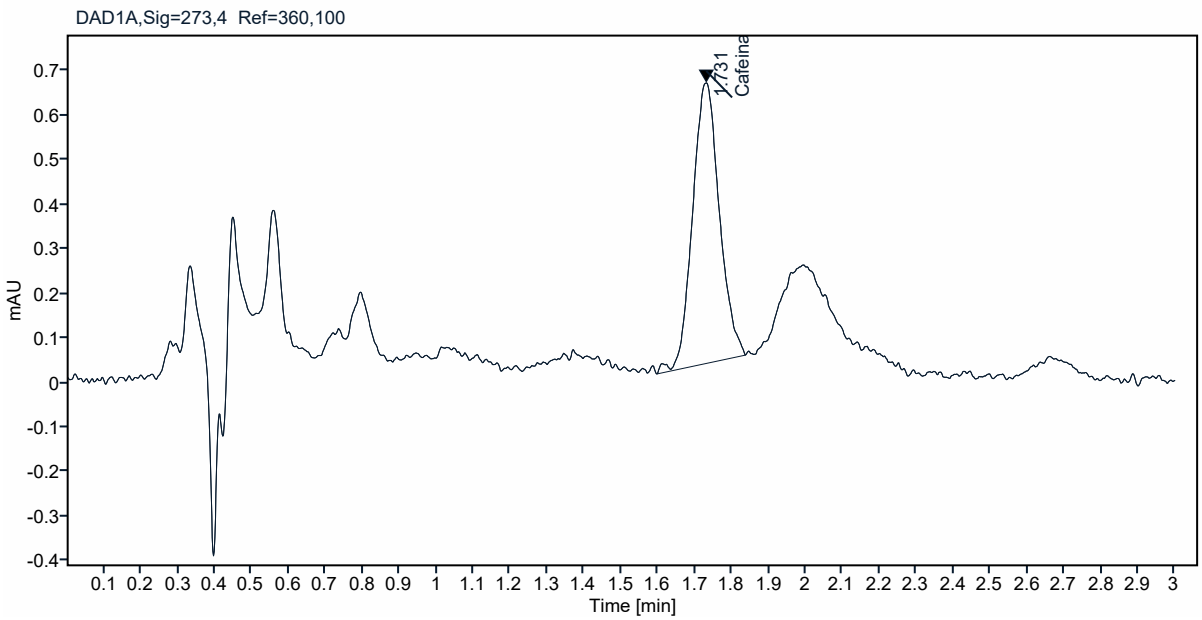


Name	RT [min]	Area	Peak Height
Cafeina	1.731	3.179	0.630

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 01.dx		
Sample name:	PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 12:38:22-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

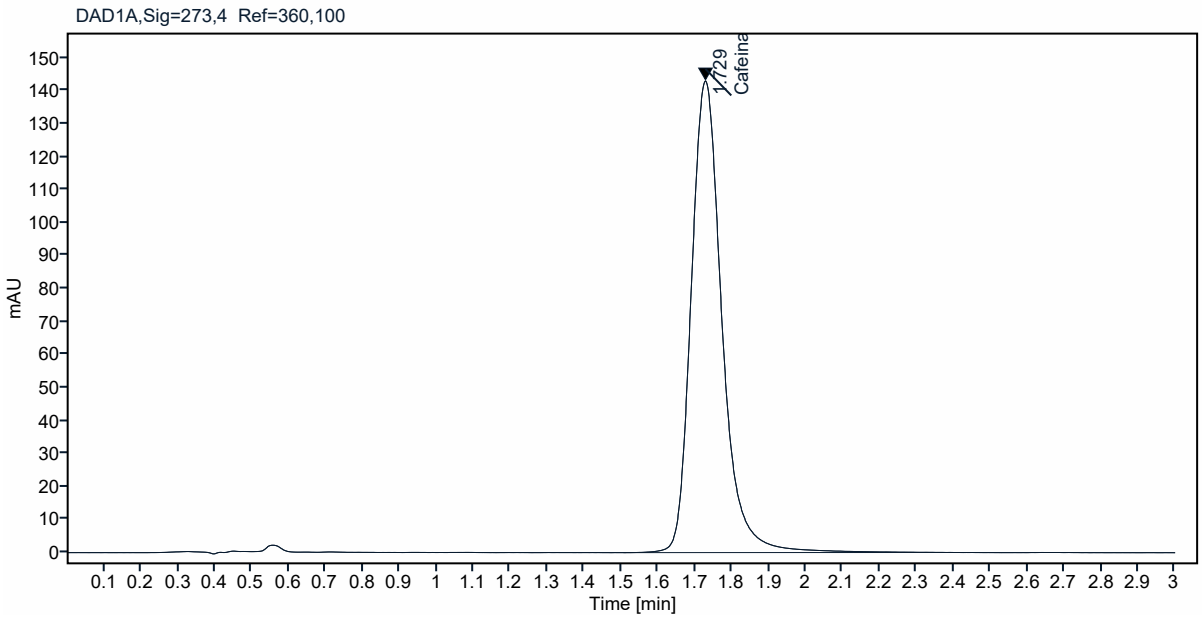


Name	RT [min]	Area	Peak Height
Cafeina	1.729	828.843	143.003

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 02.dx		
Sample name:	PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 12:42:09-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

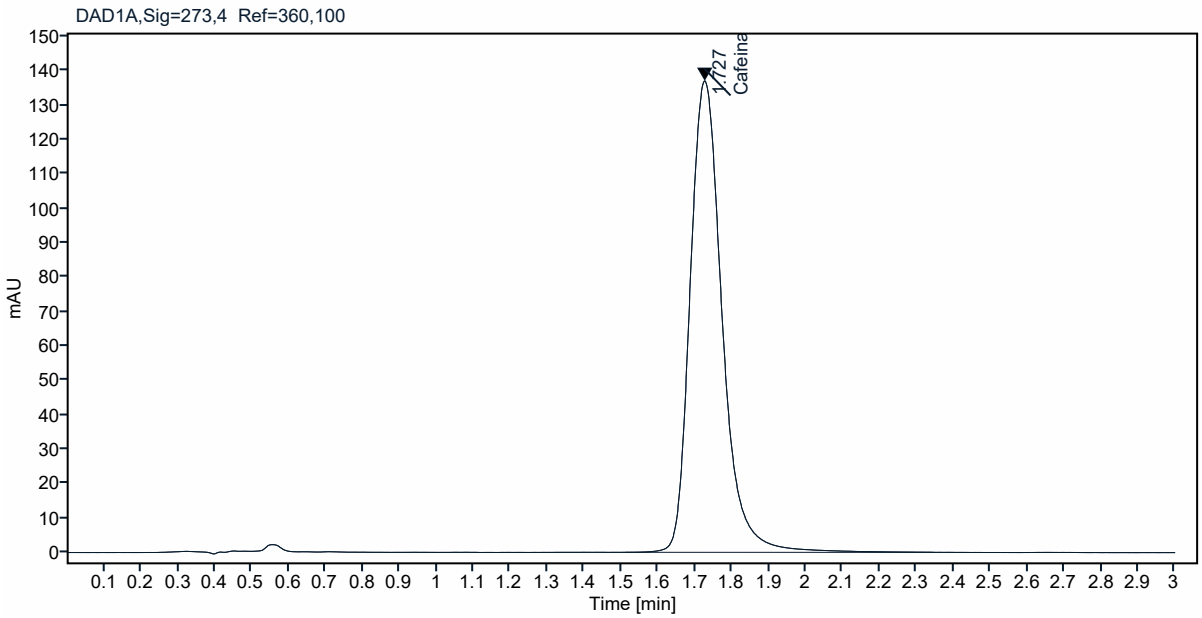


Name	RT [min]	Area	Peak Height
Cafeina	1.727	827.149	137.101

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 03.dx		
Sample name:	PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 12:45:54-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

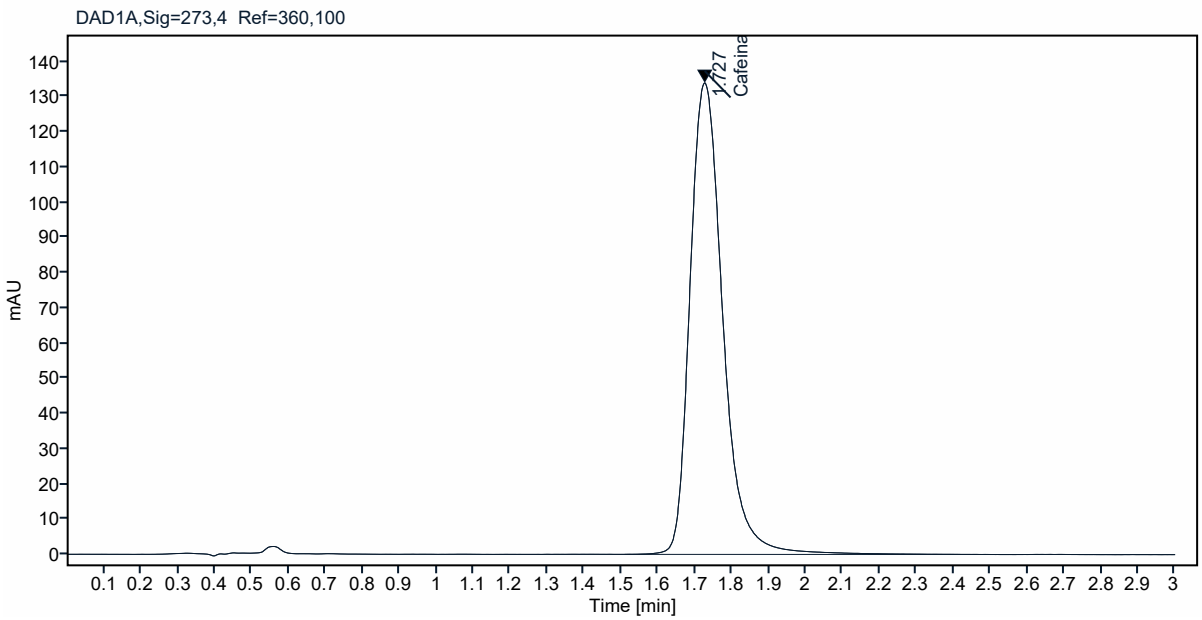


Name	RT [min]	Area	Peak Height
Cafeina	1.727	828.934	133.915

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\Branco PCIN 02.dx		
Sample name:	Branco PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A3
Injection date:	2025-08-27 12:49:41-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

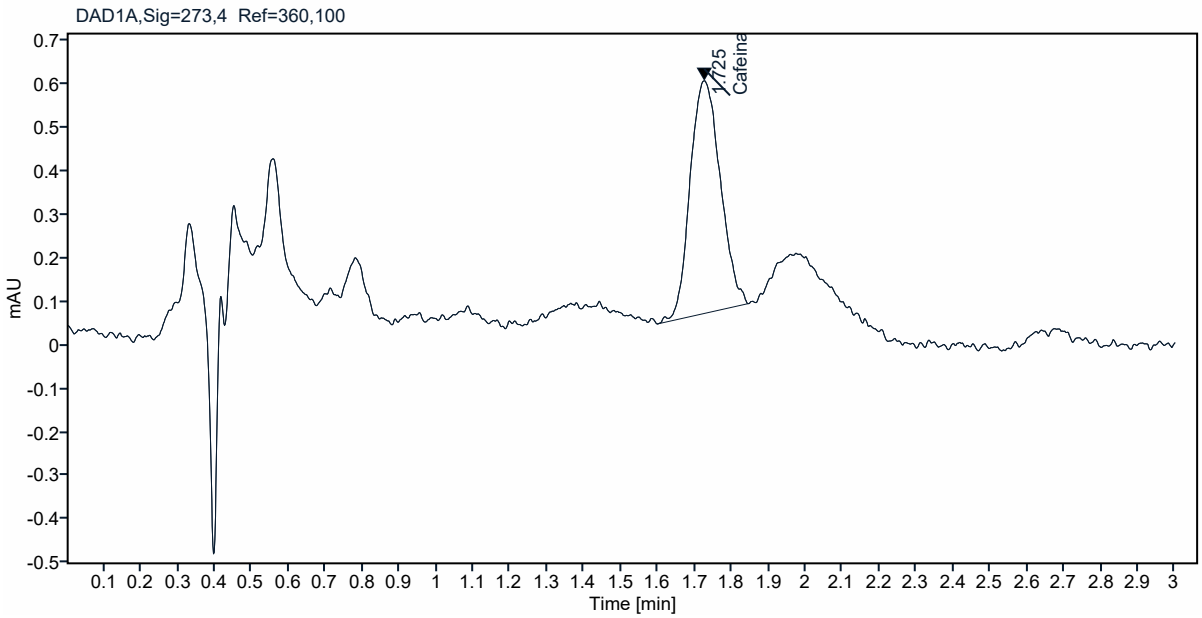


Name	RT [min]	Area	Peak Height
Cafeina	1.725	3.047	0.535

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 04.dx		
Sample name:	PCIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 12:53:27-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

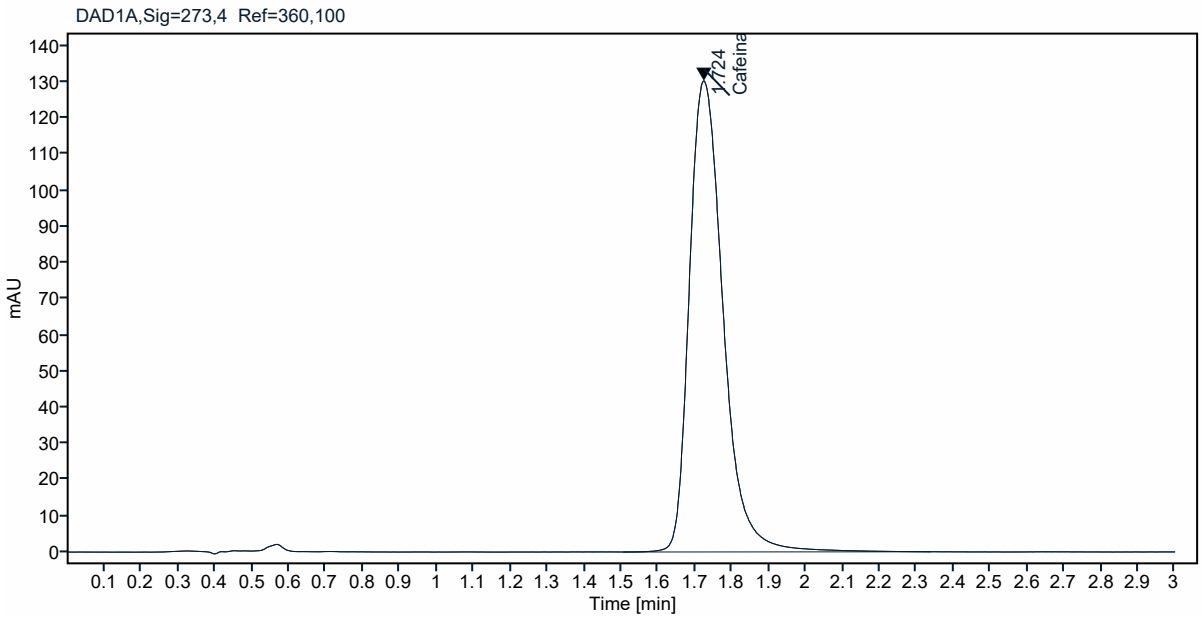


Name	RT [min]	Area	Peak Height
Cafeina	1.724	828.599	130.231

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 05.dx		
Sample name:	PCIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 12:57:13-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

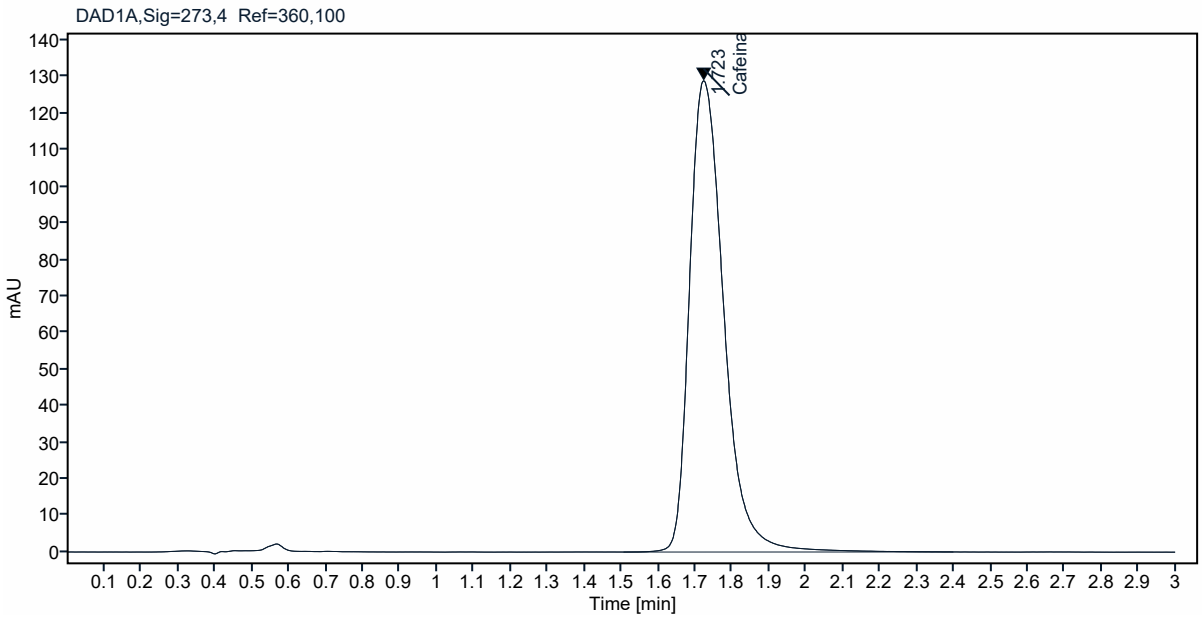


Name	RT [min]	Area	Peak Height
Cafeina	1.723	829.731	128.945

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\PCIN 06.dx		
Sample name:	PCIN 06		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A4
Injection date:	2025-08-27 13:00:58-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

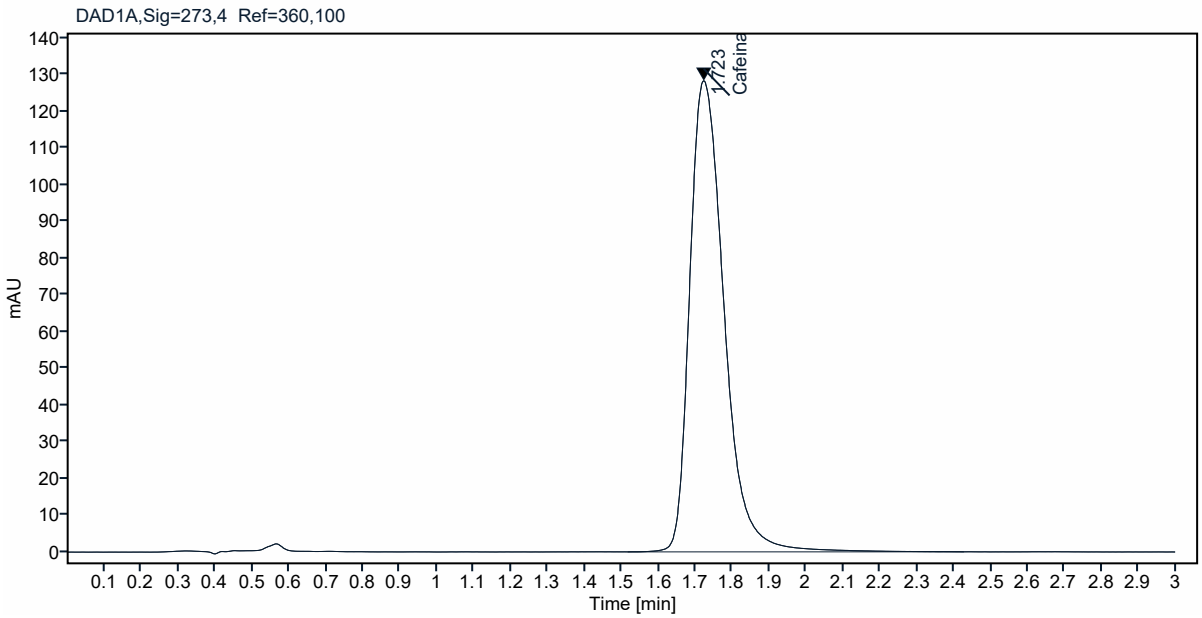


Name	RT [min]	Area	Peak Height
Cafeina	1.723	829.313	128.261

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\PCIN 001.rslt\Branco PCIN 03.dx		
Sample name:	Branco PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A3
Injection date:	2025-08-27 13:04:45-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:02:43-03:00		

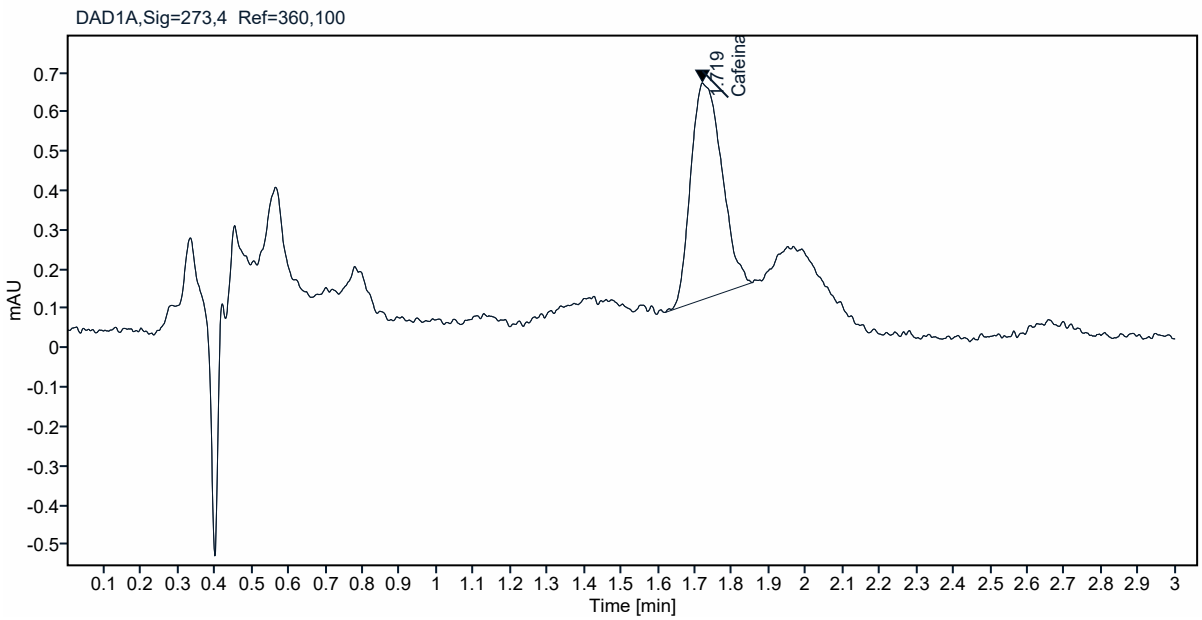


Name	RT [min]	Area	Peak Height
Cafeina	1.719	3.219	0.551

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LDUV 003.rslt\LDUV 01.dx		
Sample name:	LDUV 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A5
Injection date:	2025-08-27 14:32:47-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:54:10-03:00		

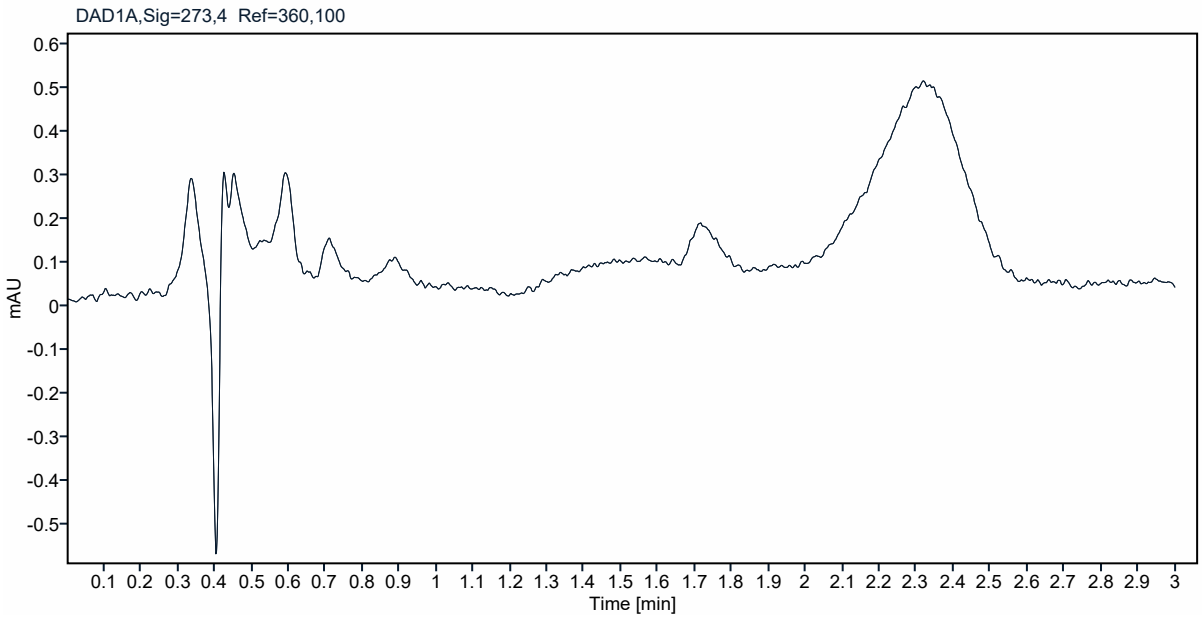


Name	RT [min]	Area	Peak Height

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LDUV 003.rslt\LDUV 02.dx		
Sample name:	LDUV 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A6
Injection date:	2025-08-27 14:36:34-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:54:10-03:00		

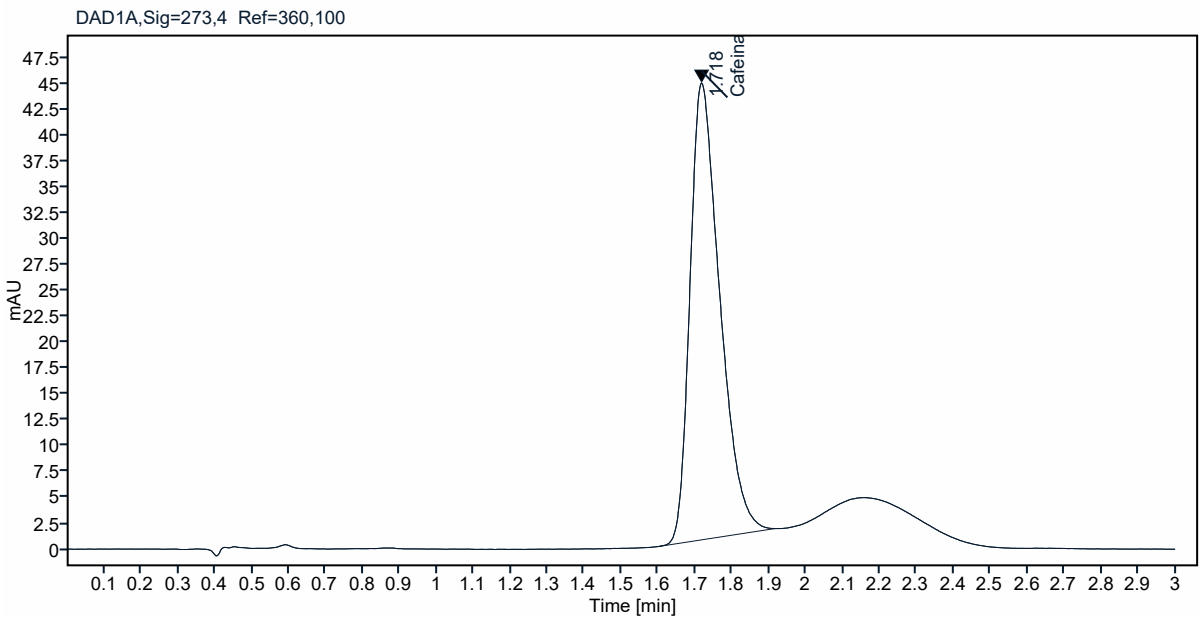


Name	RT [min]	Area	Peak Height
Cafeina	1.718	247.388	44.114

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LDUV 003.rslt\LDUV 03.dx		
Sample name:	LDUV 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A7
Injection date:	2025-08-27 14:40:18-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:54:10-03:00		

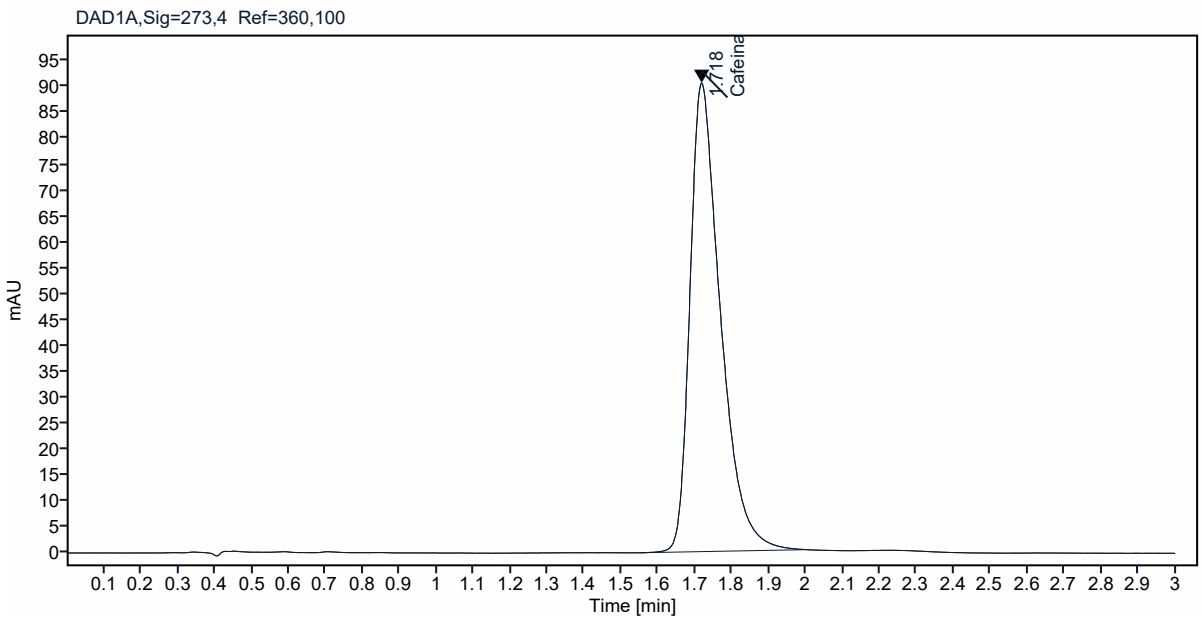


Name	RT [min]	Area	Peak Height
Cafeina	1.718	519.667	90.477

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LDUV 003.rslt\LDUV 04.dx		
Sample name:	LDUV 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A8
Injection date:	2025-08-27 14:44:04-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:54:10-03:00		

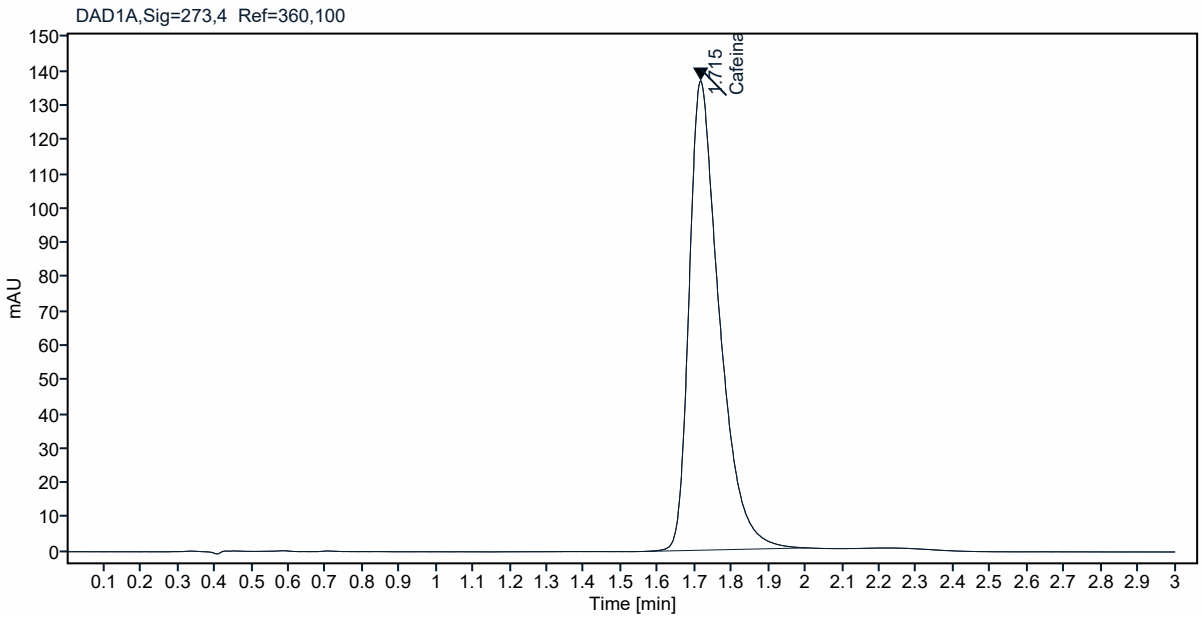


Name	RT [min]	Area	Peak Height
Cafeina	1.715	778.509	136.913

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LDUV 003.rslt\LDUV 05.dx		
Sample name:	LDUV 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A9
Injection date:	2025-08-27 14:47:49-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	*Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:54:10-03:00		

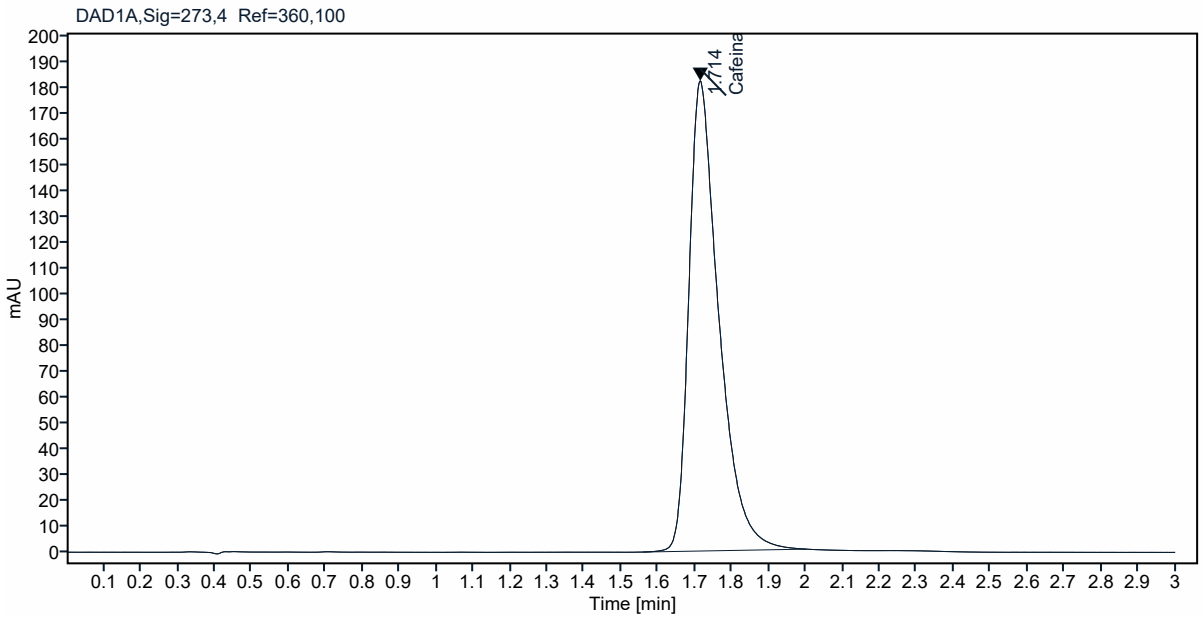


Name	RT [min]	Area	Peak Height
Cafeina	1.714	1029.749	182.308

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LIIN 003.rslt\LIIN 01.dx		
Sample name:	LIIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A10
Injection date:	2025-08-27 14:51:41-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	0.100
Analysis method:	Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:11:23-03:00		

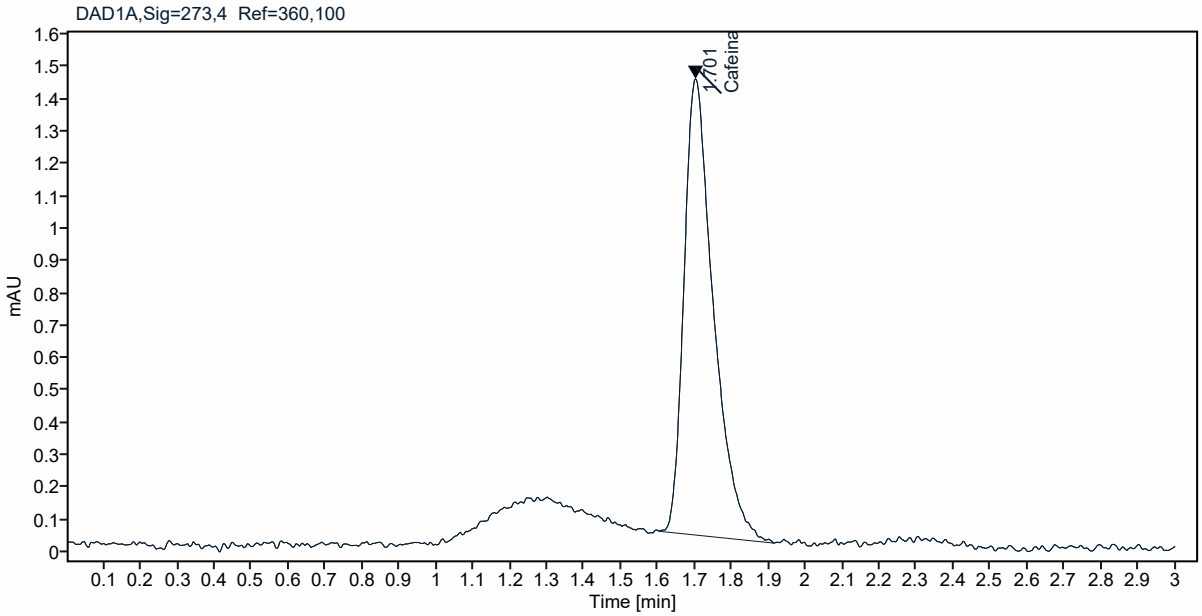


Name	RT [min]	Area	Peak Height
Cafeina	1.701	7.823	1.411

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LIIN 003.rslt\LIIN 02.dx		
Sample name:	LIIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A10
Injection date:	2025-08-27 14:55:23-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	5.000
Analysis method:	Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:11:23-03:00		

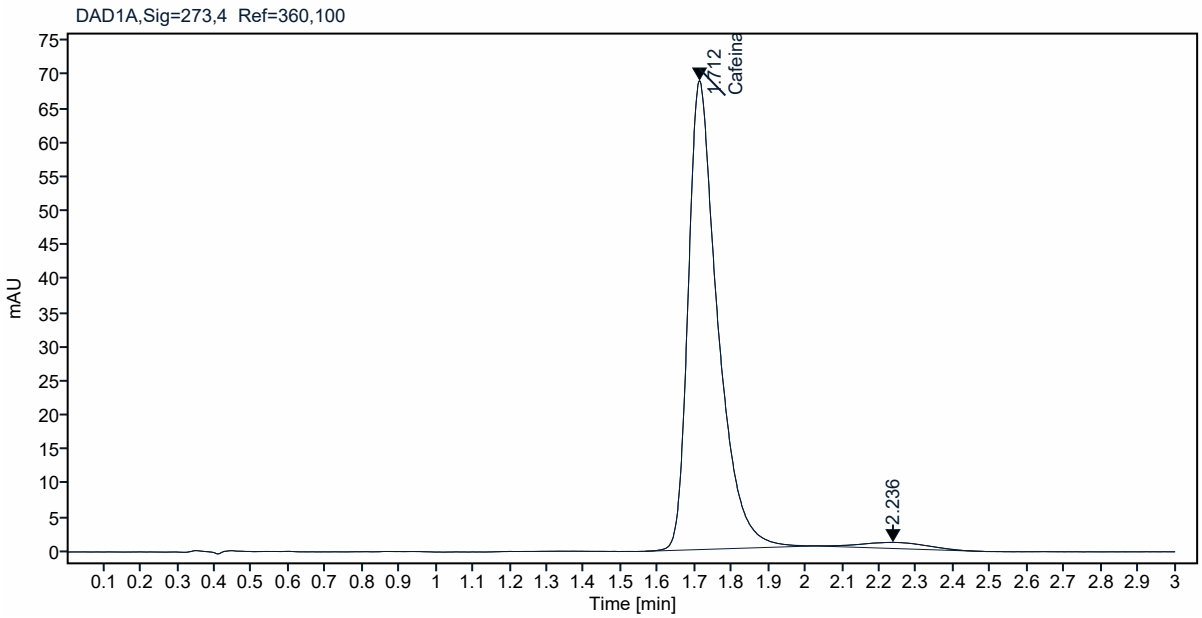


Name	RT [min]	Area	Peak Height
Cafeina	1.712	381.255	68.777

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LIIN 003.rslt\LIIN 03.dx		
Sample name:	LIIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A10
Injection date:	2025-08-27 14:59:09-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000
Analysis method:	Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:11:23-03:00		

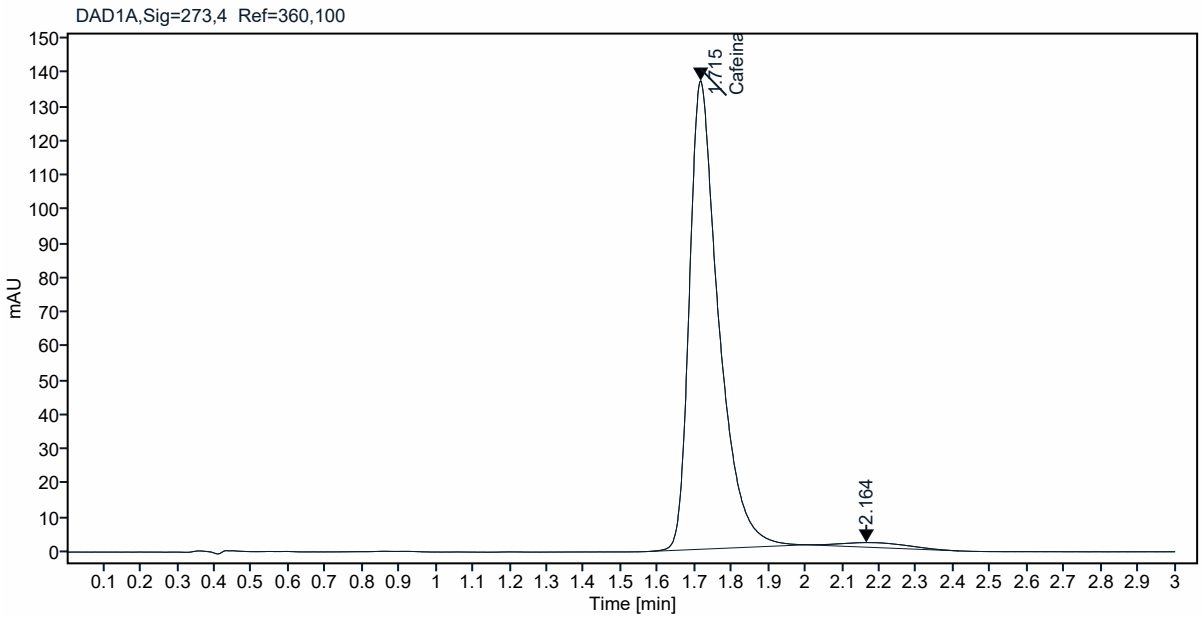


Name	RT [min]	Area	Peak Height
Cafeina	1.715	754.478	136.858

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LIIN 003.rslt\LIIN 04.dx		
Sample name:	LIIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A10
Injection date:	2025-08-27 15:02:57-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	15.000
Analysis method:	Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:11:23-03:00		

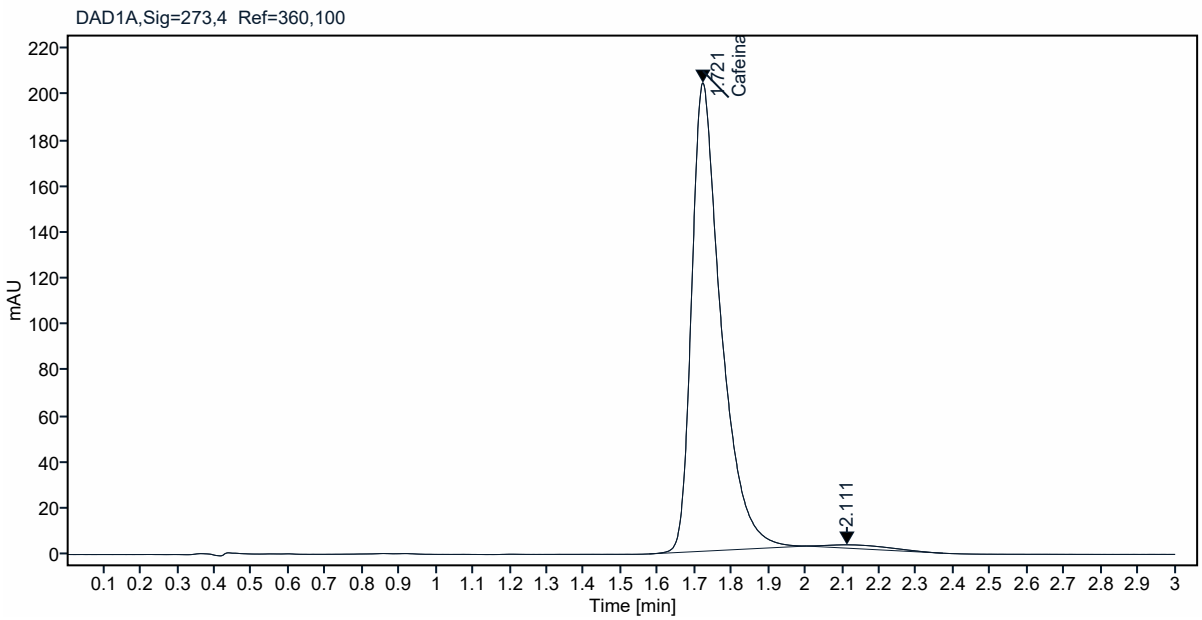


Name	RT [min]	Area	Peak Height
Cafeina	1.721	1129.611	203.763

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\LIIN 003.rslt\LIIN 05.dx		
Sample name:	LIIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	P1-A10
Injection date:	2025-08-27 15:06:49-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	20.000
Analysis method:	Qualificação.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 14:11:23-03:00		

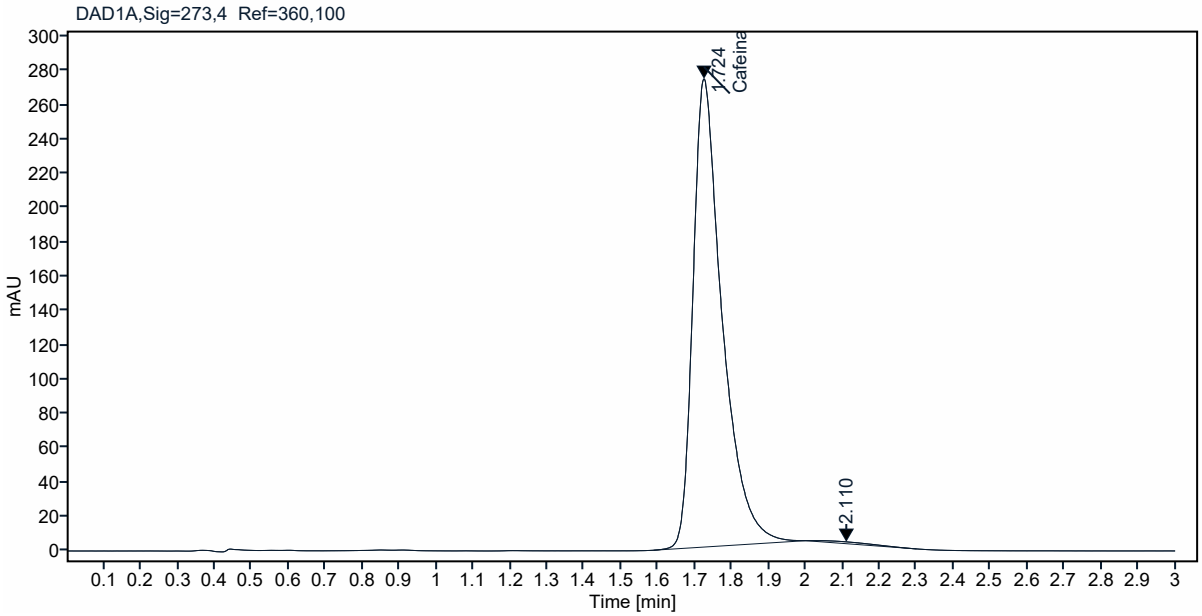


Name	RT [min]	Area	Peak Height
Cafeina	1.724	1504.392	272.995

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\GRAD AB 002.sirslt\GRAD AB 002.dx		
Sample name:	GRAD AB 002		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	
Injection date:	2025-08-27 16:06:15-03:00	**Injection:**	1 of 1
Acq. method:	Grad AB.amx	**Injection volume:**	0.000
Analysis method:	*Grad AB.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 16:32:16-03:00		

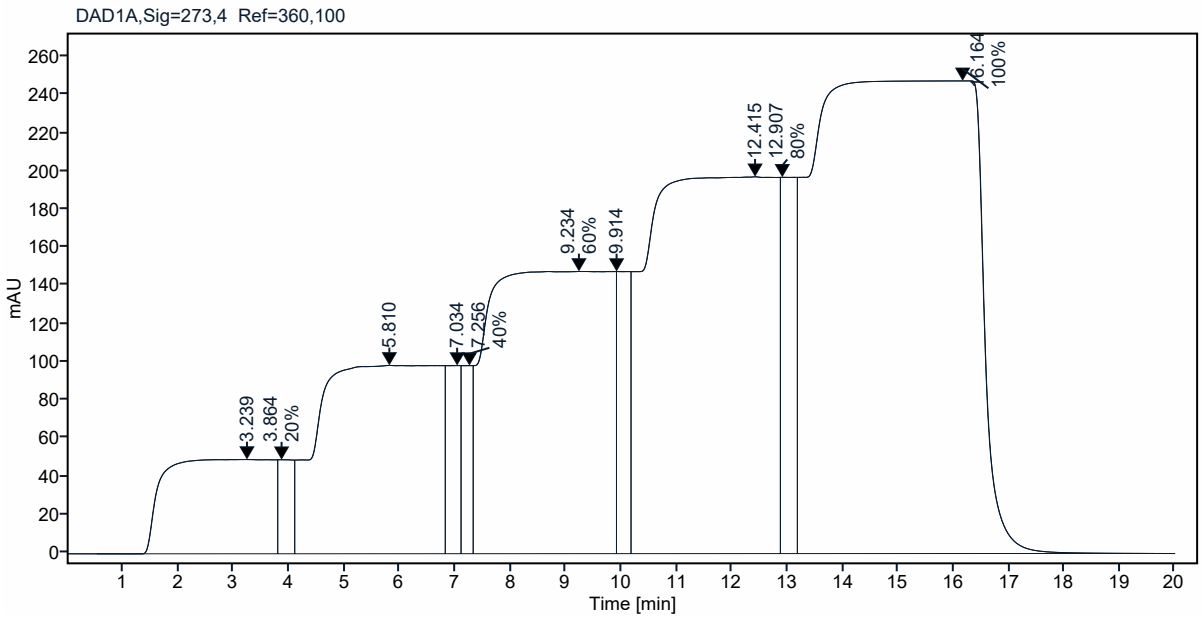


Name	RT [min]	Area	Peak Height
20%	3.864	906.813	49.292
40%	7.256	1297.076	98.607
60%	9.234	22151.789	147.946
80%	12.907	3633.341	197.283
100%	16.164	49589.994	247.808

Single Injection Report

Agilent Technologies

Data file:	C:\CDSProjects\Qualificação\Results\2025\CL-LABMAR-003\GRAD CD 001.sirslt\GRAD CD 001.dx		
Sample name:	GRAD CD 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CL-LABMAR-003	**Location:**	
Injection date:	2025-08-27 16:26:24-03:00	**Injection:**	1 of 1
Acq. method:	Grad CD.amx	**Injection volume:**	0.000
Analysis method:	*Grad AB.pmx	**Acq. operator:**	QPackSA
Last changed:	2025-08-27 16:52:03-03:00		

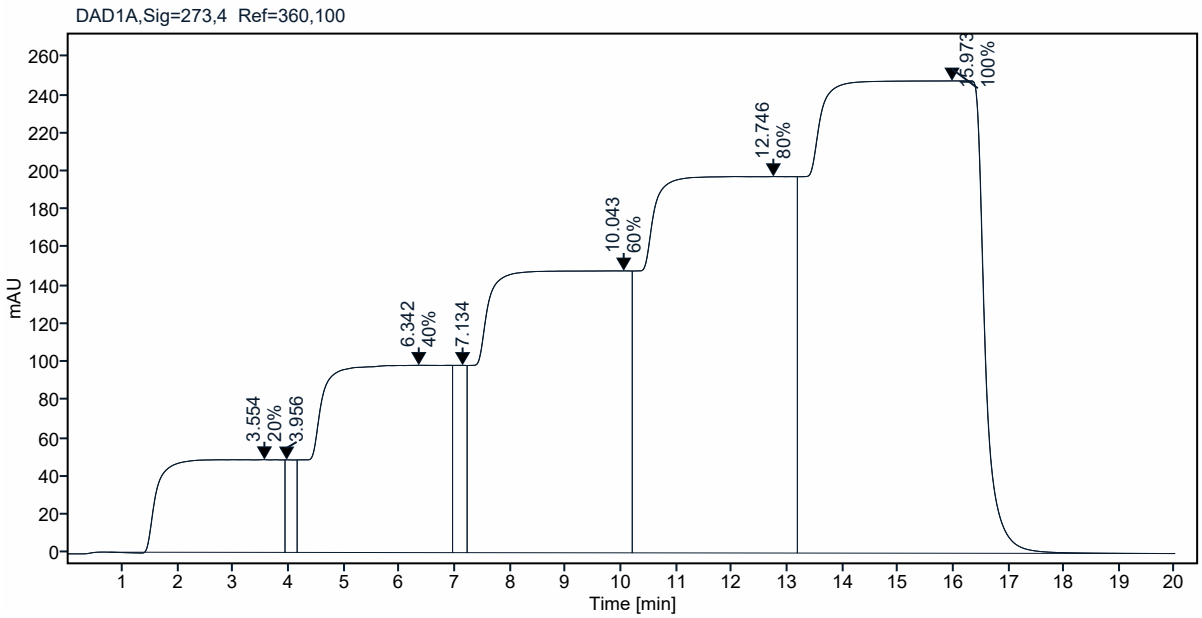

Name	RT [min]	Area	Peak Height
20%	3.554	6765.373	48.652
40%	6.342	15166.265	98.254
60%	10.043	25310.158	147.903
80%	12.746	34134.846	197.479
100%	15.973	49508.631	247.780