

Teste EDUV


Injection Details

Injection Name:	**EDUV**	*Run Time (min):*	**5,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 15:53**	*Sample Weight:*	**1,0000**

Chromatogram

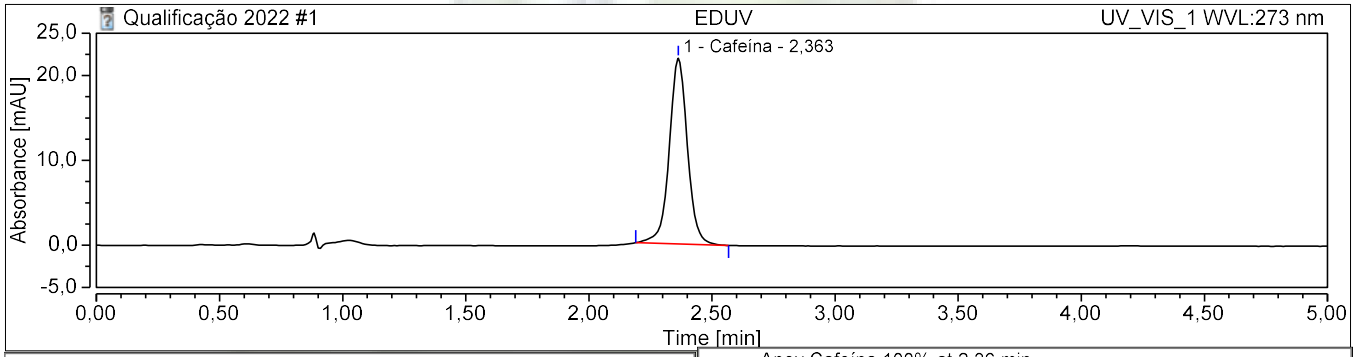

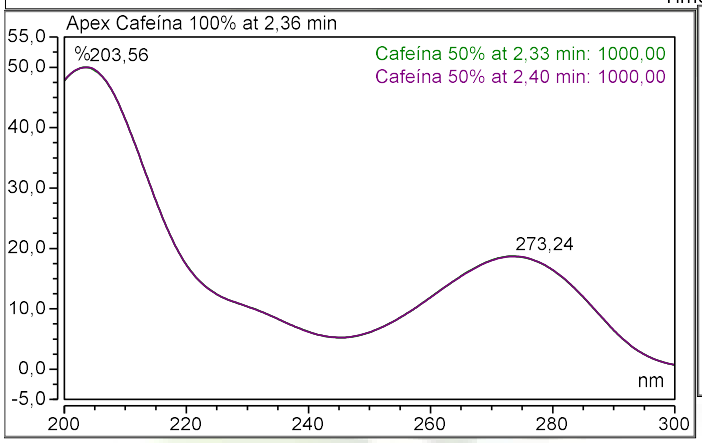

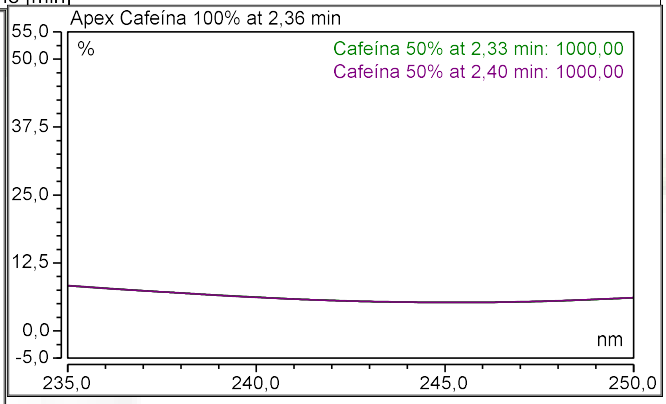

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,363	1,871	21,898	100,00	100,00	n.a.

Teste PCIN

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:00**	*Sample Weight:*	**1,0000**

Chromatogram

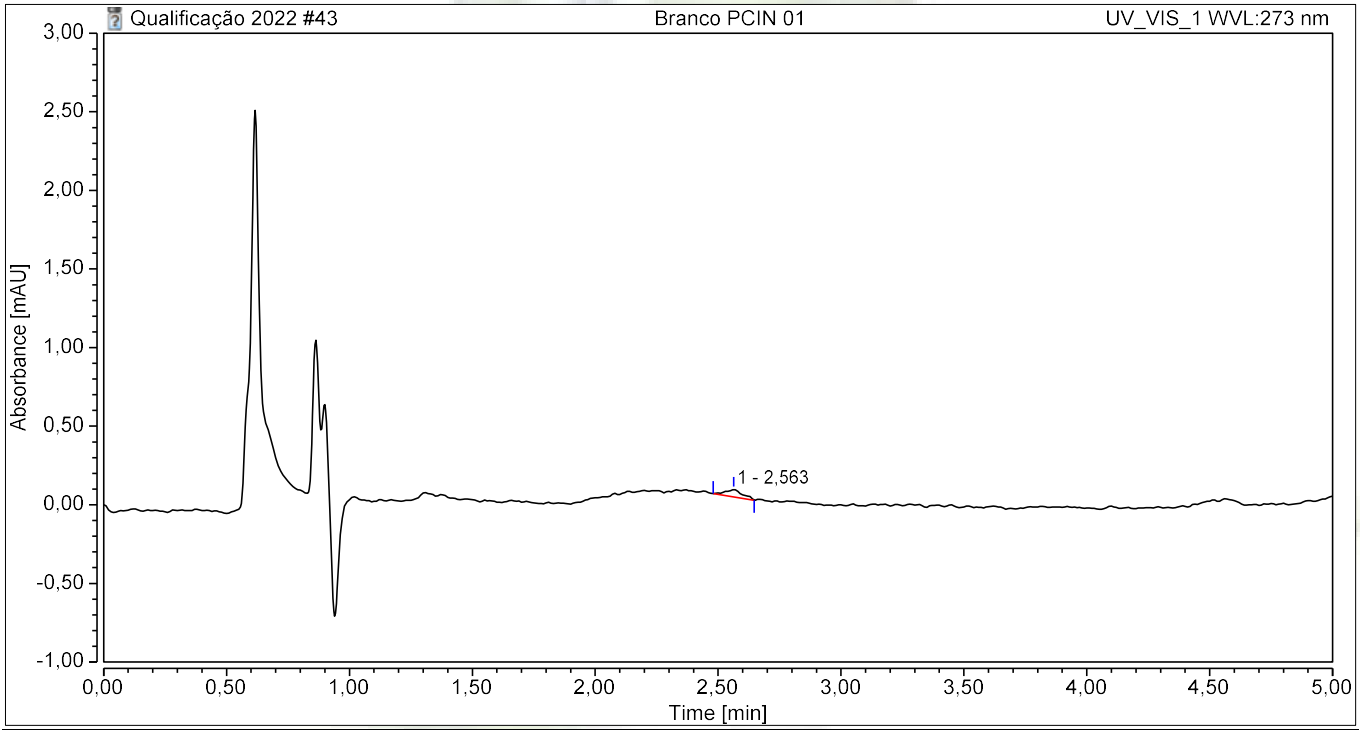

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,563	0,004	0,047	100,00	100,00	n.a.
Total:			**0,004**	**0,047**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste PCIN

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:05**	*Sample Weight:*	**1,0000**

Chromatogram

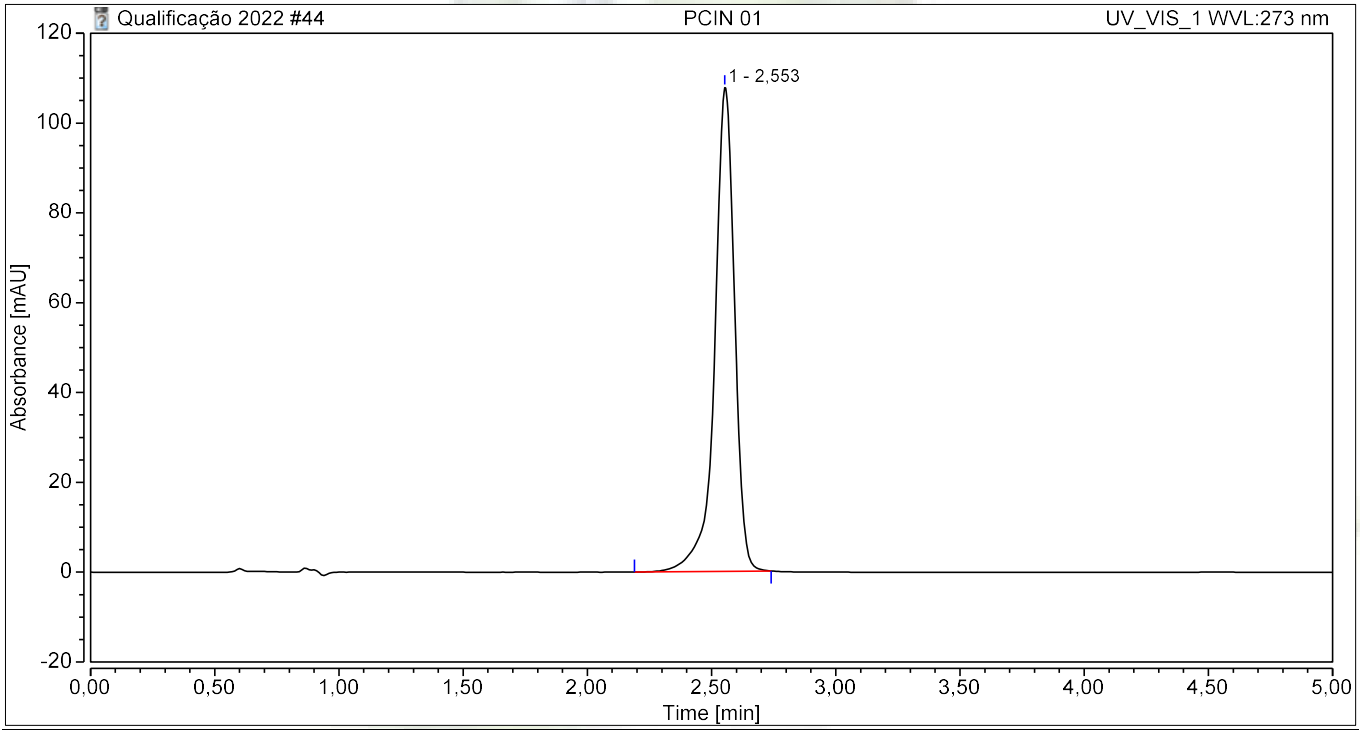

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a. 1	Cafeína	n.a. 2,553	n.a. 9,973	n.a. 107,696	n.a. 100,00	n.a. 100,00	n.a. n.a.
Total:			**9,973**	**107,696**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste PCIN

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:11**	*Sample Weight:*	**1,0000**

Chromatogram

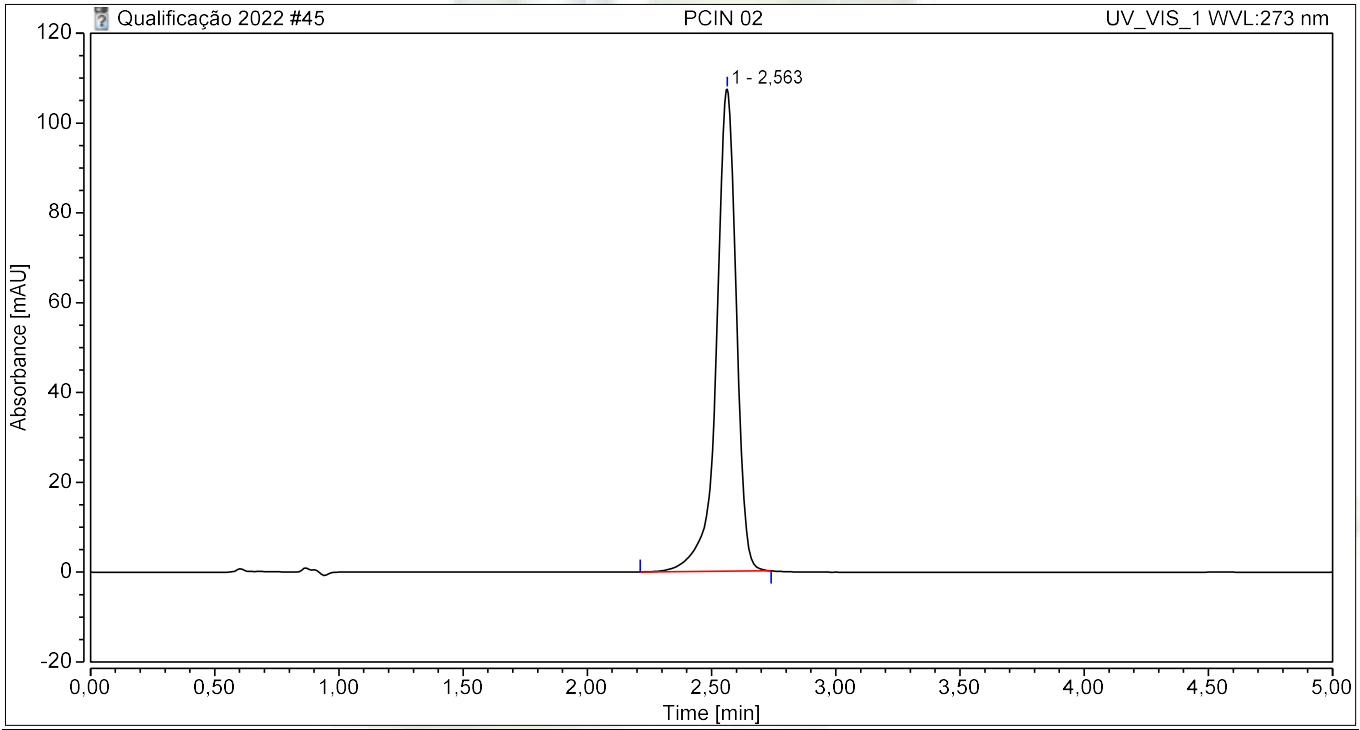

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a. 1	Cafeína	n.a. 2,563	n.a. 9,946	n.a. 107,292	n.a. 100,00	n.a. 100,00	n.a. n.a.
Total:			**9,946**	**107,292**	**100,00**	**100,00**	

Teste PCIN

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:17**	*Sample Weight:*	**1,0000**

Chromatogram

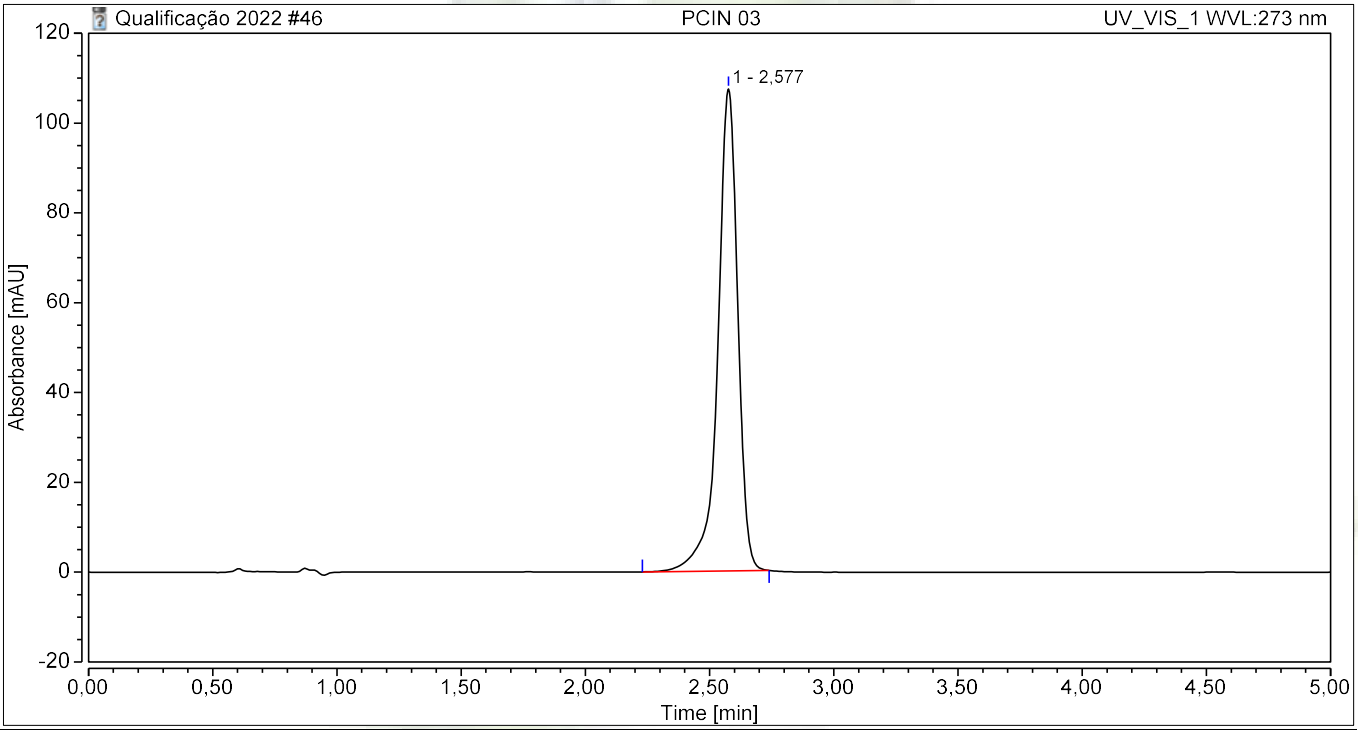

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,577	9,964	107,319	100,00	100,00	n.a.
Total:			**9,964**	**107,319**	**100,00**	**100,00**	

Teste PCIN

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:23**	*Sample Weight:*	**1,0000**

Chromatogram

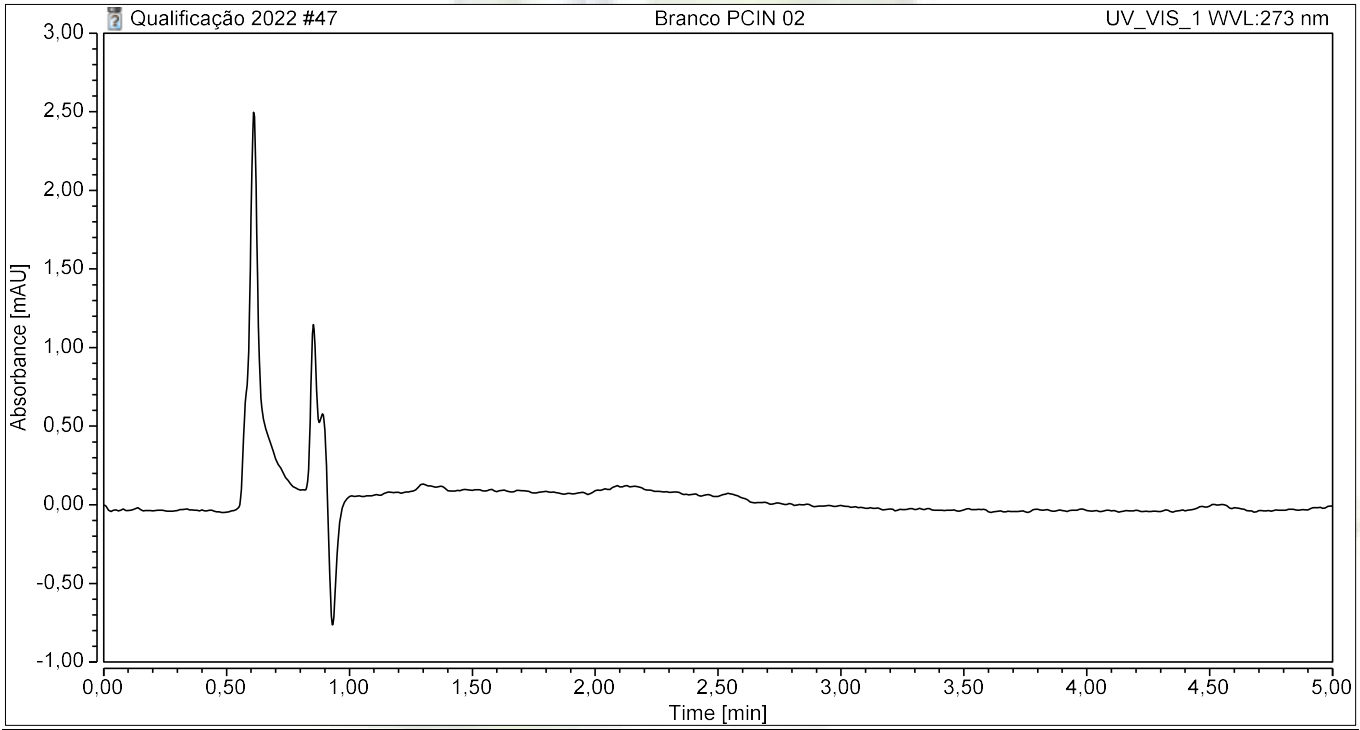

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	

Teste PCIN

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:29**	*Sample Weight:*	**1,0000**

Chromatogram

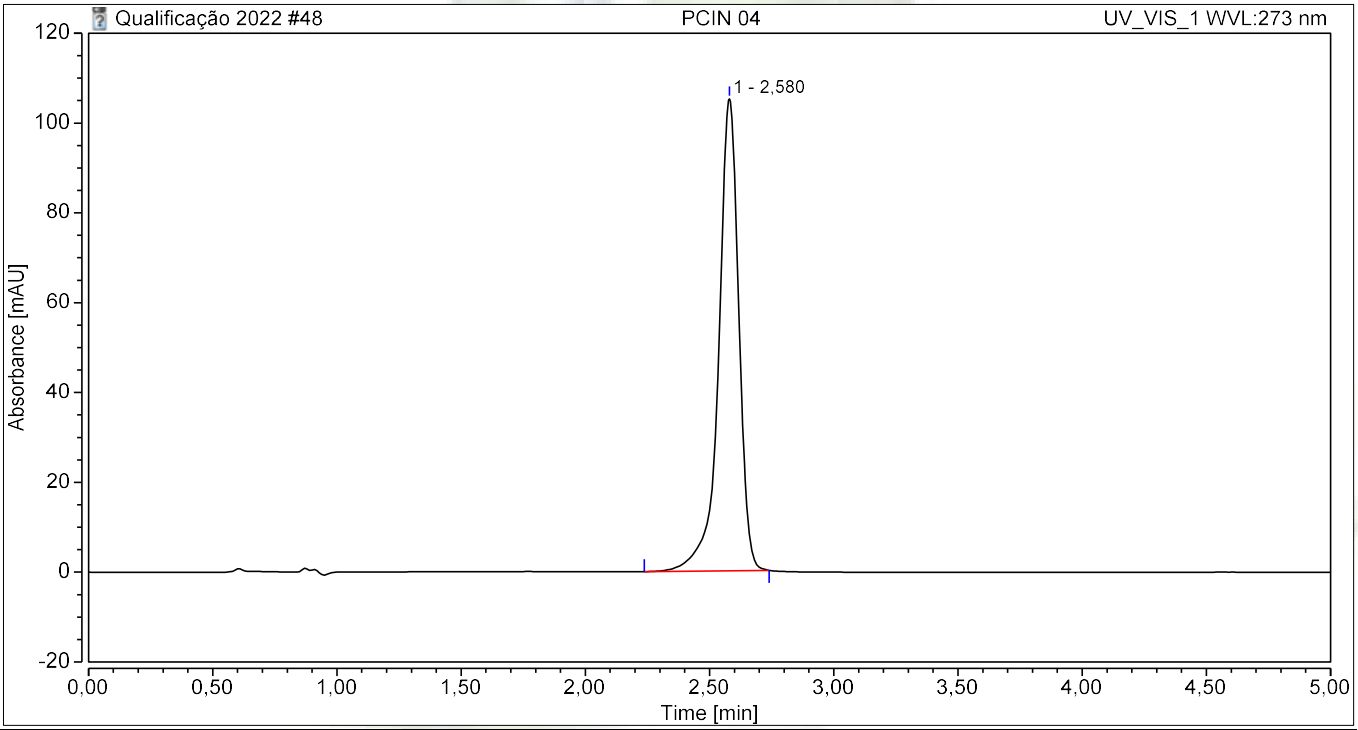

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,580	9,856	105,078	100,00	100,00	n.a.
Total:			**9,856**	**105,078**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste PCIN

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:35**	*Sample Weight:*	**1,0000**

Chromatogram

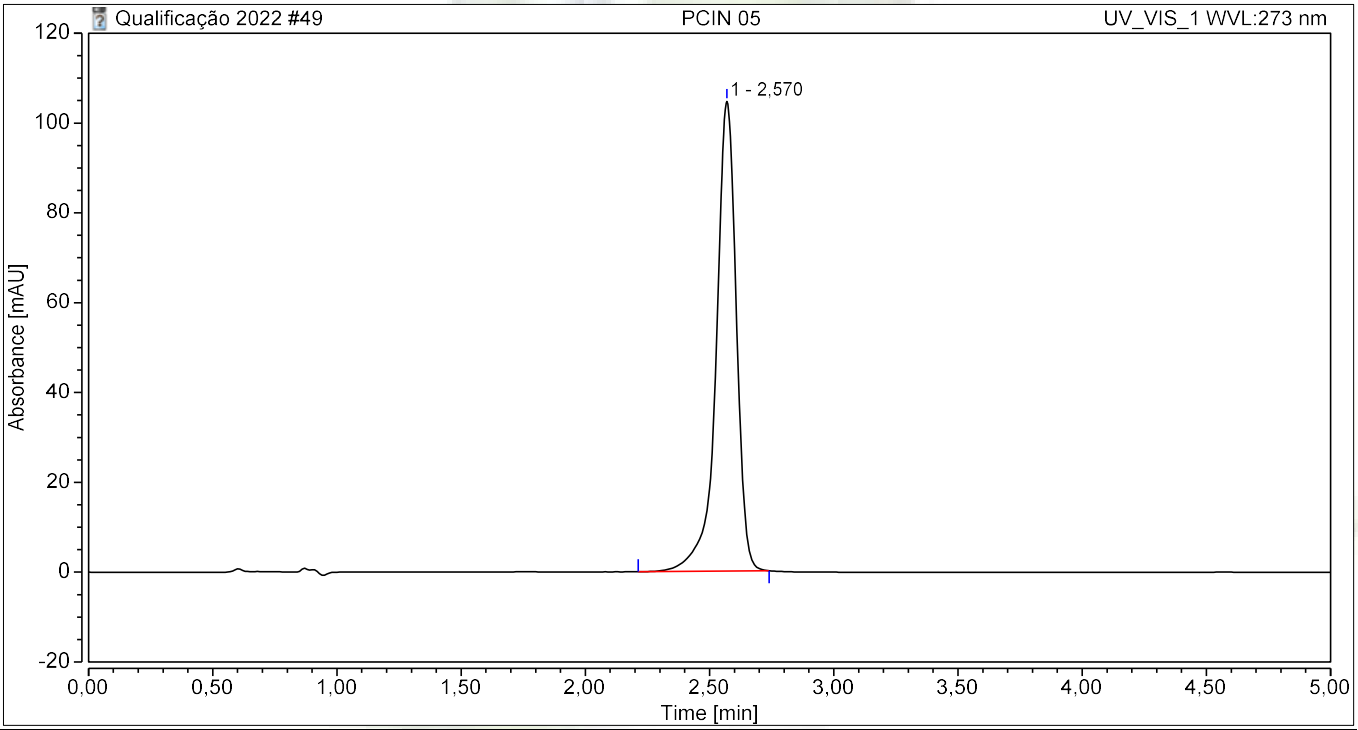

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a. 1	Cafeína	n.a. 2,570	n.a. 9,822	n.a. 104,585	n.a. 100,00	n.a. 100,00	n.a. n.a.
Total:			**9,822**	**104,585**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste PCIN

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:41**	*Sample Weight:*	**1,0000**

Chromatogram

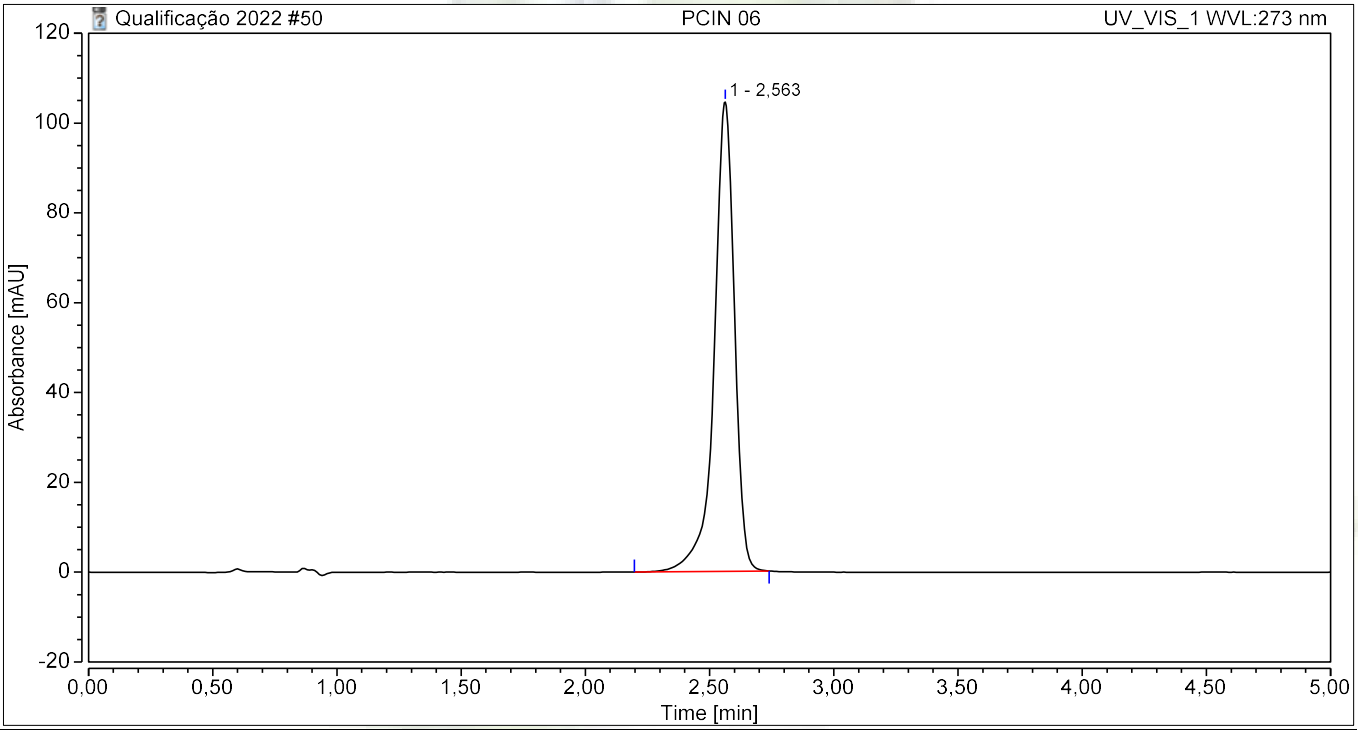

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,563	9,831	104,476	100,00	100,00	n.a.
Total:			**9,831**	**104,476**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste PCIN

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:47**	*Sample Weight:*	**1,0000**

Chromatogram

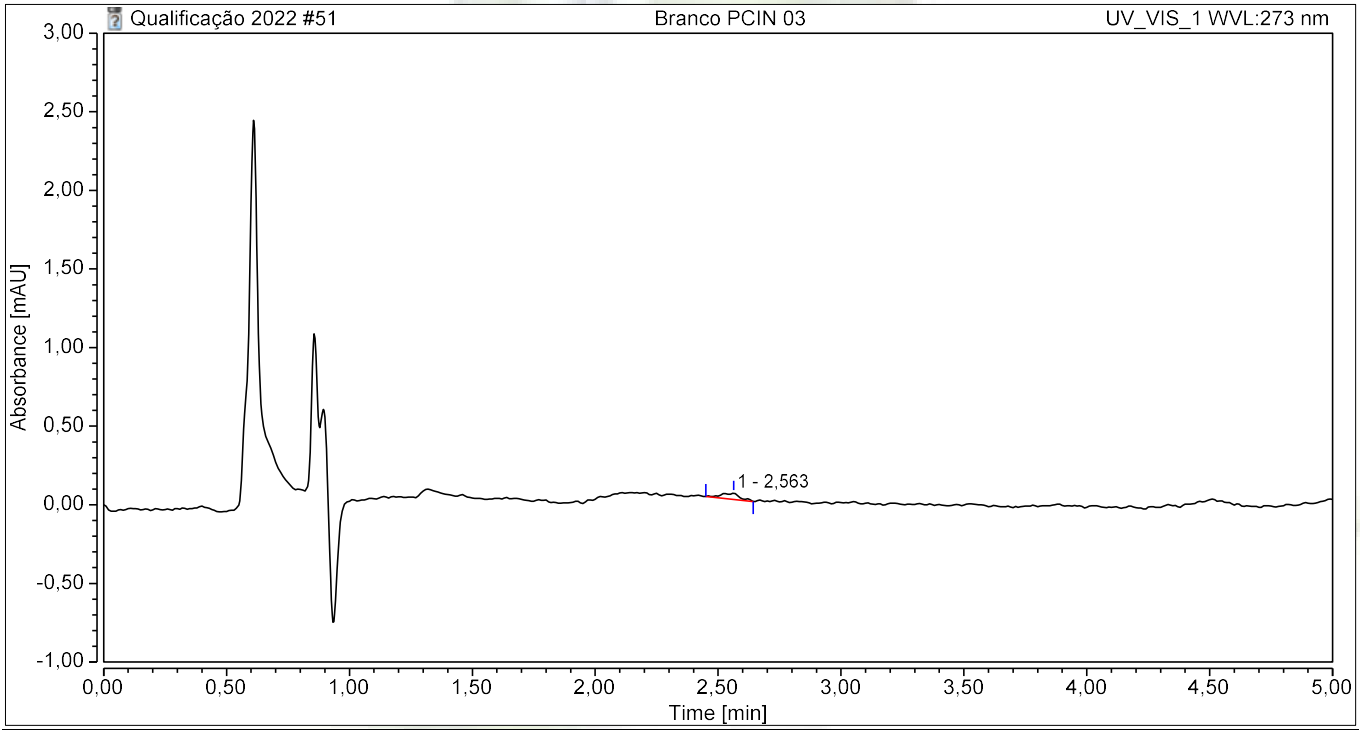

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,563	0,003	0,040	100,00	100,00	n.a.
Total:			**0,003**	**0,040**	**100,00**	**100,00**	

Teste LDUV

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:53**	*Sample Weight:*	**1,0000**

Chromatogram

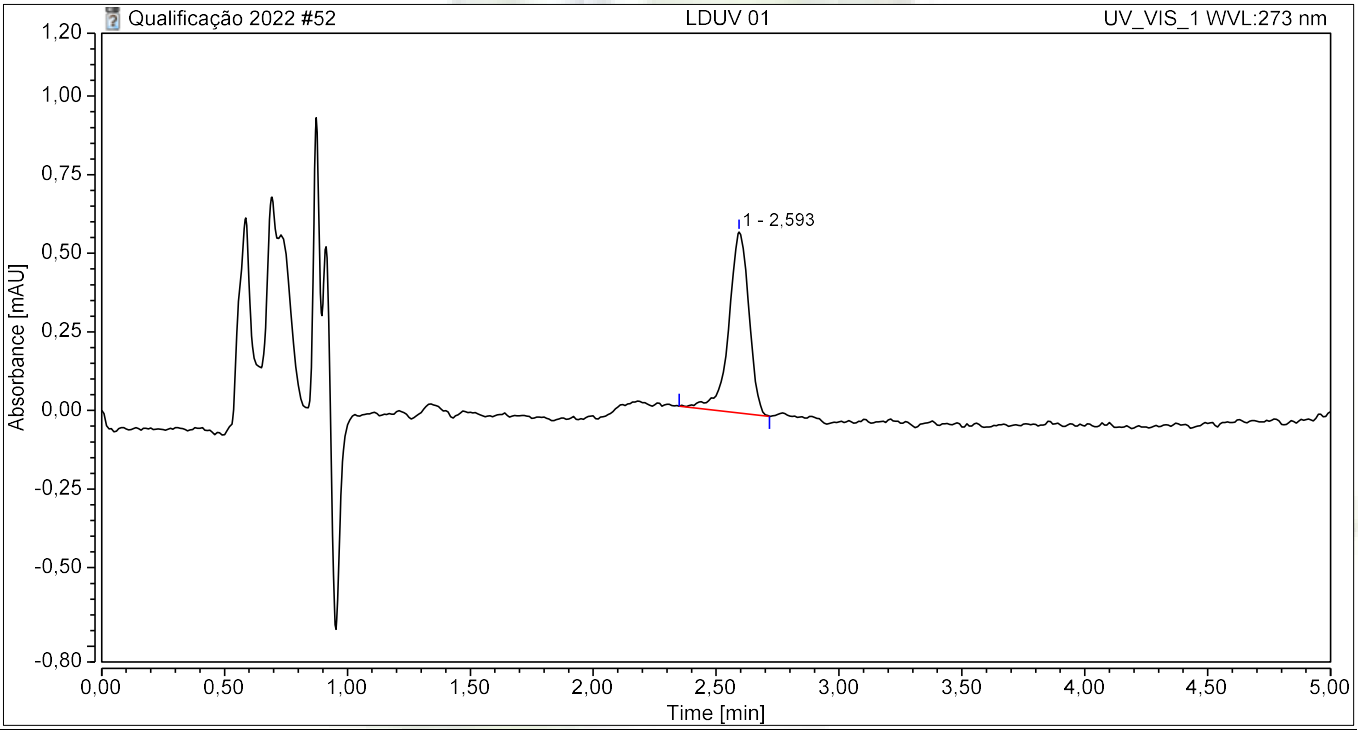

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,593	0,055	0,575	100,00	100,00	n.a.
Total:			**0,055**	**0,575**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste LDUV

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 20:59**	*Sample Weight:*	**1,0000**

Chromatogram

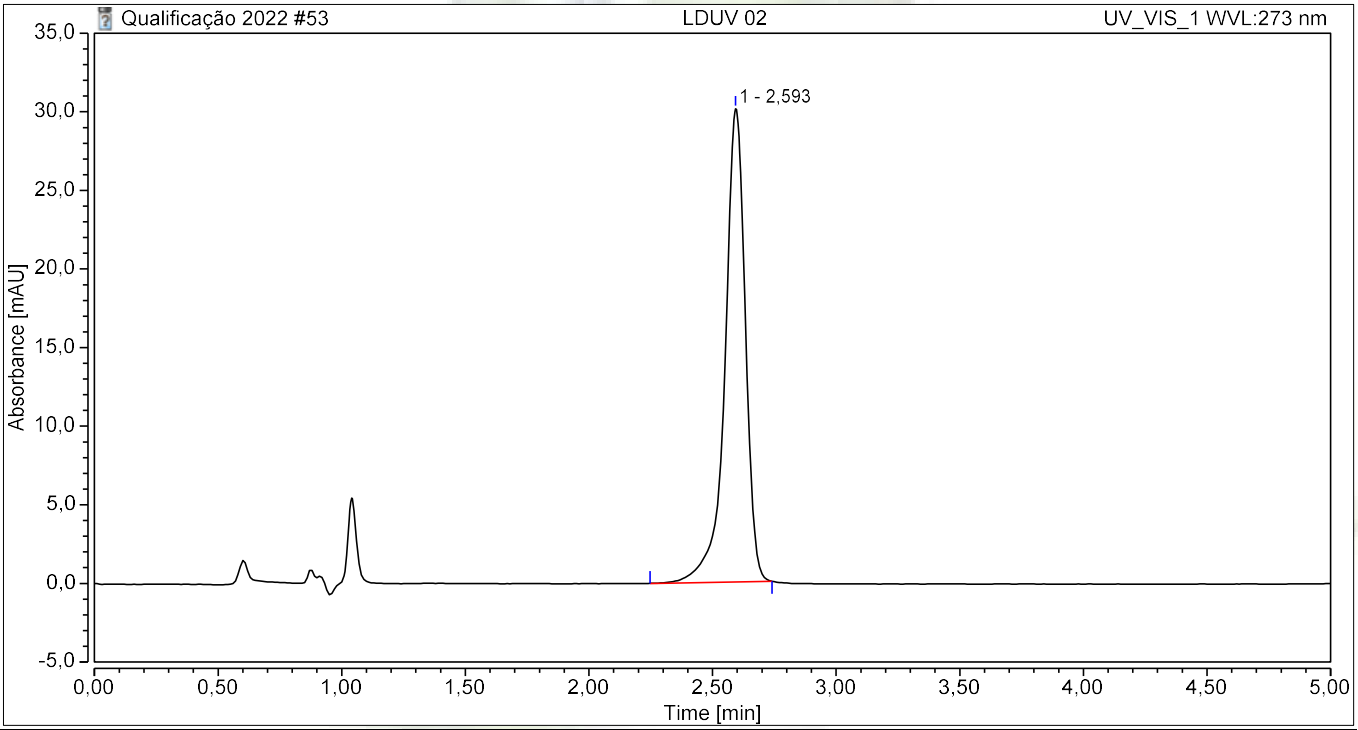

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
1		2,593	2,873	30,106	100,00	100,00	n.a.
Total:			**2,873**	**30,106**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste LDUV

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:04**	*Sample Weight:*	**1,0000**

Chromatogram

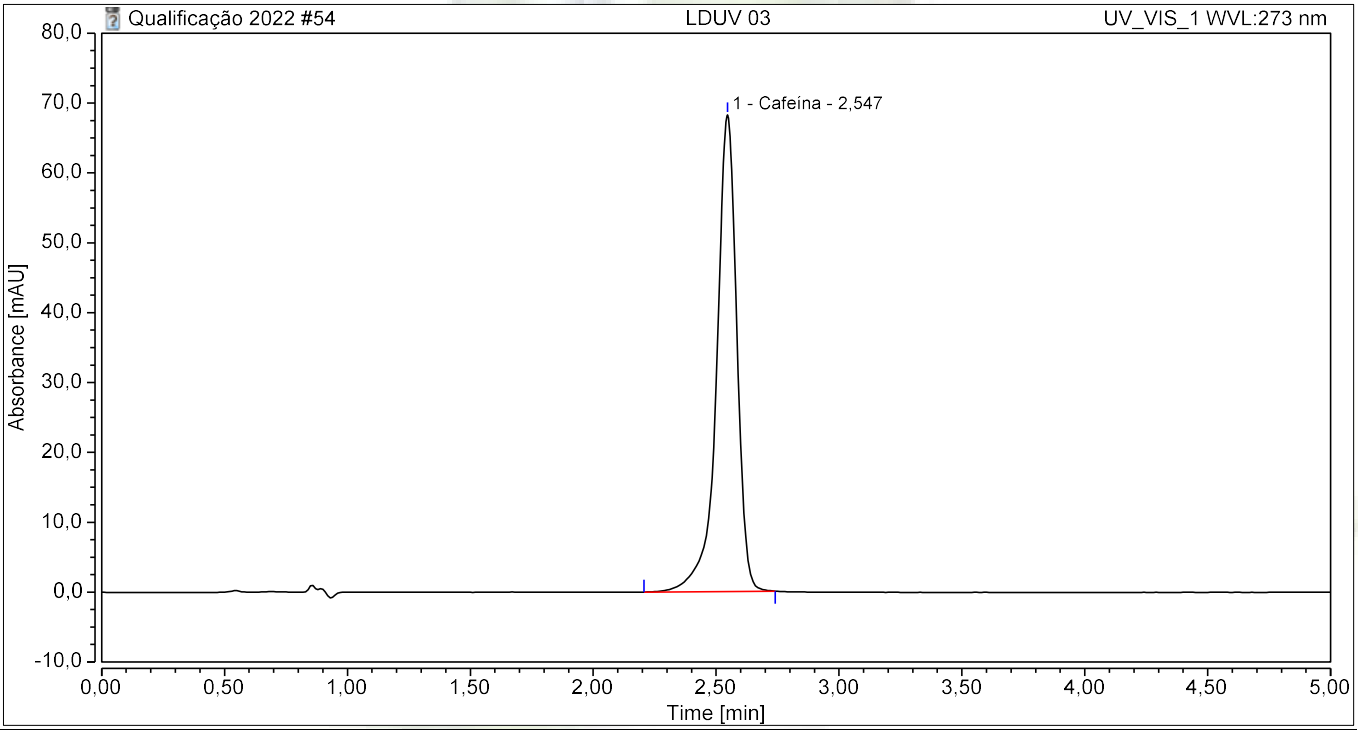

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,547	6,504	68,212	100,00	100,00	n.a.
Total:			**6,504**	**68,212**	**100,00**	**100,00**	

Teste LDUV

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**5,00**
Vial Number:	**RA8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:10**	*Sample Weight:*	**1,0000**

Chromatogram

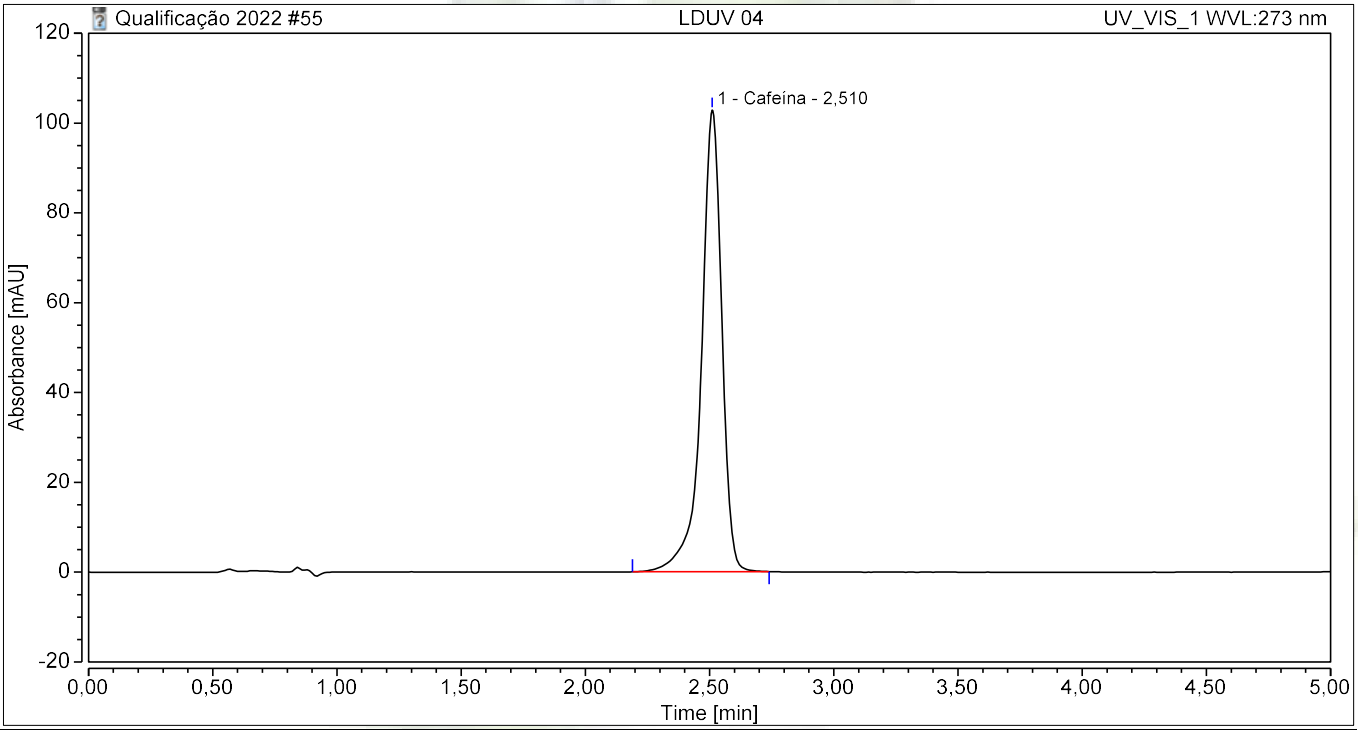

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,510	9,751	102,750	100,00	100,00	n.a.
Total:			**9,751**	**102,750**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste LDUV

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:16**	*Sample Weight:*	**1,0000**

Chromatogram

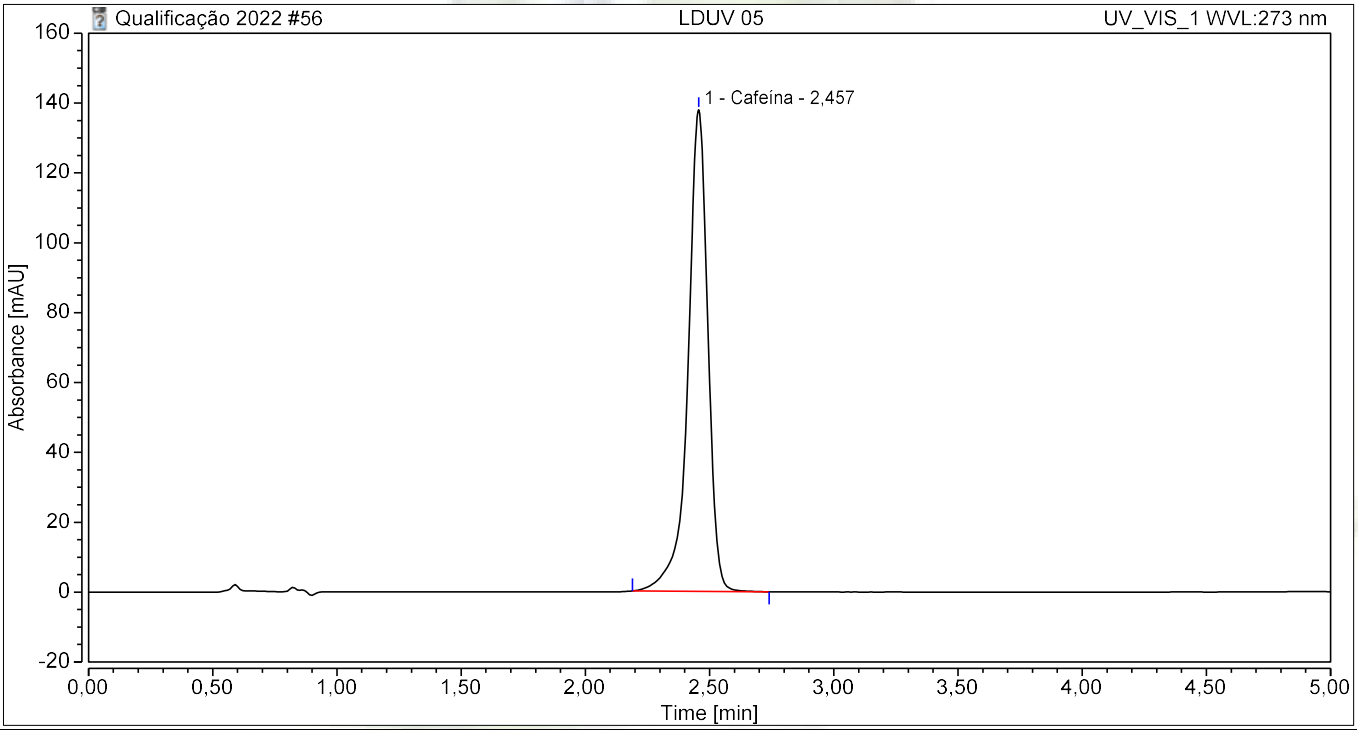

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,457	12,774	137,821	100,00	100,00	n.a.
Total:			**12,774**	**137,821**	**100,00**	**100,00**	

Teste LIIN

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RB2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:22**	*Sample Weight:*	**1,0000**

Chromatogram

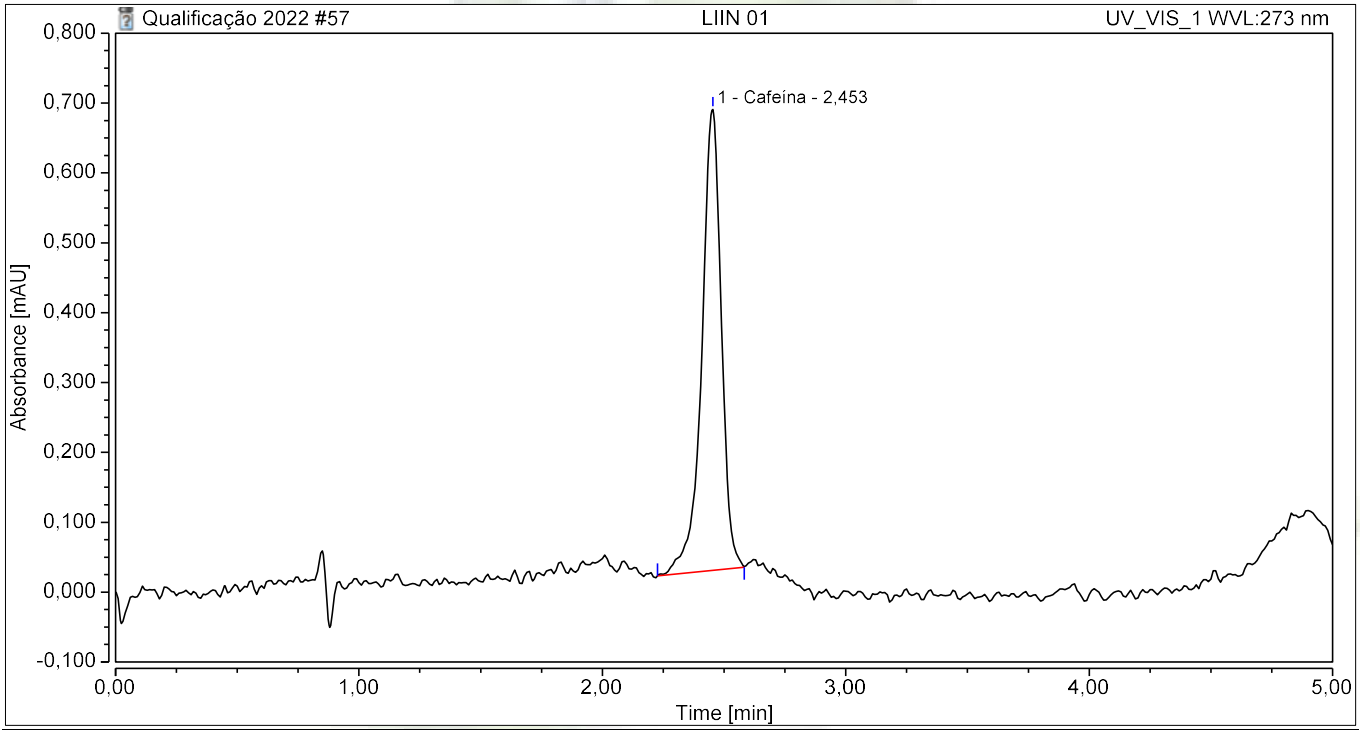

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,453	0,061	0,660	100,00	100,00	n.a.
Total:			**0,061**	**0,660**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste LIIN

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:28**	*Sample Weight:*	**1,0000**

Chromatogram

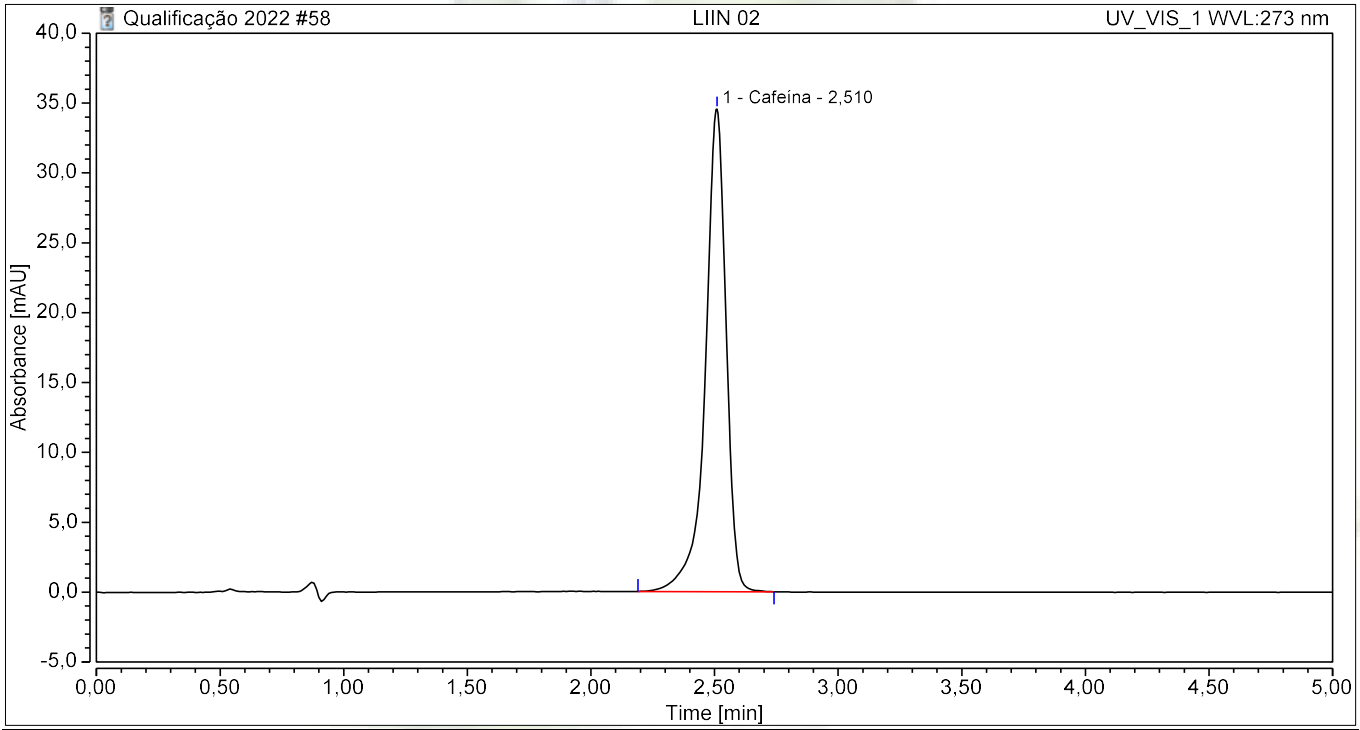

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,510	3,352	34,523	100,00	100,00	n.a.
Total:			**3,352**	**34,523**	**100,00**	**100,00**	

Teste LIIN

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RB2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:34**	*Sample Weight:*	**1,0000**

Chromatogram

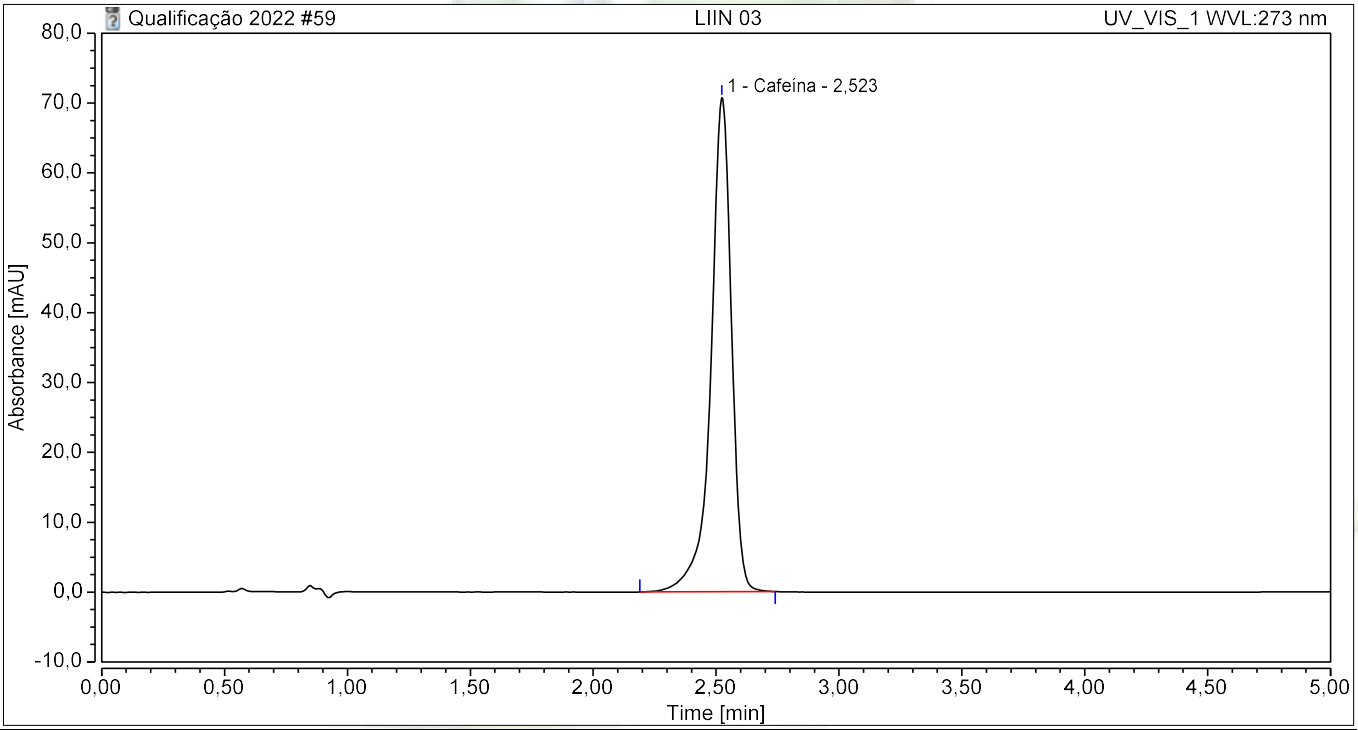

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,523	6,825	70,718	100,00	100,00	n.a.
Total:			**6,825**	**70,718**	**100,00**	**100,00**	

Teste LIIN

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**5,00**
Vial Number:	**RB2**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:40**	*Sample Weight:*	**1,0000**

Chromatogram

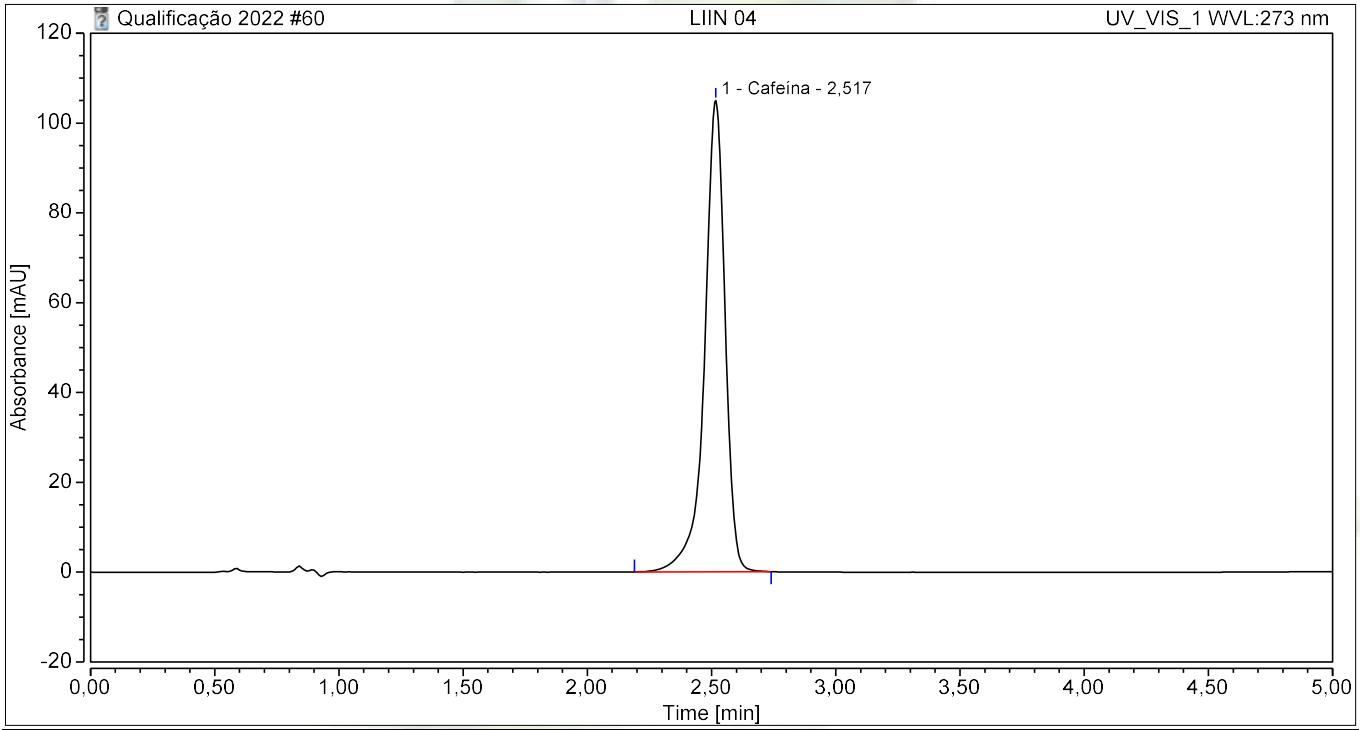

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,517	10,006	104,926	100,00	100,00	n.a.
Total:			**10,006**	**104,926**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Teste LIIN

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**5,00**
Vial Number:	**RB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**11/set/23 21:45**	*Sample Weight:*	**1,0000**

Chromatogram

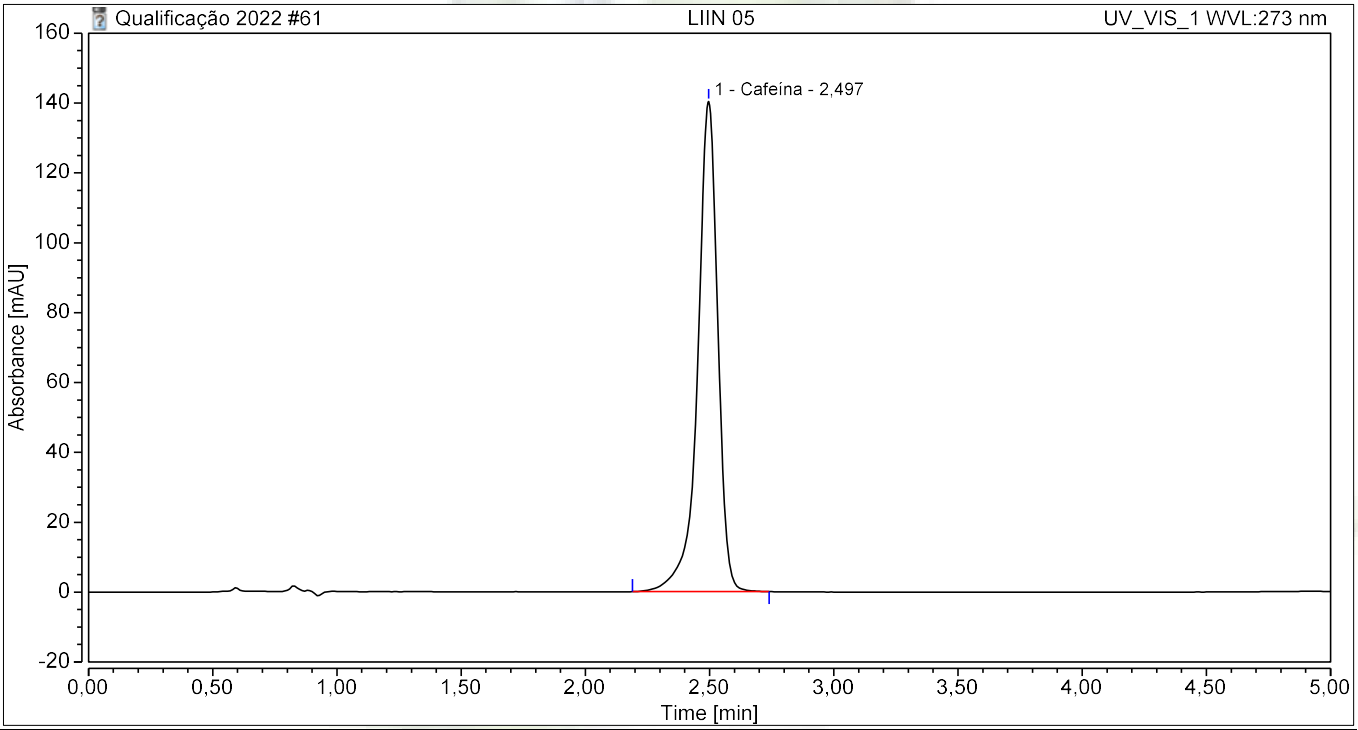

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,497	13,149	140,301	100,00	100,00	n.a.
Total:			**13,149**	**140,301**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB 3**	*Run Time (min):*	**18,00**
Vial Number:	**RA5**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/set/23 13:26**	*Sample Weight:*	**1,0000**

Chromatogram

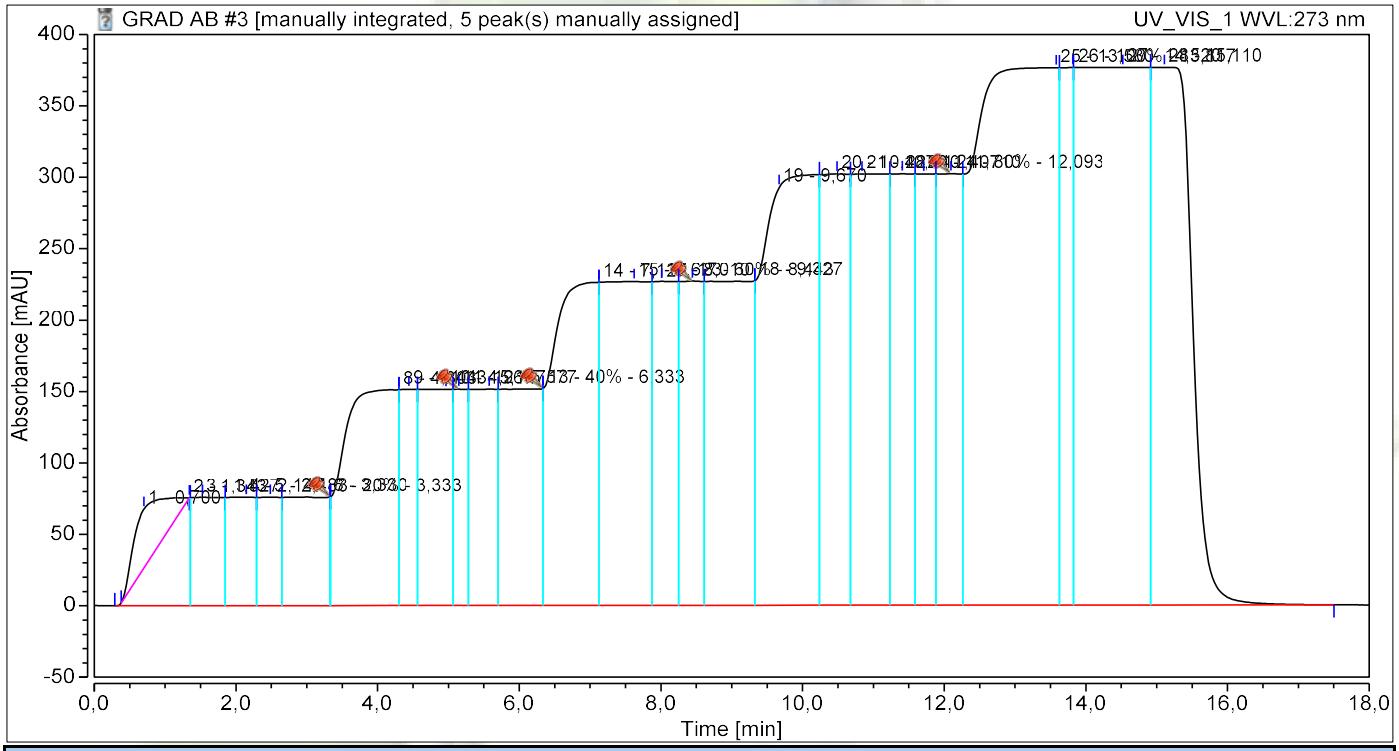

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		0,700	22,391	41,161	0,66	0,70	n.a.
2		1,343	38,351	75,608	1,13	1,29	n.a.
3		1,527	37,387	75,890	1,10	1,30	n.a.
4		2,147	33,653	76,024	0,99	1,30	n.a.
5		2,483	27,053	75,989	0,80	1,30	n.a.
6		3,330	51,556	76,118	1,52	1,30	n.a.
7	20%	3,333	0,254	76,196	0,01	1,30	n.a.
8		4,303	130,829	151,063	3,85	2,58	n.a.
9		4,443	39,344	151,446	1,16	2,59	n.a.
10		4,967	75,670	151,408	2,23	2,59	n.a.
11		5,147	33,301	151,440	0,98	2,59	n.a.
12		5,577	63,575	151,501	1,87	2,59	n.a.
13	40%	6,333	95,400	151,849	2,81	2,60	n.a.
14		7,127	164,207	226,167	4,83	3,87	n.a.
15		7,623	169,153	226,700	4,98	3,88	n.a.
16		8,010	85,392	226,856	2,51	3,88	n.a.
17	60%	8,443	81,649	227,034	2,40	3,88	n.a.
18		9,327	162,489	227,159	4,78	3,88	n.a.
19		9,670	259,950	292,531	7,65	5,00	n.a.
20		10,487	131,754	301,995	3,88	5,16	n.a.
21		10,840	168,012	301,934	4,95	5,16	n.a.


22		11,407	106,666	302,001	3,14	5,16	n.a.
23		11,710	89,539	301,900	2,64	5,16	n.a.
24	80%	12,093	113,717	302,017	3,35	5,17	n.a.
25		13,580	494,114	376,230	14,55	6,43	n.a.
26	100%	13,817	73,995	376,288	2,18	6,44	n.a.
27		14,520	410,166	376,329	12,07	6,44	n.a.
28		15,110	237,499	376,306	6,99	6,44	n.a.
Total:			**3397,069**	**5847,139**	**100,00**	**100,00**	

Teste GRBO - Gradiente Canais C e D

Injection Details

Injection Name:	**GRAD CD 3**	*Run Time (min):*	**18,00**
Vial Number:	**RA2**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**12/set/23 15:08**	*Sample Weight:*	**1,0000**

Chromatogram

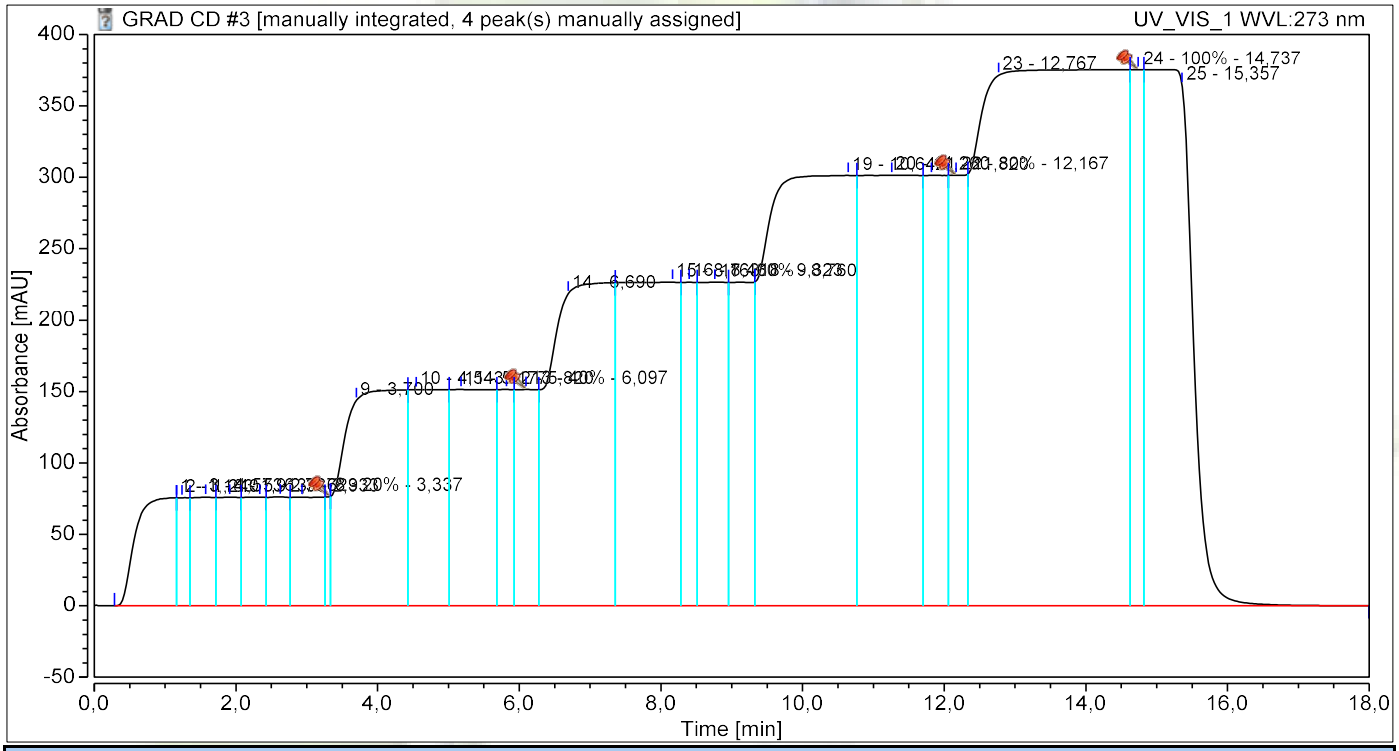

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1		1,163	46,227	75,526	1,36	1,57	n.a.
2		1,240	14,121	75,684	0,42	1,58	n.a.
3		1,573	27,812	76,032	0,82	1,58	n.a.
4		1,913	27,080	76,062	0,80	1,58	n.a.
5		2,337	26,844	76,094	0,79	1,59	n.a.
6		2,623	25,607	76,247	0,75	1,59	n.a.
7		2,933	37,476	76,084	1,10	1,59	n.a.
8	20%	3,337	6,099	76,645	0,18	1,60	n.a.
9		3,700	149,695	143,639	4,41	2,99	n.a.
10		4,543	87,742	151,360	2,59	3,15	n.a.
11		5,177	101,904	151,477	3,00	3,16	n.a.
12		5,820	36,836	151,452	1,09	3,16	n.a.
13	40%	6,097	52,972	151,463	1,56	3,16	n.a.
14		6,690	223,833	218,334	6,60	4,55	n.a.
15		8,163	210,542	226,497	6,21	4,72	n.a.
16		8,400	52,083	226,563	1,54	4,72	n.a.
17	60%	8,760	100,406	226,648	2,96	4,72	n.a.
18		9,323	83,026	226,643	2,45	4,72	n.a.
19		10,643	418,908	301,323	12,35	6,28	n.a.
20		11,260	281,265	301,501	8,29	6,28	n.a.
21		11,820	107,464	301,364	3,17	6,28	n.a.


22	80%	12,167	83,398	301,452	2,46	6,28	n.a.
23		12,767	845,911	371,279	24,94	7,74	n.a.
24	100%	14,737	72,555	375,296	2,14	7,82	n.a.
25		15,357	272,103	364,436	8,02	7,59	n.a.
Total:			**3391,910**	**4799,100**	**100,00**	**100,00**	

Teste RELB

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**254**
Instrument Method:	**RELB**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 10:32**	*Sample Weight:*	**1,0000**


Chromatogram

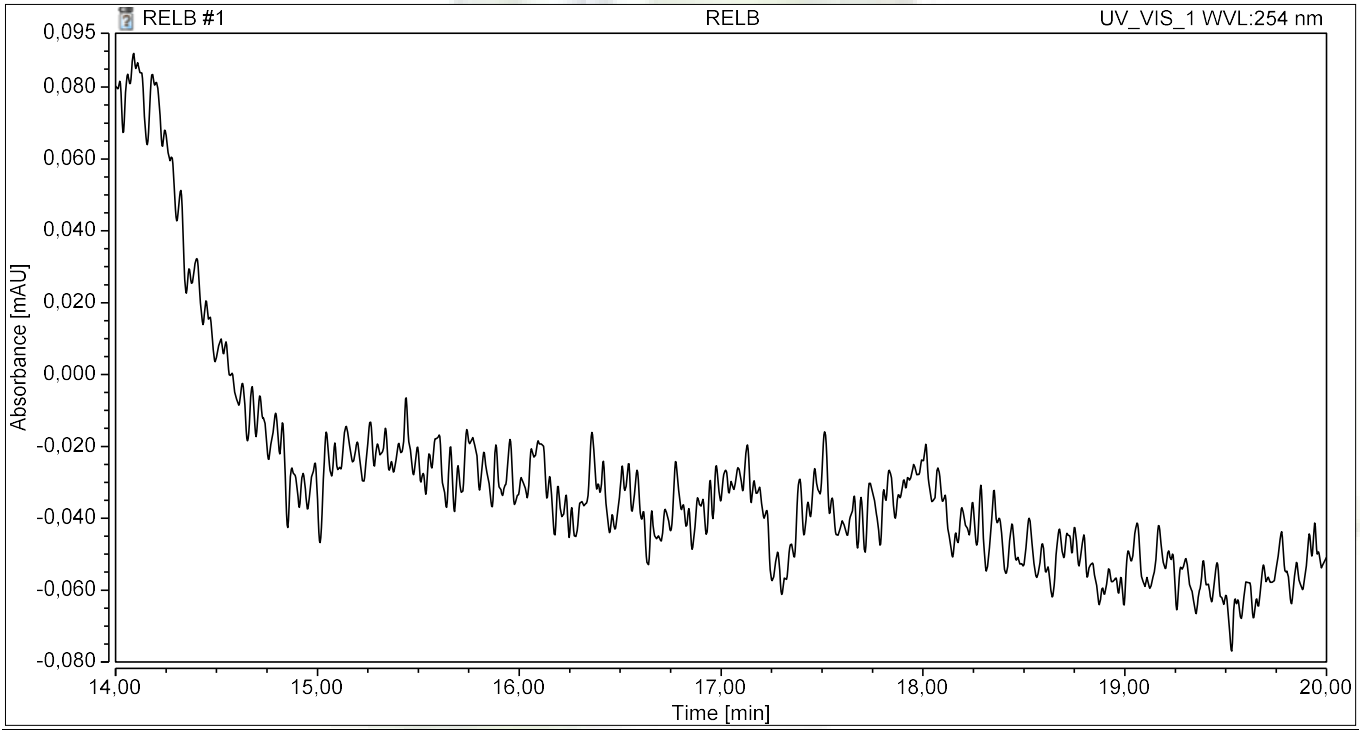


Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,527	11,101	96,324	100,00	100,00	n.a.
Total:			**11,101**	**96,324**	**100,00**	**100,00**	

Teste RELB

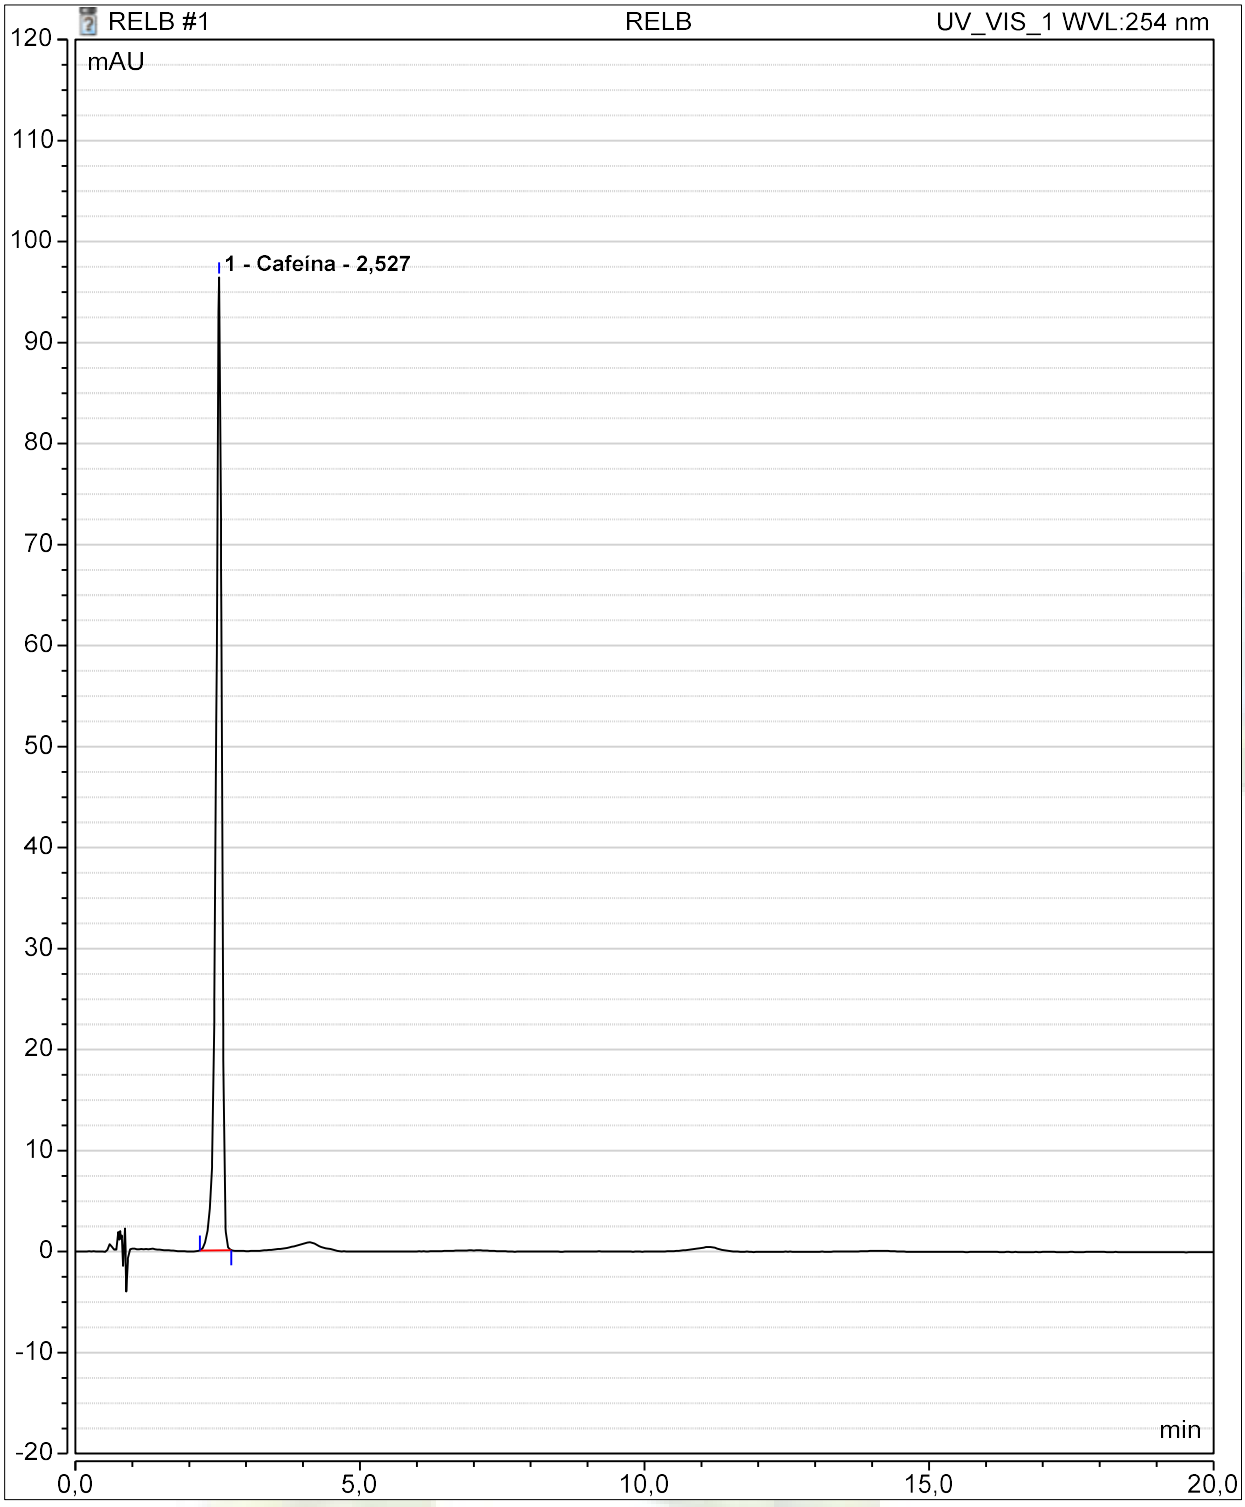
RELB #1
RELB
UV_VIS_1 WVL:254 nm
mAU
120
110
100
90
80
70
60
50
40
30
20
10
0
-10
-20
1 - Cafeína - 2,527
min
0,0
5,0
10,0
15,0
20,0




Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_01**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 12:56**	*Sample Weight:*	**1,0000**

Chromatogram

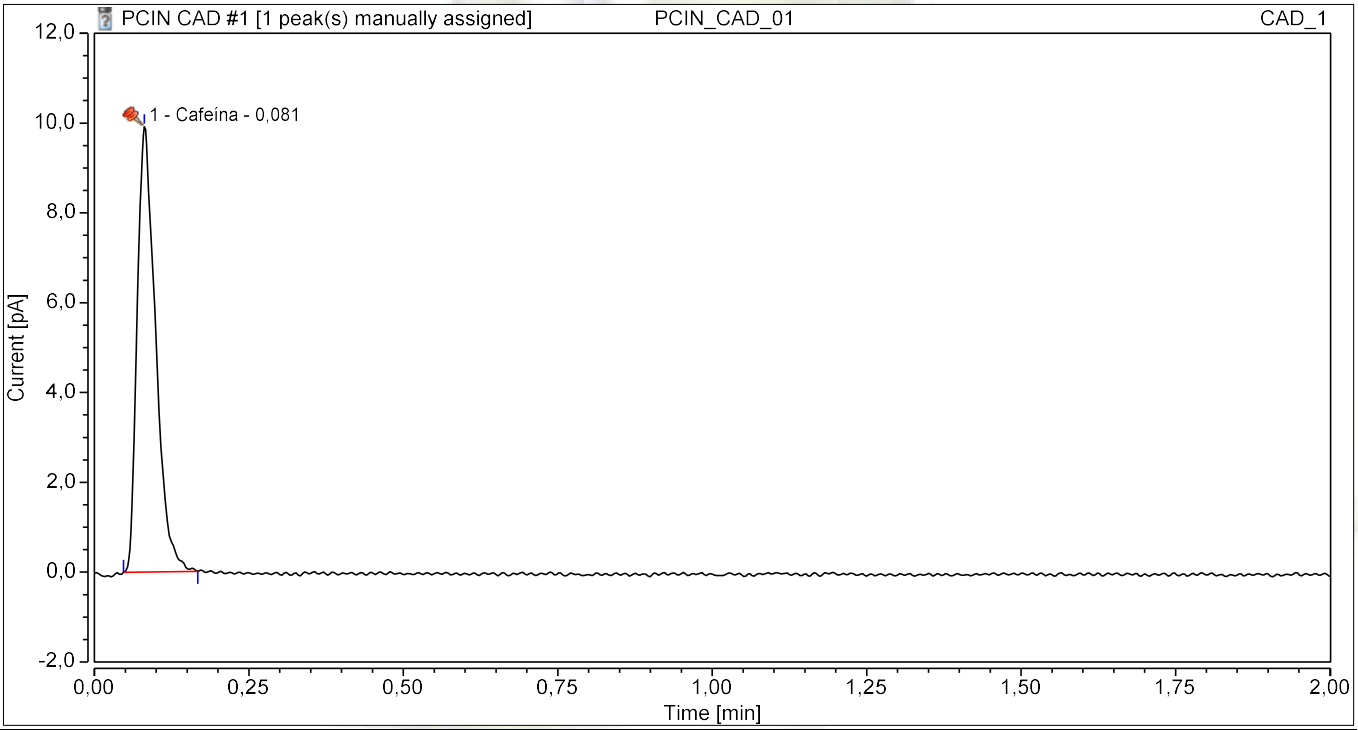

Integration Results


No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1	Cafeína	0,081	0,344	9,921	100,00	100,00	n.a.
Total:			**0,344**	**9,921**	**100,00**	**100,00**	

Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_02**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 12:59**	*Sample Weight:*	**1,0000**

Chromatogram

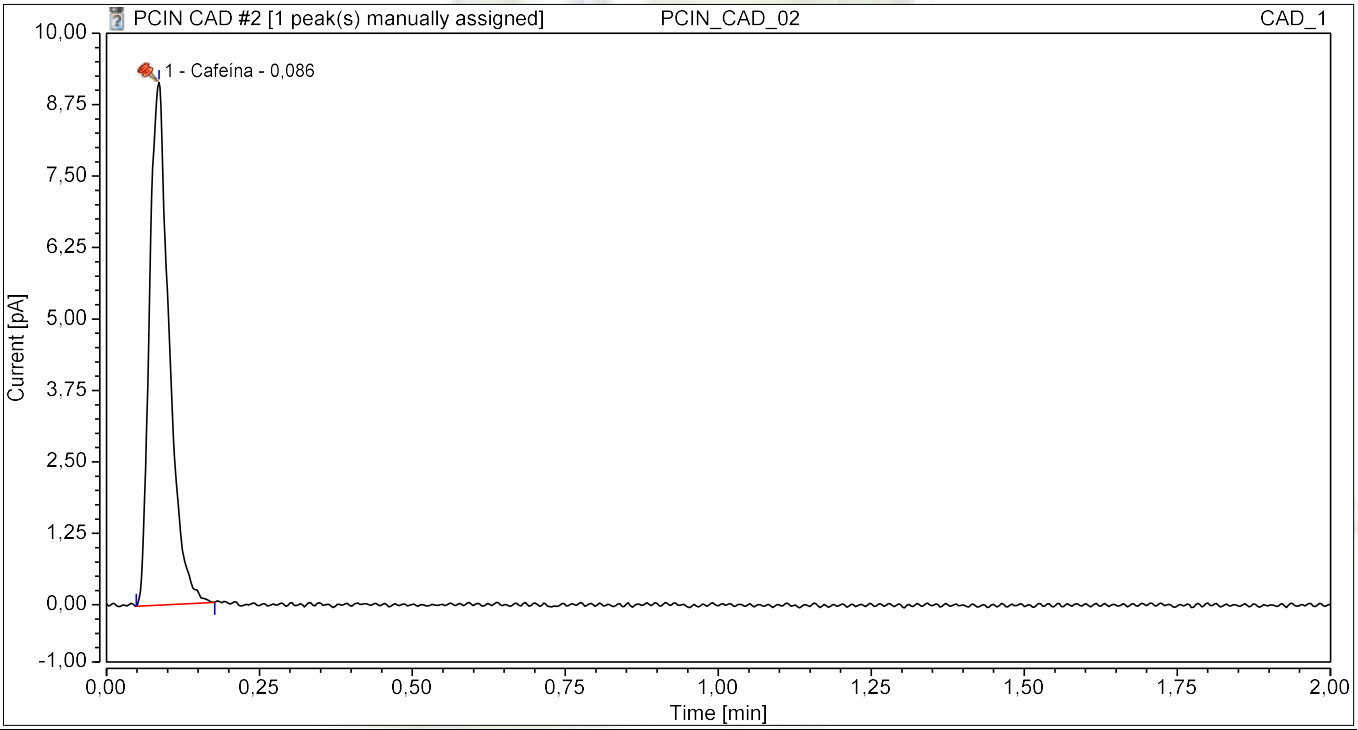

Integration Results


No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1	Cafeína	0,086	0,341	9,146	100,00	100,00	n.a.
Total:			**0,341**	**9,146**	**100,00**	**100,00**	

Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_03**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 13:02**	*Sample Weight:*	**1,0000**

Chromatogram

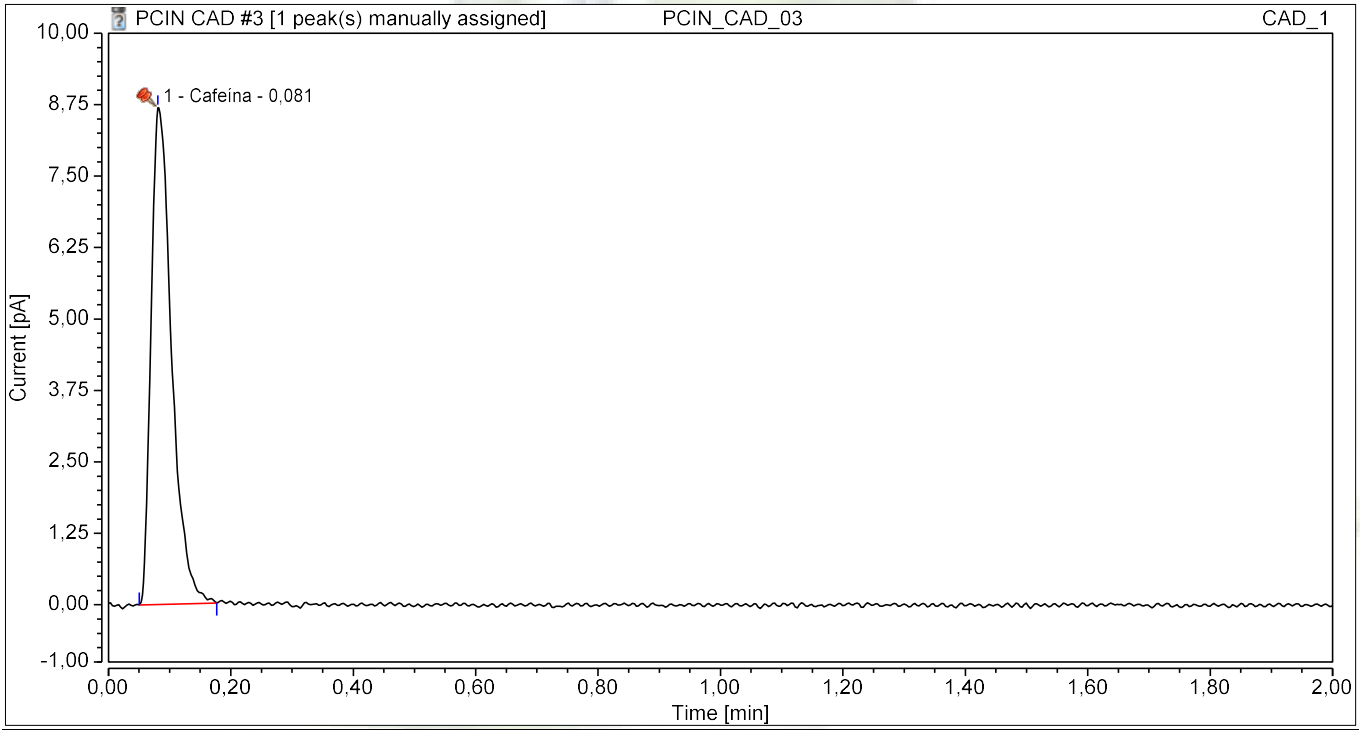

Integration Results


No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1	Cafeína	0,081	0,338	8,690	100,00	100,00	n.a.
Total:			**0,338**	**8,690**	**100,00**	**100,00**	

Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_04**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 13:05**	*Sample Weight:*	**1,0000**

Chromatogram

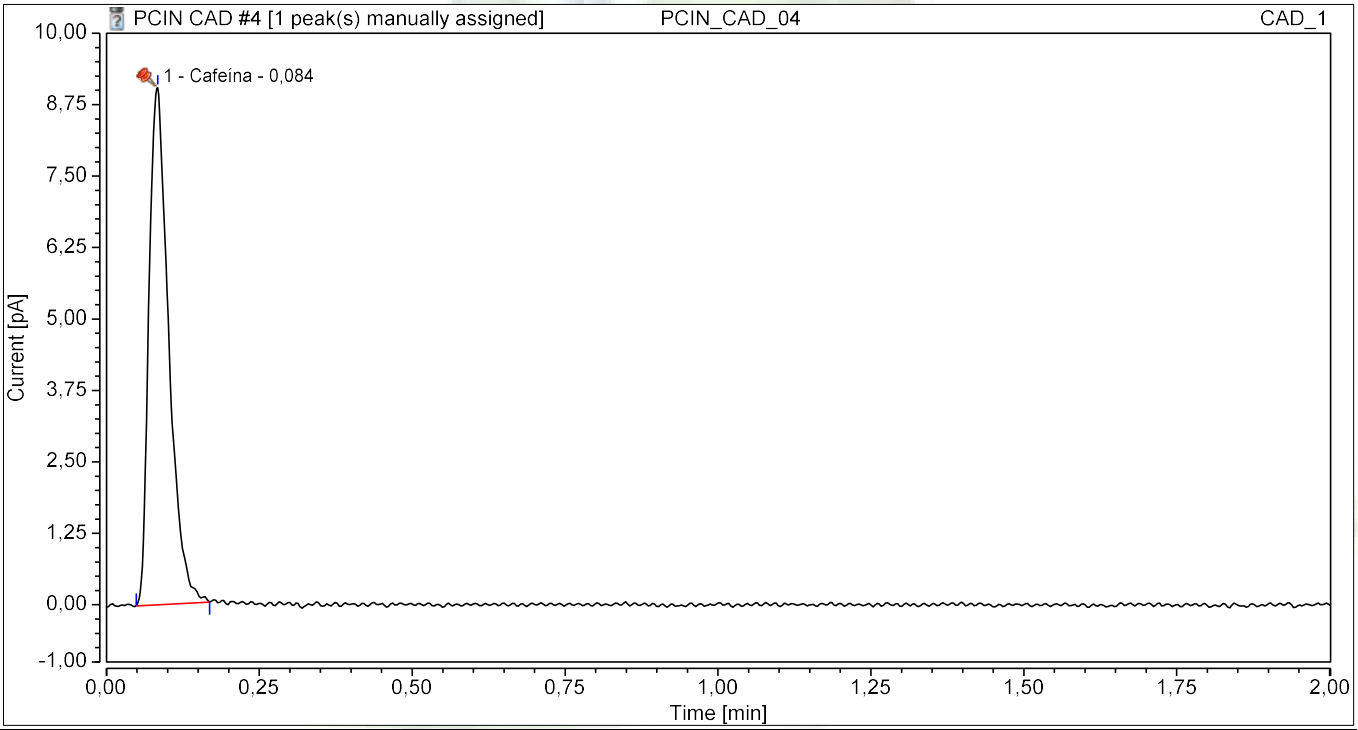

Integration Results


No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1	Cafeína	0,084	0,340	9,048	100,00	100,00	n.a.
Total:			**0,340**	**9,048**	**100,00**	**100,00**	

Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_05**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 13:08**	*Sample Weight:*	**1,0000**

Chromatogram

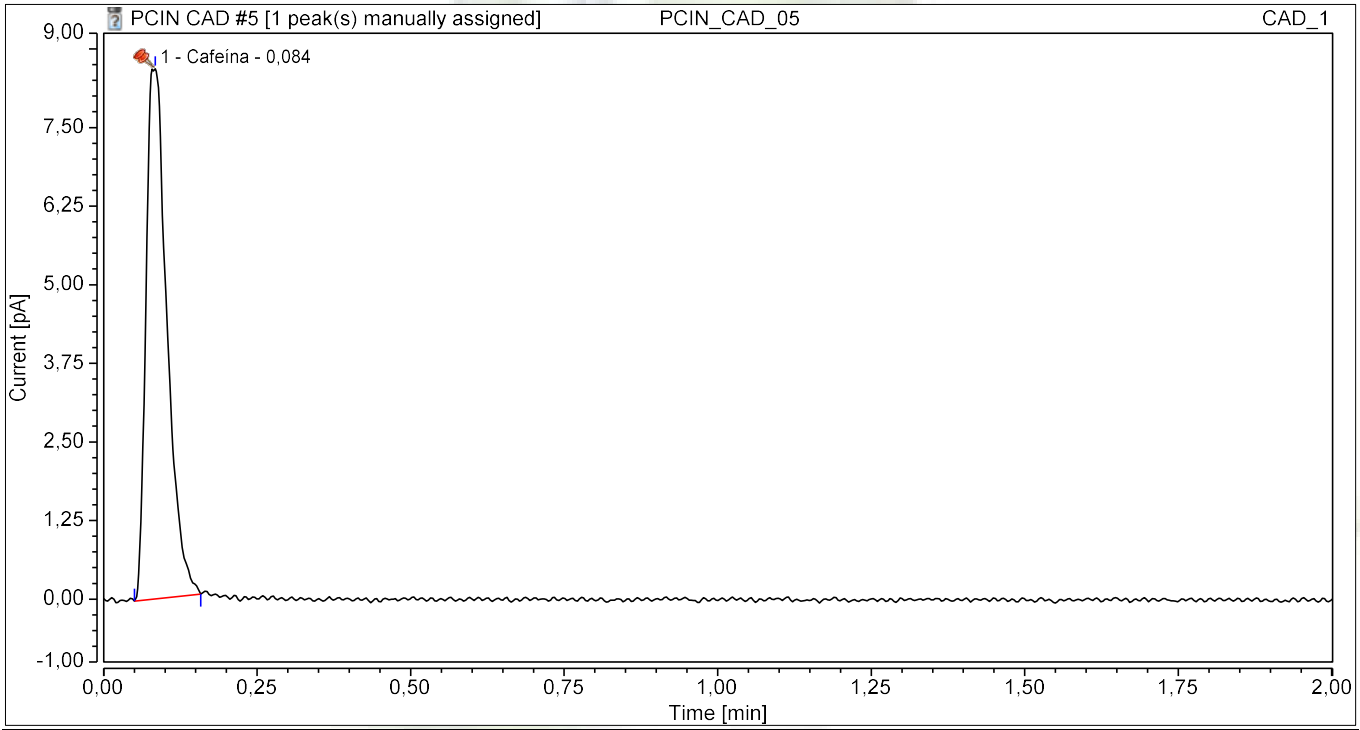

Integration Results


No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1	Cafeína	0,084	0,335	8,432	100,00	100,00	n.a.
Total:			**0,335**	**8,432**	**100,00**	**100,00**	

Teste PCIN CAD

Injection Details

Injection Name:	**PCIN_CAD_06**	*Run Time (min):*	**2,00**
Vial Number:	**RA4**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/23 13:11**	*Sample Weight:*	**1,0000**

Chromatogram

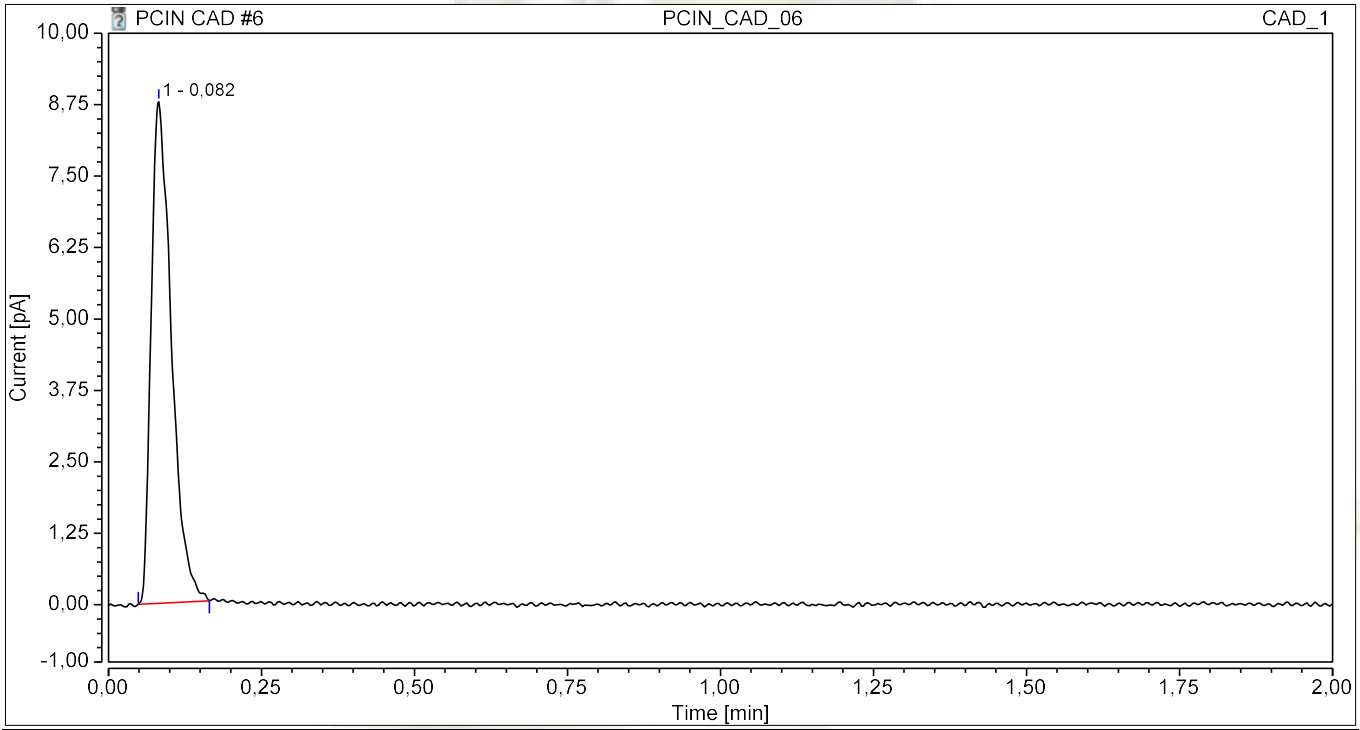

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,082	0,337	8,772	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,337**	**8,772**	**100,00**	**100,00**	