
Spectral Library Screening Results

Injection Details

Injection Name:	**EDUV**	*Run Time (min):*	**5,00**
Vial Number:	**GA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 15:29**	*Sample Weight:*	**1,0000**


UV Spectra — Cafeína

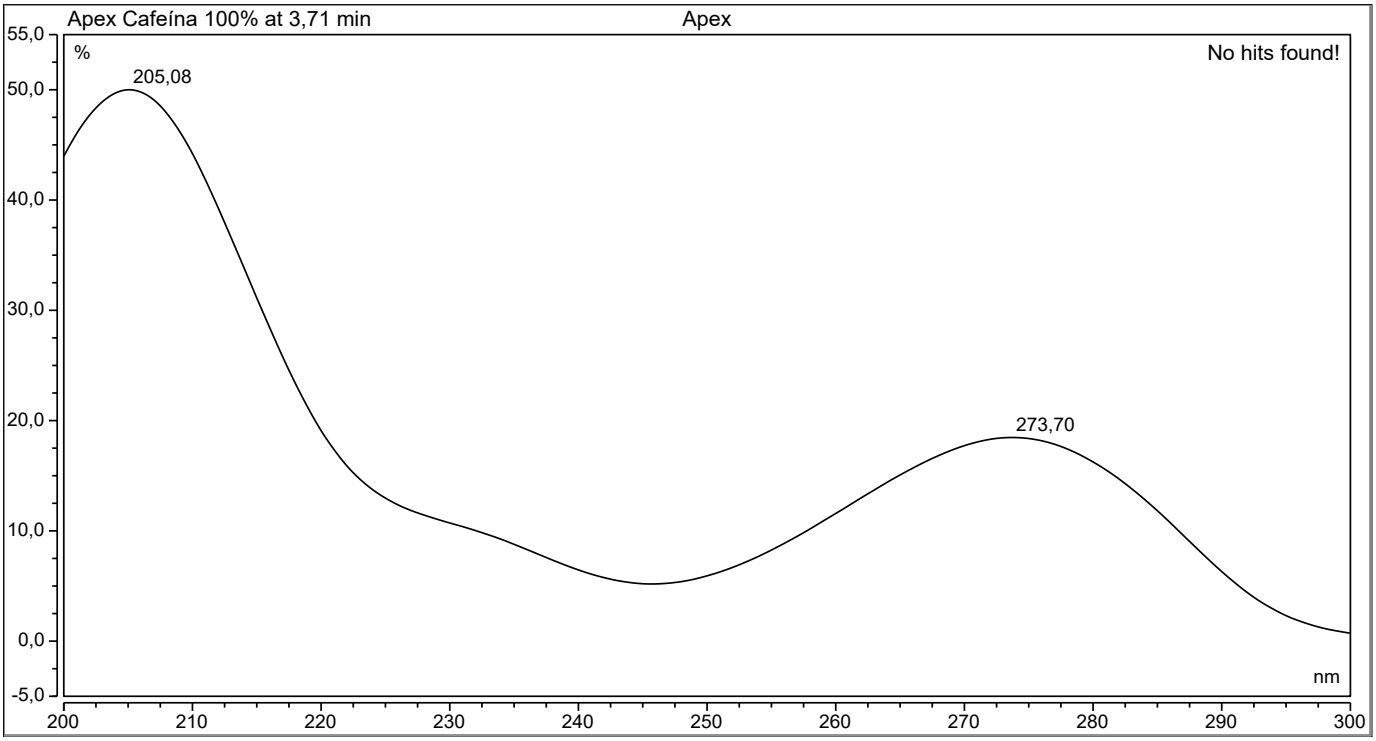

Spectral Library Screening Results

	Hit# 1	Hit# 2	Hit# 3
Library:	n.a.	n.a.	n.a.
Component:	n.a.	n.a.	n.a.
Match Factor:	n.a.	n.a.	n.a.
Ret.Time:	n.a.	n.a.	n.a.
Origin:			
Acq.Date:	n.a.	n.a.	n.a.
Instrument Method:	n.a.	n.a.	n.a.

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

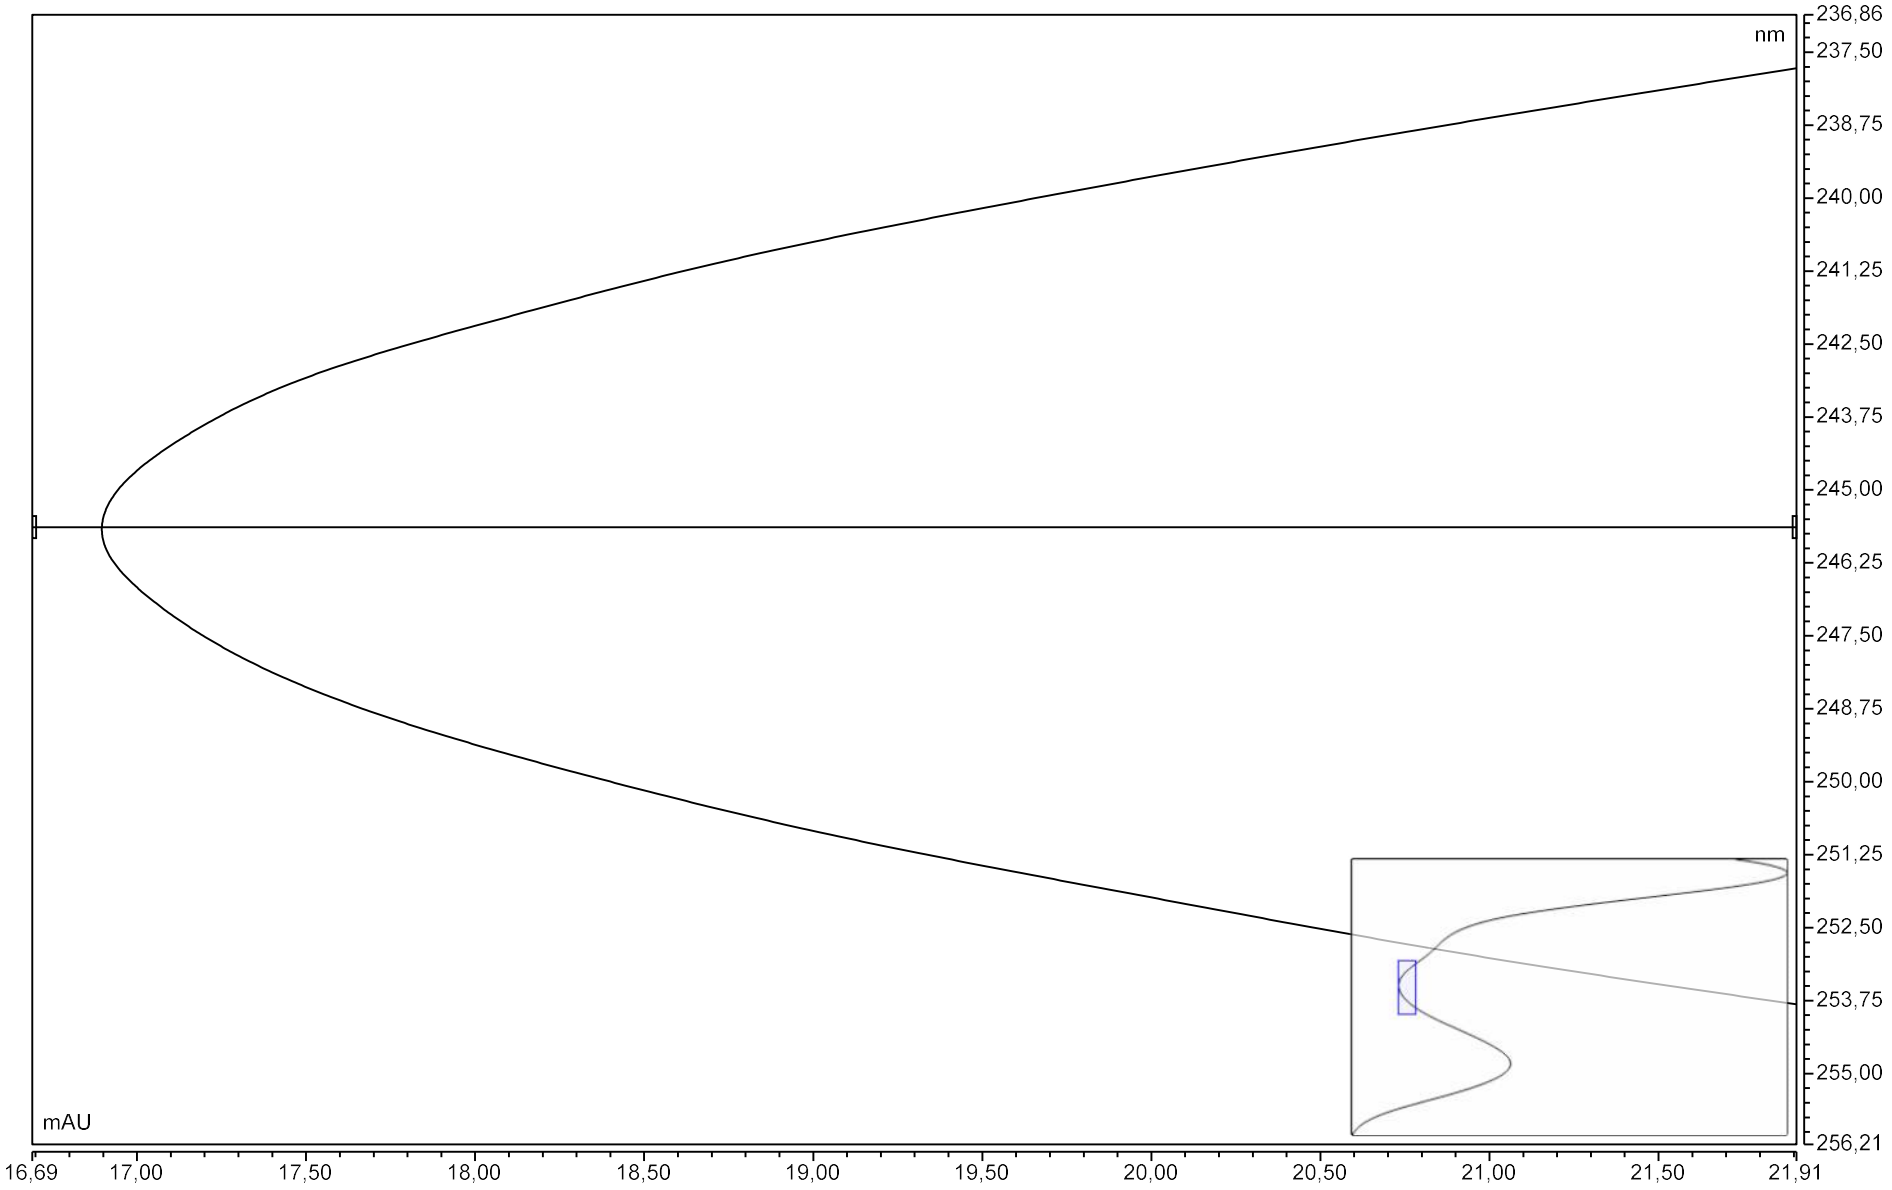

nm
236,86
237,50
238,75
240,00
241,25
242,50
243,75
245,00
246,25
247,50
248,75
250,00
251,25
252,50
253,75
255,00
256,21
mAU
16,69
17,00
17,50
18,00
18,50
19,00
19,50
20,00
20,50
21,00
21,50
21,91

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**GB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 15:41**	*Sample Weight:*	**1,0000**

Chromatogram

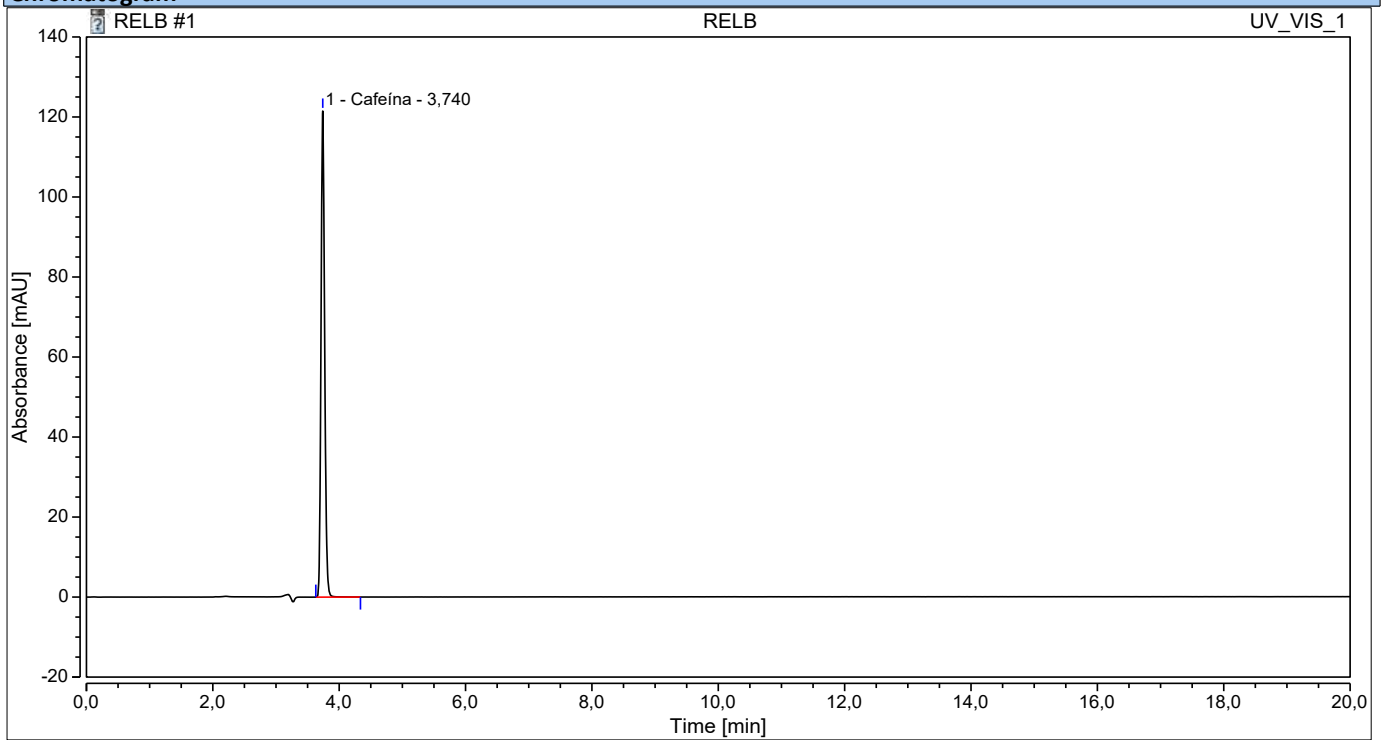

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,740	8,1142	121,507	100,00	100,00	n.a.
Total:			**8,114**	**121,507**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**GB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 15:41**	*Sample Weight:*	**1,0000**

Chromatogram

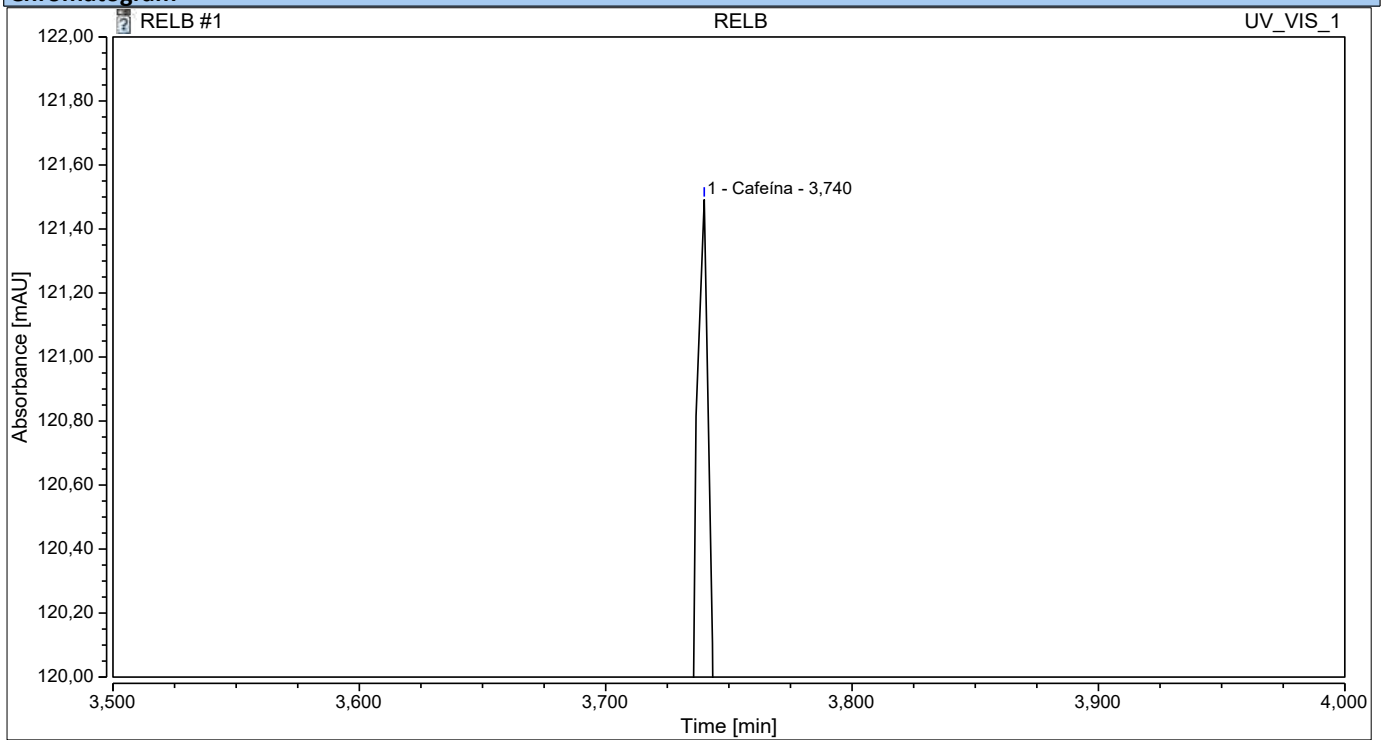

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,740	8,1142	121,507	100,00	100,00	n.a.
Total:			**8,114**	**121,507**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**GB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 15:41**	*Sample Weight:*	**1,0000**

Chromatogram

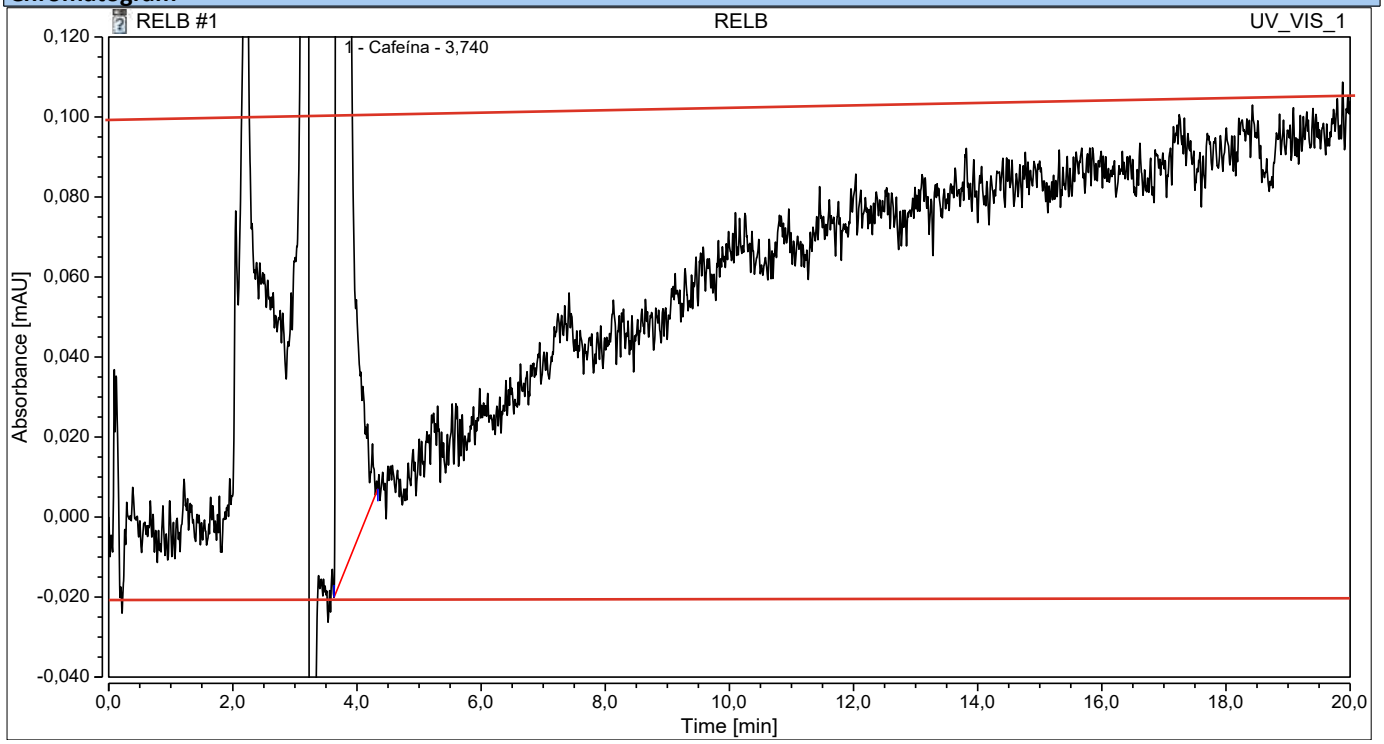

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,740	8,1142	121,507	100,00	100,00	n.a.
Total:			**8,114**	**121,507**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**GB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 15:41**	*Sample Weight:*	**1,0000**

Chromatogram

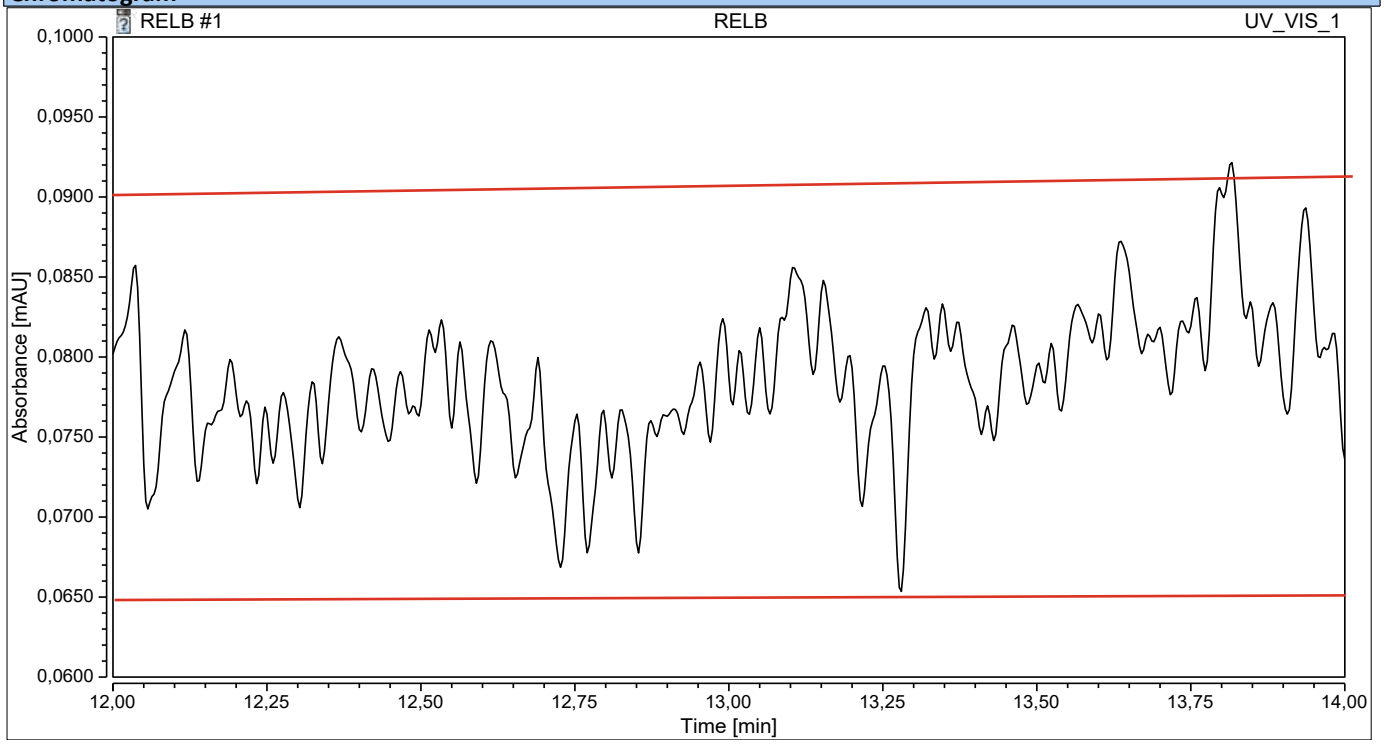

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,740	8,1142	121,507	100,00	100,00	n.a.
Total:			**8,114**	**121,507**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**GA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 16:37**	*Sample Weight:*	**1,0000**

Chromatogram

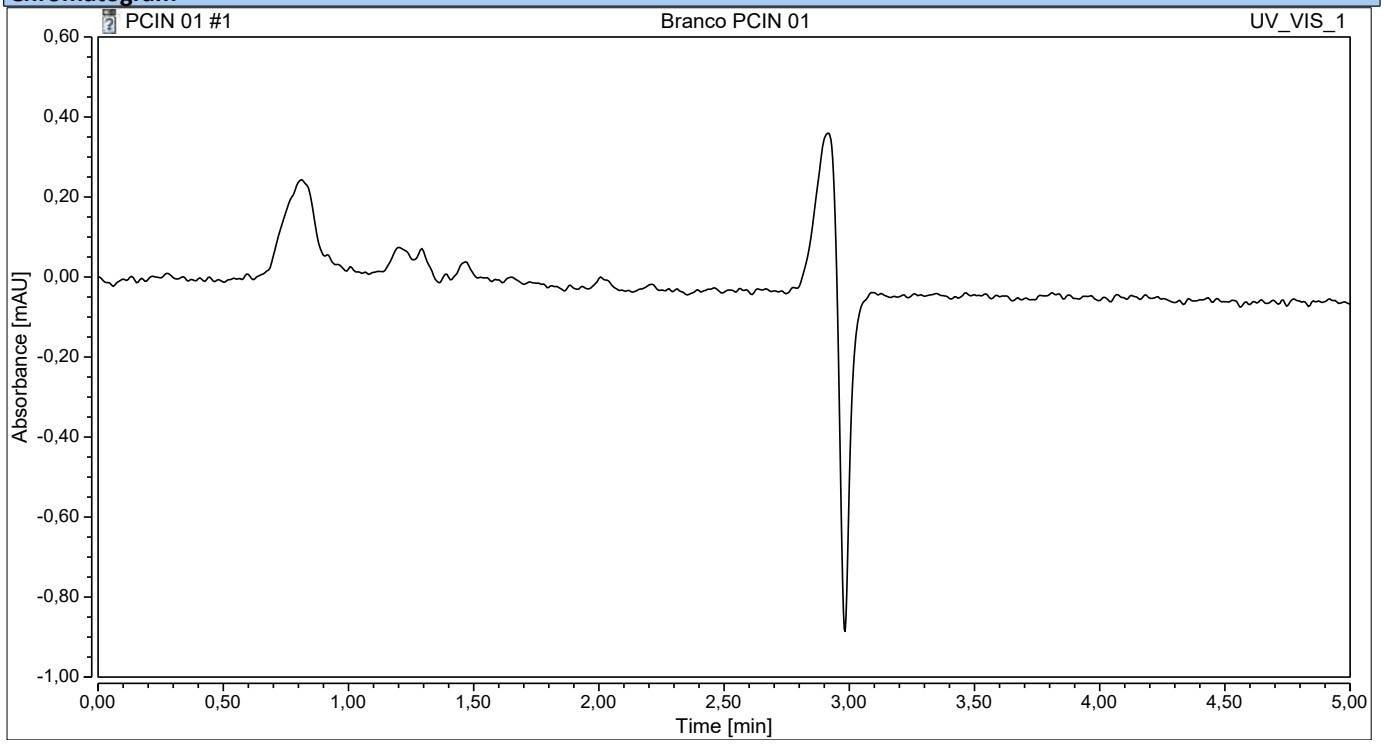

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 16:42**	*Sample Weight:*	**1,0000**

Chromatogram

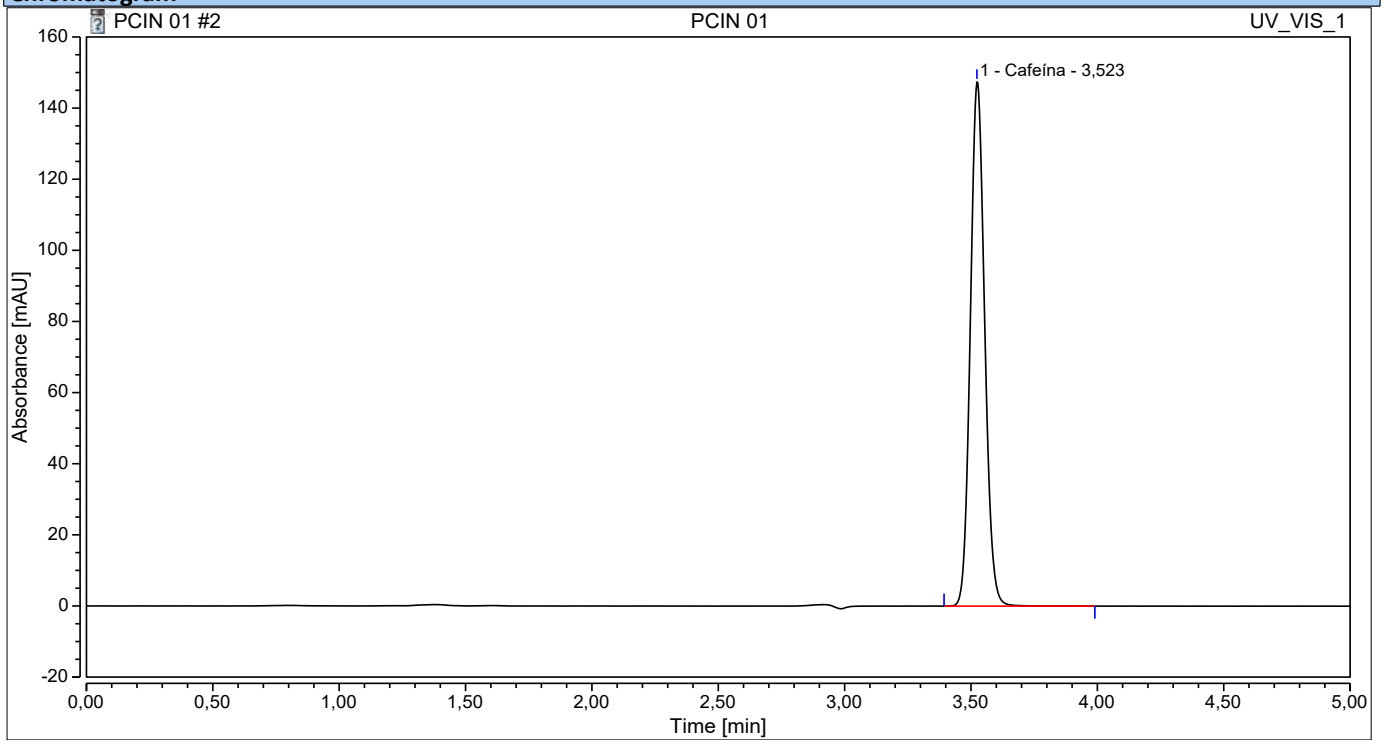

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,6994	147,408	100,00	100,00	n.a.
Total:			**9,699**	**147,408**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 16:48**	*Sample Weight:*	**1,0000**

Chromatogram

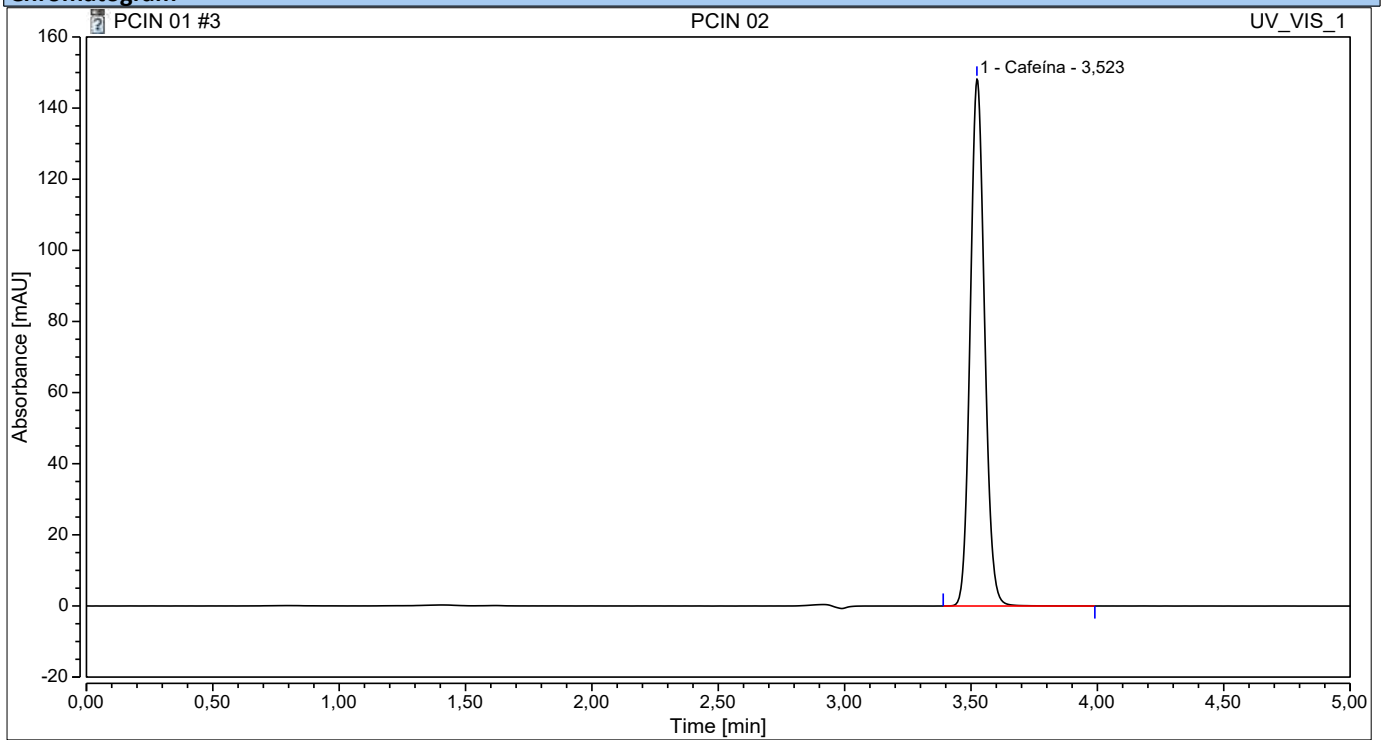

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,7728	148,226	100,00	100,00	n.a.
Total:			**9,773**	**148,226**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 16:54**	*Sample Weight:*	**1,0000**

Chromatogram

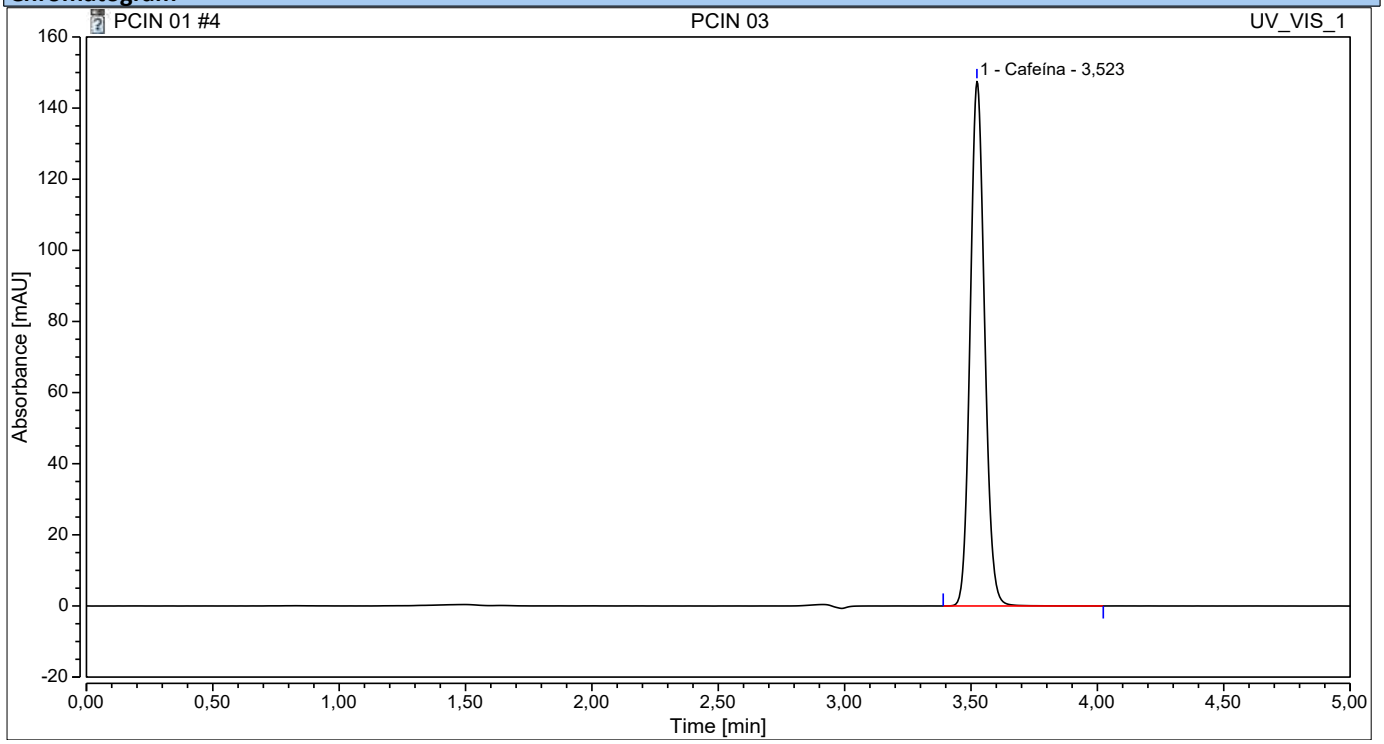

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,7627	147,501	100,00	100,00	n.a.
Total:			**9,763**	**147,501**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**GA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:00**	*Sample Weight:*	**1,0000**

Chromatogram

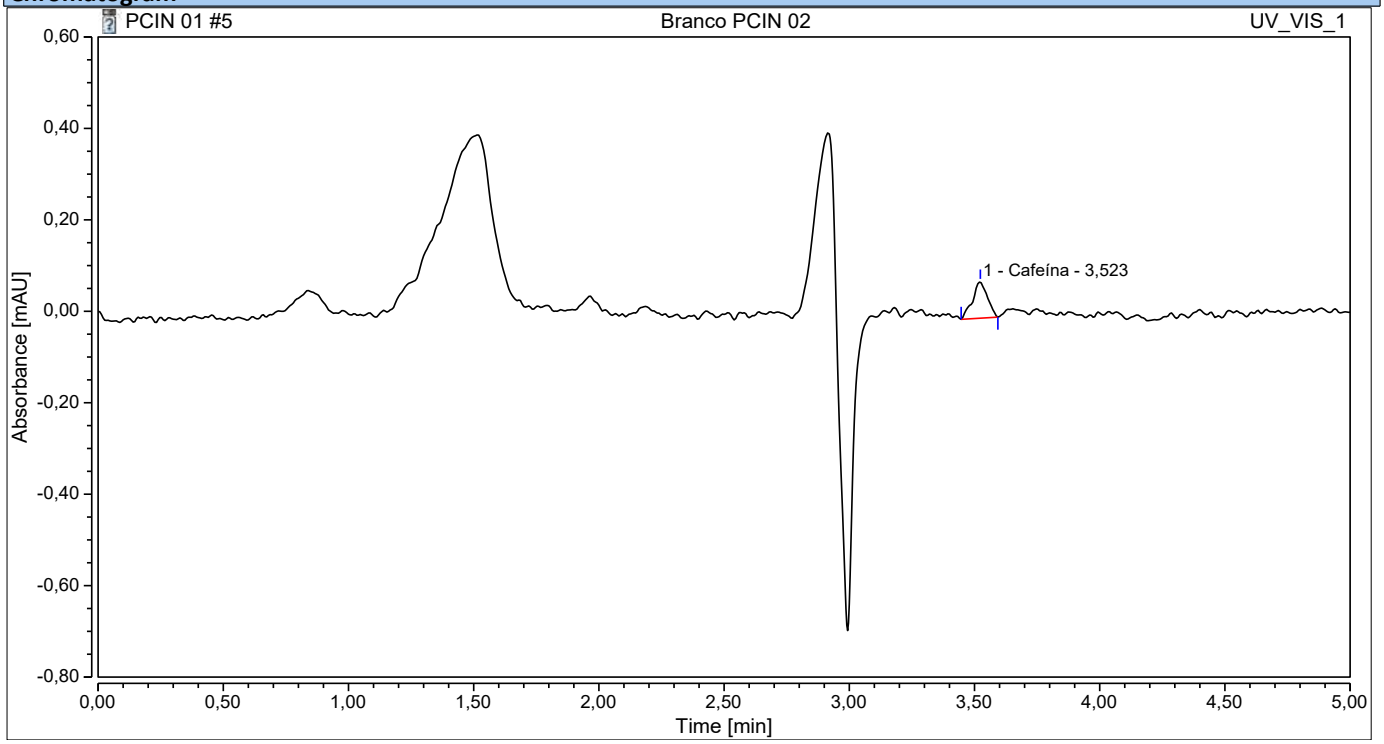

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	0,0055	0,079	100,00	100,00	n.a.
Total:			**0,005**	**0,079**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:06**	*Sample Weight:*	**1,0000**

Chromatogram

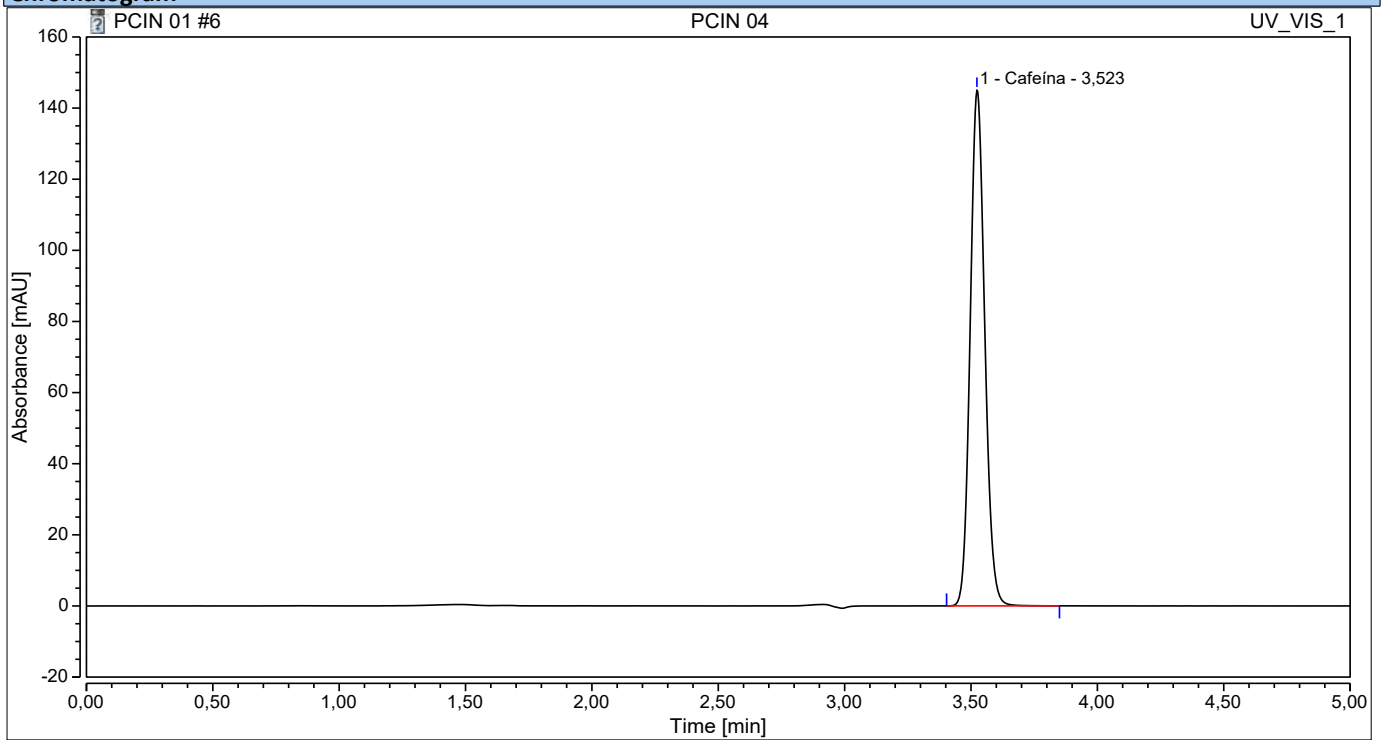

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,6818	145,065	100,00	100,00	n.a.
Total:			**9,682**	**145,065**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:12**	*Sample Weight:*	**1,0000**

Chromatogram

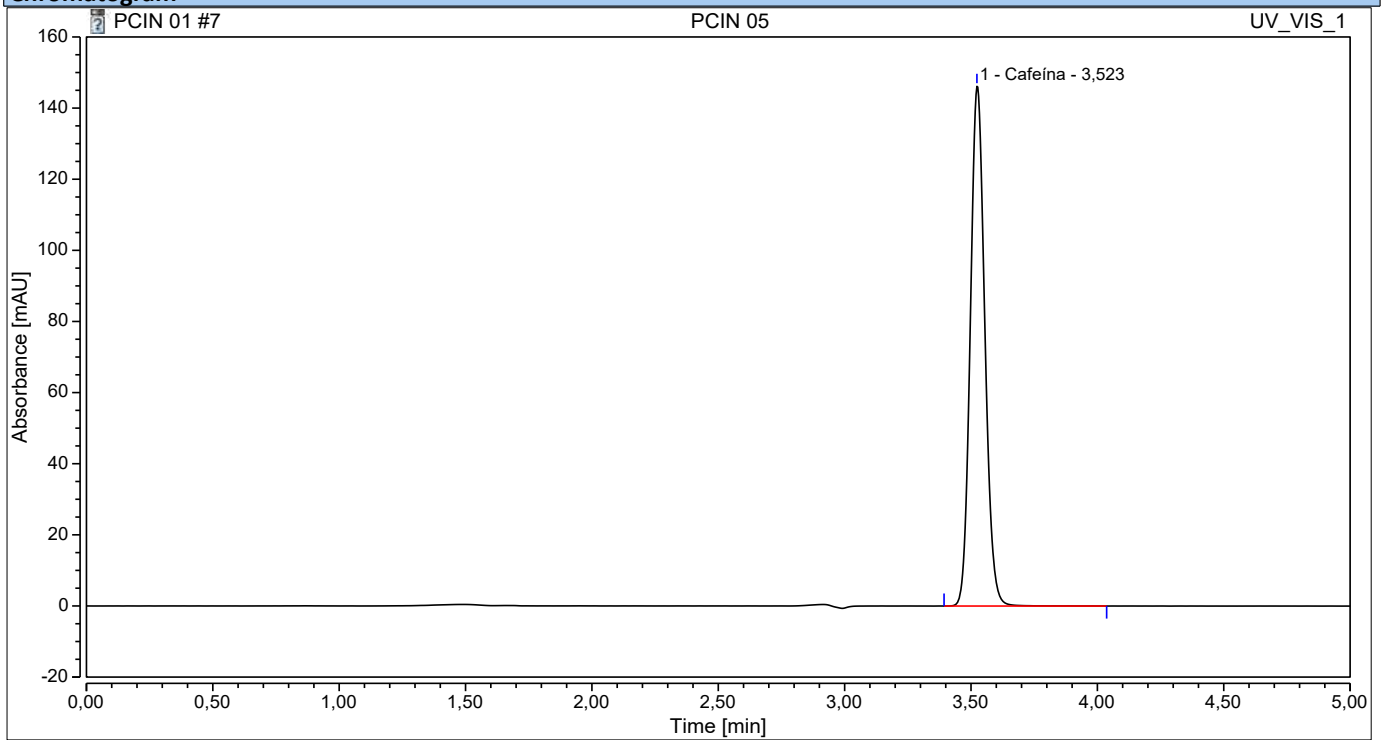

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,7413	146,144	100,00	100,00	n.a.
Total:			**9,741**	**146,144**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**5,00**
Vial Number:	**GA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:17**	*Sample Weight:*	**1,0000**

Chromatogram

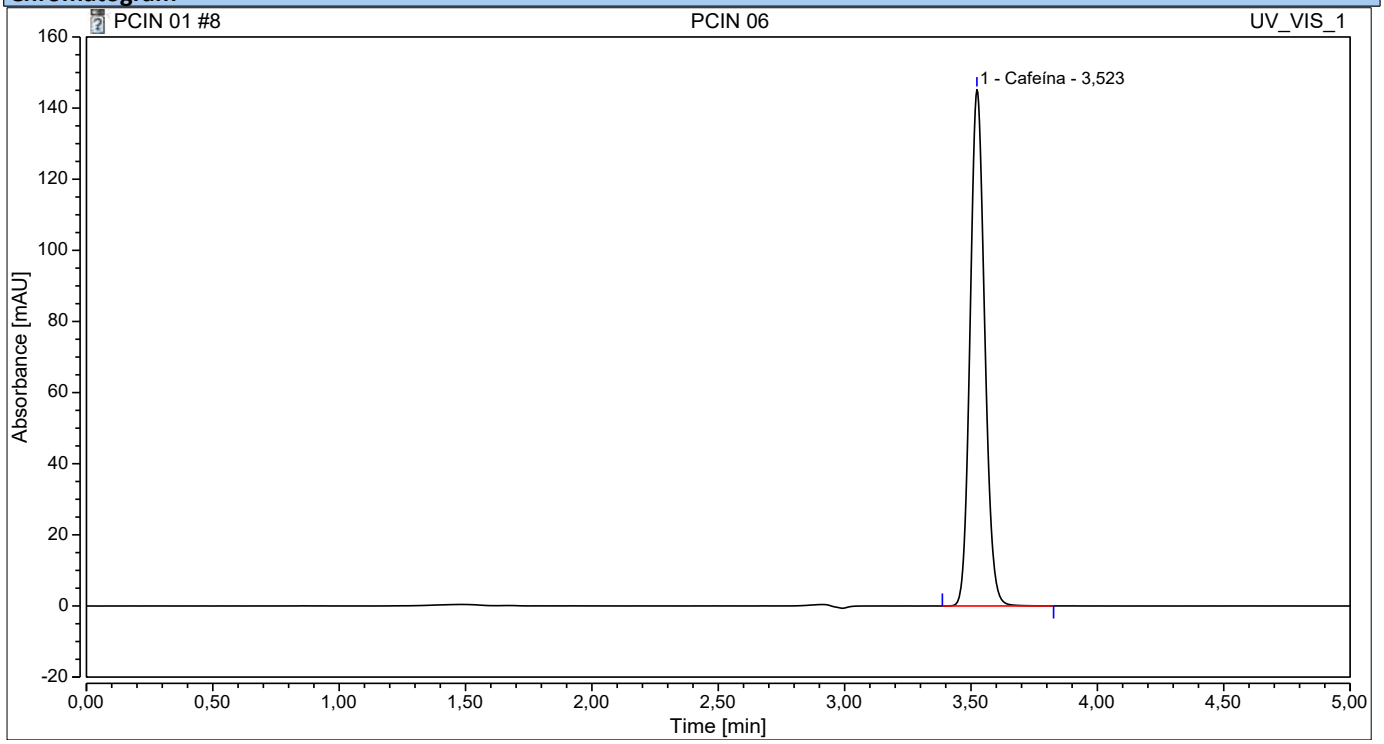

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,7334	145,197	100,00	100,00	n.a.
Total:			**9,733**	**145,197**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**GA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:23**	*Sample Weight:*	**1,0000**

Chromatogram

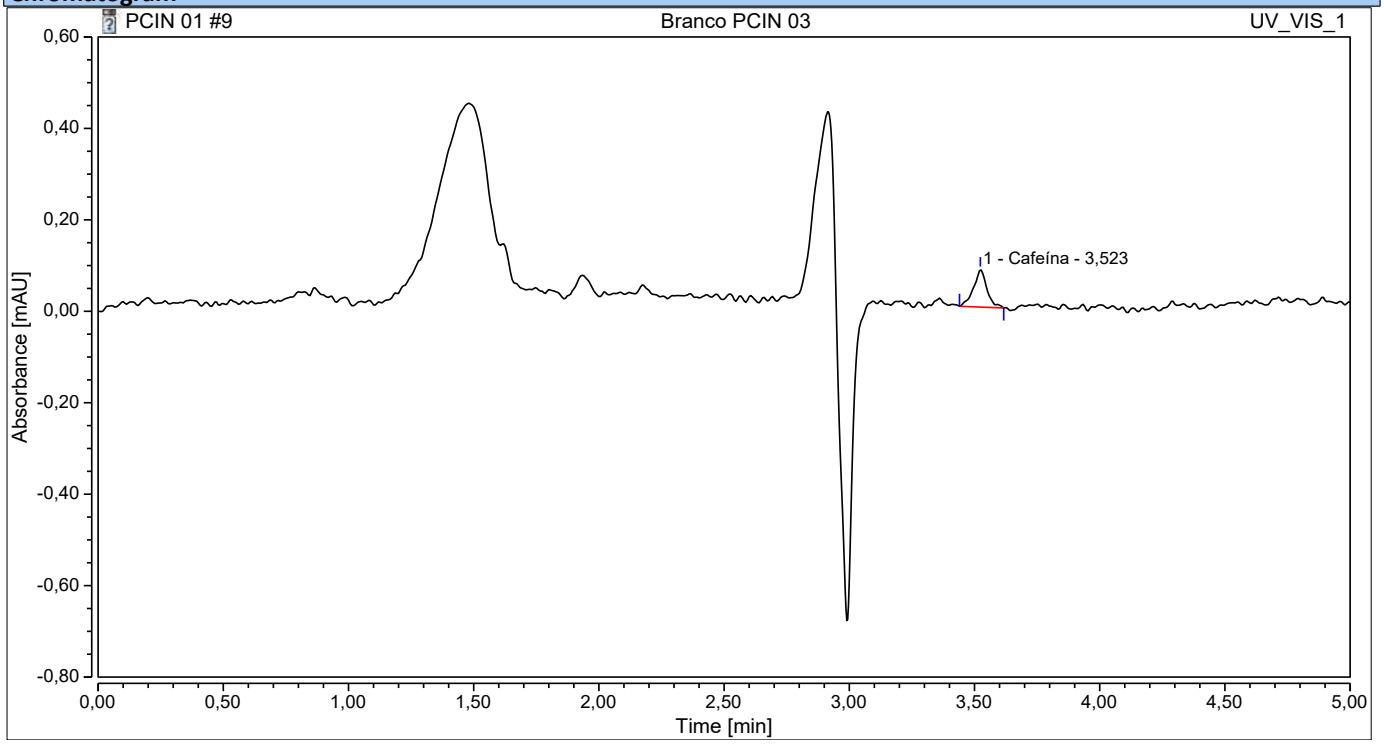

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	0,0051	0,082	100,00	100,00	n.a.
Total:			**0,005**	**0,082**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**4,50**
Vial Number:	**GA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:29**	*Sample Weight:*	**1,0000**

Chromatogram

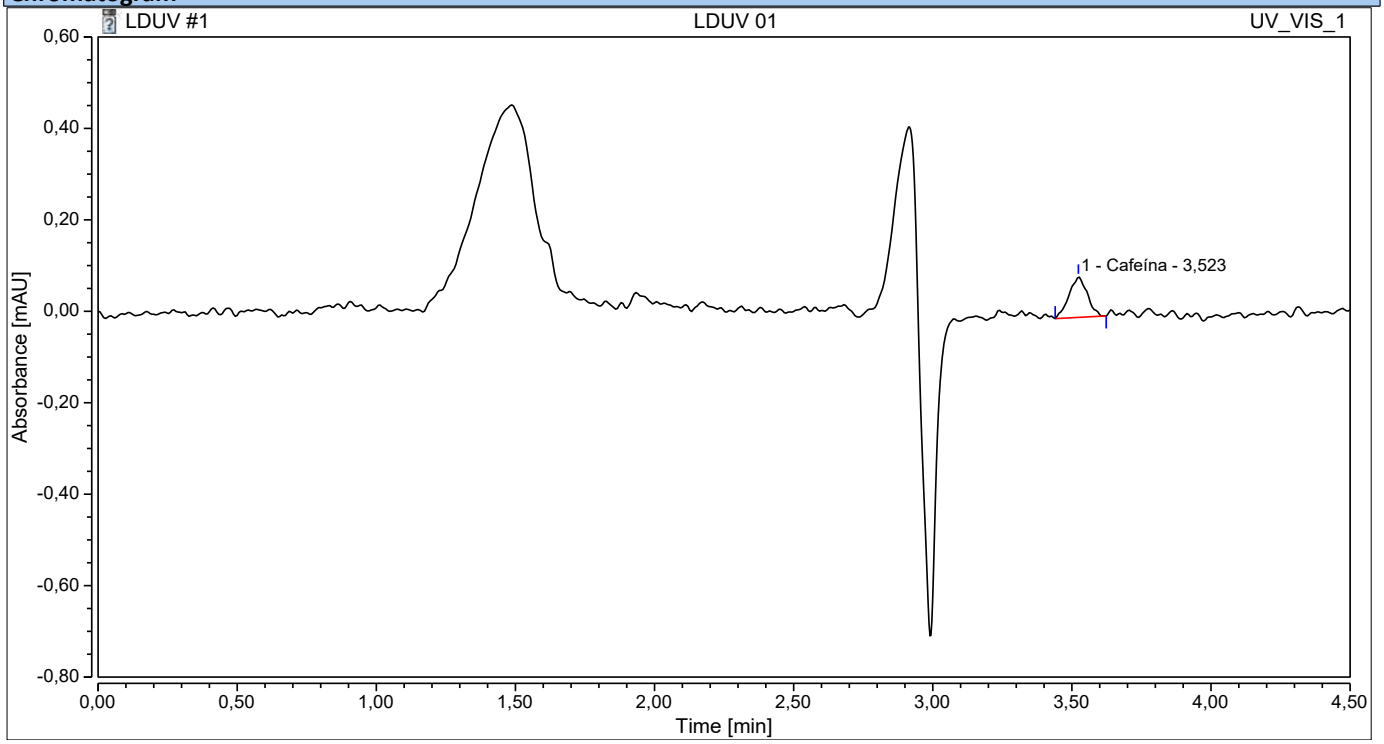

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	0,0068	0,089	100,00	100,00	n.a.
Total:			**0,007**	**0,089**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**4,50**
Vial Number:	**GA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:34**	*Sample Weight:*	**1,0000**

Chromatogram

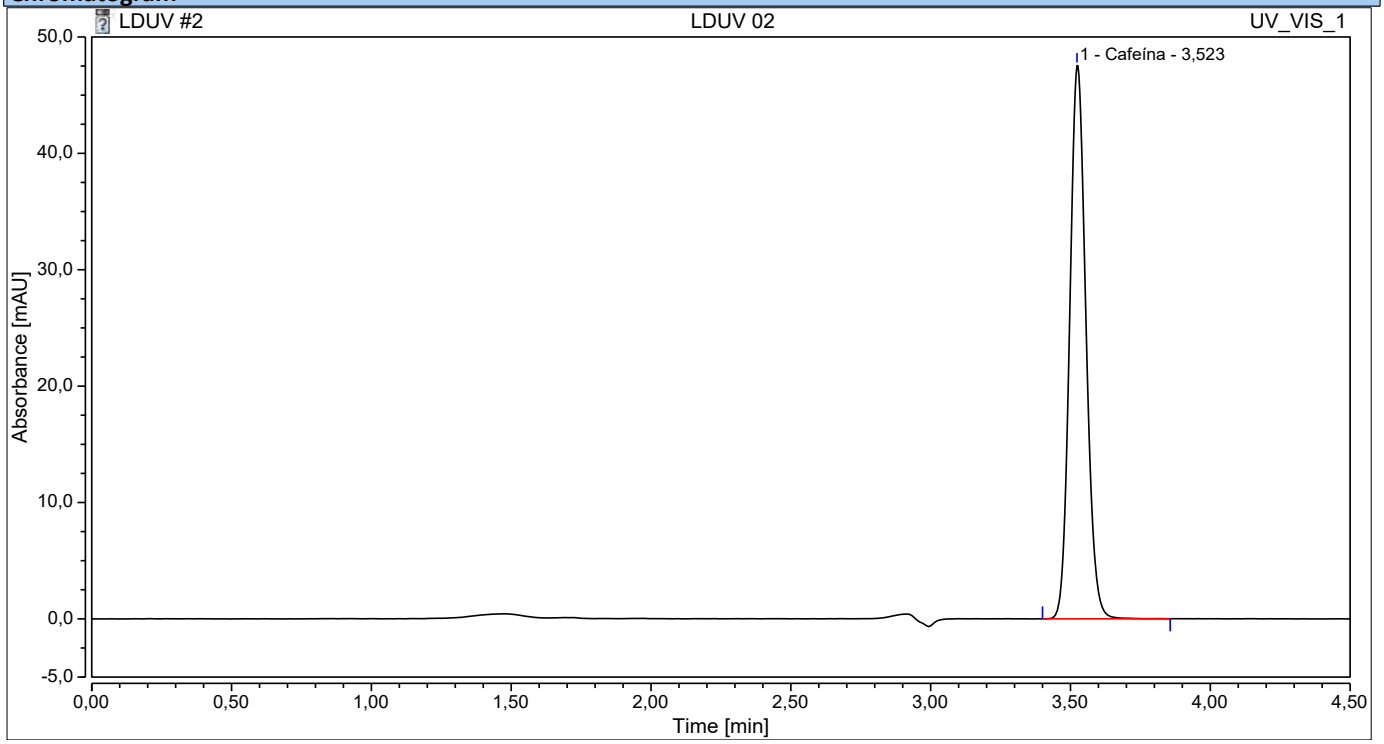

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	3,2029	47,538	100,00	100,00	n.a.
Total:			**3,203**	**47,538**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**4,50**
Vial Number:	**GA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:40**	*Sample Weight:*	**1,0000**

Chromatogram

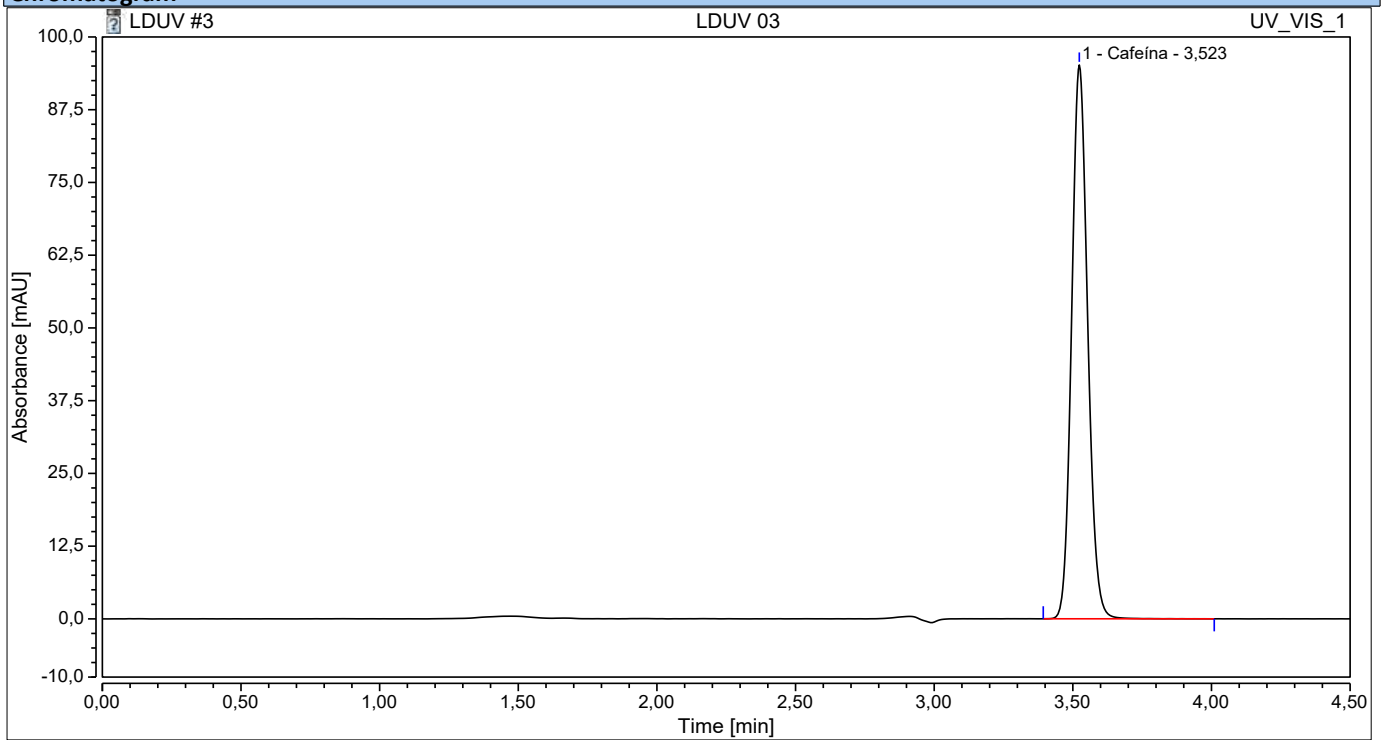

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	6,3834	95,171	100,00	100,00	n.a.
Total:			**6,383**	**95,171**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**4,50**
Vial Number:	**GA7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:45**	*Sample Weight:*	**1,0000**

Chromatogram

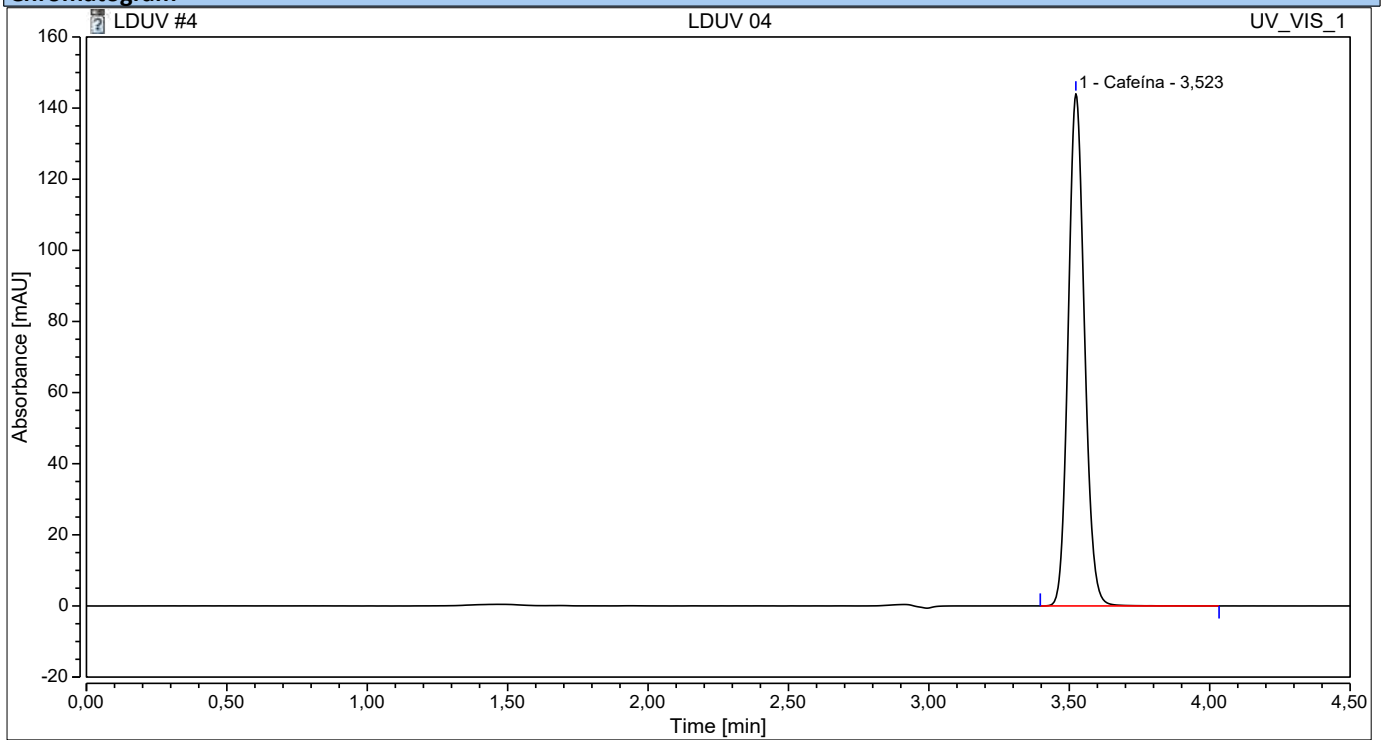

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,6686	144,025	100,00	100,00	n.a.
Total:			**9,669**	**144,025**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**4,50**
Vial Number:	**GA8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:50**	*Sample Weight:*	**1,0000**

Chromatogram

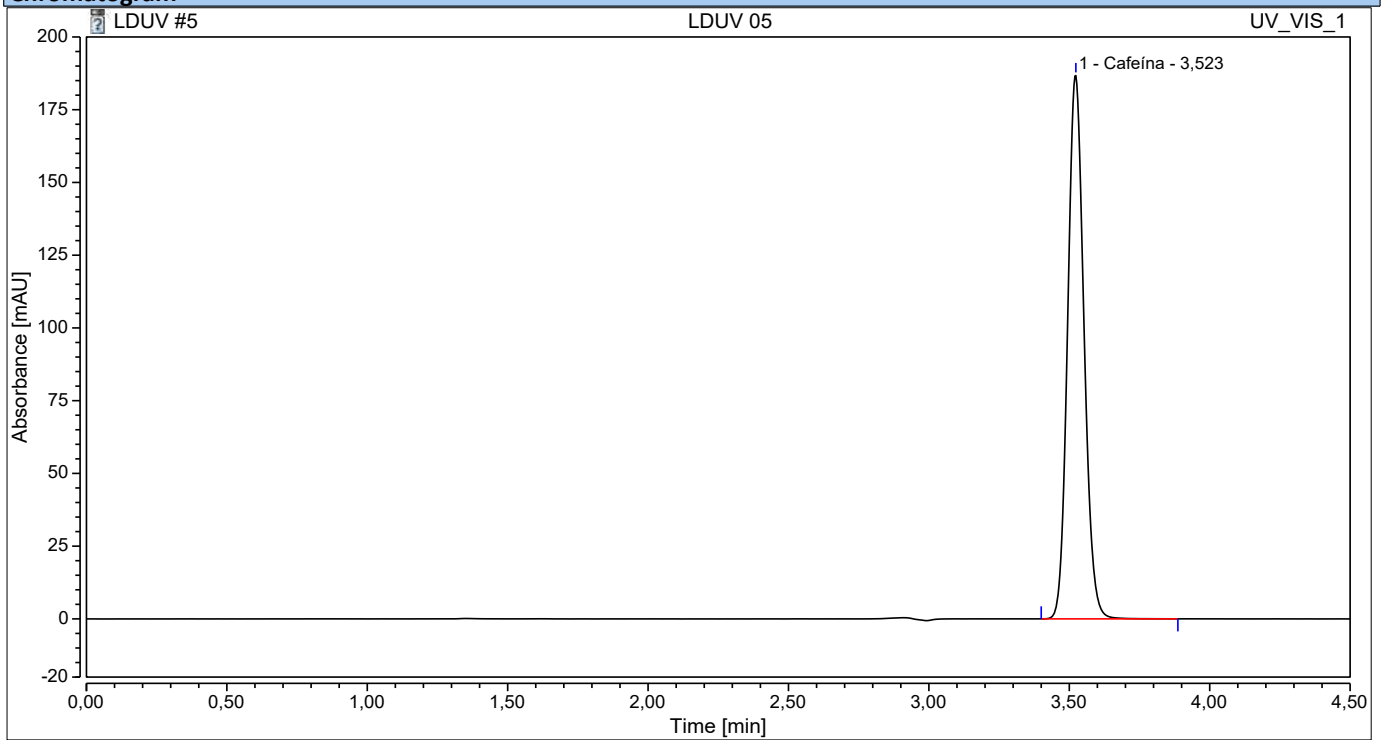

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	12,6016	186,745	100,00	100,00	n.a.
Total:			**12,602**	**186,745**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**4,50**
Vial Number:	**GB1**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 17:56**	*Sample Weight:*	**1,0000**

Chromatogram

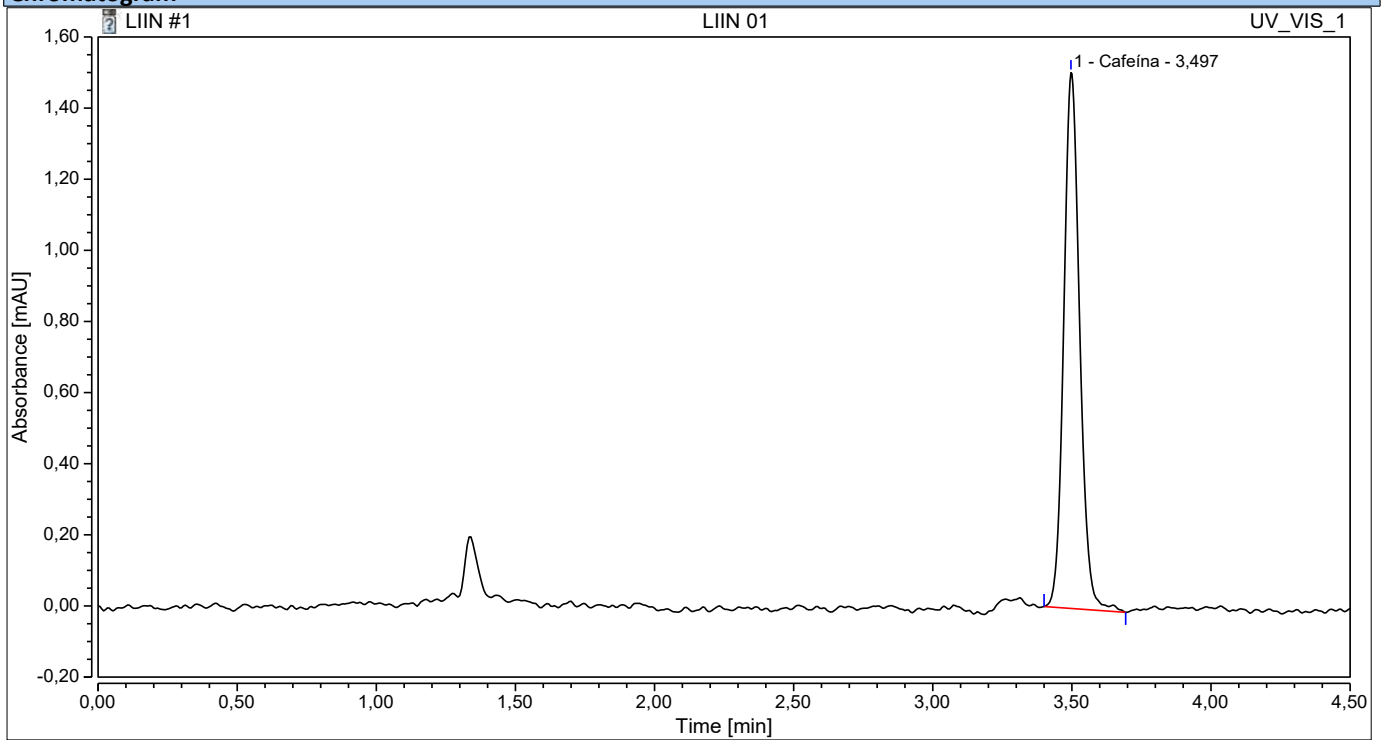

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,497	0,1003	1,507	100,00	100,00	n.a.
Total:			**0,100**	**1,507**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**4,50**
Vial Number:	**GB1**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 18:01**	*Sample Weight:*	**1,0000**

Chromatogram

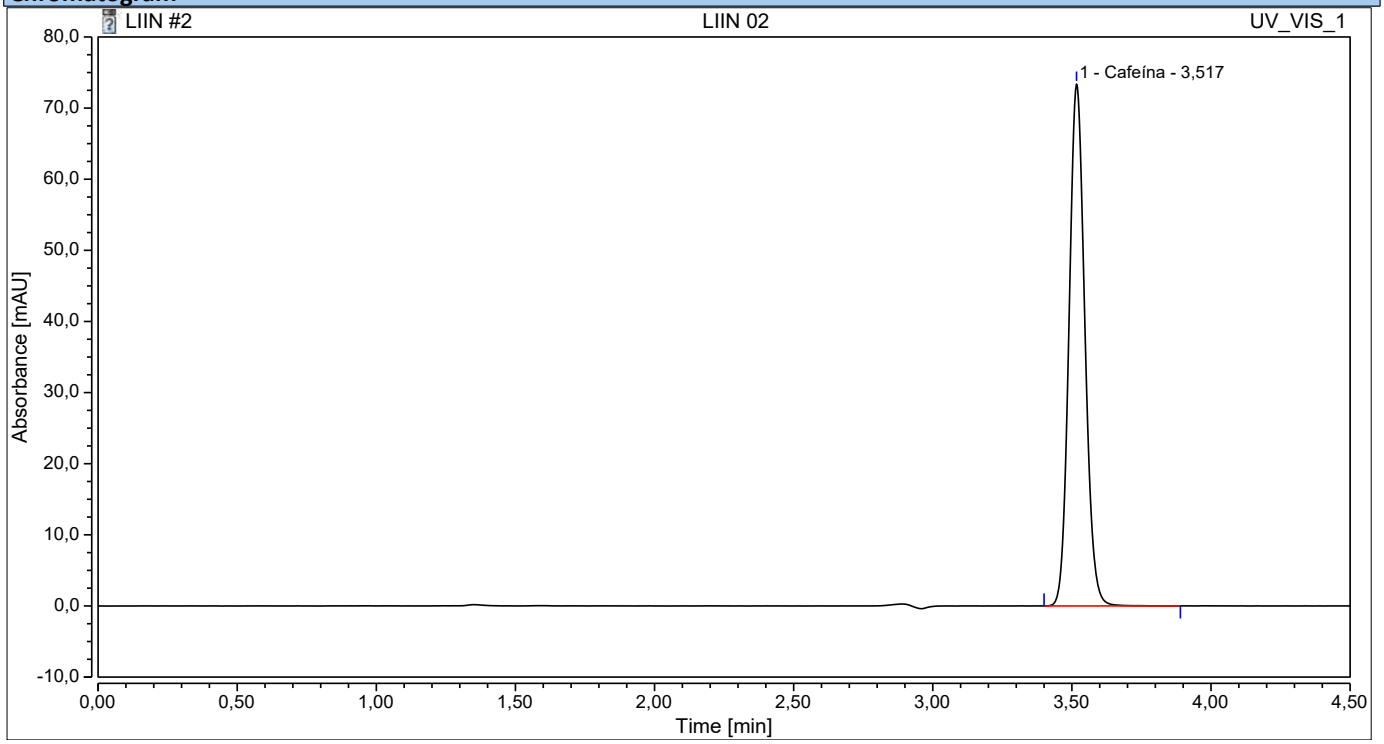

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,517	4,8462	73,375	100,00	100,00	n.a.
Total:			**4,846**	**73,375**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**4,50**
Vial Number:	**GB1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 18:06**	*Sample Weight:*	**1,0000**

Chromatogram

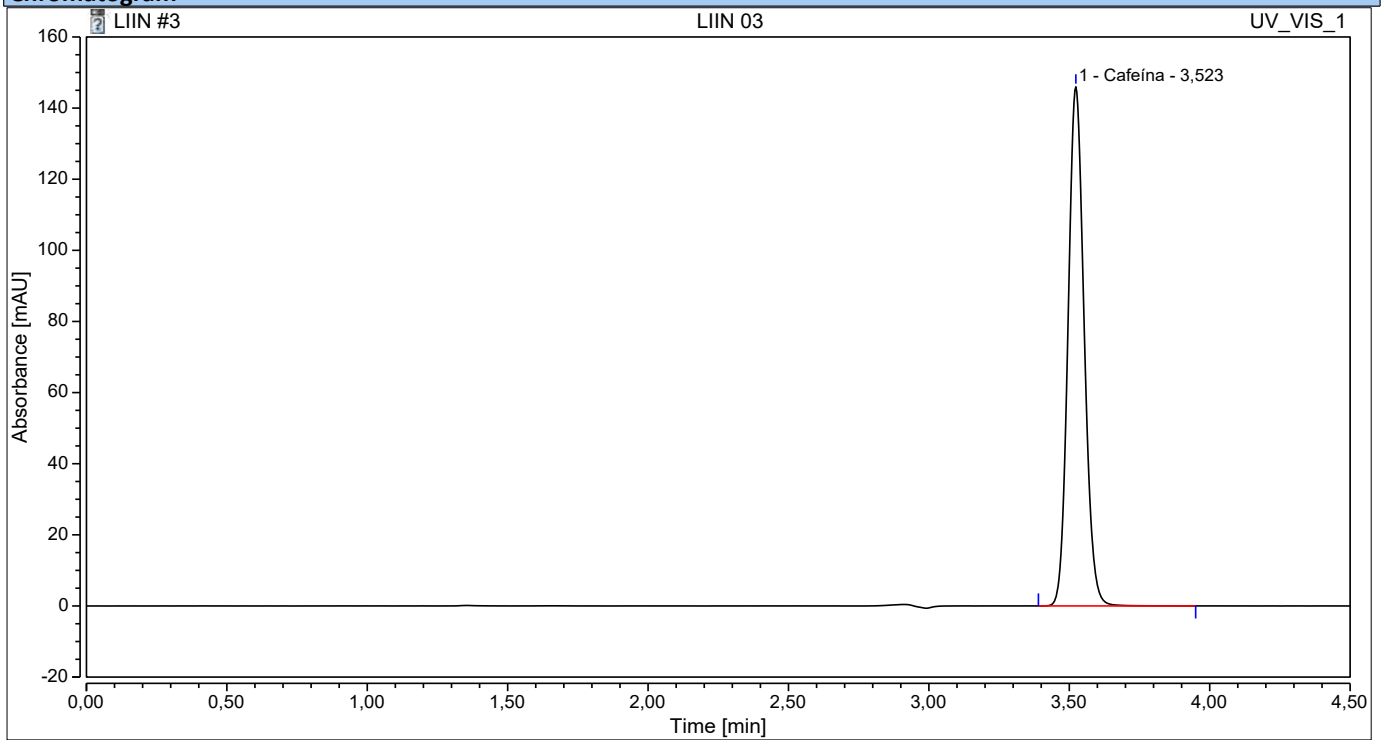

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,523	9,7014	145,984	100,00	100,00	n.a.
Total:			**9,701**	**145,984**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**4,50**
Vial Number:	**GB1**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 18:12**	*Sample Weight:*	**1,0000**

Chromatogram

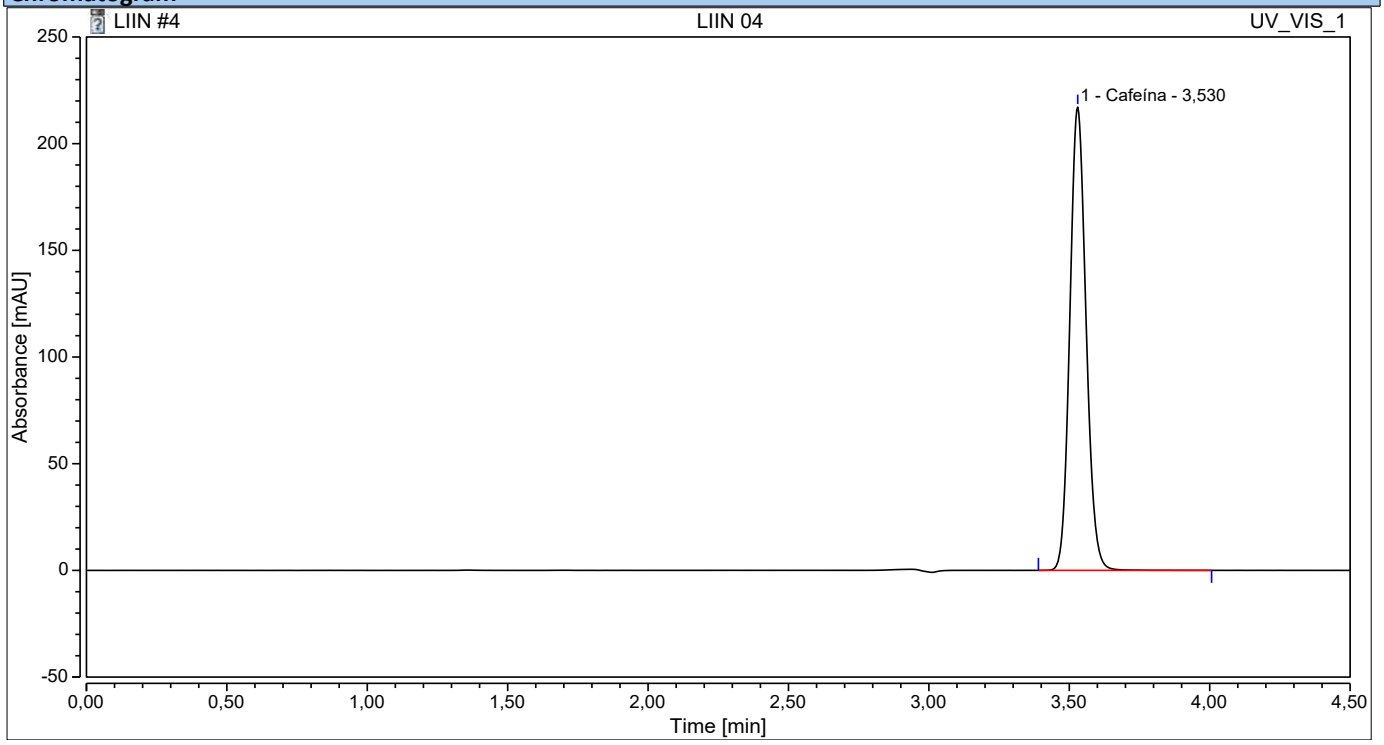

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,530	14,5574	217,101	100,00	100,00	n.a.
Total:			**14,557**	**217,101**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**4,50**
Vial Number:	**GB1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**02/set/26 18:17**	*Sample Weight:*	**1,0000**

Chromatogram

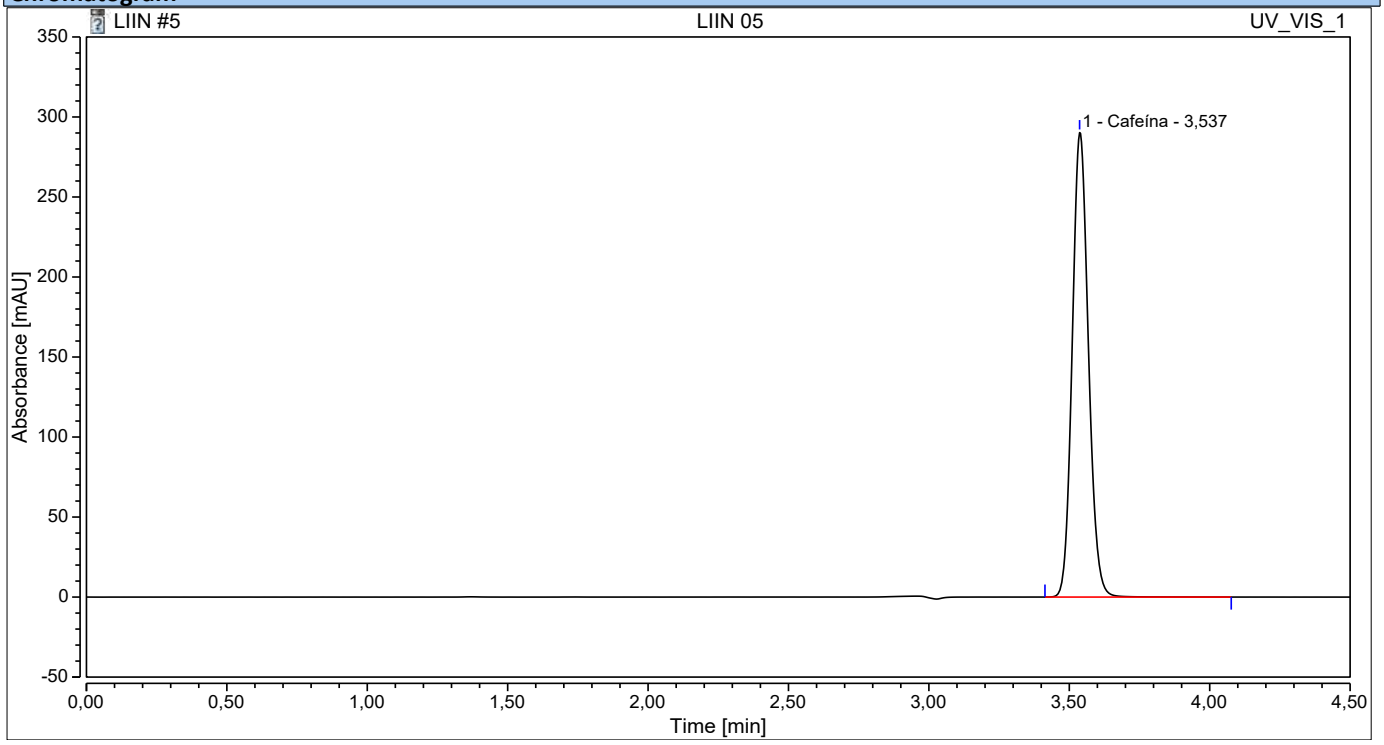

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,537	19,3791	290,252	100,00	100,00	n.a.
Total:			**19,379**	**290,252**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB**	*Run Time (min):*	**20,00**
Vial Number:	**GA2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 10:05**	*Sample Weight:*	**1,0000**

Chromatogram

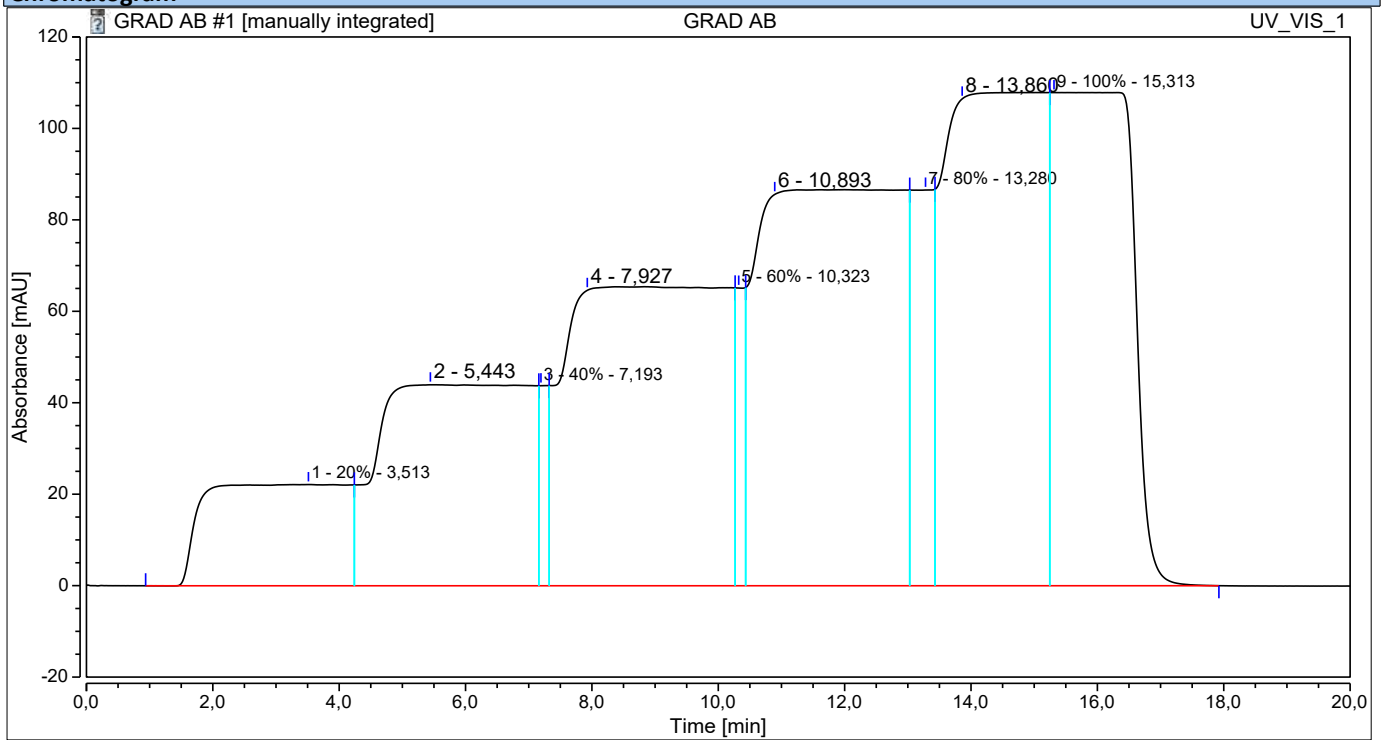

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	20%	3,513	56,2482	22,140	5,76	3,54	n.a.
3	40%	7,193	7,1485	43,757	0,73	6,99	n.a.
5	60%	10,323	10,8528	65,115	1,11	10,40	n.a.
7	80%	13,280	34,6170	86,550	3,54	13,82	n.a.
9	100%	15,313	152,4251	107,865	15,61	17,23	n.a.
Total:			**261,292**	**325,427**	**26,756**	**51,980**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD CD**	*Run Time (min):*	**20,00**
Vial Number:	**GA2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD HPLC 03**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 10:36**	*Sample Weight:*	**1,0000**

Chromatogram

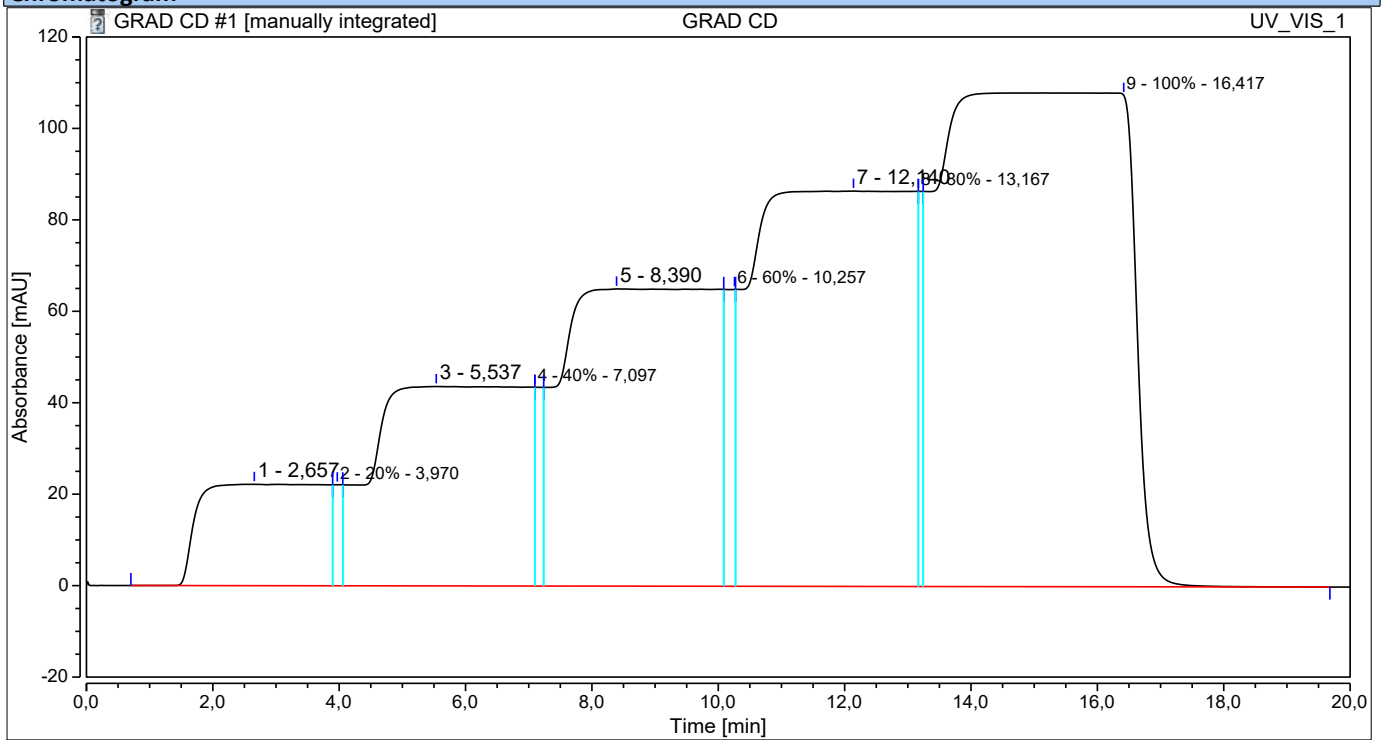

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	3,970	3,5346	22,102	0,36	4,08	n.a.
4	40%	7,097	6,0843	43,481	0,62	8,03	n.a.
6	60%	10,257	12,1153	64,929	1,24	11,99	n.a.
8	80%	13,167	6,6252	86,427	0,68	15,95	n.a.
9	100%	16,417	360,2025	107,519	36,94	19,85	n.a.
Total:			**388,562**	**324,459**	**39,853**	**59,895**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.