
Spectral Library Screening Results

Injection Details

Injection Name:	**EDUV**	*Run Time (min):*	**4,50**
Vial Number:	**BA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 16:37**	*Sample Weight:*	**1,0000**

UV Spectra — Cafeína

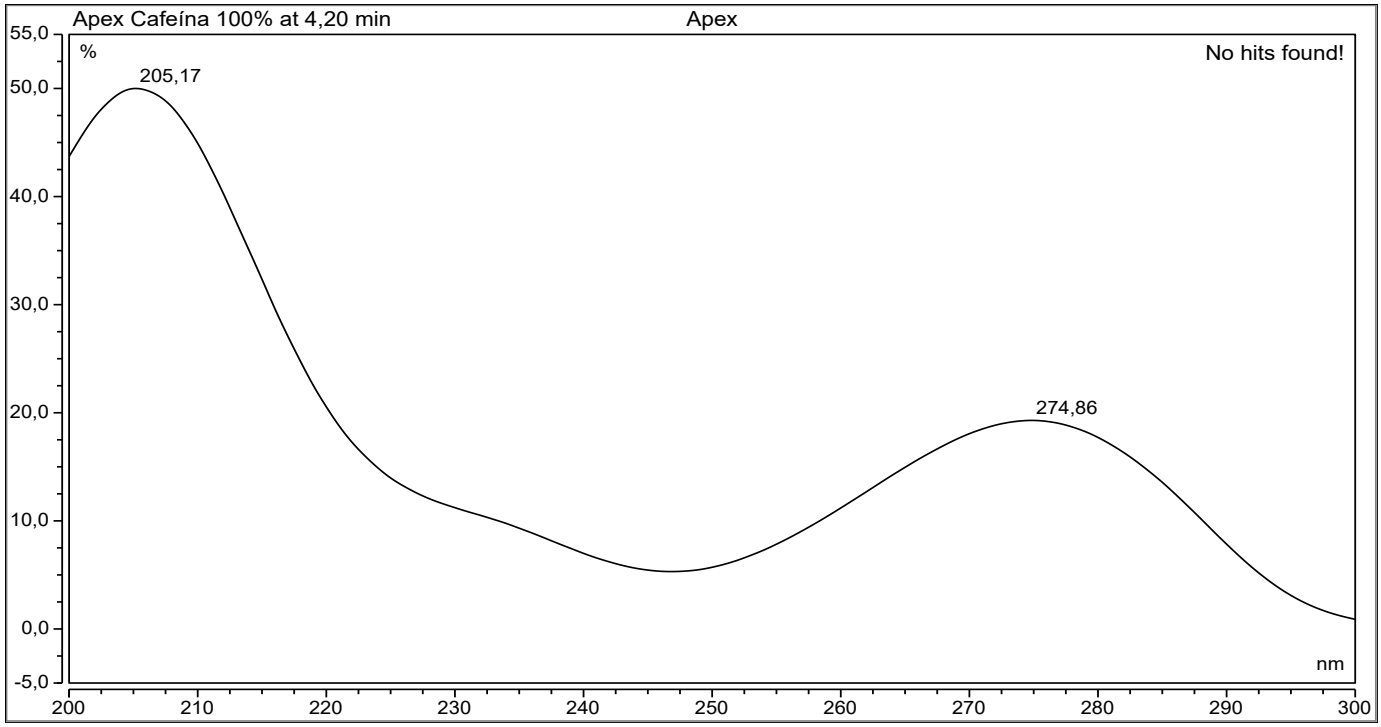


Spectral Library Screening Results

	Hit# 1		Hit# 2		Hit# 3	
Library:	n.a.		n.a.		n.a.	
Component:	n.a.		n.a.		n.a.	
Match Factor:		n.a.		n.a.		n.a.
Ret.Time:		n.a.		n.a.		n.a.
Origin:						
Acq.Date:	n.a.		n.a.		n.a.	
Instrument Method:	n.a.		n.a.		n.a.	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Contour Spectral View

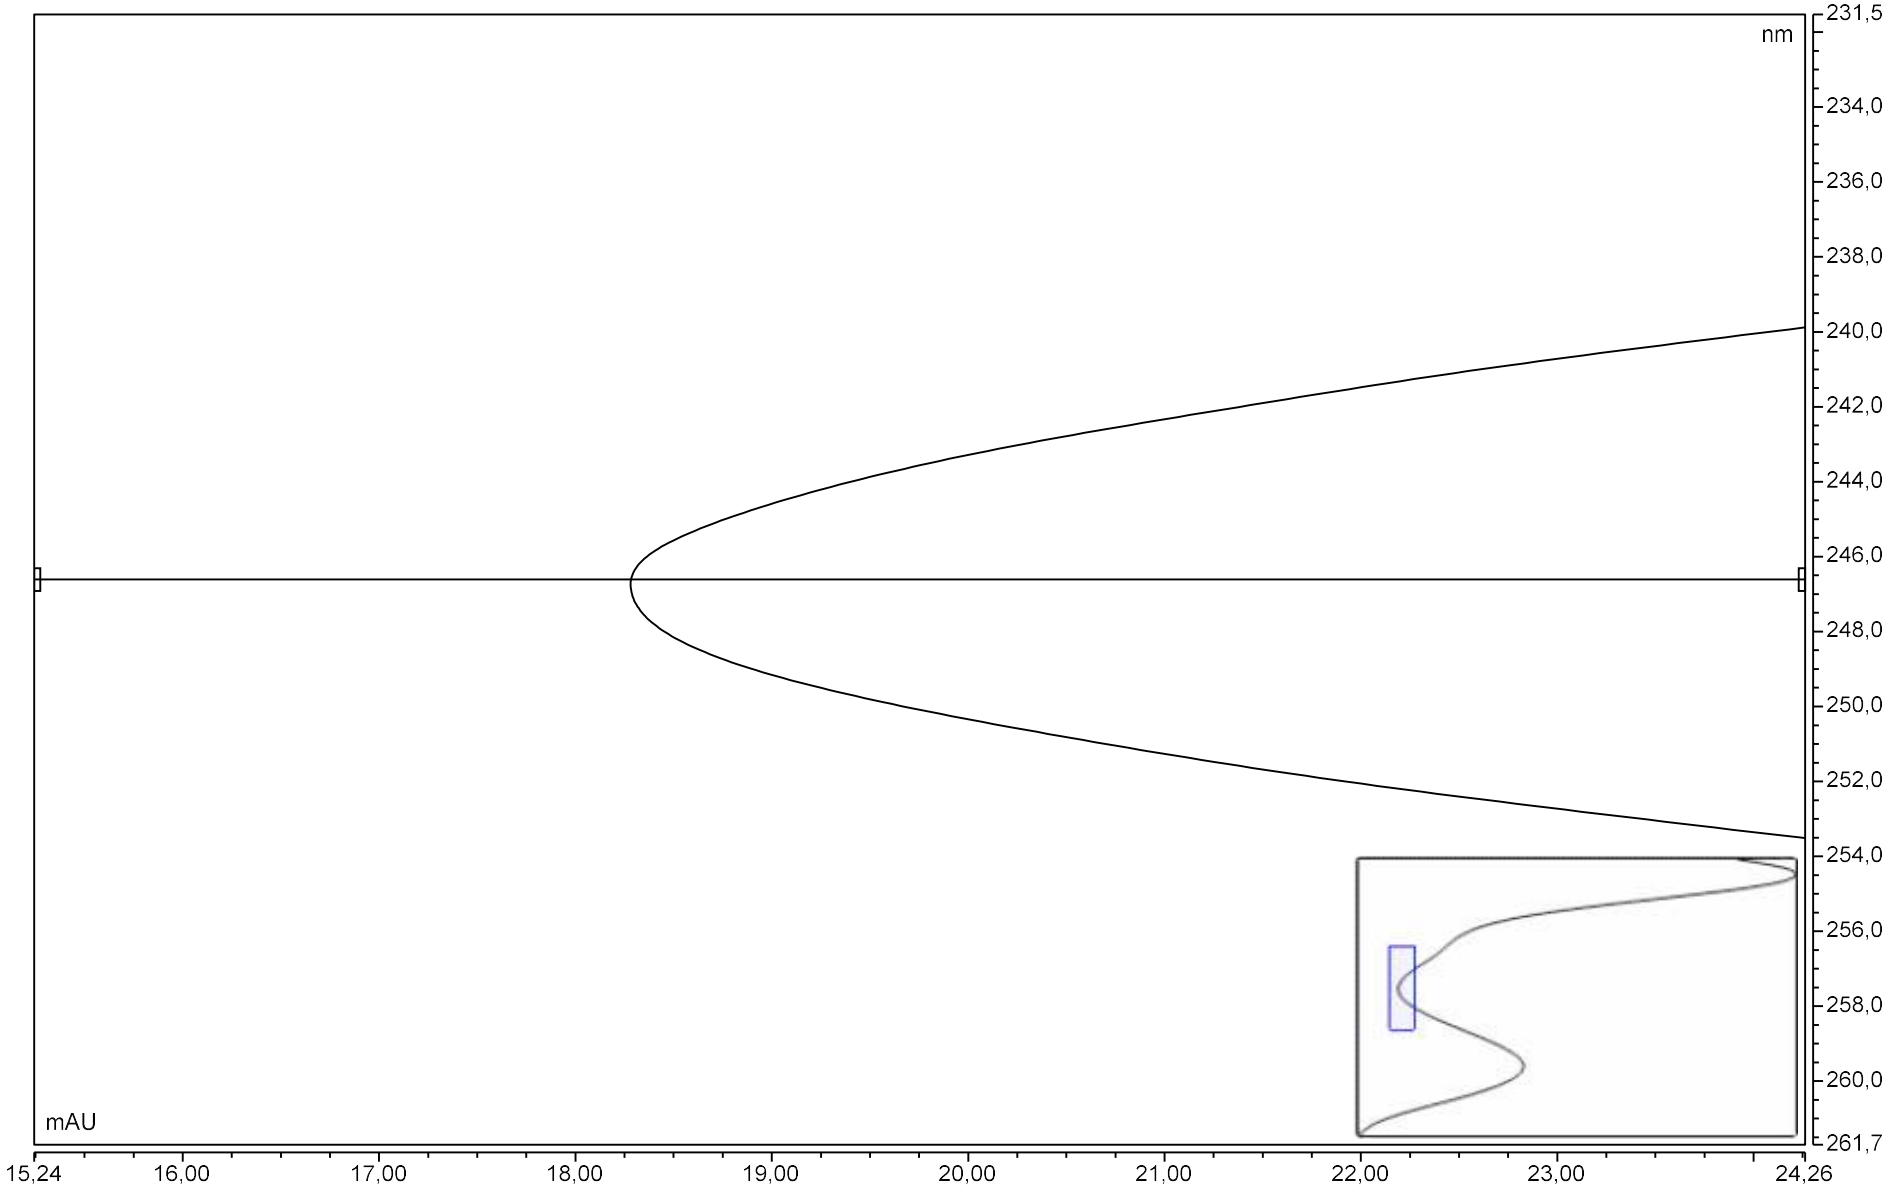


Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:03**	*Sample Weight:*	**1,0000**

Chromatogram

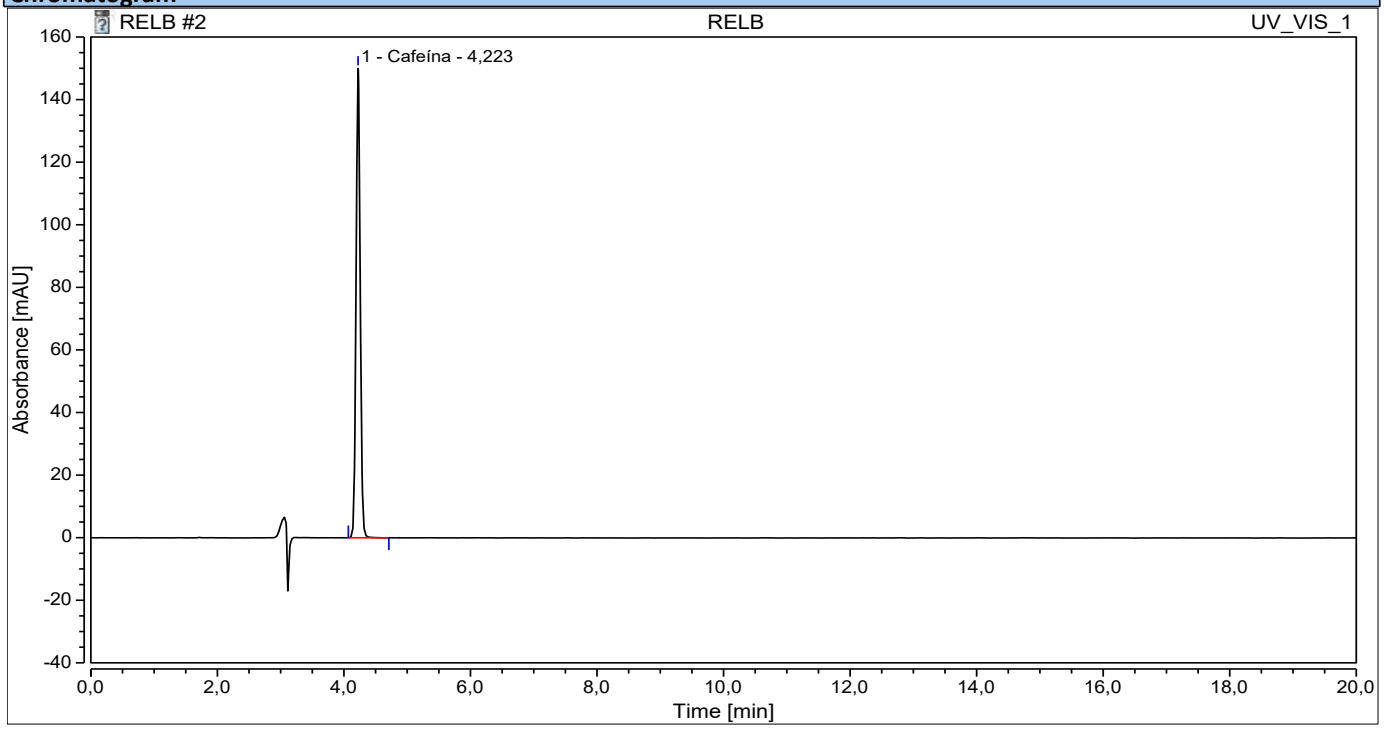

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,223	11,4140	150,000	100,00	100,00	n.a.
Total:			**11,414**	**150,000**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:03**	*Sample Weight:*	**1,0000**

Chromatogram

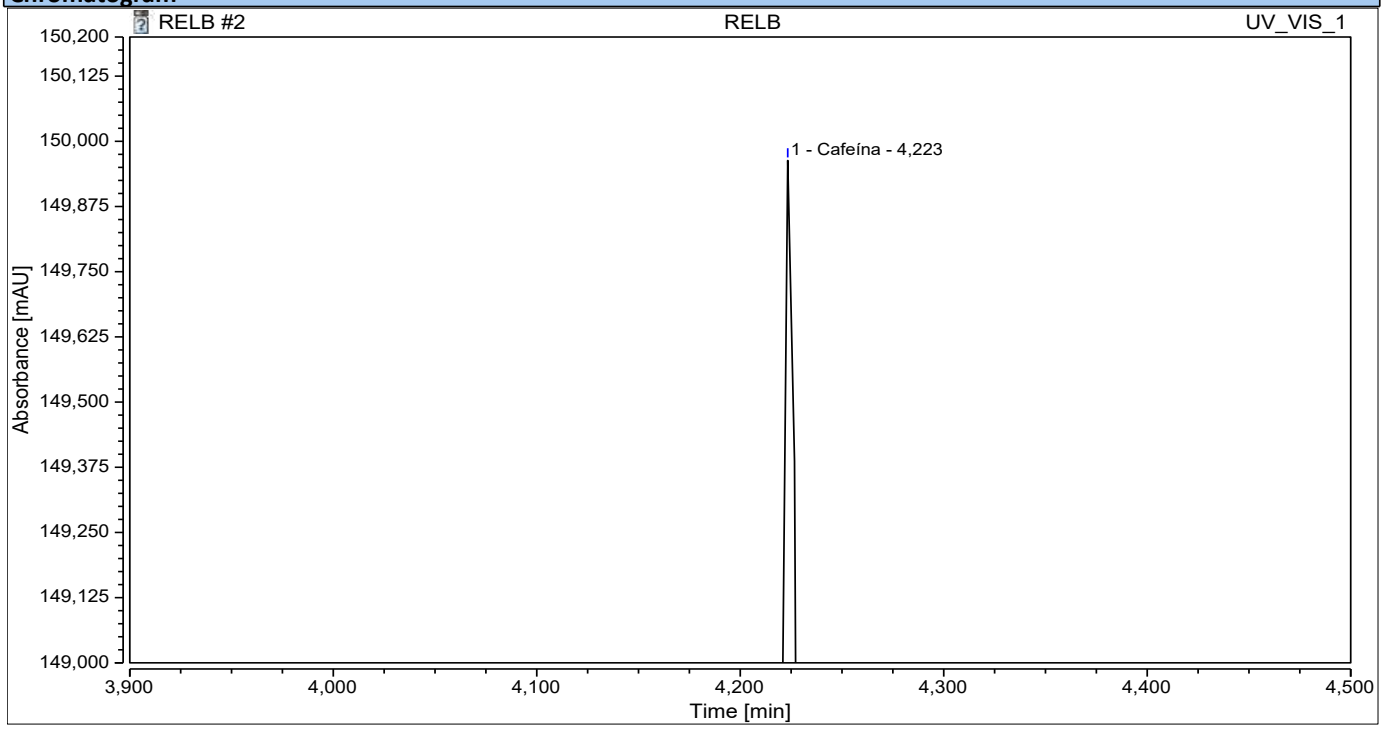

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,223	11,4140	150,000	100,00	100,00	n.a.
Total:			**11,414**	**150,000**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:03**	*Sample Weight:*	**1,0000**

Chromatogram

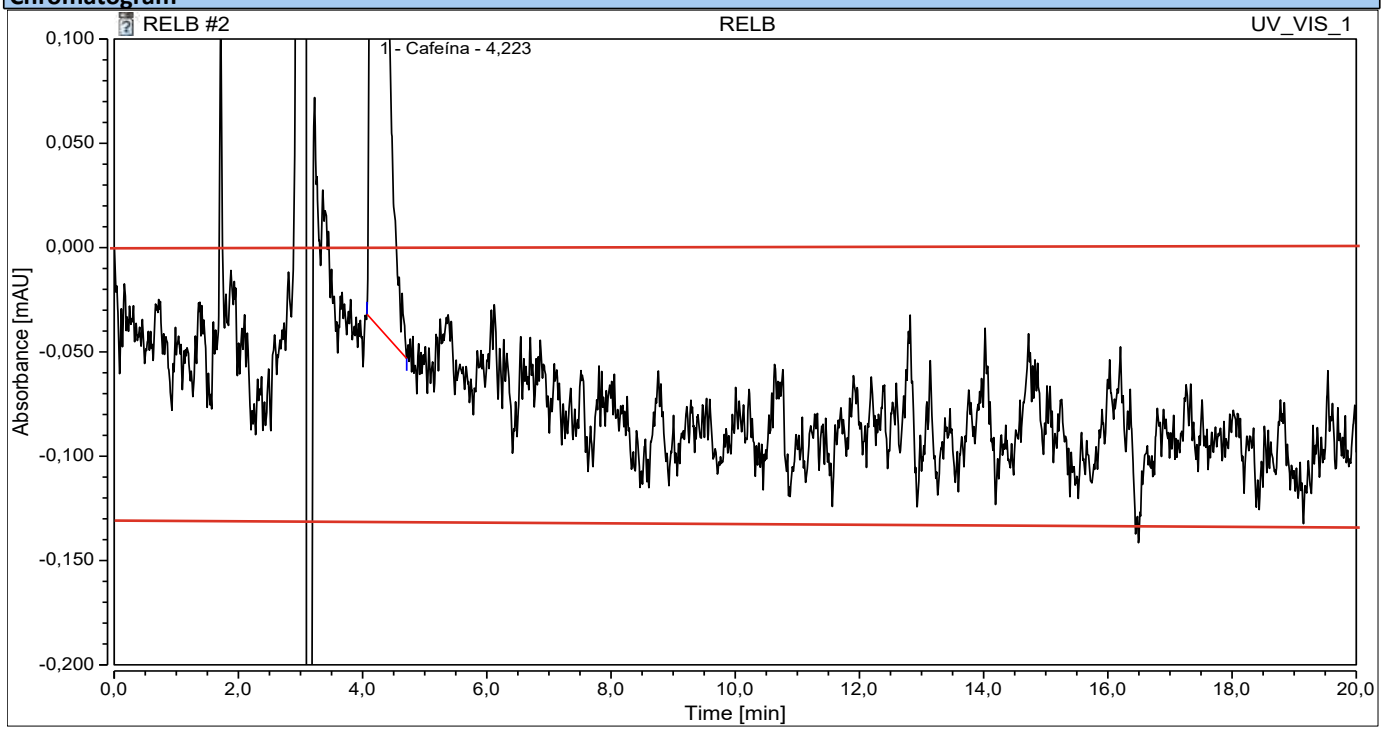

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,223	11,4140	150,000	100,00	100,00	n.a.
Total:			**11,414**	**150,000**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB**	*Run Time (min):*	**20,00**
Vial Number:	**BB2**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:03**	*Sample Weight:*	**1,0000**

Chromatogram

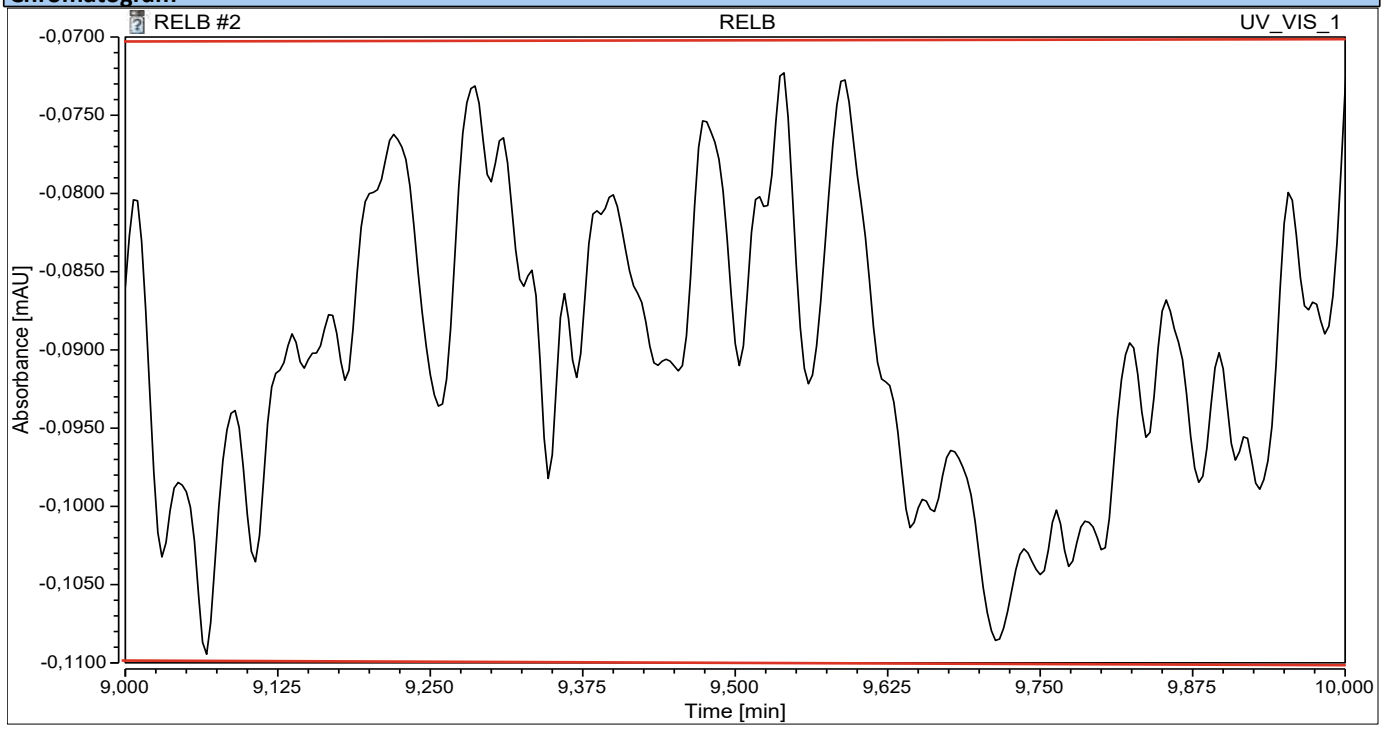

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,223	11,4140	150,000	100,00	100,00	n.a.
Total:			**11,414**	**150,000**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**4,50**
Vial Number:	**BA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:45**	*Sample Weight:*	**1,0000**

Chromatogram

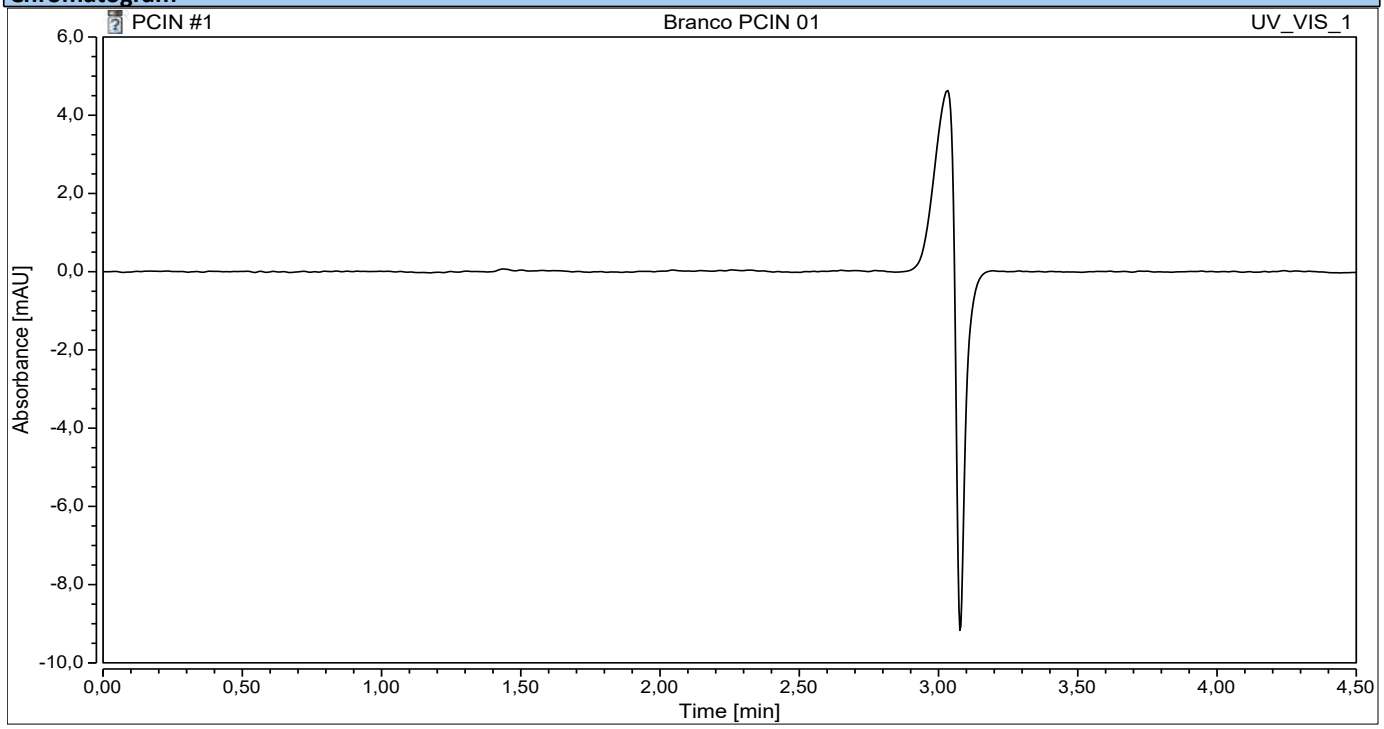

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:51**	*Sample Weight:*	**1,0000**

Chromatogram

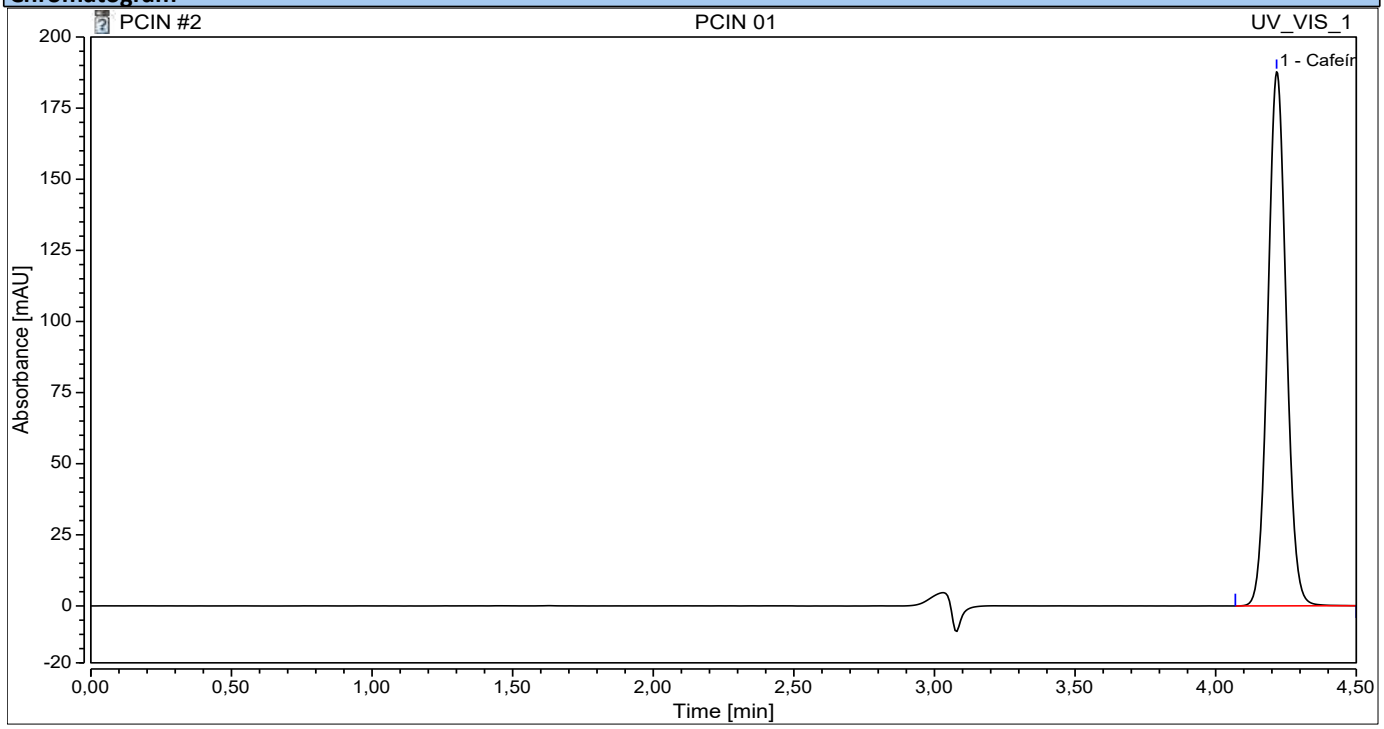

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,217	14,2742	187,766	100,00	100,00	n.a.
Total:			**14,274**	**187,766**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 17:56**	*Sample Weight:*	**1,0000**

Chromatogram

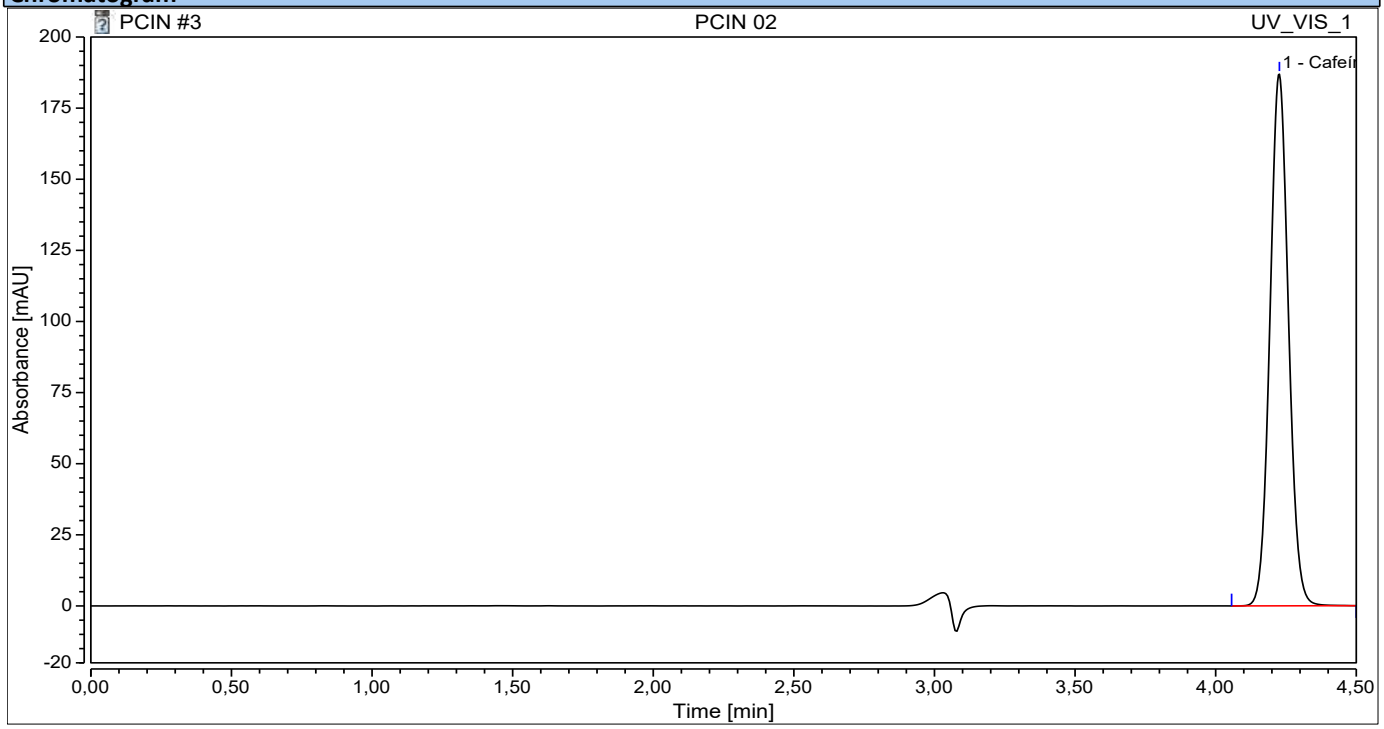

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,227	14,2812	186,920	100,00	100,00	n.a.
Total:			**14,281**	**186,920**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:01**	*Sample Weight:*	**1,0000**

Chromatogram

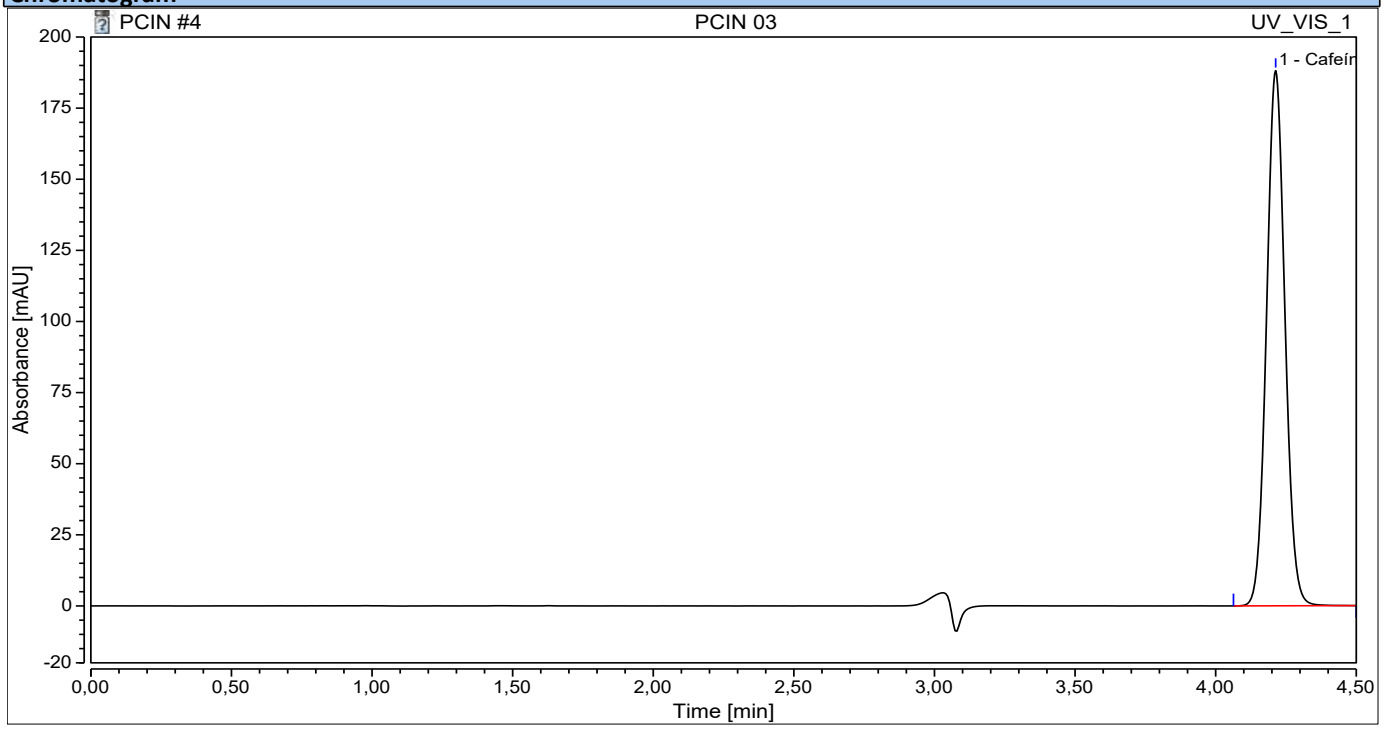

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,213	14,2670	188,150	100,00	100,00	n.a.
Total:			**14,267**	**188,150**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**4,50**
Vial Number:	**BA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:07**	*Sample Weight:*	**1,0000**

Chromatogram

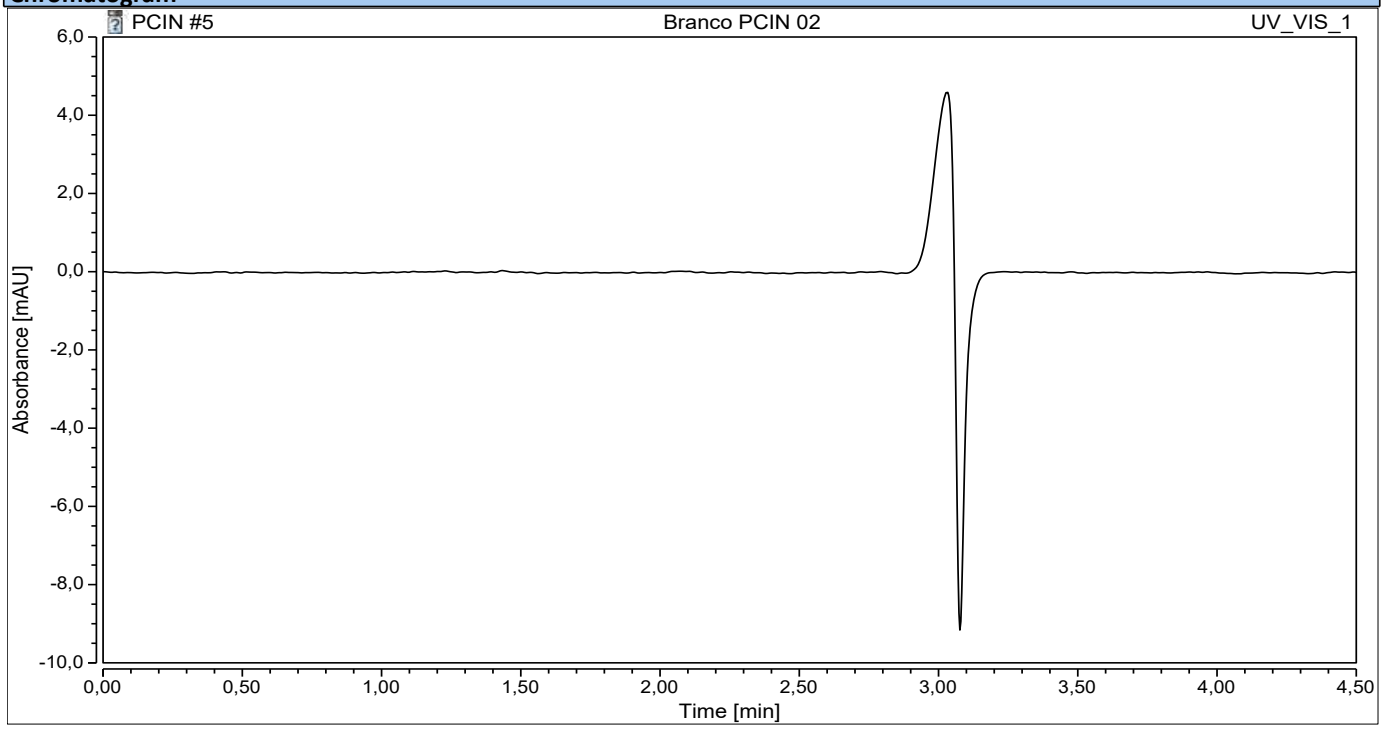

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:12**	*Sample Weight:*	**1,0000**

Chromatogram

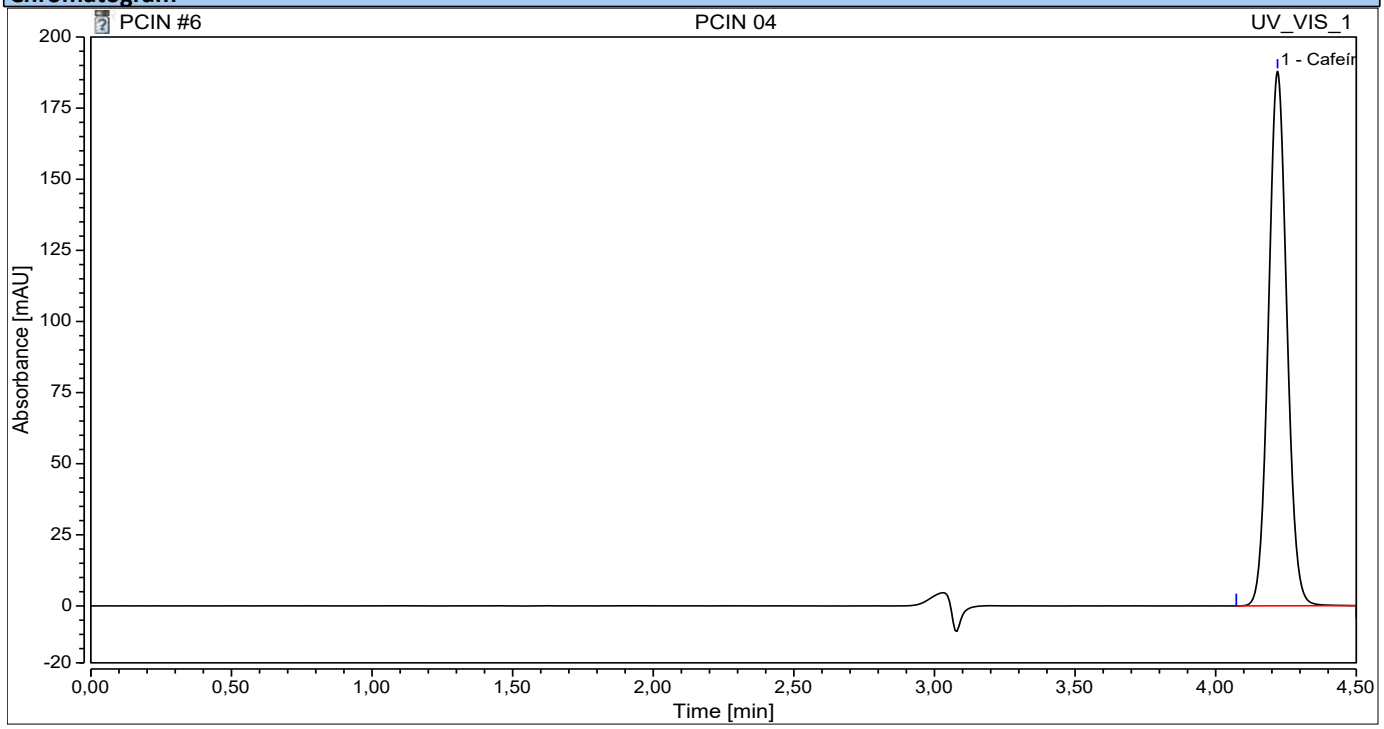

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,220	14,2573	187,883	100,00	100,00	n.a.
Total:			**14,257**	**187,883**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:18**	*Sample Weight:*	**1,0000**

Chromatogram

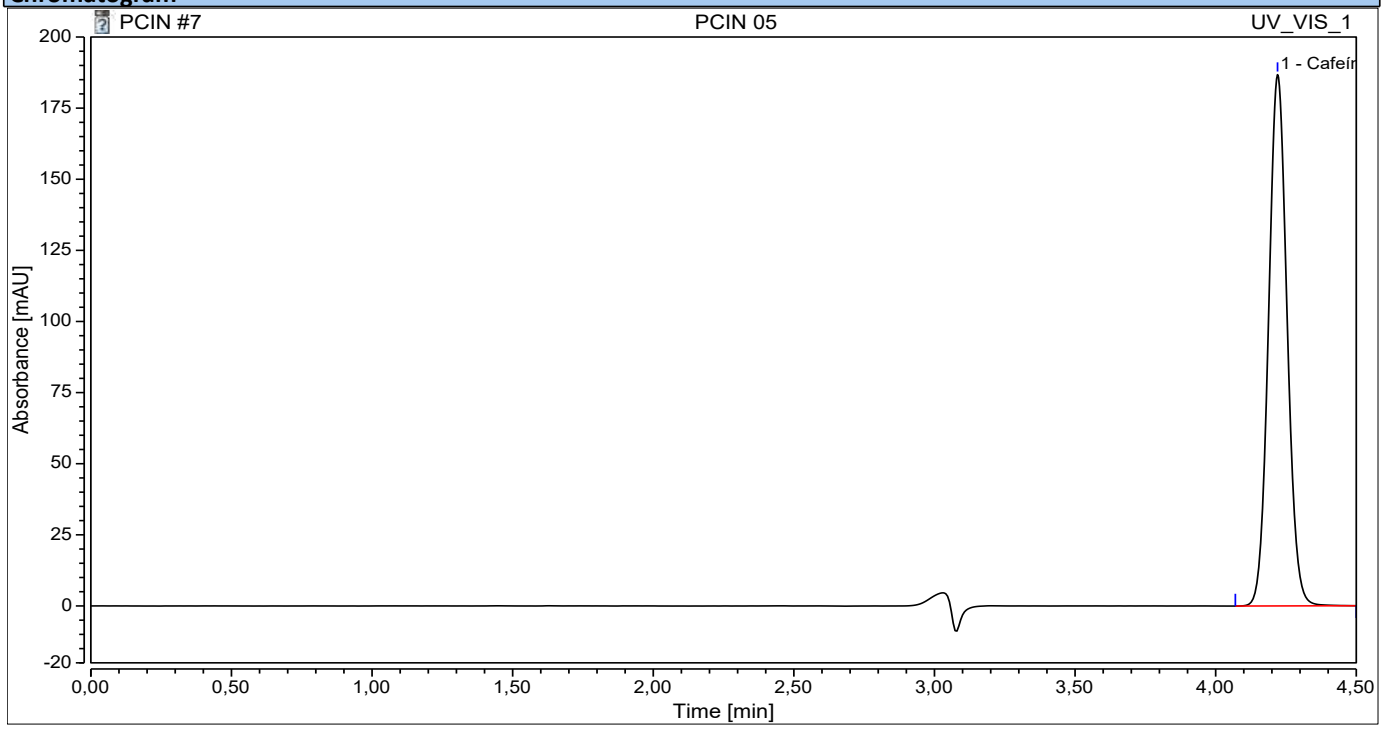

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,220	14,2669	186,781	100,00	100,00	n.a.
Total:			**14,267**	**186,781**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**4,50**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:23**	*Sample Weight:*	**1,0000**

Chromatogram

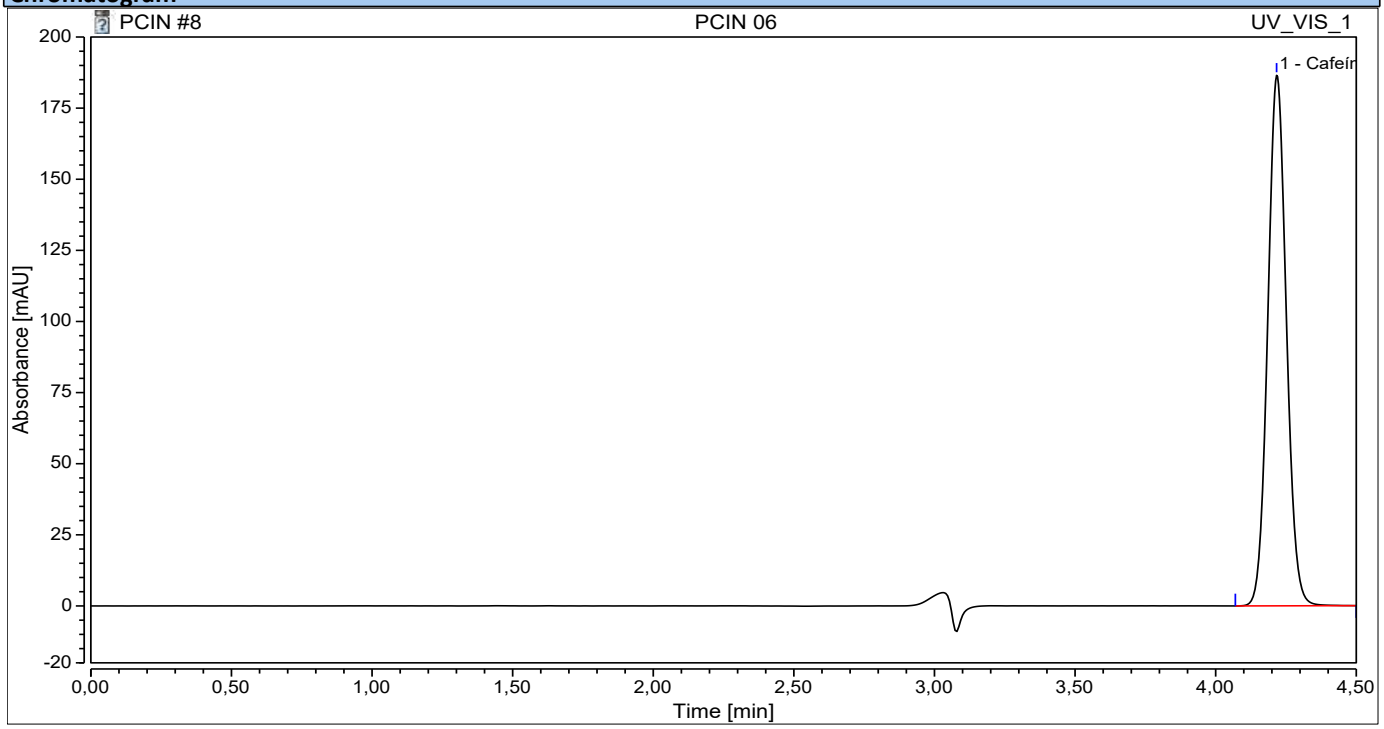

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,217	14,2632	186,497	100,00	100,00	n.a.
Total:			**14,263**	**186,497**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**4,50**
Vial Number:	**BA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:28**	*Sample Weight:*	**1,0000**

Chromatogram

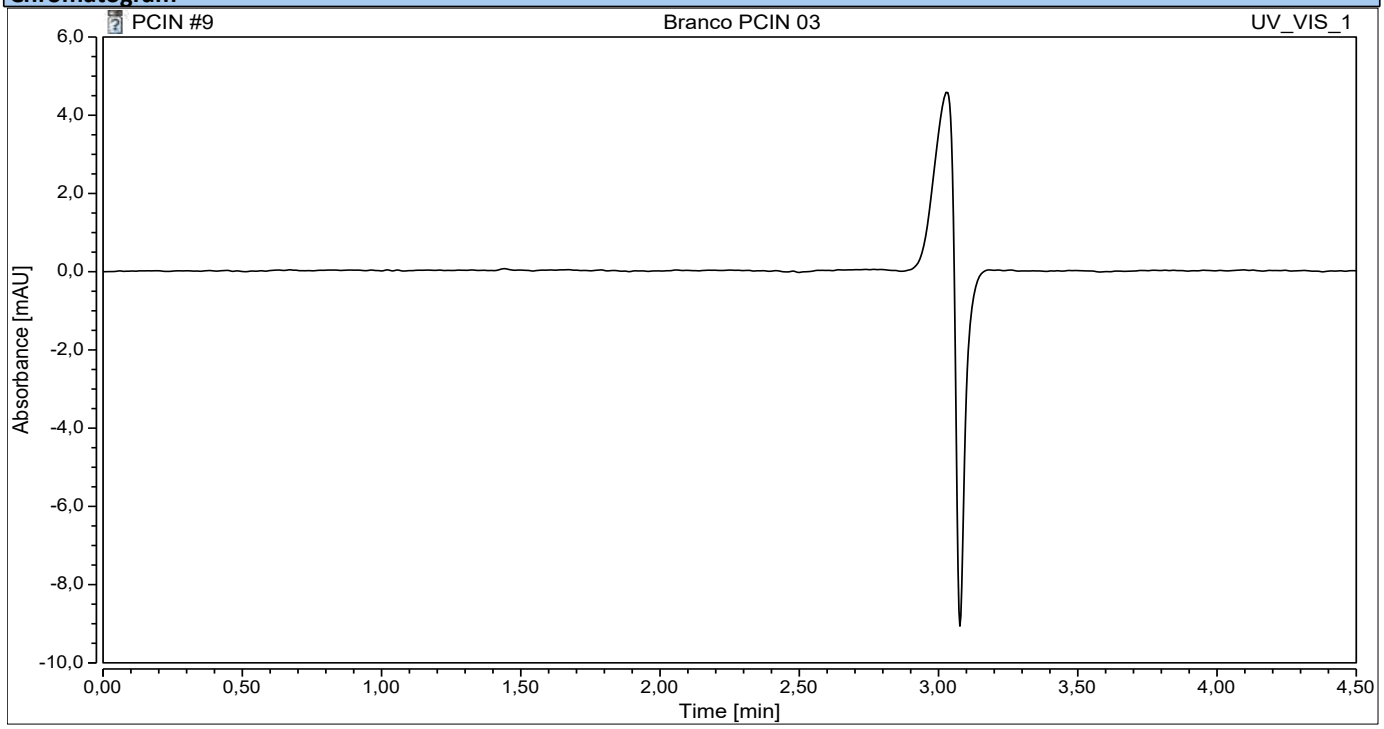

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**4,50**
Vial Number:	**BA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:34**	*Sample Weight:*	**1,0000**

Chromatogram

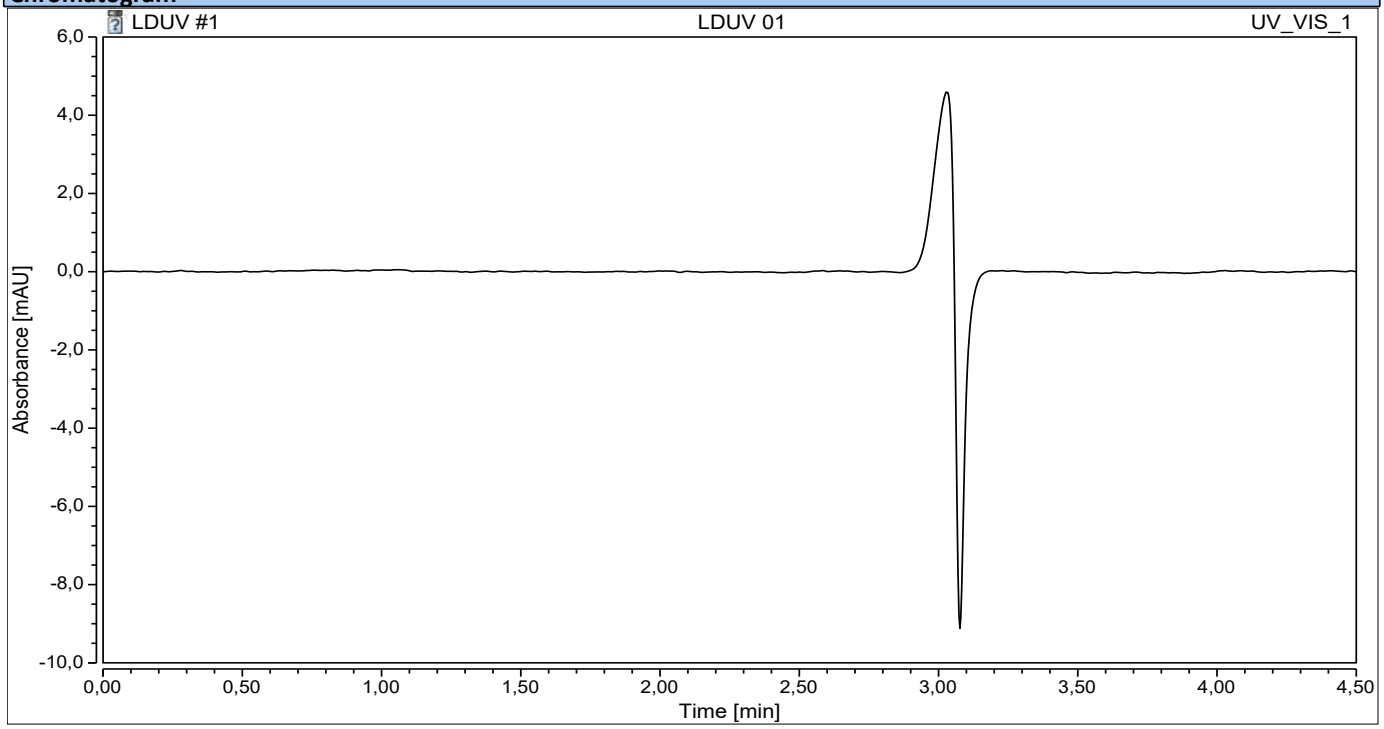

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**4,50**
Vial Number:	**BA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:39**	*Sample Weight:*	**1,0000**

Chromatogram

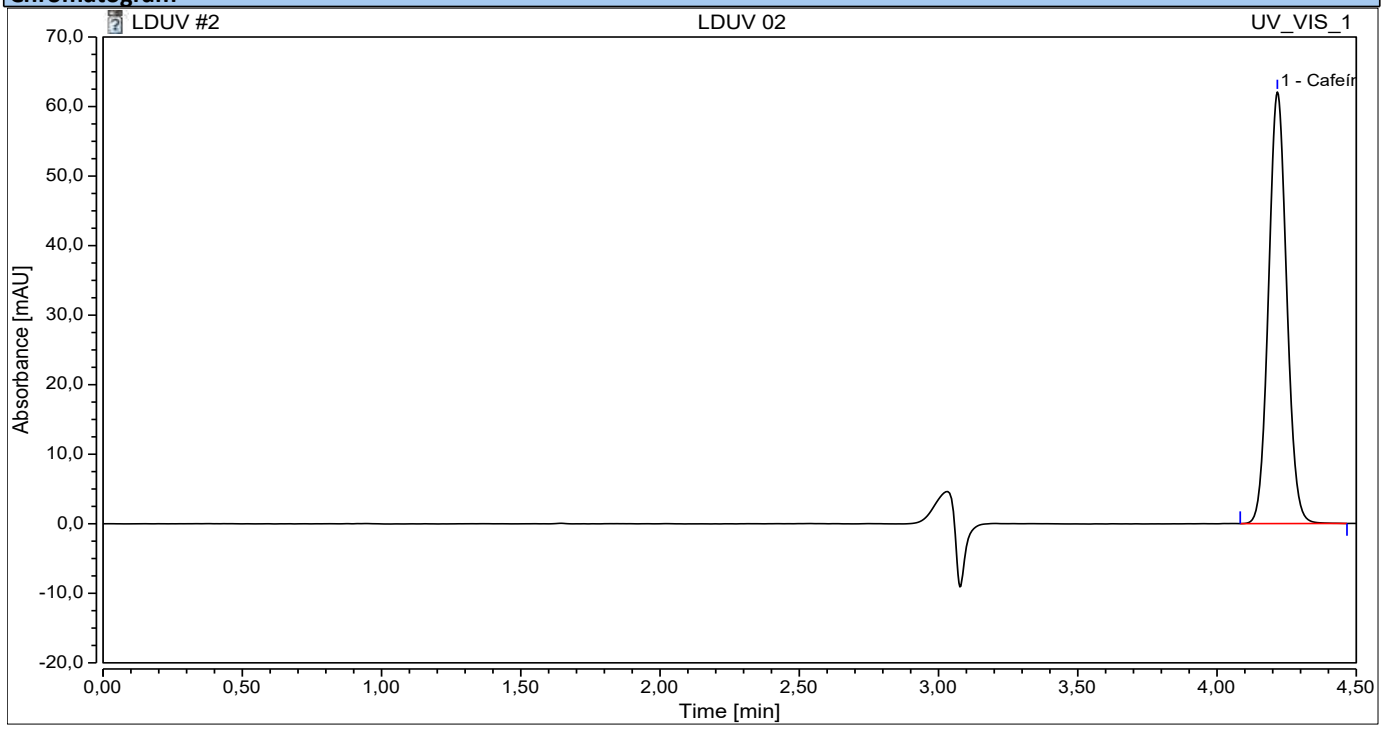

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,217	4,6889	62,069	100,00	100,00	n.a.
Total:			**4,689**	**62,069**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**4,50**
Vial Number:	**BA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:45**	*Sample Weight:*	**1,0000**

Chromatogram

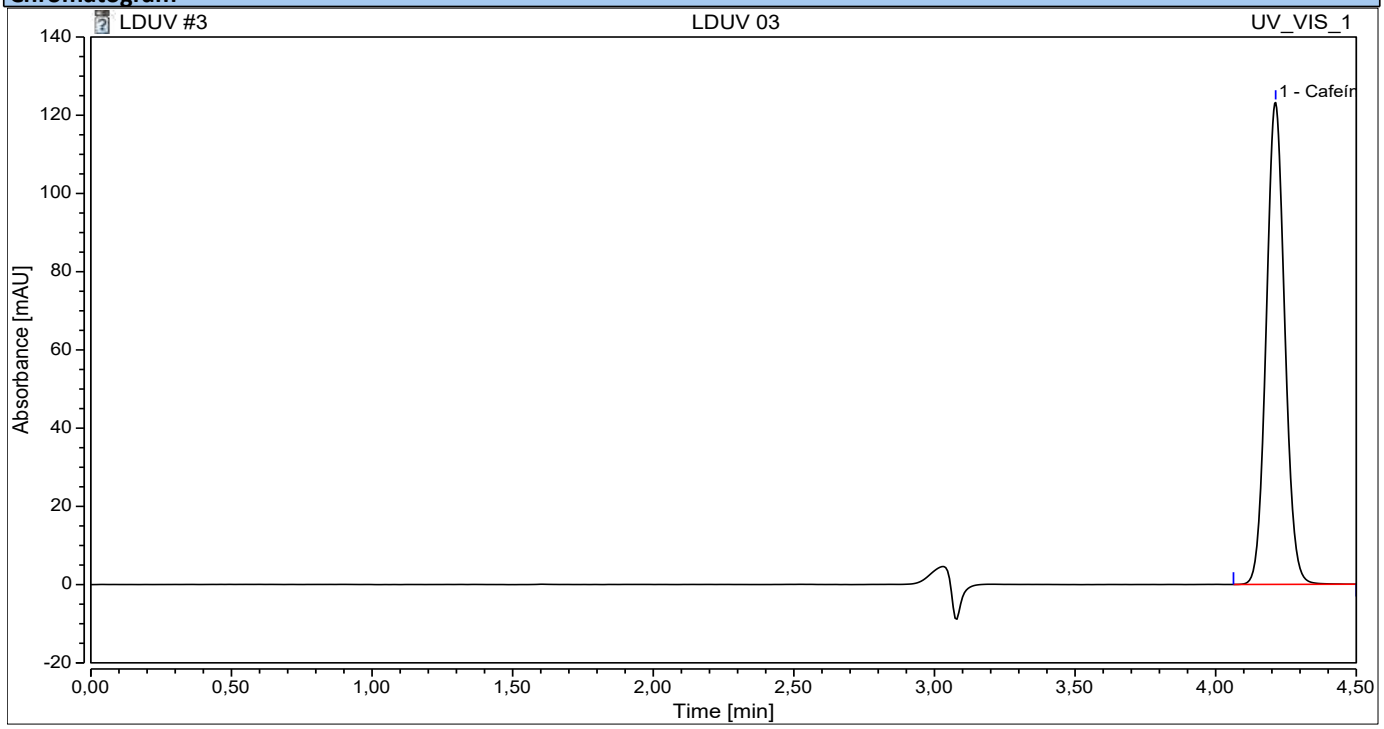

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,213	9,3800	123,203	100,00	100,00	n.a.
Total:			**9,380**	**123,203**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**4,50**
Vial Number:	**BA7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:50**	*Sample Weight:*	**1,0000**

Chromatogram

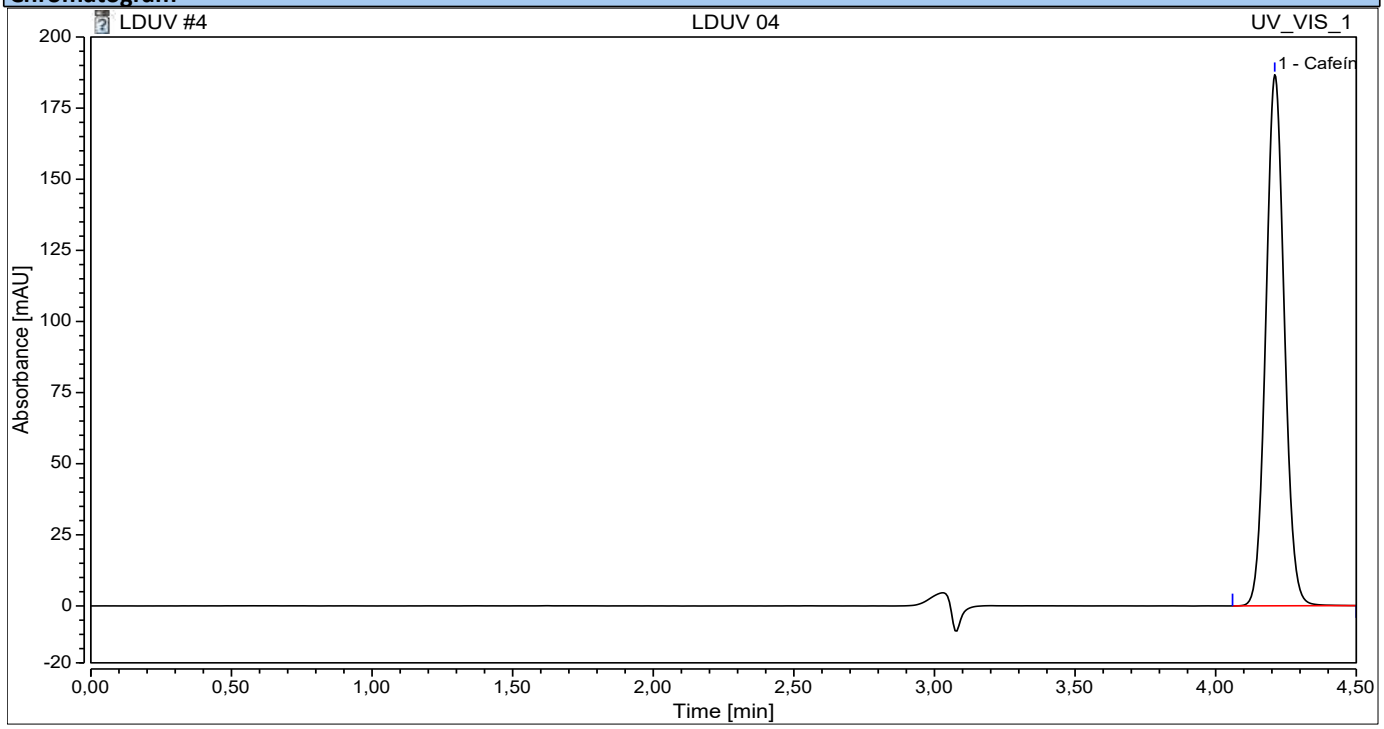

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,210	14,2004	186,704	100,00	100,00	n.a.
Total:			**14,200**	**186,704**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**4,50**
Vial Number:	**BA8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**03/set/26 18:55**	*Sample Weight:*	**1,0000**

Chromatogram

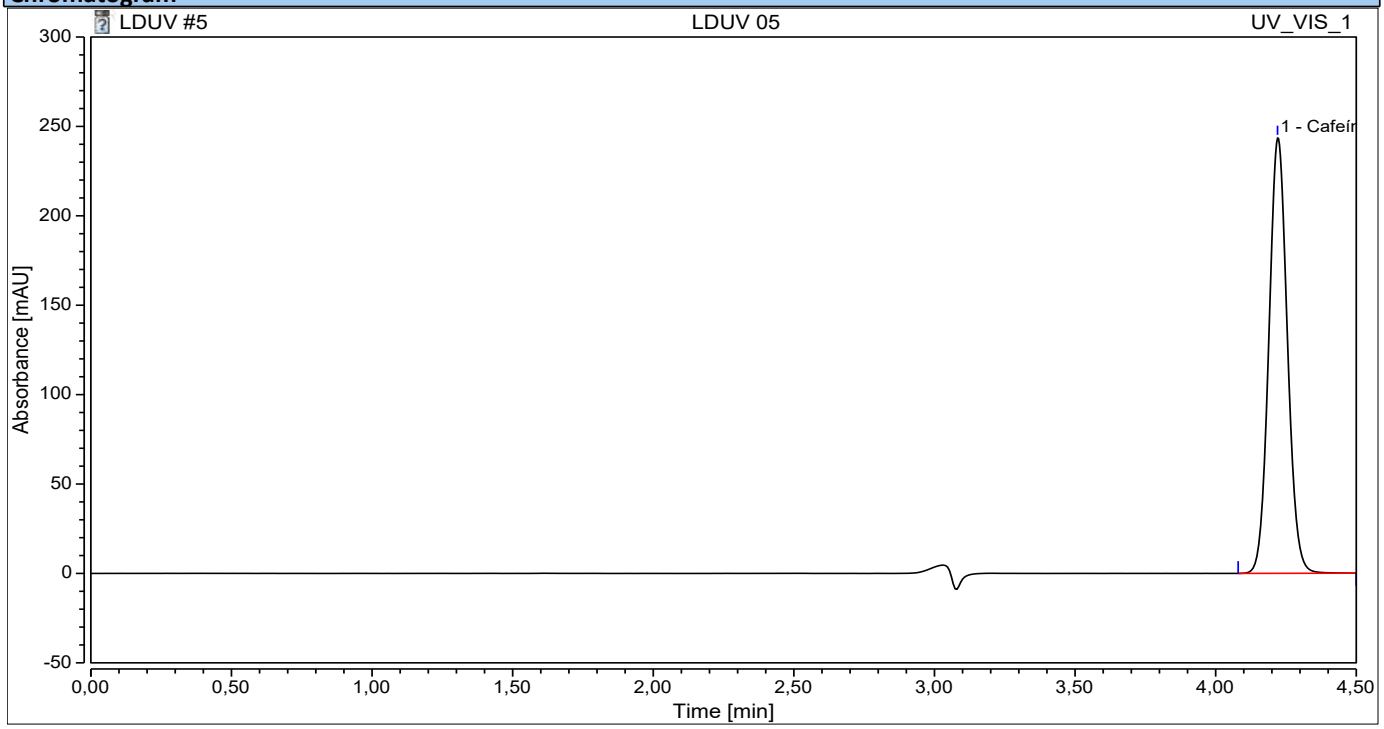

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,220	18,5654	243,513	100,00	100,00	n.a.
Total:			**18,565**	**243,513**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**4,50**
Vial Number:	**BB1**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 09:44**	*Sample Weight:*	**1,0000**

Chromatogram

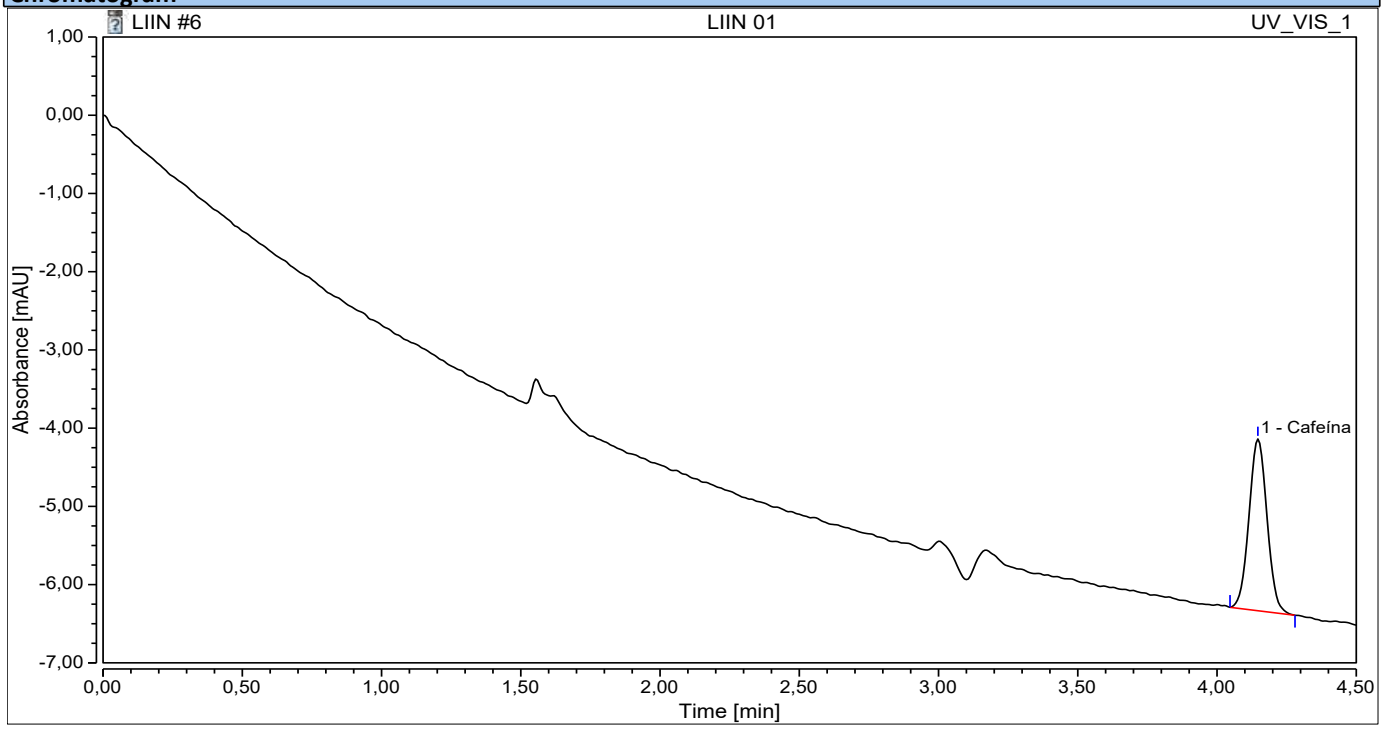

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,147	0,1652	2,196	100,00	100,00	n.a.
Total:			**0,165**	**2,196**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**4,50**
Vial Number:	**BB1**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 09:49**	*Sample Weight:*	**1,0000**

Chromatogram

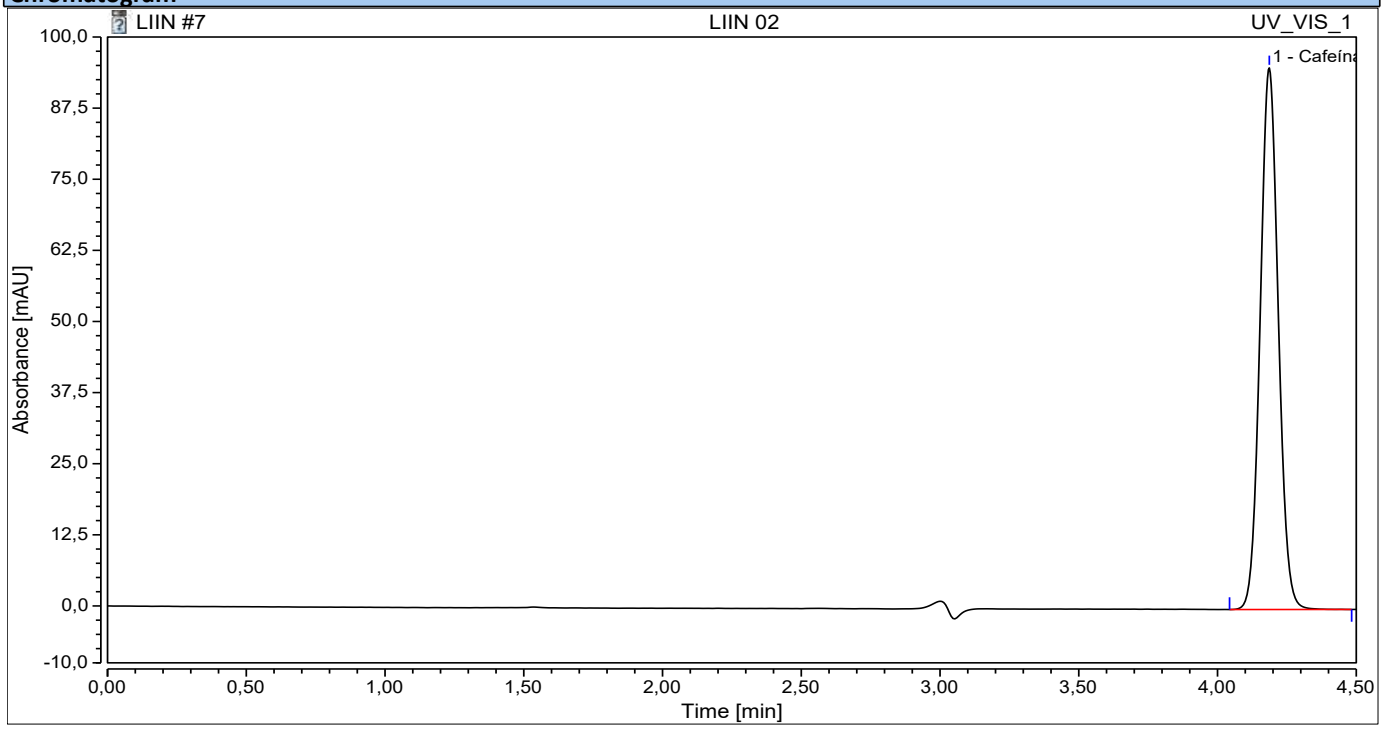

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,187	7,2126	95,203	100,00	100,00	n.a.
Total:			**7,213**	**95,203**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**4,50**
Vial Number:	**BB1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 09:54**	*Sample Weight:*	**1,0000**

Chromatogram

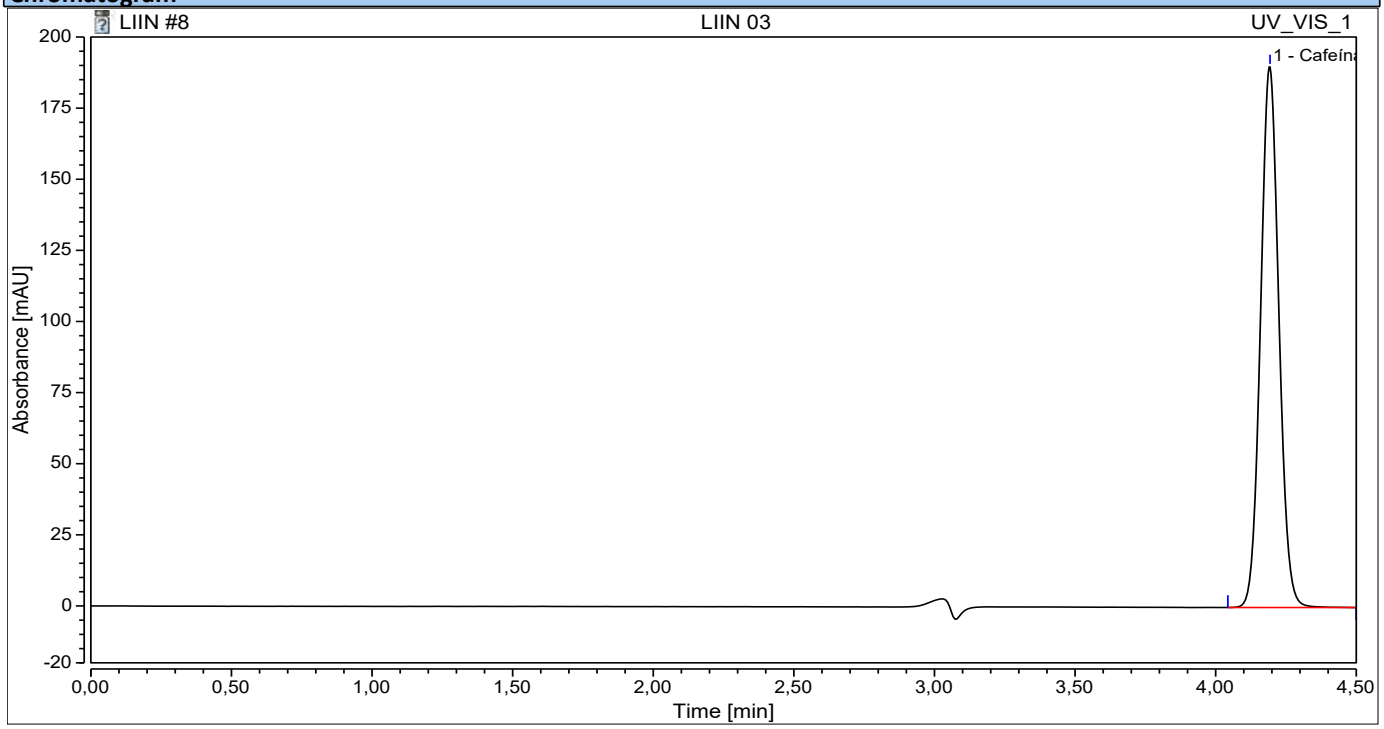

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,193	14,3485	190,036	100,00	100,00	n.a.
Total:			**14,348**	**190,036**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**4,50**
Vial Number:	**BB1**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 10:00**	*Sample Weight:*	**1,0000**

Chromatogram

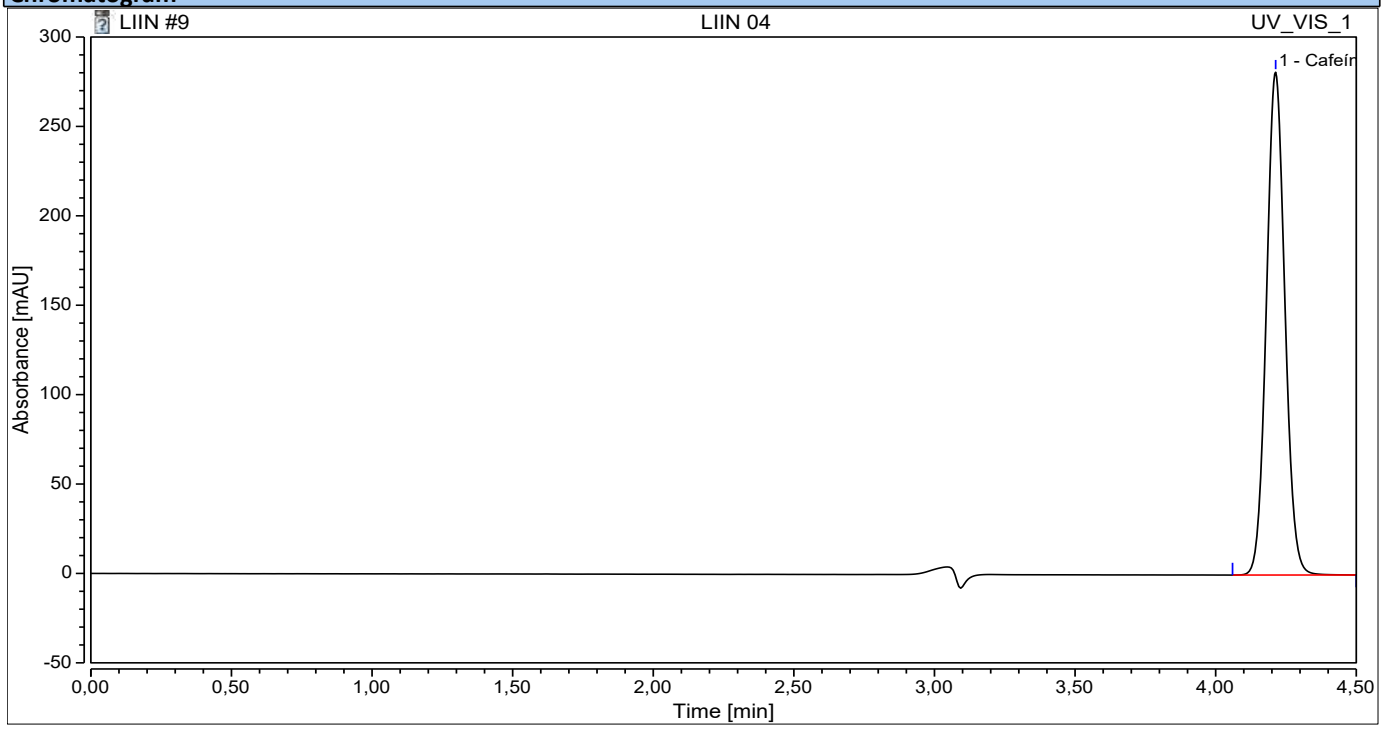

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,213	21,3894	281,204	100,00	100,00	n.a.
Total:			**21,389**	**281,204**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**4,50**
Vial Number:	**BB1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 02 DAD**	*Bandwidth:*	**3**
Processing Method:	**Cafeína QPack**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 10:05**	*Sample Weight:*	**1,0000**

Chromatogram

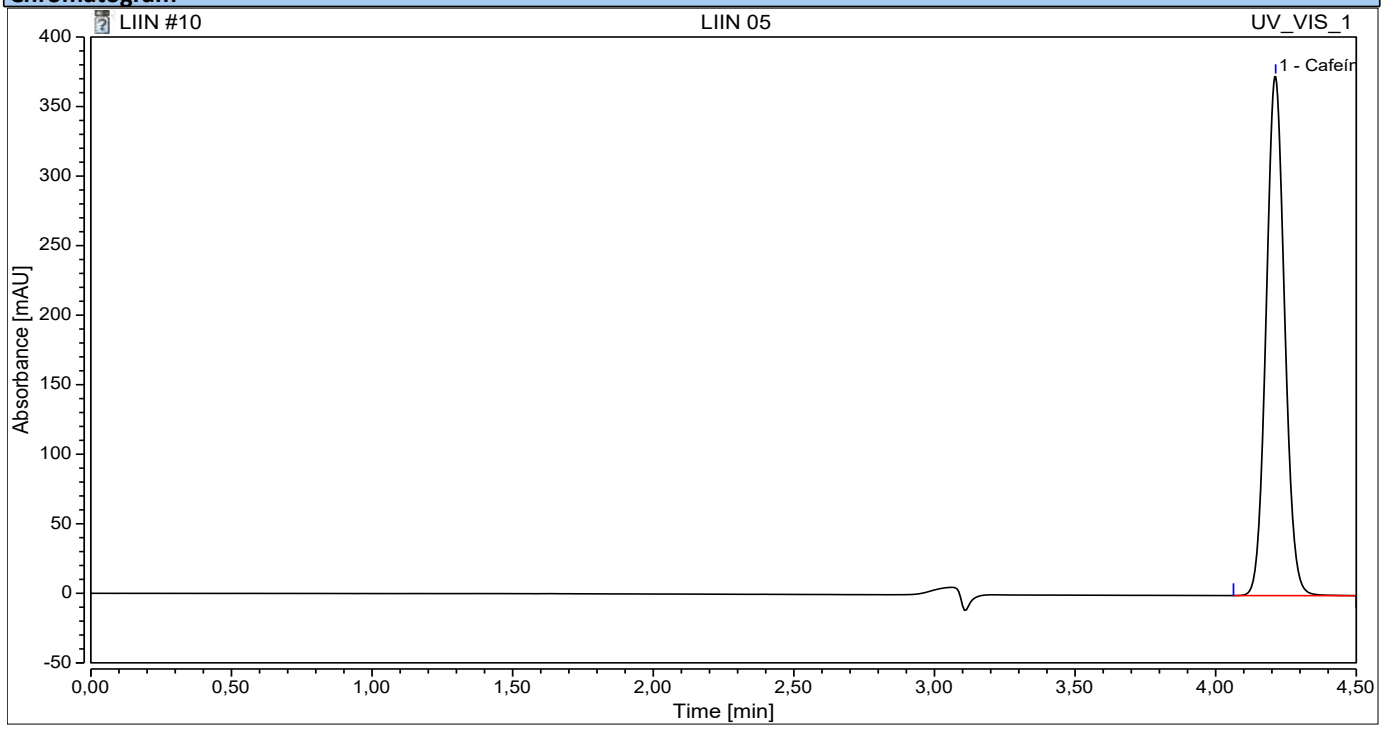

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	4,213	28,4580	373,221	100,00	100,00	n.a.
Total:			**28,458**	**373,221**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:12**	*Sample Weight:*	**1,0000**

Chromatogram

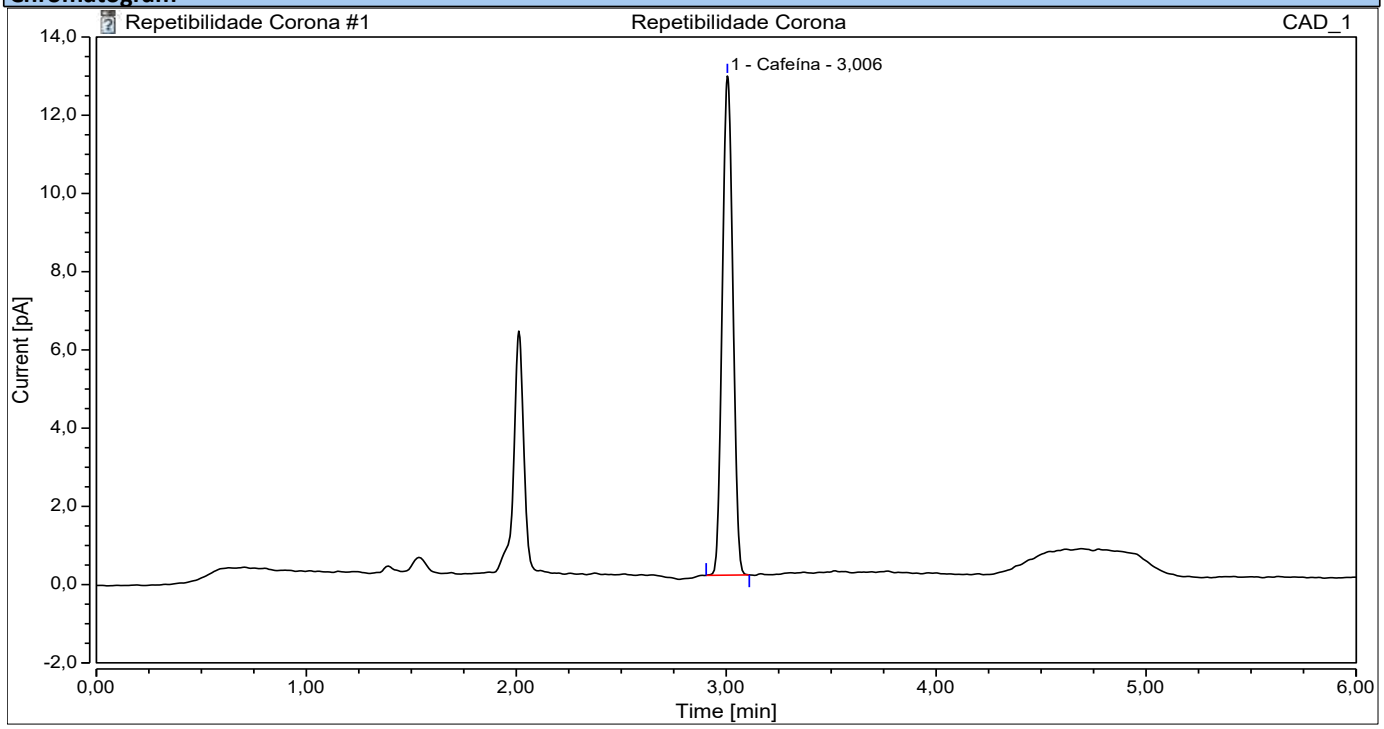

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,006	0,7476	12,761	100,00	100,00	n.a.
Total:			**0,748**	**12,761**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:19**	*Sample Weight:*	**1,0000**

Chromatogram

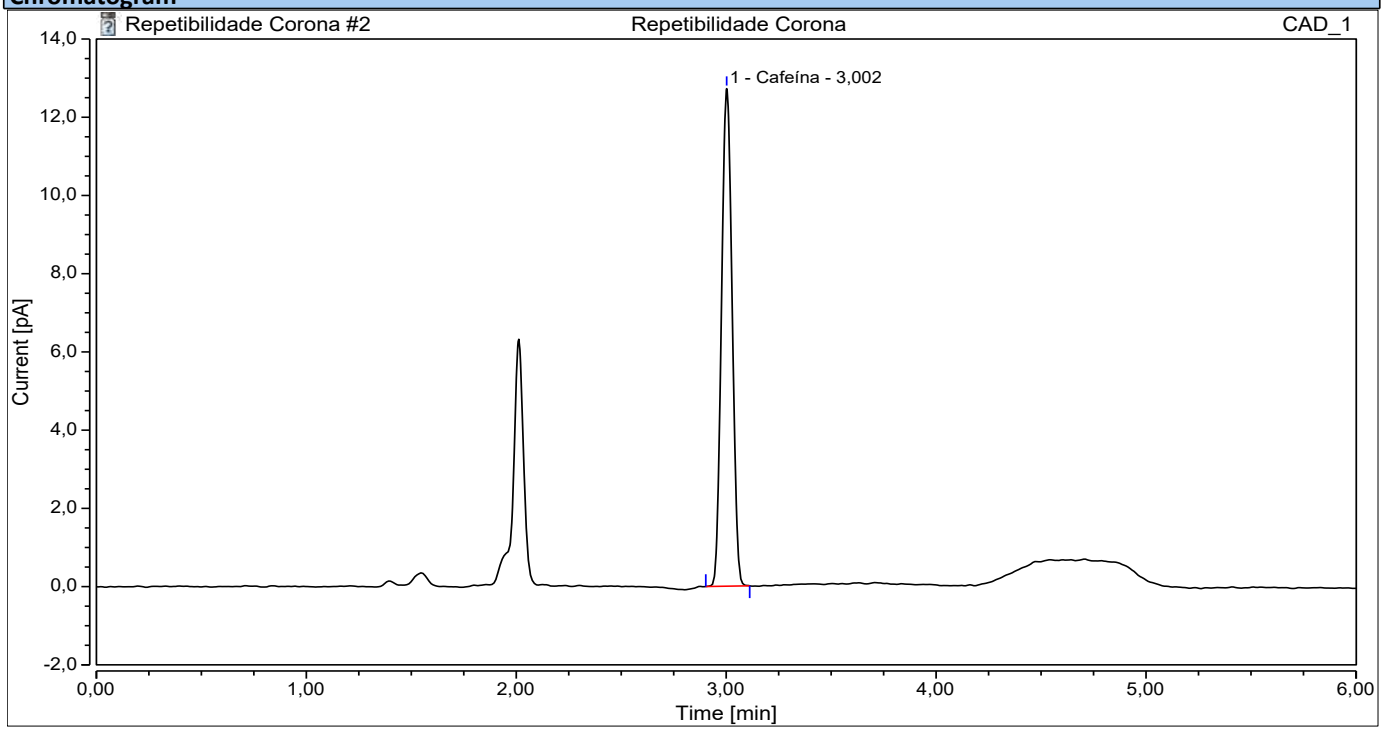

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,002	0,7469	12,721	100,00	100,00	n.a.
Total:			**0,747**	**12,721**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:26**	*Sample Weight:*	**1,0000**

Chromatogram

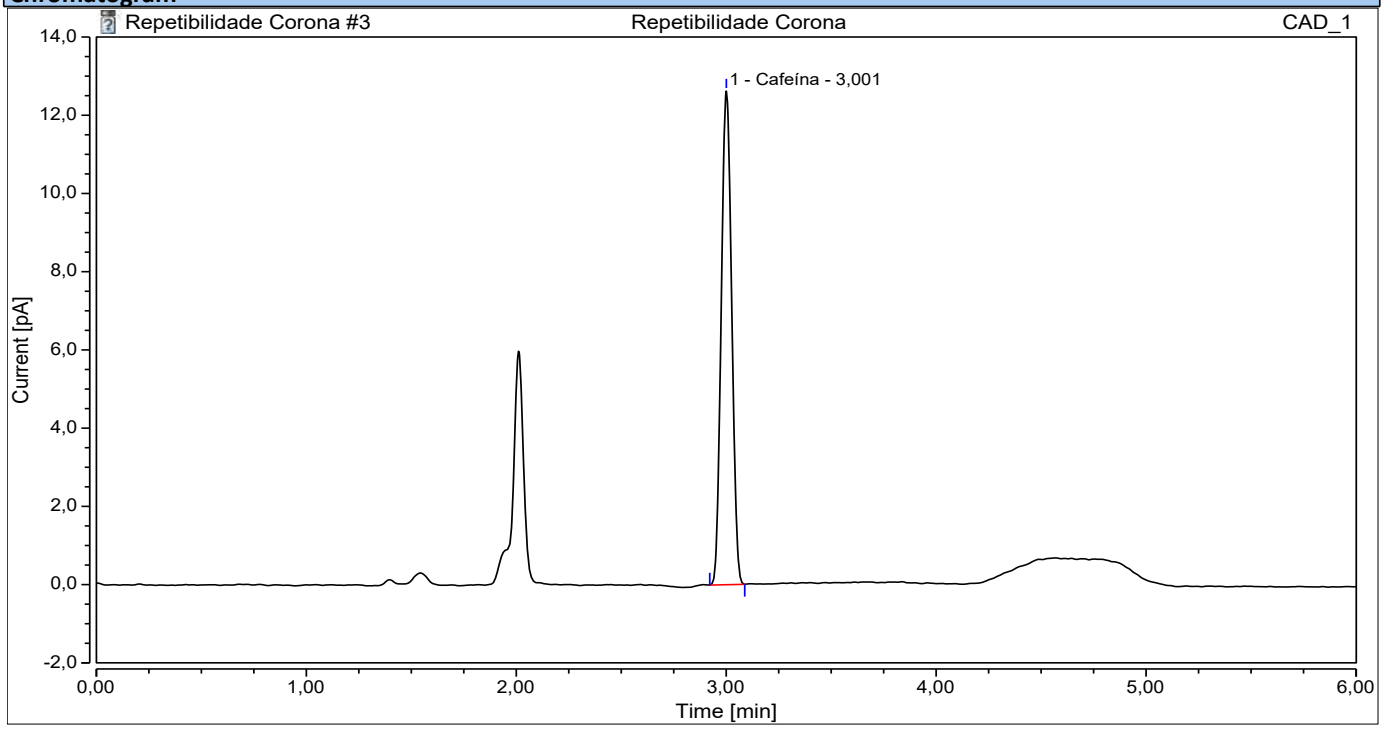

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,001	0,7278	12,620	100,00	100,00	n.a.
Total:			**0,728**	**12,620**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:32**	*Sample Weight:*	**1,0000**

Chromatogram

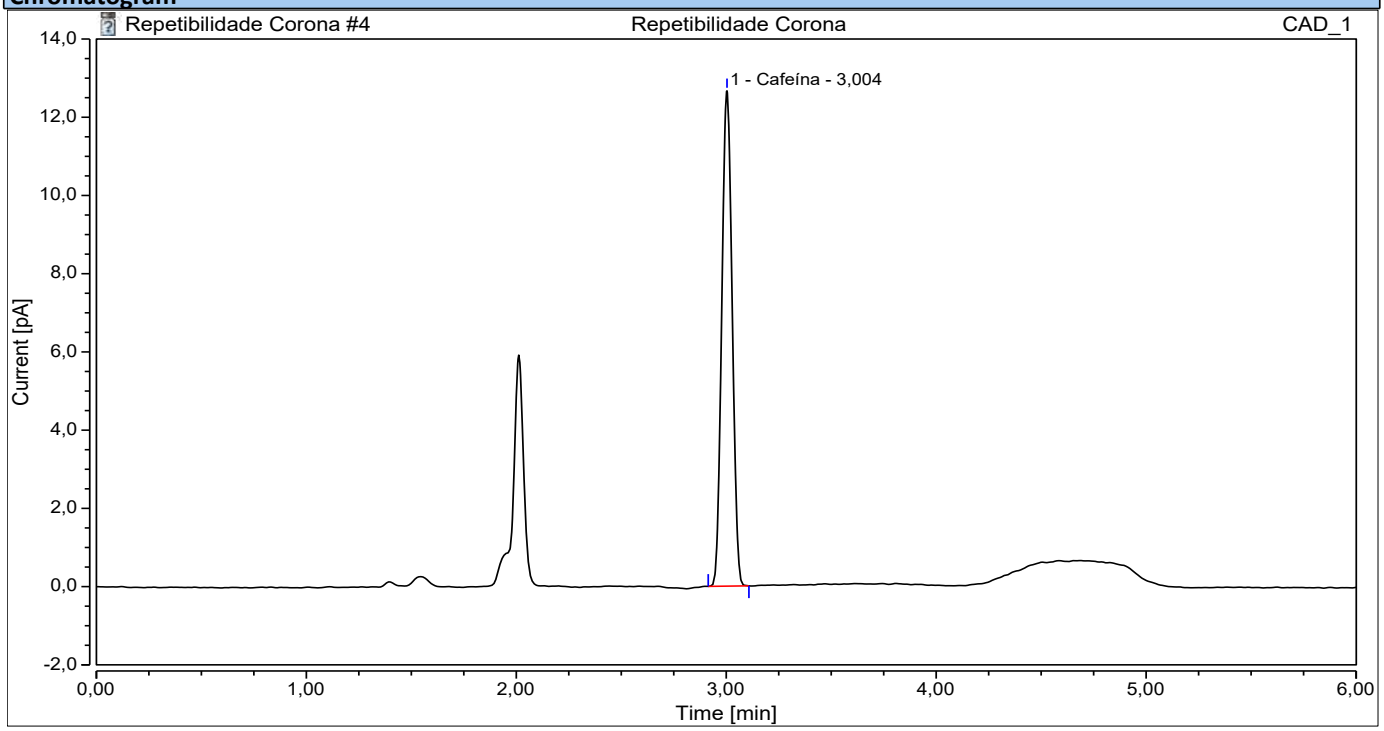

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,004	0,7267	12,663	100,00	100,00	n.a.
Total:			**0,727**	**12,663**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:39**	*Sample Weight:*	**1,0000**

Chromatogram

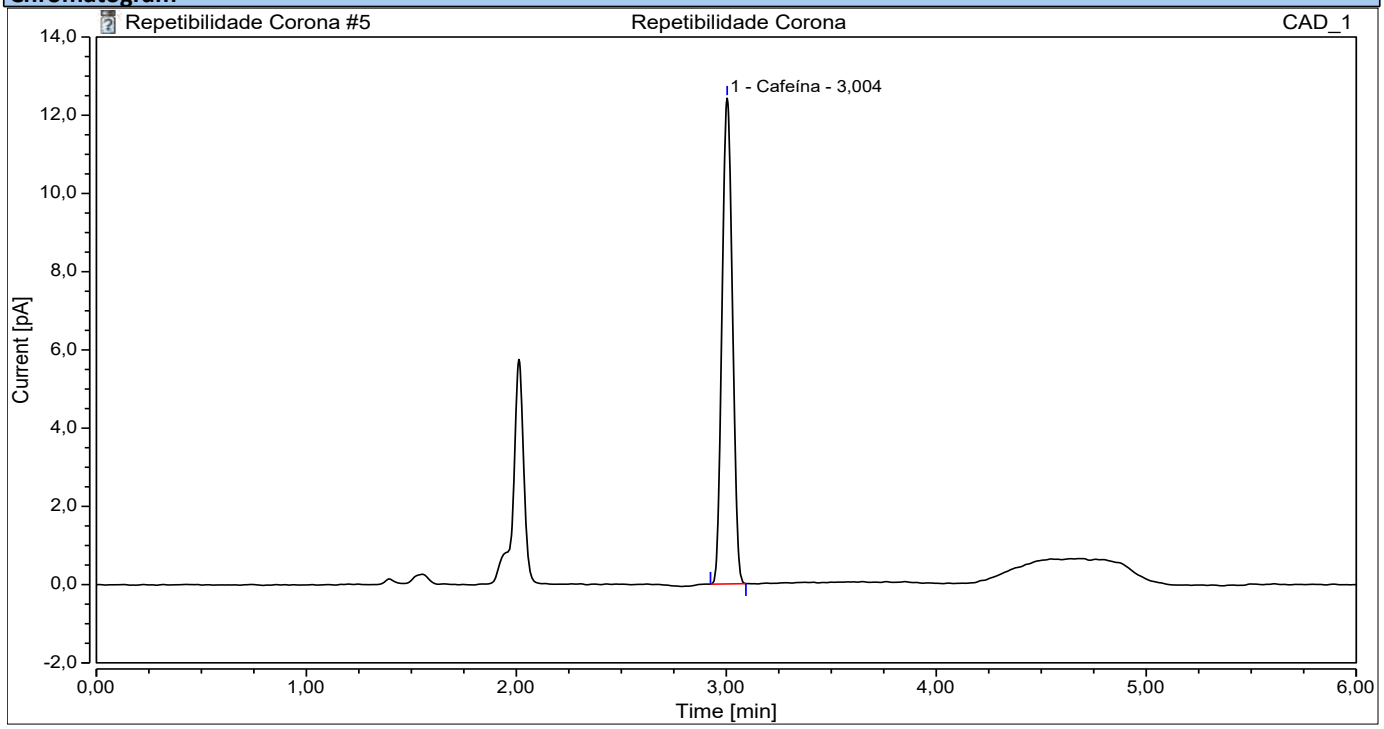

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,004	0,7146	12,418	100,00	100,00	n.a.
Total:			**0,715**	**12,418**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Repetibilidade Corona**	*Run Time (min):*	**6,00**
Vial Number:	**BA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação HPLC 02 Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína CAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 11:46**	*Sample Weight:*	**1,0000**

Chromatogram

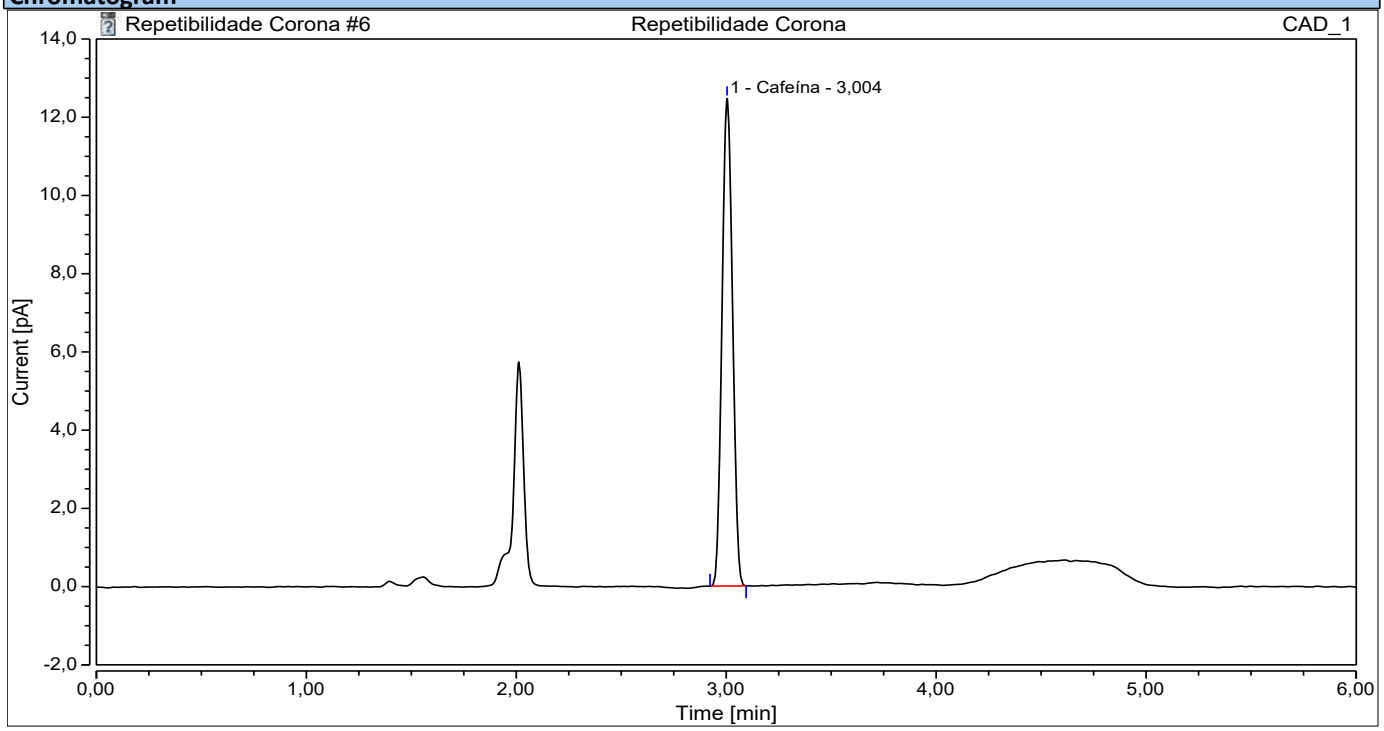

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeína	3,004	0,7239	12,463	100,00	100,00	n.a.
Total:			**0,724**	**12,463**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB**	*Run Time (min):*	**20,00**
Vial Number:	**BA2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**GRAD HPLC 02**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 13:39**	*Sample Weight:*	**1,0000**

Chromatogram

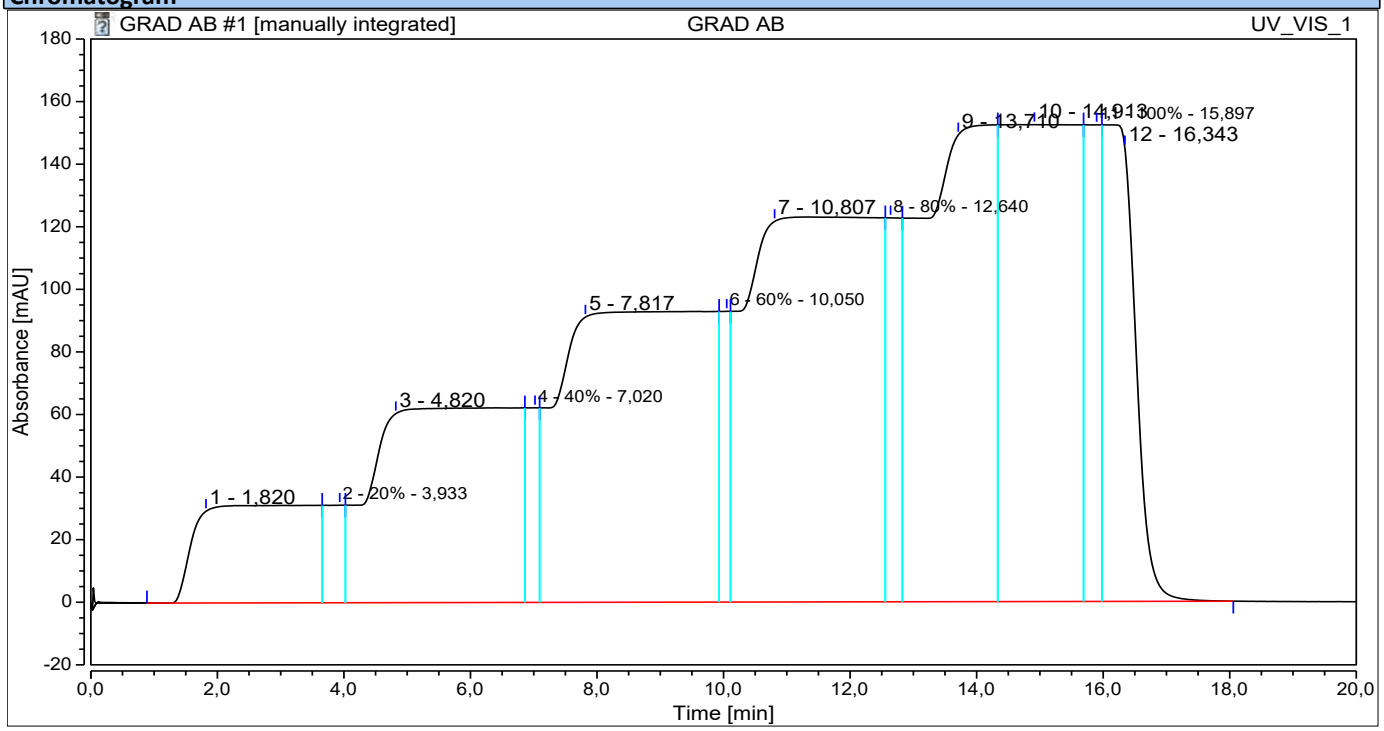

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	3,933	11,4226	31,193	0,83	2,58	n.a.
4	40%	7,020	14,5088	62,205	1,05	5,14	n.a.
6	60%	10,050	16,7222	92,923	1,21	7,68	n.a.
8	80%	12,640	33,1205	122,704	2,39	10,14	n.a.
11	100%	15,897	44,1669	152,314	3,19	12,58	n.a.
Total:			**119,941**	**461,340**	**8,665**	**38,115**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD CD**	*Run Time (min):*	**20,00**
Vial Number:	**BA2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD HPLC 02**	*Bandwidth:*	**3**
Processing Method:	**GRAD HPLC 02**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**04/set/26 14:09**	*Sample Weight:*	**1,0000**

Chromatogram

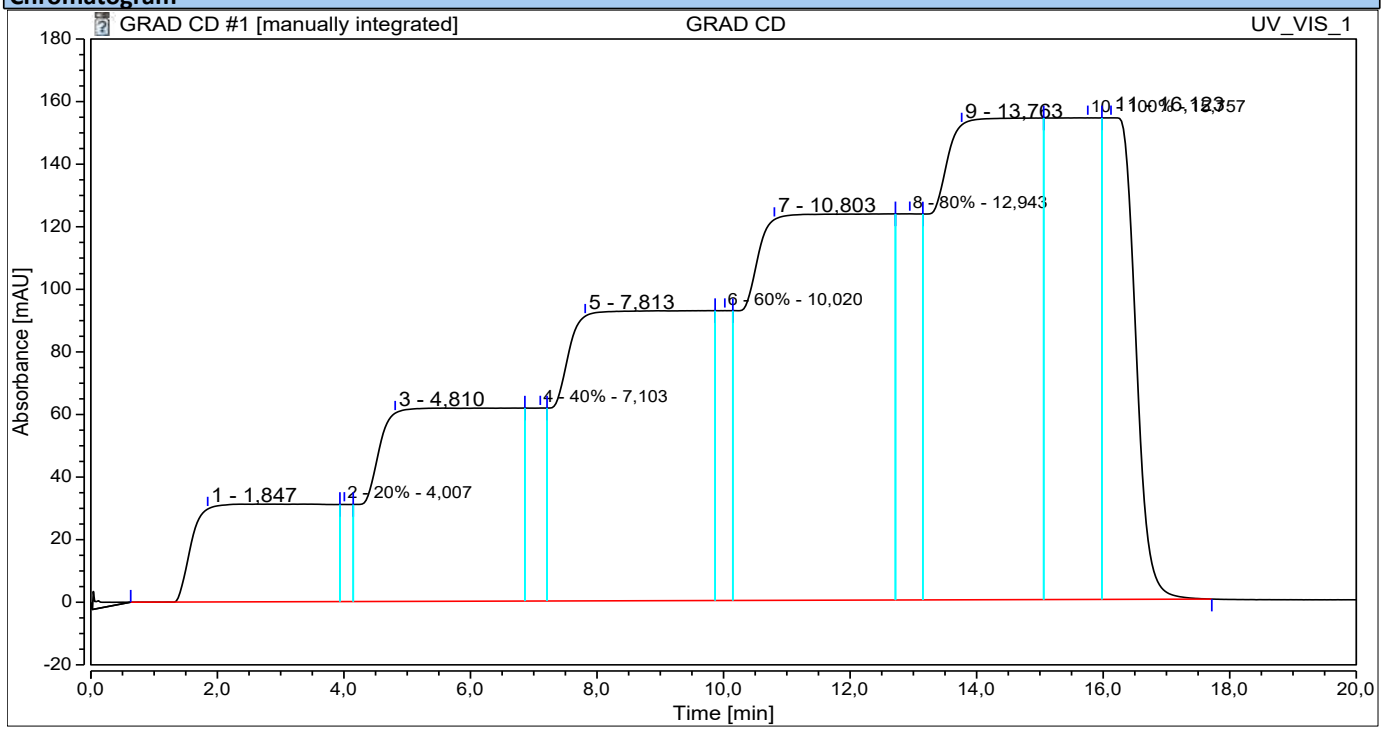

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,007	6,5163	31,054	0,47	2,90	n.a.
4	40%	7,103	21,5799	61,679	1,55	5,76	n.a.
6	60%	10,020	25,9325	92,636	1,87	8,65	n.a.
8	80%	12,943	53,4628	123,410	3,85	11,52	n.a.
10	100%	15,757	141,5775	153,910	10,20	14,37	n.a.
Total:			**249,069**	**462,690**	**17,947**	**43,207**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.