
Spectral Library Screening Results

Injection Details

Injection Name:	**EDUV**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 08:39**	*Sample Weight:*	**1,0000**

UV Spectra — Cafeina

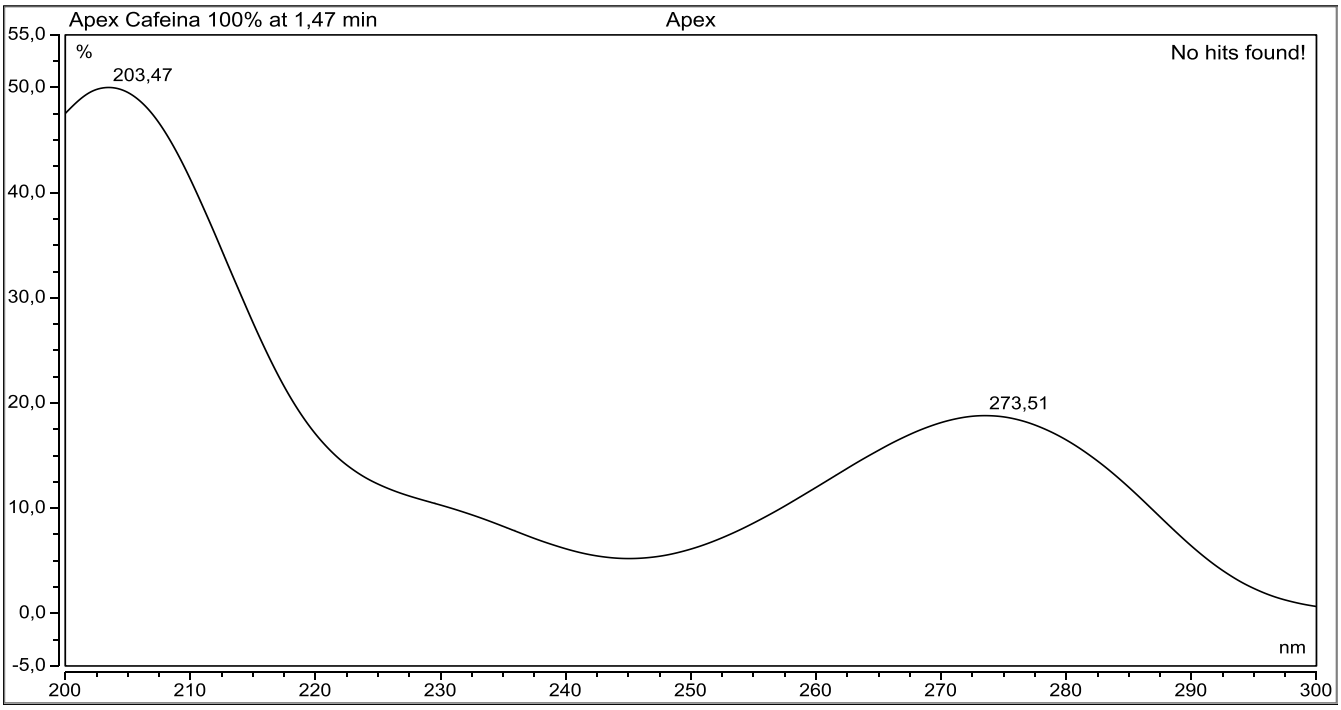

Spectral Library Screening Results

	Hit# 1	Hit# 2	Hit# 3
Library:	n.a.	n.a.	n.a.
Component:	n.a.	n.a.	n.a.
Match Factor:	n.a.	n.a.	n.a.
Ret.Time:	n.a.	n.a.	n.a.
Origin:			
Acq.Date:	n.a.	n.a.	n.a.
Instrument Method:	n.a.	n.a.	n.a.


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 1**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:00**	*Sample Weight:*	**1,0000**

Chromatogram

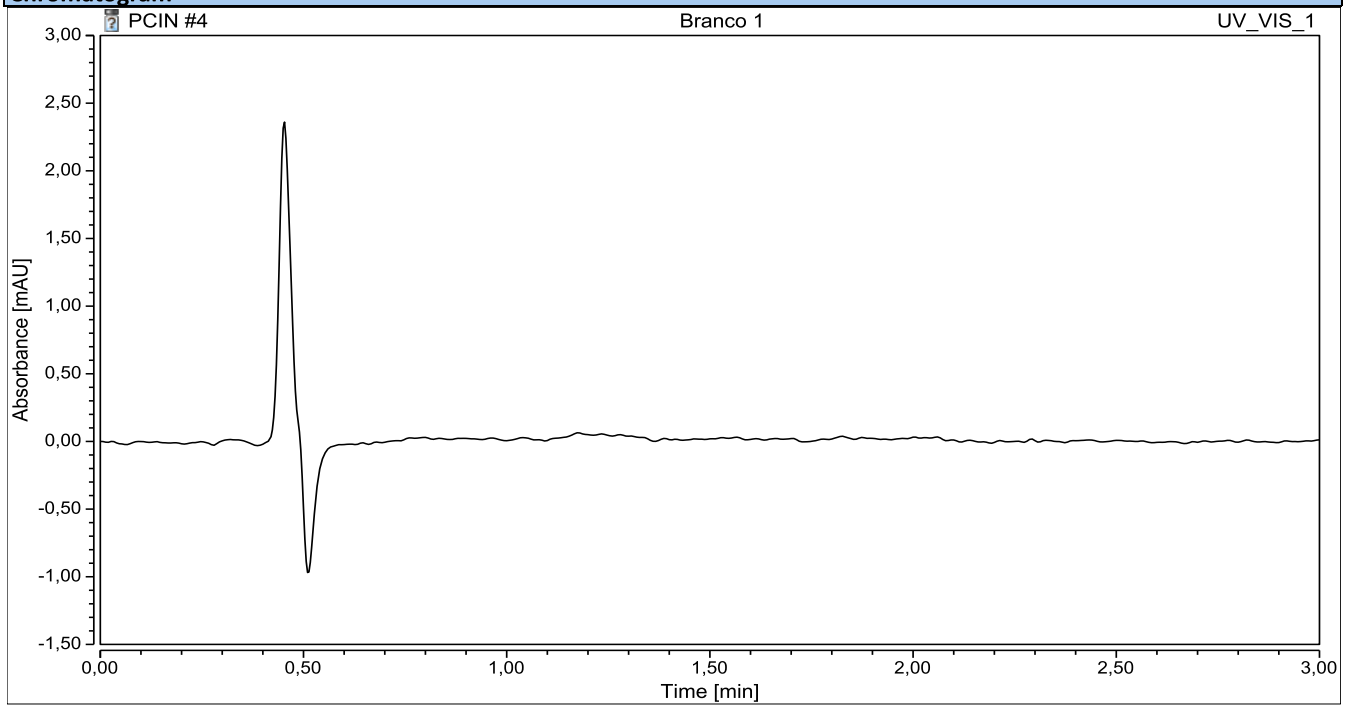

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeina	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 1**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:04**	*Sample Weight:*	**1,0000**

Chromatogram

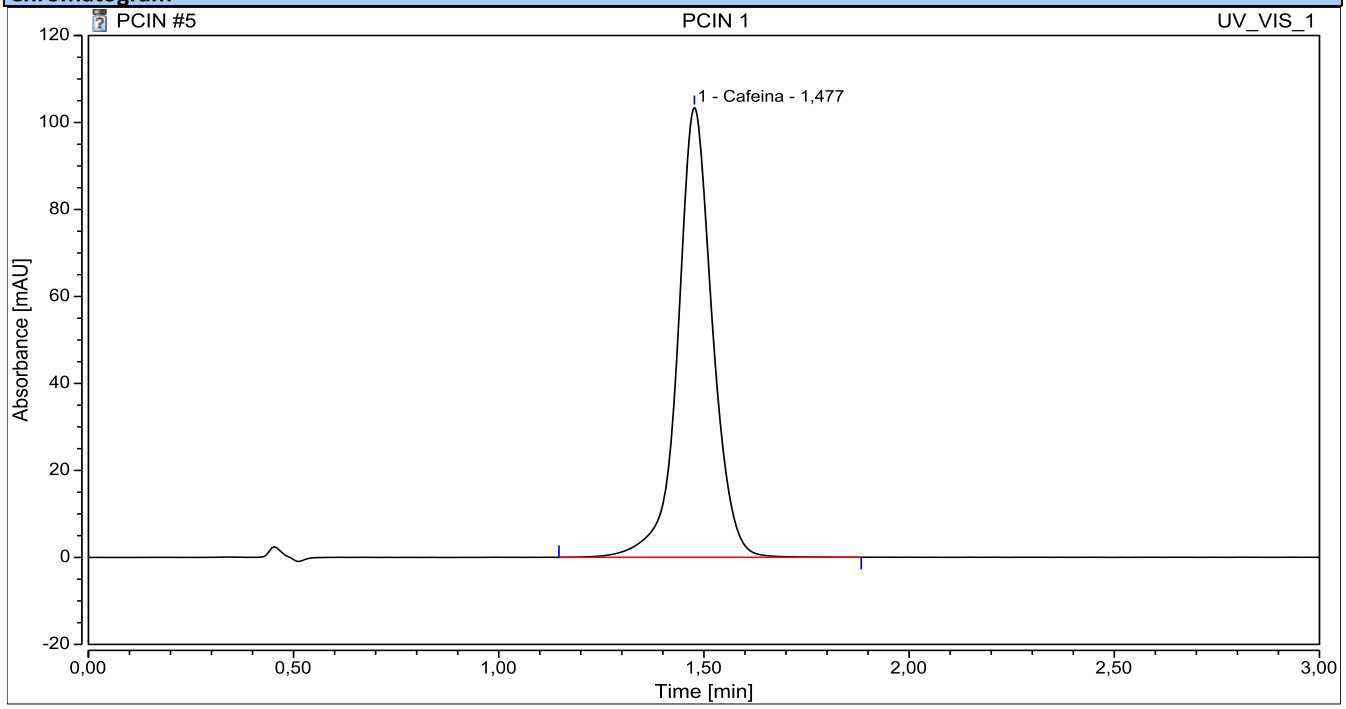

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,477	10,1170	103,418	100,00	100,00	n.a.
Total:			**10,117**	**103,418**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 2**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:08**	*Sample Weight:*	**1,0000**

Chromatogram

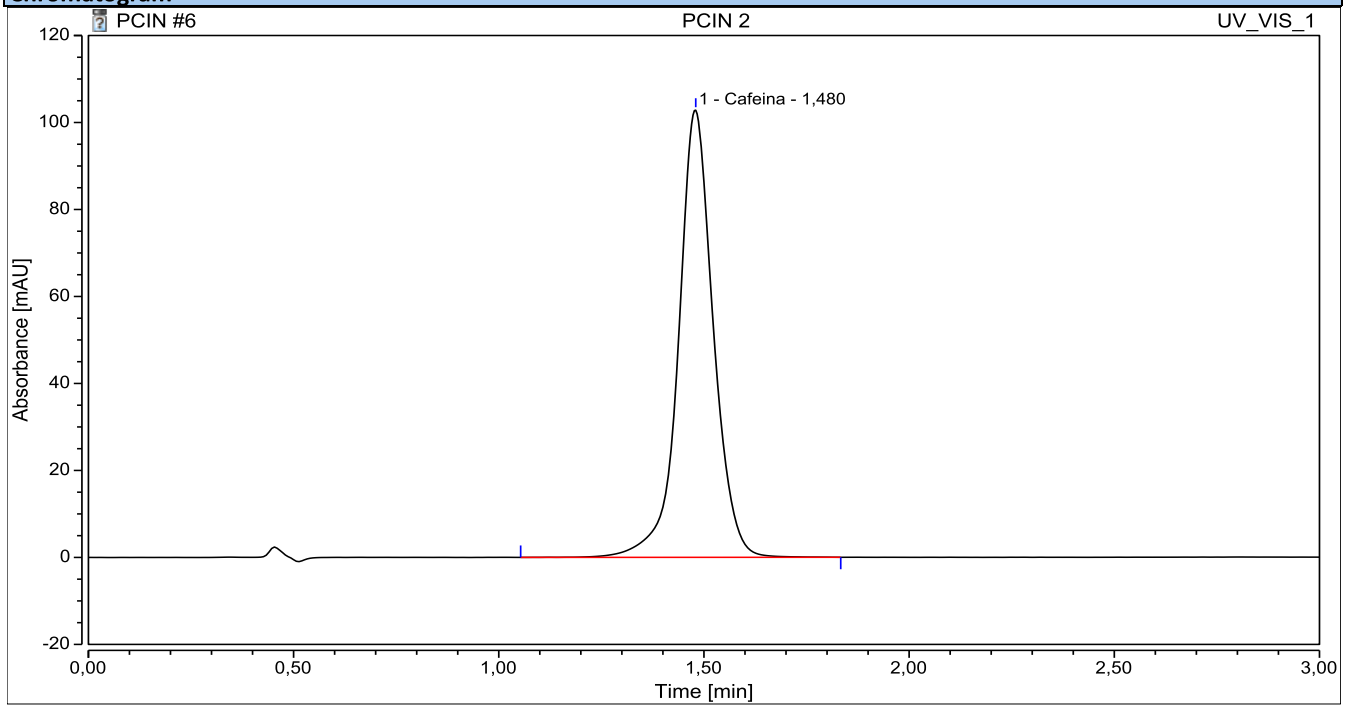

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,480	10,1163	102,812	100,00	100,00	n.a.
Total:			**10,116**	**102,812**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 3**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:12**	*Sample Weight:*	**1,0000**

Chromatogram

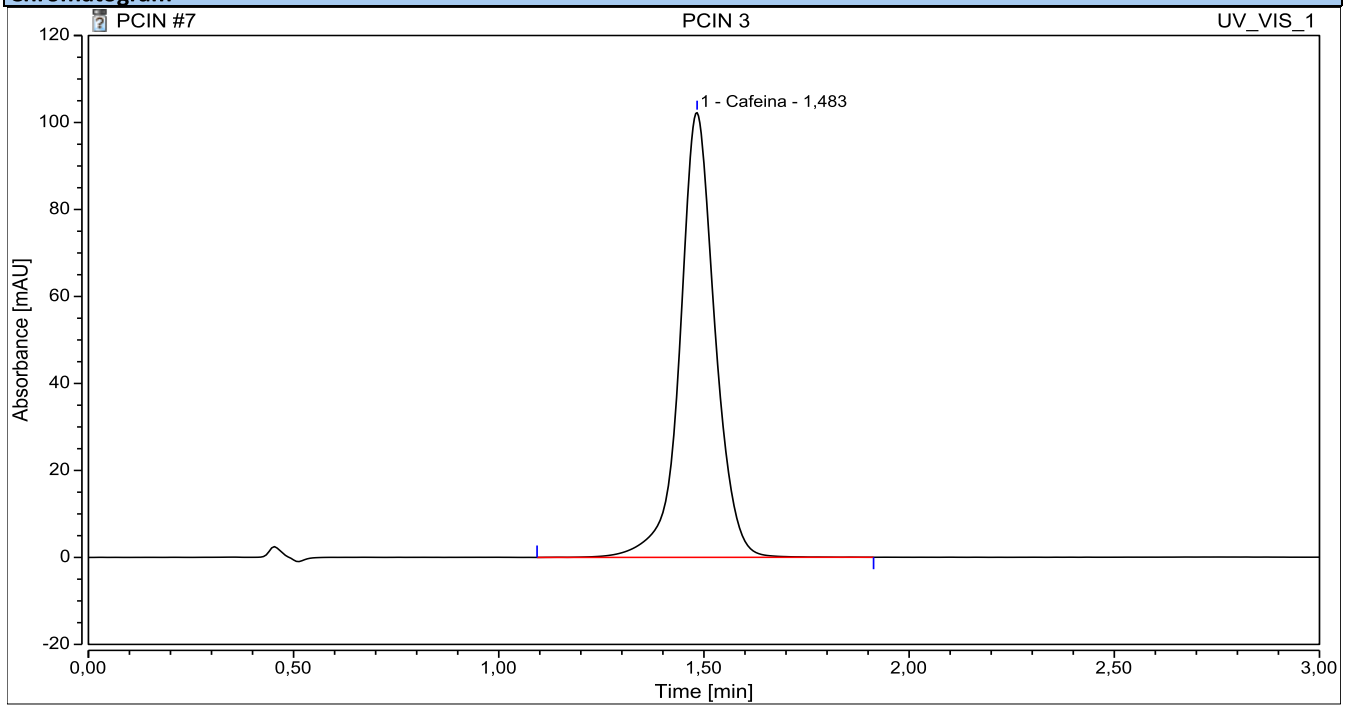

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,483	10,1154	102,249	100,00	100,00	n.a.
Total:			**10,115**	**102,249**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 2**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:15**	*Sample Weight:*	**1,0000**

Chromatogram

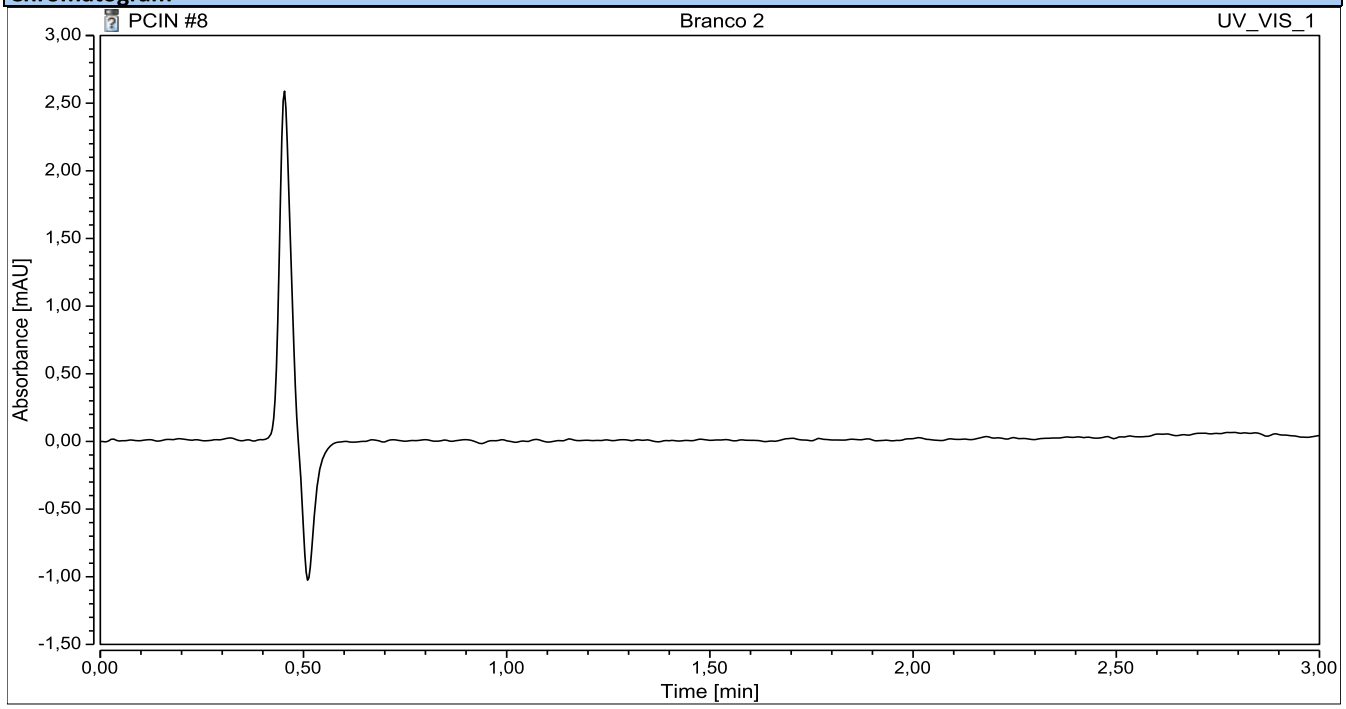

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeina	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 4**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:19**	*Sample Weight:*	**1,0000**

Chromatogram

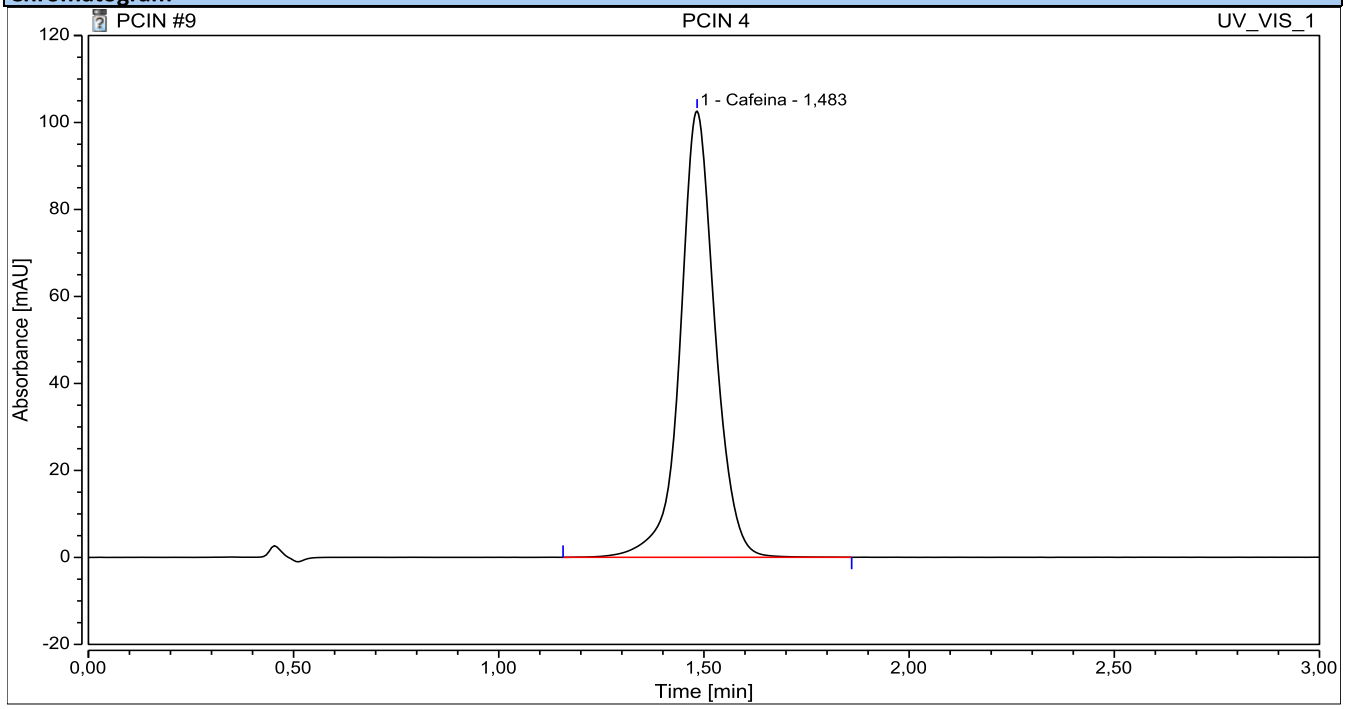

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,483	10,1087	102,602	100,00	100,00	n.a.
Total:			**10,109**	**102,602**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 5**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:23**	*Sample Weight:*	**1,0000**

Chromatogram

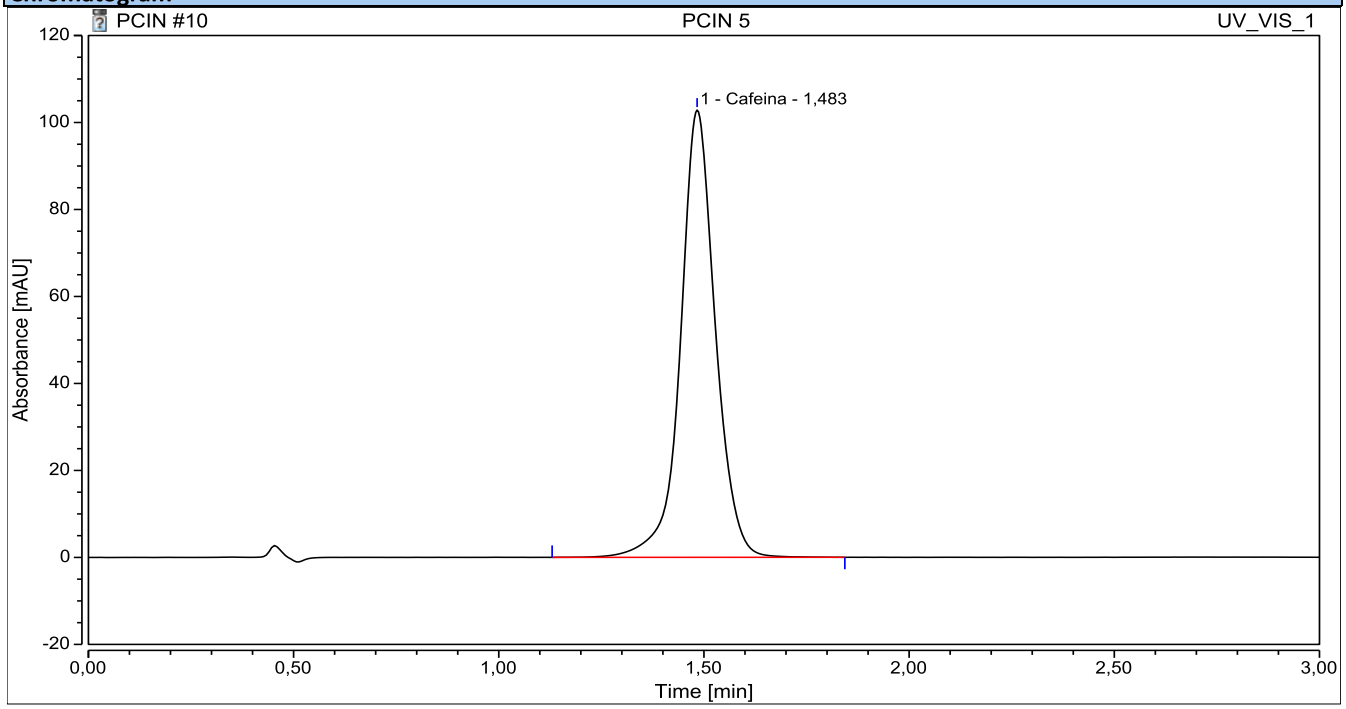

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,483	10,1085	102,840	100,00	100,00	n.a.
Total:			**10,108**	**102,840**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 6**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:27**	*Sample Weight:*	**1,0000**

Chromatogram

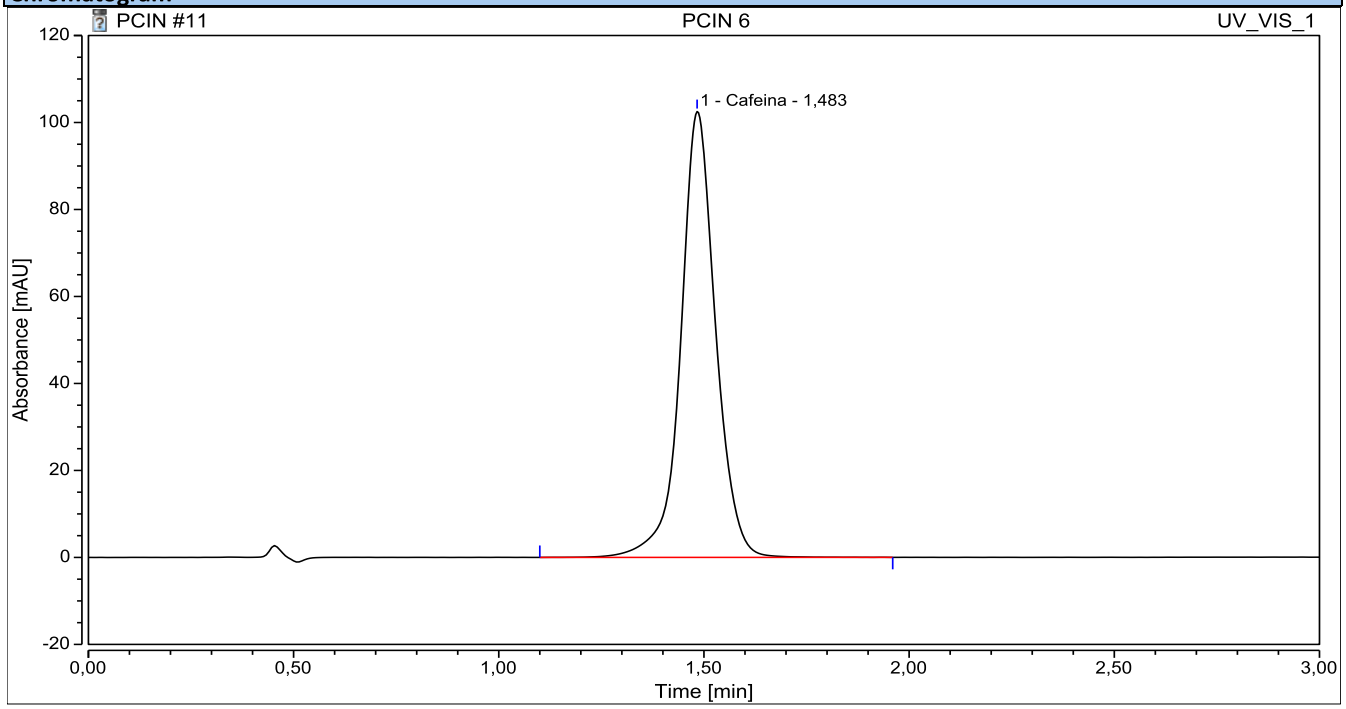

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,483	10,1011	102,513	100,00	100,00	n.a.
Total:			**10,101**	**102,513**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco 3**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 09:31**	*Sample Weight:*	**1,0000**

Chromatogram

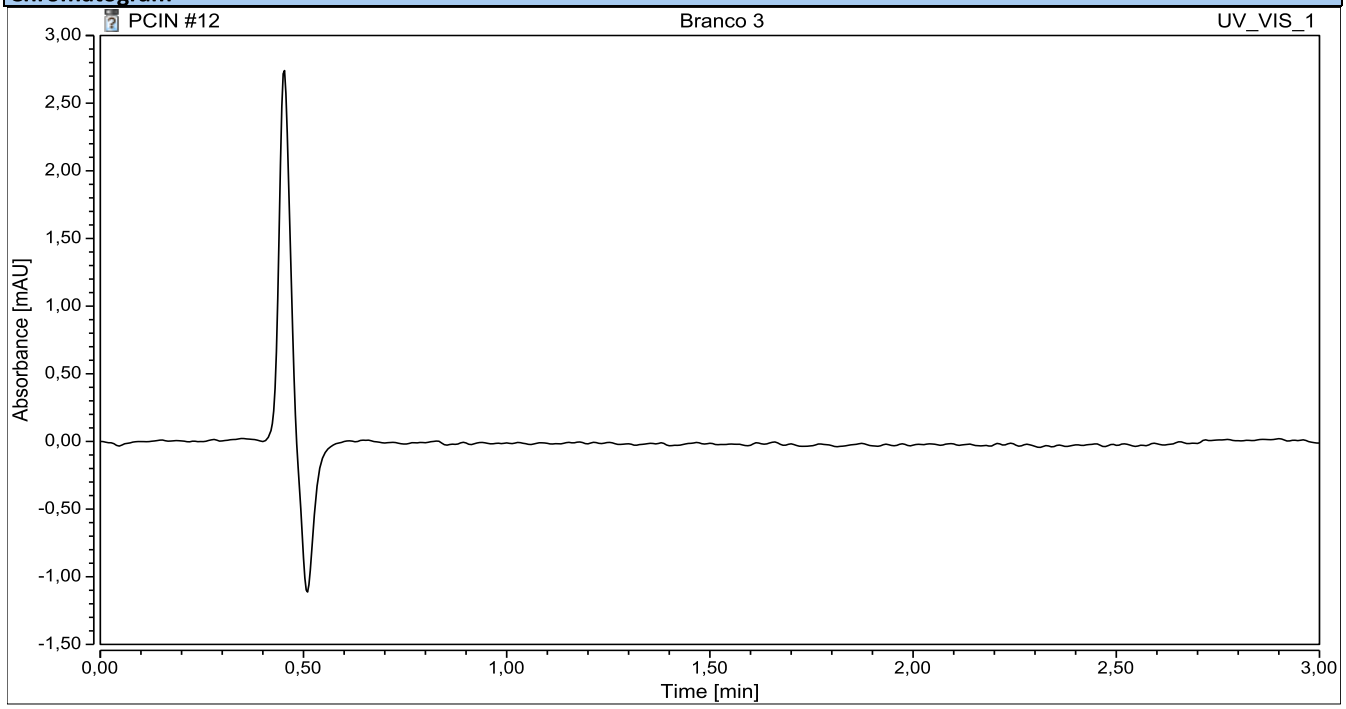

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeina	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 1**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 10:39**	*Sample Weight:*	**1,0000**

Chromatogram

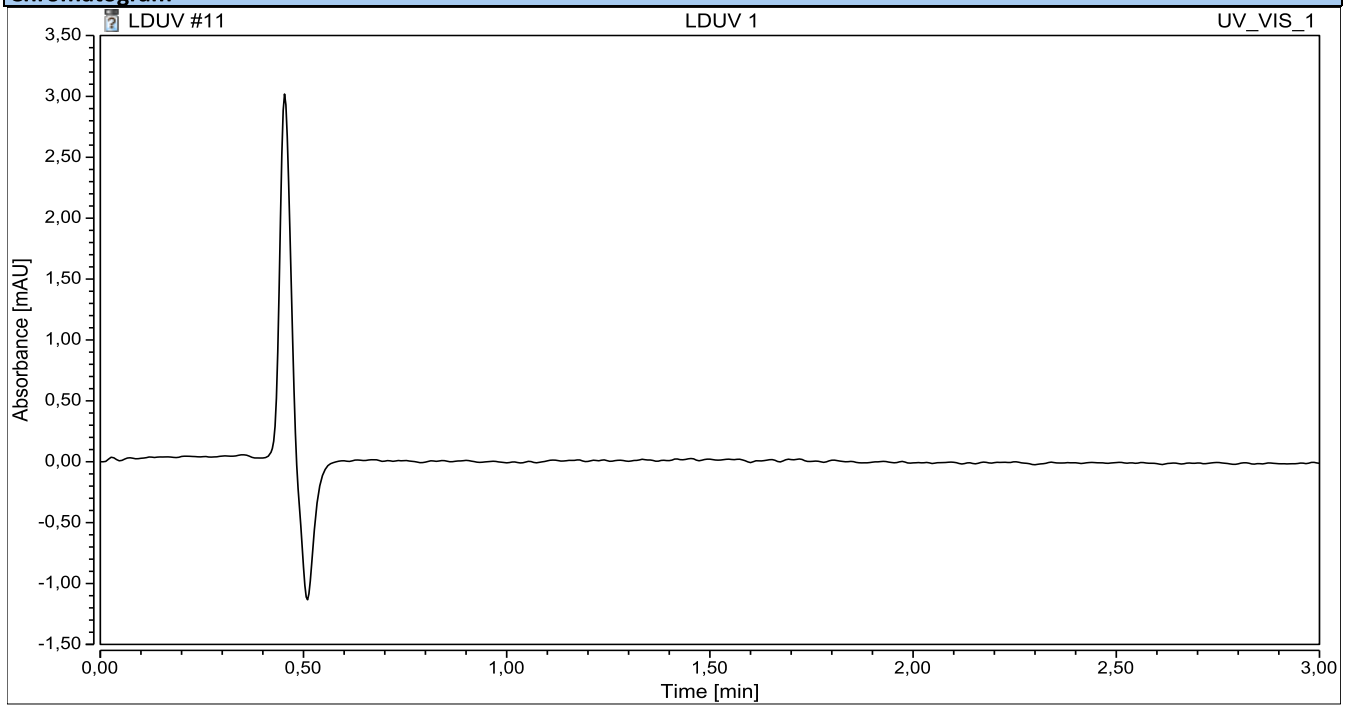

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeina	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 2**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 10:43**	*Sample Weight:*	**1,0000**

Chromatogram

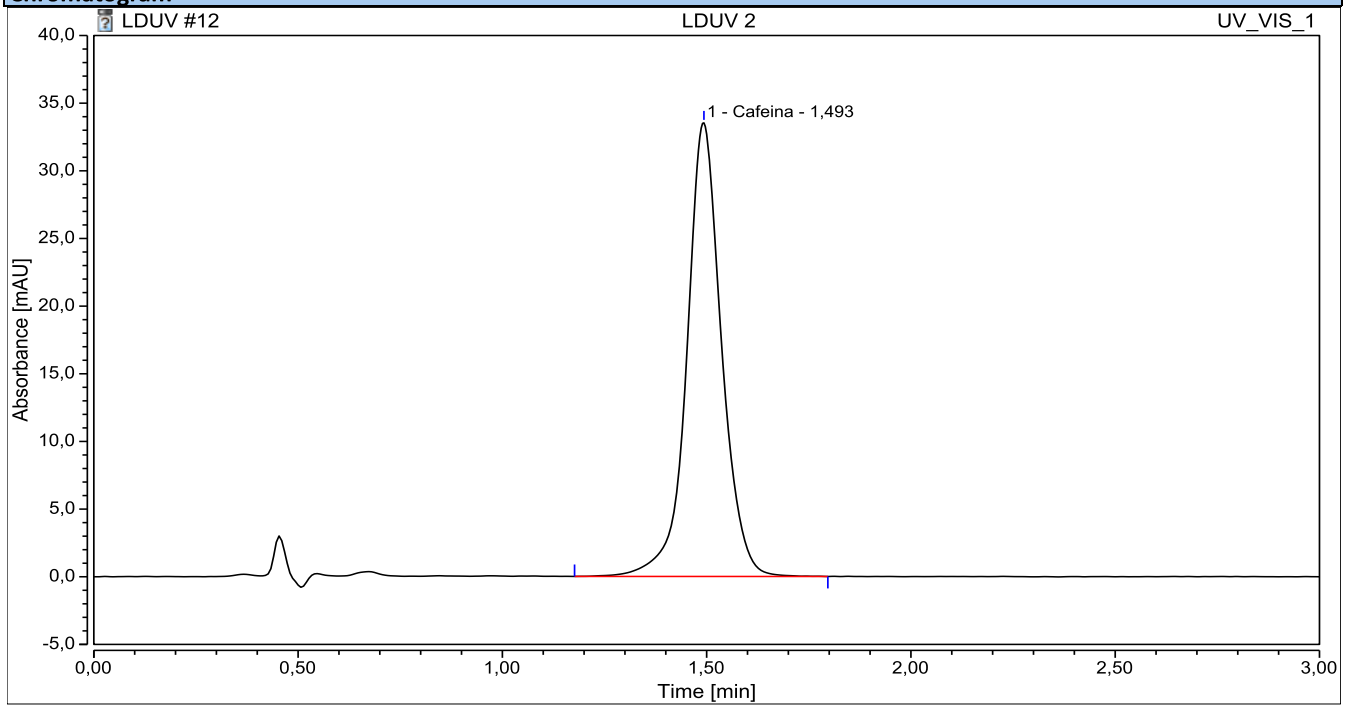

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,493	3,3055	33,523	100,00	100,00	n.a.
Total:			**3,306**	**33,523**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 3**	*Run Time (min):*	**3,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 10:47**	*Sample Weight:*	**1,0000**

Chromatogram

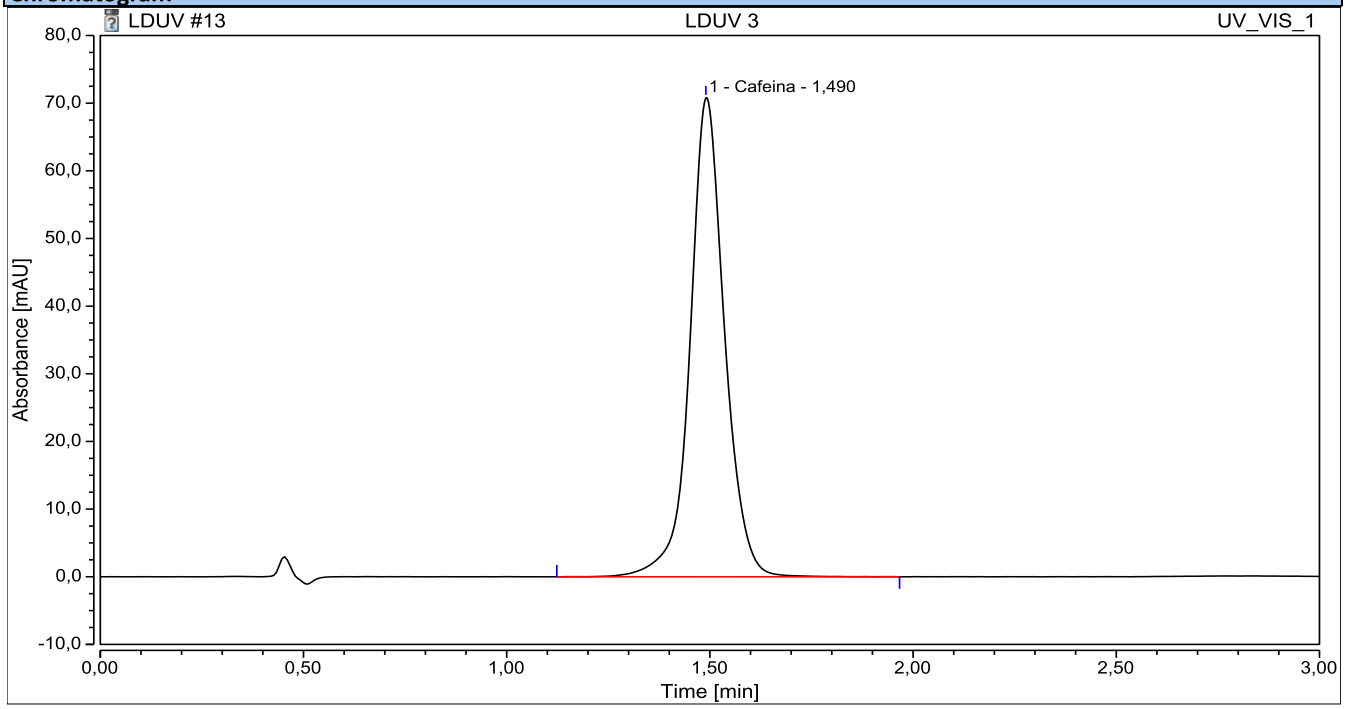

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,490	6,9820	70,801	100,00	100,00	n.a.
Total:			**6,982**	**70,801**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 4**	*Run Time (min):*	**3,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 10:50**	*Sample Weight:*	**1,0000**

Chromatogram

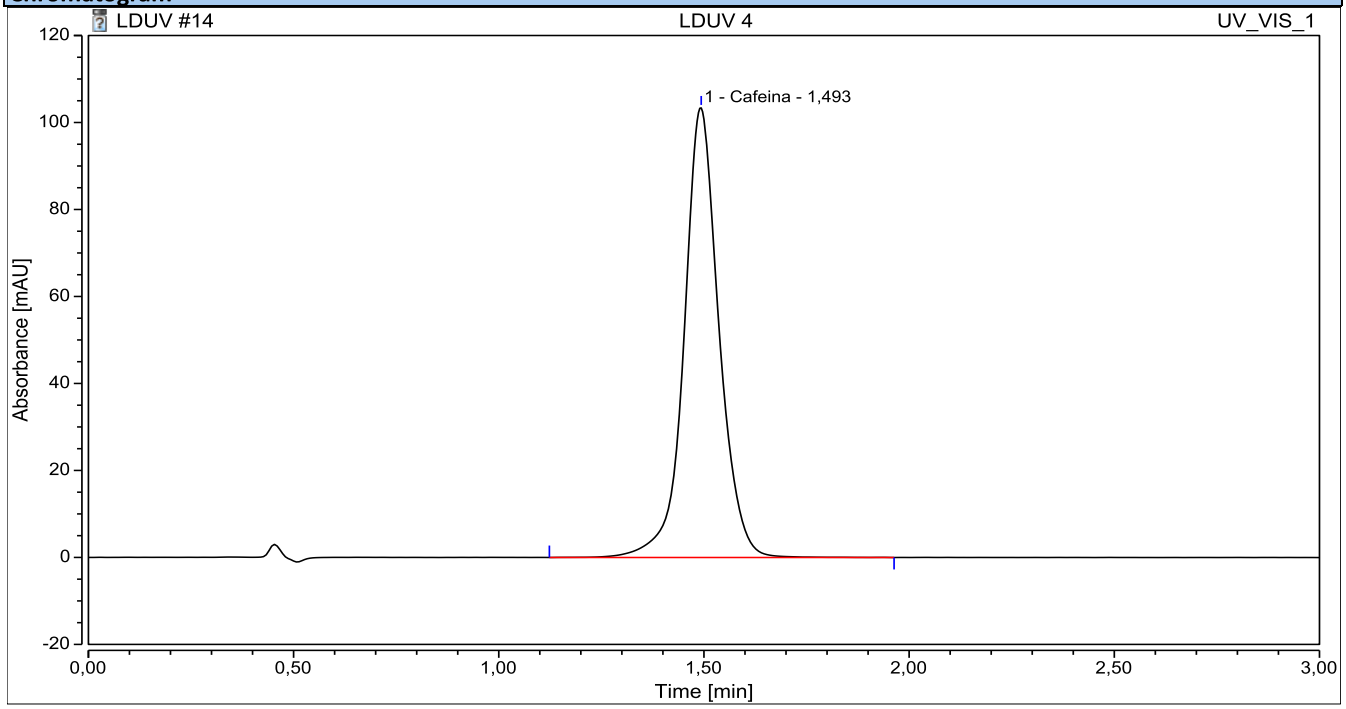

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,493	10,2044	103,370	100,00	100,00	n.a.
Total:			**10,204**	**103,370**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 5**	*Run Time (min):*	**3,00**
Vial Number:	**RA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 10:54**	*Sample Weight:*	**1,0000**

Chromatogram

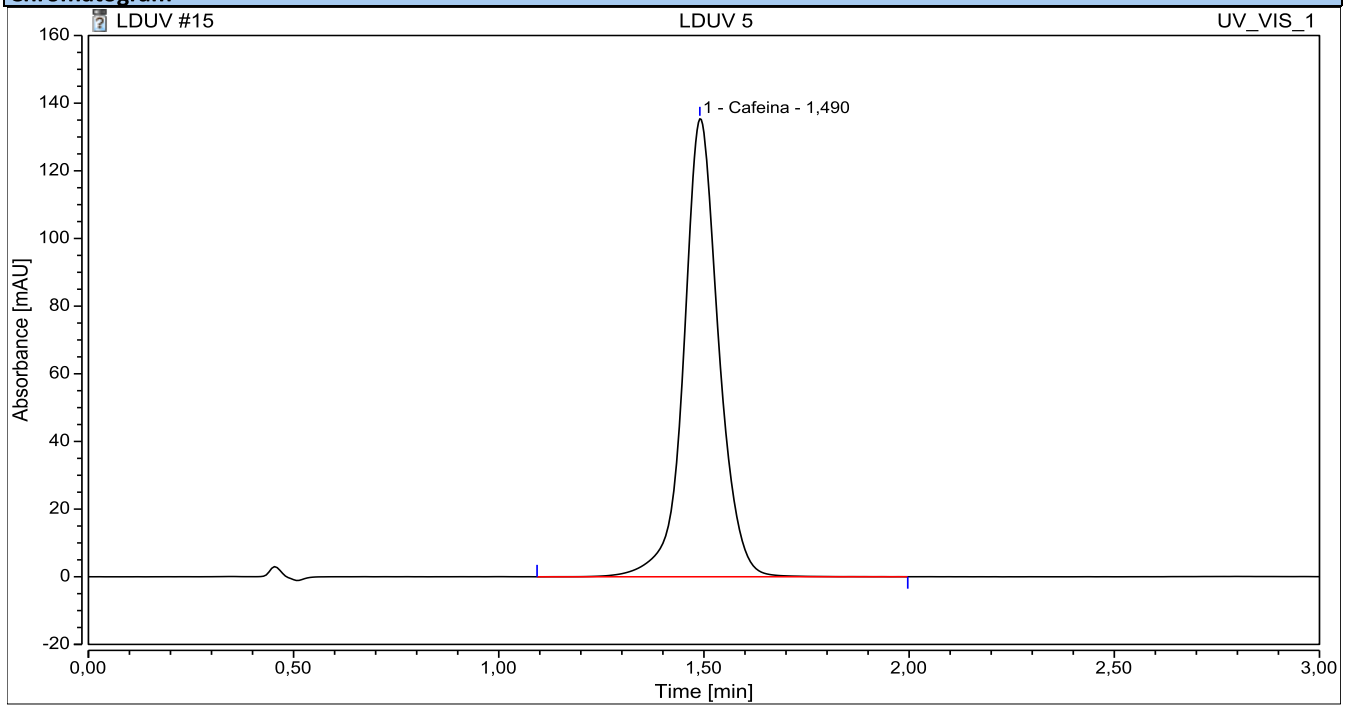

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,490	13,3493	135,392	100,00	100,00	n.a.
Total:			**13,349**	**135,392**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Sinal - Ruido**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**Sinal-Ruido**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 11:23**	*Sample Weight:*	**1,0000**

Chromatogram

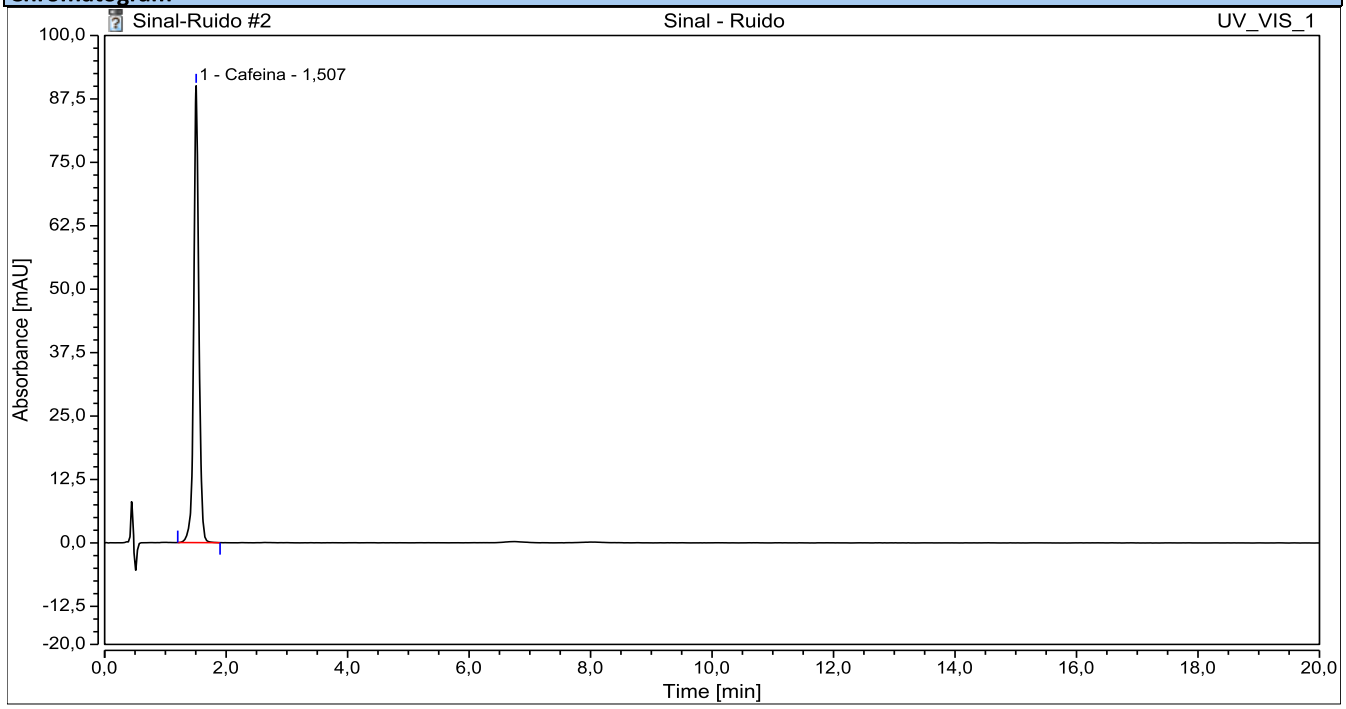

Integration Results


No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,507	8,7624	90,027	100,00	100,00	n.a.
Total:			**8,762**	**90,027**	**100,000**	**100,000**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Certificado Nº: 404/24 - RELB	Início da Qualificação: 10/09/2024	Página 1 de 3

Resultado obtido na altura do pico

	ALTURA DO PICO (mAU)
Resultado:	**90.0270**

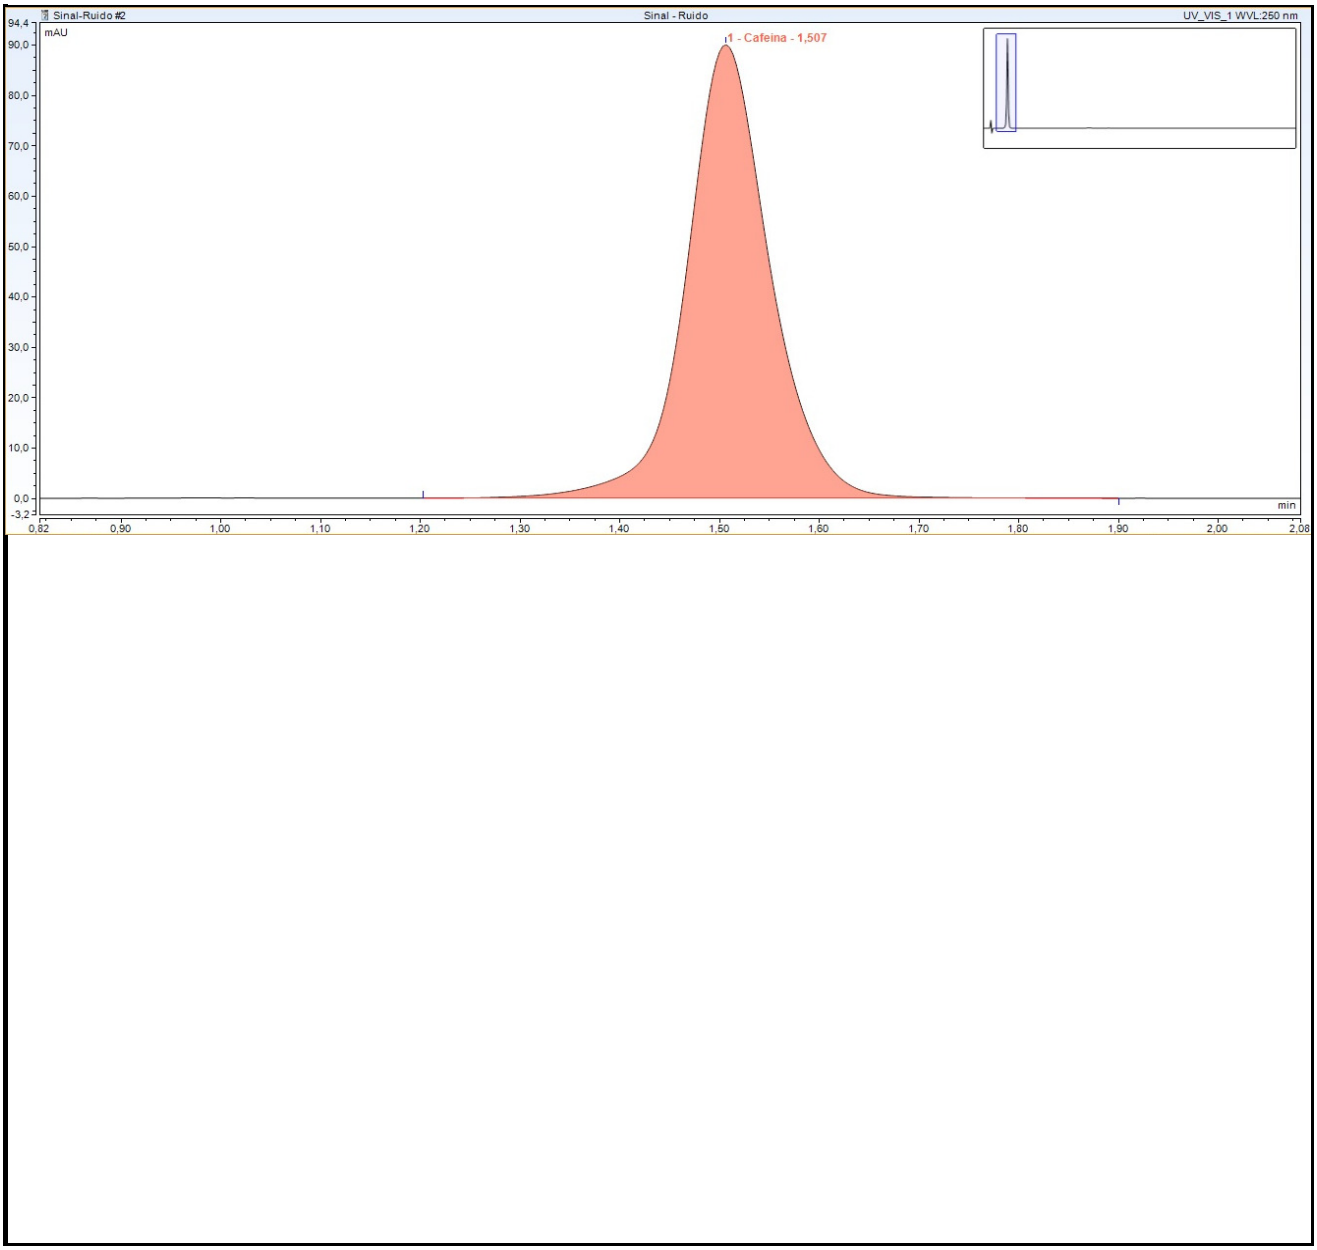


Certificado Nº: 404/24 - RELB	Início da Qualificação: 10/09/2024	Página 2 de 3

Resultado obtido no teste de sinal/ruído

Resultado:	Ruído (mAU)
VALOR MÁXIMO:	**0.0044**
VALOR MÍNIMO:	**-0.0079**


Ruído
0.0123

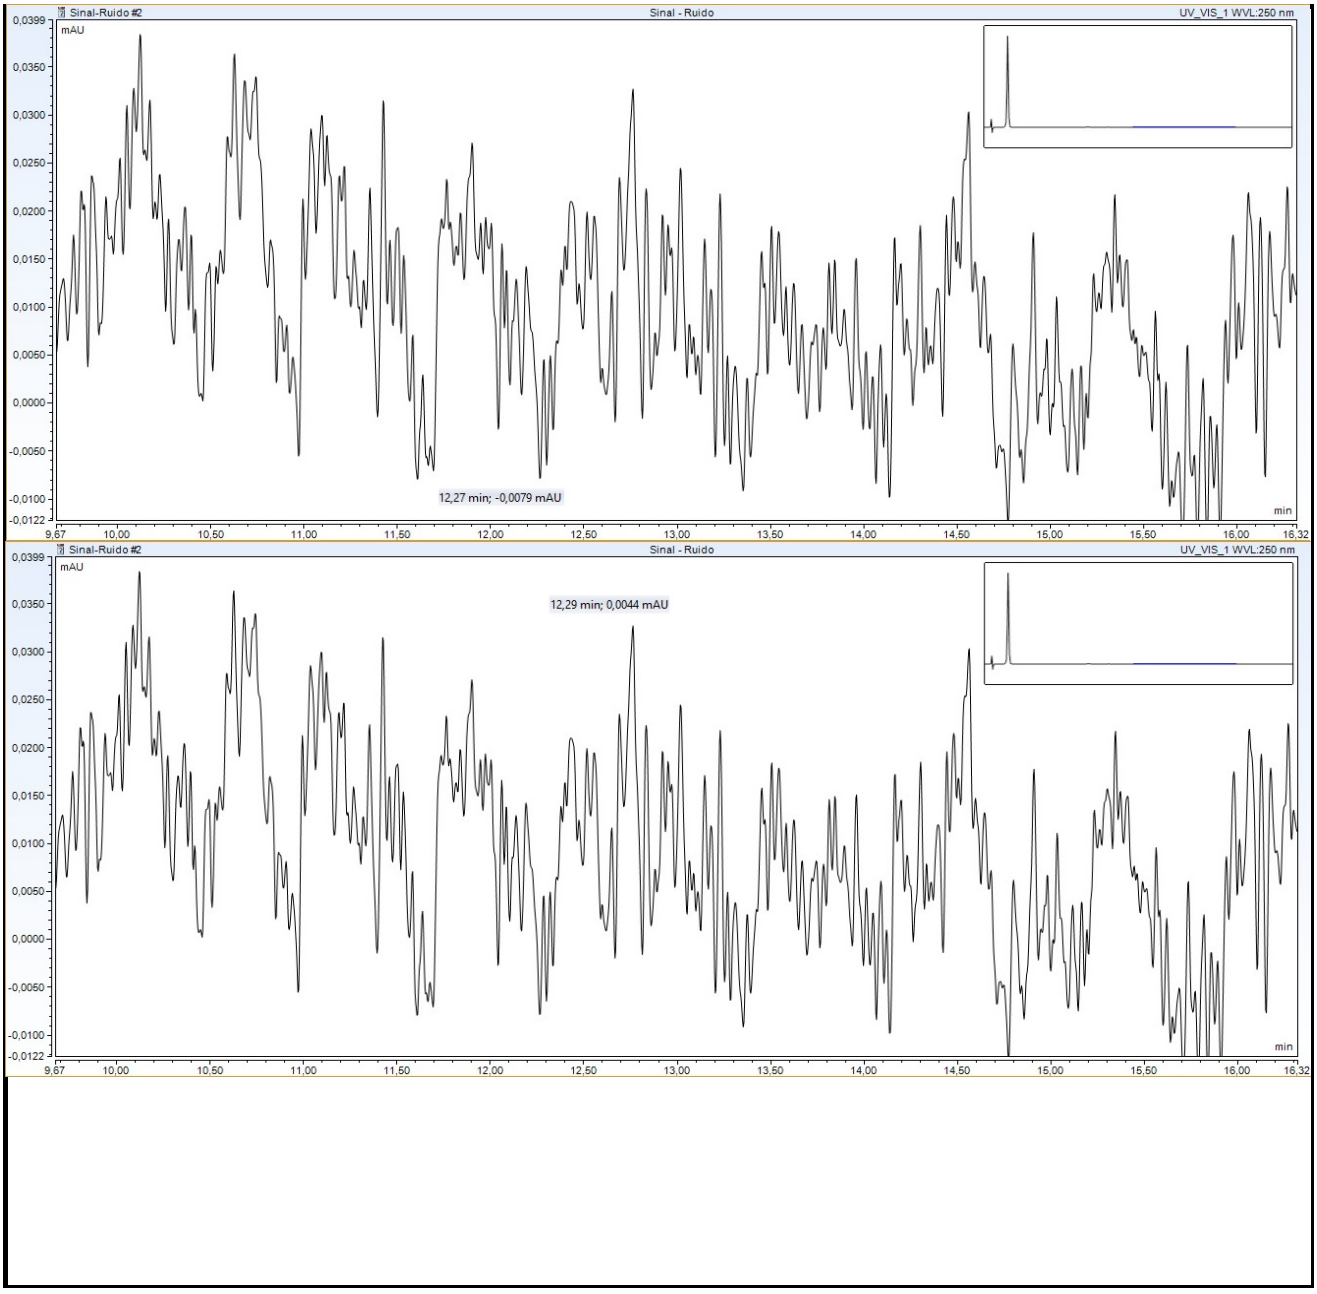

Certificado Nº: 404/24 - RELB	Início da Qualificação: 10/09/2024	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	-0.0003	0.0252
VALOR MÍNIMO:	-0.0087	
Resultado:	0.0084	

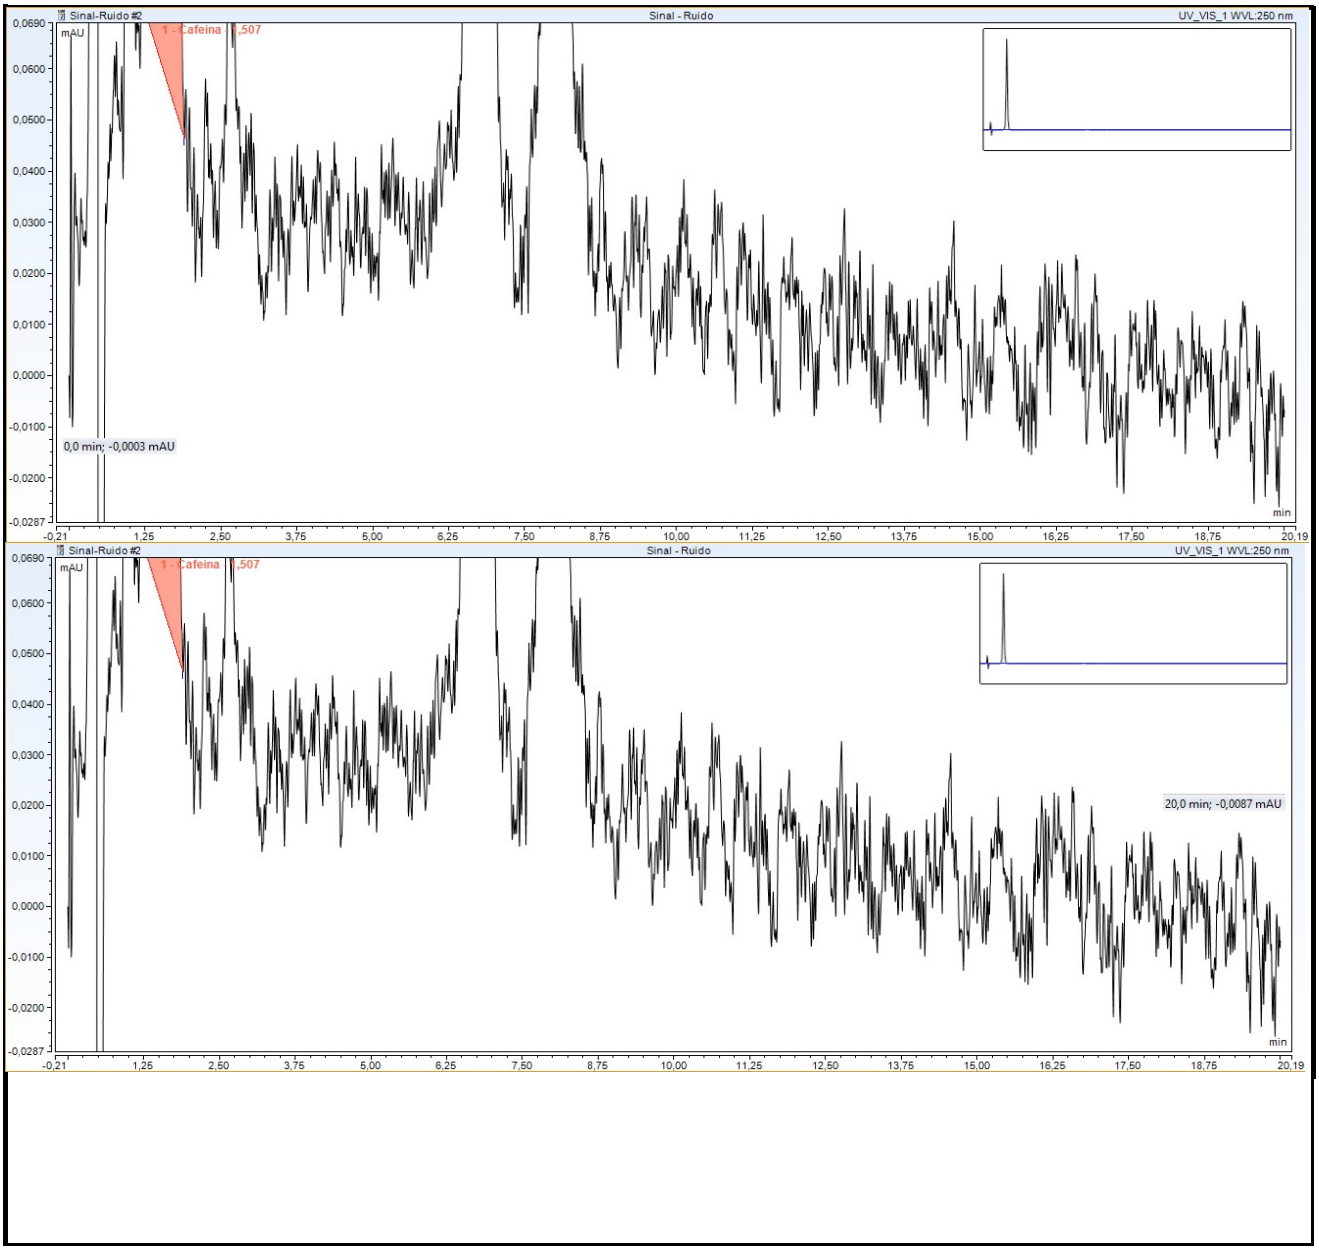


Chromatogram and Results

Injection Details

Injection Name:	**LIIN 1**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**1,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 11:53**	*Sample Weight:*	**1,0000**

Chromatogram

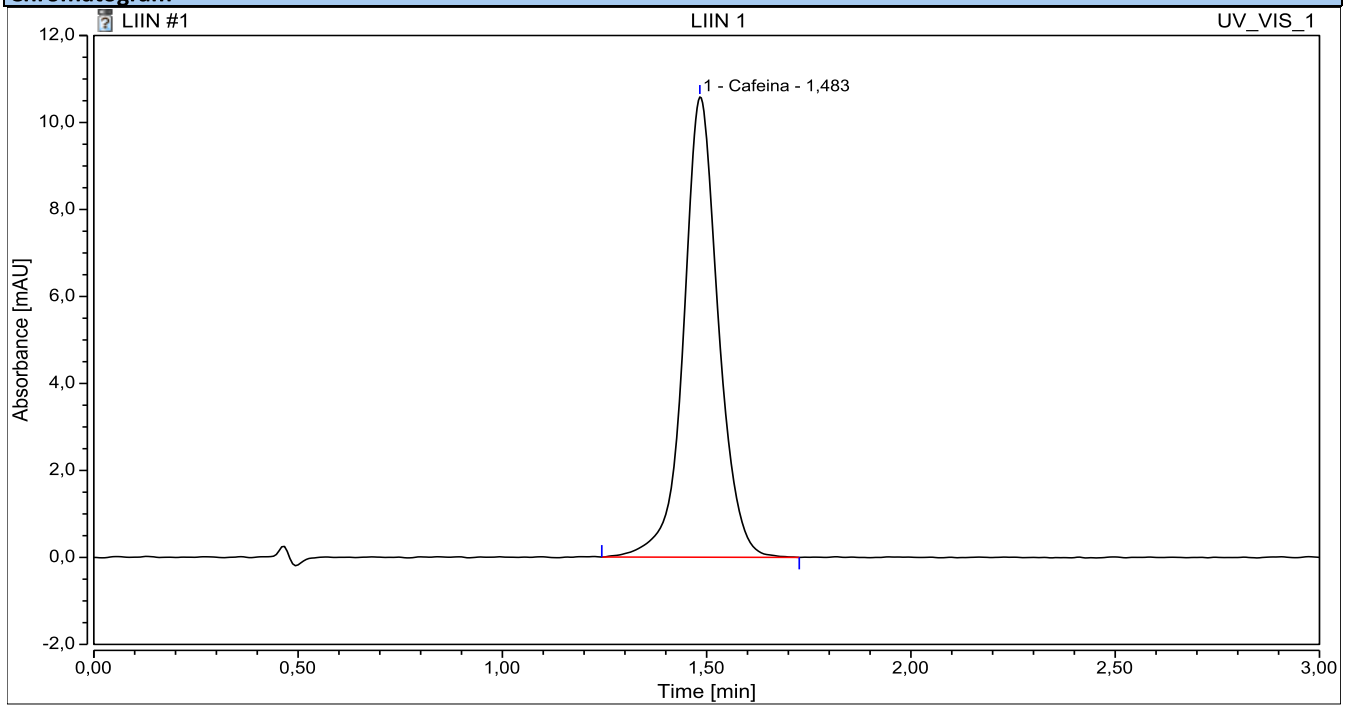

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,483	1,0438	10,582	100,00	100,00	n.a.
Total:			**1,044**	**10,582**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 2**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 11:57**	*Sample Weight:*	**1,0000**

Chromatogram

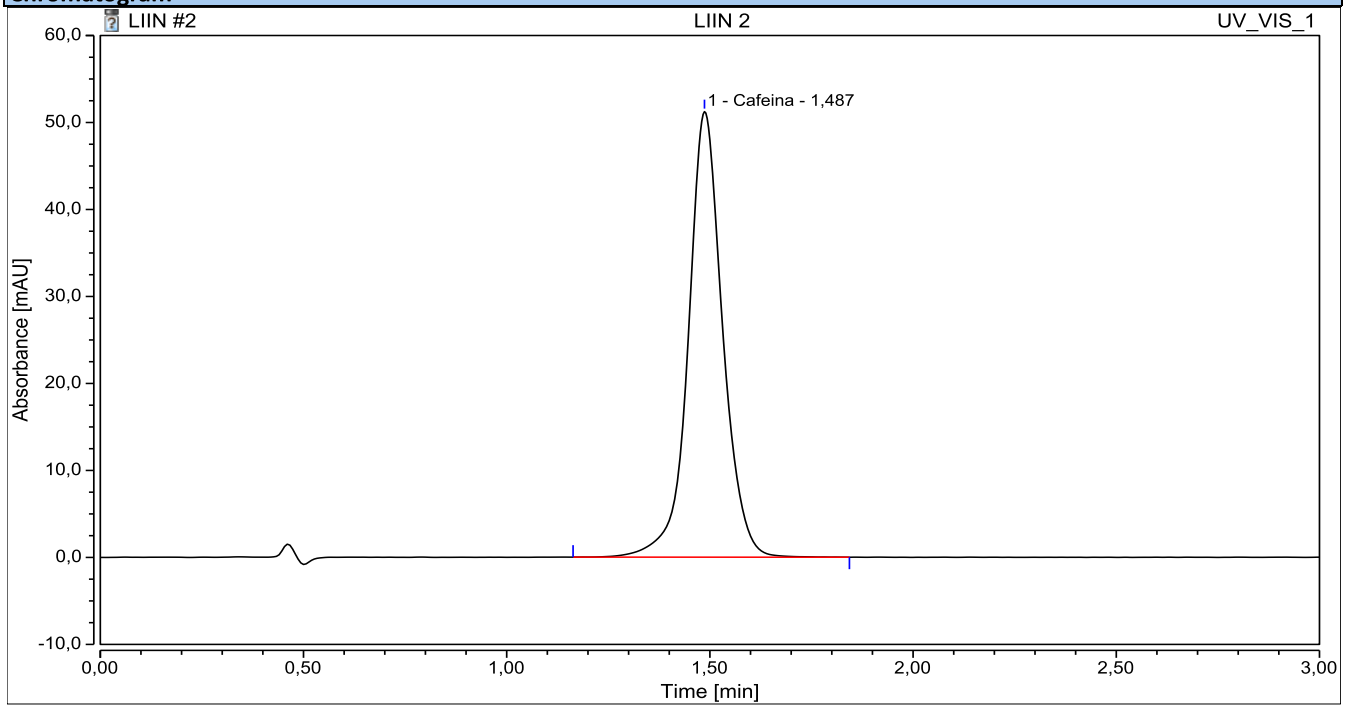

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,487	5,0223	51,222	100,00	100,00	n.a.
Total:			**5,022**	**51,222**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 3**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 12:01**	*Sample Weight:*	**1,0000**

Chromatogram

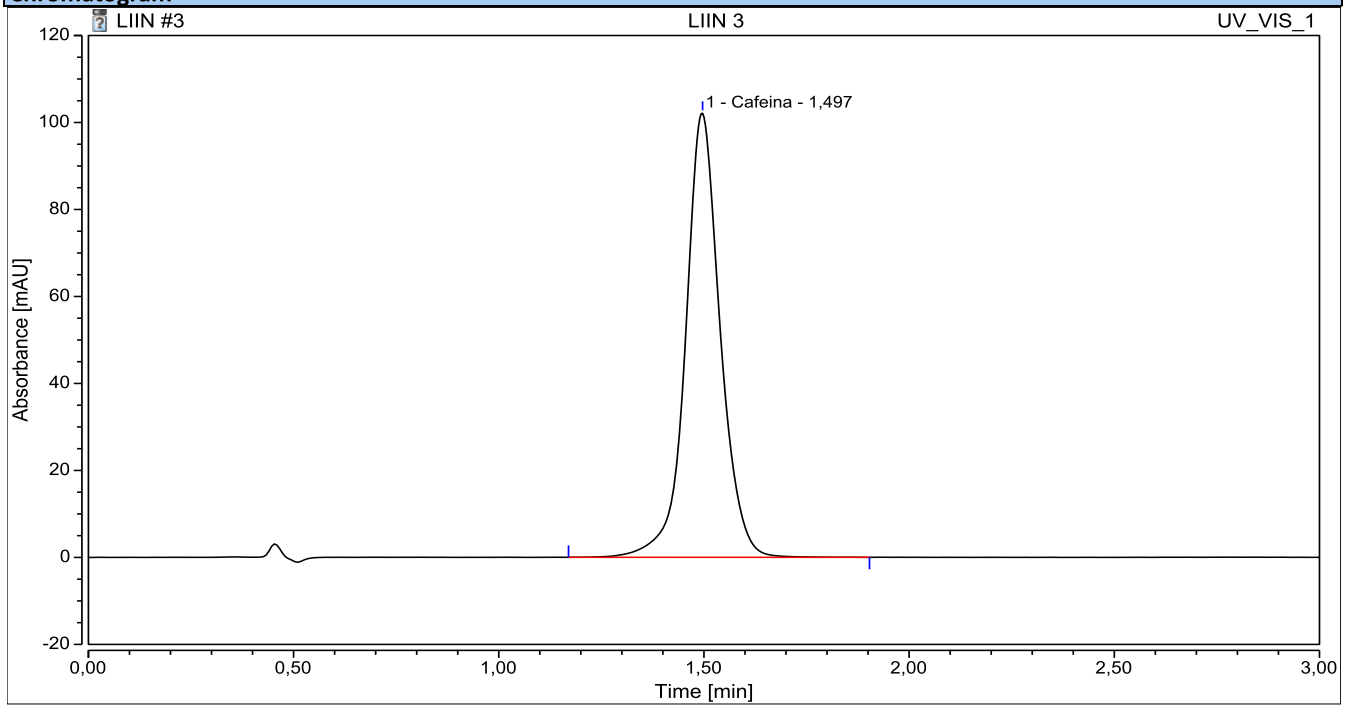

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,497	10,0172	102,092	100,00	100,00	n.a.
Total:			**10,017**	**102,092**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 4**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 12:05**	*Sample Weight:*	**1,0000**

Chromatogram

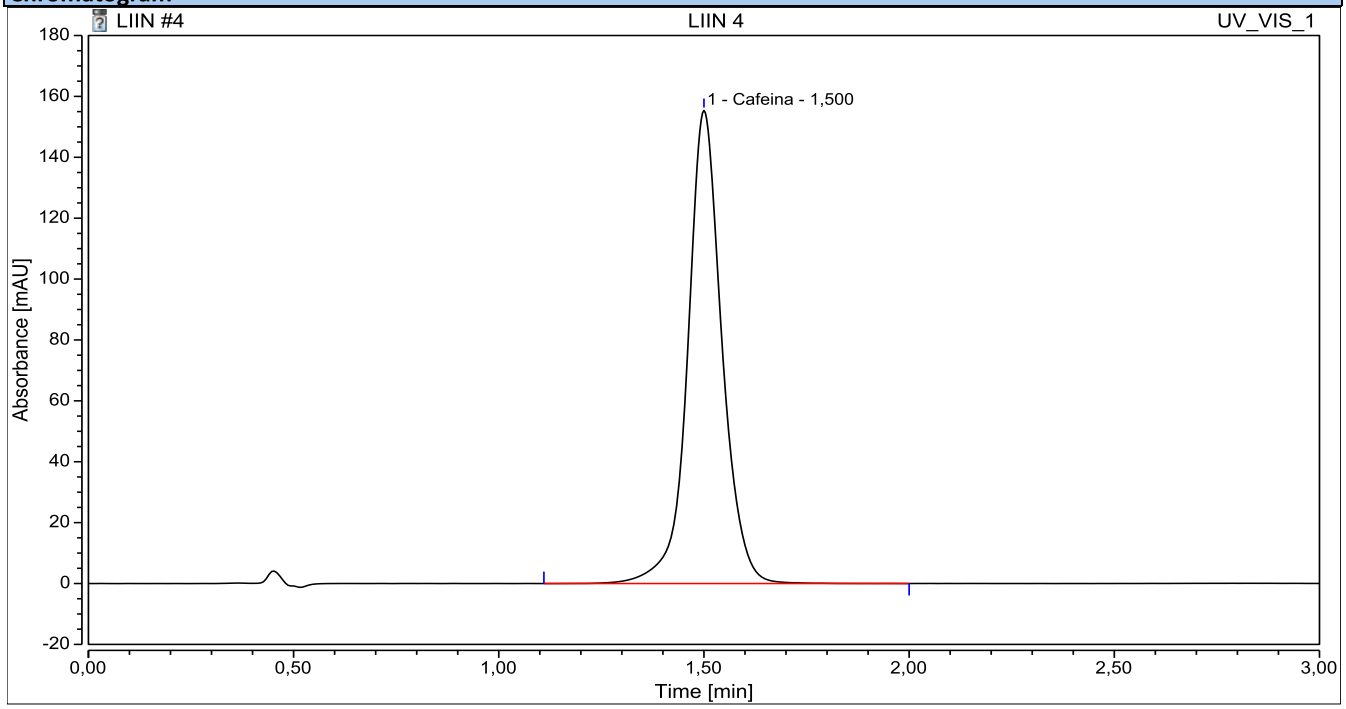

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,500	15,0473	155,372	100,00	100,00	n.a.
Total:			**15,047**	**155,372**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 5**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**3**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 12:08**	*Sample Weight:*	**1,0000**

Chromatogram

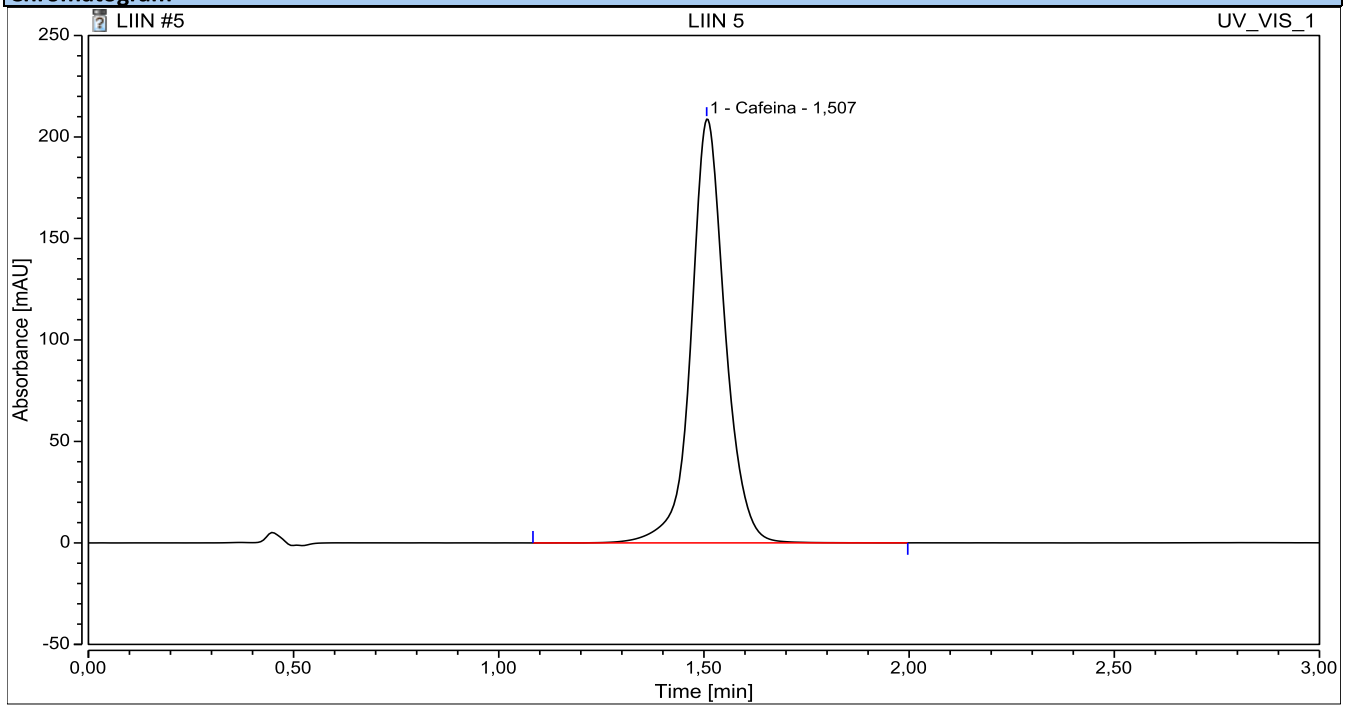

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeina	1,507	20,0575	208,787	100,00	100,00	n.a.
Total:			**20,058**	**208,787**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Grad AB**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Grad AB**	*Bandwidth:*	**3**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 15:06**	*Sample Weight:*	**1,0000**

Chromatogram

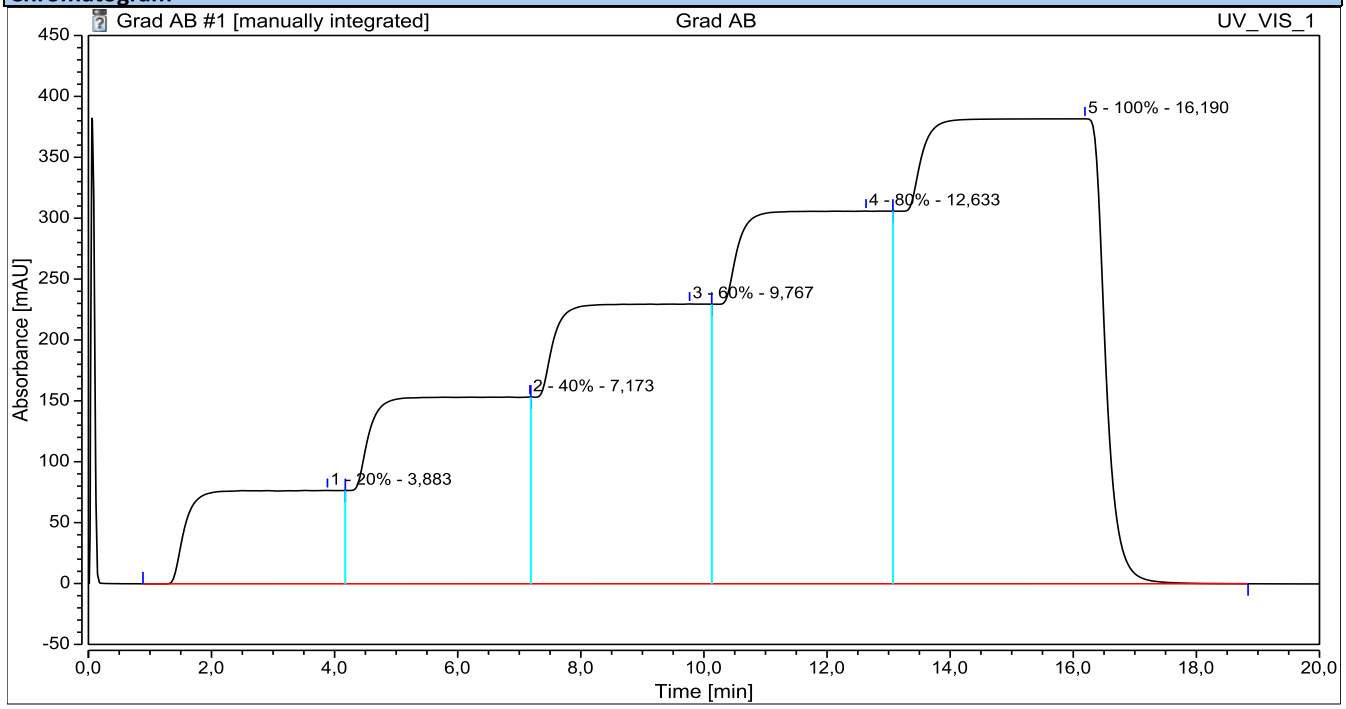

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	20%	3,883	199,6519	76,667	5,80	6,68	n.a.
2	40%	7,173	432,3348	153,348	12,56	13,36	n.a.
3	60%	9,767	646,8667	229,781	18,80	20,02	n.a.
4	80%	12,633	868,2516	306,037	25,23	26,67	n.a.
5	100%	16,190	1293,9482	381,772	37,60	33,27	n.a.
Total:			**3441,053**	**1147,606**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Grad CD**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Grad CD**	*Bandwidth:*	**3**
Processing Method:	**Gradiente**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 15:32**	*Sample Weight:*	**1,0000**

Chromatogram

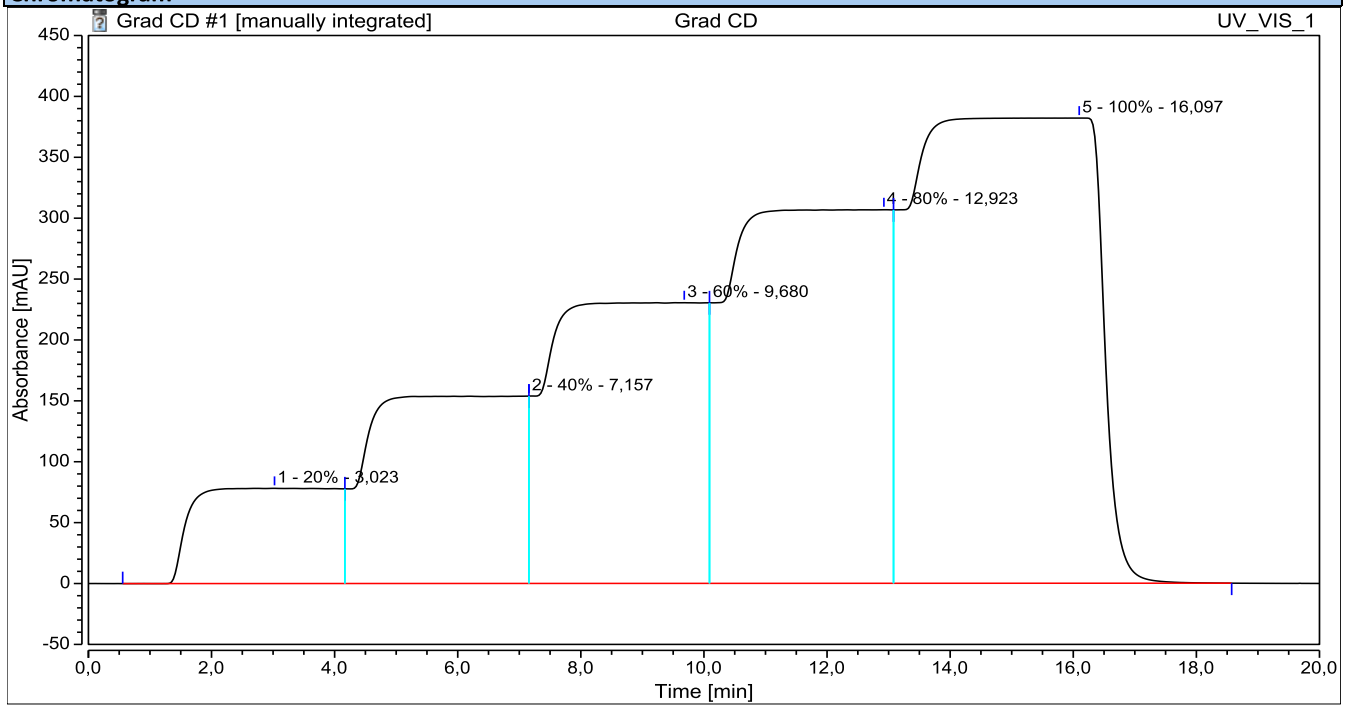

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	20%	3,023	203,1451	78,192	5,88	6,79	n.a.
2	40%	7,157	430,1937	153,855	12,46	13,36	n.a.
3	60%	9,680	645,3139	230,480	18,69	20,02	n.a.
4	80%	12,923	881,9775	306,757	25,55	26,65	n.a.
5	100%	16,097	1291,8025	381,965	37,42	33,18	n.a.
Total:			**3452,433**	**1151,249**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 1**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:32**	*Sample Weight:*	**1,0000**

Chromatogram

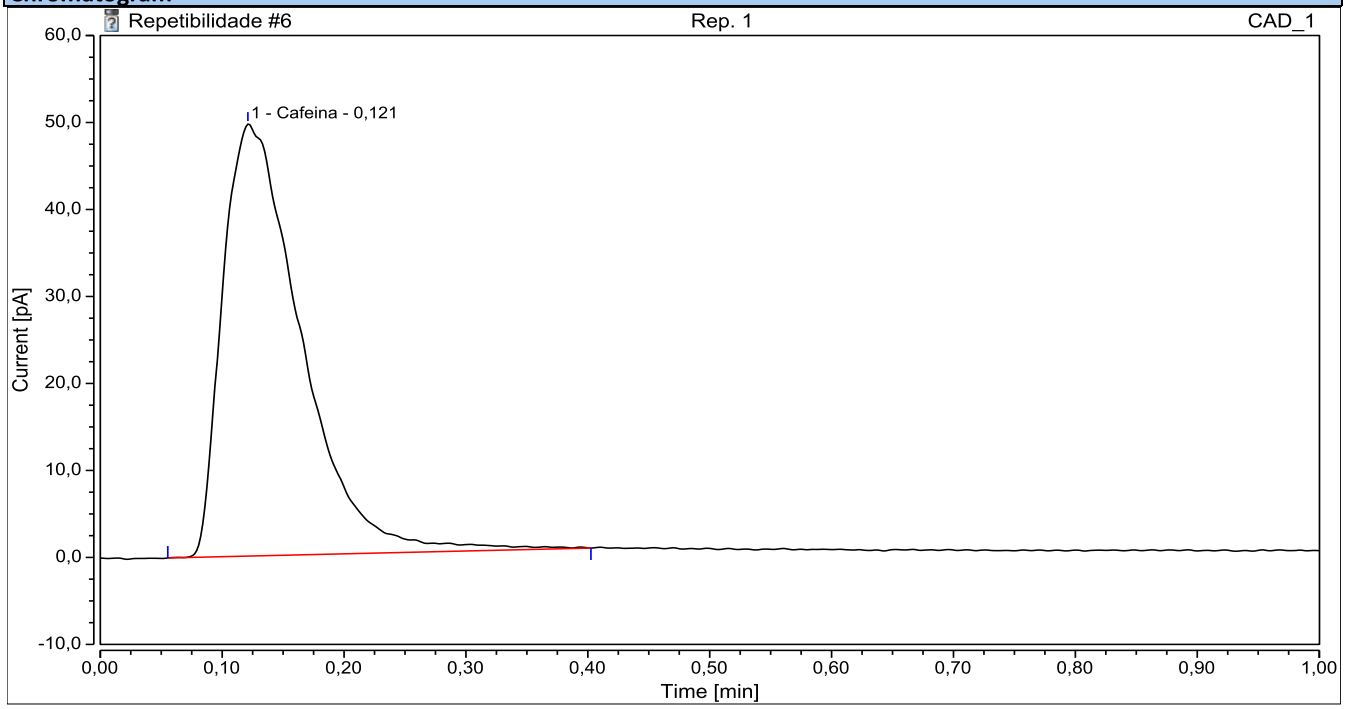

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,121	3,7050	49,667	100,00	100,00	n.a.
Total:			**3,705**	**49,667**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 2**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:34**	*Sample Weight:*	**1,0000**

Chromatogram

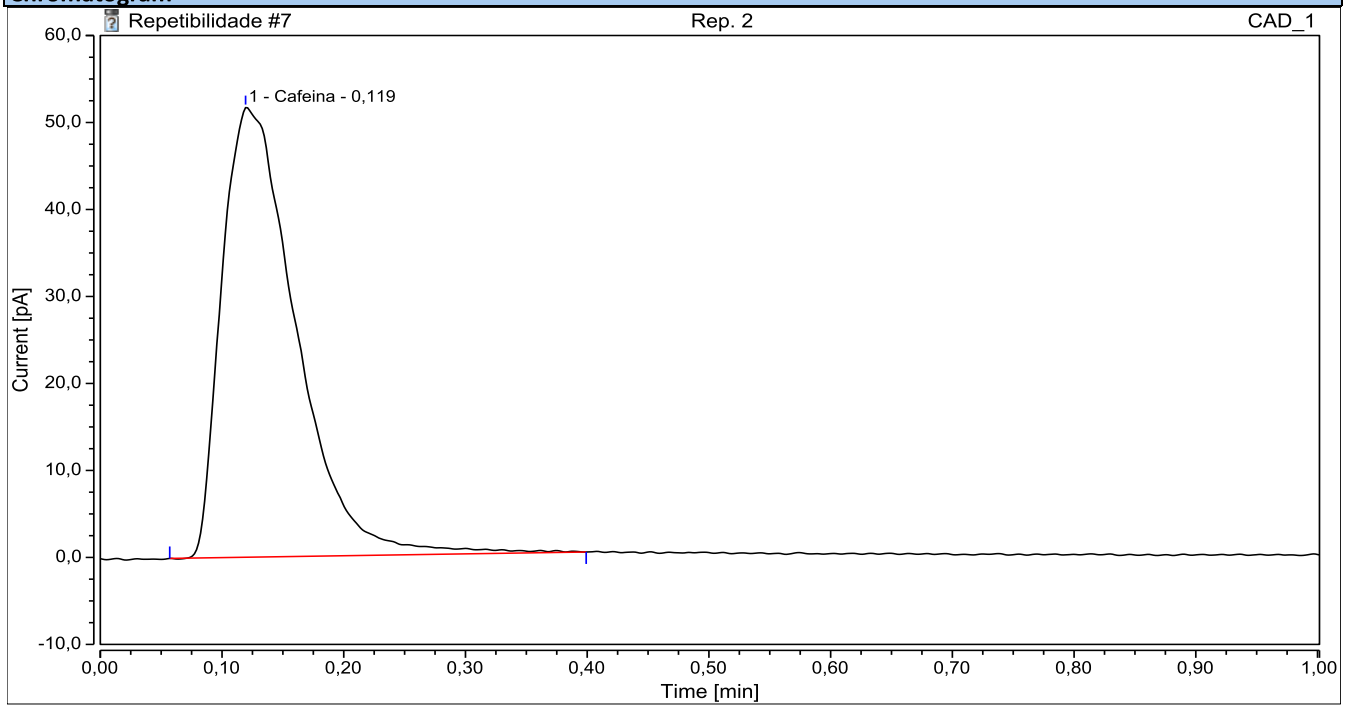

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,119	3,6573	51,696	100,00	100,00	n.a.
Total:			**3,657**	**51,696**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 3**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:36**	*Sample Weight:*	**1,0000**

Chromatogram

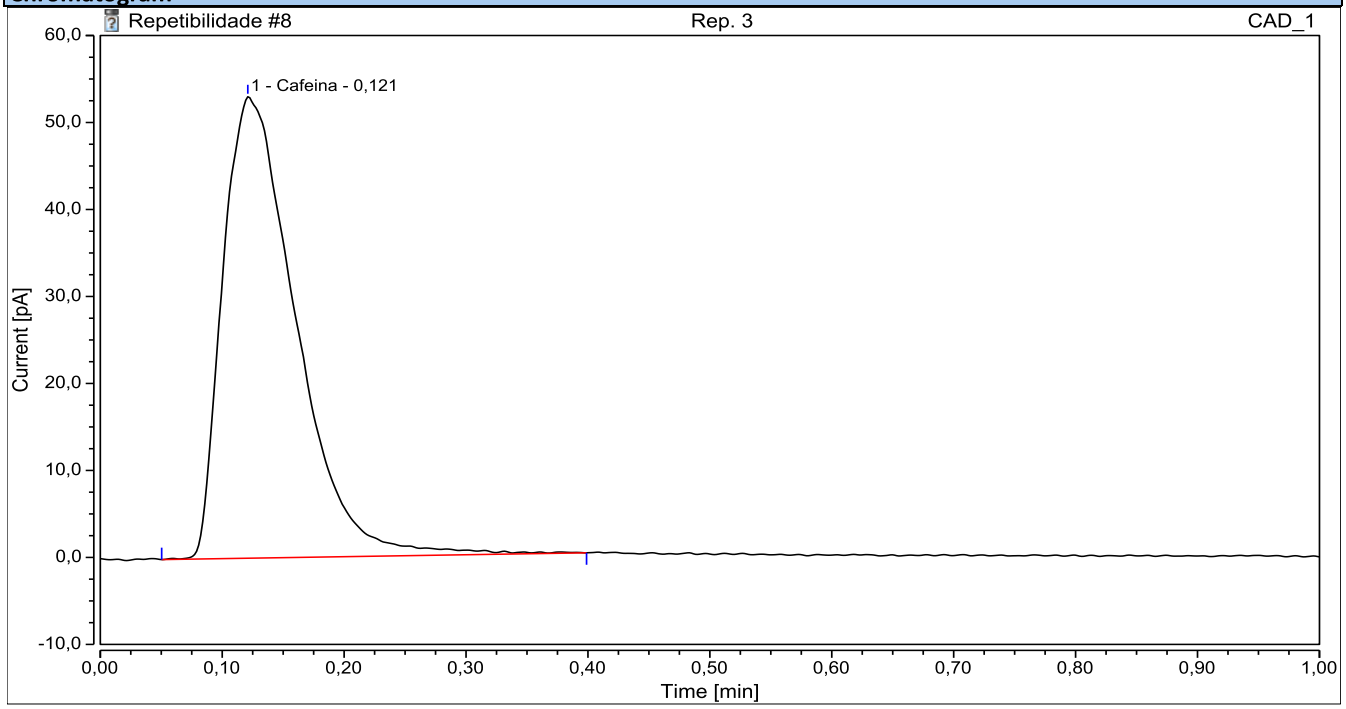

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,121	3,6889	53,054	100,00	100,00	n.a.
Total:			**3,689**	**53,054**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 4**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:38**	*Sample Weight:*	**1,0000**

Chromatogram

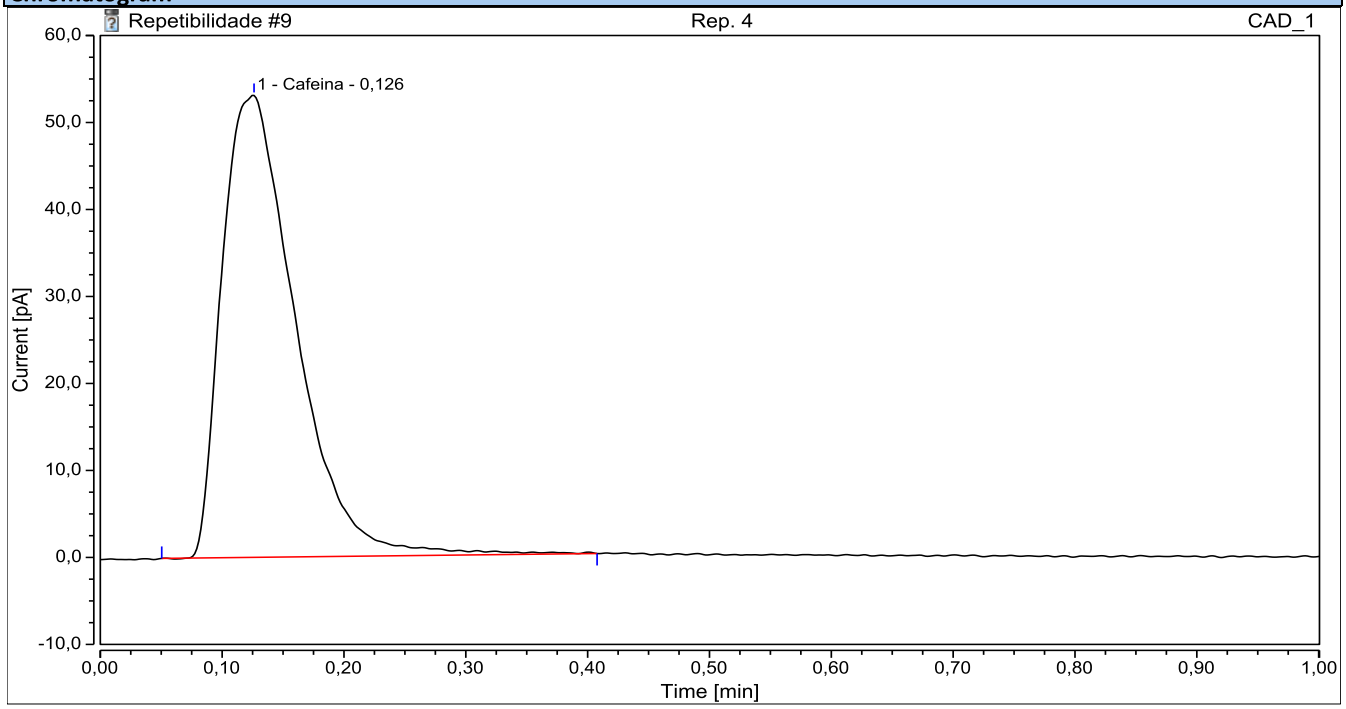

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,126	3,7102	53,105	100,00	100,00	n.a.
Total:			**3,710**	**53,105**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 5**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:40**	*Sample Weight:*	**1,0000**

Chromatogram

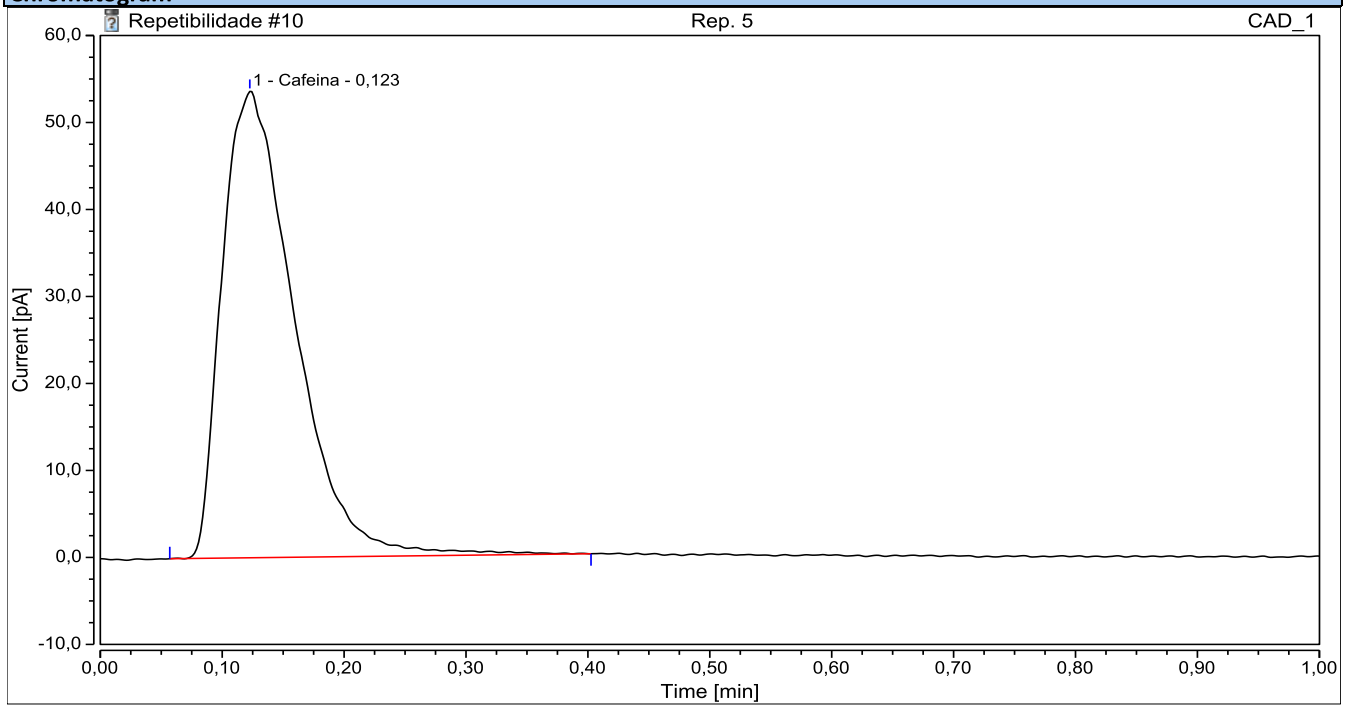

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,123	3,6897	53,618	100,00	100,00	n.a.
Total:			**3,690**	**53,618**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Rep. 6**	*Run Time (min):*	**1,00**
Vial Number:	**RA1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação Corona**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação Corona**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/24 14:42**	*Sample Weight:*	**1,0000**

Chromatogram

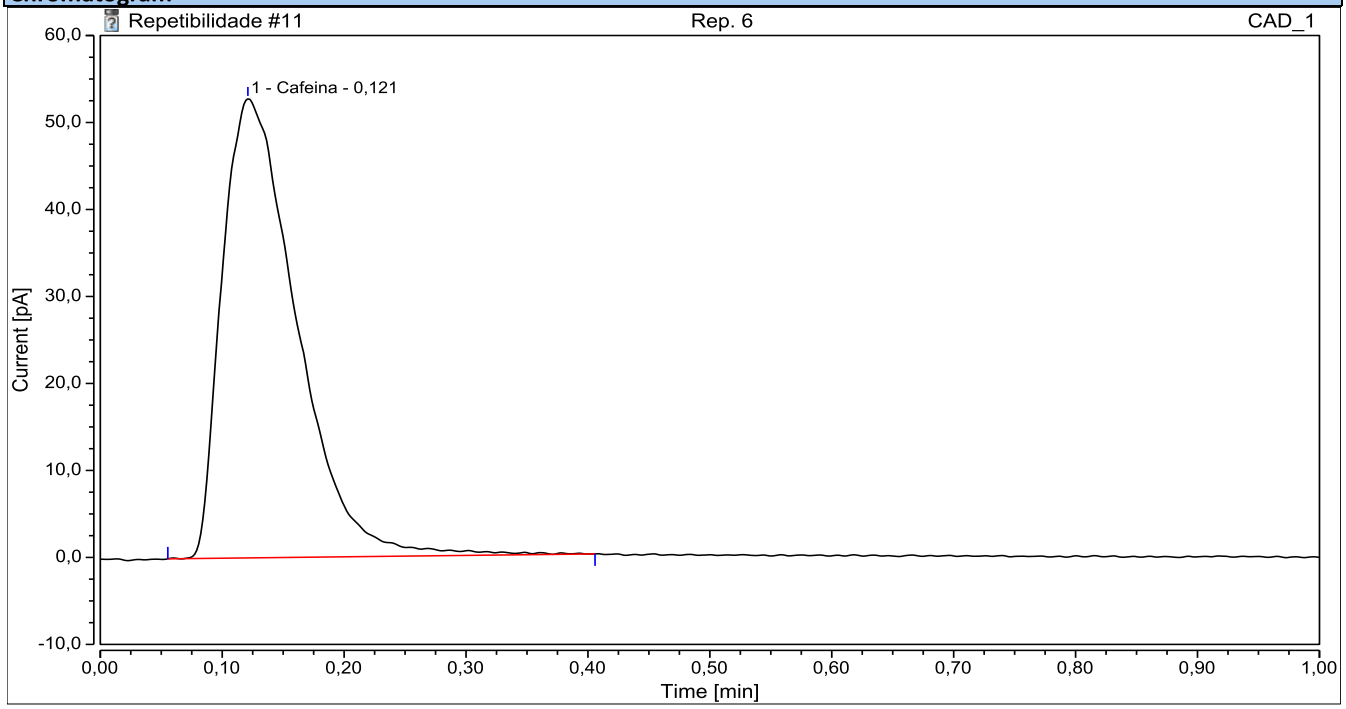

Integration Results

No.	Peakname	RetentionTime min	Area pA*min	Height pA	Relative Area %	Rel.Height %	Amount
1	Cafeina	0,121	3,7379	52,771	100,00	100,00	n.a.
Total:			**3,738**	**52,771**	**100,000**	**100,000**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.