
Chromatogram

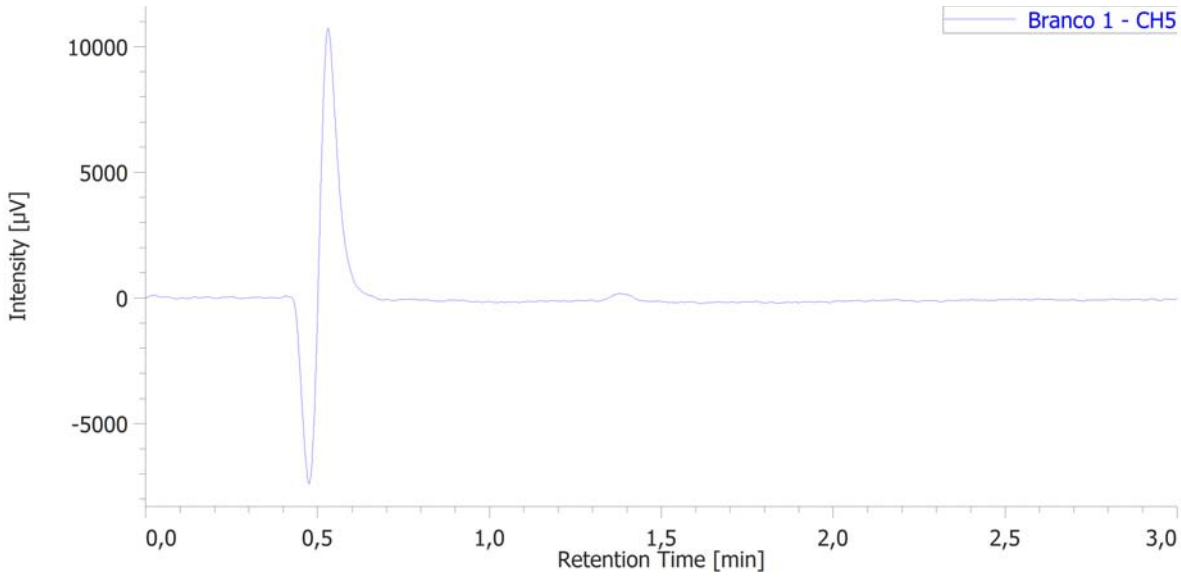


Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:04
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:29:18
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

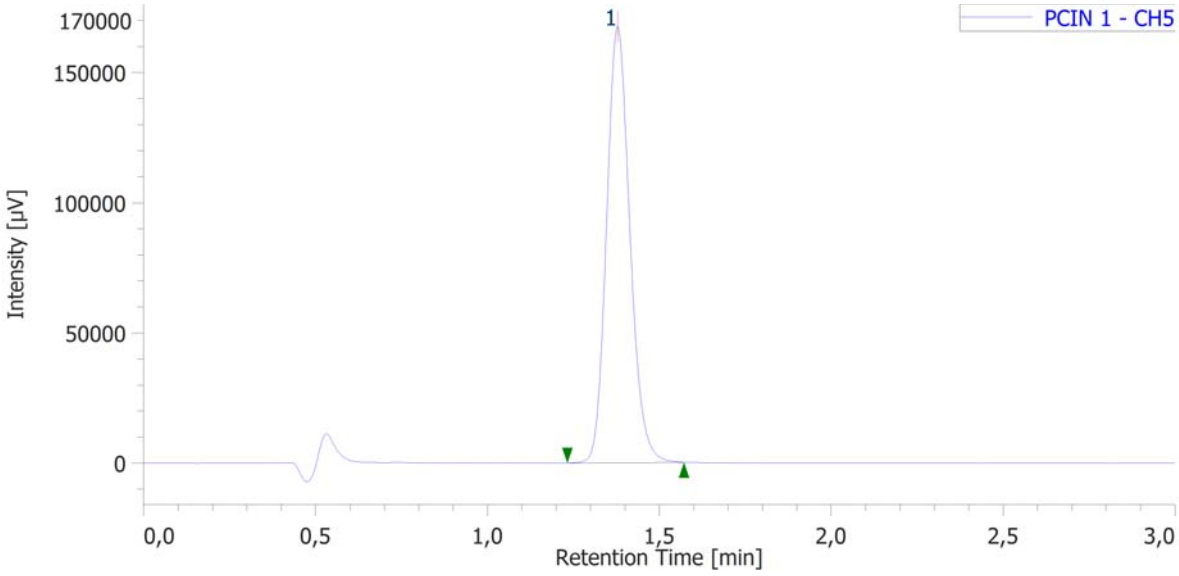

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:05
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:32:30
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,378	789326	167523	100,000	100,000	N/A	2033	N/A	1,152		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

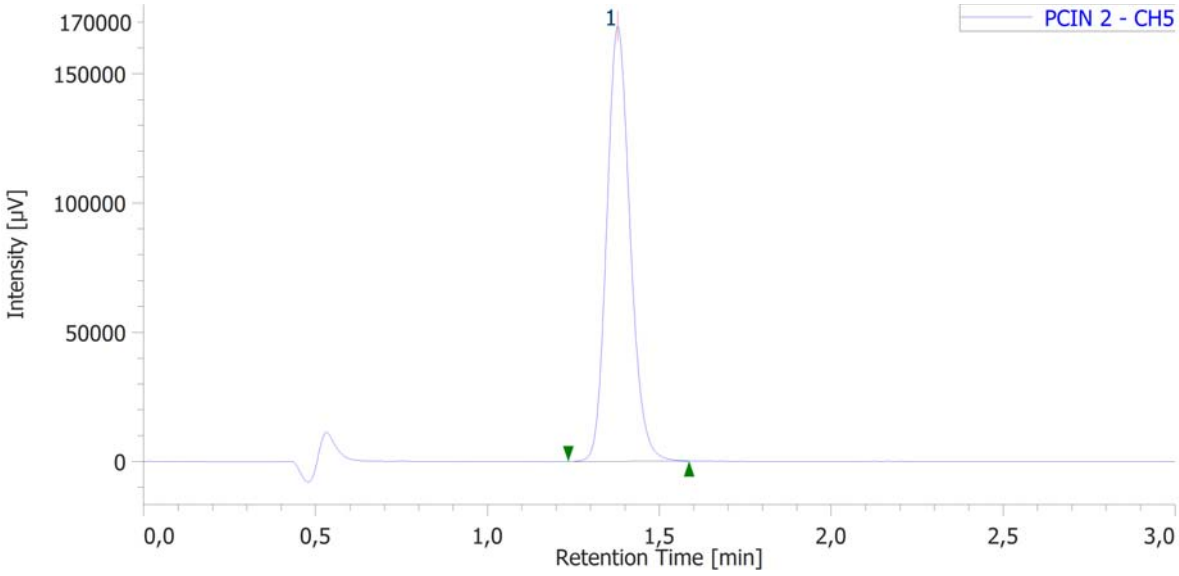

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:05
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:35:42
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,378	794145	168166	100,000	100,000	N/A	2025	N/A	1,163		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

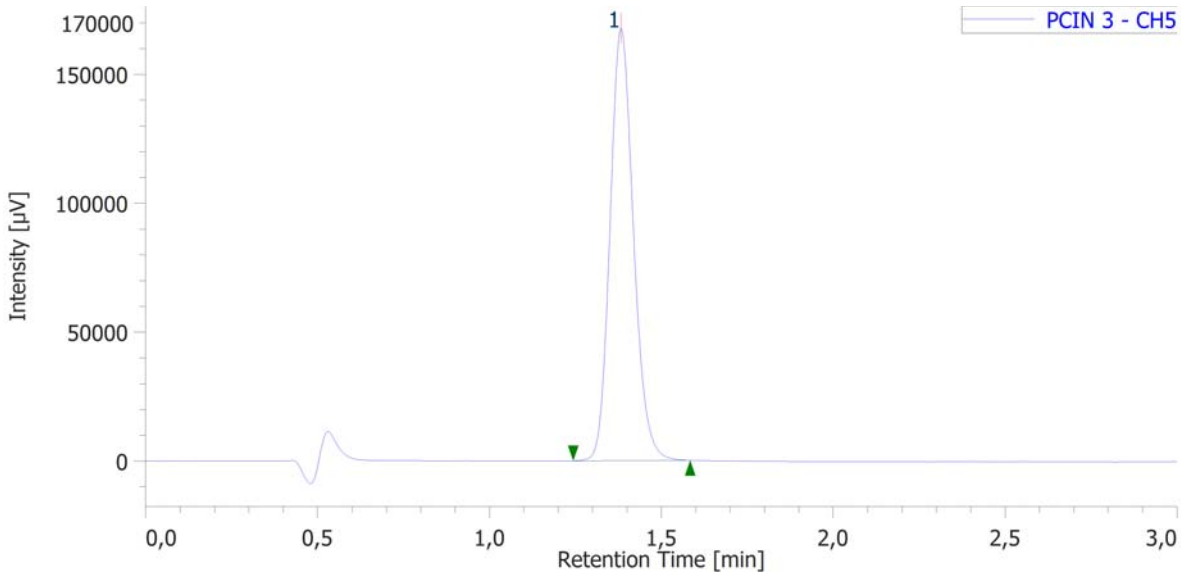

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:05
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:38:54
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,382	793056	167637	100,000	100,000	N/A	2028	N/A	1,174		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

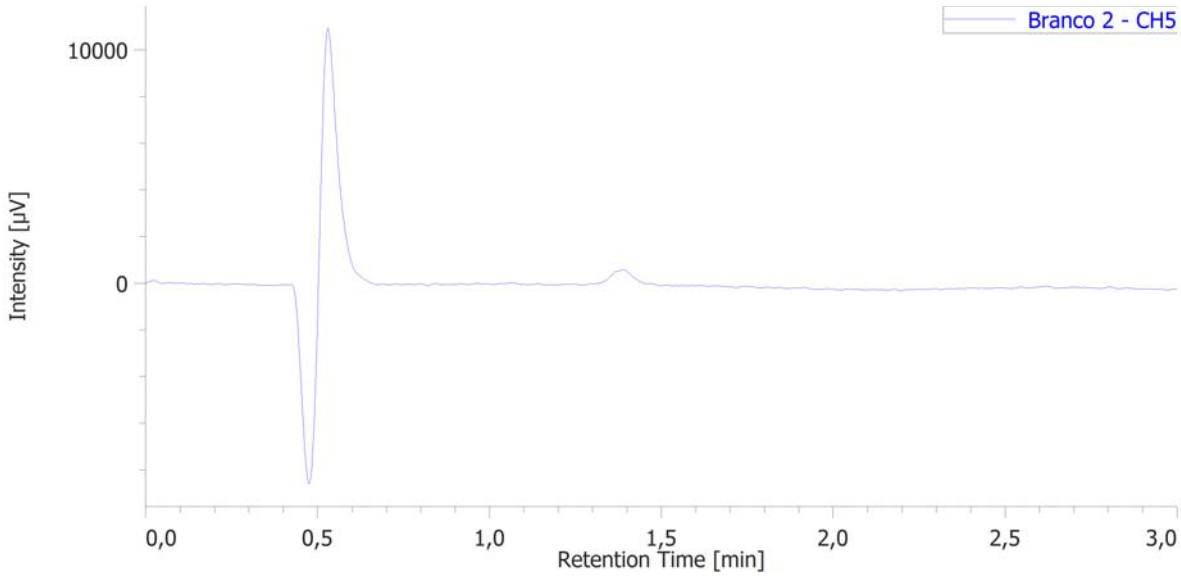


Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:06
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:42:07
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

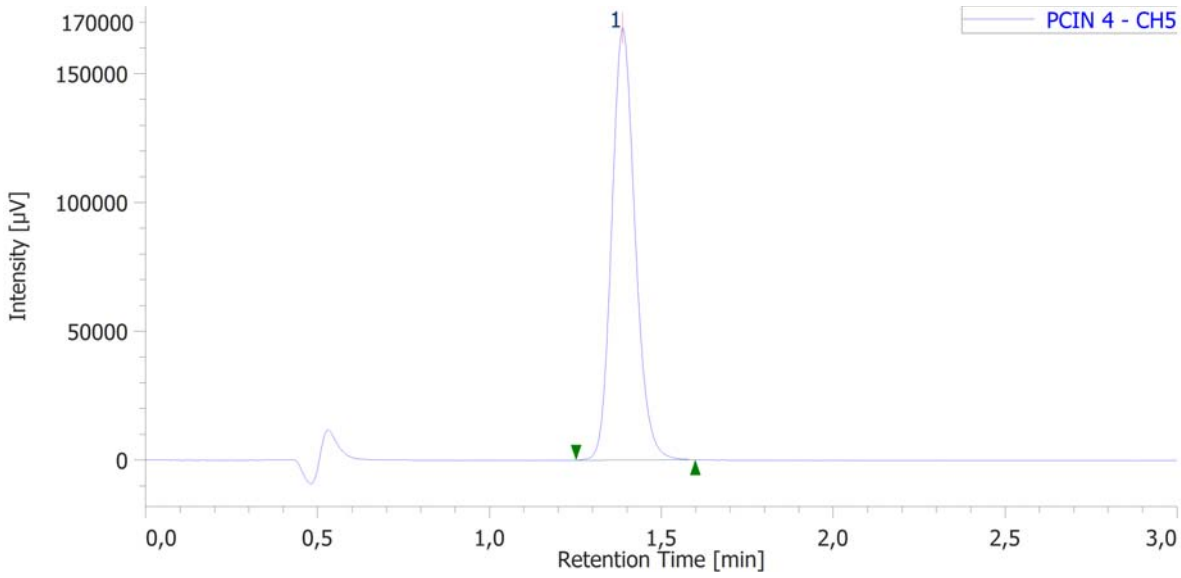

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:06
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:45:19
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,387	790549	167506	100,000	100,000	N/A	2059	N/A	1,167		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

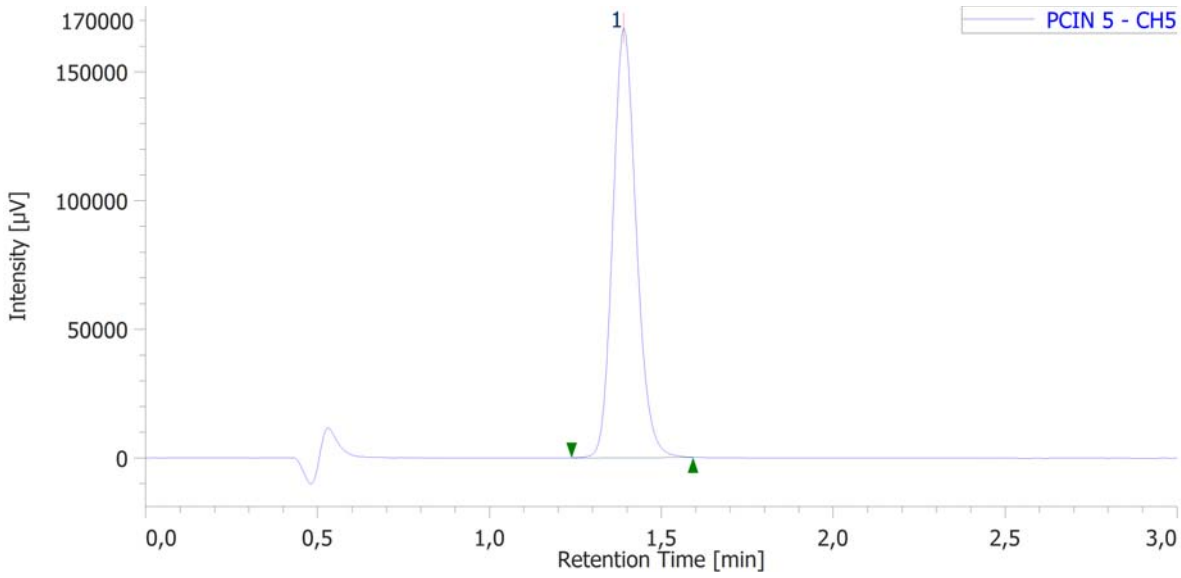

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:06
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:48:31
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,390	791607	166773	100,000	100,000	N/A	2044	N/A	1,166		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

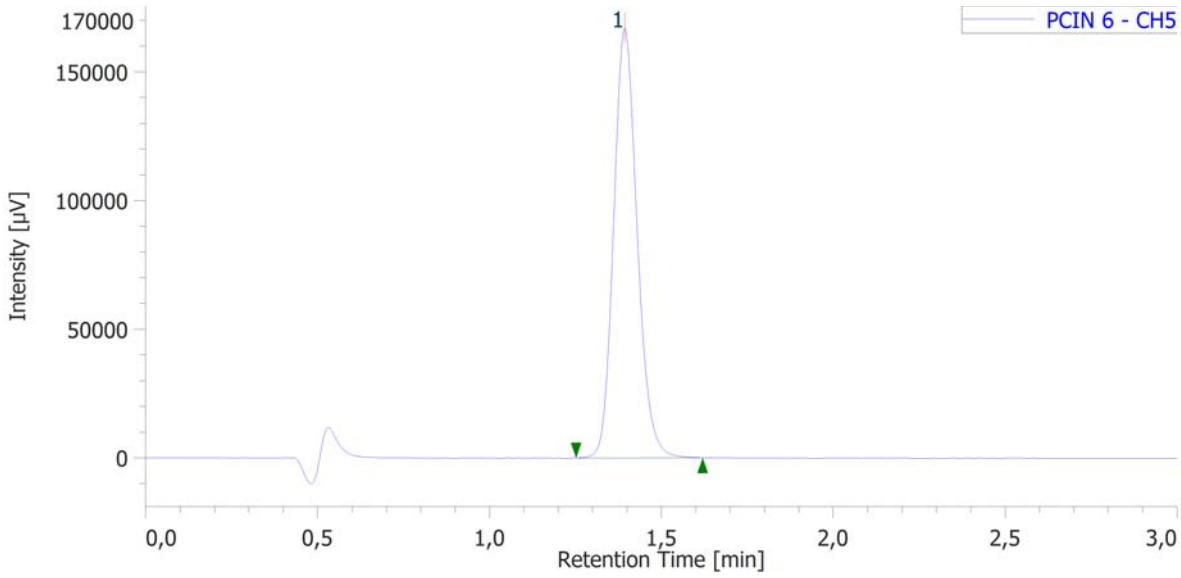

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:07
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:51:43
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,393	792771	166846	100,000	100,000	N/A	2052	N/A	1,154		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

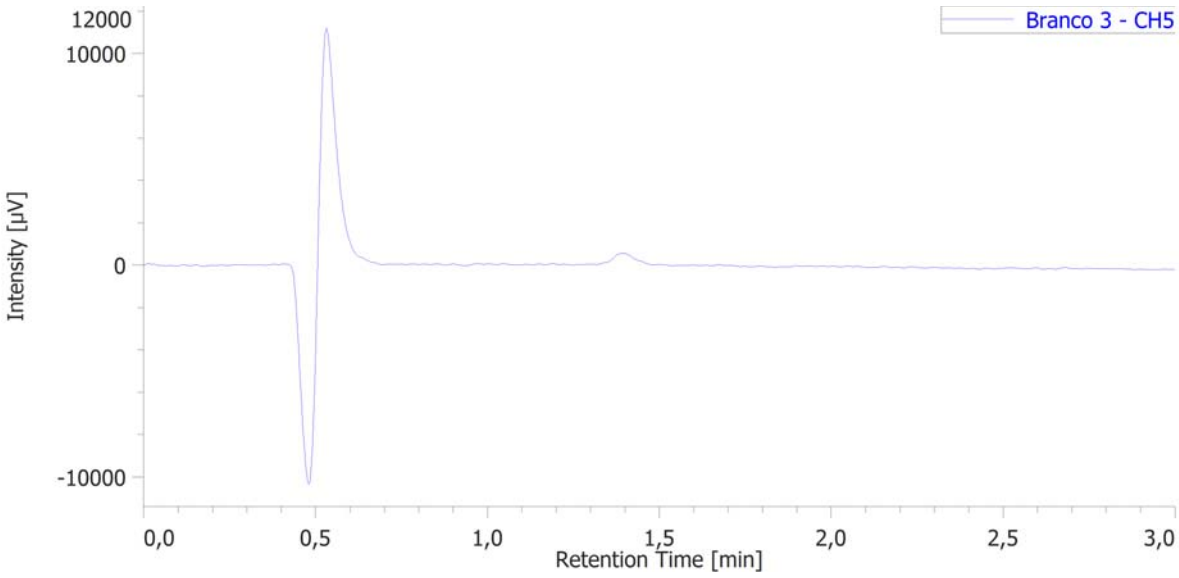


Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:02:07
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 10:54:55
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

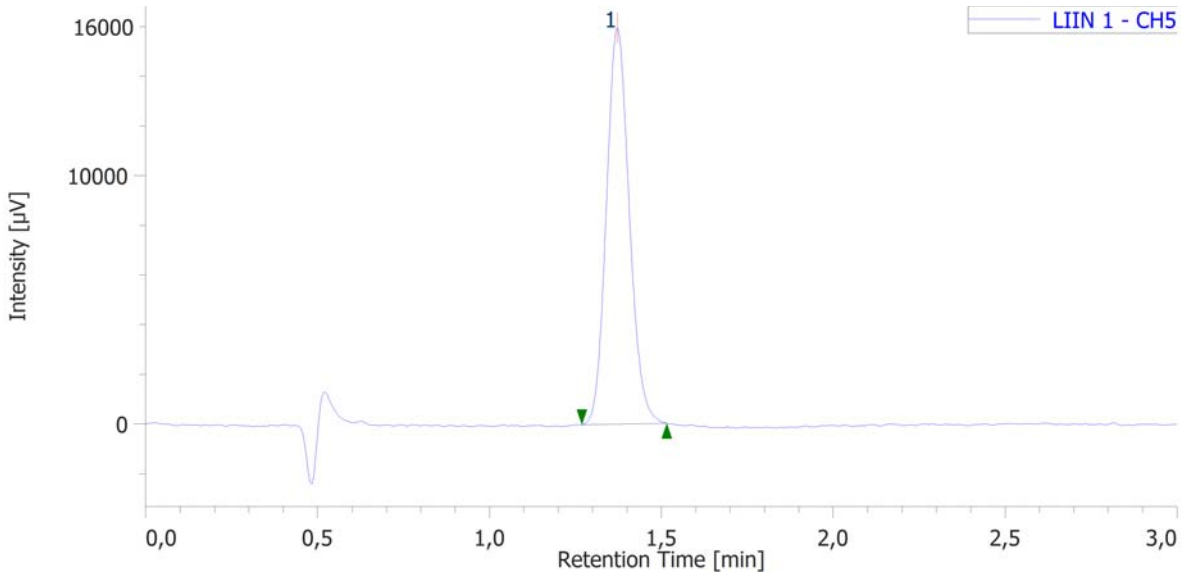

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:27:16
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 11:06:07
Volume	1,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,372	73812	15933	100,000	100,000	N/A	2050	N/A	1,127		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

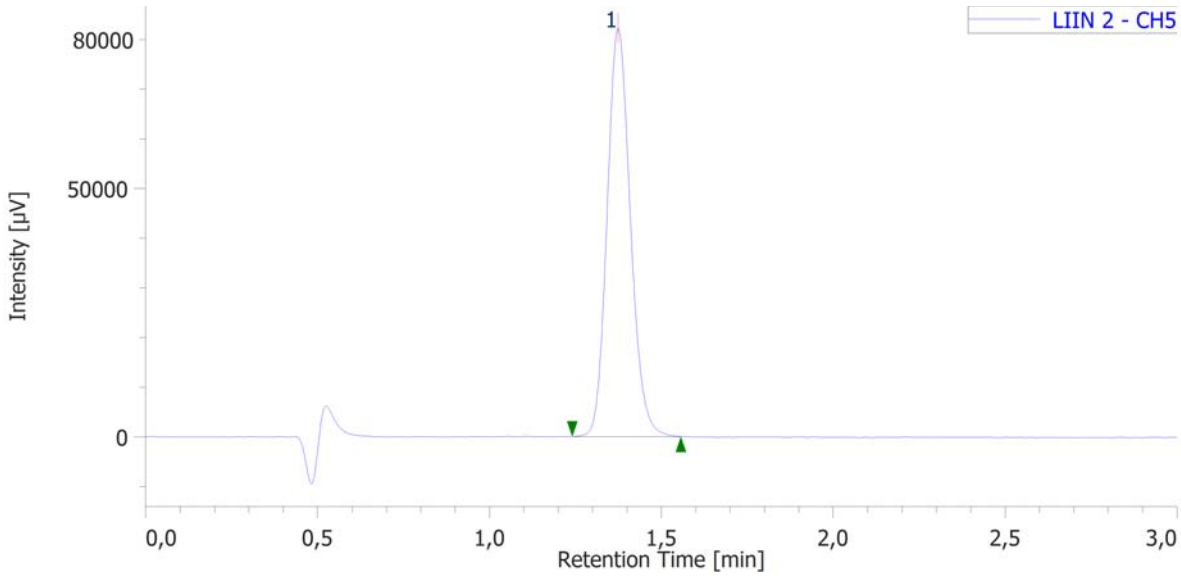

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:27:16
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 11:09:20
Volume	5,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,373	386596	82186	100,000	100,000	N/A	2015	N/A	1,155		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

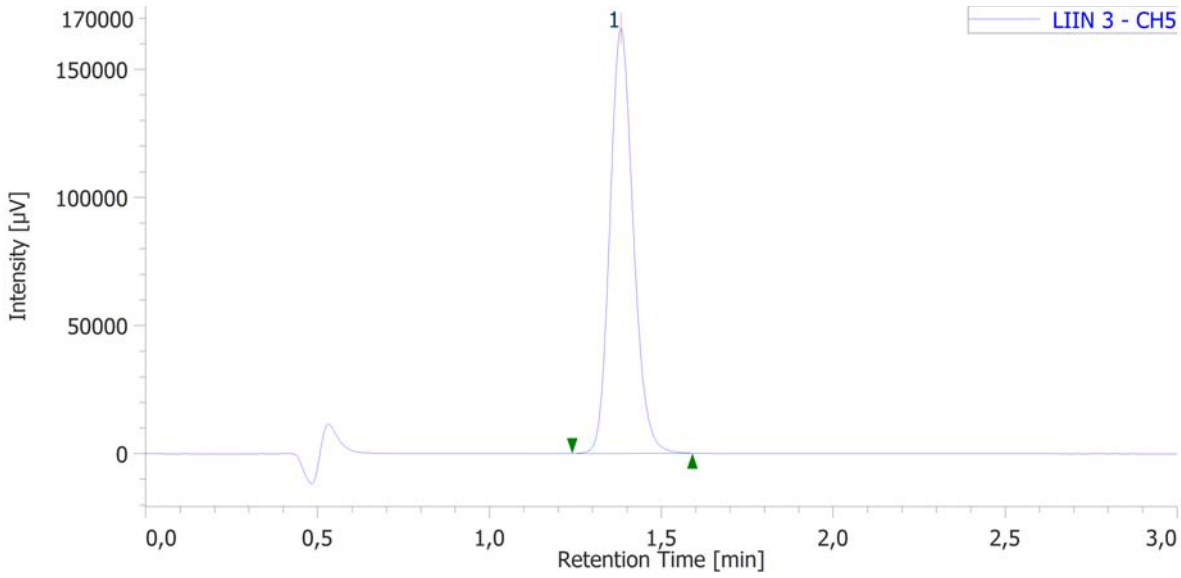

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:27:16
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 11:12:32
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,382	784285	165879	100,000	100,000	N/A	2030	N/A	1,163		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

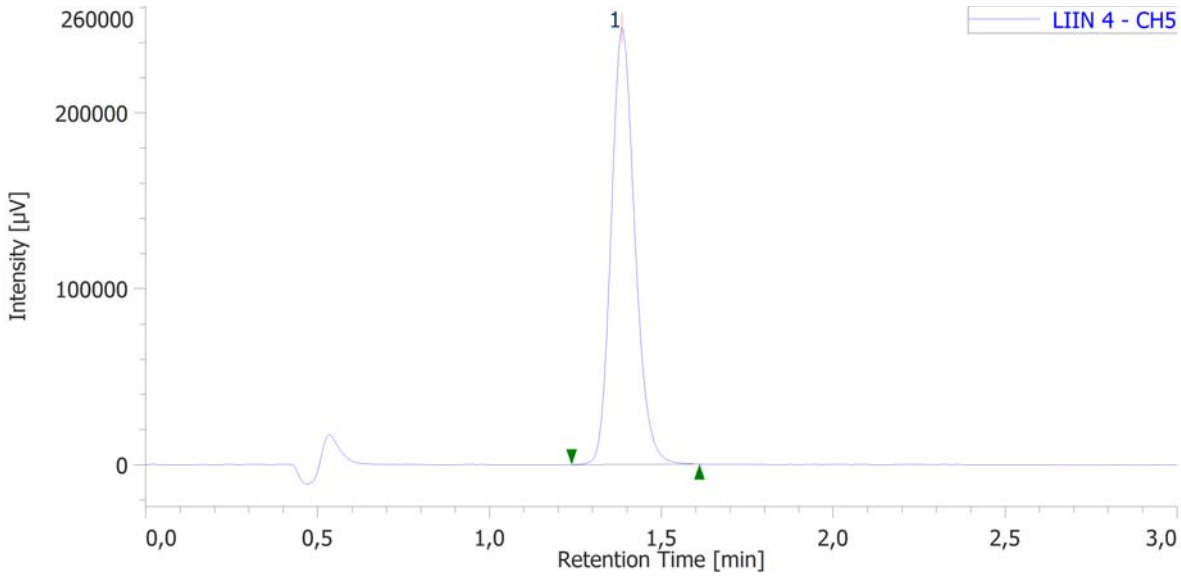

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:27:17
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 11:15:46
Volume	15,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,385	1190089	247819	100,000	100,000	N/A	1988	N/A	1,188		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

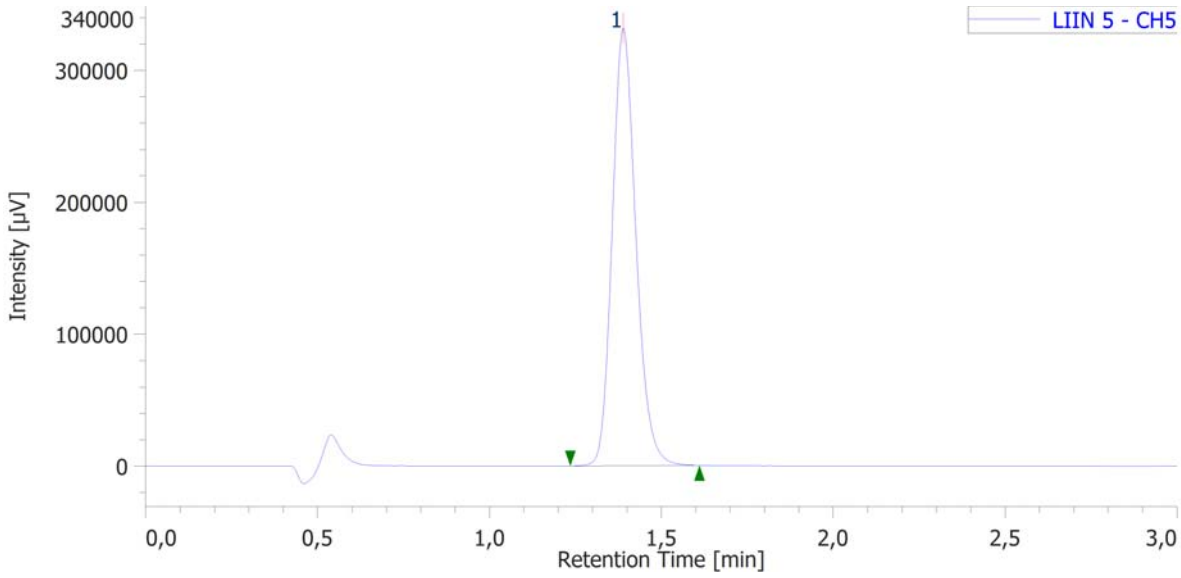

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 11:27:17
Description	
HPLC System Name	HP06
Injection Date	09/09/2026 11:19:08
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Cafeína	5	1,388	1586559	331600	100,000	100,000	N/A	2020	N/A	1,190		N/A

Creator QPackSA
Reviewer
Approver

Peak Find - EDFL.jws

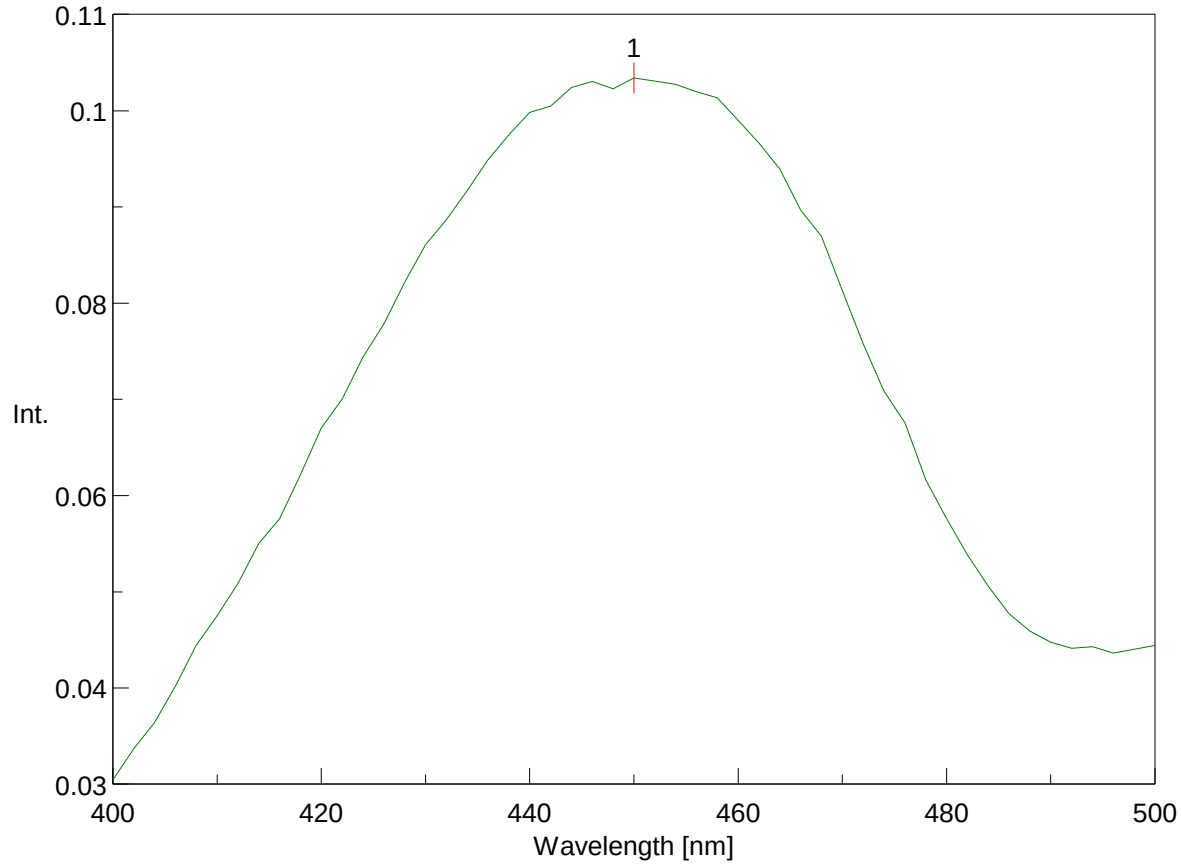

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	09/09/2026 12:19

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	0.103394			

Chromatogram

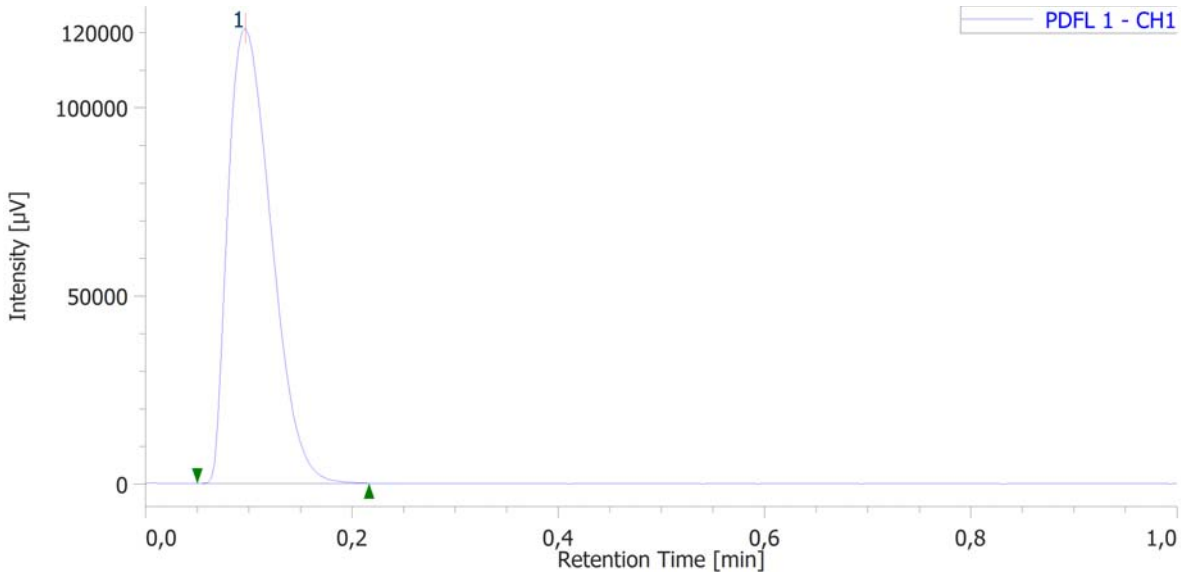

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:02
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:29:39
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,097	352801	120874	100,000	100,000	N/A	24	N/A	1,512		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

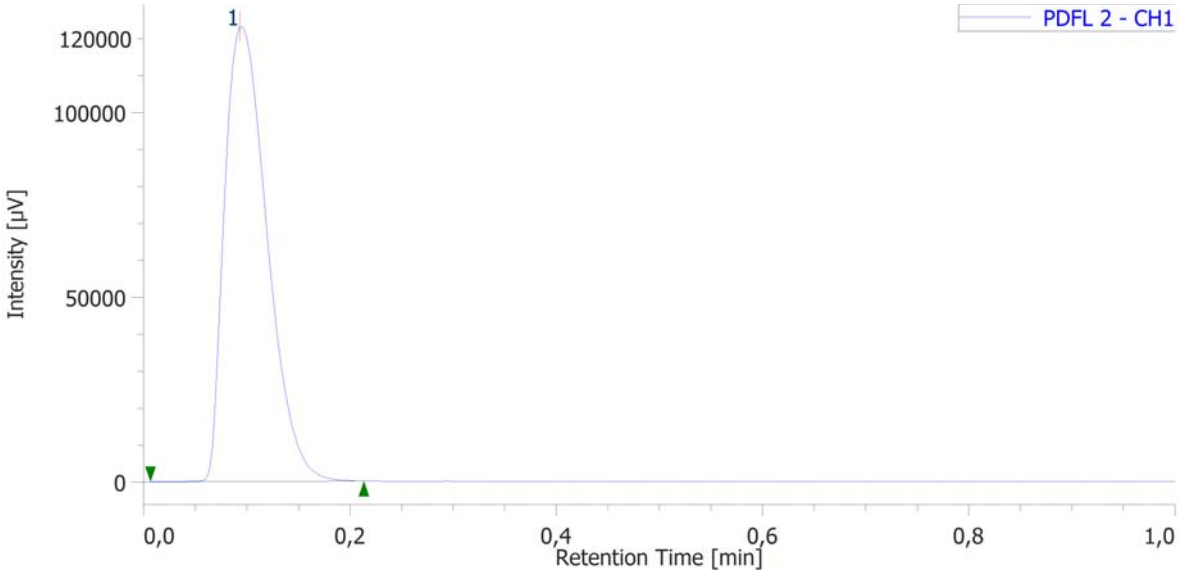

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:02
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:33:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,093	353665	123116	100,000	100,000	N/A	23	N/A	1,590		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

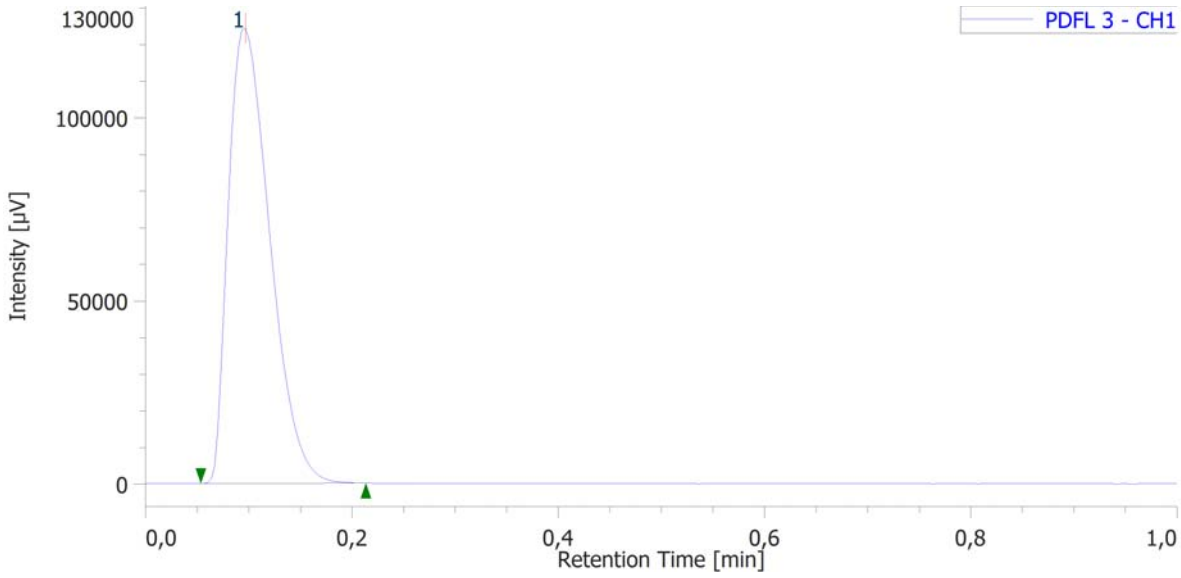

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:02
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:37:03
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,097	347643	124161	100,000	100,000	N/A	26	N/A	1,503		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

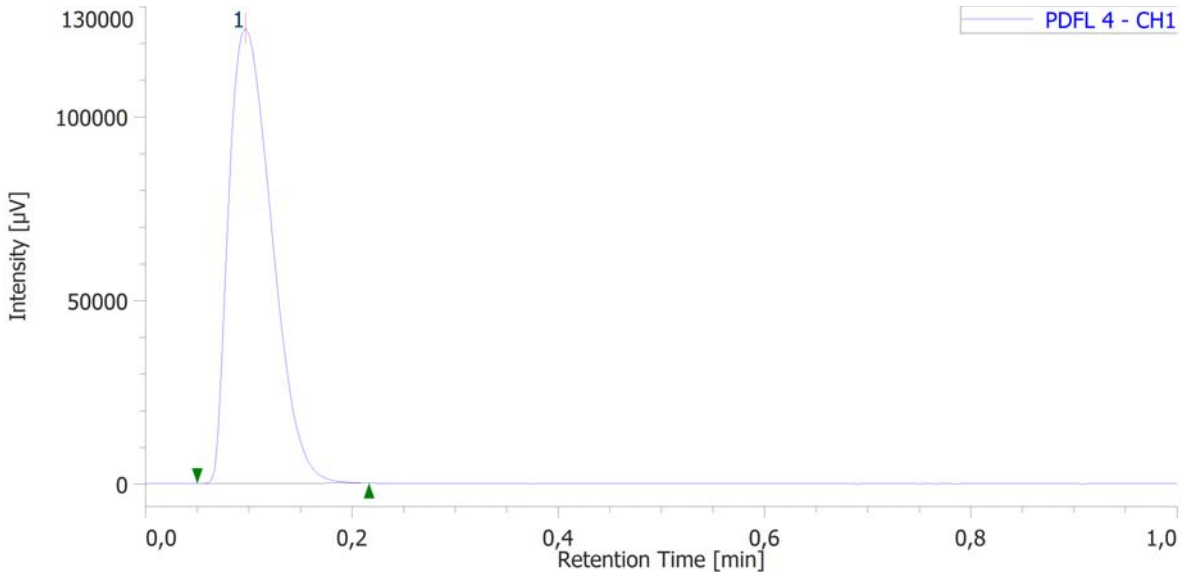

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:03
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:40:46
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,097	359468	123845	100,000	100,000	N/A	24	N/A	1,534		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

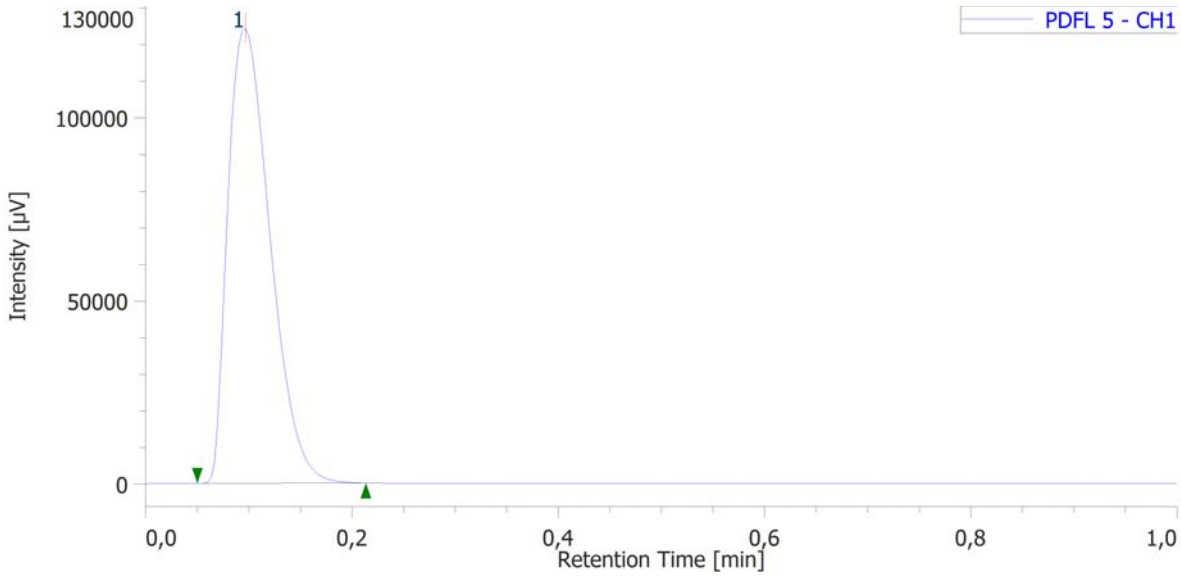

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:03
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:44:29
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,097	353433	124226	100,000	100,000	N/A	25	N/A	1,491		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

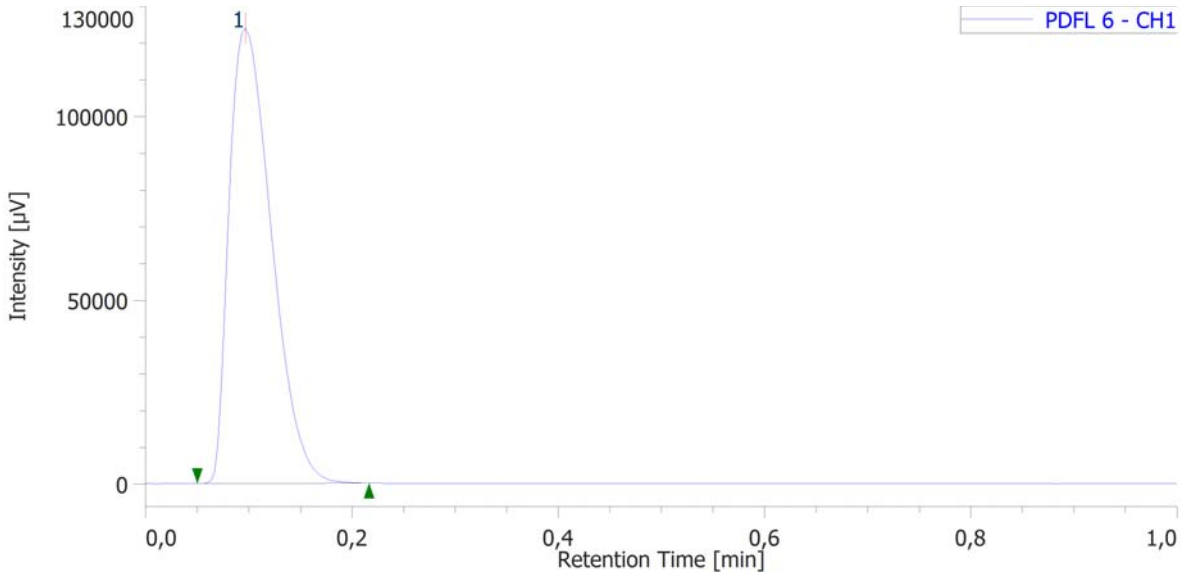

Chromatogram Information	
User Name	QPackSA
Date Modified	09/09/2026 12:51:03
Description	
HPLC System Name	HP06 – Det FL
Injection Date	09/09/2026 12:48:11
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL
Peak ID Table	PDFL
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PDFL 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	PDFL

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	PDFL	1	0,097	353923	123773	100,000	100,000	N/A	25	N/A	1,565		N/A

Creator QPackSA
Reviewer
Approver