URL chrom://desktop-pos9hfk/ChromeleonLocal/Qualificação/2022/Qualificação.seq/609.smp/3DFIELD.field
Channel UV_VIS_1

Injection Information:
Data Vault ChromeleonLocal
Sequence Qualificação
Name EDUV
Number 1
Position RA2
Comment
Processing Method Qualificação
Instrument Method Qualificação
Type Unknown
Status Finished
Inject Time 10/11/2022 09:51:30 -03:00
Volume (µl) 10,000
Dilution Factor 1,0000
Weight 1,0000

Raw Data Information:
Data Points 201
Wavelength Min. (nm) 200,000000
Wavelength Max. (nm) 300,000000
Retention Time (min) 1,786667

Raw Data:
Wavelength (nm) Value (mAU)
200,0 81,091886
200,5 82,055895
201,0 82,959359
201,5 83,748655
202,0 84,397857
202,5 84,887084
203,0 85,192924
203,5 85,290987
204,0 85,156505
204,5 84,771905
205,0 84,148770
205,5 83,303510
206,0 82,242673
206,5 80,971870
207,0 79,502826
207,5 77,851879
208,0 76,047723
208,5 74,122472
209,0 72,109584
209,5 70,037395
210,0 67,912404
210,5 65,742042
211,0 63,559298
211,5 61,393792
212,0 59,236113
212,5 57,075810


213,0 54,937306
213,5 52,844371
214,0 50,783280
214,5 48,737849
215,0 46,719554
215,5 44,743019
216,0 42,807820
216,5 40,913785
217,0 39,076807
217,5 37,310604
218,0 35,604121
218,5 33,947130
219,0 32,357456
219,5 30,857301
220,0 29,458286
220,5 28,167552
221,0 26,984872
221,5 25,907244
222,0 24,927916
222,5 24,041390
223,0 23,250939
223,5 22,559163
224,0 21,957220
224,5 21,430915
225,0 20,956100
225,5 20,513115
226,0 20,110191
226,5 19,757485
227,0 19,444944
227,5 19,157763
228,0 18,882335
228,5 18,608367
229,0 18,337608
229,5 18,072380
230,0 17,805220
230,5 17,527597
231,0 17,236472
231,5 16,931846
232,0 16,620399
232,5 16,308522
233,0 15,994788
233,5 15,675407
234,0 15,344978
234,5 14,999872
235,0 14,645160
235,5 14,288442
236,0 13,938726
236,5 13,601596
237,0 13,267518
237,5 12,927668
238,0 12,591184
238,5 12,269141
239,0 11,962415
239,5 11,670518

240,0 11,397720
240,5 11,147757
241,0 10,917485
241,5 10,702899
242,0 10,503412
242,5 10,321810
243,0 10,170937
243,5 10,061786
244,0 9,987891
244,5 9,941149
245,0 9,924353
245,5 9,942037
246,0 9,994805
246,5 10,083018
247,0 10,209978
247,5 10,377161
248,0 10,575772
248,5 10,798044
249,0 11,050583
249,5 11,340535
250,0 11,662842
250,5 12,010115
251,0 12,377859
251,5 12,763658
252,0 13,170541
252,5 13,601804
253,0 14,056385
253,5 14,532300
254,0 15,028239
254,5 15,543239
255,0 16,077043
255,5 16,628842
256,0 17,194928
256,5 17,772019
257,0 18,361450
257,5 18,964277
258,0 19,575835
258,5 20,190962
259,0 20,808221
259,5 21,427486
260,0 22,050144
260,5 22,676601
261,0 23,301841
261,5 23,920327
262,0 24,529876
262,5 25,130424
263,0 25,727035
263,5 26,322063
264,0 26,901902
264,5 27,453794
265,0 27,984323
265,5 28,502124
266,0 29,004695
266,5 29,487300

267,0	29,947402
267,5	30,382213
268,0	30,785741
268,5	31,152983
269,0	31,486096
269,5	31,787587
270,0	32,054188
270,5	32,282422
271,0	32,473745
271,5	32,628080
272,0	32,734277
272,5	32,782677
273,0	32,780649
273,5	32,736855
274,0	32,648088
274,5	32,508567
275,0	32,314064
275,5	32,064403
276,0	31,774046
276,5	31,454780
277,0	31,093063
277,5	30,674032
278,0	30,202867
278,5	29,688670
279,0	29,136183
279,5	28,548236
280,0	27,924361
280,5	27,263248
281,0	26,563527
281,5	25,825561
282,0	25,056721
282,5	24,262768
283,0	23,436011
283,5	22,567834
284,0	21,659376
284,5	20,717298
285,0	19,760610
285,5	18,805272
286,0	17,842711
286,5	16,864038
287,0	15,883626
287,5	14,916512
288,0	13,957144
288,5	13,001104
289,0	12,069107
289,5	11,180228
290,0	10,321856
290,5	9,481450
291,0	8,678437
291,5	7,933274
292,0	7,238567
292,5	6,583816
293,0	5,973935
293,5	5,413816

294,0	4,892826
294,5	4,402521
295,0	3,958702
295,5	3,575383
296,0	3,235161
296,5	2,918219
297,0	2,626479
297,5	2,366740
298,0	2,143562
298,5	1,957631
299,0	1,796365
299,5	1,645787
300,0	1,499593

Contour Spectral View

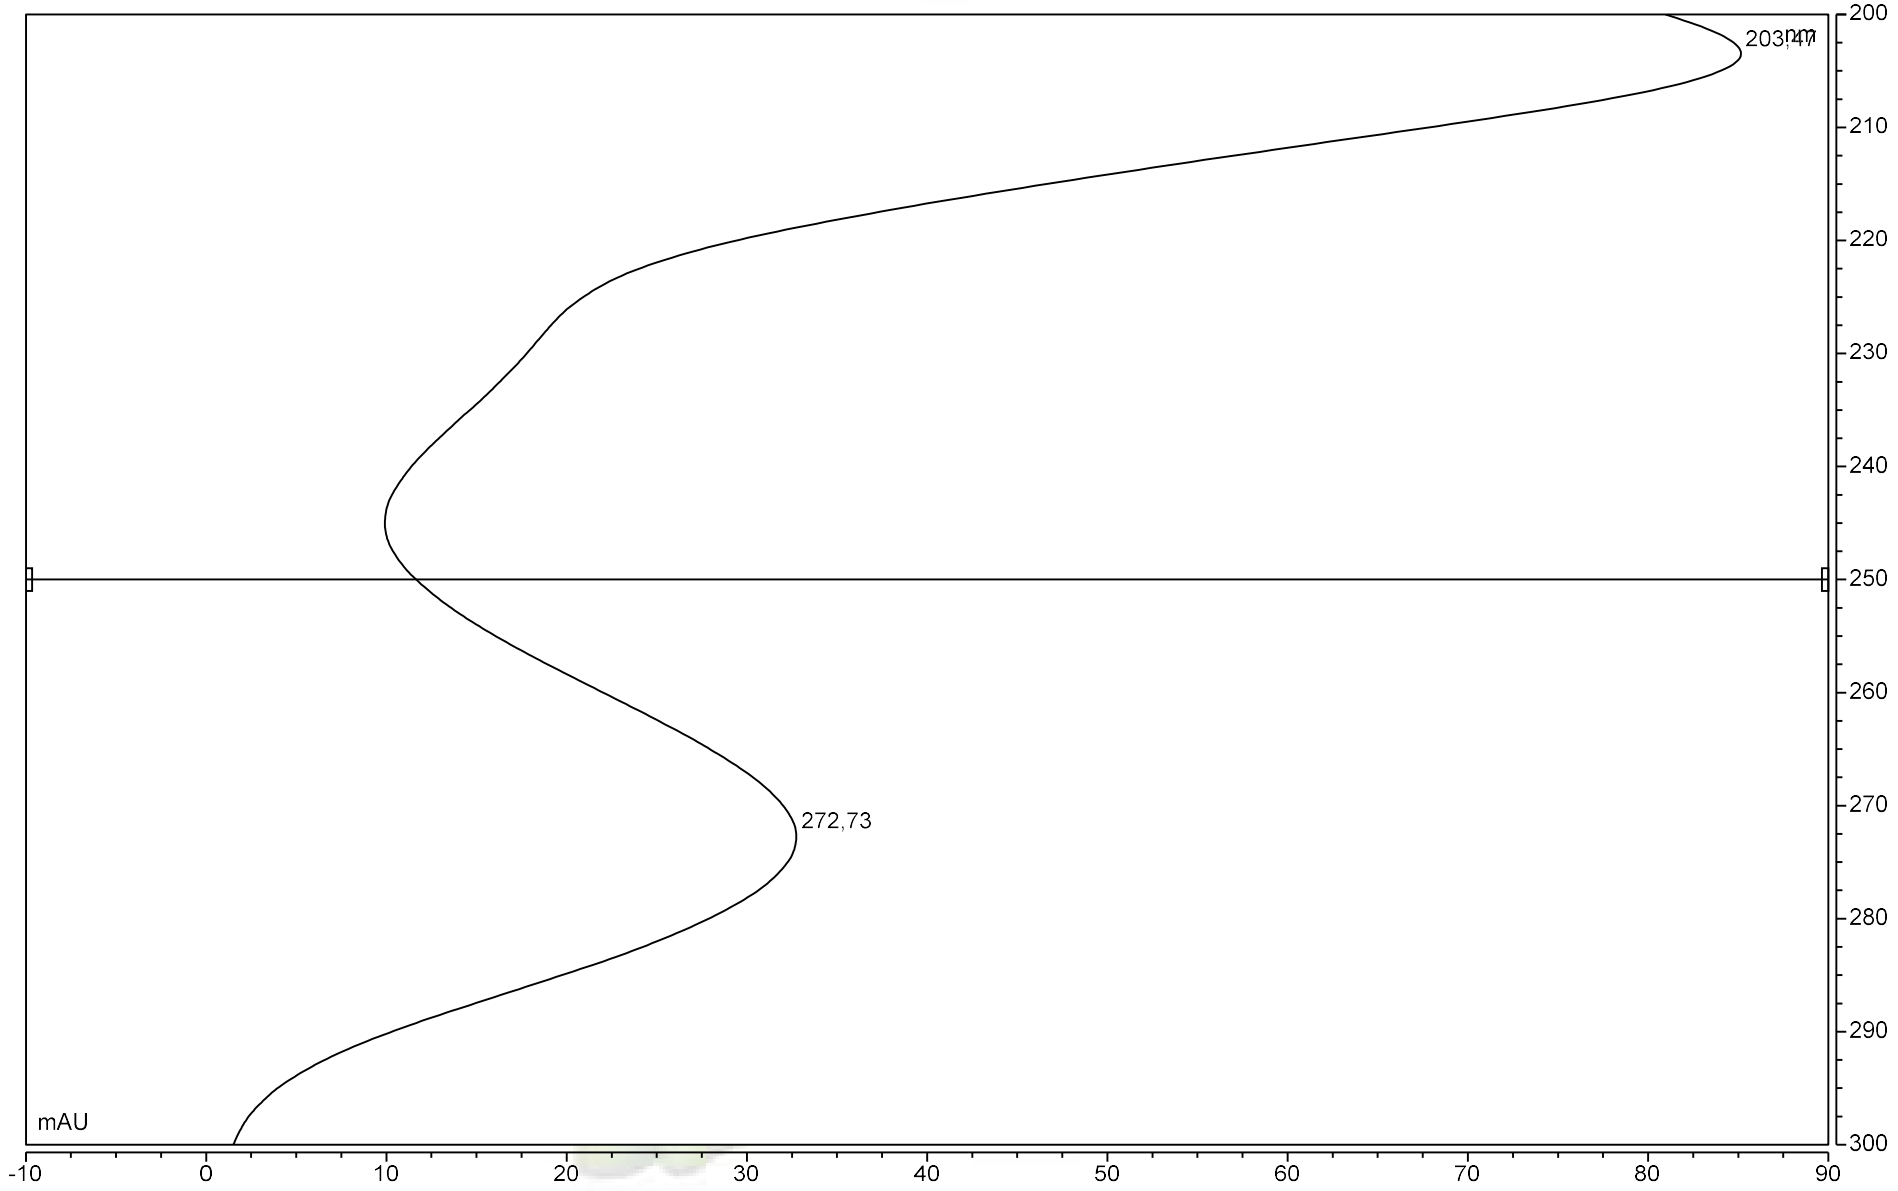


Chromatogram and Results

Injection Details

Injection Name:	**Branco 01**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 09:55**	*Sample Weight:*	**1,0000**

Chromatogram

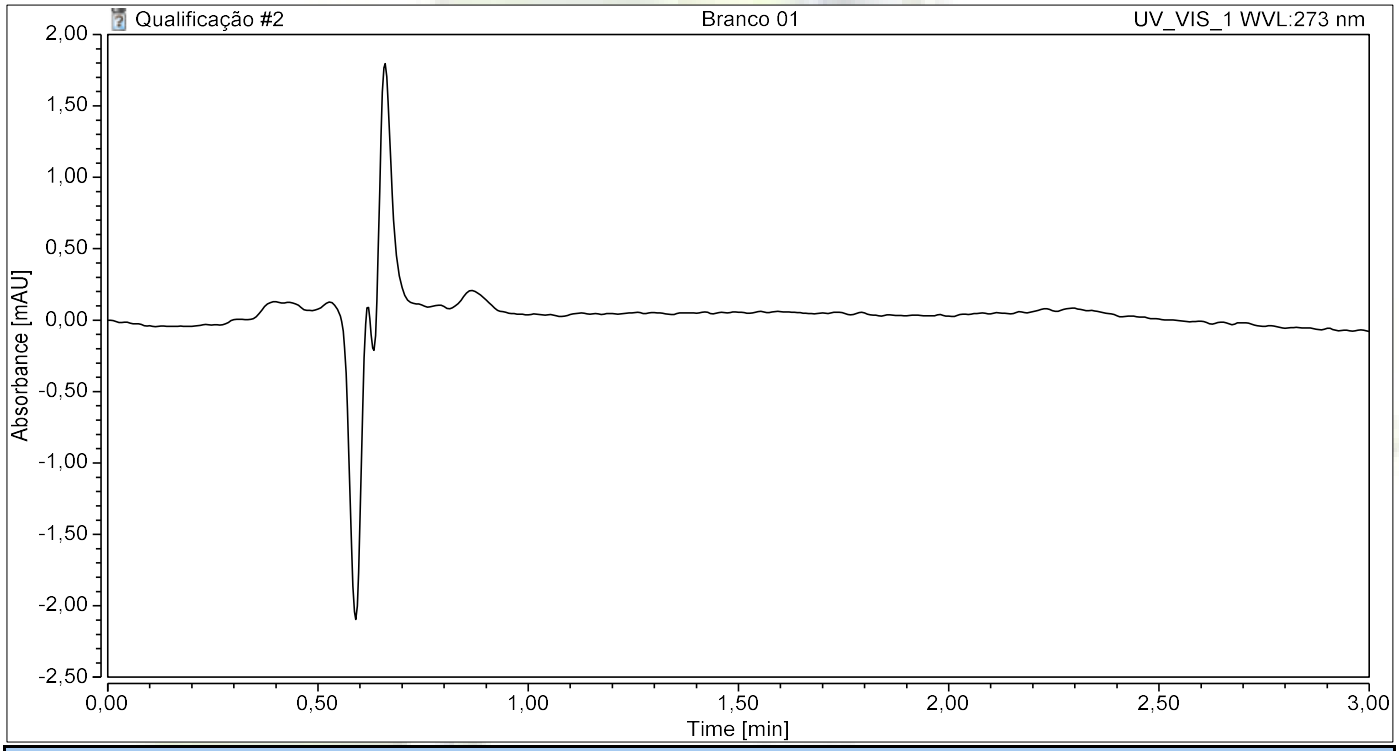

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.24543

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 09:59**	*Sample Weight:*	**1,0000**

Chromatogram

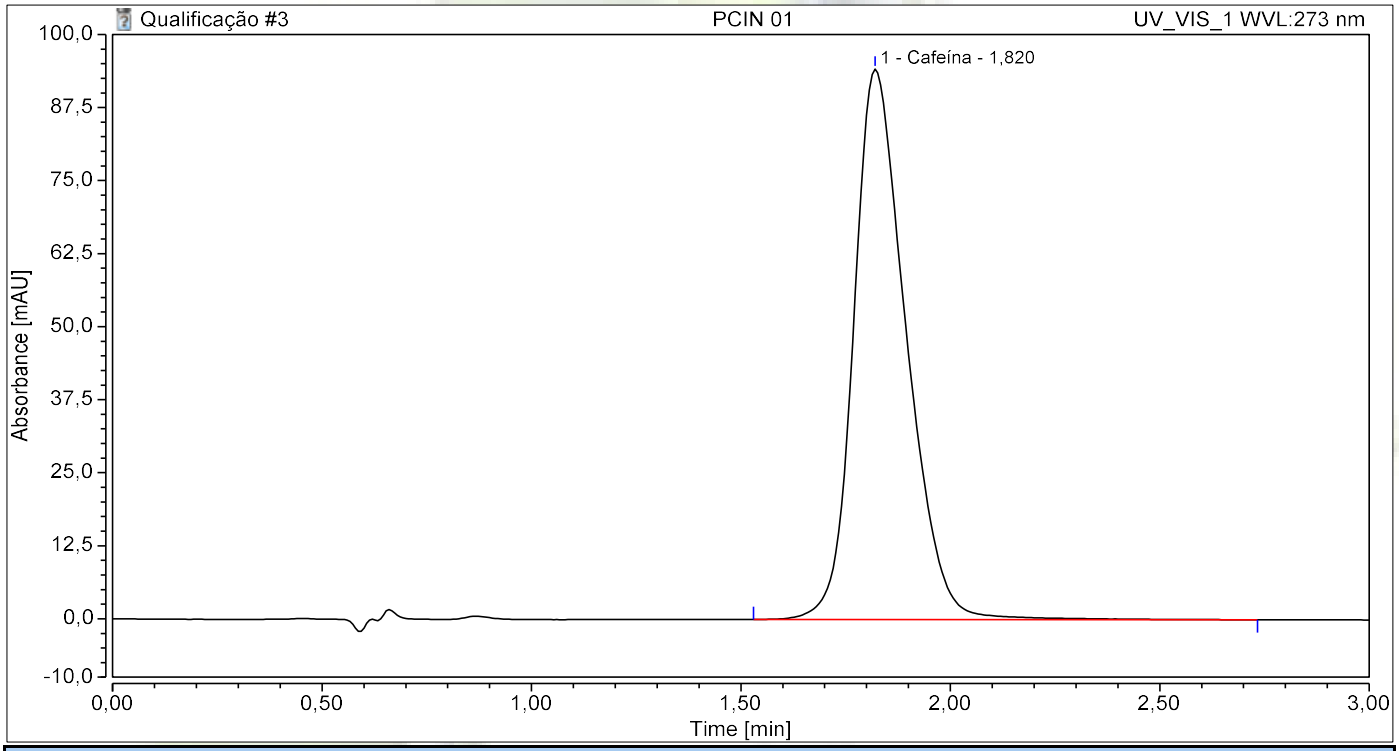

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,820	13,676	94,183	100,00	100,00	n.a.
Total:			**13,676**	**94,183**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:03**	*Sample Weight:*	**1,0000**

Chromatogram

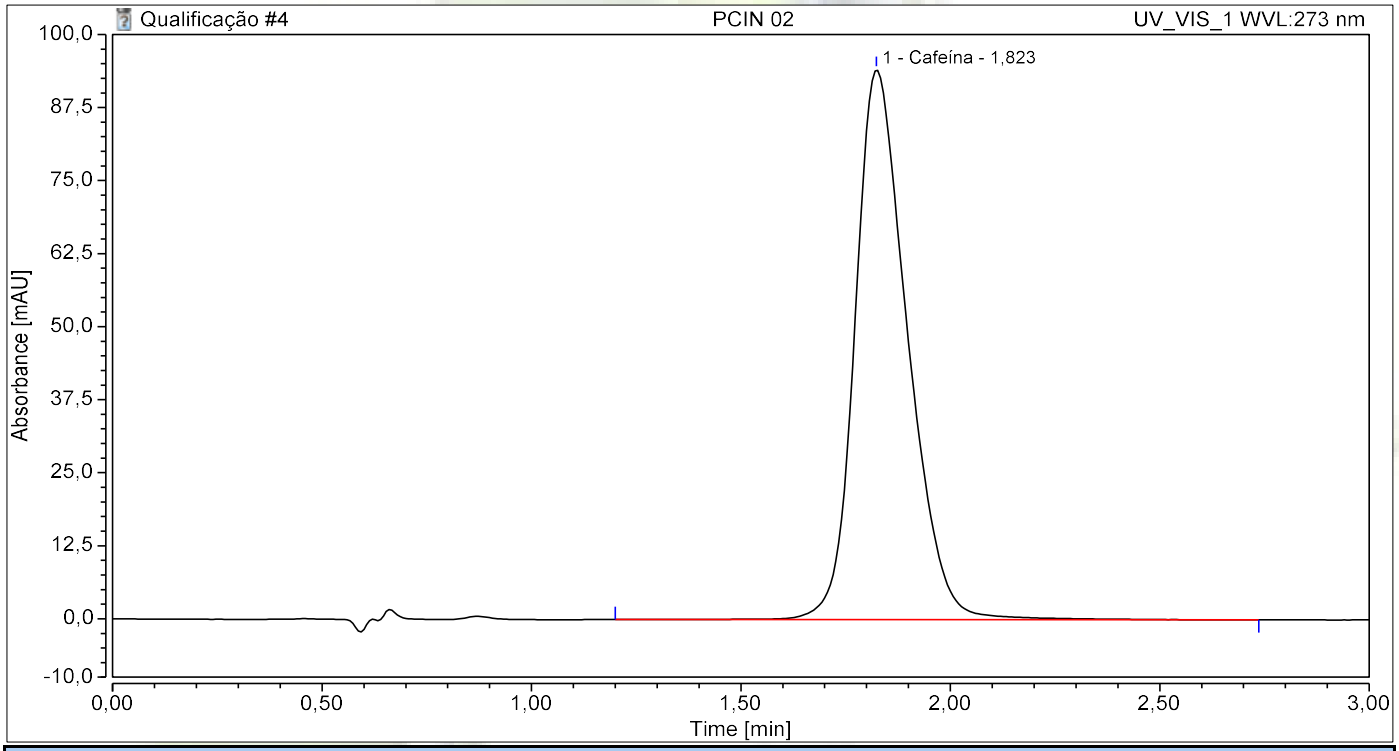

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,823	13,667	94,166	100,00	100,00	n.a.
Total:			**13,667**	**94,166**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:06**	*Sample Weight:*	**1,0000**

Chromatogram

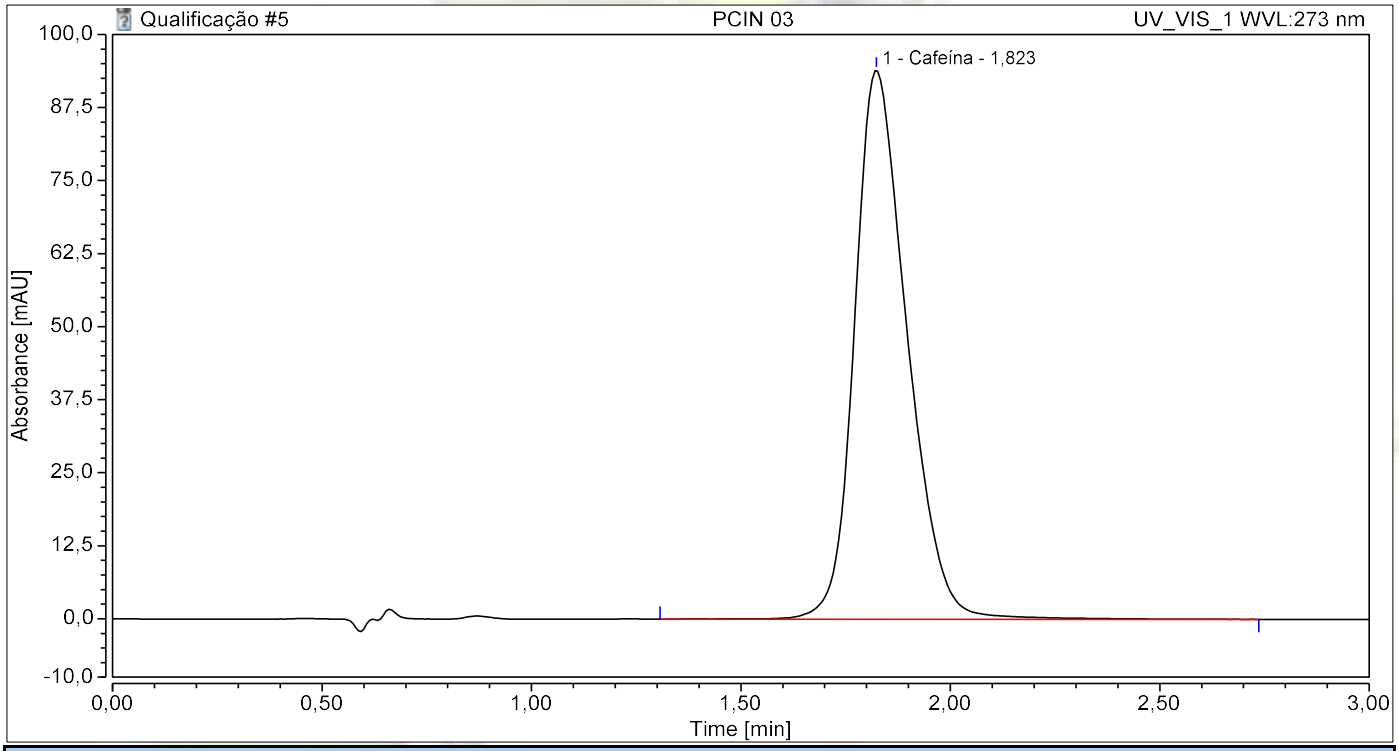

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,823	13,637	93,995	100,00	100,00	n.a.
Total:			**13,637**	**93,995**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**Branco 02**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:10**	*Sample Weight:*	**1,0000**

Chromatogram

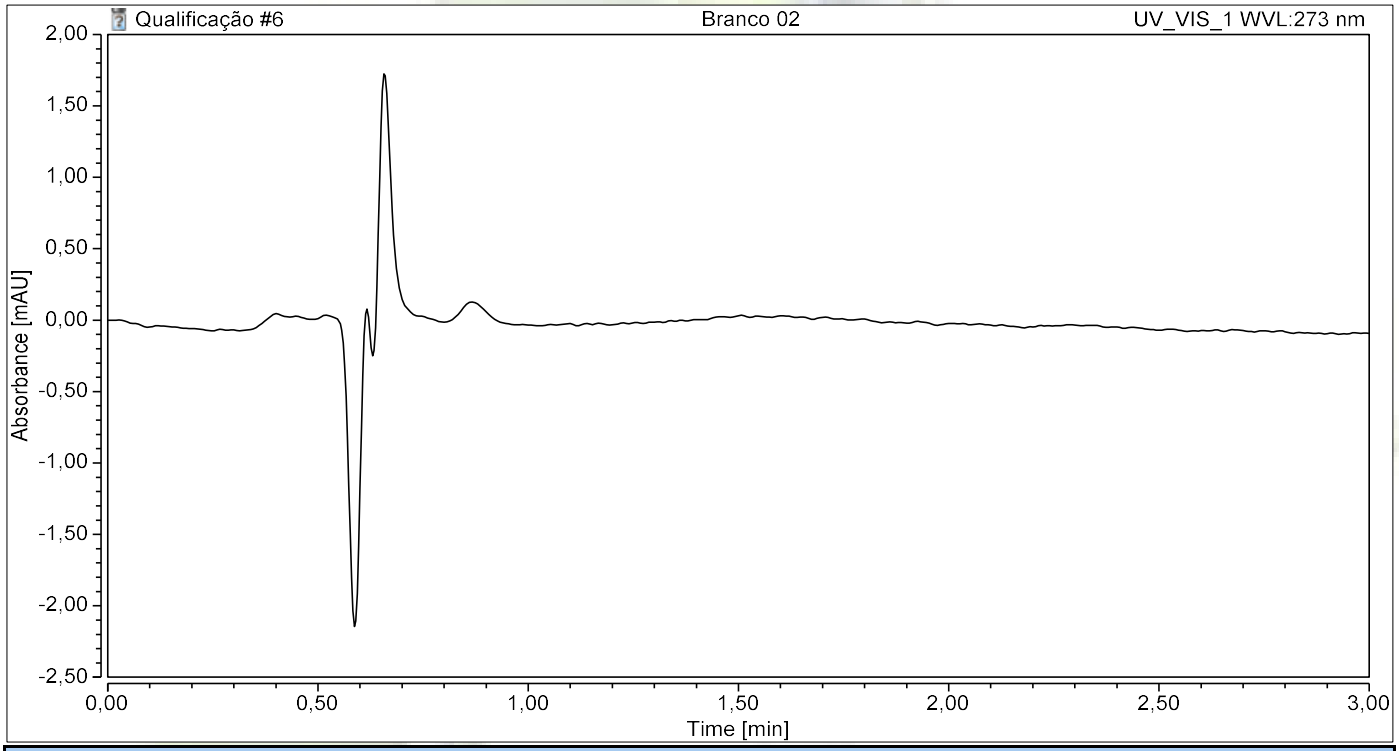

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.24543

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:14**	*Sample Weight:*	**1,0000**

Chromatogram

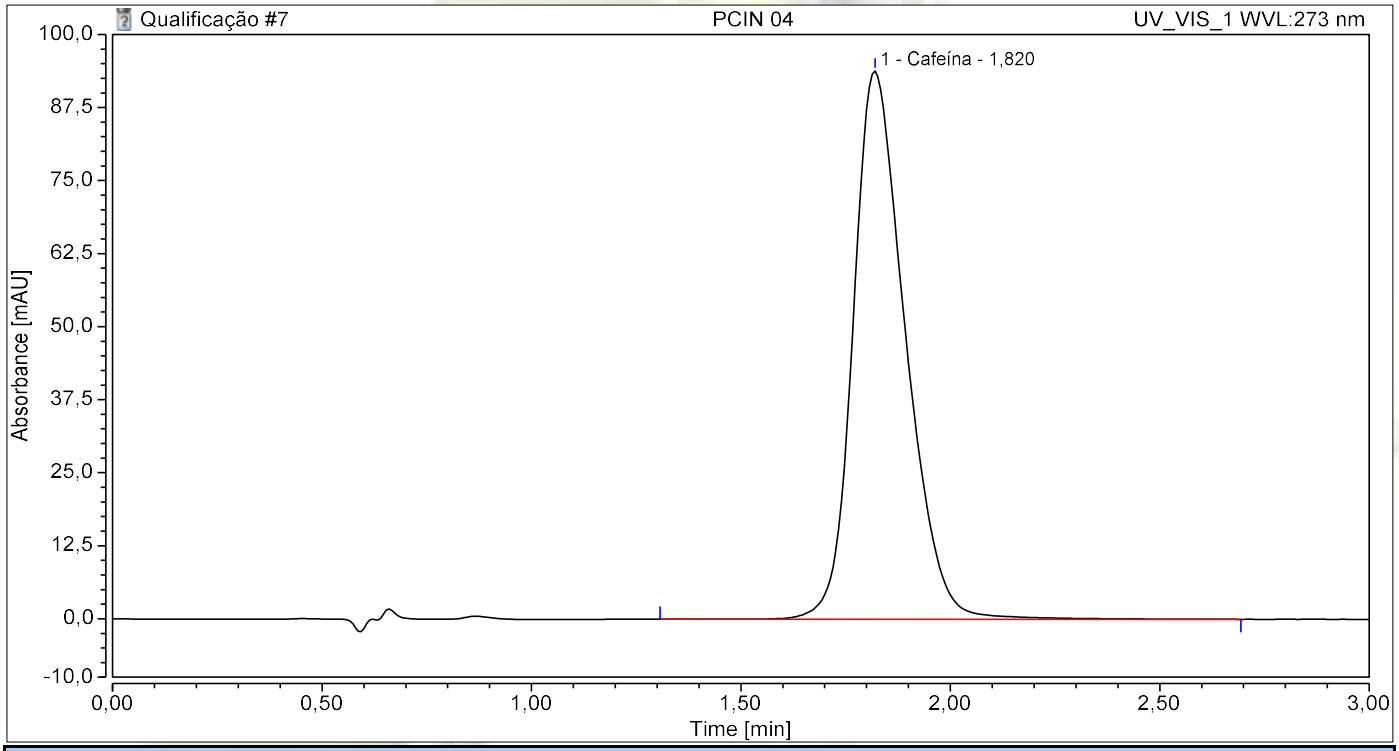

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,820	13,562	93,850	100,00	100,00	n.a.
Total:			**13,562**	**93,850**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:18**	*Sample Weight:*	**1,0000**

Chromatogram

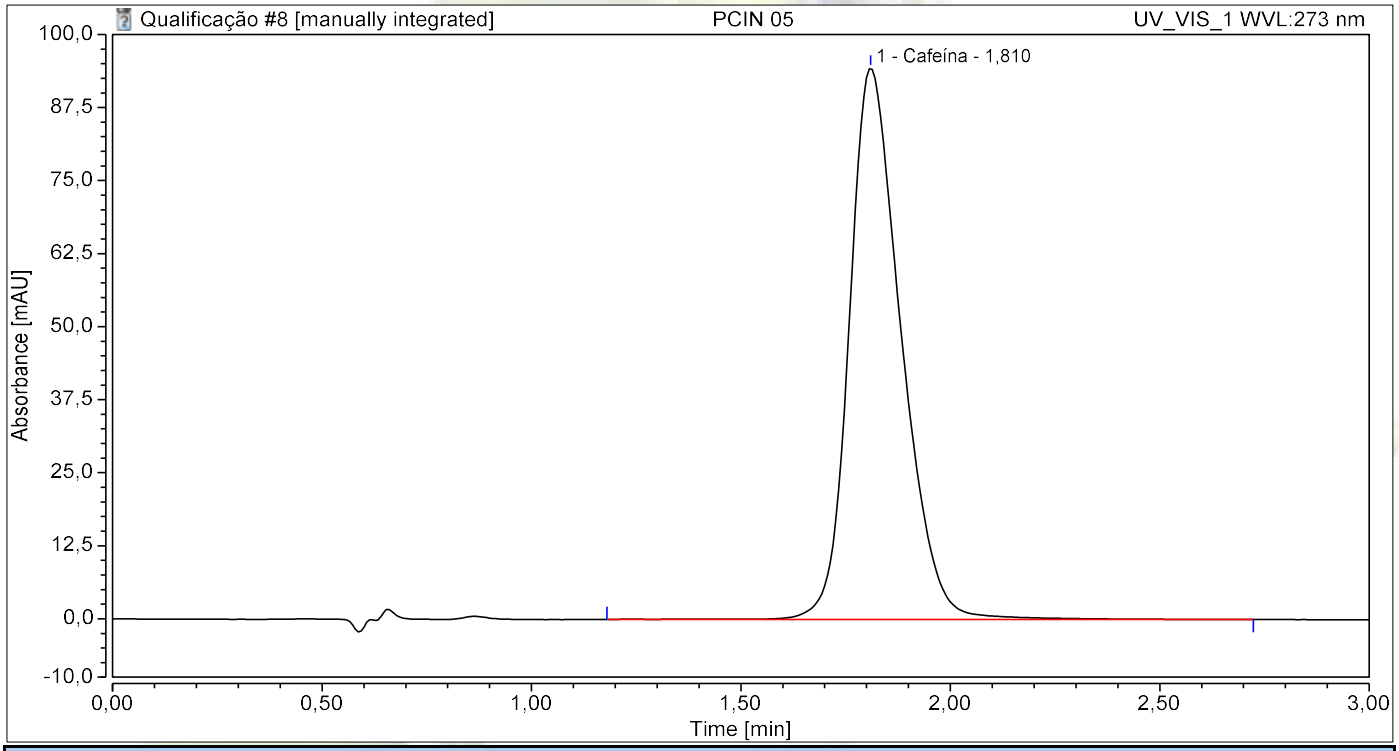

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,810	13,520	94,373	100,00	100,00	n.a.
Total:			**13,520**	**94,373**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:22**	*Sample Weight:*	**1,0000**

Chromatogram

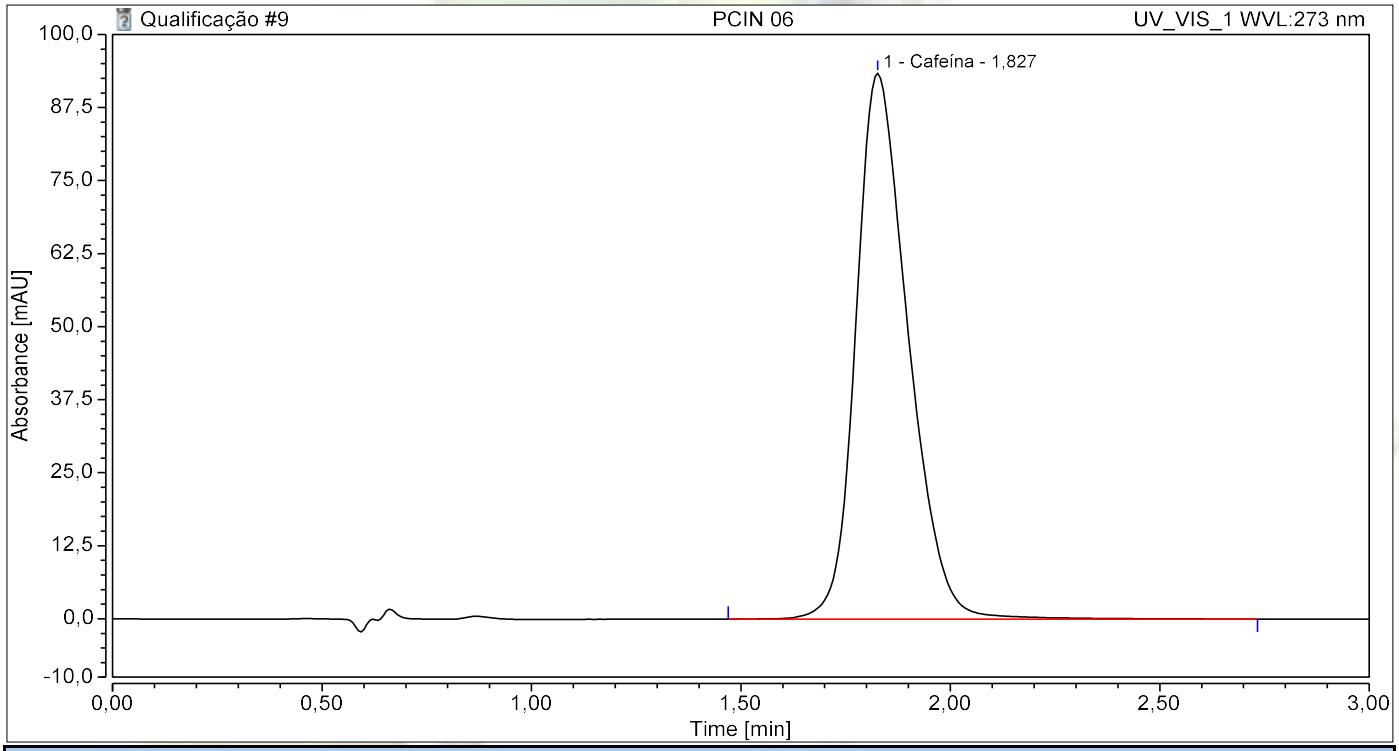

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,827	13,516	93,420	100,00	100,00	n.a.
Total:			**13,516**	**93,420**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**Branco 03**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:26**	*Sample Weight:*	**1,0000**

Chromatogram

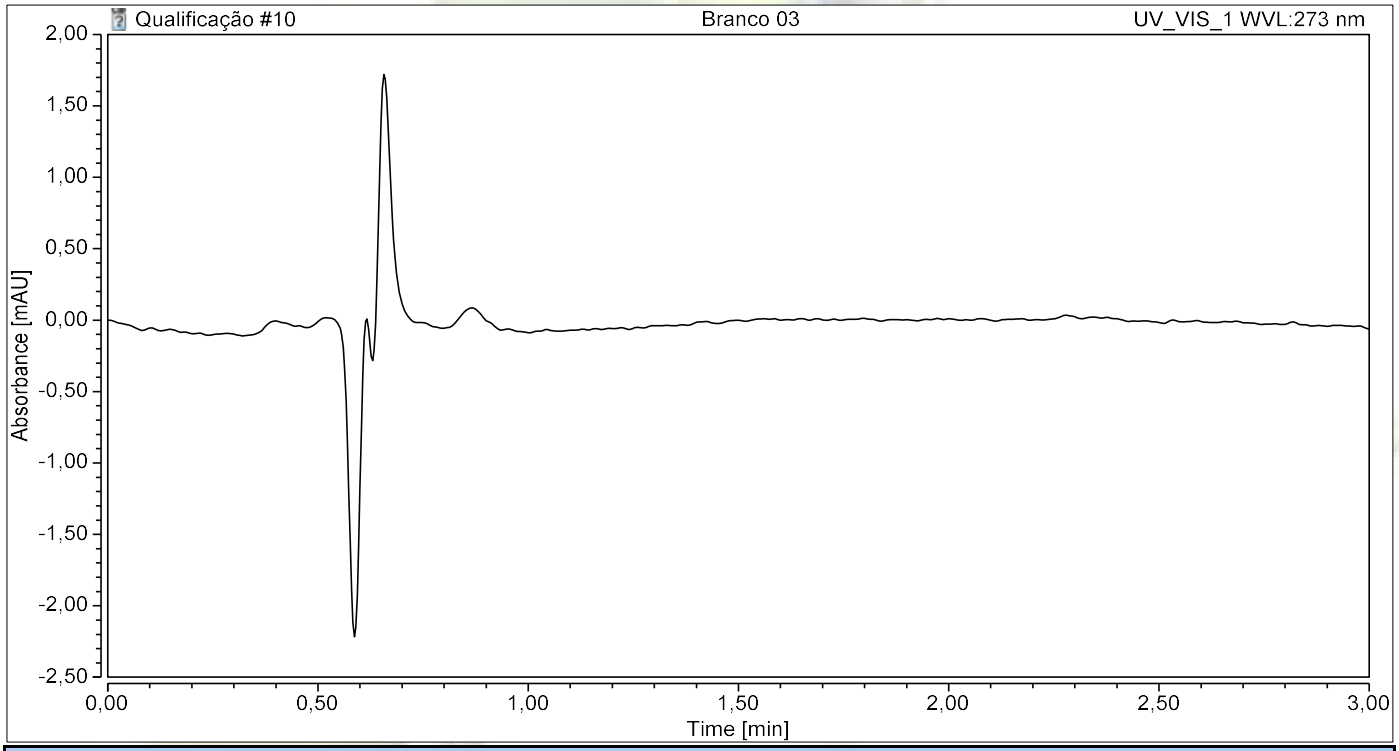

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**3,00**
Vial Number:	**RA1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:30**	*Sample Weight:*	**1,0000**

Chromatogram

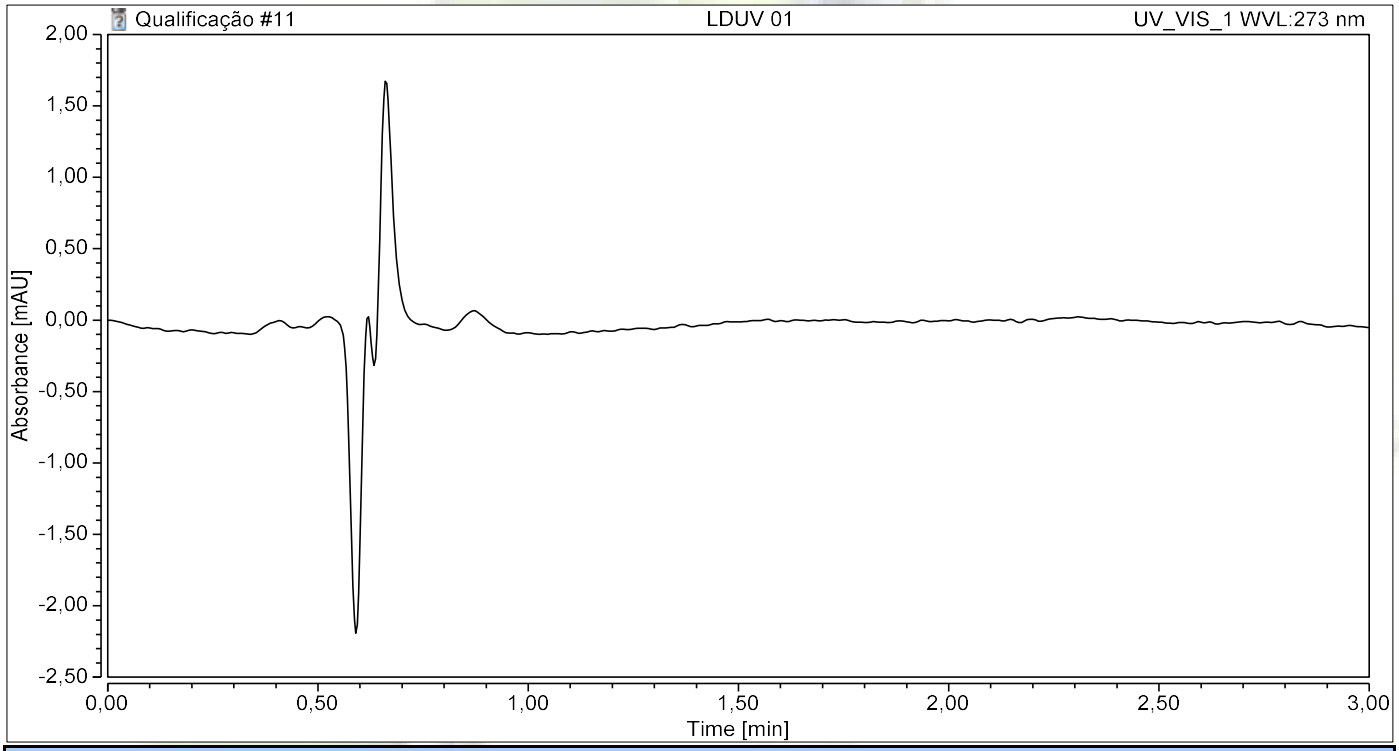

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**3,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:33**	*Sample Weight:*	**1,0000**

Chromatogram

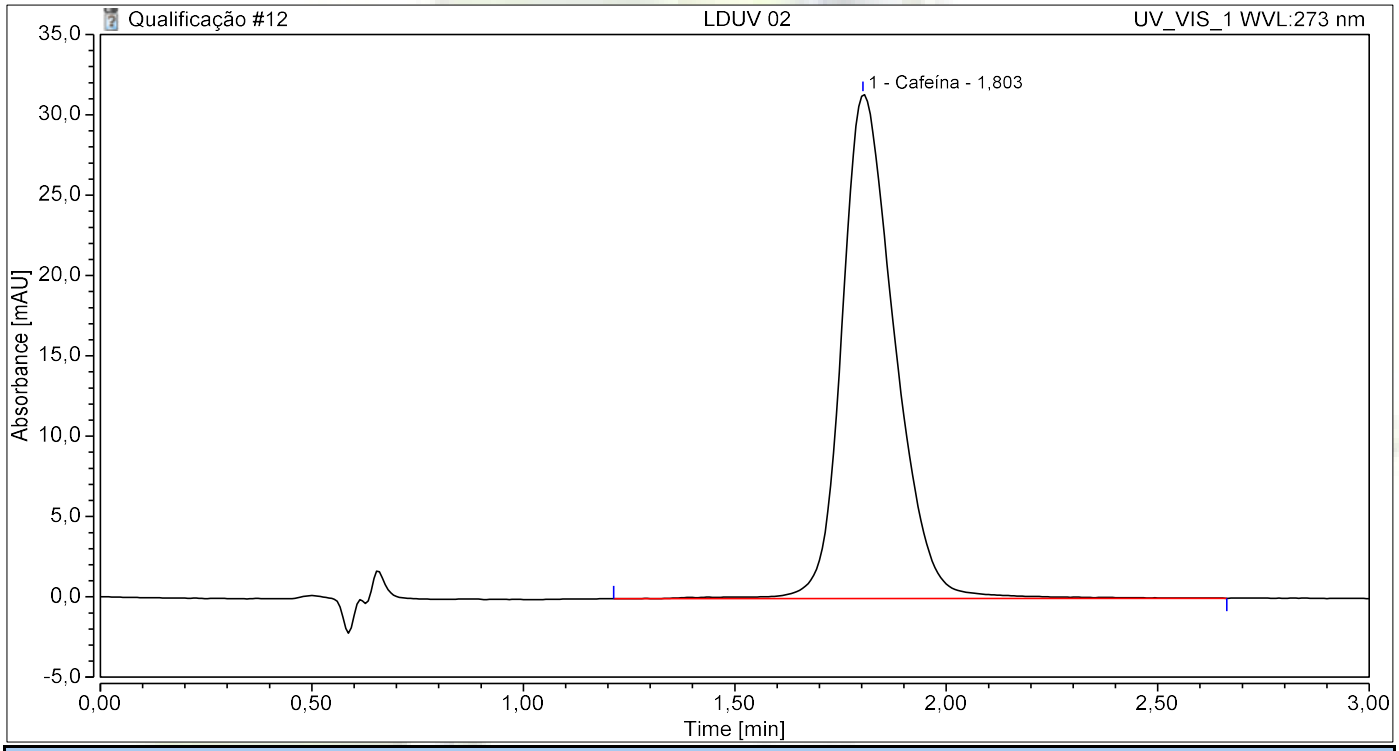

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,803	4,542	31,372	100,00	100,00	n.a.
Total:			**4,542**	**31,372**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**3,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:37**	*Sample Weight:*	**1,0000**

Chromatogram

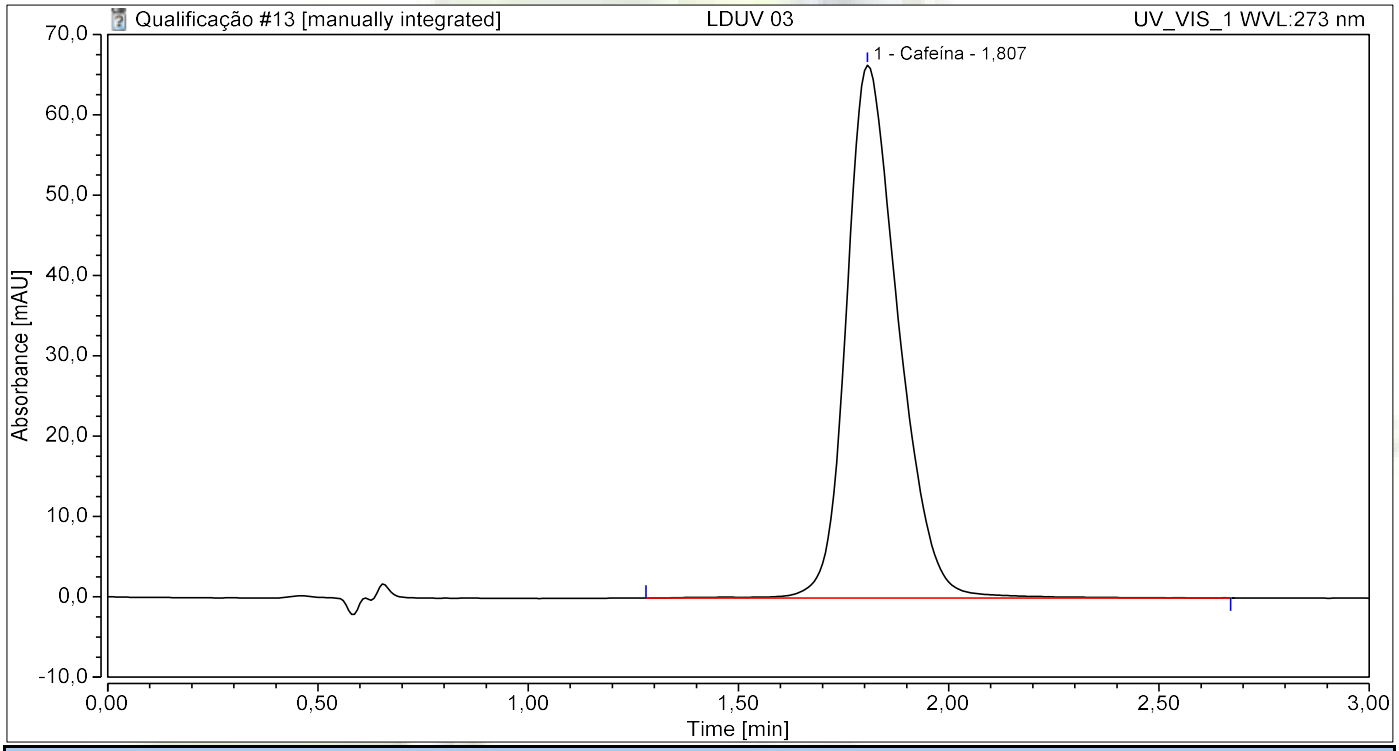

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,807	9,523	66,342	100,00	100,00	n.a.
Total:			**9,523**	**66,342**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**3,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:41**	*Sample Weight:*	**1,0000**

Chromatogram

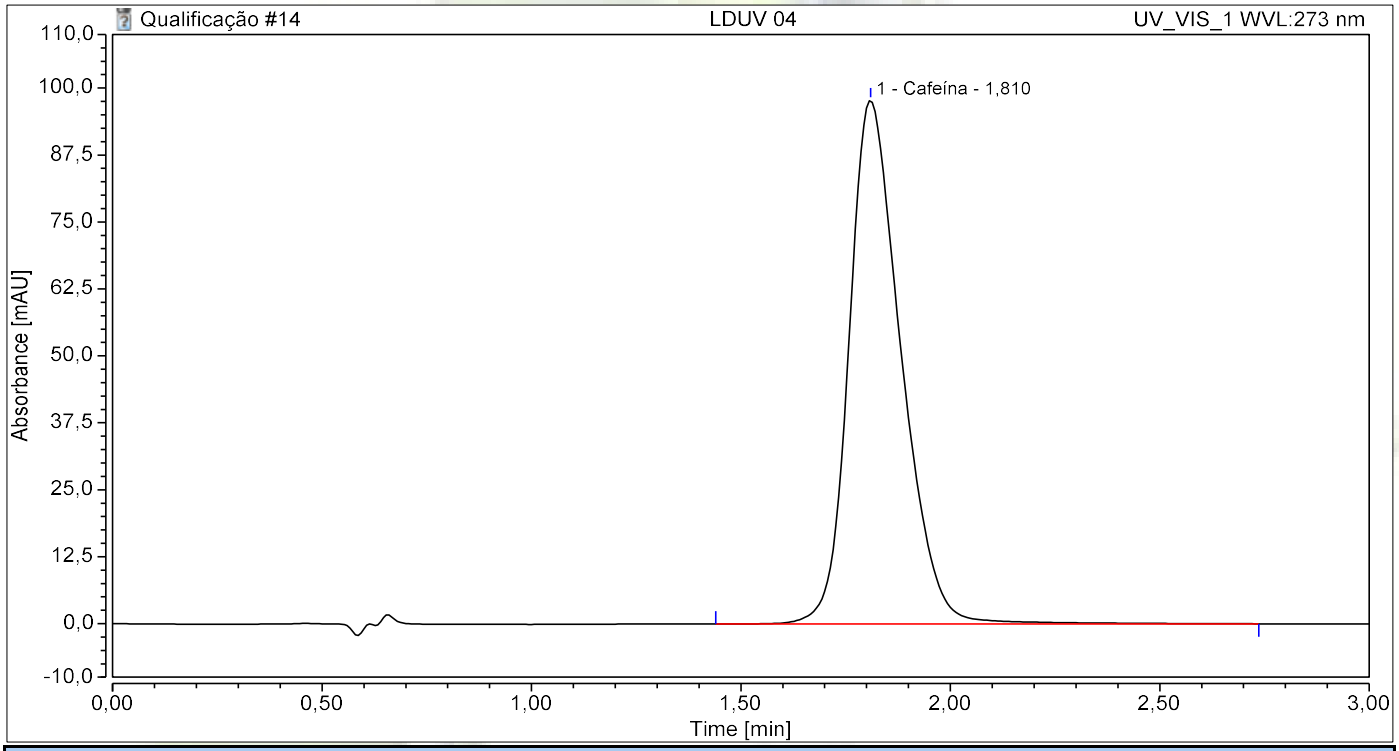

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,810	14,055	97,710	100,00	100,00	n.a.
Total:			**14,055**	**97,710**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 05**	*Run Time (min):*	**3,00**
Vial Number:	**RA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:45**	*Sample Weight:*	**1,0000**

Chromatogram

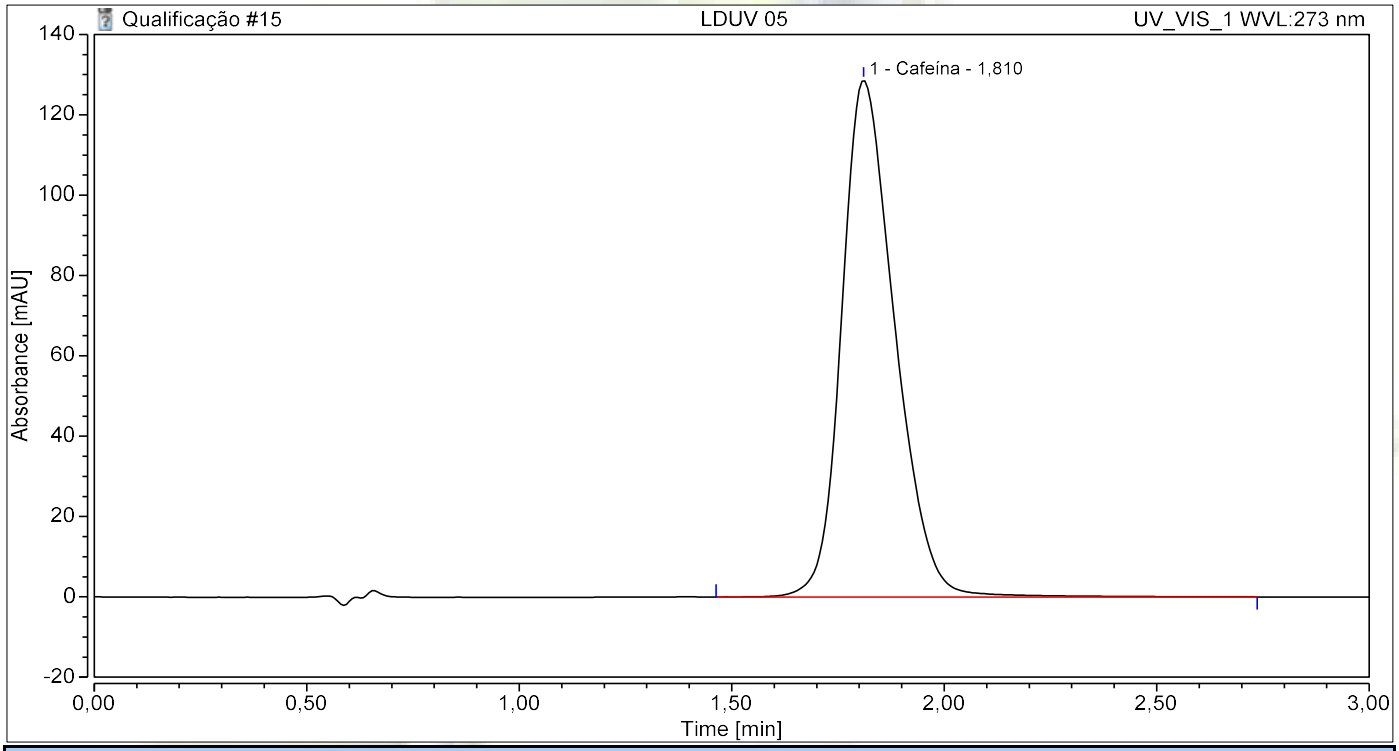

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,810	18,639	128,696	100,00	100,00	n.a.
Total:			**18,639**	**128,696**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:49**	*Sample Weight:*	**1,0000**

Chromatogram

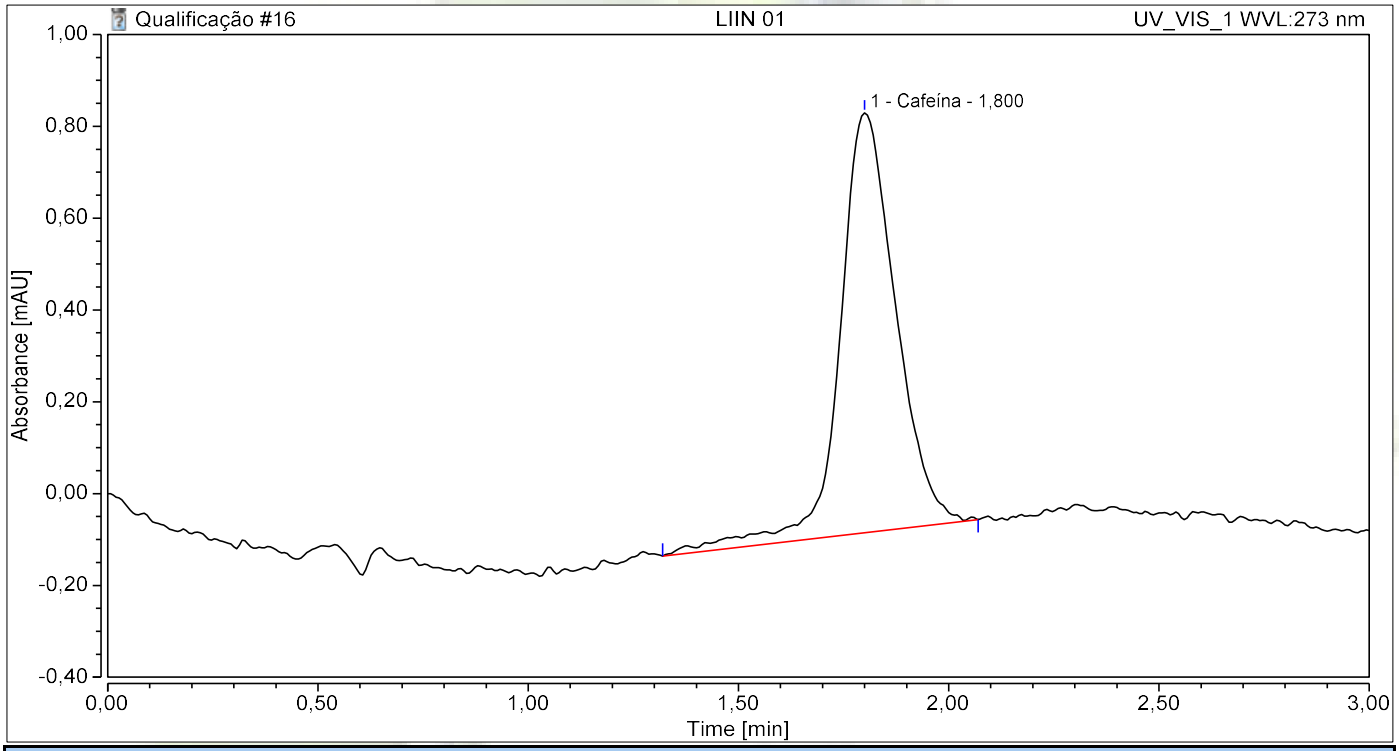

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,800	0,142	0,915	100,00	100,00	n.a.
Total:			**0,142**	**0,915**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:53**	*Sample Weight:*	**1,0000**

Chromatogram

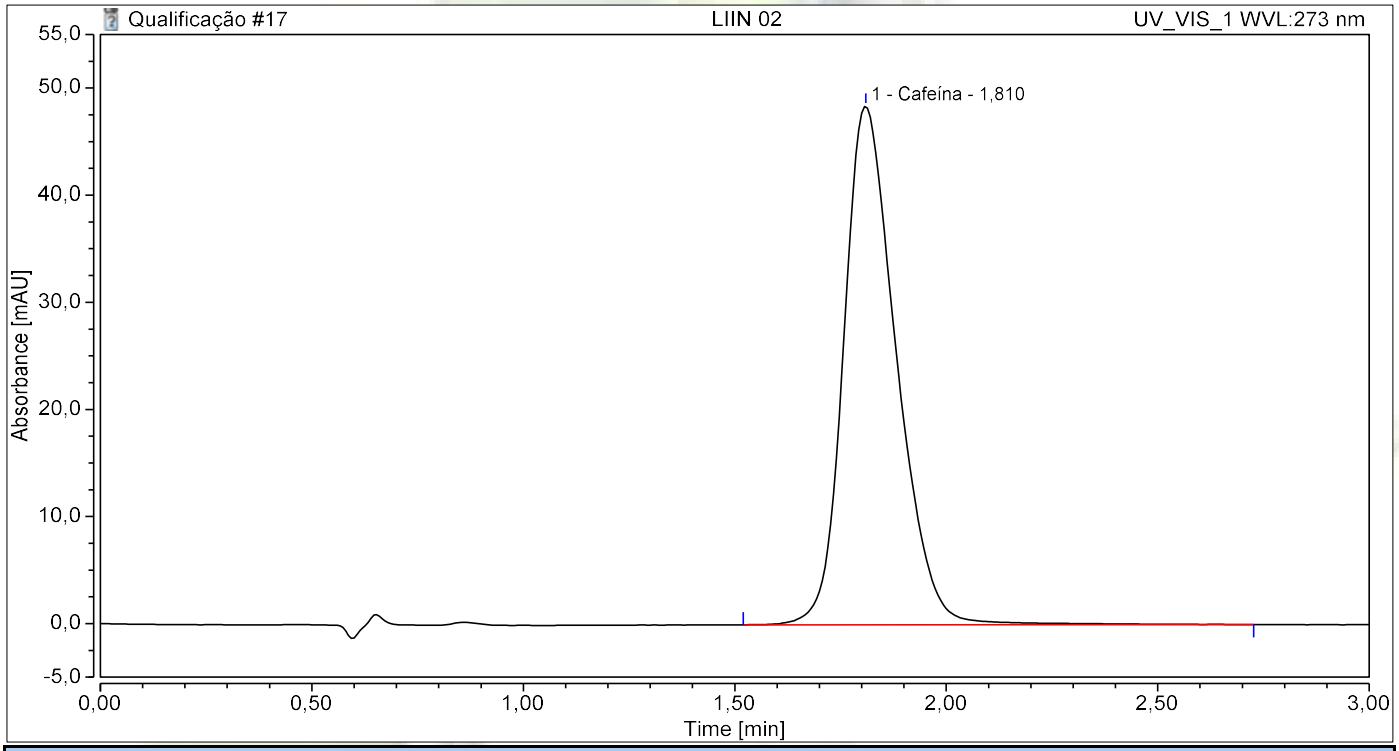

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,810	6,991	48,417	100,00	100,00	n.a.
Total:			**6,991**	**48,417**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 10:56**	*Sample Weight:*	**1,0000**

Chromatogram

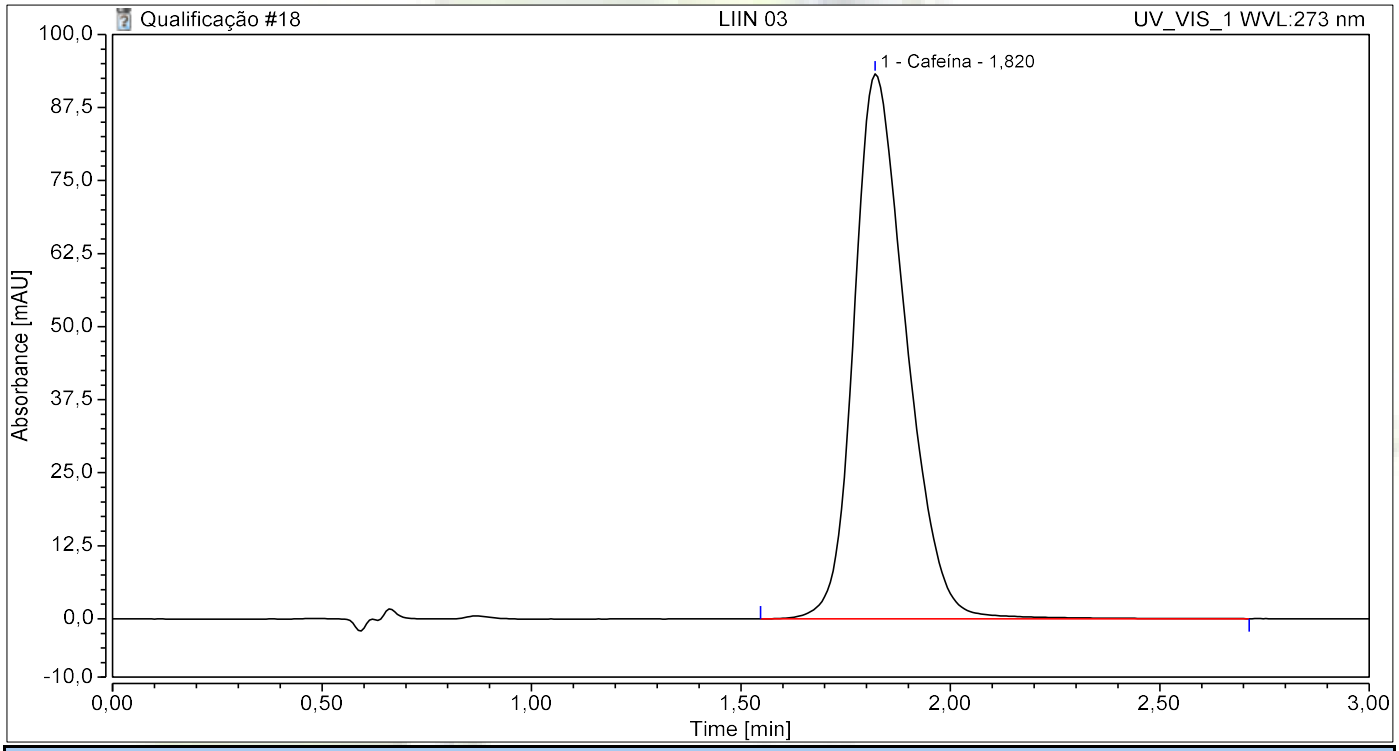

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,820	13,487	93,267	100,00	100,00	n.a.
Total:			**13,487**	**93,267**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 11:00**	*Sample Weight:*	**1,0000**

Chromatogram

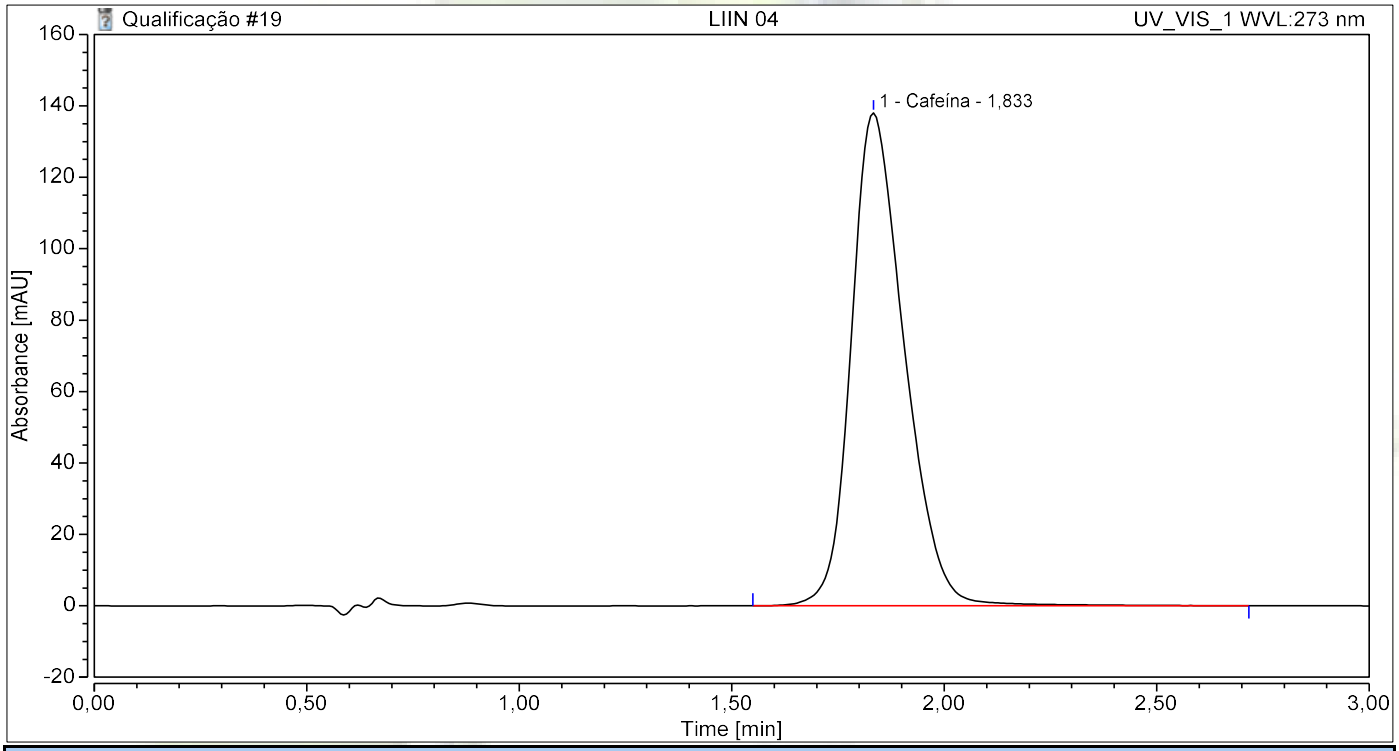

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,833	19,999	138,079	100,00	100,00	n.a.
Total:			**19,999**	**138,079**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**3,00**
Vial Number:	**RA6**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 11:04**	*Sample Weight:*	**1,0000**

Chromatogram

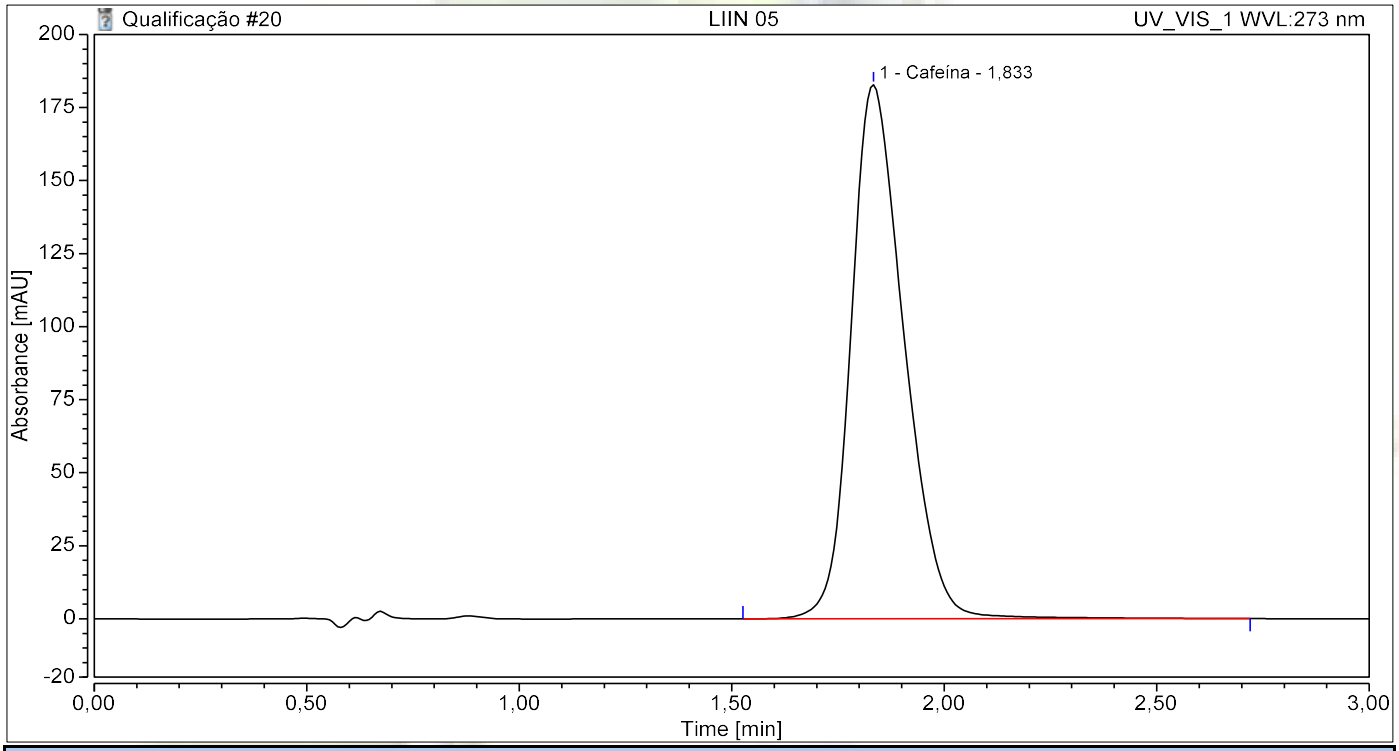

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,833	26,447	182,839	100,00	100,00	n.a.
Total:			**26,447**	**182,839**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**Gradiente AB**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Gradiente AB**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 11:22**	*Sample Weight:*	**1,0000**

Chromatogram

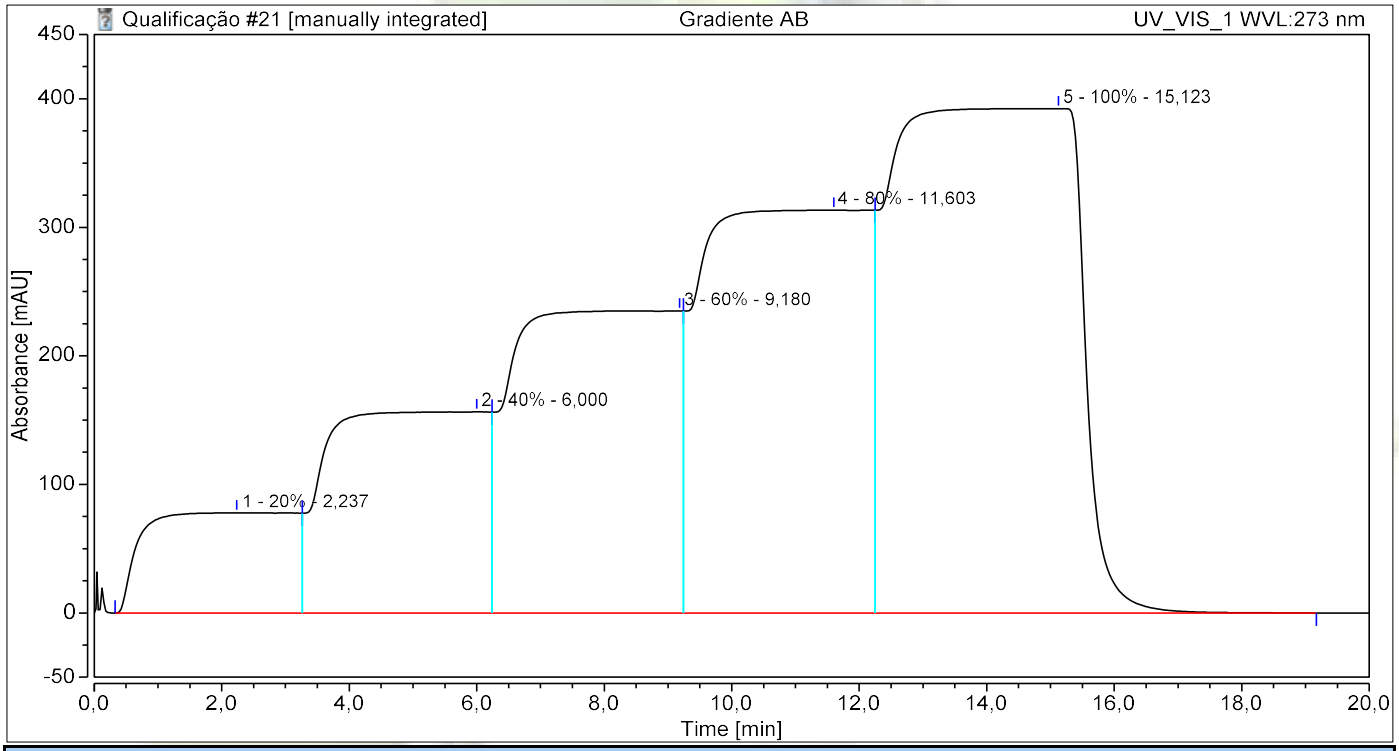

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	20%	2,237	204,731	78,114	5,81	6,64	n.a.
2	40%	6,000	437,640	156,638	12,41	13,32	n.a.
3	60%	9,180	676,086	235,087	19,17	20,00	n.a.
4	80%	11,603	915,152	313,457	25,95	26,66	n.a.
5	100%	15,123	1293,024	392,384	36,66	33,38	n.a.
Total:			**3526,633**	**1175,680**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**Gradiente CD**	*Run Time (min):*	**20,00**
Vial Number:	**RA1**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Gradiente CD**	*Bandwidth:*	**1**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 11:43**	*Sample Weight:*	**1,0000**

Chromatogram

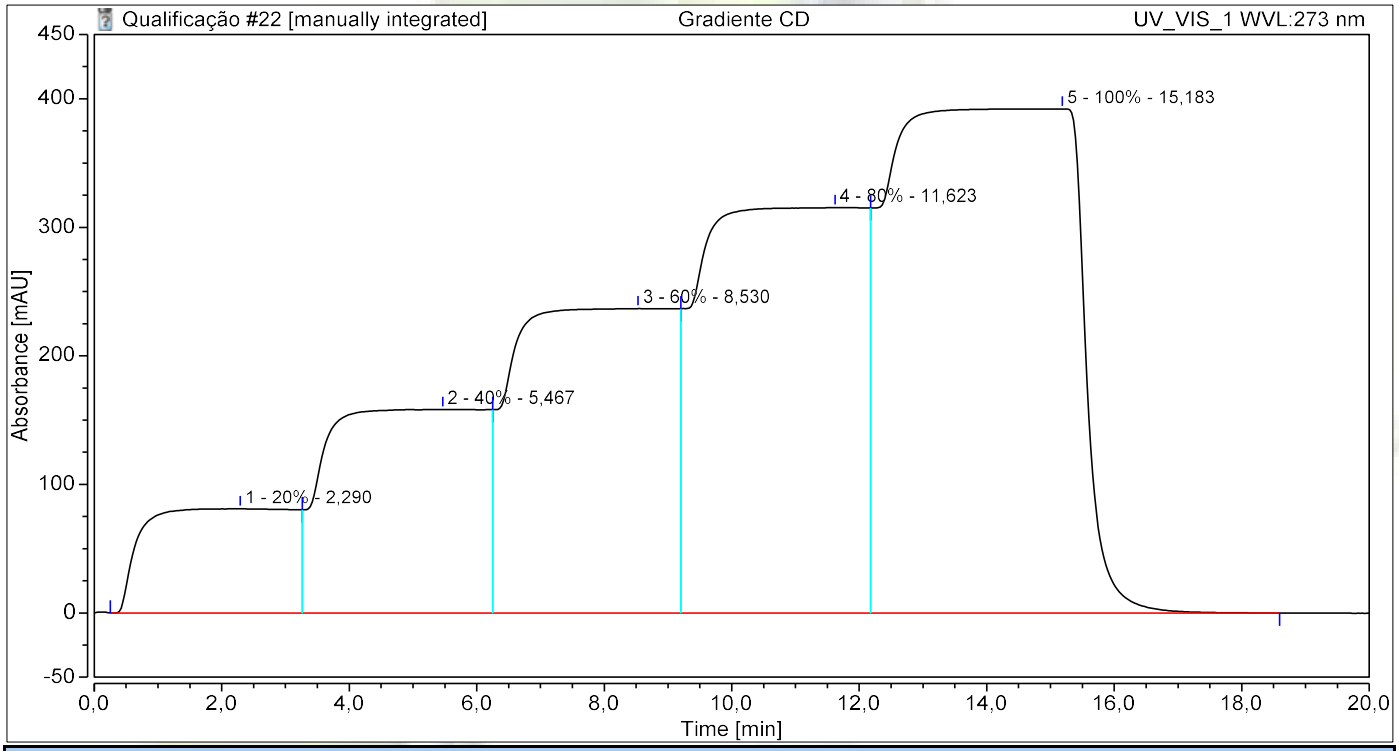

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	20%	2,290	212,547	80,997	5,99	6,84	n.a.
2	40%	5,467	445,111	158,248	12,54	13,37	n.a.
3	60%	8,530	670,050	236,814	18,87	20,01	n.a.
4	80%	11,623	907,050	315,386	25,55	26,65	n.a.
5	100%	15,183	1315,747	392,118	37,06	33,13	n.a.
Total:			**3550,505**	**1183,562**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.24543

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 01**	*Run Time (min):*	**1,00**
Vial Number:	**RB1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**RI**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 12:44**	*Sample Weight:*	**1,0000**

Chromatogram

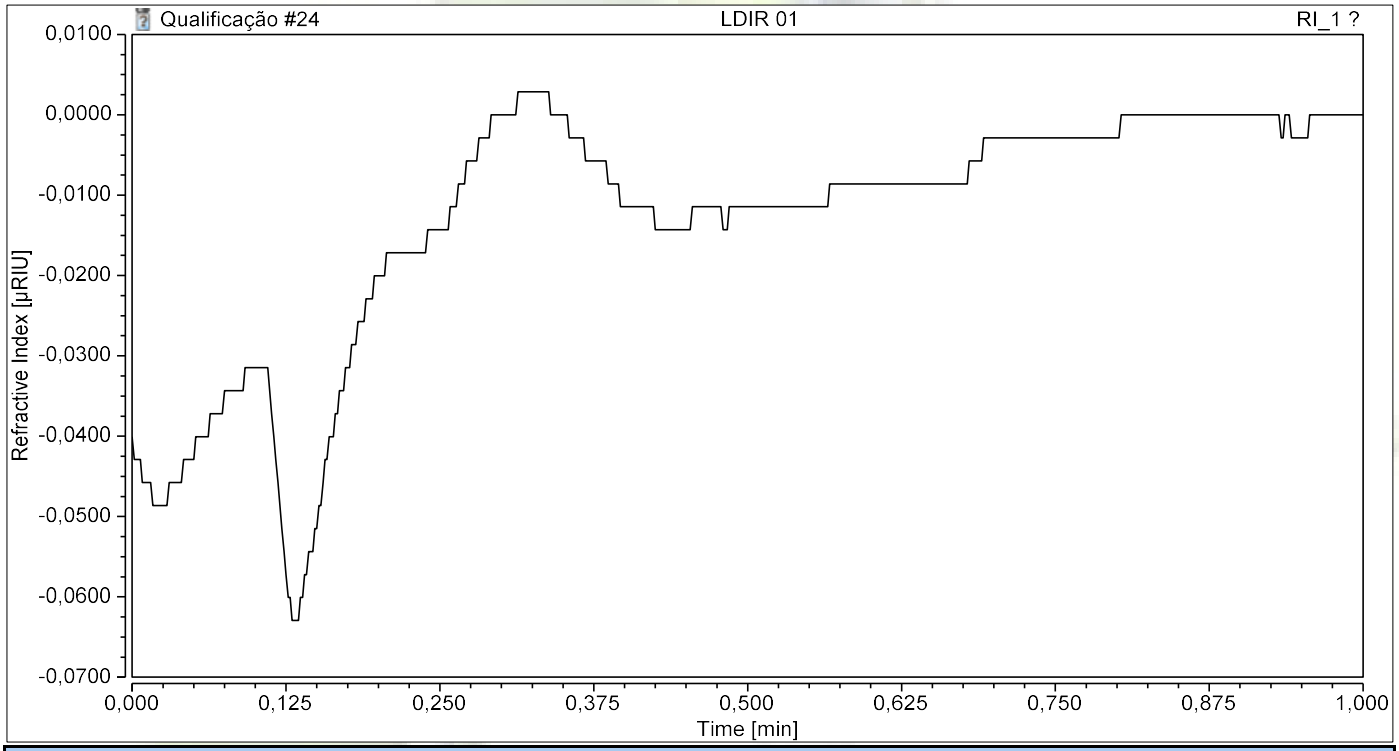

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
n.a.	PDRI	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.24543

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 02**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**RI**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 12:45**	*Sample Weight:*	**1,0000**

Chromatogram

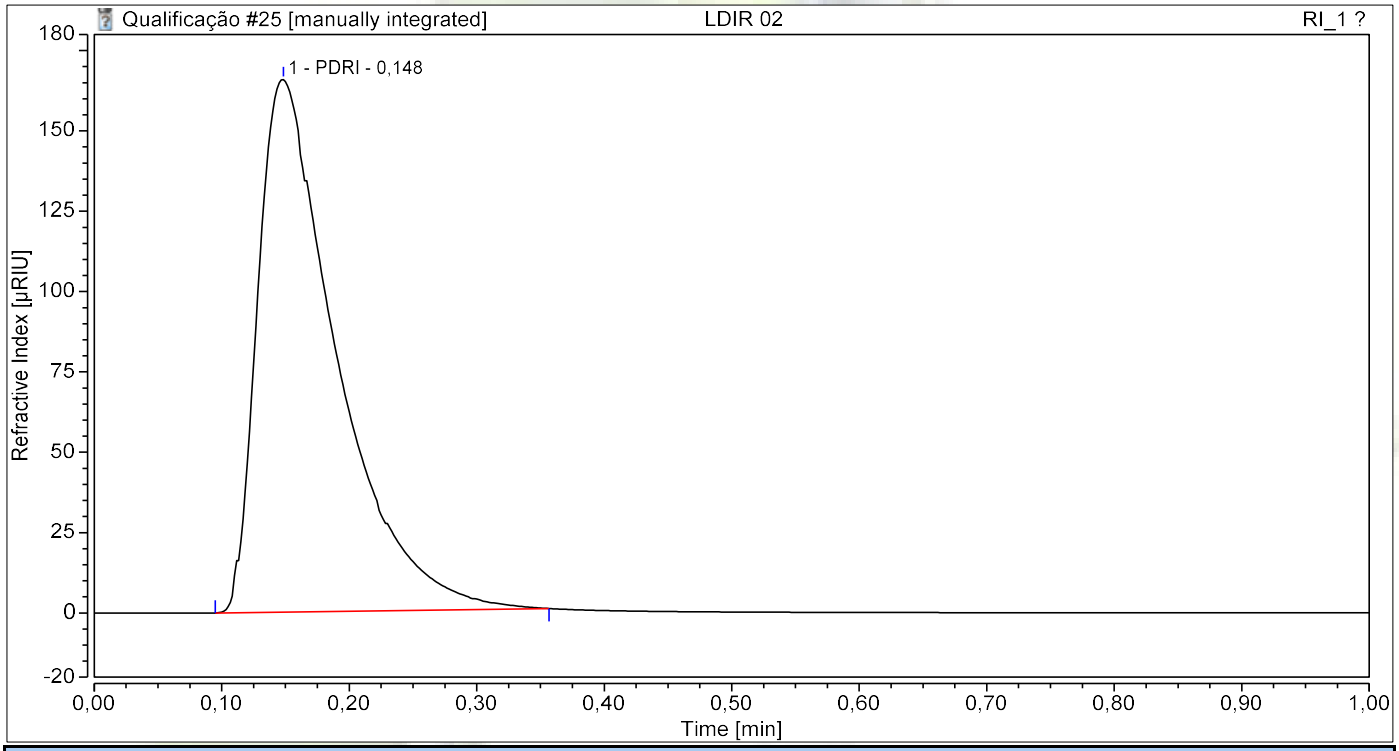

Integration Results


No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	PDRI	0,148	11,879	165,703	100,00	100,00	n.a.
Total:			**11,879**	**165,703**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 03**	*Run Time (min):*	**1,00**
Vial Number:	**RB3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**RI**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 12:47**	*Sample Weight:*	**1,0000**

Chromatogram

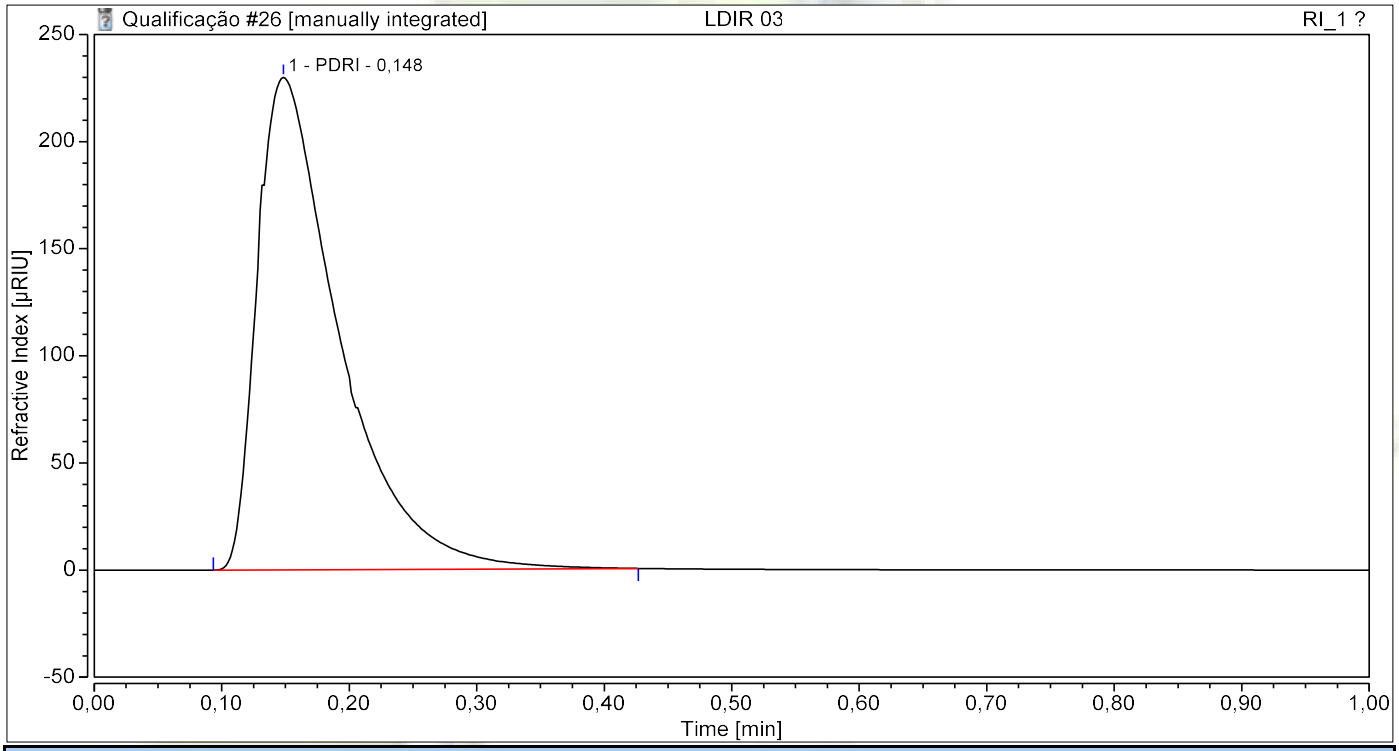

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	PDRI	0,148	17,130	229,867	100,00	100,00	n.a.
Total:			**17,130**	**229,867**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.24543

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 04**	*Run Time (min):*	**1,00**
Vial Number:	**RB4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**RI**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 12:49**	*Sample Weight:*	**1,0000**

Chromatogram

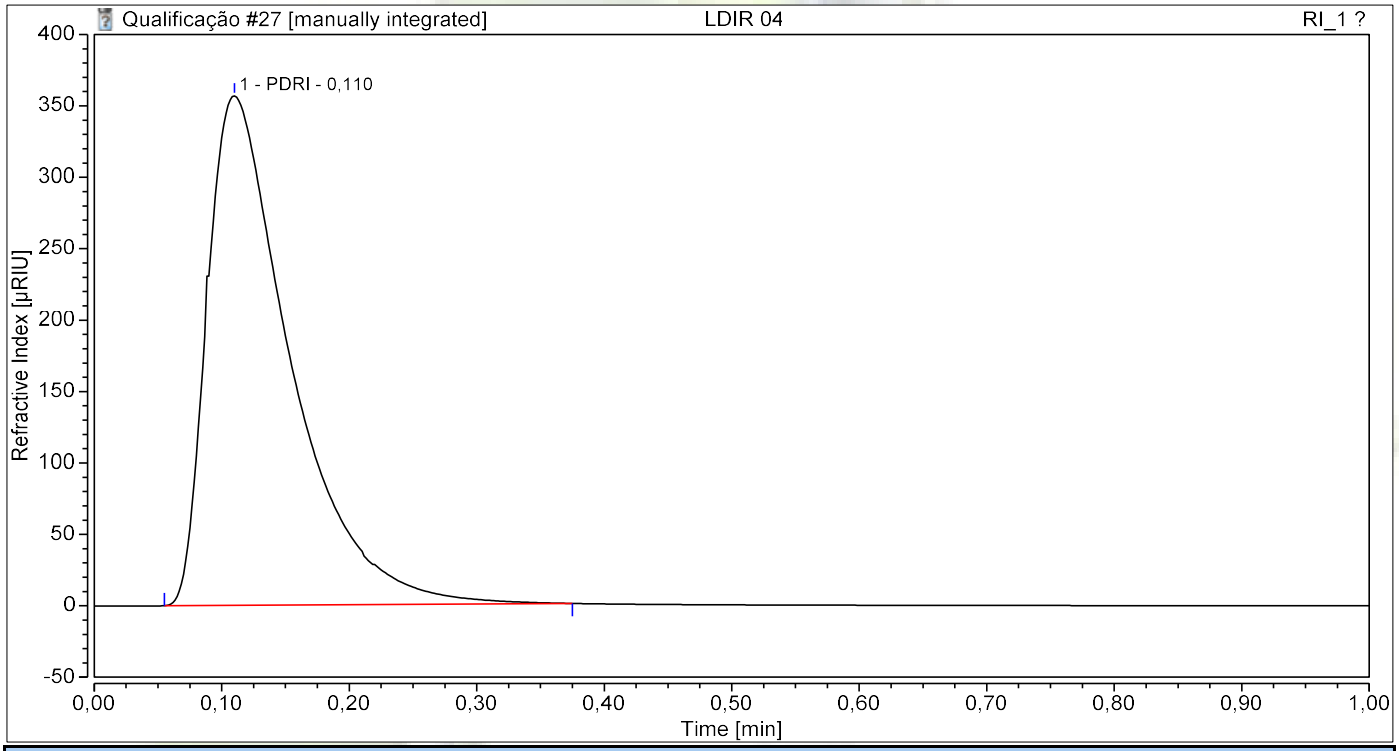

Integration Results


No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	PDRI	0,110	27,060	356,584	100,00	100,00	n.a.
Total:			**27,060**	**356,584**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 05**	*Run Time (min):*	**1,00**
Vial Number:	**RB5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**RI**	*Bandwidth:*	**n.a.**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/nov/22 12:51**	*Sample Weight:*	**1,0000**

Chromatogram

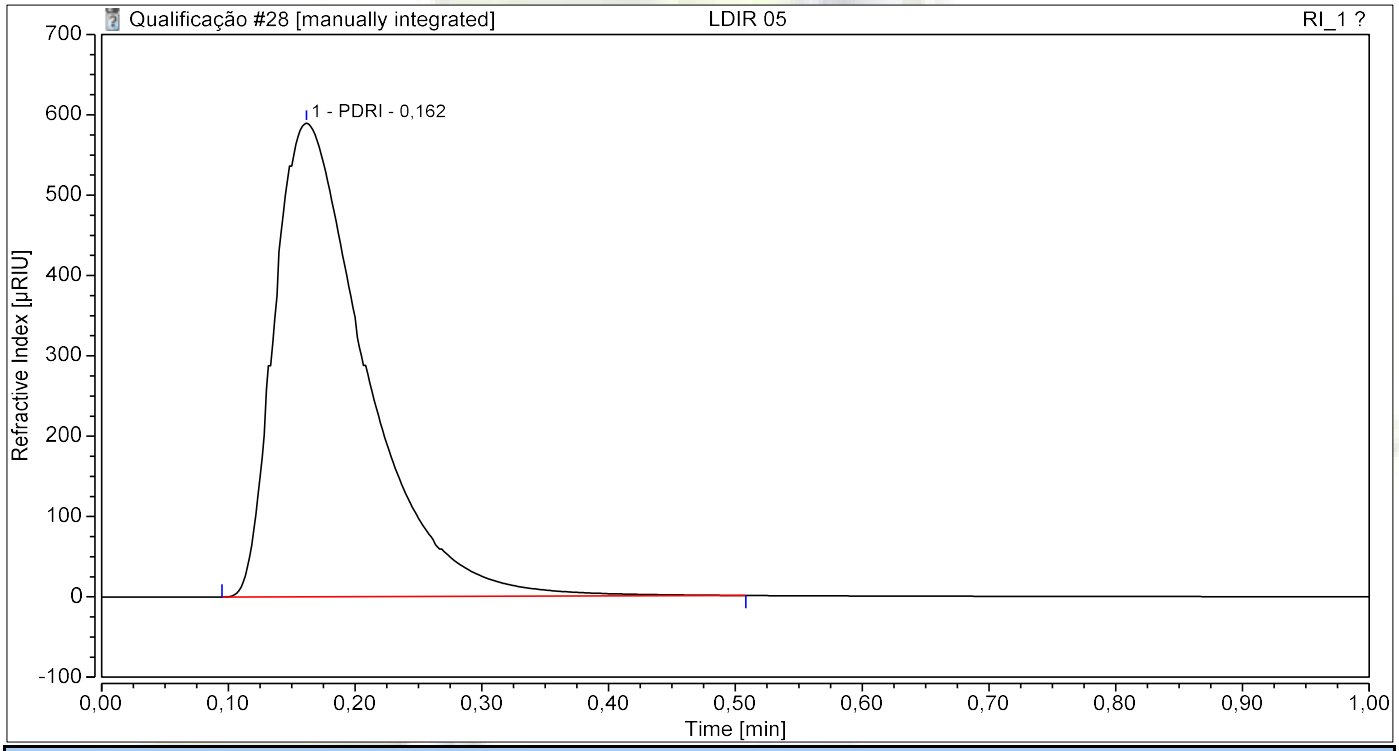

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	PDRI	0,162	49,300	589,288	100,00	100,00	n.a.
Total:			**49,300**	**589,288**	**100,00**	**100,00**	