Agilent 21-CFR-11 package active

Equiplex Industria Farmaceutica

Cary Validation Report

on PC160 at Local time:9/17/2025 11:01:48 AM GMT: 9/17/2025 2:01:48 PM by Administrador\IQOQ_ESFO0003\THAYS = Thays Pereira Rocha ;Serial Number: G6860A MY20369207;

Report time	9/17/2025 11:02:08 AM
Method:	
Report	PC160\SQLEXPRESS|VAIMDB_ESFO0003(000)|IQOQ\Set_2025\201 EXATIDAO COMP ONDA1.BVO
Version	5.1.3.1042
Instrument	Cary 60
Operator	Administrador\IQOQ_ESFO0003\THAYS (Thays Pereira Rocha)

Wavelength Accuracy Test - Holmium Oxide Method

9/17/2025 11:02:14 AM
Instrument Settings

Filter Serial Number :	B050-7805
SBW :	1.50 nm
Ave Time :	0.100 sec
Interval :	0.15 nm
Scan range :	648.00 nm to 269.50 nm

638.000 line found at 637.508 PASSED
Tolerance for 638.000 nm ±1.00 nm

536.300 line found at 536.517 PASSED
Tolerance for 536.300 nm ±1.00 nm


453.900 line found at 453.729 PASSED
Tolerance for 453.900 nm ±1.00 nm

419.000 line found at 418.779 PASSED
Tolerance for 419.000 nm ±1.00 nm

361.300 line found at 360.582 PASSED
Tolerance for 361.300 nm ±1.00 nm

287.600 line found at 287.098 PASSED
Tolerance for 287.600 nm ±1.00 nm

279.500 line found at 278.687 PASSED
Tolerance for 279.500 nm ±1.00 nm

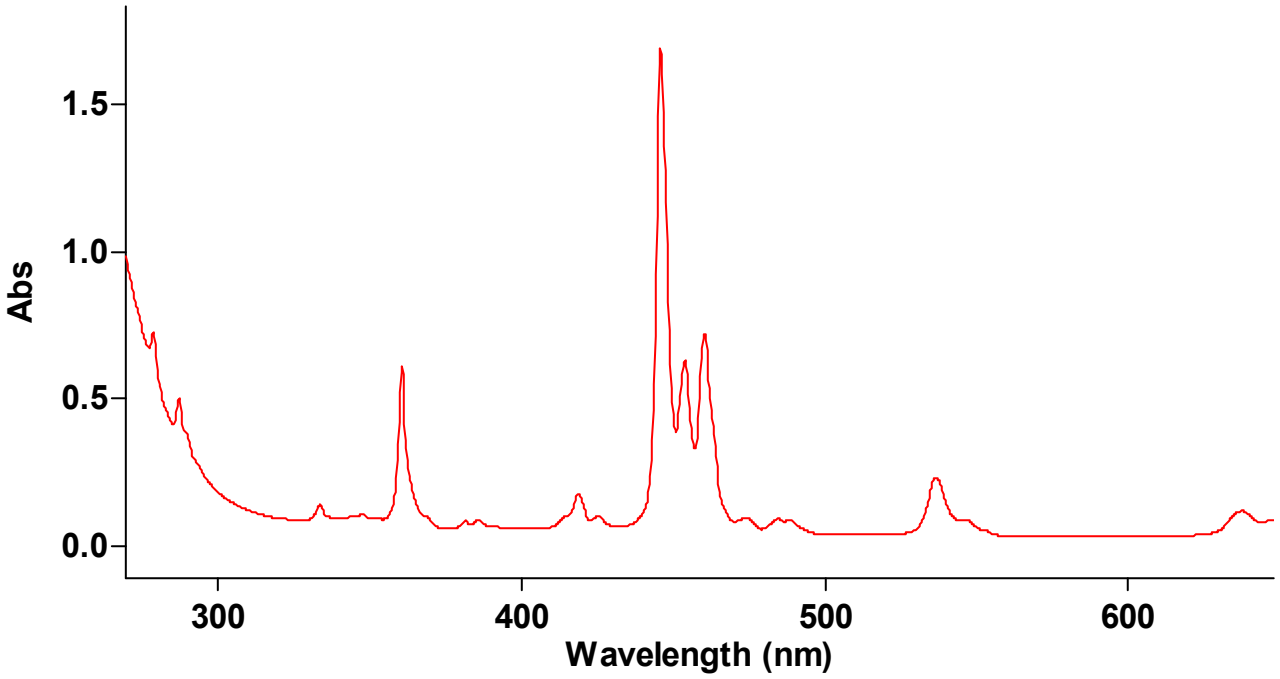

Wavelength Accuracy Test - Holmium Oxide Method PASSED

Operator Signature :_____ Date : _____

Supervisor Signature :_____ Date : _____