
Agilent 21-CF R-11 package active

Zero Report

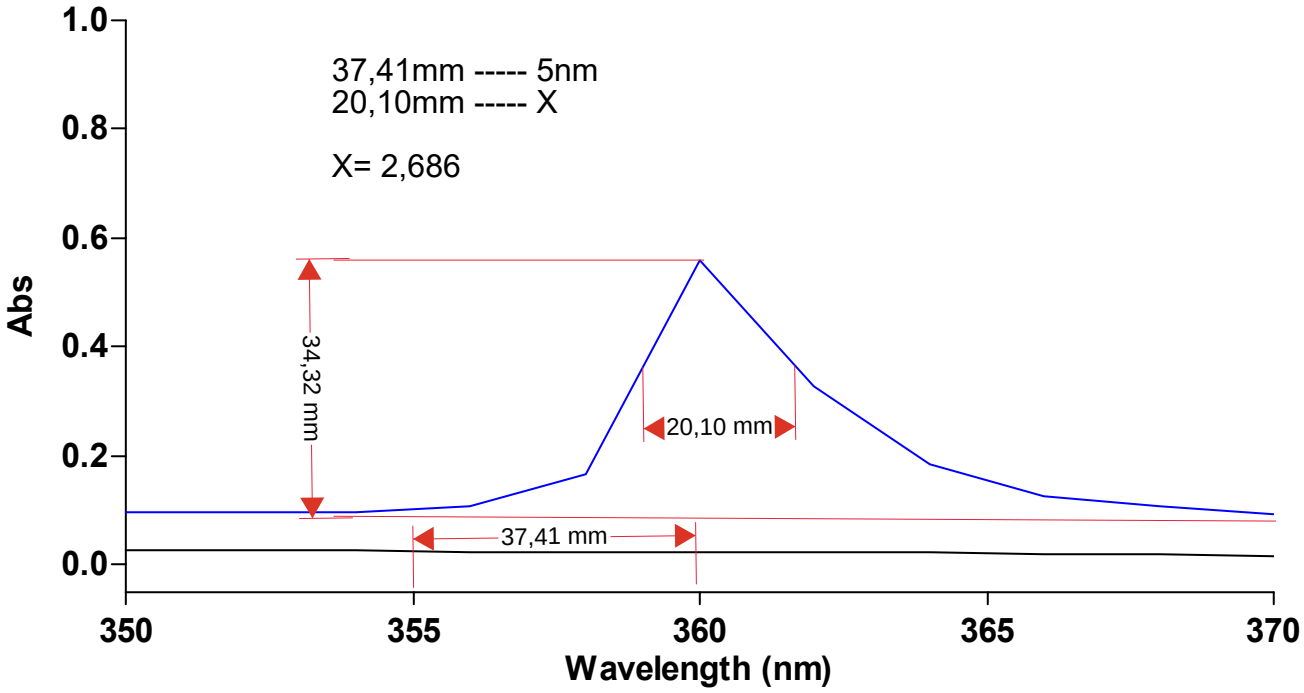

Read	Abs (370.0 nm)
Zero	0.0178

Equiplex Industria Farmaceutica

Scan Analysis Report

on PC160 at Local time:9/17/2025 2:54:48 PM GMT: 9/17/2025 5:54:48 PM by Administrador\IQOQ_ESFO0003\Thays = Thays Pereira Rocha ;Serial Number: G6860A MY20369207;

Report Time :	Wed 17 Sep 02:55:01 PM 2025
Method	
Batch:	PC160\SQLEXPRESS|VAIMDB_ESFO0003(000)|IQOQ\Set_2025\20 3 RESOLUCAO-BSW.BSW
Software version:	5.1.3.1042
Operator:	Administrador\IQOQ_ESFO0003\Thays (Thays Pereira Rocha)

Instrument Parameters

Instrument	Cary 60
Instrument Version	2.00
Start (nm)	370.0
Stop (nm)	350.0
X Mode	Nanometers
Y Mode	Abs
UV-Vis Scan Rate (nm/min)	4800.00
UV-Vis Data Interval (nm)	1.00
UV-Vis Ave. Time (sec)	0.0125
Beam Mode	Dual Beam
Baseline Correction	Off
Cycle Mode	Off
Comments	

Zero Report

Read	Abs (370.0 nm)
Zero	0.0178

Sample Name: sample1

Collection Time	9/17/2025 2:55:06 PM

Peak Table

Peak Style	Peaks
Peak Threshold	0.0100
Range	370.0nm to 350.0nm

Wavelength (nm)	Abs
360.0	0.531