Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\EDUV 001.sirslt\EDUV 001.dx		
Sample name:	EDUV 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A1
Injection date:	2022-11-08 10:24:25-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*3D UV Quantitative_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 10:41:00-03:00		

RT:

0.961


Compound Name:

Cafeína

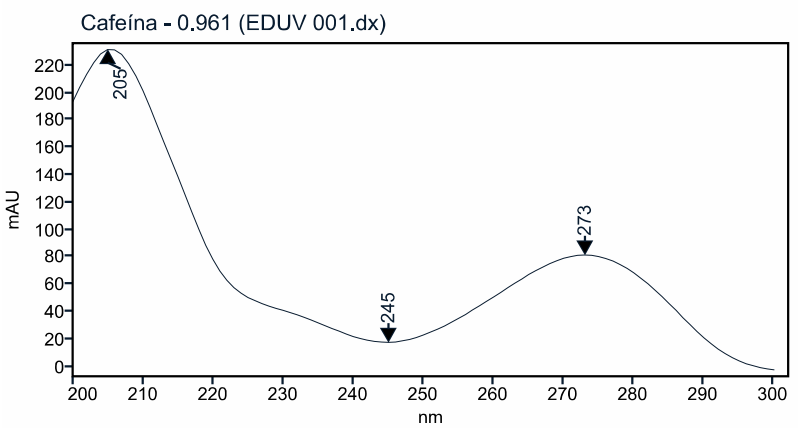

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 10-47-47-03-00-01.dx		
Sample name:	Branco PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A2
Injection date:	2022-11-08 10:48:43-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

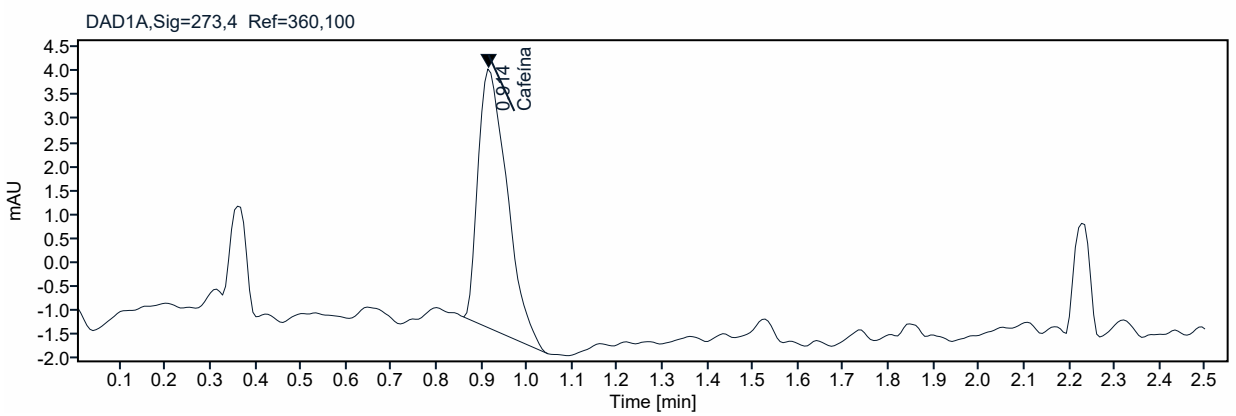

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.914	24.2710			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 10-51-20-03-00-02.dx		
Sample name:	PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 10:52:16-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

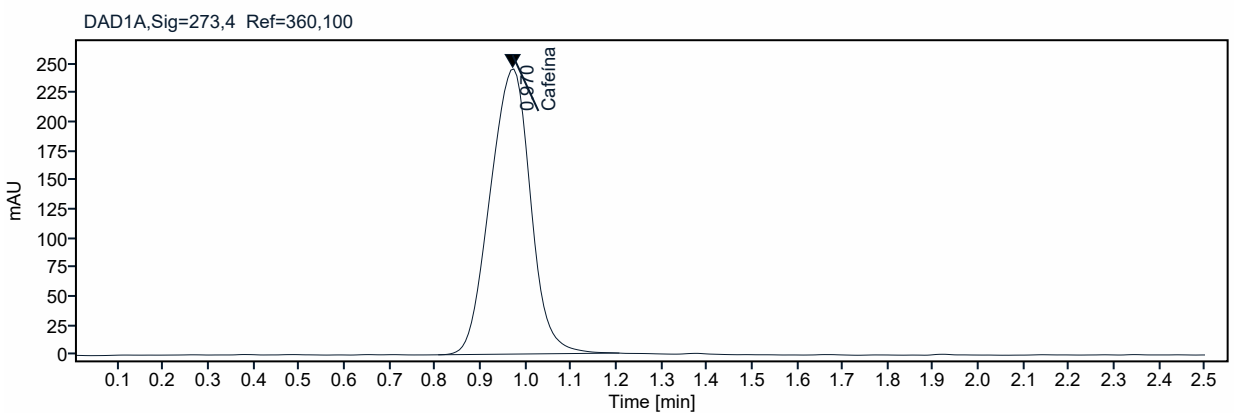

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.970	1521.4007			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 10-54-52-03-00-03.dx		
Sample name:	PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 10:55:50-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

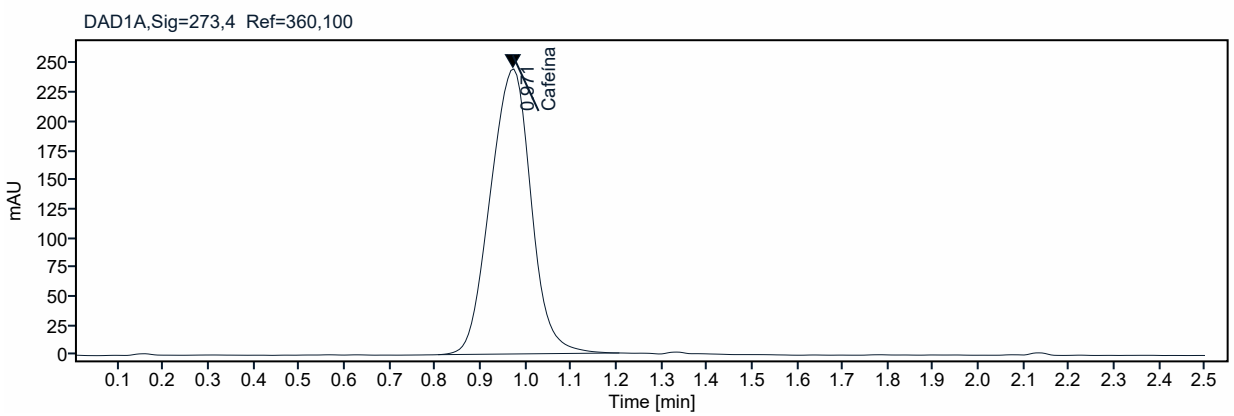

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.971	1531.1787			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 10-58-27-03-00-04.dx		
Sample name:	PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 10:59:23-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

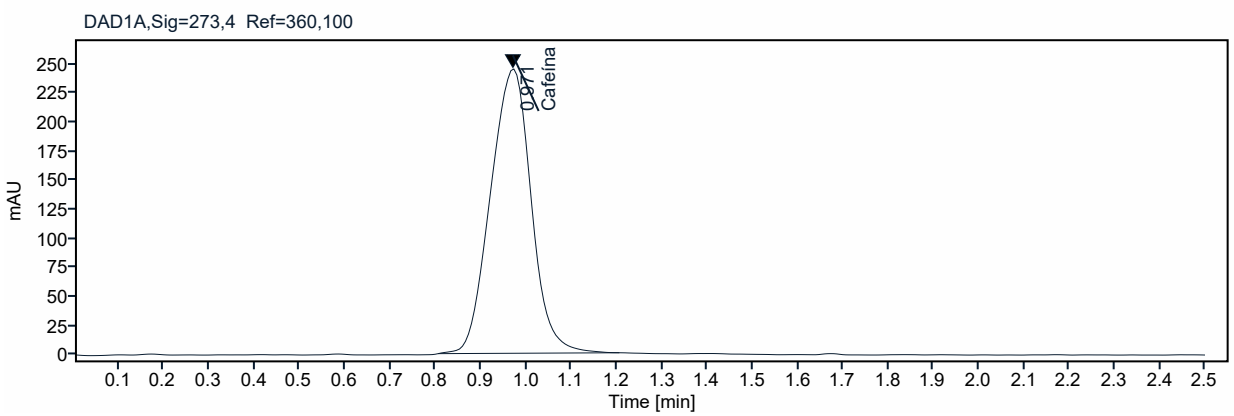

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.971	1527.3036			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 11-02-00-03-00-05.dx		
Sample name:	Branco PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A2
Injection date:	2022-11-08 11:02:57-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

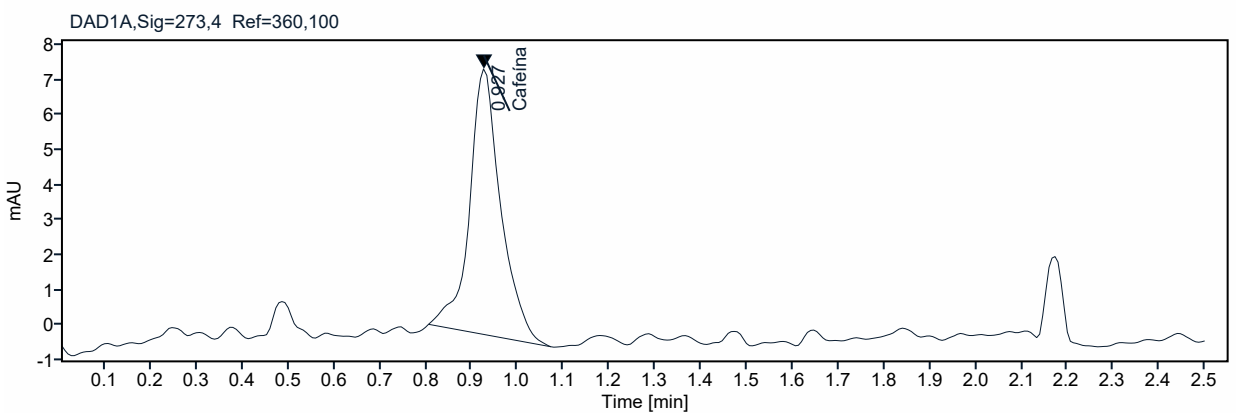

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.927	36.0184			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 11-05-34-03-00-06.dx		
Sample name:	PCIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 11:06:31-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

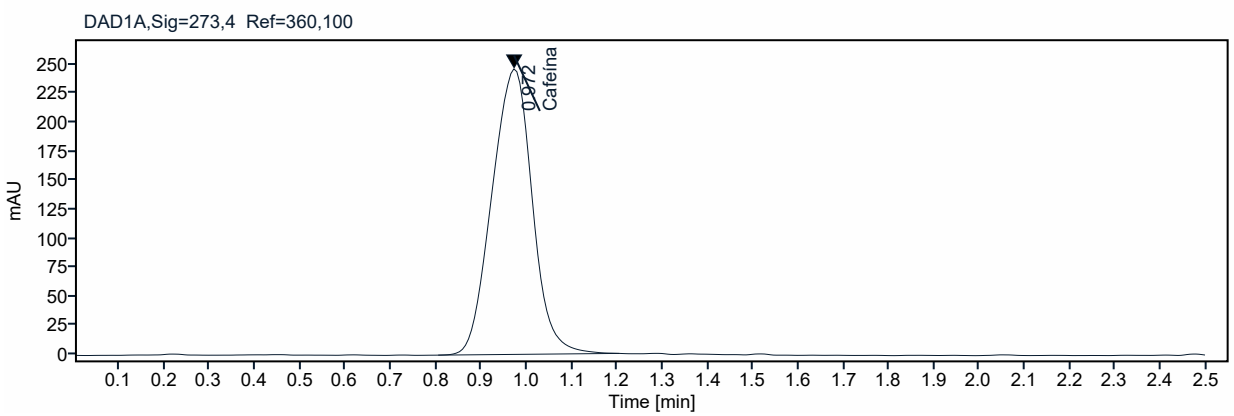

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.972	1522.8391			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 11-09-07-03-00-07.dx		
Sample name:	PCIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 11:10:03-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

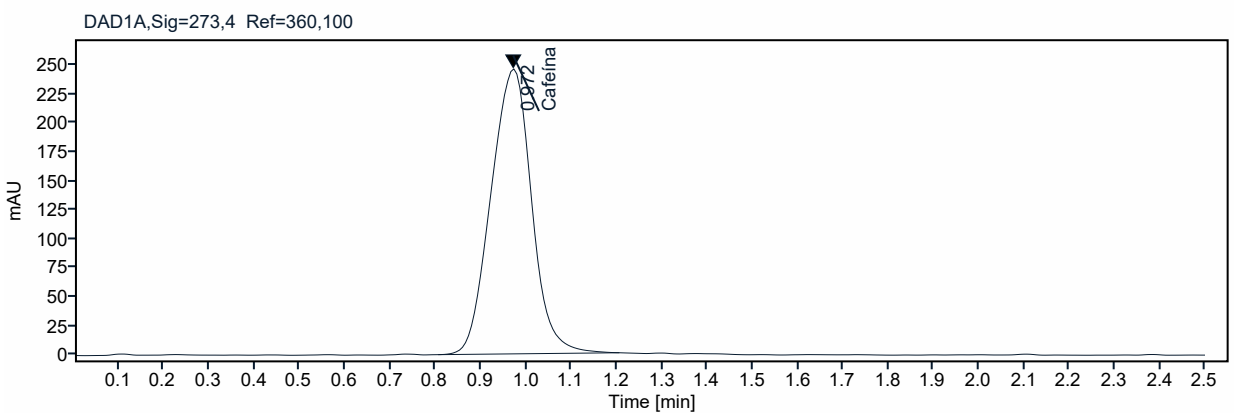

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.972	1532.0269			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 11-12-41-03-00-08.dx		
Sample name:	PCIN 06		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A3
Injection date:	2022-11-08 11:13:39-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

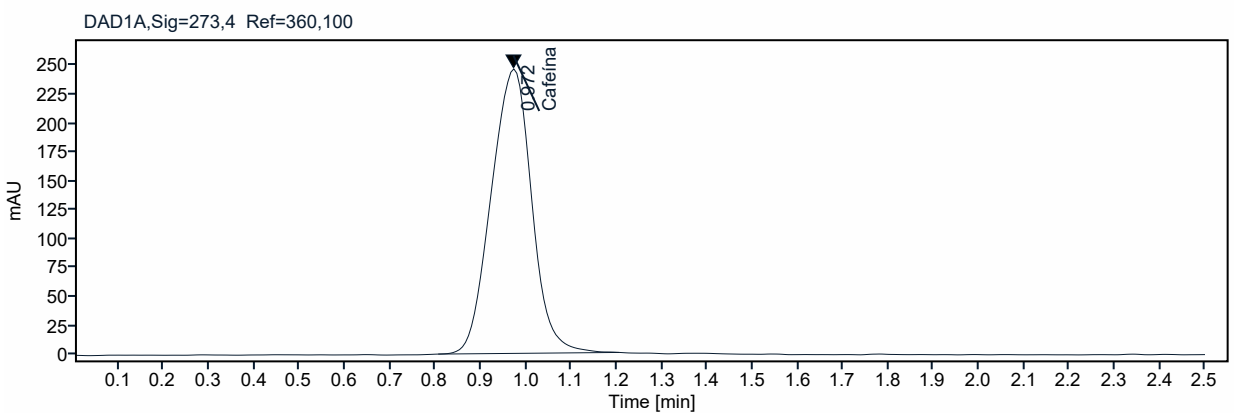

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.972	1528.1174			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\PCIN.rslt\2022-11-08 11-16-15-03-00-09.dx		
Sample name:	Branco PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A2
Injection date:	2022-11-08 11:17:12-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:26:12-03:00		

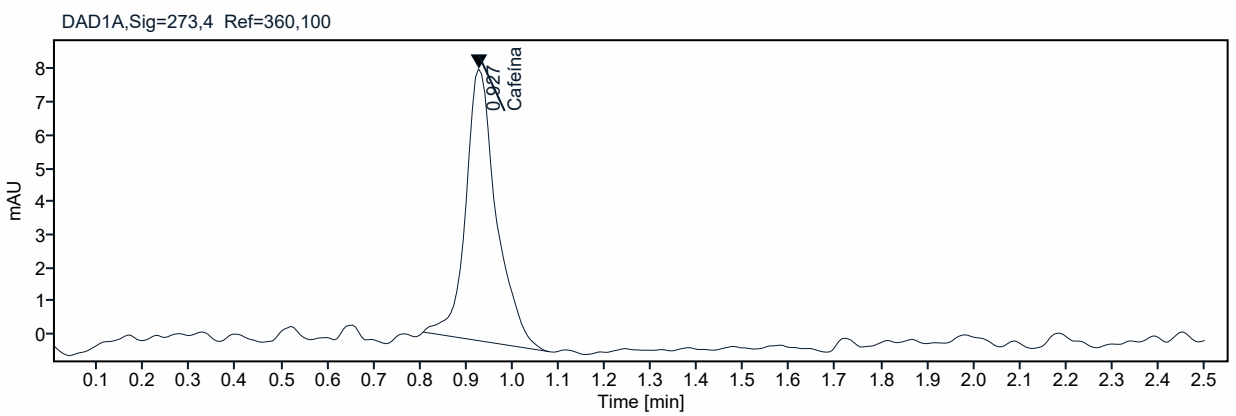

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.927	38.0087			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 11-52-55-03-00-01.dx		
Sample name:	LDUV 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A4
Injection date:	2022-11-08 11:53:53-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

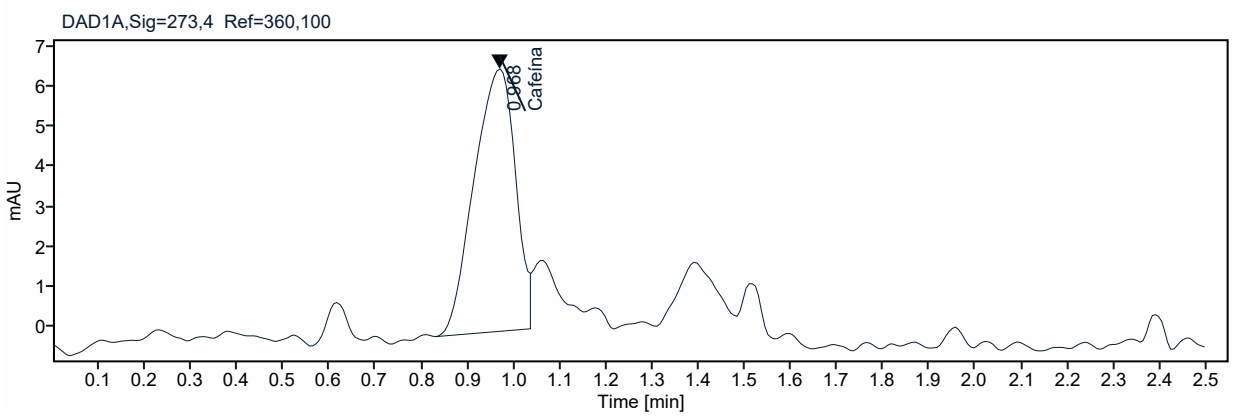

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.968	40.5720			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 11-56-29-03-00-02.dx		
Sample name:	LDUV 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A5
Injection date:	2022-11-08 11:57:24-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

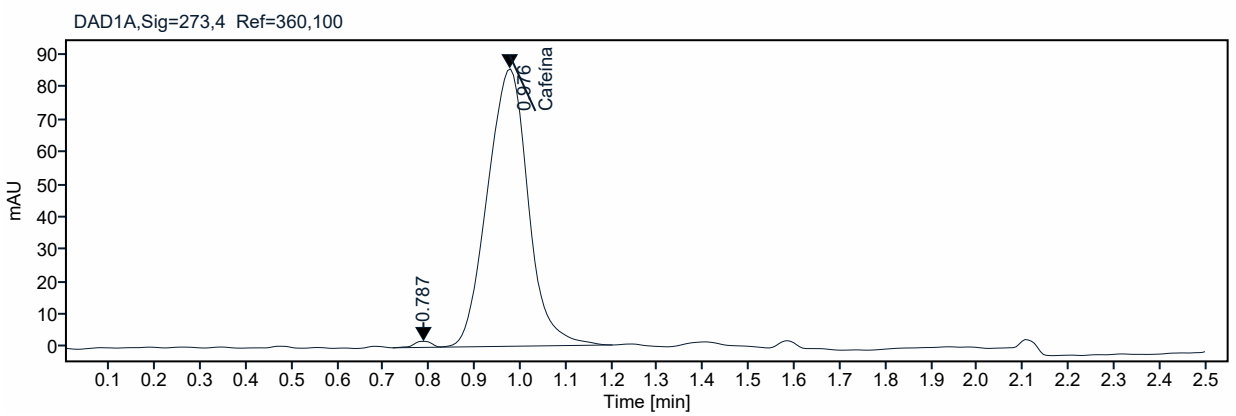

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	530.9493			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-00-02-03-00-03.dx		
Sample name:	LDUV 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A6
Injection date:	2022-11-08 12:00:59-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

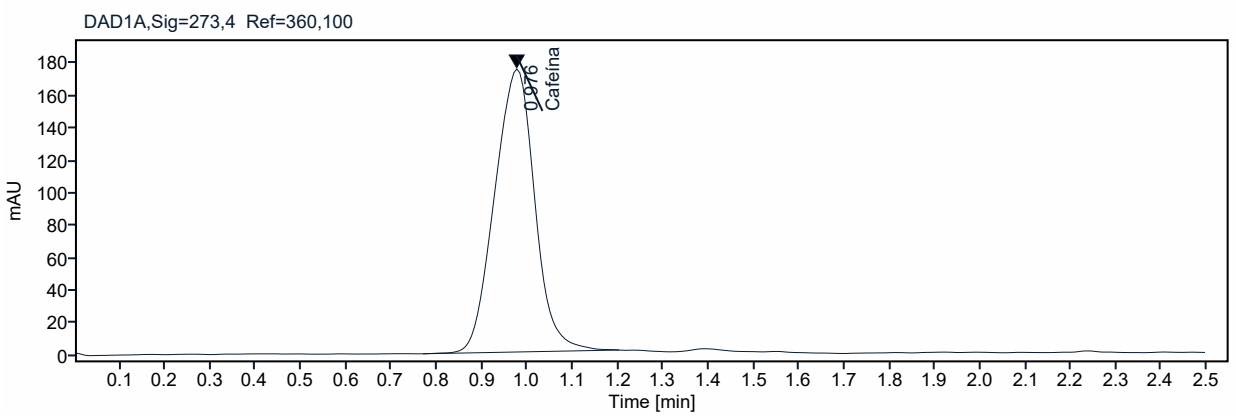

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	1073.3224			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-03-36-03-00-04.dx		
Sample name:	LDUV 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A7
Injection date:	2022-11-08 12:04:33-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

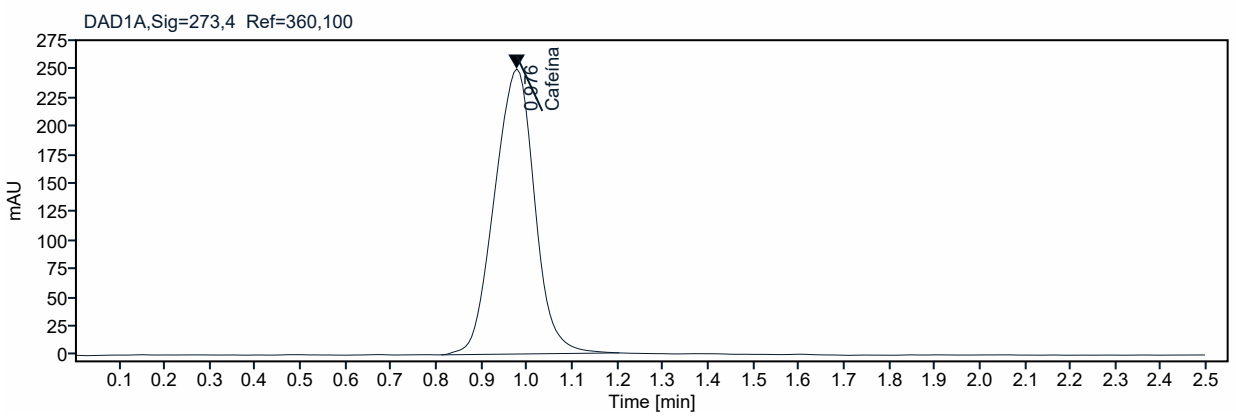

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	1536.4114			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-07-11-03-00-05.dx		
Sample name:	LDUV 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A8
Injection date:	2022-11-08 12:08:08-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

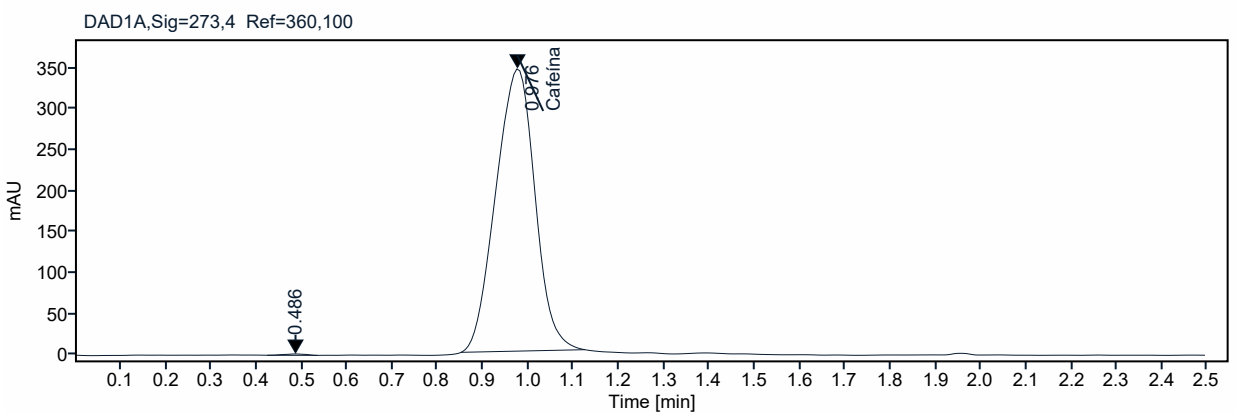

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	2072.2660			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 11-56-29-03-00-02.dx		
Sample name:	LDUV 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A5
Injection date:	2022-11-08 11:57:24-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

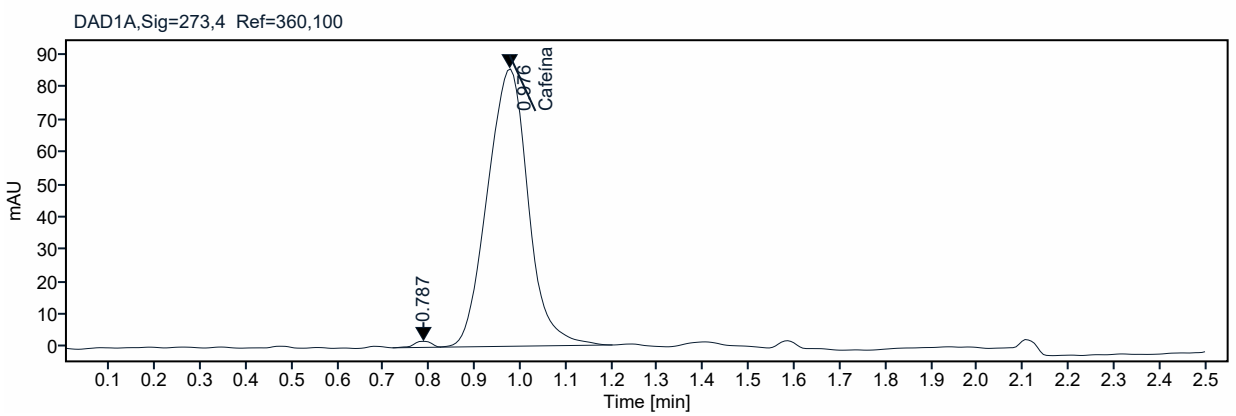

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	530.9493			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-00-02-03-00-03.dx		
Sample name:	LDUV 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A6
Injection date:	2022-11-08 12:00:59-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

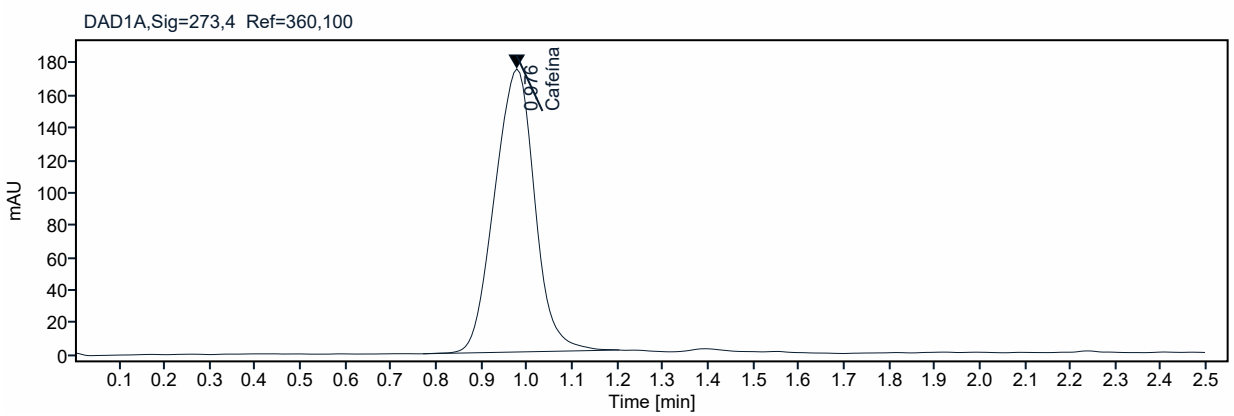

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	1073.3224			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-03-36-03-00-04.dx		
Sample name:	LDUV 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A7
Injection date:	2022-11-08 12:04:33-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

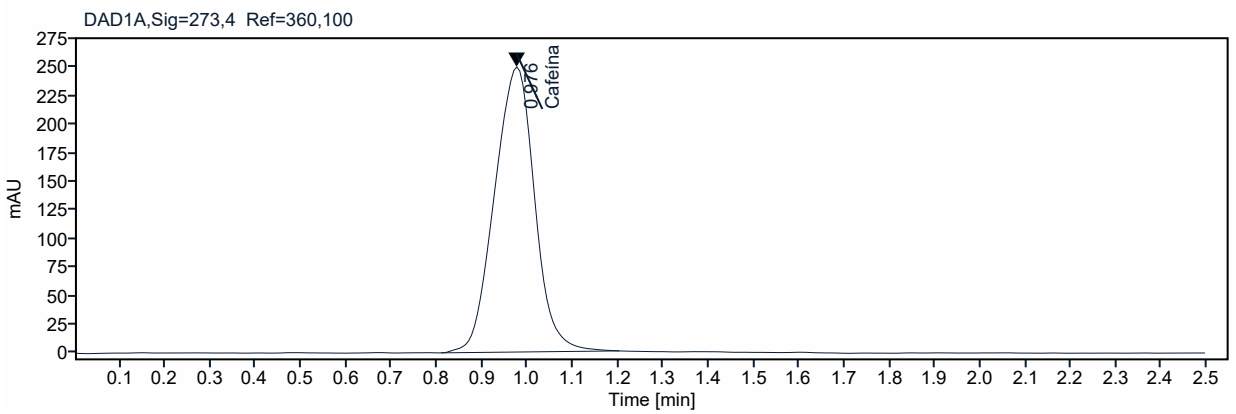

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	1536.4114			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LDUV 01.rslt\2022-11-08 12-07-11-03-00-05.dx		
Sample name:	LDUV 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A8
Injection date:	2022-11-08 12:08:08-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

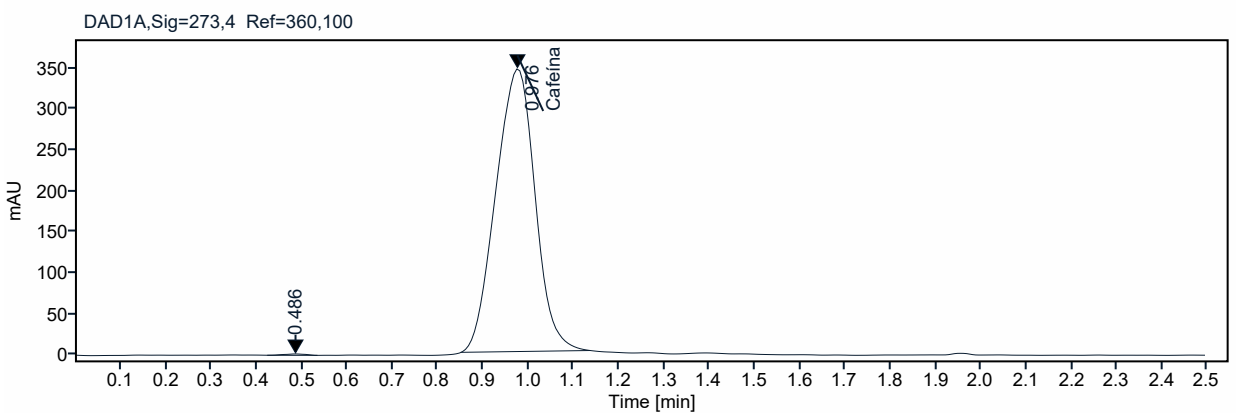

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.976	2081.8125			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LIIN.rslt\2022-11-08 12-55-05-03-00-01.dx		
Sample name:	LIIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A9
Injection date:	2022-11-08 12:55:59-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	0.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

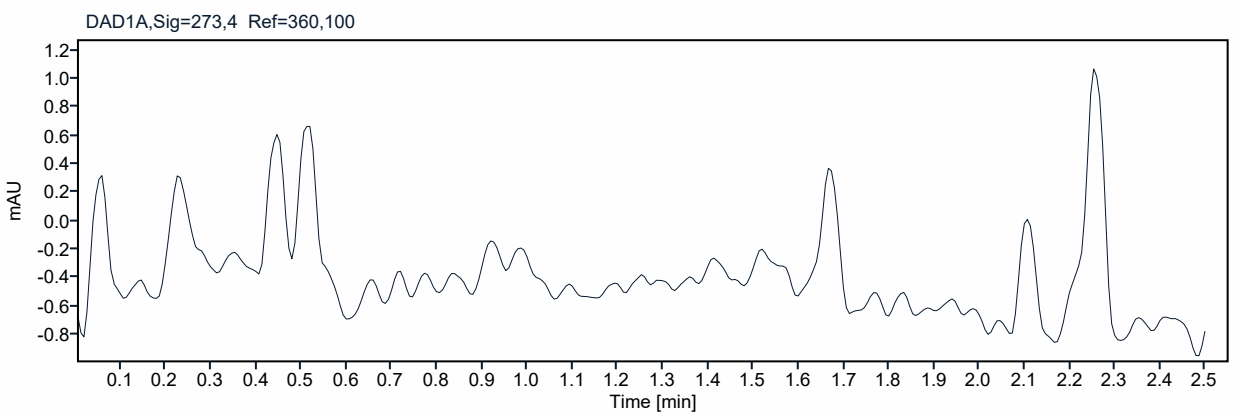

Name	RT [min]	Area	RF	Amount []	Concentration []

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LIIN.rslt\2022-11-08 12-58-35-03-00-02.dx		
Sample name:	LIIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A9
Injection date:	2022-11-08 12:59:27-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	5.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

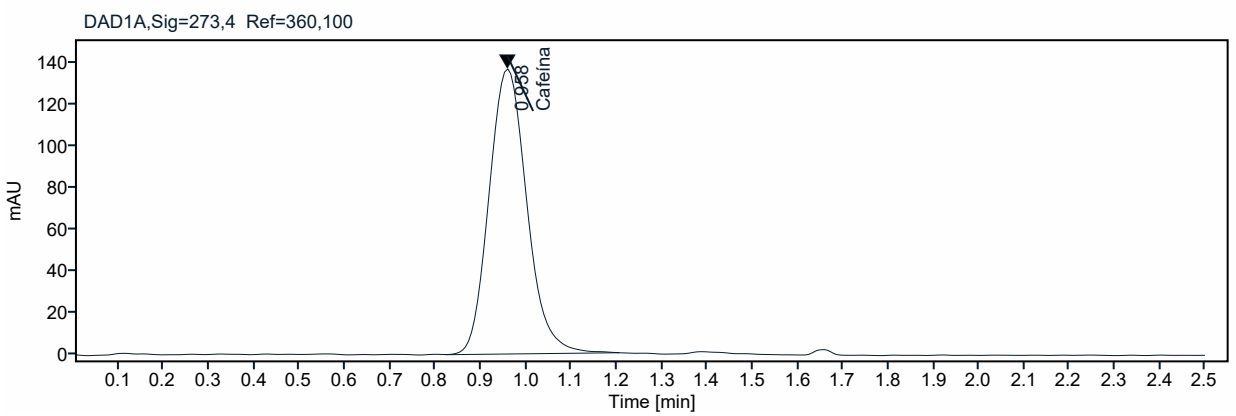

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.958	795.2624			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LIIN.rslt\2022-11-08 13-02-04-03-00-03.dx		
Sample name:	LIIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A9
Injection date:	2022-11-08 13:02:59-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	10.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

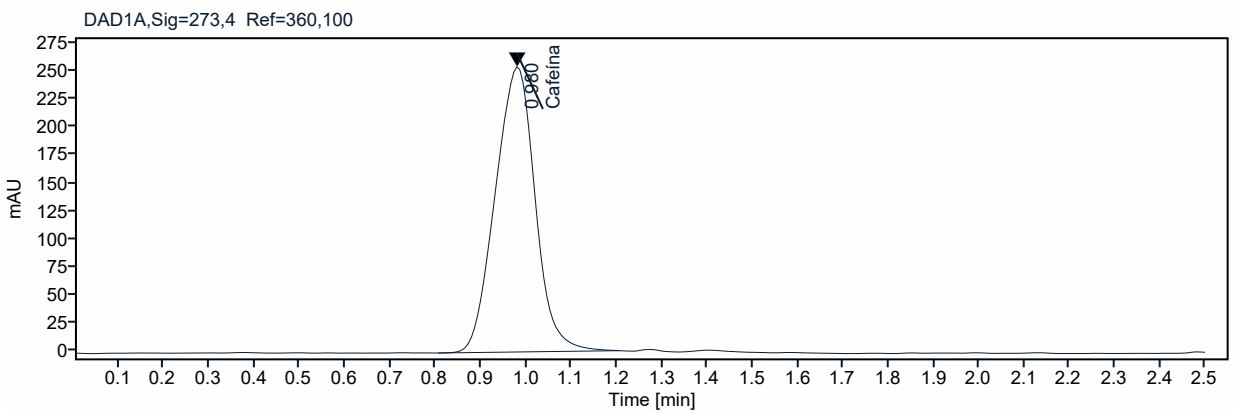

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	0.980	1565.8852			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LIIN.rslt\2022-11-08 13-05-36-03-00-04.dx		
Sample name:	LIIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A9
Injection date:	2022-11-08 13:06:34-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	15.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

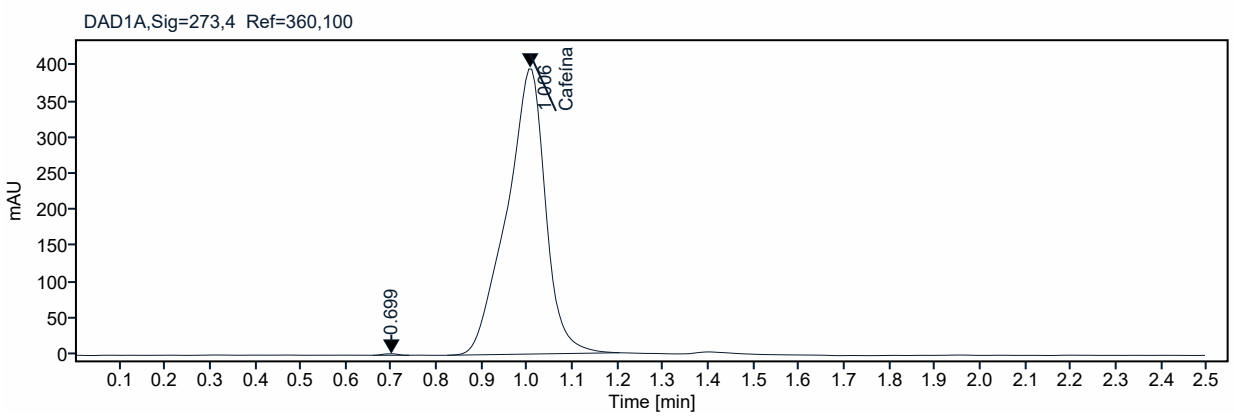

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	1.006	2352.0874			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\LIIN.rslt\2022-11-08 13-09-12-03-00-05.dx		
Sample name:	LIIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A9
Injection date:	2022-11-08 13:10:13-03:00	**Injection:**	1 of 1
Acq. method:	Qualificação.amx	**Injection volume:**	20.000 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 11:50:22-03:00		

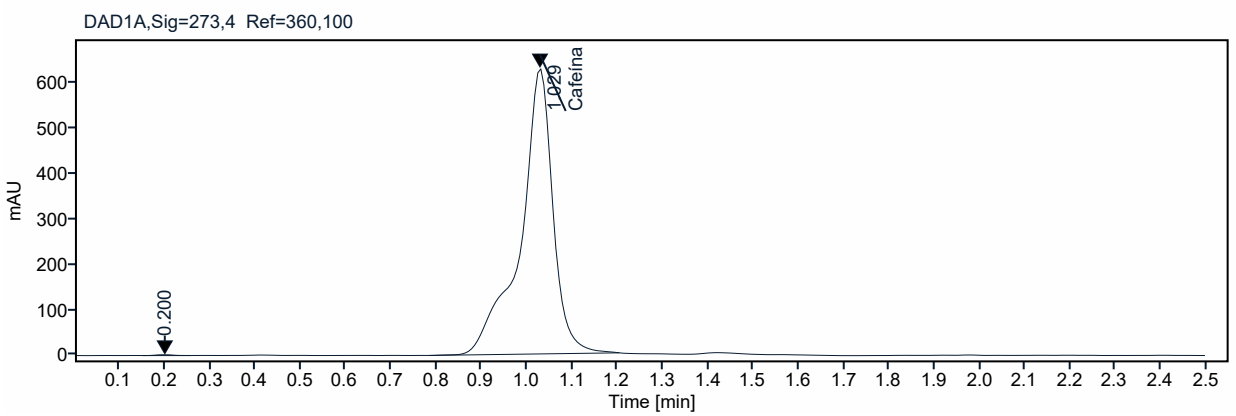

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	1.029	3143.4483			

Single Injection Report


Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\GRAD AB 001.sirslt\GRAD AB 001.dx		
Sample name:	GRAD AB 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A2
Injection date:	2022-11-08 14:18:49-03:00	**Injection:**	1 of 1
Acq. method:	GRAD AB.amx	**Injection volume:**	0.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 14:48:34-03:00		

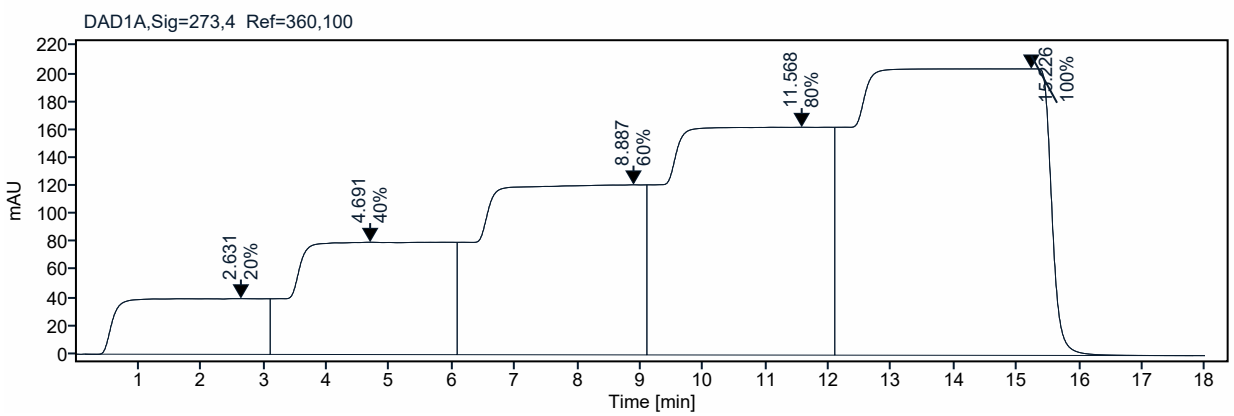

Name	Peak Noise	RT [min]	Area	Peak Height
20%		2.631	5975.4219	39.762
40%		4.691	13145.9010	80.144
60%		8.887	20663.5389	121.385
80%		11.568	28008.0687	162.608
100%		15.226	41463.9547	204.477

Single Injection Report

Data file:	C:\CDSProjects\Agilent\Results\Qualificação 2022\GRAD CD 002.sirslt\GRAD CD 002.dx		
Sample name:	GRAD CD 002		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	CMLI03	**Location:**	P2-A2
Injection date:	2022-11-08 15:03:59-03:00	**Injection:**	1 of 1
Acq. method:	GRAD CD.amx	**Injection volume:**	0.000 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	SYSTEM (SYSTEM)
Last changed:	2022-11-08 15:24:21-03:00		

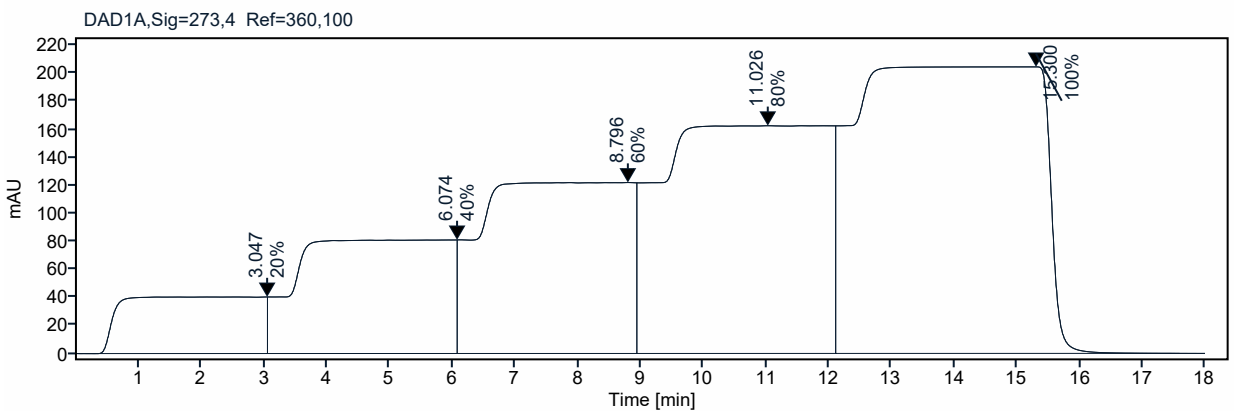

Name	Peak Noise	RT [min]	Area	Peak Height
20%		3.047	5998.7183	40.363
40%		6.074	13404.3471	81.054
60%		8.796	19716.0940	121.983
80%		11.026	29332.5828	162.497
100%		15.300	41310.5720	204.466