
Peak Find - EDUV_001 PDA_2,7100.JWS

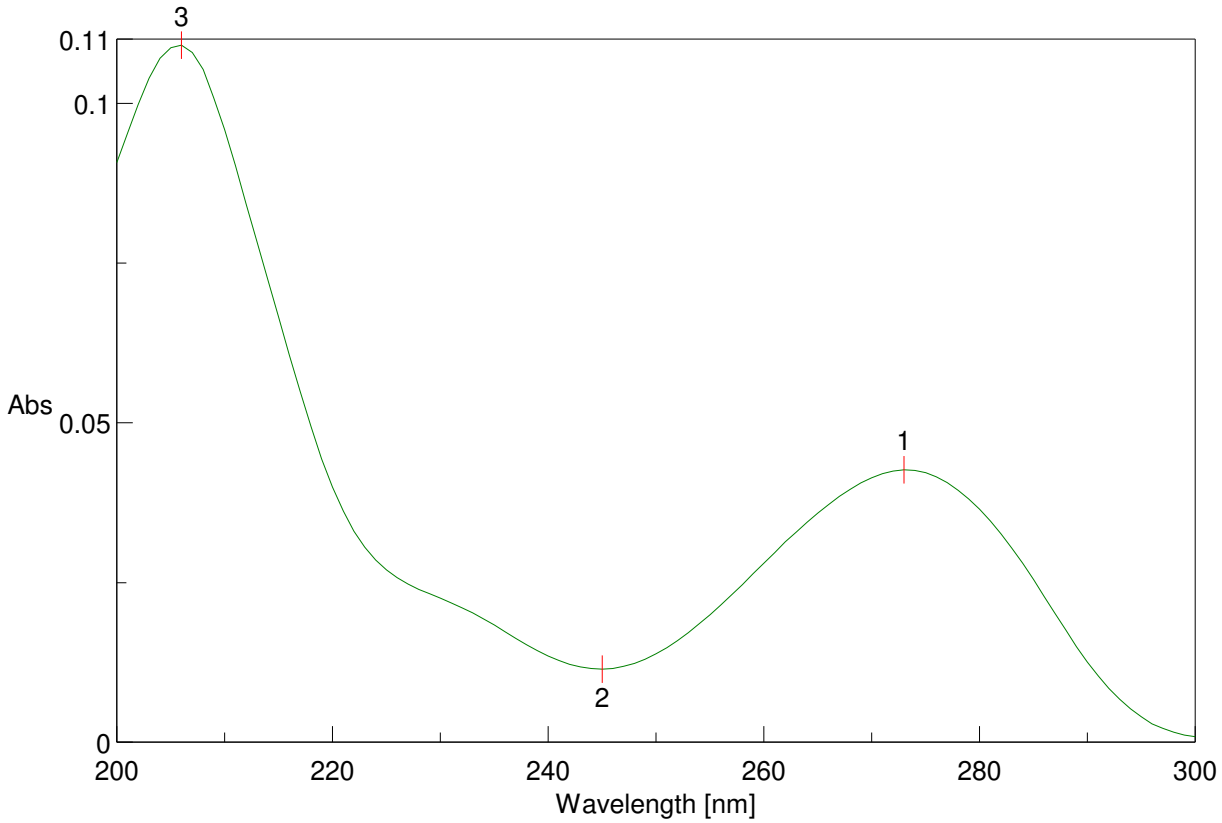

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	03/10/2023 09:43

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A011361665
ROM version	V1.02.14

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.042603	2	245	0.011407
3	206	0.109058			

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 10:22:08
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 10:01:57
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	RELB
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

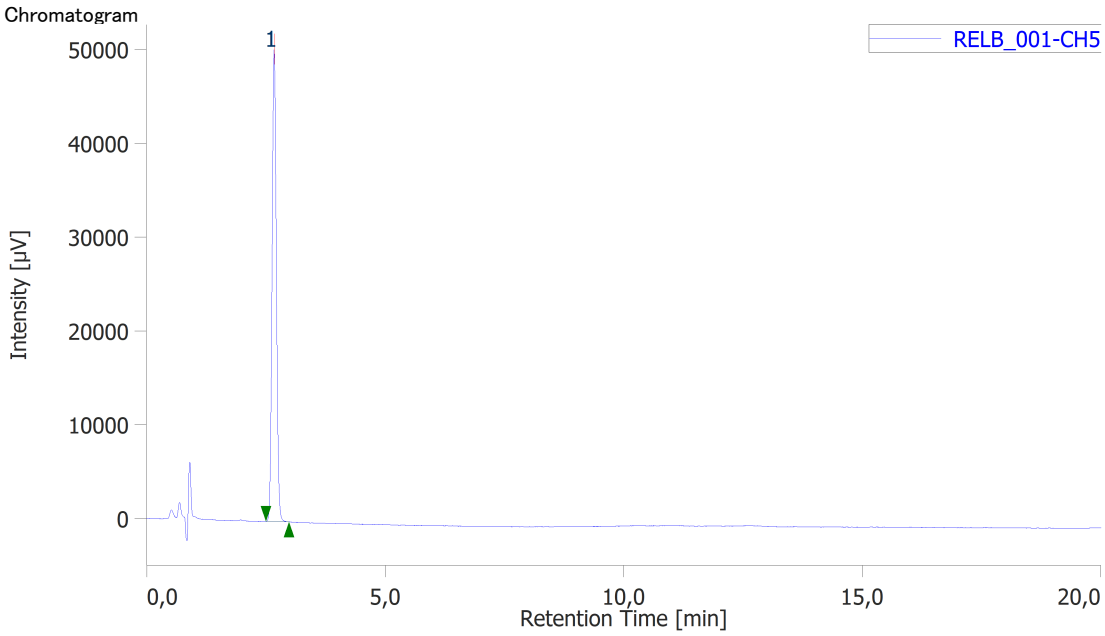


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,673	312772	50358	100,000	100,000	N/A	4313	N/A	1,061	

Creator

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 10:22:08
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 10:01:57
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	RELB
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

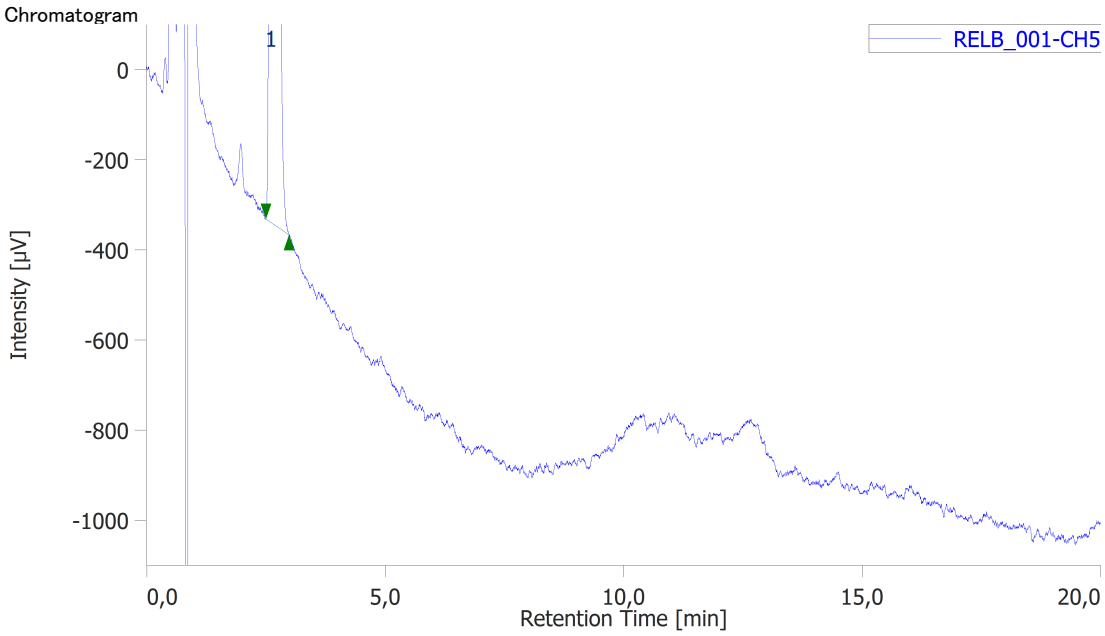


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,673	312772	50358	100,000	100,000	N/A	4313	N/A	1,061	

Creator

Chromatogram

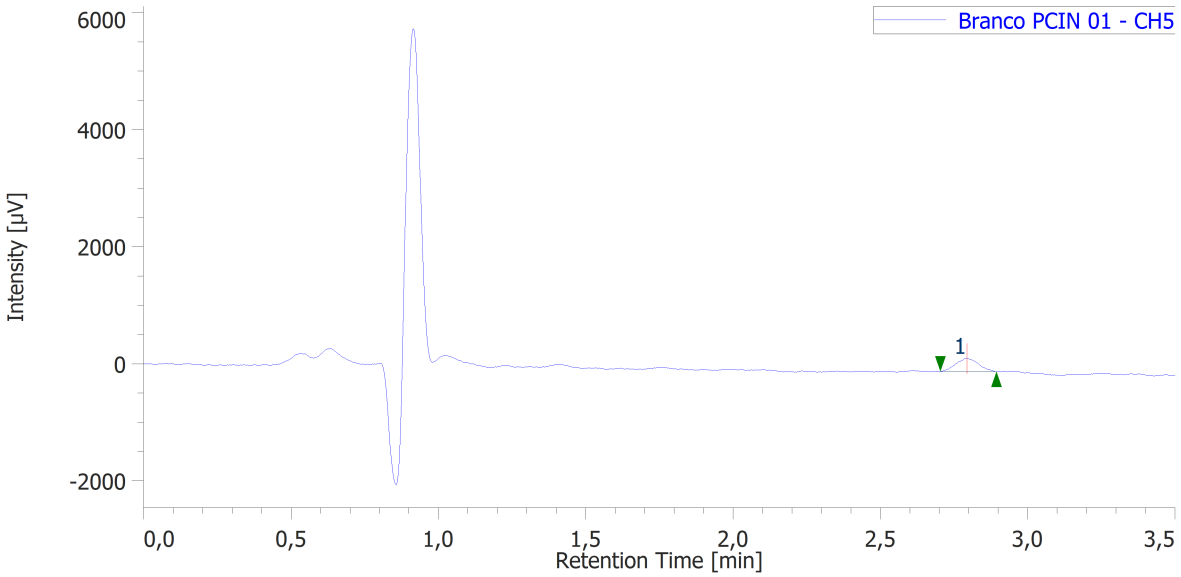

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:15:21
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:11:39
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,793	1198	220	100,000	100,000	N/A	5857	N/A	1,056	

Creator QPackSA


Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:19:16
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:15:34
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

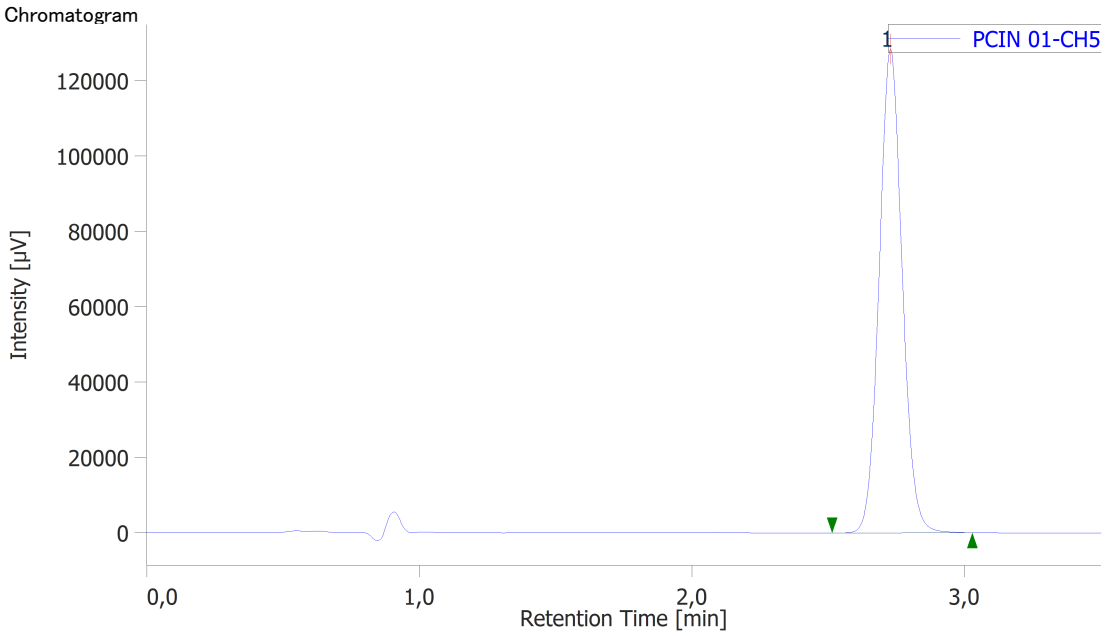

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,727	751675	128374	100,000	100,000	N/A	5138	N/A	1,074	


Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:23:11
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:19:29
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

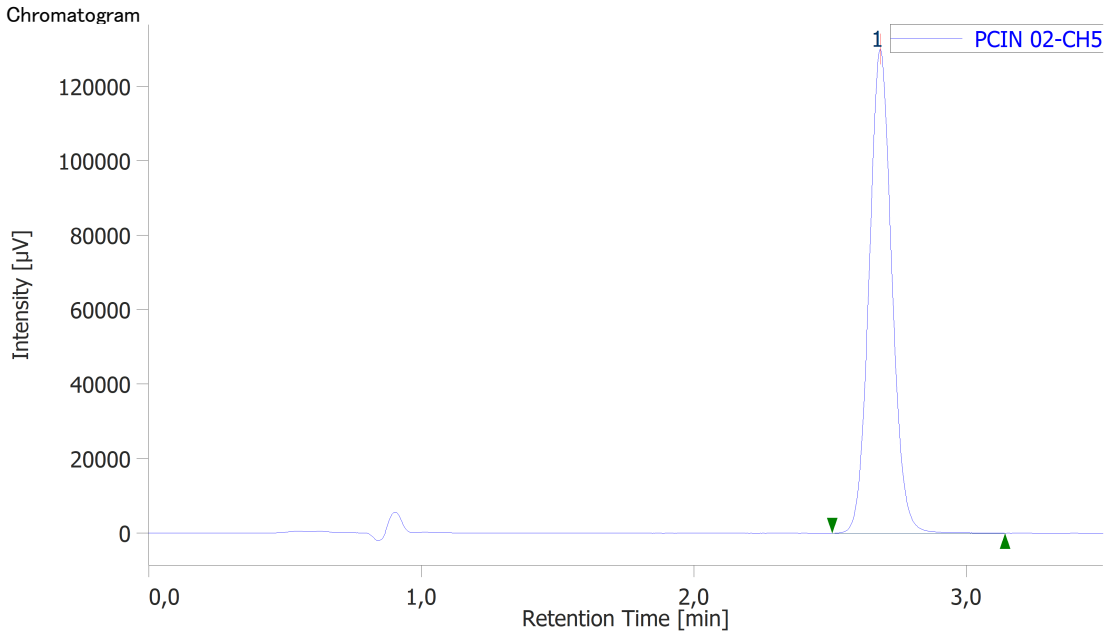

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,683	752795	130034	100,000	100,000	N/A	5108	N/A	1,057	

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:27:06
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:23:24
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

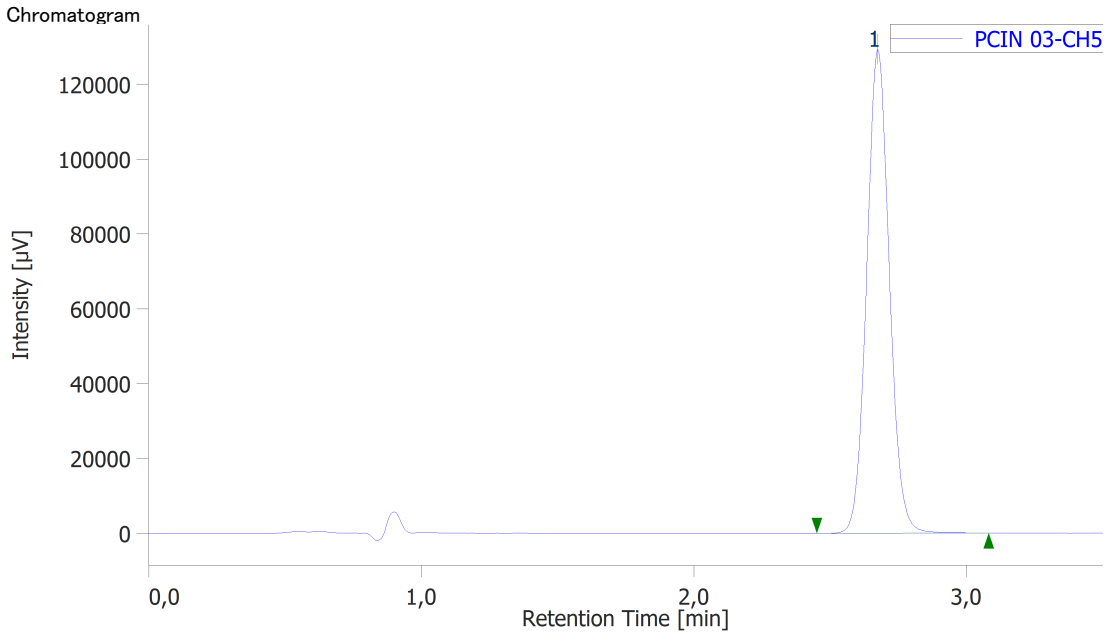


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,673	746351	129344	100,000	100,000	N/A	5093	N/A	1,069	

PCIN Branco PCIN 02 03/10/2023 11:51:11

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:31:01
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:27:19
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

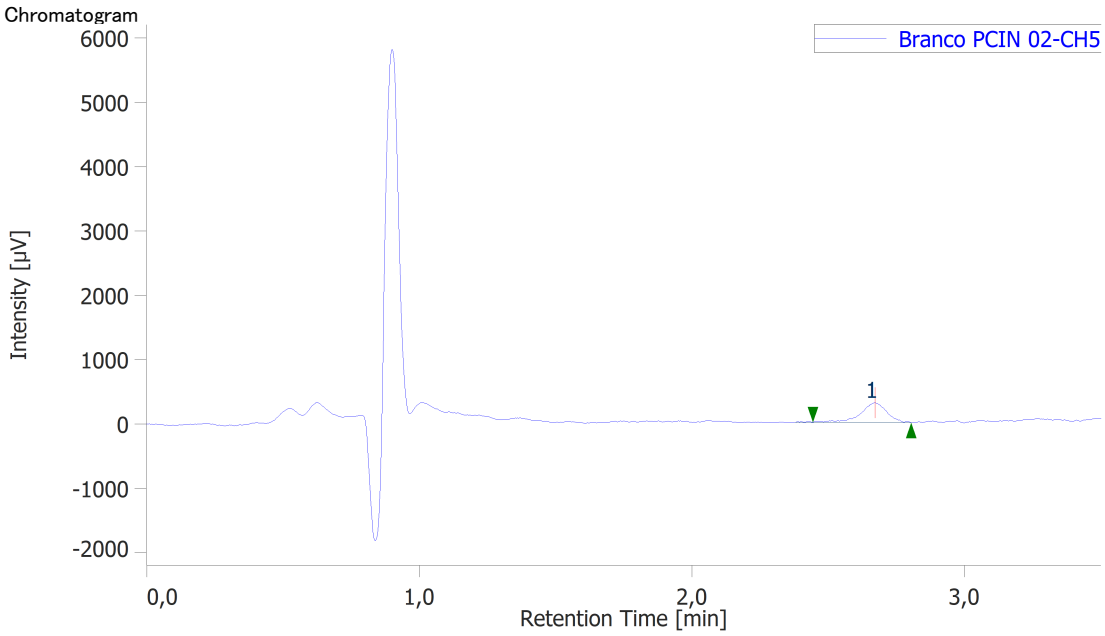


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,670	2119	310	100,000	100,000	N/A	4441	N/A	0,794	

Creator QPackSA

Chromatogram Information


User Name	QPackSA
Date Modified	03/10/2023 11:34:56
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:31:14
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

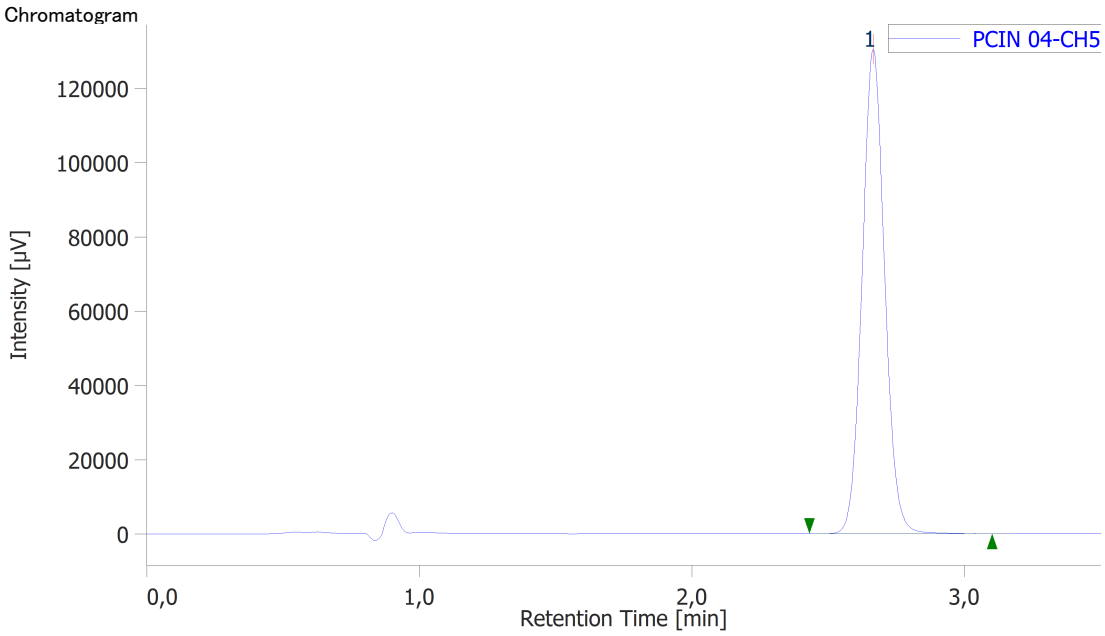

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,663	747394	130439	100,000	100,000	N/A	5129	N/A	1,072	


Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:38:51
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:35:09
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

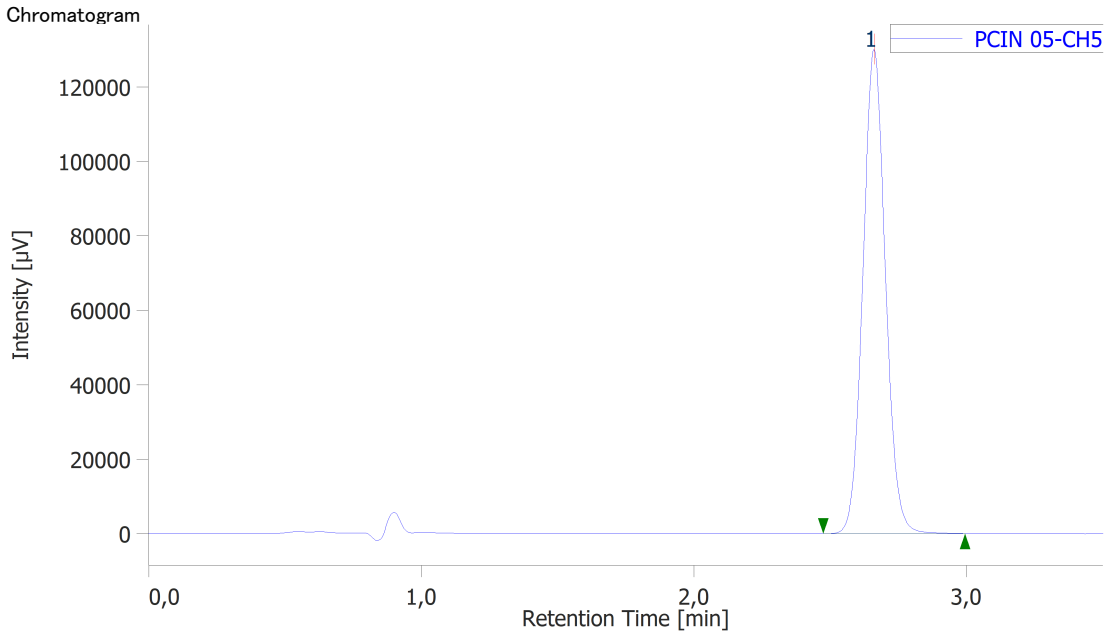

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,660	744488	130097	100,000	100,000	N/A	5121	N/A	1,059	

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:42:46
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:39:04
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

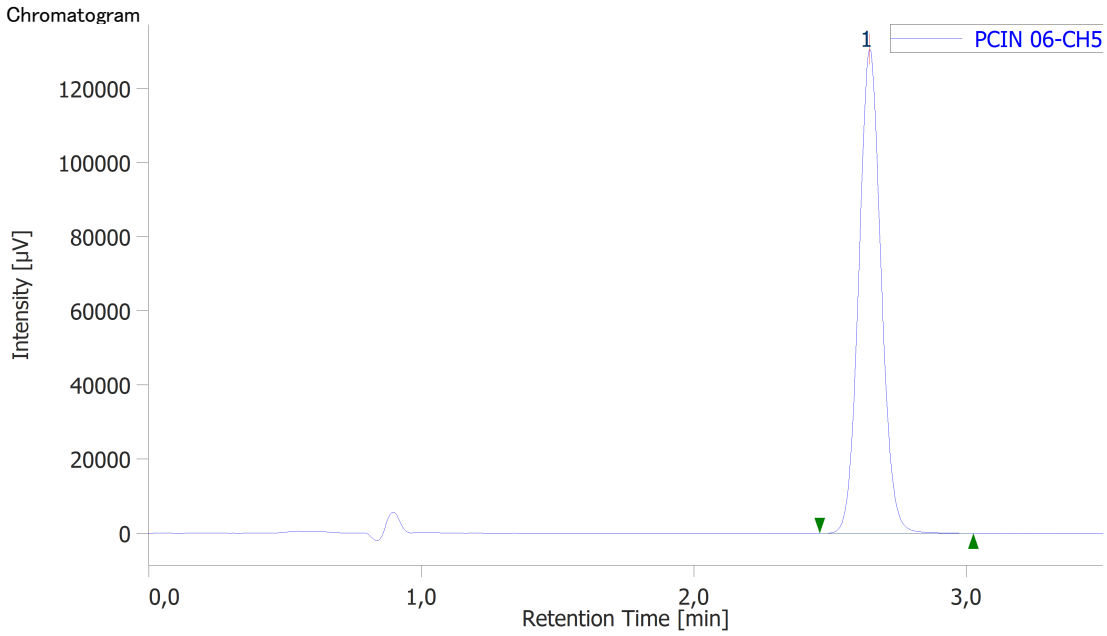


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,643	742196	130618	100,000	100,000	N/A	5117	N/A	1,071	

PCIN Branco PCIN 03 03/10/2023 11:53:10

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:46:40
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:42:58
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

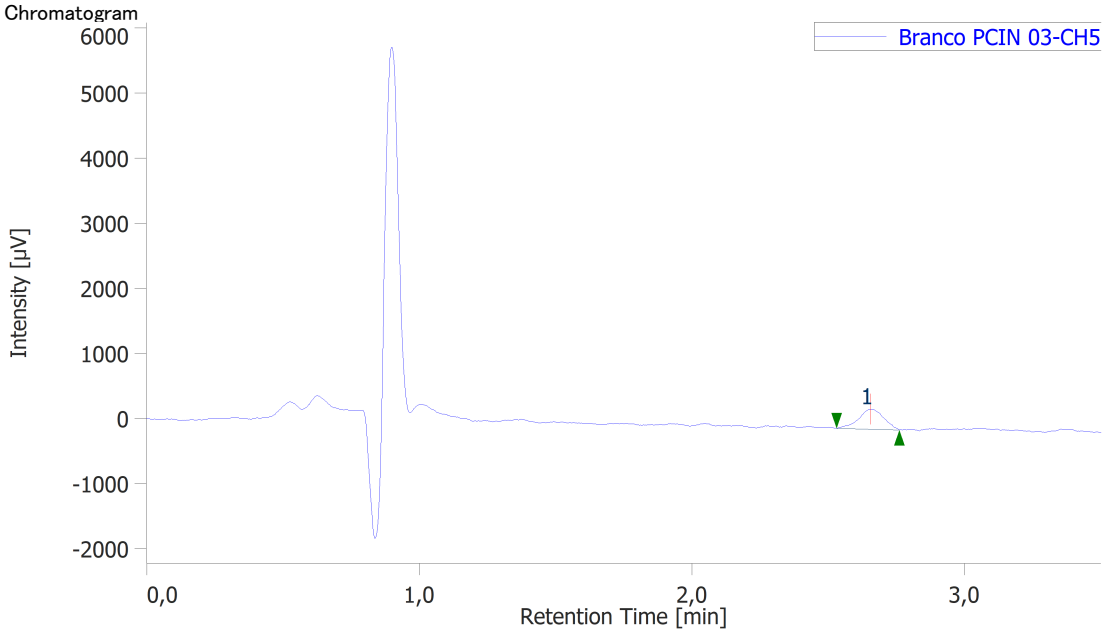


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,653	1965	308	100,000	100,000	N/A	4127	N/A	0,956	

Creator QPackSA


LDUV LDUV 01 03/10/2023 12:16:46

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:54:34
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:50:52
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

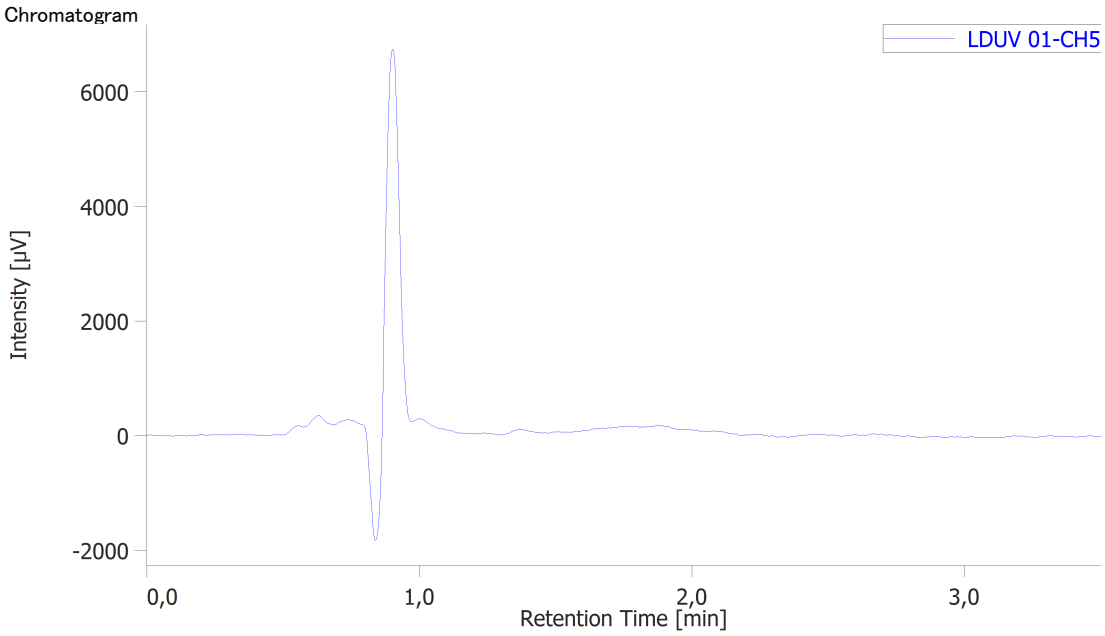

Peak Information – No data.


Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 11:58:27
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:54:46
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

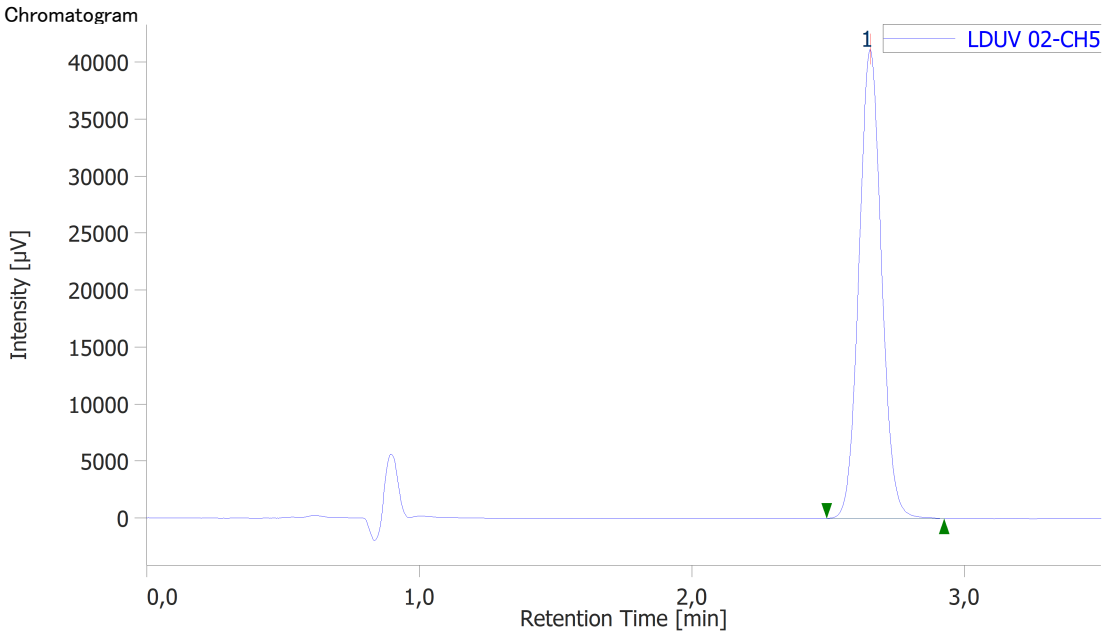

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,653	236490	41161	100,000	100,000	N/A	5003	N/A	1,049	

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:02:22
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 11:58:40
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

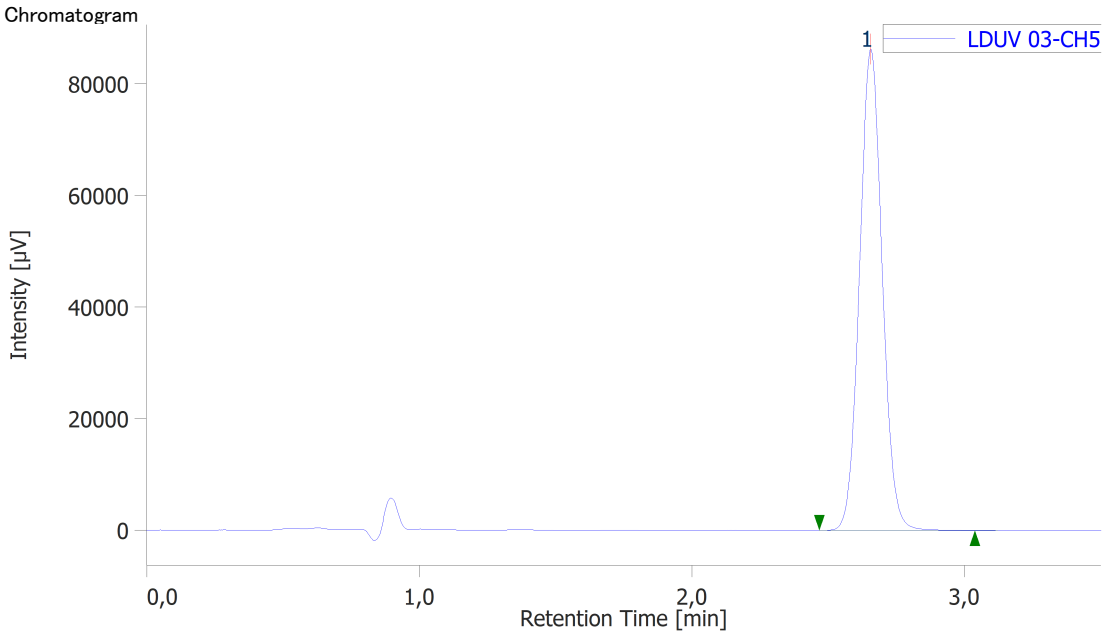


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,653	498986	86258	100,000	100,000	N/A	4964	N/A	1,074	

LDUV LDUV 04 03/10/2023 12:18:48

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:06:17
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:02:35
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

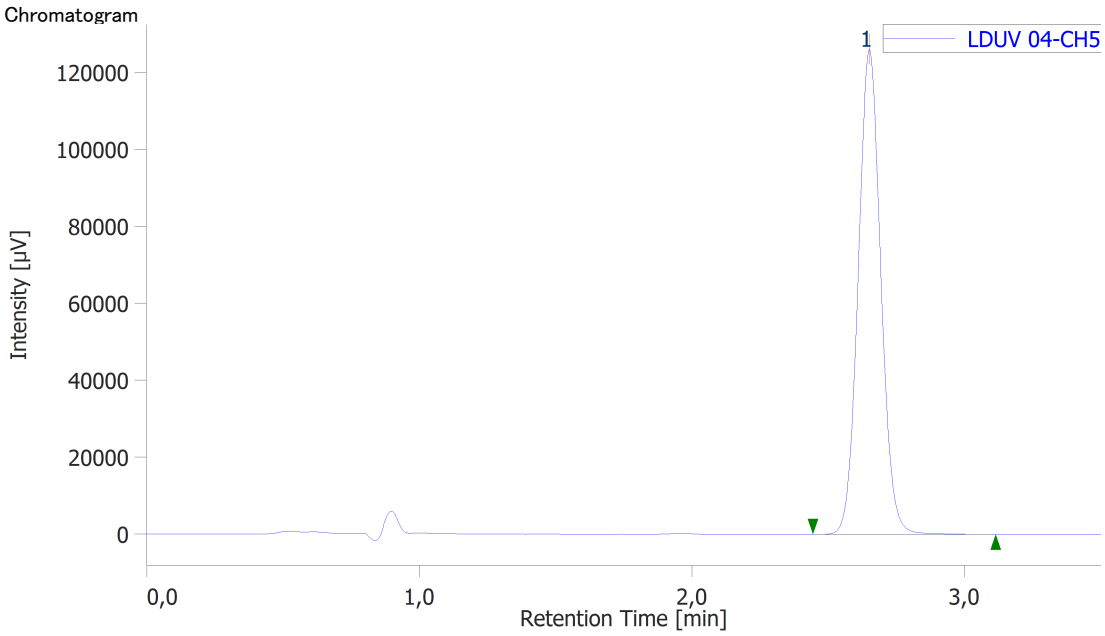


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,650	726324	126124	100,000	100,000	N/A	5017	N/A	1,055	

Creator QPackSA

Chromatogram Information

User Name	QPackSA
Date Modified	03/10/2023 12:10:10
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:06:28
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

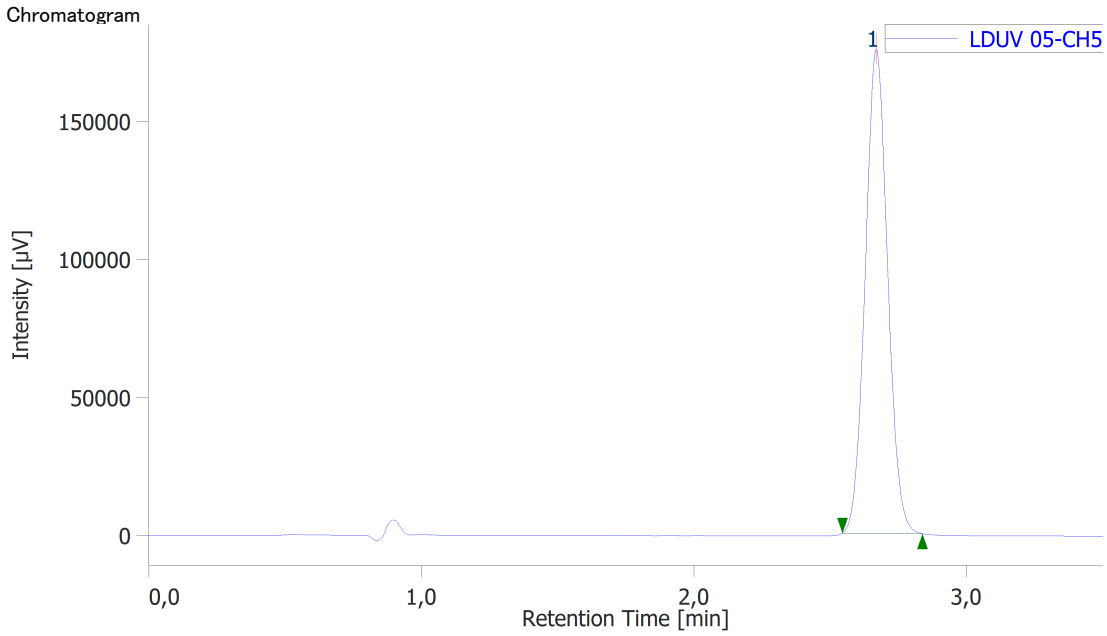


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,667	996668	175339	100,000	100,000	N/A	5109	N/A	1,069	

LIIN LIIN 01 03/10/2023 13:25:33

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:23:05
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:19:23
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

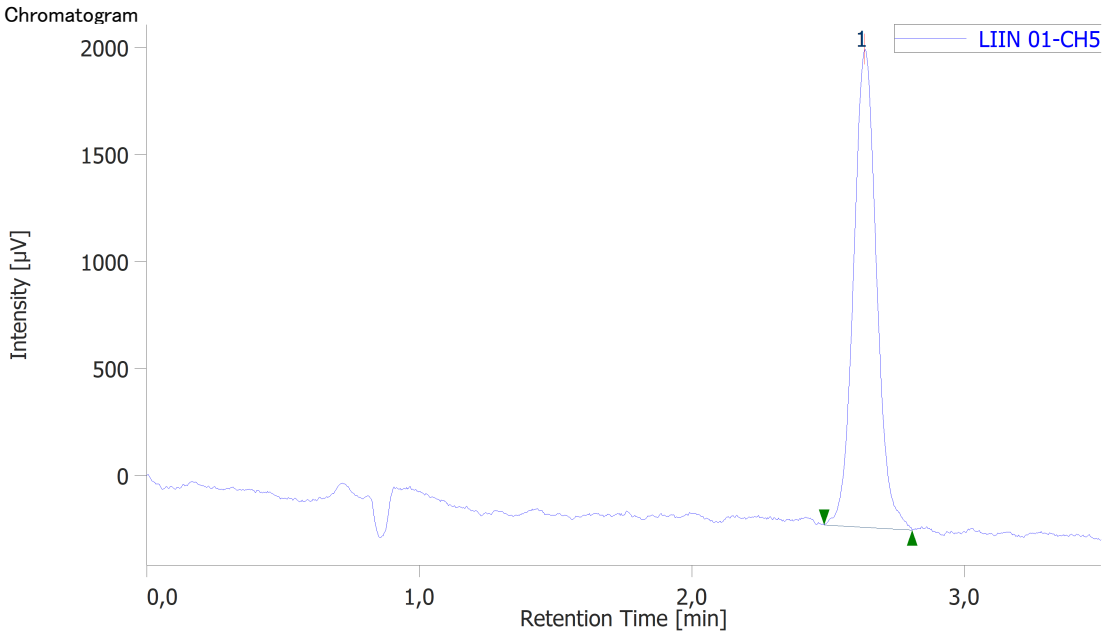

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,633	13083	2234	100,000	100,000	N/A	4857	N/A	1,059	

Creator QPackSA

LIIN LIIN 02 03/10/2023 13:26:06

Chromatogram Information

User Name	QPackSA
Date Modified	03/10/2023 12:26:47
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:23:05
Volume	5,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

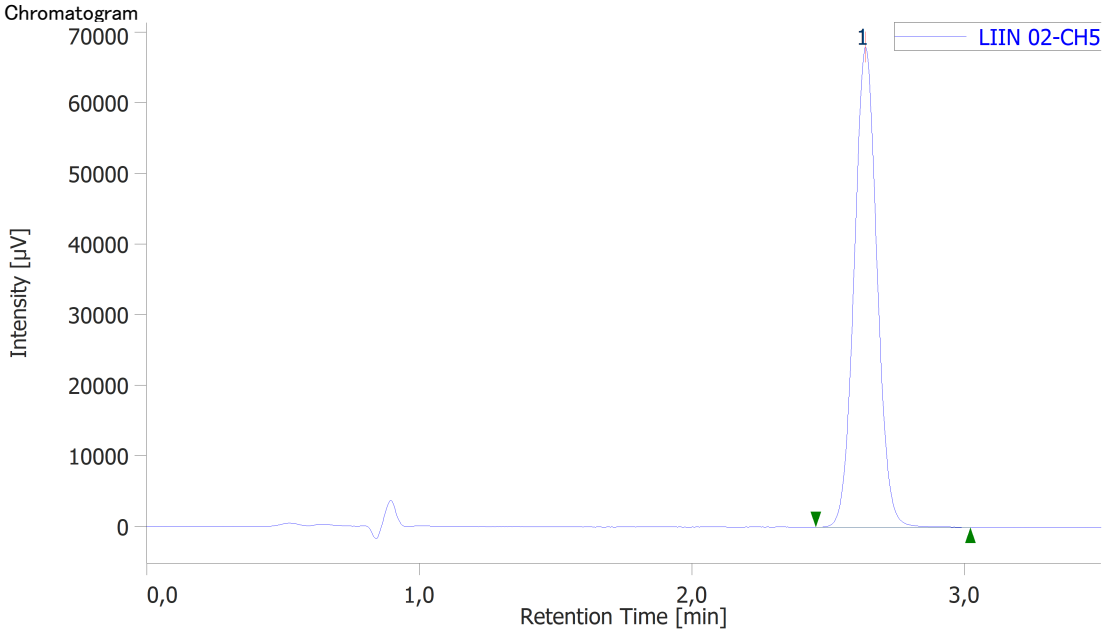


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,637	395497	67978	100,000	100,000	N/A	4818	N/A	1,032	

Creator QPackSA

LIIN LIIN 03 03/10/2023 13:26:33

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:30:40
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:26:58
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

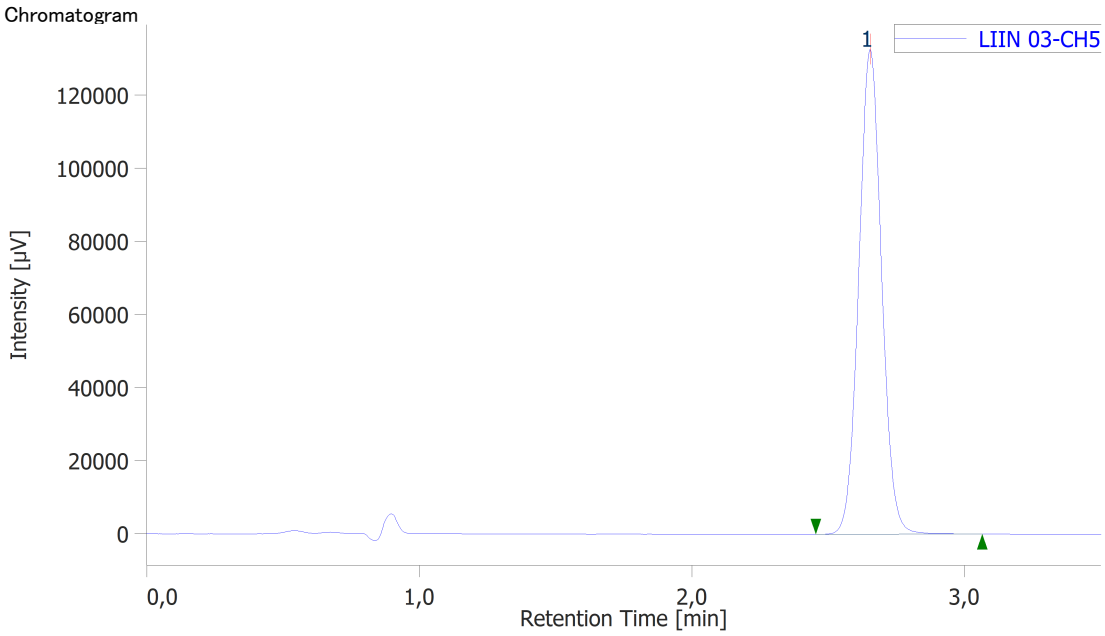


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,653	769422	132598	100,000	100,000	N/A	4926	N/A	1,035	

Creator QPackSA

LIIN LIIN 04 03/10/2023 13:27:02

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:34:48
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:31:06
Volume	15,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

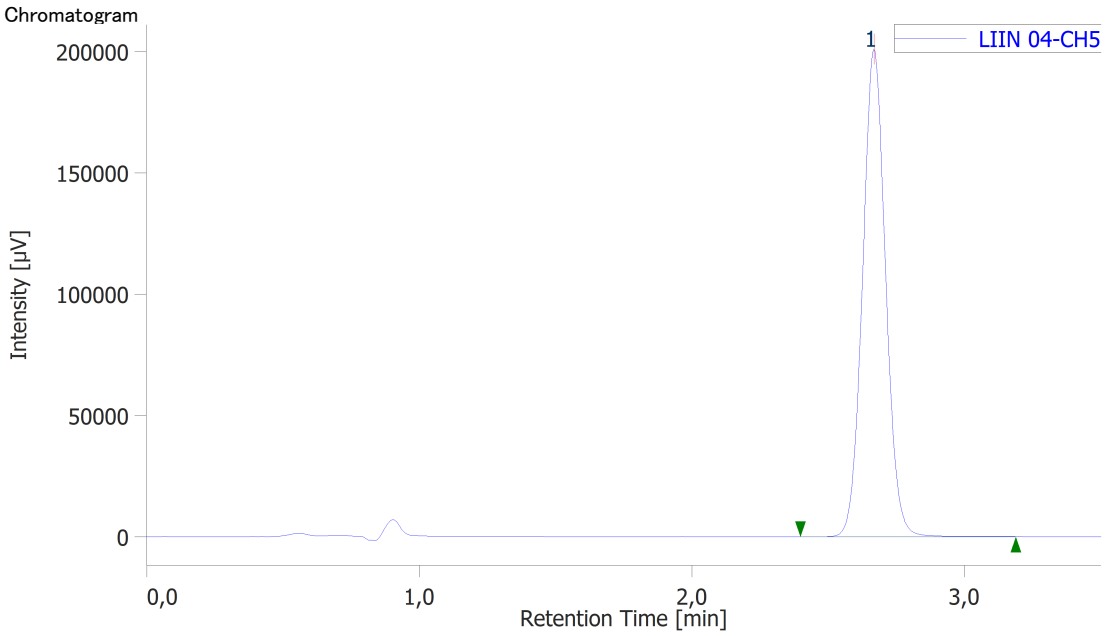


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,667	1178718	200939	100,000	100,000	N/A	4903	N/A	1,048	

Creator QPackSA

LIIN LIIN 05 03/10/2023 13:27:33

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 12:39:13
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 12:35:31
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação Cafeína
Calibration Method	
Additional Information	
Column Info	

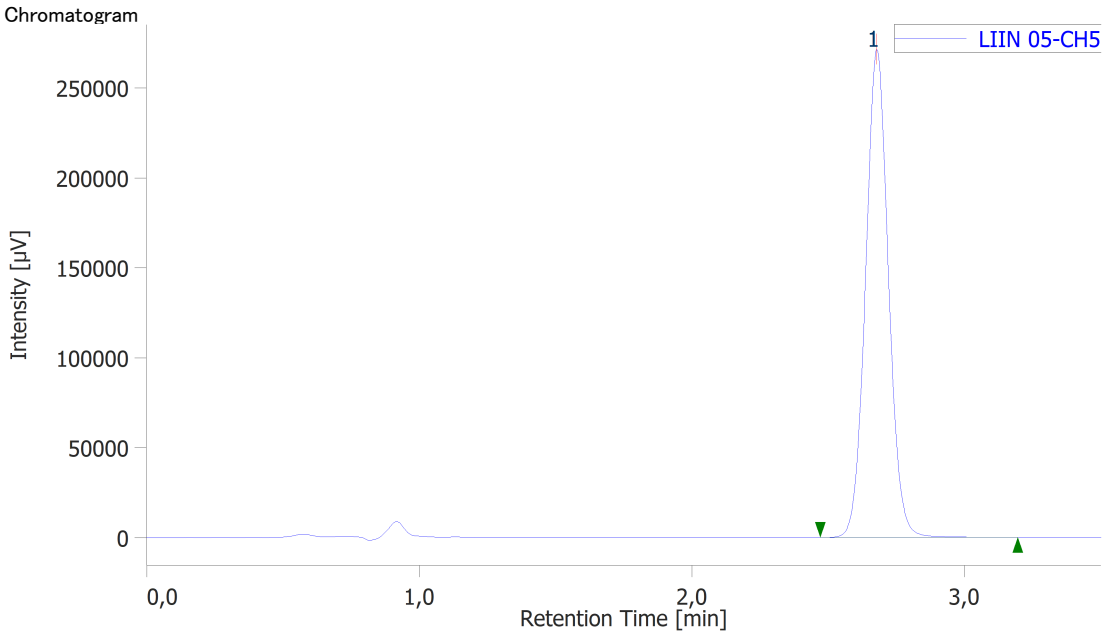


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,677	1579828	271399	100,000	100,000	N/A	5045	N/A	1,056	

Creator QPackSA


Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 14:56:59
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 14:38:47
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	GRAD AB
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

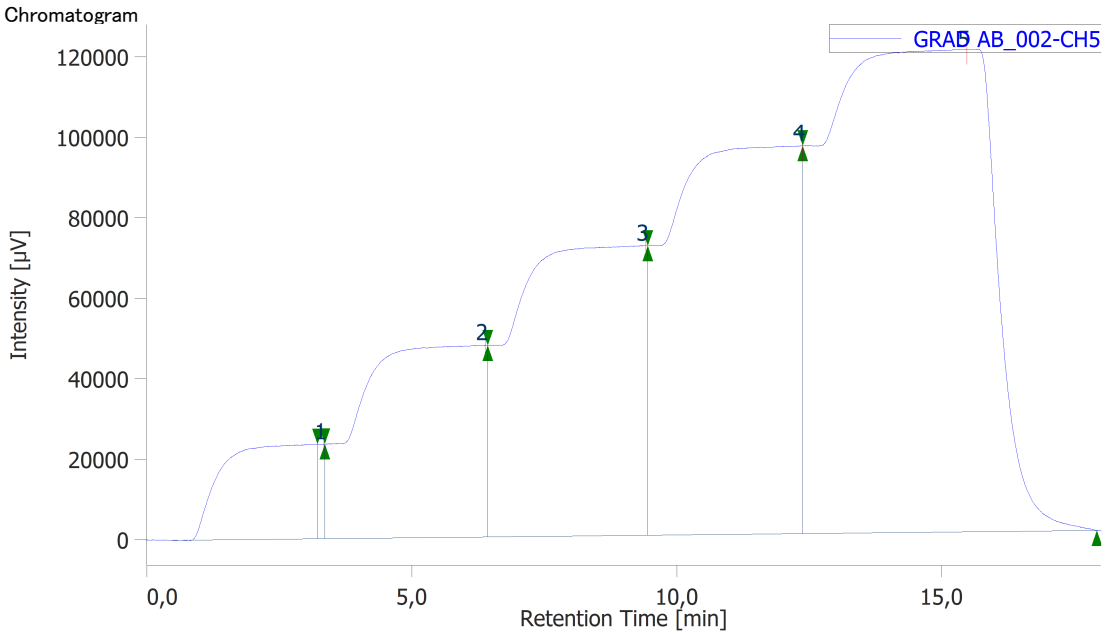

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,340	197066	23432	0,320	6,525	N/A	N/A	N/A	N/A	
2	Unknown	5	6,383	7602766	47597	12,335	13,255	N/A	N/A	N/A	N/A	
3	Unknown	5	9,413	11945515	71901	19,381	20,023	N/A	N/A	N/A	N/A	
4	Unknown	5	12,363	15821503	96316	25,669	26,822	N/A	N/A	N/A	N/A	
5	Unknown	5	15,467	26069337	119842	42,296	33,374	N/A	N/A	N/A	N/A	

Chromatogram Information	
User Name	QPackSA
Date Modified	03/10/2023 15:42:03
Description	
HPLC System Name	HPL 19
Injection Date	03/10/2023 15:23:51
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	GRAD AC
Peak ID Table	
Calibration Method	
Additional Information	
Column Info	

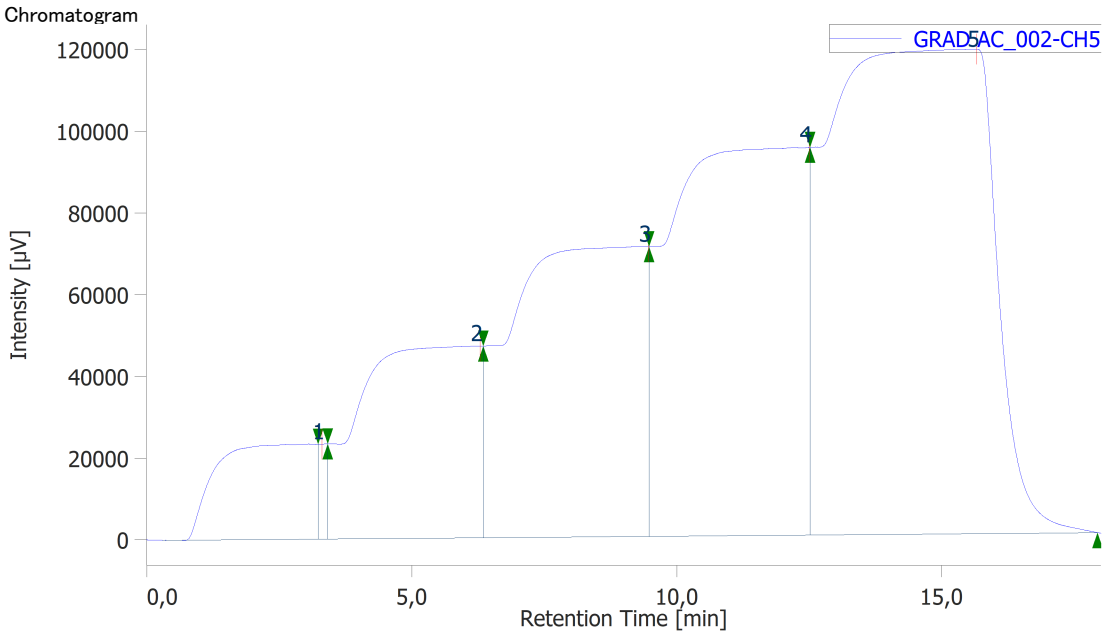

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,307	250608	23193	0,412	6,546	N/A	N/A	N/A	N/A	
2	Unknown	5	6,287	7213896	46905	11,858	13,238	N/A	N/A	N/A	N/A	
3	Unknown	5	9,463	12147418	70869	19,968	20,002	N/A	N/A	N/A	N/A	
4	Unknown	5	12,493	16261827	94812	26,731	26,759	N/A	N/A	N/A	N/A	
5	Unknown	5	15,650	24961538	118537	41,031	33,455	N/A	N/A	N/A	N/A	