
Chromatogram

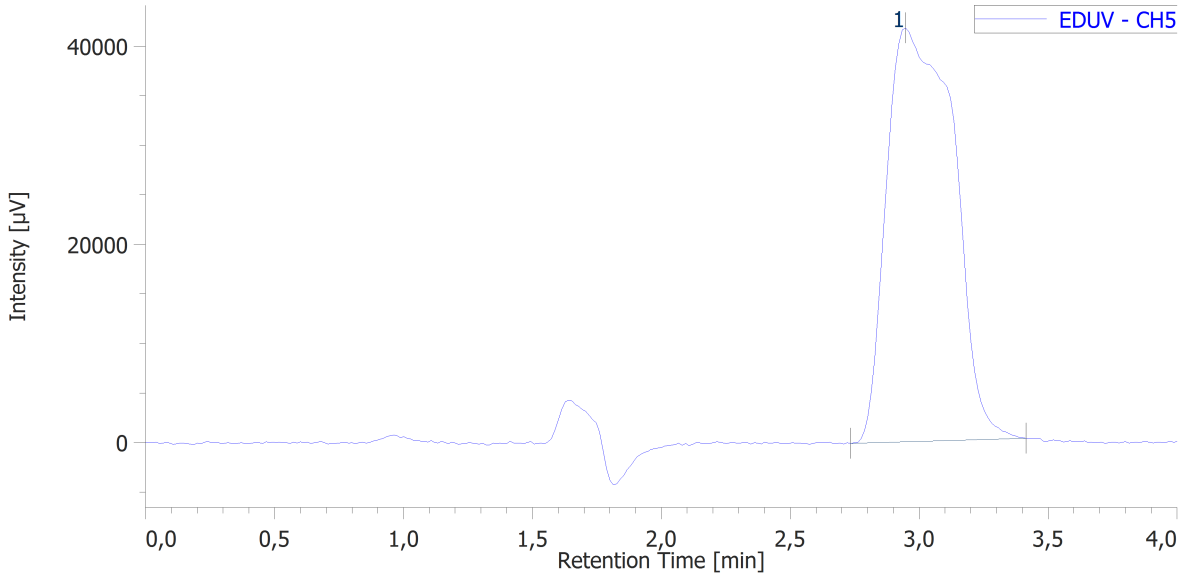

Chromatogram Information	
User Name	QPackSA
Date Modified	09/10/2023 16:03:39
Description	
HPLC System Name	HPL25
Injection Date	09/10/2023 15:59:38
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	EDUV-CH5
Sample Name	EDUV
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,947	755271	41747	100,000	100,000	N/A	508	N/A	1,560	

Creator
Reviewer
Approver

Peak Find - EDUV PDA_2,9333.JWS

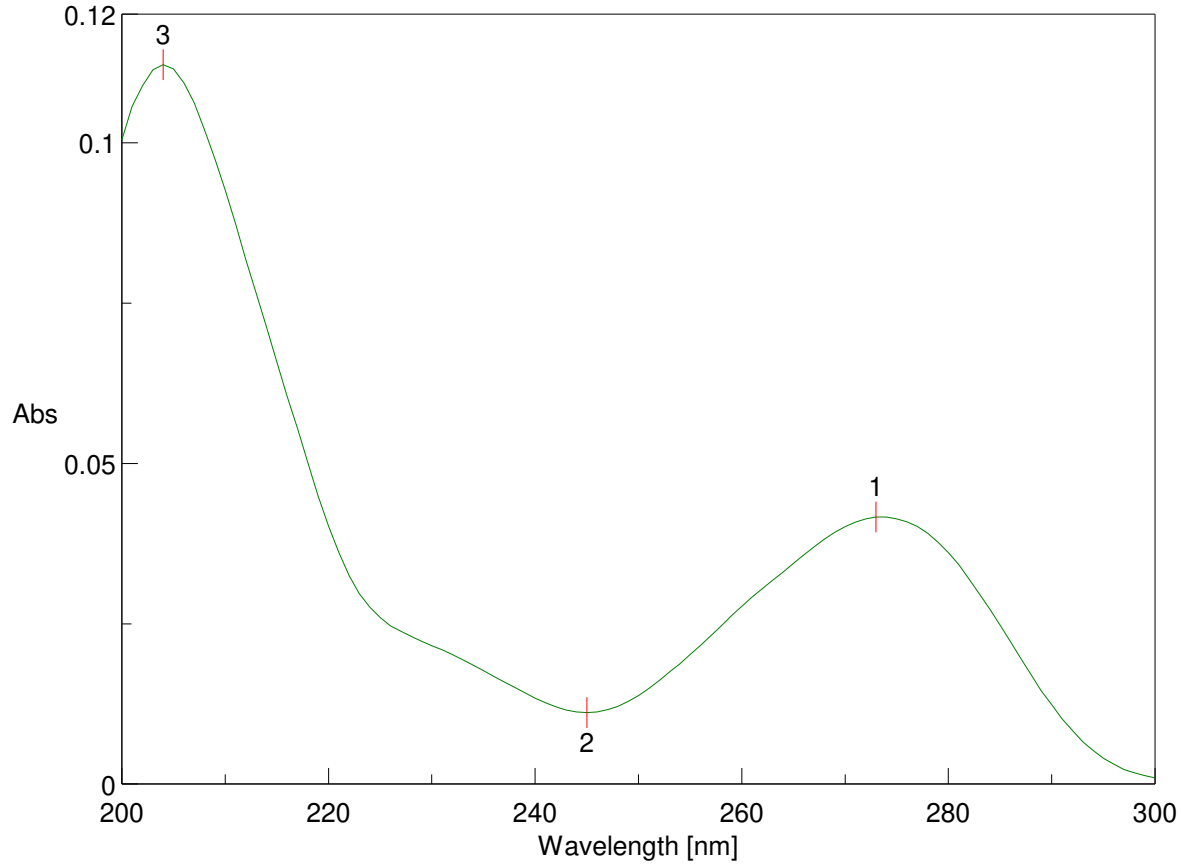

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	09/10/2023 15:59
Date modified	10/10/2023 10:24

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	072260870
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.041635	2	245	0.011144
3	204	0.112127			

Chromatogram

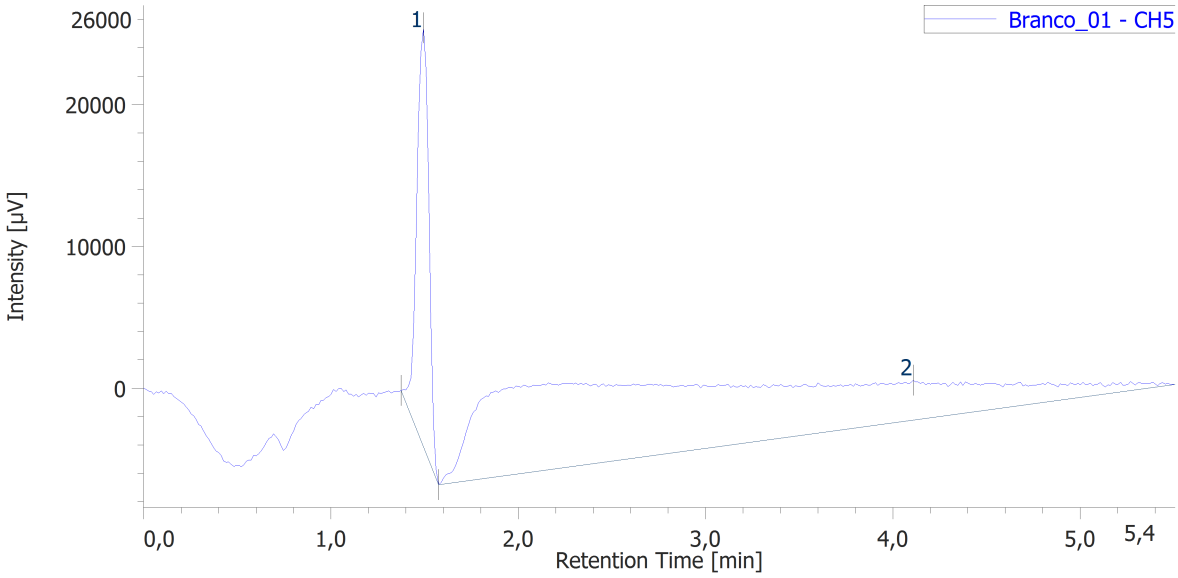

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 13:55:36
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 13:50:03
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	Branco_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,493	132460	29509	14,799	91,324	N/A	2394	0,992	0,878	
2	Unknown	5	4,107	762623	2803	85,201	8,676	N/A	10	N/A	0,771	

Creator QPackSA
Reviewer
Approver

Chromatogram

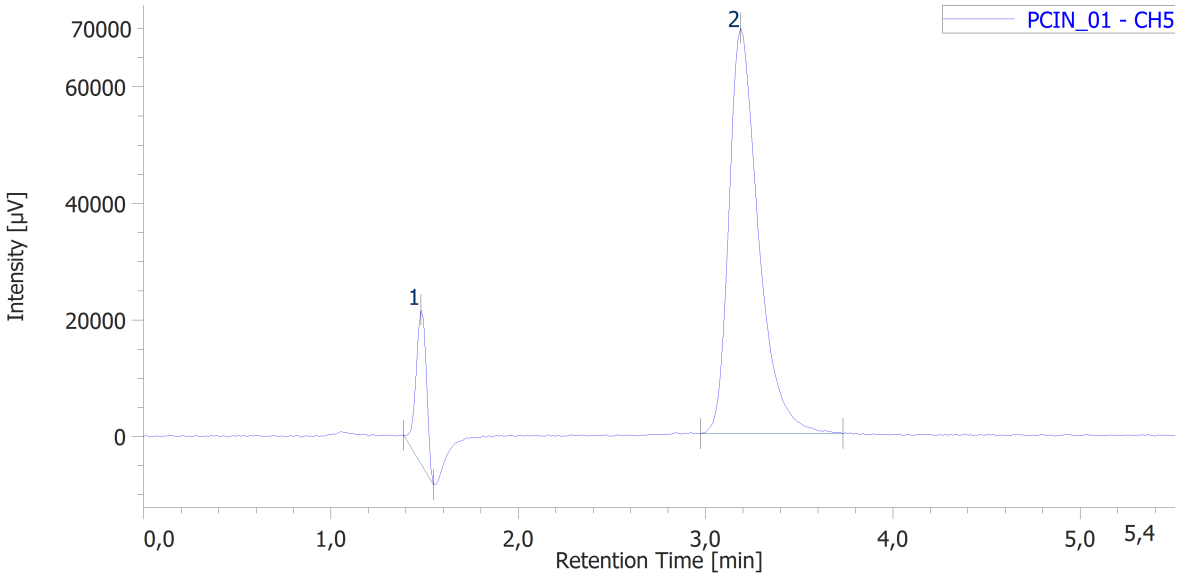

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:01:18
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 13:55:45
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	PCIN_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	102632	26467	11,887	27,551	N/A	3212	9,072	0,919	
2	Cafeína	5	3,187	760759	69600	88,113	72,449	N/A	2183	N/A	1,474	

Creator
Reviewer
Approver

Chromatogram

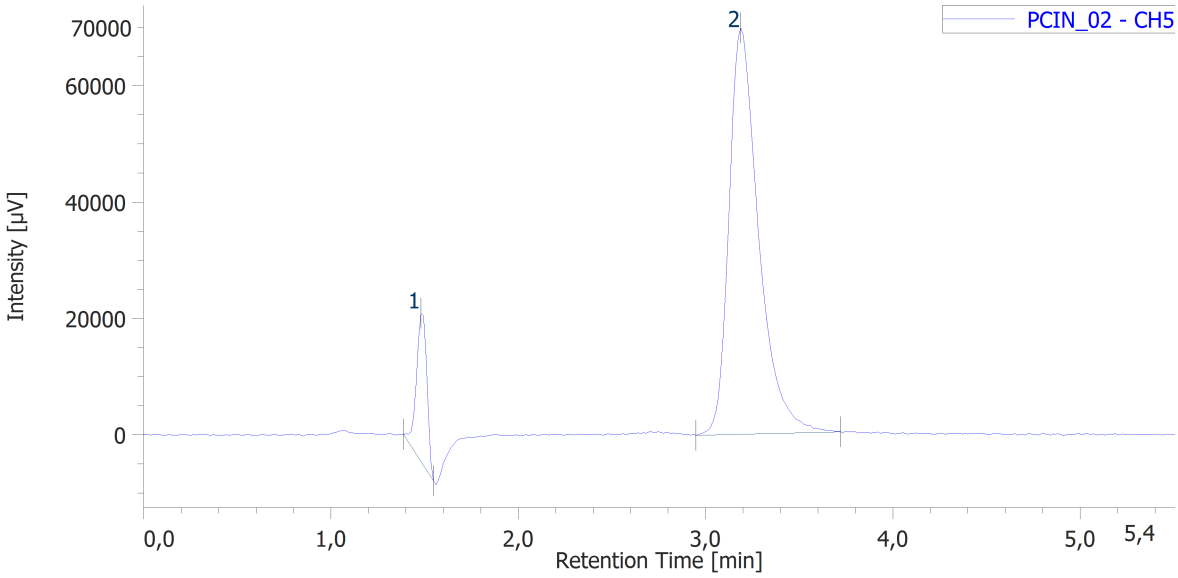

Chromatogram Information

User Name	QPackSA
Date Modified	10/10/2023 14:10:27
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:01:28
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	PCIN_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	99784	25471	11,498	26,743	N/A	3250	9,072	0,937	
2	Cafeína	5	3,187	768049	69774	88,502	73,257	N/A	2174	N/A	1,479	

Creator QPackSA
Reviewer
Approver

Chromatogram

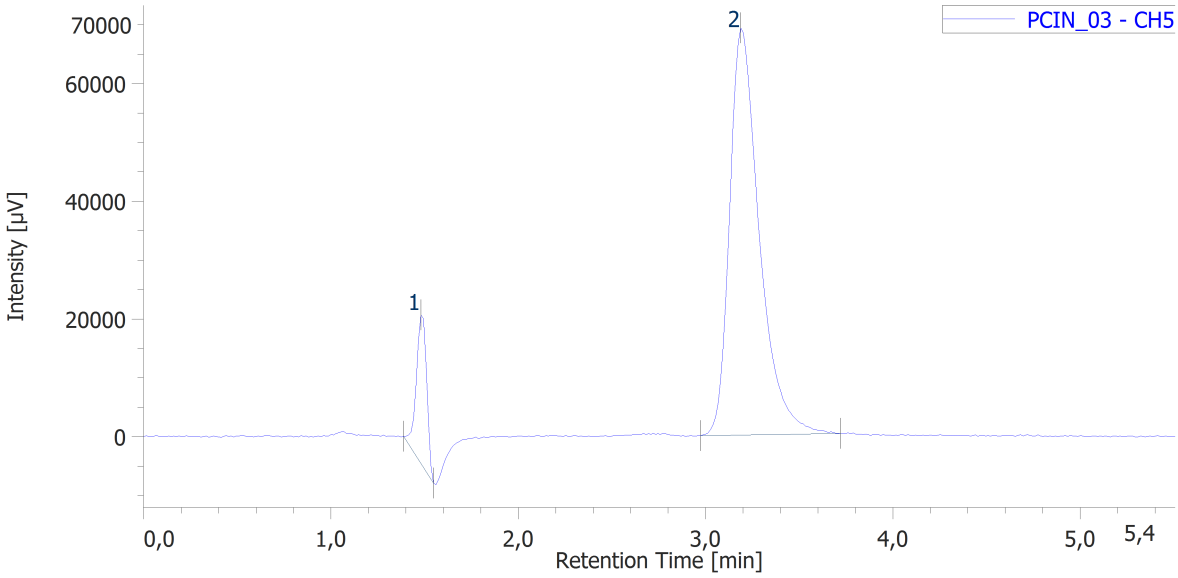

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:12:42
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:07:10
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH5
Sample Name	PCIN_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	98416	25278	11,444	26,773	N/A	3305	9,056	0,920	
2	Cafeína	5	3,187	761600	69140	88,556	73,227	N/A	2150	N/A	1,522	

Creator
Reviewer
Approver

Chromatogram

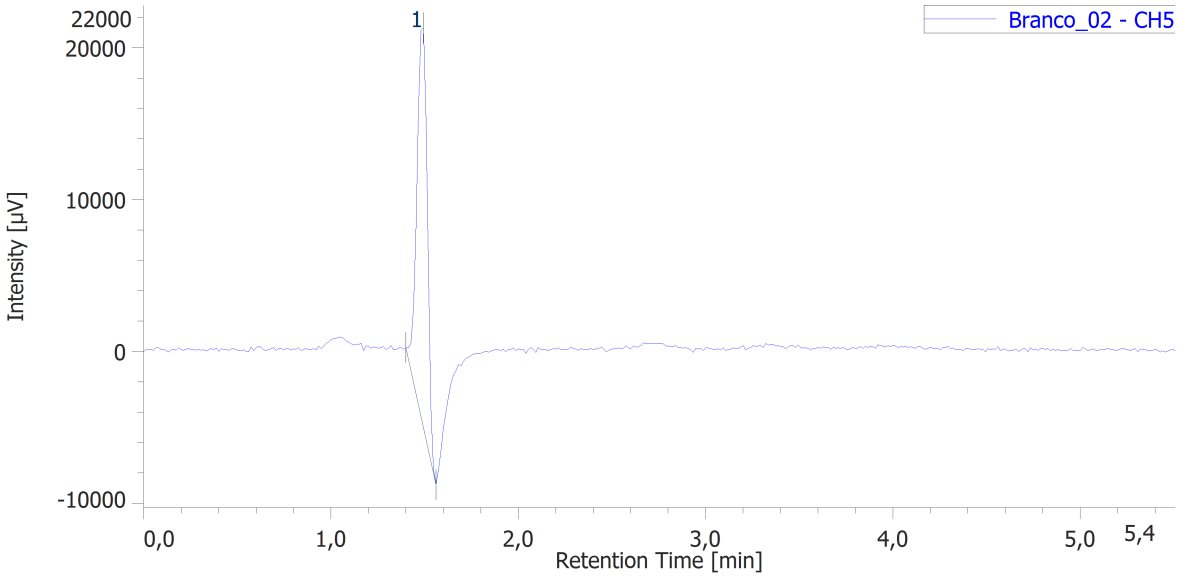

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:18:26
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:12:53
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_02-CH5
Sample Name	Branco_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,493	100592	26296	100,000	100,000	N/A	3339	N/A	0,837	

Creator QPackSA
Reviewer
Approver

Chromatogram

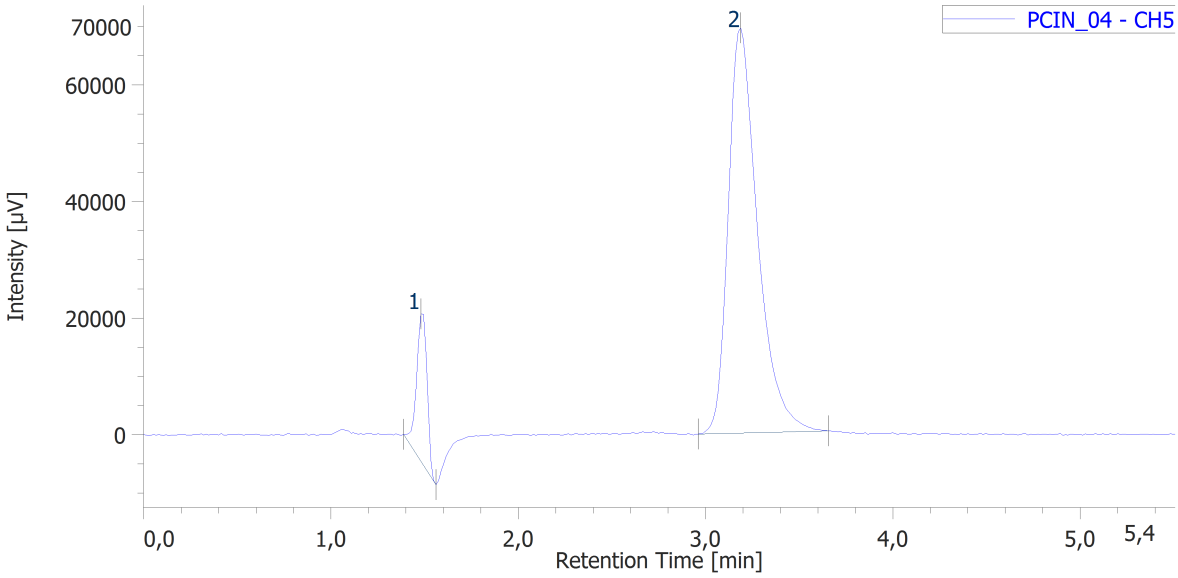

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:24:08
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:18:35
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	PCIN_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,480	99768	25289	11,658	26,692	N/A	3255	9,063	0,938	
2	Unknown	5	3,187	756007	69453	88,342	73,308	N/A	2167	N/A	1,412	

Creator QPackSA
Reviewer
Approver

Chromatogram

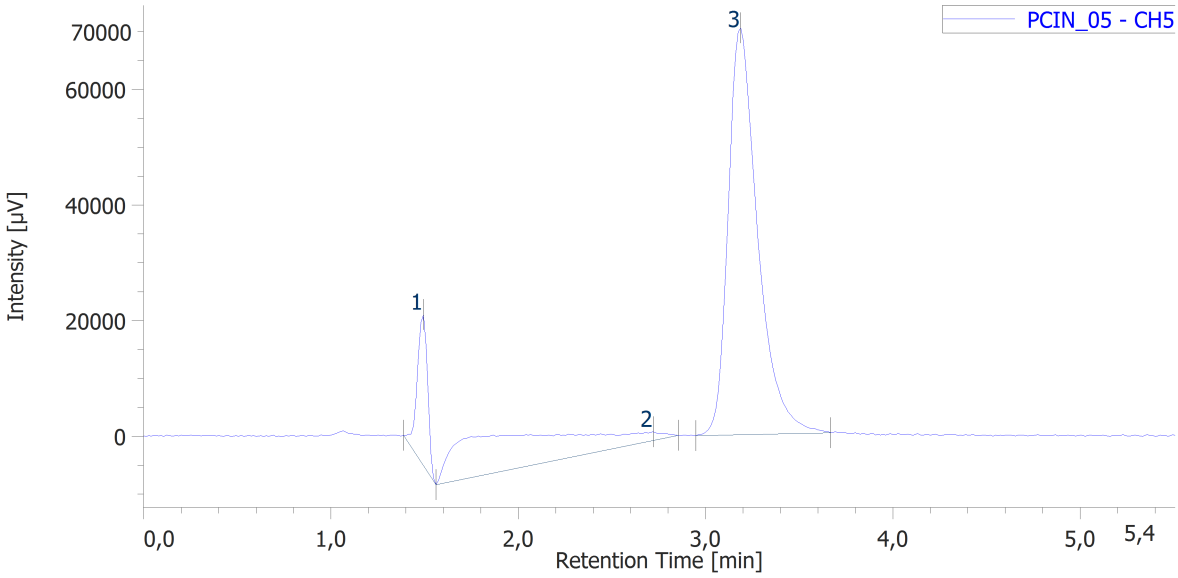

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:29:49
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:24:17
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	PCIN_05
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,493	99749	26134	8,492	26,678	N/A	3450	1,138	0,805	
2	Unknown	5	2,720	304822	1511	25,952	1,542	N/A	28	0,401	0,555	
3	Cafeína	5	3,187	769993	70317	65,556	71,780	N/A	2177	N/A	1,424	

Creator
Reviewer
Approver

Chromatogram

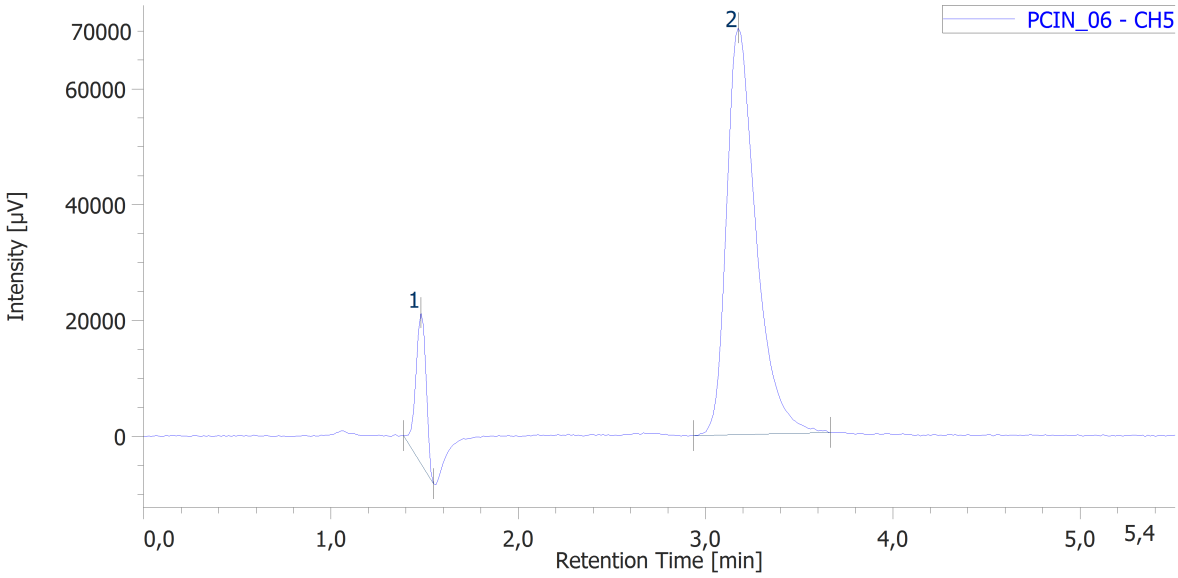

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:35:32
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:30:00
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	PCIN_06
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,480	99304	26096	11,438	27,104	N/A	3309	9,003	0,893	
2	Unknown	5	3,173	768888	70185	88,562	72,896	N/A	2142	N/A	1,493	

Creator QPackSA
Reviewer
Approver

Chromatogram

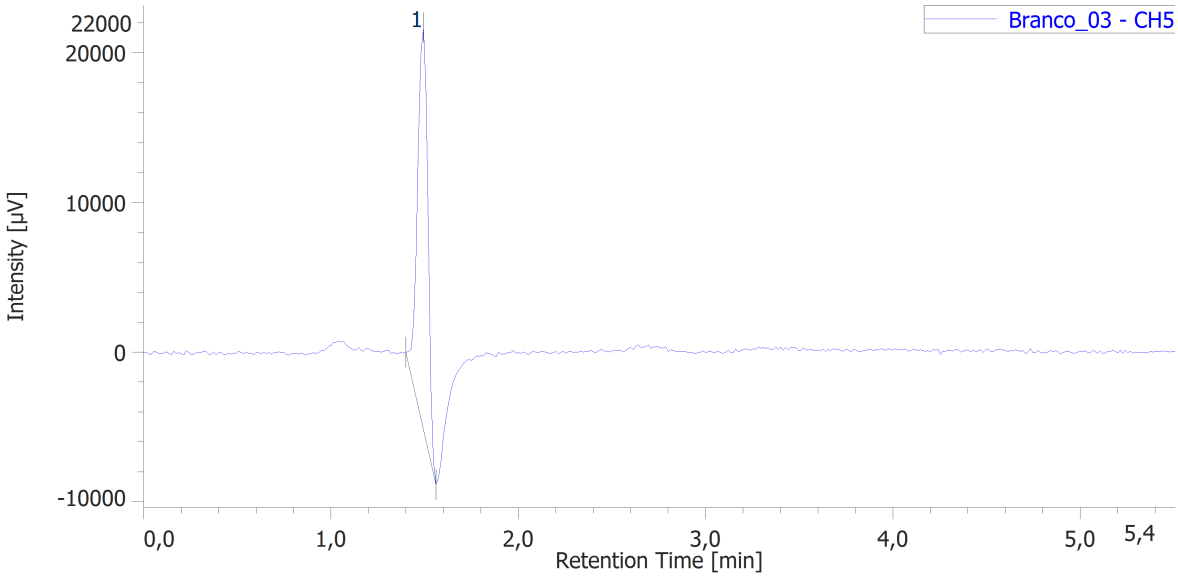

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:41:15
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:35:43
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	Branco_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,493	102340	26806	100,000	100,000	N/A	3318	N/A	0,860	

Creator QPackSA
Reviewer
Approver

Chromatogram

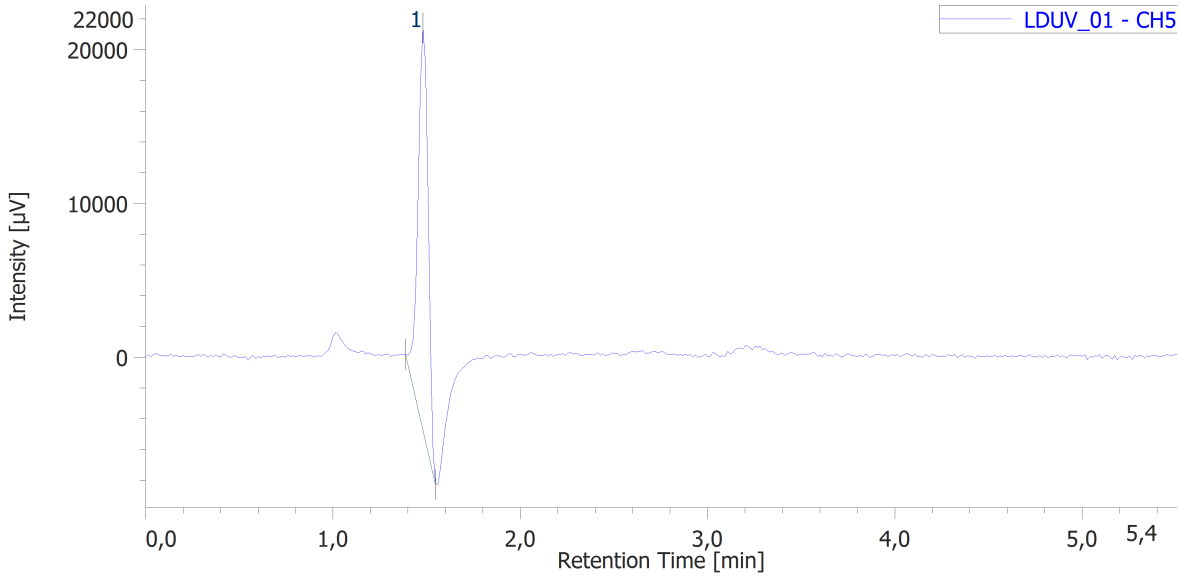

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:46:57
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:41:25
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH5
Sample Name	LDUV_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,480	99498	26161	100,000	100,000	N/A	3343	N/A	0,904	

Creator QPackSA
Reviewer
Approver

Chromatogram

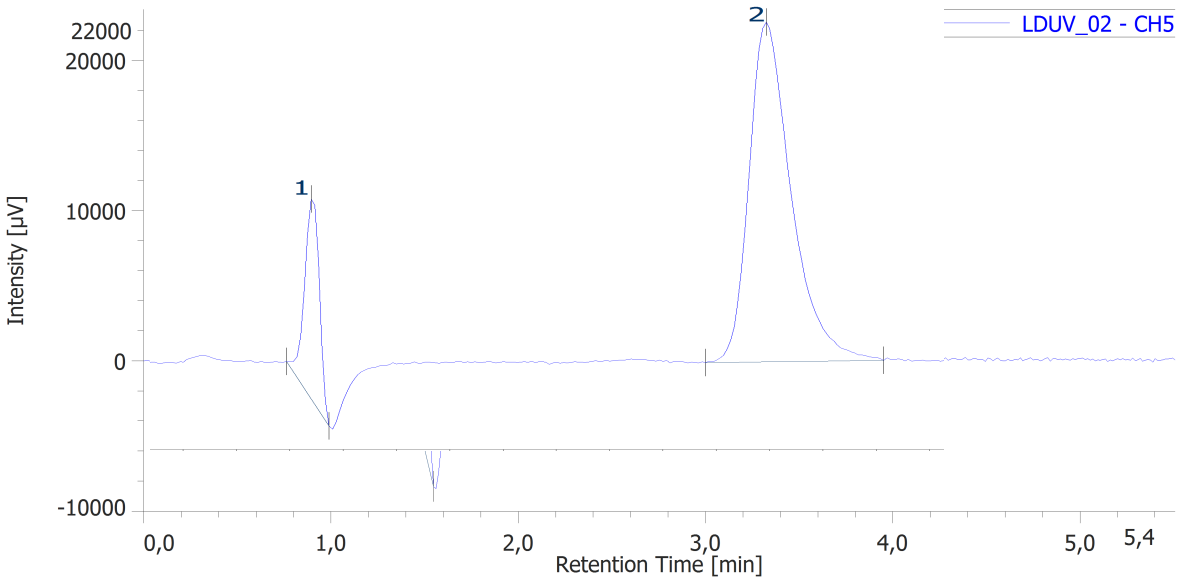

Chromatogram Information

User Name	QPackSA
Date Modified	10/10/2023 14:52:40
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:47:07
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH5
Sample Name	LDUV_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	102949	26723	57,477	79,492	N/A	3258	8,843	0,906	
2	Cafeína	5	3,200	76166	6894	42,523	20,508	N/A	1999	N/A	1,385	

Creator
Reviewer
Approver

Chromatogram

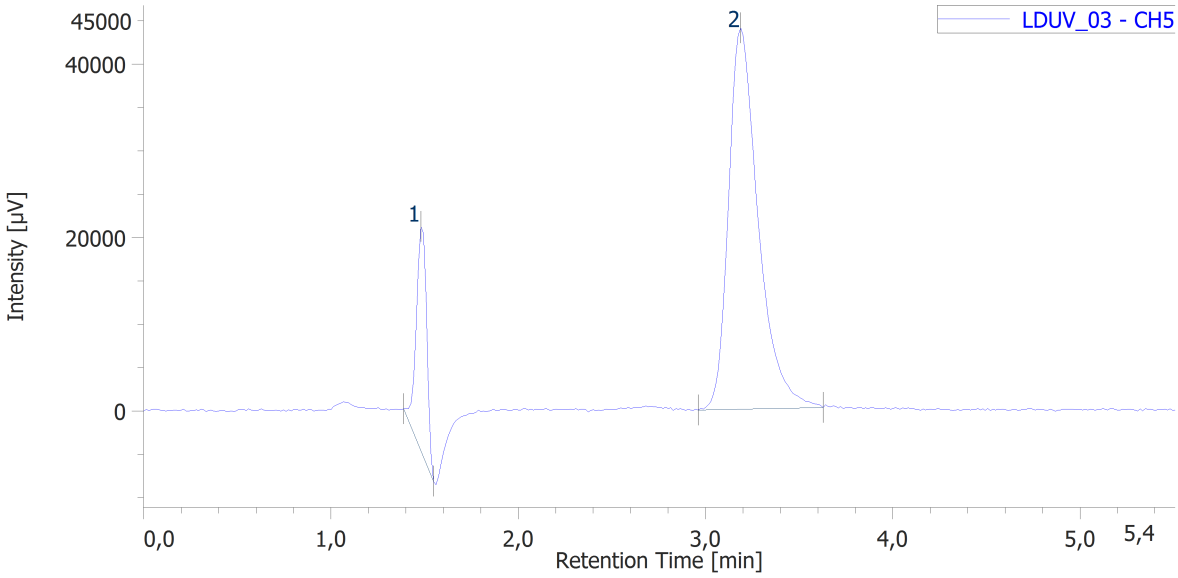

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 14:58:22
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:52:50
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH5
Sample Name	LDUV_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	102070	25909	17,374	37,082	N/A	3166	8,981	0,938	
2	Cafeína	5	3,187	485402	43960	82,626	62,918	N/A	2135	N/A	1,429	

Creator
Reviewer
Approver

Chromatogram

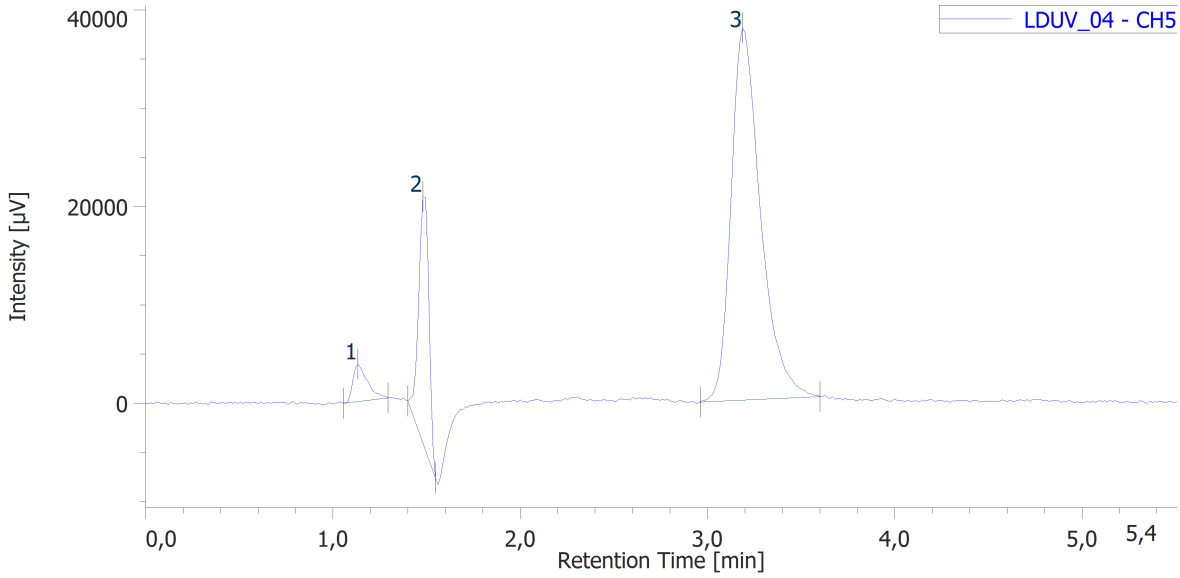

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:04:07
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 14:58:35
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH5
Sample Name	LDUV_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,133	20395	3783	3,833	5,674	N/A	994	2,800	1,921	
2	Peak-001	5	1,480	97561	25053	18,333	37,578	N/A	3210	9,016	0,981	
3	Cafeína	5	3,187	414195	37833	77,834	56,747	N/A	2147	N/A	1,440	

Creator
Reviewer
Approver

Chromatogram

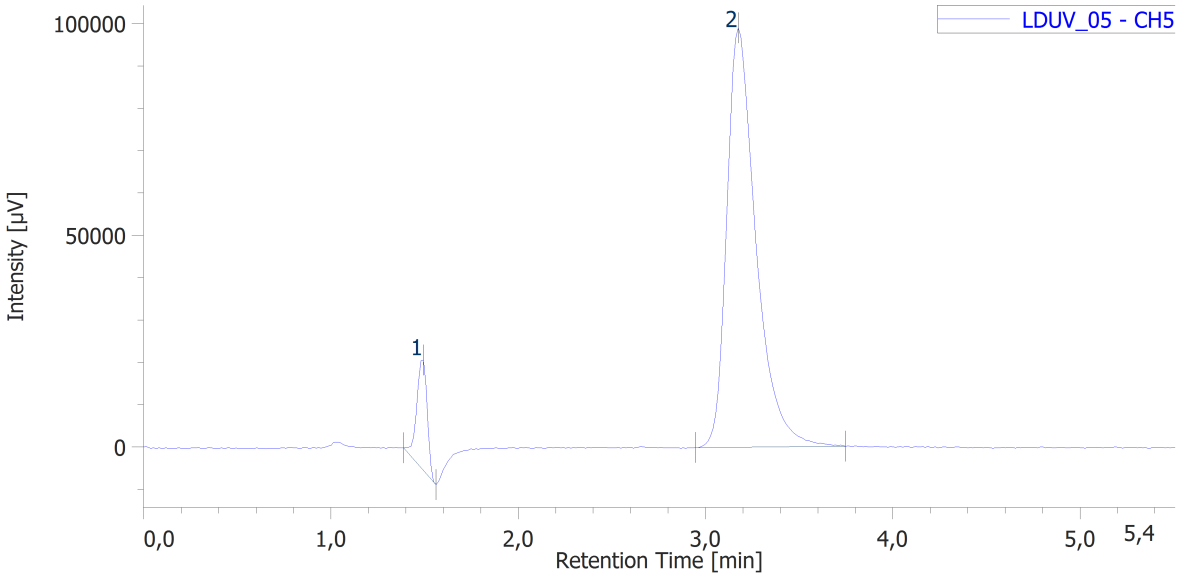

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:09:52
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:04:20
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH5
Sample Name	LDUV_05
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,493	101240	26077	8,624	20,859	N/A	3354	9,031	0,789	
2	Cafeína	5	3,173	1072632	98940	91,376	79,141	N/A	2212	N/A	1,497	

Creator
Reviewer
Approver

Chromatogram

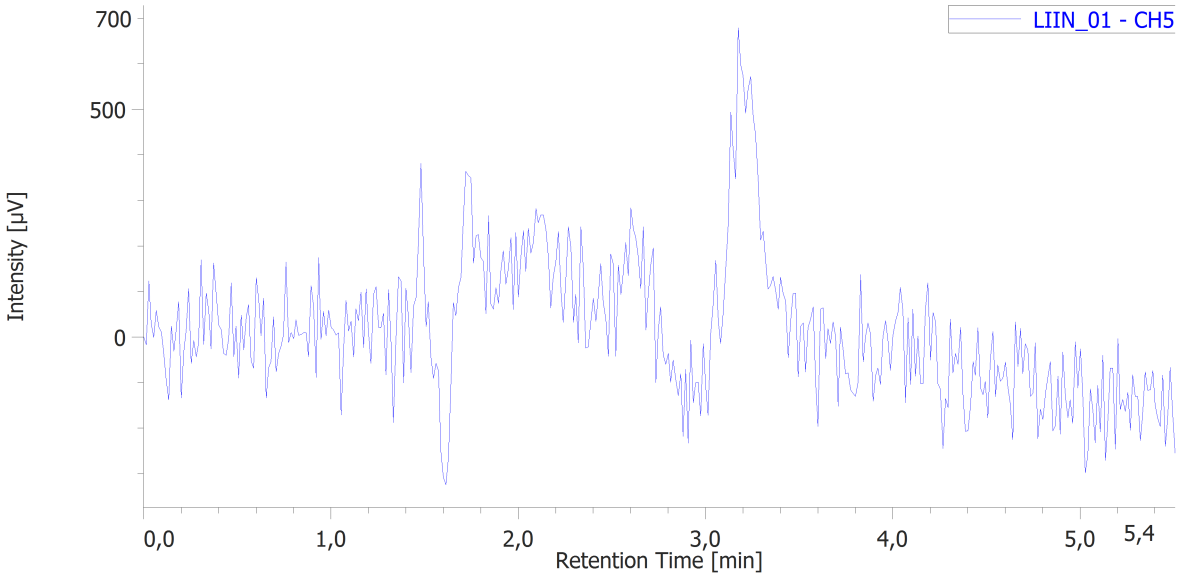


Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:15:37
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:10:04
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	LIIN_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

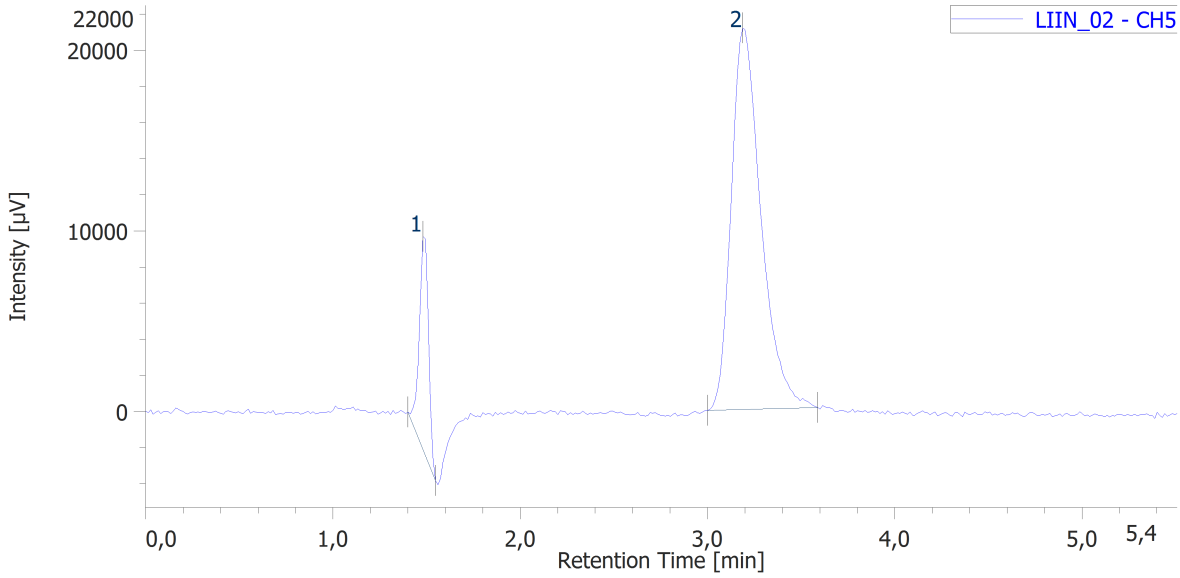

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:21:21
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:15:49
Volume	5,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	LIIN_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,480	41242	11790	15,043	35,840	N/A	4193	9,201	0,988	
2	Cafeína	5	3,187	232915	21106	84,957	64,160	N/A	2065	N/A	1,437	

Creator
Reviewer
Approver

Chromatogram

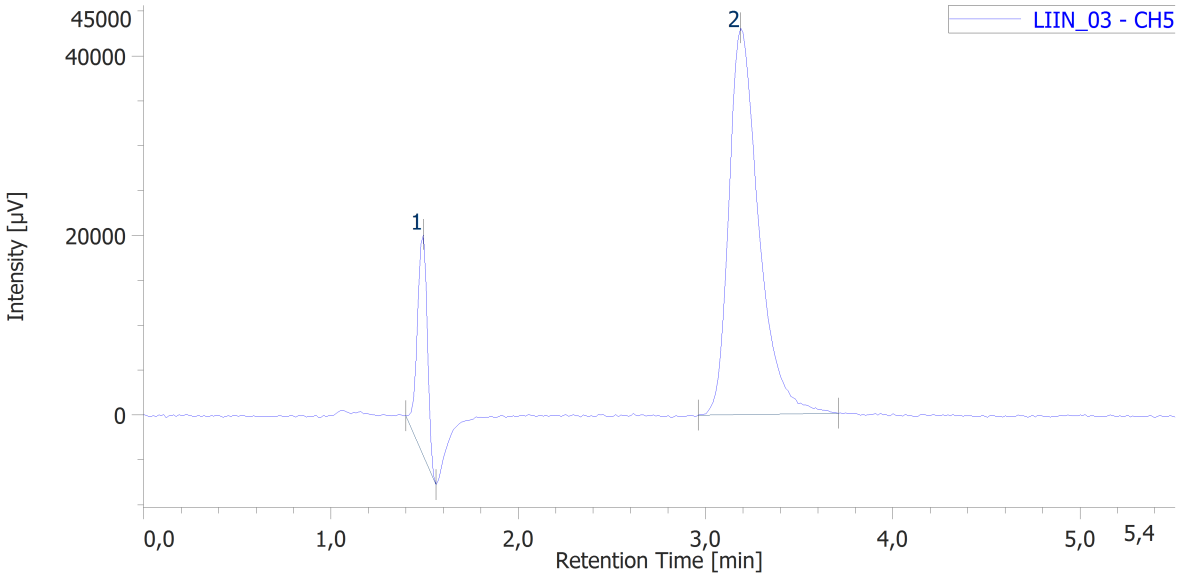

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:27:07
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:21:34
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	LIIN_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,493	90967	24666	16,006	36,430	N/A	3632	9,037	0,846	
2	Cafeína	5	3,187	477358	43042	83,994	63,570	N/A	2123	N/A	1,455	

Creator
Reviewer
Approver

Chromatogram

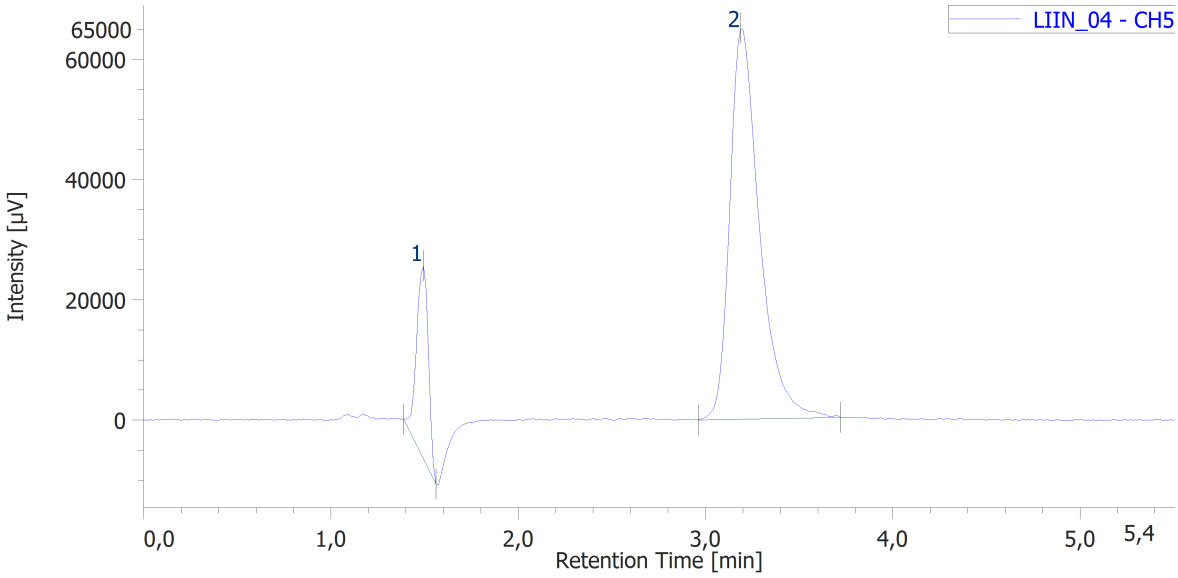

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:32:51
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:27:19
Volume	15,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	LIIN_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,493	140390	32083	16,388	33,050	N/A	2462	8,608	0,844	
2	Cafeína	5	3,187	716295	64991	83,612	66,950	N/A	2163	N/A	1,523	

Creator
Reviewer
Approver

Chromatogram

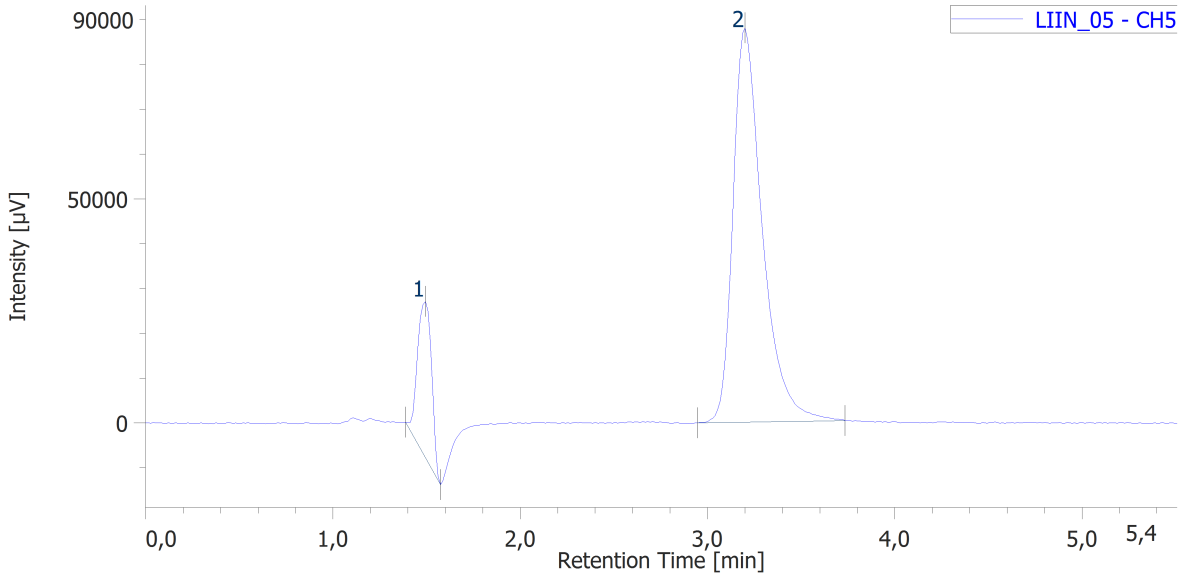

Chromatogram Information	
User Name	QPackSA
Date Modified	10/10/2023 15:38:37
Description	
HPLC System Name	HPL25
Injection Date	10/10/2023 15:33:04
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	5,5 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH5
Sample Name	LIIN_05
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	5	1,493	182108	34867	15,964	28,395	N/A	1626	8,170	0,890	
2	Cafeína	5	3,200	958608	87927	84,036	71,605	N/A	2235	N/A	1,443	

Creator
Reviewer
Approver

Chromatogram Information

User Name	QPackSA
Date Modified	17/10/2023 15:56:02
HPLC System Name	HPL25
Injection Date	17/10/2023 15:10:50
Volume	0,1 [µL]
Project Name	Qualificação

Chromatogram

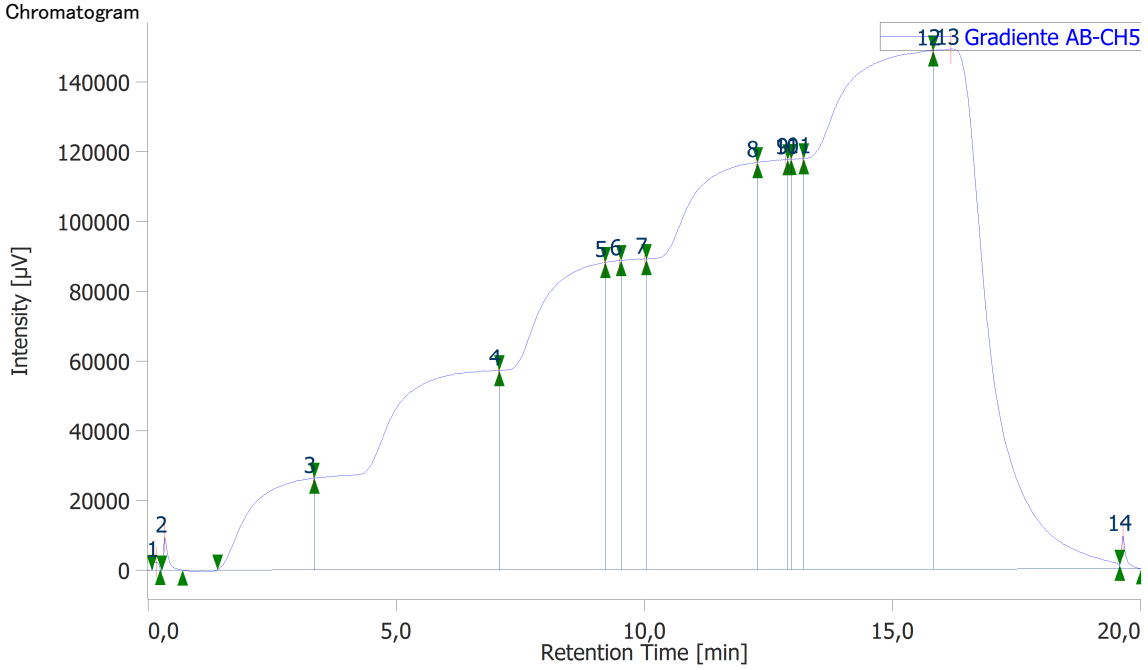

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	Unknown	5	0,167	16289	2326
2	Unknown	5	0,340	59984	9335
3	Unknown	5	3,327	2146622	29434
4	40	5	7,060	9830221	59180
5	Unknown	5	9,187	9698099	88203
6	Unknown	5	9,493	1662073	88715
7	60	5	10,007	2737702	89111
8	Unknown	5	12,247	14210614	116799
9	Unknown	5	12,847	4264798	117606
10	Unknown	5	12,927	470116	117684
11	80	5	13,180	1788677	119879
12	Unknown	5	15,787	21771796	148734
13	100	5	16,167	11174695	149218
14	Unknown	5	19,633	60834	9509

Chromatogram Information

User Name	QPackSA
Date Modified	17/10/2023 15:56:02
Description	
HPLC System Name	HPL25
Injection Date	17/10/2023 15:10:50
Volume	0,1 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB

Creator QPackSA
Reviewer
Approver


Peak ID Table	GRAD AB
Calibration Method	
Additional Information	
Column Info	

Creator QPackSA
Reviewer
Approver

Chromatogram Information

User Name	QPackSA
Date Modified	17/10/2023 15:51:04
HPLC System Name	HPL25
Injection Date	17/10/2023 15:31:03
Volume	0,1 [µL]
Project Name	Qualificação

Chromatogram

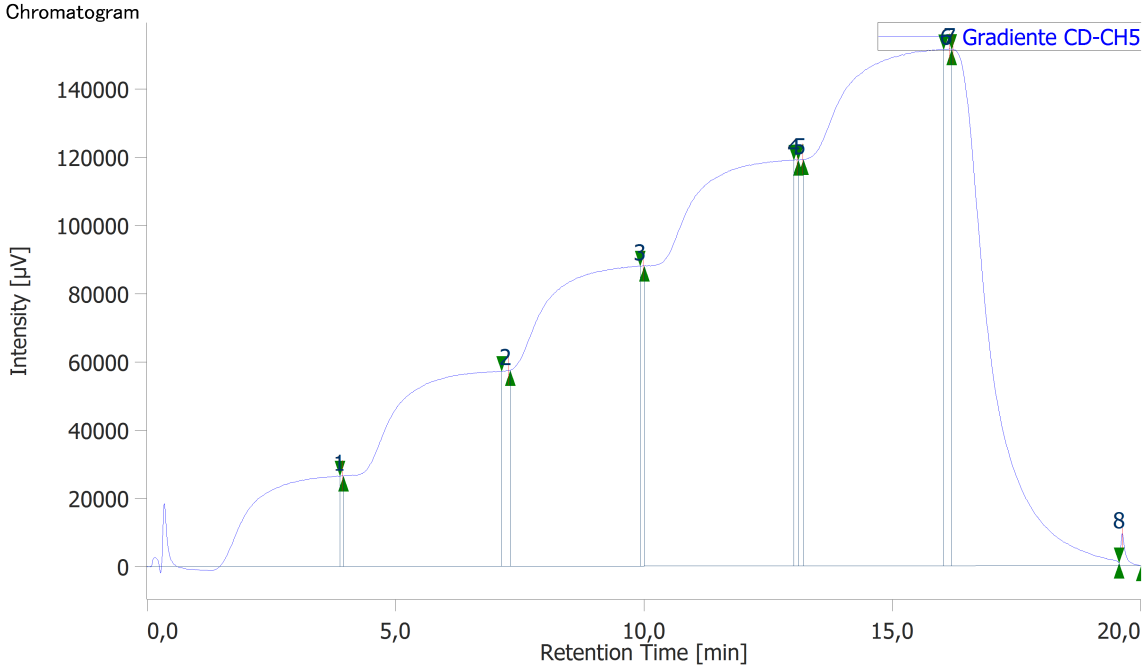

Peak Information


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]
1	20	5	3,933	106151	29637
2	40	5	7,280	595563	59474
3	60	5	9,980	457350	90114
4	Unknown	5	13,080	618676	119038
5	80	5	13,193	761979	120180
6	100	5	16,140	1452880	151527
7	Unknown	5	16,213	7860688	151403
8	Unknown	5	19,620	63049	9541

Chromatogram Information

User Name	QPackSA
Date Modified	17/10/2023 15:51:04
Description	
HPLC System Name	HPL25
Injection Date	17/10/2023 15:31:03
Volume	0,1 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD
Peak ID Table	GRAD CD
Calibration Method	
Additional Information	
Column Info	

Creator
Reviewer
Approver

Chromatogram

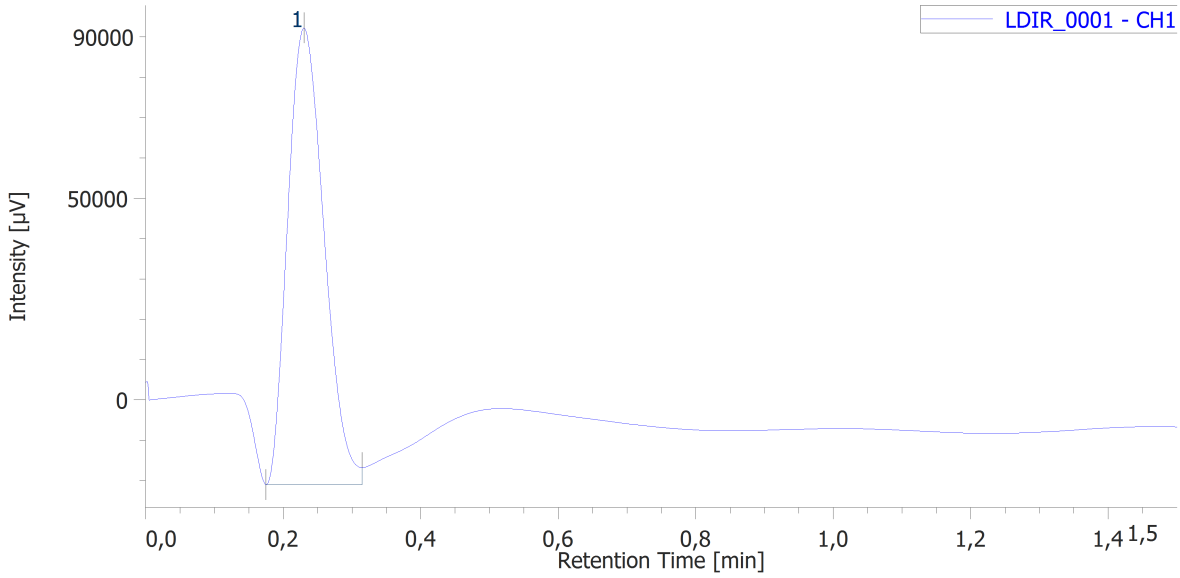

Chromatogram Information	
User Name	QPackSA
Date Modified	18/10/2023 13:56:56
Description	
HPLC System Name	HPL 25 RI
Injection Date	18/10/2023 13:55:24
Volume	4,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	LDIR_
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR_0001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	LDIR_

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,230	414807	113137	100,000	100,000	N/A	86	N/A	1,285	

Creator
Reviewer
Approver

Chromatogram

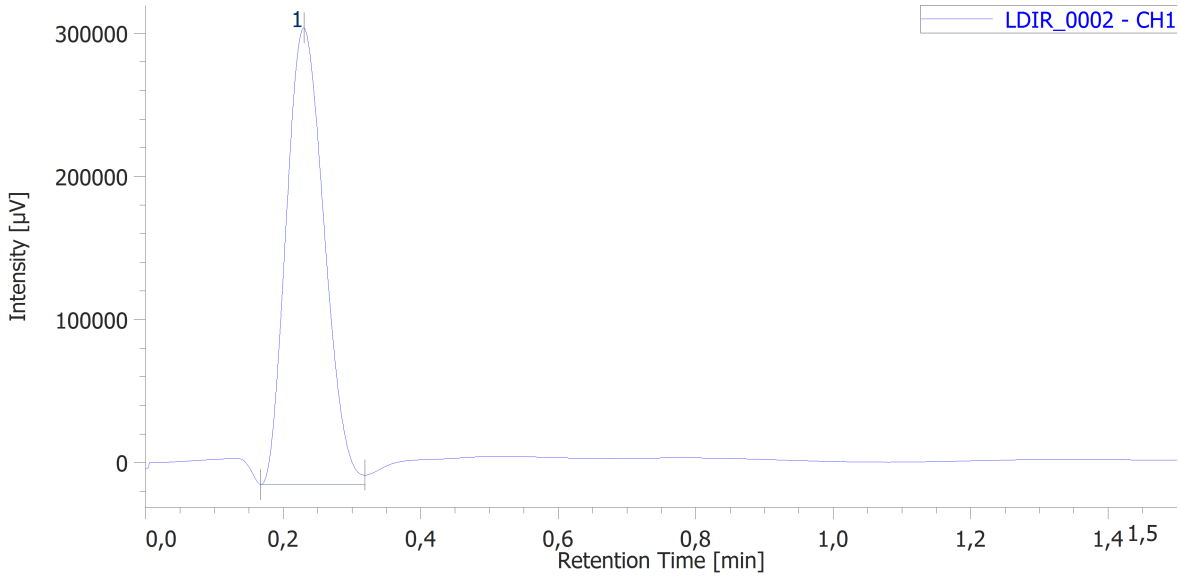

Chromatogram Information	
User Name	QPackSA
Date Modified	18/10/2023 13:59:54
Description	
HPLC System Name	HPL 25 RI
Injection Date	18/10/2023 13:58:22
Volume	8,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	LDIR_
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR_0002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	LDIR_

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,230	1291093	318845	100,000	100,000	N/A	79	N/A	1,188	

Creator
Reviewer
Approver

Chromatogram

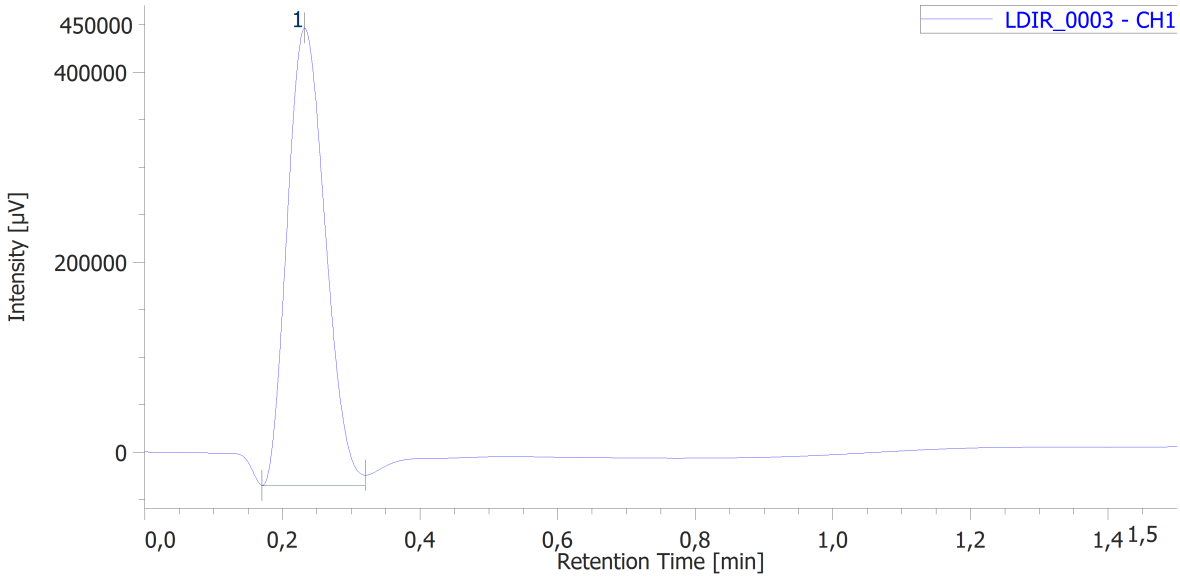

Chromatogram Information	
User Name	QPackSA
Date Modified	18/10/2023 14:02:54
Description	
HPLC System Name	HPL 25 RI
Injection Date	18/10/2023 14:01:22
Volume	12,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	LDIR_
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR_0003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	LDIR_

#	Peak Name	CH	tR [min]	Area [µV*sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	0,232	1781358	481209	100,000	100,000	N/A	81	N/A	1,206	

Creator
Reviewer
Approver

Chromatogram

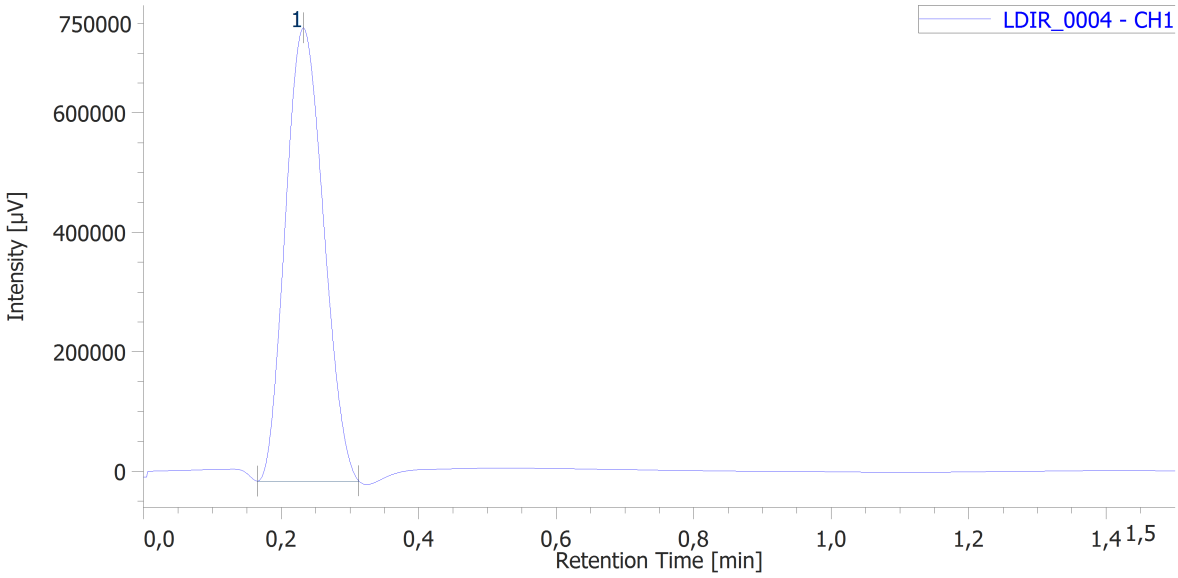

Chromatogram Information	
User Name	QPackSA
Date Modified	18/10/2023 14:05:54
Description	
HPLC System Name	HPL 25 RI
Injection Date	18/10/2023 14:04:22
Volume	16,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	LDIR_
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR_0004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	LDIR_

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,233	2599752	758338	100,000	100,000	N/A	78	N/A	1,114	

Creator
Reviewer
Approver

Chromatogram

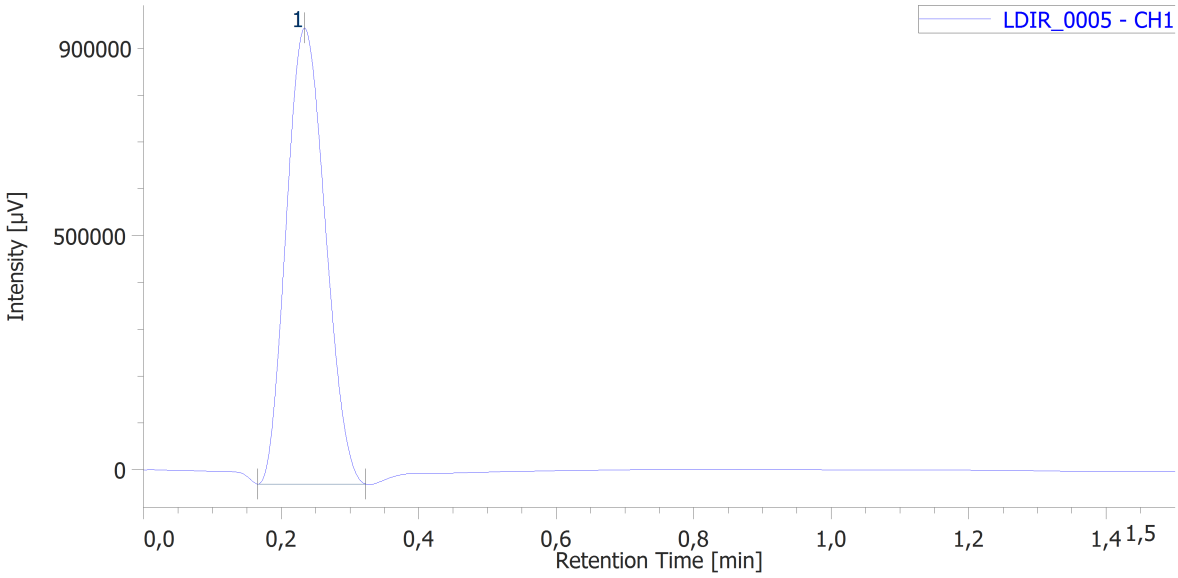

Chromatogram Information	
User Name	QPackSA
Date Modified	18/10/2023 14:08:56
Description	
HPLC System Name	HPL 25 RI
Injection Date	18/10/2023 14:07:24
Volume	20,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	LDIR_
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR_0005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	LDIR_

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,234	4823135	974271	100,000	100,000	N/A	76	N/A	1,133	

Creator
Reviewer
Approver