
Peak Find - ESPECTRO 01-HP01.jws

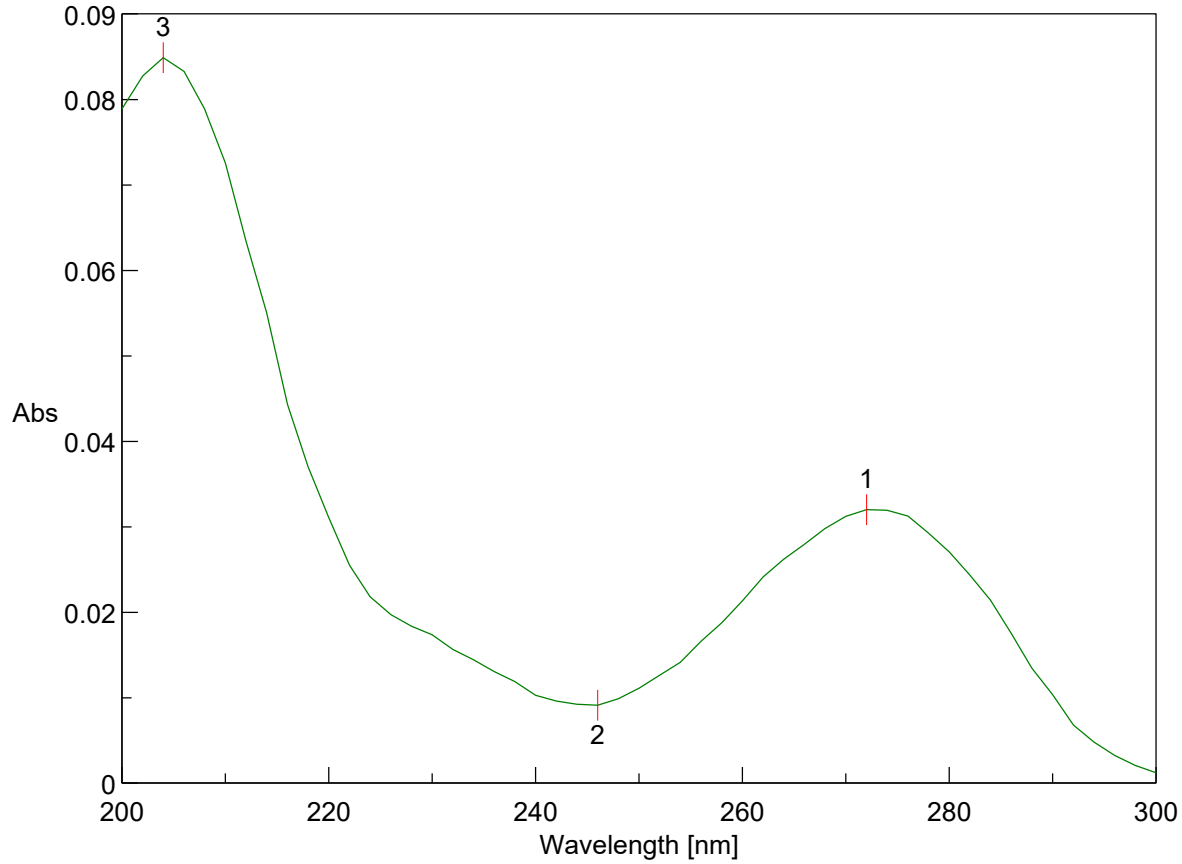

[Comments]


User	Mateus
Division	
Company	QPack
Creation date	13/12/2022 12:02

[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	600 nm	
Data interval	2 nm	
Data points	200	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.03199	2	246	0.00910497
3	204	0.0848655			

Chromatogram

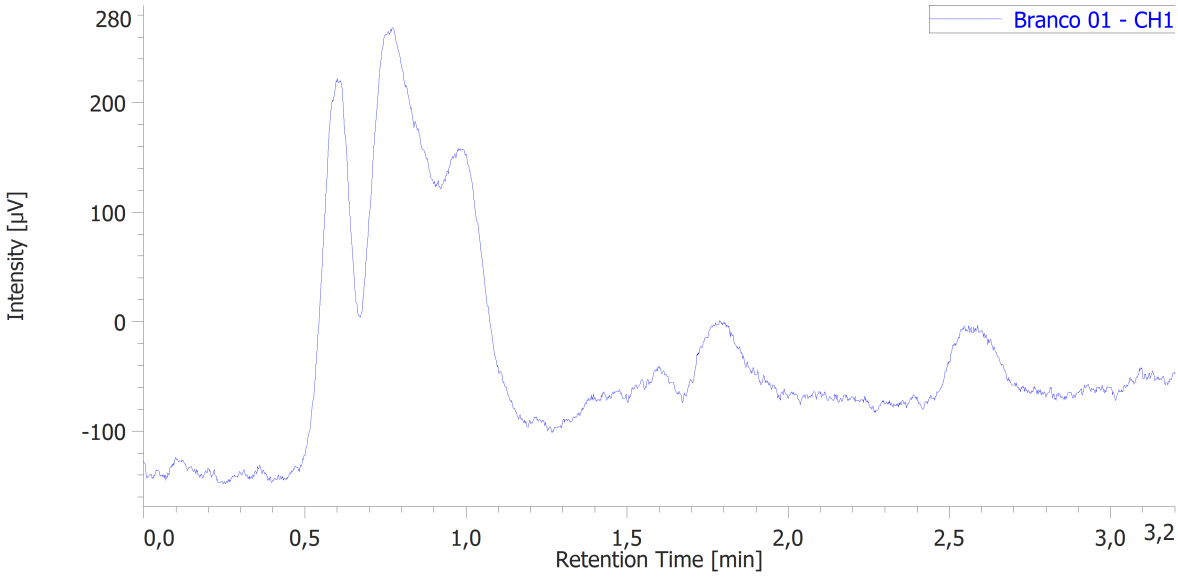


Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:34
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:32:10
Volume	10,0 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator QPackSA
Reviewer
Approver

Chromatogram

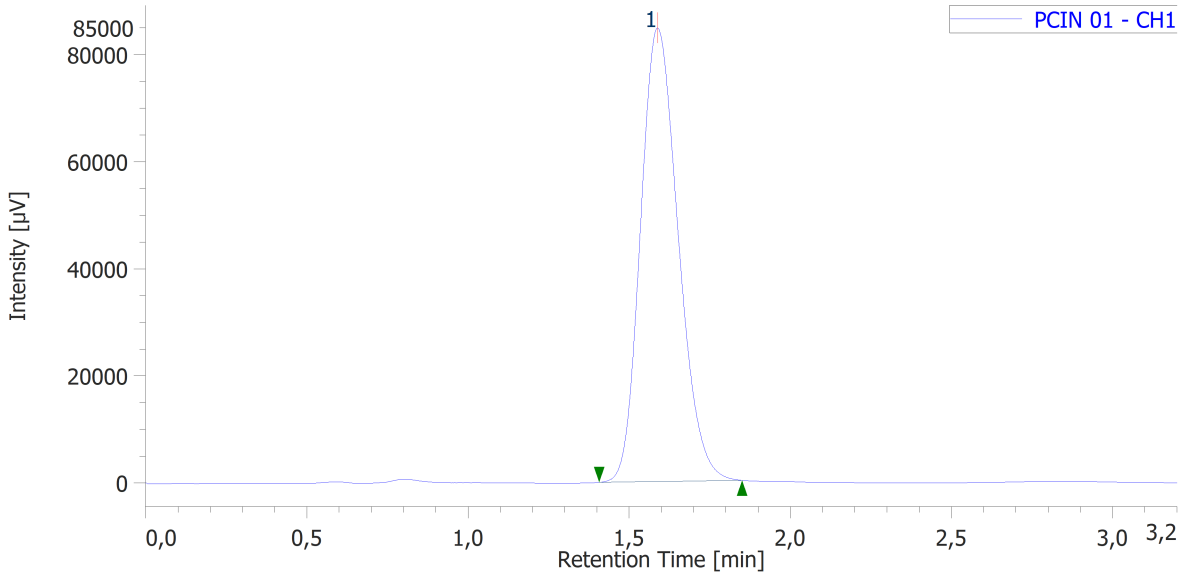

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:34
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:35:56
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,588	688832	84669	100,000	100,000	N/A	875	N/A	1,195		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

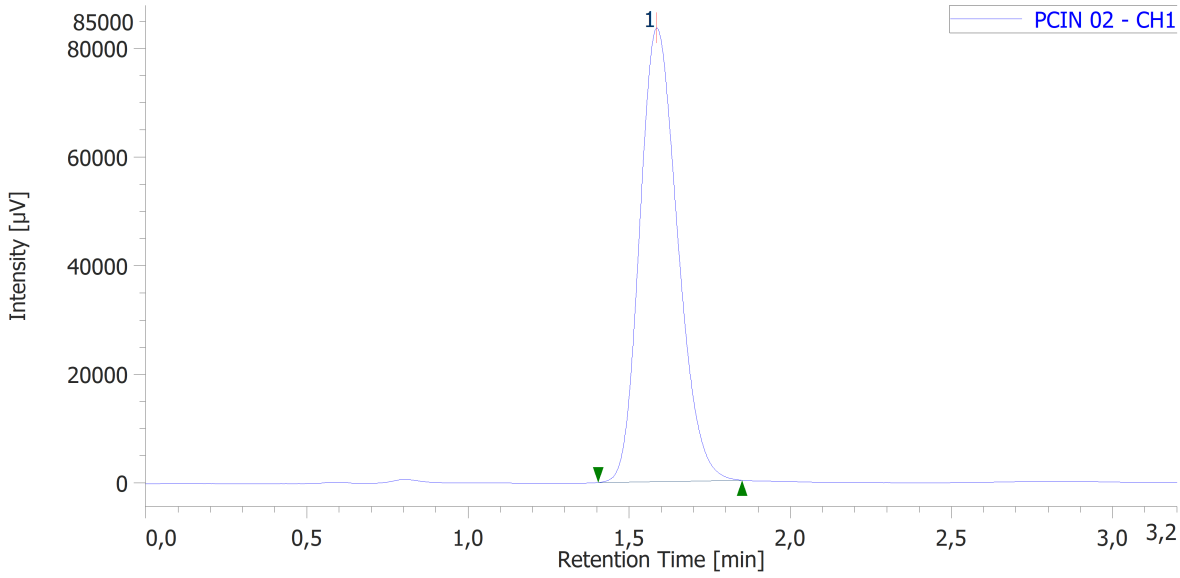

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:34
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:39:42
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,585	681964	83481	100,000	100,000	N/A	866	N/A	1,211		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

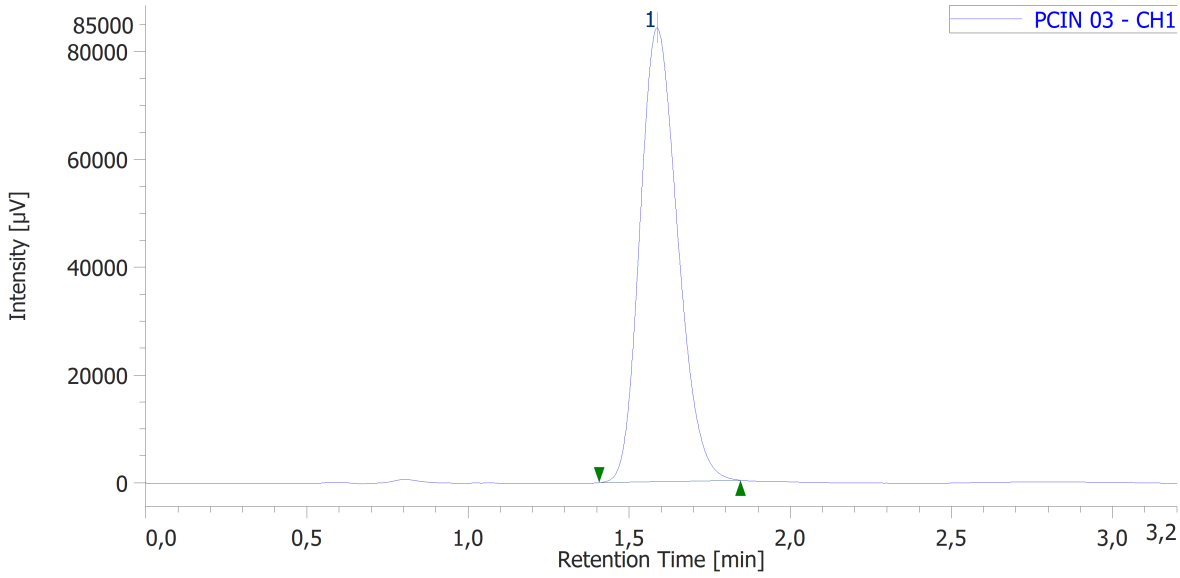

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:35
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:43:31
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,587	686567	84134	100,000	100,000	N/A	868	N/A	1,199		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

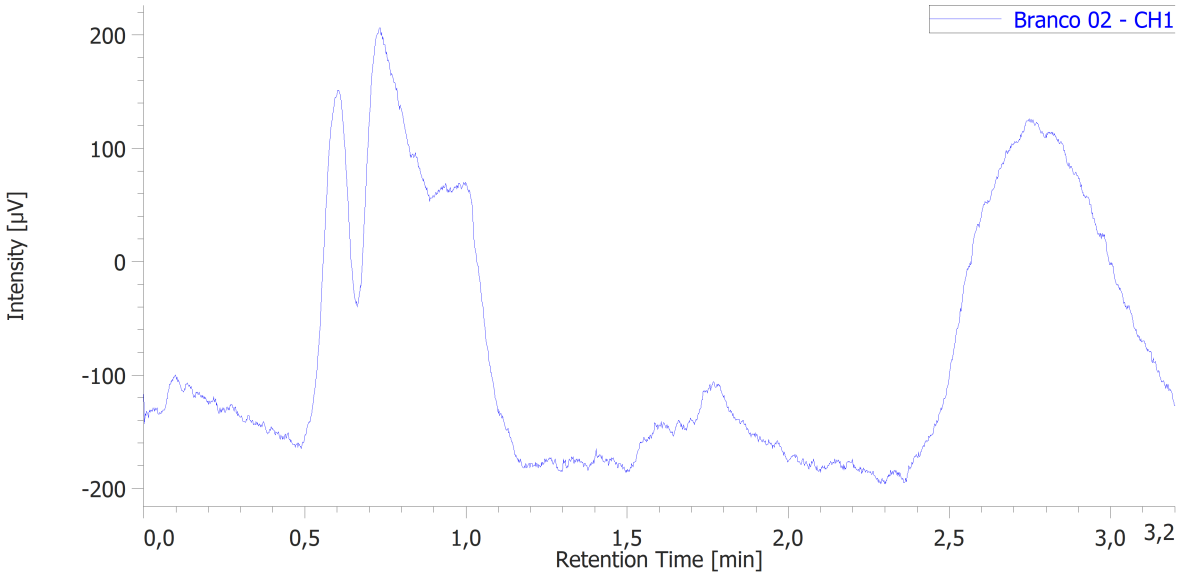


Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:35
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:47:20
Volume	10,0 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator QPackSA
Reviewer
Approver

Chromatogram

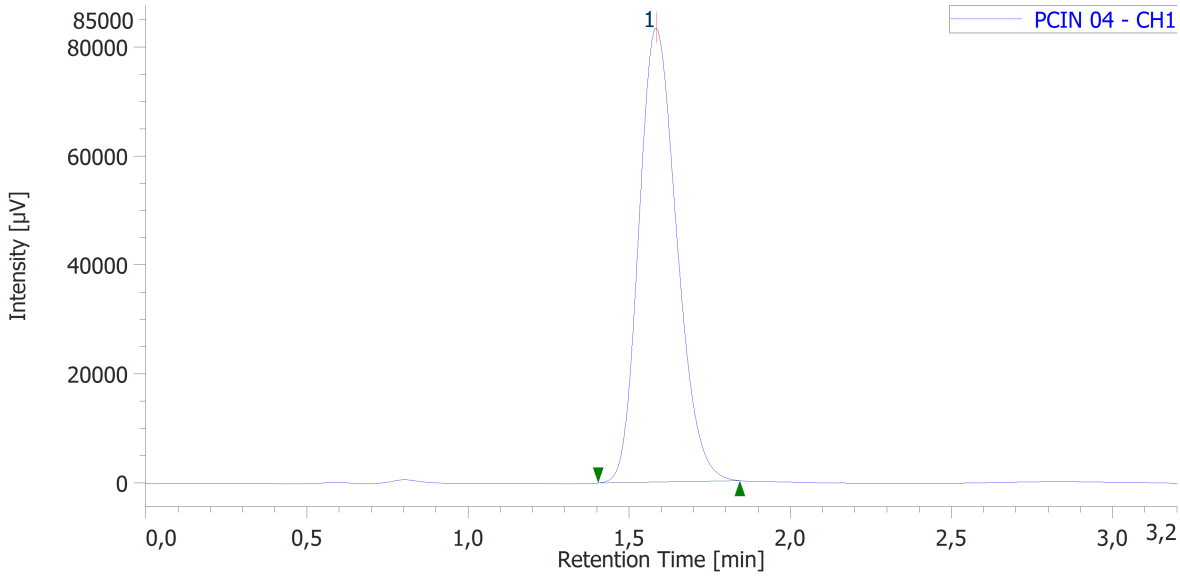

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:35
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:51:06
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,583	679930	83318	100,000	100,000	N/A	860	N/A	1,201		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

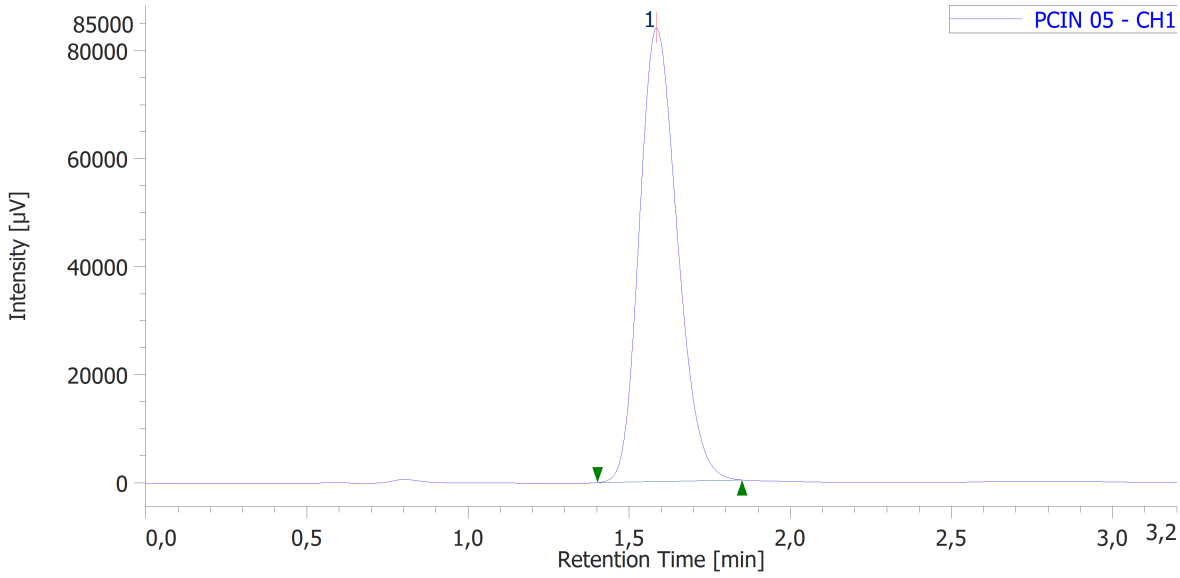

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:35
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:54:54
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,585	688436	83947	100,000	100,000	N/A	860	N/A	1,200		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

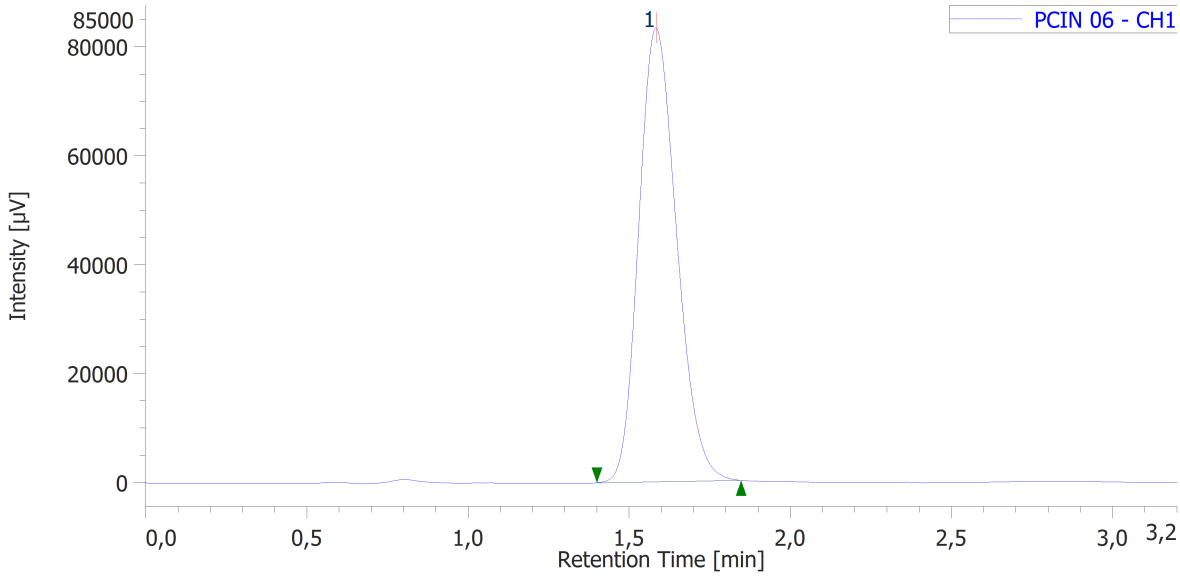

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:35
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 12:58:41
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,583	681855	83301	100,000	100,000	N/A	857	N/A	1,197		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

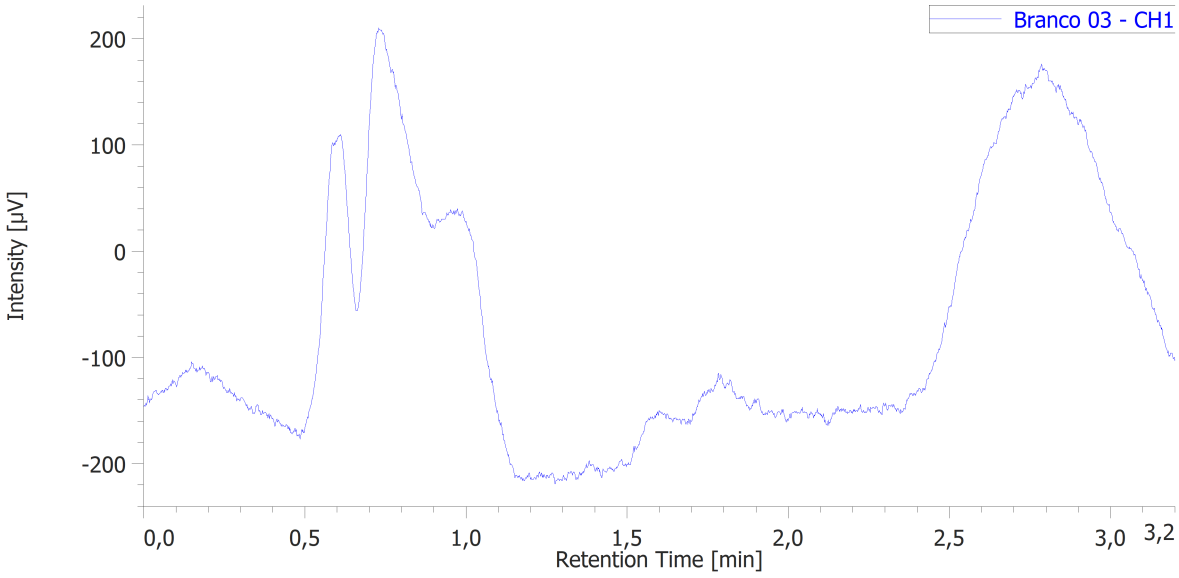


Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:36
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:02:29
Volume	10,0 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator QPackSA
Reviewer
Approver

Chromatogram

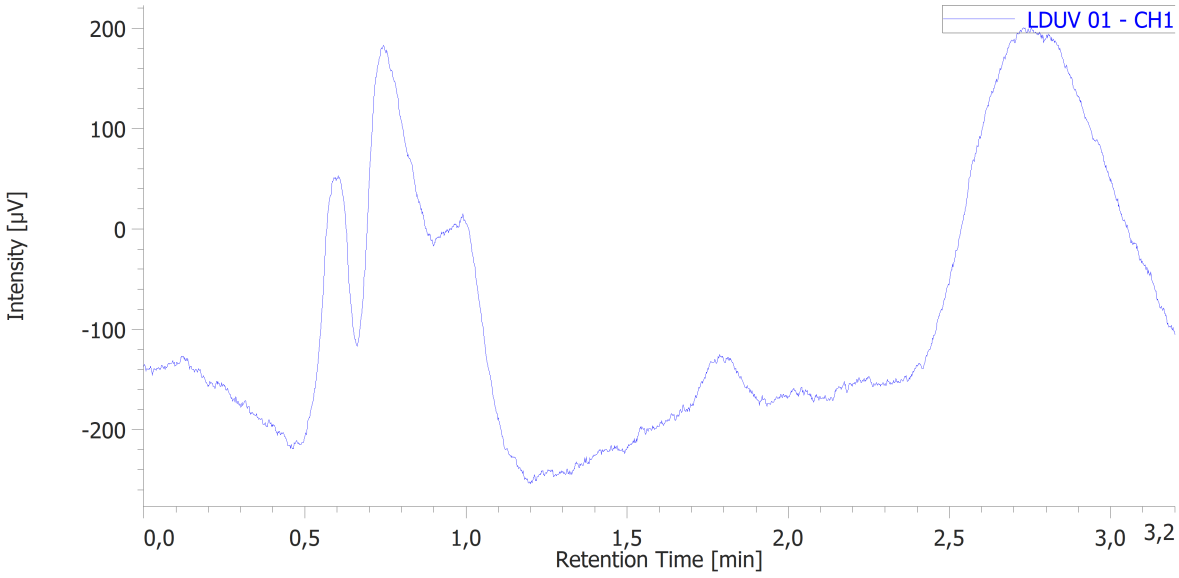


Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:36
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:06:18
Volume	10,0 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

Creator QPackSA
Reviewer
Approver

Chromatogram

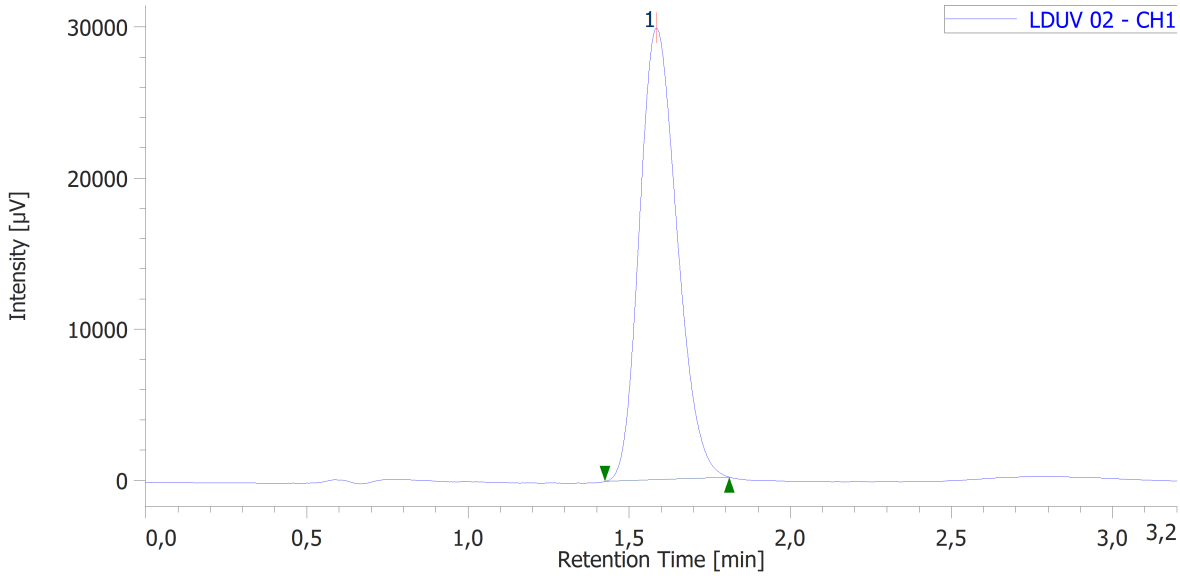

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:36
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:10:07
Volume	10,0 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,585	242341	29863	100,000	100,000	N/A	868	N/A	1,197		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

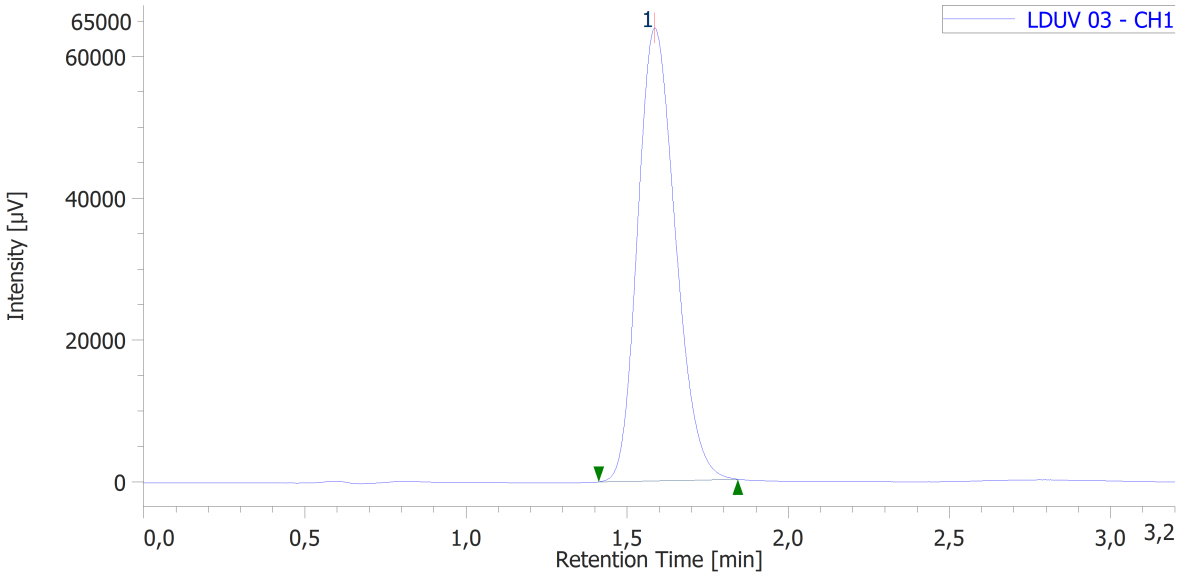

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:36
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:13:55
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,585	521329	63861	100,000	100,000	N/A	865	N/A	1,211		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

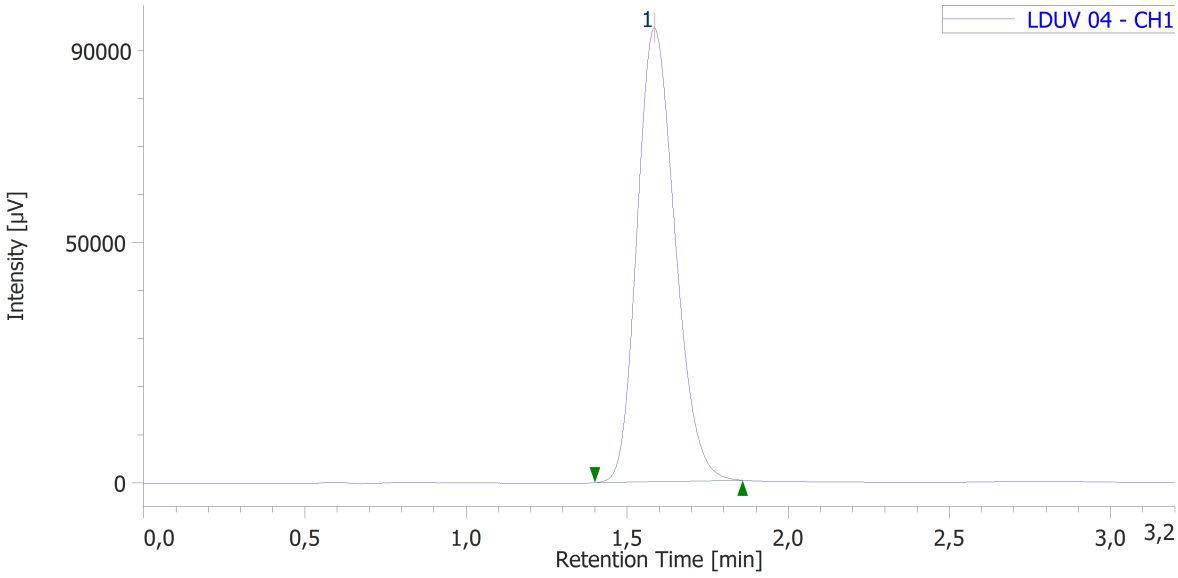

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:36
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:17:44
Volume	10,0 [µL]
Sample #	4
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,583	772799	94469	100,000	100,000	N/A	863	N/A	1,212		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

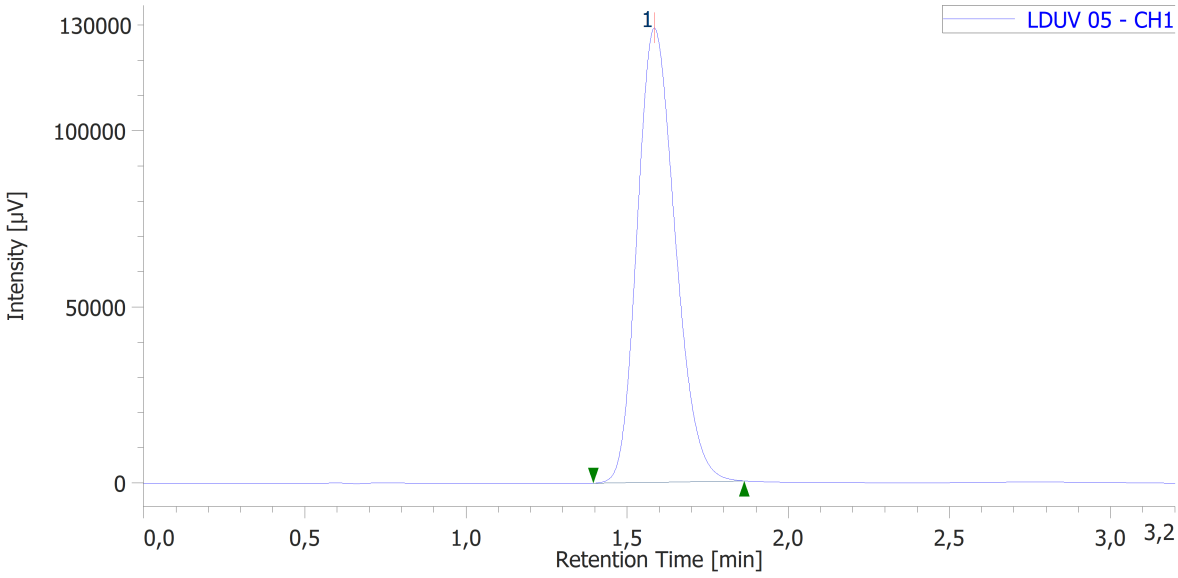

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:37
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:21:33
Volume	10,0 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,583	1057086	128881	100,000	100,000	N/A	857	N/A	1,219		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

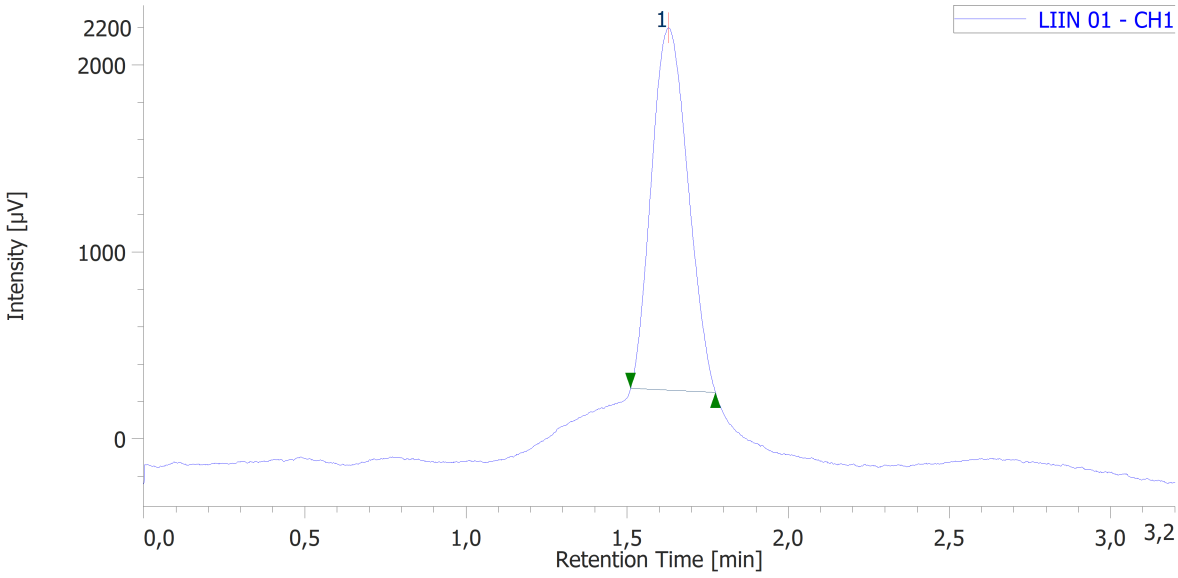

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:37
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:46:45
Volume	0,1 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,628	15222	1936	100,000	100,000	N/A	904	N/A	1,117		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

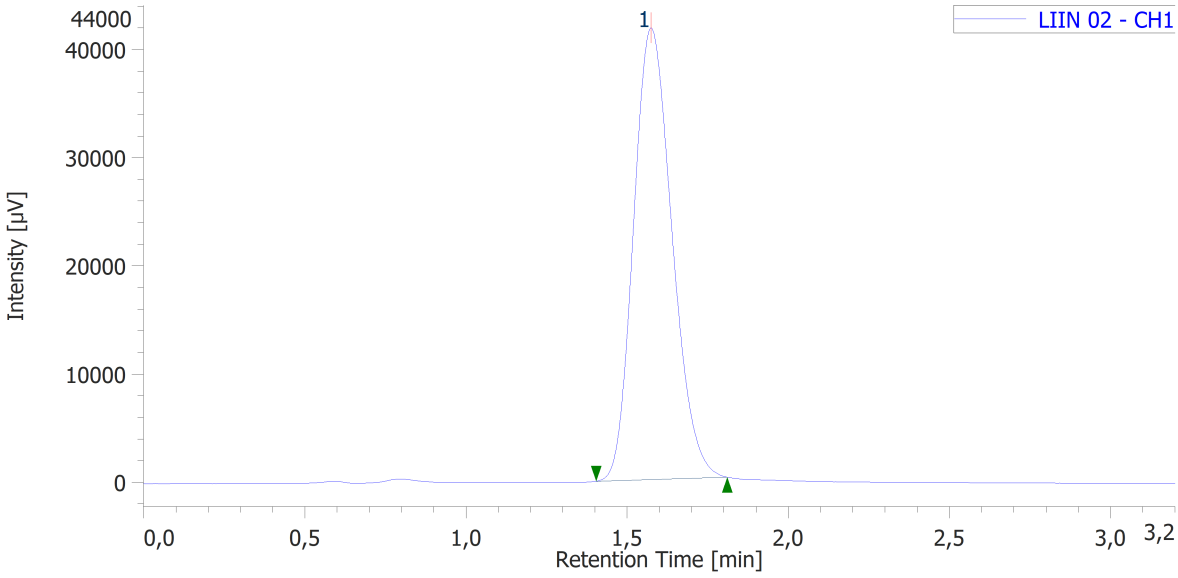

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:37
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:50:29
Volume	5,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,573	346446	41723	100,000	100,000	N/A	818	N/A	1,199		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

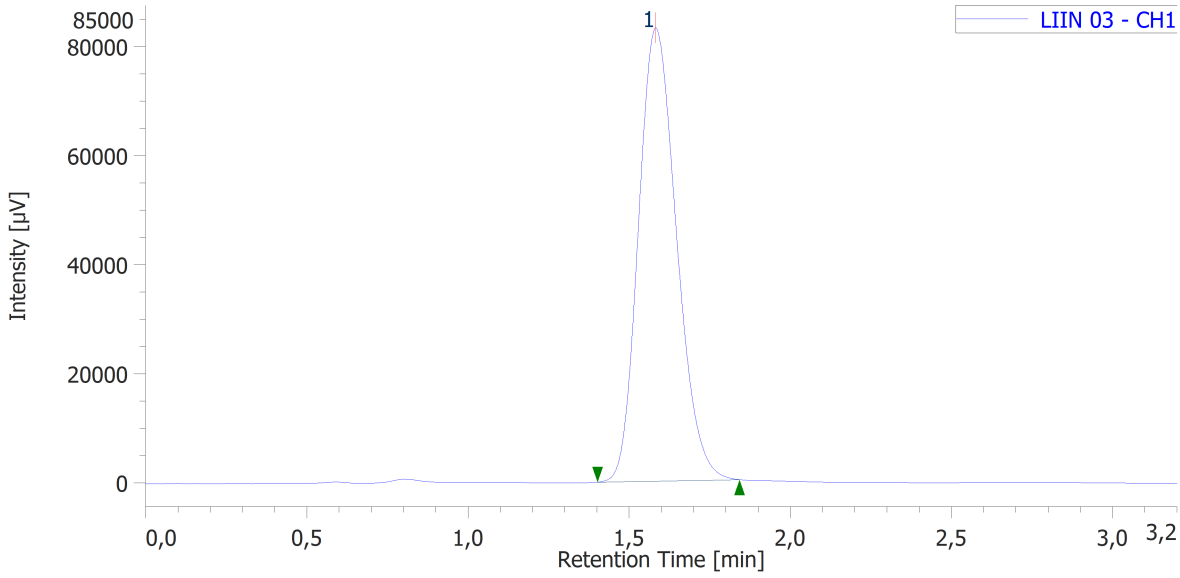

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:37
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:54:18
Volume	10,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,582	682491	83061	100,000	100,000	N/A	848	N/A	1,203		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

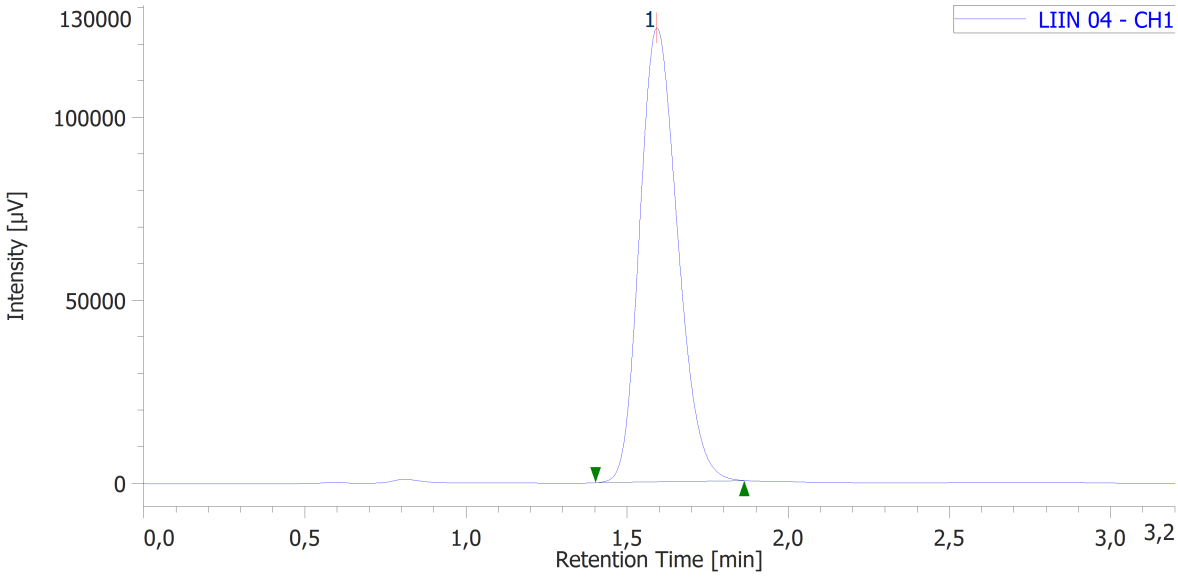

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:37
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 13:58:10
Volume	15,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,592	1016224	123933	100,000	100,000	N/A	866	N/A	1,203		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

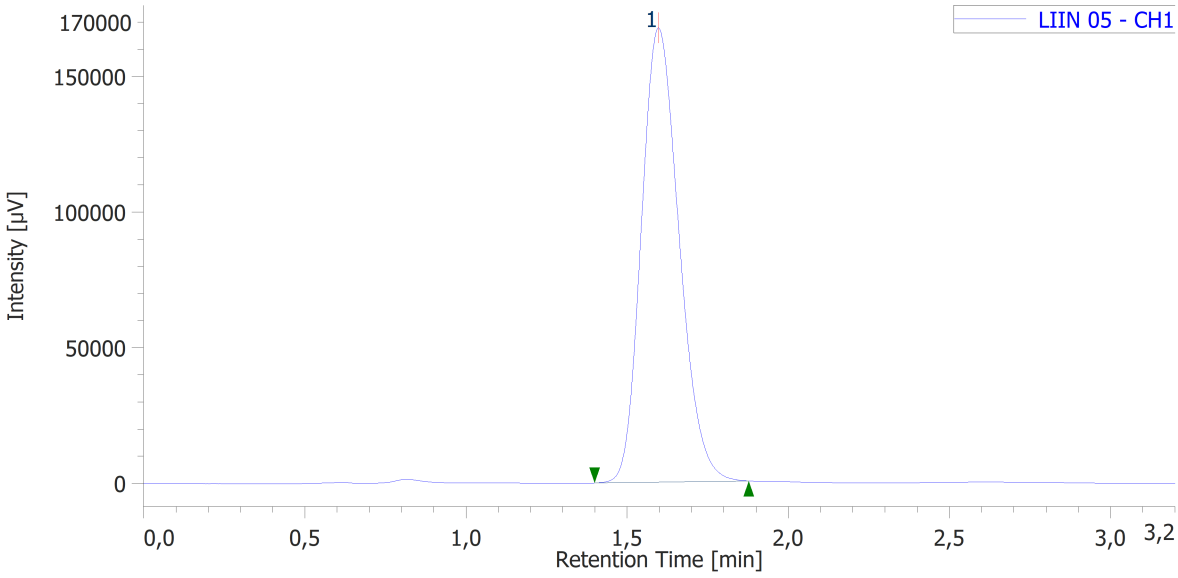

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 14:07:38
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 14:02:08
Volume	20,0 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Int

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,597	1362136	167360	100,000	100,000	N/A	883	N/A	1,204		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

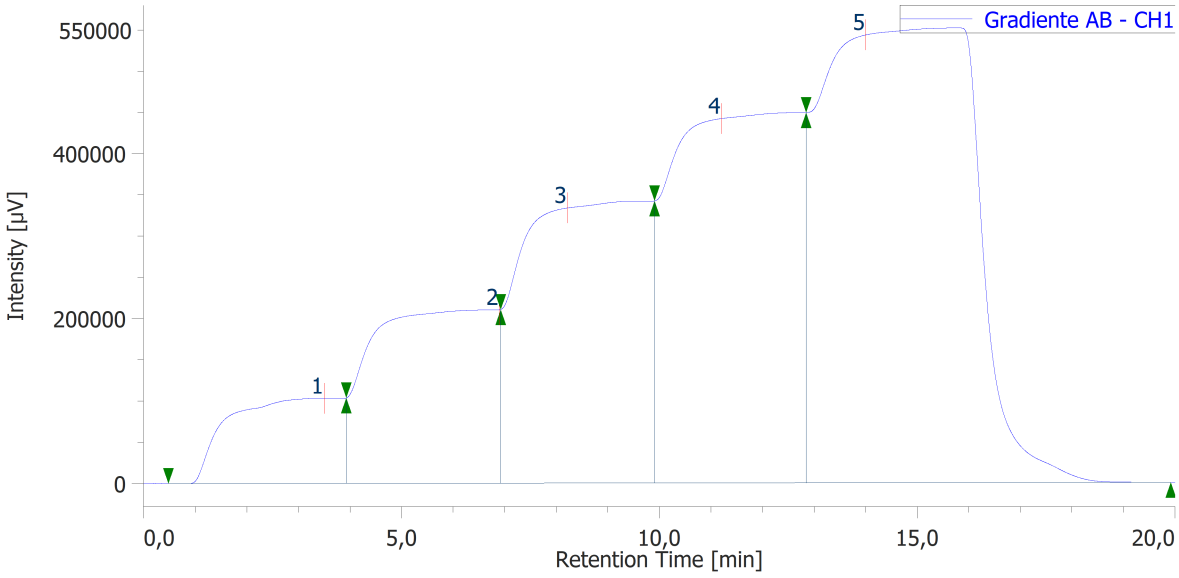

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 17:36:22
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 16:16:48
Volume	0,1 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	20%	1	3,500	15166739	102904	5,100	6,310	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,893	34734659	209999	11,680	12,877	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	8,212	57347275	333411	19,284	20,445	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	11,195	75895578	441598	25,522	27,079	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	14,000	114231219	542856	38,413	33,288	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

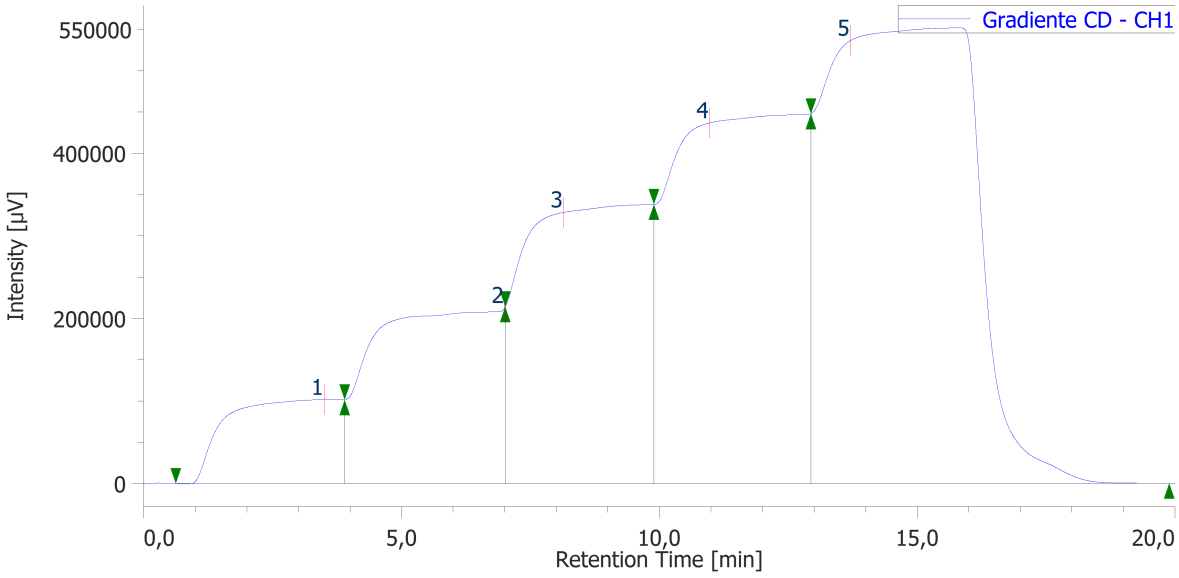

Chromatogram Information	
User Name	QPackSA
Date Modified	13/12/2022 17:36:23
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2022 15:23:46
Volume	0,1 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	20%	1	3,500	15077337	101625	5,097	6,297	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,995	35607776	212363	12,037	13,158	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	8,138	55161837	328099	18,647	20,329	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	10,963	78014104	436140	26,373	27,023	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	13,700	111954484	535751	37,846	33,194	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver