
Chromatogram

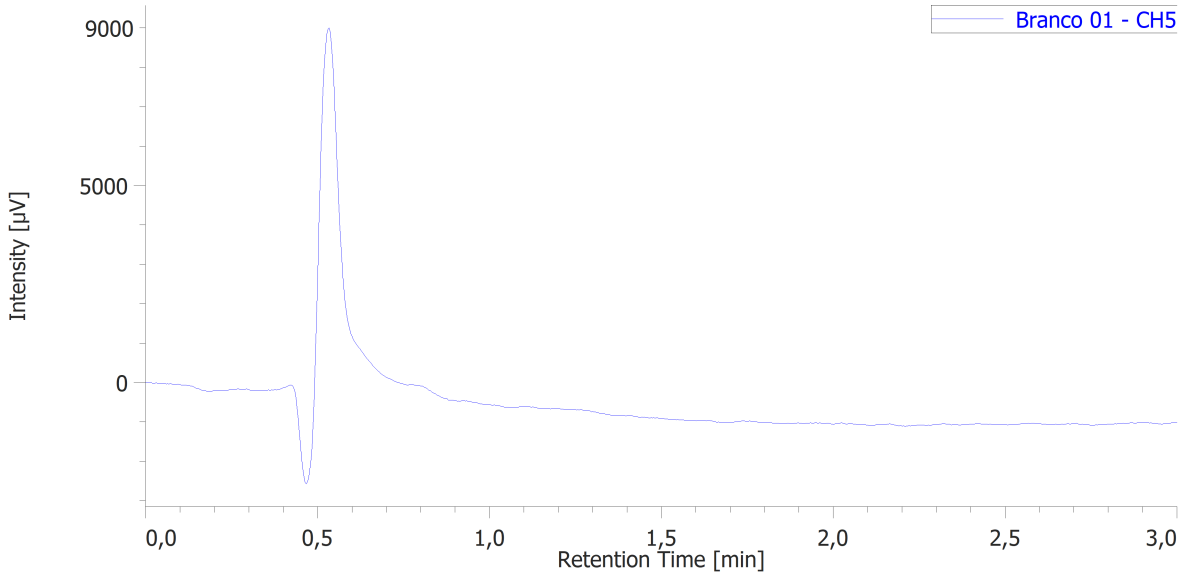


Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:32
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:09:48
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

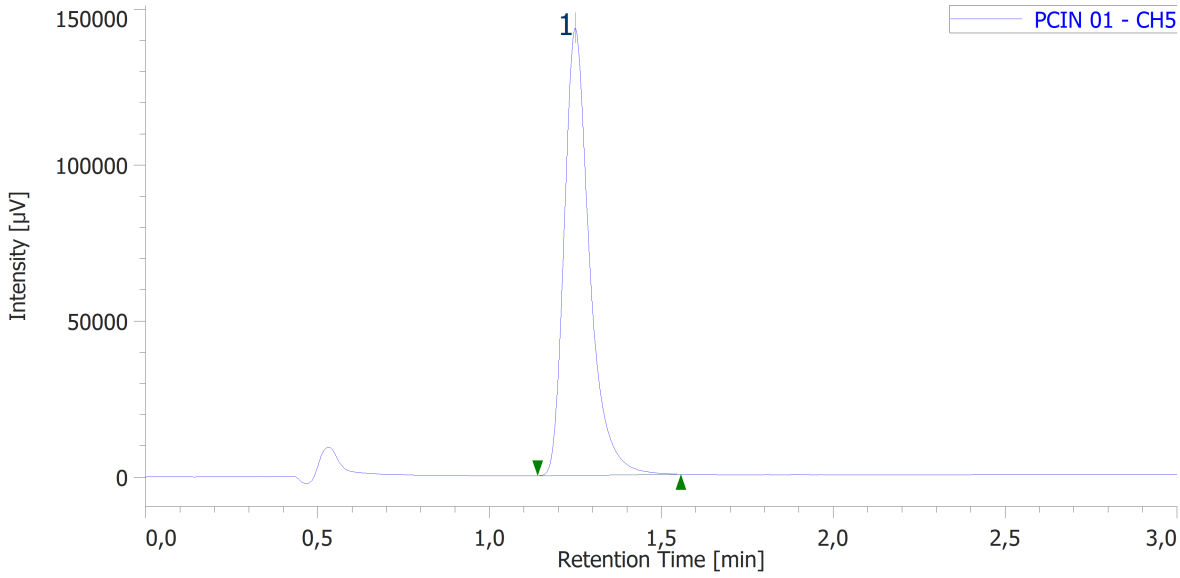

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:34
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:13:00
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,250	733645	143384	100,000	100,000	N/A	1550	N/A	1,369	

Creator QPackSA
Reviewer
Approver

Chromatogram

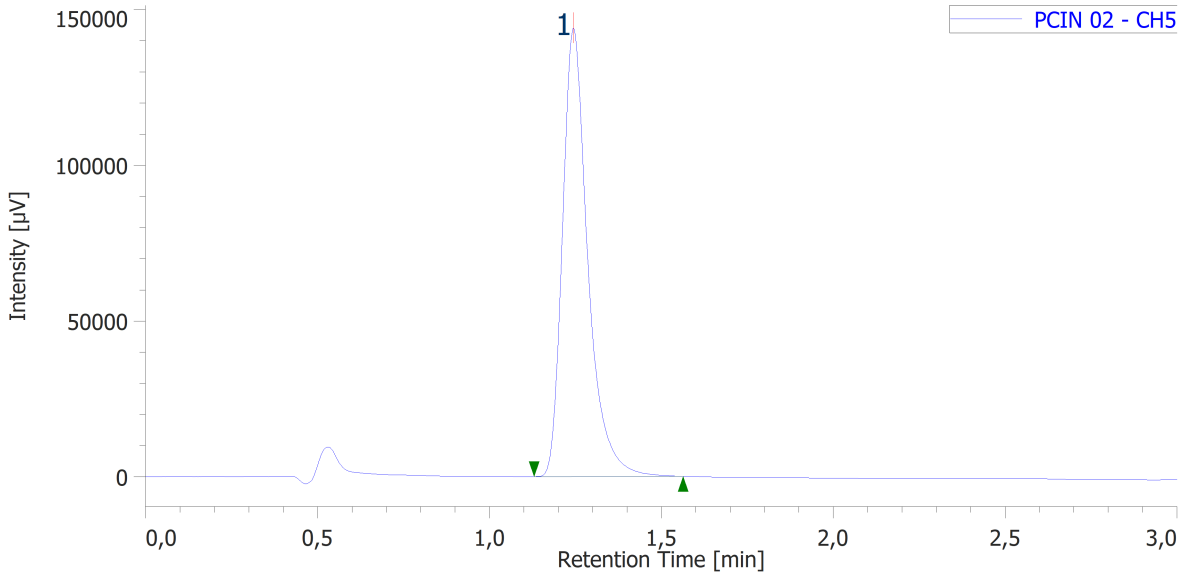

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:34
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:16:12
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,243	736932	143975	100,000	100,000	N/A	1538	N/A	1,408	

Creator QPackSA
Reviewer
Approver

Chromatogram

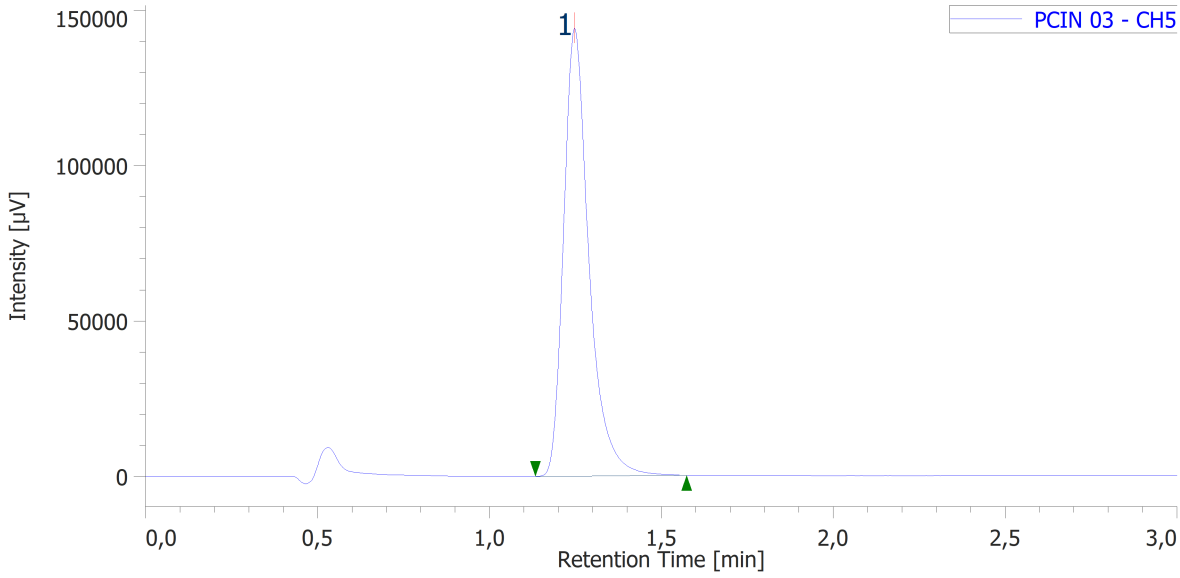

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:34
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:19:24
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,247	737435	144098	100,000	100,000	N/A	1546	N/A	1,404	

Creator QPackSA
Reviewer
Approver

Chromatogram

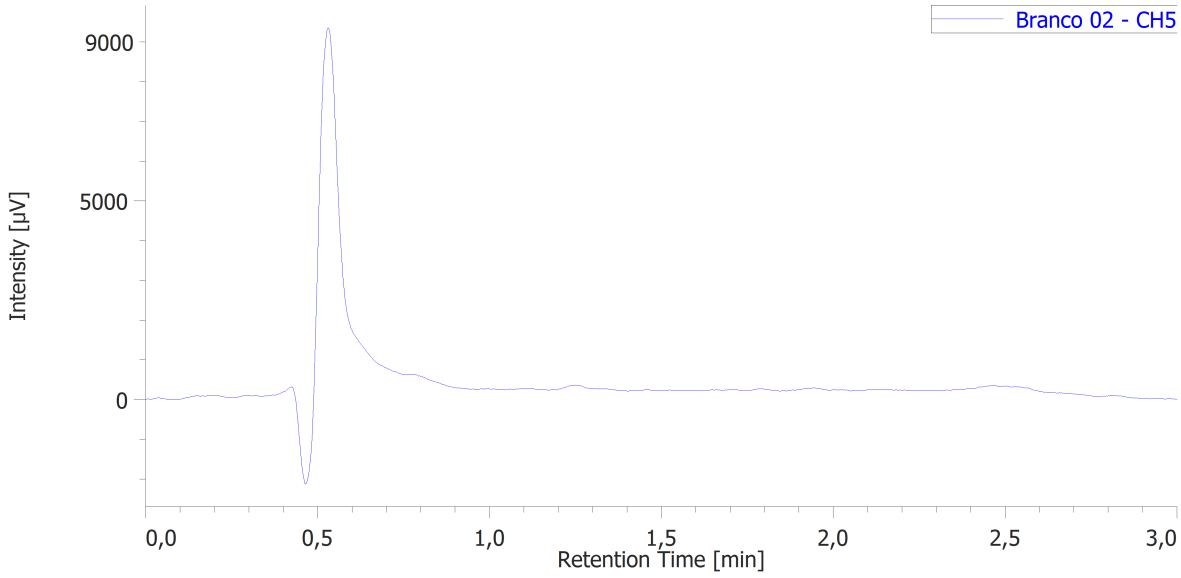


Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:34
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:22:36
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

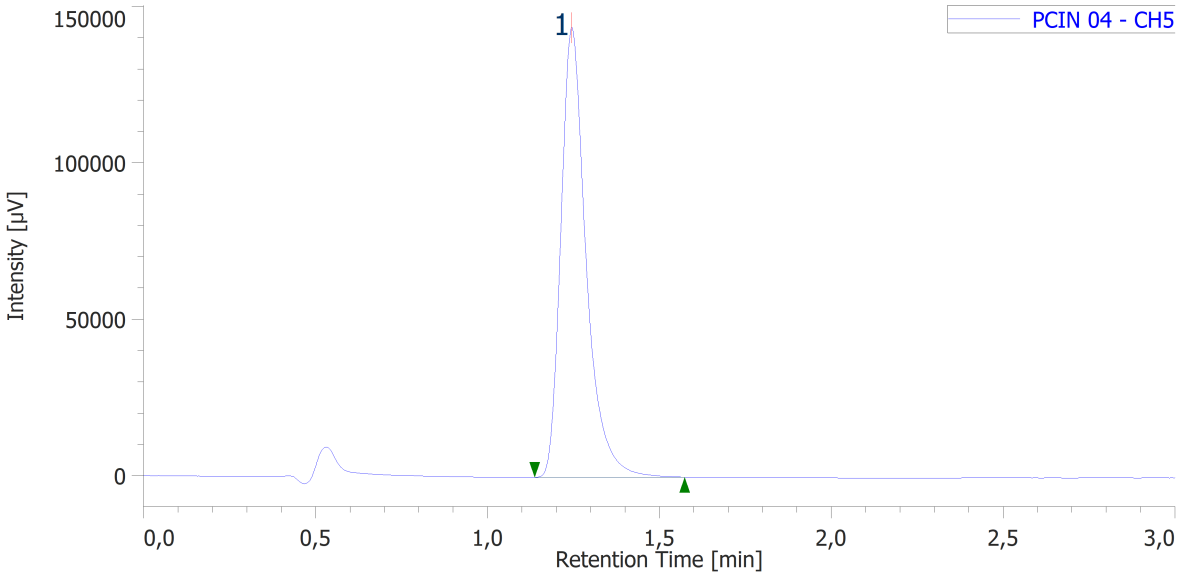

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:34
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:25:48
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,243	733651	143568	100,000	100,000	N/A	1541	N/A	1,427	

Creator QPackSA
Reviewer
Approver

Chromatogram

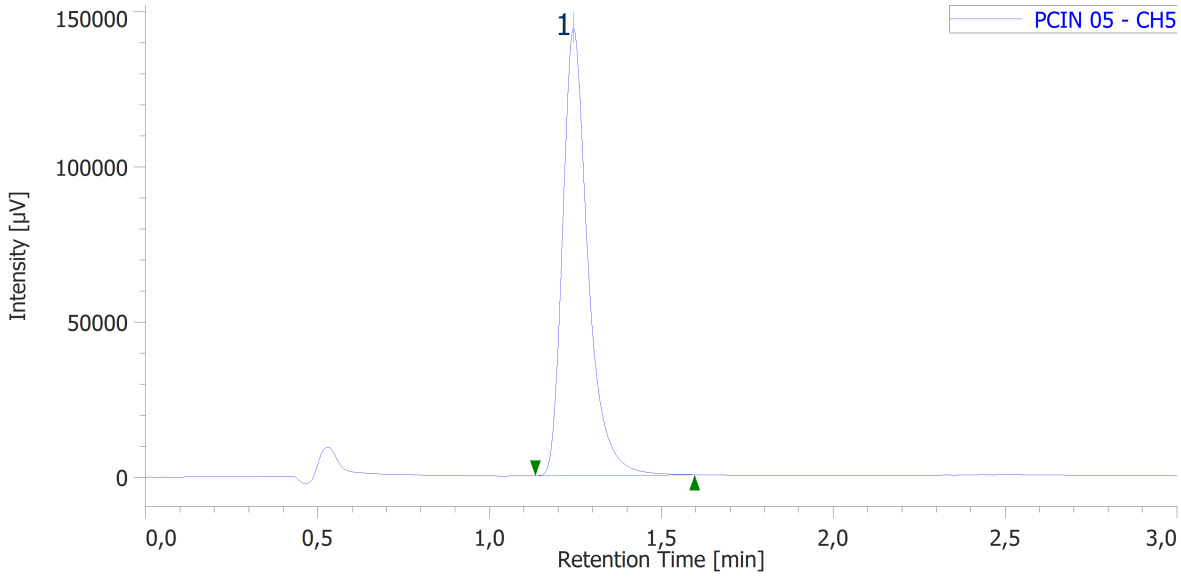

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:35
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:29:00
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,243	738006	144268	100,000	100,000	N/A	1544	N/A	1,413	

Creator QPackSA
Reviewer
Approver

Chromatogram

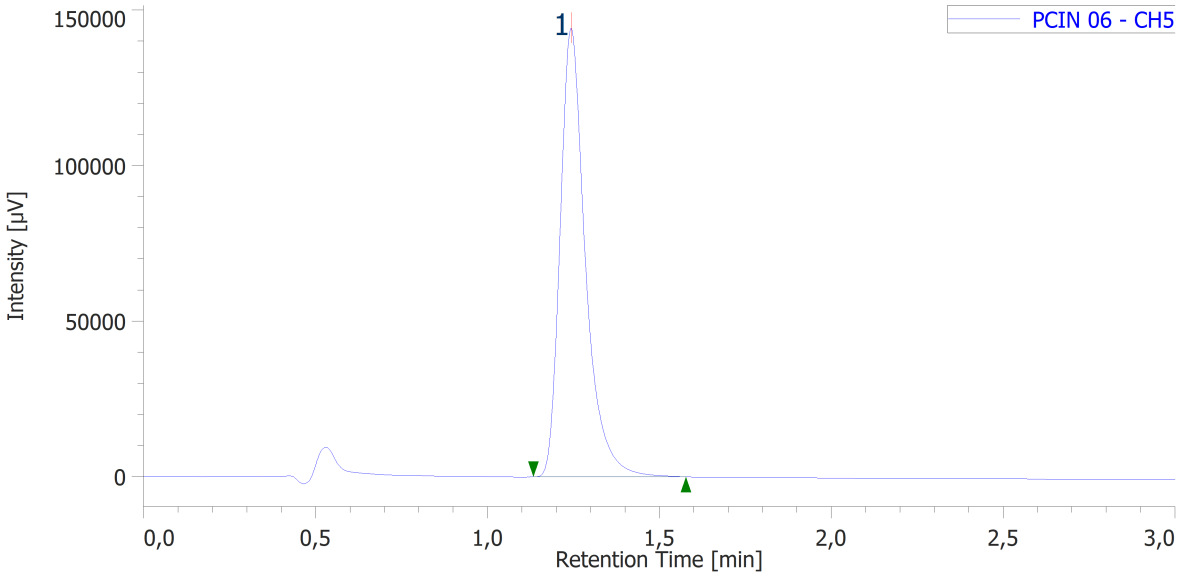

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:36:53
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:32:12
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,243	737275	144228	100,000	100,000	N/A	1546	N/A	1,386	

Creator QPackSA
Reviewer
Approver

Chromatogram

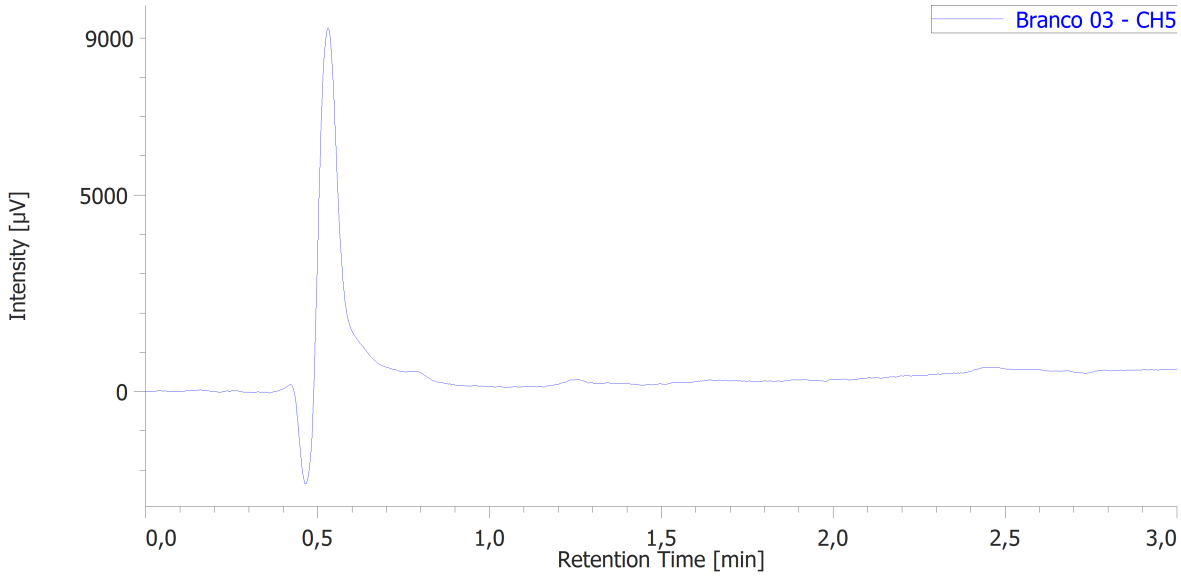


Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:30
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:35:24
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

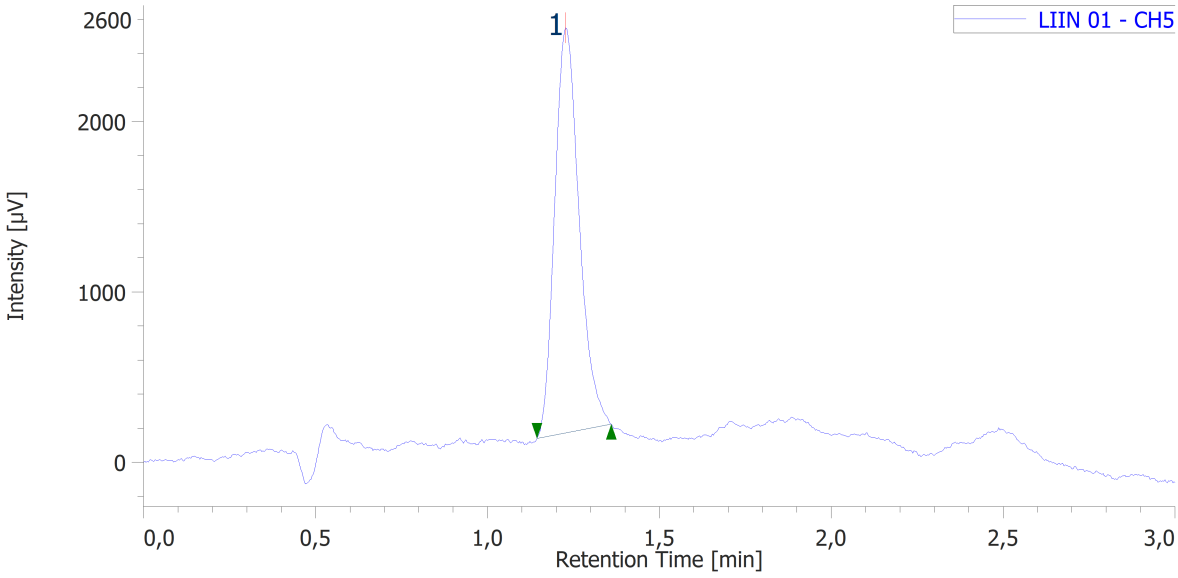

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:30
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:38:36
Volume	0,1 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,227	11757	2378	100,000	100,000	N/A	1442	N/A	1,272	

Creator QPackSA
Reviewer
Approver

Chromatogram

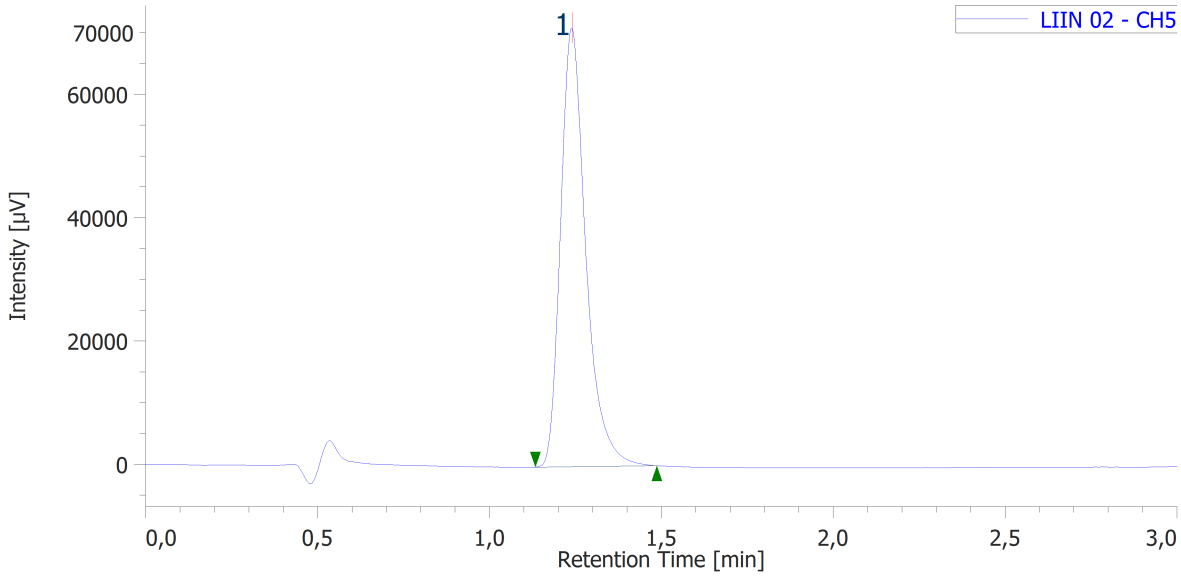

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:30
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:41:48
Volume	5,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,240	362097	71109	100,000	100,000	N/A	1509	N/A	1,341	

Creator QPackSA
Reviewer
Approver

Chromatogram

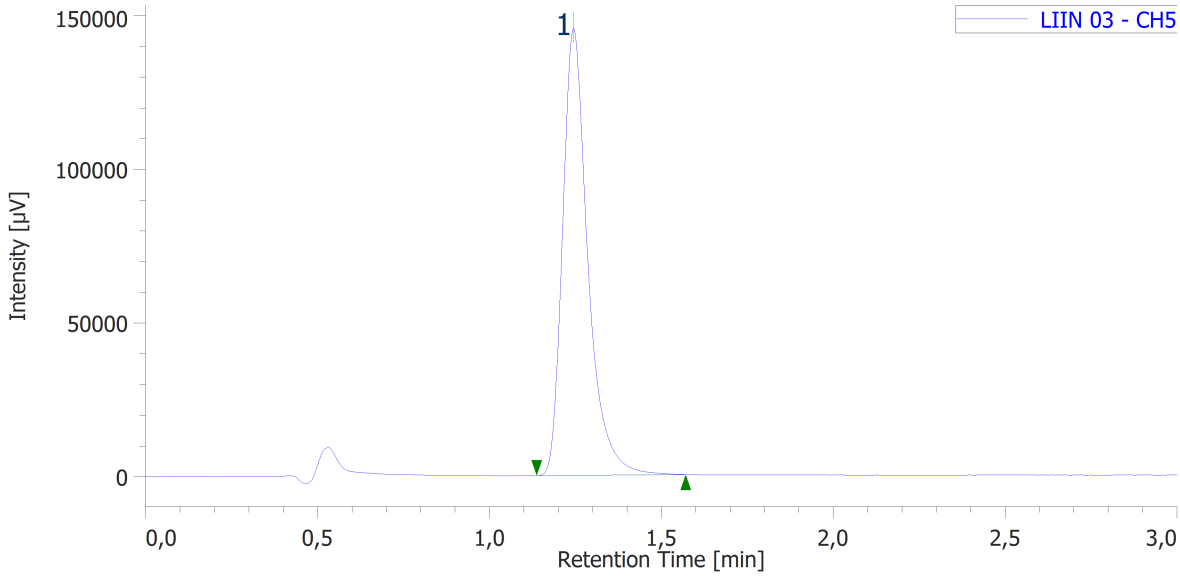

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:30
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:45:00
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,243	742304	145477	100,000	100,000	N/A	1549	N/A	1,410	

Creator QPackSA
Reviewer
Approver

Chromatogram

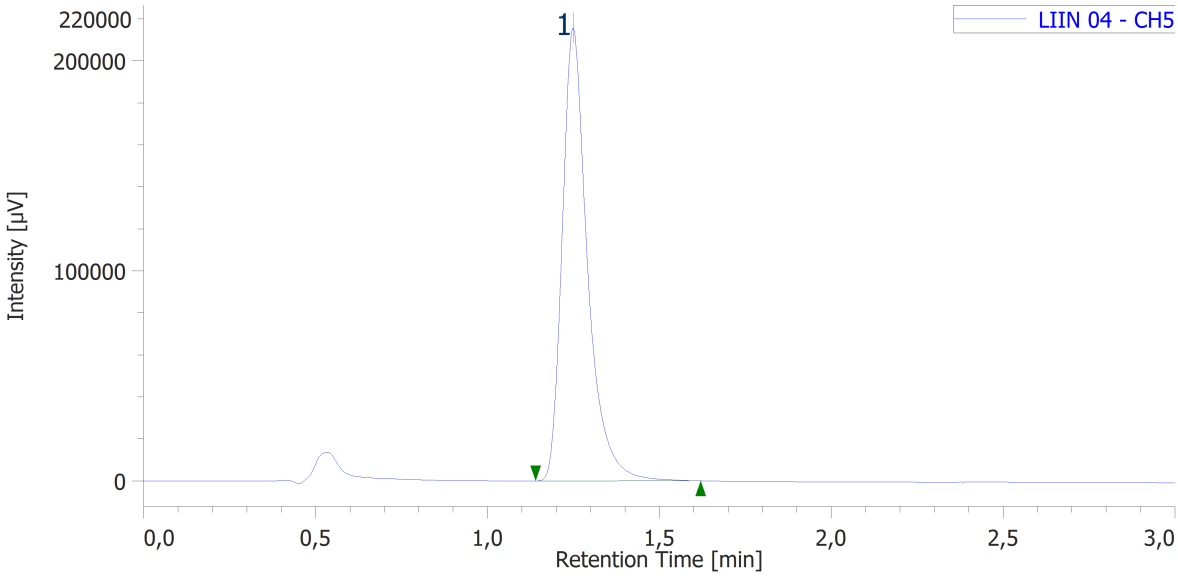

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:30
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:48:12
Volume	15,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,250	1103023	215602	100,000	100,000	N/A	1583	N/A	1,384	

Creator QPackSA
Reviewer
Approver

Chromatogram

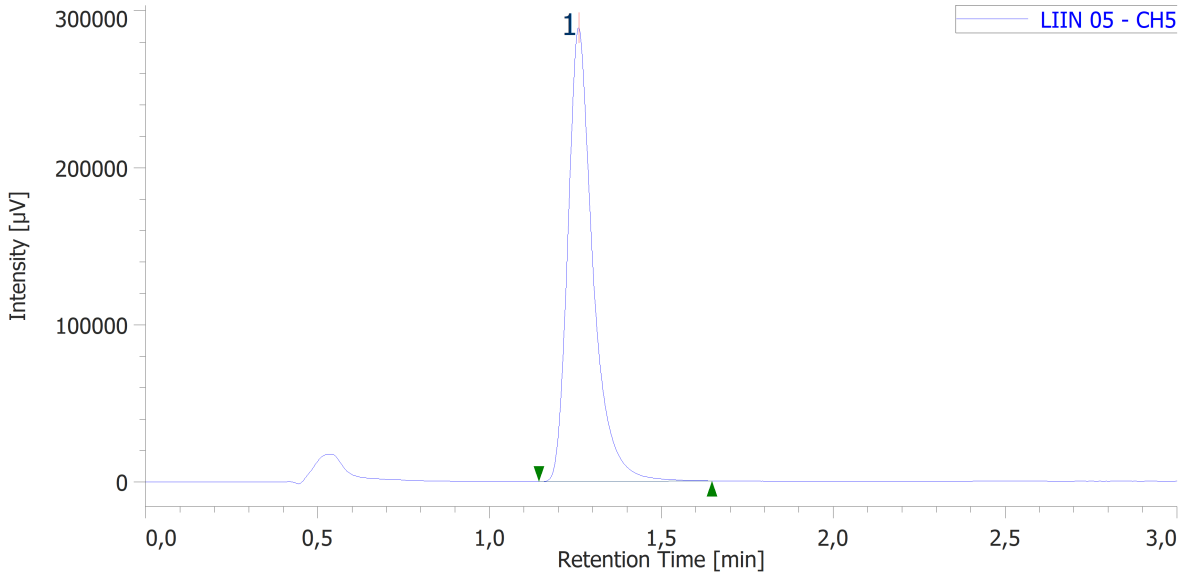

Chromatogram Information	
User Name	QPackSA
Date Modified	28/10/2024 12:55:31
Description	
HPLC System Name	01-HP-03
Injection Date	28/10/2024 12:51:24
Volume	20,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação Injetor
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,260	1460485	288525	100,000	100,000	N/A	1660	N/A	1,388	

Creator QPackSA
Reviewer
Approver