
Chromatogram and Results

Injection Details

Injection Name:	**BRANCO 01**	*Run Time (min):*	**2.00**
Vial Number:	**20**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:02**	*Sample Weight:*	**1.0000**

Chromatogram

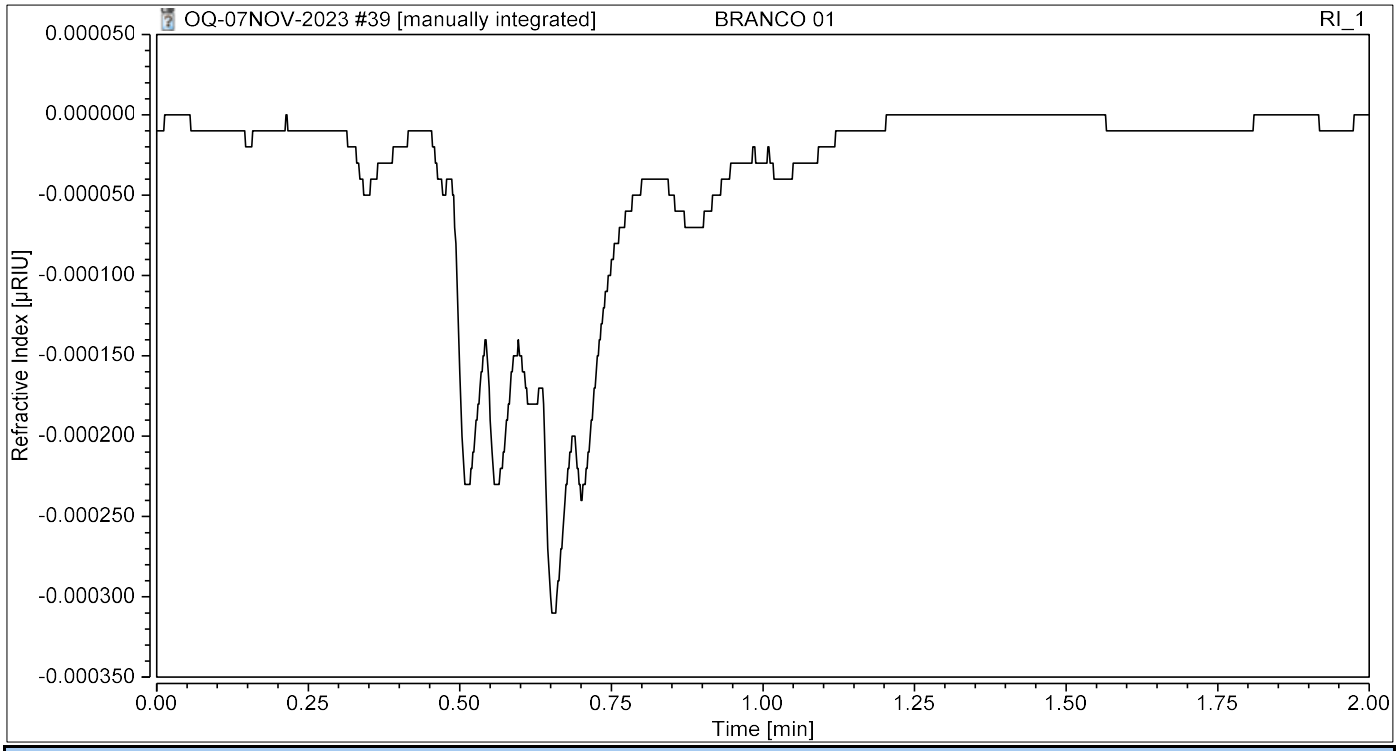

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
n.a.	Component 1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.00**	**0.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:06**	*Sample Weight:*	**1.0000**

Chromatogram

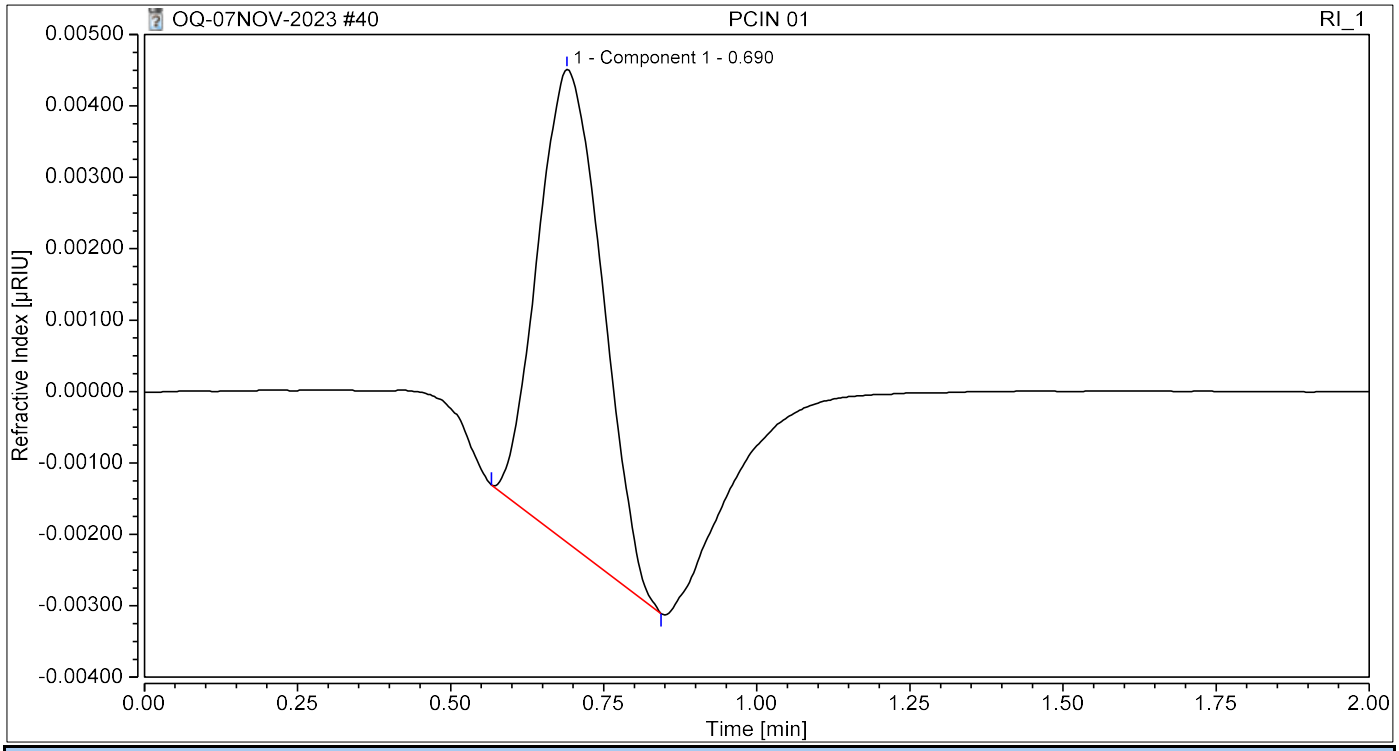

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.690	0.000813	0.007	100.00	100.00	n.a.
Total:			**0.001**	**0.007**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:09**	*Sample Weight:*	**1.0000**

Chromatogram

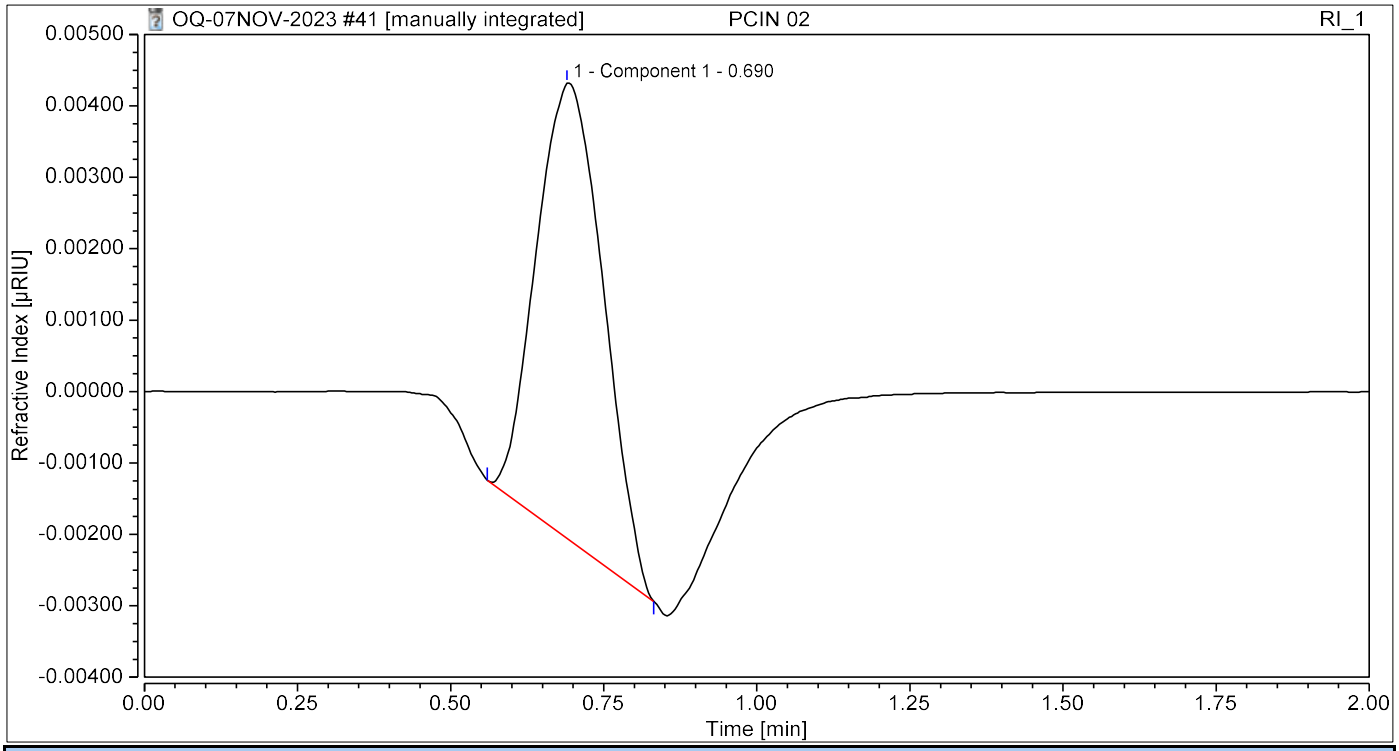

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.690	0.000813	0.006	100.00	100.00	n.a.
Total:			**0.001**	**0.006**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:13**	*Sample Weight:*	**1.0000**

Chromatogram

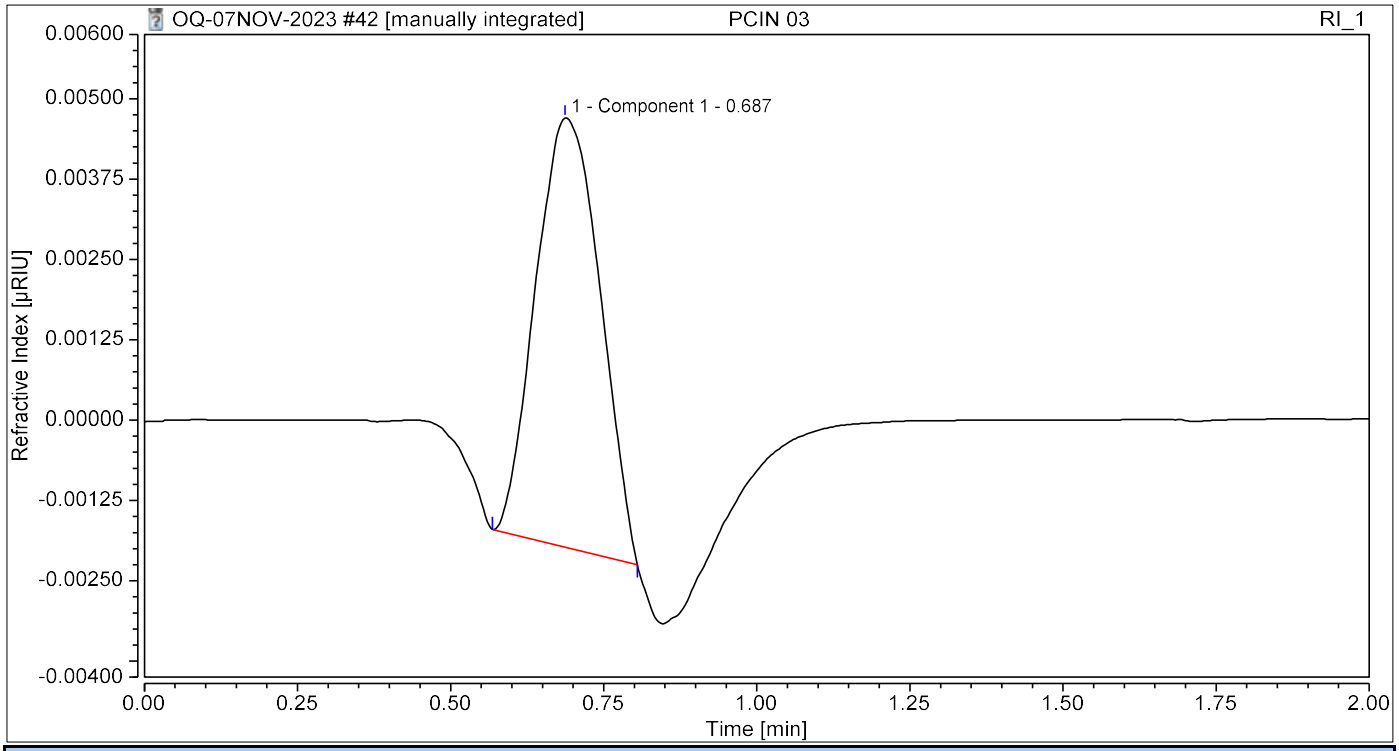

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.687	0.000818	0.007	100.00	100.00	n.a.
Total:			**0.001**	**0.007**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**BRANCO 02**	*Run Time (min):*	**2.00**
Vial Number:	**20**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:16**	*Sample Weight:*	**1.0000**

Chromatogram

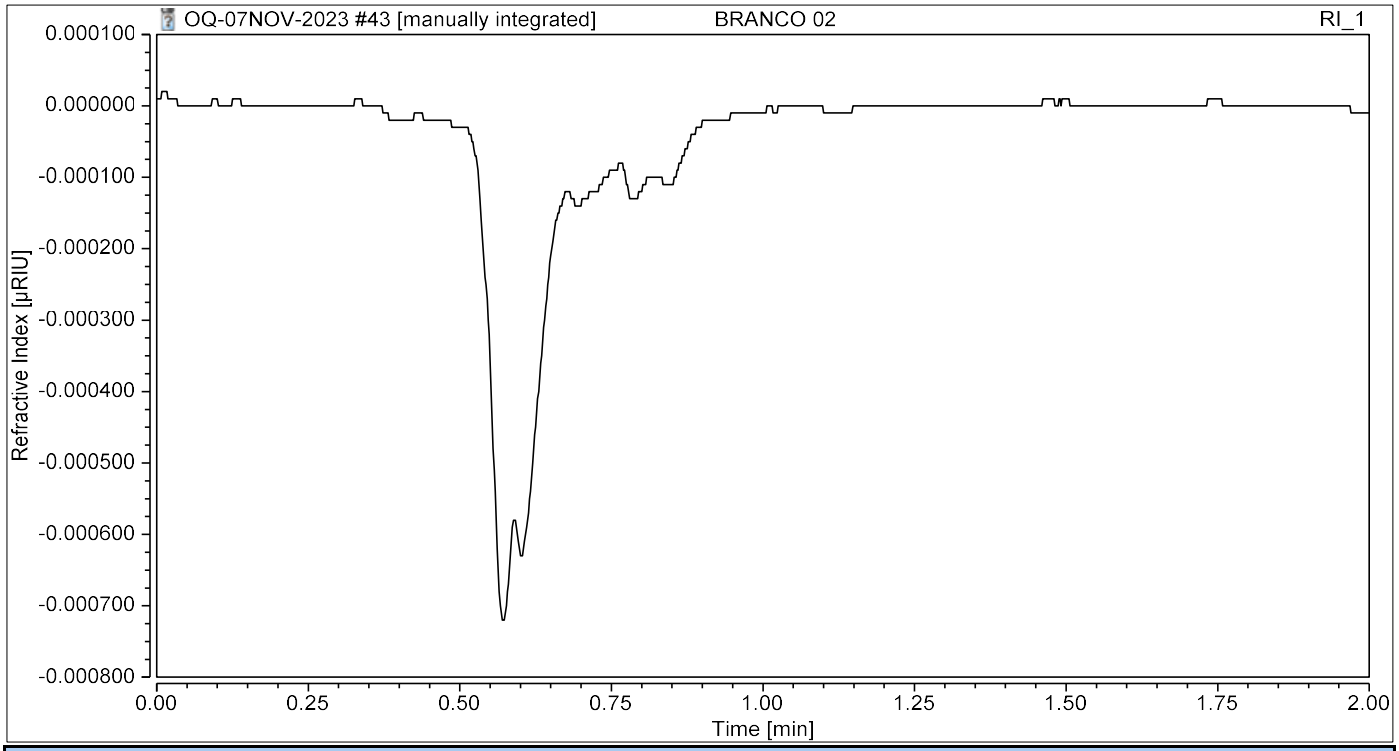

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
n.a.	Component 1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.00**	**0.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:20**	*Sample Weight:*	**1.0000**

Chromatogram

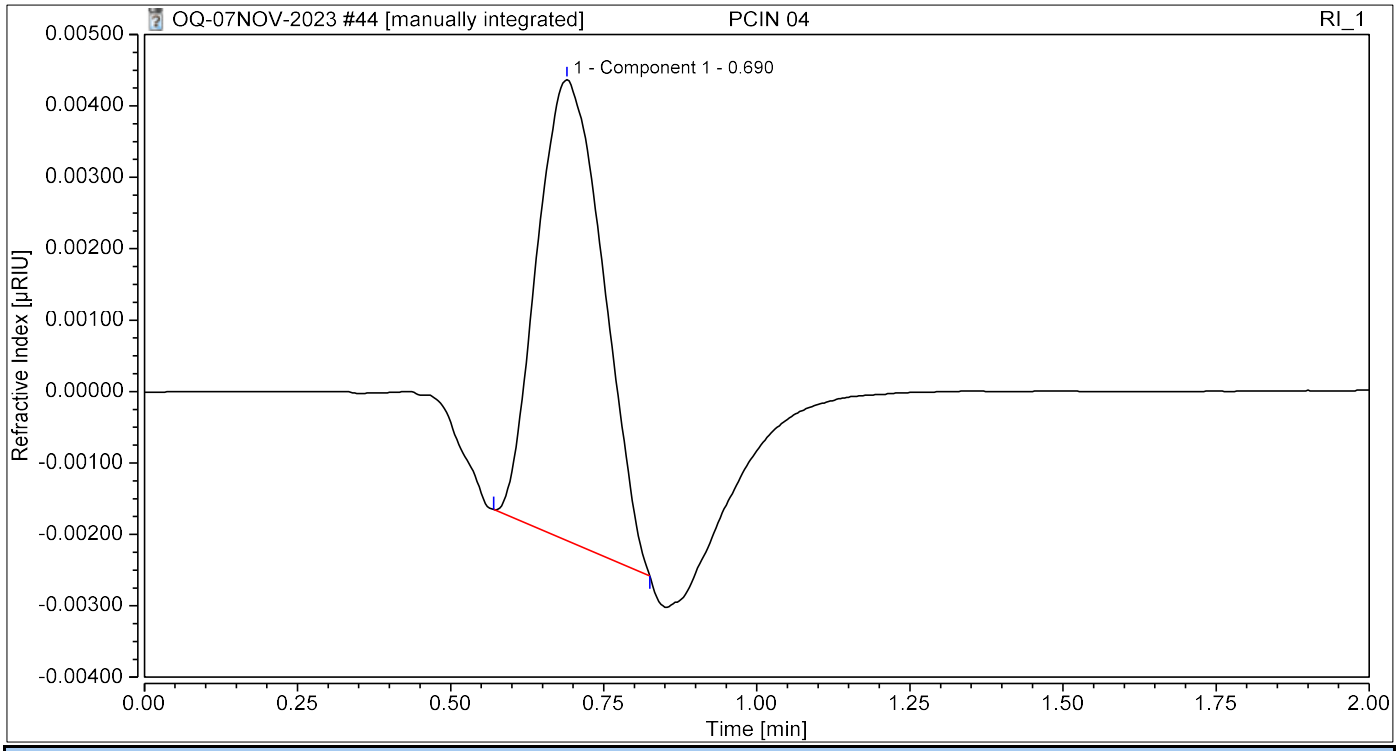

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.690	0.000814	0.006	100.00	100.00	n.a.
Total:			**0.001**	**0.006**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:23**	*Sample Weight:*	**1.0000**

Chromatogram

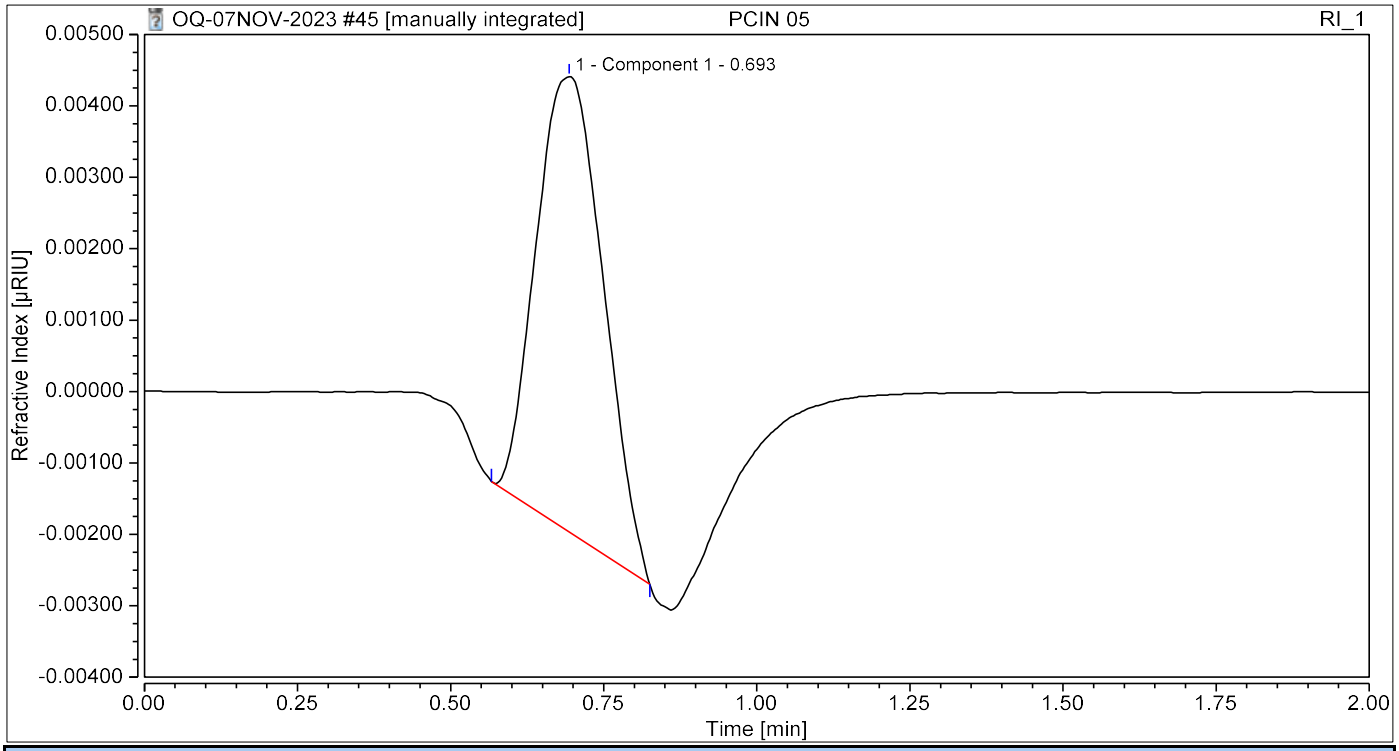

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.693	0.000813	0.006	100.00	100.00	n.a.
Total:			**0.001**	**0.006**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**2.00**
Vial Number:	**5**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:26**	*Sample Weight:*	**1.0000**

Chromatogram

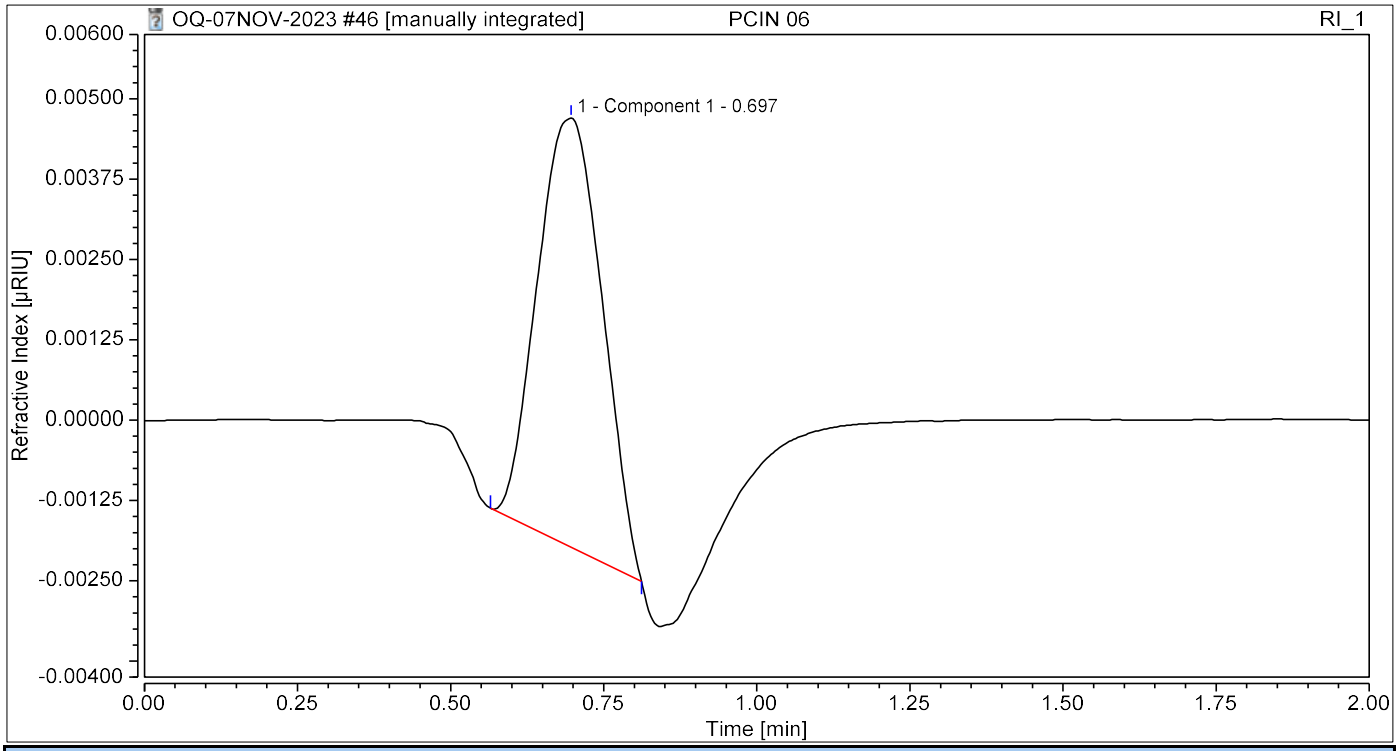

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.697	0.000819	0.007	100.00	100.00	n.a.
Total:			**0.001**	**0.007**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**BRANCO 03**	*Run Time (min):*	**2.00**
Vial Number:	**20**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 11:30**	*Sample Weight:*	**1.0000**

Chromatogram

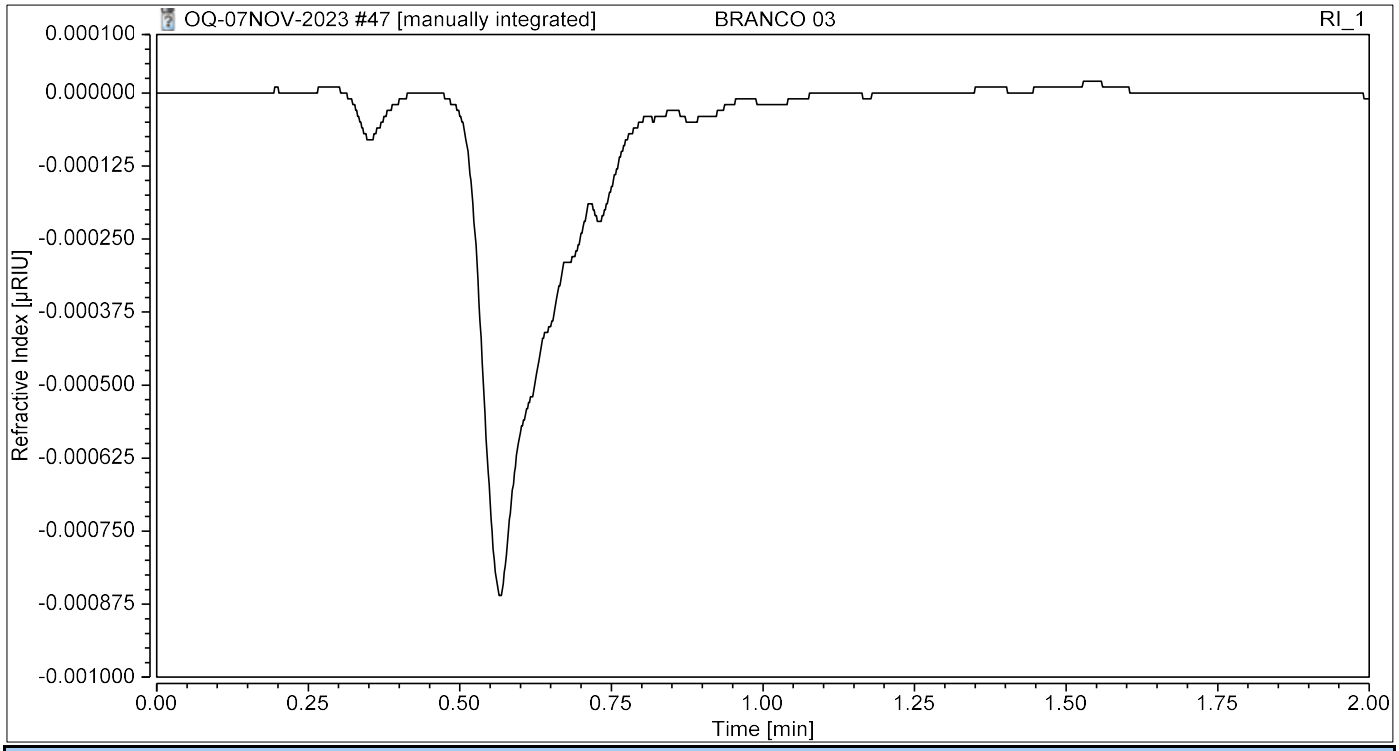

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
n.a.	Component 1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.00**	**0.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 01**	*Run Time (min):*	**2.00**
Vial Number:	**0**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 09:23**	*Sample Weight:*	**1.0000**

Chromatogram

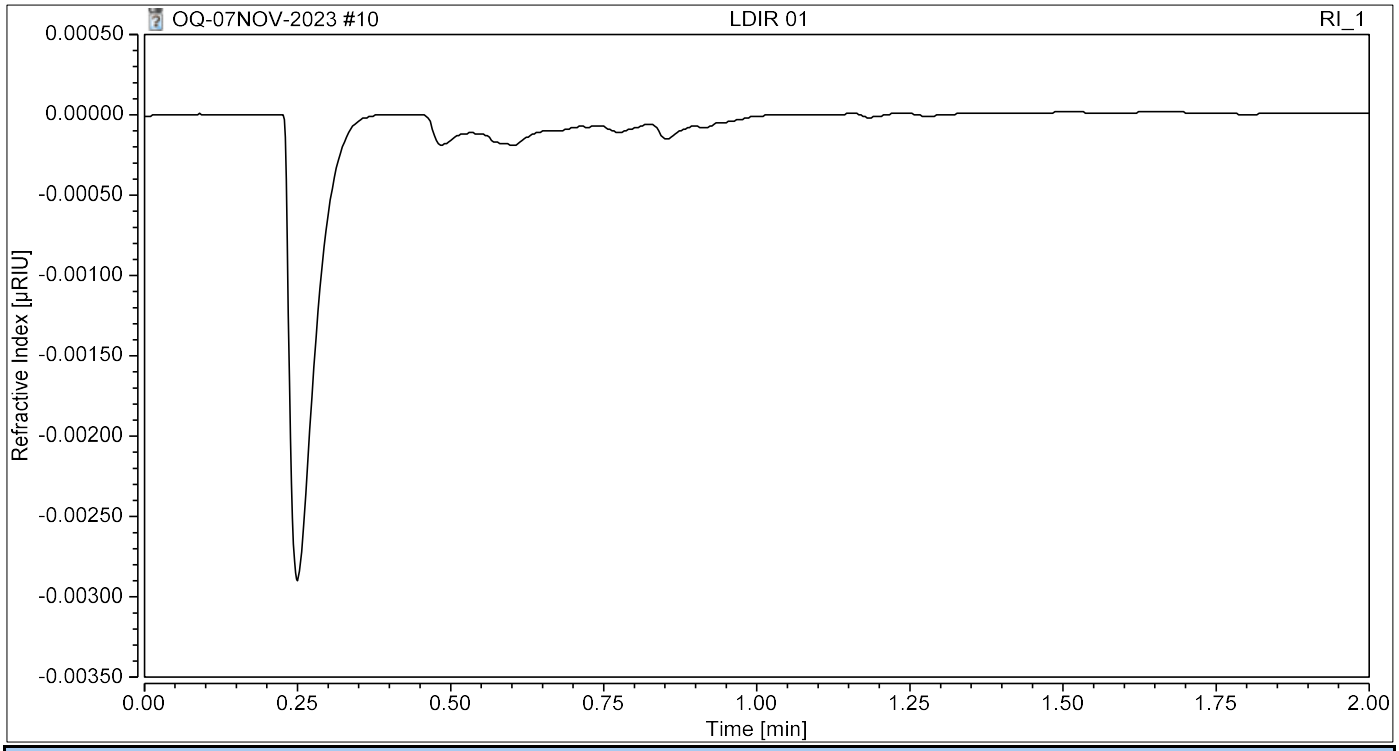

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
n.a.	Component 1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0.000**	**0.000**	**0.00**	**0.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 02**	*Run Time (min):*	**2.00**
Vial Number:	**1**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 09:26**	*Sample Weight:*	**1.0000**

Chromatogram

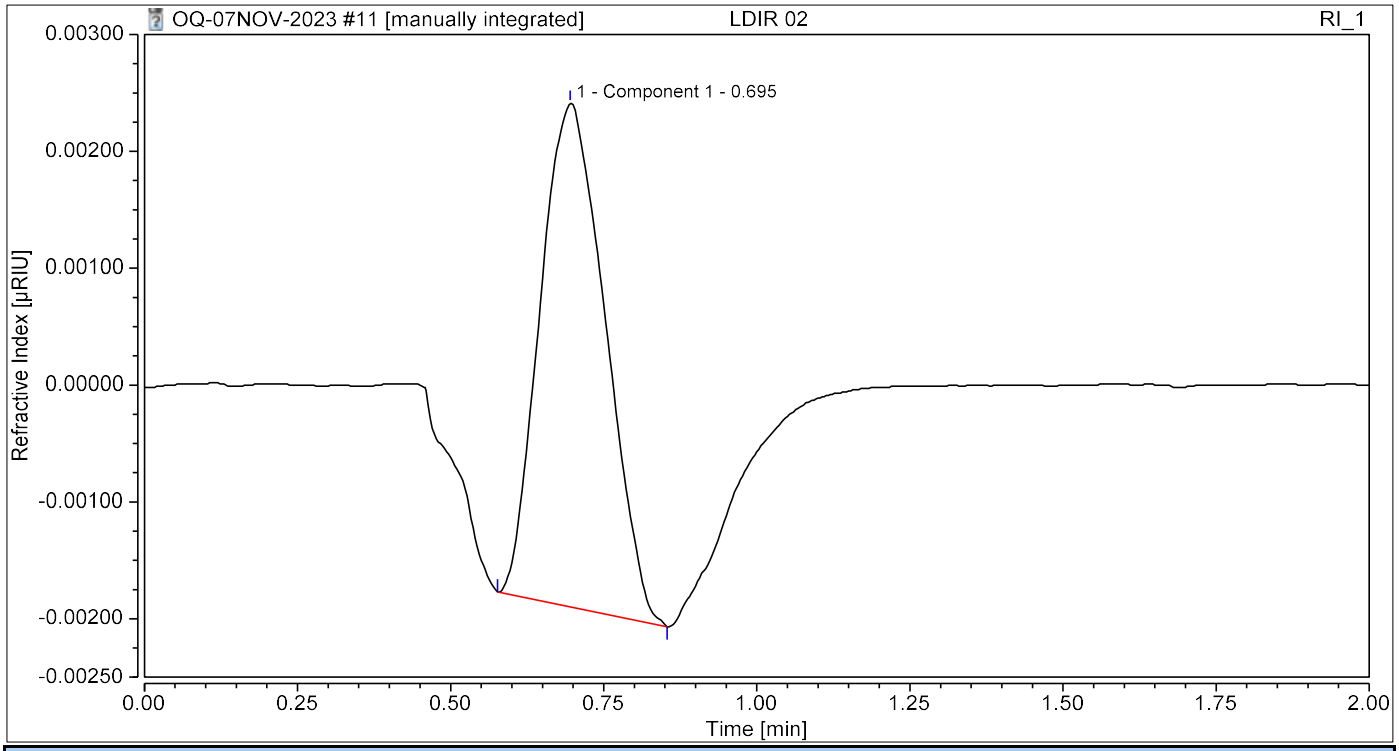

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.695	0.000531	0.004	100.00	100.00	n.a.
Total:			**0.001**	**0.004**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 03**	*Run Time (min):*	**2.00**
Vial Number:	**2**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 09:29**	*Sample Weight:*	**1.0000**

Chromatogram

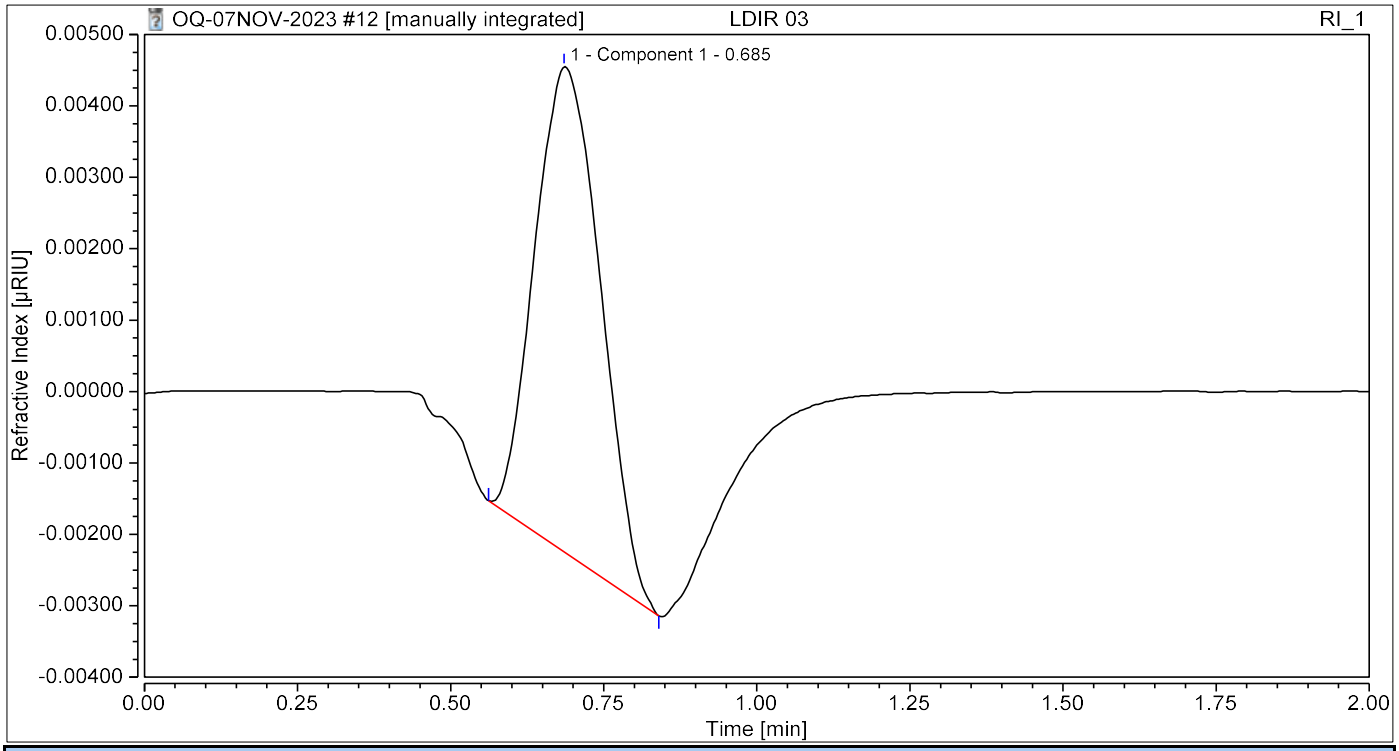

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.685	0.000851	0.007	100.00	100.00	n.a.
Total:			**0.001**	**0.007**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 04**	*Run Time (min):*	**2.00**
Vial Number:	**3**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 09:33**	*Sample Weight:*	**1.0000**

Chromatogram

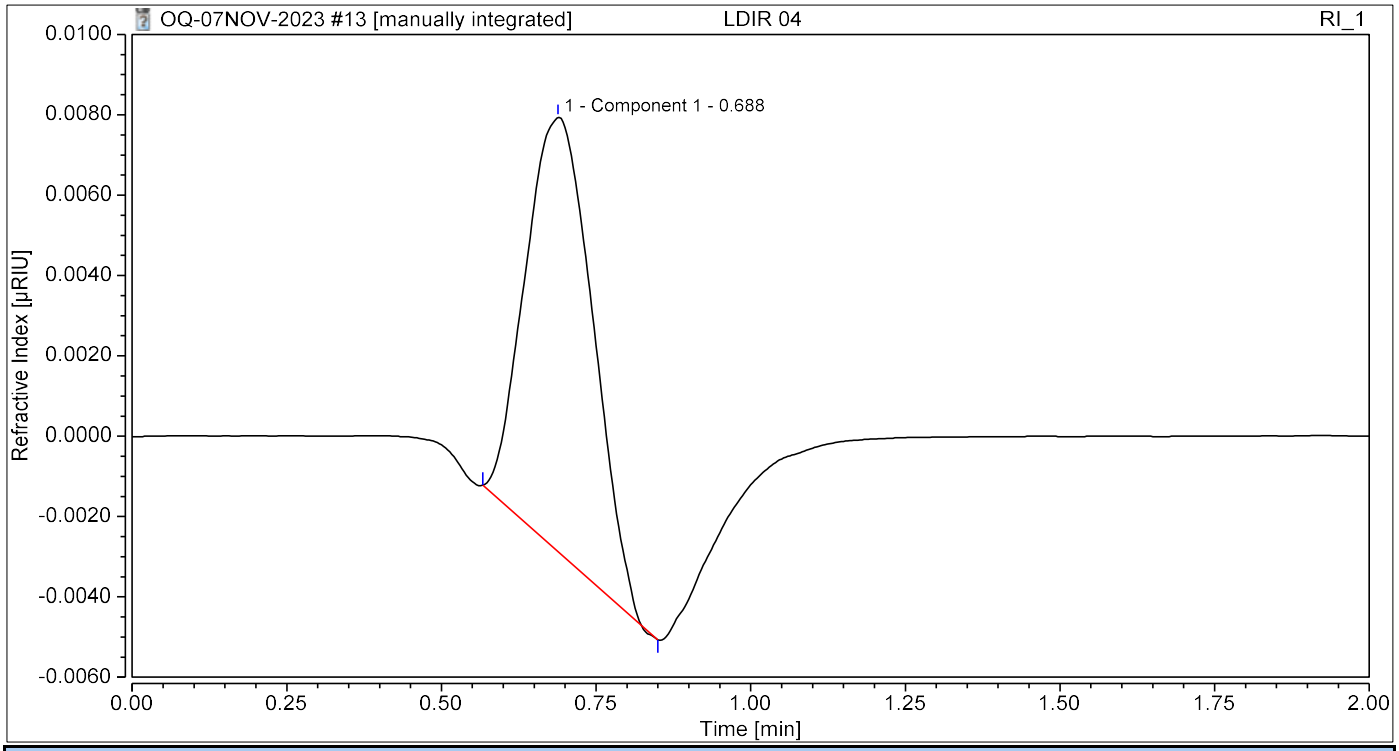

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.688	0.001372	0.011	100.00	100.00	n.a.
Total:			**0.001**	**0.011**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDIR 05**	*Run Time (min):*	**2.00**
Vial Number:	**4**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 09:36**	*Sample Weight:*	**1.0000**

Chromatogram

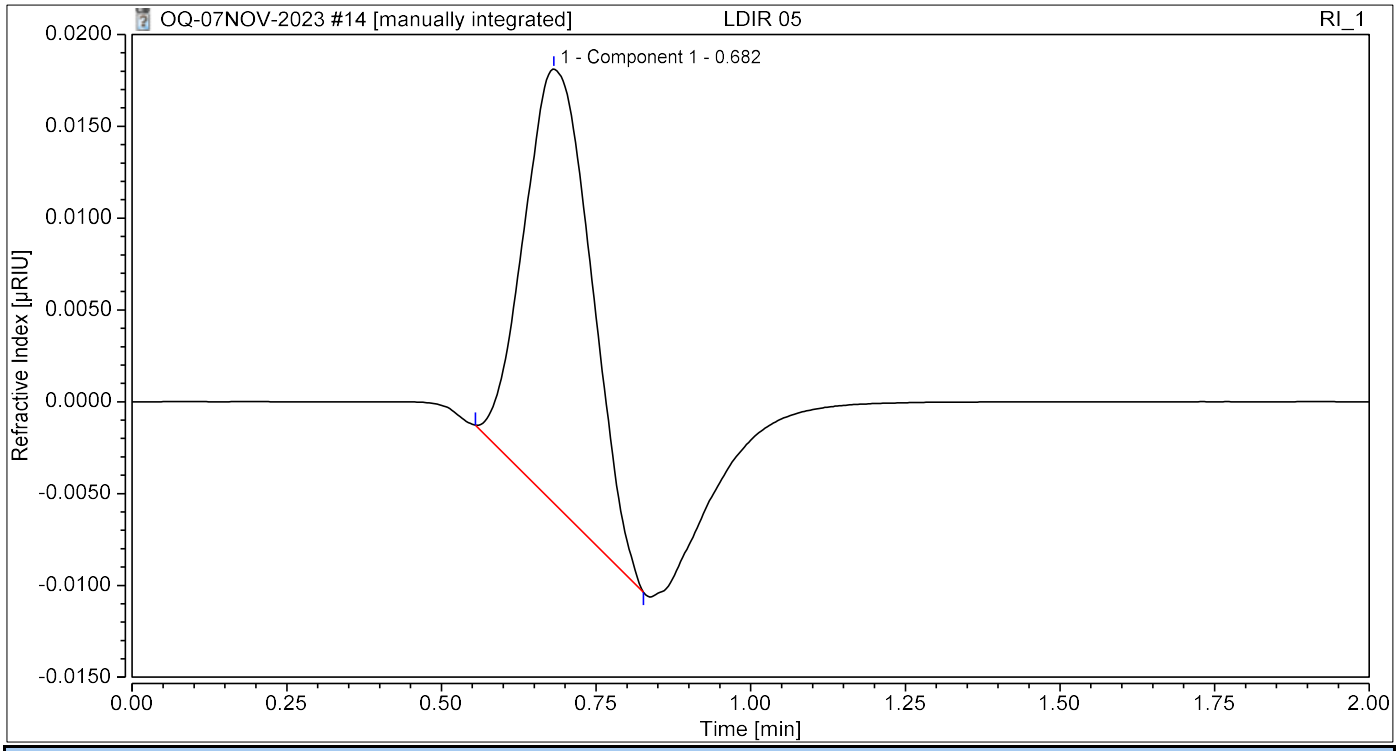

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.682	0.003011	0.024	100.00	100.00	n.a.
Total:			**0.003**	**0.024**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**2.00**
Vial Number:	**6**	*Injection Volume:*	**1.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 10:45**	*Sample Weight:*	**1.0000**

Chromatogram

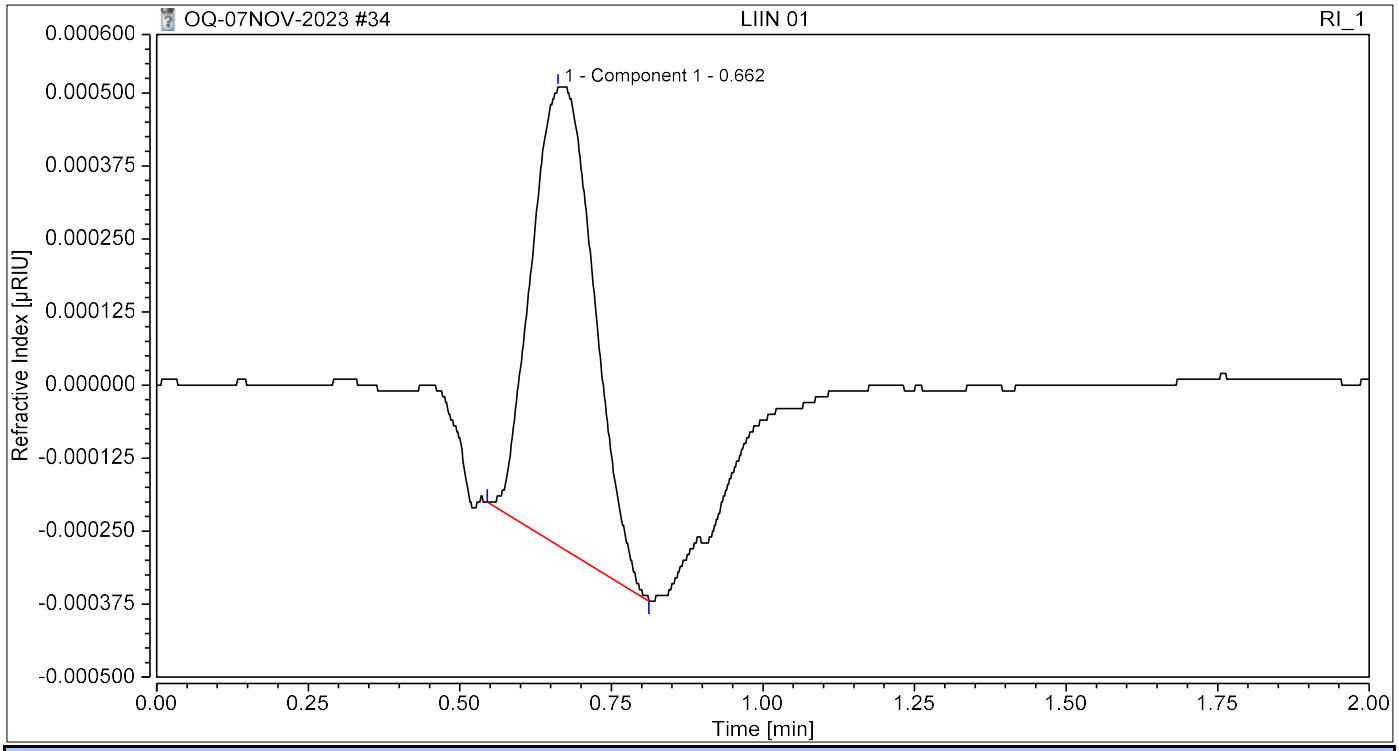

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.662	0.000095	0.001	100.00	100.00	n.a.
Total:			**0.000**	**0.001**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**2.00**
Vial Number:	**6**	*Injection Volume:*	**5.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 10:49**	*Sample Weight:*	**1.0000**

Chromatogram

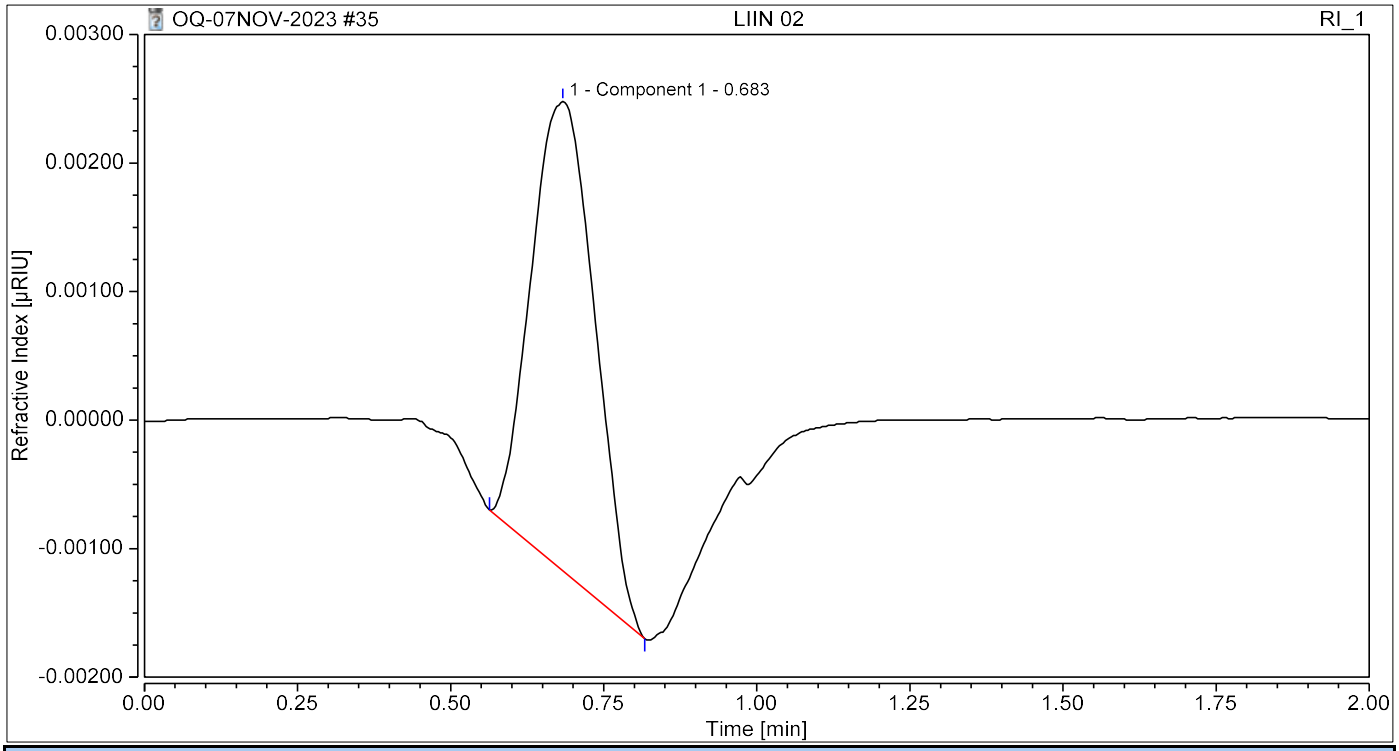

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.683	0.000441	0.004	100.00	100.00	n.a.
Total:			**0.000**	**0.004**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**2.00**
Vial Number:	**6**	*Injection Volume:*	**10.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 10:52**	*Sample Weight:*	**1.0000**

Chromatogram

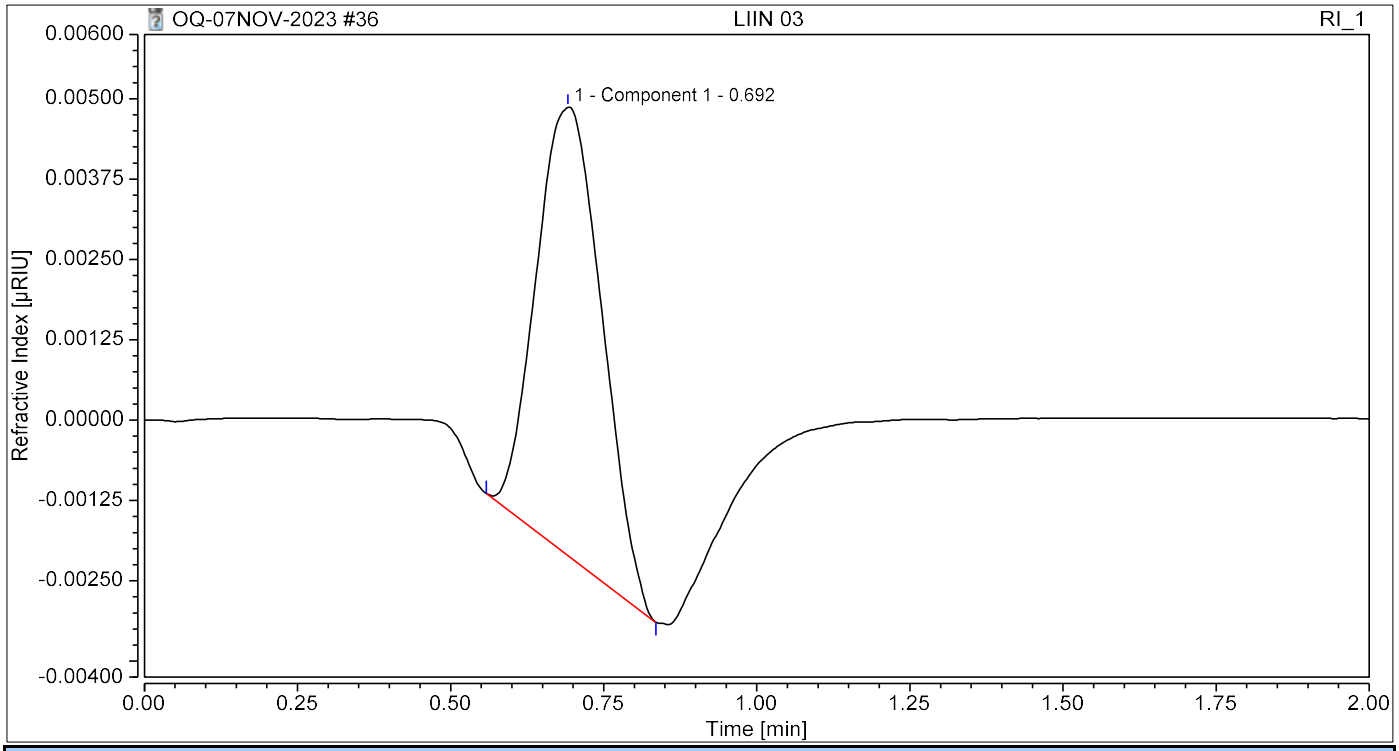

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.692	0.000872	0.007	100.00	100.00	n.a.
Total:			**0.001**	**0.007**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.
Chromeleon 7.3.1.6889

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**2.00**
Vial Number:	**6**	*Injection Volume:*	**15.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 10:55**	*Sample Weight:*	**1.0000**

Chromatogram

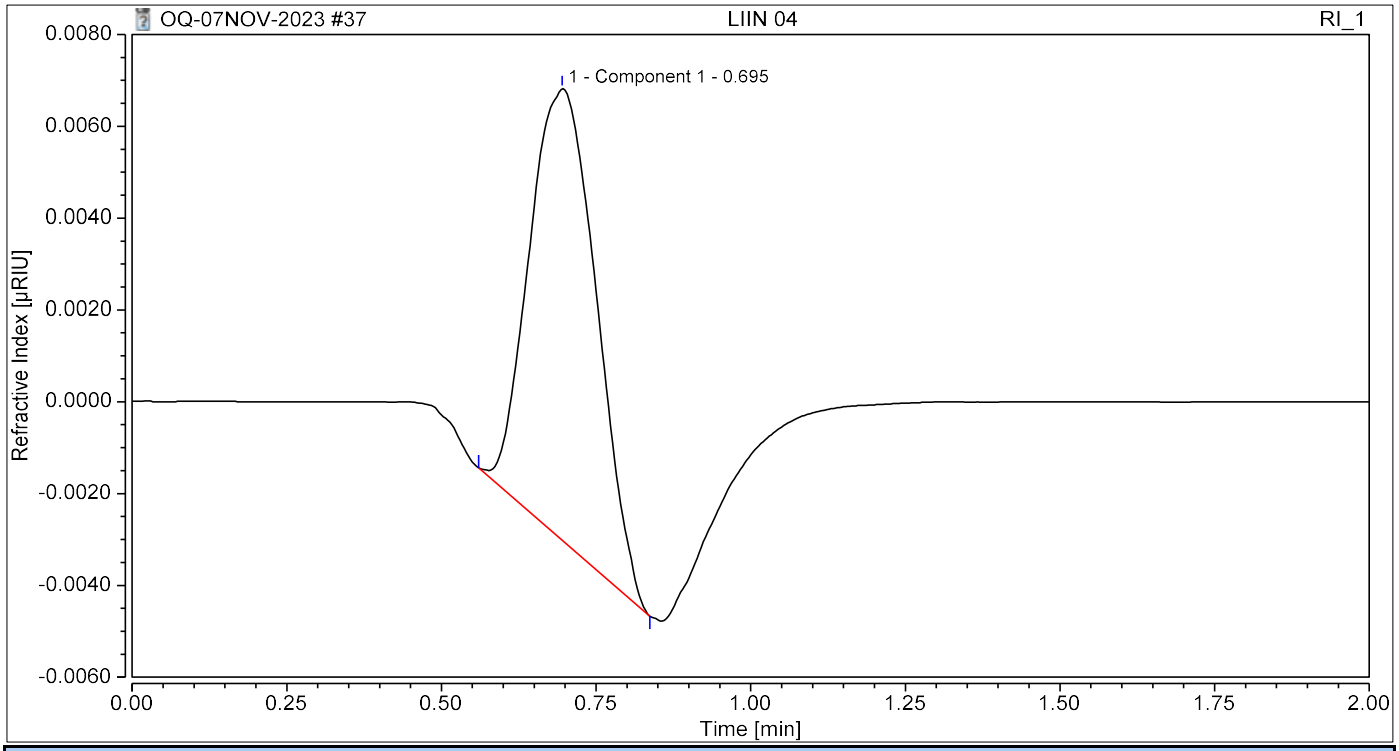

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.695	0.001240	0.010	100.00	100.00	n.a.
Total:			**0.001**	**0.010**	**100.00**	**100.00**	


© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**2.00**
Vial Number:	**6**	*Injection Volume:*	**20.00**
Injection Type:	**Unknown**	*Channel:*	**RI_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação**	*Bandwidth:*	**n.a.**
Processing Method:	**OQ-NOV-2023**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	**08/Nov/23 10:59**	*Sample Weight:*	**1.0000**

Chromatogram

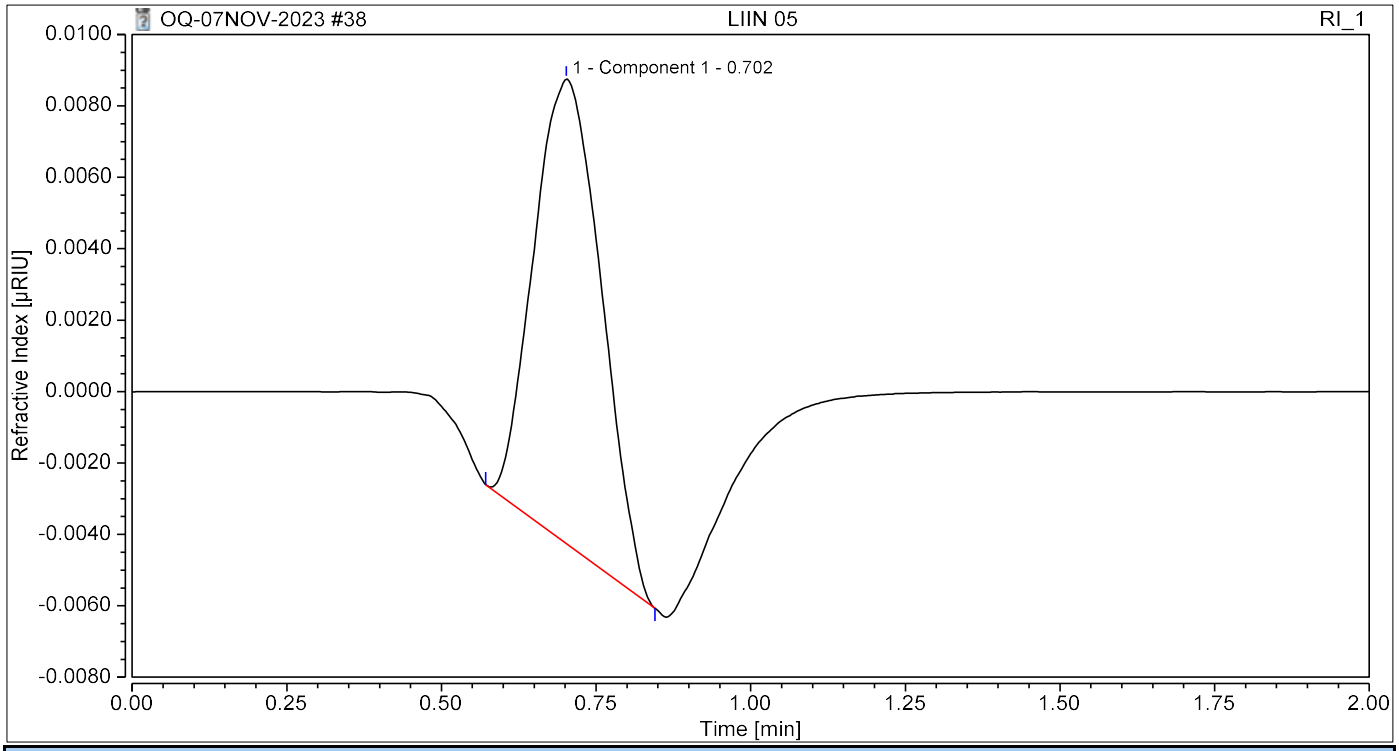

Integration Results

No.	Peak Name	Retention Time min	Area µRIU*min	Height µRIU	Relative Area %	Relative Height %	Amount
1	Component 1	0.702	0.001655	0.013	100.00	100.00	n.a.
Total:			**0.002**	**0.013**	**100.00**	**100.00**	

© 2009-2020 Thermo Fisher Scientific Inc. All rights reserved.