
Peak Find - EDUV_002 UV_tR2,09 D.jws

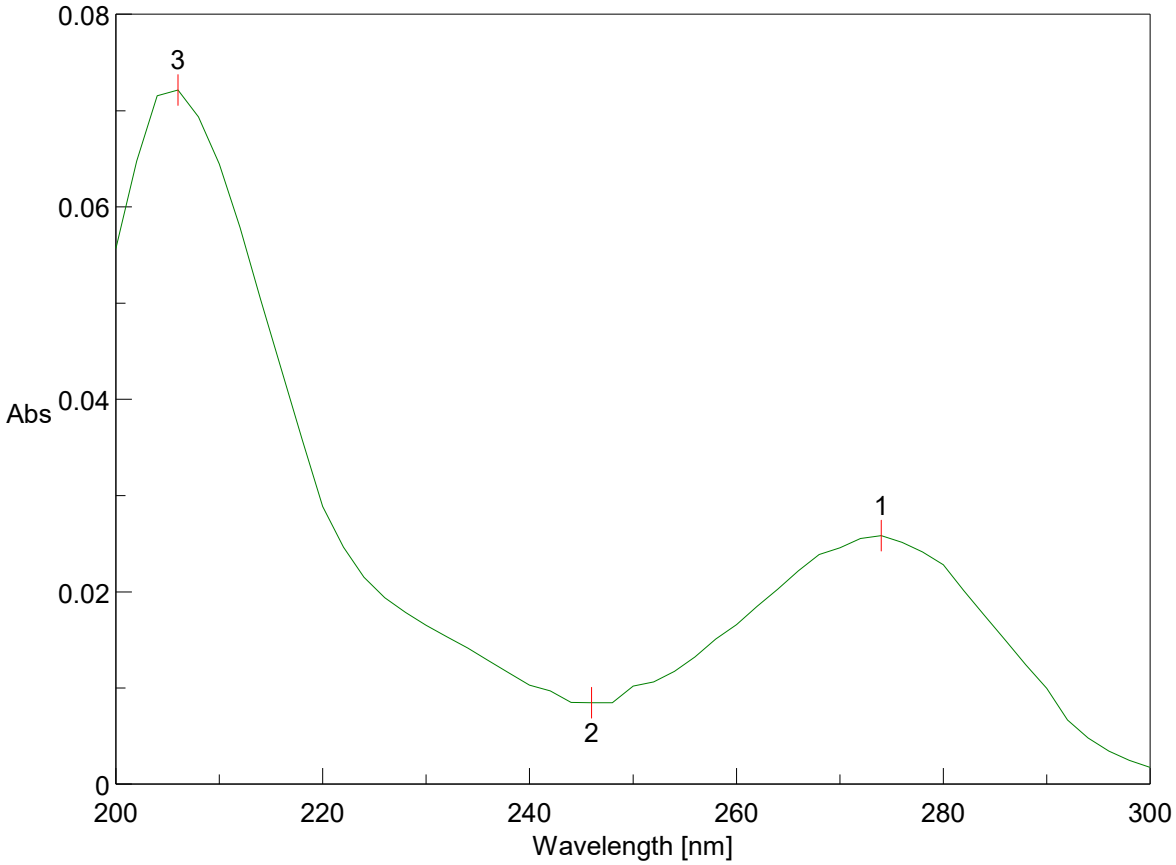

[Comments]

User	Administrator
Division	---
Company	BBA
Creation date	08/11/2023 14:43

[Detailed Information]


Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	86


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	C044061657
ROM version	1.01.16


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0258029	2	246	0.00844812
3	206	0.0721257			

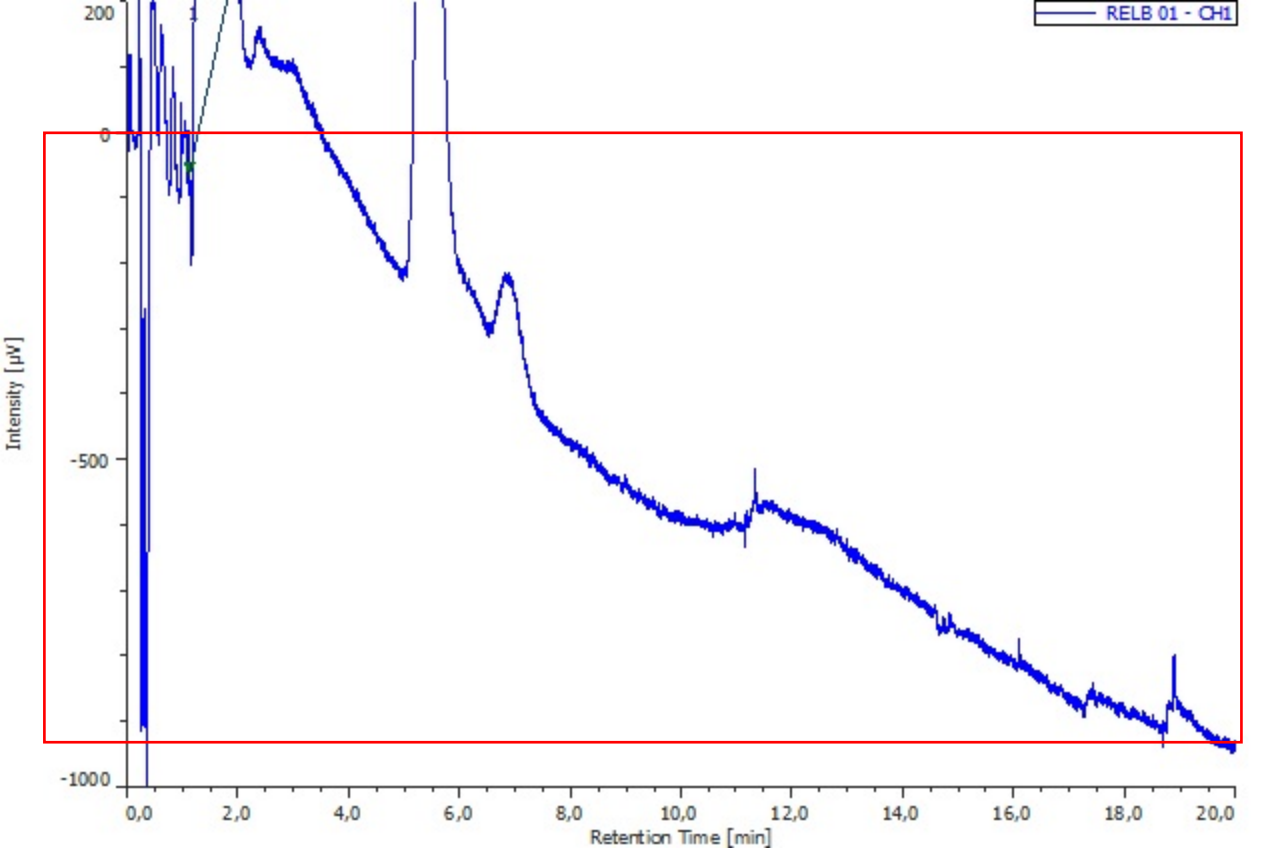
RELB 01 - CH1
200
0
-500
-1000
Intensity [µV]
0,0
2,0
4,0
6,0
8,0
10,0
12,0
14,0
16,0
18,0
20,0
Retention Time [min]

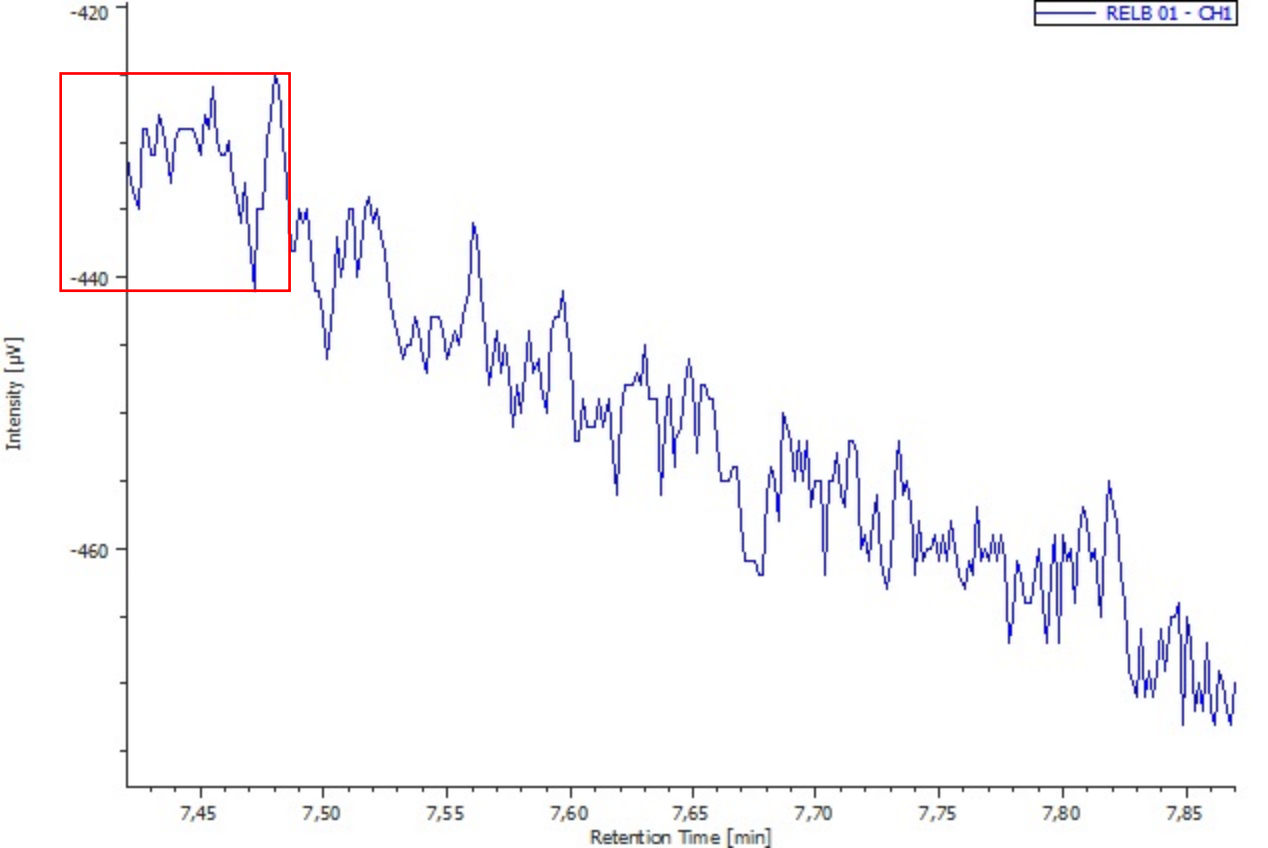
RELB 01 - CH1
-420
-440
-460
Intensity [µV]
7,45
7,50
7,55
7,60
7,65
7,70
7,75
7,80
7,85
Retention Time [min]

Chromatogram

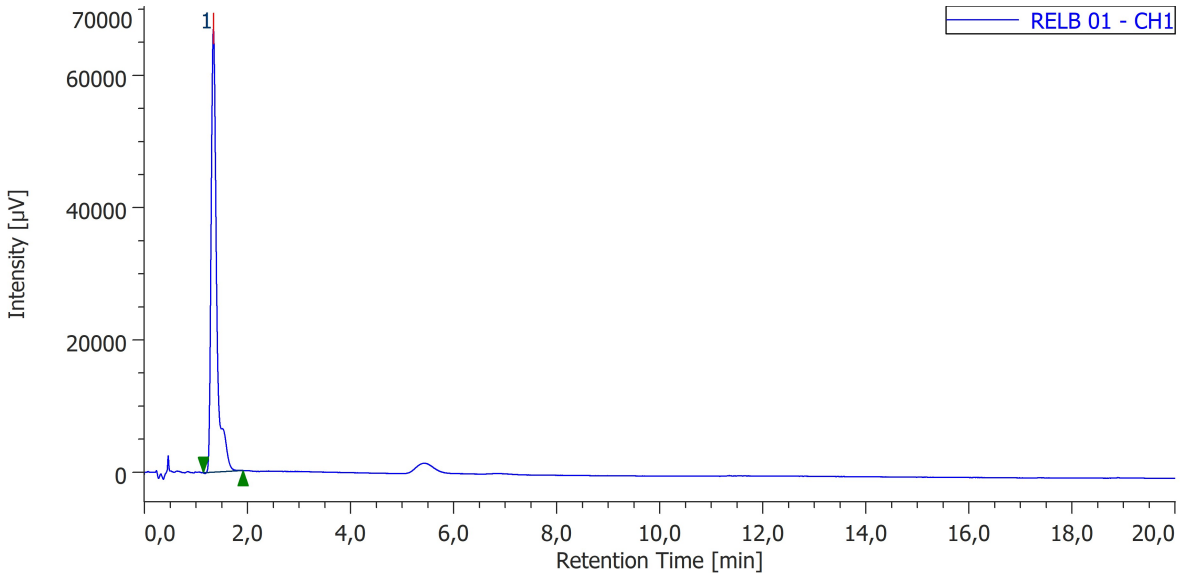

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 12:36:49
Description	
HPLC System Name	BBA HPLC 03
Injection Date	08/11/2023 18:51:15
Volume	20,0 [µL]
Sample #	5
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)
Formula1	{SN;Cafeína}/{HEIGHT;Cafeína}

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,338	504008	67013	100,000	100,000	N/A	928	N/A	1,926		3350,7	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

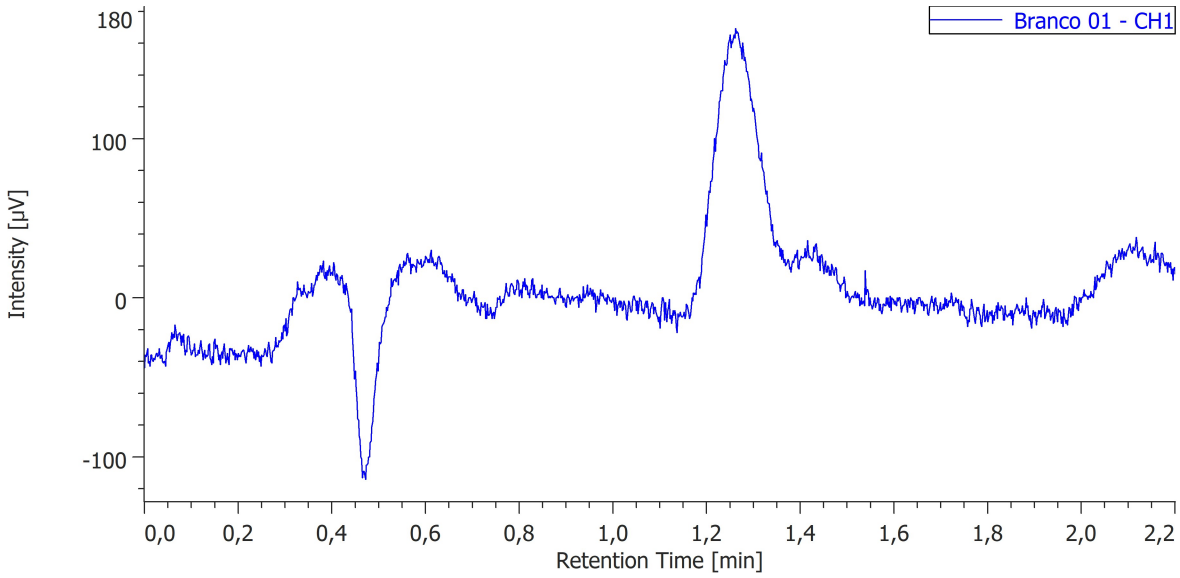


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:41
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:23:58
Volume	2,0 [µL]
Sample #	6
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

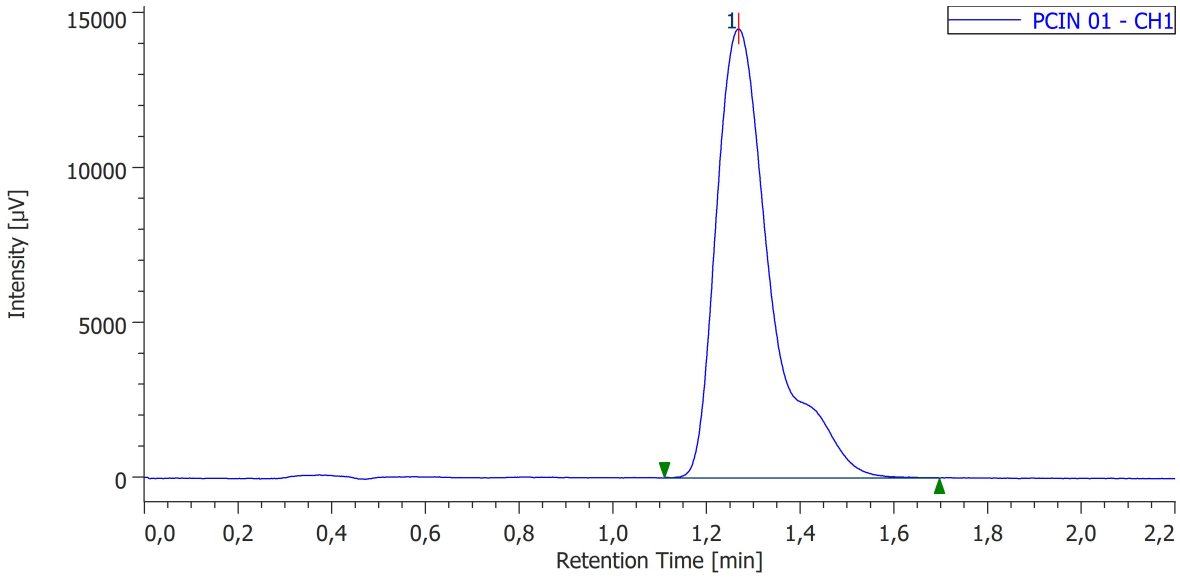

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:41
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:26:22
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,268	117462	14505	100,000	100,000	N/A	690	N/A	1,703		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

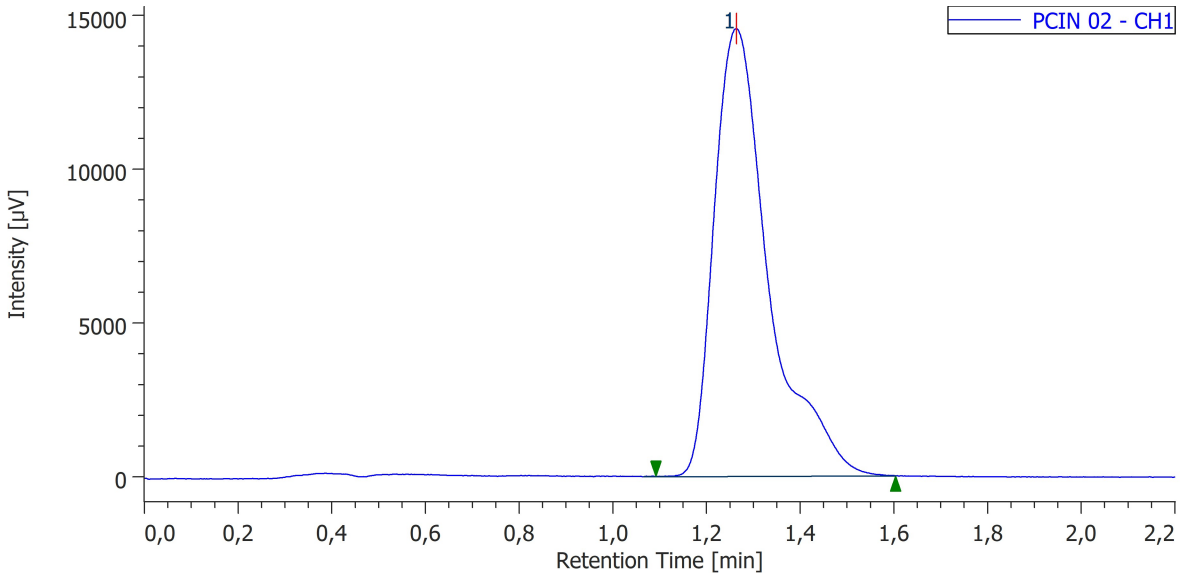

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:41
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:28:46
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,263	117963	14549	100,000	100,000	N/A	681	N/A	1,675		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

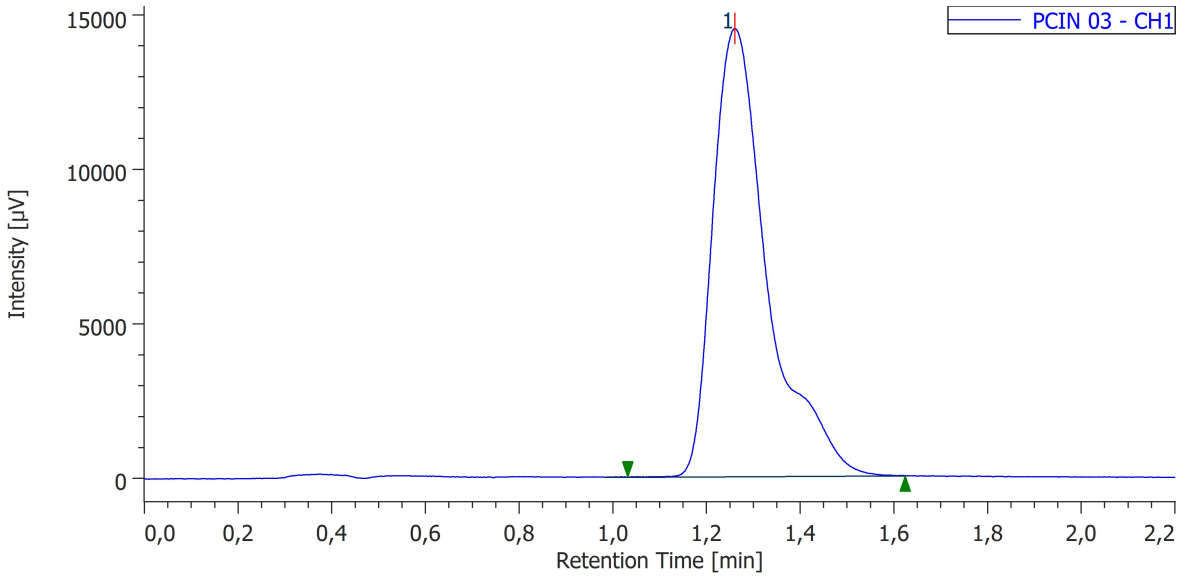

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:31:10
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,260	117704	14487	100,000	100,000	N/A	677	N/A	1,687		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

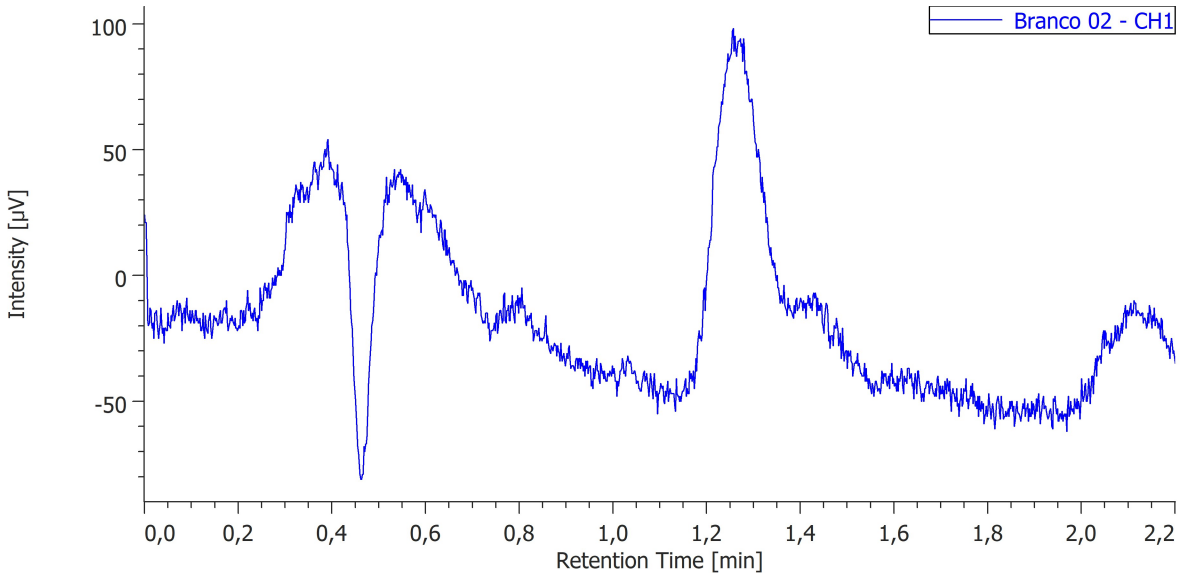


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:33:34
Volume	2,0 [µL]
Sample #	6
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

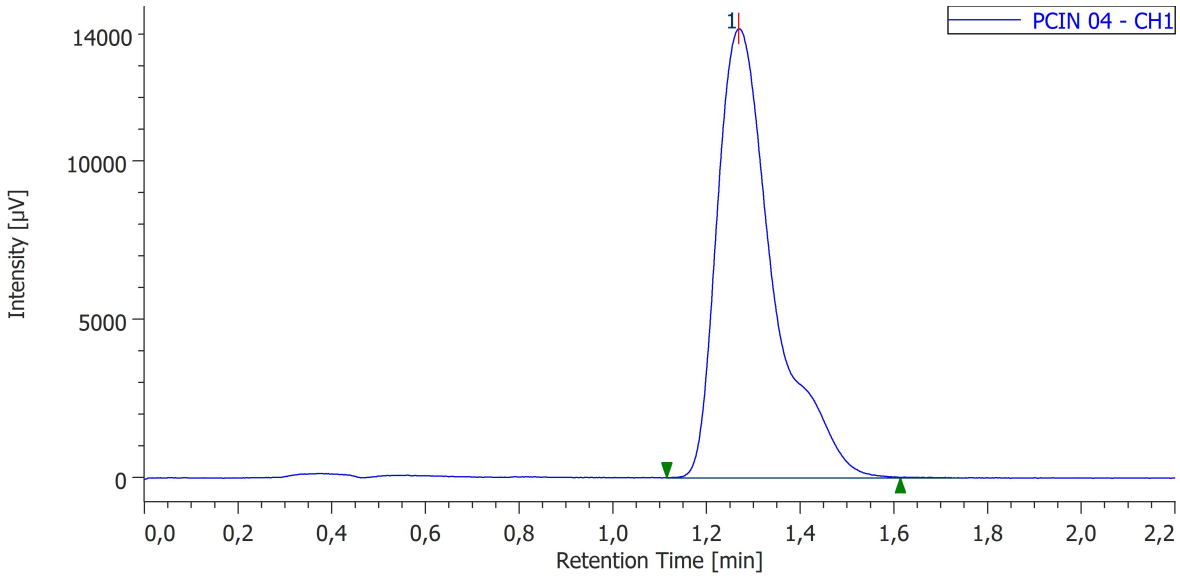

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:35:58
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,268	117868	14188	100,000	100,000	N/A	656	N/A	1,703		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

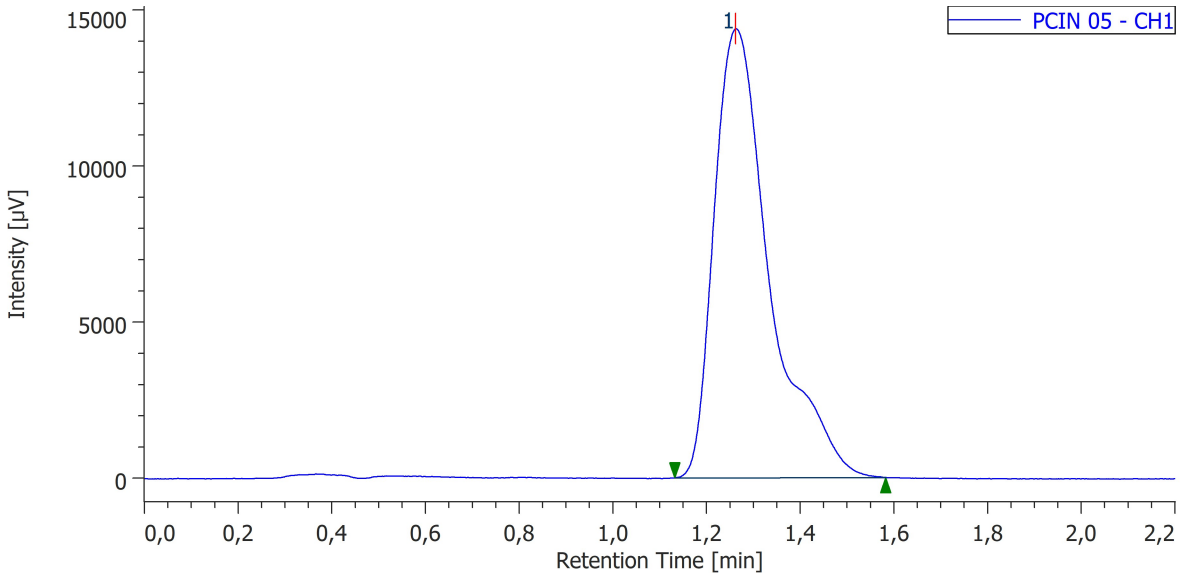

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:38:22
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,262	118620	14383	100,000	100,000	N/A	653	N/A	1,707		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

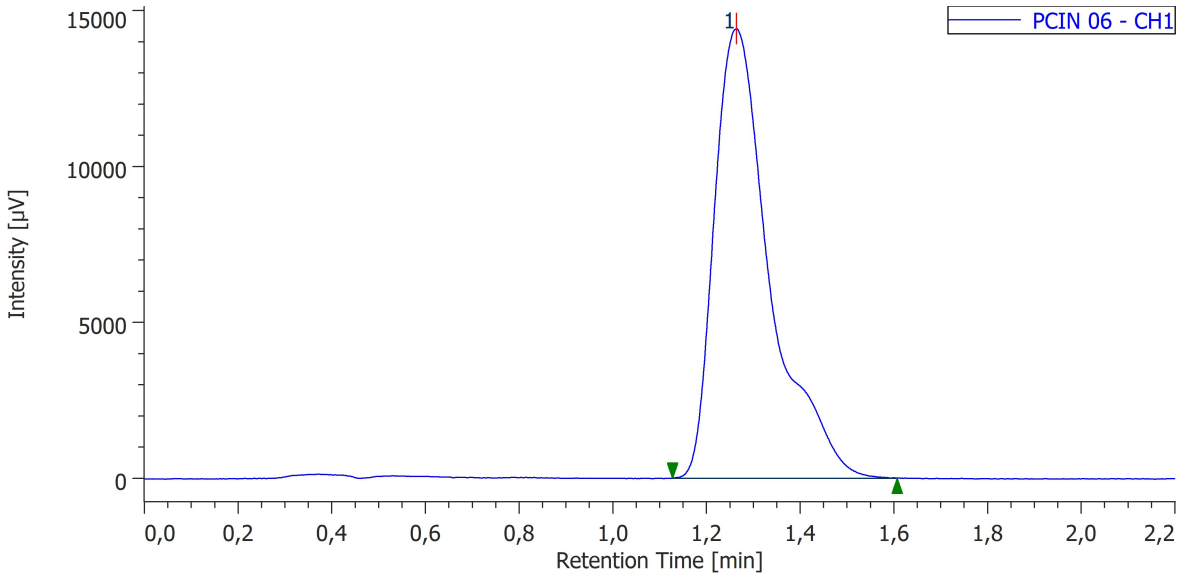

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:40:46
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,263	119082	14409	100,000	100,000	N/A	655	N/A	1,668		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

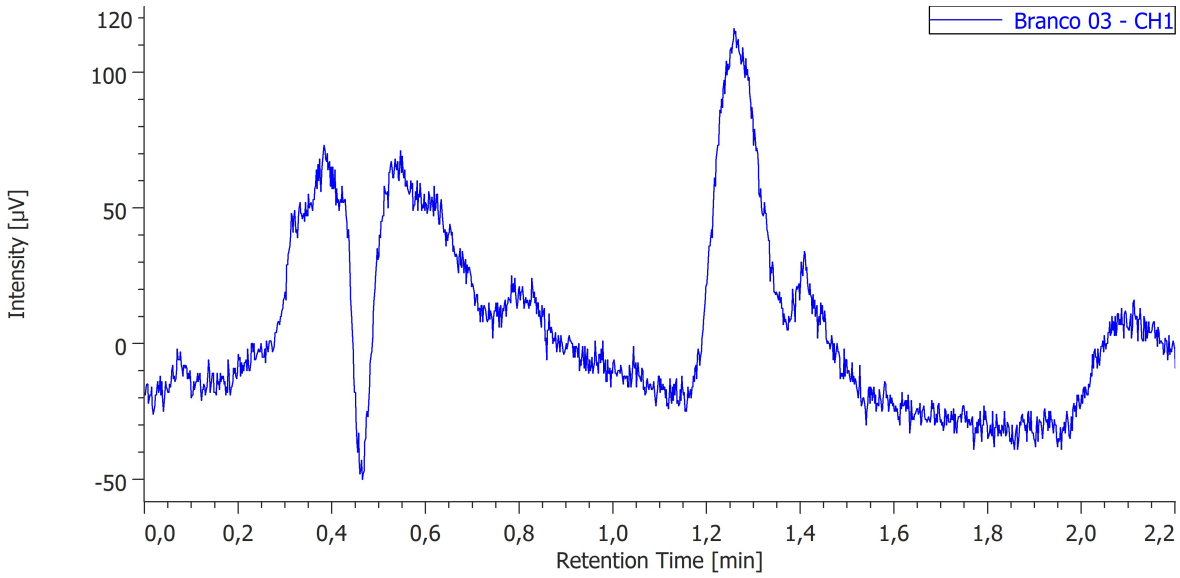


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:43:10
Volume	2,0 [µL]
Sample #	6
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

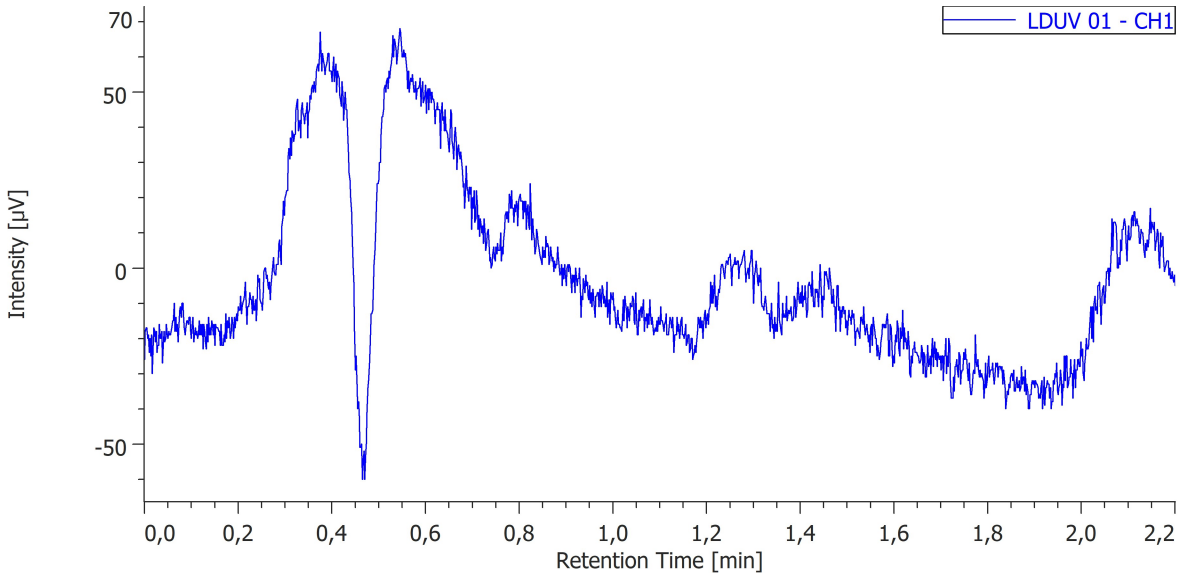


Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:45:34
Volume	2,0 [µL]
Sample #	1
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

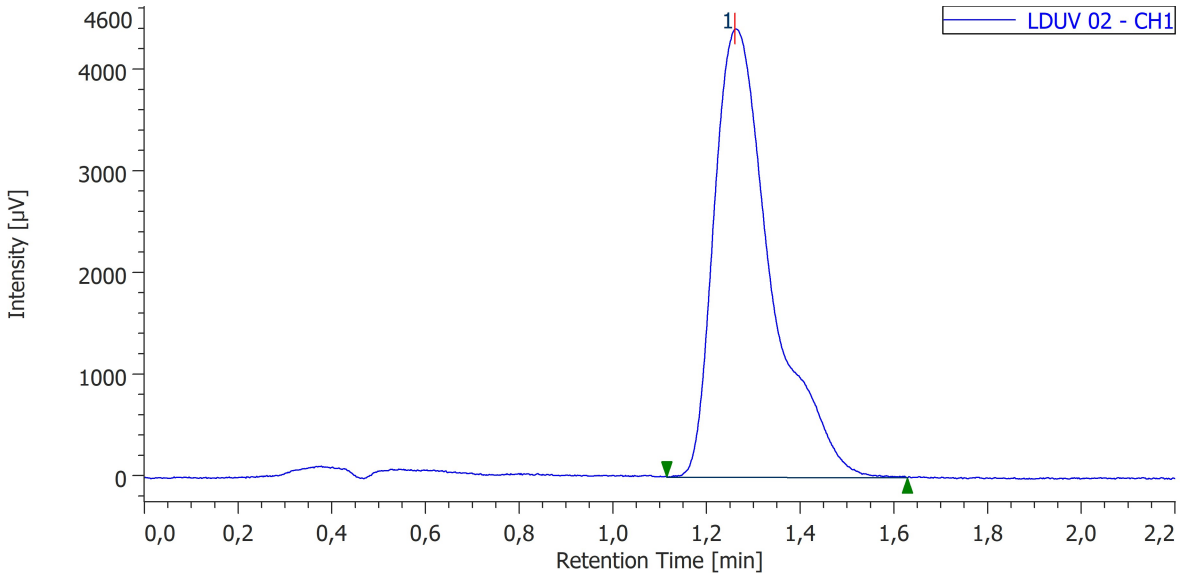

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:47:58
Volume	2,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,260	37316	4411	100,000	100,000	N/A	625	N/A	1,725		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

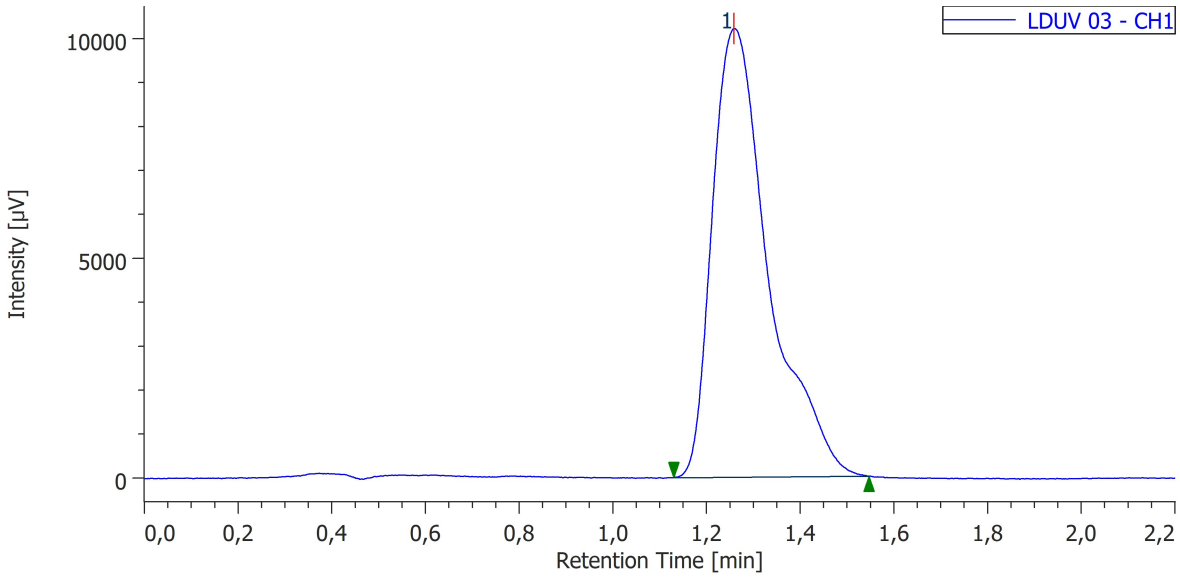

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:50:22
Volume	2,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,258	85456	10211	100,000	100,000	N/A	622	N/A	1,656		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

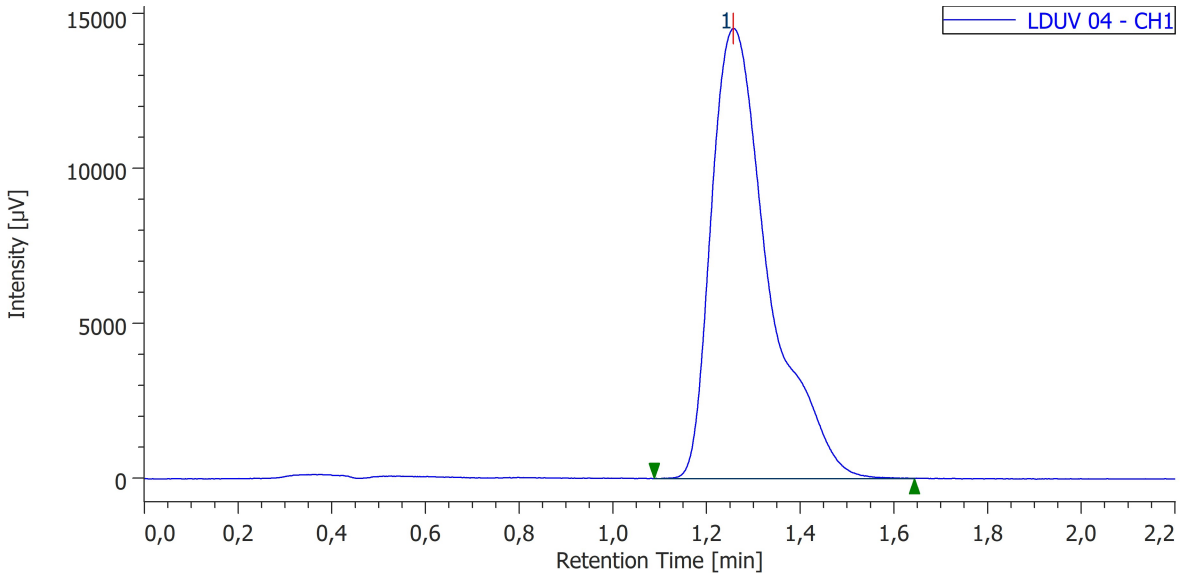

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:52:46
Volume	2,0 [µL]
Sample #	4
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,257	123832	14516	100,000	100,000	N/A	606	N/A	1,673		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

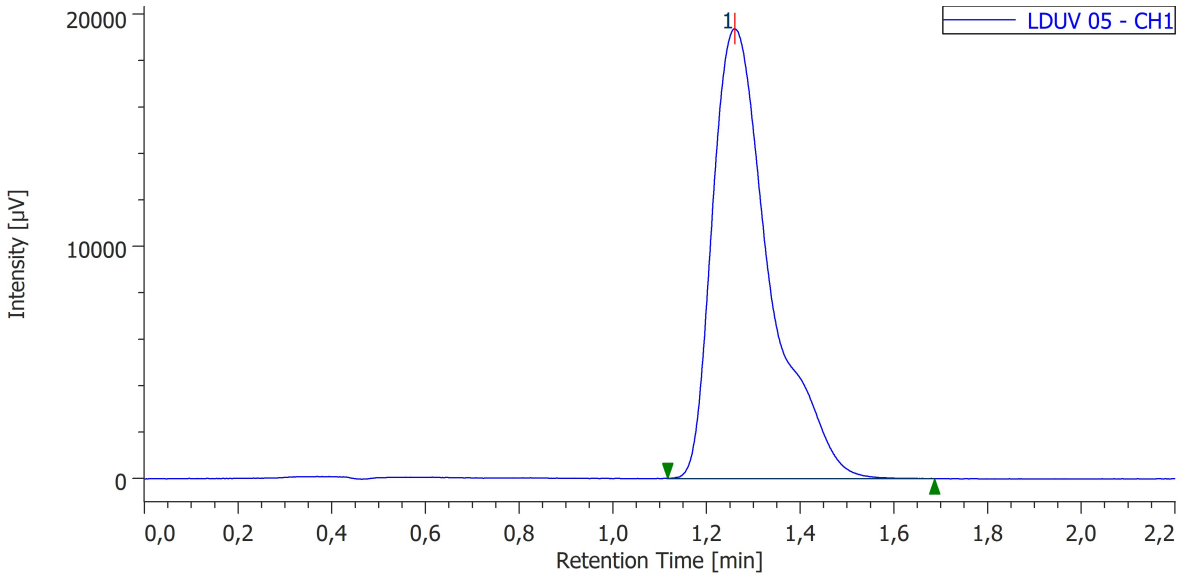

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:55:10
Volume	2,0 [µL]
Sample #	5
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,260	164908	19370	100,000	100,000	N/A	612	N/A	1,652		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

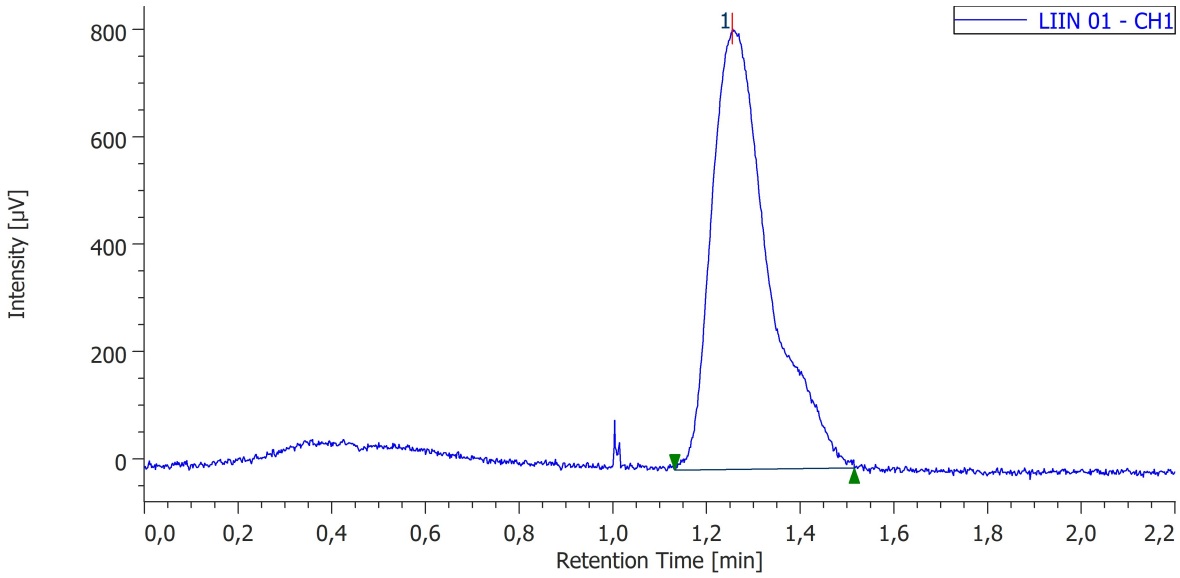

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:57:34
Volume	0,1 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,255	6920	821	100,000	100,000	N/A	614	N/A	1,662		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

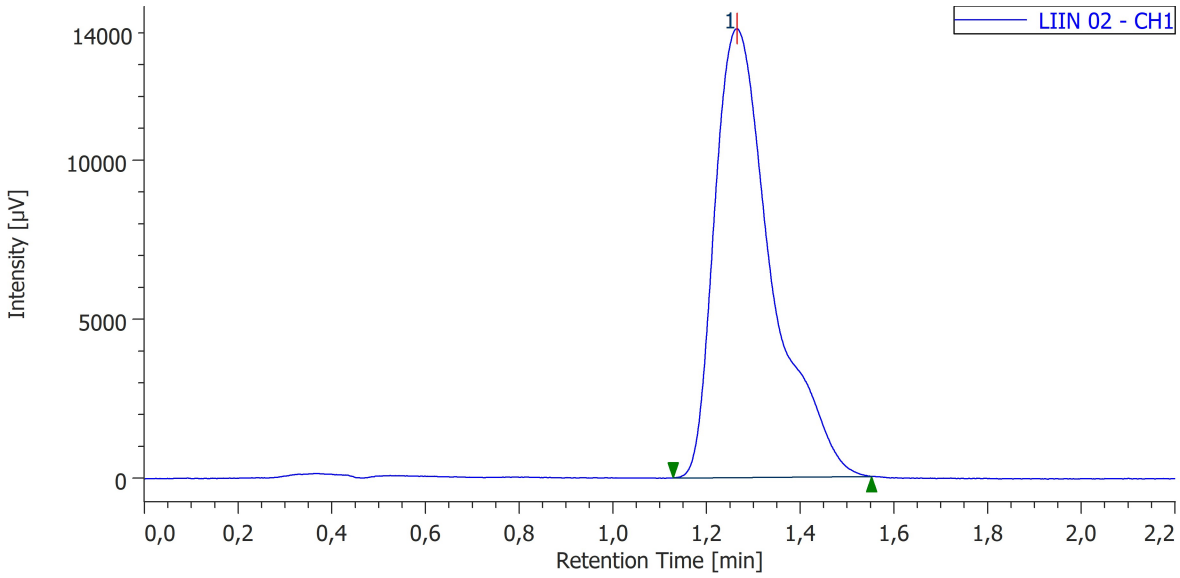

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 10:59:58
Volume	2,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,265	119694	14105	100,000	100,000	N/A	617	N/A	1,634		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

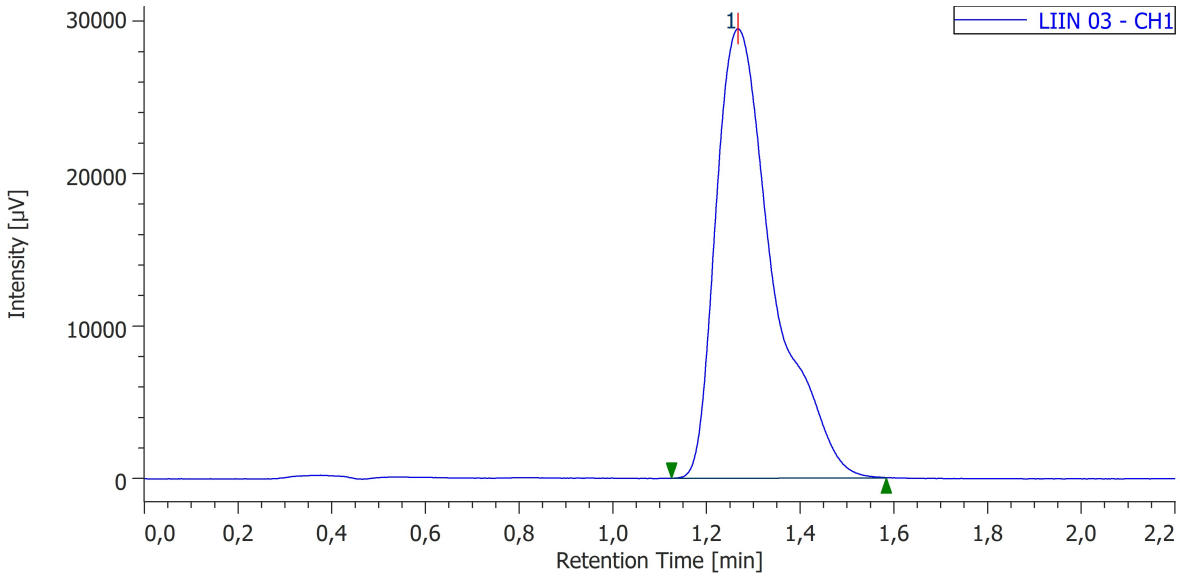

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 11:02:22
Volume	4,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,267	250709	29481	100,000	100,000	N/A	617	N/A	1,643		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

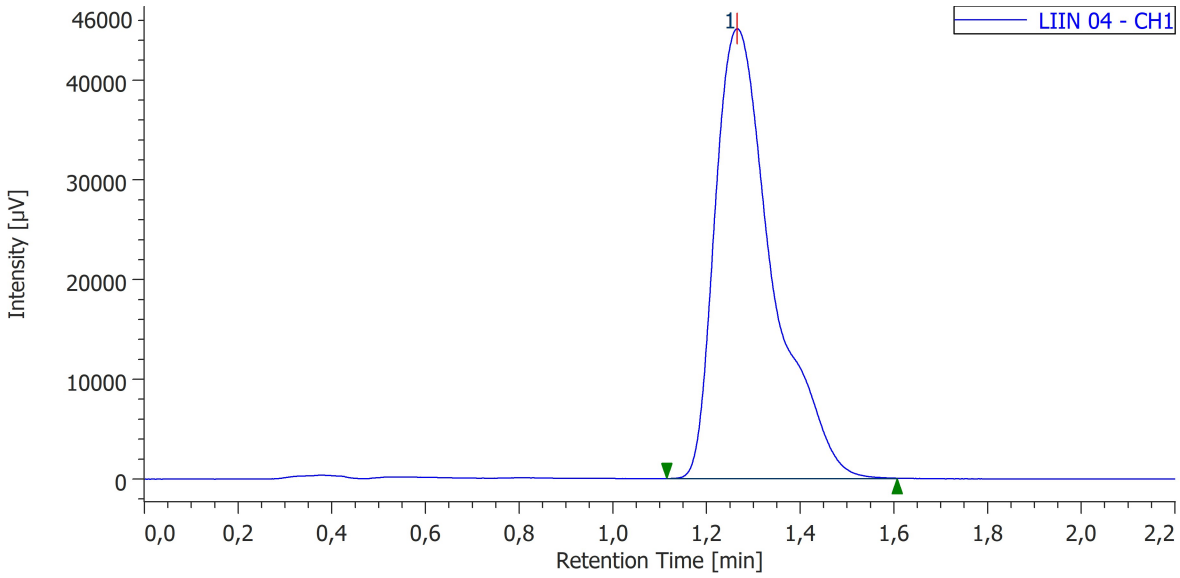

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:44
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 11:04:46
Volume	6,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,265	384057	45098	100,000	100,000	N/A	614	N/A	1,635		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

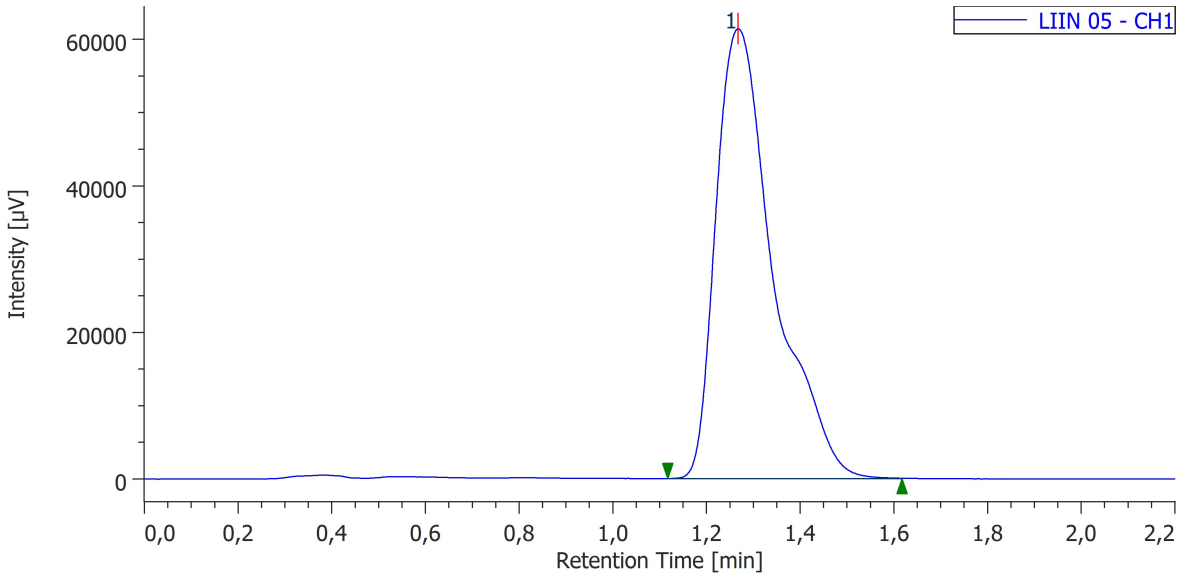

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 11:17:44
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 11:07:10
Volume	8,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,2 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	Cafeína	1	1,267	524631	61375	100,000	100,000	N/A	610	N/A	1,636		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

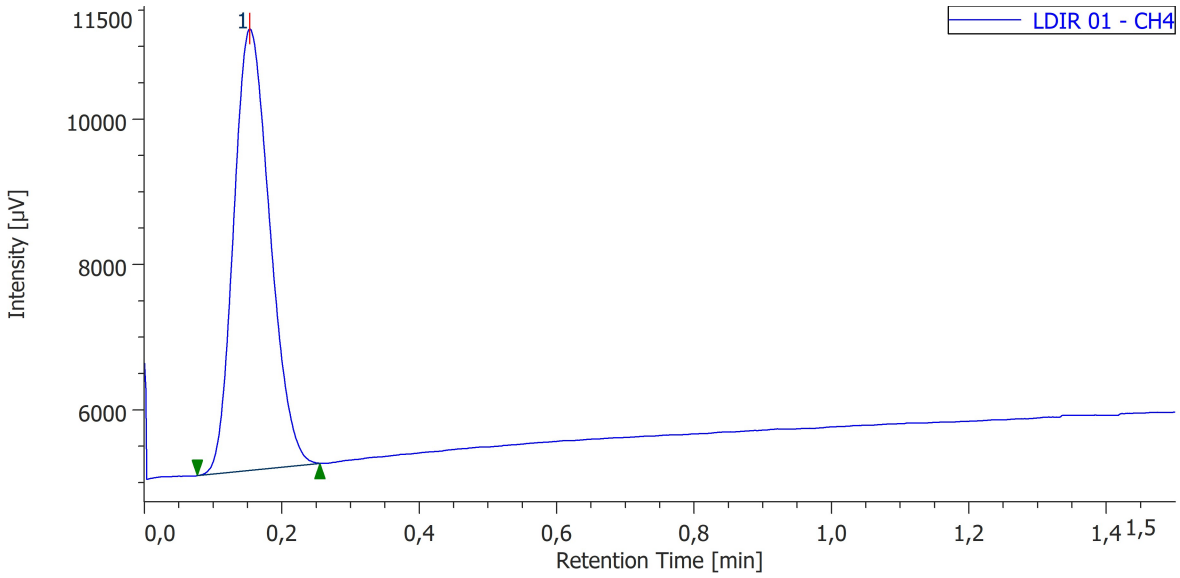

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 15:05:42
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 14:54:30
Volume	0,1 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	PDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH4
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	PDRI	4	0,153	22240	6075	100,000	100,000	N/A	40	N/A	1,205		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

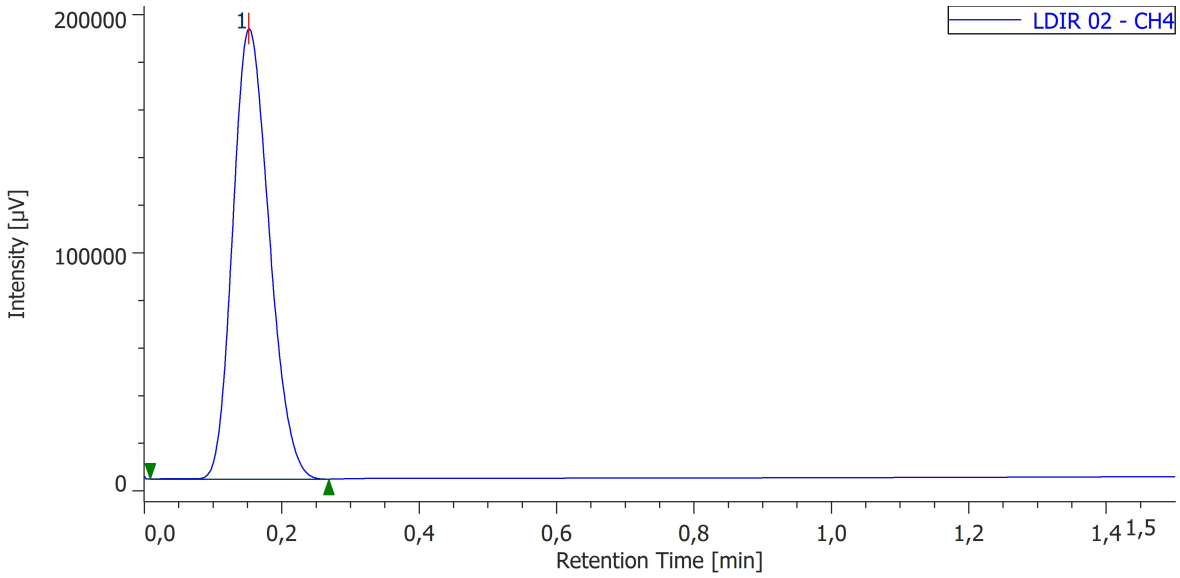

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 15:05:43
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 14:56:32
Volume	2,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	PDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH4
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	PDRI	4	0,152	696013	189112	100,000	100,000	N/A	38	N/A	1,217		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

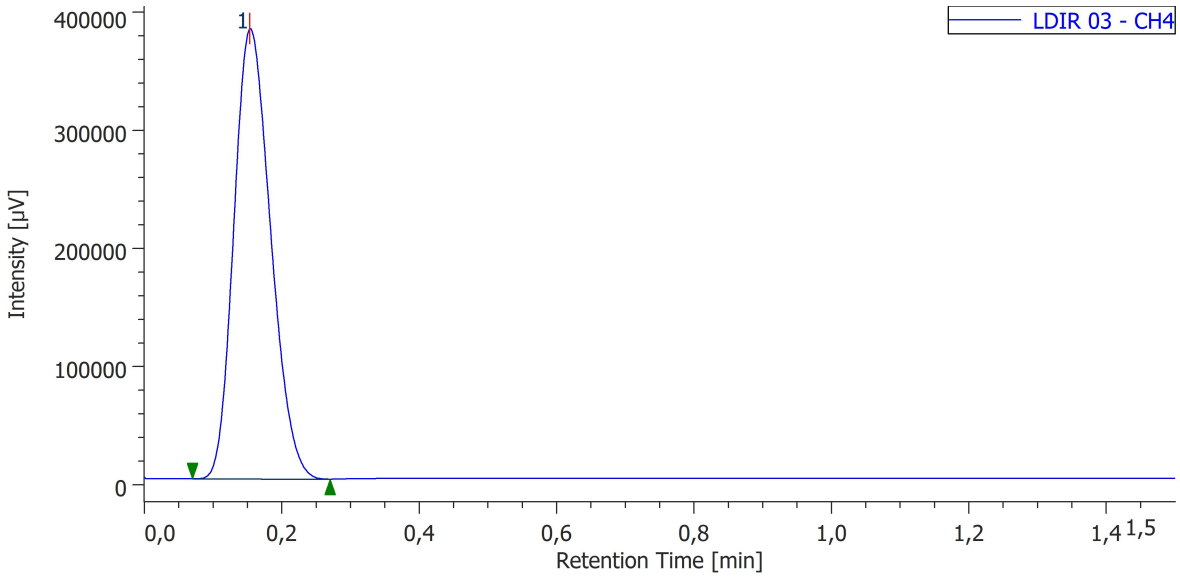

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 15:05:44
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 14:58:37
Volume	4,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	PDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH4
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	PDRI	4	0,153	1416336	380947	100,000	100,000	N/A	38	N/A	1,220		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

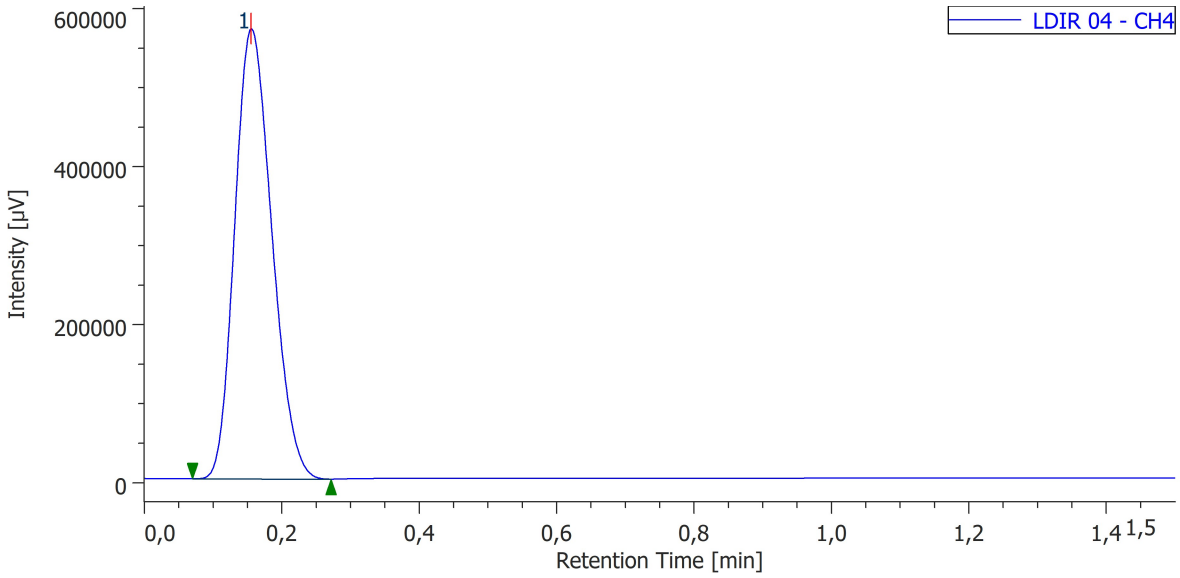

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 15:05:44
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 15:00:46
Volume	6,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	PDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH4
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	PDRI	4	0,155	2137494	569633	100,000	100,000	N/A	38	N/A	1,212		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

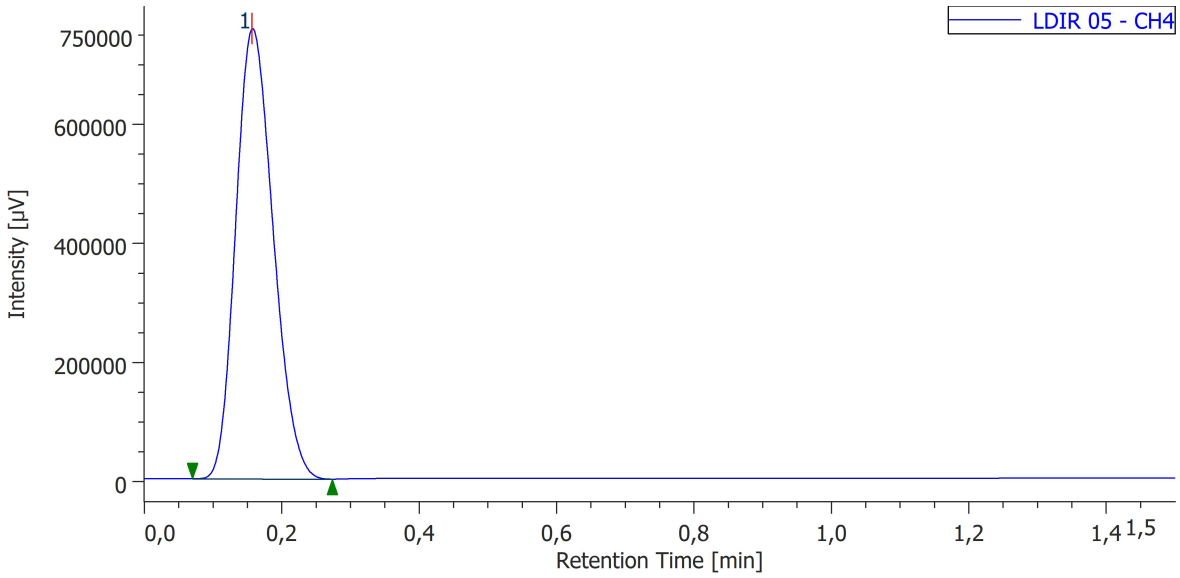

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 15:05:45
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 15:03:00
Volume	8,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	PDRI
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH4
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	PDRI	4	0,157	2866704	755602	100,000	100,000	N/A	38	N/A	1,209		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

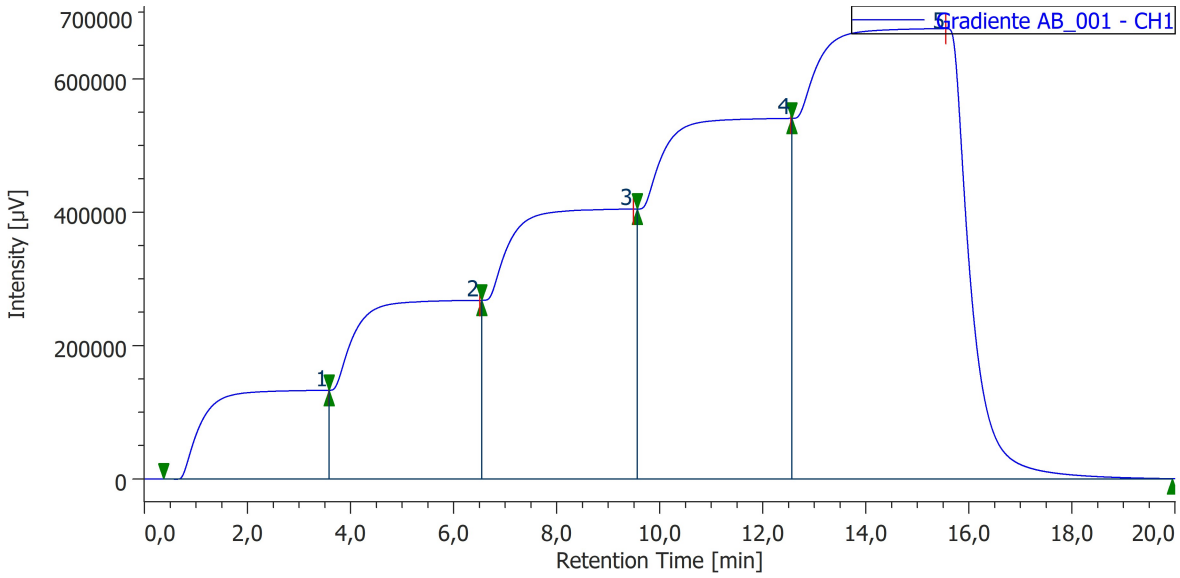

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 12:50:20
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 11:57:13
Volume	0,0 [µL]
Sample #	–
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	GRBO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	20%	1	3,578	19851544	132876	5,453	6,578	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,505	43616810	267587	11,982	13,247	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	9,485	68849940	404417	18,913	20,021	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	12,540	93018041	540248	25,552	26,746	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	15,548	138693894	674788	38,100	33,407	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

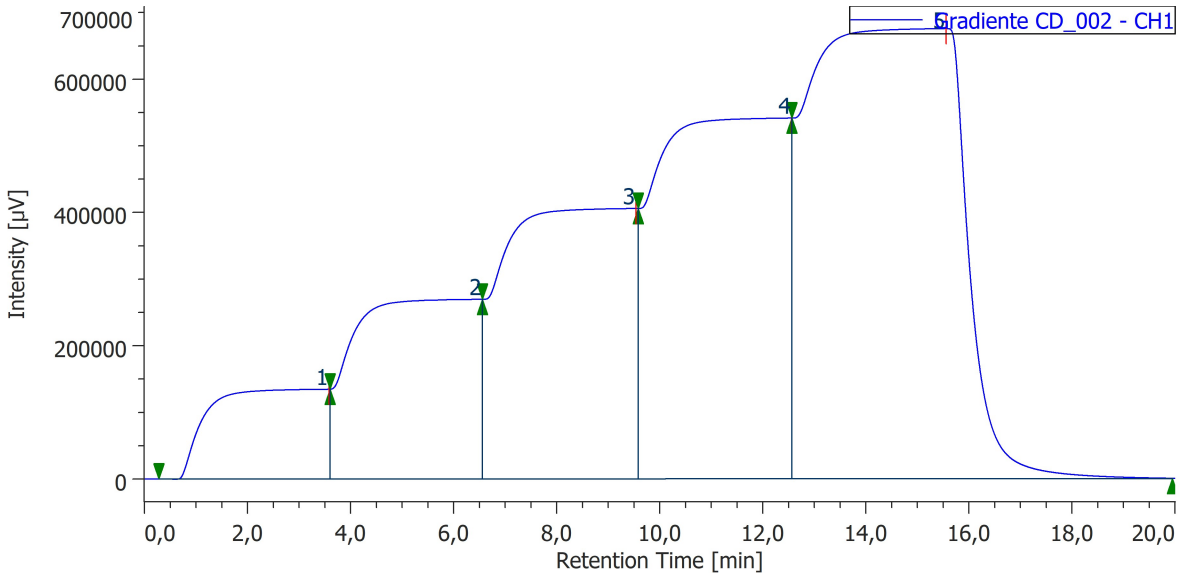

Chromatogram Information	
User Name	QPackSA
Date Modified	09/11/2023 12:50:13
Description	
HPLC System Name	BBA HPLC 03
Injection Date	09/11/2023 12:18:24
Volume	0,0 [µL]
Sample #	–
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	GRBO
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N	Ruído
1	20%	1	3,580	20279261	134562	5,552	6,647	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,558	44077020	269244	12,068	13,299	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	9,540	69238226	405233	18,957	20,017	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	12,557	92699561	540668	25,380	26,706	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	15,553	138953118	674776	38,044	33,331	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver