
PID = 07014378-041515

Peak Find - Nivel de energia 2.jws

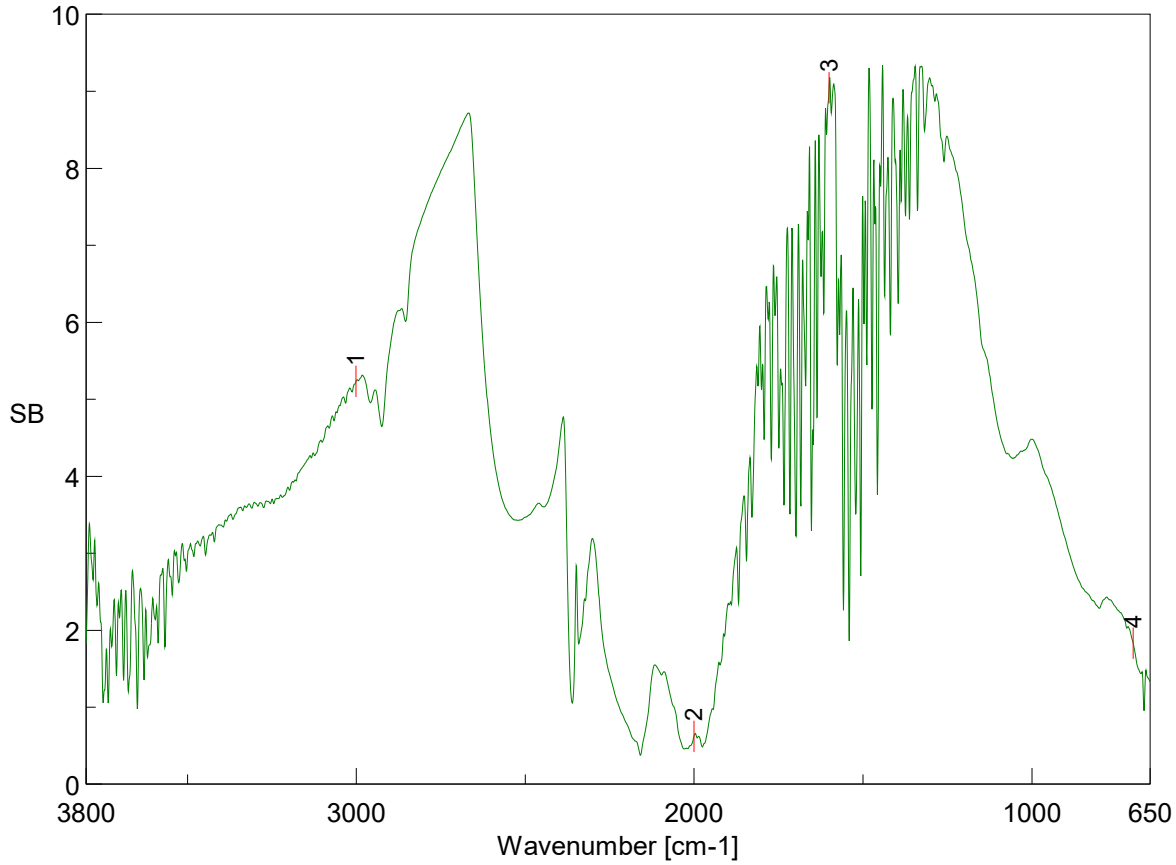

[Comments]

Sample name	
Comment	
Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 11:17
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	SB
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.964233 cm-1
Data points	3268

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 11:14
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	4 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (7.1 mm)
Scan speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)


PID = 07014378-041515

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	3000.69	5.23099	2	2000.78	0.620238
3	1600.63	9.04437	4	700.034	1.83053

PID = 07014378-121964

Peak Find - exatidão do numero de onda 2.jws

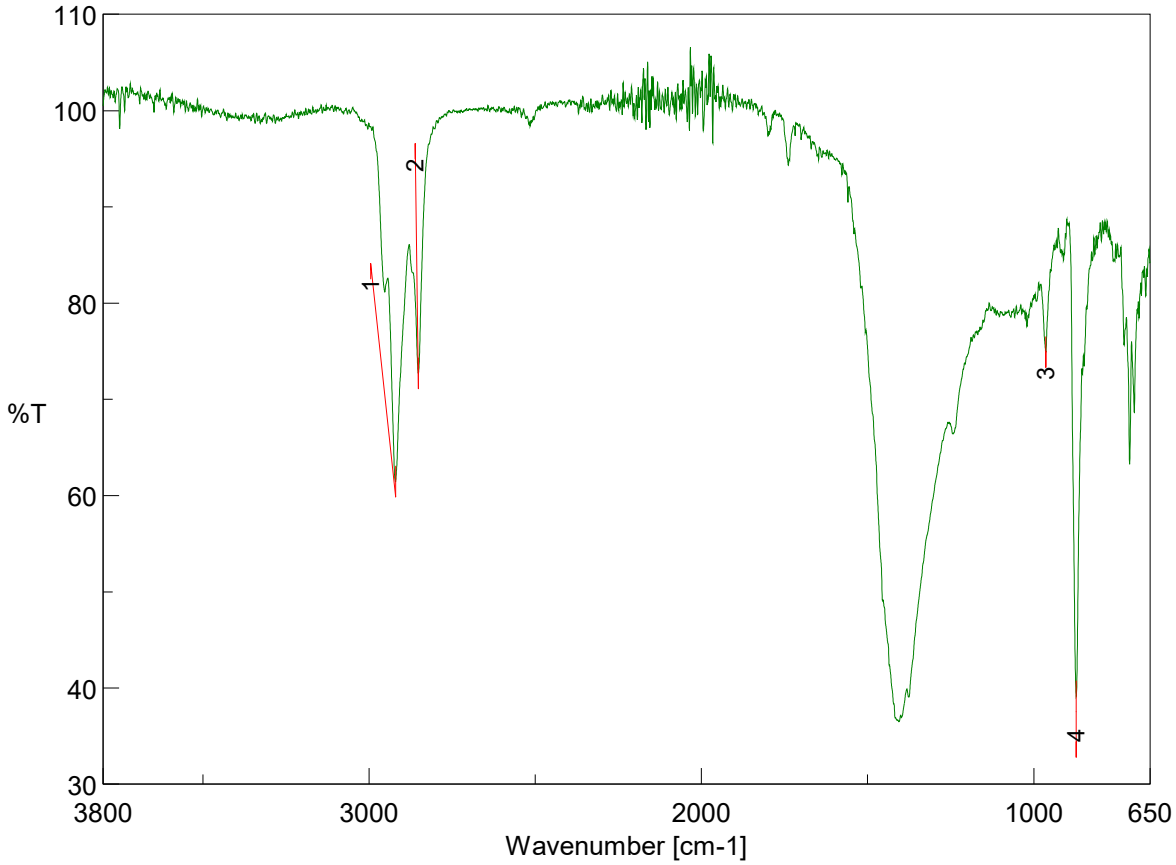

[Comments]
Sample name
Comment

Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 12:35
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 12:32
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\Exatidão numero de onda .irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)

Current time zone : -3:00	Creation	QPack Soluções Analíticas Ltda	06/11/2026 12:35
	Review		
	Approval		


PID = 07014378-121964

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2920.18	61.433	2	2851.72	72.6927
3	963.751	74.8772	4	872.149	39.1224

PID = 07014378-095500

Peak Find - resolução.jws

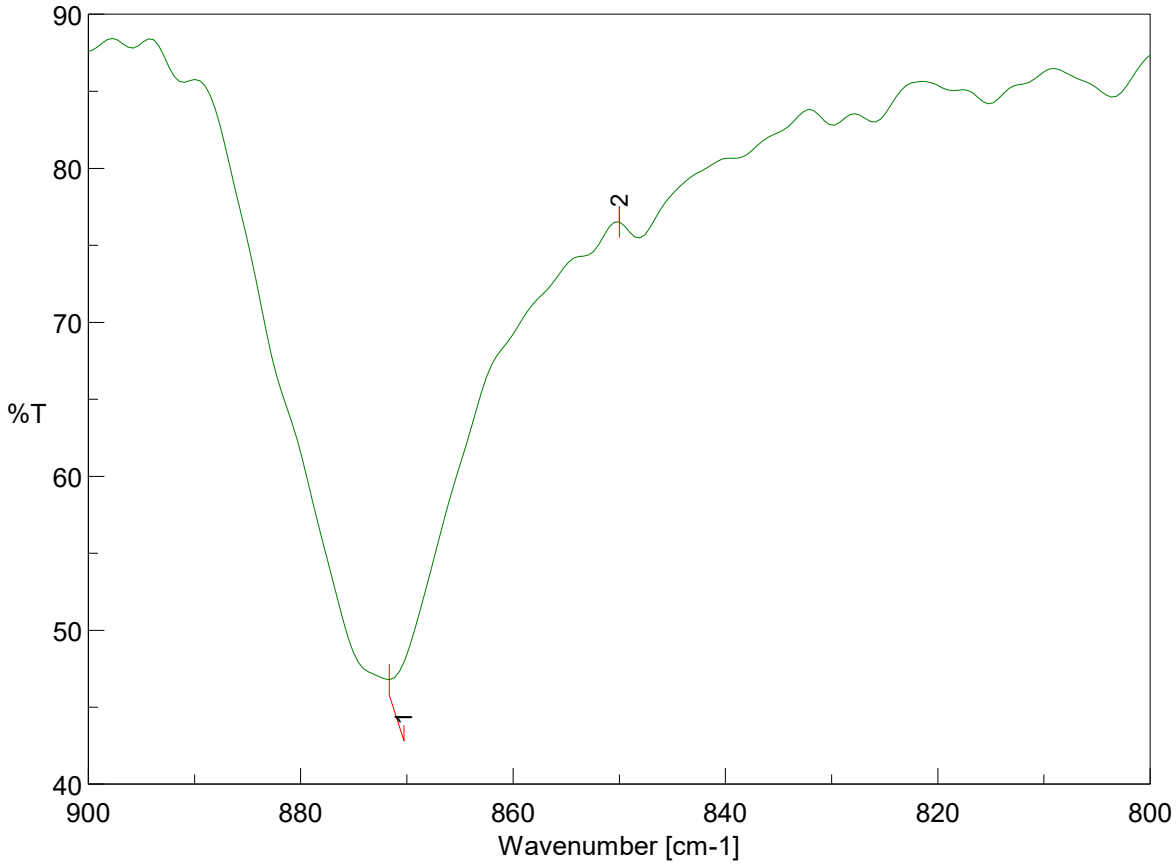

[Comments]
Sample name
Comment

Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 12:40
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 12:38
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\resolucao.irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Current time zone : -3:00 Creation QPack Soluções Analíticas Ltda 06/11/2026 12:40
Review
Approval


PID = 07014378-095500

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	871.667	46.7732	2	849.972	76.4992

PID = 07014378-091660

Peak Find - Repetibilidade numero de onda.jws

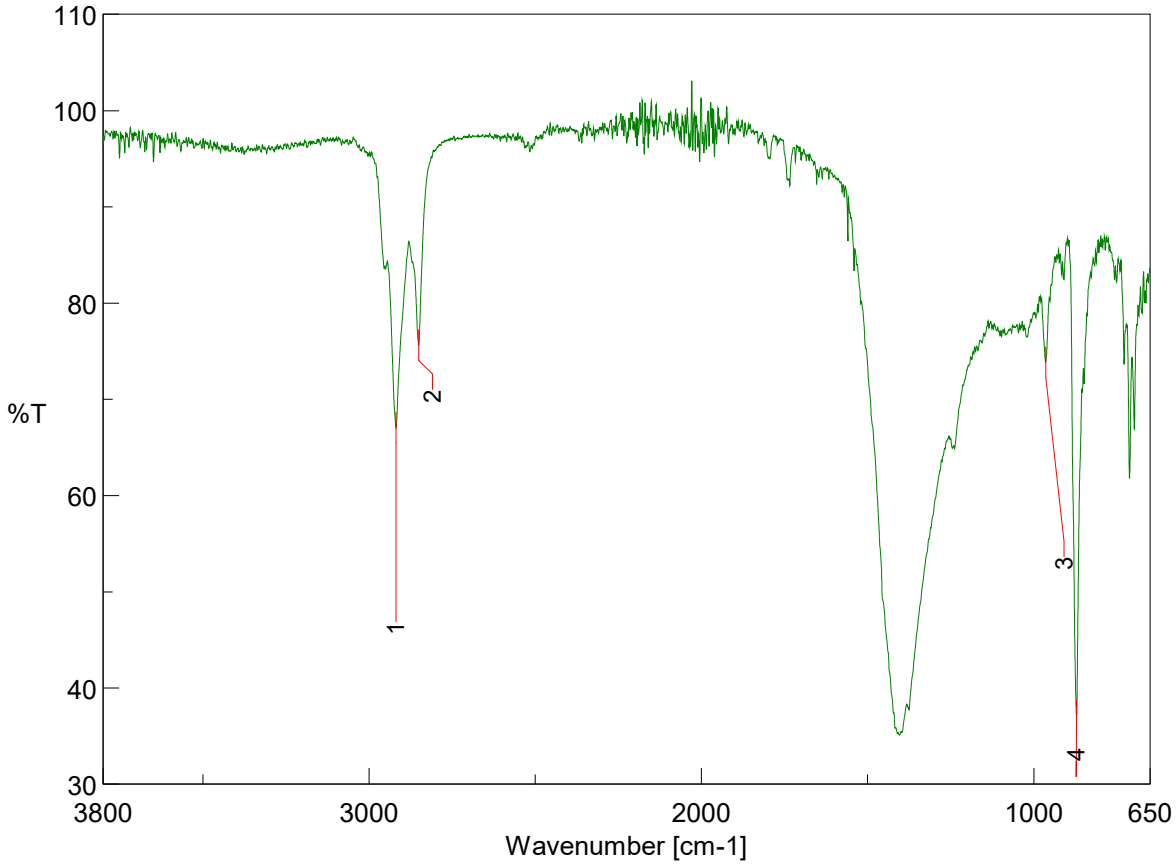

[Comments]
Sample name
Comment

Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 12:45
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 12:43
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\repetibilidade de numero de onda.irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)

Current time zone : -3:00	Creation	QPack Soluções Analíticas Ltda	06/11/2026 12:45
	Review		
	Approval		


PID = 07014378-091660

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2919.22	67.0539	2	2850.27	75.5948
3	964.233	73.8444	4	871.185	37.127

PID = 07014378-017932

Peak Find - Repetibilidade numero de onda 02.jws

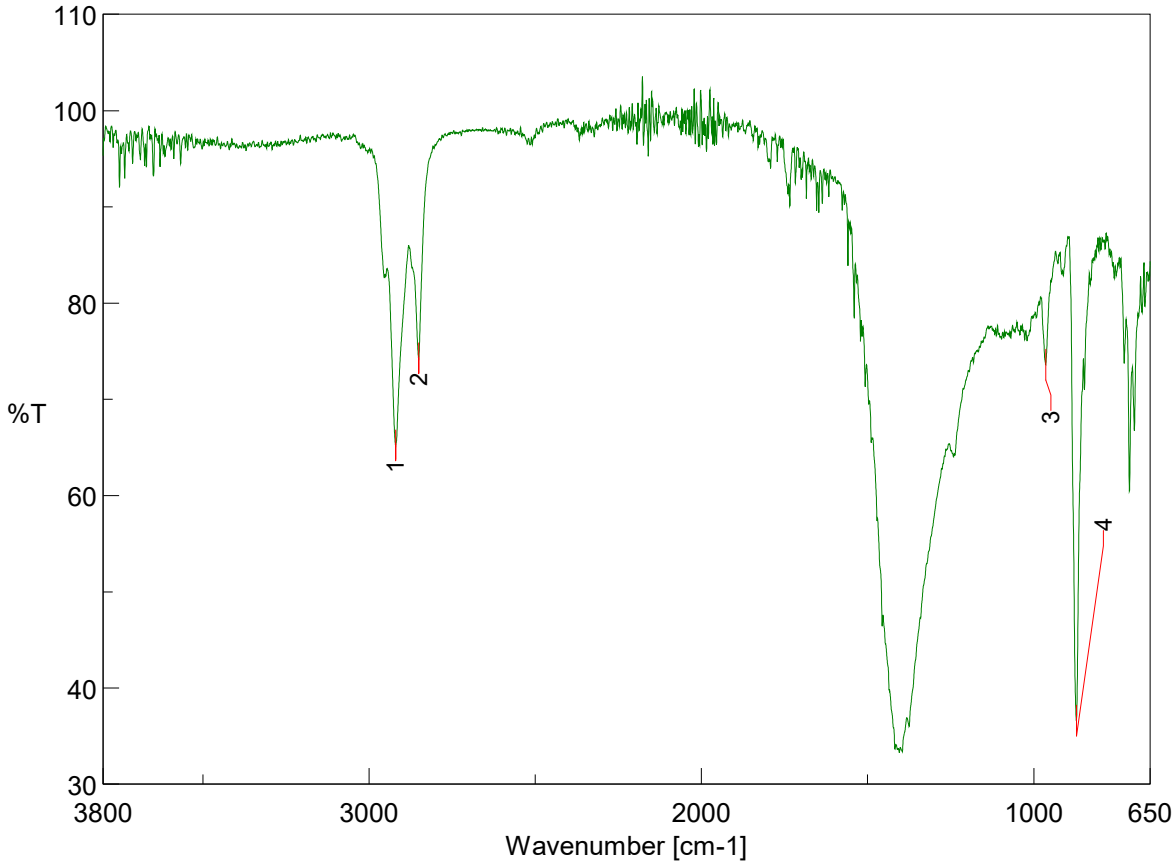

[Comments]
Sample name
Comment

Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 12:47
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 12:45
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\repetibilidade de numero de onda.irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)

Current time zone : -3:00 Creation QPack Soluções Analíticas Ltda 06/11/2026 12:47
Review
Approval


PID = 07014378-017932

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2920.18	65.2076	2	2850.76	74.2451
3	964.233	73.5731	4	871.667	36.5766

PID = 07014378-105389

Peak Find - repetibilidade fotometrica.jws

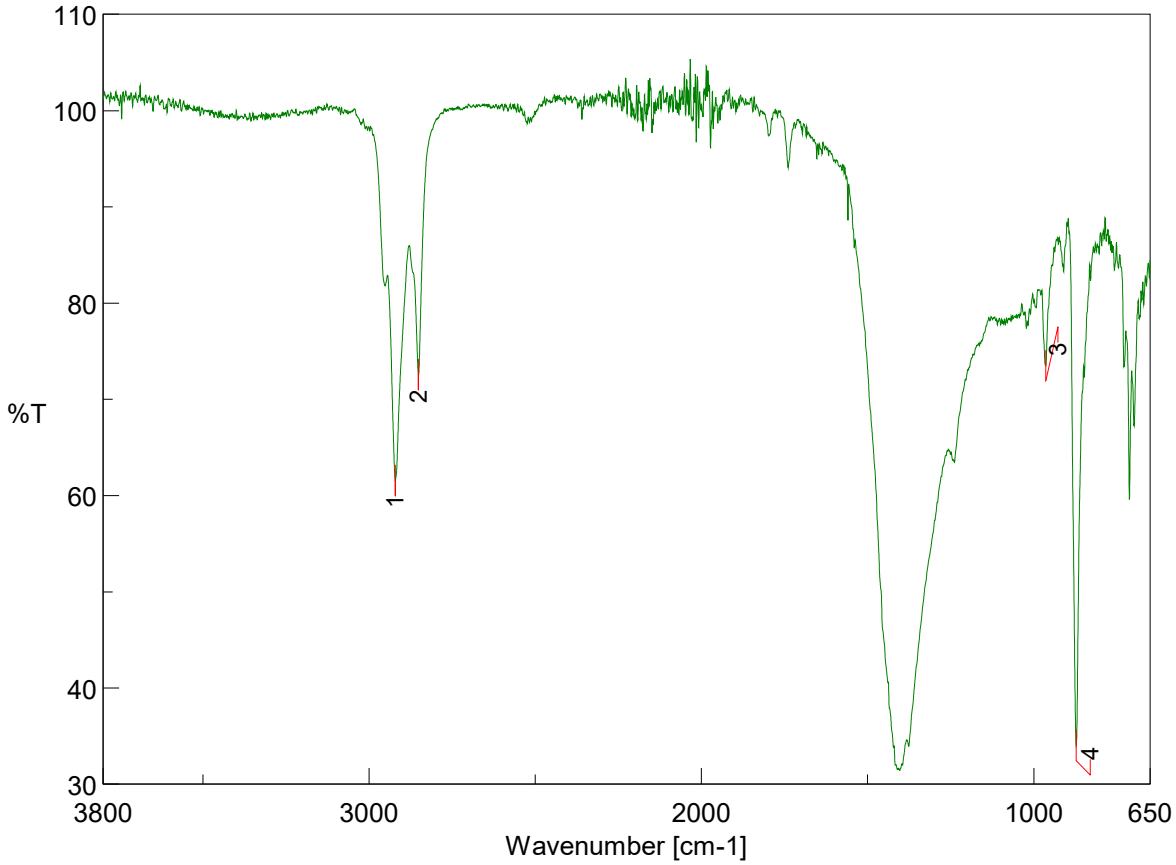

[Comments]

Sample name	
Comment	
Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 13:28
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 13:25
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\Nova pasta\repetibilidade fotometrica.irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)

Current time zone : -3:00	Creation	QPack Soluções Analíticas Ltda	06/11/2026 13:28
	Review		
	Approval		


PID = 07014378-105389

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2921.15	61.527	2	2851.24	72.5298
3	964.233	73.4883	4	872.149	34.0136

PID = 07014378-025549

Peak Find - repetibilidade fotometrica 02.jws

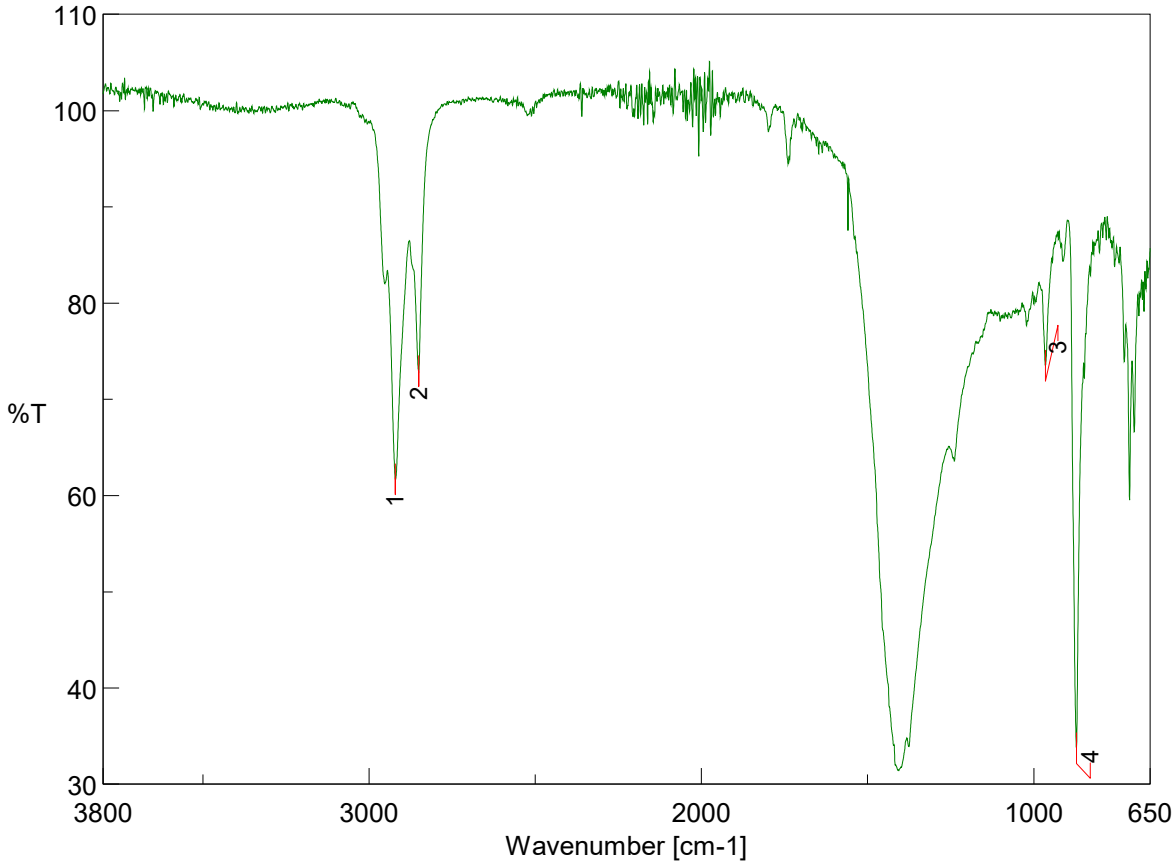

[Comments]
Sample name
Comment

Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 13:29
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.482117 cm-1
Data points	6535

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 13:26
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\Nova pasta\repetibilidade fotometrica.irxp
Light source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scan speed	Auto (2 mm/sec)

Current time zone : -3:00 Creation QPack Soluções Analíticas Ltda 06/11/2026 13:29
Review
Approval


PID = 07014378-025549

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2920.66	61.6597	2	2850.76	72.9237
3	965.198	73.4876	4	871.667	33.7122

PID = 07014378-019661

Peak Find - Sensibilidade.jws

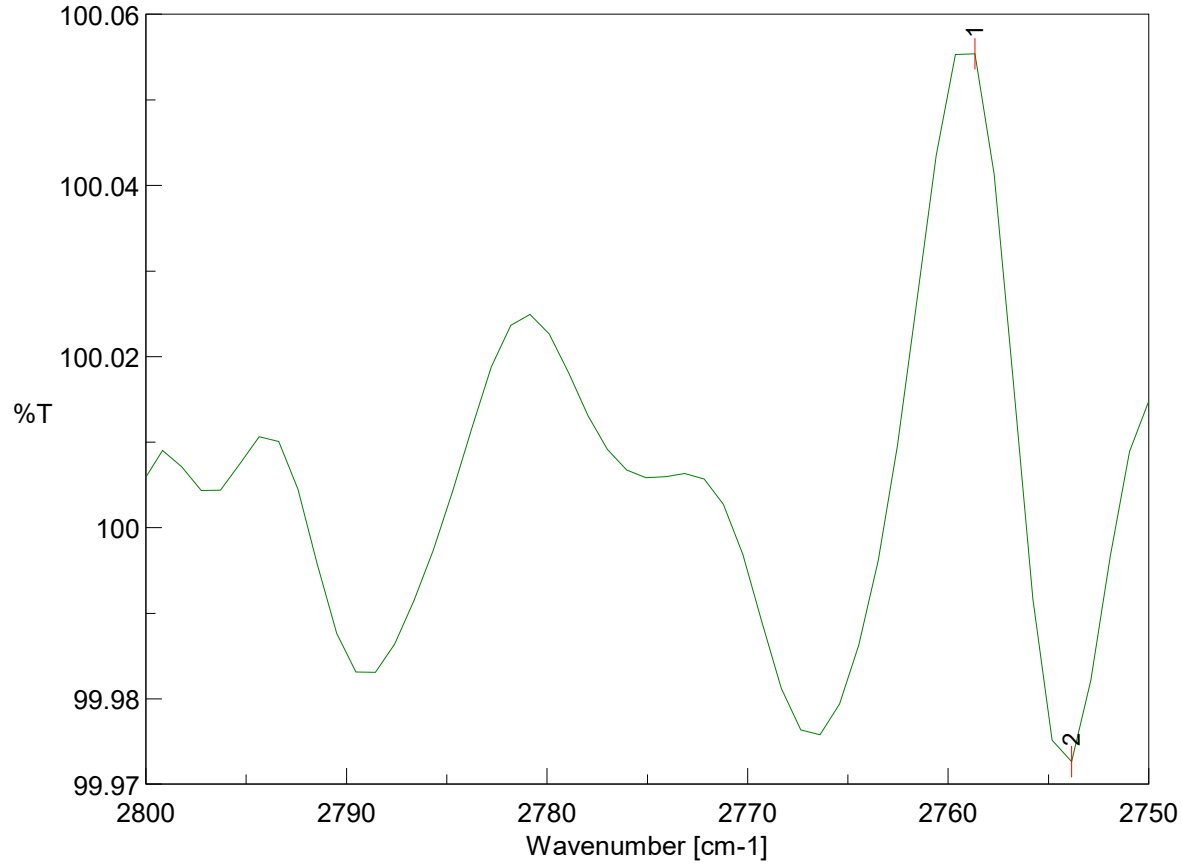

[Comments]
Sample name
Comment
Username QPackSA
Workgroup Jasco - Tecnico
Division Suporte Técnico
Organization BIOAGRI LABORATÓRIOS

[Detailed Information]
Creation date 06/11/2026 13:37

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 649.893 cm-1
End 3800.04 cm-1
Data interval 0.964233 cm-1
Data points 3268

[Measurement Information]
Model name FT/IR-4700typeA
Serial No. C005161788

Accessory ATR PRO ONE
Accessory S/N A010361809

Measurement date 06/11/2026 13:34

Parameter file C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\sensibilidade.irxp
Light source Standard
Detector TGS
Accumulation 48
Resolution 4 cm-1
Zero filling On
Apodization Cosine
Gain Auto (8)
Aperture Auto (7.1 mm)
Scan speed Auto (2 mm/sec)
Filter Auto (30000 Hz)

Current time zone : -3:00 Creation QPack Soluções Analíticas Ltda 06/11/2026 13:37
Review
Approval


PID = 07014378-019661

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2758.67	100.055	2	2753.85	99.9726

PID = 07014378-066733

Peak Find - Sensibilidade.jws

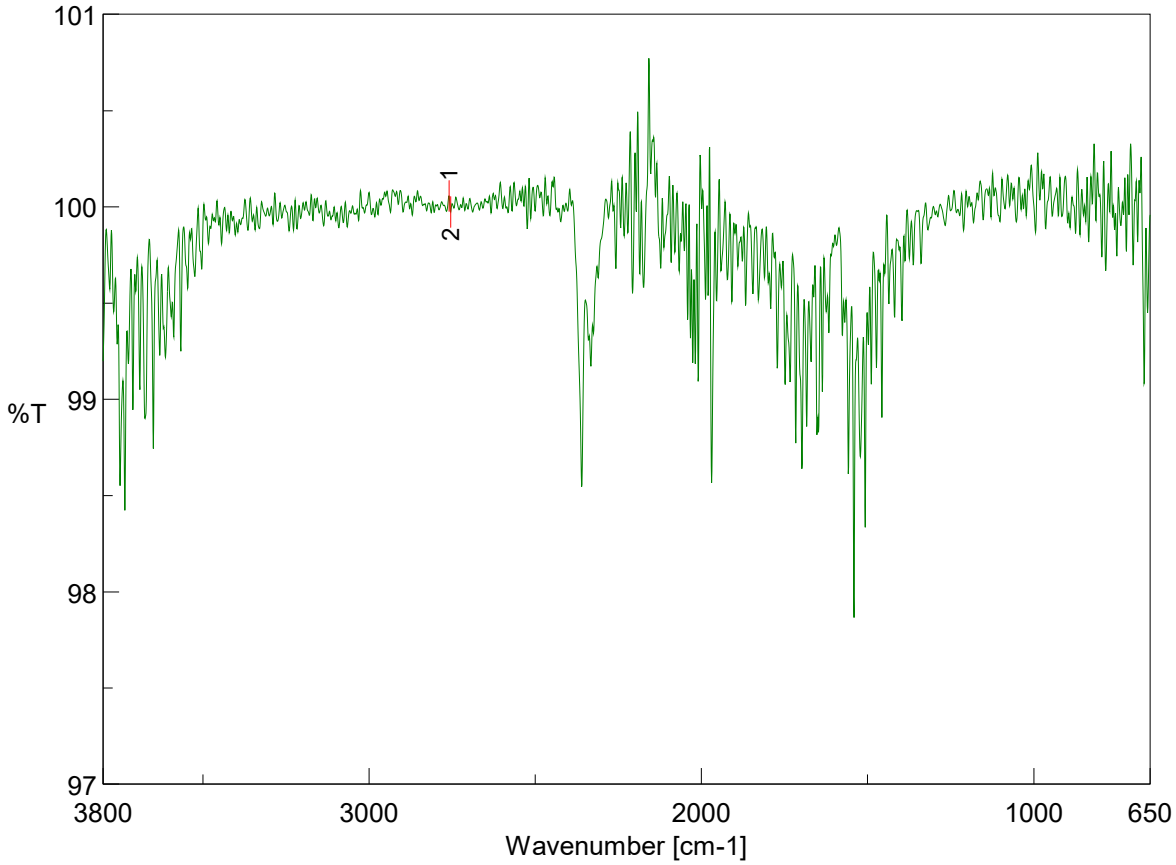

[Comments]

Sample name	
Comment	
Username	QPackSA
Workgroup	Jasco - Tecnico
Division	Suporte Técnico
Organization	BIOAGRI LABORATÓRIOS

[Detailed Information]

Creation date	06/11/2026 13:37
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	649.893 cm-1
End	3800.04 cm-1
Data interval	0.964233 cm-1
Data points	3268

[Measurement Information]

Model name	FT/IR-4700typeA
Serial No.	C005161788
Accessory	ATR PRO ONE
Accessory S/N	A010361809
Measurement date	06/11/2026 13:34
Parameter file	C:\WorkGroupFolder\Jasco - Tecnico\Qualificação 2026\ATR\sensibilidade.irxp
Light source	Standard
Detector	TGS
Accumulation	48
Resolution	4 cm-1
Zero filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (7.1 mm)
Scan speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Current time zone : -3:00	Creation	QPack Soluções Analíticas Ltda	06/11/2026 13:37
	Review		
	Approval		

PID = 07014378-066733

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2758.67	100.055	2	2753.85	99.9726