
Chromatogram

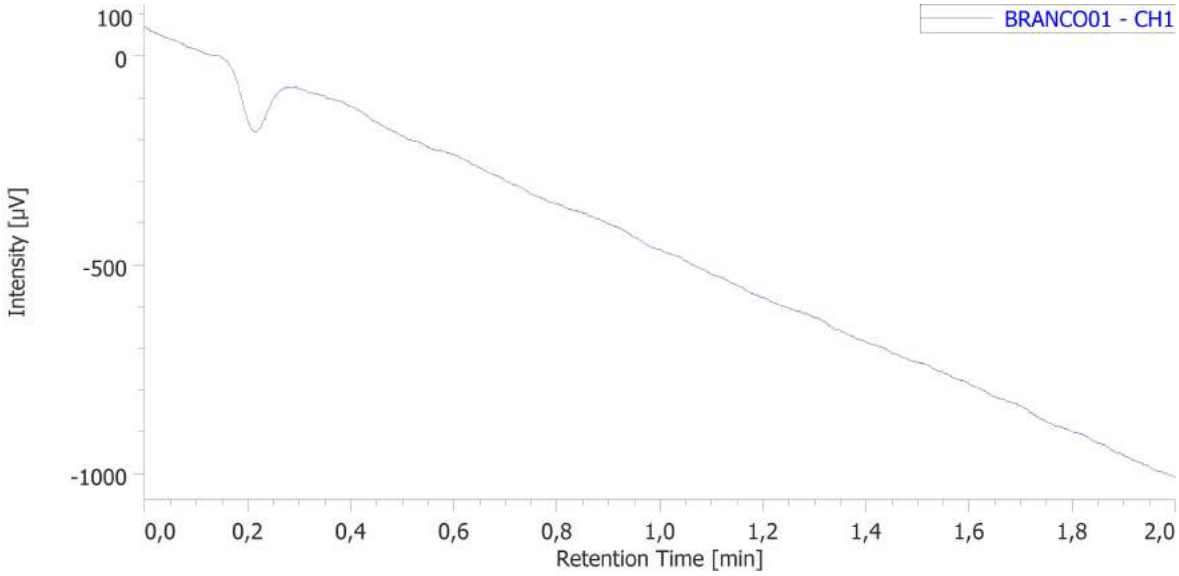


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:12:20
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:10:17
Volume	10,0 [µL]
Sample #	50
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

Chromatogram

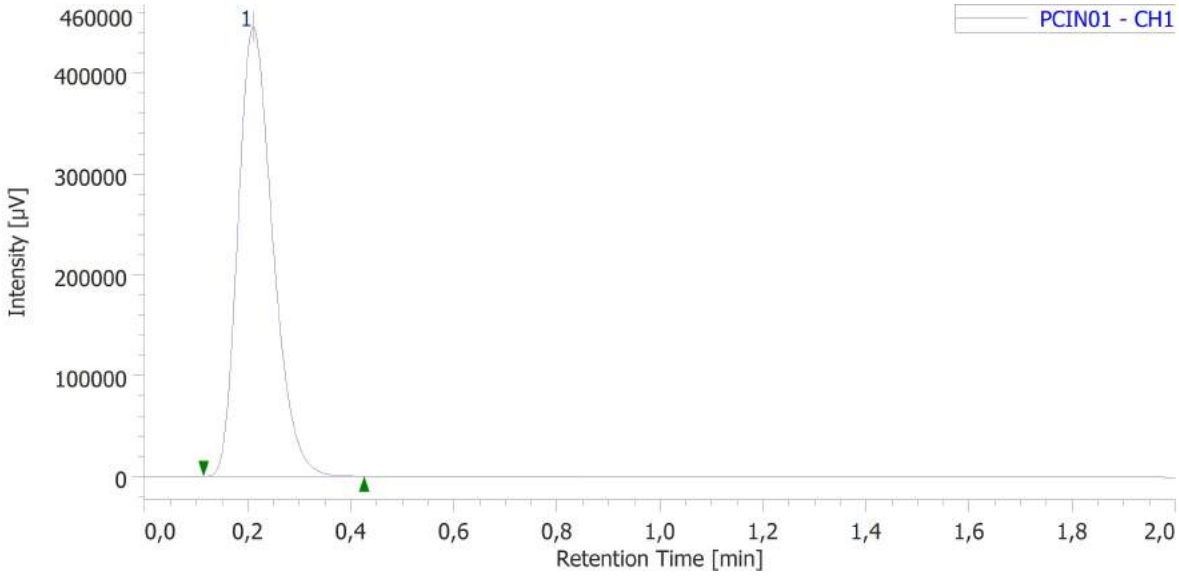


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:15:18
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:13:16
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,211	2086359	445624	100,000	100,000	N/A	47	N/A	1,281	

Chromatogram

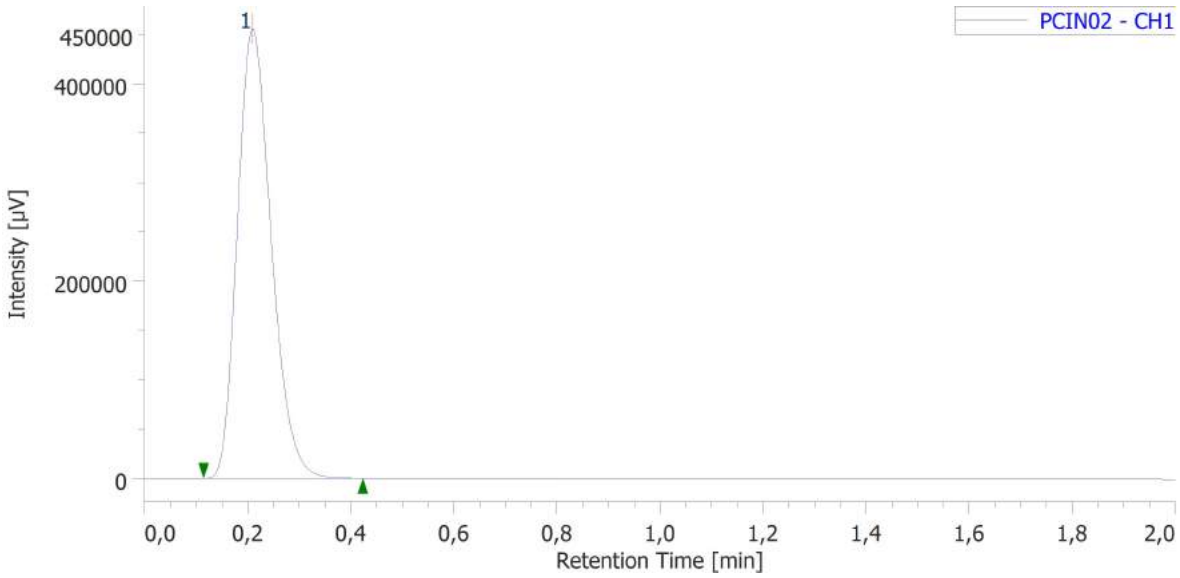


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:18:16
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:16:14
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,209	2075342	455270	100,000	100,000	N/A	49	N/A	1,246	

Chromatogram

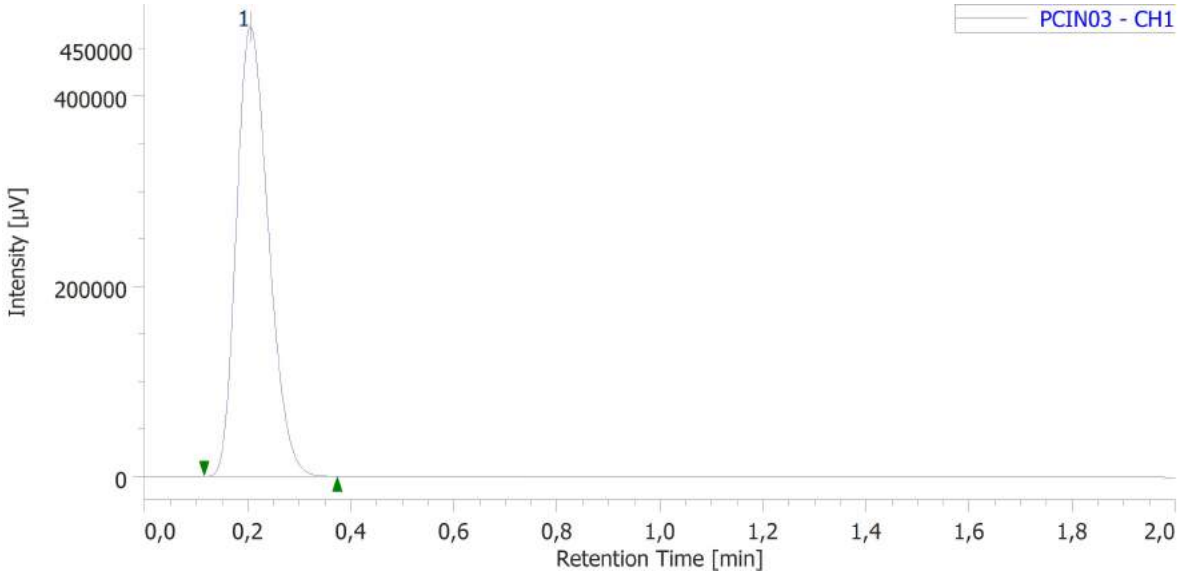


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:21:16
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:19:13
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,205	2039815	472598	100,000	100,000	N/A	52	N/A	1,253	

Chromatogram

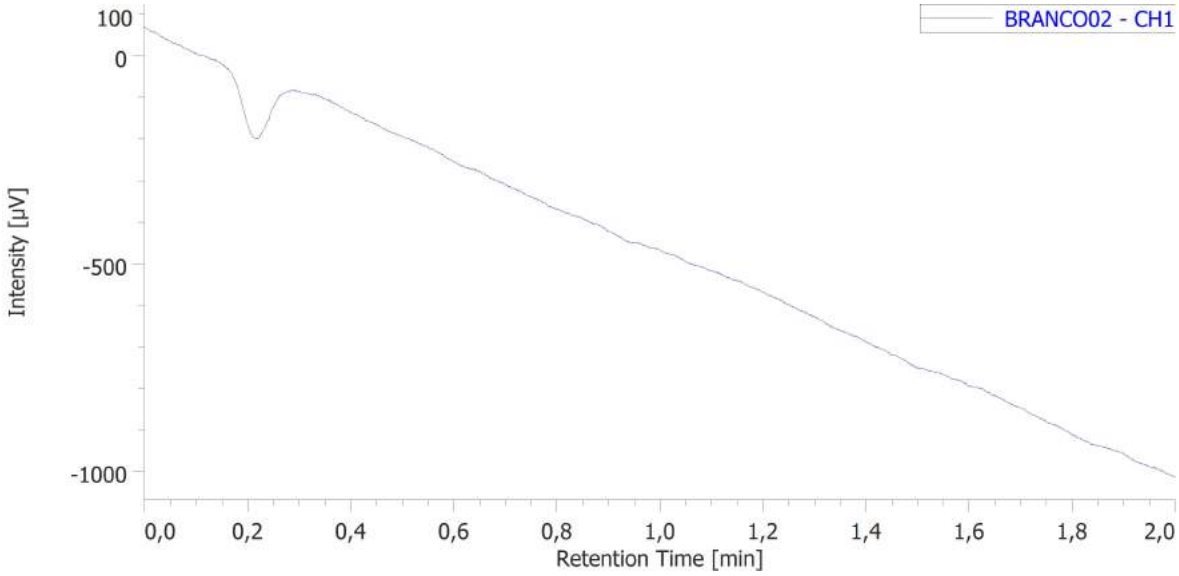


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:24:12
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:22:10
Volume	10,0 [µL]
Sample #	50
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

Chromatogram

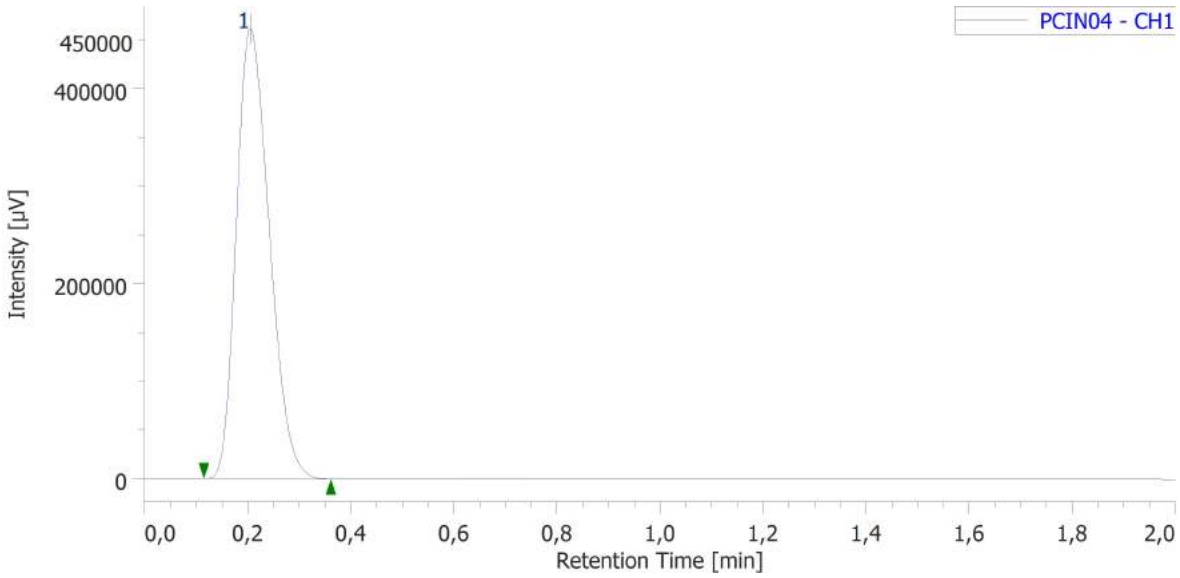


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:27:12
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:25:09
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,205	2052305	461682	100,000	100,000	N/A	48	N/A	1,275	

Chromatogram

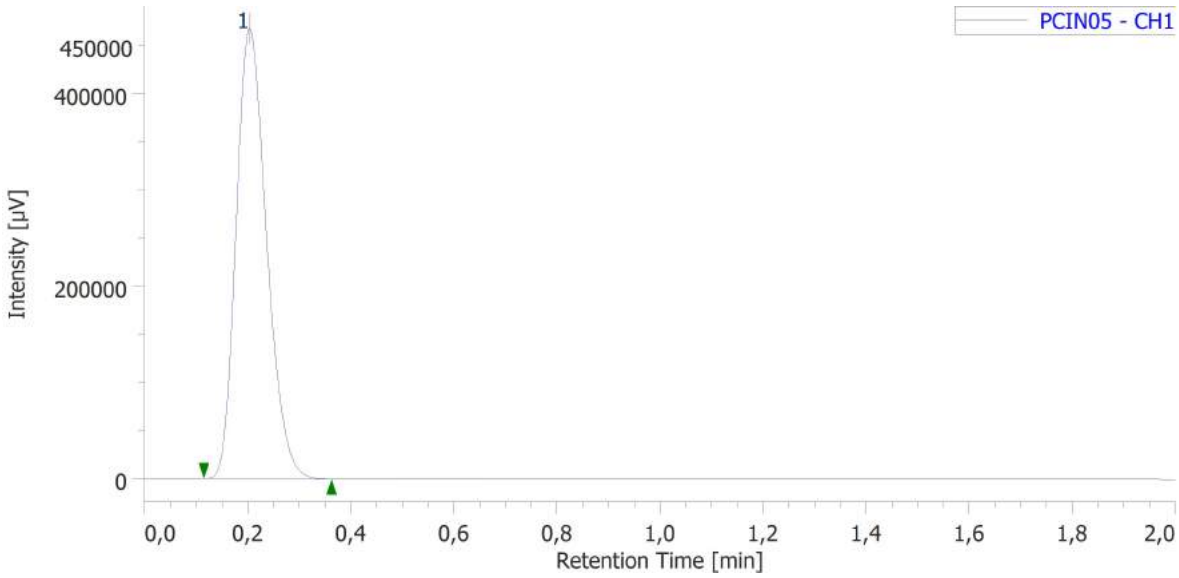


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:30:10
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:28:07
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,204	2019459	467110	100,000	100,000	N/A	57	N/A	1,236	

Chromatogram

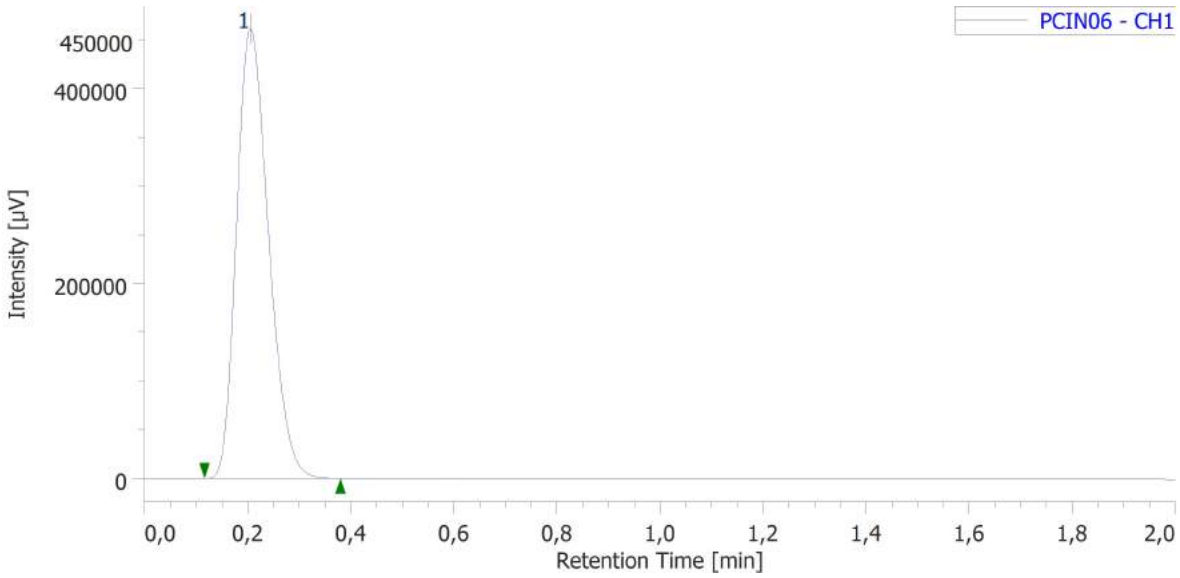


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:33:08
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:31:06
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,205	1992160	461222	100,000	100,000	N/A	52	N/A	1,268	

Chromatogram

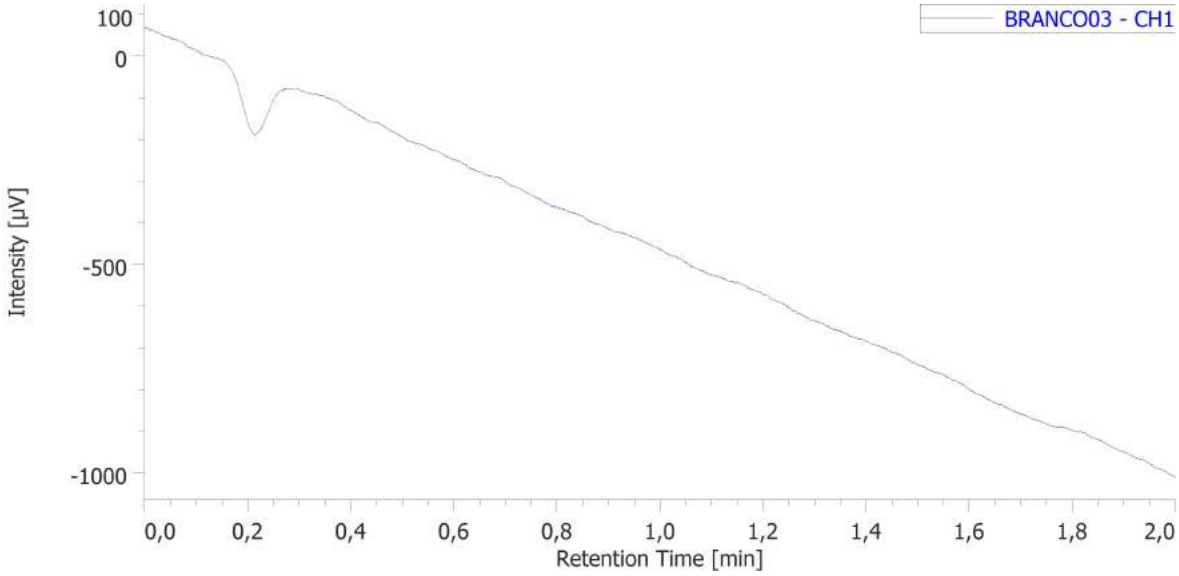


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:36:03
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:34:02
Volume	10,0 [µL]
Sample #	50
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

Chromatogram

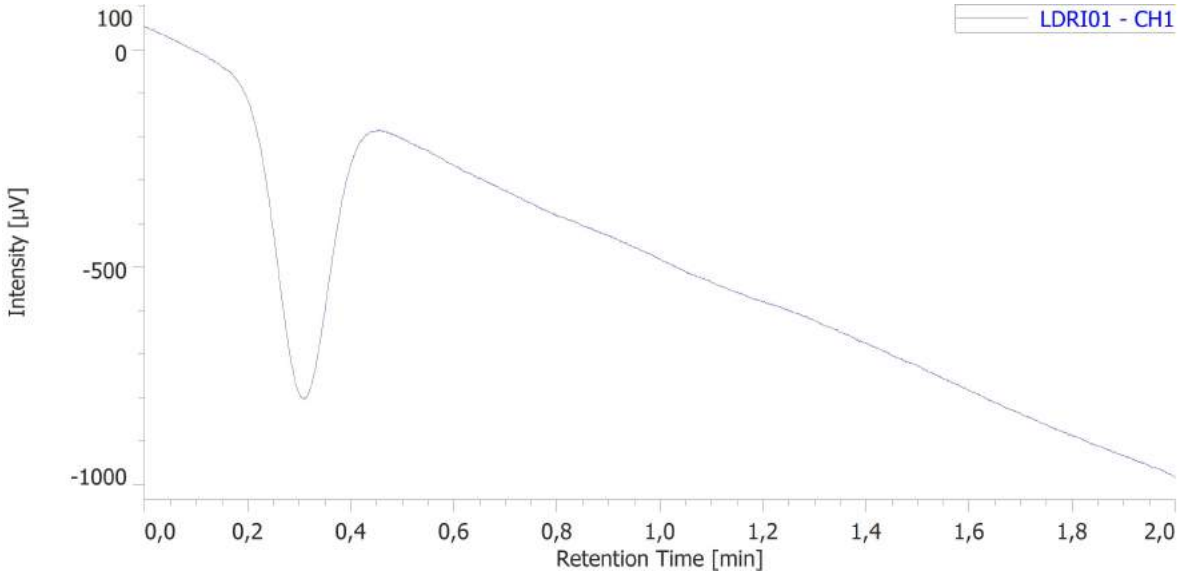


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 20:21:19
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 20:19:17
Volume	10,0 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

Chromatogram

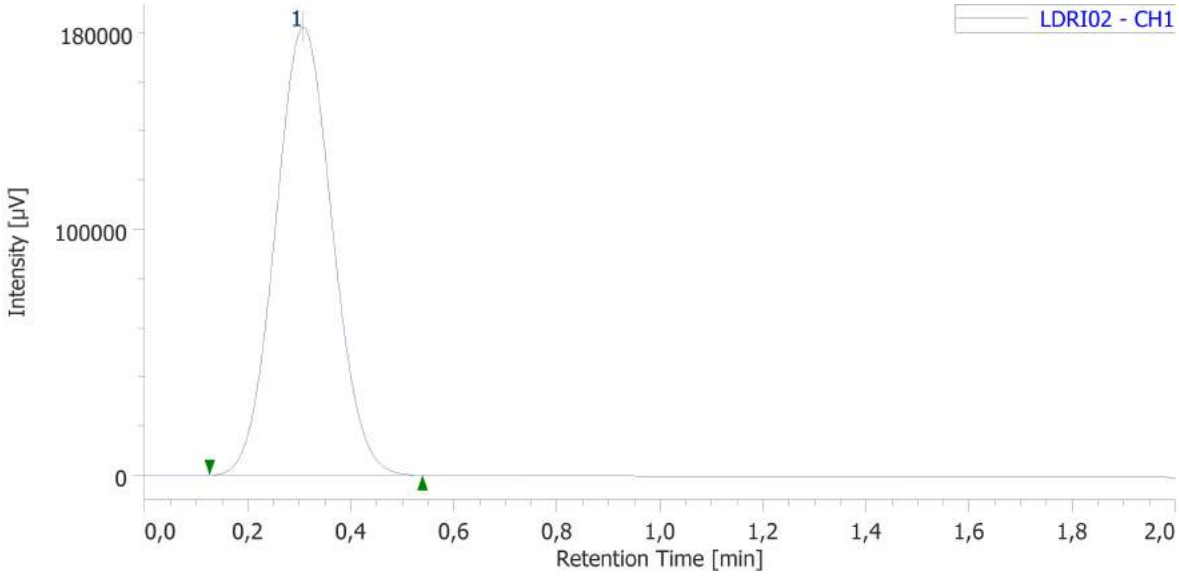


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 20:24:17
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 20:22:15
Volume	10,0 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,308	1402716	182257	100,000	100,000	N/A	36	N/A	1,055	

Chromatogram

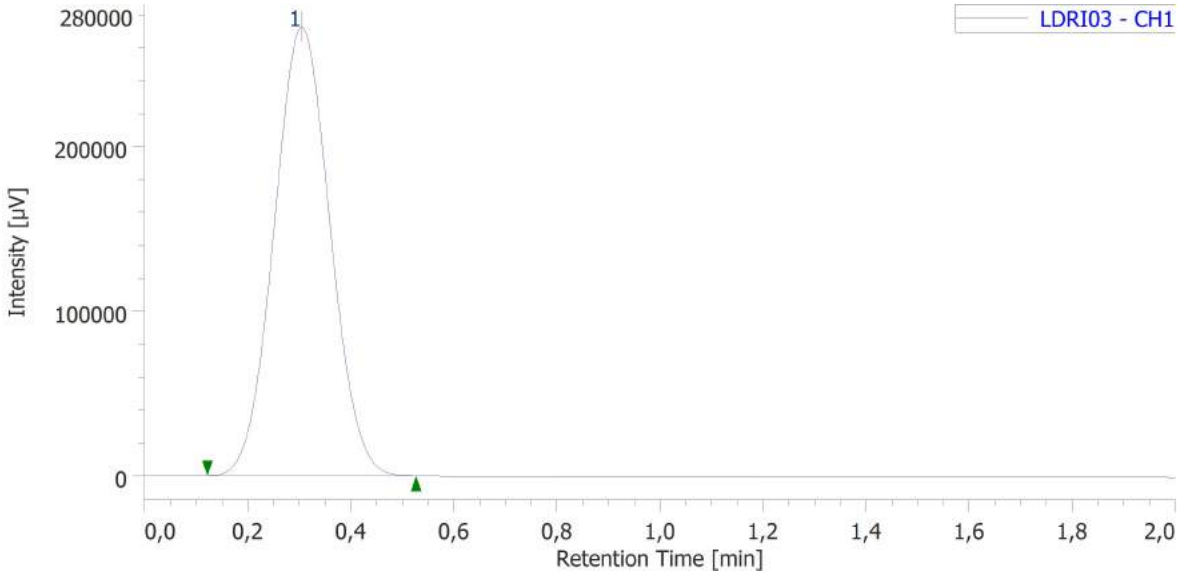


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 20:27:17
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 20:25:14
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,305	2058861	272579	100,000	100,000	N/A	37	N/A	1,042	

Chromatogram

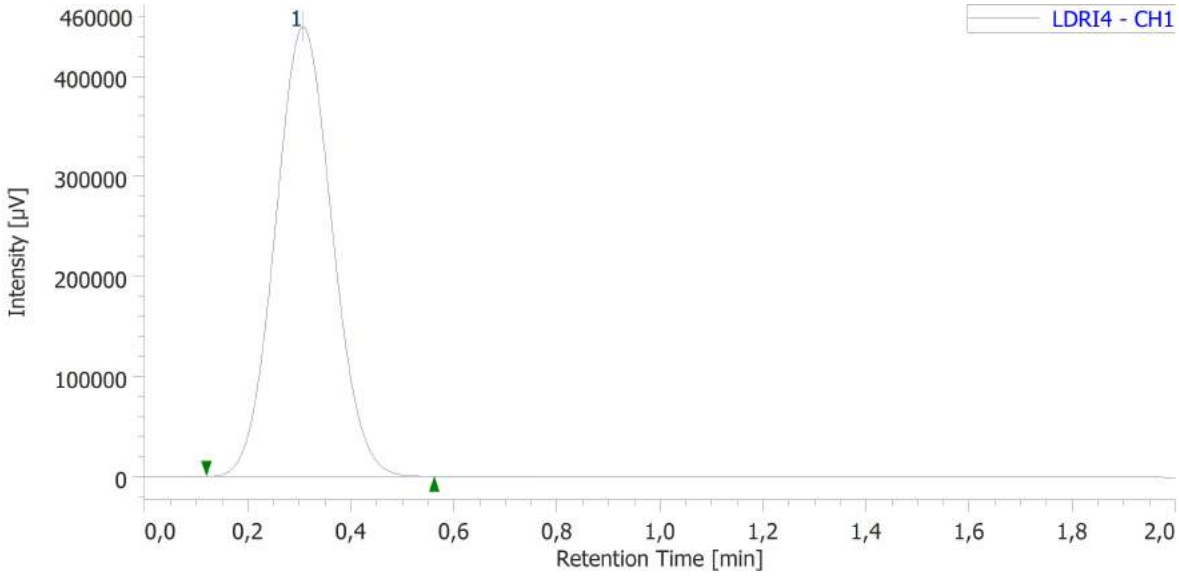


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 20:30:15
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 20:28:12
Volume	10,0 [µL]
Sample #	4
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,307	3455398	449150	100,000	100,000	N/A	36	N/A	1,059	

Chromatogram

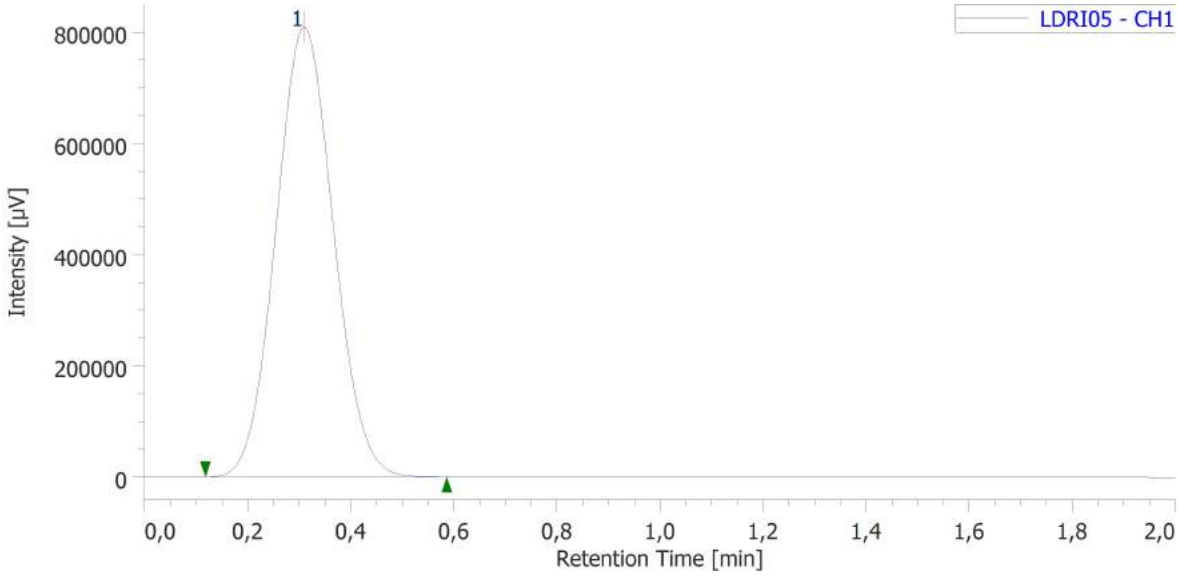

Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 20:33:13
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 20:31:11
Volume	10,0 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,309	6276731	809091	100,000	100,000	N/A	36	N/A	1,062	


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 18:38:55
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:36:53
Volume	0,1 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	
Column Info	

Chromatogram

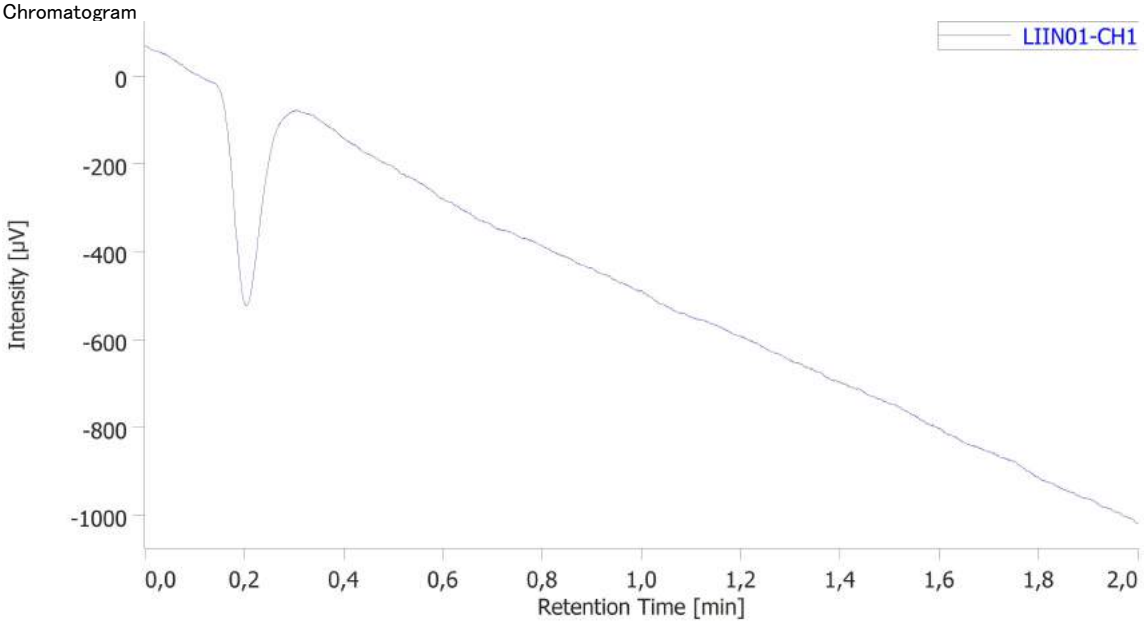

Peak Information – No data.

Chromatogram

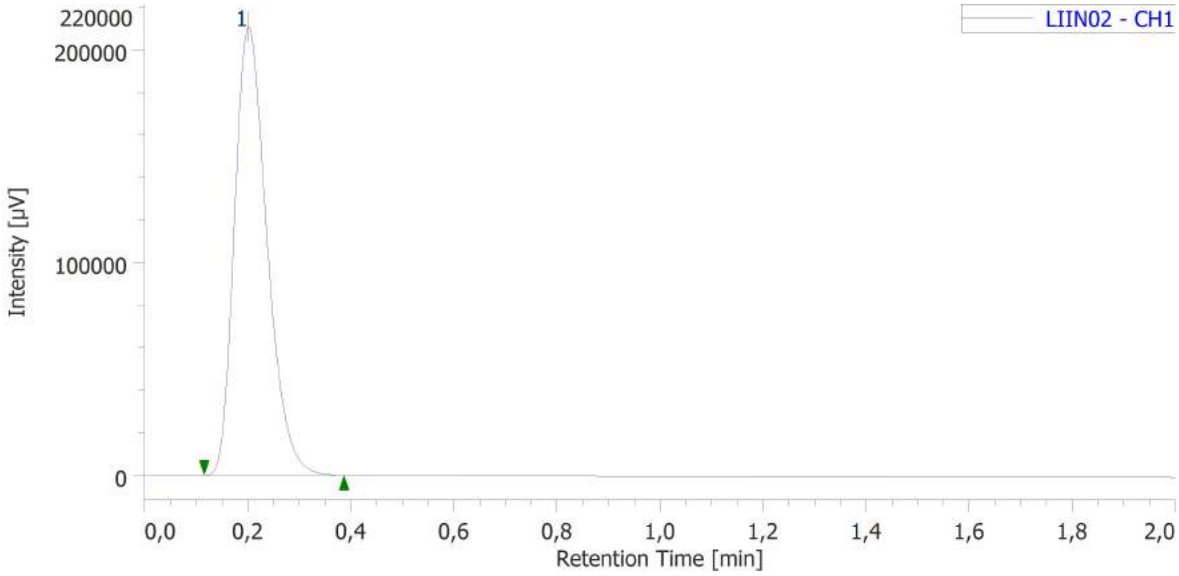


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 19:25:00
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:39:48
Volume	5,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,201	923158	210507	100,000	100,000	N/A	49	N/A	1,313	

Chromatogram

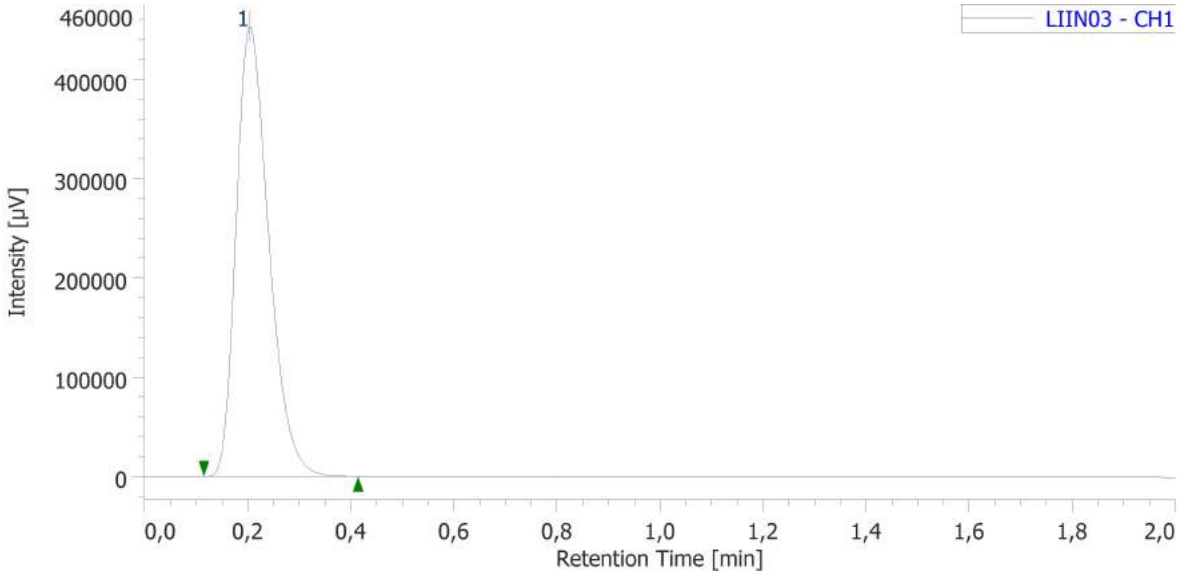


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 19:25:00
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:42:46
Volume	10,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,204	1991987	452523	100,000	100,000	N/A	50	N/A	1,346	

Chromatogram

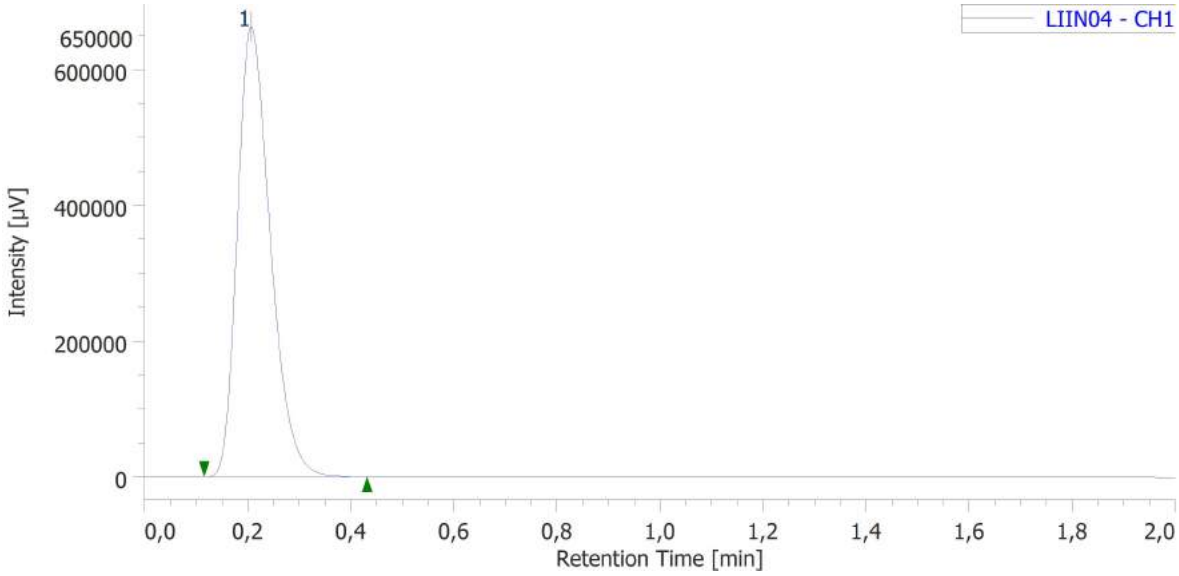


Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 19:25:00
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:45:47
Volume	15,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,207	2941886	662280	100,000	100,000	N/A	51	N/A	1,341	

Chromatogram

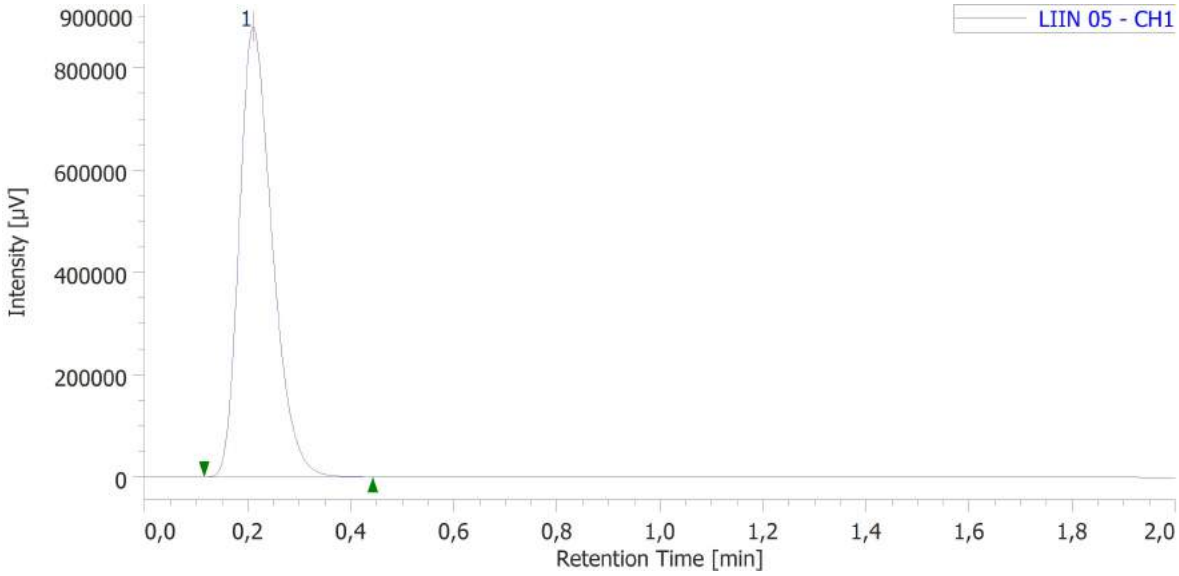

Chromatogram Information	
User Name	Administrator
Date Modified	15/02/2022 19:25:00
Description	
HPLC System Name	BBA HPLC 01
Injection Date	15/02/2022 18:48:52
Volume	20,0 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	2,0 [min]
Acquisition Sequence	OQ HPLC_01 FEV_2022
Control Method	Qualificação
Peak ID Table	ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Integração Trein

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão	1	0,211	3899995	879513	100,000	100,000	N/A	53	N/A	1,326	