

PDA

Sequence Name EDUV_1113 13/11/2025 11:34:11
Chromatogram Name EDUV_001
Sample Name

Contour+Chrom+Spec

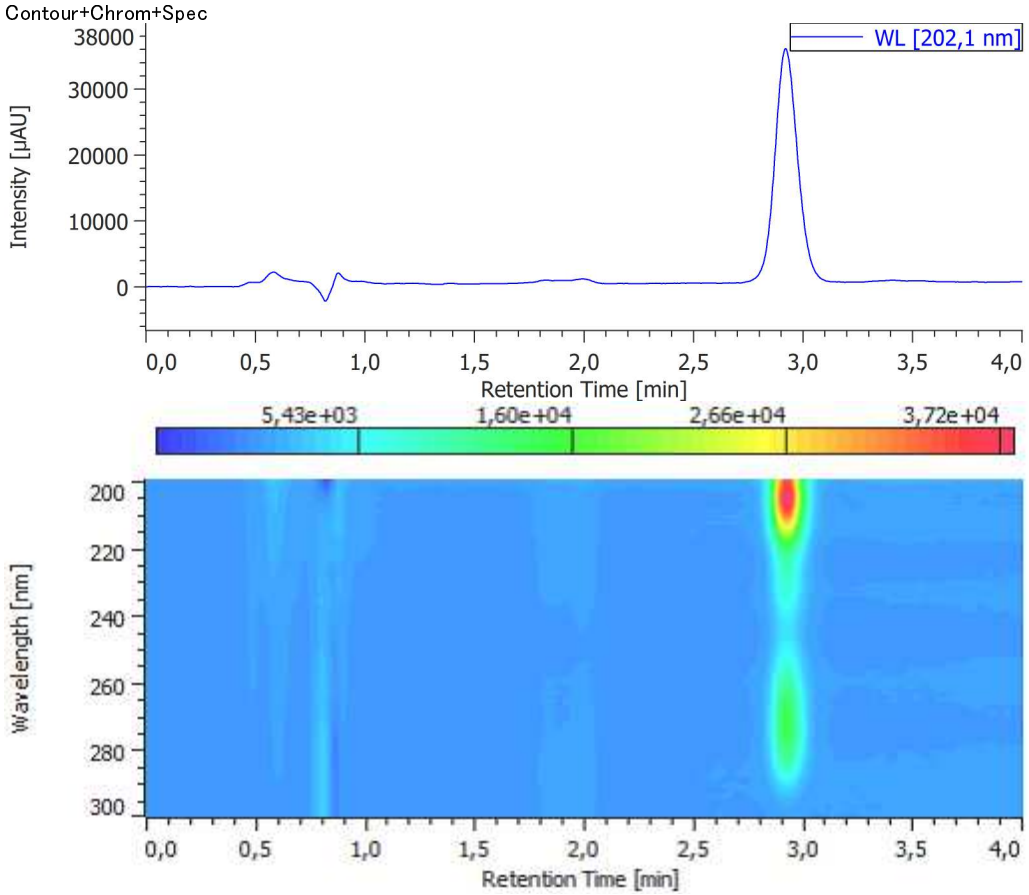


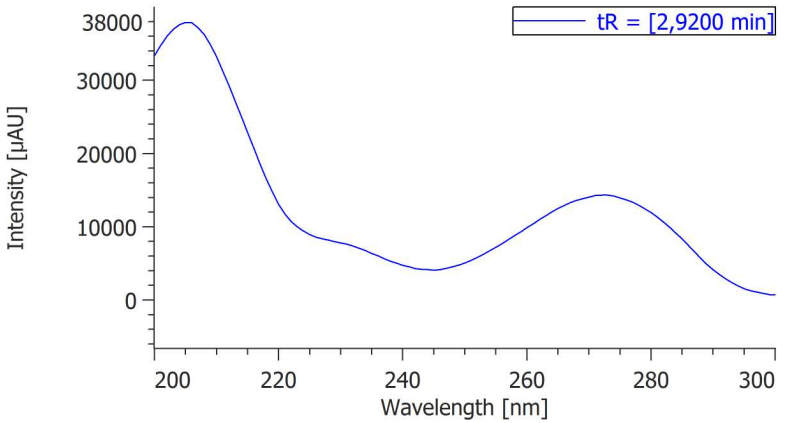


PDA

Sequence Name EDUV_1113 13/11/2025 11:34:11
Chromatogram Name EDUV_001
Sample Name

Contour+Chrom+Spec

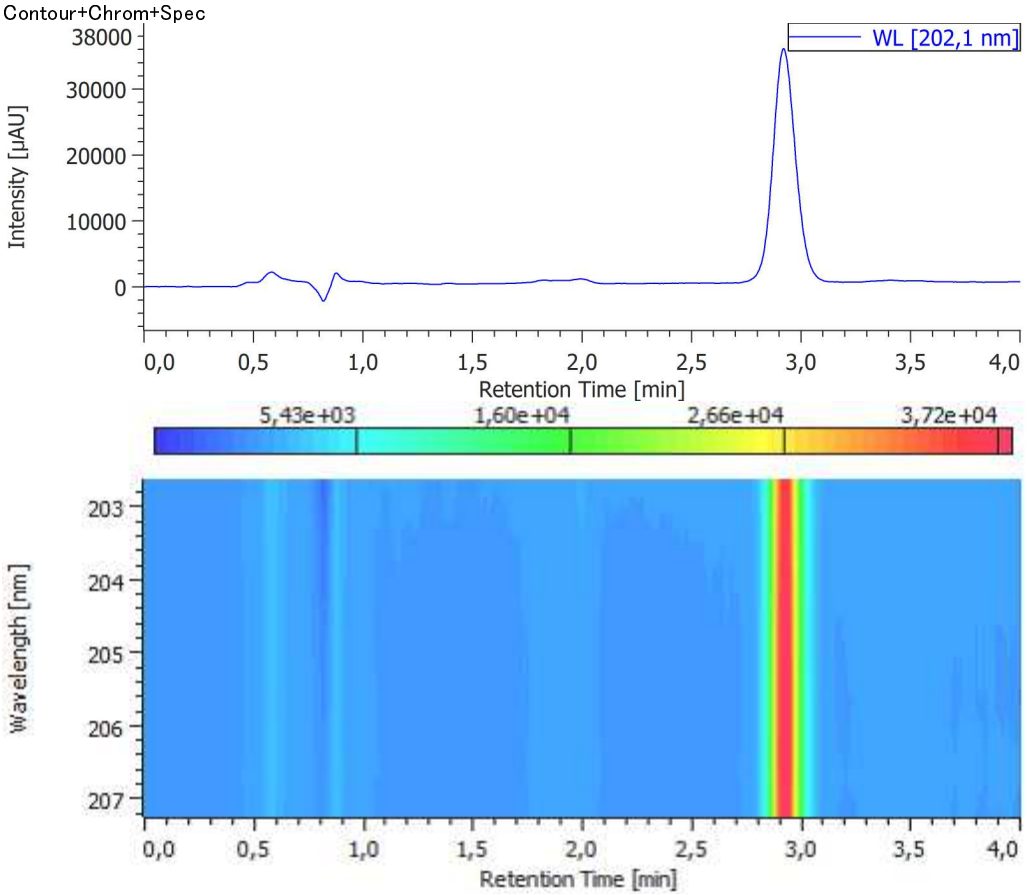


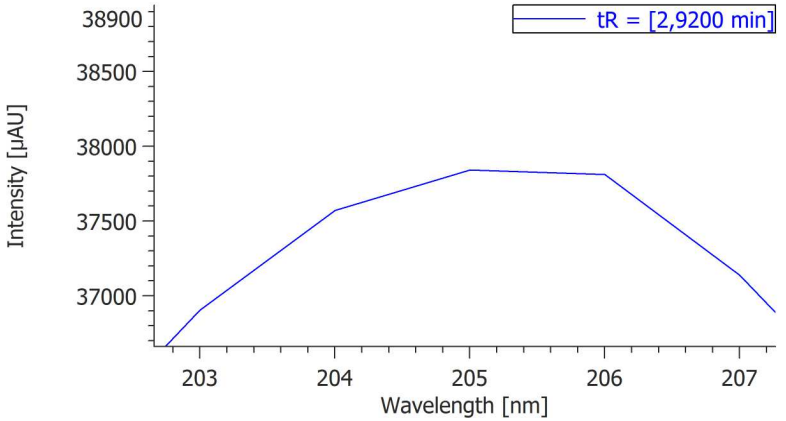


PDA

Sequence Name EDUV_1113 13/11/2025 11:34:11
Chromatogram Name EDUV_001
Sample Name

Contour+Chrom+Spec

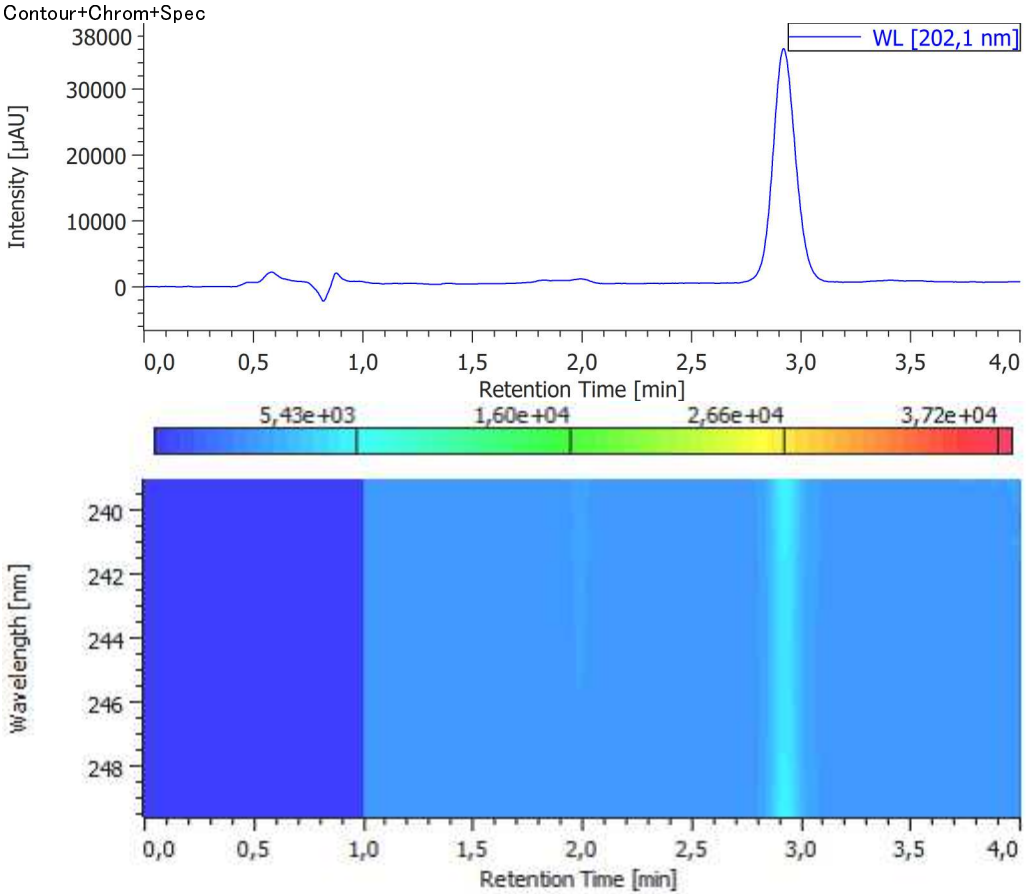


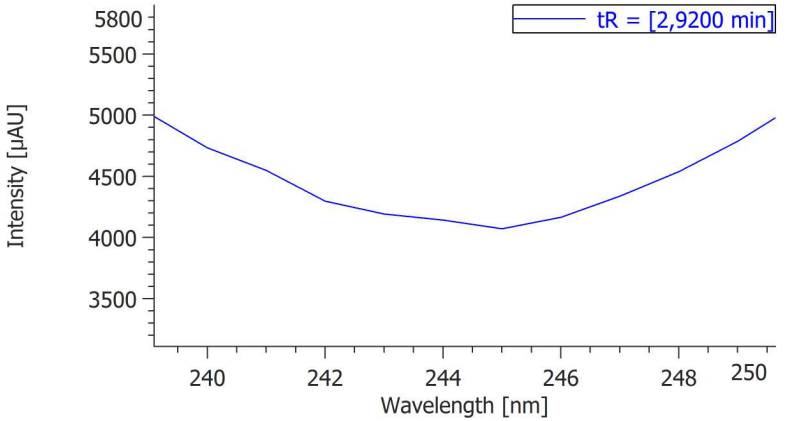


PDA


Sequence Name EDUV_1113 13/11/2025 11:34:11
Chromatogram Name EDUV_001
Sample Name

Contour+Chrom+Spec

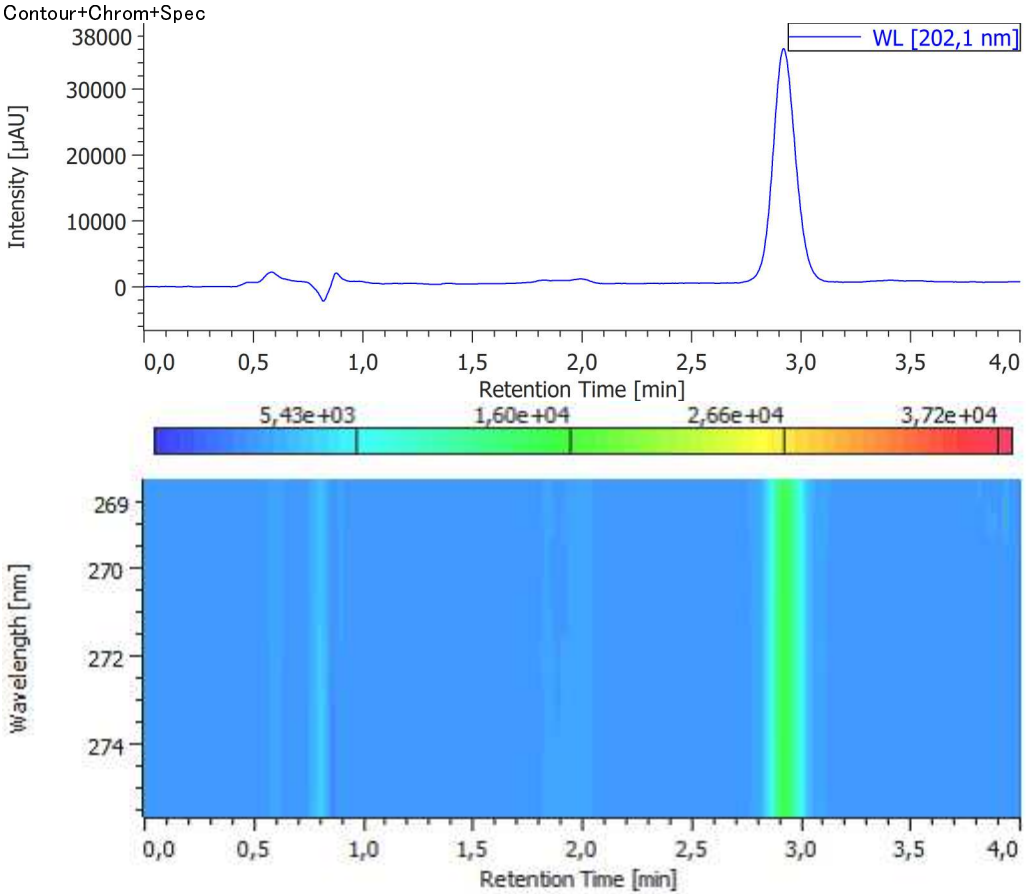

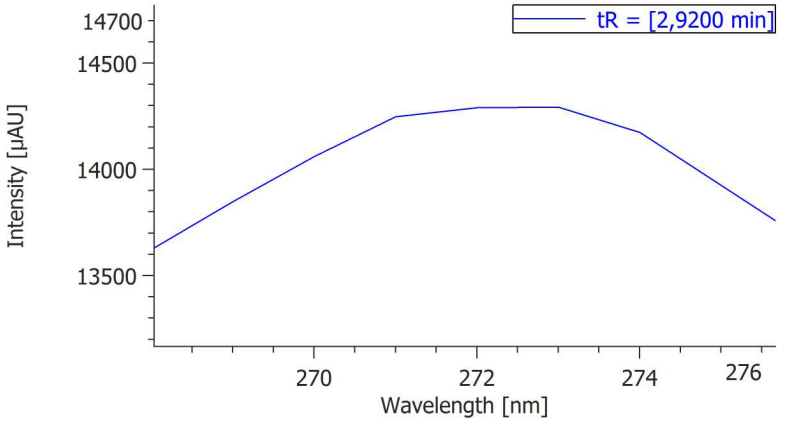

Chromatogram

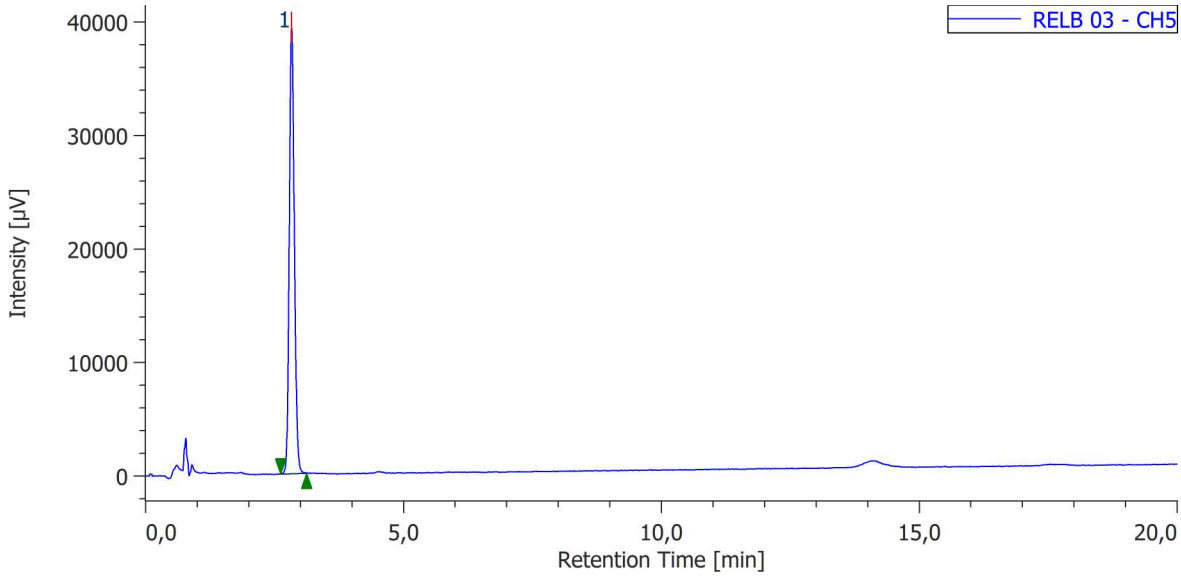

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:54:43
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:34:42
Volume	20,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	RELB
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 03-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,827	268710	39277	100,000	100,000	N/A	4032	N/A	1,167	

Creator
Reviewer
Approver

Chromatogram

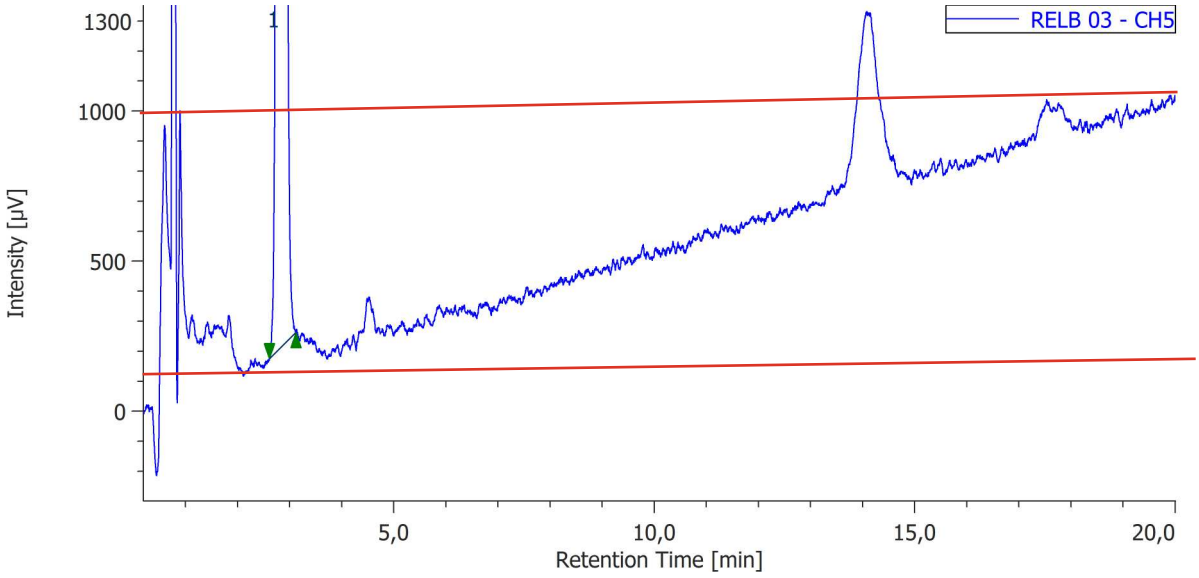

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:54:43
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:34:42
Volume	20,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	RELB
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 03-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,827	268710	39277	100,000	100,000	N/A	4032	N/A	1,167	

Creator
Reviewer
Approver

Chromatogram

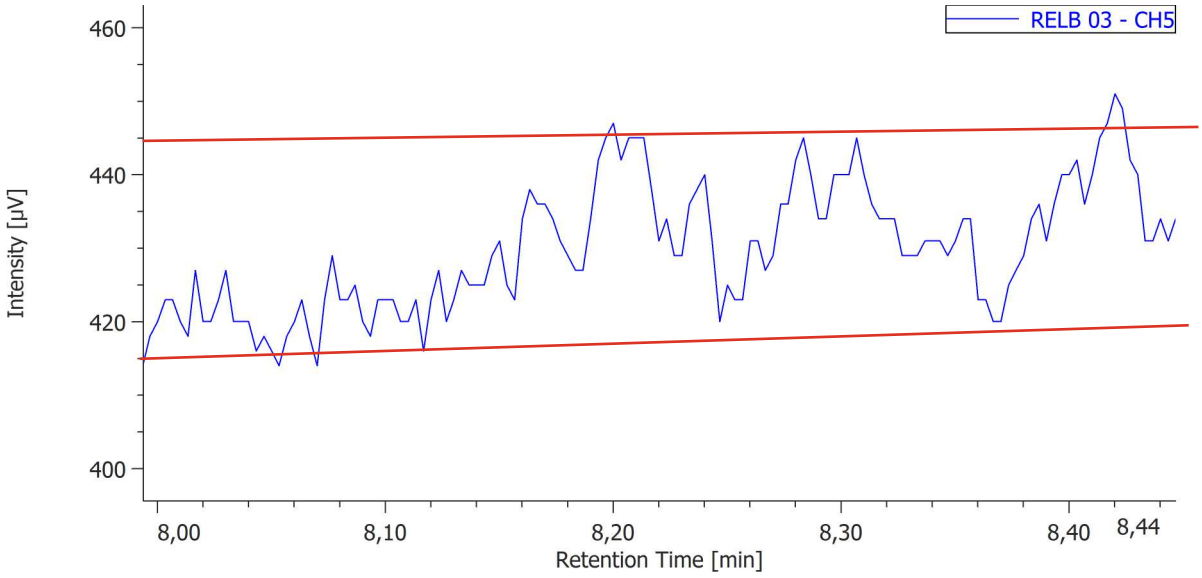

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:54:43
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:34:42
Volume	20,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	RELB
Control Method	RELB
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 03-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,827	268710	39277	100,000	100,000	N/A	4032	N/A	1,167	

Creator
Reviewer
Approver

Chromatogram

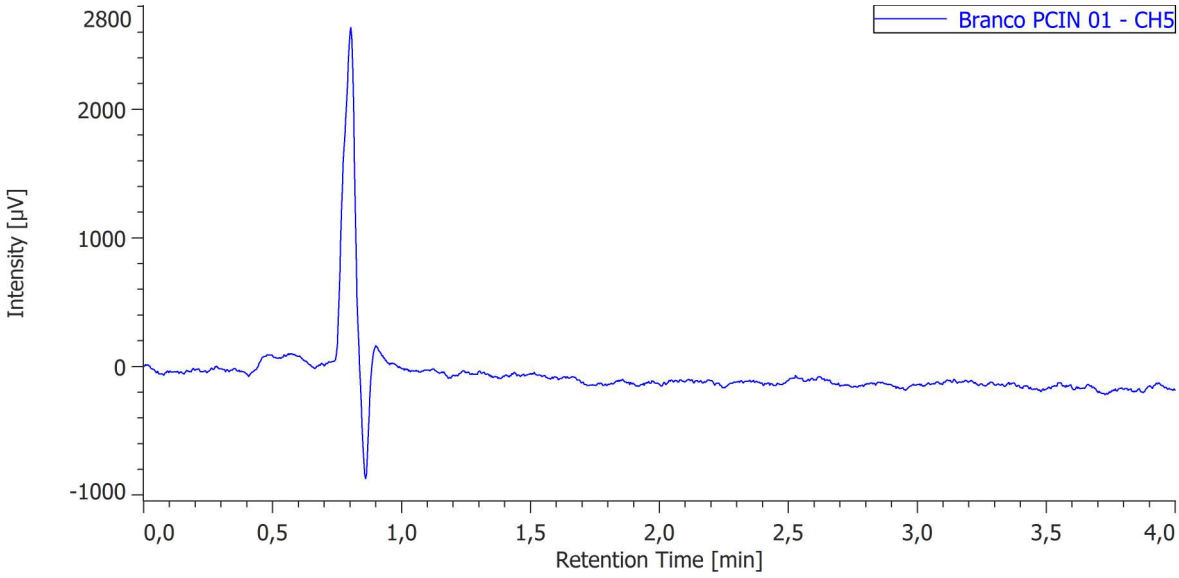


Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 12:40:43
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:36:42
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

Creator
Reviewer
Approver

Chromatogram

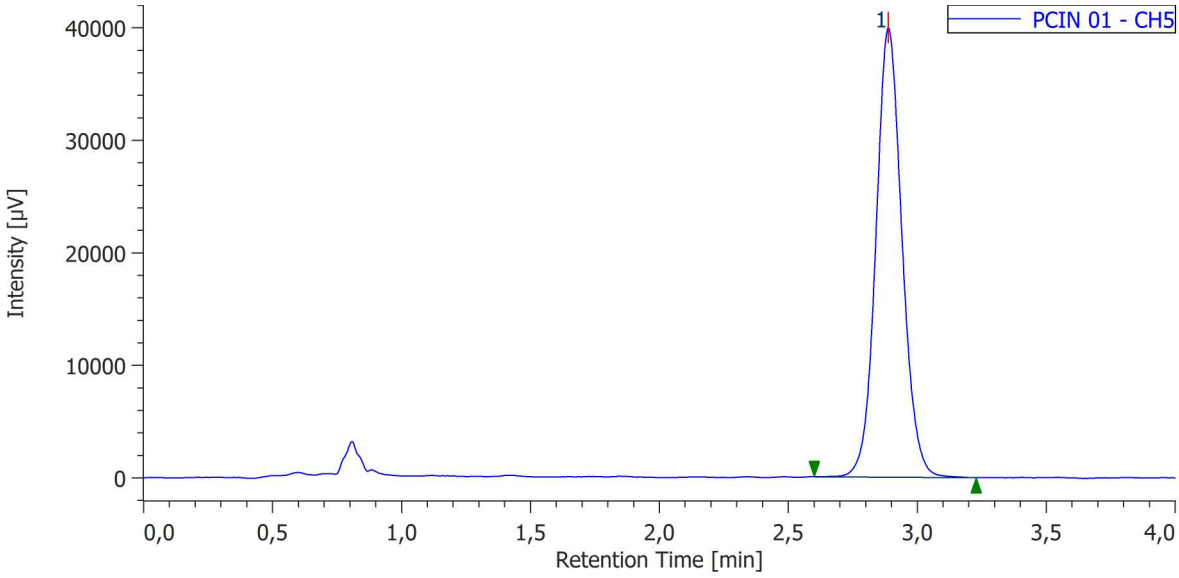

Chromatogram Information

User Name	QPackSA
Date Modified	13/11/2025 12:44:55
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:40:54
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.887	281238	39941	100.000	100.000	N/A	4075	N/A	1.078	

Creator
Reviewer
Approver

Chromatogram

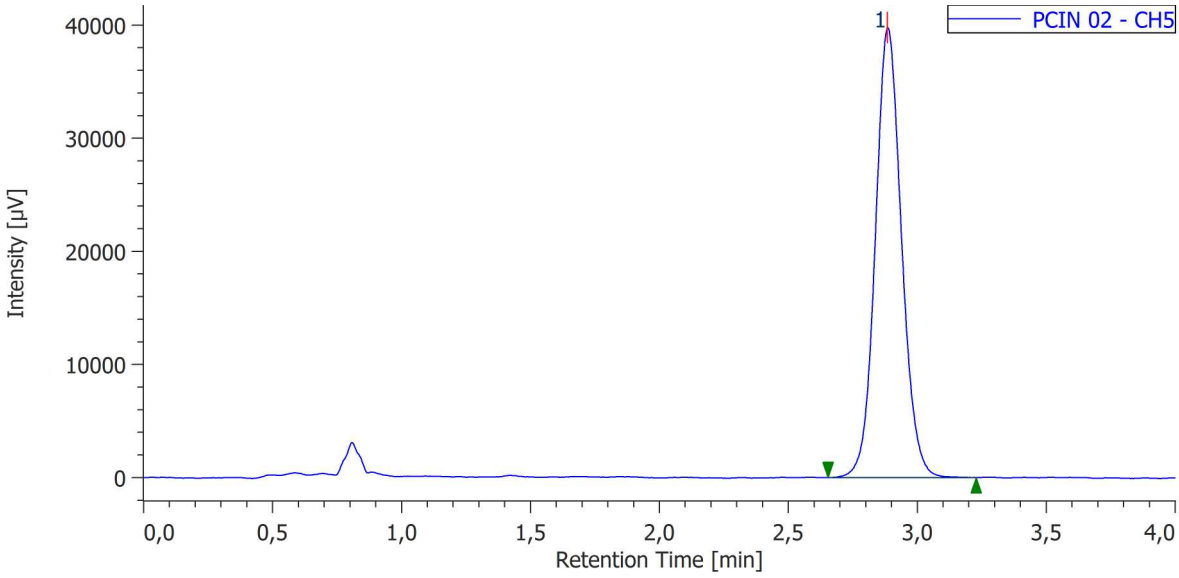

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 12:49:07
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:45:06
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.883	280948	39769	100.000	100.000	N/A	4024	N/A	1.096	

Creator
Reviewer
Approver

Chromatogram

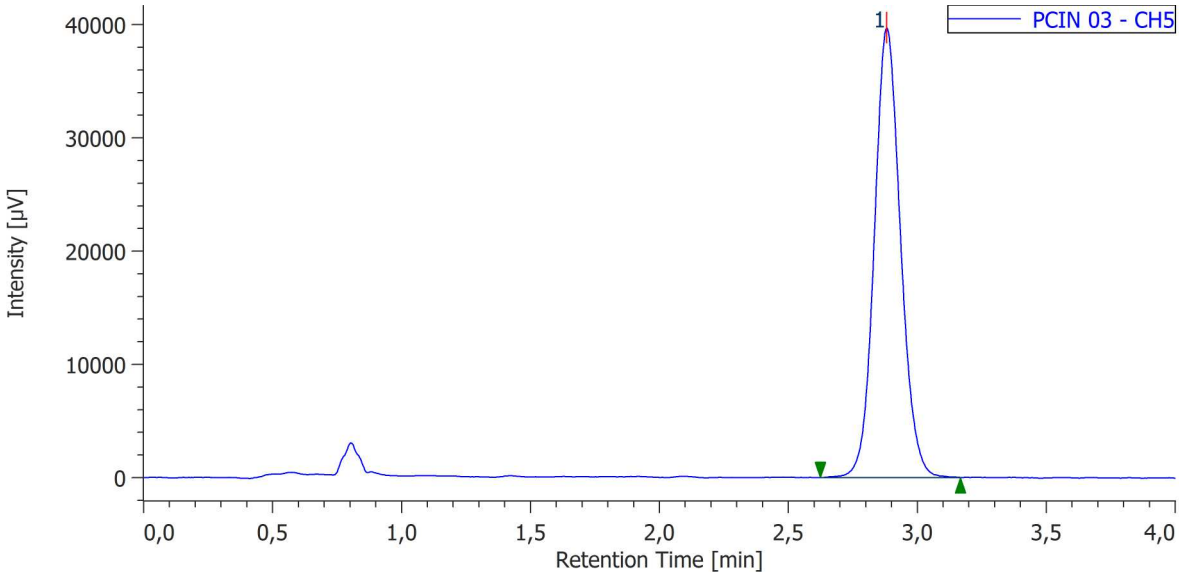

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 12:53:19
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:49:18
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.880	280627	39717	100.000	100.000	N/A	4003	N/A	1.100	

Creator
Reviewer
Approver

Chromatogram

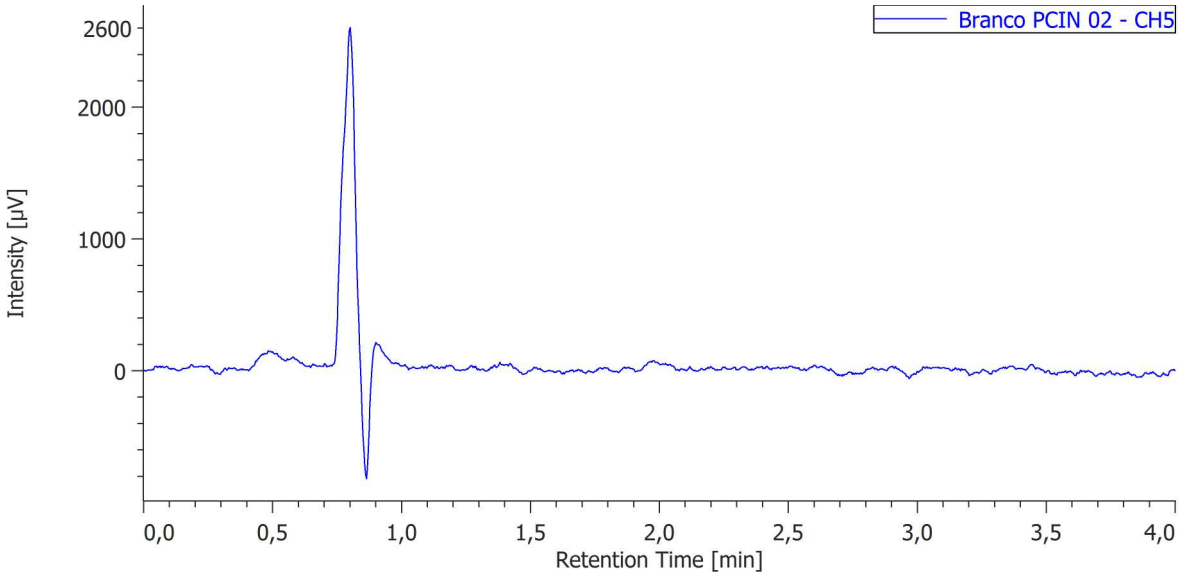


Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 12:57:31
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:53:30
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

Creator
Reviewer
Approver

Chromatogram

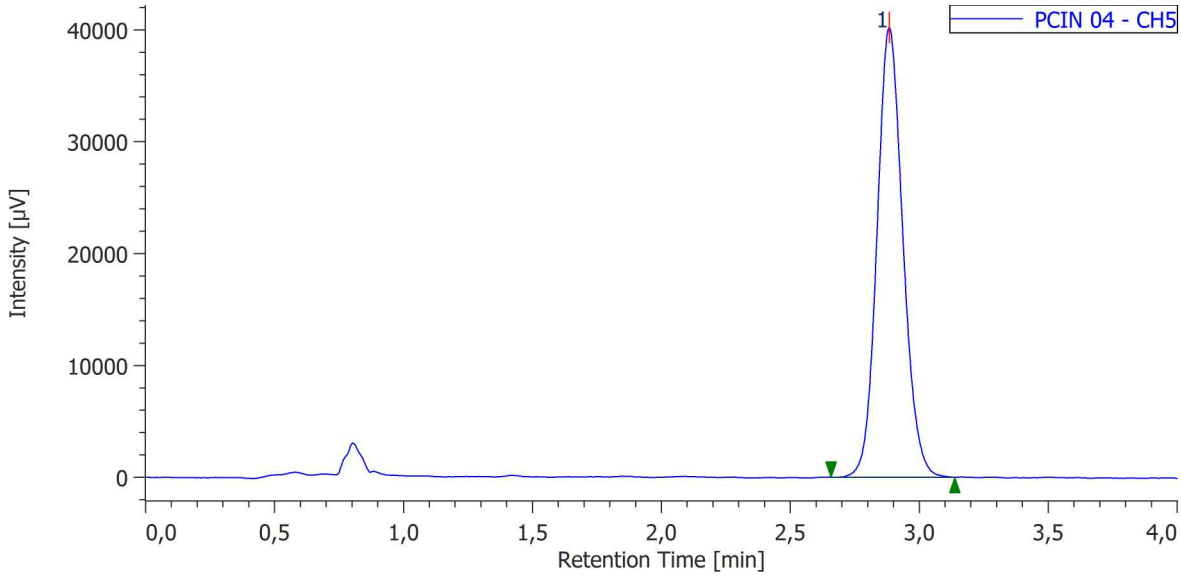

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:01:43
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 12:57:42
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.883	280619	40180	100.000	100.000	N/A	4060	N/A	1.101	

Creator
Reviewer
Approver

Chromatogram

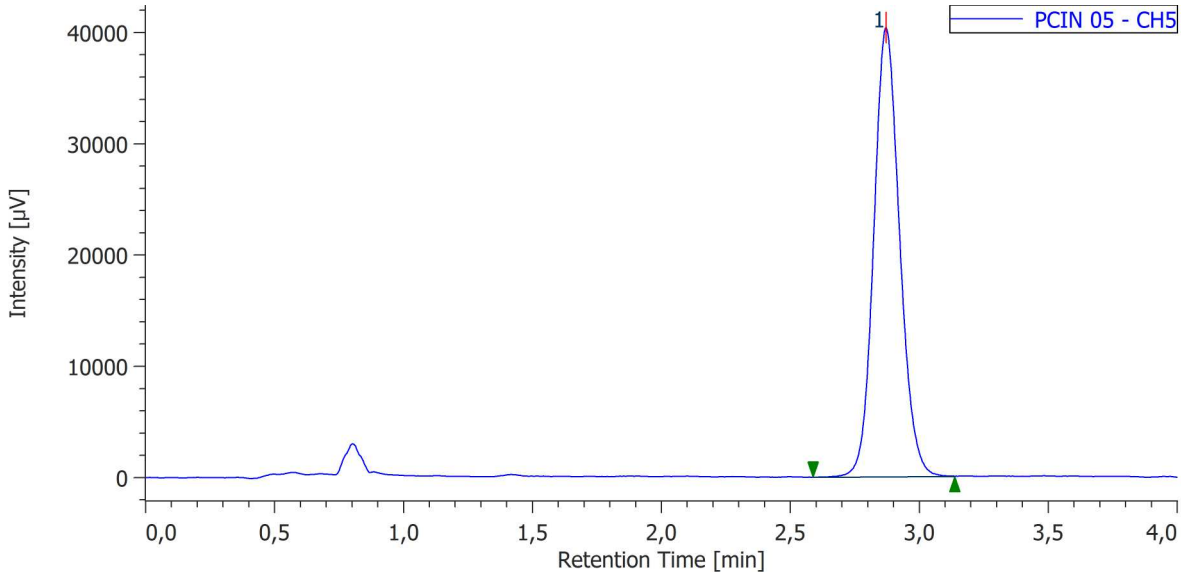

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:05:55
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:01:54
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.870	281339	40348	100.000	100.000	N/A	4048	N/A	1.111	

Creator
Reviewer
Approver

Chromatogram

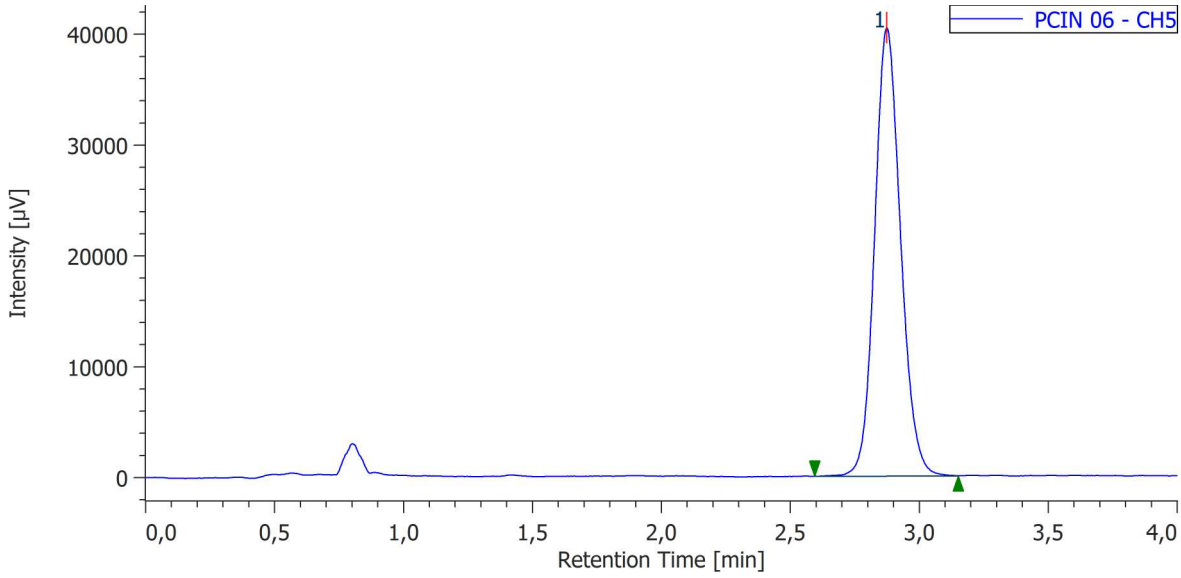

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:10:07
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:06:06
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.873	282551	40434	100.000	100.000	N/A	4040	N/A	1.117	

Creator
Reviewer
Approver

Chromatogram

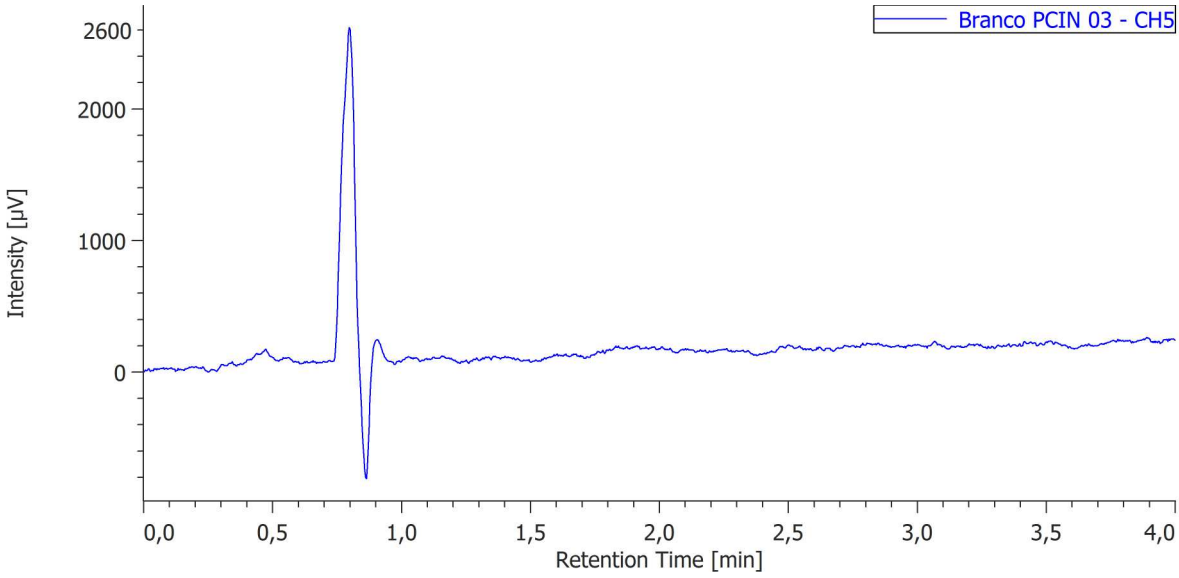


Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 13:14:19
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 13:10:18
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	RELB
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

Creator
Reviewer
Approver

Chromatogram

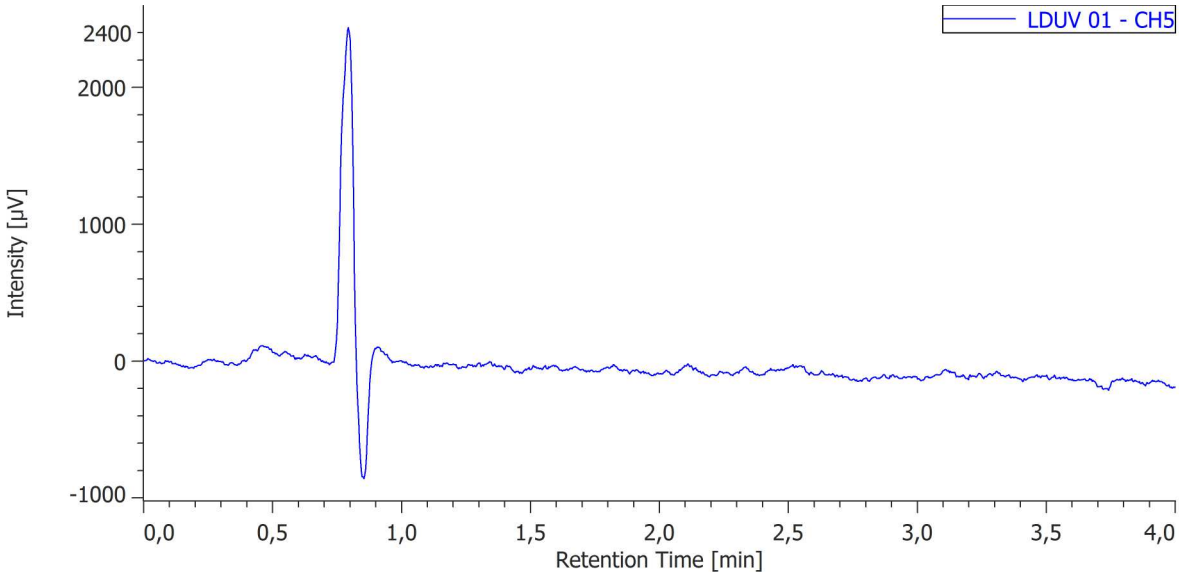


Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:15:46
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:11:45
Volume	10.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

Creator
Reviewer
Approver

Chromatogram

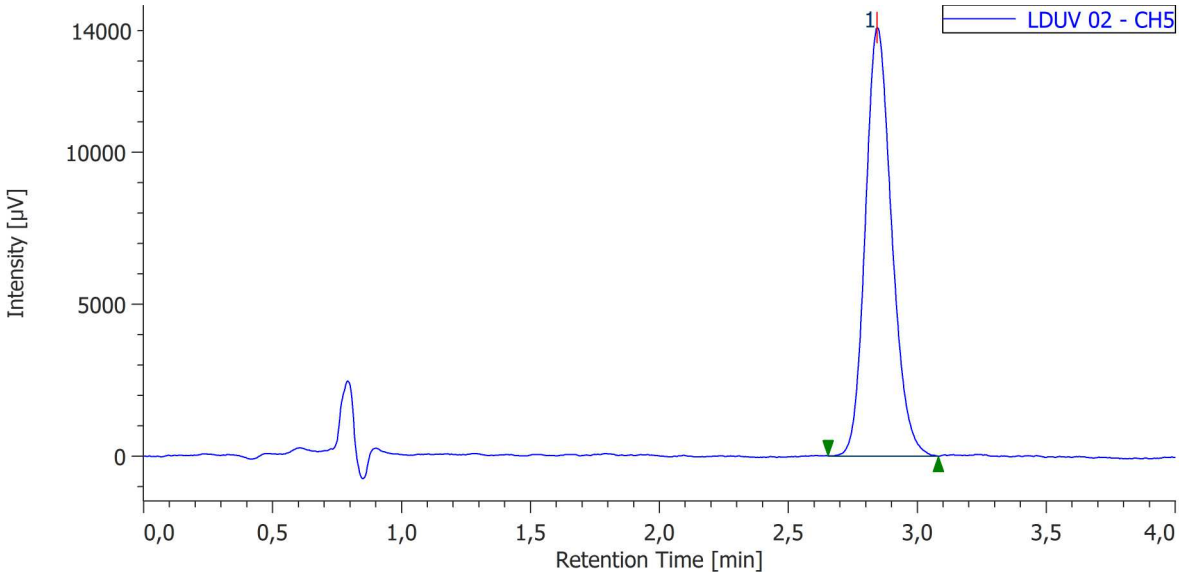

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:19:57
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:15:57
Volume	10.0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.843	100120	14085	100.000	100.000	N/A	3795	N/A	1.189	

Creator
Reviewer
Approver

Chromatogram

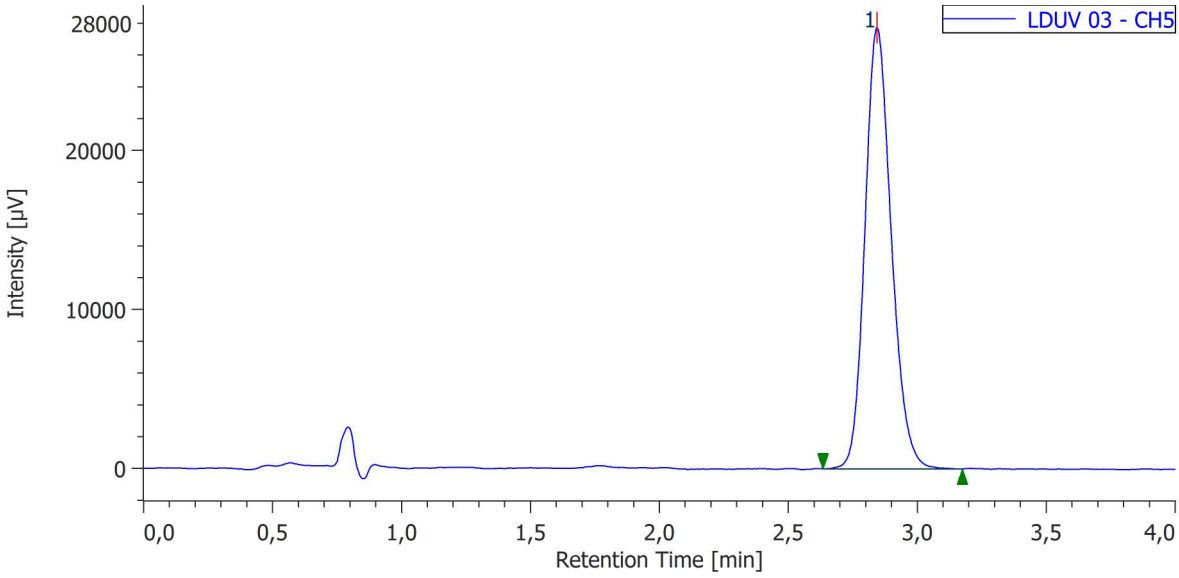

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:24:10
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:20:09
Volume	10.0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.843	197328	27742	100.000	100.000	N/A	3818	N/A	1.170	

Creator
Reviewer
Approver

Chromatogram

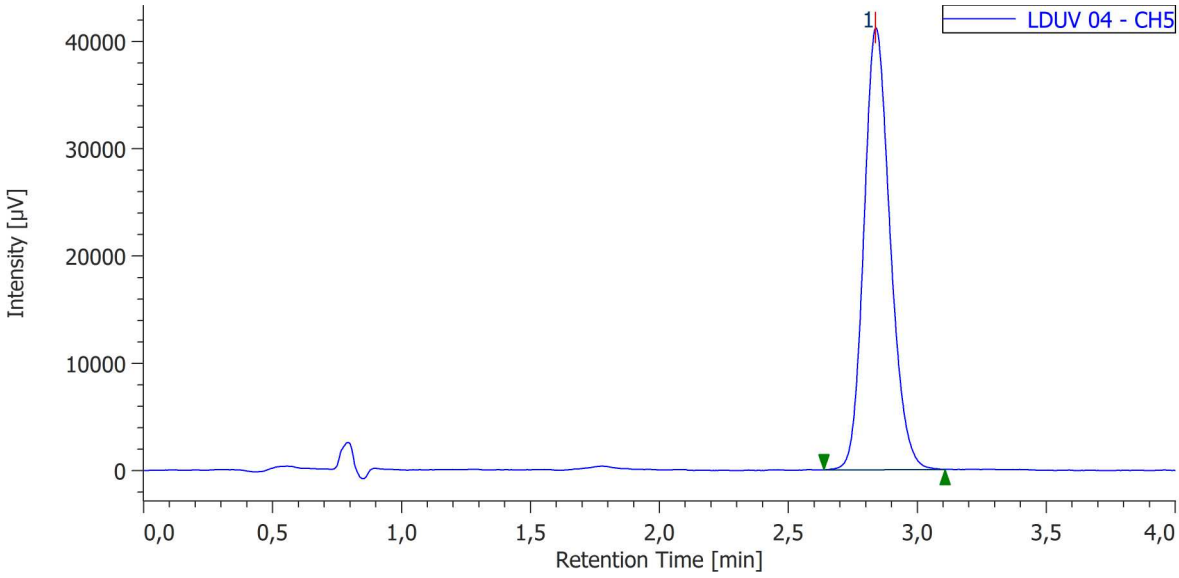

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:28:22
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:24:21
Volume	10.0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.837	291437	41181	100.000	100.000	N/A	3820	N/A	1.195	

Creator
Reviewer
Approver

Chromatogram

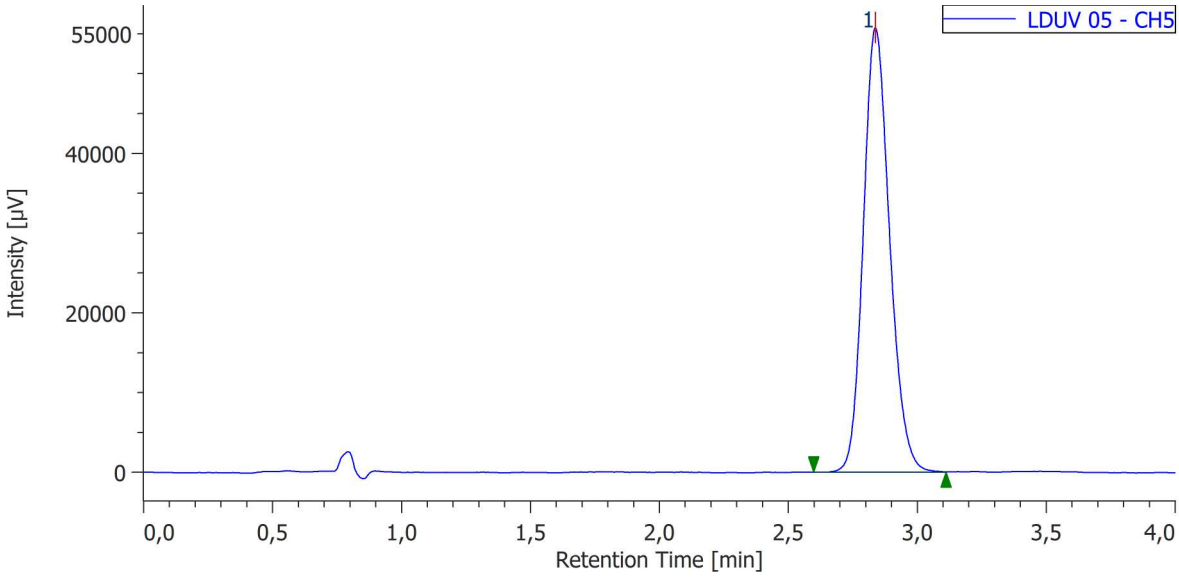

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:32:34
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:28:33
Volume	10.0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.837	394903	55724	100.000	100.000	N/A	3800	N/A	1.165	

Creator
Reviewer
Approver

Chromatogram

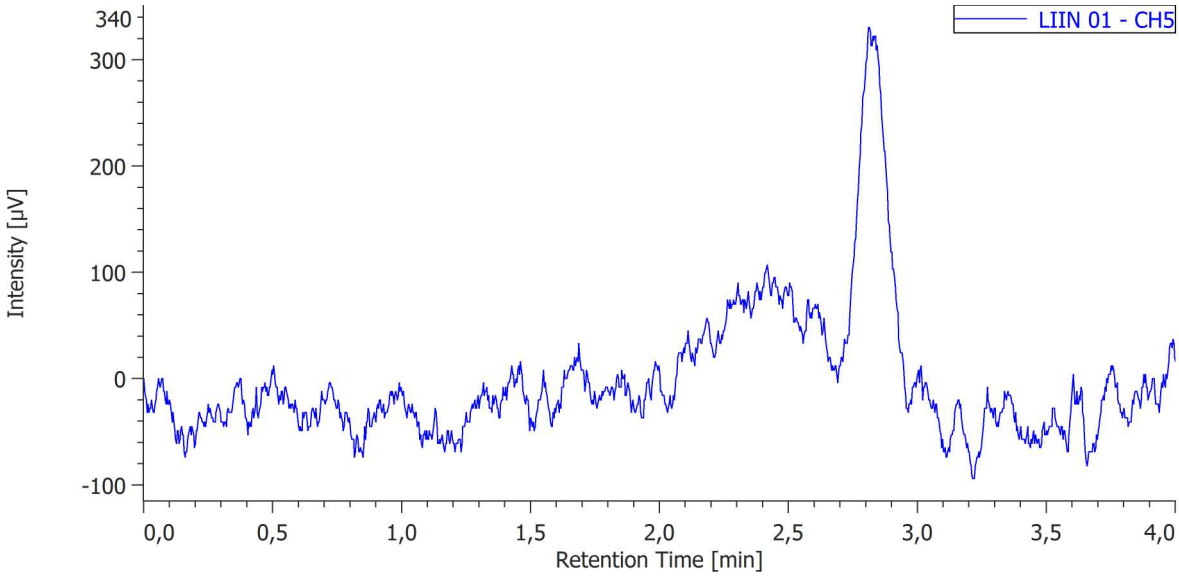


Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:40:15
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:36:13
Volume	0.1 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

Creator
Reviewer
Approver

Chromatogram

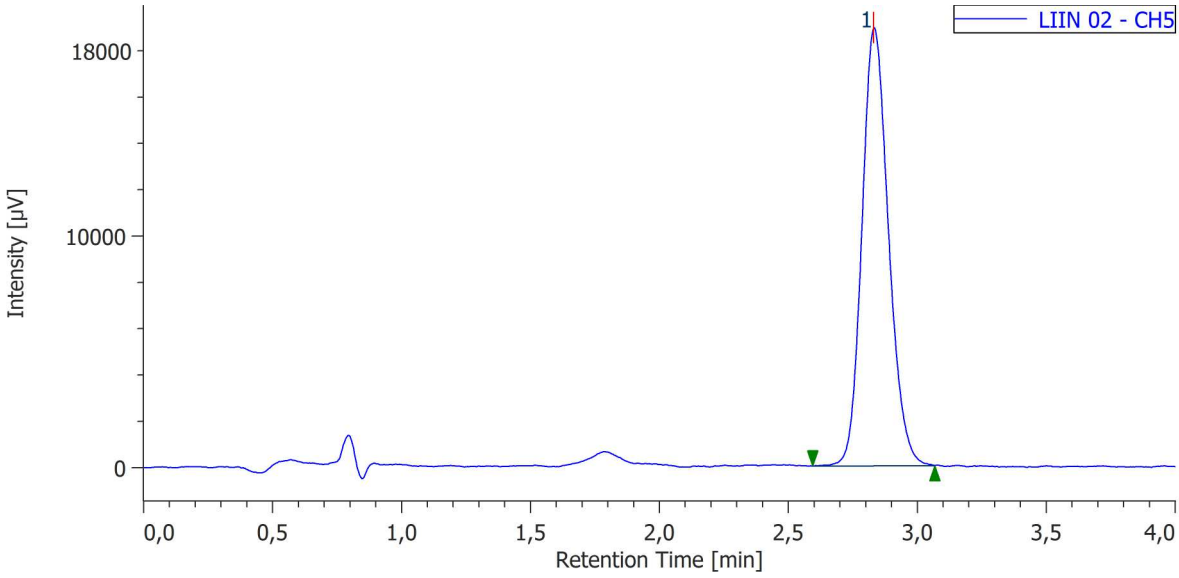

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:44:27
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:40:25
Volume	5.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.830	135363	18908	100.000	100.000	N/A	3688	N/A	1.181	

Creator
Reviewer
Approver

Chromatogram

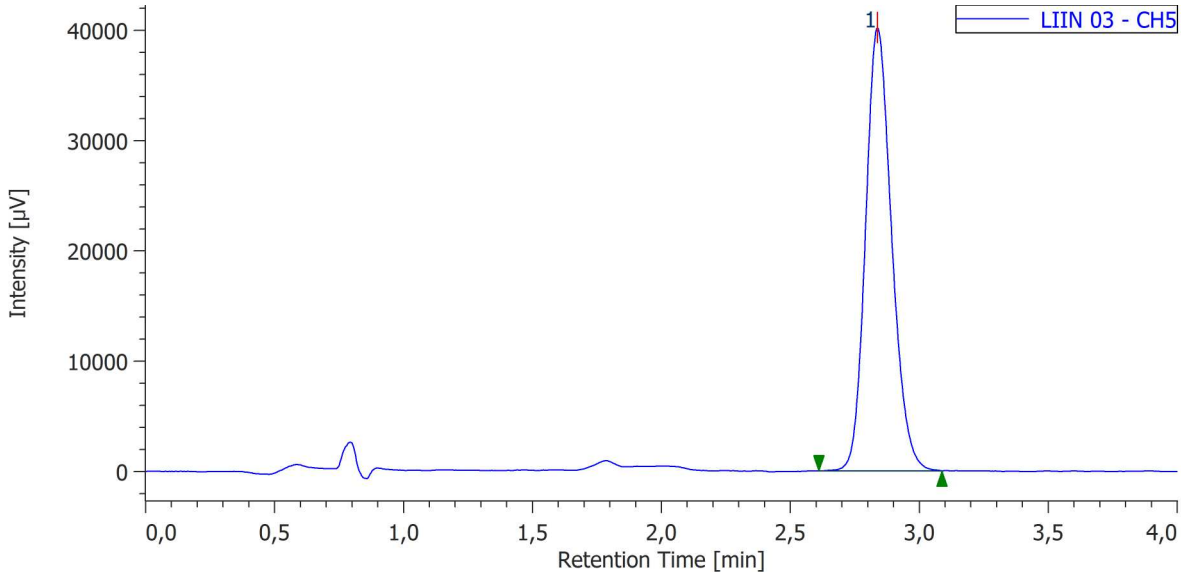

Chromatogram Information

User Name	QPackSA
Date Modified	13/11/2025 17:48:39
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:44:37
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.837	283022	40175	100.000	100.000	N/A	3841	N/A	1.176	

Creator
Reviewer
Approver

Chromatogram

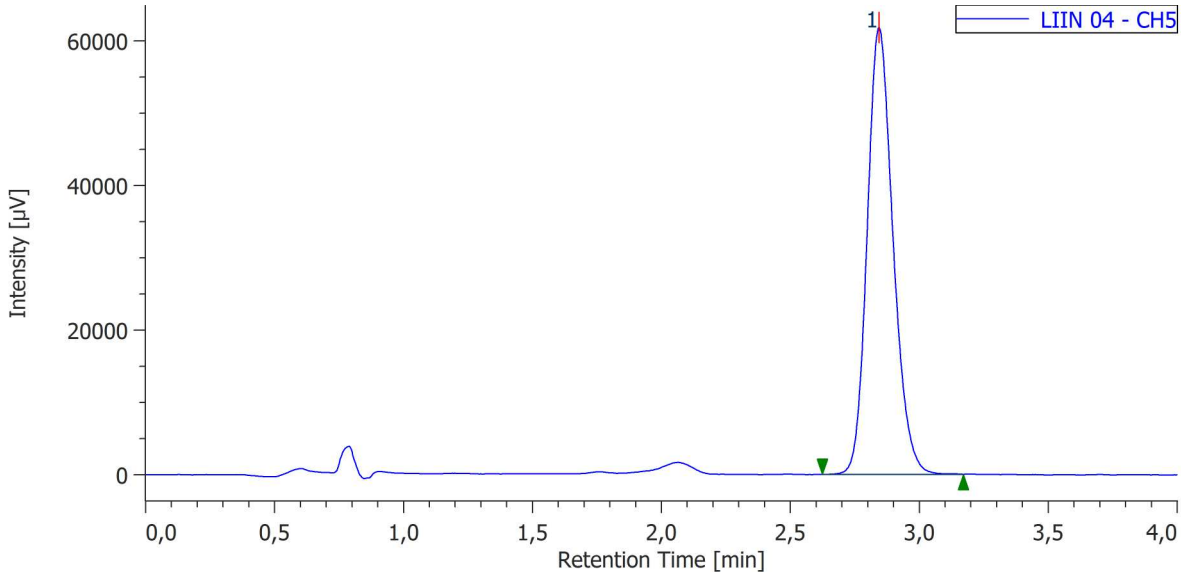

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:52:51
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:48:49
Volume	15,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,843	430273	61746	100,000	100,000	N/A	3971	N/A	1,174	

Creator
Reviewer
Approver

Chromatogram

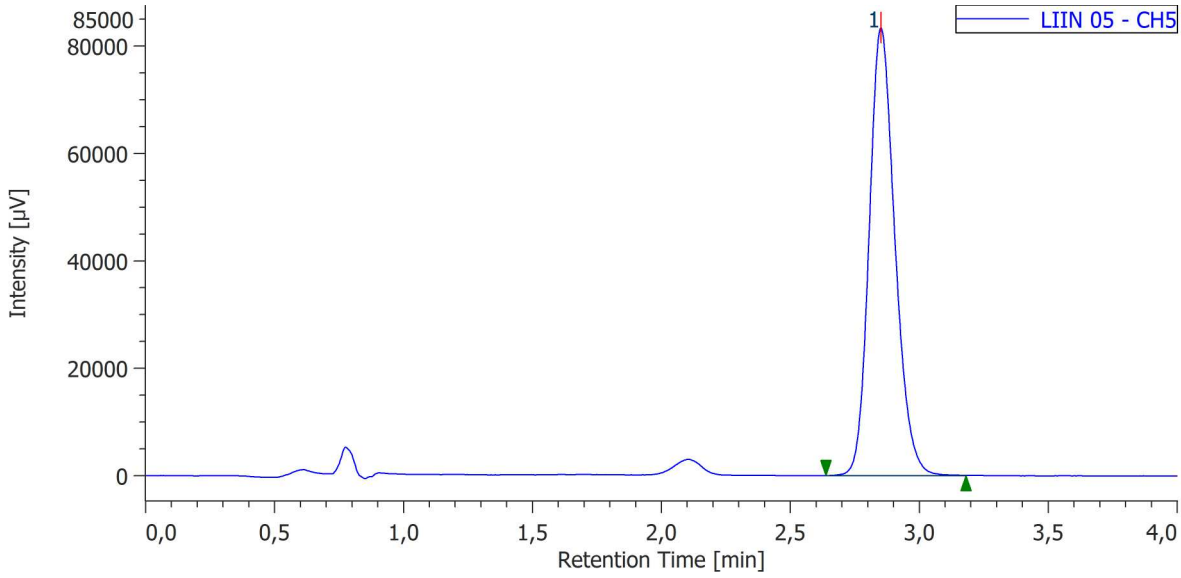

Chromatogram Information	
User Name	QPackSA
Date Modified	13/11/2025 17:57:03
Description	
HPLC System Name	HPLC 03
Injection Date	13/11/2025 17:53:01
Volume	20.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	4.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2.850	577976	83314	100.000	100.000	N/A	4031	N/A	1.185	

Creator
Reviewer
Approver

Chromatogram

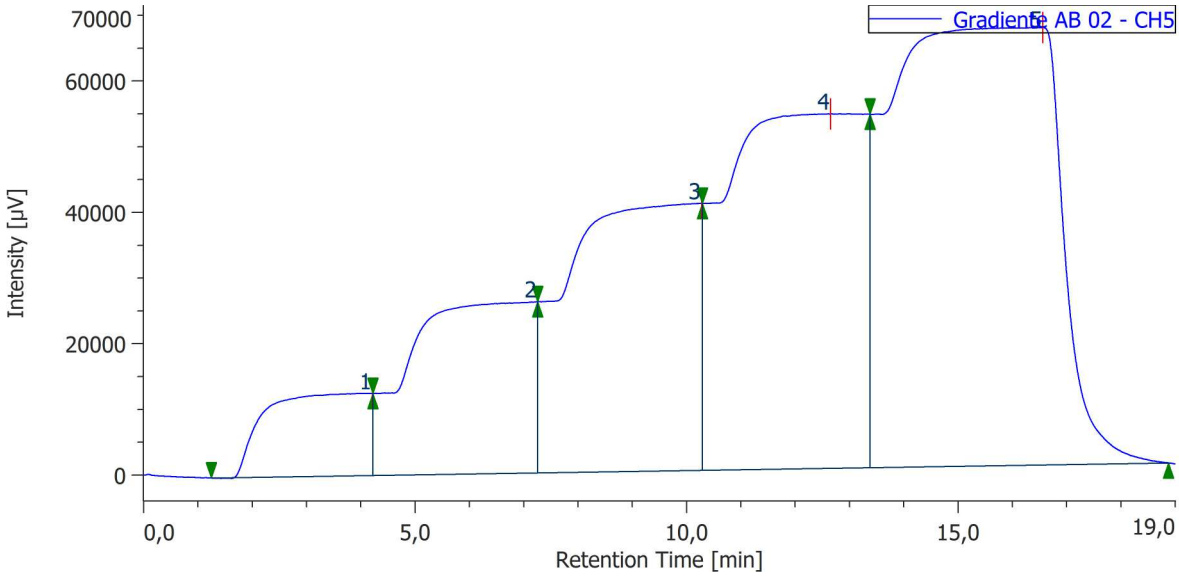

Chromatogram Information	
User Name	QPackSA
Date Modified	12/11/2025 17:56:46
Description	
HPLC System Name	HPLC 03
Injection Date	12/11/2025 17:37:45
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,213	1625192	12498	4,525	6,260	N/A	N/A	N/A	N/A	
2	40%	5	7,253	4063986	26045	11,314	13,046	N/A	N/A	N/A	N/A	
3	60%	5	10,277	6663792	40628	18,552	20,351	N/A	N/A	N/A	N/A	
4	80%	5	12,647	9402312	53931	26,177	27,014	N/A	N/A	N/A	N/A	
5	100%	5	16,557	14163494	66536	39,432	33,328	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

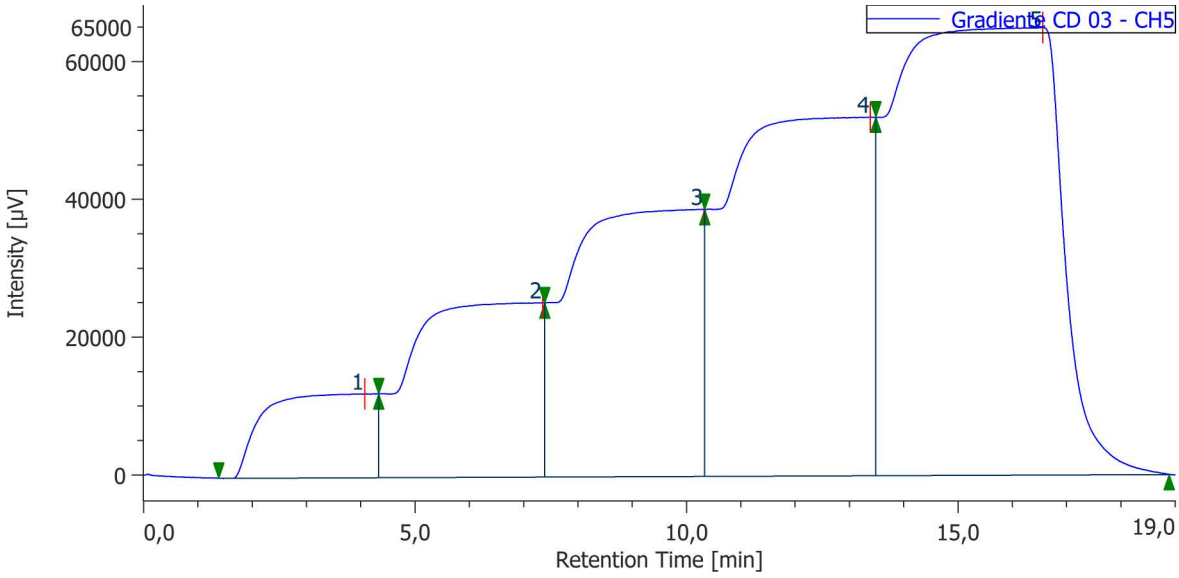

Chromatogram Information

User Name	QPackSA
Date Modified	12/11/2025 19:13:33
Description	
HPLC System Name	HPLC 03
Injection Date	12/11/2025 18:54:33
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,070	1651952	12154	4,761	6,297	N/A	N/A	N/A	N/A	
2	40%	5	7,347	4062369	25270	11,708	13,091	N/A	N/A	N/A	N/A	
3	60%	5	10,317	6281470	38725	18,103	20,062	N/A	N/A	N/A	N/A	
4	80%	5	13,383	9262140	51998	26,693	26,938	N/A	N/A	N/A	N/A	
5	100%	5	16,557	13440716	64881	38,736	33,612	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver