
Peak Find - EDUV_001 UV_tR0,22 D.jws

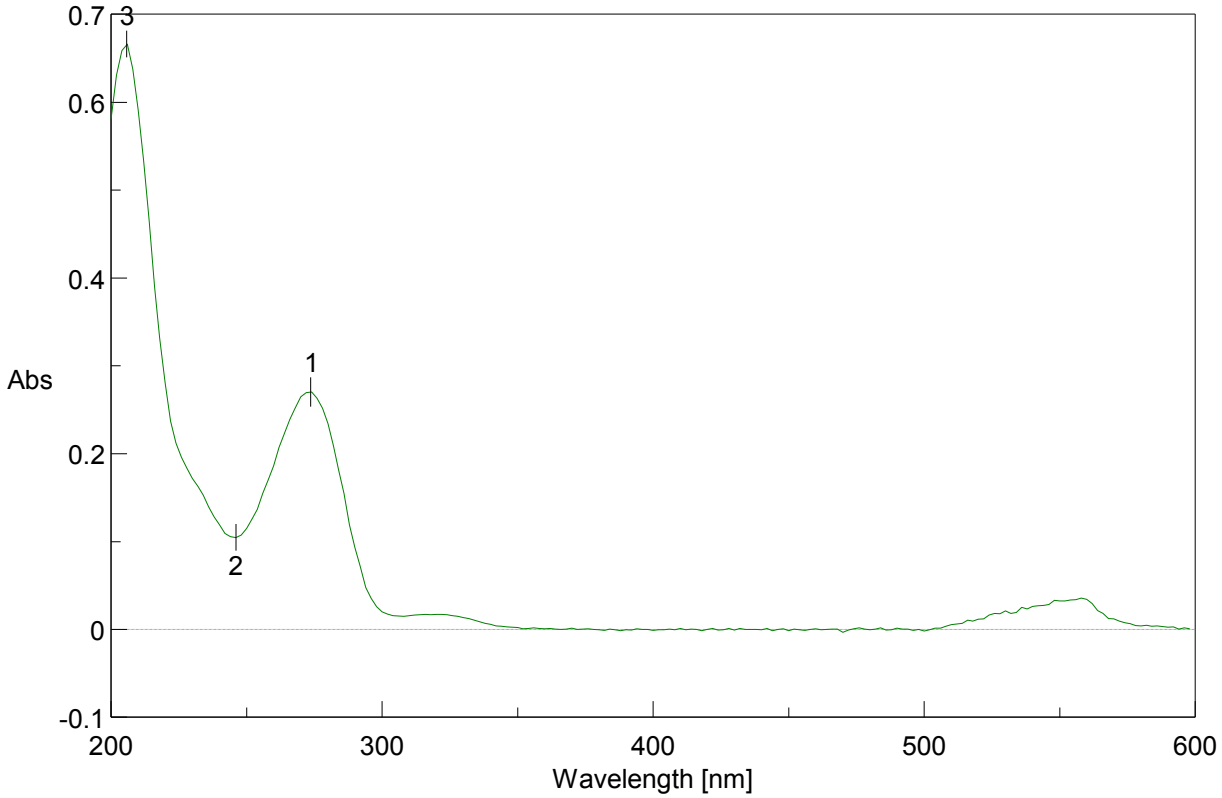

[Comments]

User	Administrator
Division	---
Company	Myralis
Creation date	25/01/2017 08:41

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200

[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45


[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.269825	2	246	0.104386
3	206	0.665739			

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 16:07:42
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 15:34:10
Volume	0,10 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	33,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente ACD
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

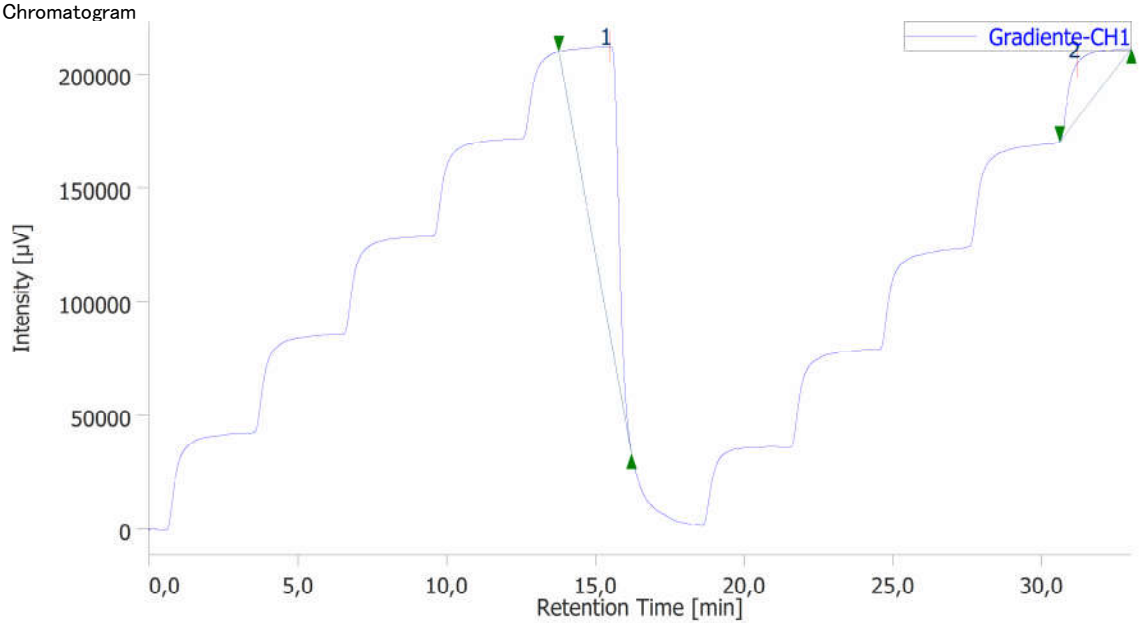


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Unknown	15,477	9130314	125511
2	Unknown	31,198	2048676	24587

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:19:02
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:47:13
Volume	10,00 [µL]
Sample #	3
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

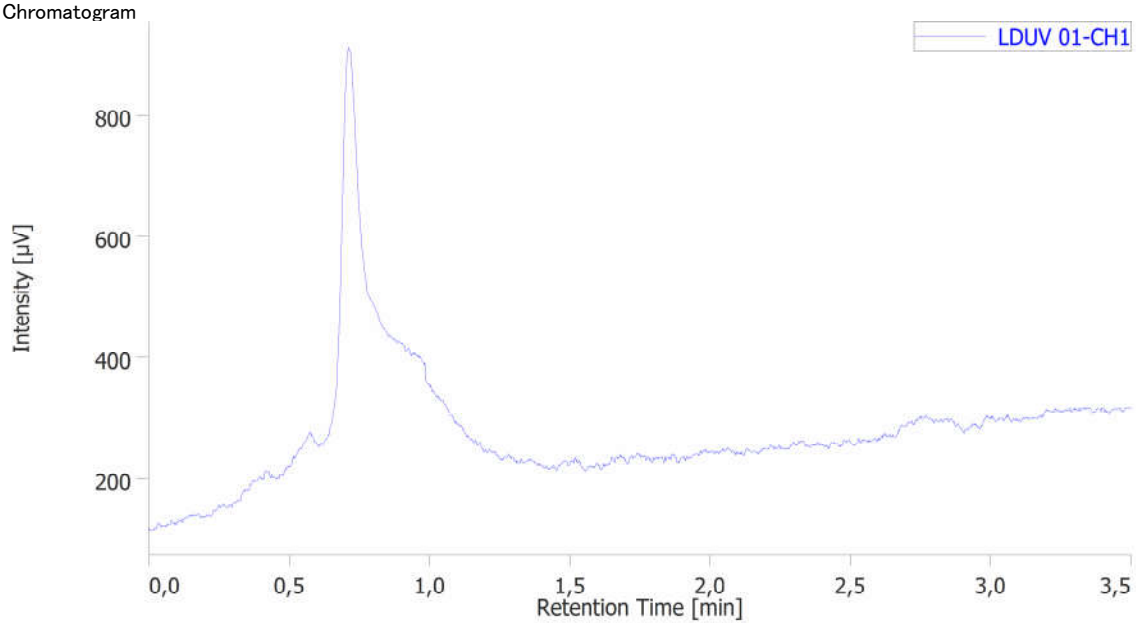


Peak Information – No data.

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:19:21
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:51:05
Volume	10,00 [µL]
Sample #	4
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

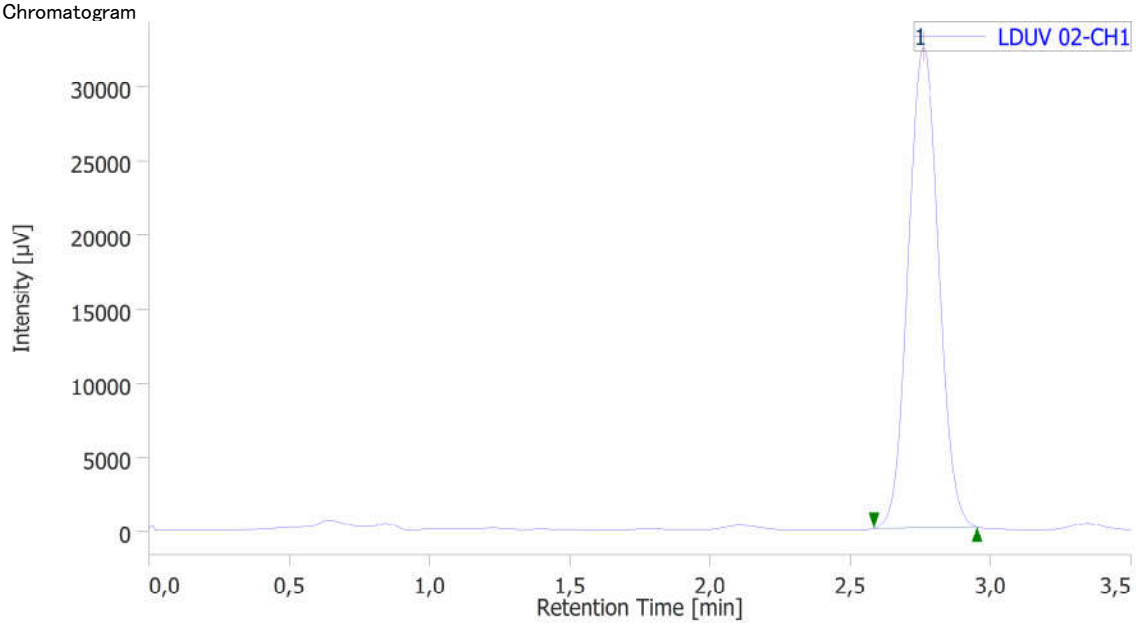


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,760	244346	32447

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:19:33
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:54:58
Volume	10,00 [µL]
Sample #	5
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

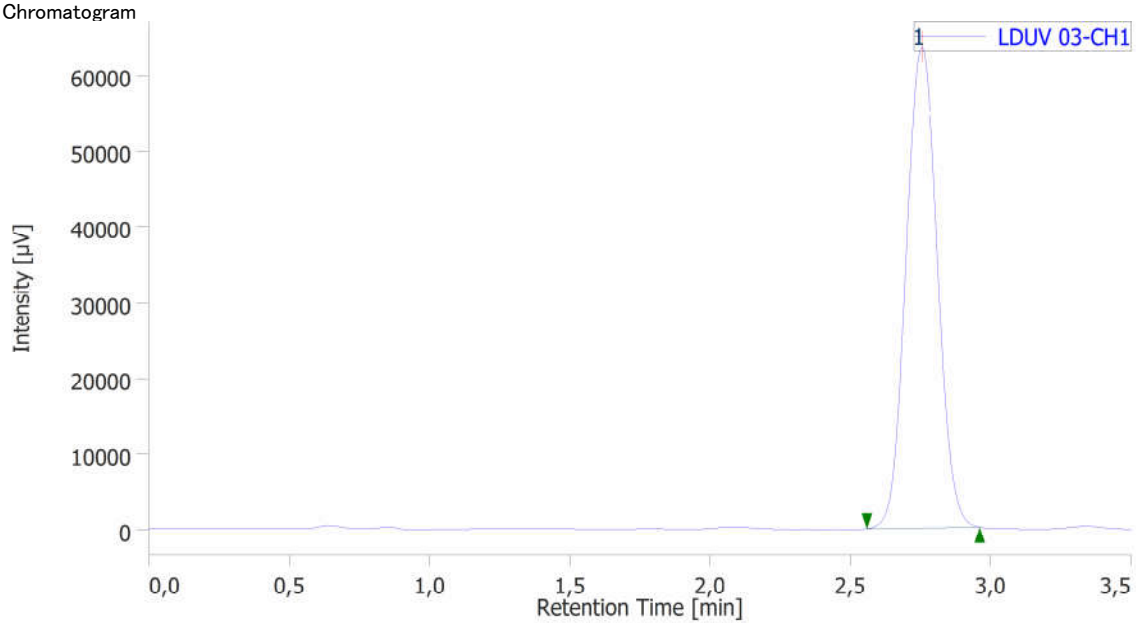


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,753	492938	63559

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:19:52
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:58:50
Volume	10,00 [µL]
Sample #	6
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

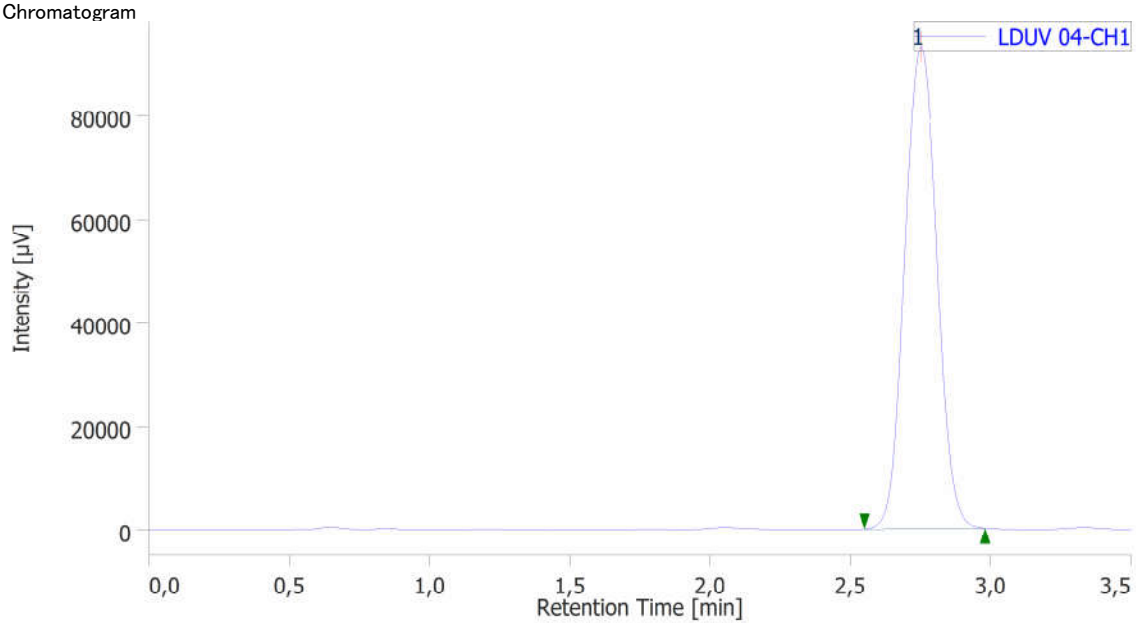


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,752	744169	93182

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:20:04
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:02:45
Volume	10,00 [µL]
Sample #	7
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

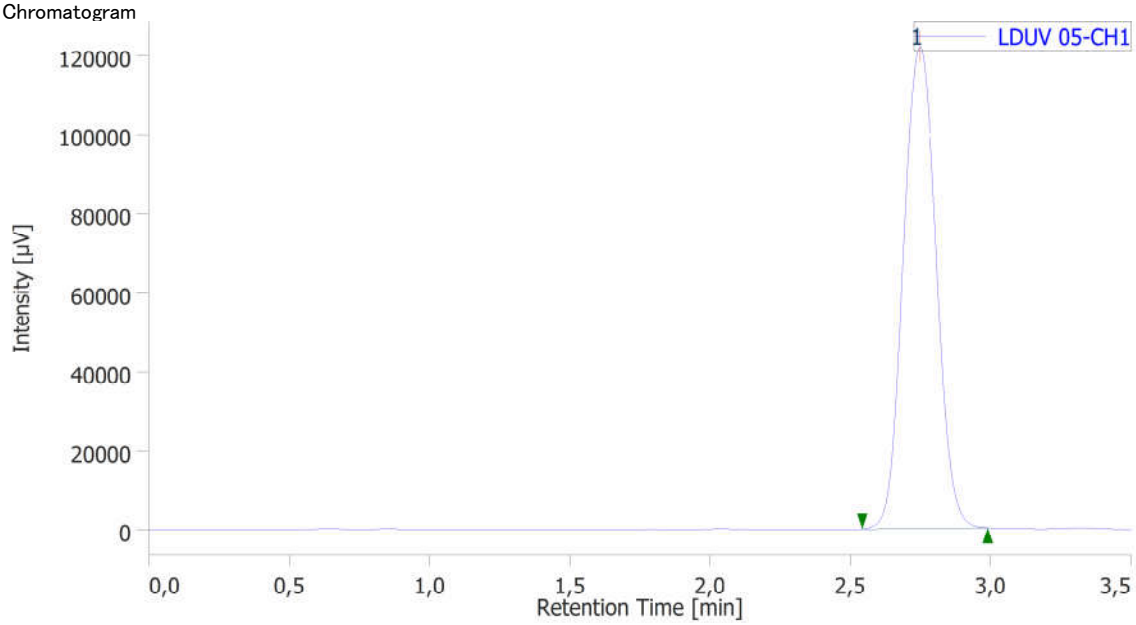


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,747	991548	121821

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 13:31:49
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:34:39
Volume	0,10 [µL]
Sample #	8
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

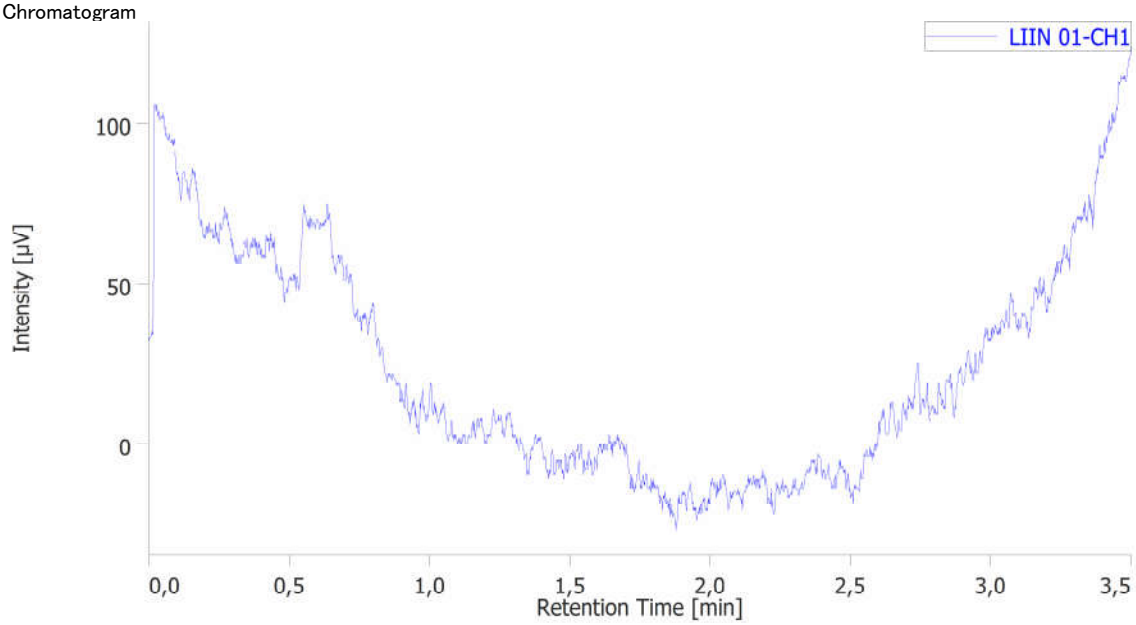


Peak Information – No data.

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 13:32:07
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:38:31
Volume	5,00 [µL]
Sample #	8
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

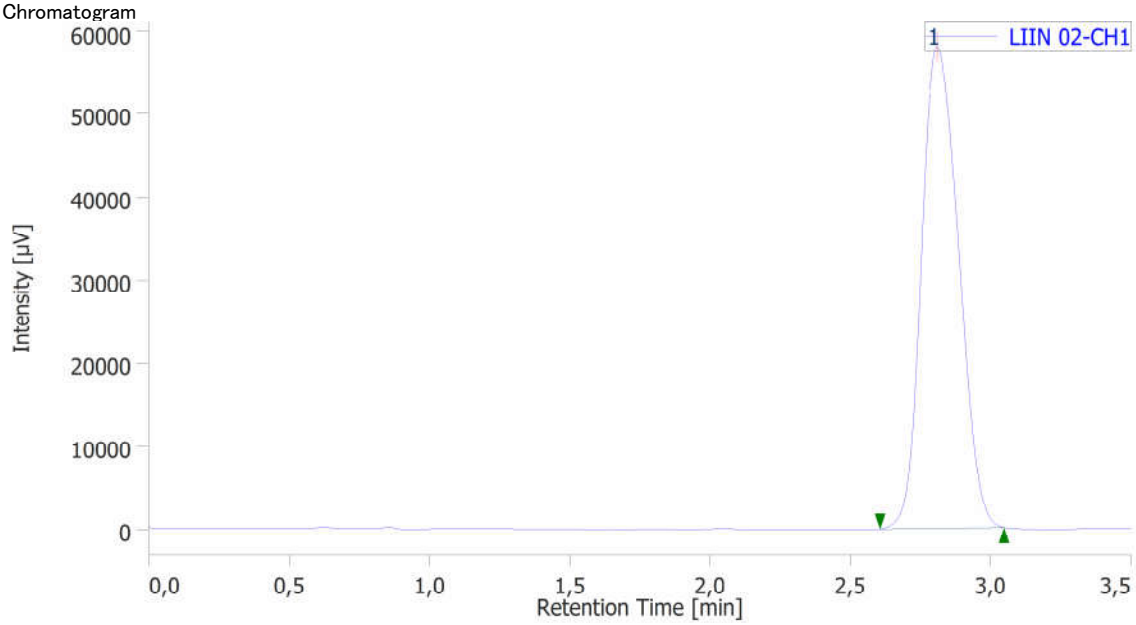


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,808	532885	58000

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 13:32:19
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:42:26
Volume	10,00 [µL]
Sample #	8
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

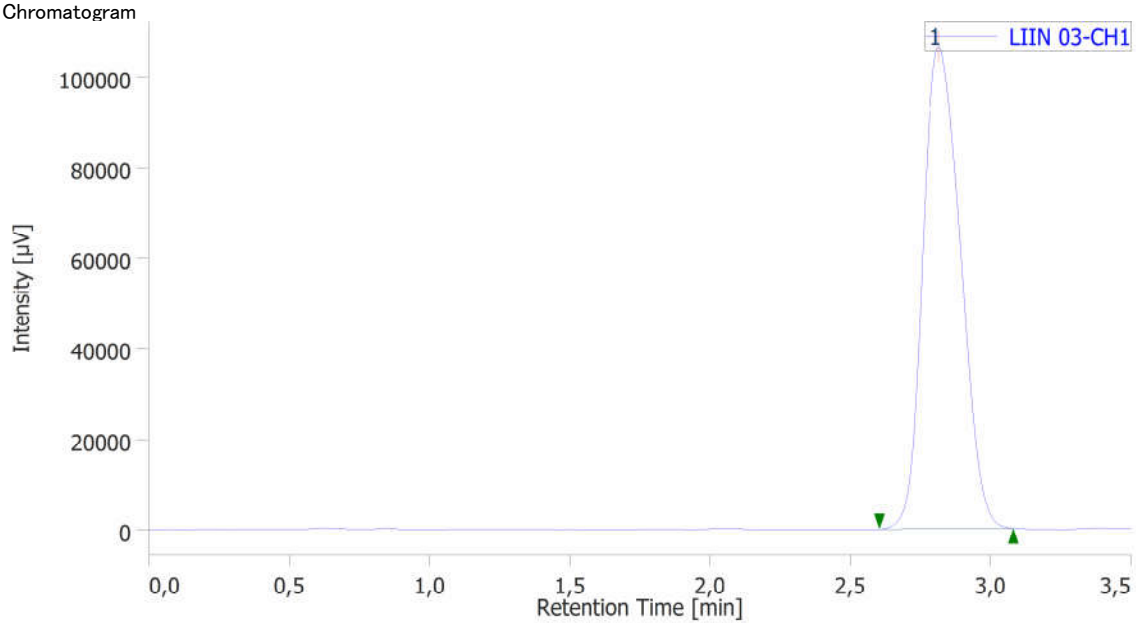


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,813	990603	106492

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 13:32:30
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:46:24
Volume	15,00 [µL]
Sample #	8
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

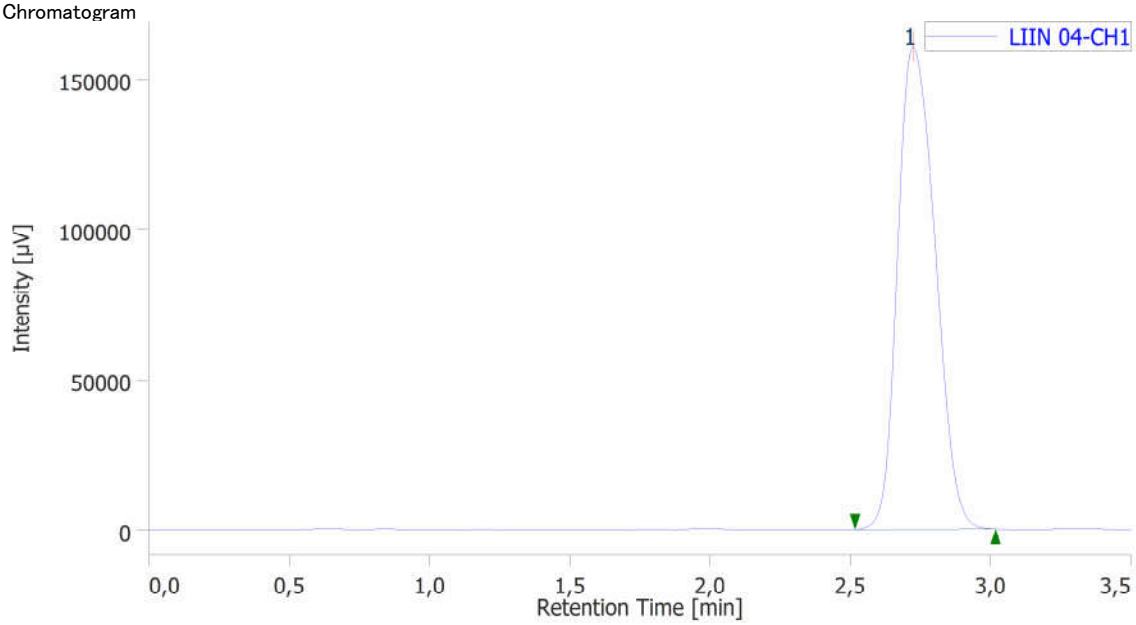


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,723	1495049	160476

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 13:32:42
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 10:50:24
Volume	20,00 [µL]
Sample #	8
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

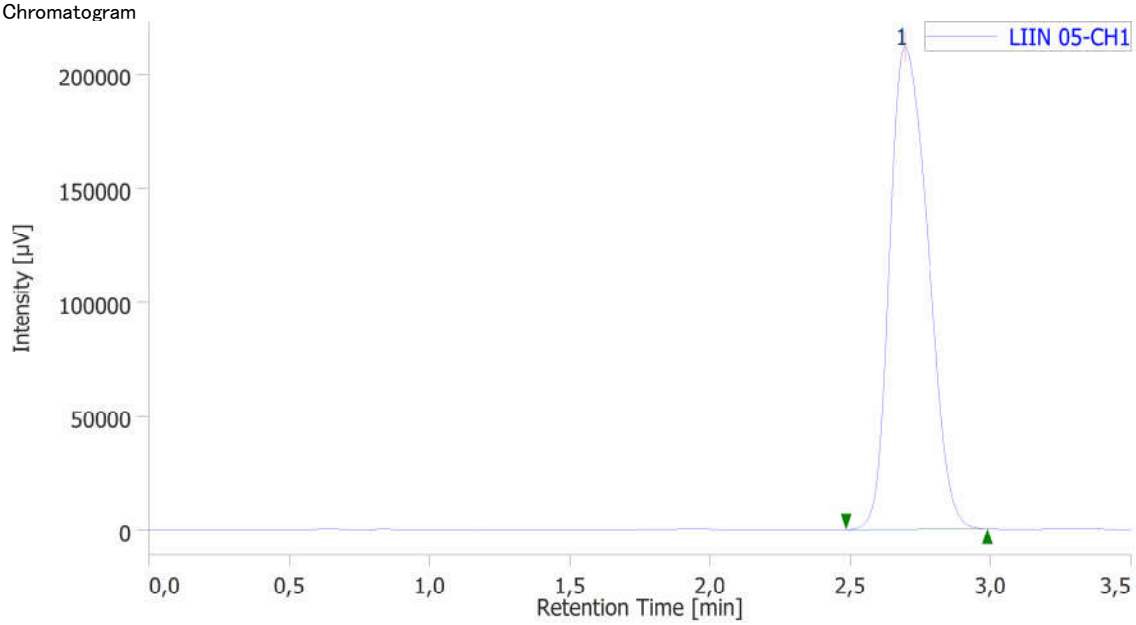


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,693	2008426	211713

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:17:17
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:10:24
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

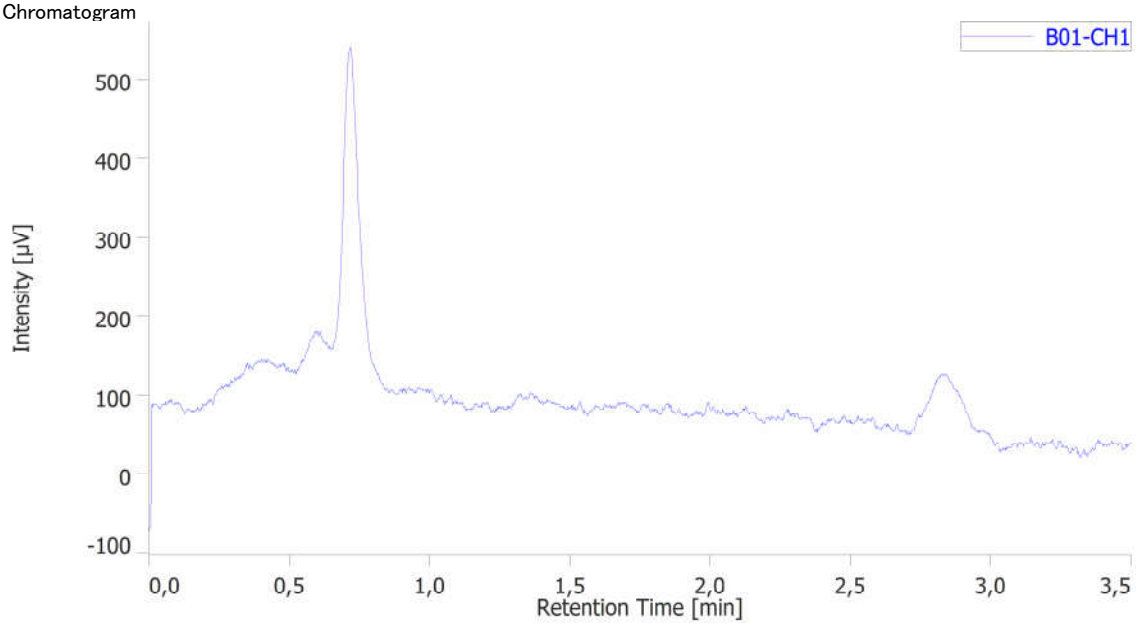


Peak Information – No data.

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:17:28
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:14:15
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

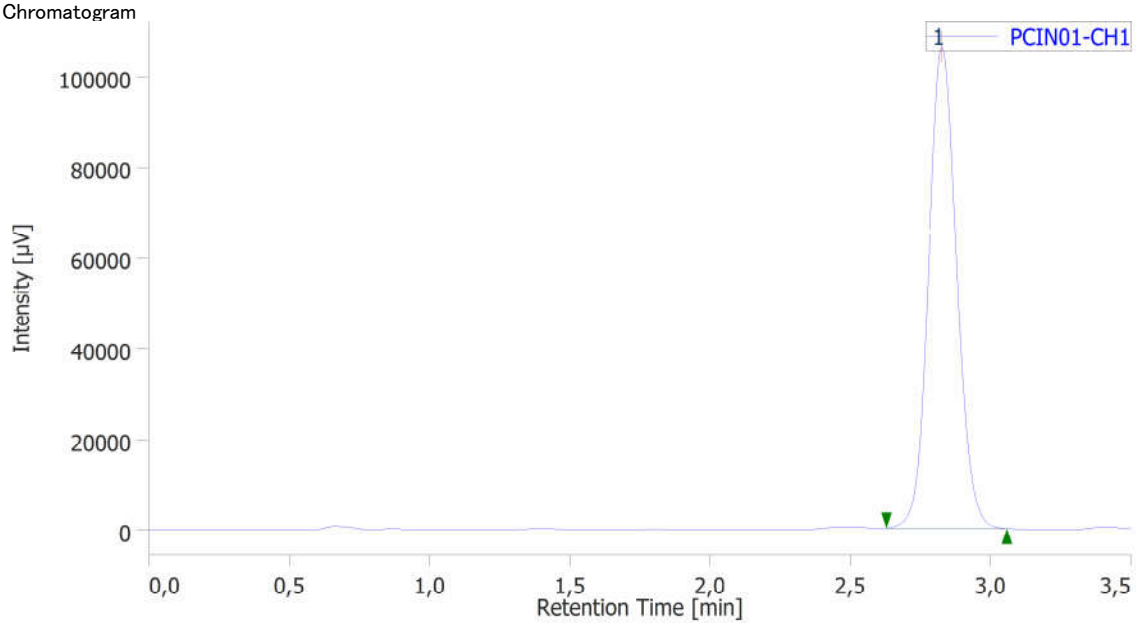


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,825	738467	106180

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:17:40
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:18:05
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

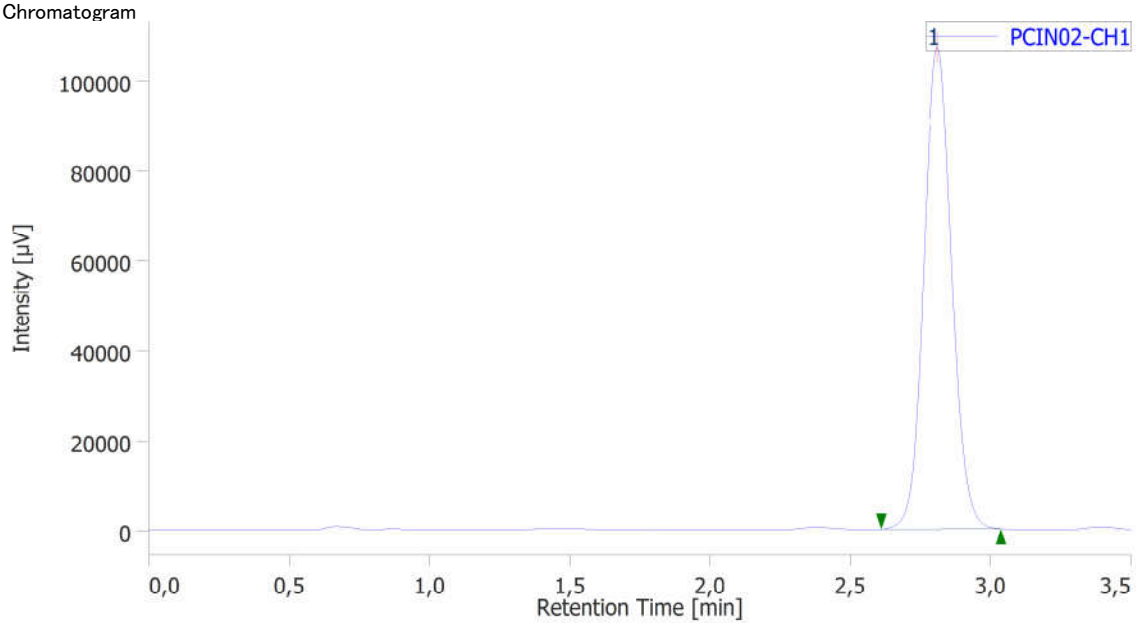


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,808	737291	107235

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:17:52
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:21:55
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

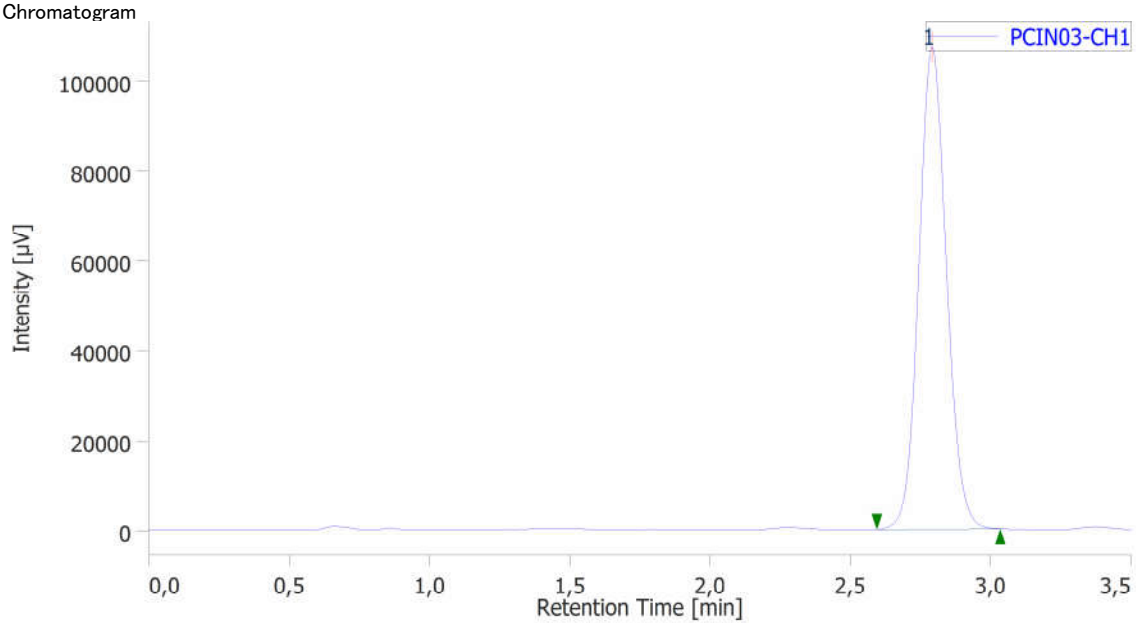


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,790	737382	107377

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:18:04
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:25:45
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

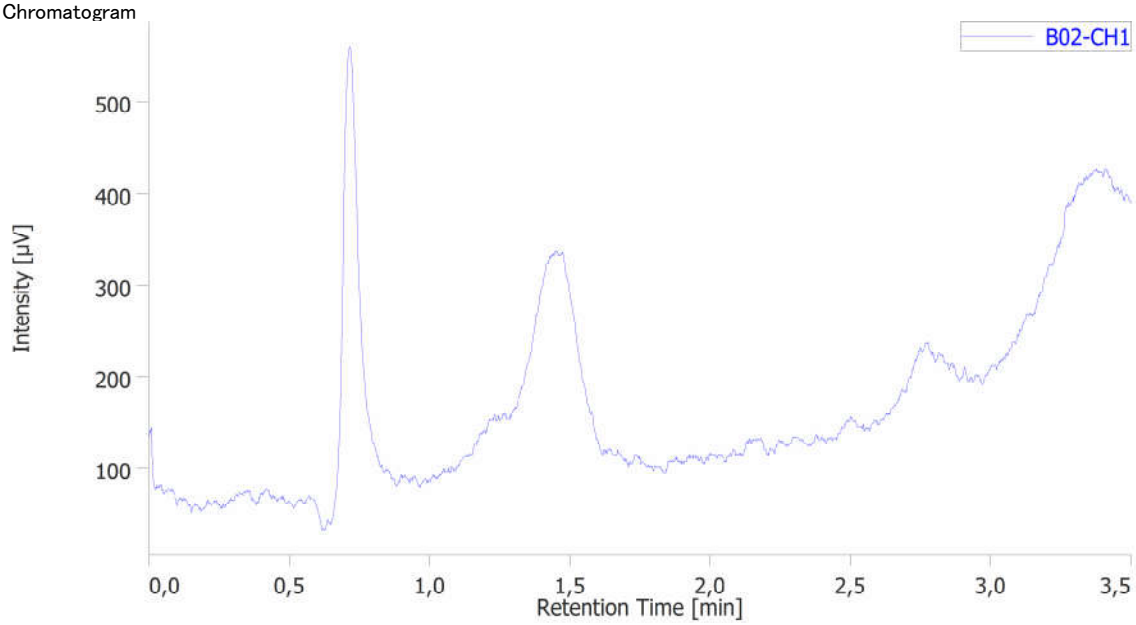


Peak Information – No data.

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:18:13
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:29:35
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

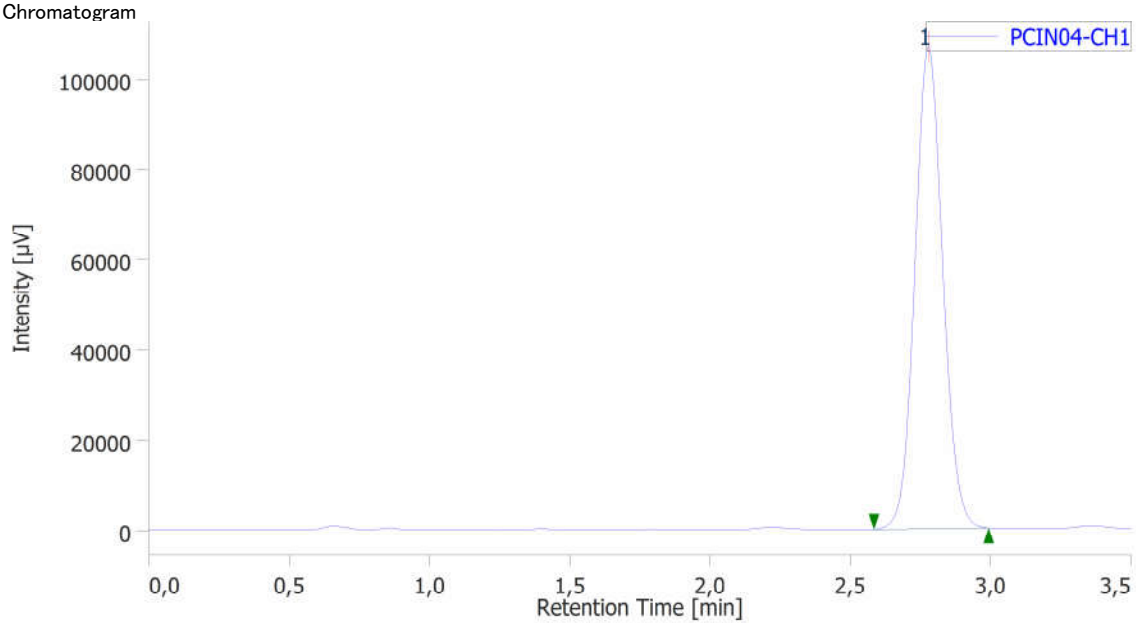


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,777	738897	106804

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:18:25
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:33:25
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

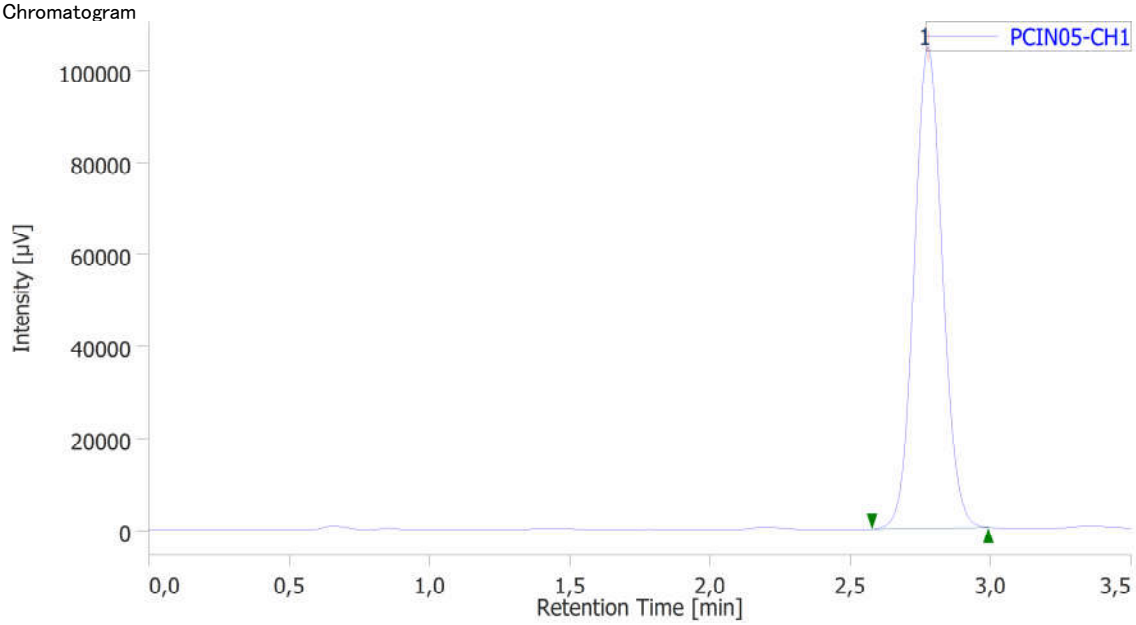


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,775	736463	104807

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:18:40
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:37:15
Volume	10,00 [µL]
Sample #	2
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

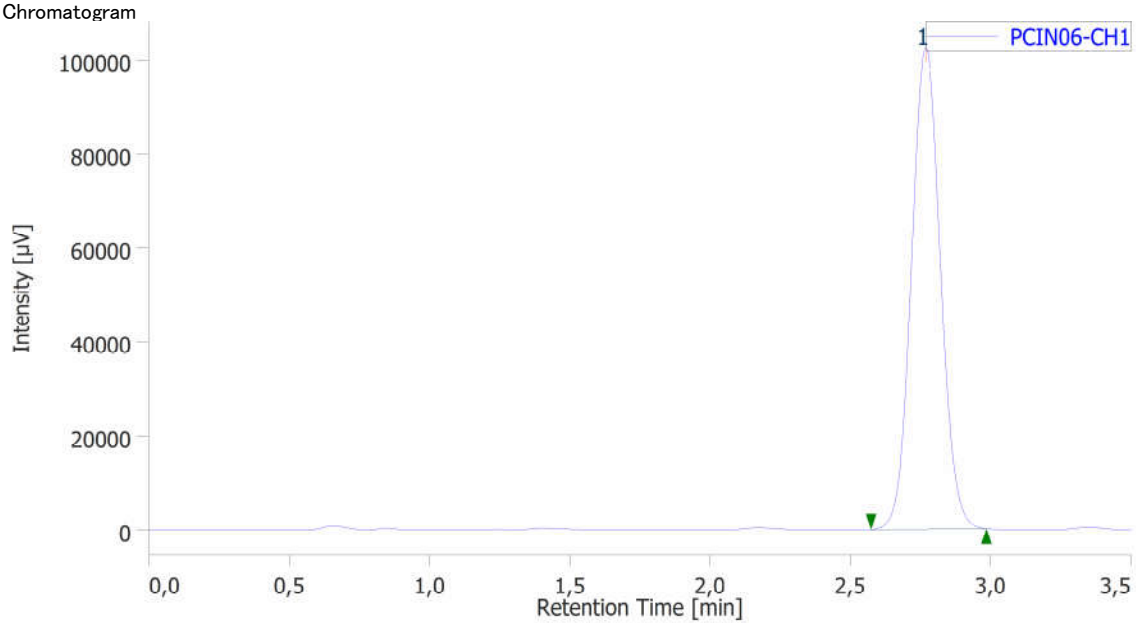


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeina	2,768	737528	102620

Qualificação CQ 475 – 2017

Chromatogram Information	
User Name	Administrator
Date Modified	25/01/2017 10:18:53
Description	
HPLC System Name	CQ-475
Injection Date	25/01/2017 09:41:03
Volume	10,00 [µL]
Sample #	1
Project Name	Jasco
Acquisition Time	3,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2017
Peak ID Table	Id Cafeina
Calibration Method	
Additional Information	
Column Info	

Chromatogram

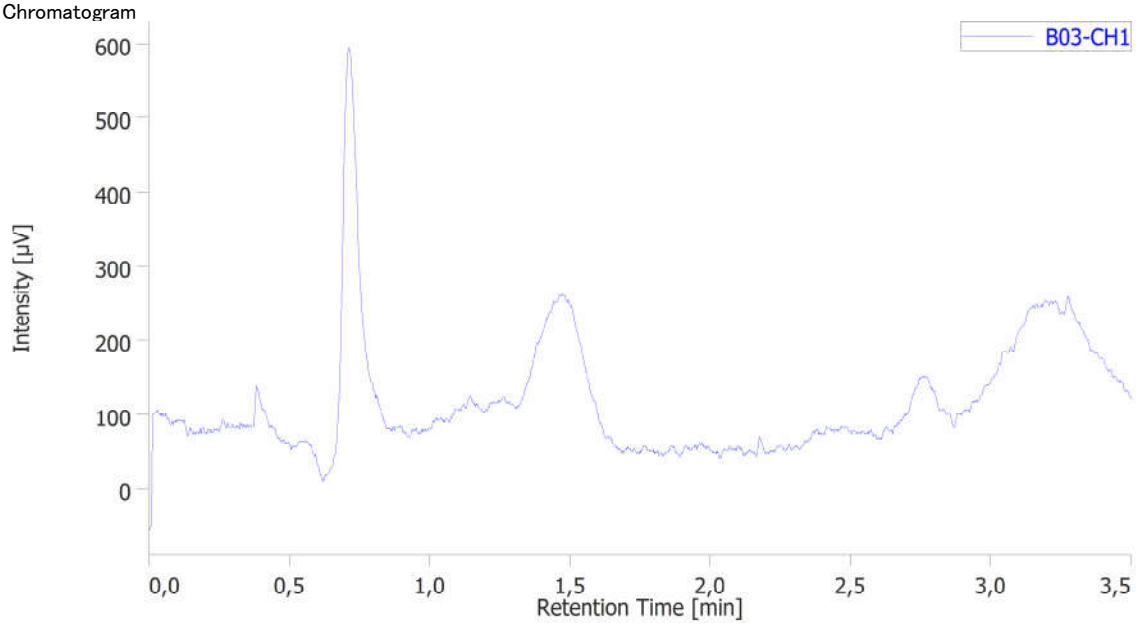

Peak Information – No data.