Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:

Sample ID: 01 - Exatidão do número de onda

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificação 2024\ 01 - Exatidãoa2r.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:

Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 11:44:40 AM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:

Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack

Report Generation Date: 11/21/2024 11:46:40 AM

Report Generation GMT Date:11/21/2024 2:46:40 PM

Sample ID:01 - Exatidão do número de onda

Sample Scans:16

Background Scans:16

Resolution:2

System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m


User:LCQ\LCQ\QPack

Date/Time:11/21/2024 11:44:40 AM

Range:3000 - 650

Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\01 - Exatidãoa2r.a2r

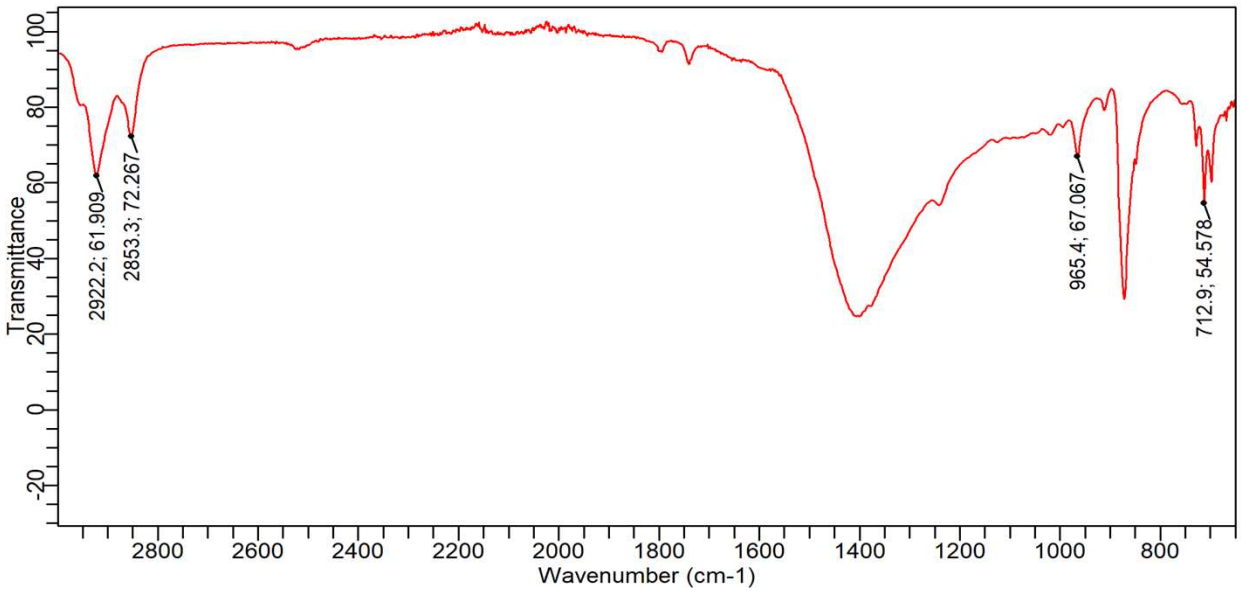

Peak Number	Wavenumber (cm^{-1})	Intensity
1	712.85336	54.57799
2	965.38050	67.06737
3	2853.27711	72.26703
4	2922.23286	61.90863

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:

Sample ID: 02 - Resolução

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificação 2024\ 02 - Resolução.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:

Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 11:51:16 AM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:

Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack

Report Generation Date: 11/21/2024 11:53:59 AM

Report Generation GMT Date:11/21/2024 2:53:59 PM

Sample ID:02 - Resolução

Sample Scans:16

Background Scans:16

Resolution:2

System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m


User:LCQ\LCQ\QPack

Date/Time:11/21/2024 11:51:16 AM

Range:3000 - 650

Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\02 - Resolução.a2r

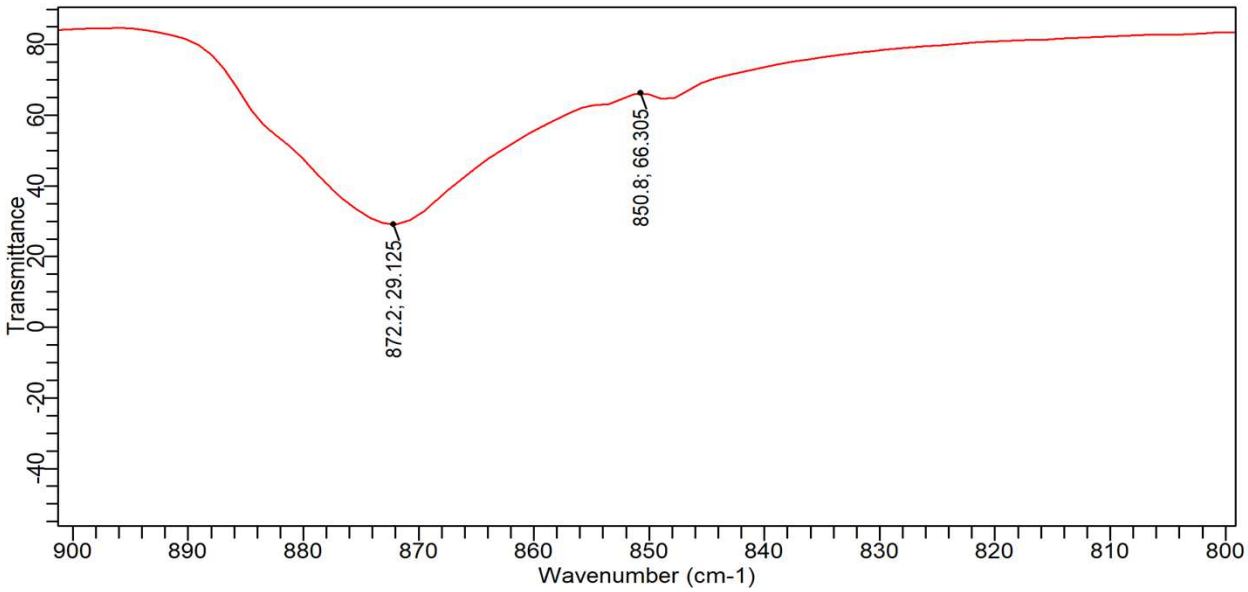

Peak Number	Wavenumber (cm^{-1})	Intensity
1	850.76486	66.30528
2	872.19705	29.12498

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:

Sample ID: 03a - Repetibilidade do número de onda

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\ 03a - Repetibilidade do número de onda.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:

Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 11:56:14 AM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:

Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack


Report Generation Date: 11/21/2024 11:58:32 AM
Report Generation GMT Date:11/21/2024 2:58:32 PM

Sample ID:03a - Repetibilidade do número de onda

Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m
User:LCQ\LCQ\QPack
Date/Time:11/21/2024 11:56:14 AM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\03a - Repetibilidade do número de onda.a2r

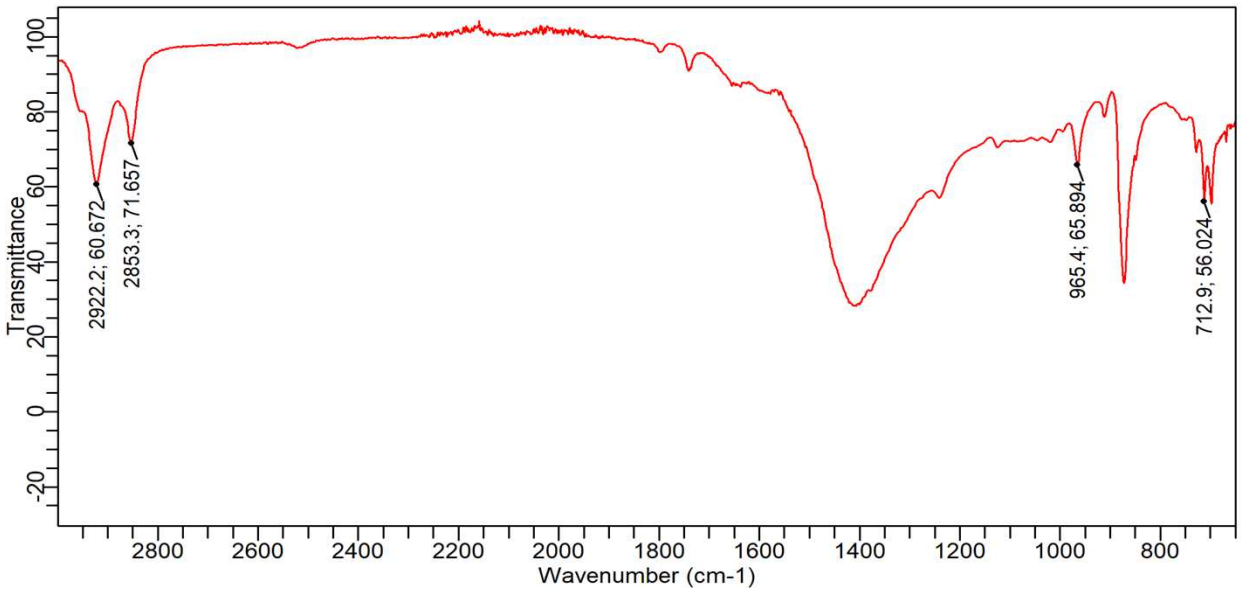

Peak Number	Wavenumber (cm^{-1})	Intensity
1	712.85336	56.02394
2	965.38050	65.89385
3	2853.27711	71.65708
4	2922.23286	60.67249

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:

Sample ID: 03b - Repetibilidade do número de onda

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\ 03b - Repetibilidade do número de ondaa2r.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:

Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 12:00:23 PM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:

Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack


Report Generation Date: 11/21/2024 12:03:10 PM
Report Generation GMT Date:11/21/2024 3:03:10 PM

Sample ID:03b - Repetibilidade do número de onda

Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m
User:LCQ\LCQ\QPack
Date/Time:11/21/2024 12:00:23 PM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\03b - Repetibilidade do número de ondaa2r.a2r

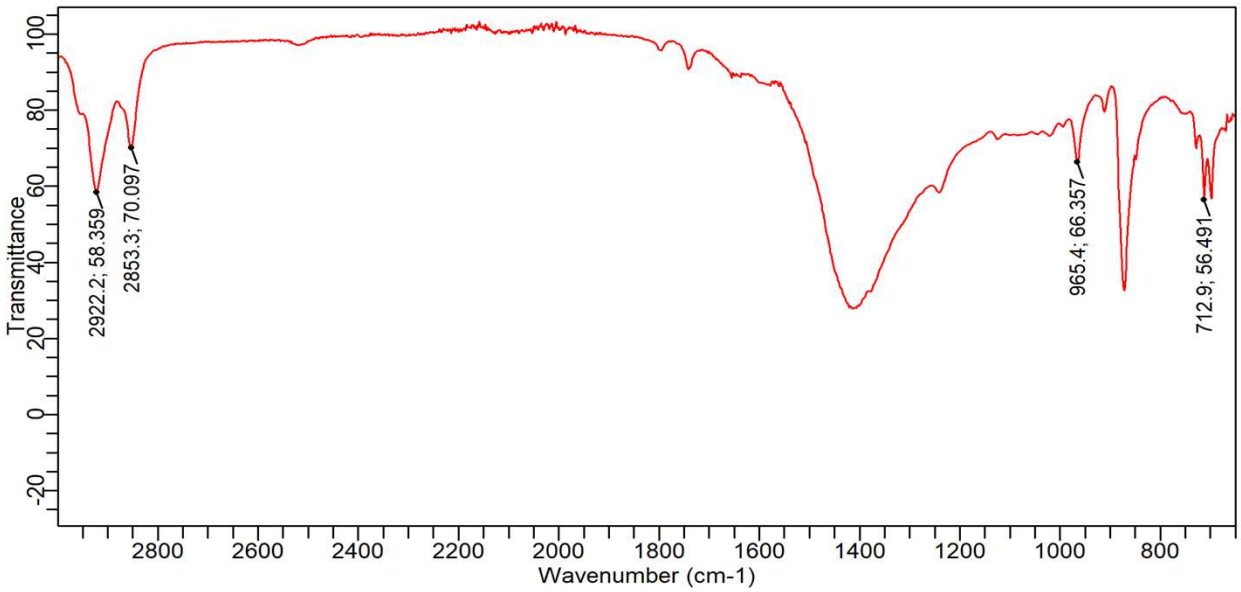

Peak Number	Wavenumber (cm^{-1})	Intensity
1	712.85336	56.49125
2	965.38050	66.35733
3	2853.27711	70.09728
4	2922.23286	58.35939

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:

Sample ID: 04a- Repetibilidade fotométrica

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificação 2024\Reject\ 04 - Repetibilidade fotométrica11.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:

Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 1:36:31 PM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:

Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack


Report Generation Date: 11/21/2024 1:37:28 PM
Report Generation GMT Date:11/21/2024 4:37:28 PM

Sample ID:04a- Repetibilidade fotométrica

Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m
User:LCQ\LCQ\QPack
Date/Time:11/21/2024 1:36:31 PM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\Reject\04 - Repetibilidade fotométrica11.a2r

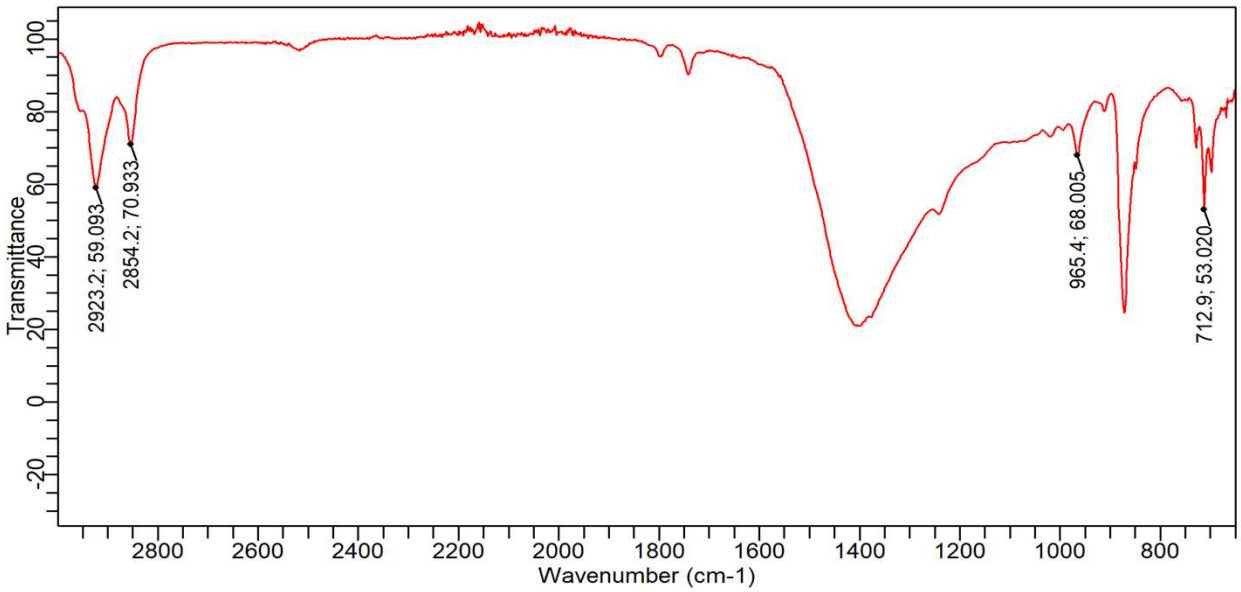

Peak Number	Wavenumber (cm^{-1})	Intensity
1	712.85336	53.02026
2	965.38050	68.00547
3	2854.20895	70.93331
4	2923.16470	59.09272

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 04b- Repetibilidade fotométrica

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_Public(000)|Public Results\ 04b- Repetibilidade fotométrica_2024-11-21T13-38-16.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:
Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 1:38:16 PM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:
Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack


Report Generation Date: 11/21/2024 1:38:54 PM
Report Generation GMT Date:11/21/2024 4:38:54 PM

Sample ID:04b- Repetibilidade fotométrica

Sample Scans:16
Background Scans:16
Resolution:2
System Status:Good

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m
User:LCQ\LCQ\QPack
Date/Time:11/21/2024 1:38:16 PM
Range:3000 - 650
Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_Public(000)|Public Results\04b-Repetibilidade fotométrica_2024-11-21T13-38-16.a2r

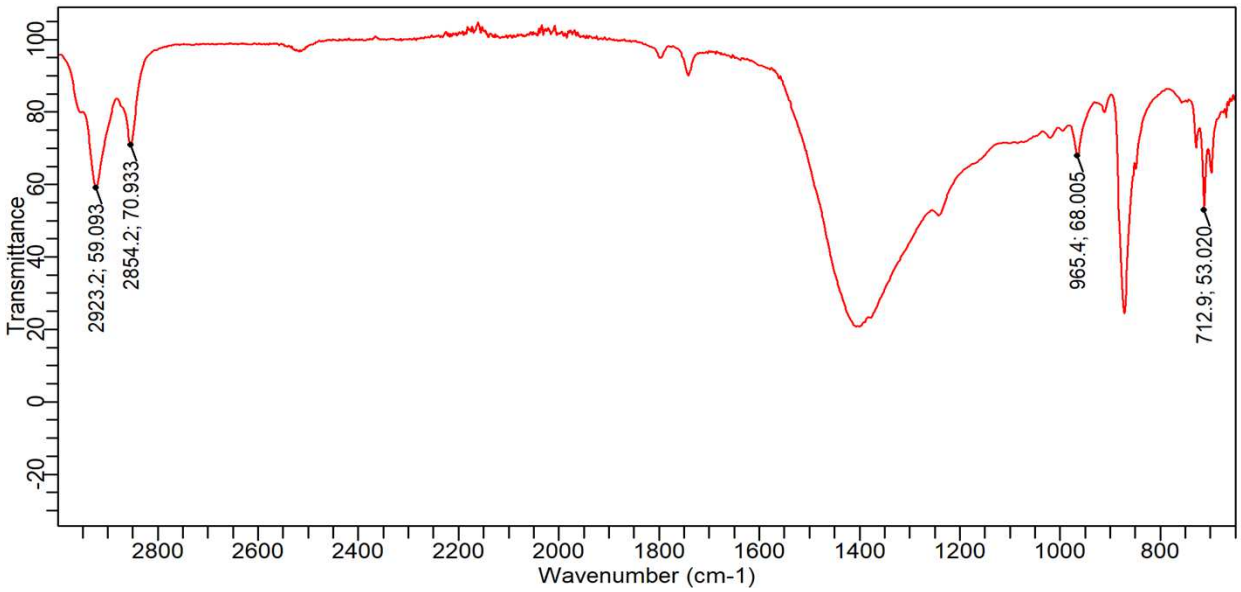

Peak Number	Wavenumber (cm^{-1})	Intensity
1	712.85336	53.02026
2	965.38050	68.00547
3	2854.20895	70.93331
4	2923.16470	59.09272

E-SIGNATURES

Signature

Agilent Technologies

This Report was generated under a 21 CFR 11 Environment

System Information:
Sample ID: 05 - Sensibilidade

System Status: Good

File Location: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificação 2024\ 05 - Sensibilidade.a2r

PC/Workstation ID: DESKTOP-ECT6L24

Software Version:MicroLab PC(21CFR11): 5.6.2135.0

FW Version:1.96.00.0

Data Information:
Method Name: DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

User: LCQ\LCQ\QPack

Date/Time: 11/21/2024 1:59:49 PM

Instrument Model: Cary630

Instrument S/N: MY2134CU14

Reporting Information:
Report Template: Spectrum.docx

Report Generated By: LCQ\LCQ\QPack

Report Generation Date: 11/21/2024 2:14:09 PM
Report Generation GMT Date:11/21/2024 5:14:09 PM

Sample ID:05 - Sensibilidade

Method Name:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|IQOQ_29112023\Qualificação QPack.a2m

Sample Scans:48

User:LCQ\LCQ\QPack

Background Scans:48

Date/Time:11/21/2024 1:59:49 PM


Resolution:4

Range:3000 - 650

System Status:Good

Apodization:Happ-Genzel

File Location:DESKTOP-ECT6L24\SQLEXPRESS|VAIMDB_FTIR23(000)|Qualificaão 2024\05 - Sensibilidade.a2r

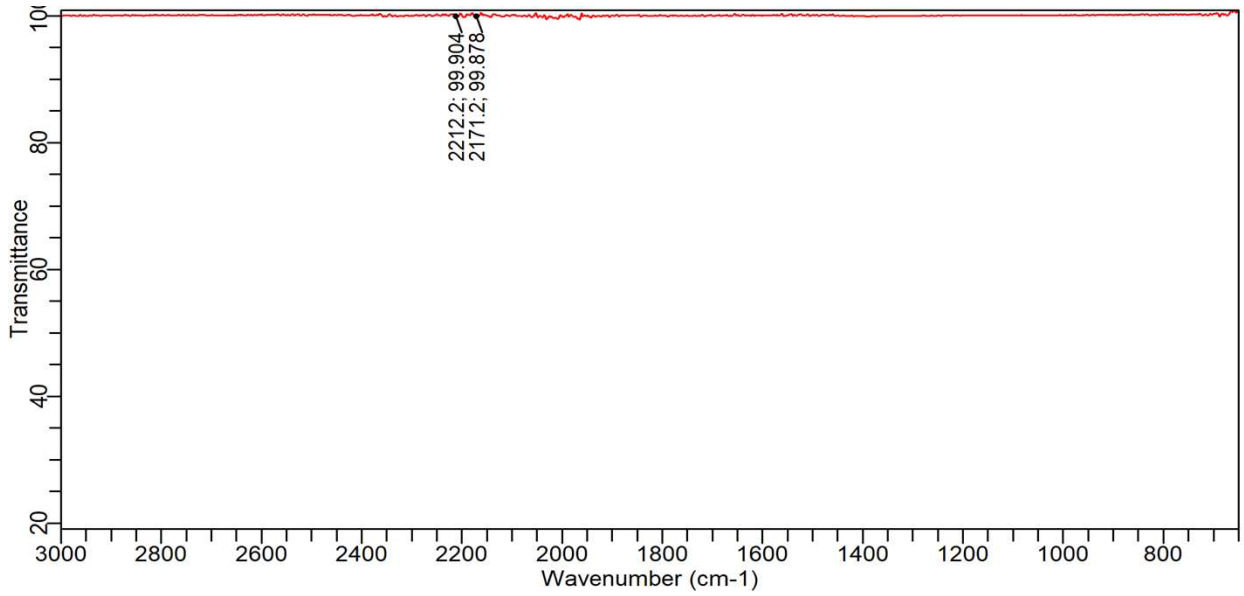

Peak Number	Wavenumber (cm^{-1})	Intensity
1	2171.17429	99.87818
2	2212.17501	99.90418

E-SIGNATURES

Signature

MicroLab

MicroLab

User: LCQ\LCQ\QPack


Status: Ready

Method: Qualificação QPack

21CFR11 Enabled

Current Sample

Sample

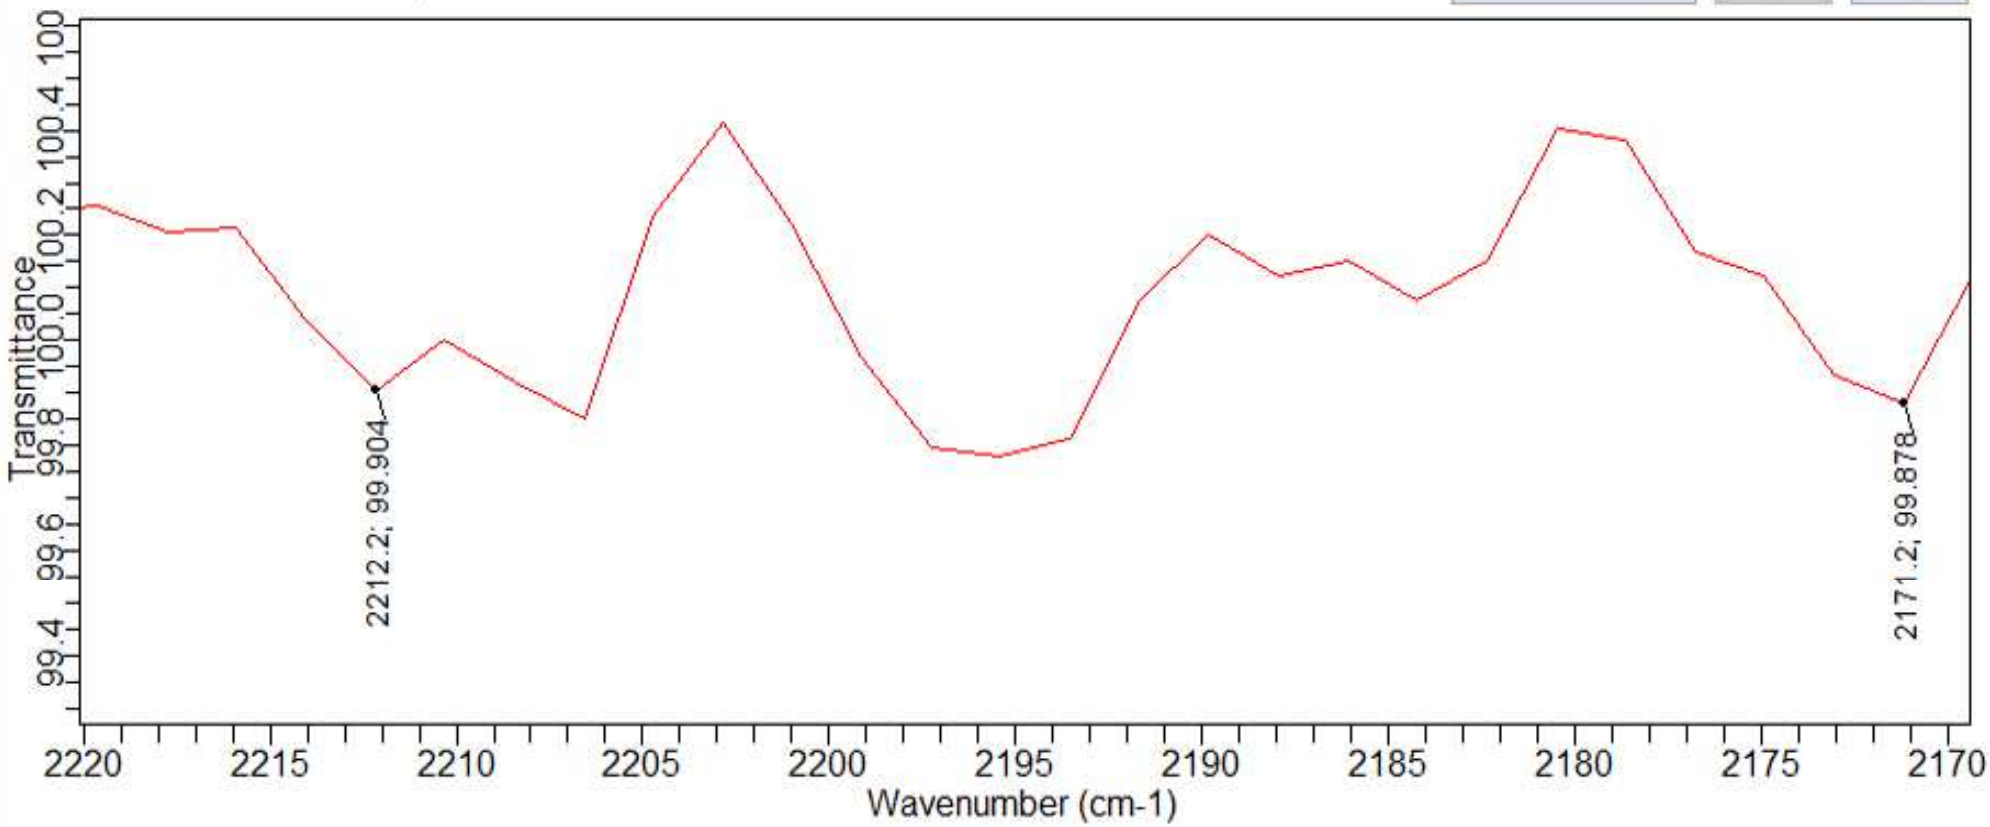

Home | Data Handling | E-Sign... | 21 CFR part 11 | Done