
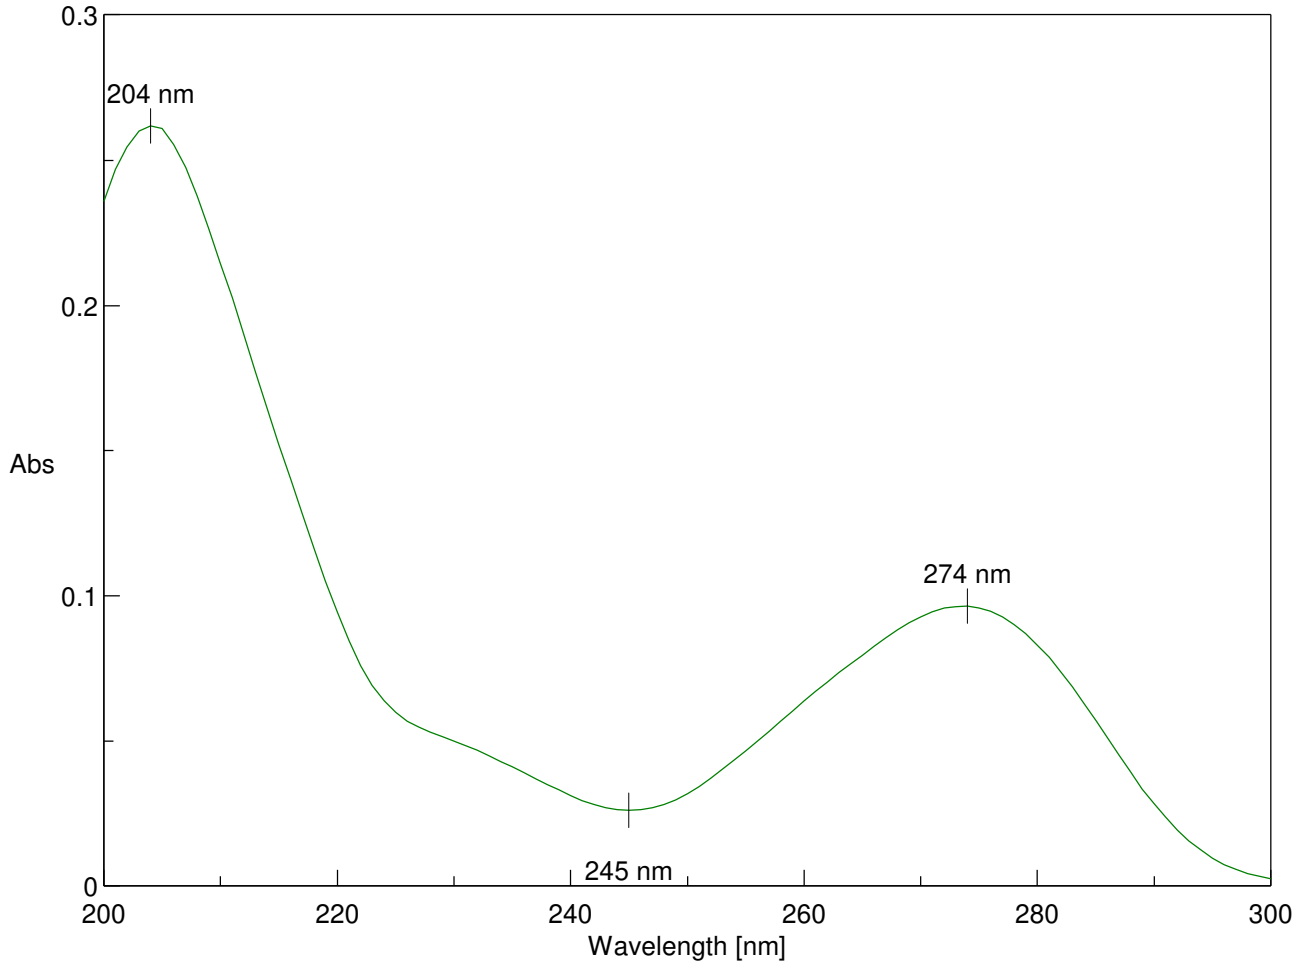


[Comments]	
User	QPackSA
Division	---
Company	Valer
Creation date	26/11/2024 10:35

[Measurement Information]	
Model Name	MD-2010
Serial No.	072260870
ROM version	V2.36

[Detailed Information]	
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101

Chromatogram

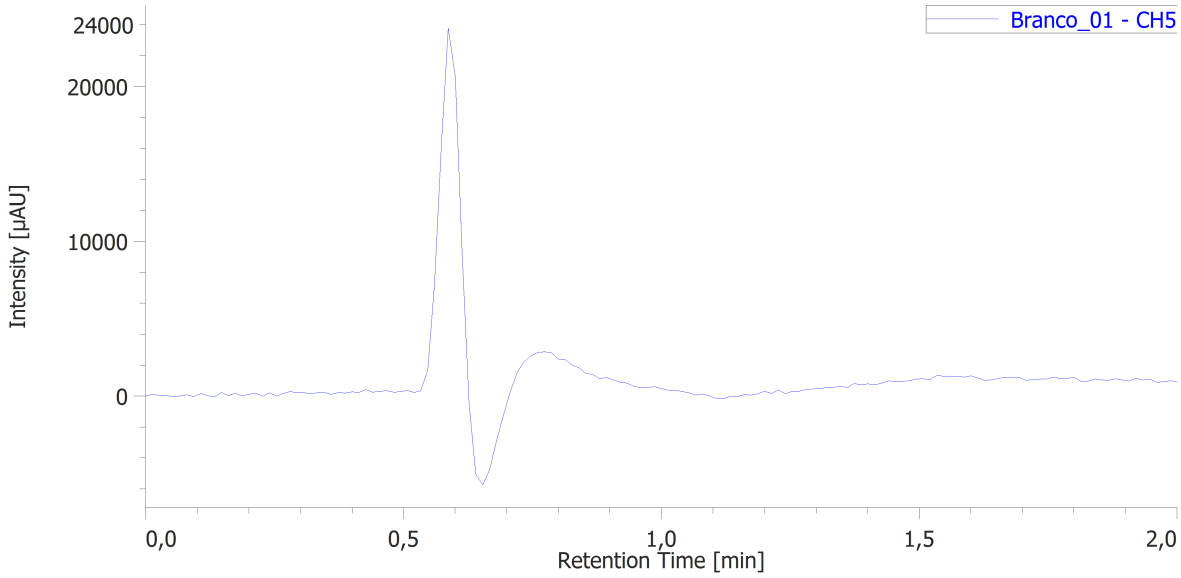


Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:21:59
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:19:57
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	Branco_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

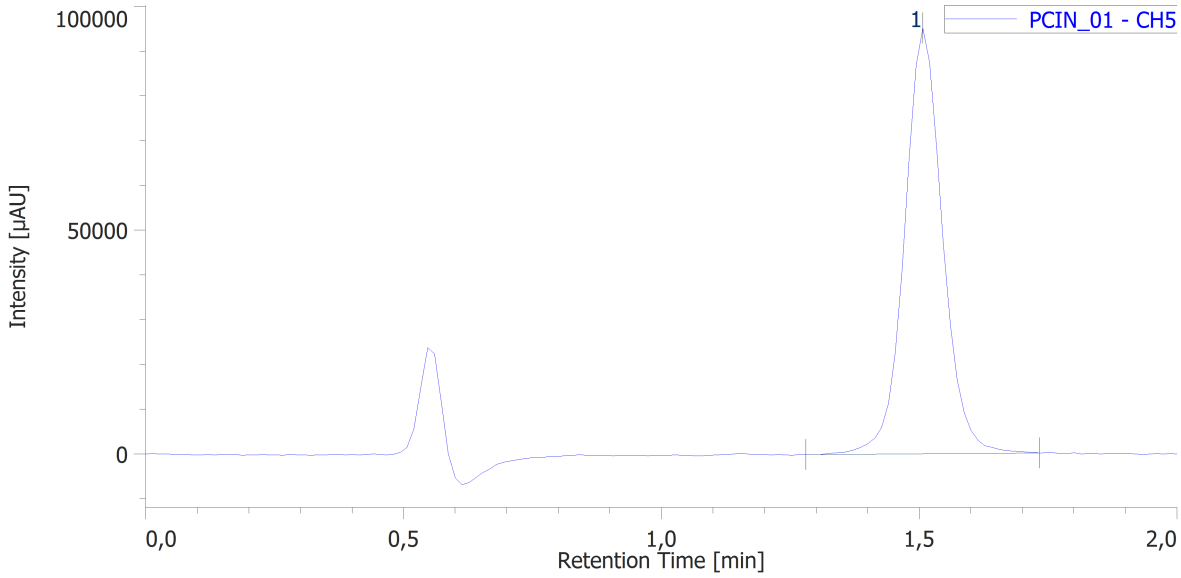

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:25:07
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:23:06
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	PCIN_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,507	488365	95101	100,000	100,000	N/A	2161	N/A	1,052	

Creator QPackSA
Reviewer
Approver

Chromatogram

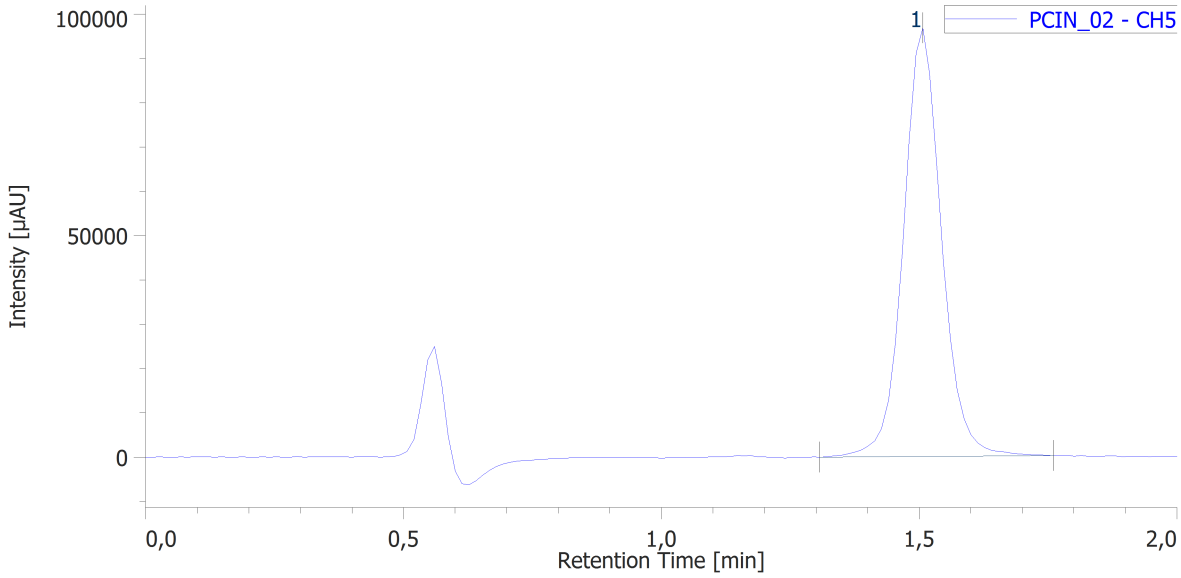

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:28:19
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:26:16
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	PCIN_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,507	496427	96711	100,000	100,000	N/A	2169	N/A	1,034	

Creator QPackSA
Reviewer
Approver

Chromatogram

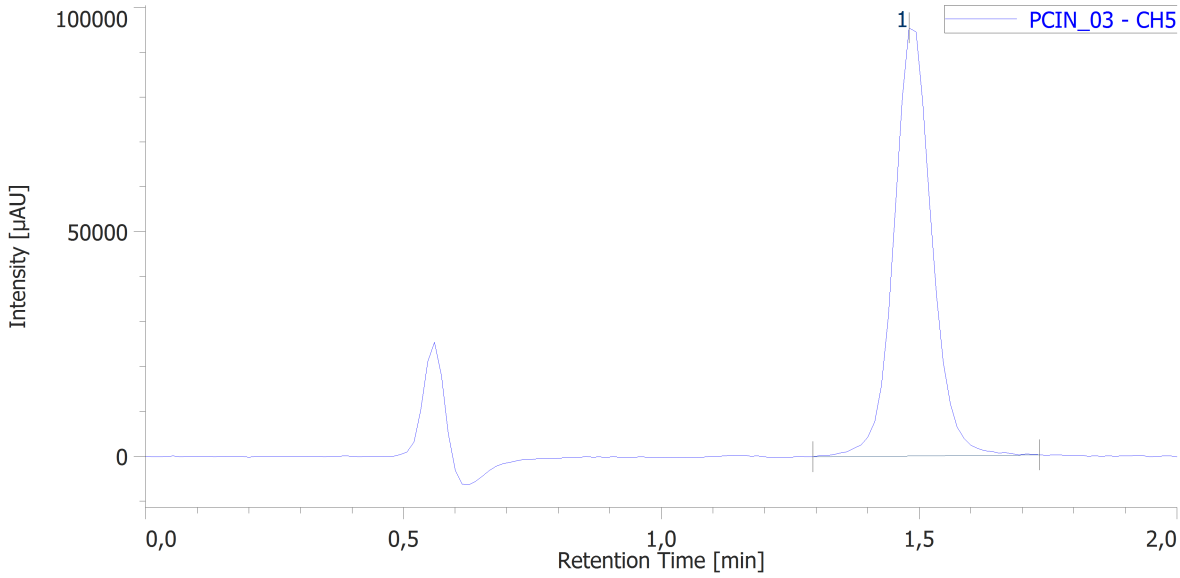

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:31:29
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:29:27
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH5
Sample Name	PCIN_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,480	488518	95321	100,000	100,000	N/A	2087	N/A	1,151	

Creator QPackSA
Reviewer
Approver

Chromatogram

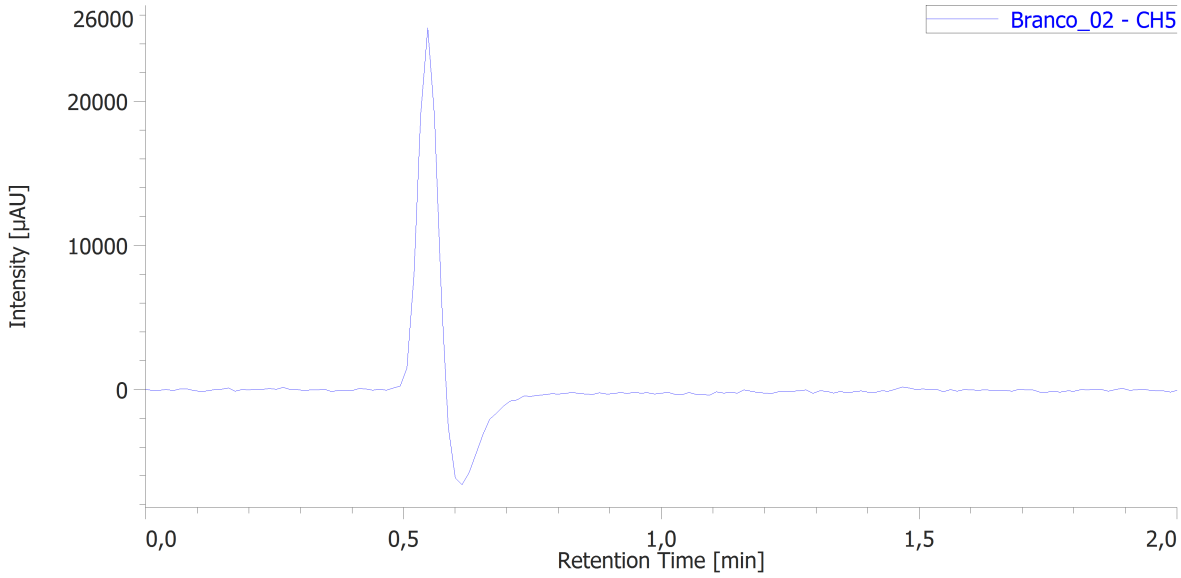


Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:34:37
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:32:36
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_02-CH5
Sample Name	Branco_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

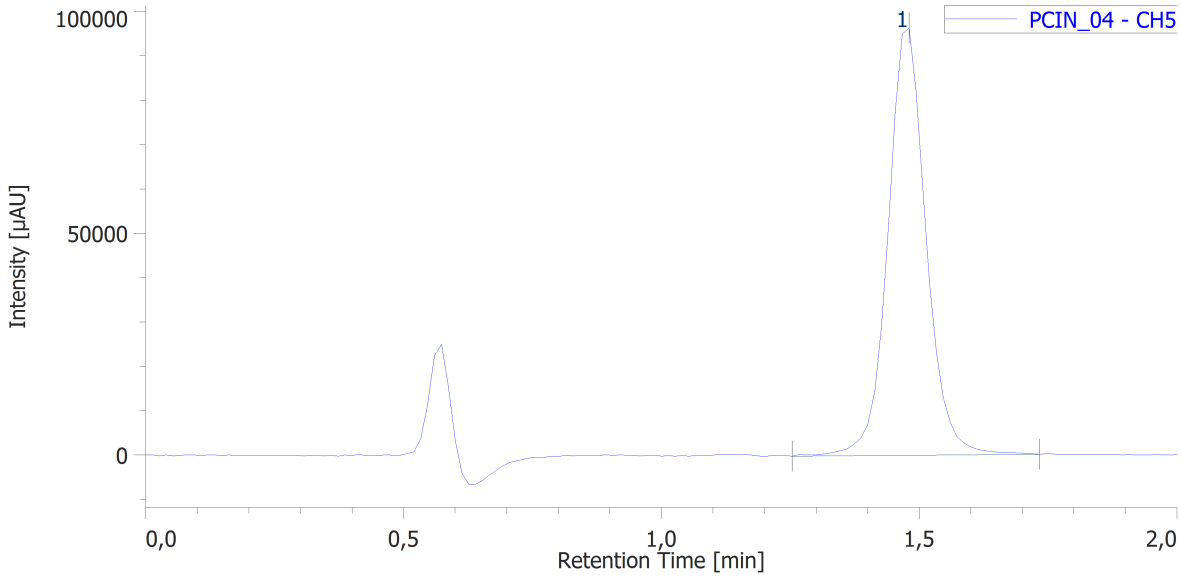

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:37:49
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:35:46
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	PCIN_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,480	495851	96255	100,000	100,000	N/A	2084	N/A	1,002	

Creator QPackSA
Reviewer
Approver

Chromatogram

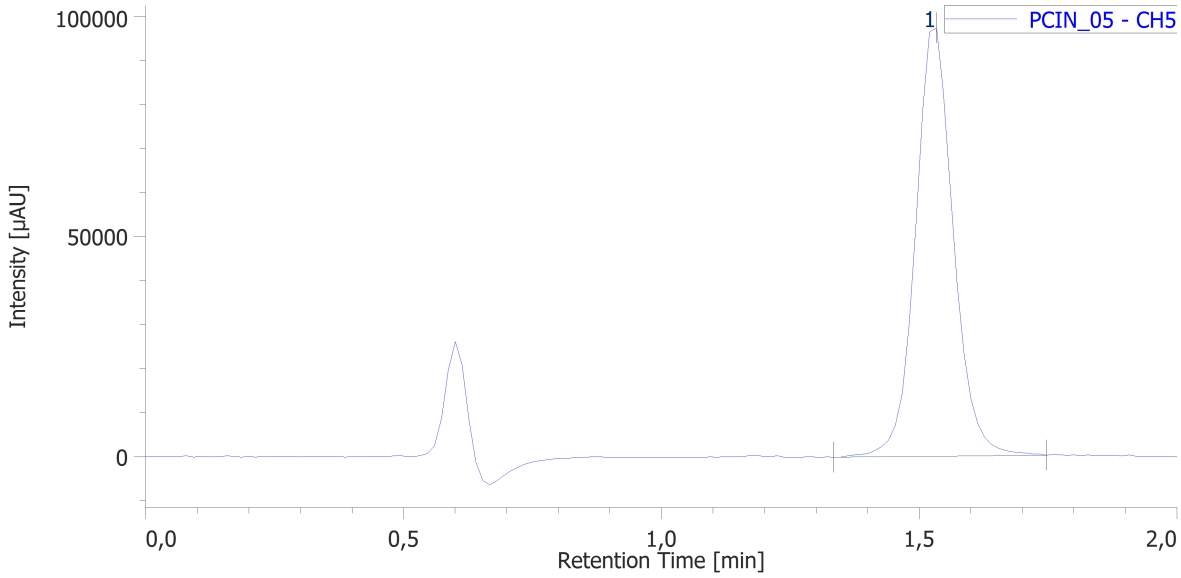

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:40:57
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:38:55
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	PCIN_05
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,533	499234	97195	100,000	100,000	N/A	2217	N/A	1,008	

Creator QPackSA
Reviewer
Approver

Chromatogram

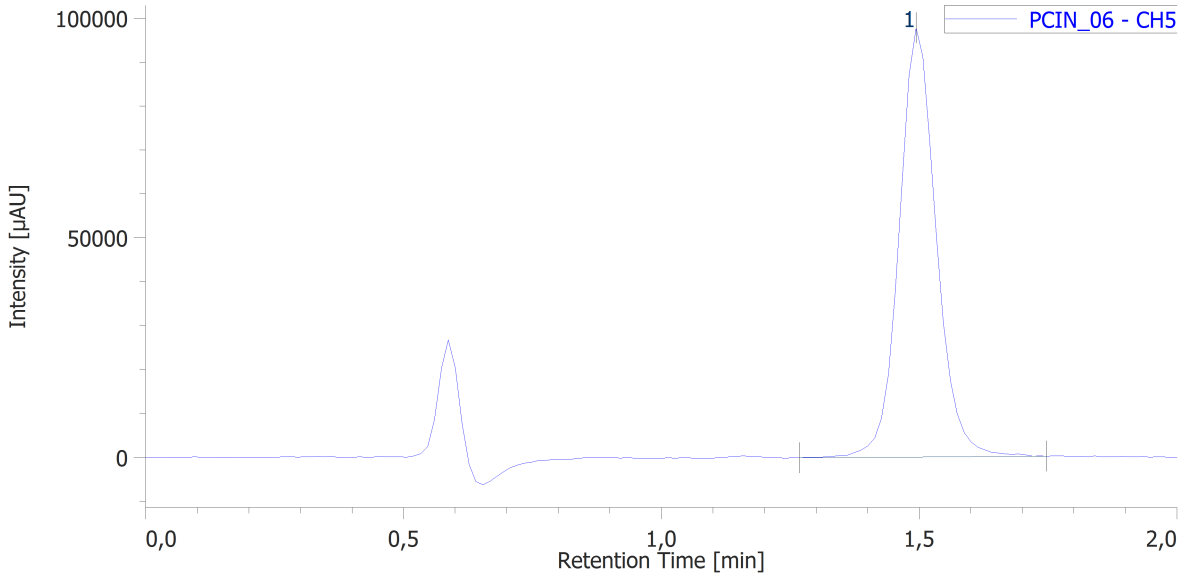

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:44:06
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:42:03
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	PCIN_06
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,493	490588	97707	100,000	100,000	N/A	2211	N/A	1,119	

Creator QPackSA
Reviewer
Approver

Chromatogram

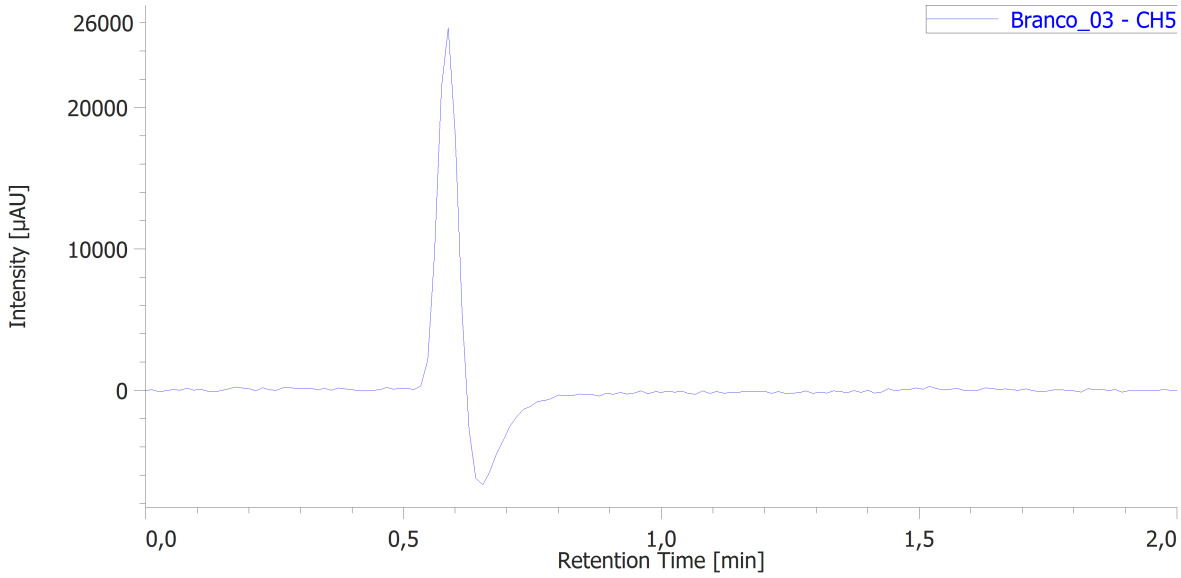


Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:47:13
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:45:12
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	Branco_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

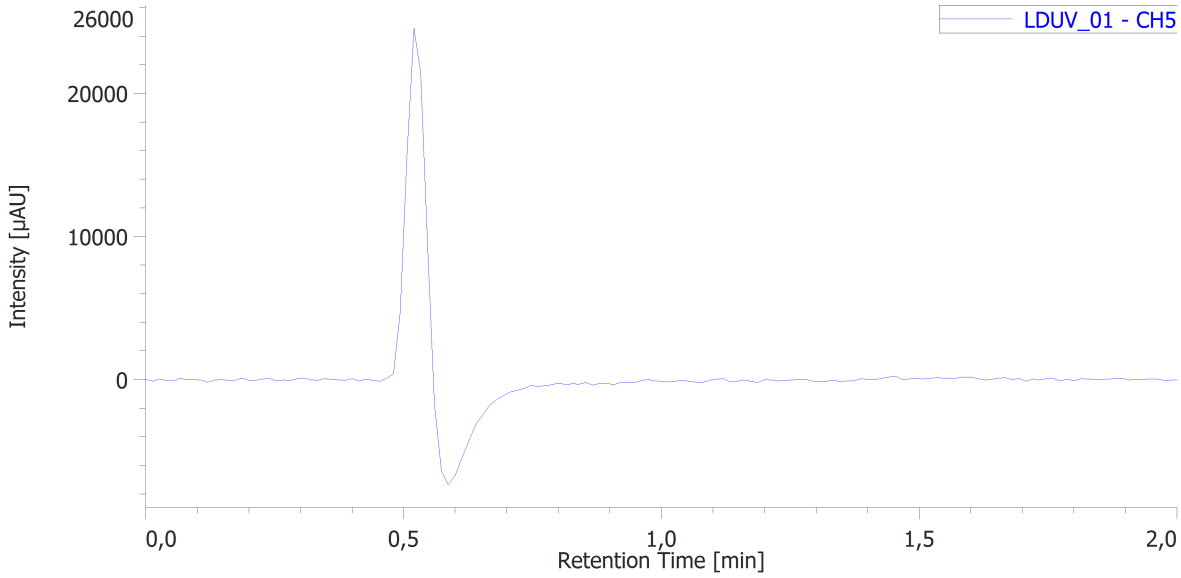


Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:50:25
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:48:23
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH5
Sample Name	LDUV_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

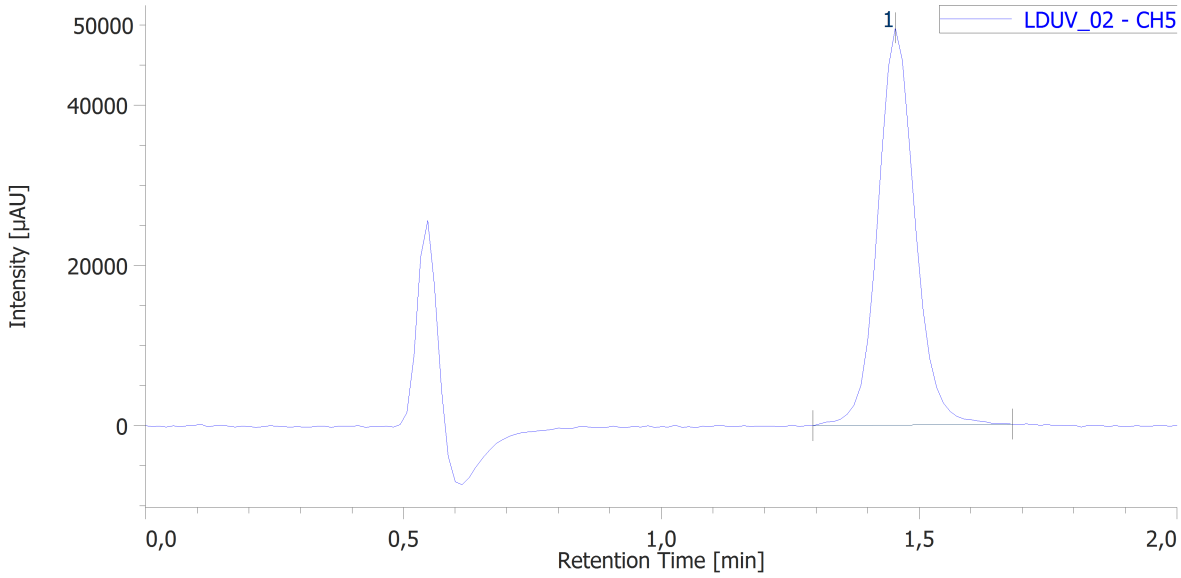

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:53:36
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:51:34
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH5
Sample Name	LDUV_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,453	248362	49544	100,000	100,000	N/A	2099	N/A	1,099	

Creator QPackSA
Reviewer
Approver

Chromatogram

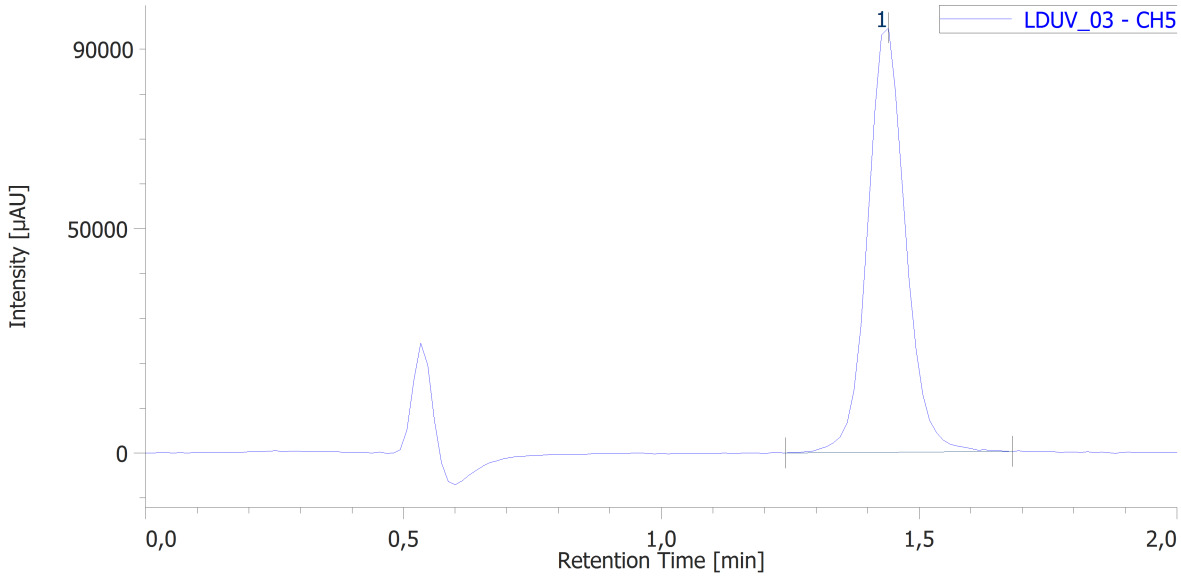

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:56:47
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:54:45
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH5
Sample Name	LDUV_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,440	484046	94502	100,000	100,000	N/A	1971	N/A	1,016	

Creator QPackSA
Reviewer
Approver

Chromatogram

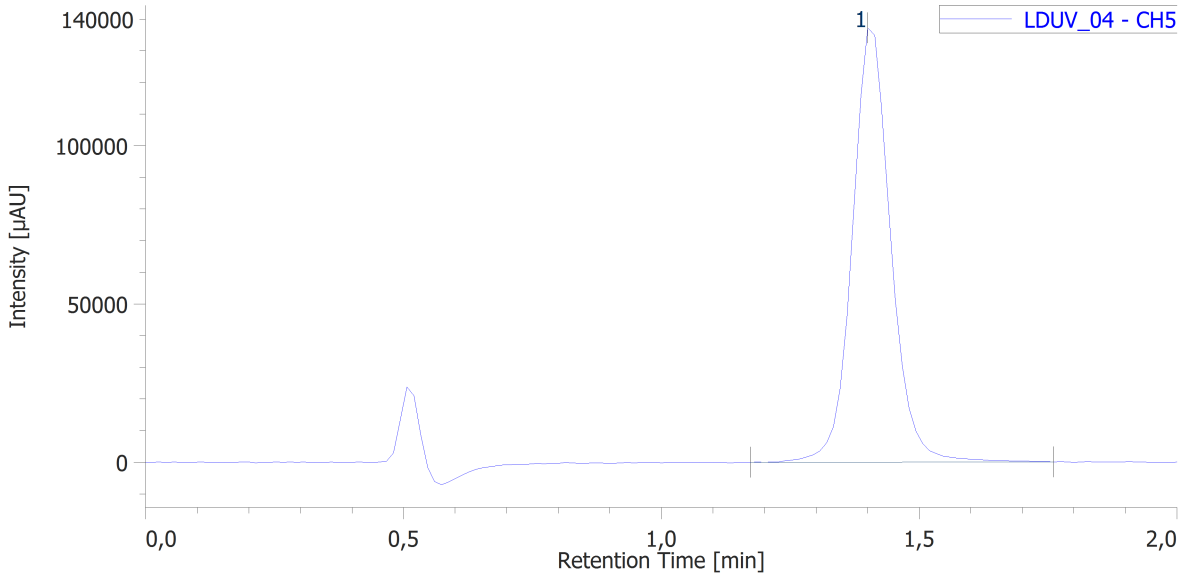

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 10:59:57
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 10:57:56
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH5
Sample Name	LDUV_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,400	711690	137097	100,000	100,000	N/A	1842	N/A	1,159	

Creator QPackSA
Reviewer
Approver

Chromatogram

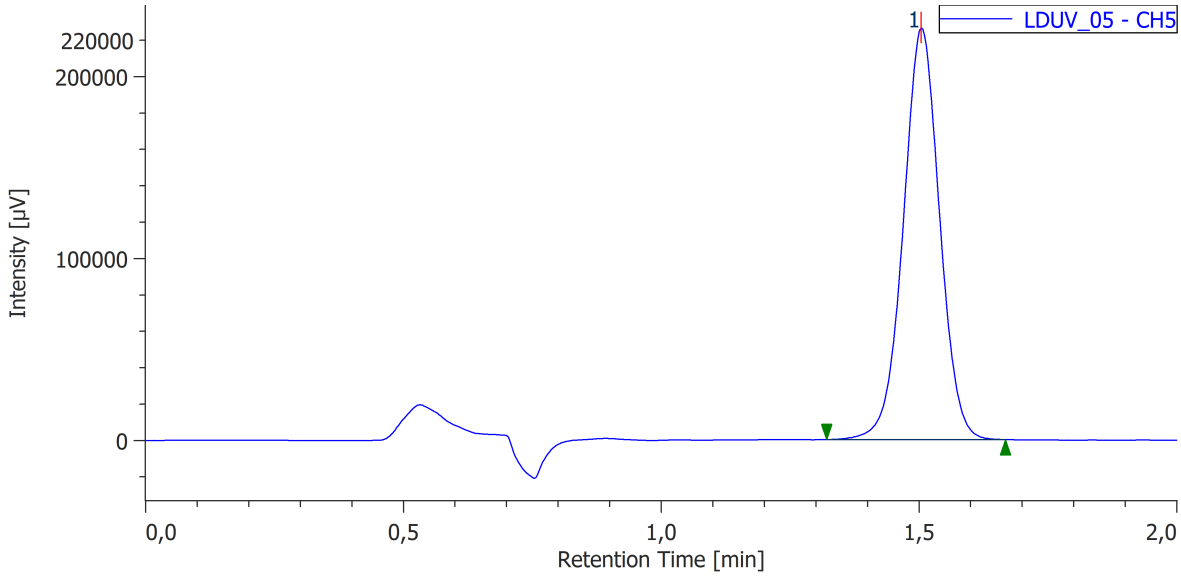

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:02::09
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:02:12
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação_
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH5
Sample Name	LDUV_05
Channel Name	273,0nm
Sampling Interval	800 [msec]

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
	Unknown	5	1,503	9371210	226356	100,000	100,000	N/A	2257	N/A	1,011	

Creator QPackSA
Reviewer
Approver

Chromatogram

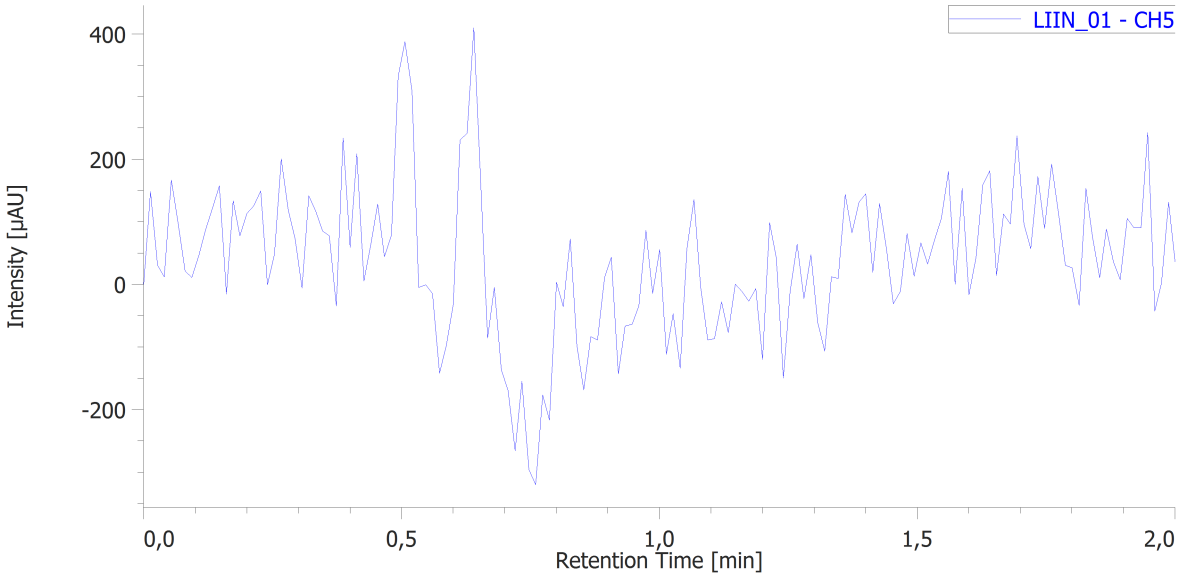


Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:27:11
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:25:08
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	LIIN_01
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

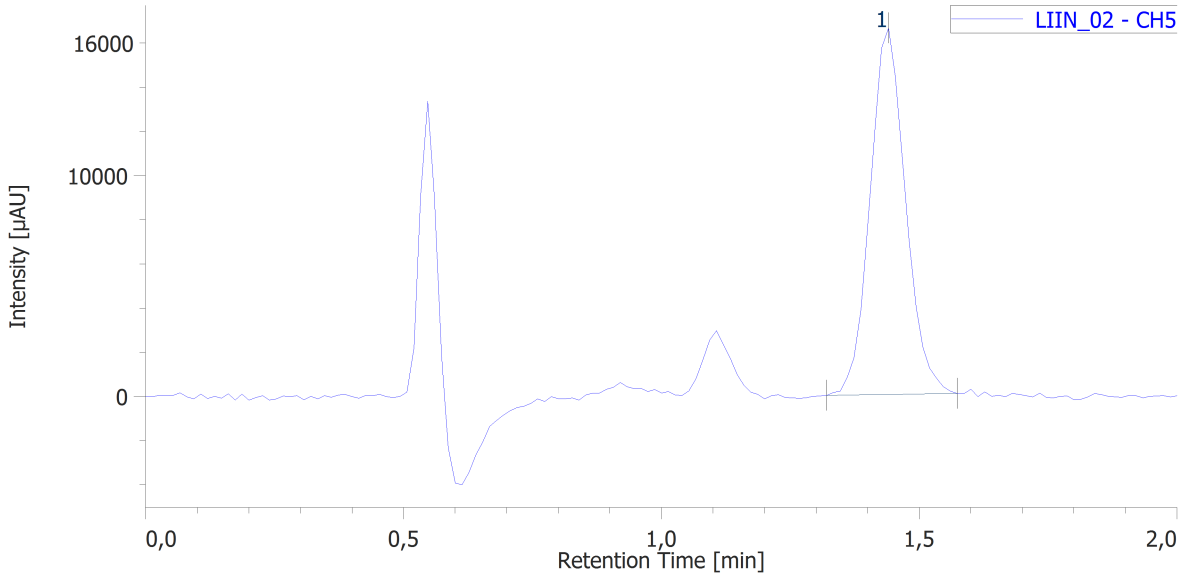

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:30:23
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:28:21
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	LIIN_02
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,440	79005	16573	100,000	100,000	N/A	2142	N/A	1,062	

Creator
Reviewer
Approver

Chromatogram

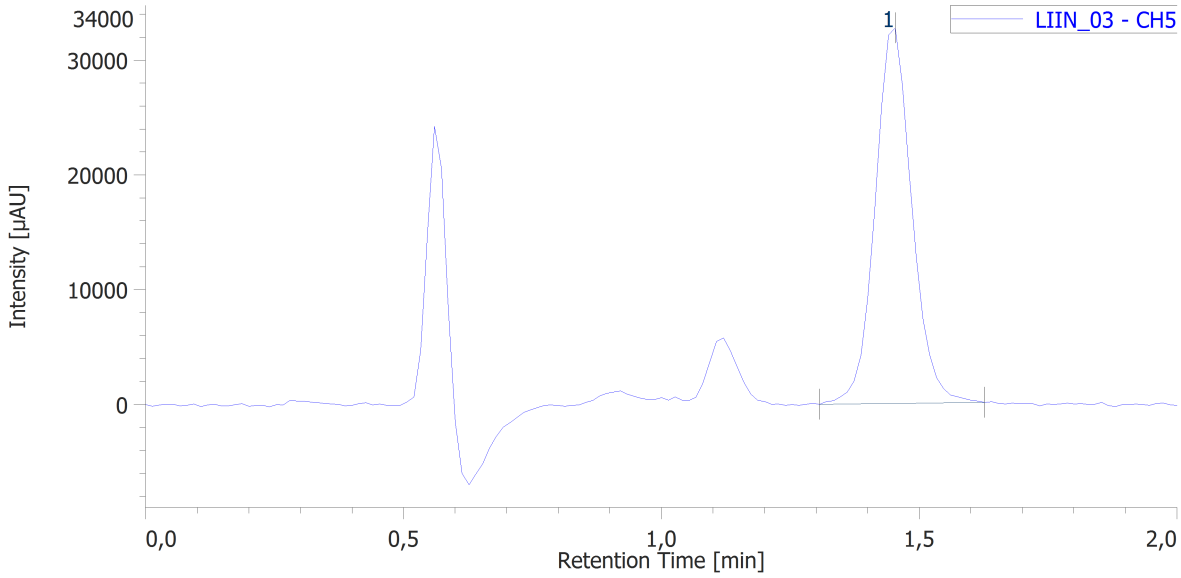

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:33:37
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:31:34
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	LIIN_03
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,453	162214	32674	100,000	100,000	N/A	2096	N/A	1,019	

Creator
Reviewer
Approver

Chromatogram

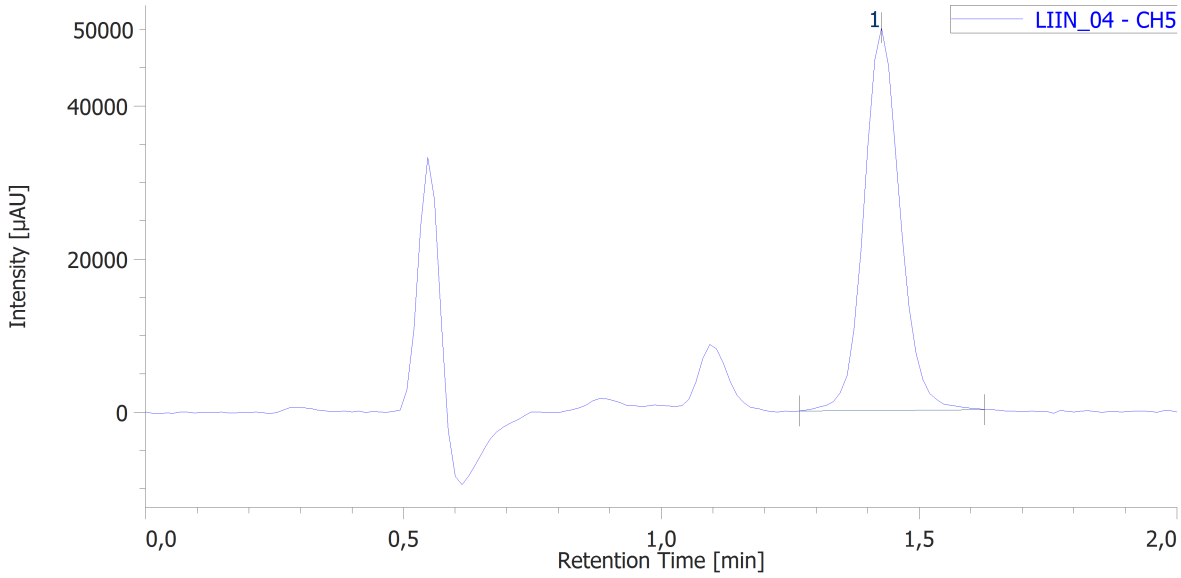

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:36:49
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:34:47
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	LIIN_04
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,427	243222	49933	100,000	100,000	N/A	2105	N/A	1,076	

Creator
Reviewer
Approver

Chromatogram

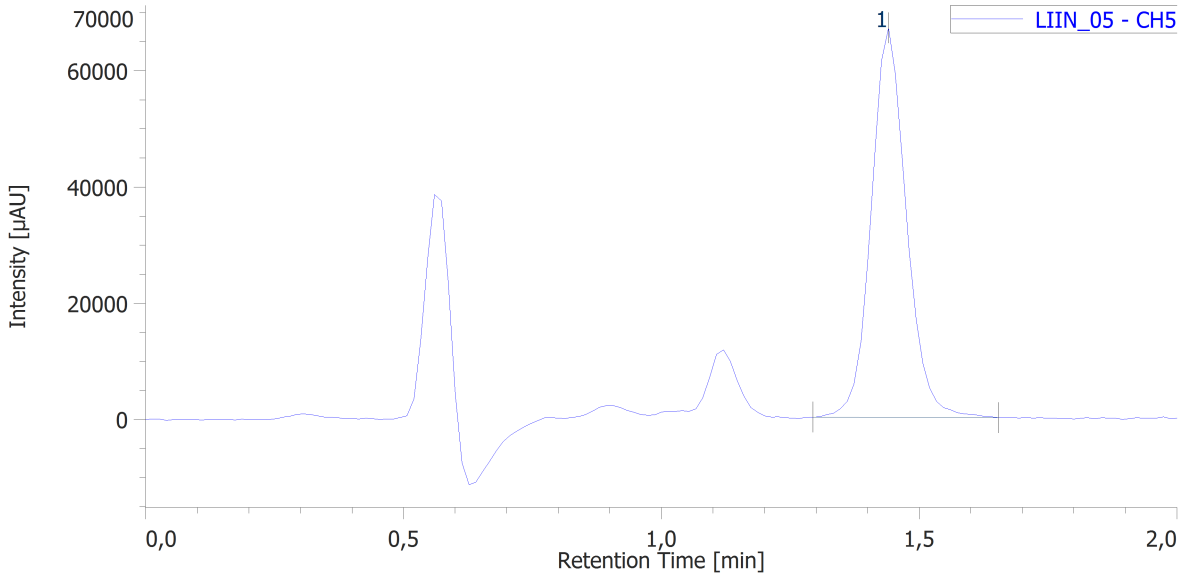

Chromatogram Information	
User Name	QPackSA
Date Modified	26/11/2024 11:40:02
Description	
HPLC System Name	HPL25
Injection Date	26/11/2024 11:38:00
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação_24
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH5
Sample Name	LIIN_05
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,440	317033	66959	100,000	100,000	N/A	2275	N/A	1,083	

Creator
Reviewer
Approver

Chromatogram

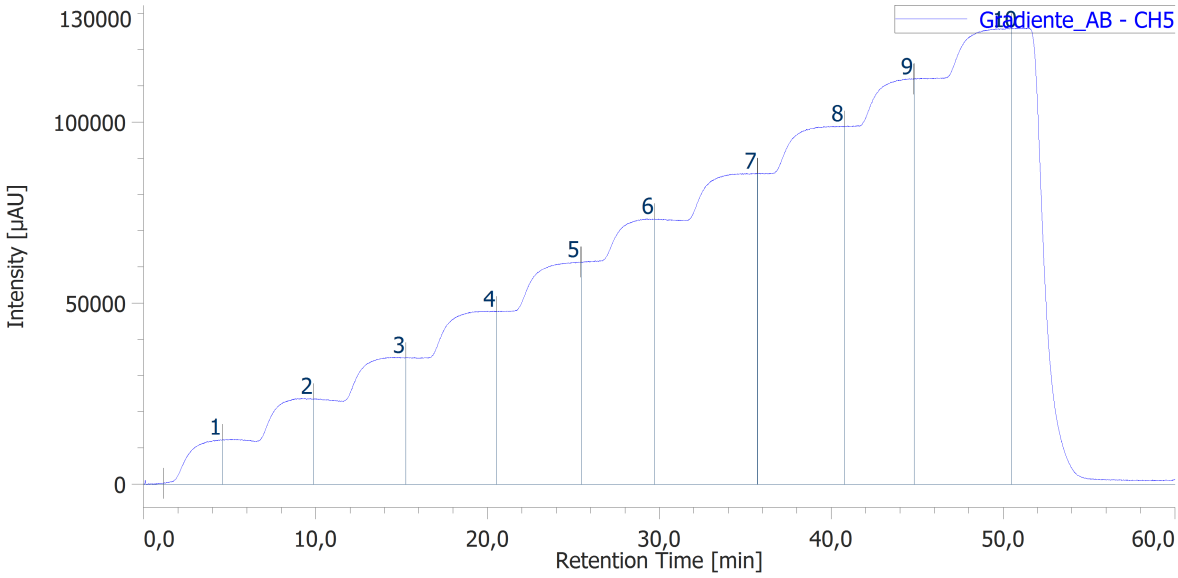

Chromatogram Information	
User Name	QPackSA
Date Modified	28/11/2024 09:14:28
Description	
HPLC System Name	HPL25
Injection Date	28/11/2024 08:14:27
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	60,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB_10 PASSOS
Peak ID Table	GRAD AB
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente_AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Grad AB_ (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	10%	5	4,567	1562224	12312	0,984	1,824	N/A	N/A	N/A	N/A	
2	20%	5	9,880	5565791	23532	3,506	3,486	N/A	N/A	N/A	N/A	
3	30%	5	15,240	9422876	34903	5,936	5,170	N/A	N/A	N/A	N/A	
4	40%	5	20,500	13338684	47634	8,403	7,056	N/A	N/A	N/A	N/A	
5	50%	5	25,380	16534585	61372	10,417	9,091	N/A	N/A	N/A	N/A	
6	60%	5	29,713	17330559	73282	10,918	10,856	N/A	N/A	N/A	N/A	
7	70%	5	35,700	68605	85752	0,043	12,703	N/A	N/A	N/A	N/A	
8	80%	5	40,747	28498302	98792	17,954	14,635	N/A	N/A	N/A	N/A	
9	90%	5	44,793	25806783	111823	16,258	16,565	N/A	N/A	N/A	N/A	
10	100%	5	50,473	40600056	125654	25,578	18,614	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

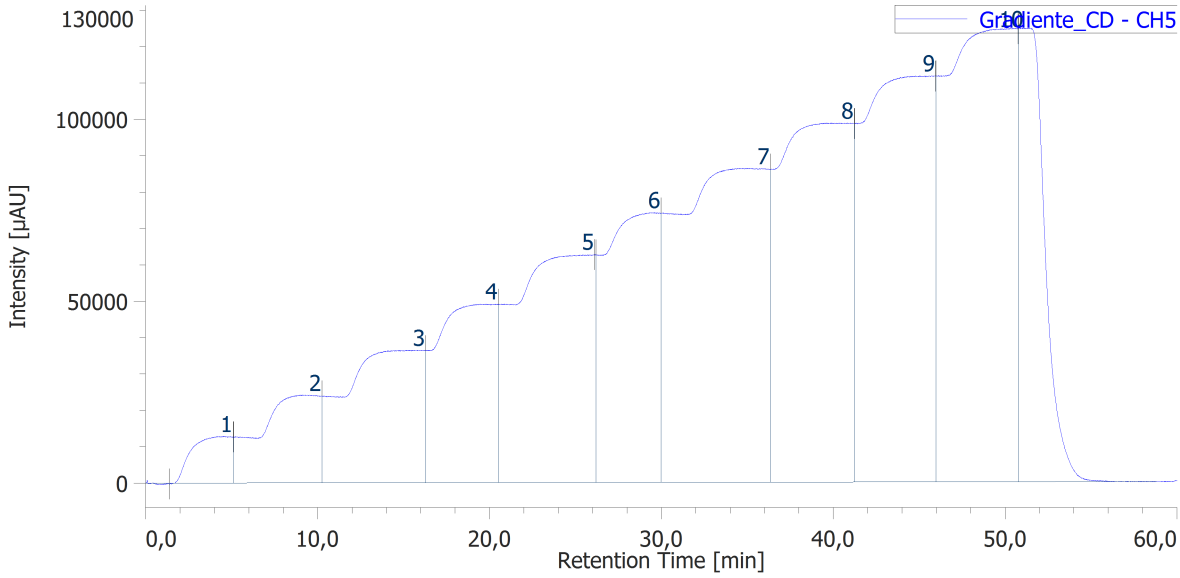

Chromatogram Information	
User Name	QPackSA
Date Modified	28/11/2024 10:14:42
Description	
HPLC System Name	HPL25
Injection Date	28/11/2024 09:14:40
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	60,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD_10 PASSOS
Peak ID Table	GRAD CD_1
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_CD-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	Grad CD (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	10%	5	5,093	2010023	12577	1,054	1,854	N/A	N/A	N/A	N/A	
2	20%	5	10,247	5825346	23820	3,056	3,511	N/A	N/A	N/A	N/A	
3	30%	5	16,293	11497573	36219	6,032	5,339	N/A	N/A	N/A	N/A	
4	40%	5	20,500	11486878	48954	6,026	7,216	N/A	N/A	N/A	N/A	
5	50%	5	26,113	19647658	62566	10,307	9,223	N/A	N/A	N/A	N/A	
6	60%	5	29,967	15901043	73946	8,342	10,900	N/A	N/A	N/A	N/A	
7	70%	5	36,327	31008216	85970	16,267	12,673	N/A	N/A	N/A	N/A	
8	80%	5	41,220	28076640	98447	14,729	14,512	N/A	N/A	N/A	N/A	
9	90%	5	45,953	30665982	111439	16,087	16,427	N/A	N/A	N/A	N/A	
10	100%	5	50,740	34506022	124455	18,101	18,346	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver