

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:40:09
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:39:08
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 200nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

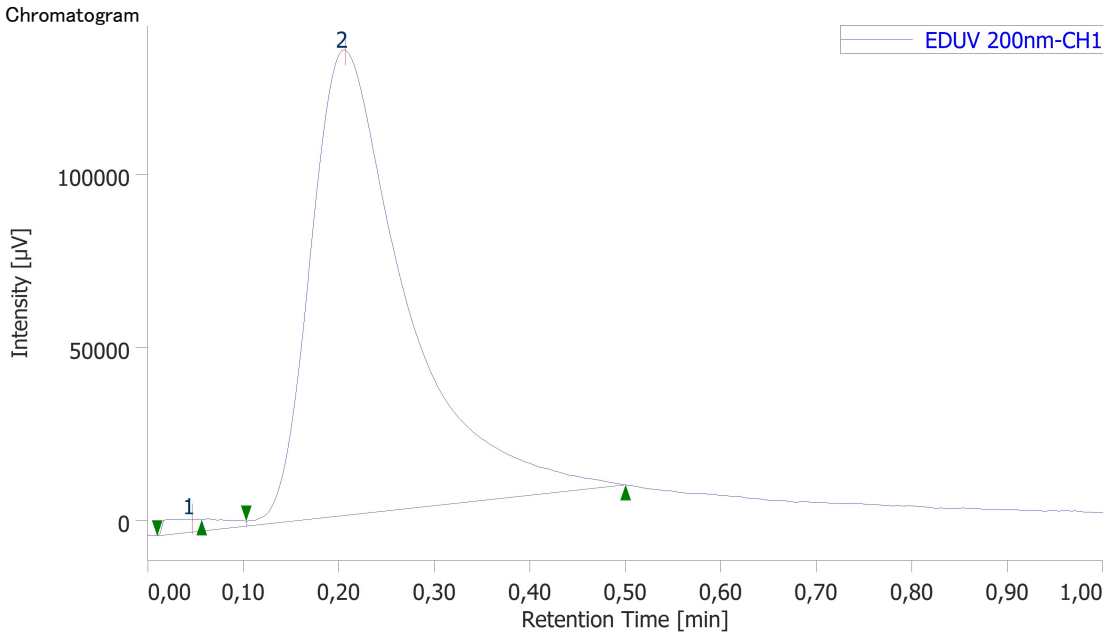

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,047	10001	3731	1,054	2,699	N/A	N/A	N/A	N/A	
2	Unknown	1	0,207	939018	134485	98,946	97,301	N/A	25	N/A	1,966	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:41:33
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:40:33
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 201nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

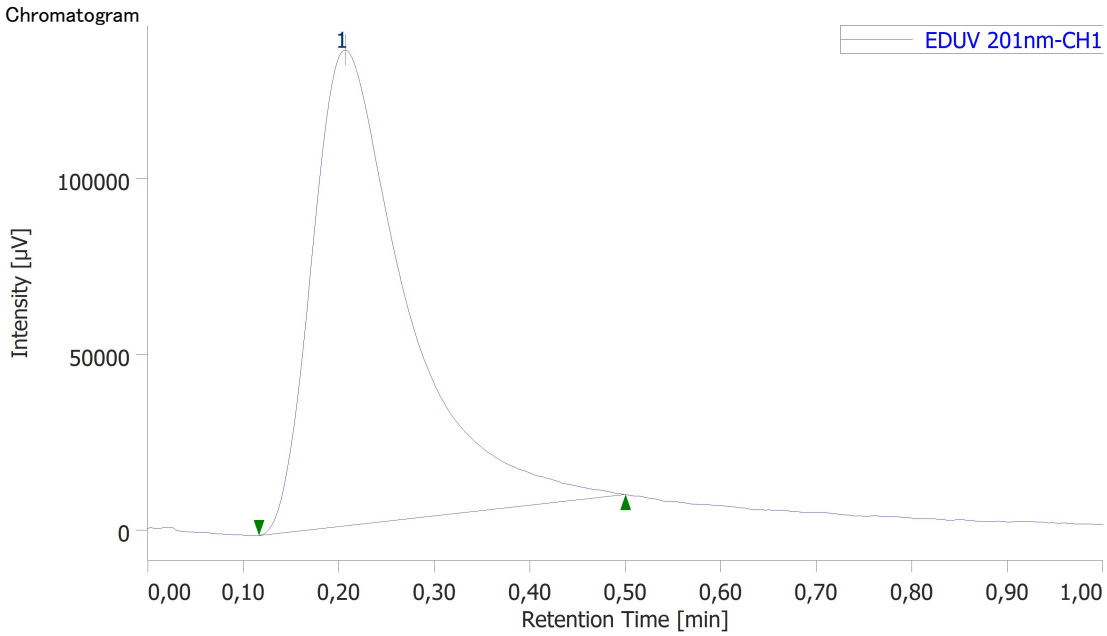

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,207	939744	135482	100,000	100,000	N/A	25	N/A	2,037	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:43:05
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:42:03
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 202nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

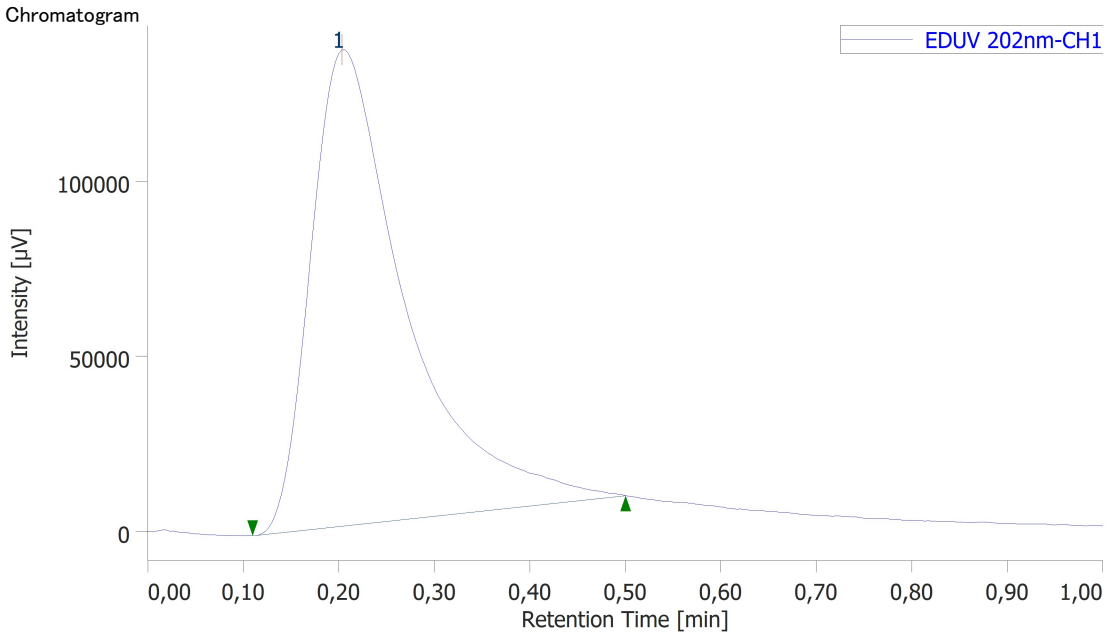

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	943543	135999	100,000	100,000	N/A	25	N/A	2,121	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:44:41
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:43:40
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 203nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

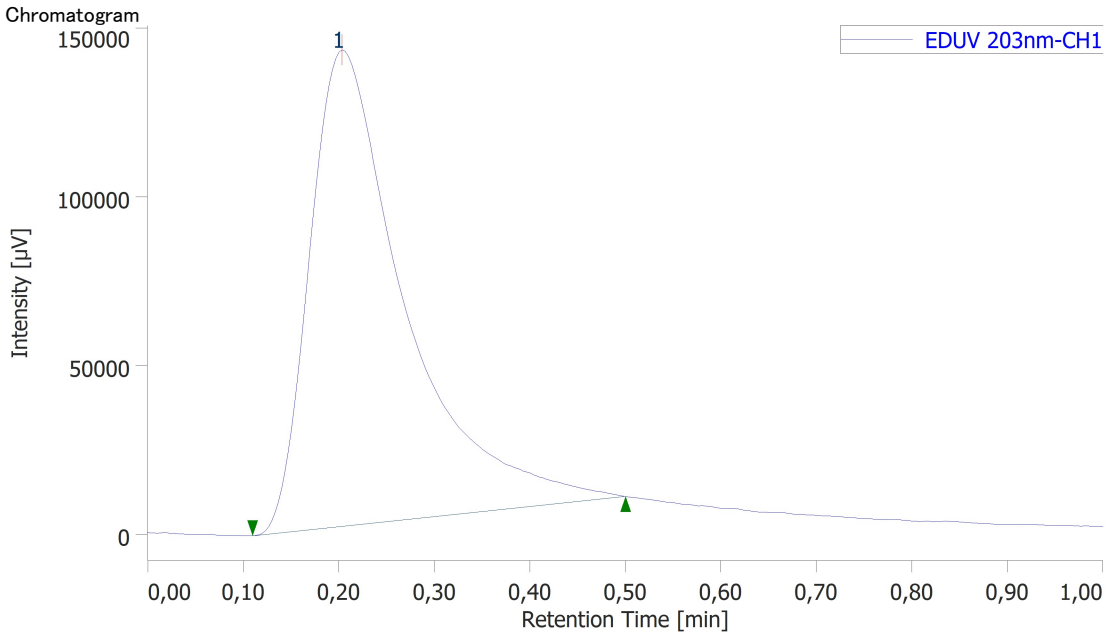


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	984884	141238	100,000	100,000	N/A	24	N/A	2,083	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:46:13
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:45:12
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 204nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

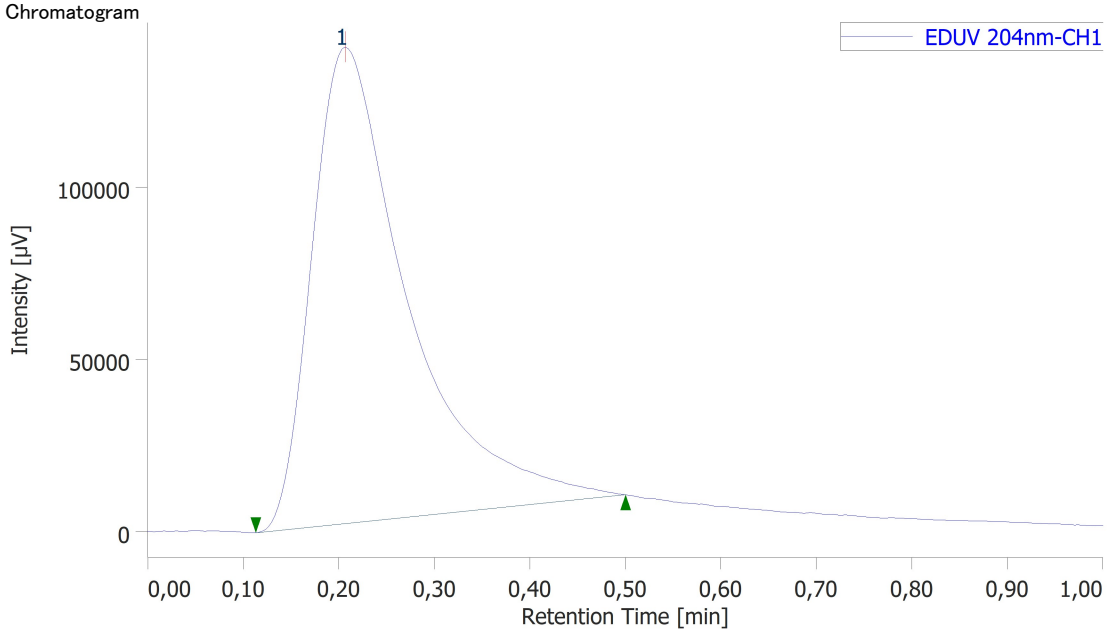

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,207	963912	138343	100,000	100,000	N/A	25	N/A	2,020	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:47:39
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:46:38
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 205nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

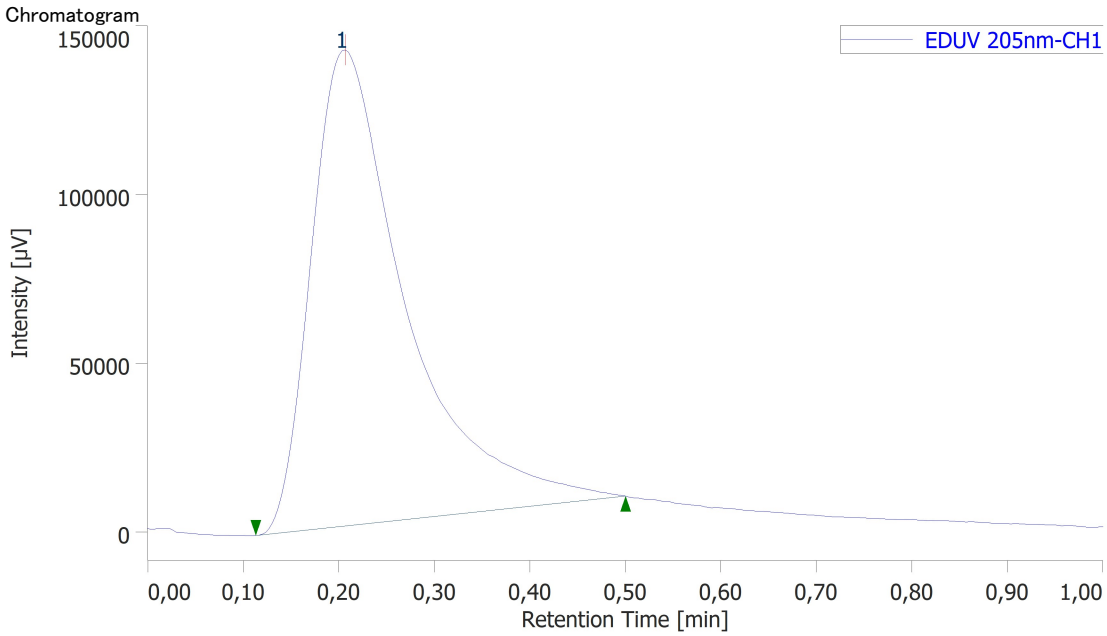

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,207	974169	141081	100,000	100,000	N/A	26	N/A	1,999	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:49:13
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:48:13
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 206nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

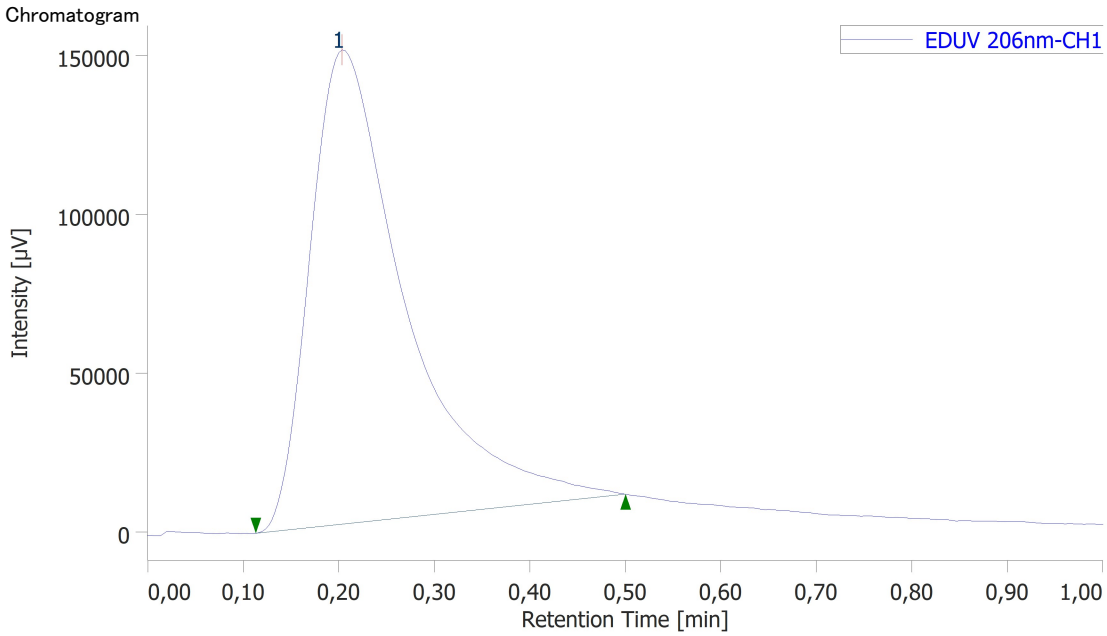

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1039012	149262	100,000	100,000	N/A	24	N/A	2,085	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:50:45
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:49:45
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 207nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

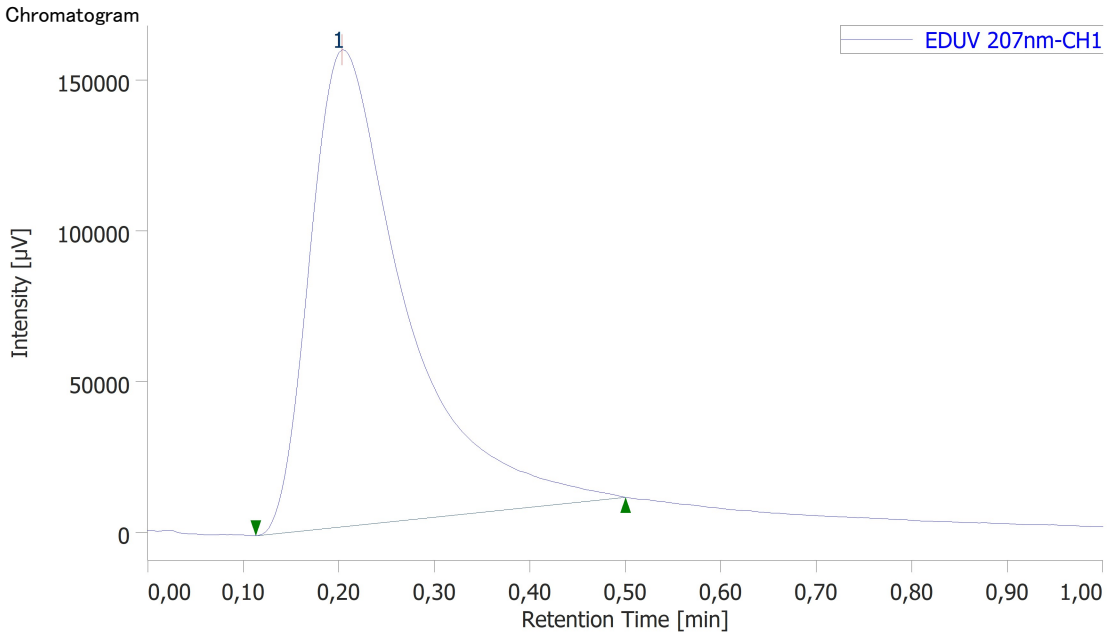

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1104142	158112	100,000	100,000	N/A	24	N/A	2,100	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:52:27
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:51:26
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 208nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

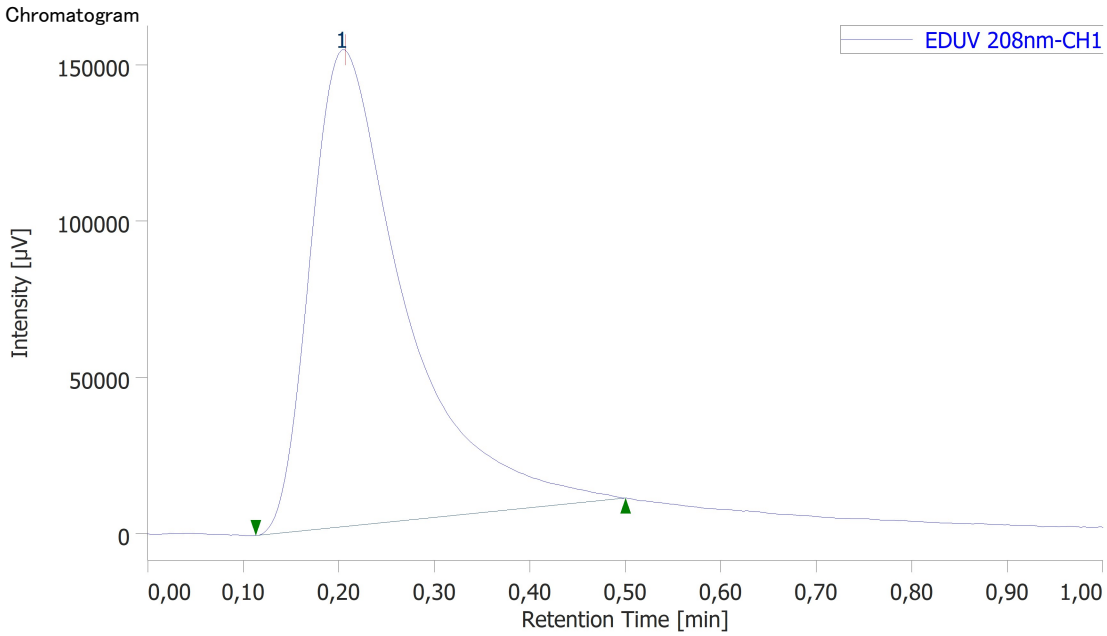


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,207	1056398	152485	100,000	100,000	N/A	25	N/A	1,985	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:57:37
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:56:36
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 240nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

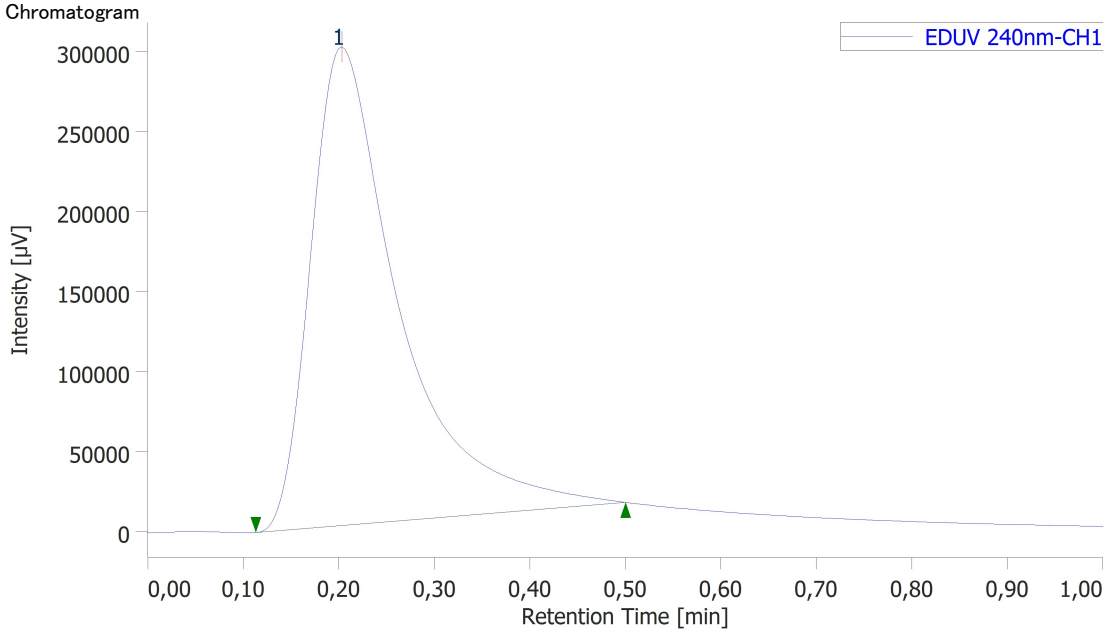


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1929978	299310	100,000	100,000	N/A	29	N/A	2,010	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 11:59:01
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:58:00
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 241nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

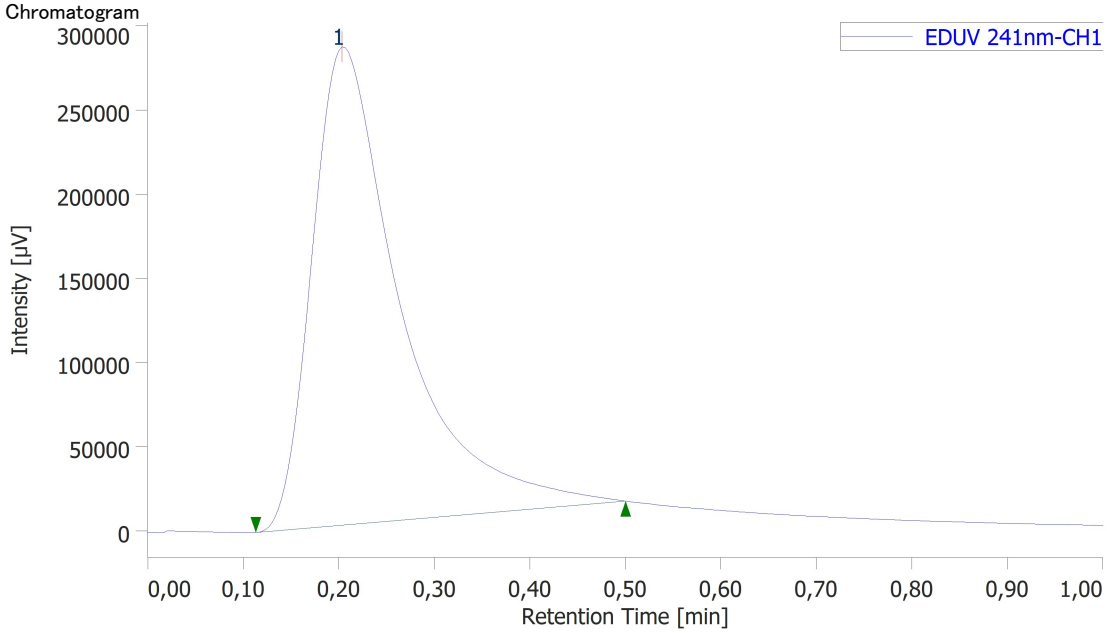


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1840401	284036	100,000	100,000	N/A	28	N/A	2,045	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:00:59
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 11:59:58
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 242nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

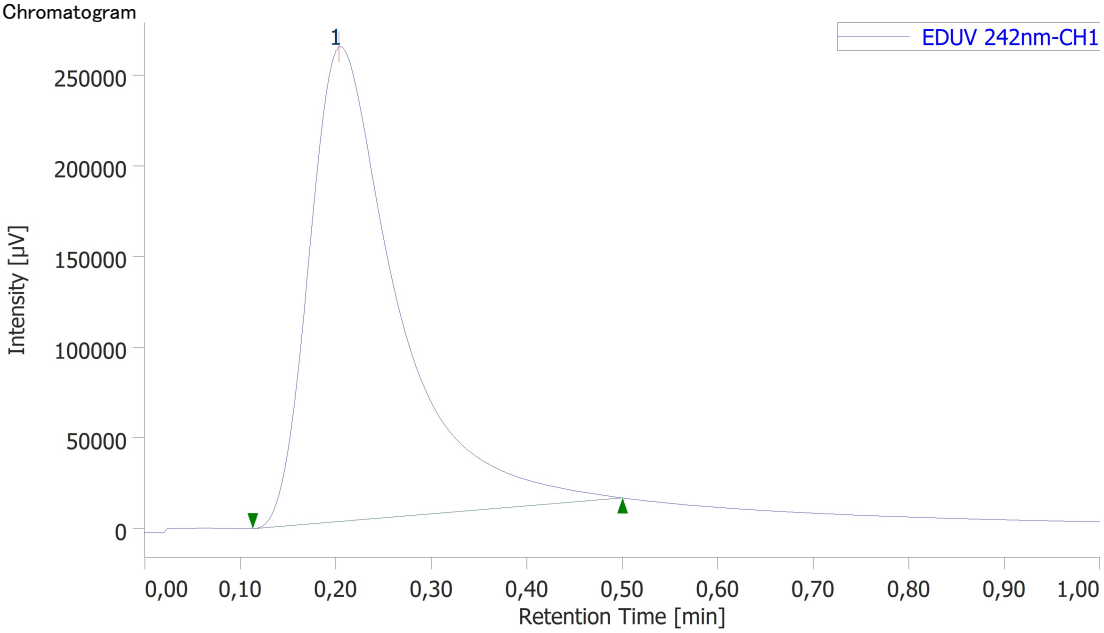

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1694930	261651	100,000	100,000	N/A	28	N/A	2,050	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:02:21
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:01:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 243nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

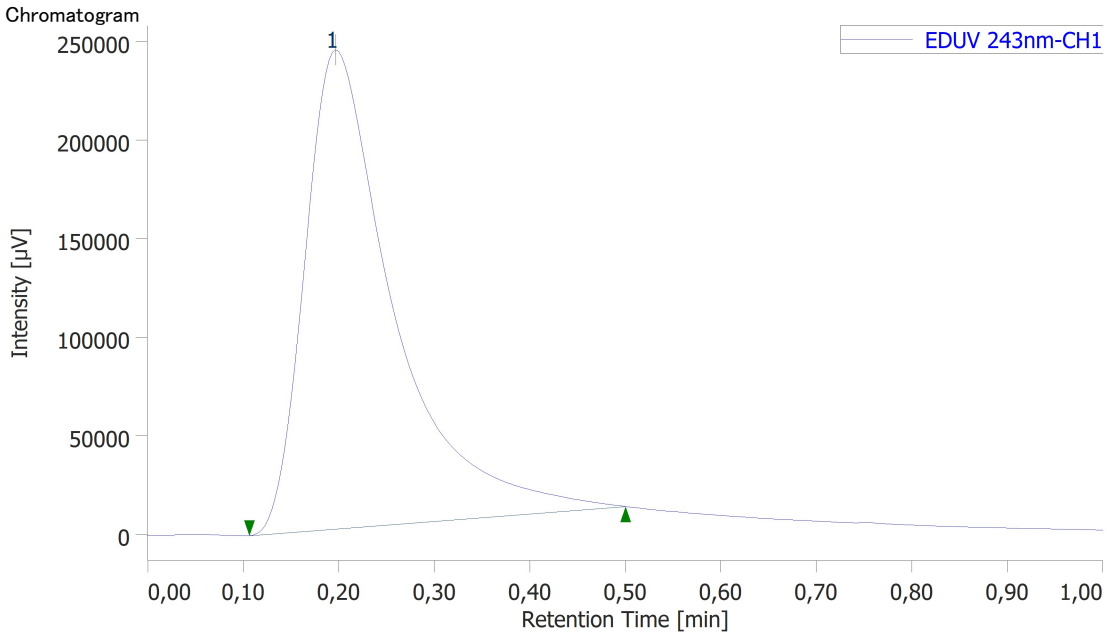

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,197	1580368	243124	100,000	100,000	N/A	26	N/A	2,028	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:03:55
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:02:55
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 244nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

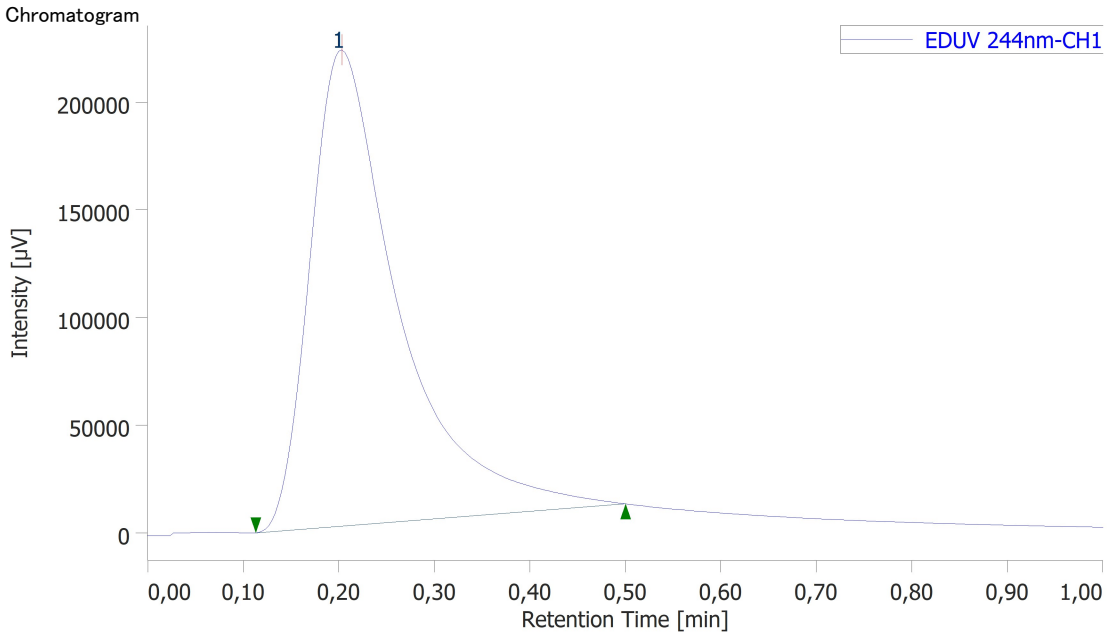


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1430455	221021	100,000	100,000	N/A	28	N/A	1,978	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:05:21
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:04:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 245nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

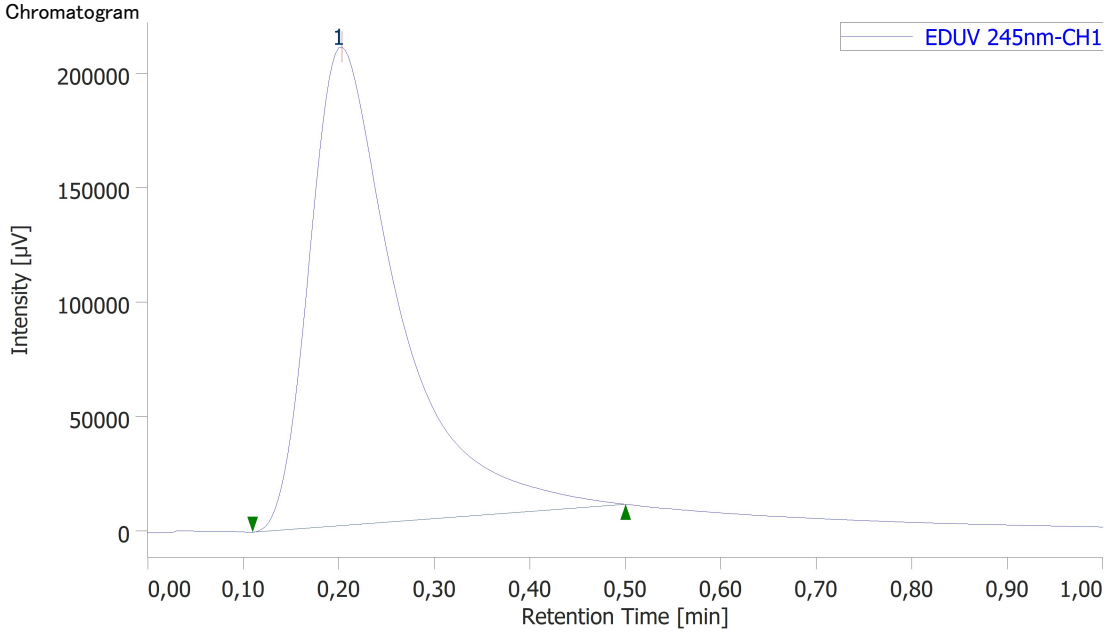

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1362637	208986	100,000	100,000	N/A	28	N/A	1,949	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:06:47
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:05:45
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 246nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

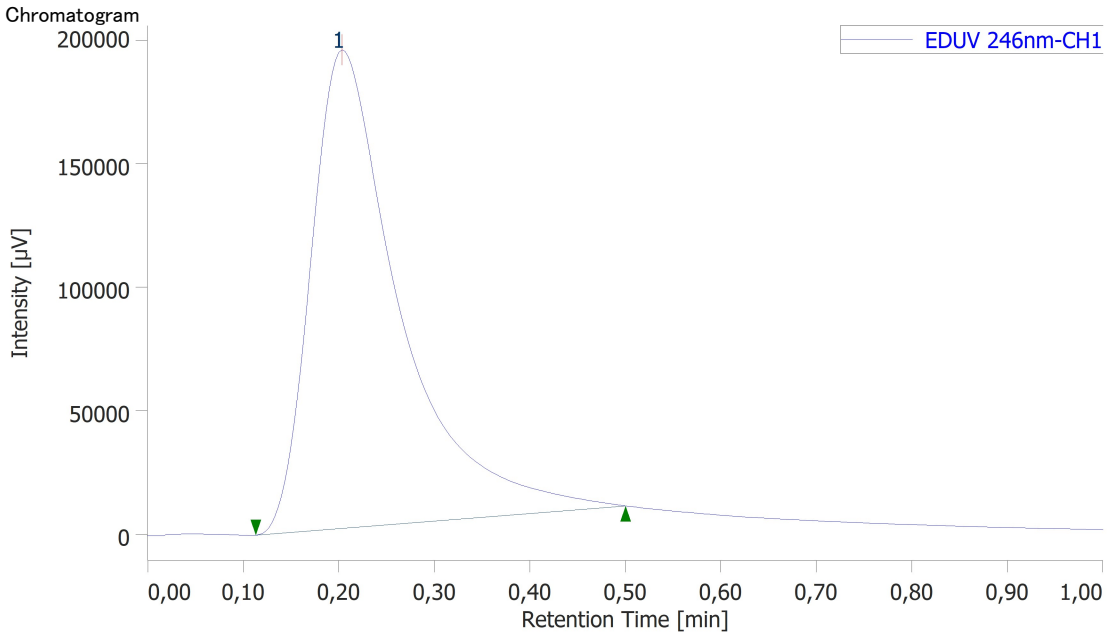

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1258927	193670	100,000	100,000	N/A	28	N/A	1,995	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:08:31
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:07:30
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 247nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

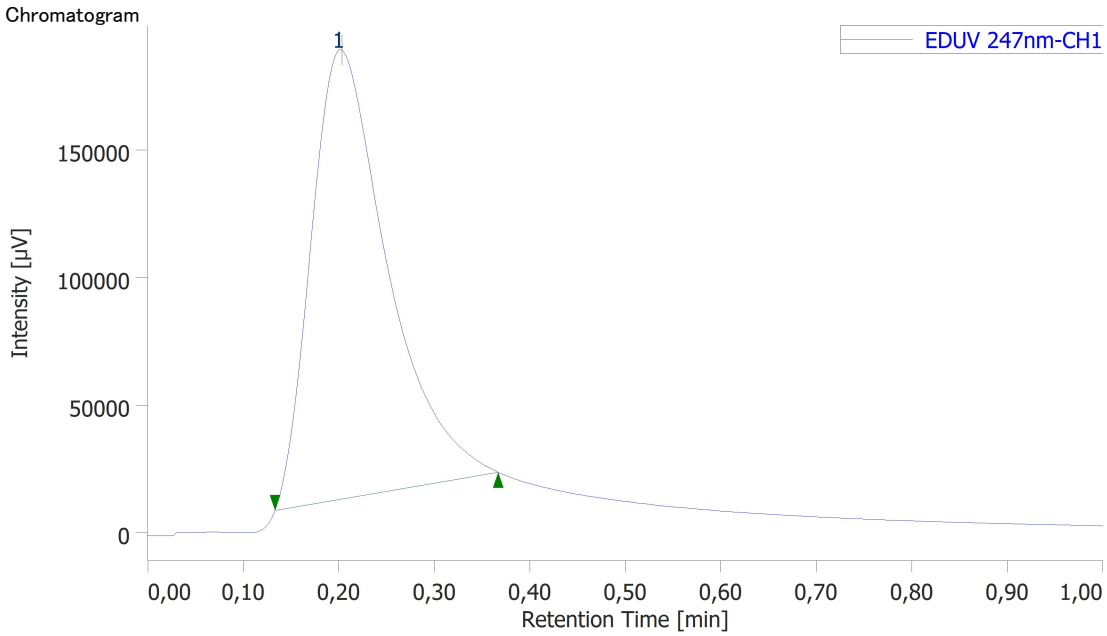

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	978894	176144	100,000	100,000	N/A	33	N/A	1,557	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 12:10:01
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 12:09:01
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 248nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

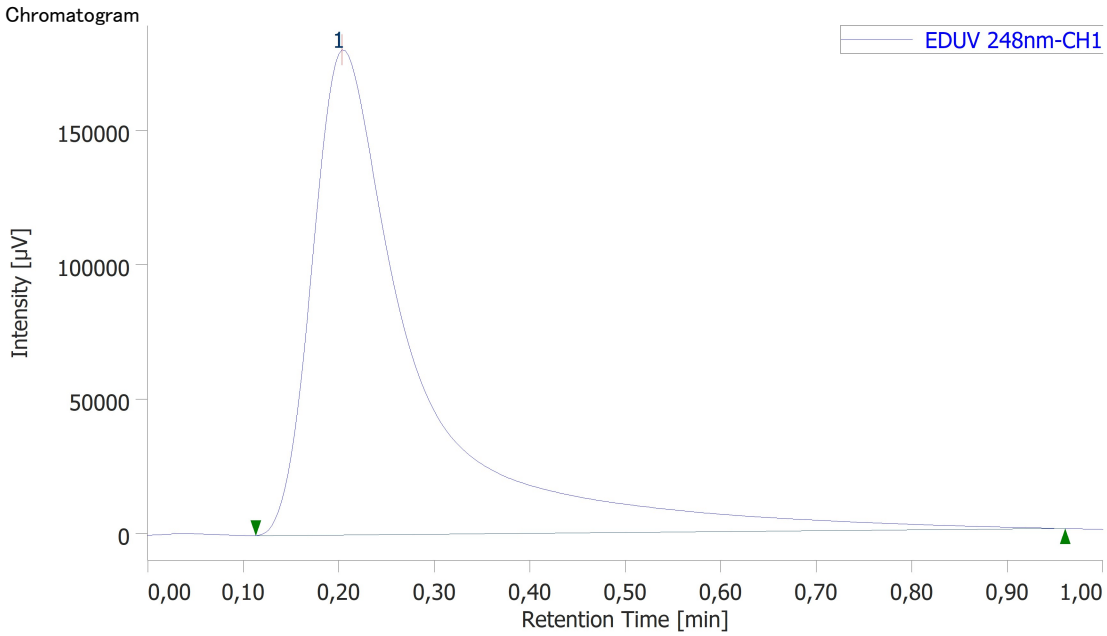

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	1373077	180507	100,000	100,000	N/A	28	N/A	2,967	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:08:15
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:07:14
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 268nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

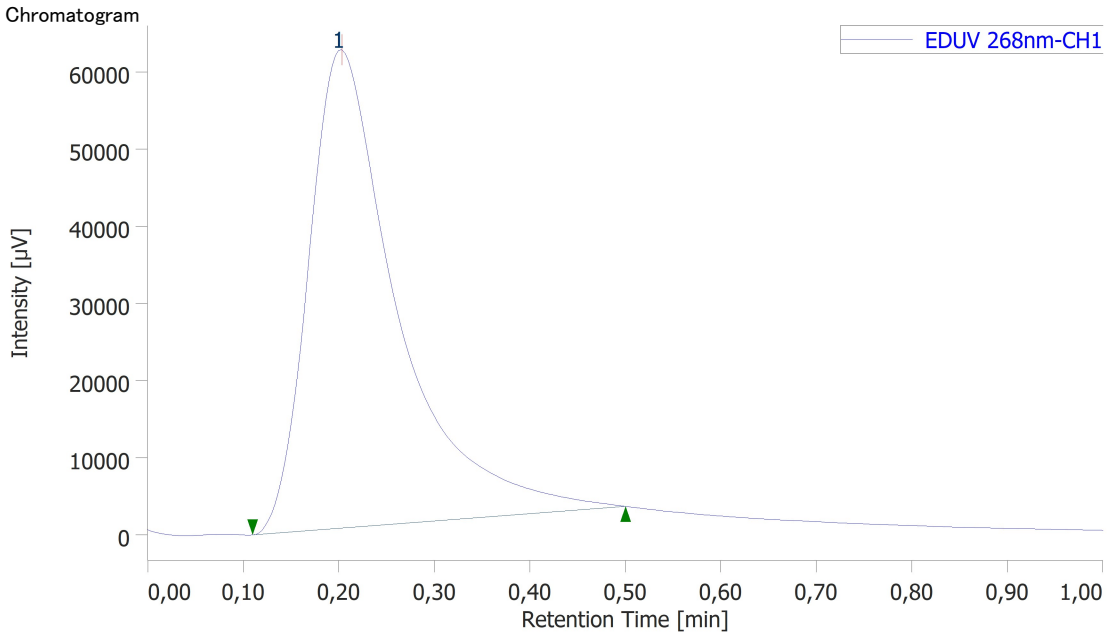


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	402977	61978	100,000	100,000	N/A	29	N/A	1,879	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:10:23
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:09:22
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 269nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

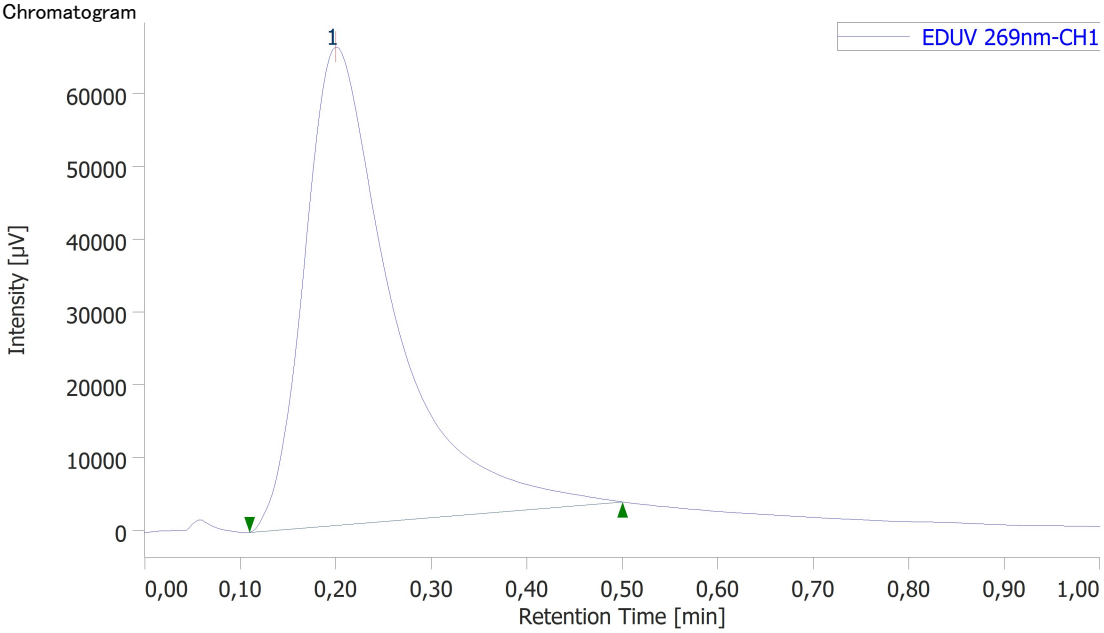

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	427886	65739	100,000	100,000	N/A	28	N/A	1,923	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:11:49
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:10:48
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 270nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

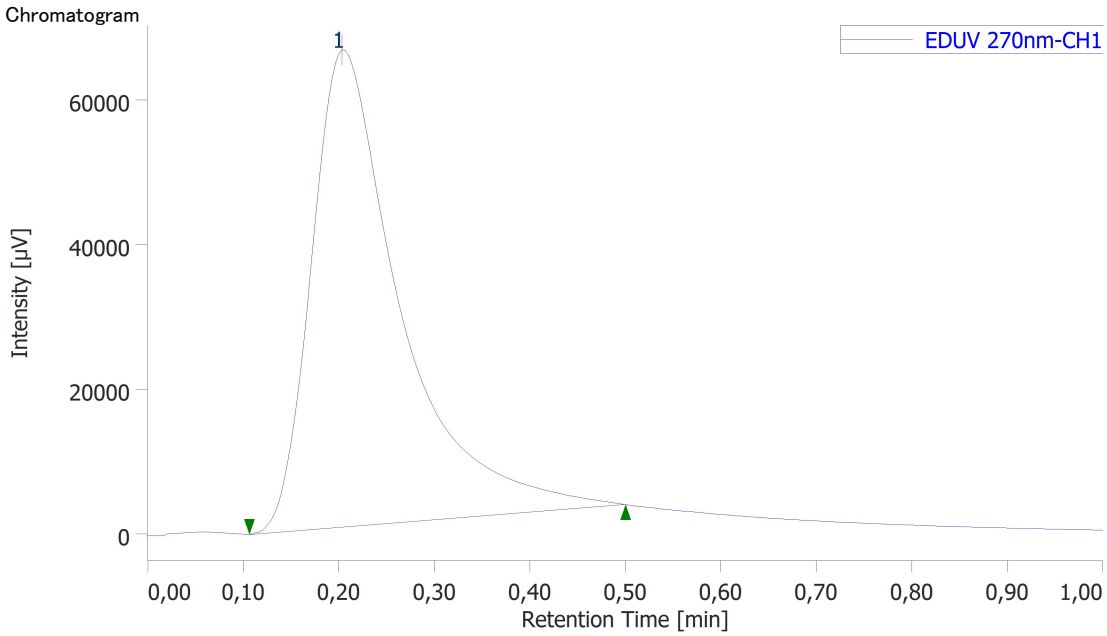

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	429637	65970	100,000	100,000	N/A	28	N/A	1,983	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:13:39
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:12:38
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 271nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

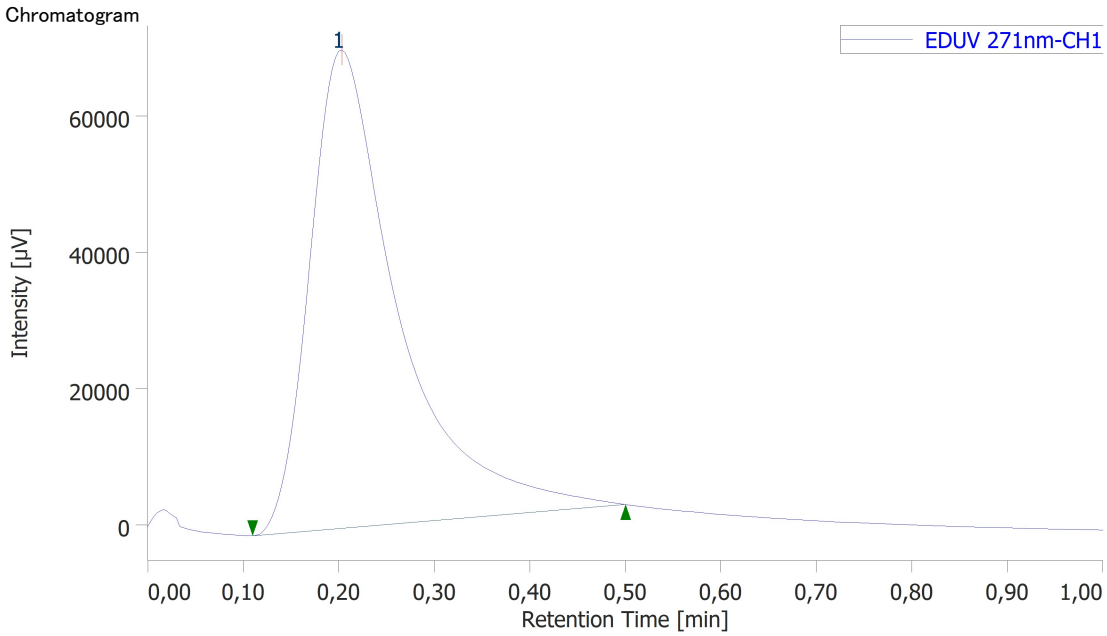

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	454337	70161	100,000	100,000	N/A	29	N/A	1,945	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:15:01
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:13:59
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 272nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

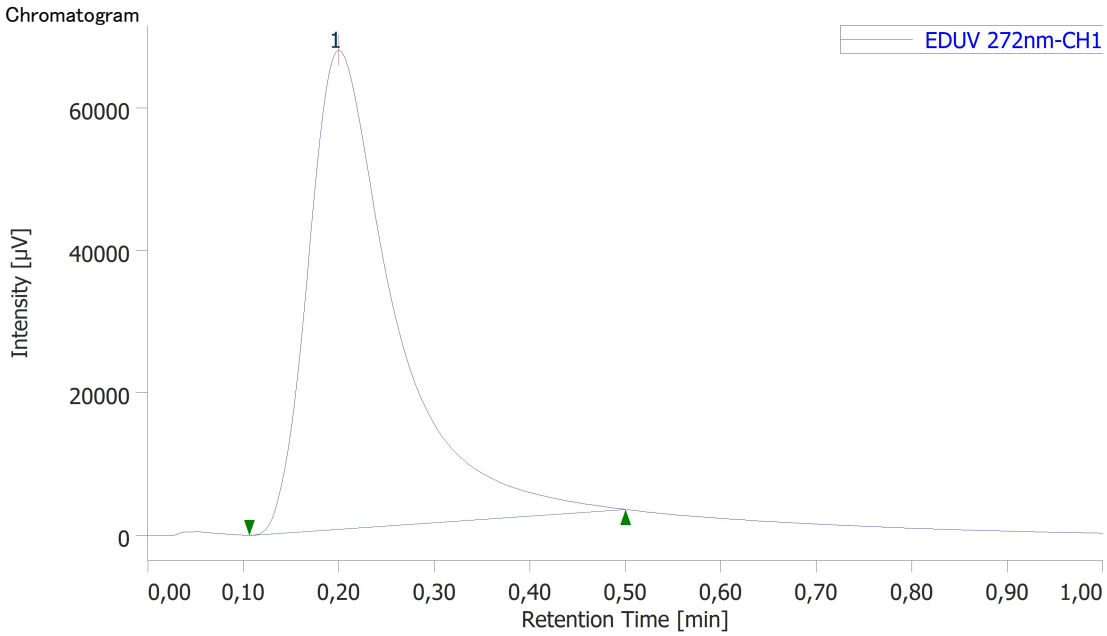


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	425664	67360	100,000	100,000	N/A	29	N/A	1,993	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:16:51
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:15:50
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 273nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

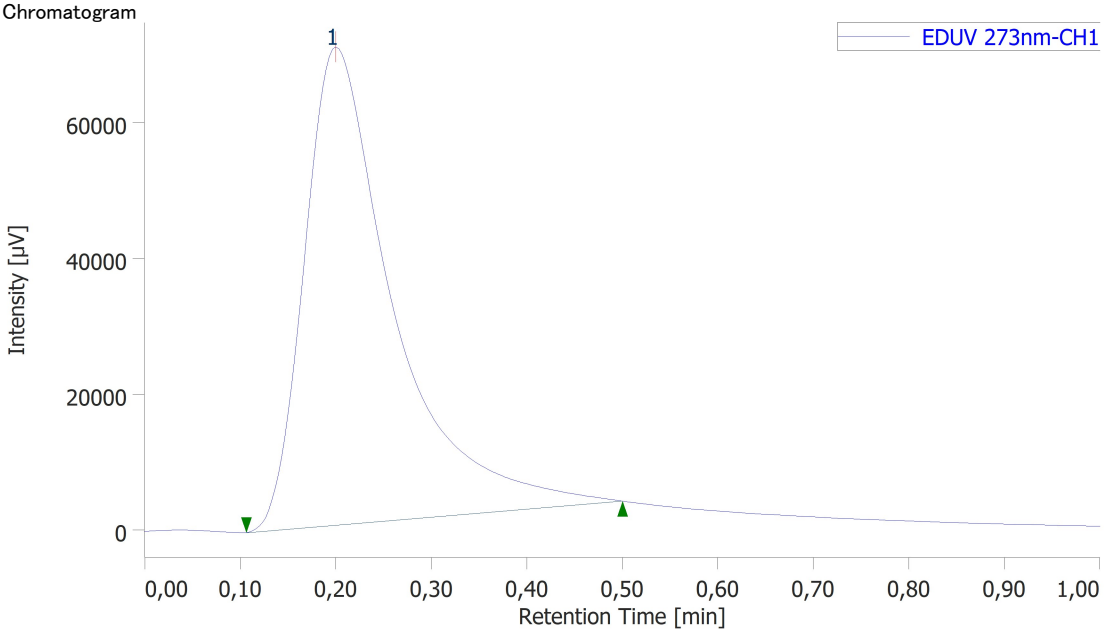

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	459138	70506	100,000	100,000	N/A	28	N/A	1,977	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:18:21
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:17:20
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 274nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

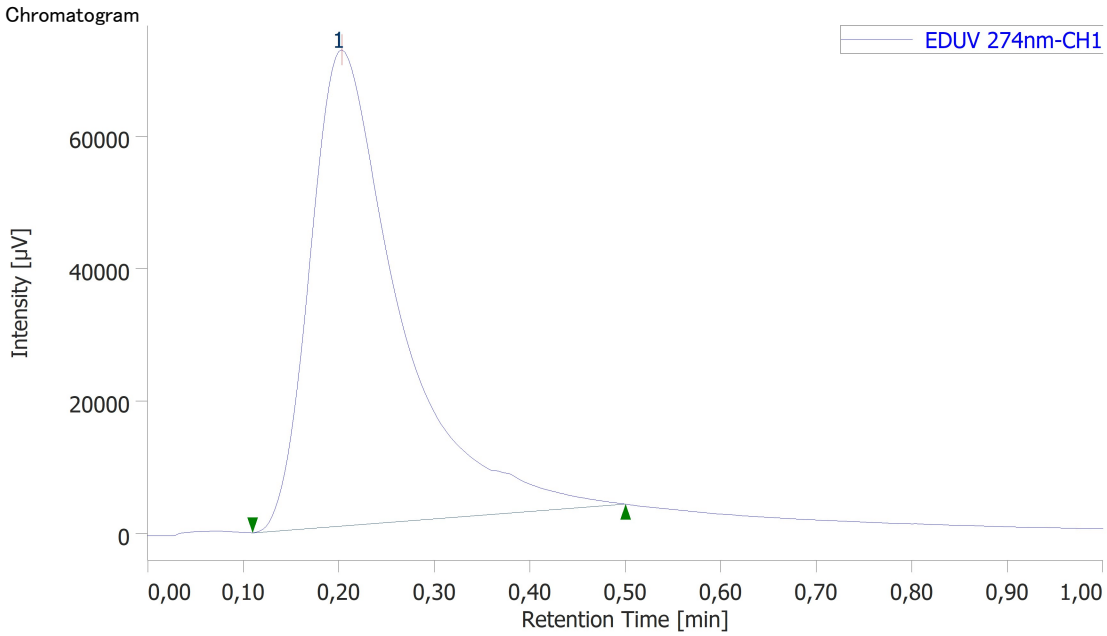

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,203	468533	71923	100,000	100,000	N/A	28	N/A	1,978	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:20:19
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:19:17
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 275nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

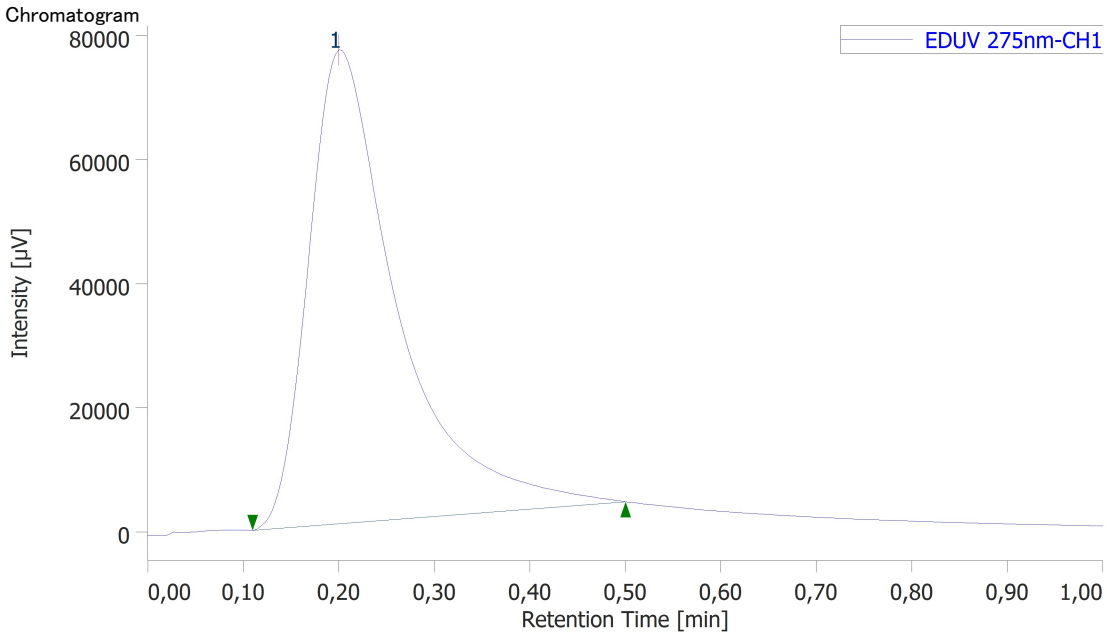


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	495068	76326	100,000	100,000	N/A	28	N/A	2,007	

Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 13:22:05
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 13:21:03
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	EDUV
Control Method	EDUV 276nm
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

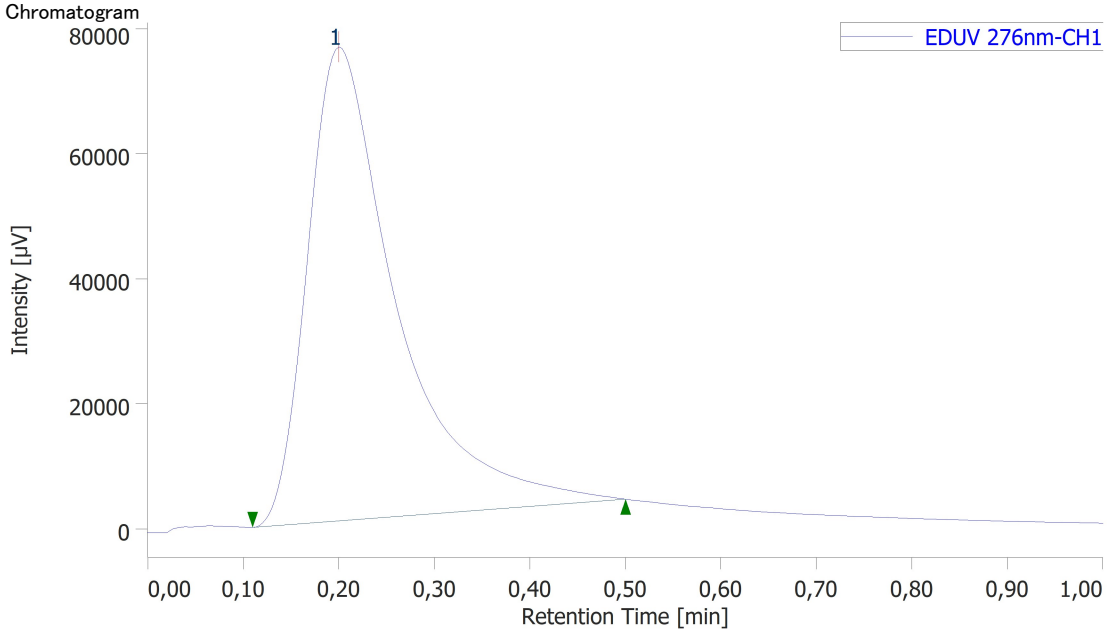

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,200	492109	75783	100,000	100,000	N/A	27	N/A	1,996	


Chromatogram Information	
User Name	Administrator
Date Modified	27/11/2023 14:26:48
Description	
HPLC System Name	HPLC
Injection Date	27/11/2023 14:06:47
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Ruído
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

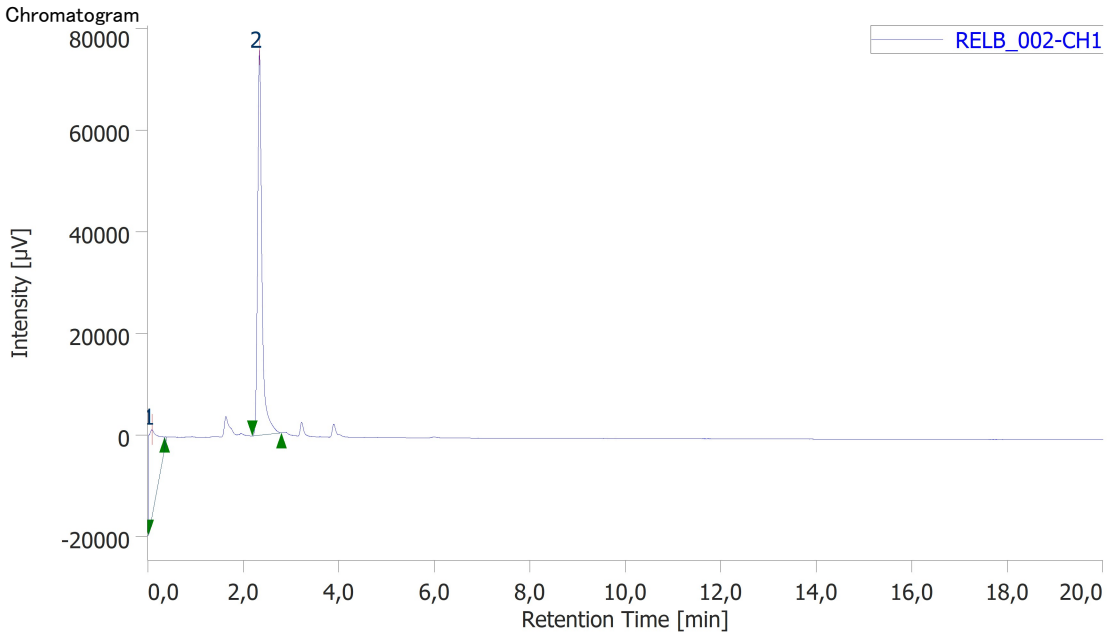

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,093	226206	17091	32,280	18,403	N/A	4	13,505	N/A	
2	Cafeína	1	2,340	474553	75780	67,720	81,597	N/A	3758	N/A	1,527	


Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:14:56
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:11:56
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

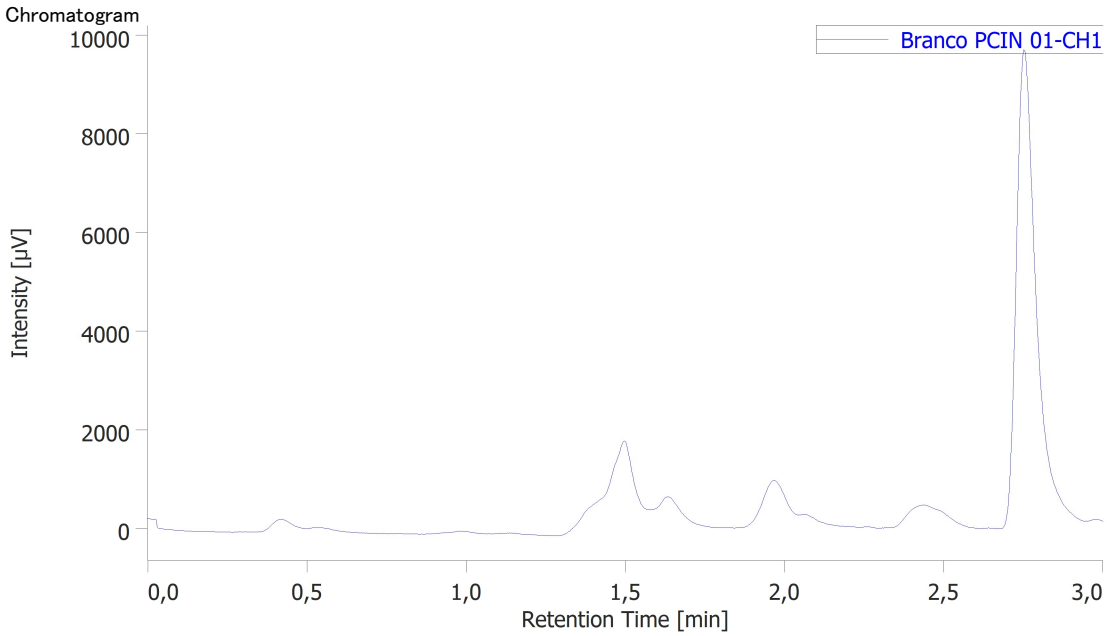

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:18:58
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:15:56
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

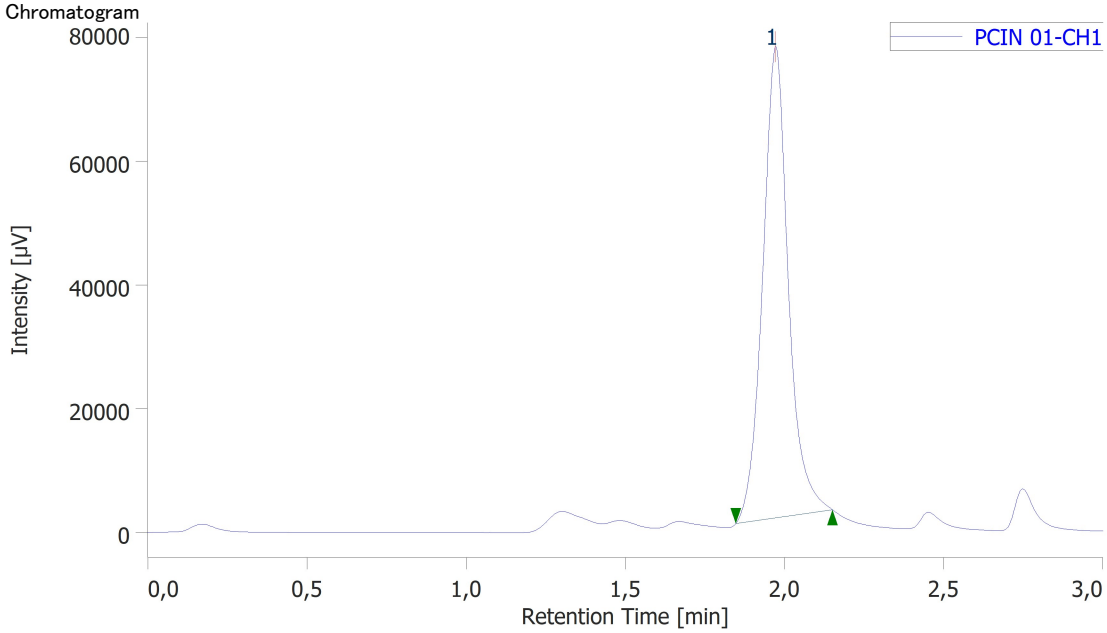


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	425531	76134	100,000	100,000	N/A	3254	N/A	1,119	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:22:42
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:19:40
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

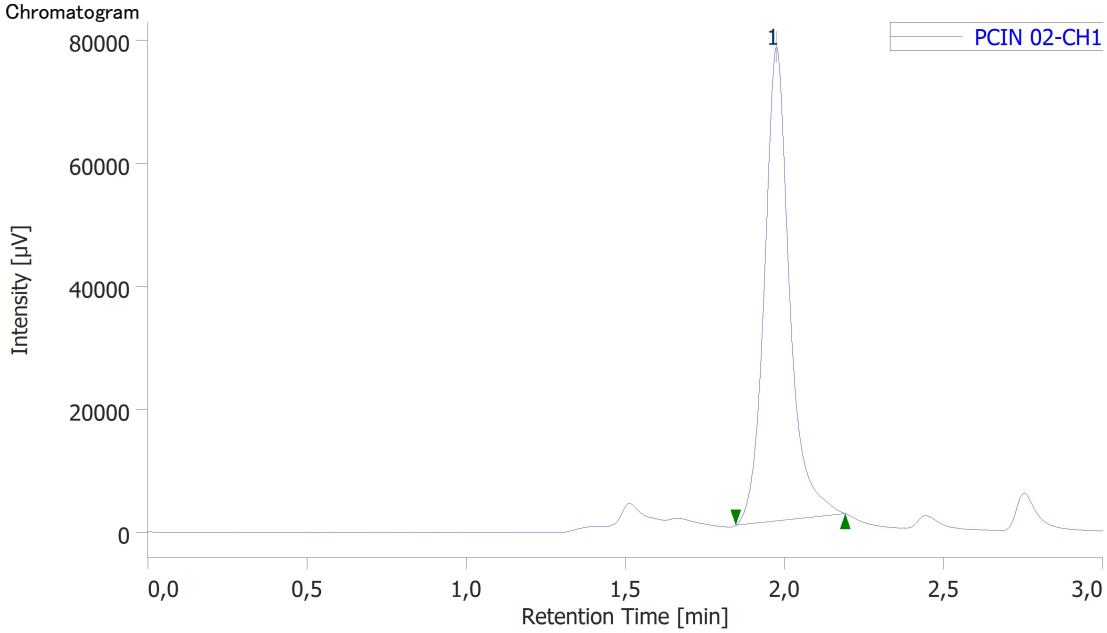


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,973	422611	77055	100,000	100,000	N/A	3569	N/A	1,210	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:31:10
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:28:09
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

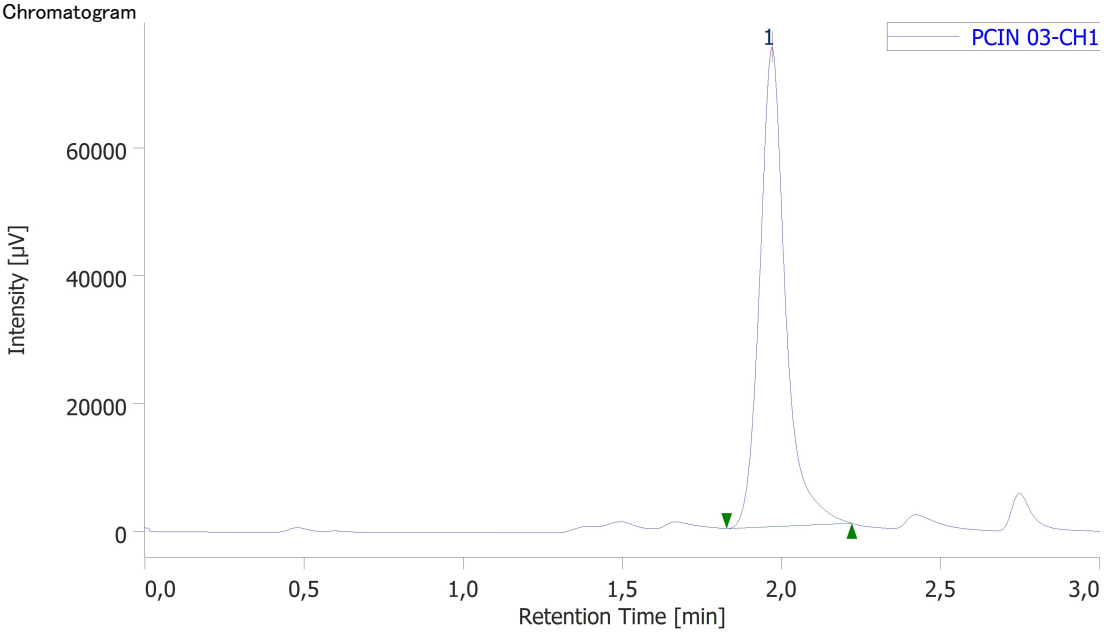


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	421784	74994	100,000	100,000	N/A	3395	N/A	1,264	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:34:54
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:31:53
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

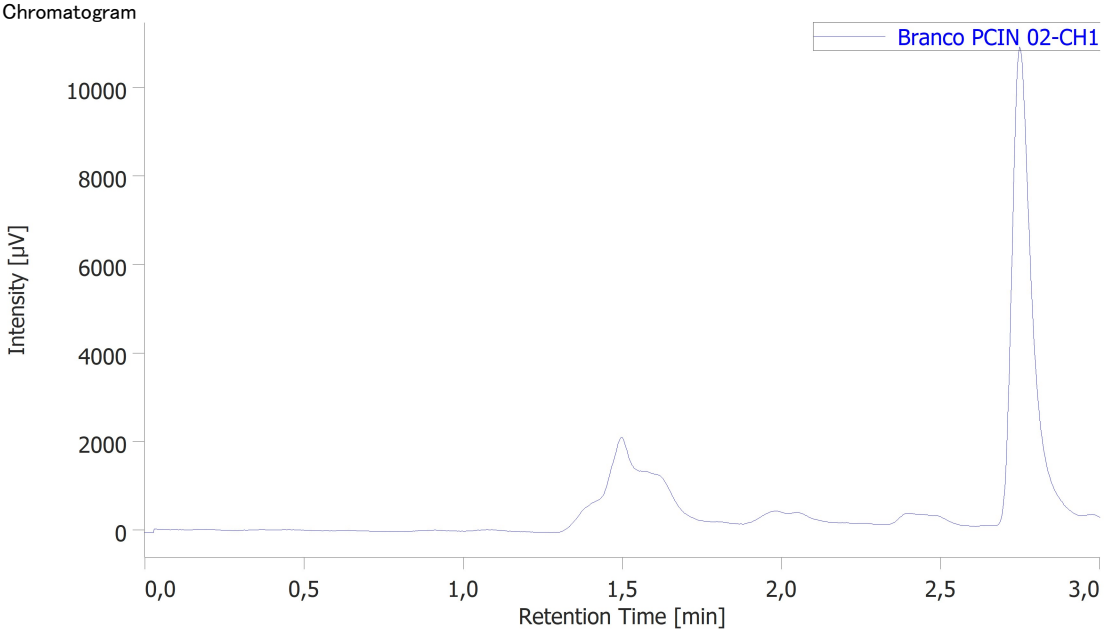

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:38:54
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:35:53
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

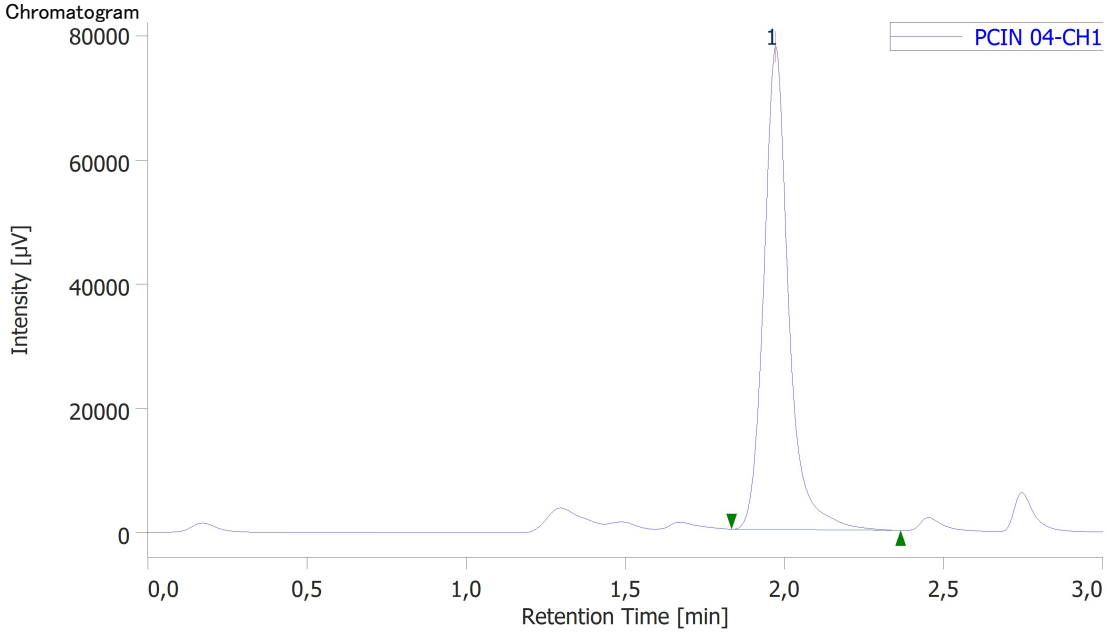


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	421082	77717	100,000	100,000	N/A	3662	N/A	1,244	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:42:32
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:39:31
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

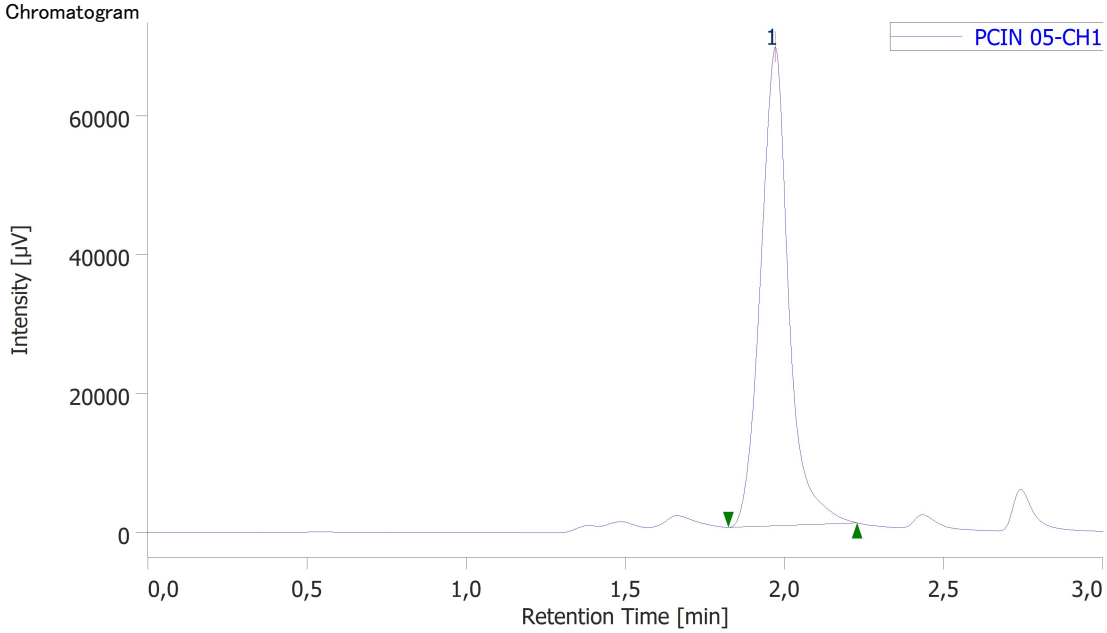


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	421820	68942	100,000	100,000	N/A	2762	N/A	1,150	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:46:04
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:43:02
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

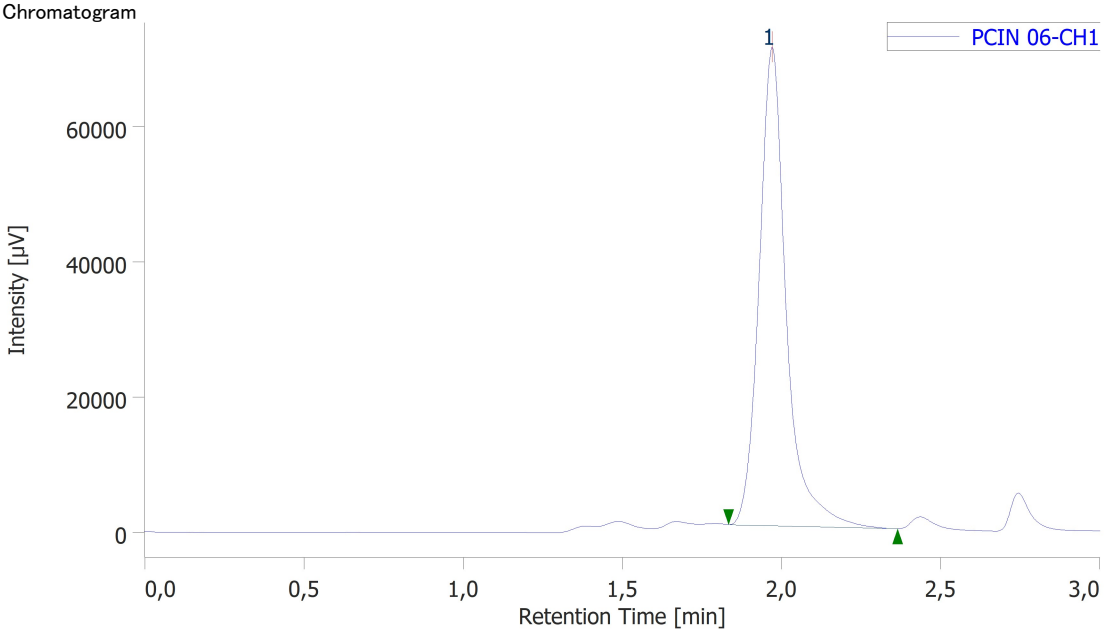


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	418034	70844	100,000	100,000	N/A	3147	N/A	1,284	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 09:49:22
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 09:46:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

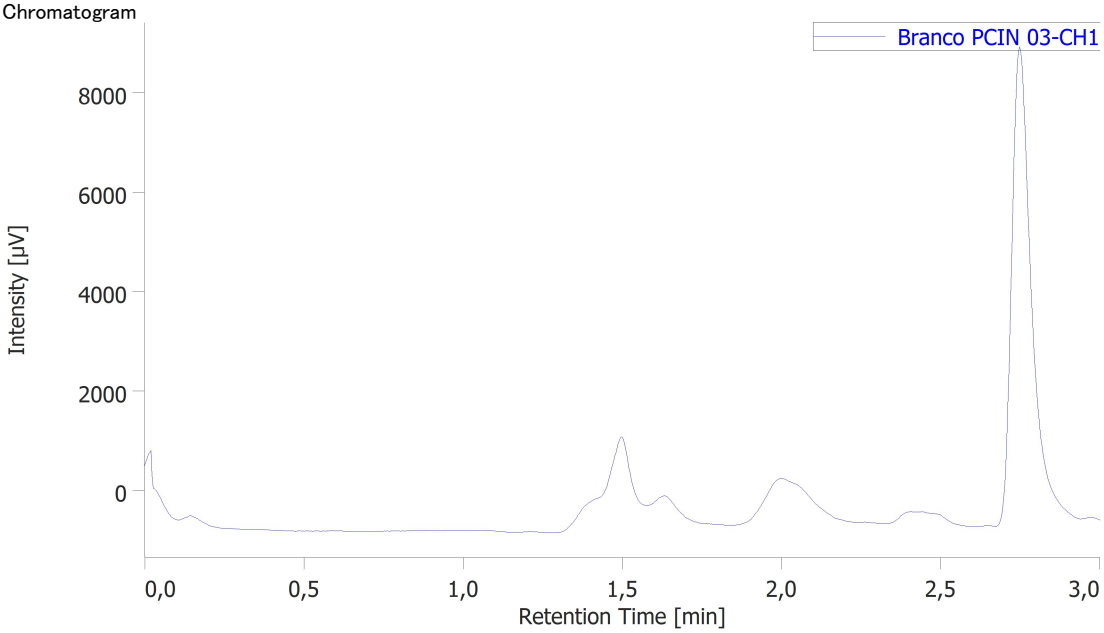

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 10:03:54
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 10:00:52
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	


Chromatogram

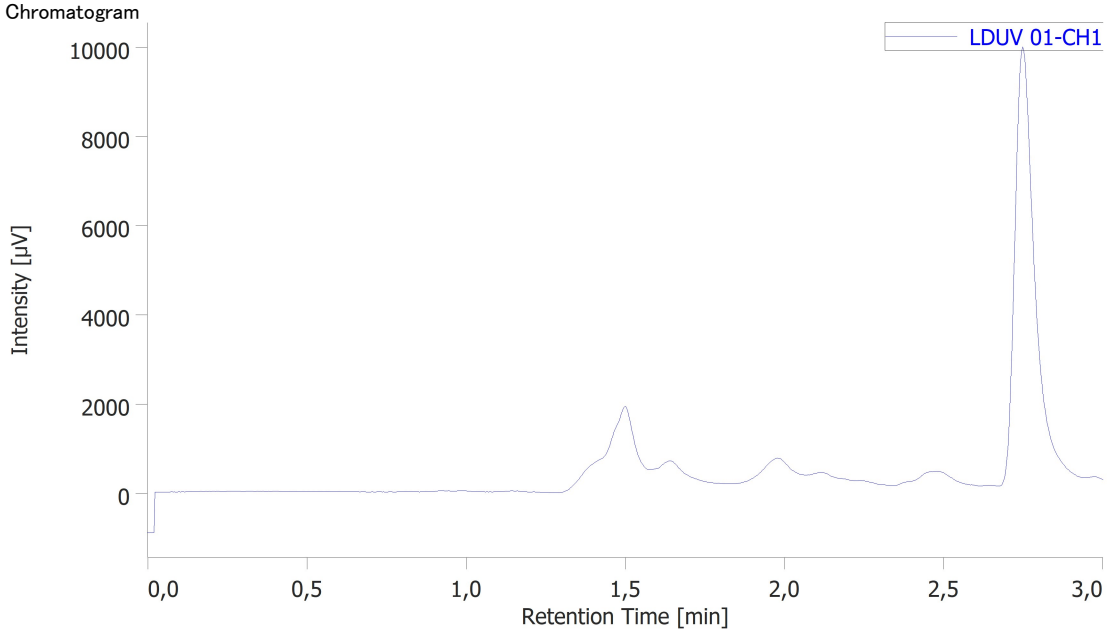

Peak Information – No data.

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 10:07:18
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 10:04:16
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

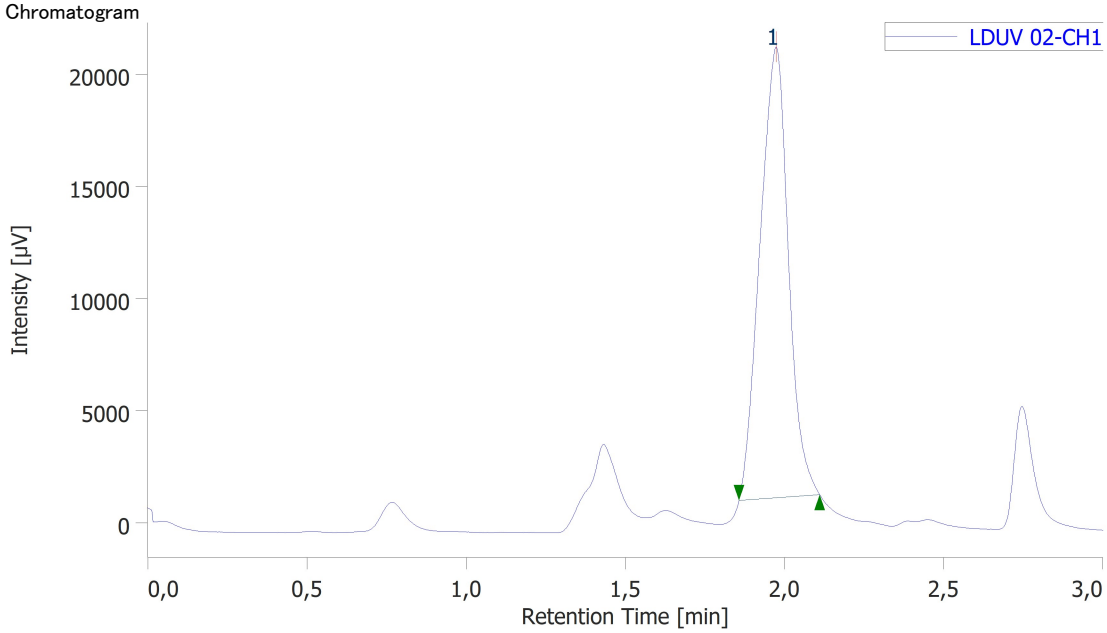


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,973	124324	20091	100,000	100,000	N/A	2295	N/A	0,998	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 10:11:06
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 10:08:05
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

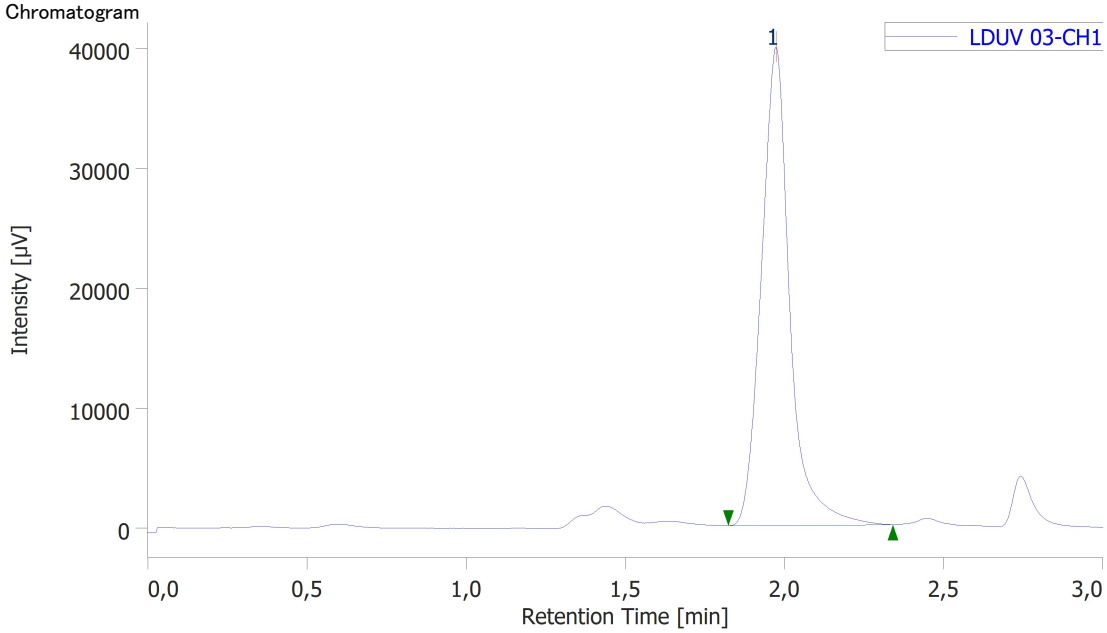


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,973	246411	39880	100,000	100,000	N/A	2764	N/A	1,183	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 10:14:52
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 10:11:50
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

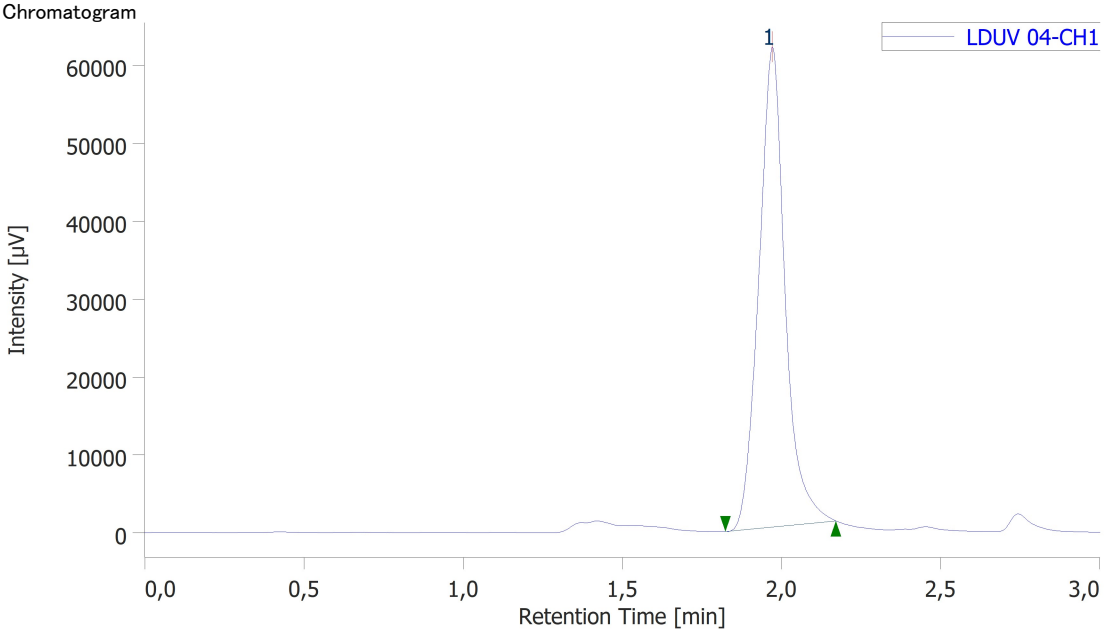


Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,970	351900	61589	100,000	100,000	N/A	3106	N/A	1,135	

Chromatogram Information	
User Name	Administrator
Date Modified	30/11/2023 10:18:52
Description	
HPLC System Name	HPLC
Injection Date	30/11/2023 10:15:50
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	PCIN
Peak ID Table	Cafeína
Calibration Method	
Additional Information	
Column Info	

Chromatogram

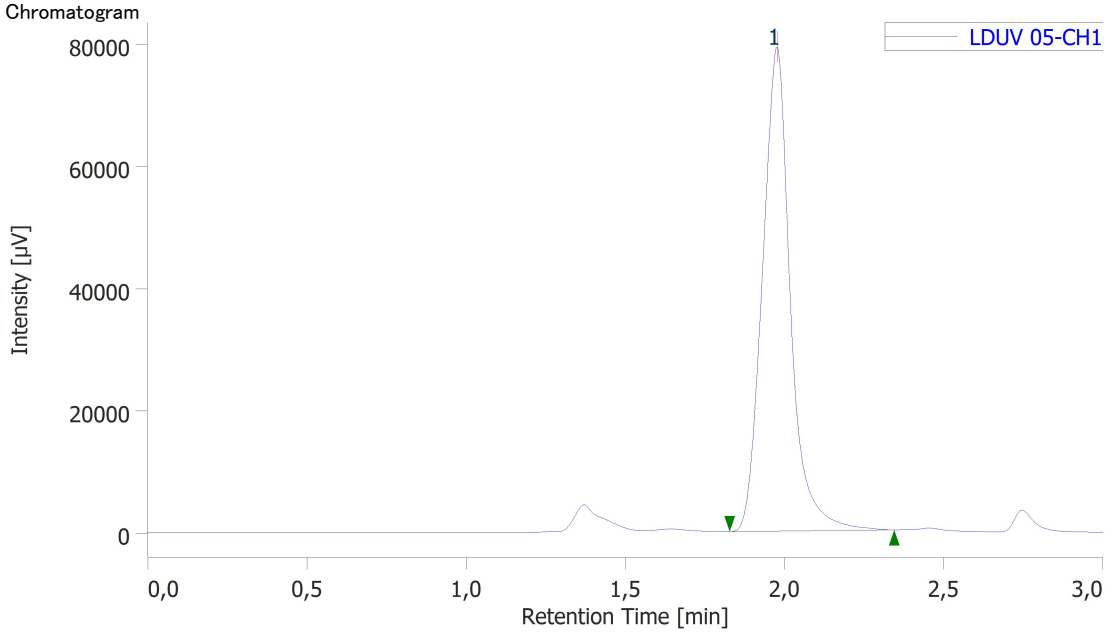

Peak Information

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,977	481513	79266	100,000	100,000	N/A	2771	N/A	1,131	