
Peak Find - Comprimento de Onda.jws

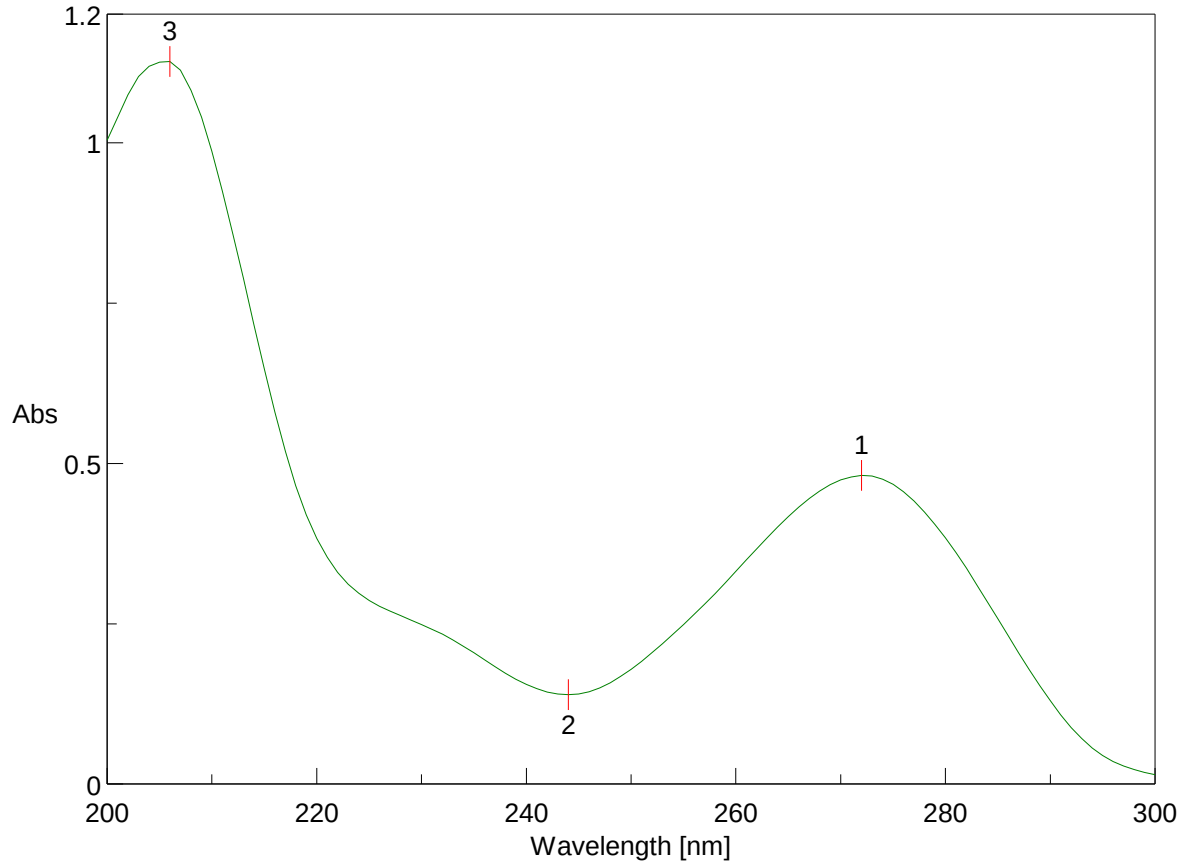

[Comments]

User	Administrator
Division	---
Company	Verde Laboratorios
Creation date	4/2/2018 13:33

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	400 nm
Data interval	1 nm
Data points	201


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.48091	2	244	0.138991
3	206	1.1263			

Chromatogram

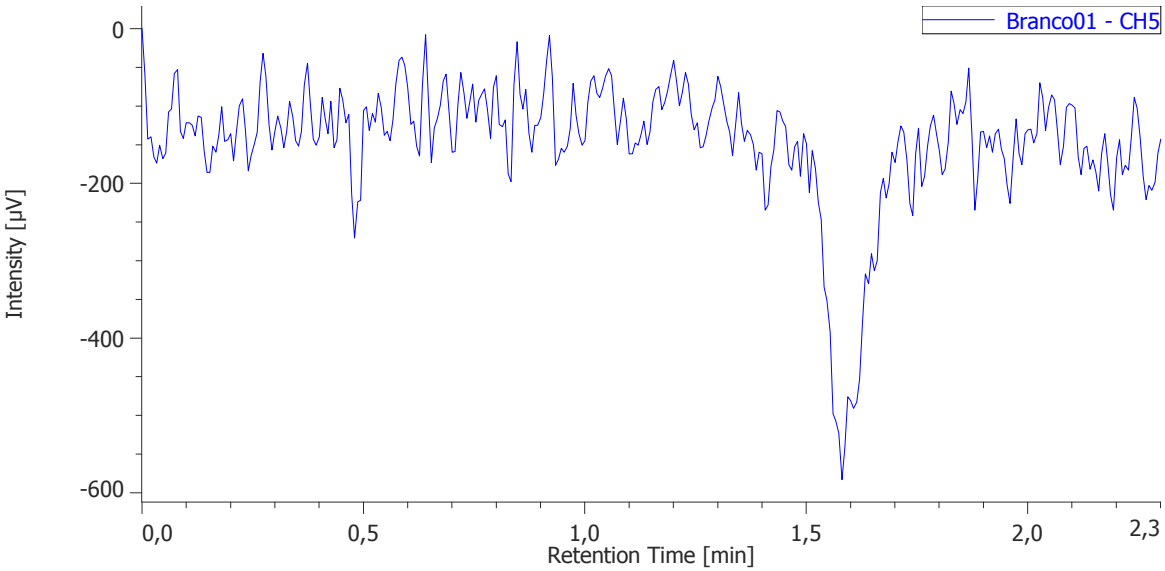


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 12:57:31
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 12:55:10
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Chromatogram

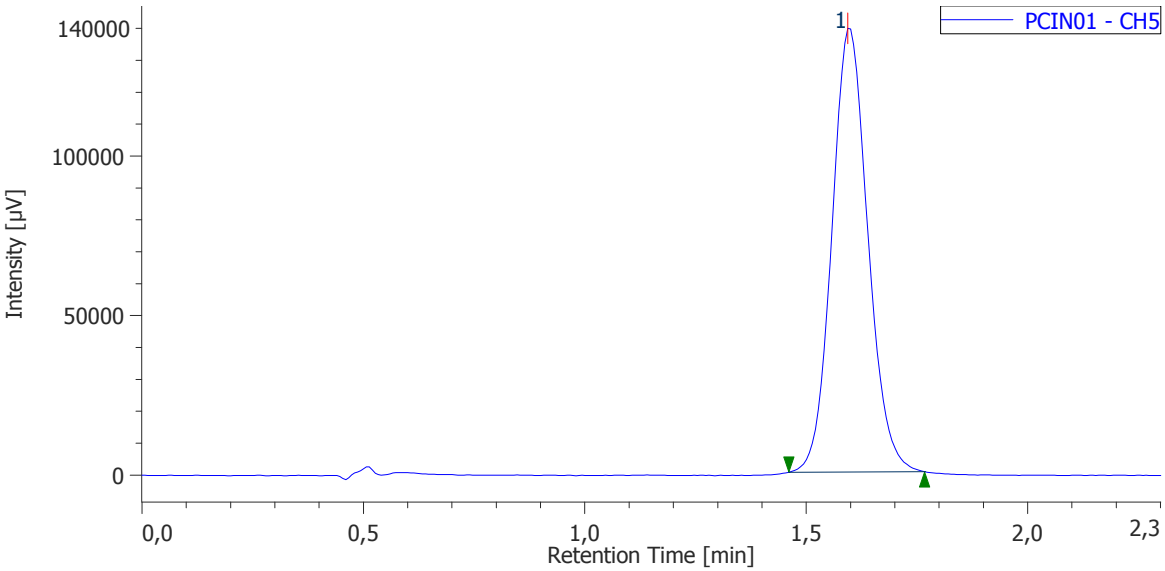


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:47:26
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 12:57:50
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,593	785345	138921	100,000	100,000	N/A	1882	N/A	1,138	

Chromatogram

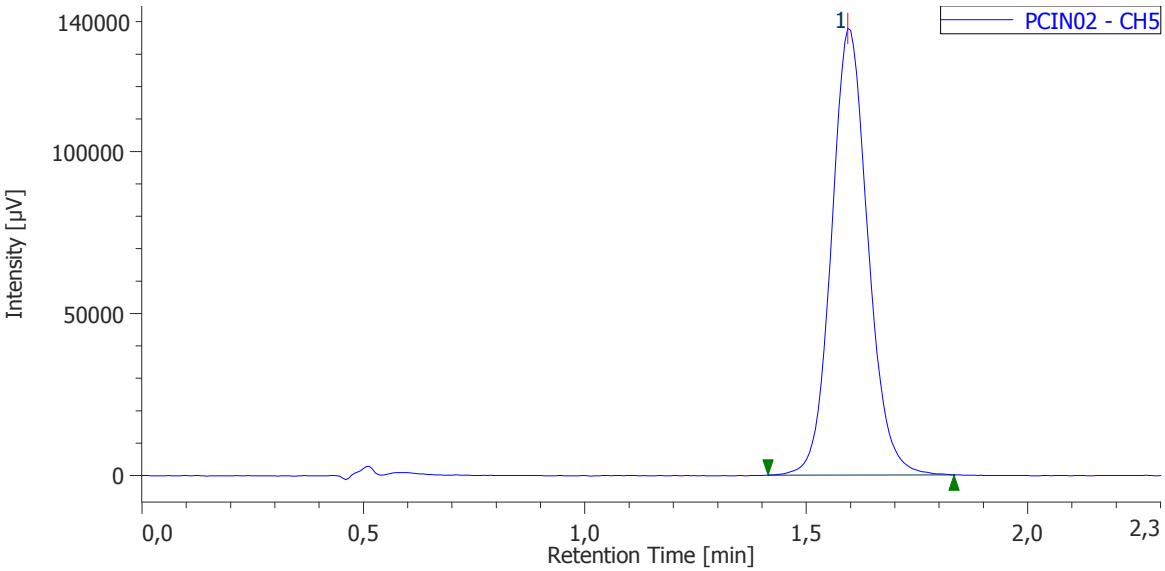


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:28:16
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:00:30
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,593	788003	137669	100,000	100,000	N/A	1881	N/A	1,137	

Chromatogram

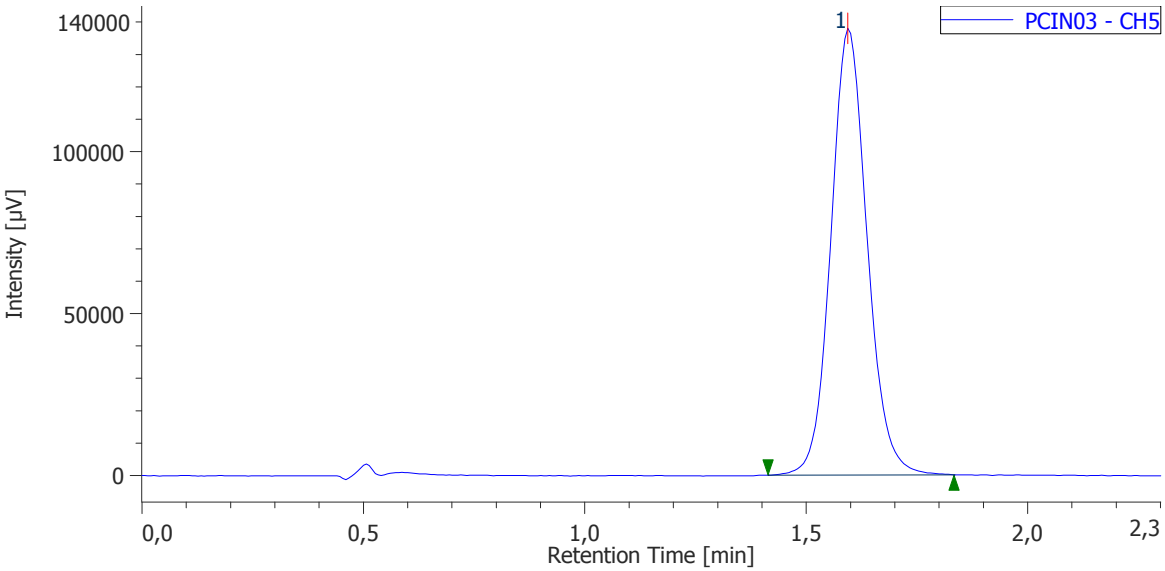


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:28:17
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:03:10
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,593	784234	137805	100,000	100,000	N/A	1901	N/A	1,111	

Chromatogram

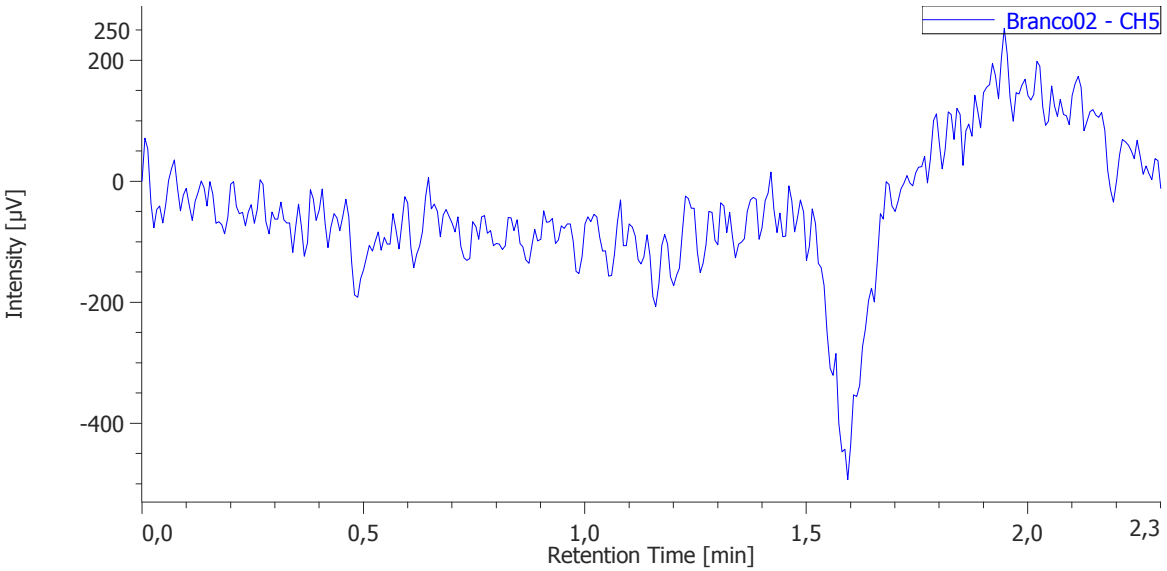


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:08:11
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:05:50
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Chromatogram

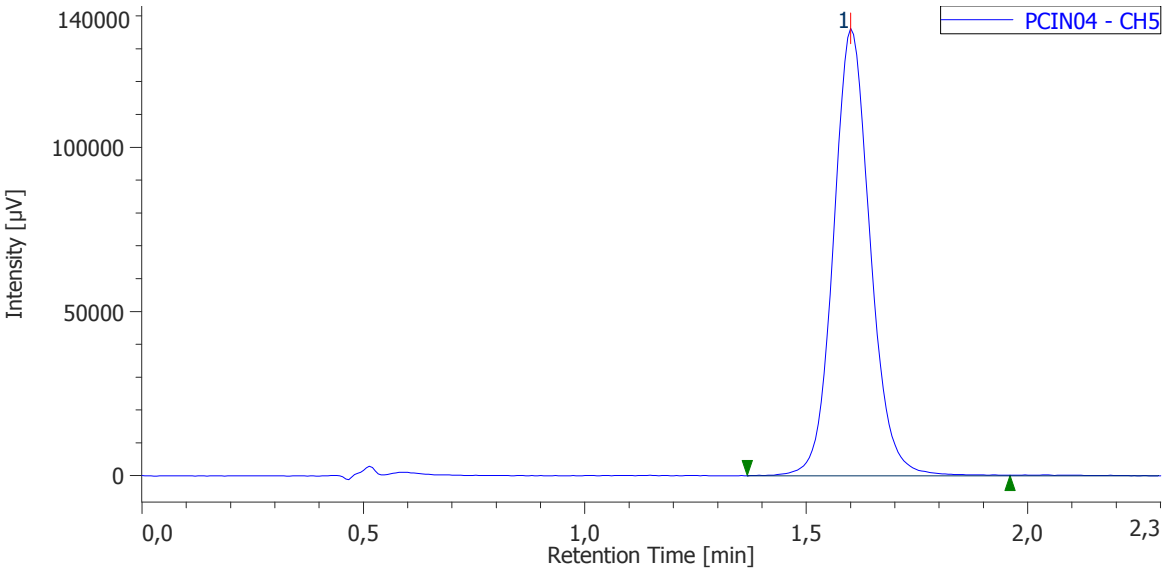


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:41:55
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:08:30
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	785140	136161	100,000	100,000	N/A	1900	N/A	1,105	

Chromatogram

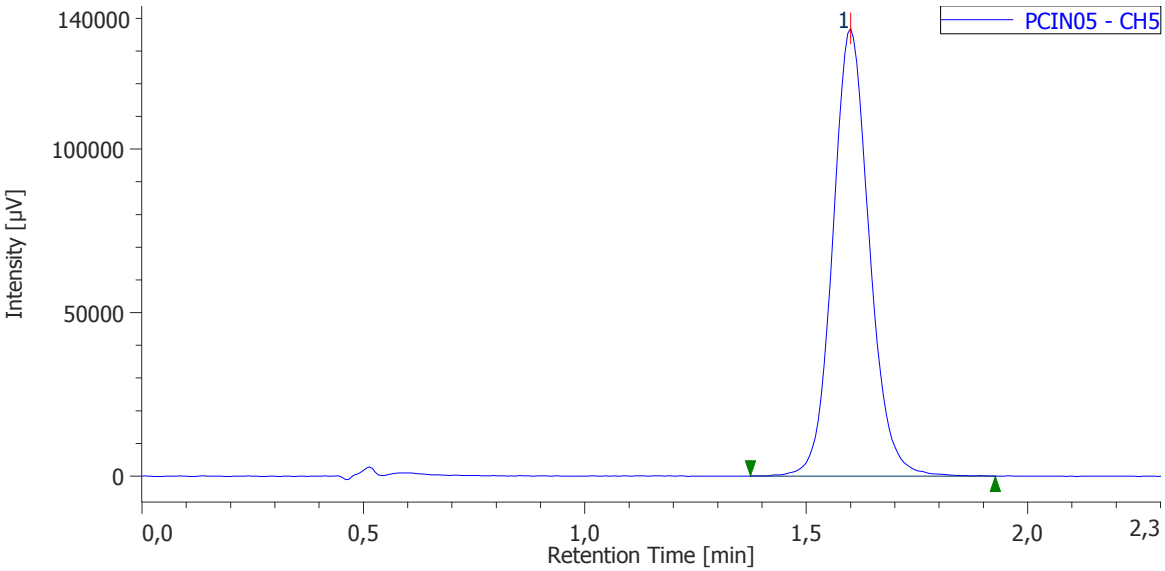


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:43:54
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:11:10
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	785450	136817	100,000	100,000	N/A	1903	N/A	1,085	

Chromatogram

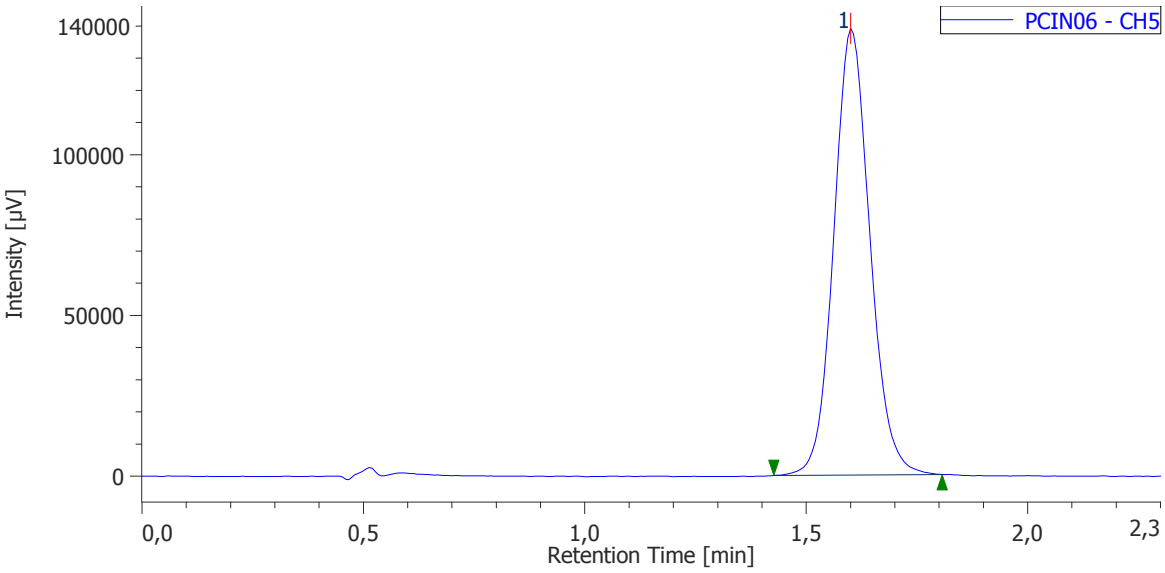


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:45:06
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:13:50
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	787179	138753	100,000	100,000	N/A	1913	N/A	1,108	

Chromatogram

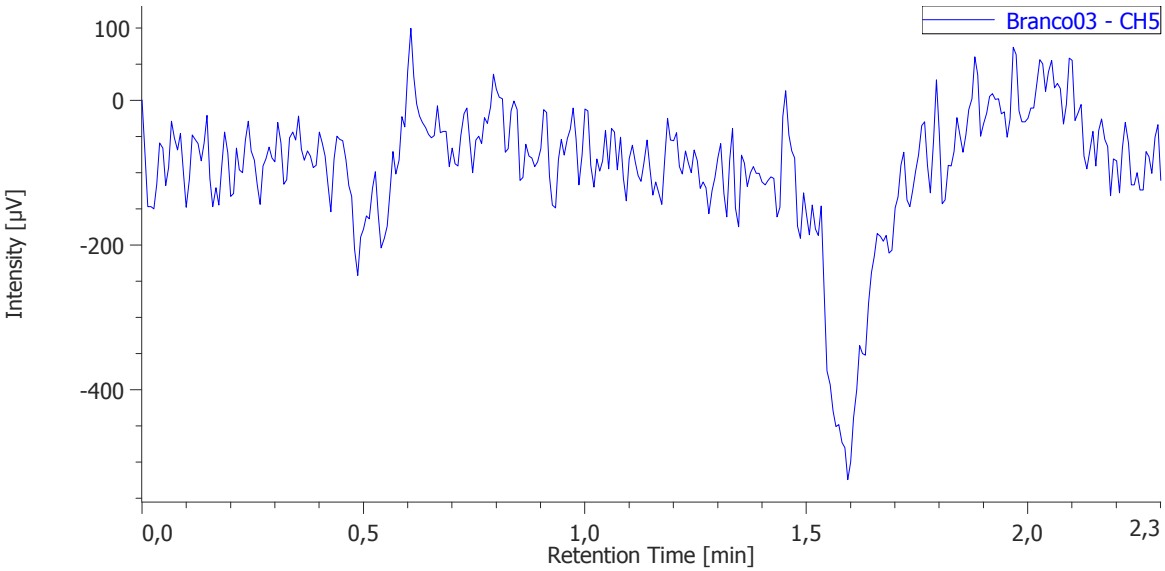


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:18:51
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:16:30
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Chromatogram

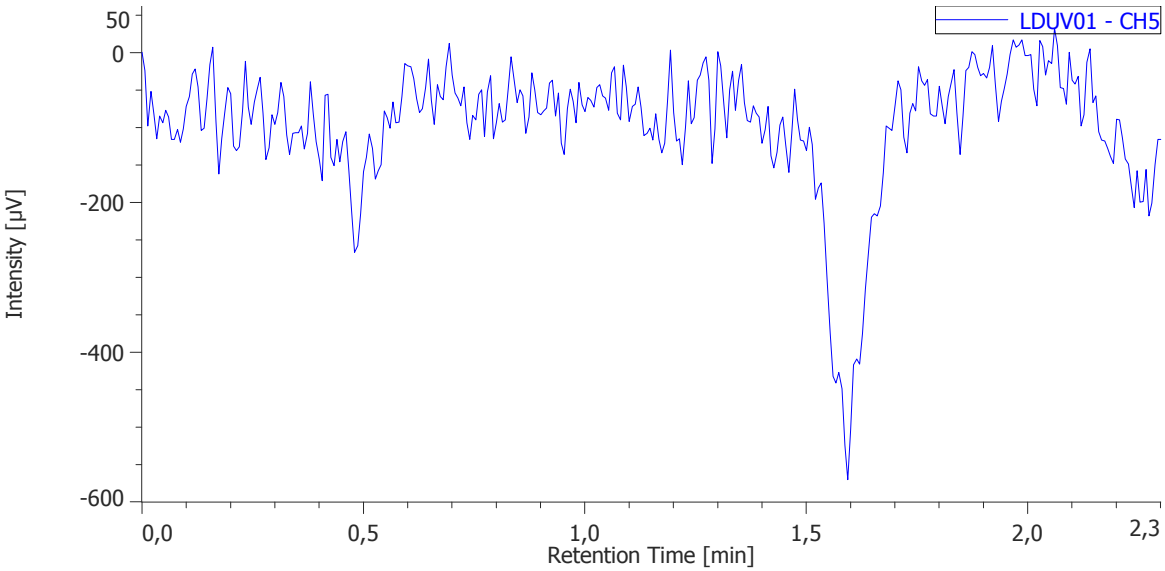


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:49:32
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:19:10
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

Chromatogram

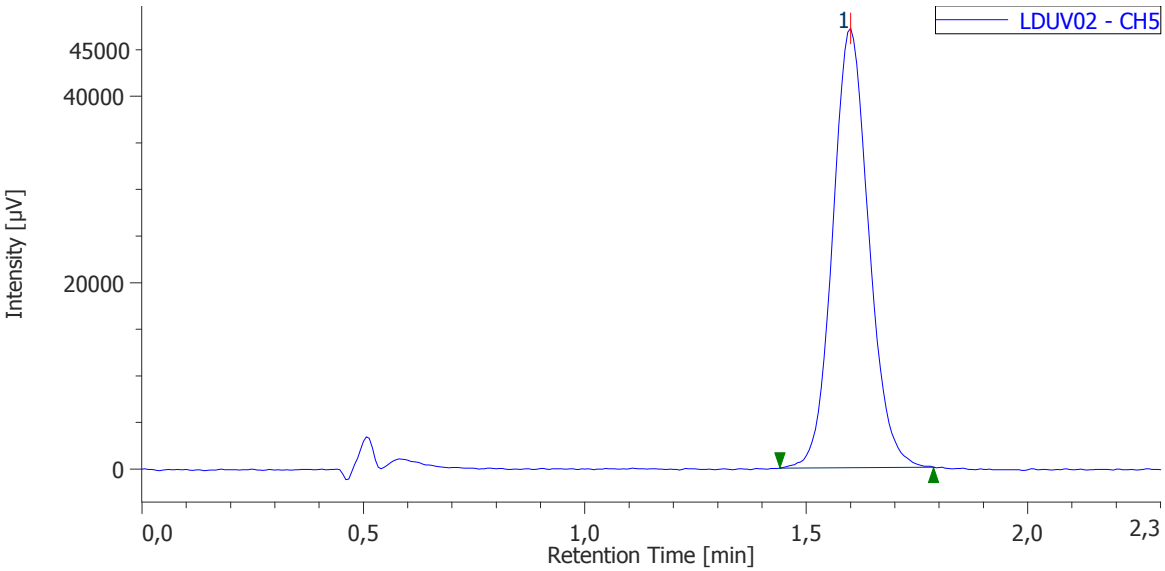


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:49:32
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:21:50
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	267008	47104	100,000	100,000	N/A	1907	N/A	1,076	

Chromatogram

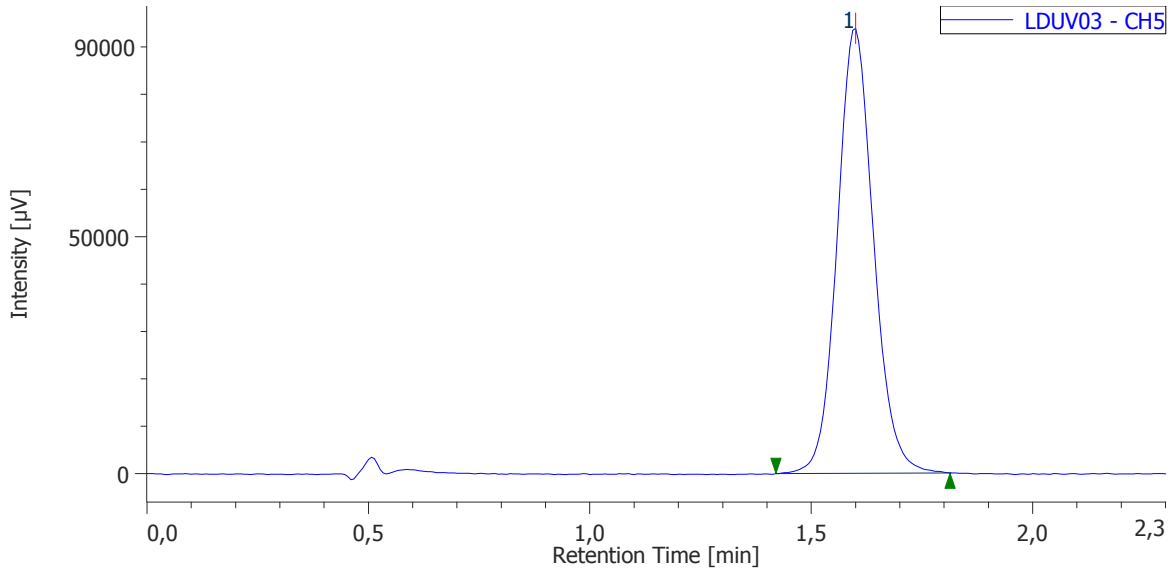


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:49:32
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:24:30
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	534539	93787	100,000	100,000	N/A	1907	N/A	1,070	

Chromatogram

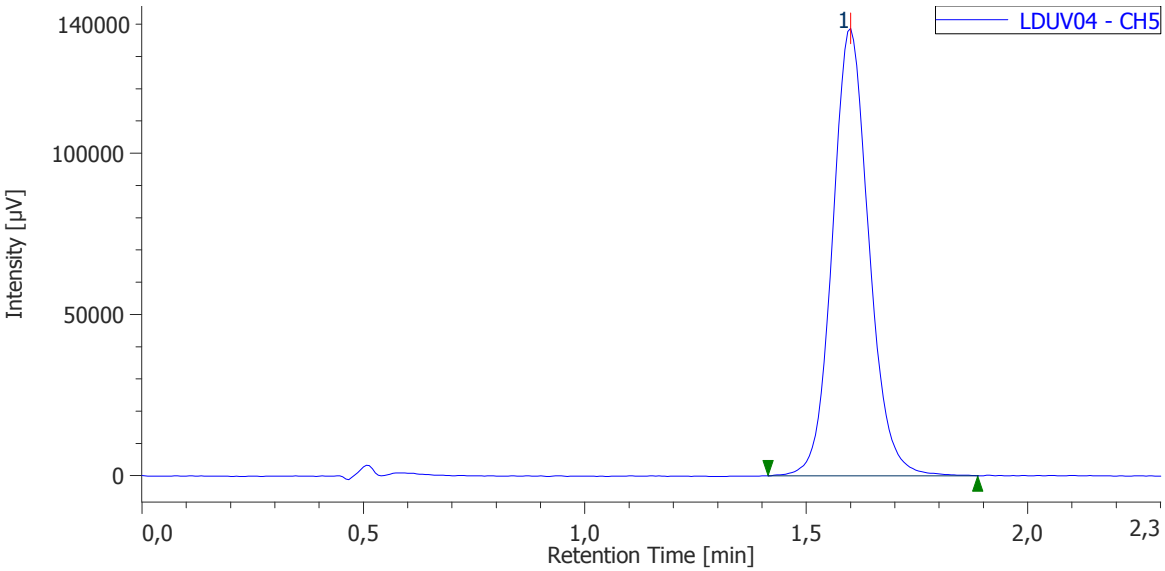


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:49:33
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:27:10
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	793186	138652	100,000	100,000	N/A	1906	N/A	1,080	

Chromatogram

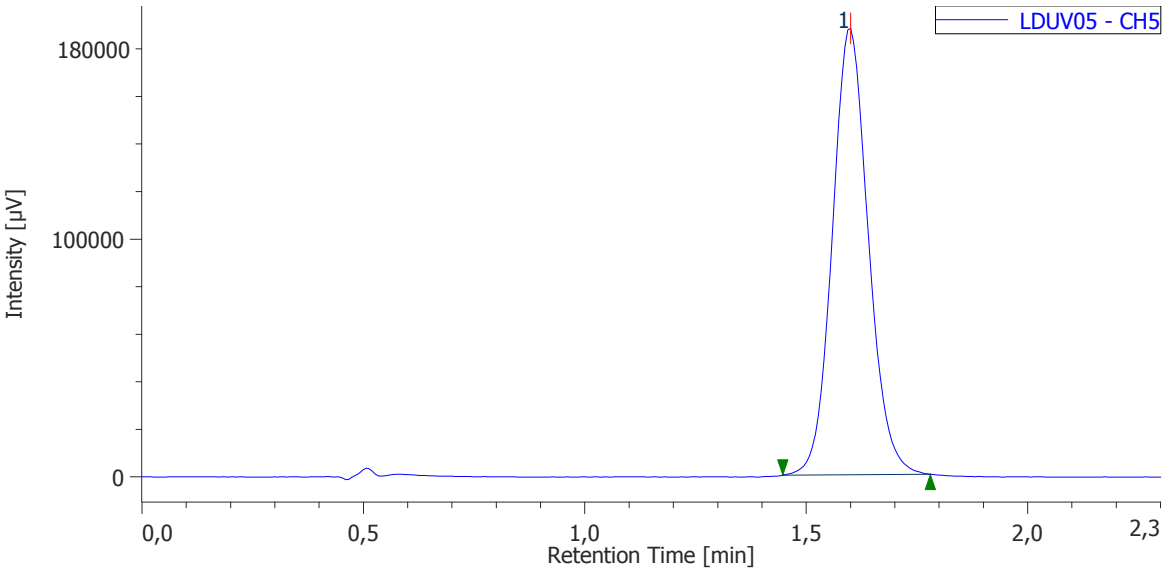


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:54:39
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:29:52
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	1061228	187594	100,000	100,000	N/A	1910	N/A	1,068	

Chromatogram

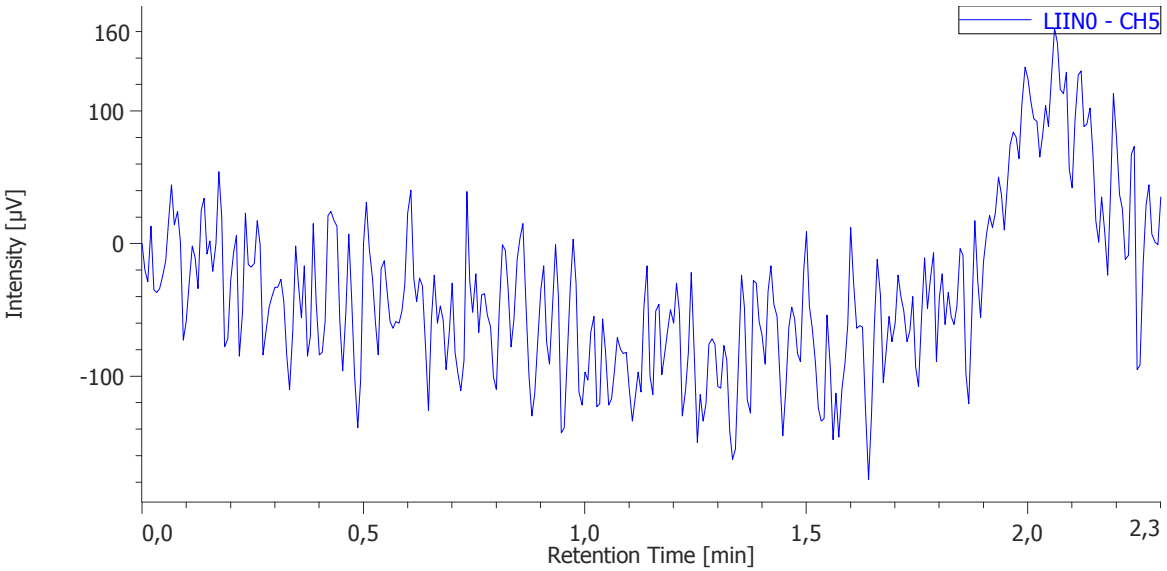


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:55:25
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:32:25
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN0-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

Chromatogram

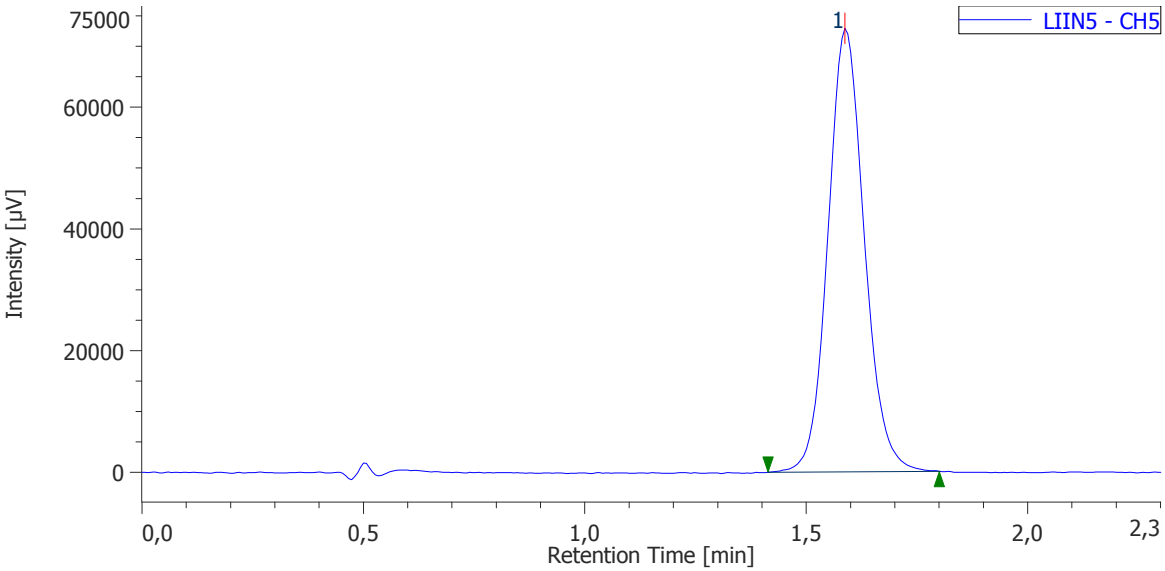


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:55:25
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:35:02
Volume	5,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,587	415520	72862	100,000	100,000	N/A	1866	N/A	1,120	

Chromatogram

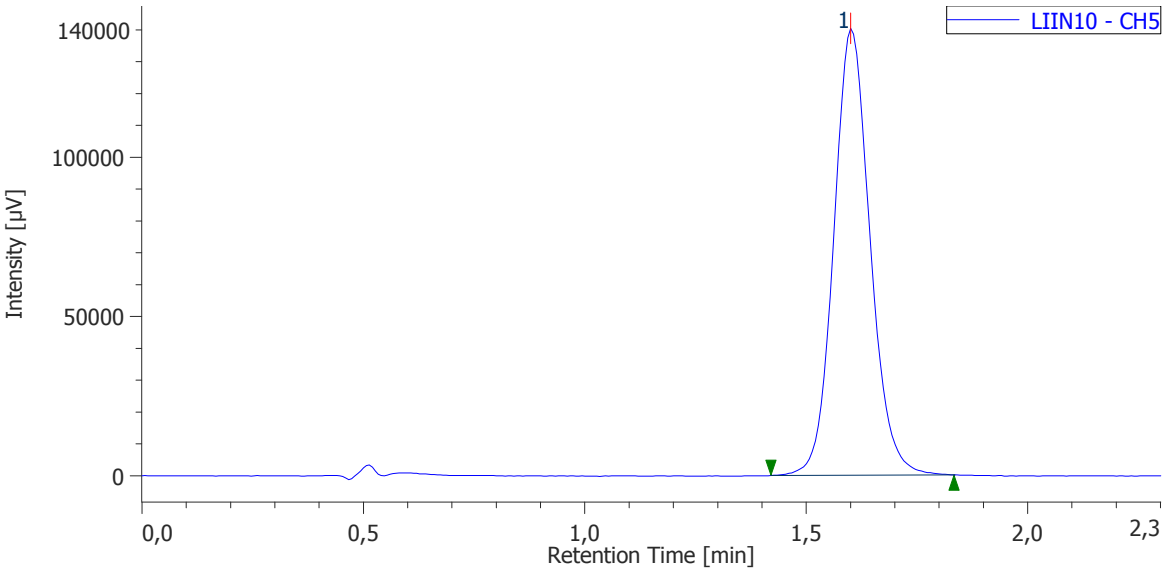


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:55:25
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:37:42
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN10-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	798302	140136	100,000	100,000	N/A	1909	N/A	1,116	

Chromatogram

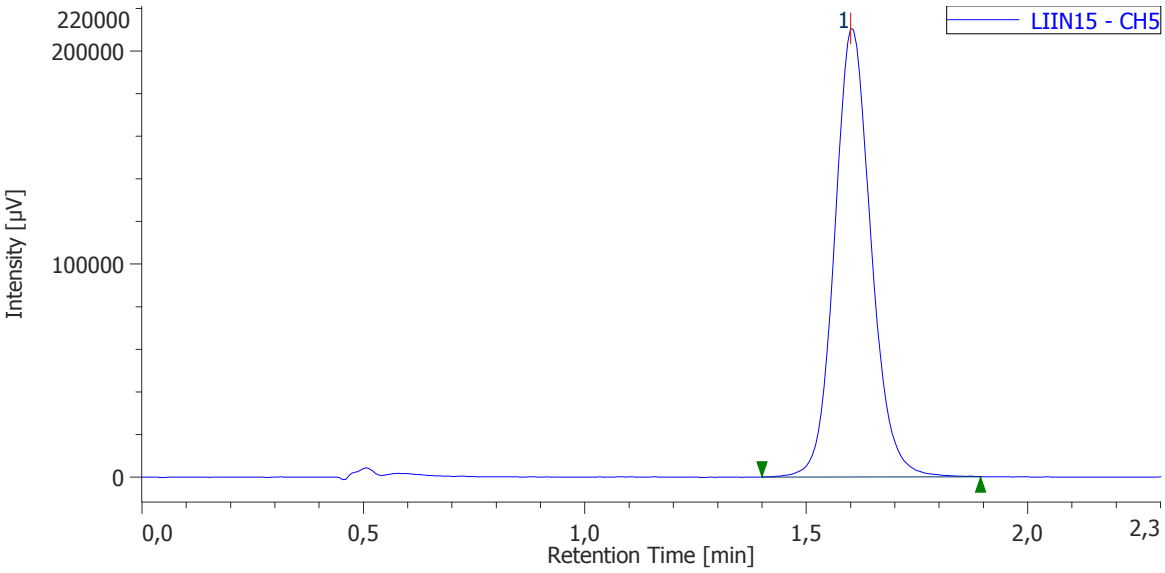


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:55:26
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:40:27
Volume	15,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN15-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	1206066	210360	100,000	100,000	N/A	1906	N/A	1,147	

Chromatogram

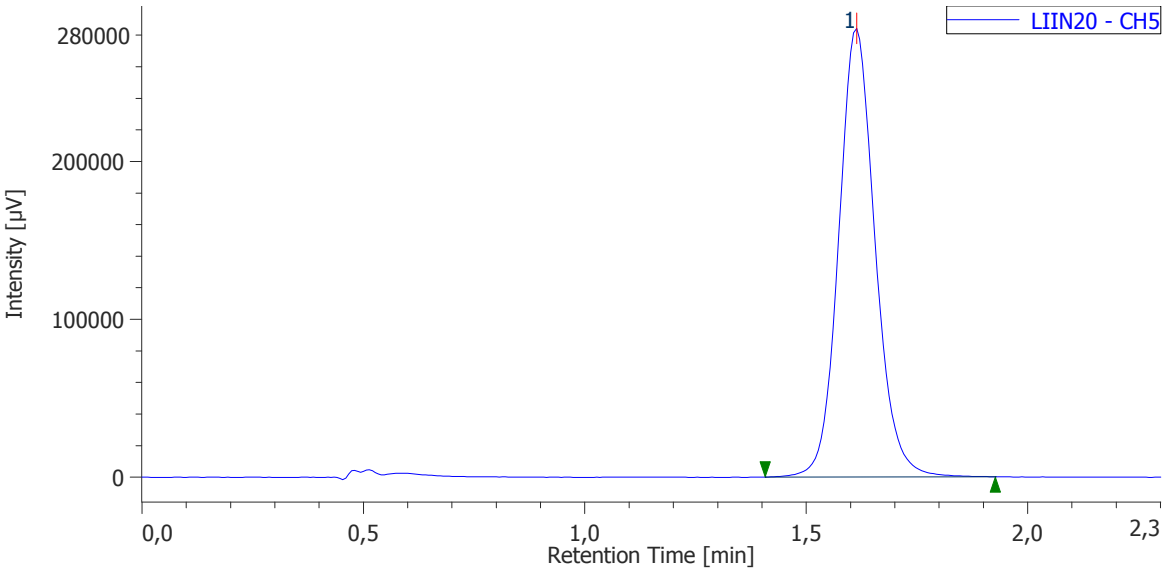


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 13:55:26
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 13:43:17
Volume	20,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,3 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 2018
Peak ID Table	ID
Calibration Method	CAL LDUV
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN20-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	1623271	283894	100,000	100,000	N/A	1950	N/A	1,094	

Chromatogram

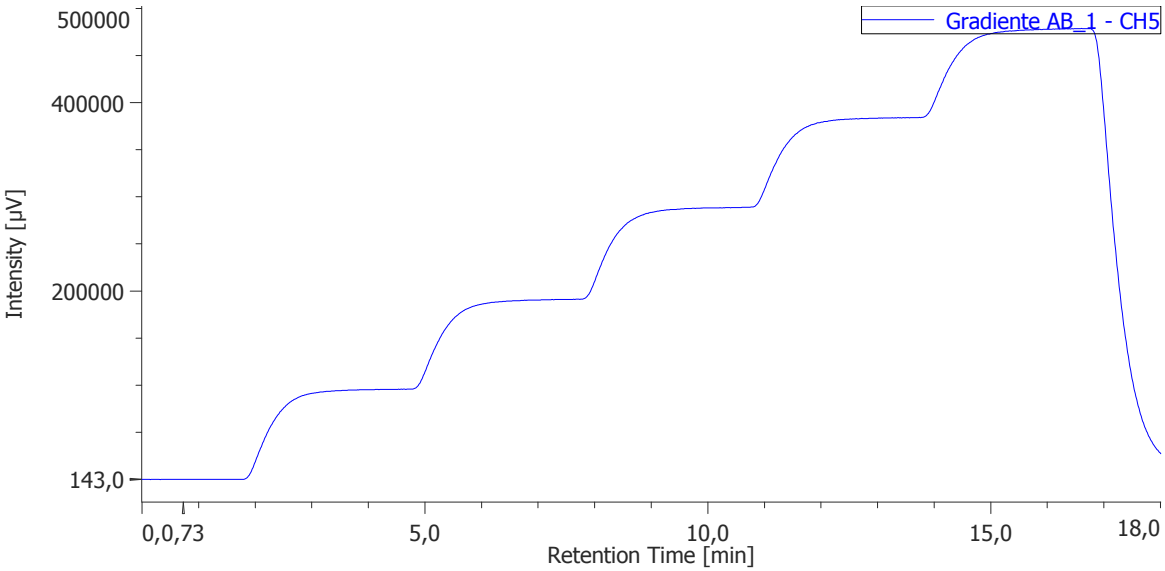


Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 14:34:58
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 14:16:56
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	

Chromatogram

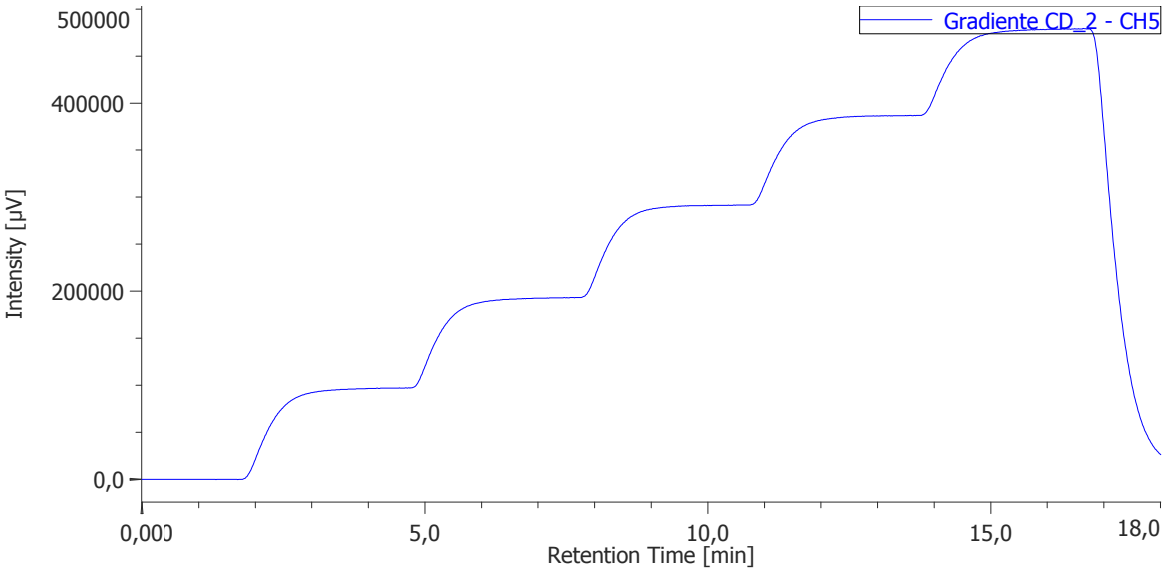

Chromatogram Information	
User Name	Administrator
Date Modified	4/2/2018 15:02:40
Description	
HPLC System Name	HPL 08
Injection Date	4/2/2018 14:44:38
Volume	0,00 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	