
Peak Find - EDUV_002 UV_tR0,55 D

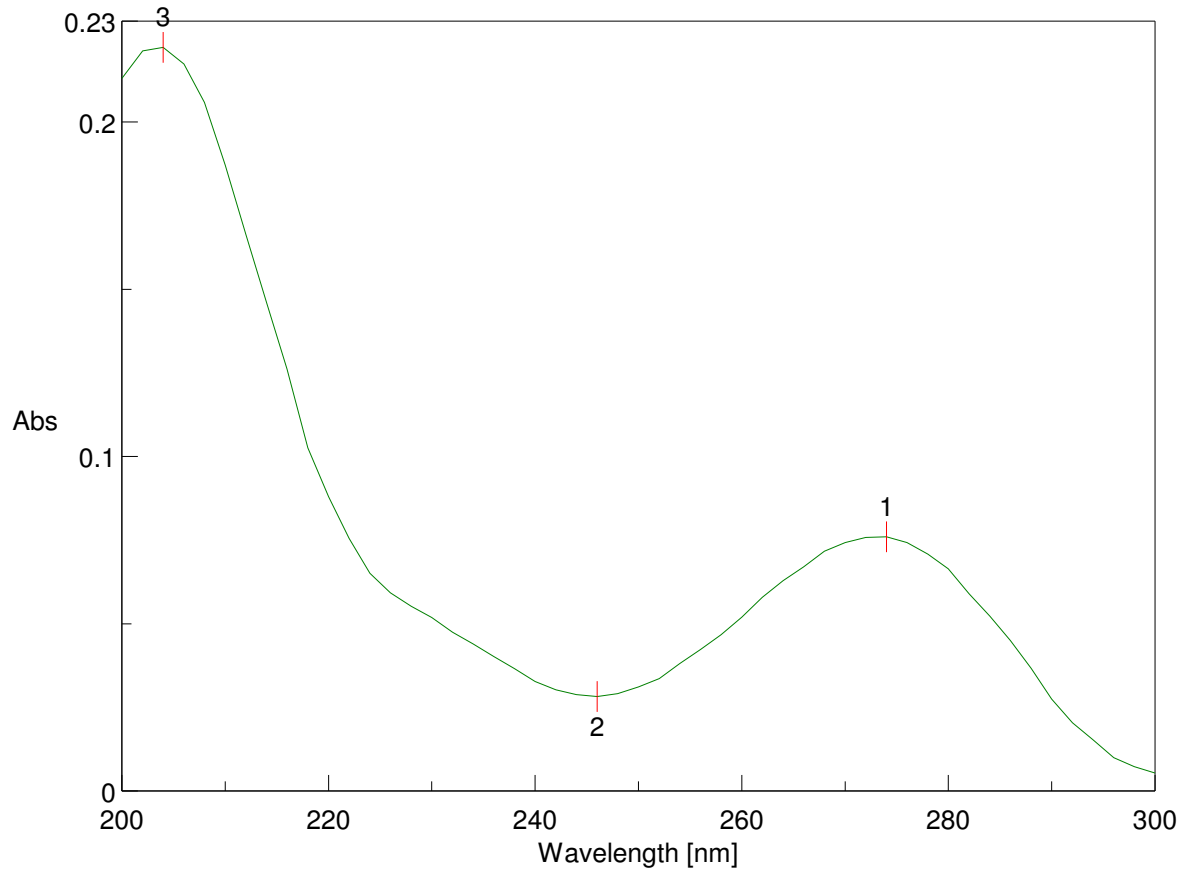

[Comments]

User	Administrator
Division	---
Company	JP
Creation date	22/04/2021 12:56

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	B113160866
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0759144	2	246	0.0281824
3	204	0.222172			

Chromatogram

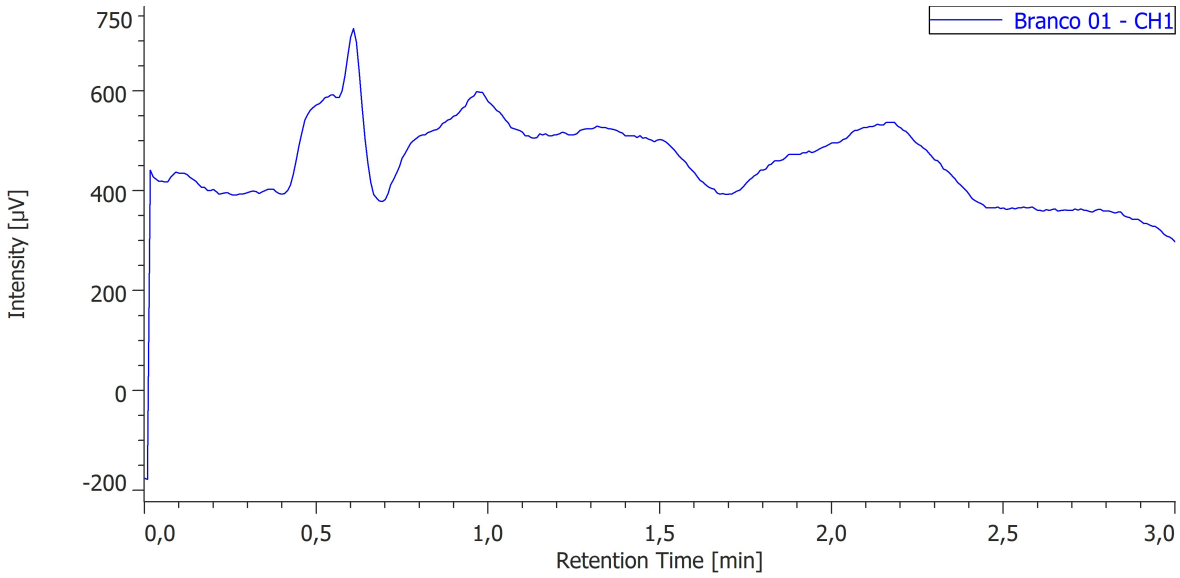


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:37:13
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:13:14
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

Chromatogram

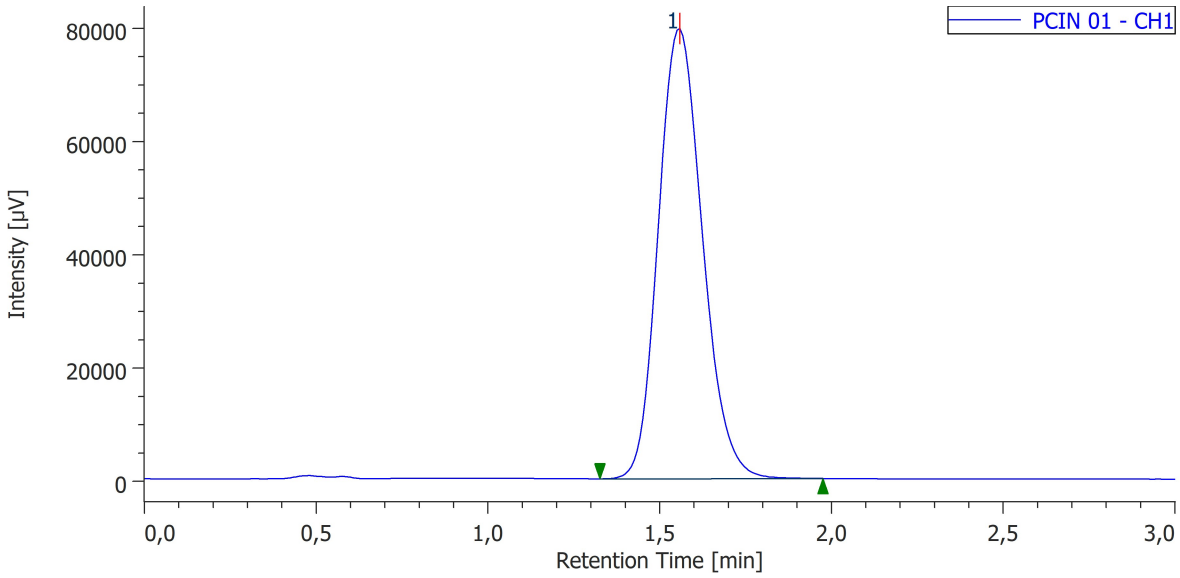


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:28:15
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:23:07
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,558	710016	79433	100,000	100,000	N/A	702	N/A	1,137	

Chromatogram

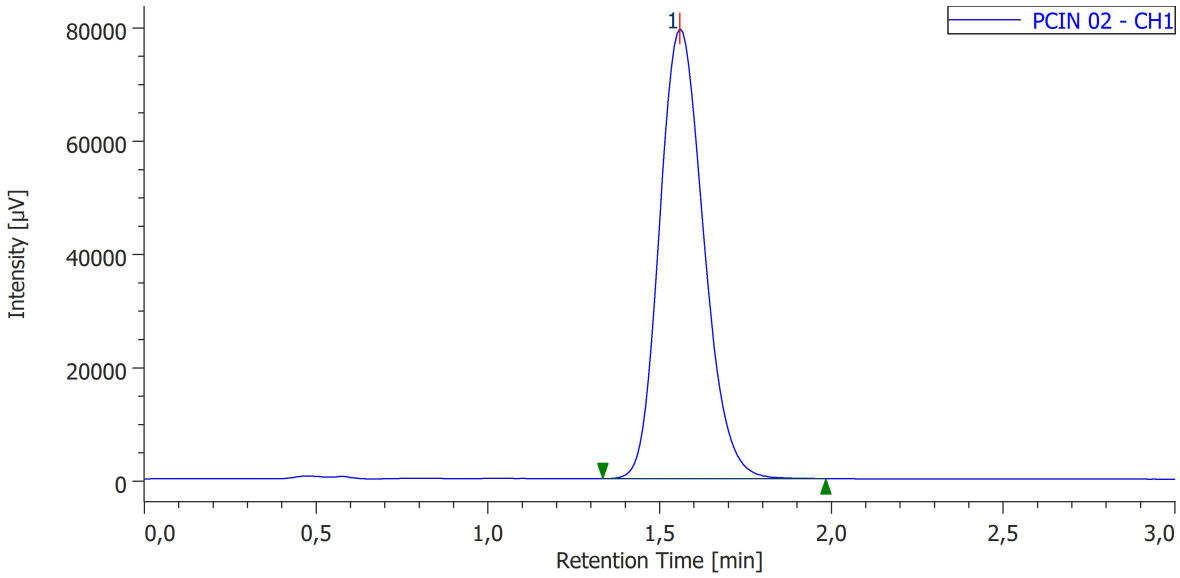


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:30:46
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:26:29
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,558	709874	79416	100,000	100,000	N/A	699	N/A	1,173	

Chromatogram

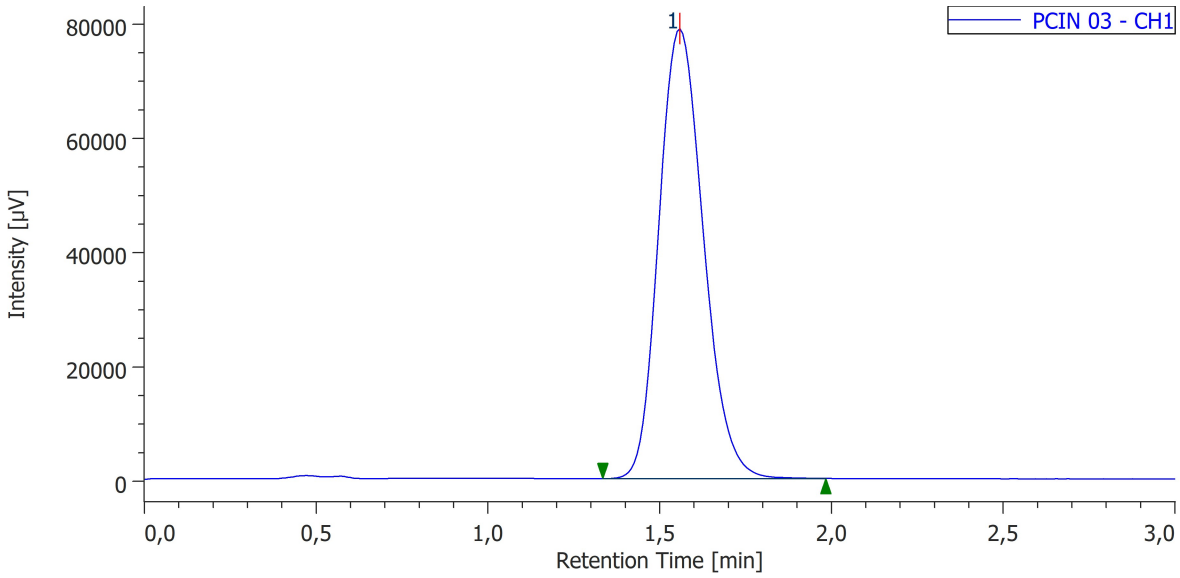


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:33:15
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:29:52
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,558	710025	78725	100,000	100,000	N/A	685	N/A	1,166	

Chromatogram

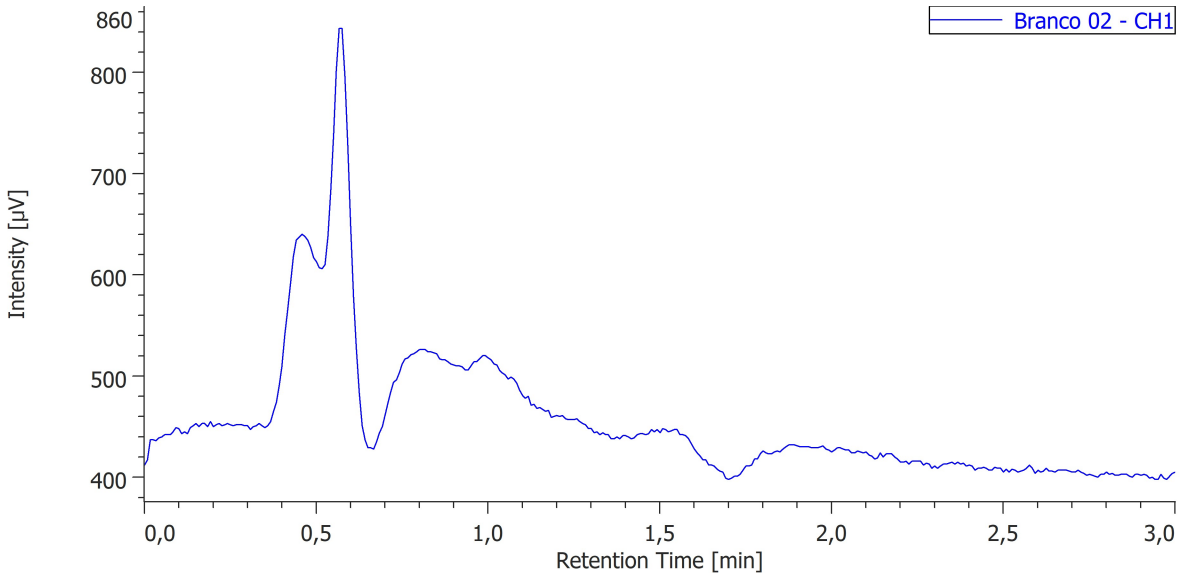


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:37:08
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:33:12
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

Chromatogram

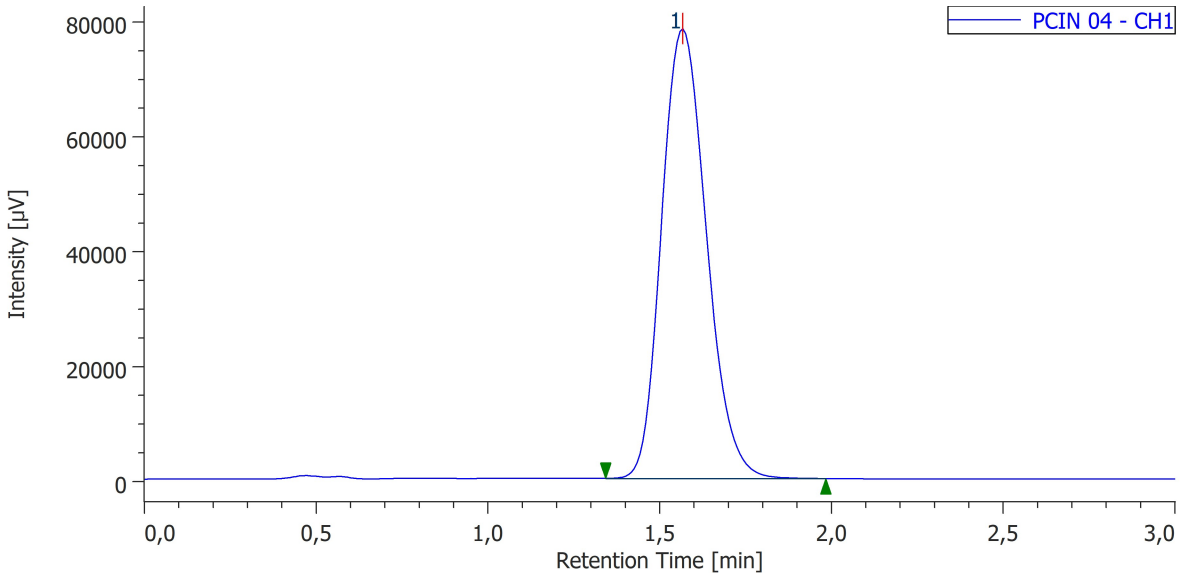


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:39:58
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:36:34
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,567	711022	78291	100,000	100,000	N/A	679	N/A	1,169	

Chromatogram

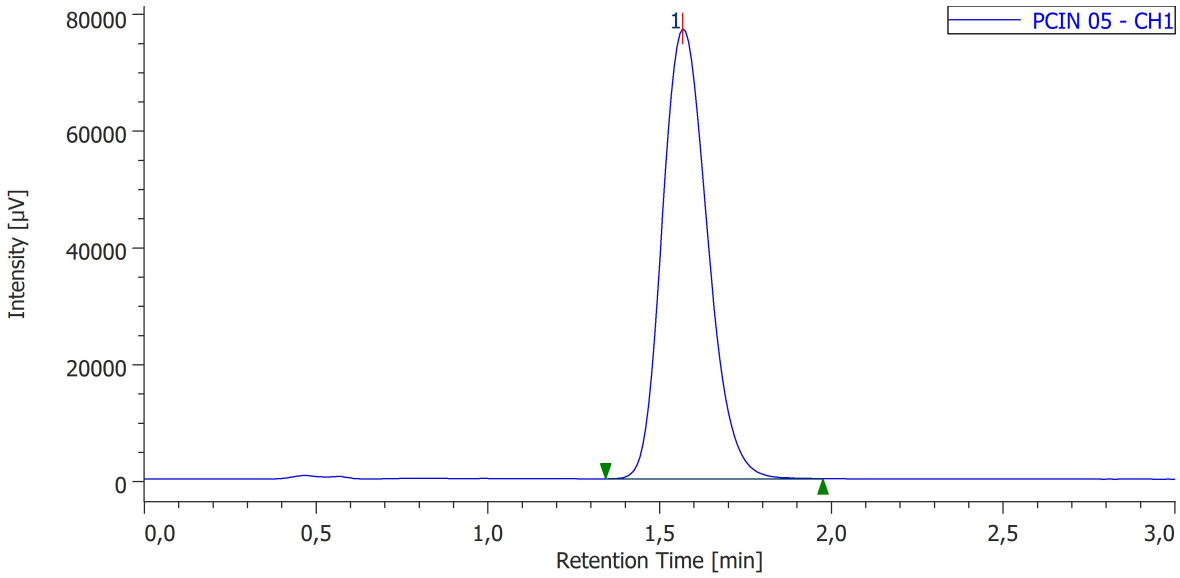


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:43:30
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:39:57
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,567	705395	77041	100,000	100,000	N/A	668	N/A	1,198	

Chromatogram

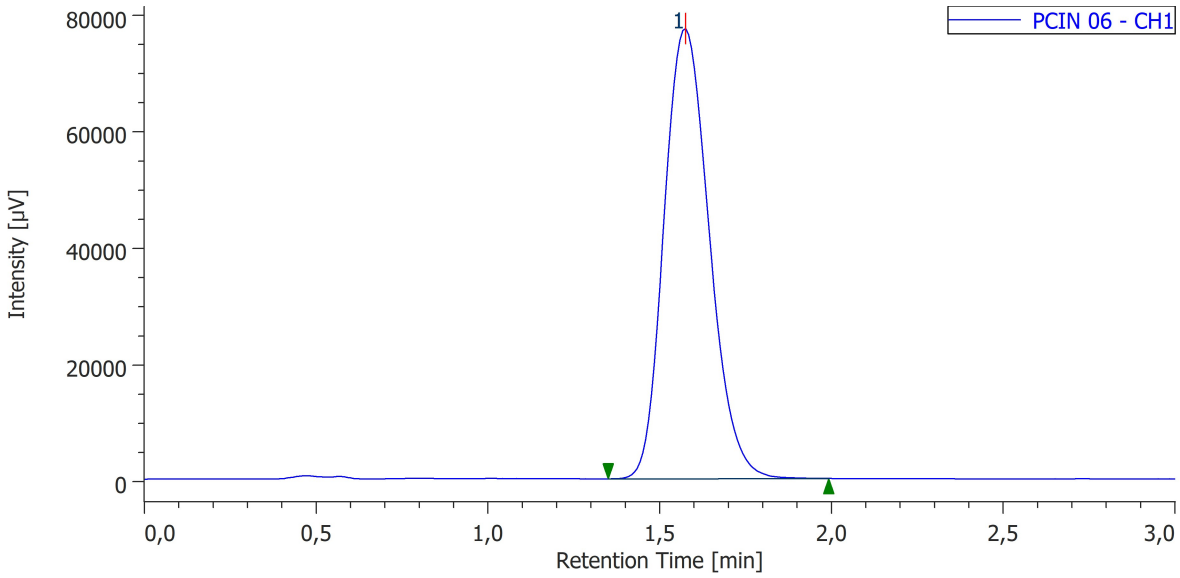


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:46:42
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:43:19
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,575	707483	77162	100,000	100,000	N/A	672	N/A	1,165	

Chromatogram

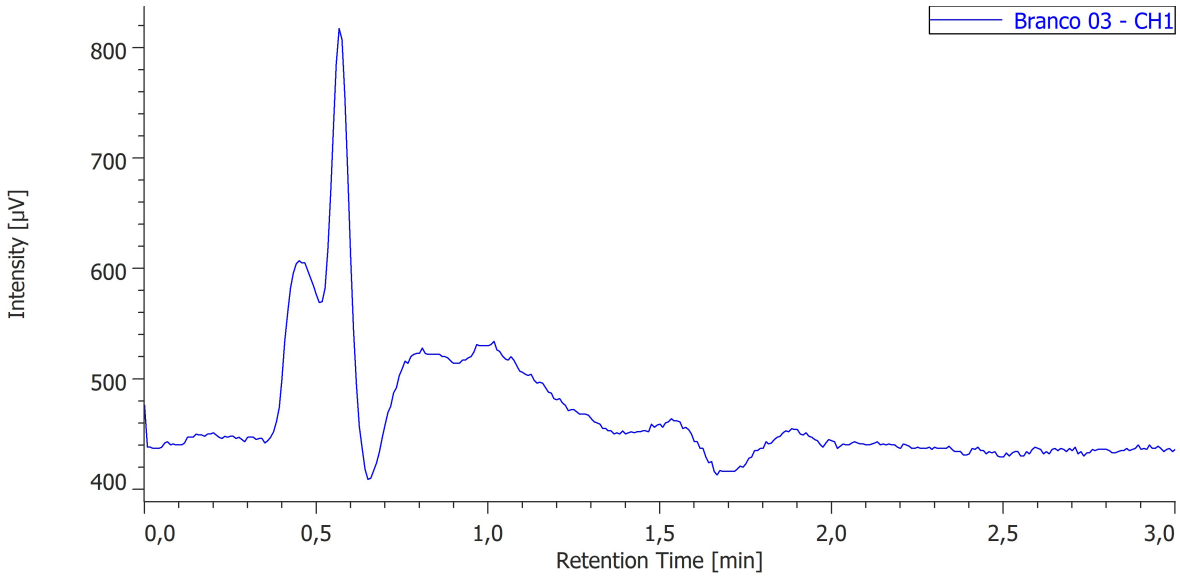


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 13:52:14
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 13:46:37
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

Chromatogram

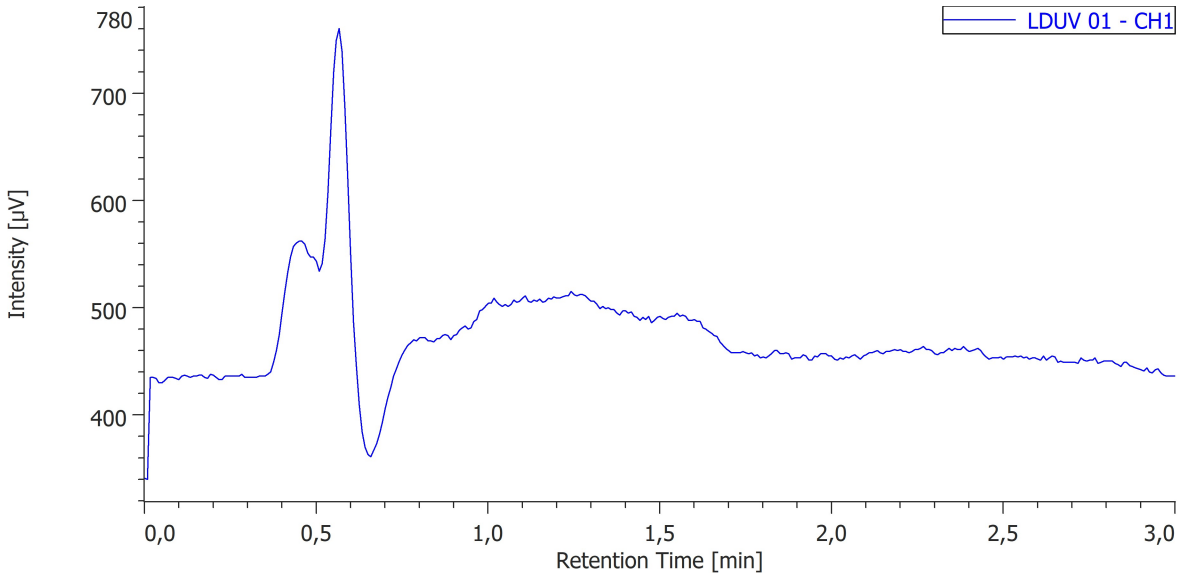


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 14:44:06
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:41:04
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

Chromatogram

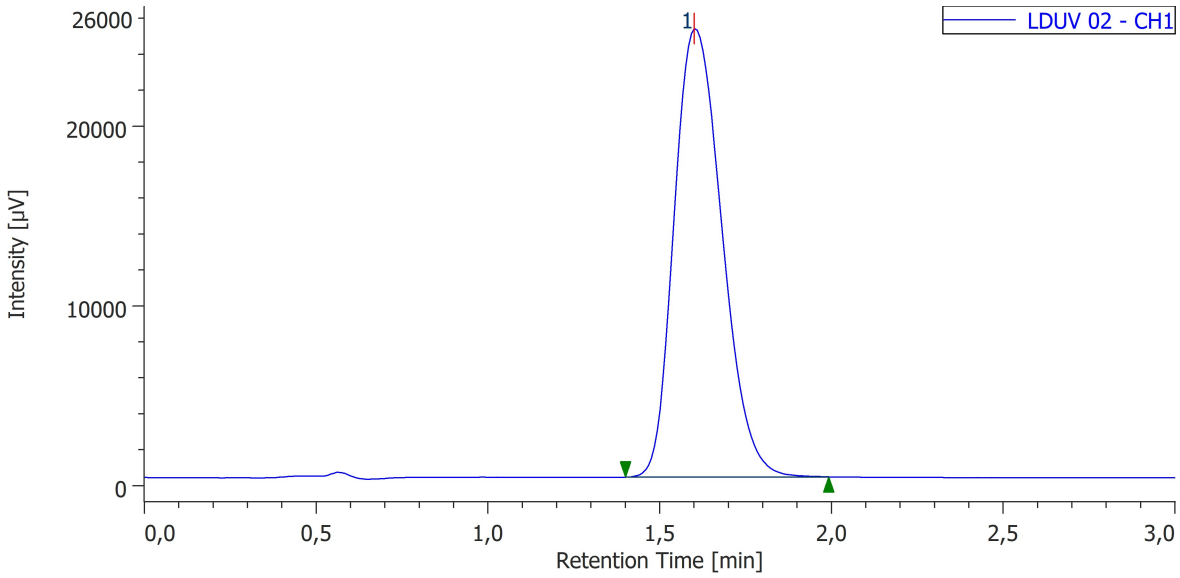


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 14:47:26
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:44:24
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,600	242132	24938	100,000	100,000	N/A	608	N/A	1,267	

Chromatogram

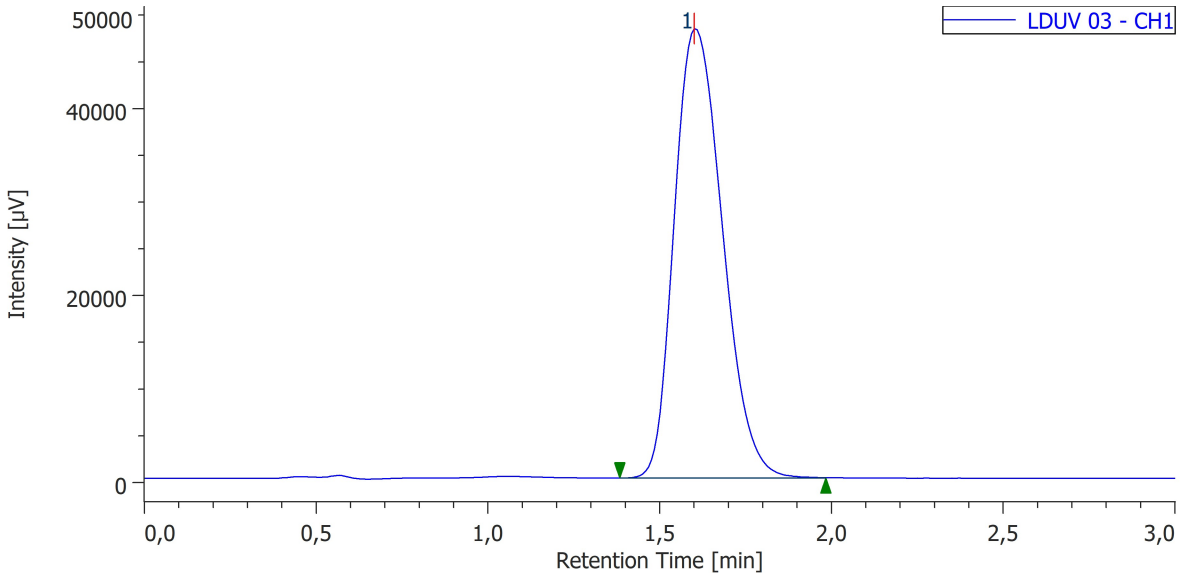


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 14:50:46
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:47:44
Volume	10,0 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,600	468694	48036	100,000	100,000	N/A	600	N/A	1,280	

Chromatogram

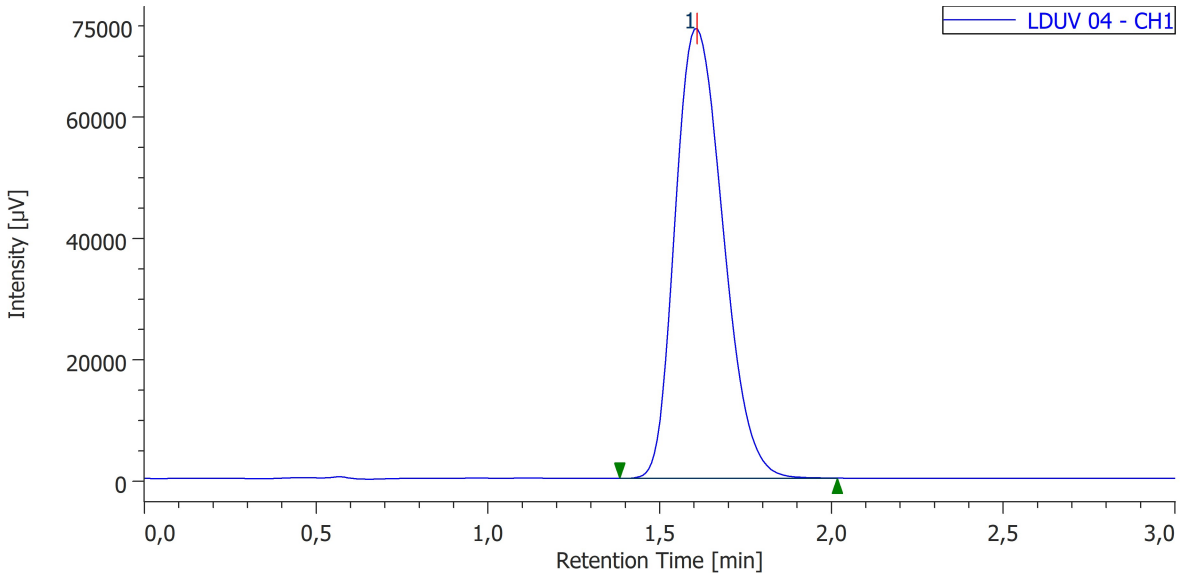


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 14:54:10
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:51:07
Volume	10,0 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,608	720782	74052	100,000	100,000	N/A	609	N/A	1,219	

Chromatogram

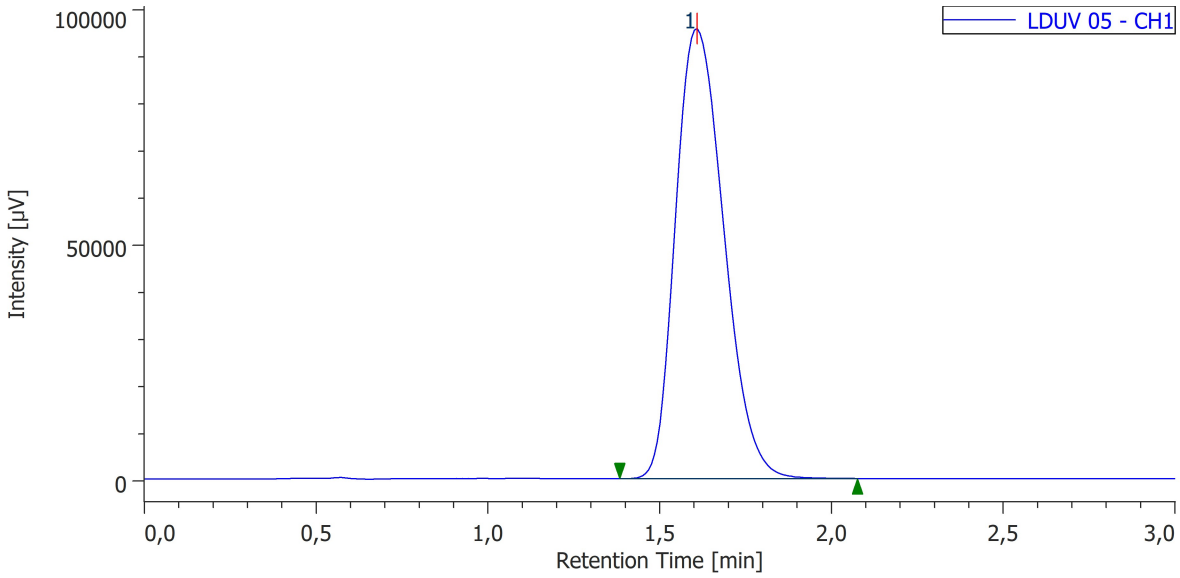


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 14:57:32
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:54:29
Volume	10,0 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,608	935774	95458	100,000	100,000	N/A	602	N/A	1,239	

Chromatogram

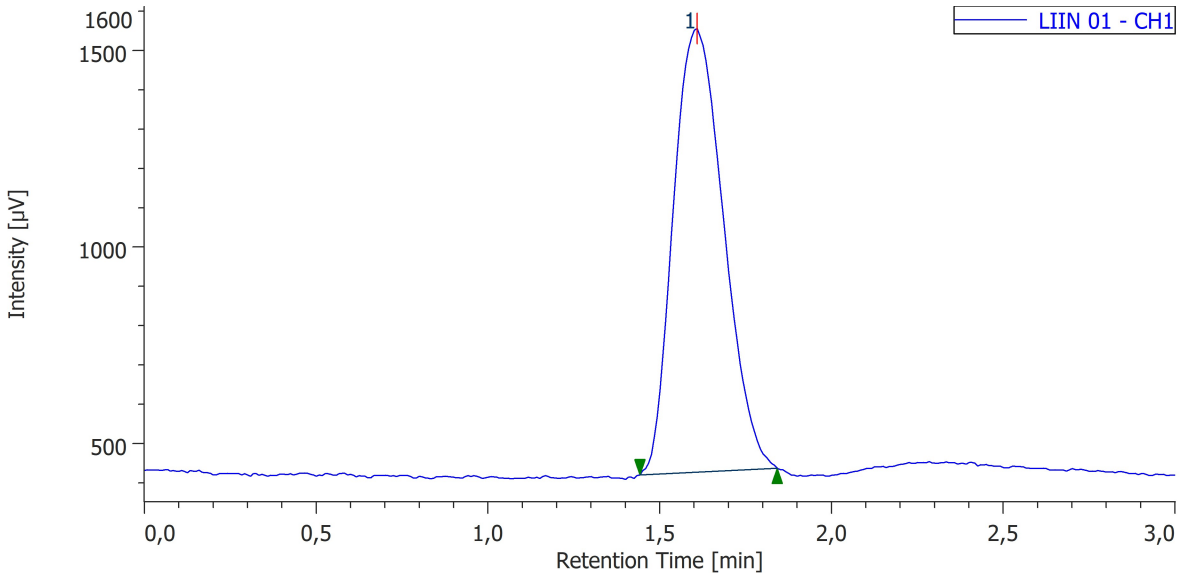


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 15:02:54
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 14:59:52
Volume	0,1 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,608	11485	1128	100,000	100,000	N/A	536	N/A	1,186	

Chromatogram

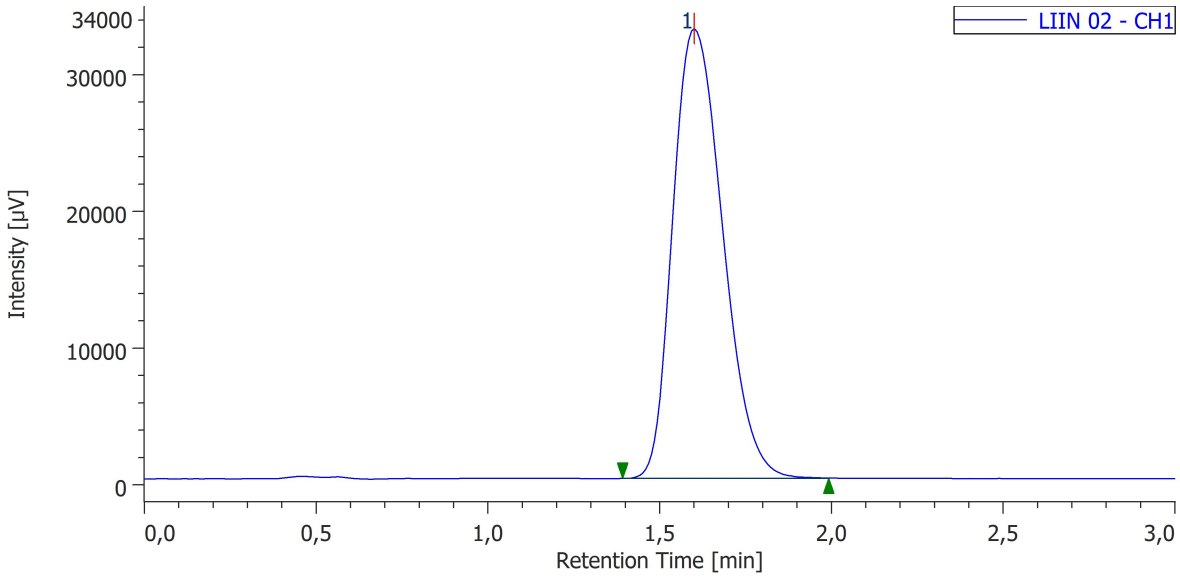


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 15:06:14
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 15:03:12
Volume	5,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,600	332276	32878	100,000	100,000	N/A	559	N/A	1,275	

Chromatogram

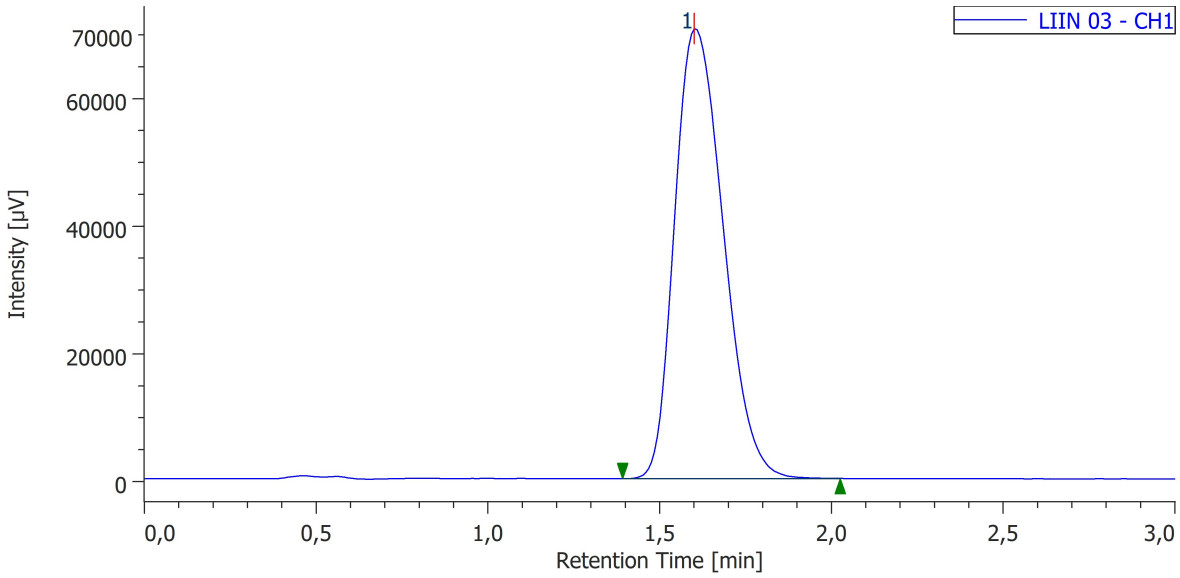


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 15:09:38
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 15:06:35
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,600	695204	70481	100,000	100,000	N/A	585	N/A	1,309	

Chromatogram

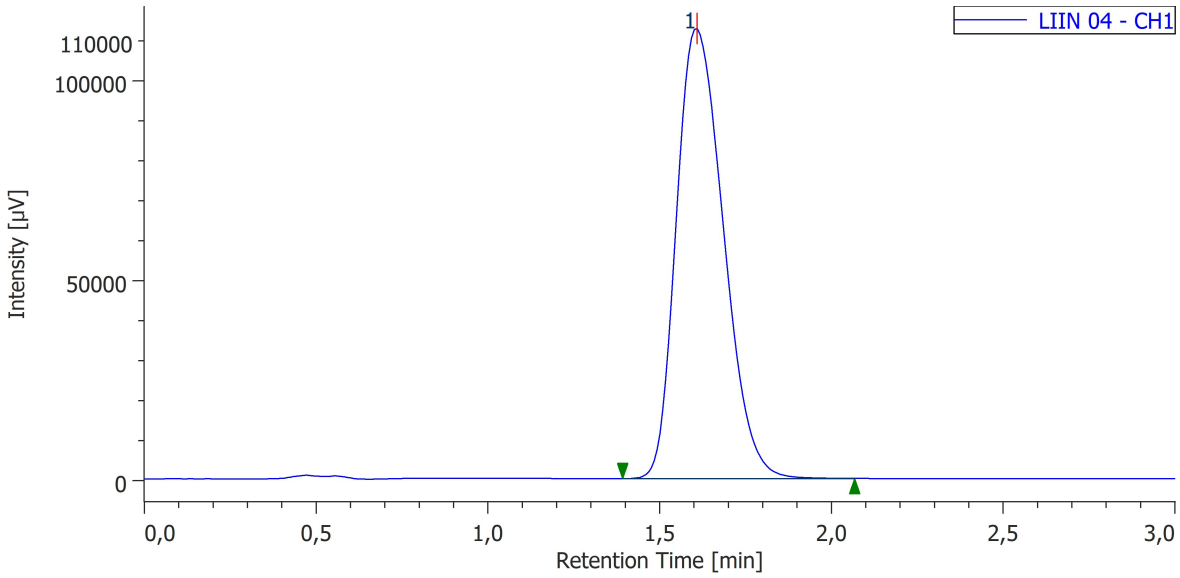


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 15:13:02
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 15:10:00
Volume	15,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,608	1072897	112486	100,000	100,000	N/A	633	N/A	1,247	

Chromatogram

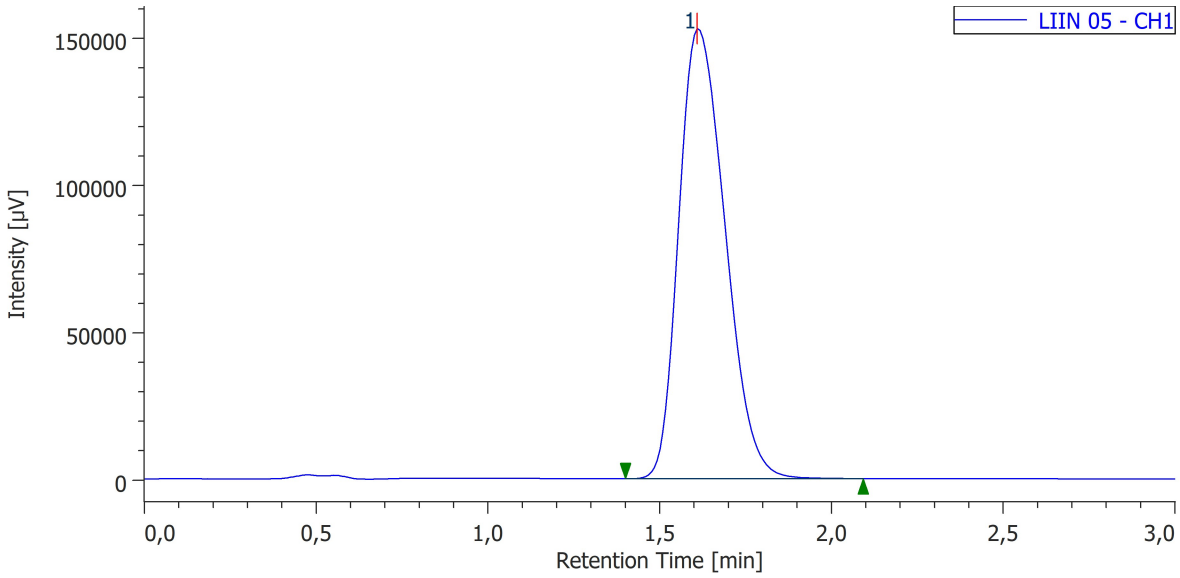


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 15:16:30
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 15:13:27
Volume	20,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 0004
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	INT

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,608	1431268	152731	100,000	100,000	N/A	653	N/A	1,316	

Chromatogram

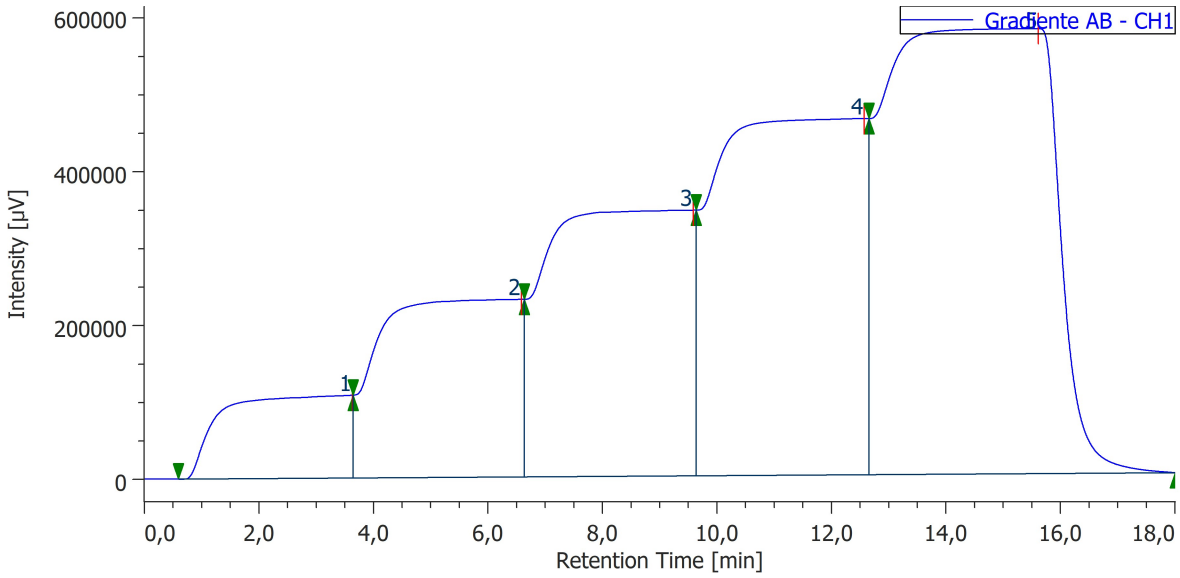


Chromatogram Information	
User Name	Administrator
Date Modified	22/04/2021 16:13:25
Description	
HPLC System Name	HPLC-0004
Injection Date	22/04/2021 15:55:24
Volume	0,1 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	18,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB 0004
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,633	15931132	107631	5,145	6,240	N/A	N/A	N/A	N/A	
2	40%	1	6,583	38040480	230738	12,286	13,378	N/A	N/A	N/A	N/A	
3	60%	1	9,583	59058879	345200	19,074	20,015	N/A	N/A	N/A	N/A	
4	80%	1	12,567	80533590	462798	26,009	26,833	N/A	N/A	N/A	N/A	
5	100%	1	15,608	116069695	578365	37,486	33,534	N/A	N/A	N/A	N/A	

Chromatogram

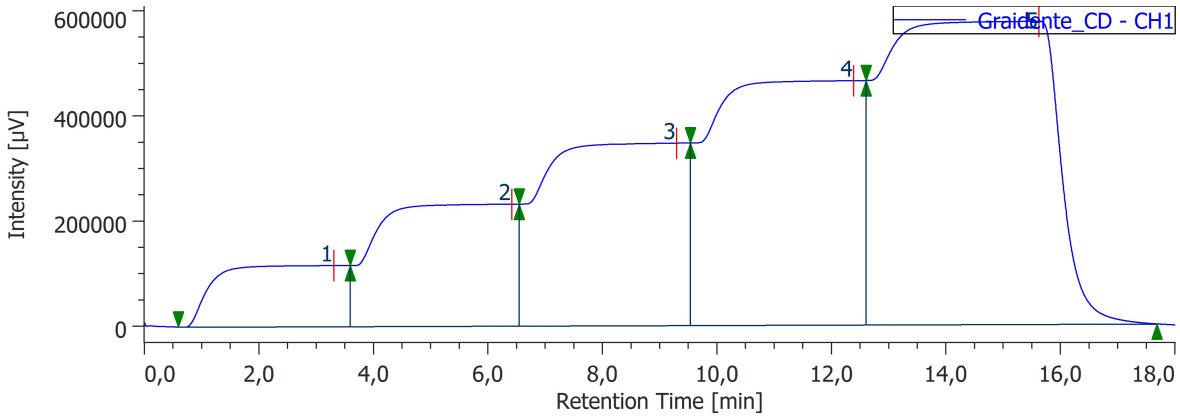

Channel & Peak Information Table

Chromatogram Name: Graidente_CD-CH1
Sample Name:
Channel Name: UV

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,308	17416624	116075	5,582	6,692	N/A	N/A	N/A	N/A	
2	40%	1	6,417	37604605	231657	12,052	13,356	N/A	N/A	N/A	N/A	
3	60%	1	9,292	58506116	346570	18,751	19,981	N/A	N/A	N/A	N/A	
4	80%	1	12,383	81587397	464257	26,149	26,766	N/A	N/A	N/A	N/A	
5	100%	1	15,617	116894744	575921	37,465	33,204	N/A	N/A	N/A	N/A	