
Peak Find - EDUV.jws

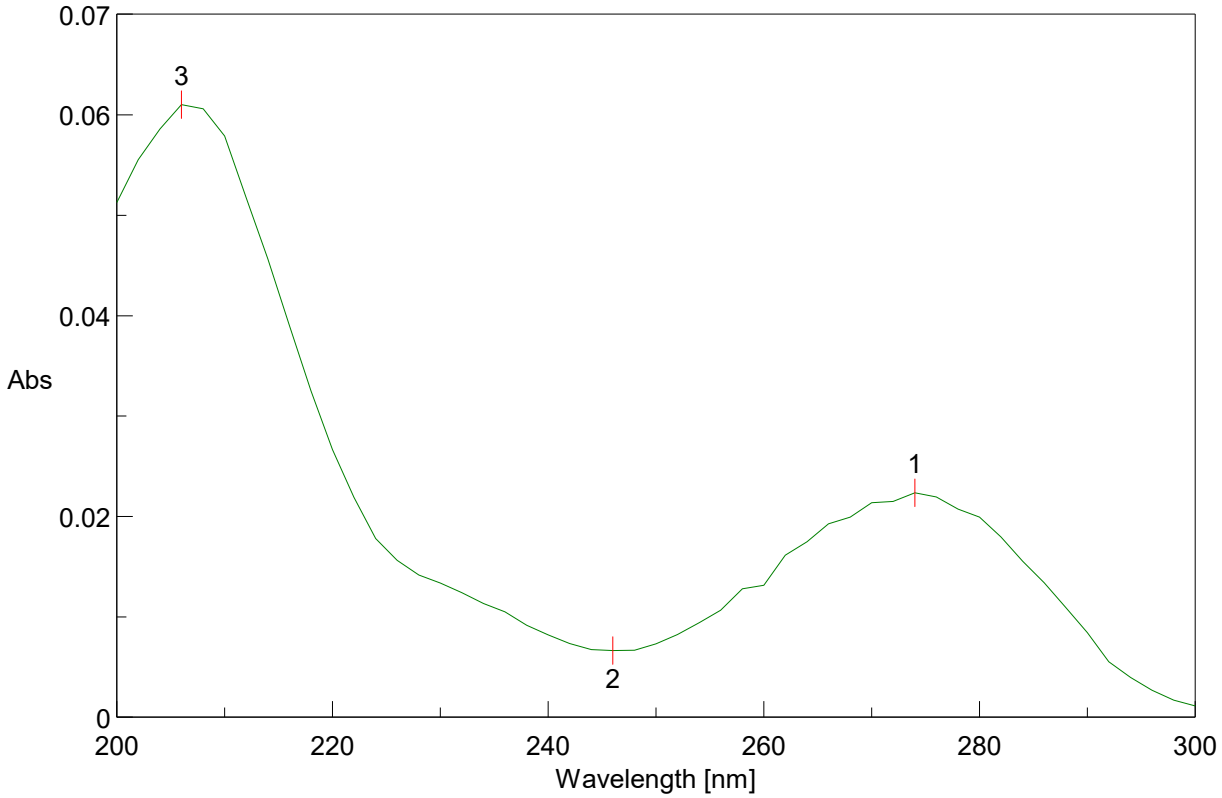

[Comments]

User	QPackSA
Division	---
Company	CEDIC
Creation date	4/5/2021 17:37

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	201


[Measurement Information]

Instrument Name	UV-4075
Model Name	UV-4075
Serial No.	C082861659
ROM version	1.01.16

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0223294	2	246	0.00662184
3	206	0.0609817			

Chromatogram

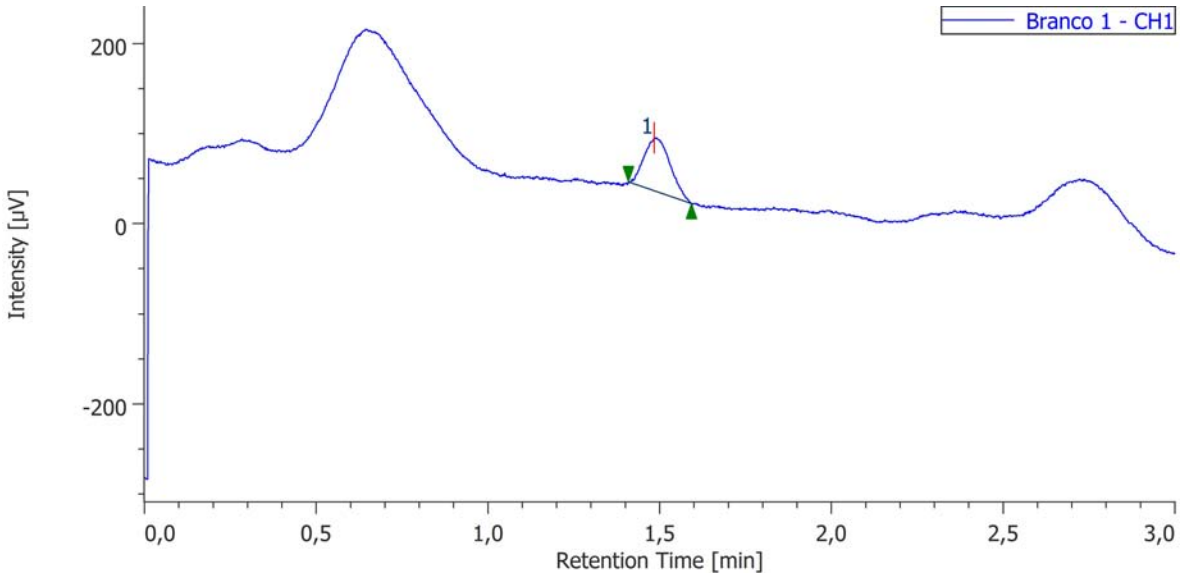


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:21:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 10:47:50
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,483	315	59	100,000	100,000	N/A	1646	N/A	1,241	

Chromatogram

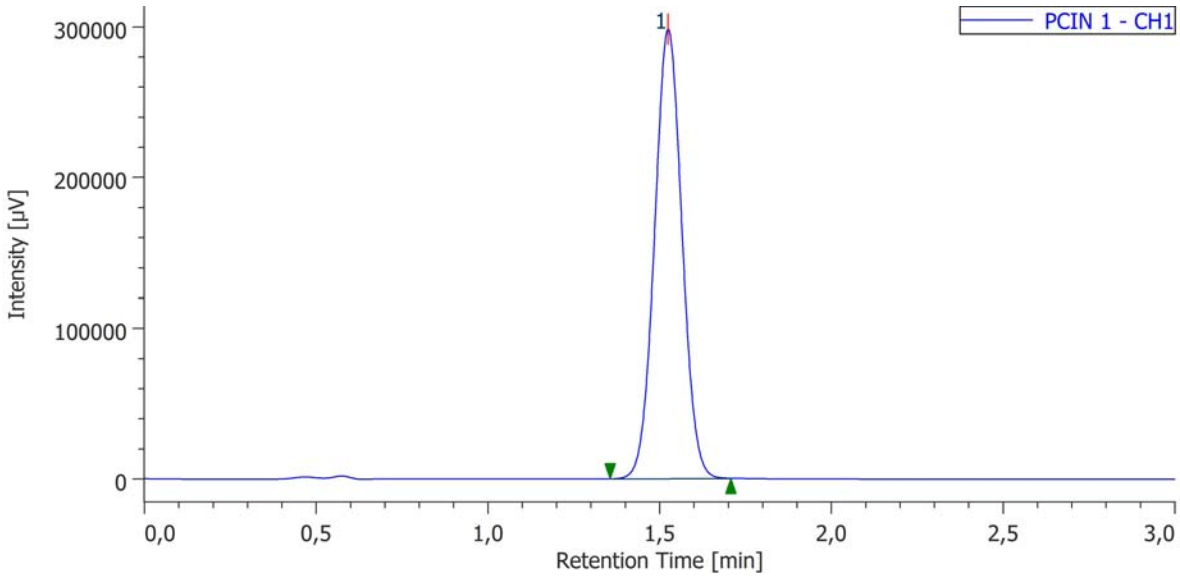


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 10:51:23
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,523	1658980	298333	100,000	100,000	N/A	1732	N/A	1,037	

Chromatogram

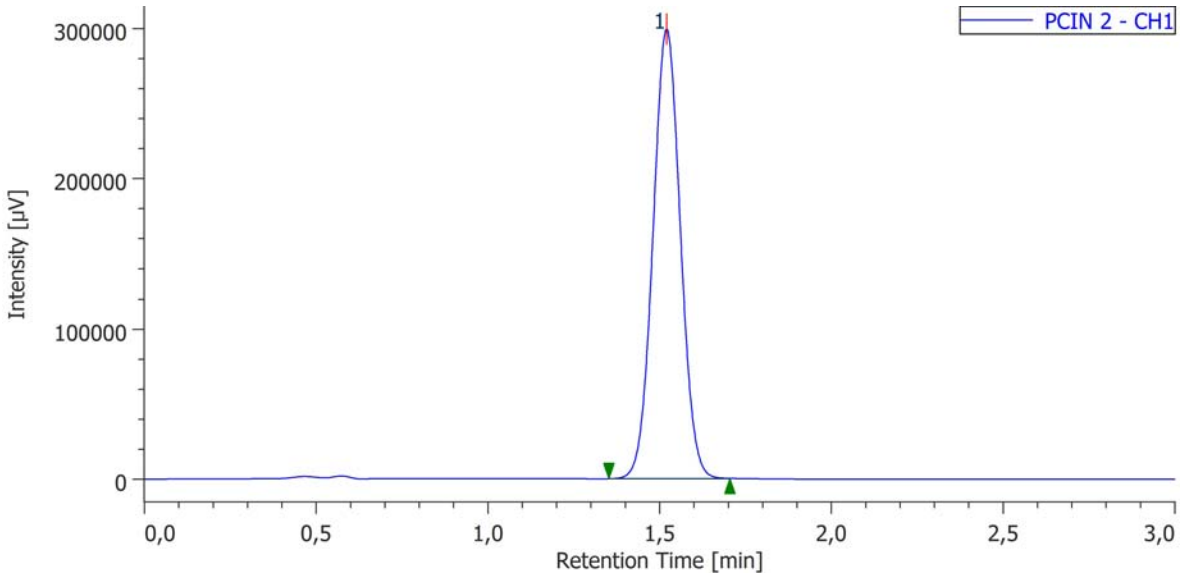


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 10:55:02
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,520	1658869	299208	100,000	100,000	N/A	1734	N/A	1,023	

Chromatogram

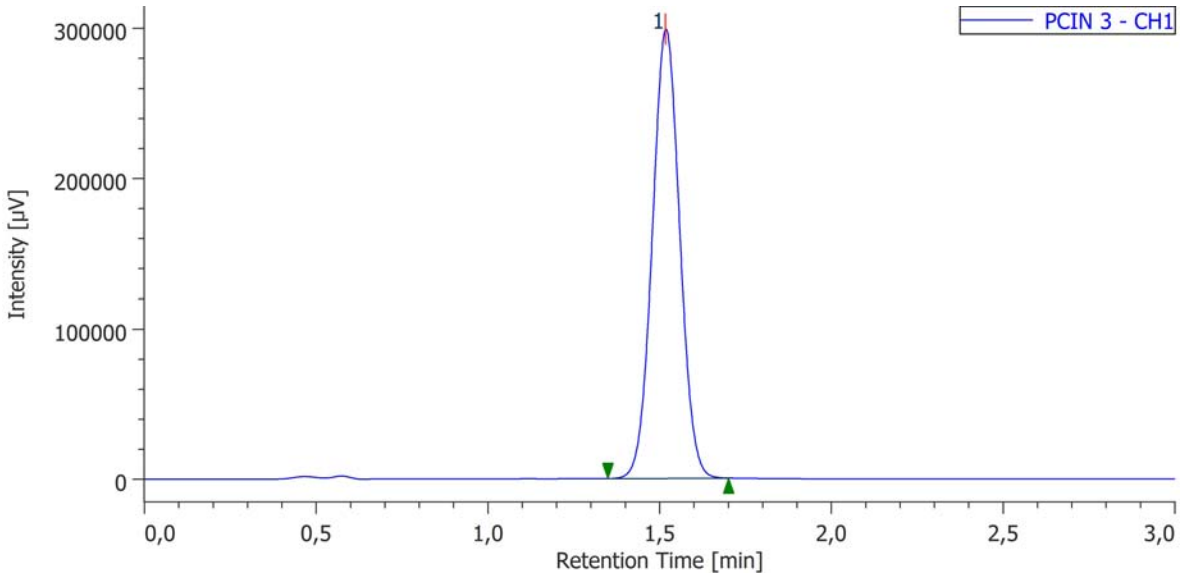


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 10:58:28
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,517	1658441	298912	100,000	100,000	N/A	1726	N/A	1,038	

Chromatogram

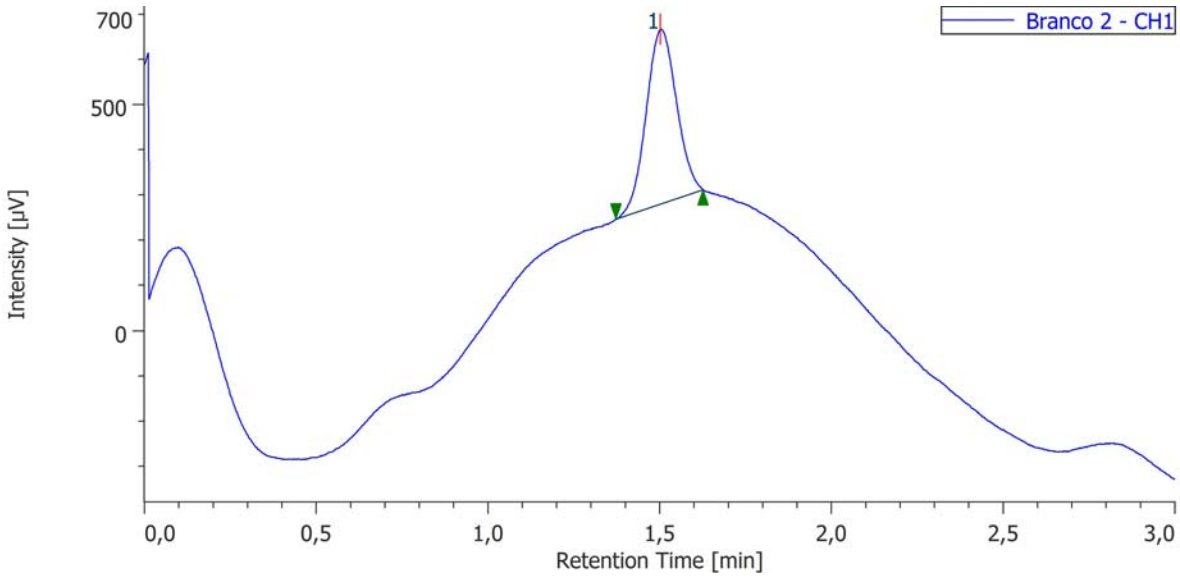


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:34:43
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:01:46
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,502	2373	388	100,000	100,000	N/A	1369	N/A	1,055	

Chromatogram

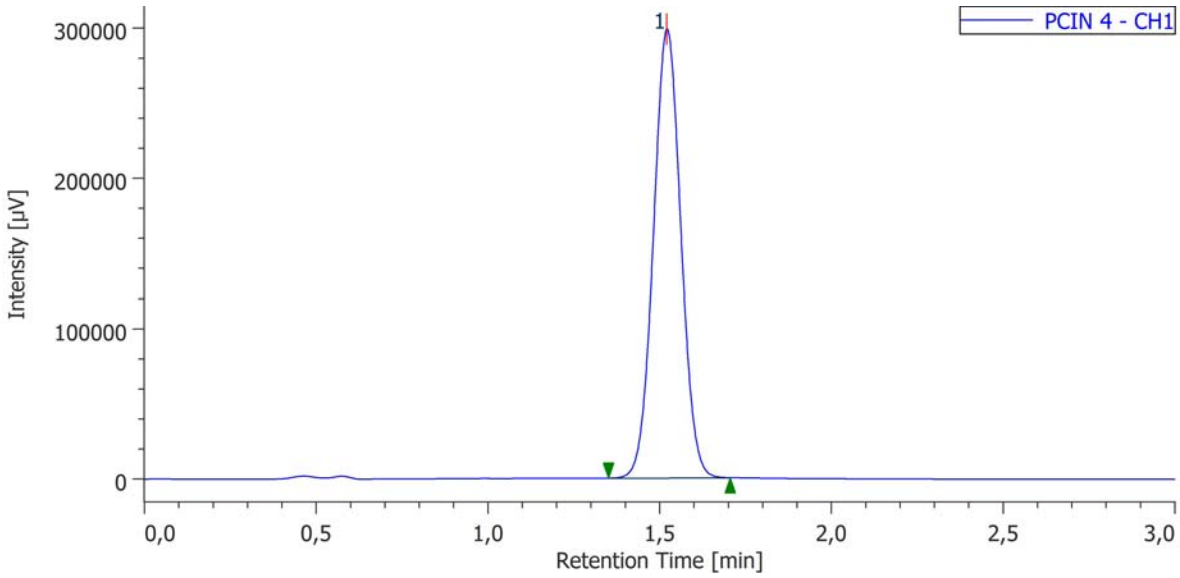


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:05:25
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,520	1657074	298657	100,000	100,000	N/A	1733	N/A	1,038	

Chromatogram

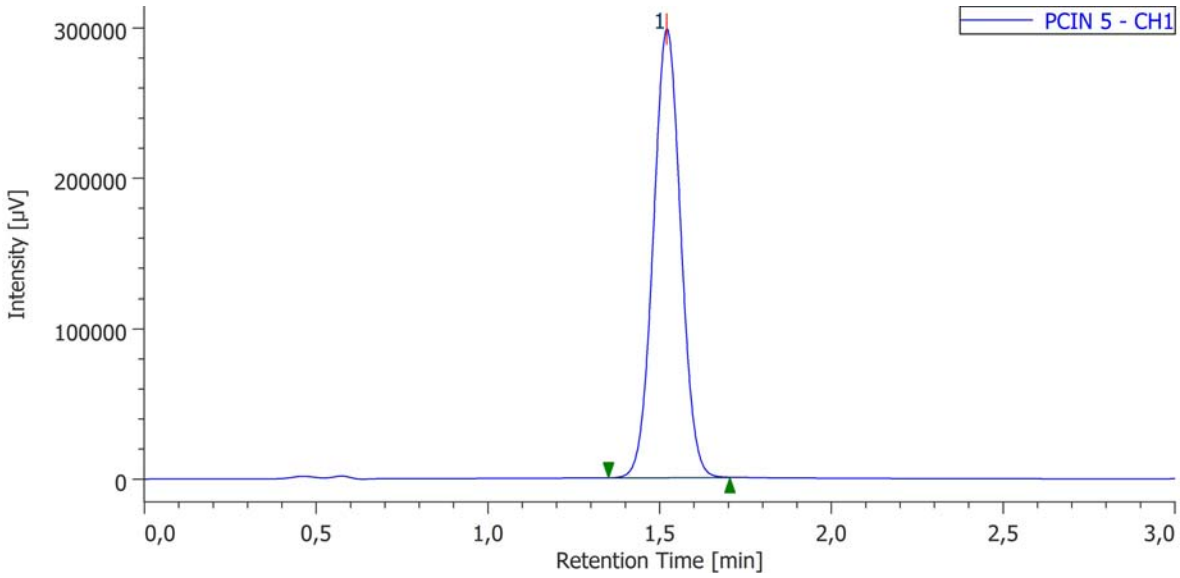


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:09:04
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,520	1657697	298269	100,000	100,000	N/A	1727	N/A	1,033	

Chromatogram

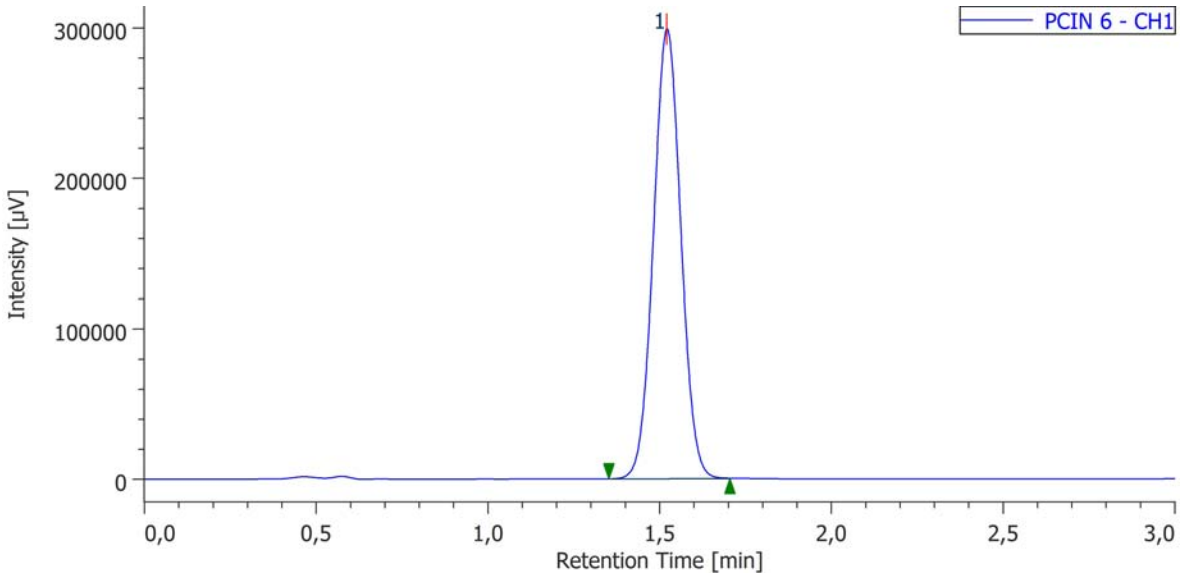


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:20:32
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:12:46
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,520	1658178	298775	100,000	100,000	N/A	1730	N/A	1,040	

Chromatogram

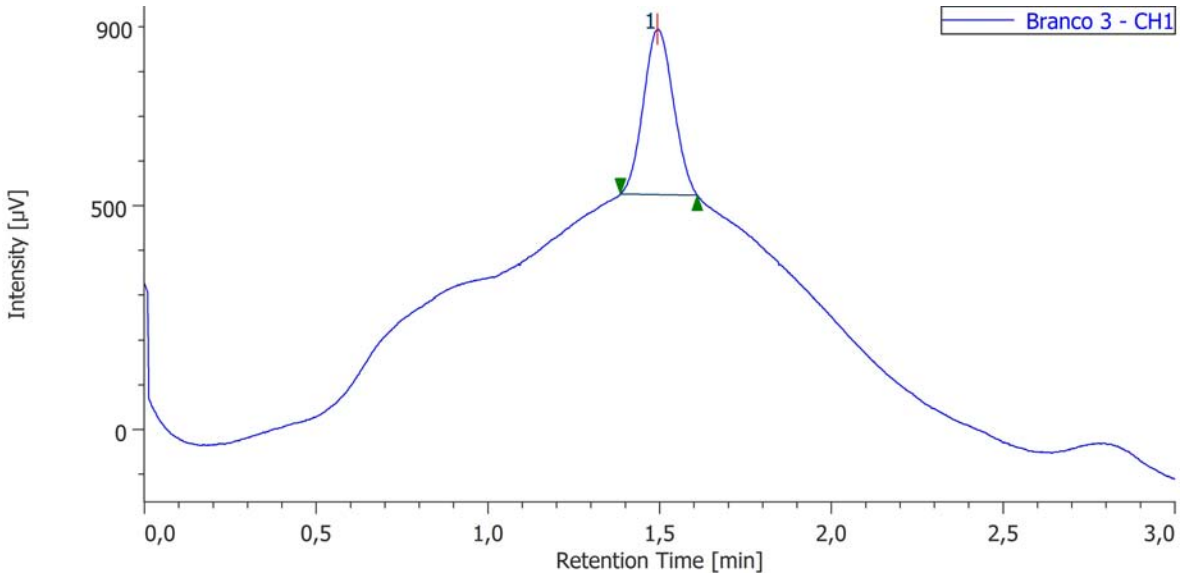


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:37:18
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:16:05
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,493	2234	370	100,000	100,000	N/A	1346	N/A	1,060	

Chromatogram

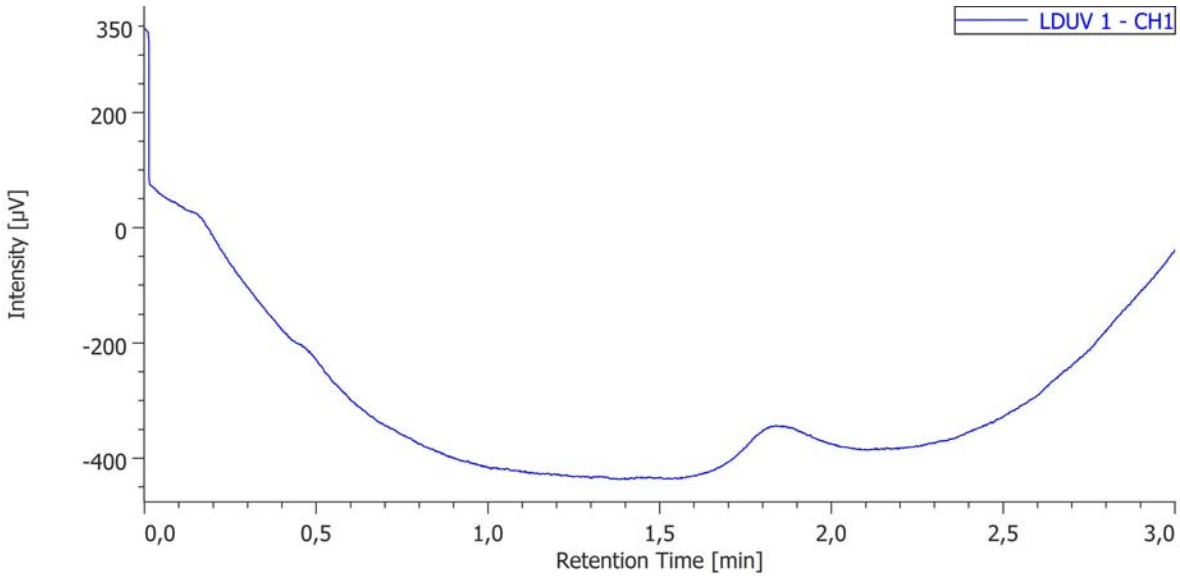


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:53:16
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:35:59
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

Chromatogram

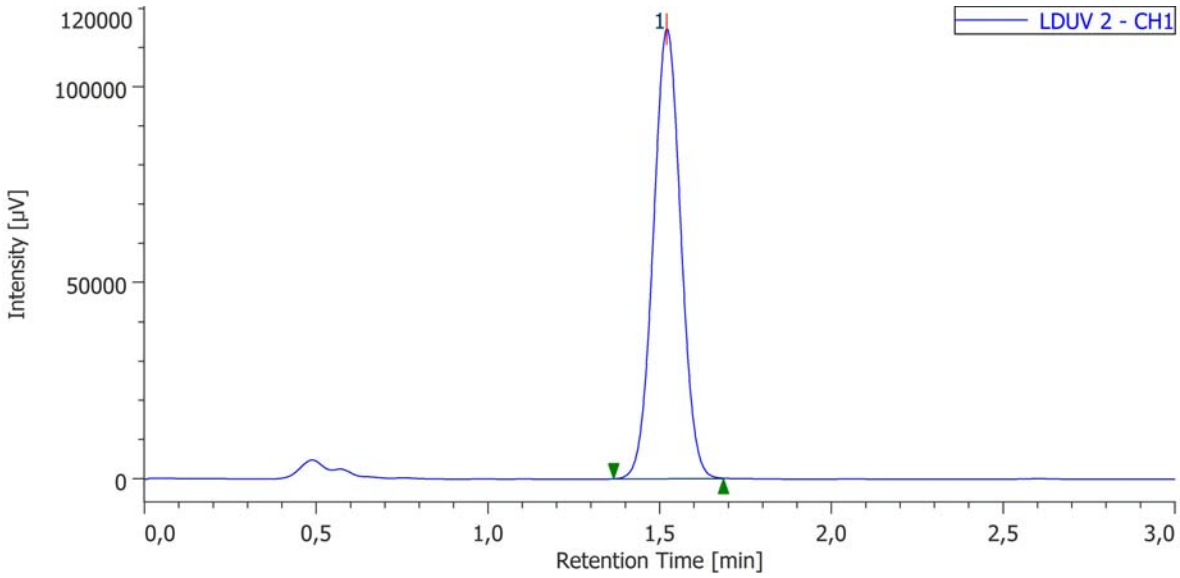


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:53:16
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:39:59
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,520	637685	114715	100,000	100,000	N/A	1723	N/A	1,032	

Chromatogram

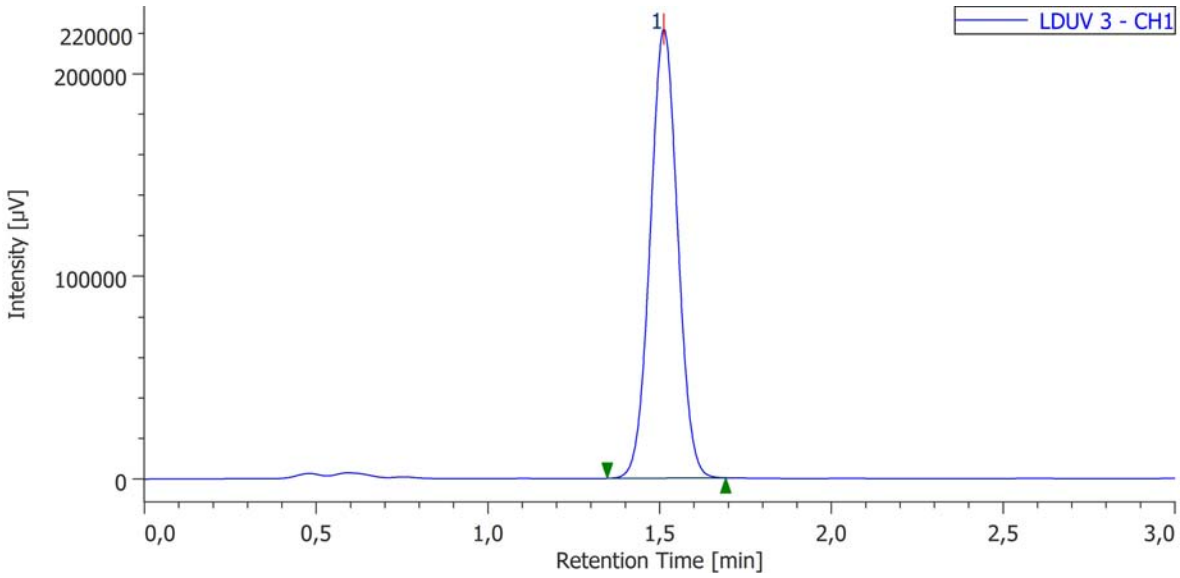


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:53:16
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:43:40
Volume	20,0 [µL]
Sample #	3
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,512	1231188	221687	100,000	100,000	N/A	1710	N/A	1,024	

Chromatogram

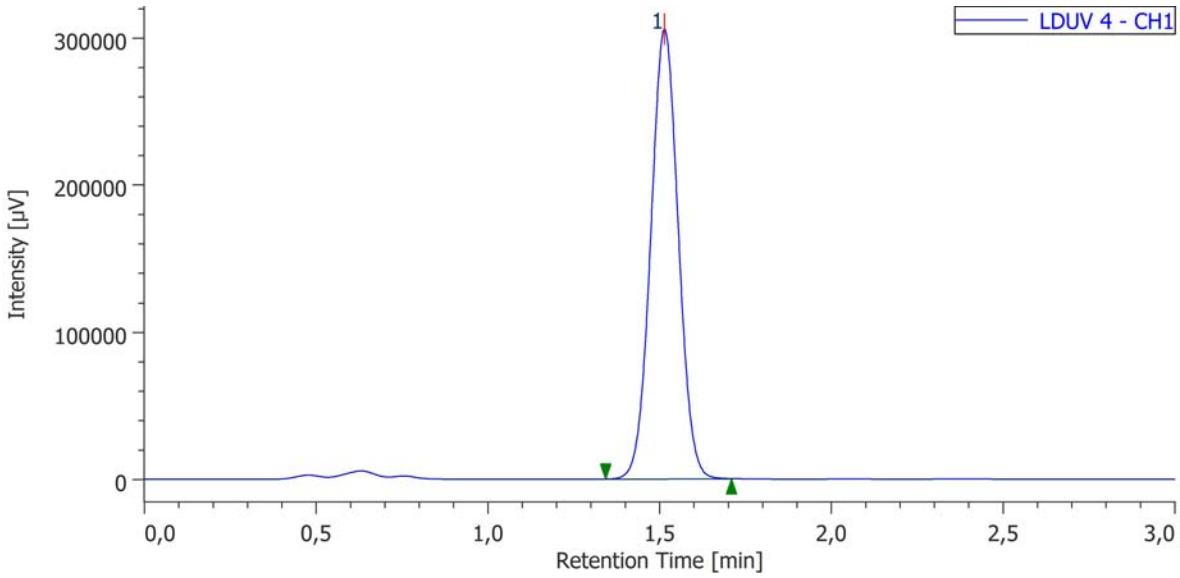


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:53:16
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:48:05
Volume	20,0 [µL]
Sample #	4
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,513	1704044	305747	100,000	100,000	N/A	1705	N/A	1,026	

Chromatogram

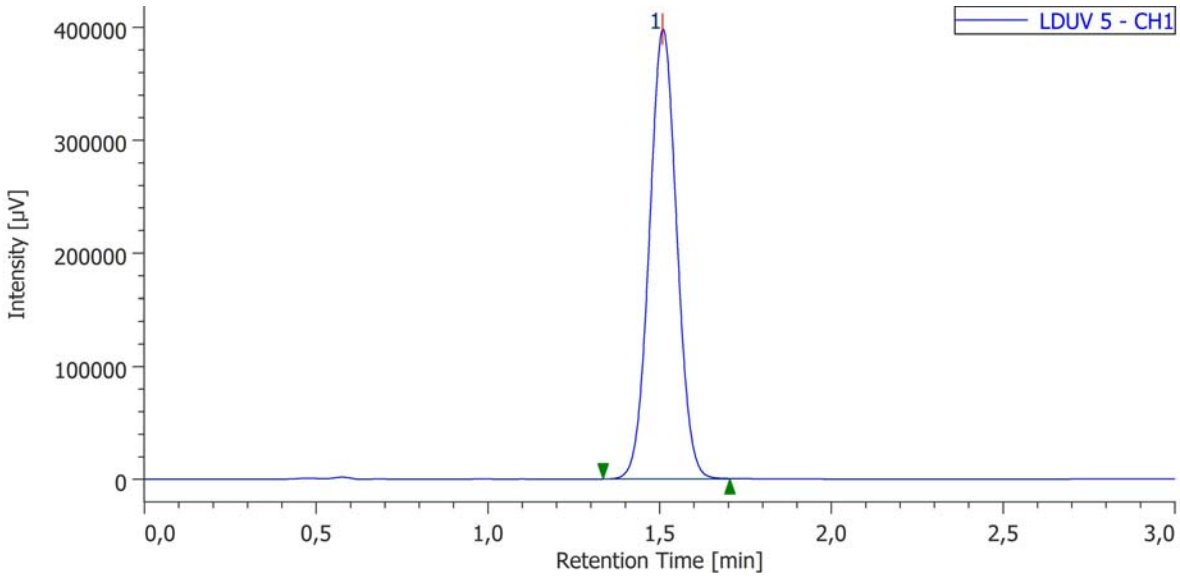


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 11:57:22
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 11:51:57
Volume	20,0 [µL]
Sample #	5
Project Name	Qualificacao
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificacao
MS Method	
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,508	2245585	398033	100,000	100,000	N/A	1712	N/A	1,035	

Chromatogram

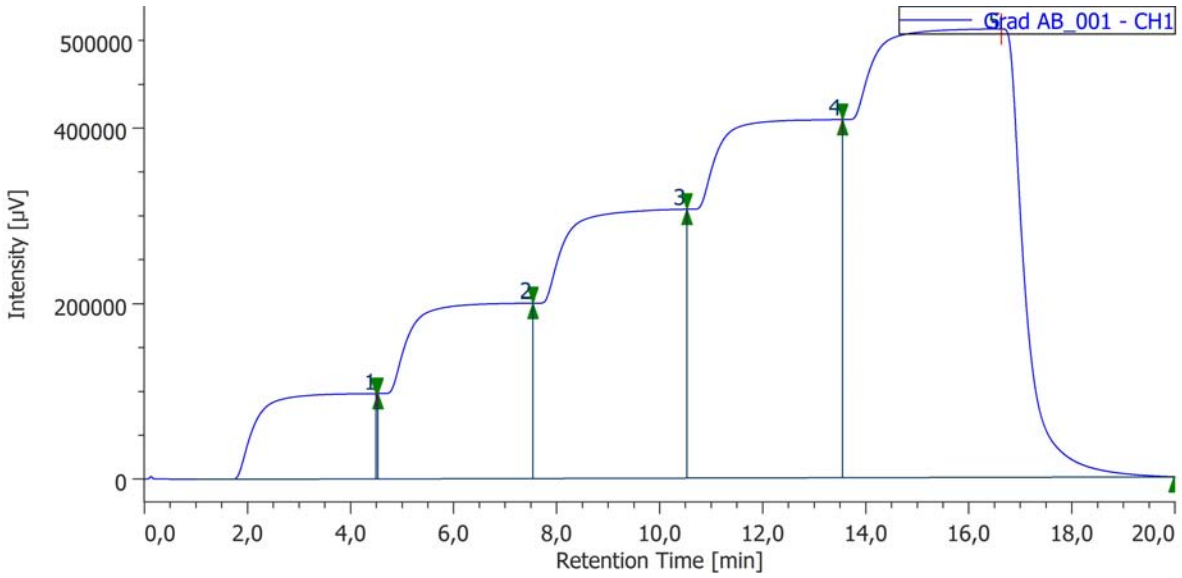


Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 12:48:54
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 12:28:53
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
MS Method	
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4,515	97185	6,385	N/A	N/A	N/A	N/A	
2	40 %	1	7,535	199901	13,134	N/A	N/A	N/A	N/A	
3	60 %	1	10,517	305969	20,103	N/A	N/A	N/A	N/A	
4	80 %	1	13,535	407946	26,803	N/A	N/A	N/A	N/A	
5	100 %	1	16,628	510990	33,574	N/A	N/A	N/A	N/A	

Chromatogram

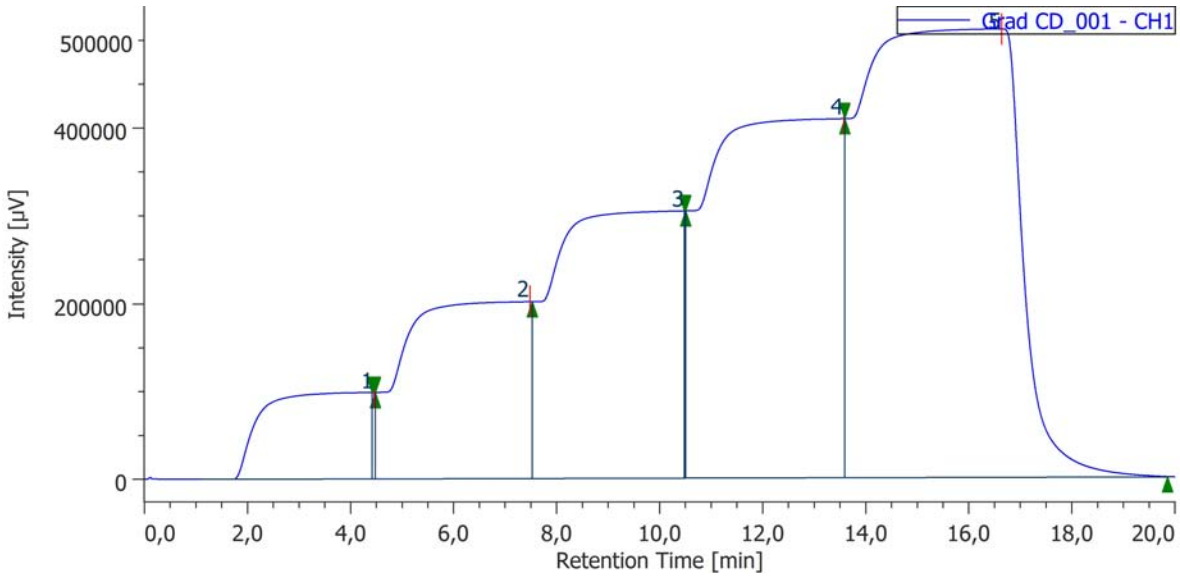

Chromatogram Information	
User Name	QPackSA
Date Modified	5/5/2021 13:17:21
Description	
HPLC System Name	HPLC Toxinas
Injection Date	5/5/2021 12:54:07
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificacao
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
MS Method	
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_001-CH1
Sample Name	
Channel Name	UV-Vis
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Height [µV]	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4,453	98561	6,474	N/A	N/A	N/A	N/A	
2	40 %	1	7,480	201448	13,232	N/A	N/A	N/A	N/A	
3	60 %	1	10,487	303766	19,953	N/A	N/A	N/A	N/A	
4	80 %	1	13,572	408377	26,824	N/A	N/A	N/A	N/A	
5	100 %	1	16,633	510261	33,517	N/A	N/A	N/A	N/A	