

On Peak Spectra

Channel Information	
Chromatogram Name	EDUV_001-CH9
Sample Name	
Channel Name	205,2nm
Sampling Interval	200 [msec]
Peak Method	

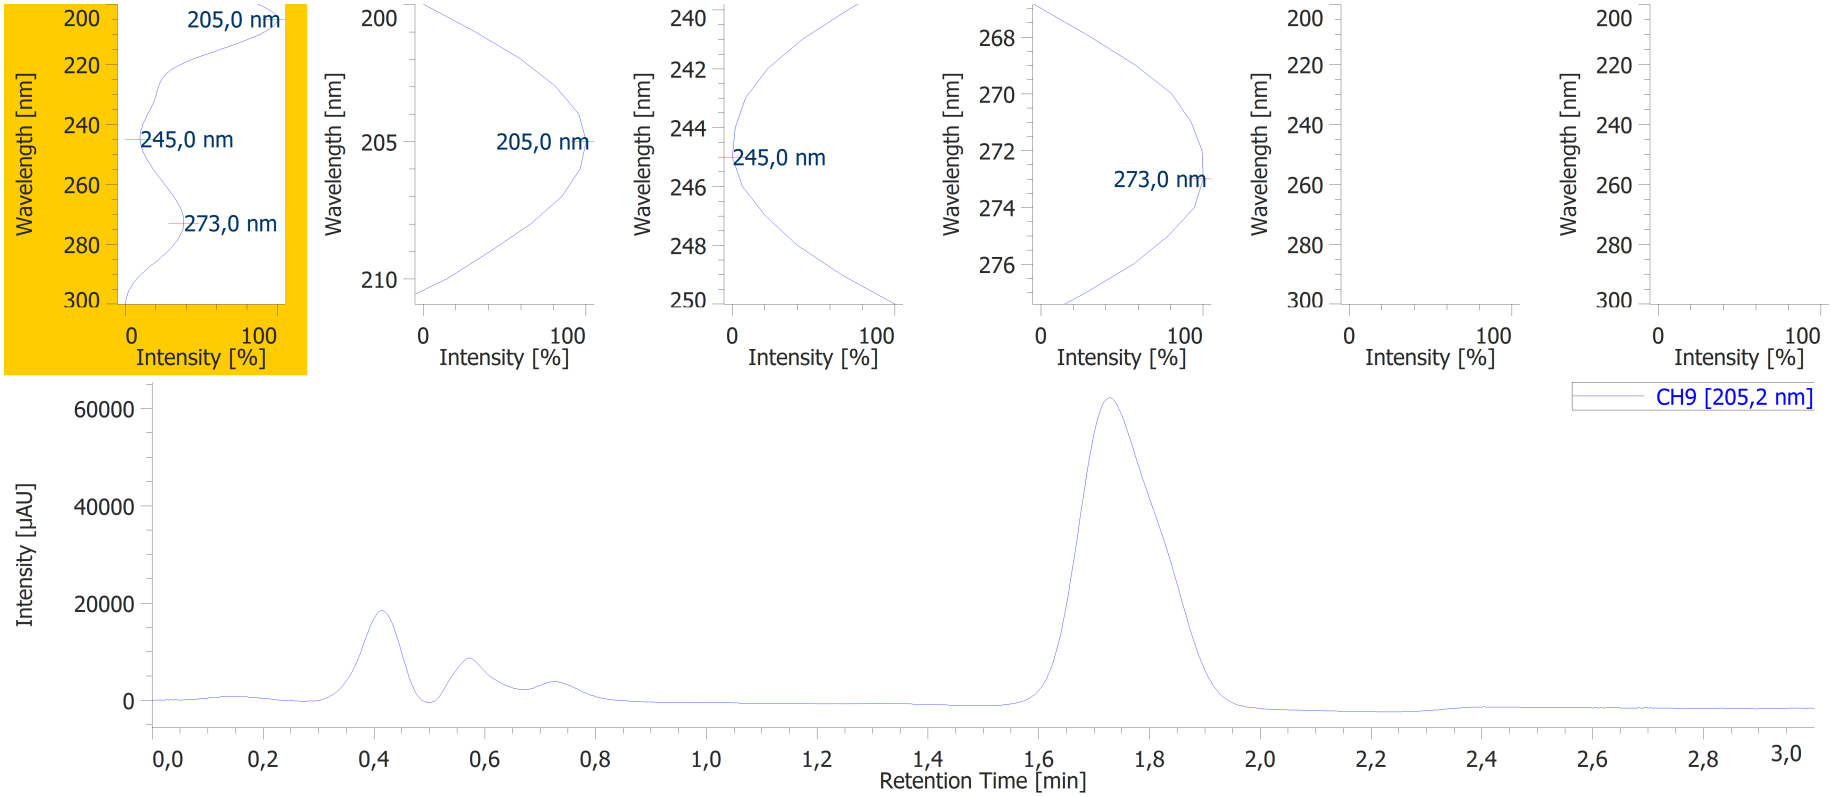

Chromatogram

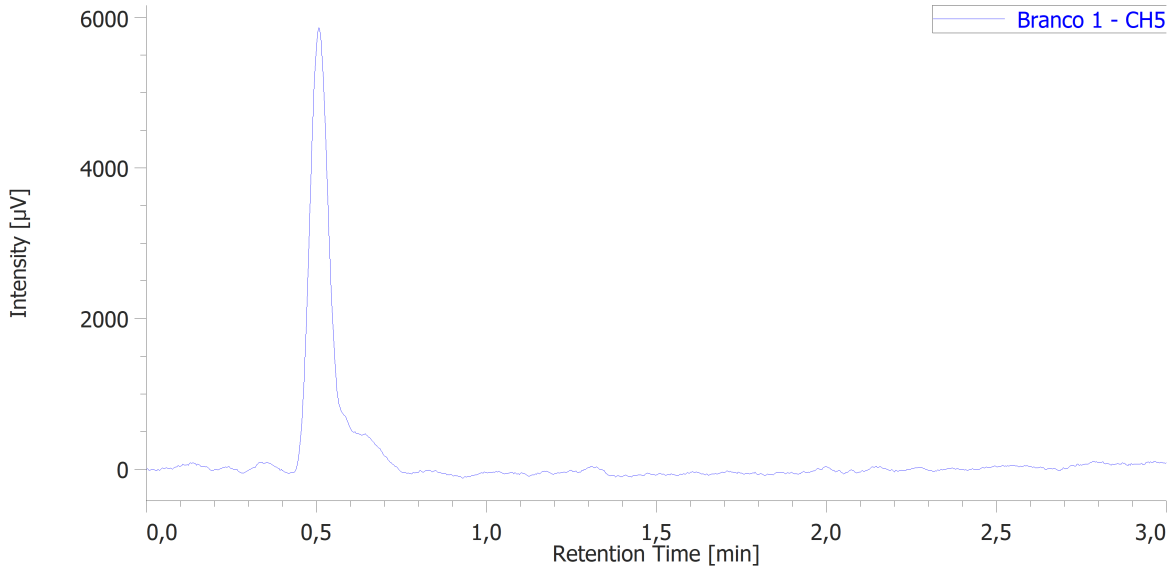


Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 09:53:35
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 09:50:33
Volume	10,00 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

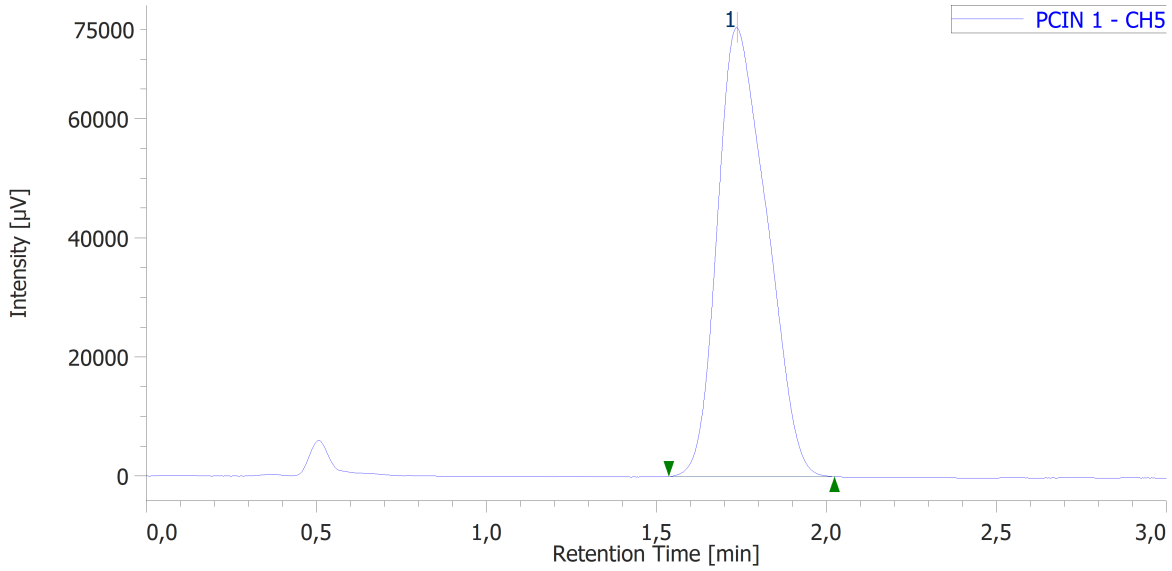

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 09:56:47
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 09:53:45
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,737	761263	75324	100,000	100,000	N/A	613	N/A	1,258	

Creator Administrator
Reviewer
Approver

Chromatogram

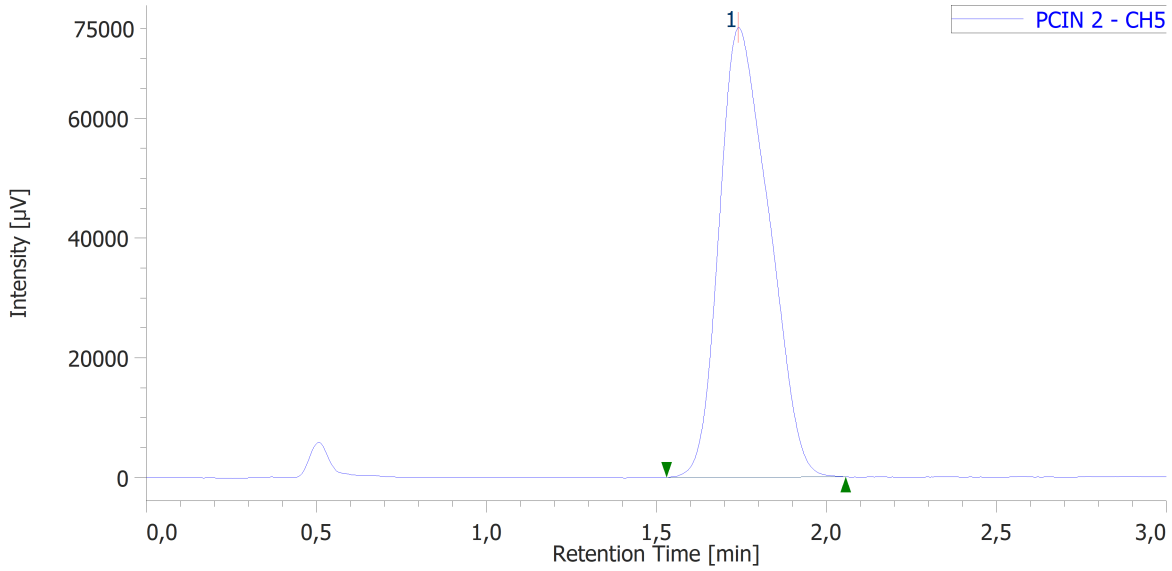

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 09:59:59
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 09:56:57
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,740	763706	75013	100,000	100,000	N/A	607	N/A	1,287	

Creator Administrator
Reviewer
Approver

Chromatogram

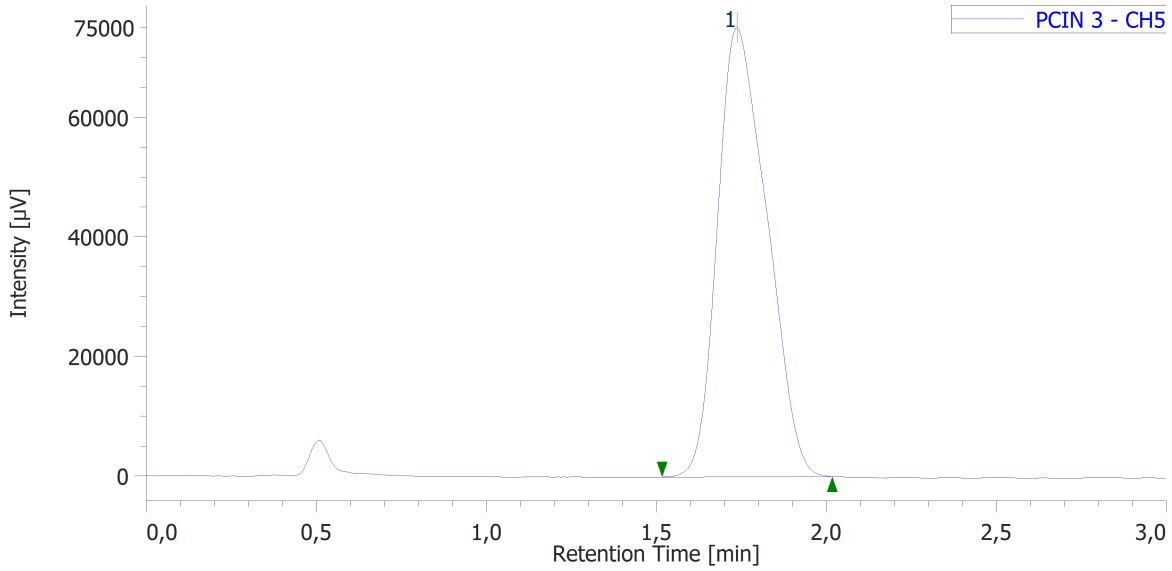

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:03:21
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:00:09
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,737	759679	75079	100,000	100,000	N/A	611	N/A	1,267	

Creator Administrator
Reviewer
Approver

Chromatogram

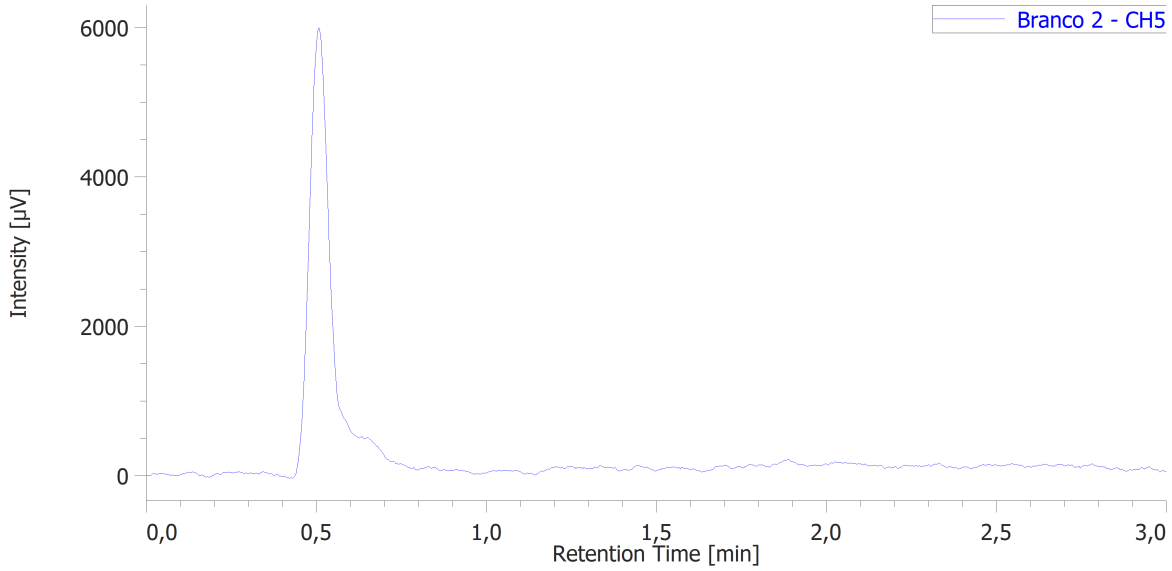


Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:06:23
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:03:21
Volume	10,00 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

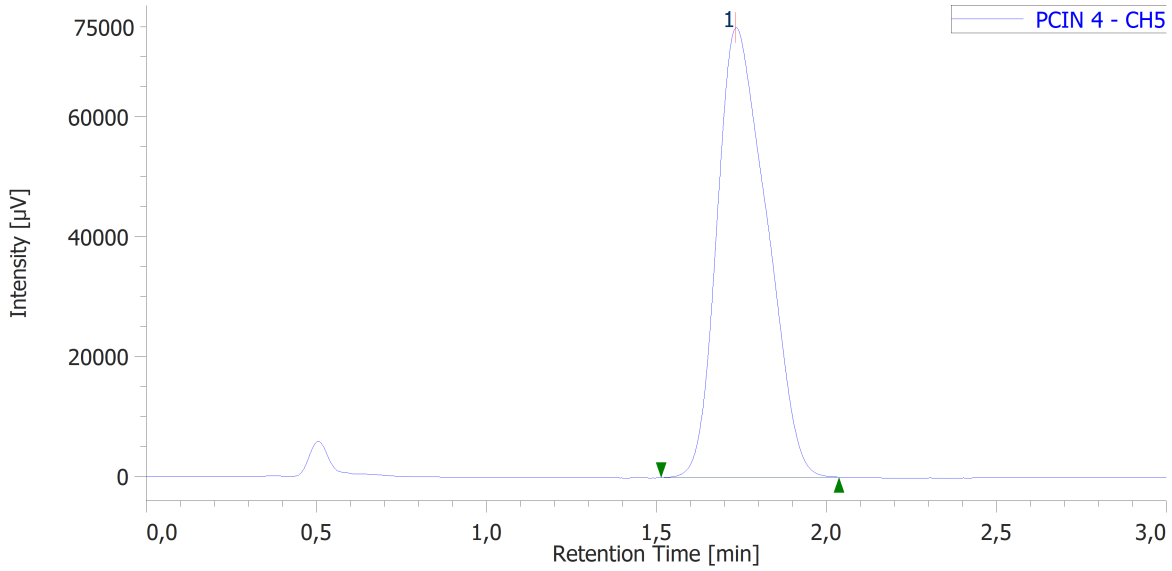

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:09:35
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:06:33
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,733	761132	75015	100,000	100,000	N/A	606	N/A	1,296	

Creator Administrator
Reviewer
Approver

Chromatogram

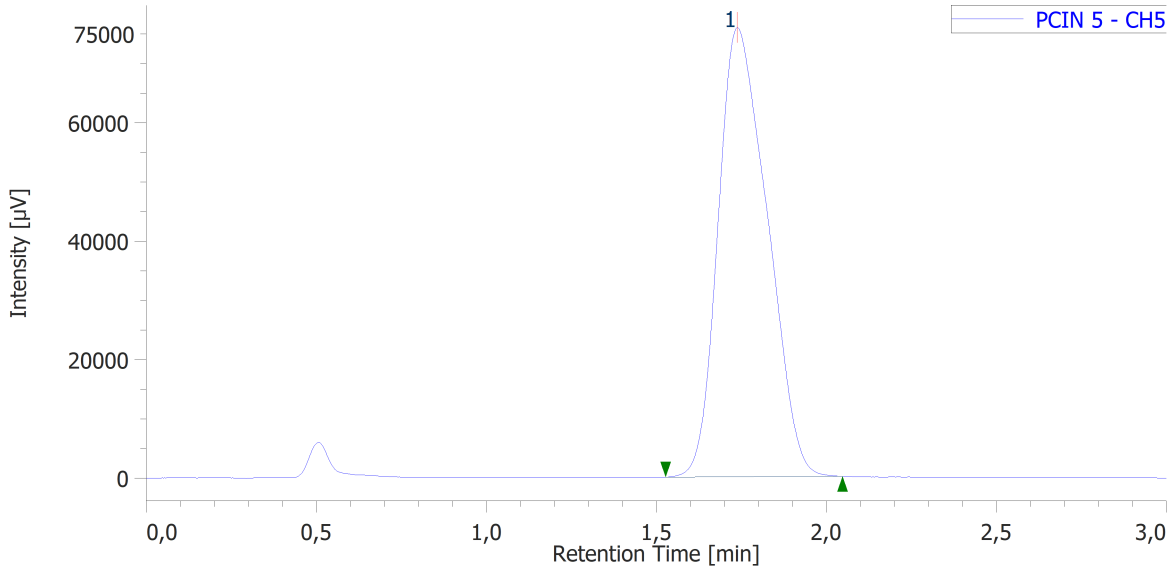

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:12:47
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:09:45
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,737	762838	75813	100,000	100,000	N/A	620	N/A	1,282	

Creator Administrator
Reviewer
Approver

Chromatogram

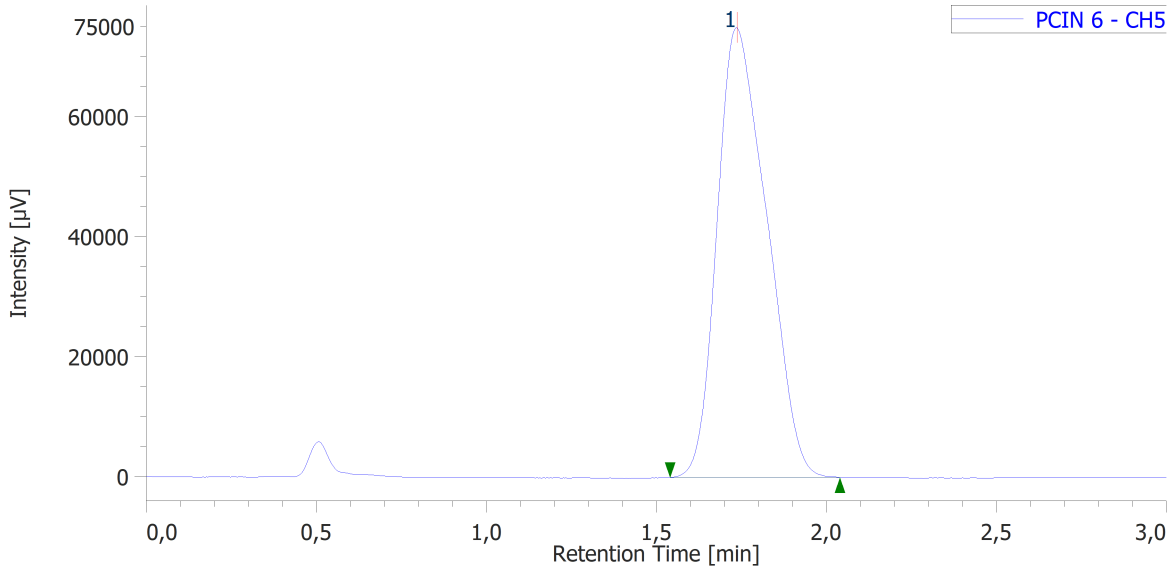

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:15:59
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:12:57
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,737	760411	74858	100,000	100,000	N/A	606	N/A	1,269	

Creator Administrator
Reviewer
Approver

Chromatogram

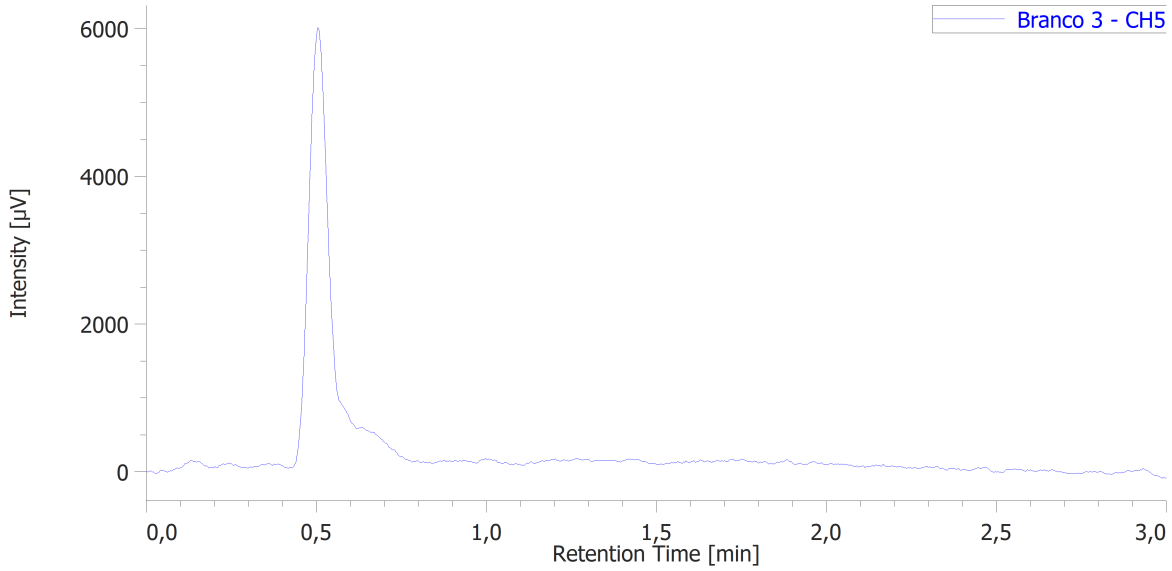


Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:19:11
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:16:09
Volume	10,00 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

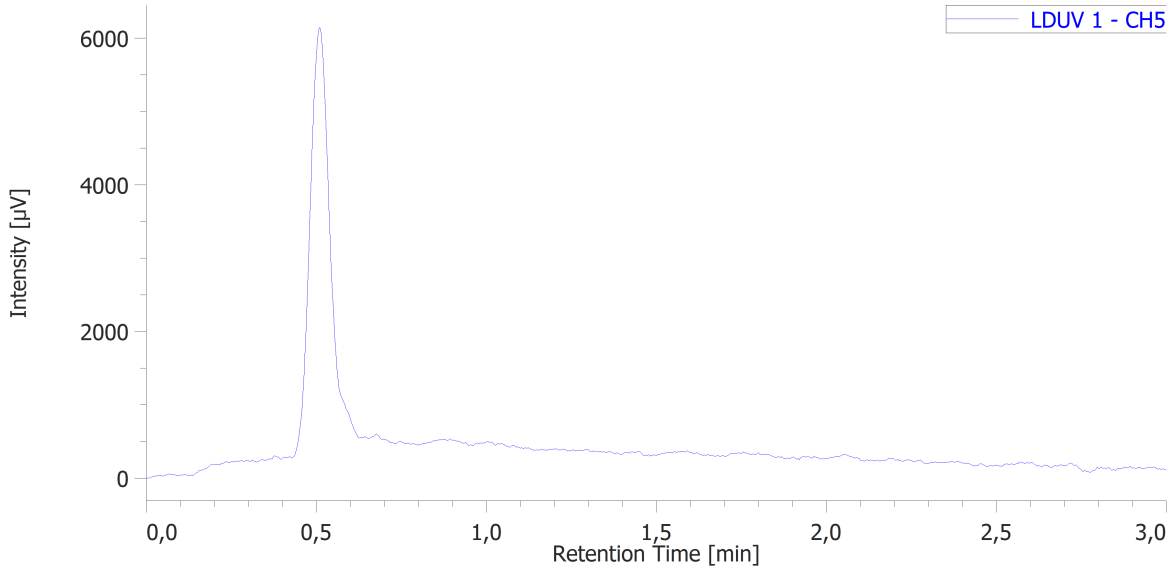


Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:25:03
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:22:00
Volume	10,00 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

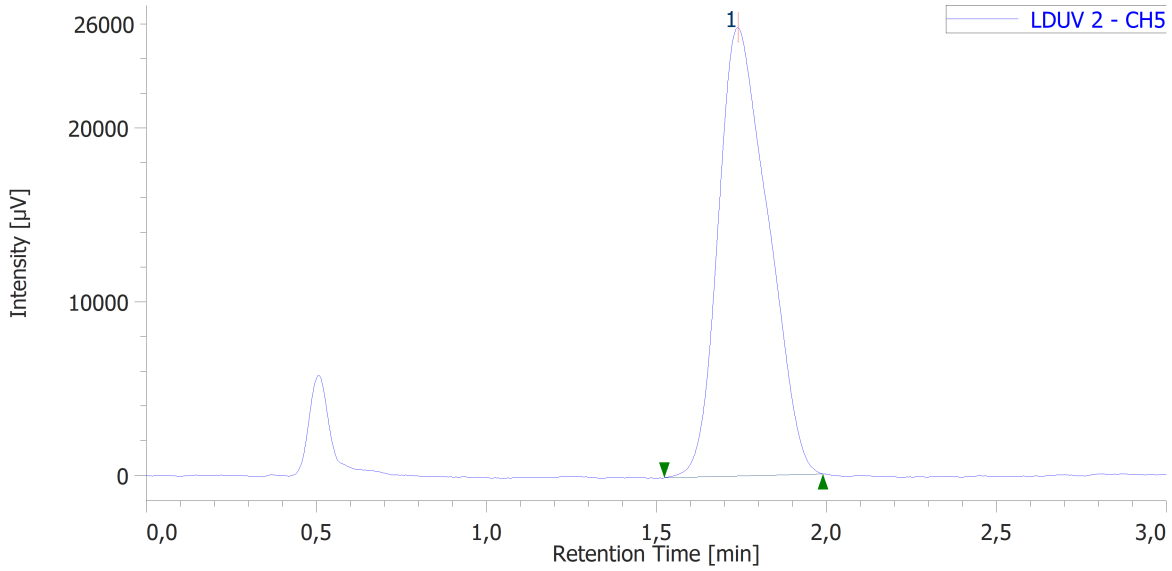

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:28:15
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:25:12
Volume	10,00 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,740	262883	25791	100,000	100,000	N/A	606	N/A	1,251	

Creator Administrator
Reviewer
Approver

Chromatogram

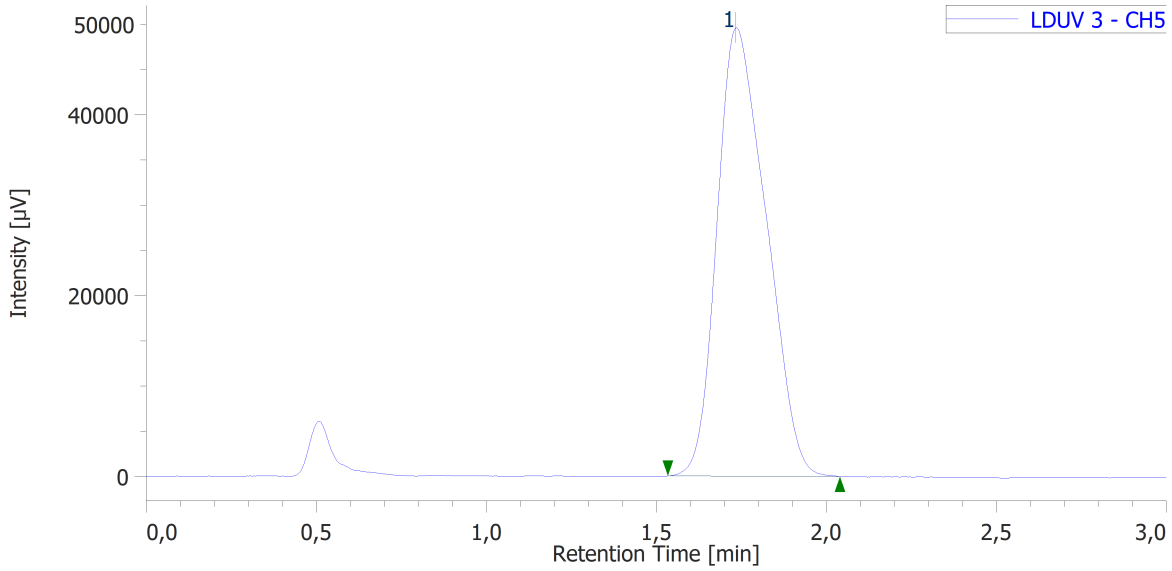

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:31:27
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:28:24
Volume	10,00 [µL]
Sample #	53
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,733	498189	49564	100,000	100,000	N/A	623	N/A	1,286	

Creator Administrator
Reviewer
Approver

Chromatogram

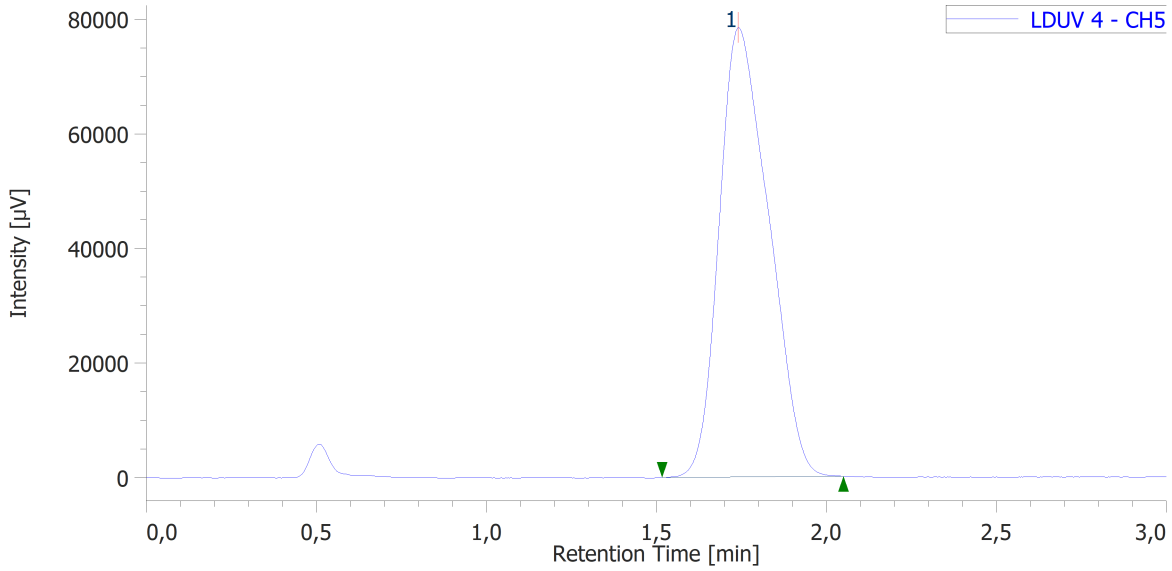

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:34:39
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:31:36
Volume	10,00 [µL]
Sample #	54
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,740	795762	78379	100,000	100,000	N/A	612	N/A	1,285	

Creator Administrator
Reviewer
Approver

Chromatogram

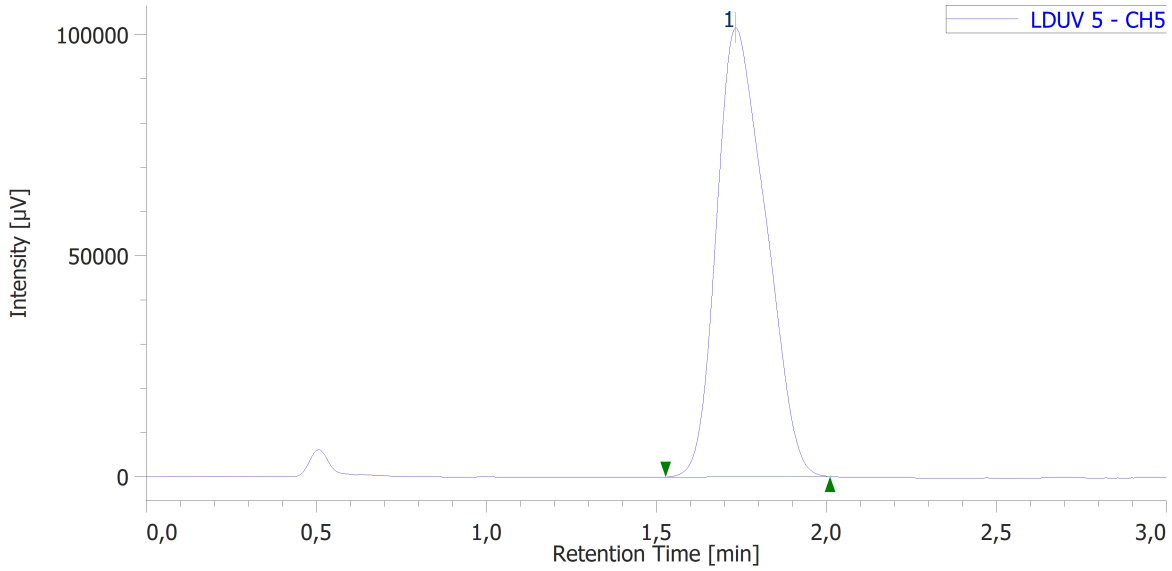

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:40:13
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:34:48
Volume	10,00 [µL]
Sample #	55
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,733	1018526	101559	100,000	100,000	N/A	623	N/A	1,270	

Creator Administrator
Reviewer
Approver

Chromatogram

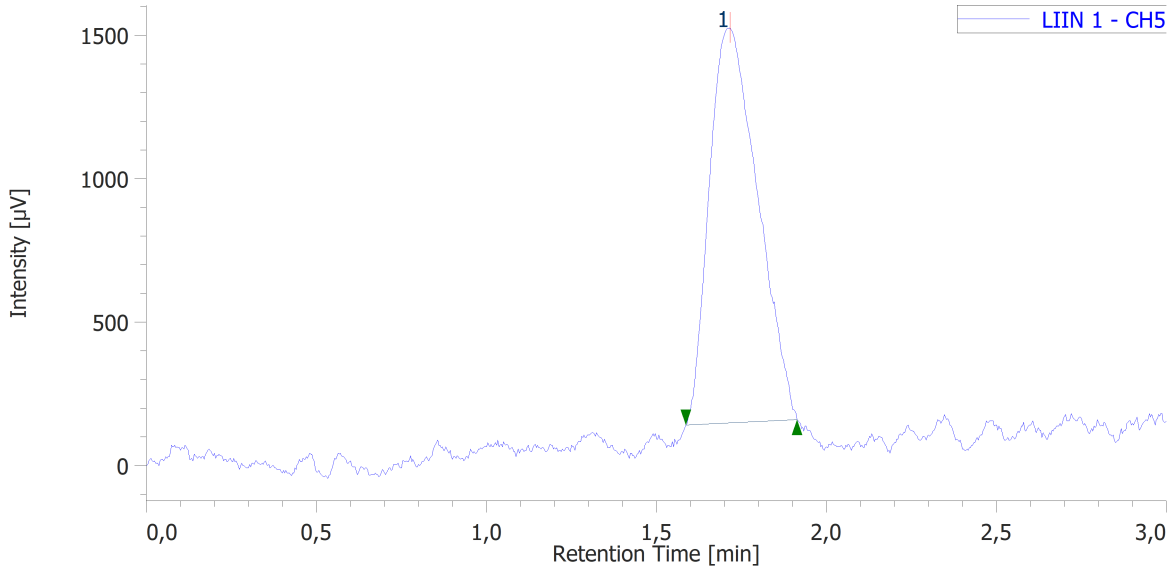

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:45:59
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:42:57
Volume	0,10 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,717	13608	1376	100,000	100,000	N/A	600	N/A	1,282	

Creator Administrator
Reviewer
Approver

Chromatogram

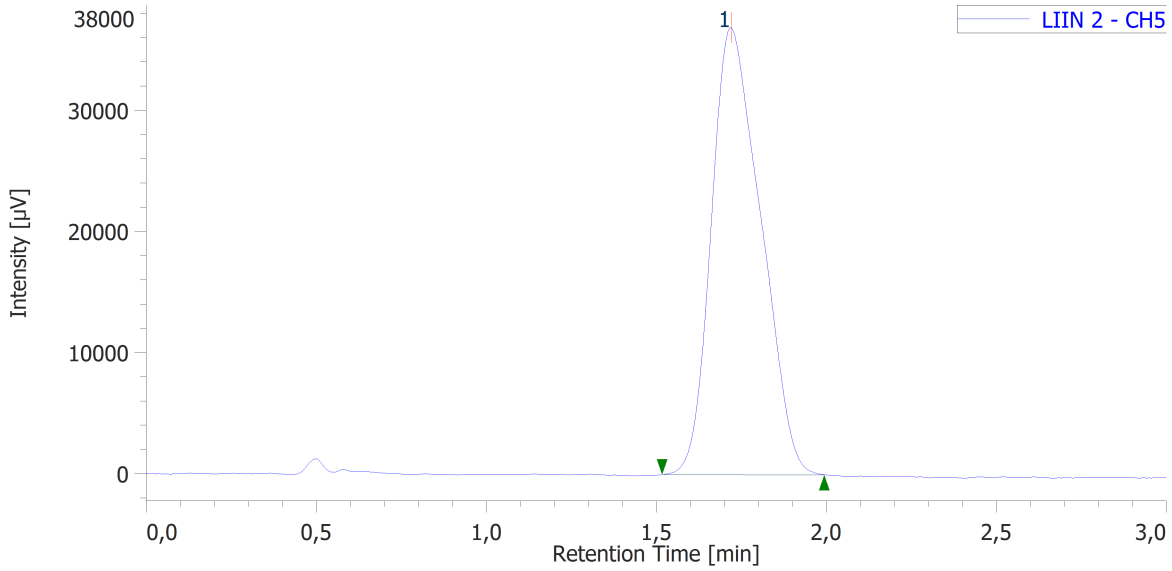

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:49:11
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:46:09
Volume	5,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,720	373422	36898	100,000	100,000	N/A	602	N/A	1,248	

Creator Administrator
Reviewer
Approver

Chromatogram

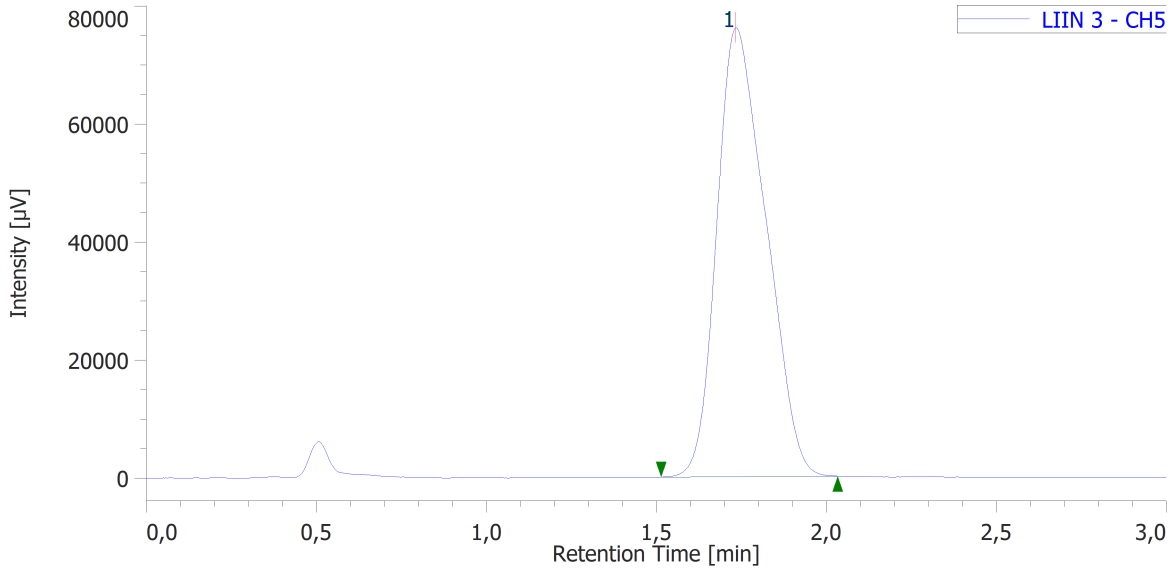

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:52:23
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:49:21
Volume	10,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,733	762794	76022	100,000	100,000	N/A	629	N/A	1,283	

Creator Administrator
Reviewer
Approver

Chromatogram

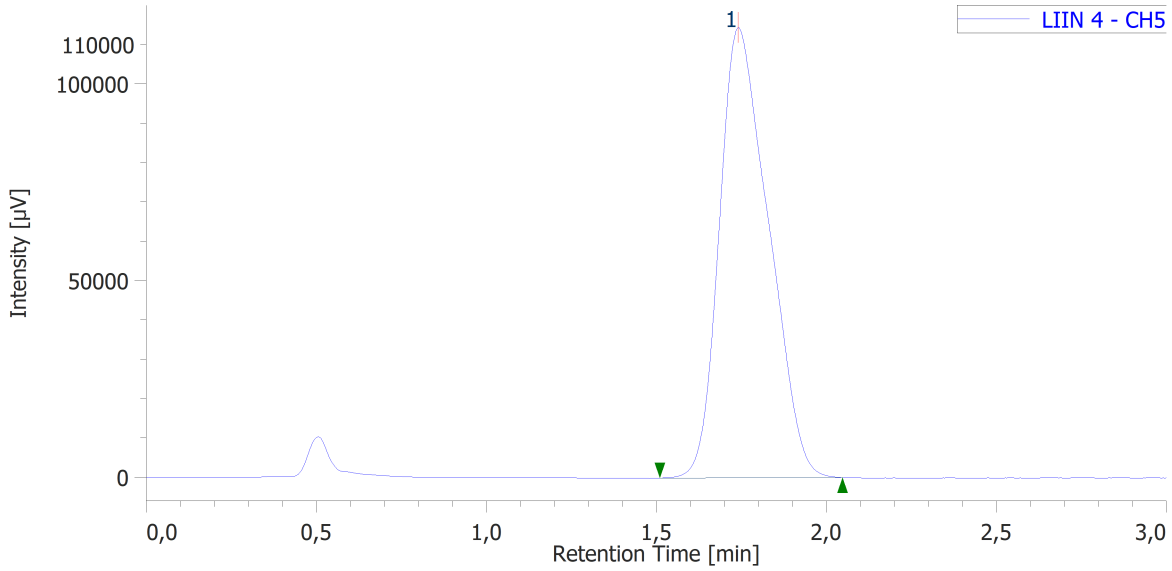

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:55:35
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:52:33
Volume	15,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,740	1151356	114351	100,000	100,000	N/A	633	N/A	1,310	

Creator Administrator
Reviewer
Approver

Chromatogram

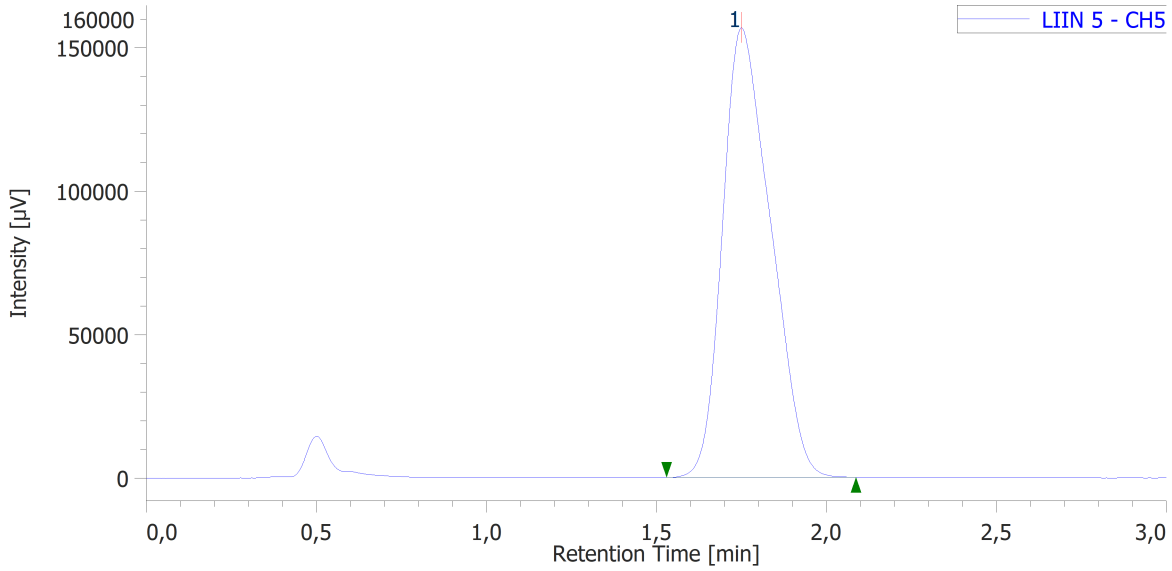

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 10:58:47
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 10:55:45
Volume	20,00 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação 4000
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,750	1541266	156649	100,000	100,000	N/A	677	N/A	1,281	

Creator Administrator
Reviewer
Approver

Chromatogram

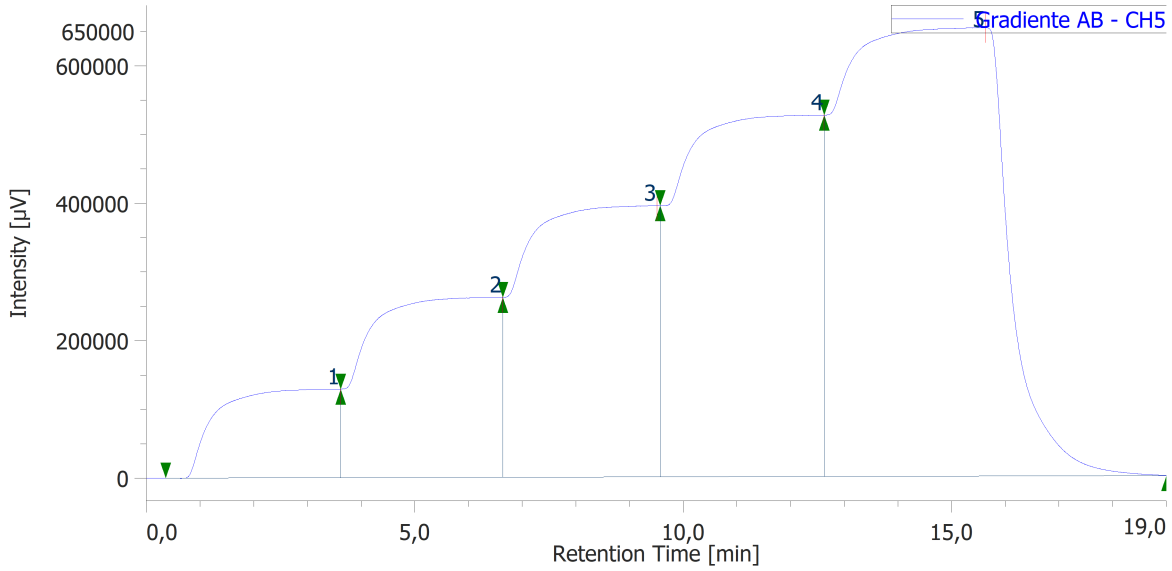

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 12:15:46
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 11:56:45
Volume	0,10 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Gradiente
Control Method	Grad AB 4000
Peak ID Table	Grad
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	3,610	18720731	128926	5,290	6,570	N/A	N/A	N/A	N/A	
2	40 %	5	6,633	43006462	261609	12,153	13,332	N/A	N/A	N/A	N/A	
3	60 %	5	9,510	65045404	394356	18,381	20,097	N/A	N/A	N/A	N/A	
4	80 %	5	12,617	91609470	525394	25,887	26,775	N/A	N/A	N/A	N/A	
5	100 %	5	15,630	135496695	651956	38,289	33,225	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

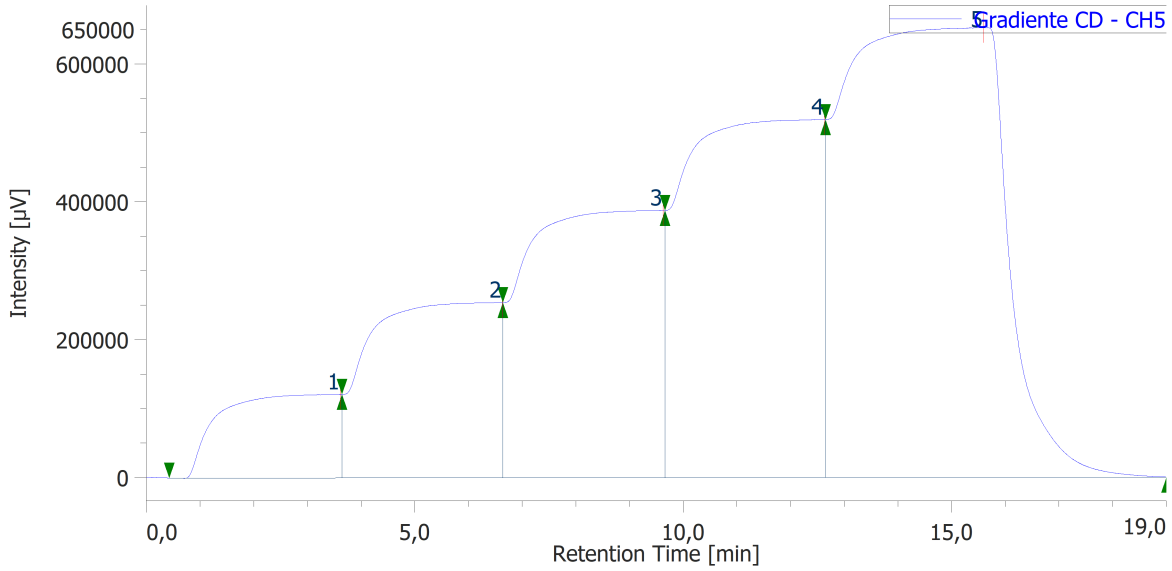

Chromatogram Information	
User Name	Administrator
Date Modified	27/04/2021 12:37:23
Description	
HPLC System Name	01-HP-03
Injection Date	27/04/2021 12:15:57
Volume	0,10 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	Gradiente
Control Method	Grad CD 4000
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	3,610	17690294	120860	5,076	6,254	N/A	N/A	N/A	N/A	
2	40 %	5	6,623	41344146	253843	11,863	13,136	N/A	N/A	N/A	N/A	
3	60 %	5	9,620	65878008	387221	18,903	20,039	N/A	N/A	N/A	N/A	
4	80 %	5	12,623	88850353	518703	25,495	26,843	N/A	N/A	N/A	N/A	
5	100 %	5	15,590	134736901	651738	38,662	33,727	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver