
Chromatogram

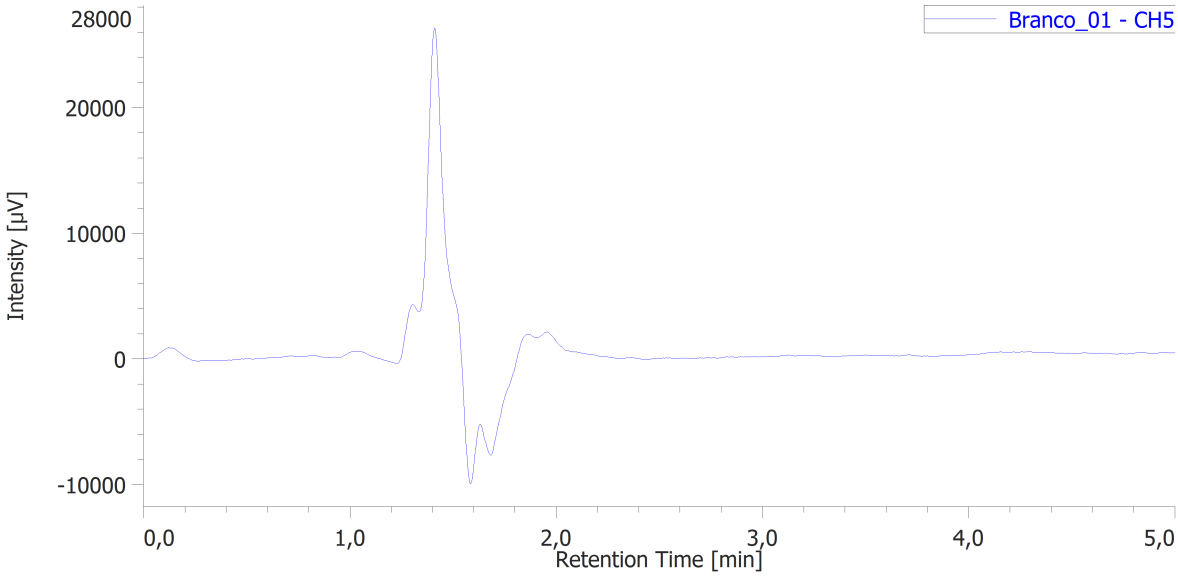


Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:24:59
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:19:58
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator
Reviewer
Approver

Chromatogram

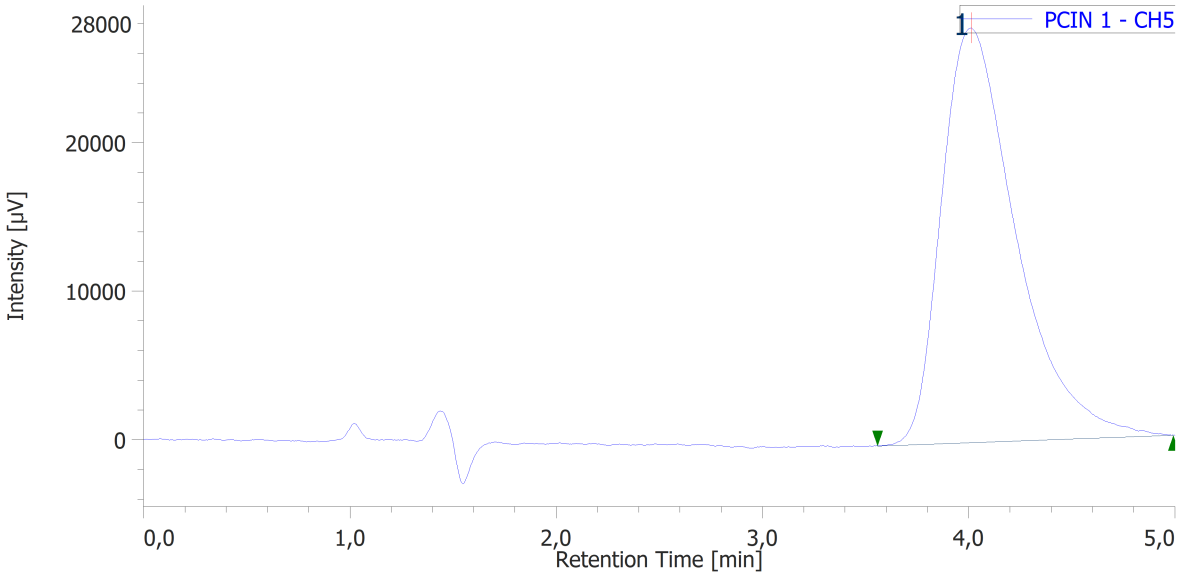

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:30:11
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:25:10
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,010	703933	27896	100,000	100,000	N/A	627	N/A	1,574	

Creator
Reviewer
Approver

Chromatogram

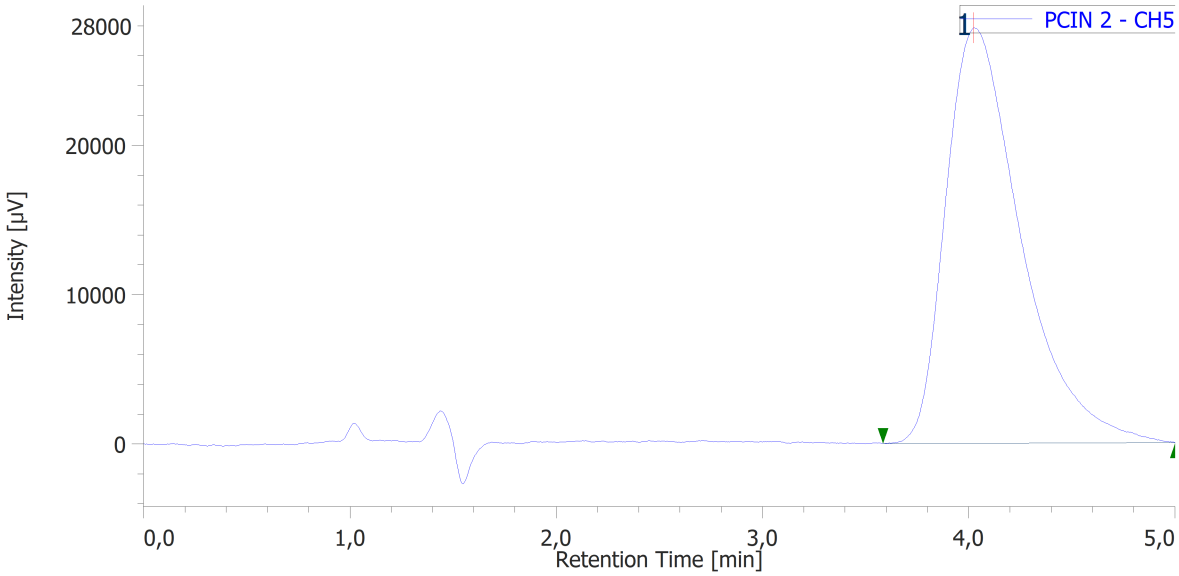

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:35:23
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:30:22
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,023	704282	27794	100,000	100,000	N/A	627	N/A	1,636	

Creator
Reviewer
Approver

Chromatogram

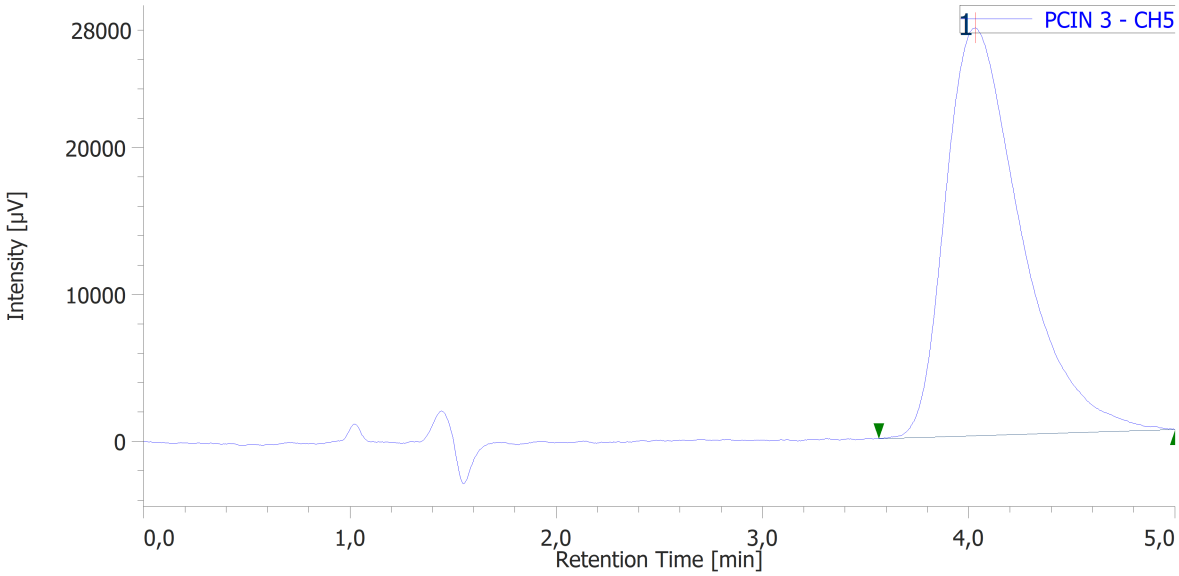

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:40:35
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:35:34
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,030	706415	27736	100,000	100,000	N/A	617	N/A	1,570	

Creator
Reviewer
Approver

Chromatogram

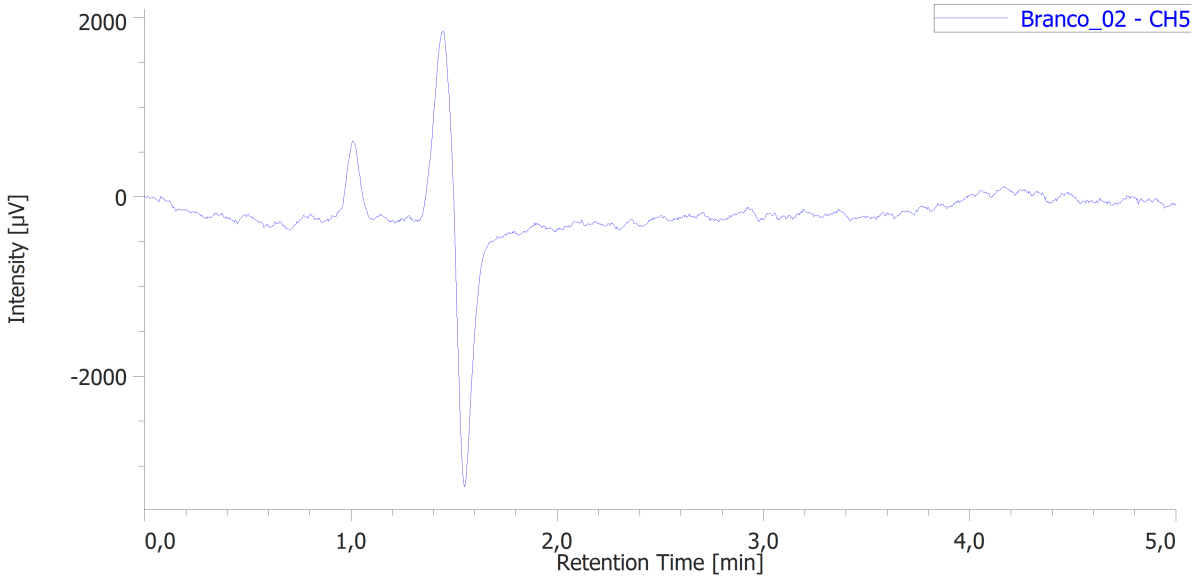


Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:06:35
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:40:27
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

C	Branco_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator
Reviewer
Approver

Chromatogram

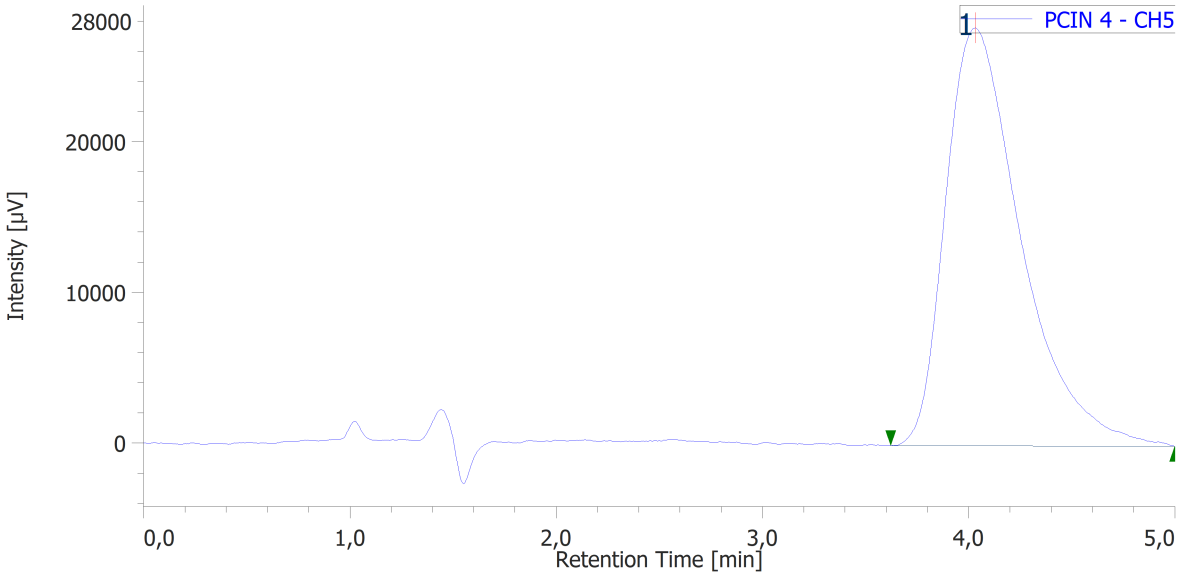

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:50:59
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:45:58
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,030	705398	27720	100,000	100,000	N/A	626	N/A	1,578	

Creator
Reviewer
Approver

Chromatogram

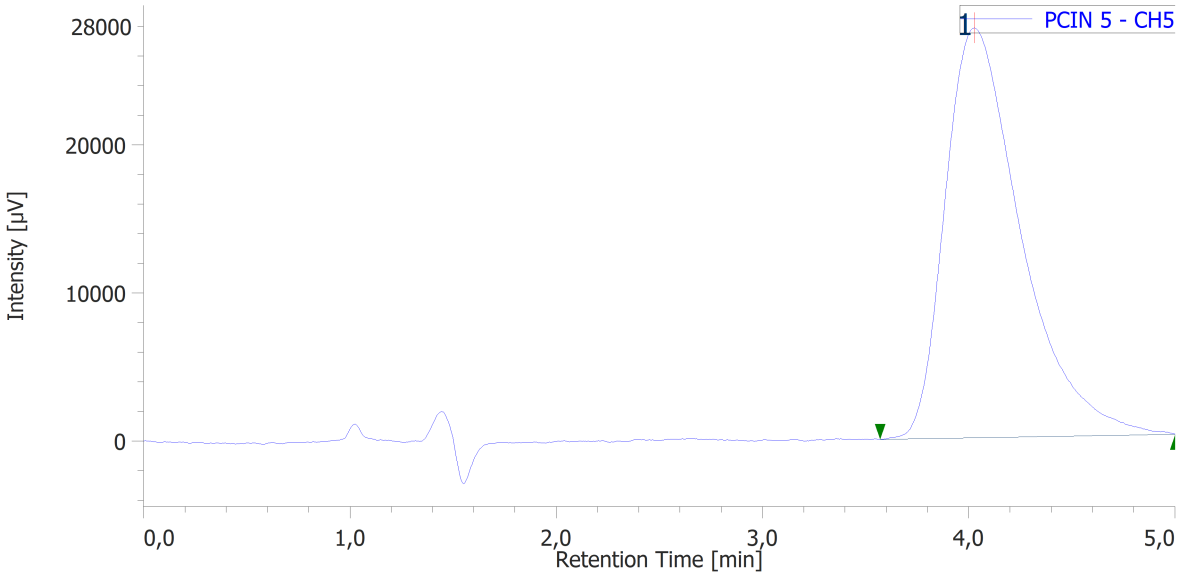

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 12:56:11
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:51:10
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,027	707281	27633	100,000	100,000	N/A	616	N/A	1,586	

Creator
Reviewer
Approver

Chromatogram

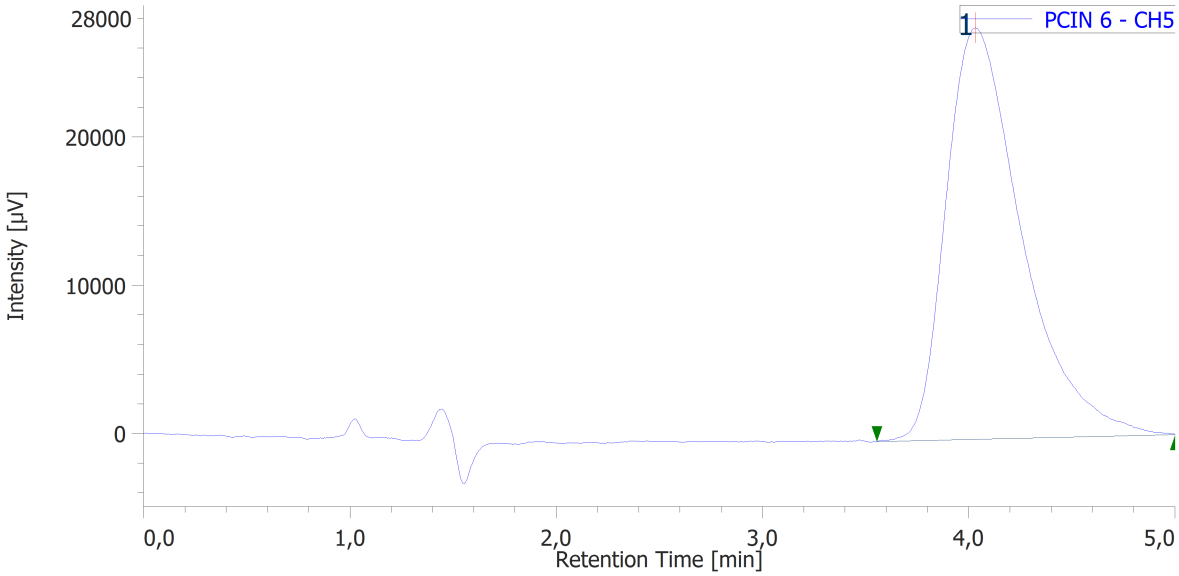

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:01:23
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 12:56:22
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,030	708662	27722	100,000	100,000	N/A	619	N/A	1,607	

Creator
Reviewer
Approver

Chromatogram

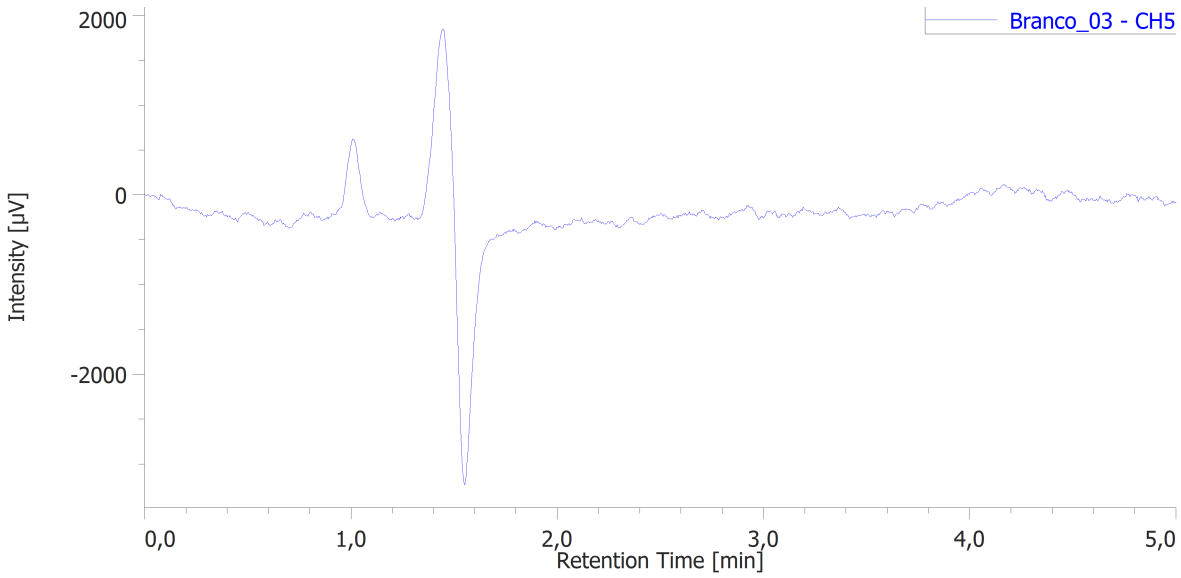


Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:06:35
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:01:34
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator
Reviewer
Approver

Chromatogram

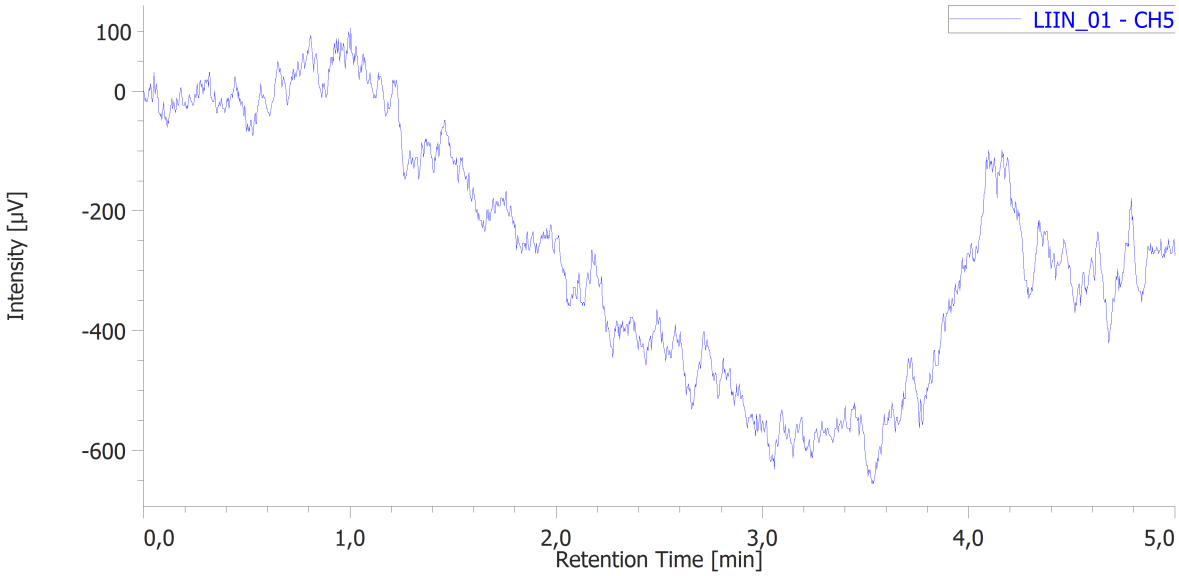


Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:11:47
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:06:46
Volume	0,1 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

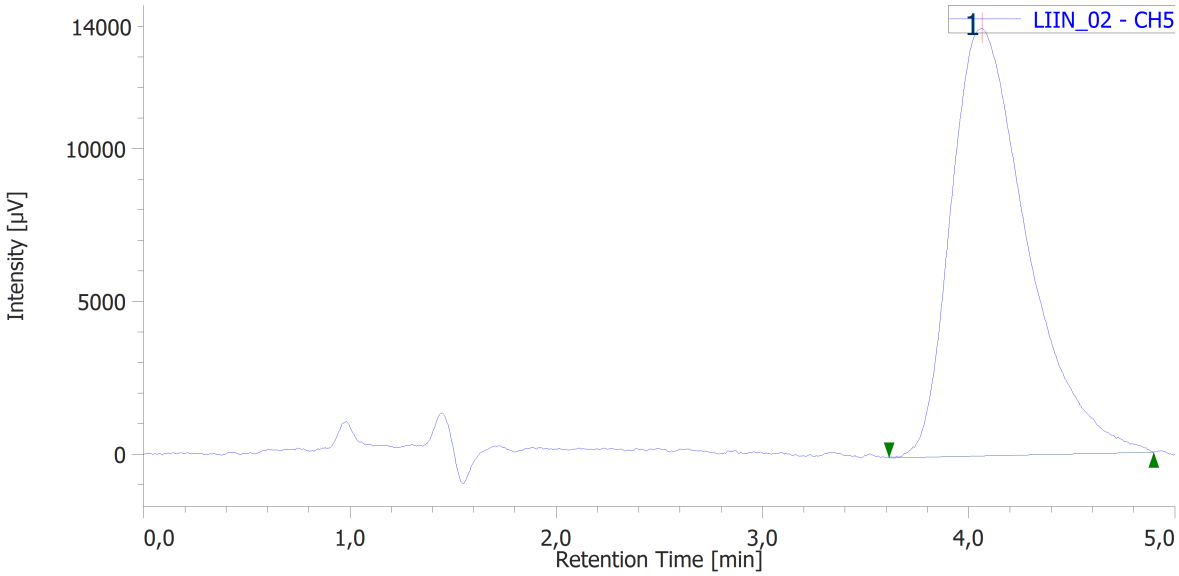

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:16:59
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:11:58
Volume	5,0 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,063	359291	14003	100,000	100,000	N/A	616	N/A	1,512	

Creator
Reviewer
Approver

Chromatogram

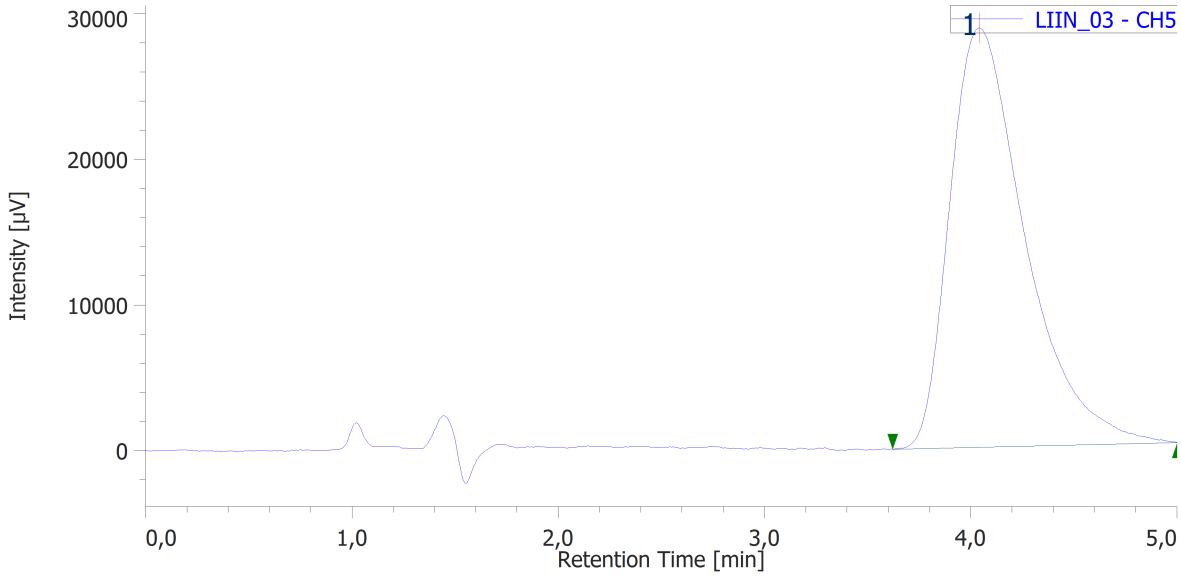

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:22:11
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:17:10
Volume	10,0 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,040	730347	28757	100,000	100,000	N/A	626	N/A	1,608	

Creator
Reviewer
Approver

Chromatogram

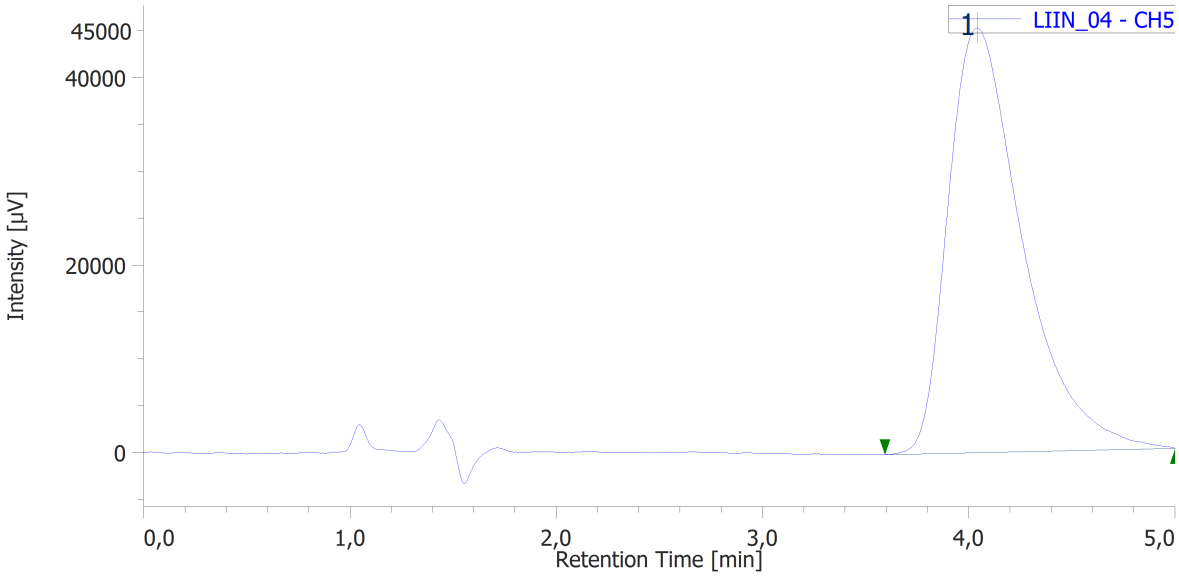

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:27:23
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:22:22
Volume	15,0 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,040	1137001	45311	100,000	100,000	N/A	643	N/A	1,601	

Creator
Reviewer
Approver

Chromatogram

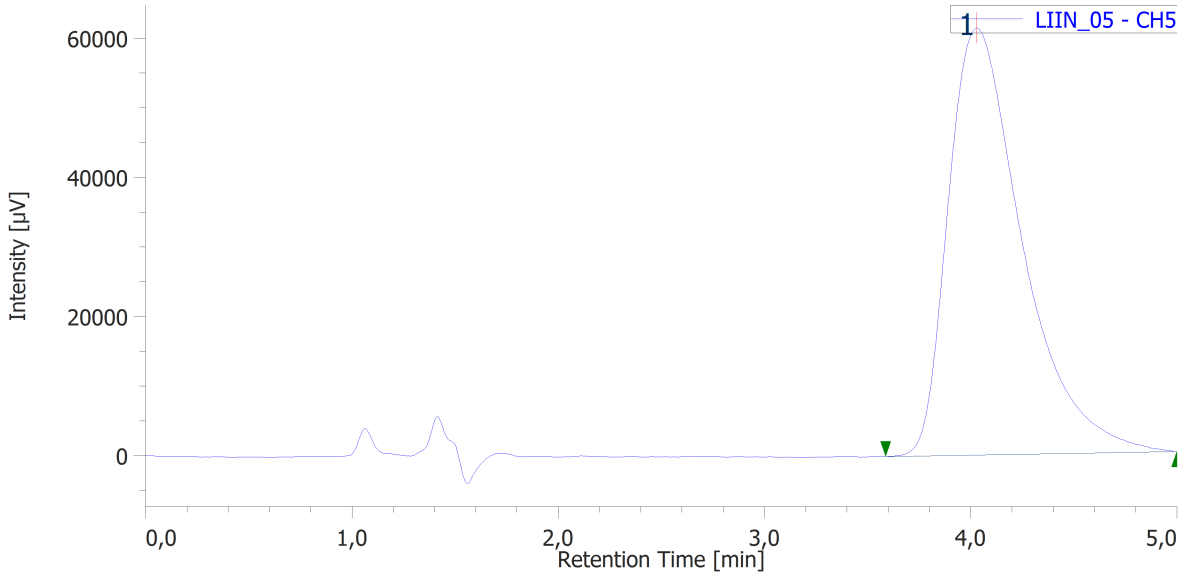

Chromatogram Information	
User Name	QPackSA
Date Modified	12/12/2023 13:32:35
Description	
HPLC System Name	01-HP-03
Injection Date	12/12/2023 13:27:34
Volume	20,0 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,027	1532835	61356	100,000	100,000	N/A	643	N/A	1,654	

Creator
Reviewer
Approver