
Area Percent Report

EDUV

Data file:	C:\Chemstation\2\Data\EDUV 2024-12-16 09-18-33\001-P1-A1-EDUV.D		
Sample name:	EDUV		
Description:	EDUV		
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	LC-1260	**Location:**	P1-A1
Injection date:	2024-12-16 09:19:34-03:00	**Injection:**	1 of 1
Acq. method:	QUALIFICAÇÃO.M	**Injection volume:**	10.000
Analysis method:	QUALIFICAÇÃO.M	**Acq. operator:**	SYSTEM
Last changed:	2024-12-16 08:45:35-03:00		

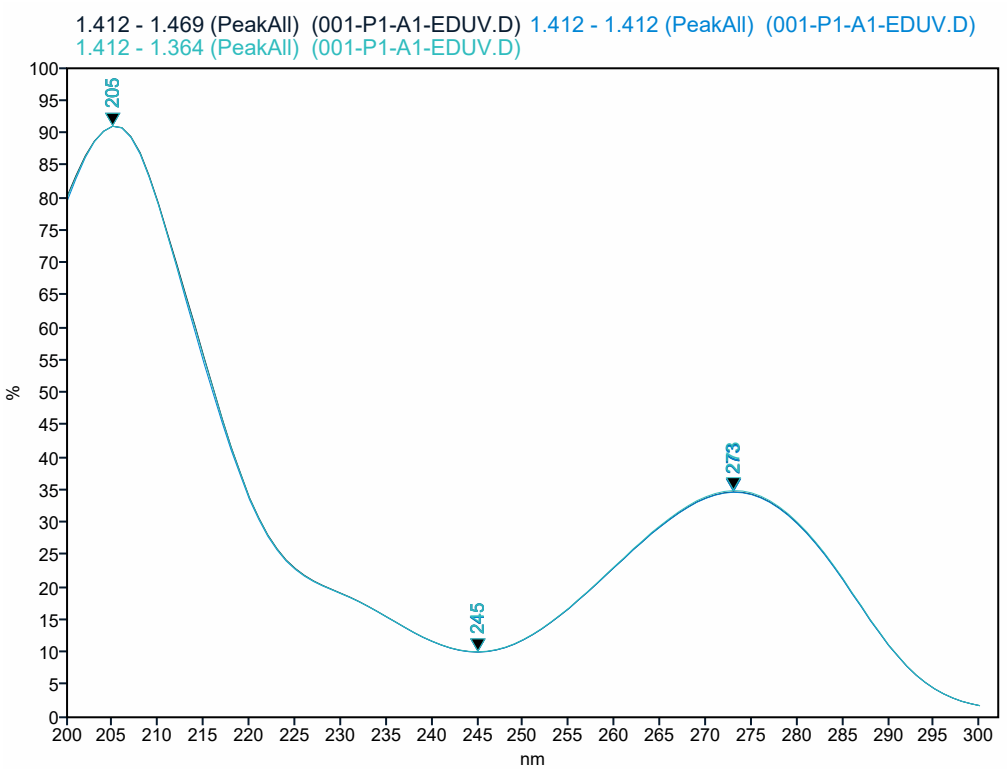


Signal: DAD1 A, Sig=273,4 Ref=360,100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
1.412	BB	0.0786	723.3008	140.4082	100.0000	
		Sum	723.3008			

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\001-P1-A1-Branco 1.D
Sample Name: Branco 1

==========

Acq. Operator	: SYSTEM	Seq. Line :	1
Sample Operator	: SYSTEM		
Acq. Instrument	: LC-1260	Location :	P1-A-01
Injection Date	: 12/16/2024 9:31:24 AM	Inj :	1
		Inj Volume :	10.000 µl
Method	: C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)		
Last changed	: 12/16/2024 8:45:35 AM by SYSTEM		

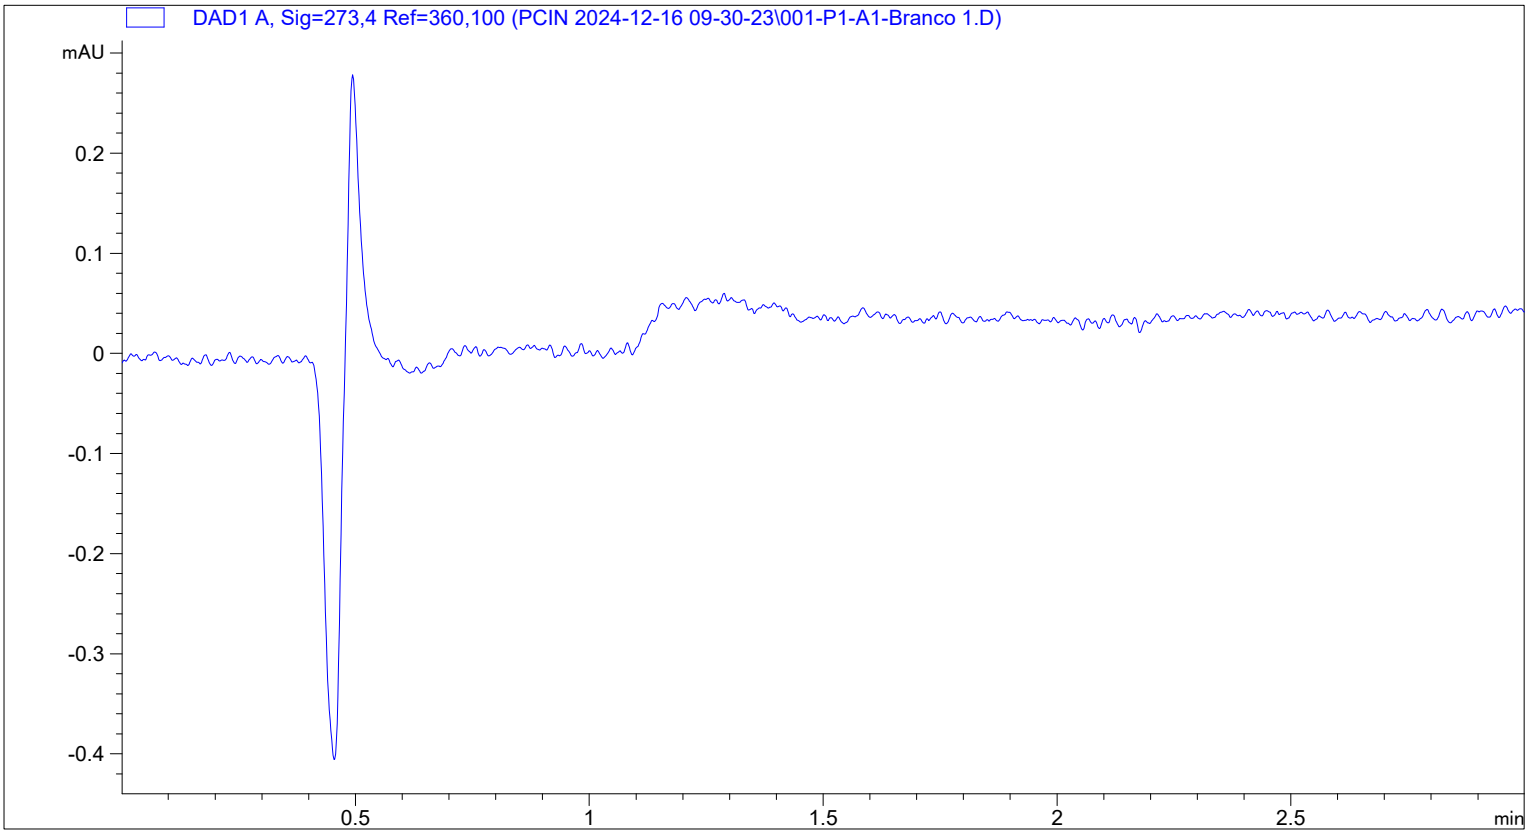

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found


==========

*** End of Report ***

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\002-P1-A2-PCIN 1.D
Sample Name: PCIN 1

==========

Acq. Operator : SYSTEM Seq. Line : 2
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-02
Injection Date : 12/16/2024 9:35:21 AM Inj : 1
Inj Volume : 10.000 µl
Method : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

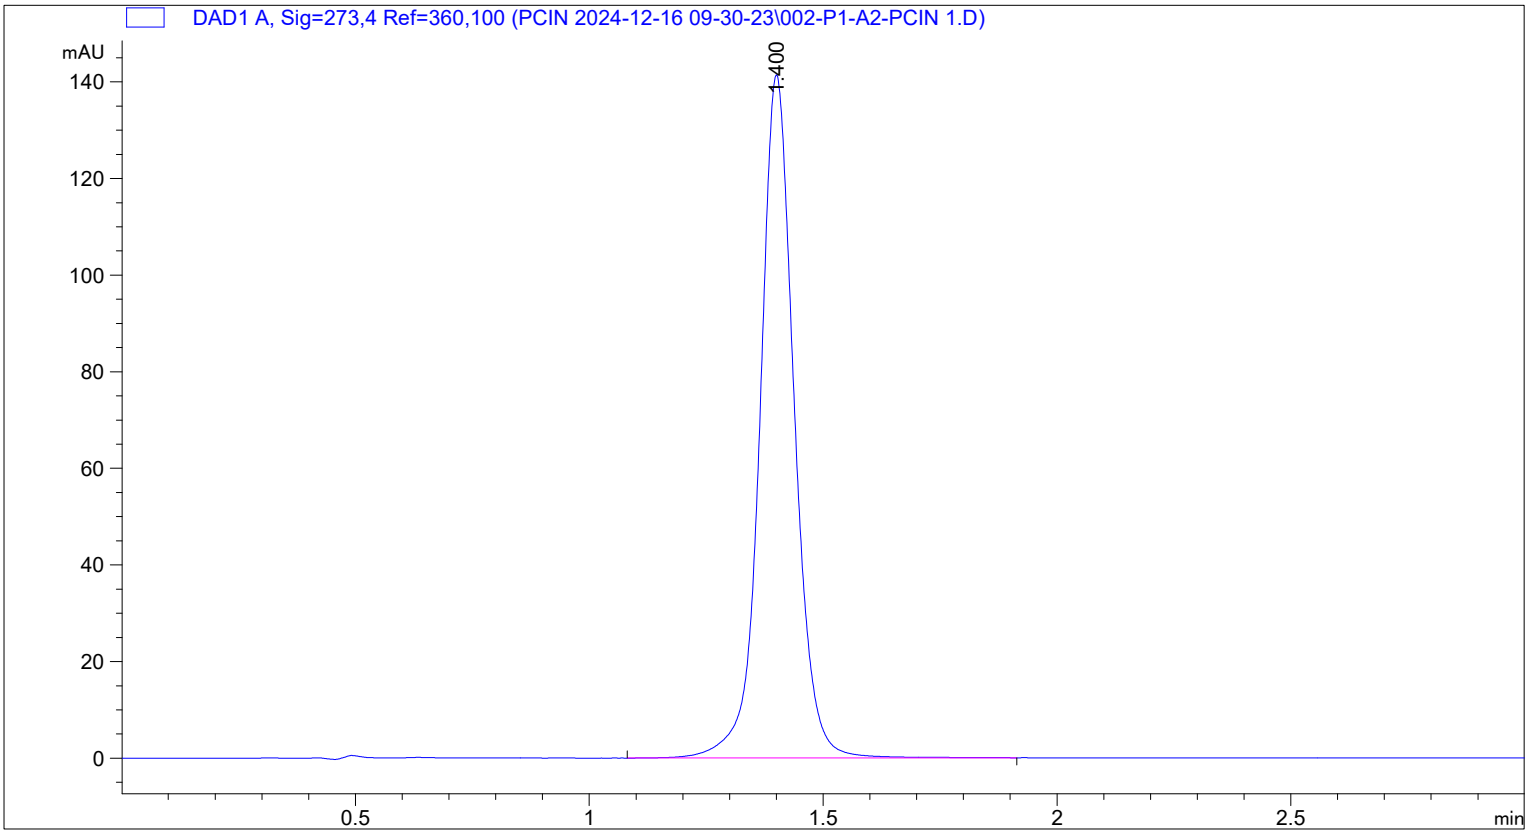

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.400	BB	0.0771	723.02600	141.43298	100.0000
Totals :				723.02600	141.43298	

==========

*** End of Report ***

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\003-P1-A2-PCIN 2.D
Sample Name: PCIN 2

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-02
Injection Date   : 12/16/2024 9:39:19 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

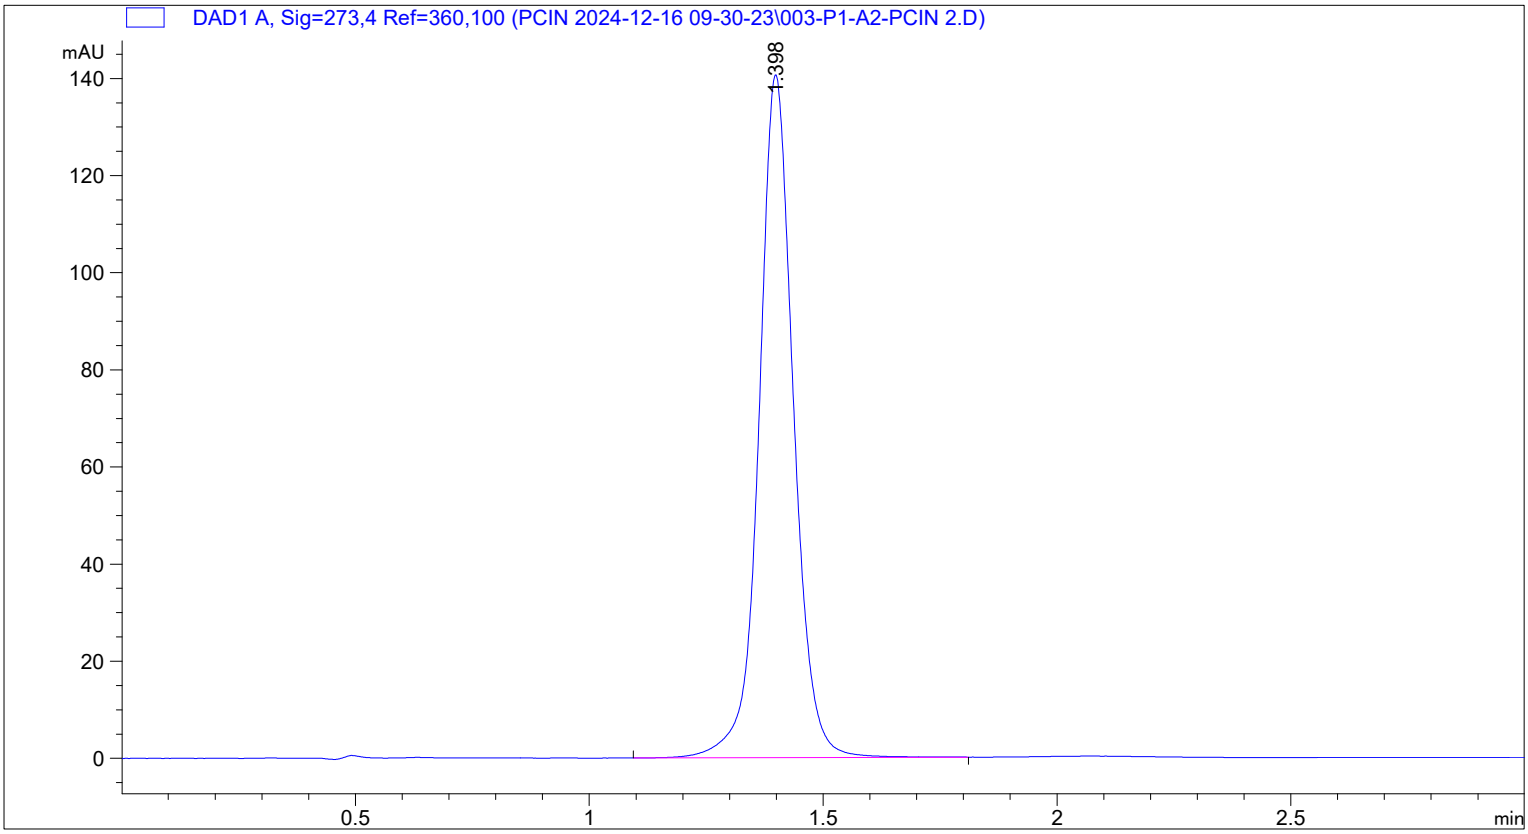


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.398 BB    0.0773  720.81543  140.64192 100.0000

Totals :                   720.81543  140.64192

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\004-P1-A2-PCIN 3.D
Sample Name: PCIN 3

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-02
Injection Date   : 12/16/2024 9:43:15 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

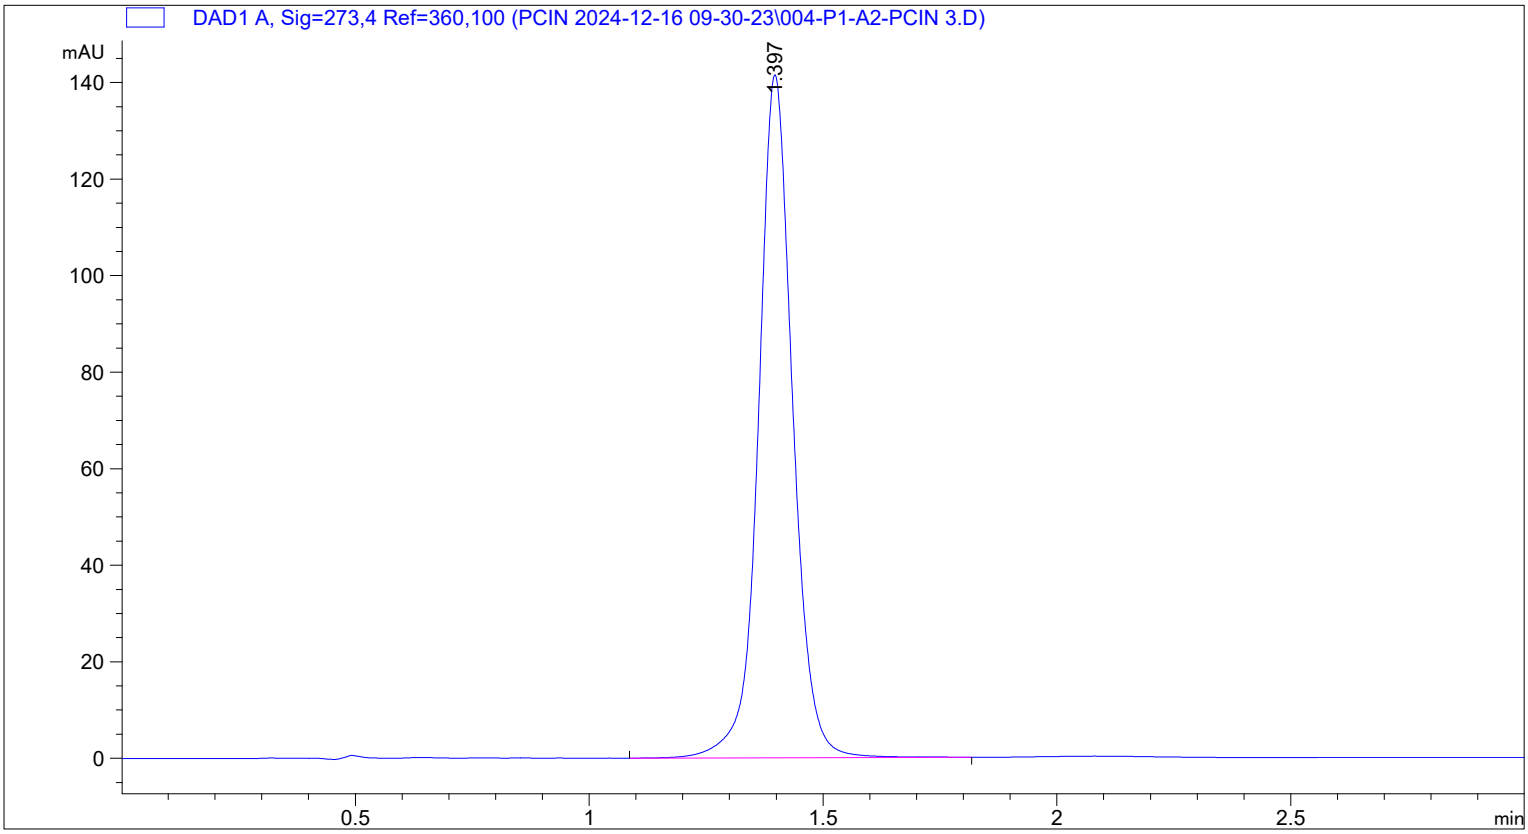


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.397 BB    0.0769  720.64618  141.50133 100.0000

Totals :                   720.64618  141.50133


==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\005-P1-A1-Branco 2.D
Sample Name: Branco 2

==========

Acq. Operator	: SYSTEM	Seq. Line	: 5
Sample Operator	: SYSTEM		
Acq. Instrument	: LC-1260	Location	: P1-A-01
Injection Date	: 12/16/2024 9:47:13 AM	Inj	: 1
		Inj Volume	: 10.000 µl

Method : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

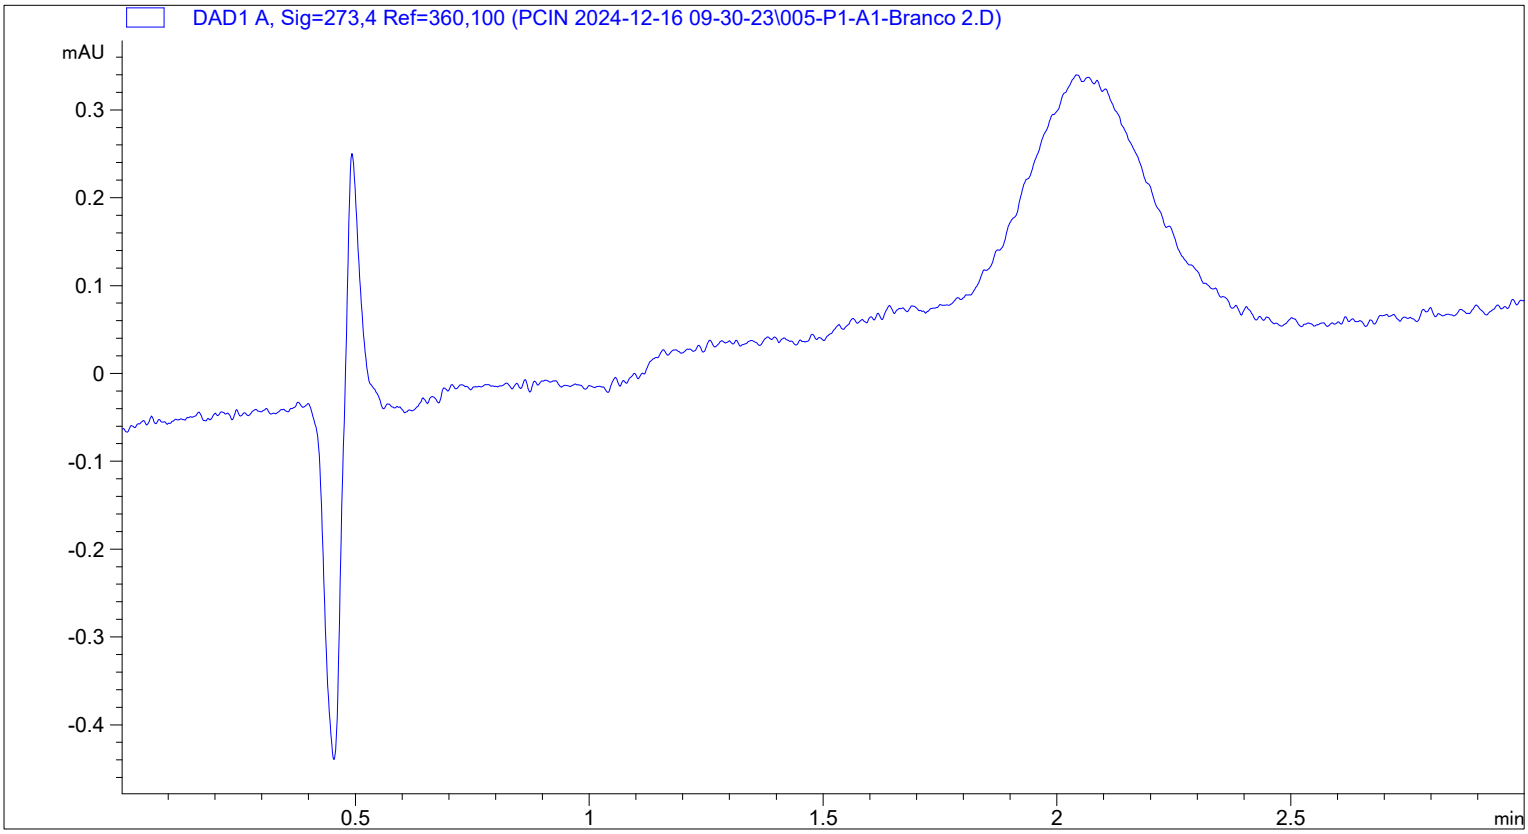

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\006-P1-A2-PCIN 4.D
Sample Name: PCIN 4

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   6
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-02
Injection Date   : 12/16/2024 9:51:10 AM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

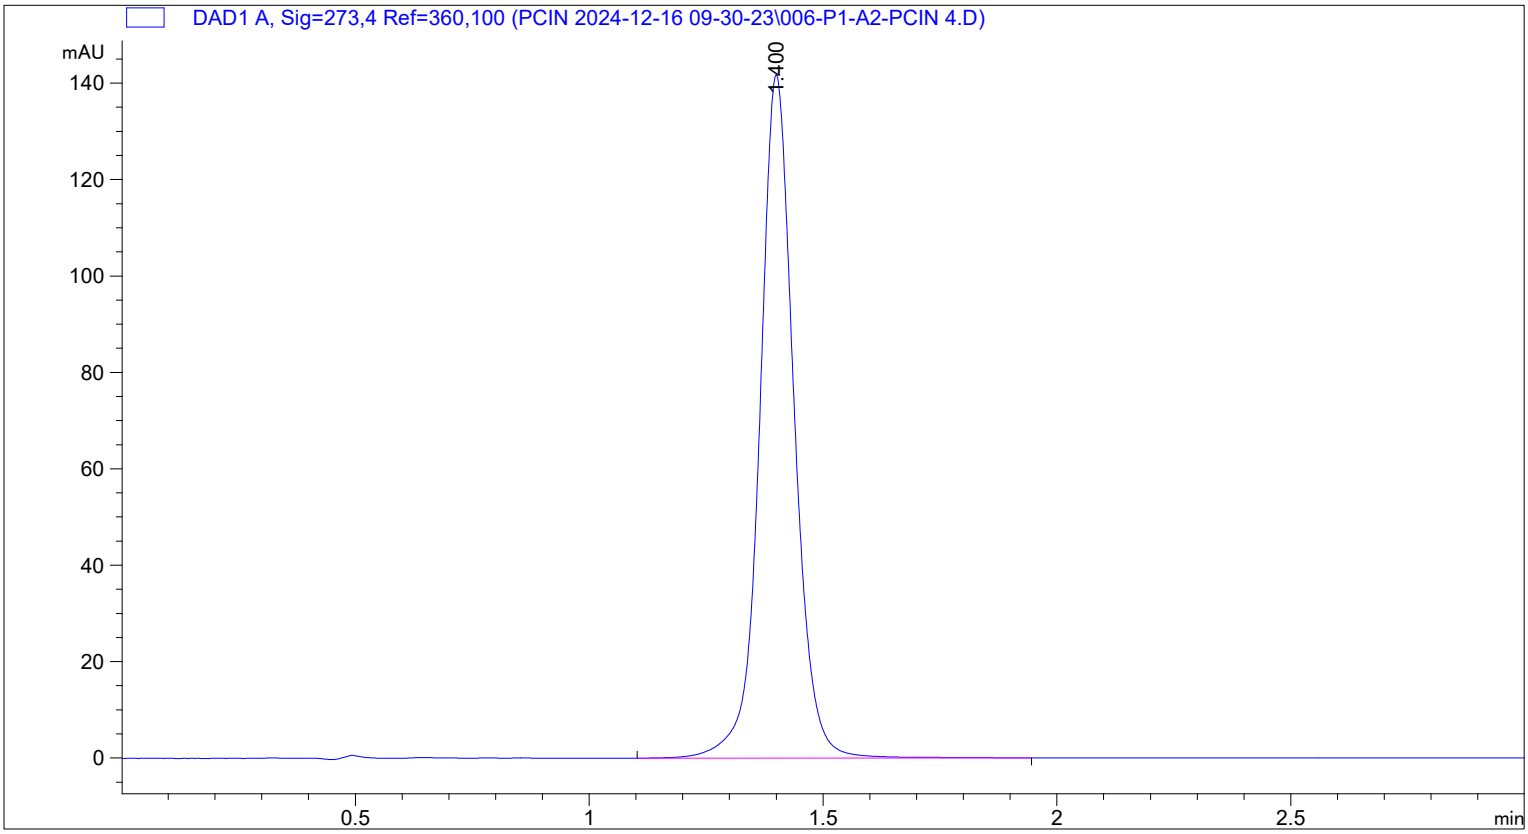


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.400 BB    0.0771  723.56879  141.73630 100.0000


Totals :                   723.56879  141.73630

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\007-P1-A2-PCIN 5.D
Sample Name: PCIN 5

==========

Acq. Operator : SYSTEM Seq. Line : 7
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-02
Injection Date : 12/16/2024 9:55:07 AM Inj : 1
Inj Volume : 10.000 µl
Method : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

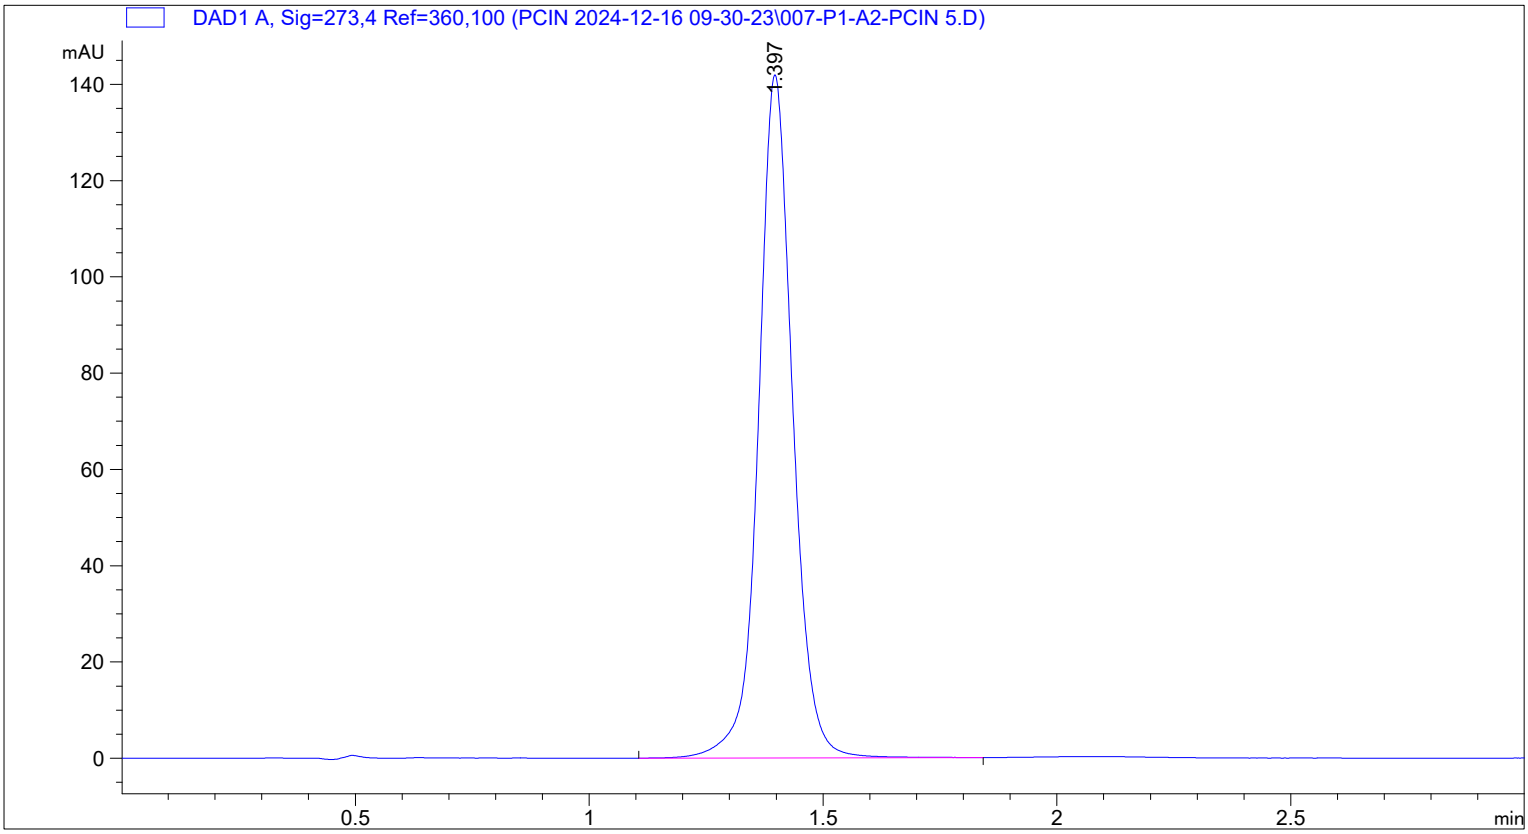

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.397	BB	0.0775	723.17493	141.91644	100.0000
Totals :				723.17493	141.91644	


==========

*** End of Report ***

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\008-P1-A2-PCIN 6.D
Sample Name: PCIN 6

==========

Acq. Operator : SYSTEM Seq. Line : 8
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-02
Injection Date : 12/16/2024 9:59:03 AM Inj : 1
Inj Volume : 10.000 µl
Method : C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

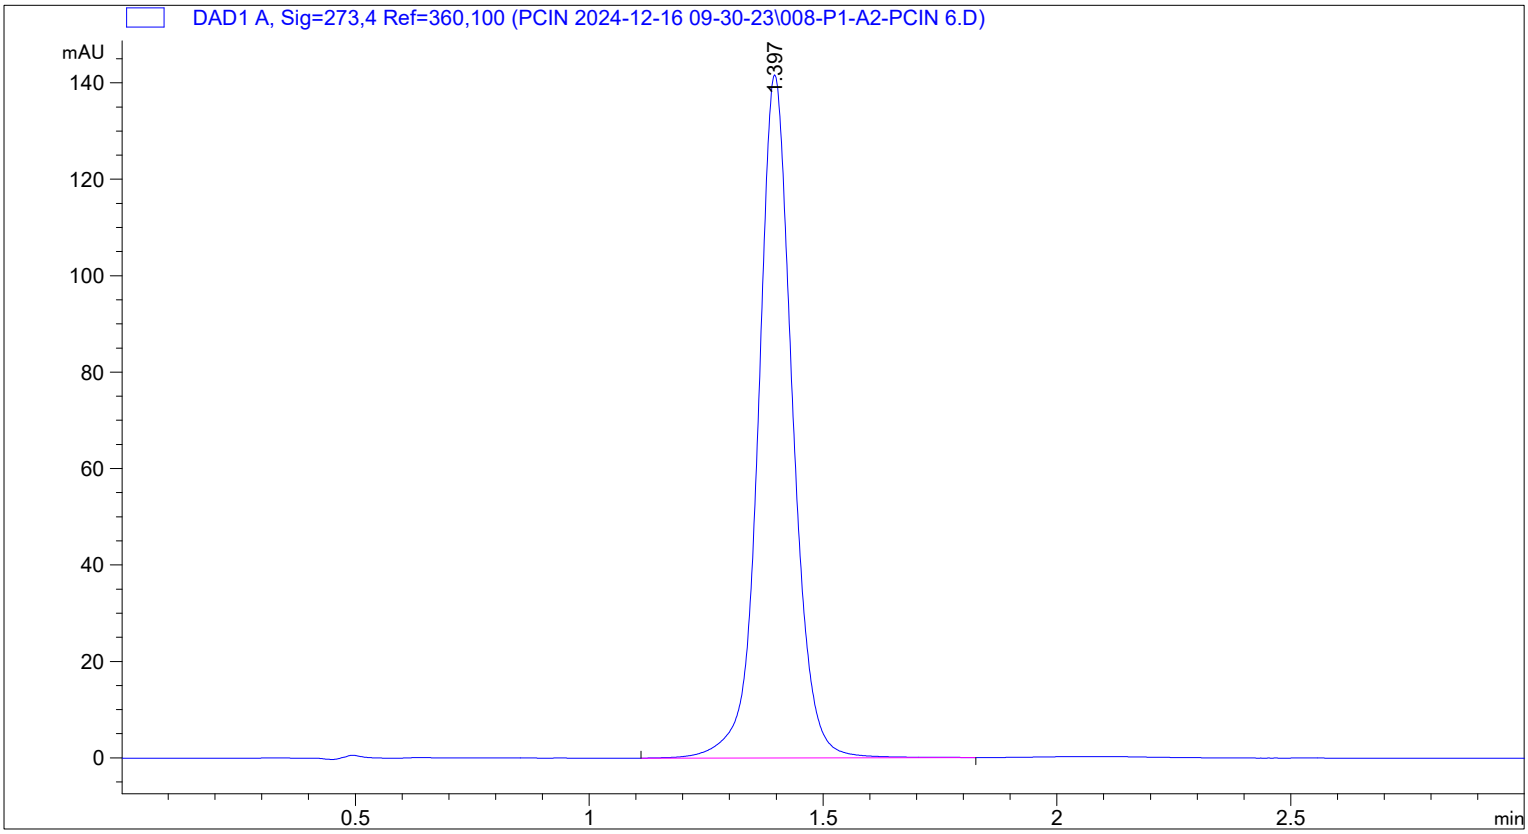

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.397	BB	0.0770	722.68994	141.68279	100.0000
Totals :				722.68994	141.68279	


==========

*** End of Report ***

Data File C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\009-P1-A1-Branco 3.D
Sample Name: Branco 3

==========

Acq. Operator	: SYSTEM	Seq. Line	: 9
Sample Operator	: SYSTEM		
Acq. Instrument	: LC-1260	Location	: P1-A-01
Injection Date	: 12/16/2024 10:03:01 AM	Inj	: 1
		Inj Volume	: 10.000 µl
Method	: C:\Chemstation\2\Data\PCIN 2024-12-16 09-30-23\QUALIFICAÇÃO.M (Sequence Method)		
Last changed	: 12/16/2024 8:45:35 AM by SYSTEM		

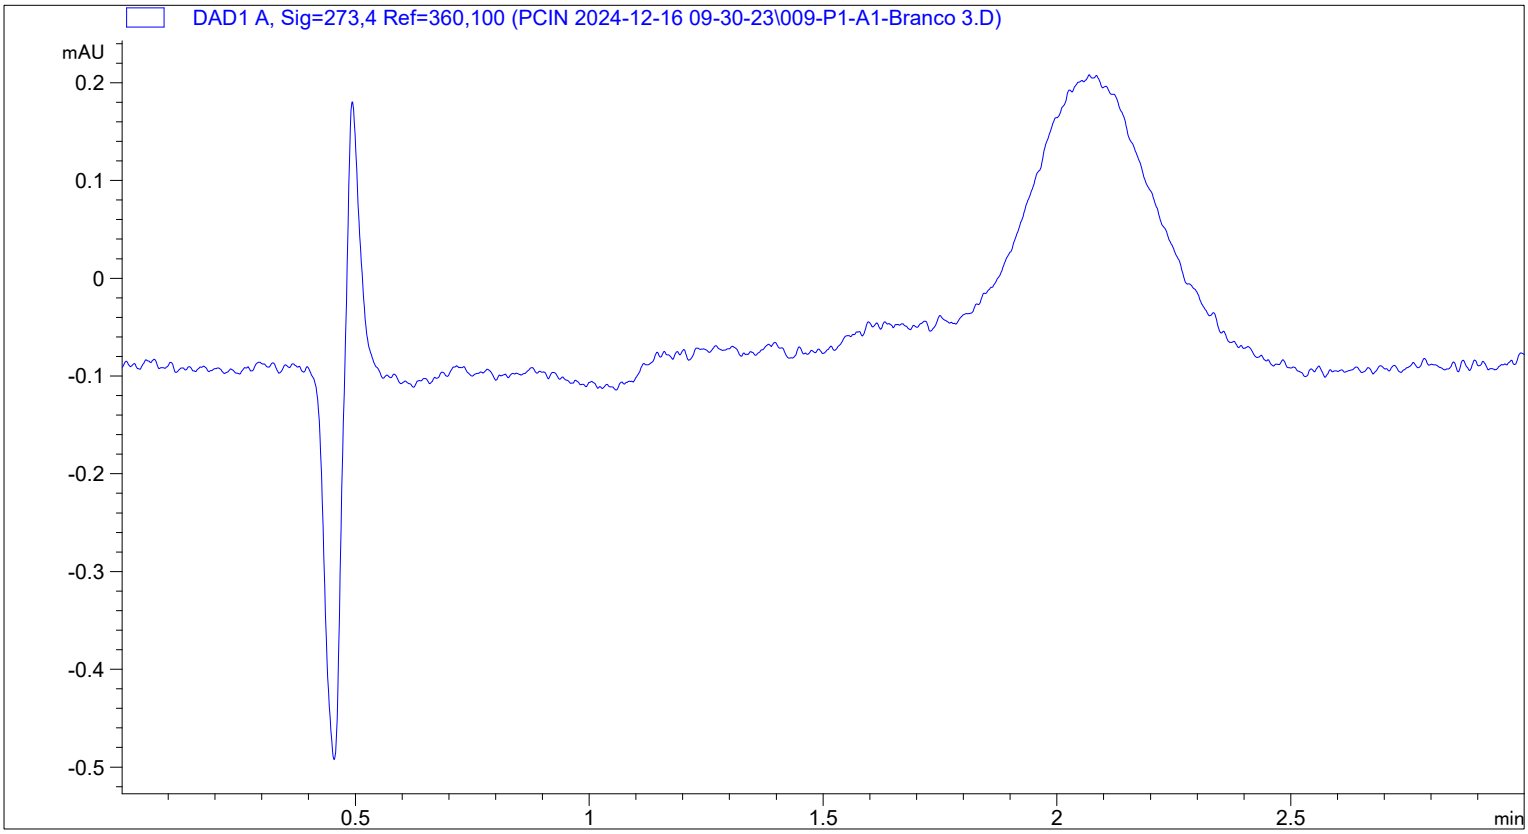

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chemstation\2\Data\Sinal-Ruido 2024-12-16 11-56-07\001-P1-A1-Sinal-Ruido.D
Sample Name: Sinal-Ruido

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Sample Operator : SYSTEM
Acq. Instrument : LC-1260                          Location :   P1-A-01
Injection Date  : 12/16/2024 11:57:09 AM                Inj :   1
                                                  Inj Volume : 20.000 µl
Acq. Method     : C:\Chemstation\2\Data\Sinal-Ruido 2024-12-16 11-56-07\SINAL-RUIDO.M
Last changed    : 12/16/2024 11:52:09 AM by SYSTEM
Analysis Method : C:\Chemstation\2\Data\Sinal-Ruido 2024-12-16 11-56-07\SINAL-RUIDO.M (
                  Sequence Method)
Last changed    : 12/16/2024 12:19:51 PM by SYSTEM
                  (modified after loading)
```

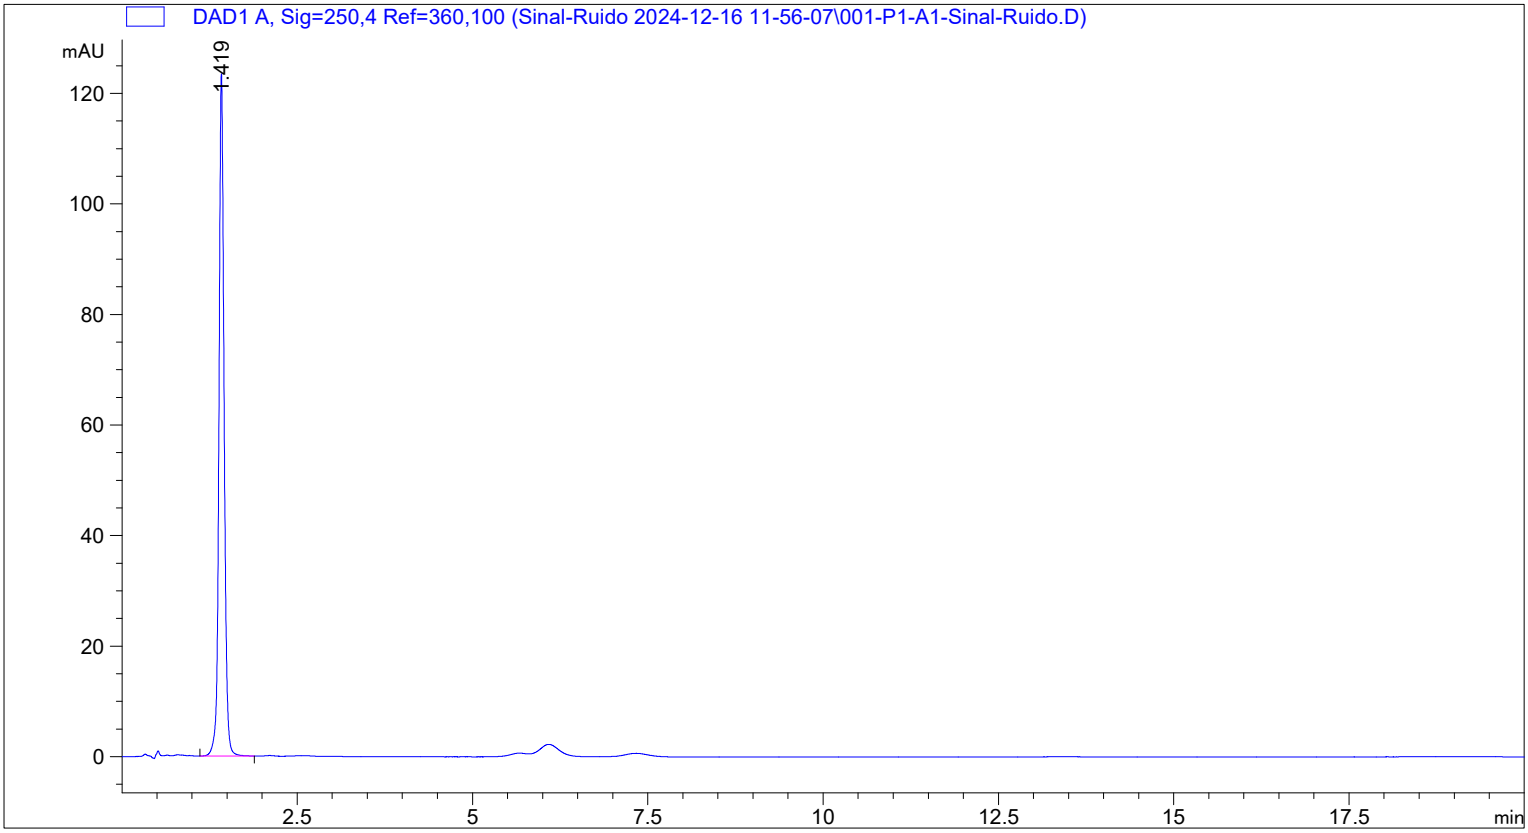


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=250,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.419 BB    0.0780  635.07123  123.41502 100.0000


Totals :                   635.07123  123.41502


==========================================================================
                        *** End of Report ***
```

Certificado Nº: 550/24 - RELB	Início da Qualificação: 16/12/2024	Página 1 de 3

Resultado obtido na altura do pico


	ALTURA DO PICO (mAU)
Resultado:	123.41502

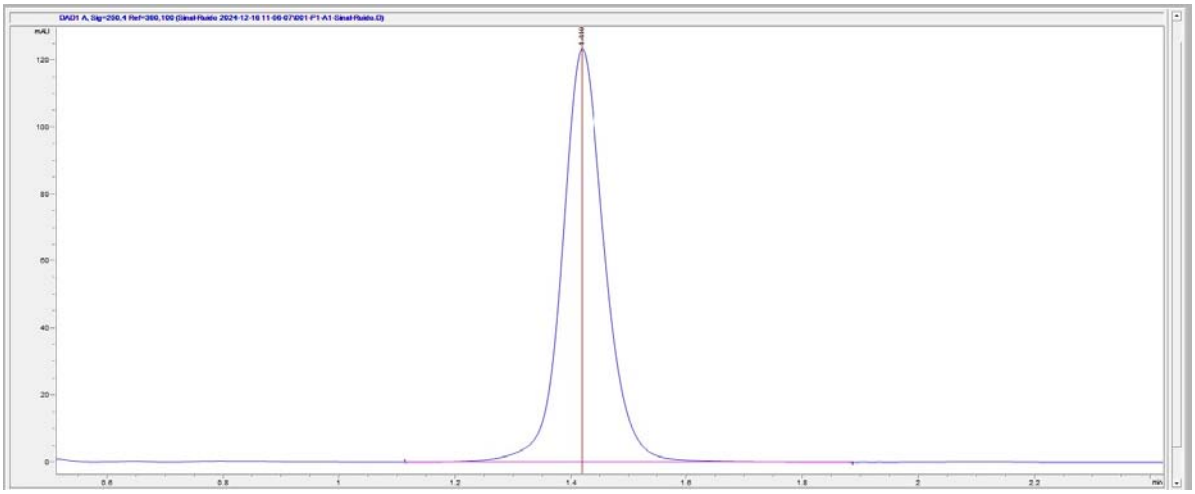

Certificado Nº: 550/24 - RELB	Início da Qualificação: 16/12/2024	Página 2 de 3

Resultado obtido no teste de sinal/ruído


Resultado:	Ruído (mAU)
VALOR MÁXIMO:	0.0460
VALOR MÍNIMO:	0.0370
	Ruído
	0.0090

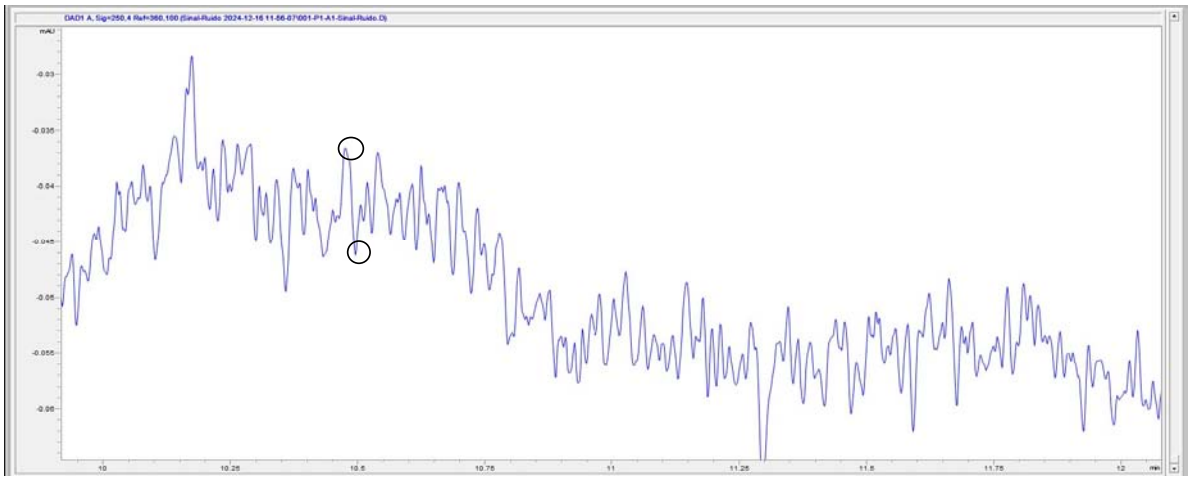

Certificado Nº: 550/24 - RELB	Início da Qualificação: 16/12/2024	Página 3 de 3

Resultado obtido no teste estabilidade da linha de base


Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	0.0350	0.0450
VALOR MÍNIMO:	0.0200	
Resultado:	0.0150	

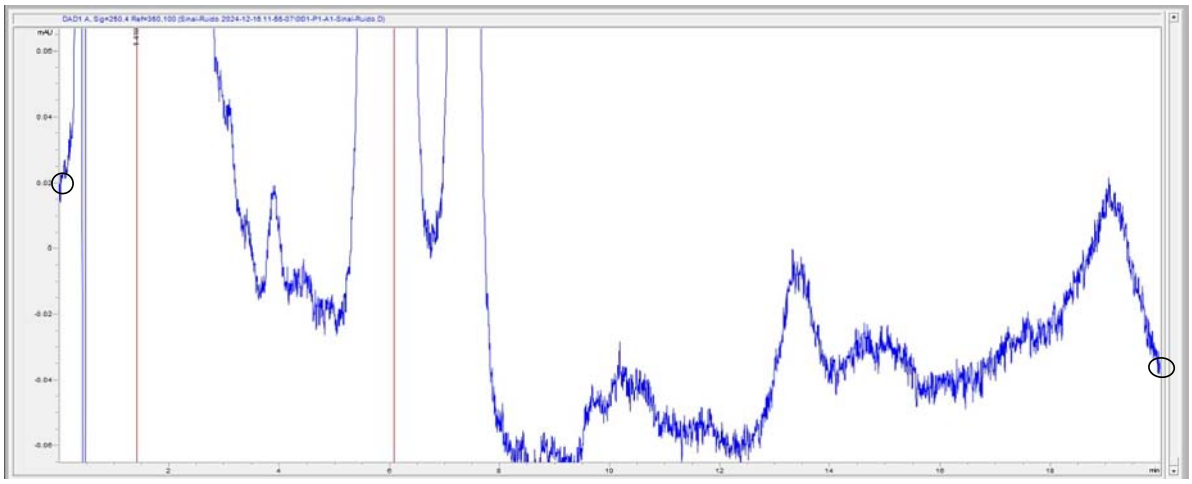

Data File C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\001-P1-A1-LDUV 1.D
Sample Name: LDUV 1

==========

Acq. Operator : SYSTEM Seq. Line : 1
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-01
Injection Date : 12/16/2024 11:31:00 AM Inj : 1
Inj Volume : 10.000 µl
Method : C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

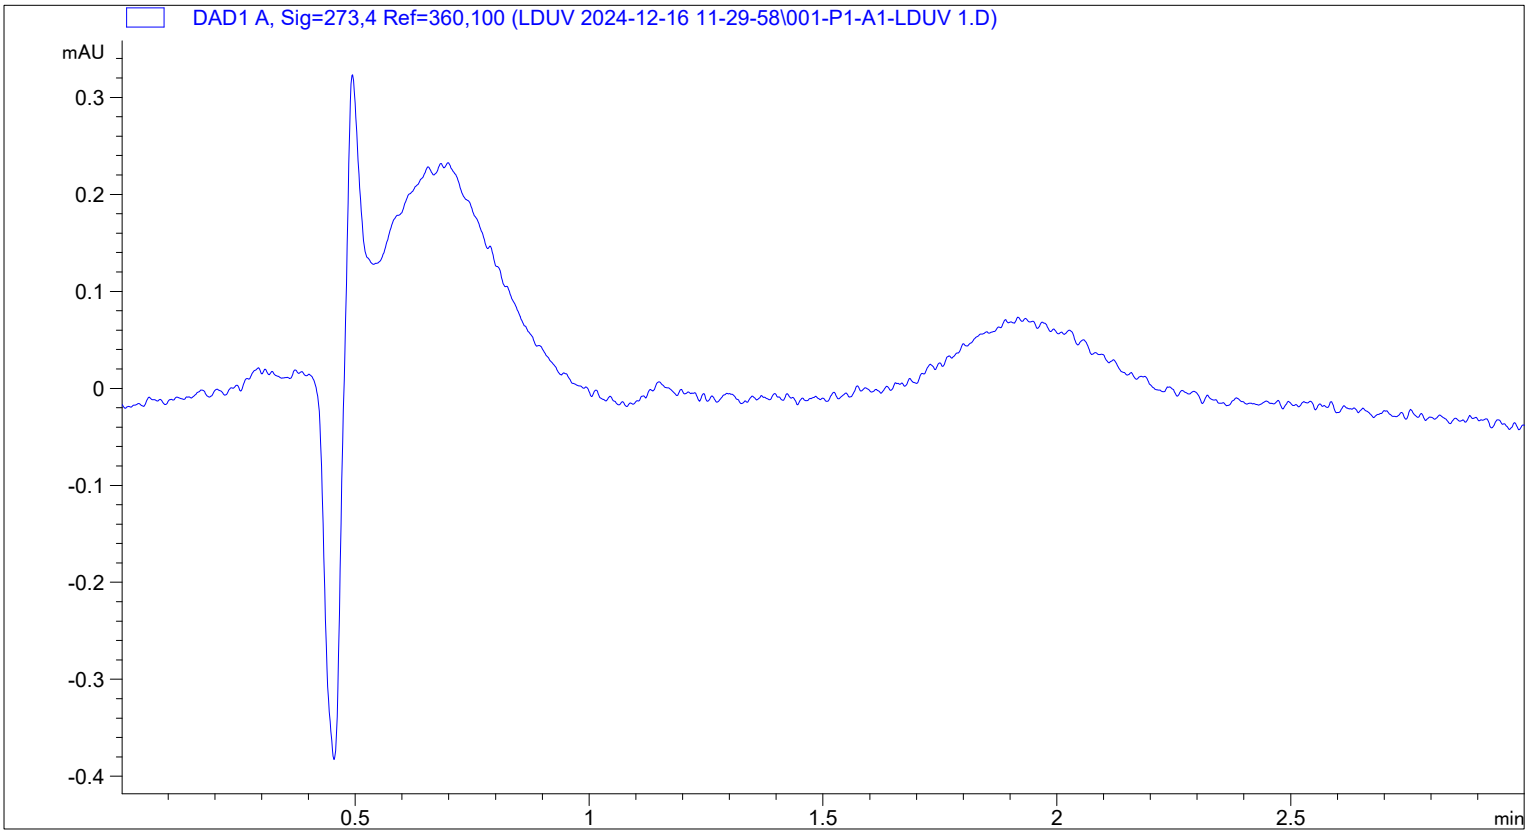

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\002-P1-A2-LDUV 2.D
Sample Name: LDUV 2

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   2
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-02
Injection Date   : 12/16/2024 11:34:57 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

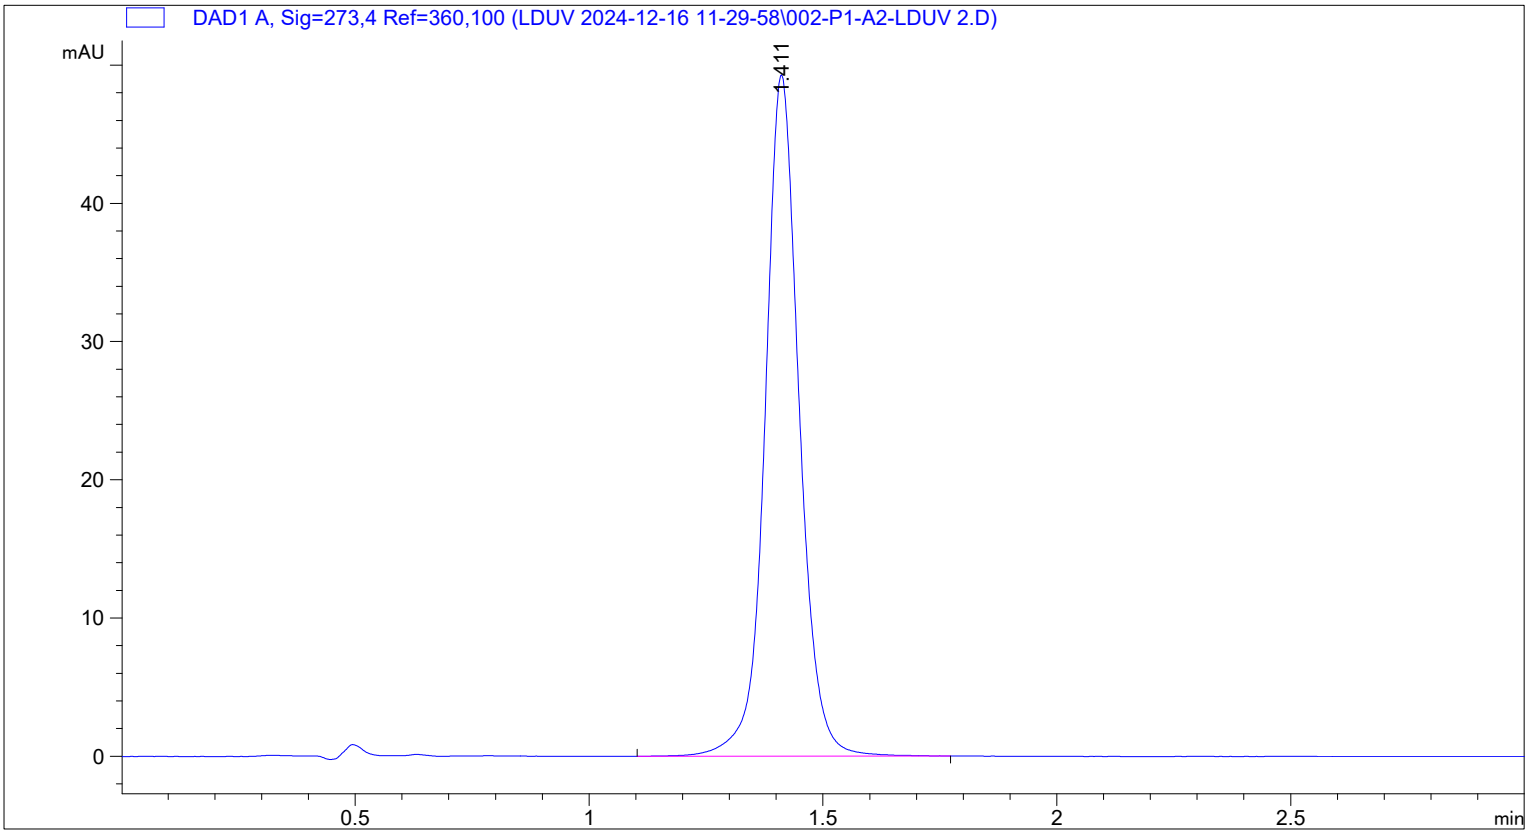


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.411 BB    0.0768  250.39871   49.29434 100.0000

Totals :                   250.39871   49.29434

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\003-P1-A3-LDUV 3.D
Sample Name: LDUV 3

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-03
Injection Date   : 12/16/2024 11:38:54 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

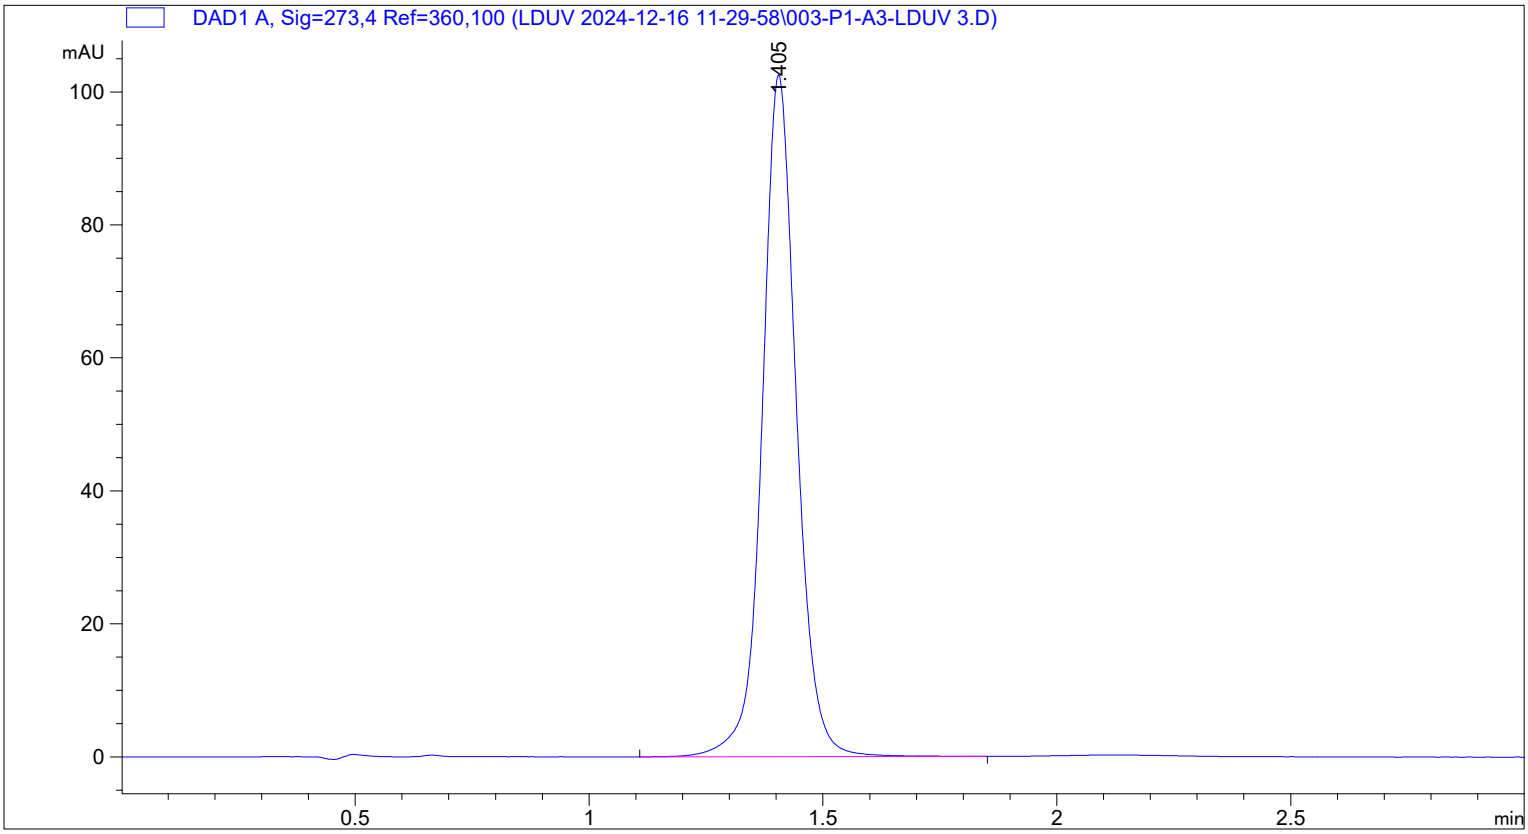


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.405 BB    0.0773  521.44659  102.54397 100.0000

Totals :                   521.44659  102.54397

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\004-P1-A4-LDUV 4.D
Sample Name: LDUV 4

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-04
Injection Date   : 12/16/2024 11:42:49 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

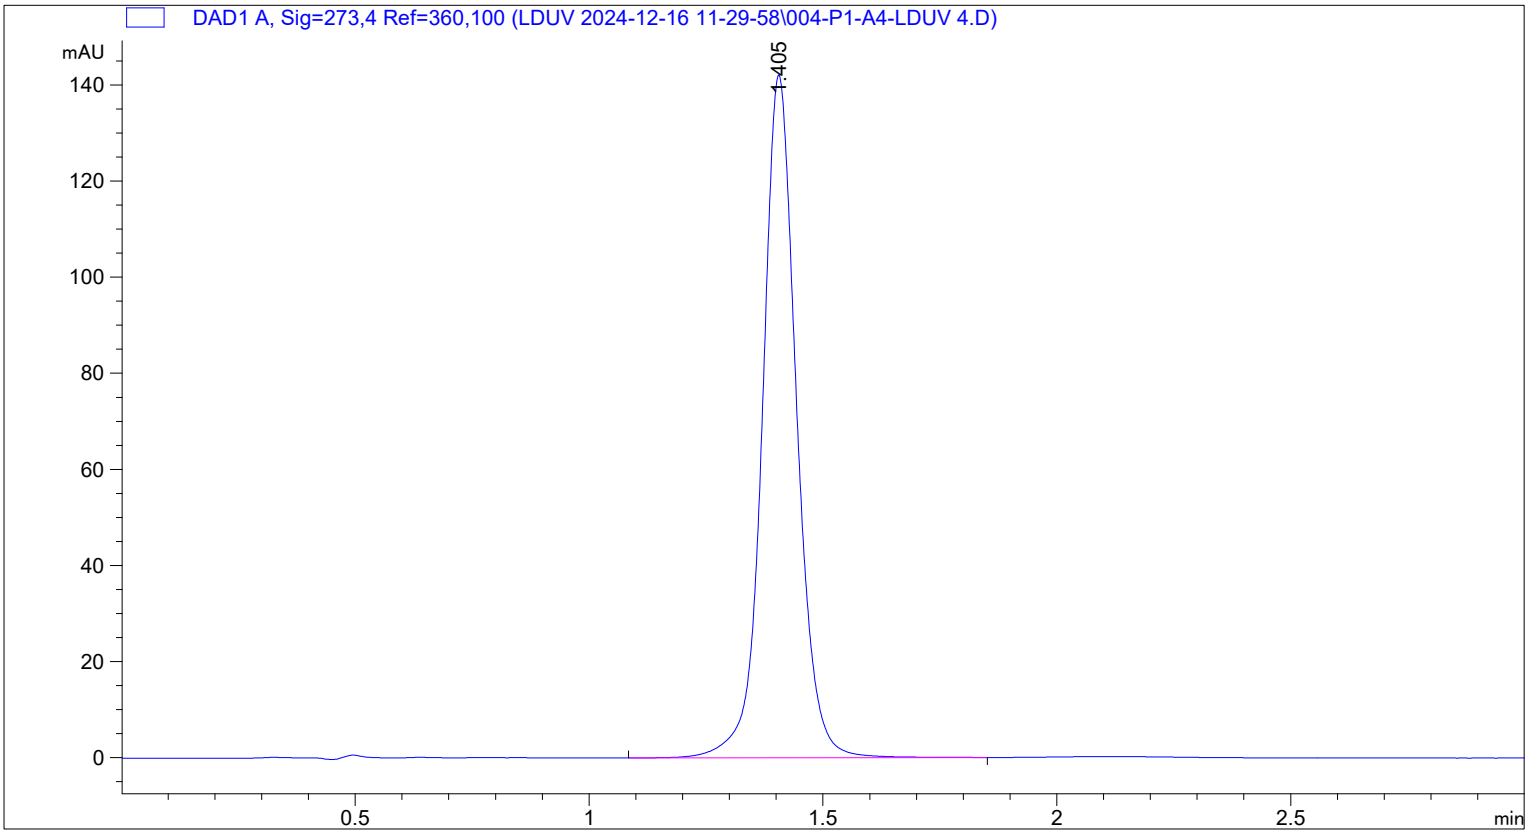


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.405 BB    0.0774  724.21649  142.14435 100.0000

Totals :                   724.21649  142.14435

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\005-P1-A5-LDUV 5.D
Sample Name: LDUV 5

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   5
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-05
Injection Date   : 12/16/2024 11:46:44 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\LDUV 2024-12-16 11-29-58\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

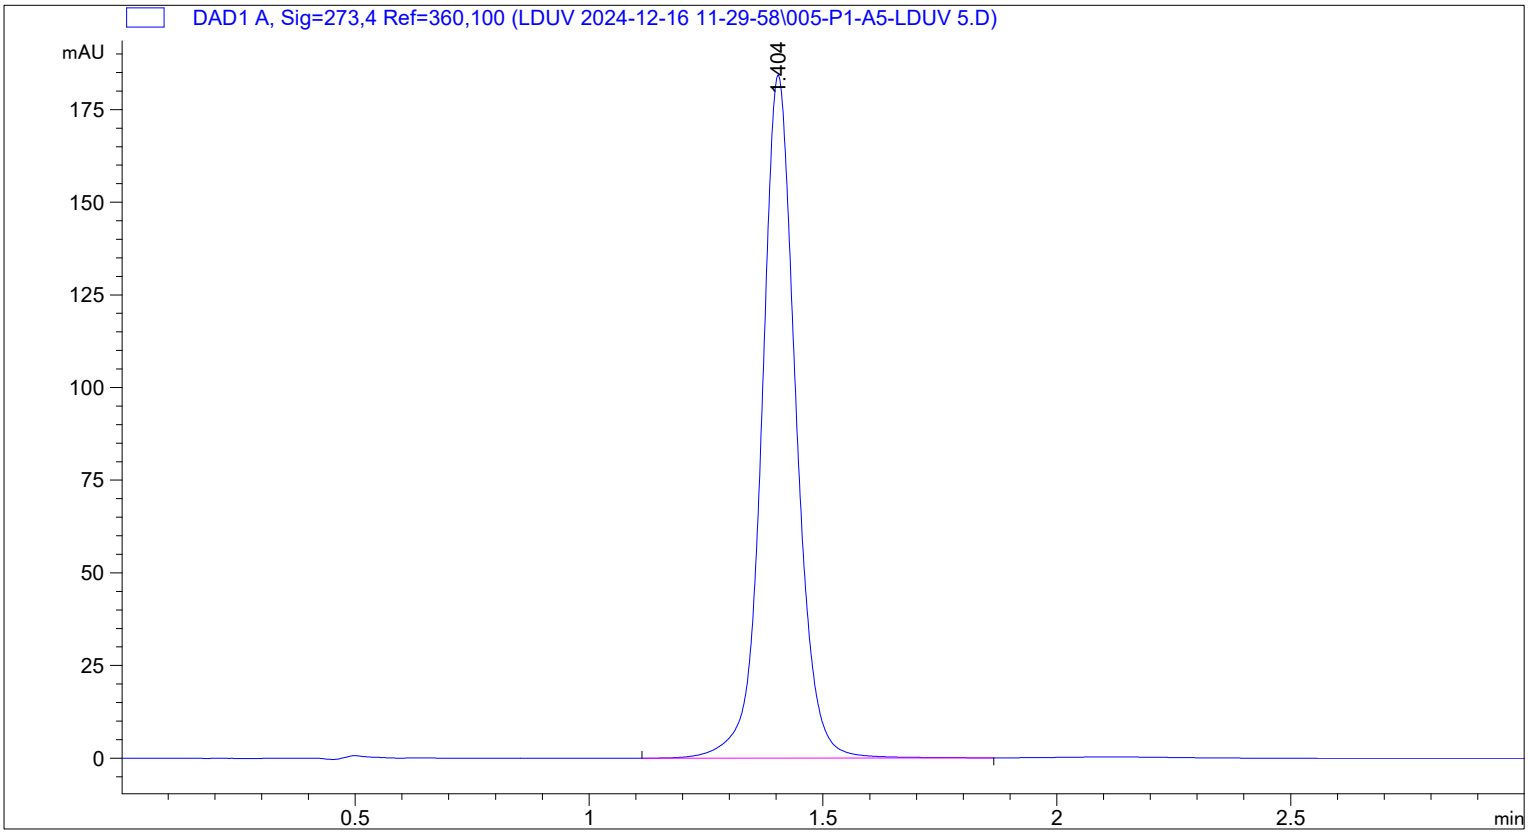


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.404 BB    0.0767  935.81390  184.36513 100.0000

Totals :                   935.81390  184.36513

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\001-P1-A1-LIIN 1.D
Sample Name: LIIN 1

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Sample Operator : SYSTEM
Acq. Instrument : LC-1260                          Location :   P1-A-01
Injection Date  : 12/16/2024 12:20:05 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 1.000 µl
Method          : C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\QUALIFICAÇÃO.M (Sequence
                  Method)
Last changed    : 12/16/2024 8:45:35 AM by SYSTEM
```

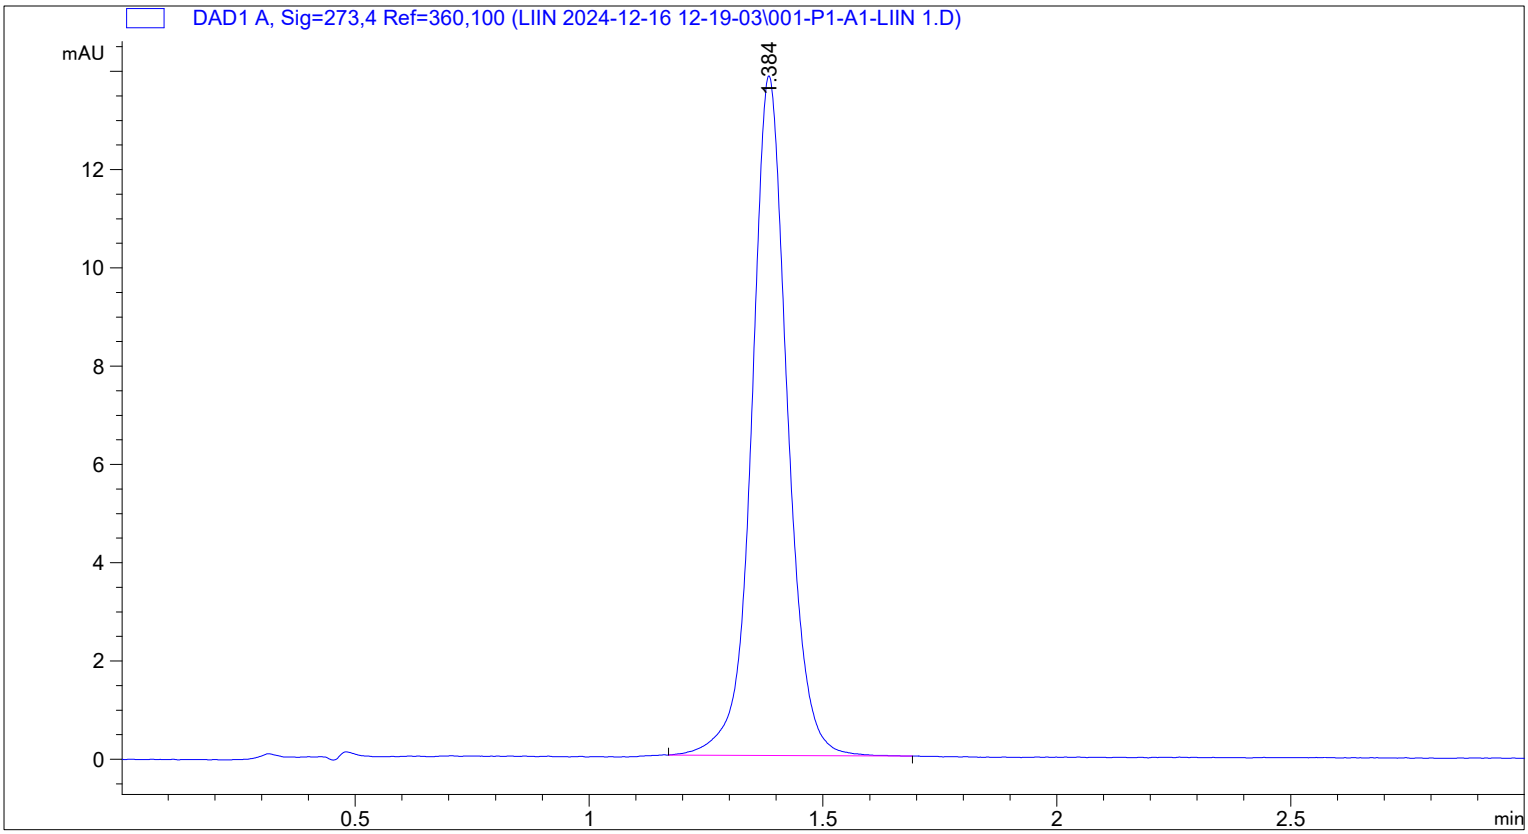


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.384 BB    0.0798   73.30111   13.83606 100.0000


Totals :                    73.30111   13.83606

==========================================================================
                         *** End of Report ***
```

Data File C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\002-P1-A1-LIIN 2.D
Sample Name: LIIN 2

==========

Acq. Operator : SYSTEM Seq. Line : 2
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-01
Injection Date : 12/16/2024 12:23:59 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 5.000 µl
Method : C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\QUALIFICAÇÃO.M (Sequence Method)
Last changed : 12/16/2024 8:45:35 AM by SYSTEM

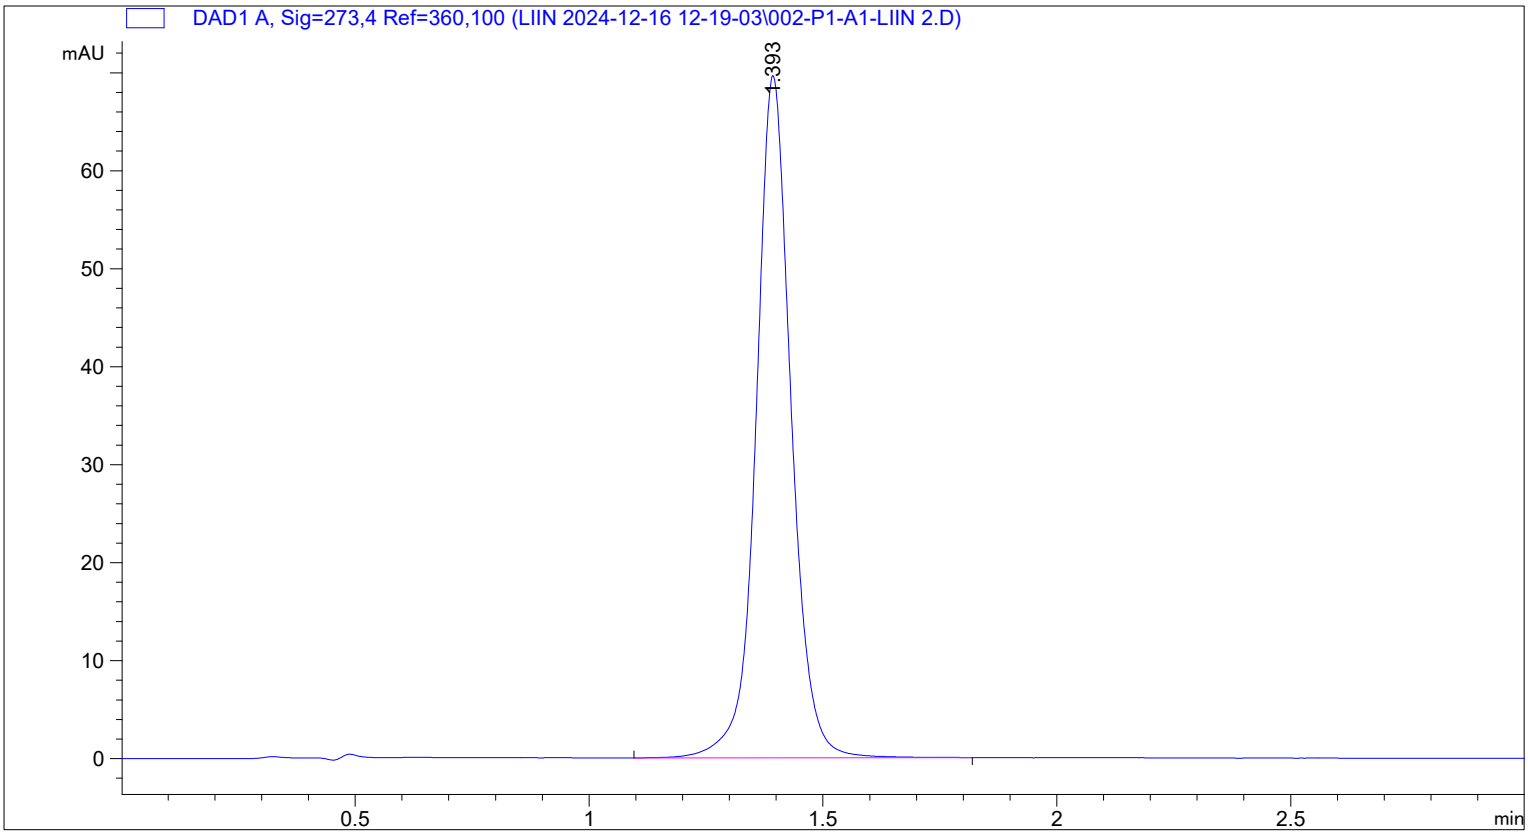

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.393	BB	0.0789	363.24539	69.62227	100.0000
Totals :				363.24539	69.62227	

==========

*** End of Report ***

Data File C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\003-P1-A1-LIIN 3.D
Sample Name: LIIN 3

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-01
Injection Date   : 12/16/2024 12:27:56 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method           : C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

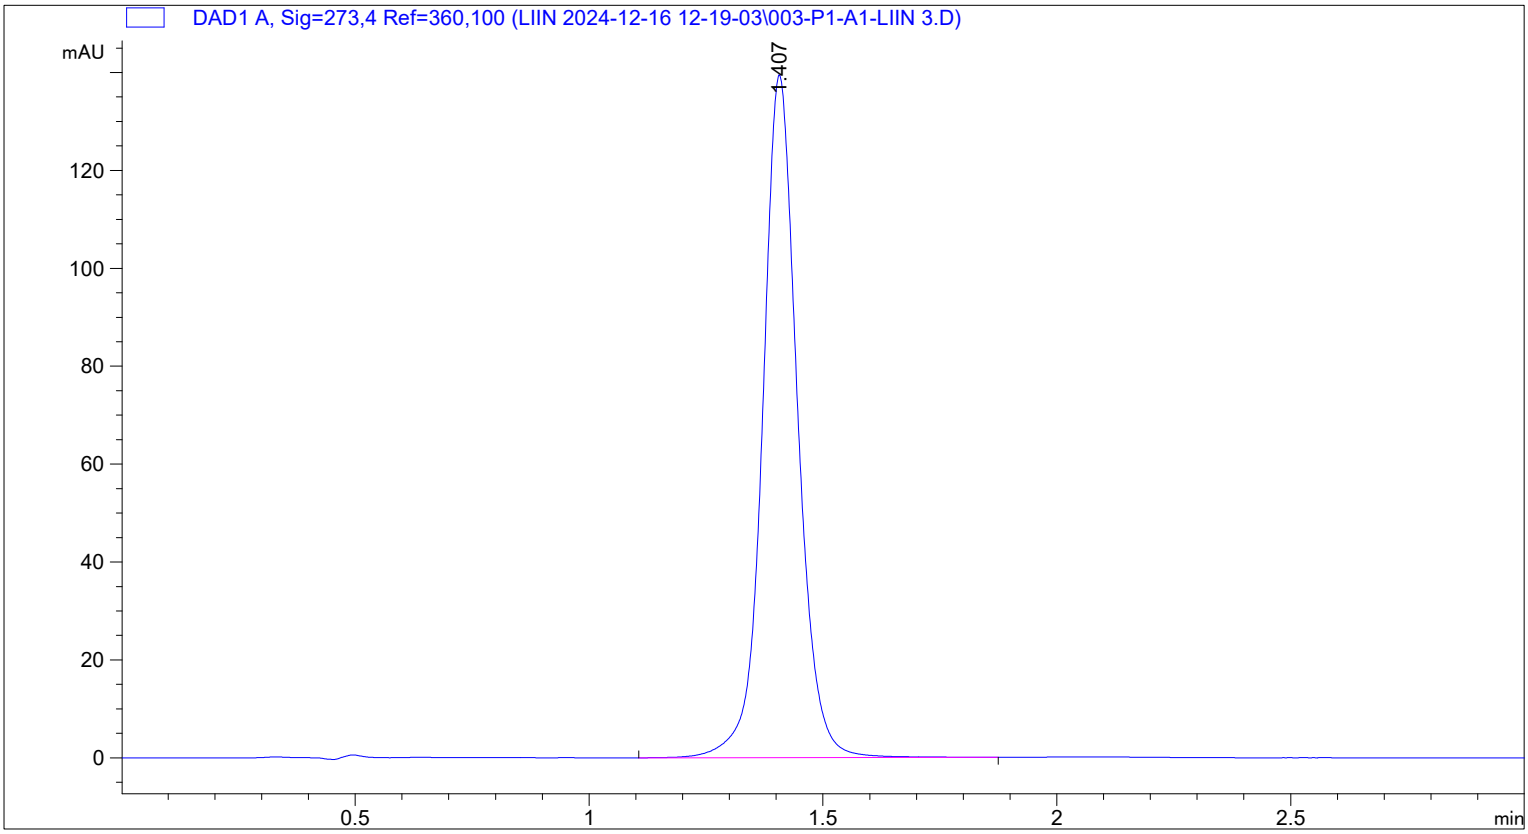


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.407 BB    0.0786  724.52838  139.48759 100.0000

Totals :                   724.52838  139.48759

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\004-P1-A1-LIIN 4.D
Sample Name: LIIN 4

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-01
Injection Date   : 12/16/2024 12:31:55 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Method           : C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

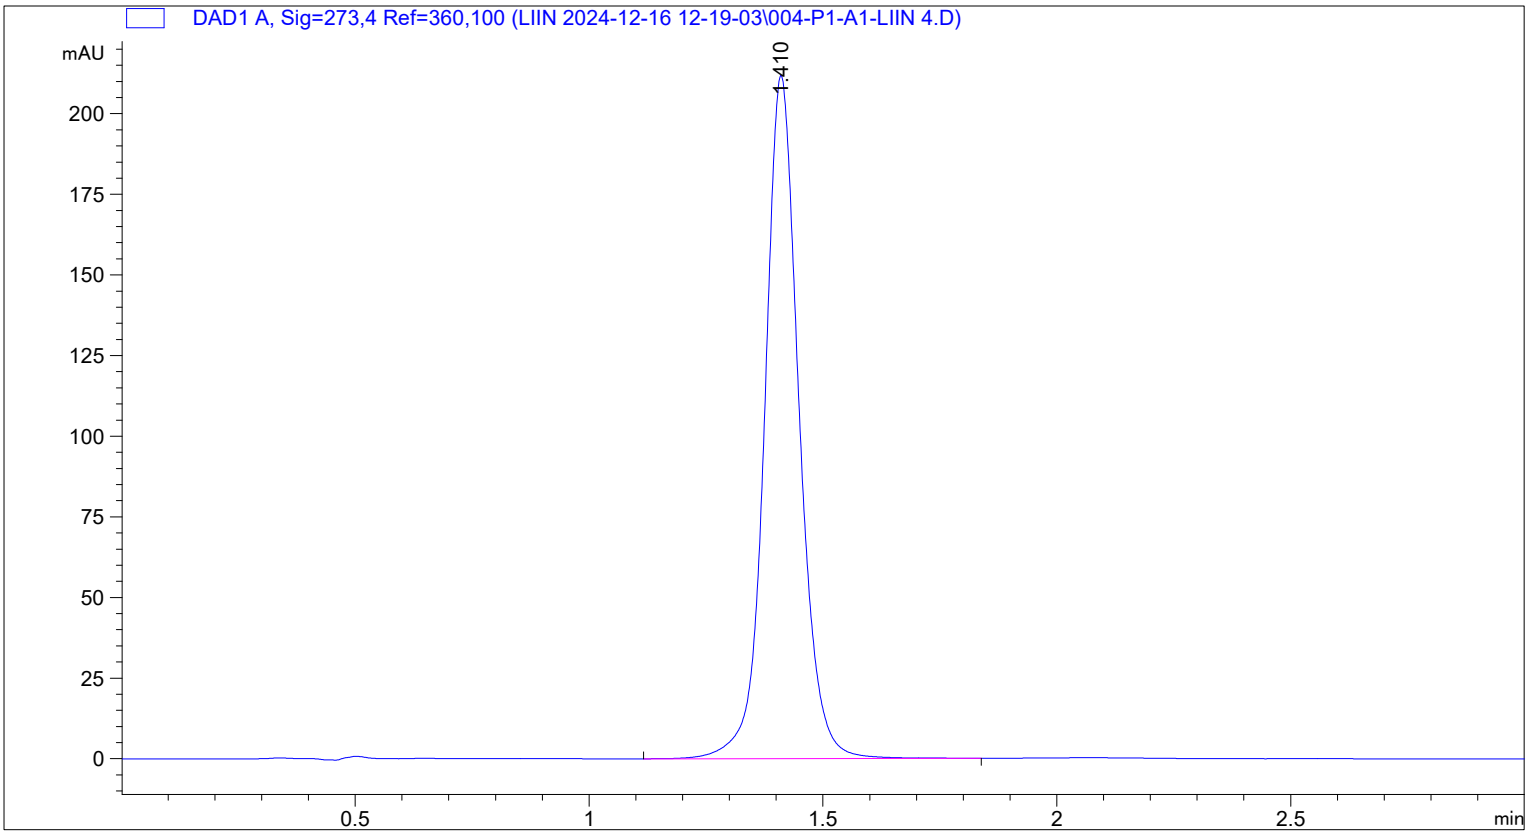


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.410 BB    0.0778 1084.82605  211.81578 100.0000

Totals :                  1084.82605  211.81578

==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\005-P1-A1-LIIN 5.D
Sample Name: LIIN 5

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   5
Sample Operator  : SYSTEM
Acq. Instrument  : LC-1260                          Location :   P1-A-01
Injection Date   : 12/16/2024 12:35:58 PM                Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Method           : C:\Chemstation\2\Data\LIIN 2024-12-16 12-19-03\QUALIFICAÇÃO.M (Sequence
                   Method)
Last changed     : 12/16/2024 8:45:35 AM by SYSTEM
```

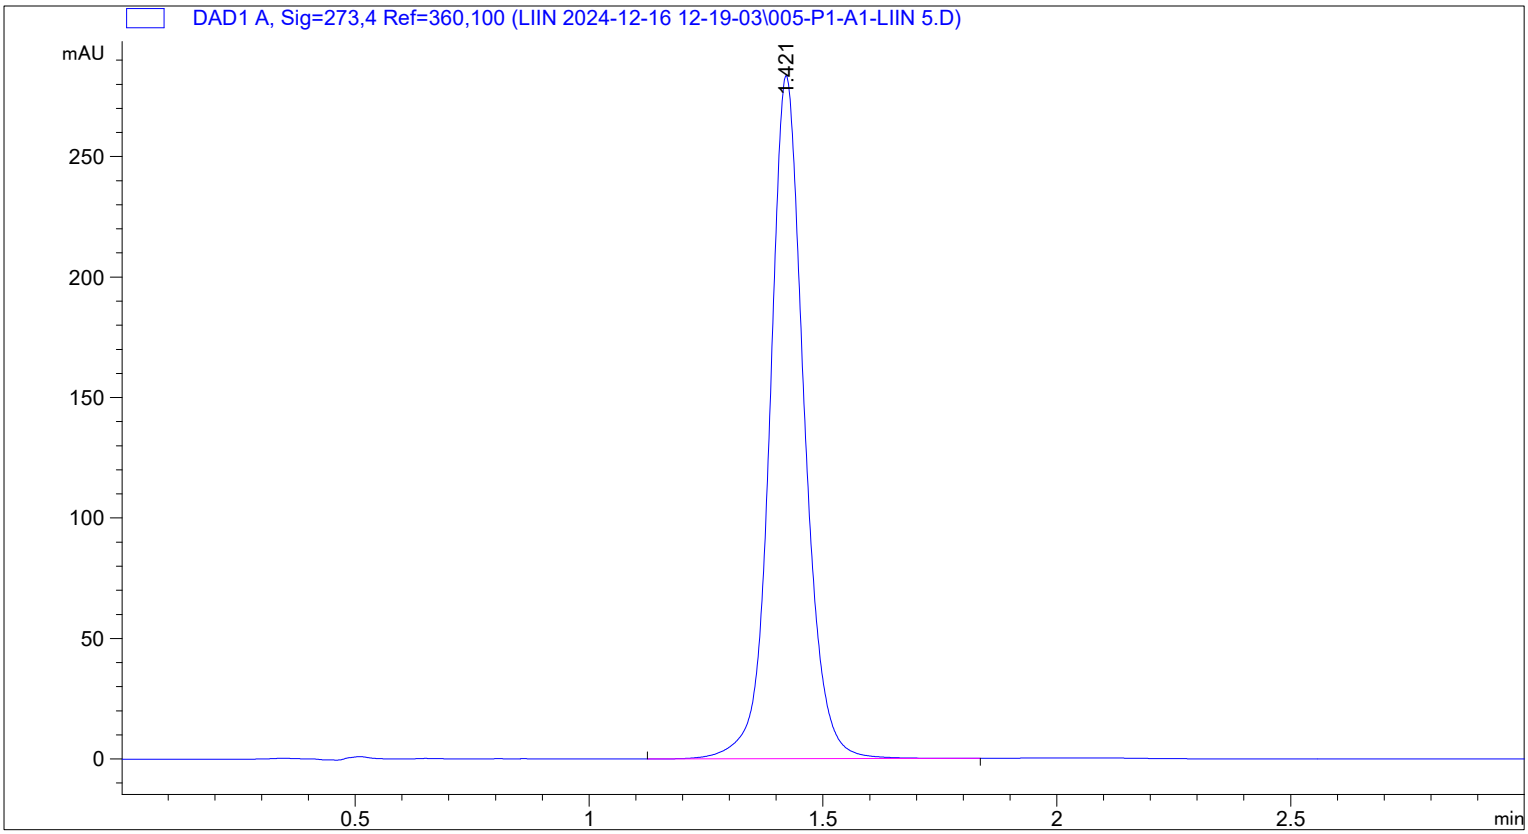


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.421 BB    0.0770 1446.79150  283.50348 100.0000


Totals :                  1446.79150  283.50348


==========================================================================
                          *** End of Report ***
```

Data File C:\Chemstation\2\Data\Grad AB 2024-12-16 13-54-19\001-P1-A1-Grad AB.D
Sample Name: Grad AB

==========

Acq. Operator : SYSTEM Seq. Line : 1
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-01
Injection Date : 12/16/2024 1:55:15 PM Inj : 1
Inj Volume : 0.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl
Method : C:\Chemstation\2\Data\Grad AB 2024-12-16 13-54-19\GRAD AB.M (Sequence Method)
Last changed : 12/16/2024 12:44:48 PM by SYSTEM
Additional Info : Peak(s) manually integrated

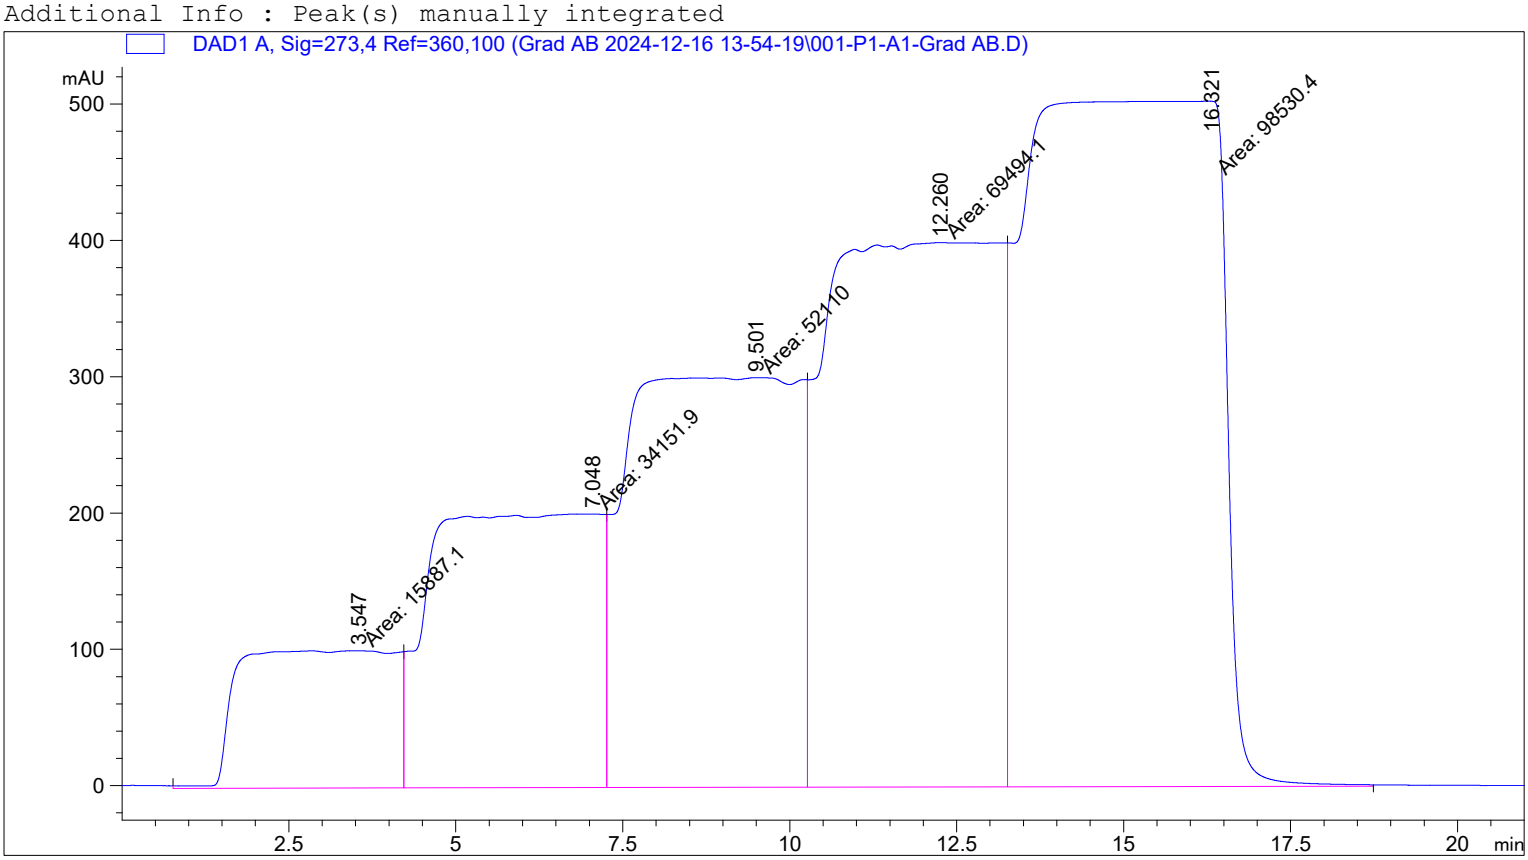

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.547	MF	2.6292	1.58871e4	100.71021	5.8803
2	7.048	MF	2.8372	3.41519e4	200.61758	12.6407
3	9.501	MF	2.8910	5.21100e4	300.41779	19.2876
4	12.260	MF	2.9012	6.94941e4	399.21945	25.7220
5	16.321	FM	3.2678	9.85304e4	502.53421	36.4693

Totals : 2.70173e5 1503.49924


==========

*** End of Report ***

Data File C:\Chemstation\2\Data\Grad CD 2024-12-16 13-31-46\001-P1-A1-Grad CD.D
Sample Name: Grad CD

==========

Acq. Operator : SYSTEM Seq. Line : 1
Sample Operator : SYSTEM
Acq. Instrument : LC-1260 Location : P1-A-01
Injection Date : 12/16/2024 1:32:42 PM Inj : 1
Inj Volume : 0.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl
Method : C:\Chemstation\2\Data\Grad CD 2024-12-16 13-31-46\GRAD CD.M (Sequence Method)
Last changed : 12/16/2024 12:47:14 PM by SYSTEM
Additional Info : Peak(s) manually integrated

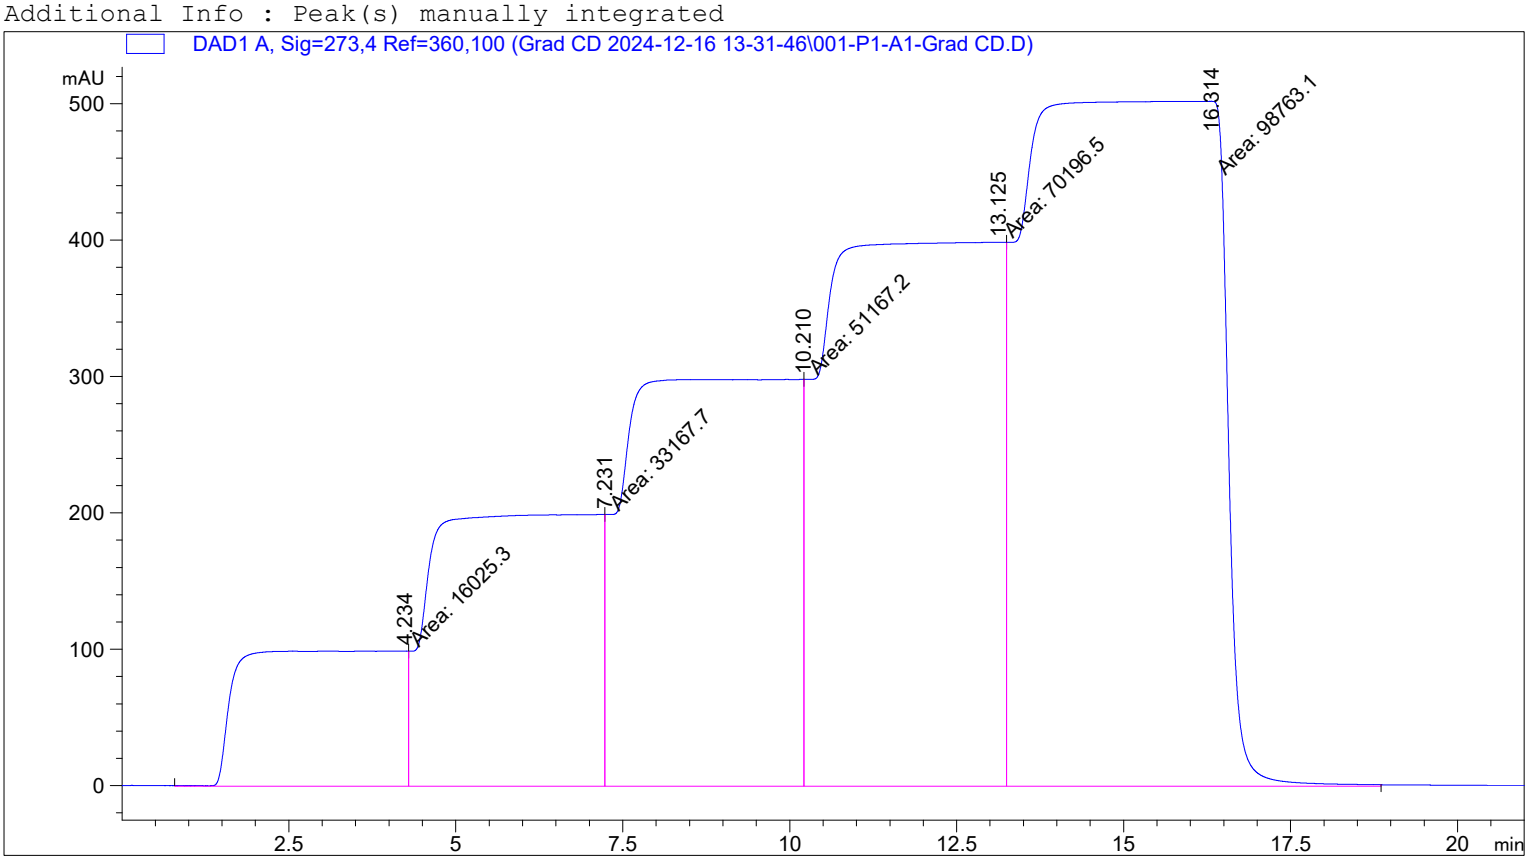

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=273,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.234	MF	2.6997	1.60253e4	98.93211	5.9503
2	7.231	MF	2.7760	3.31677e4	199.13580	12.3154
3	10.210	MF	2.8595	5.11672e4	298.22919	18.9987
4	13.125	MF	2.9345	7.01965e4	398.68549	26.0644
5	16.314	FM	3.2782	9.87631e4	502.11310	36.6713

Totals : 2.69320e5 1497.09568

==========

*** End of Report ***