
Chromatogram

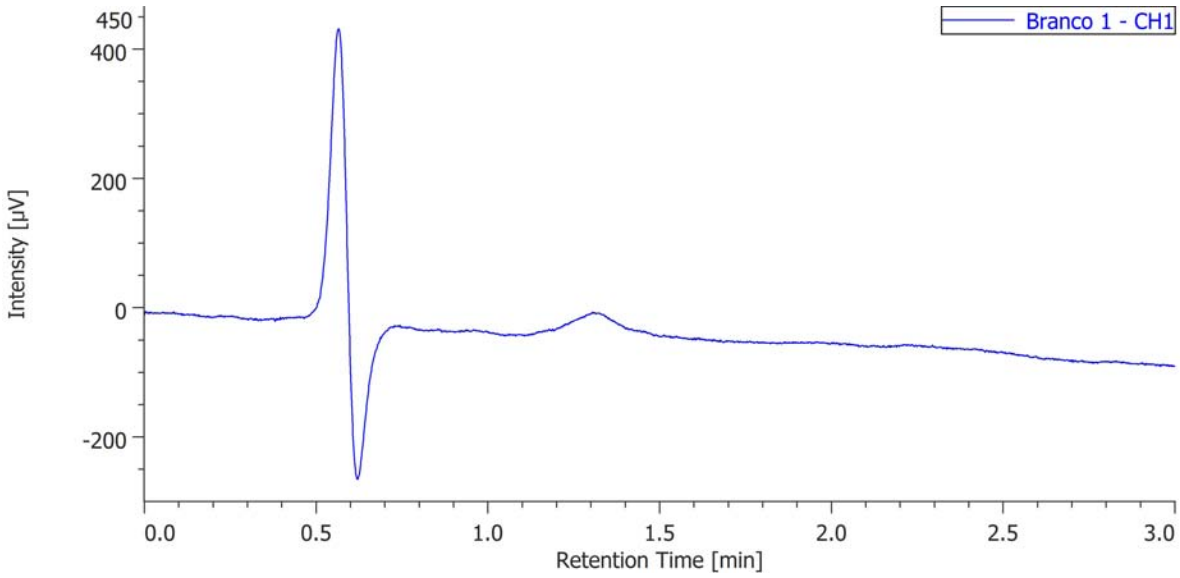


Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:09:37
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

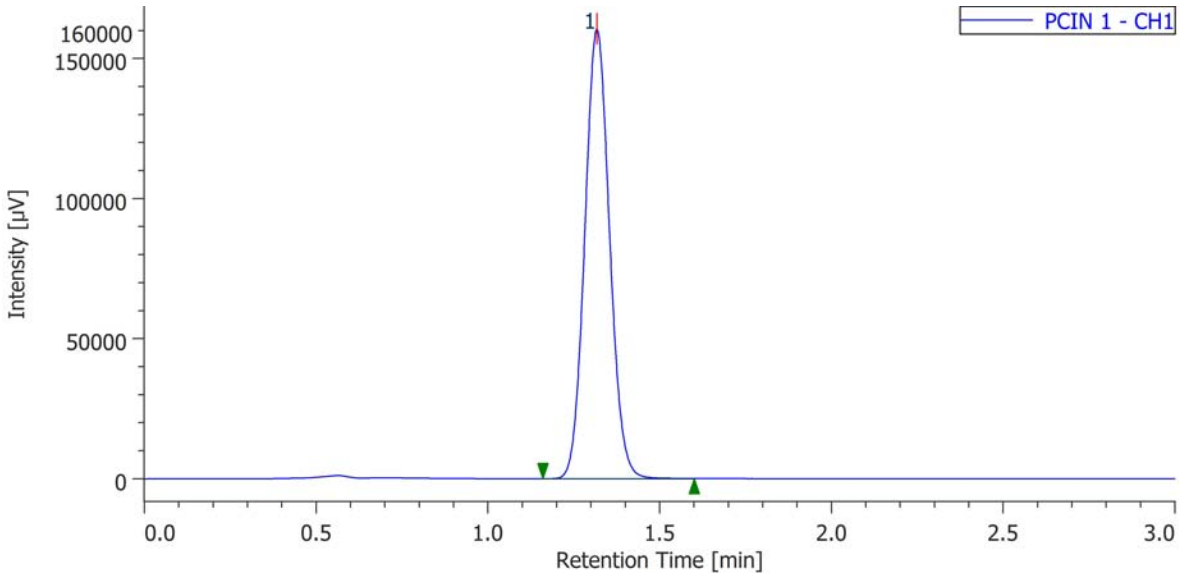

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:12:49
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.317	803104	160461	100.000	100.000	N/A	1607	N/A	1.075	

Creator QPackSA
Reviewer
Approver

Chromatogram

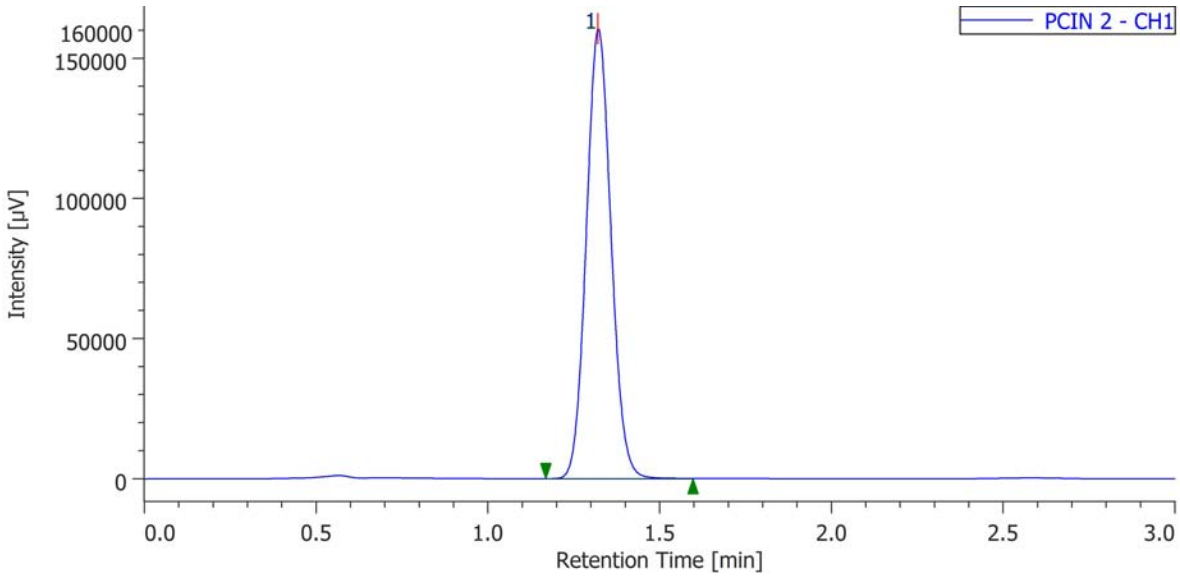

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:16:01
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.320	802683	160383	100.000	100.000	N/A	1618	N/A	1.091	

Creator QPackSA
Reviewer
Approver

Chromatogram

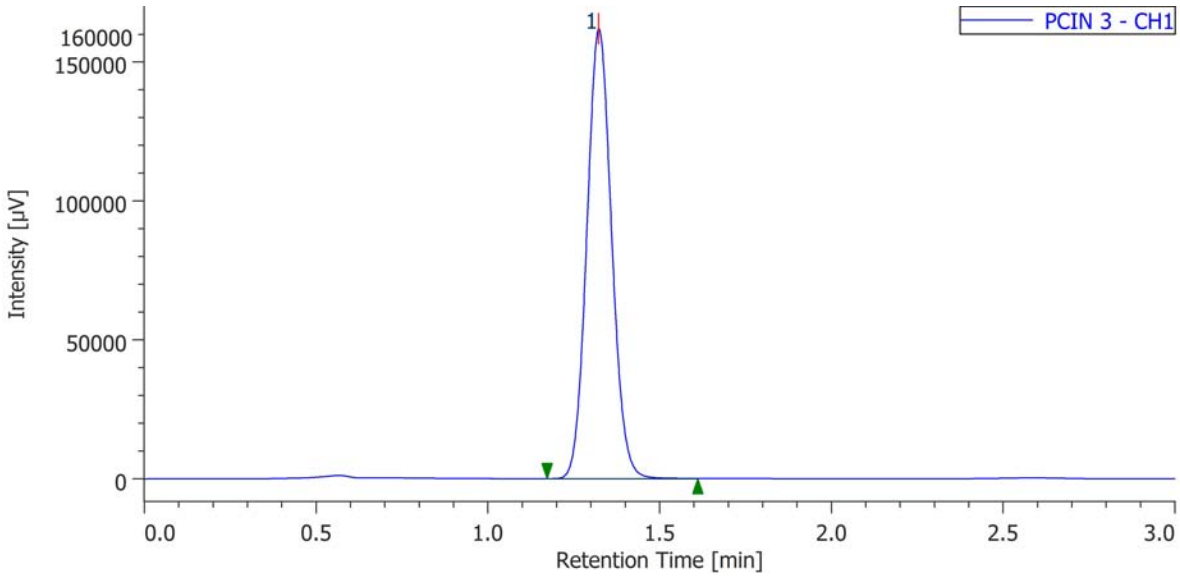

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:19:13
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.322	811405	161834	100.000	100.000	N/A	1616	N/A	1.091	

Creator QPackSA
Reviewer
Approver

Chromatogram

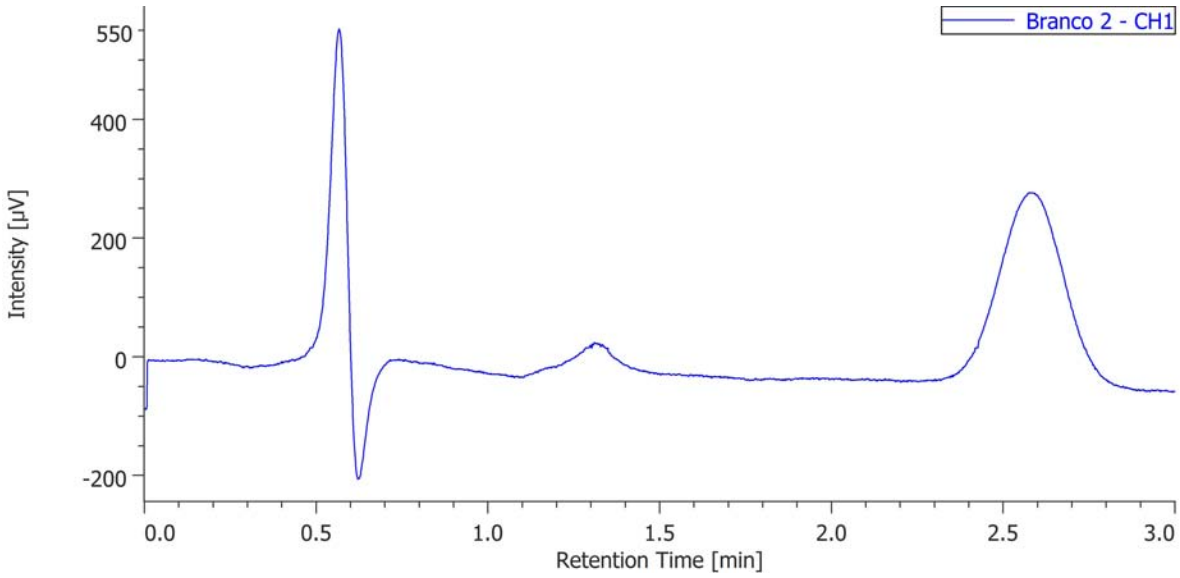


Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:22:25
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

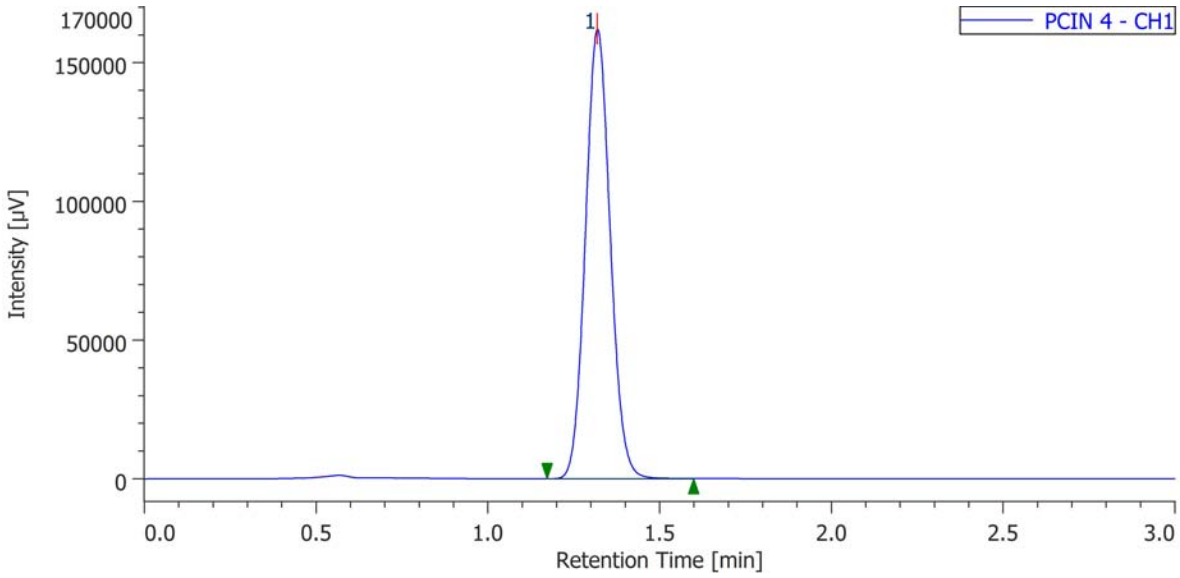

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:25:37
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.318	812439	162063	100.000	100.000	N/A	1608	N/A	1.083	

Creator QPackSA
Reviewer
Approver

Chromatogram

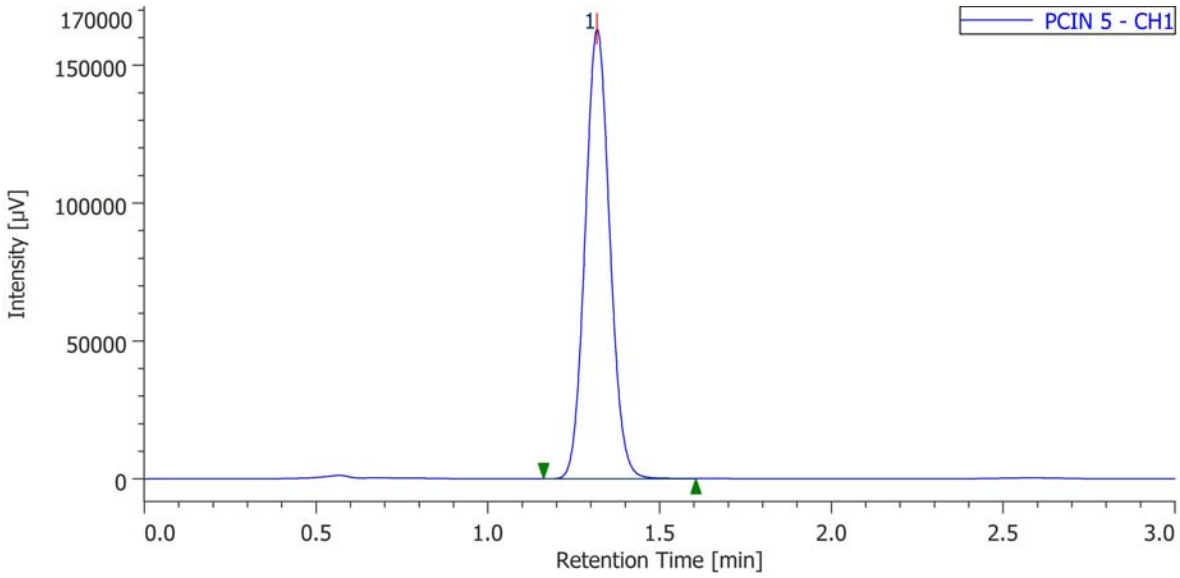

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:28:49
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.317	812106	163047	100.000	100.000	N/A	1623	N/A	1.087	

Creator QPackSA
Reviewer
Approver

Chromatogram

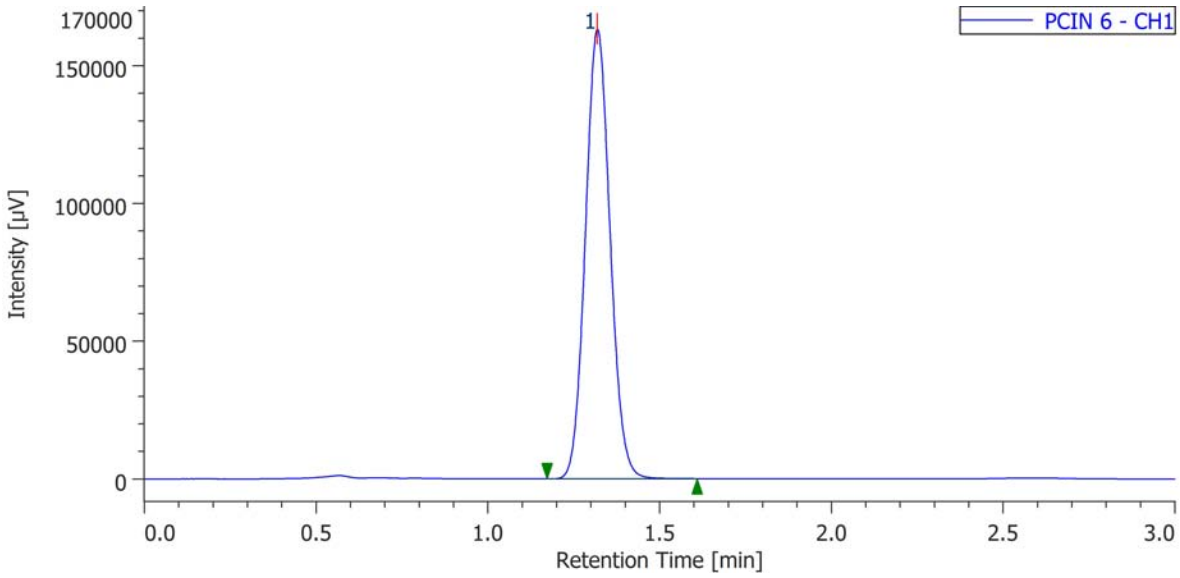

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:32:01
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.318	814894	163252	100.000	100.000	N/A	1620	N/A	1.078	

Creator QPackSA
Reviewer
Approver

Chromatogram

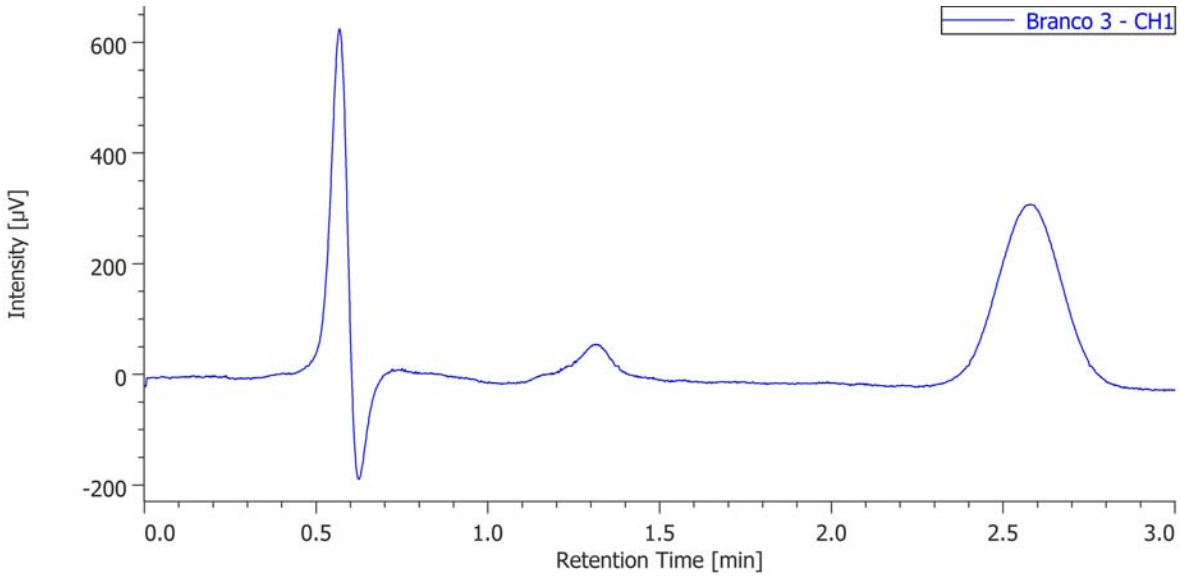


Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:44:28
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:35:13
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

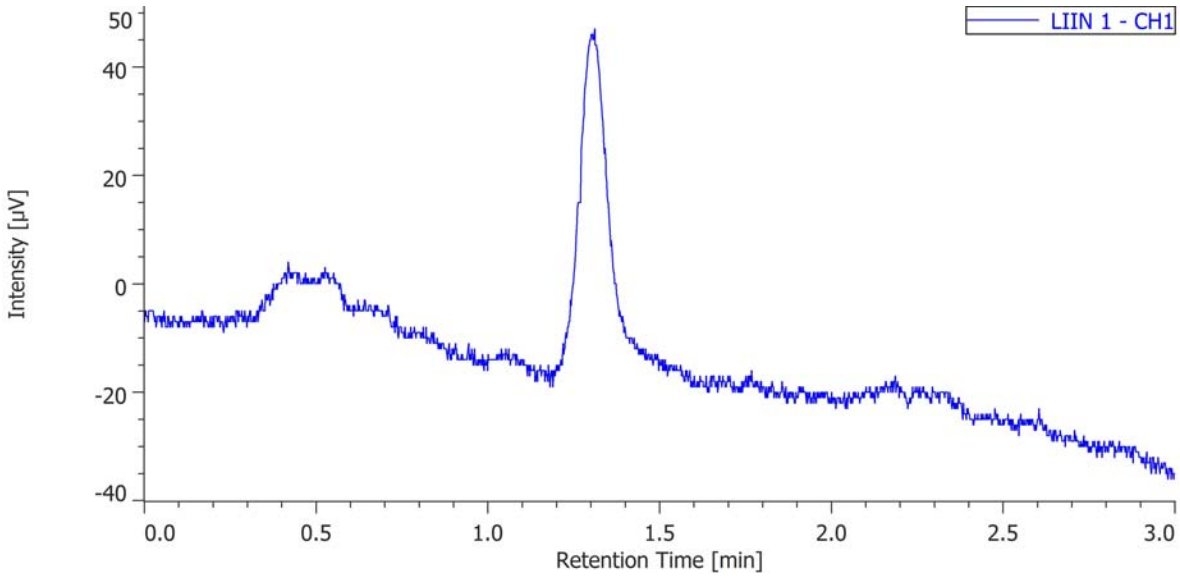


Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:59:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:39:44
Volume	0.1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

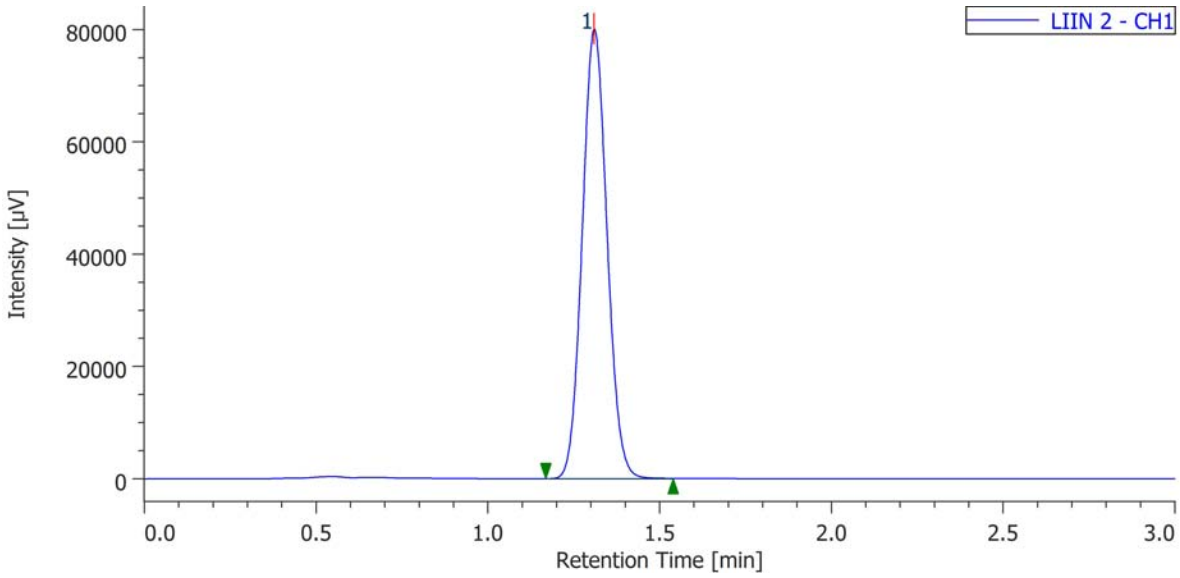

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:59:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:42:56
Volume	5.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.308	401271	80041	100.000	100.000	N/A	1572	N/A	1.086	

Creator QPackSA
Reviewer
Approver

Chromatogram

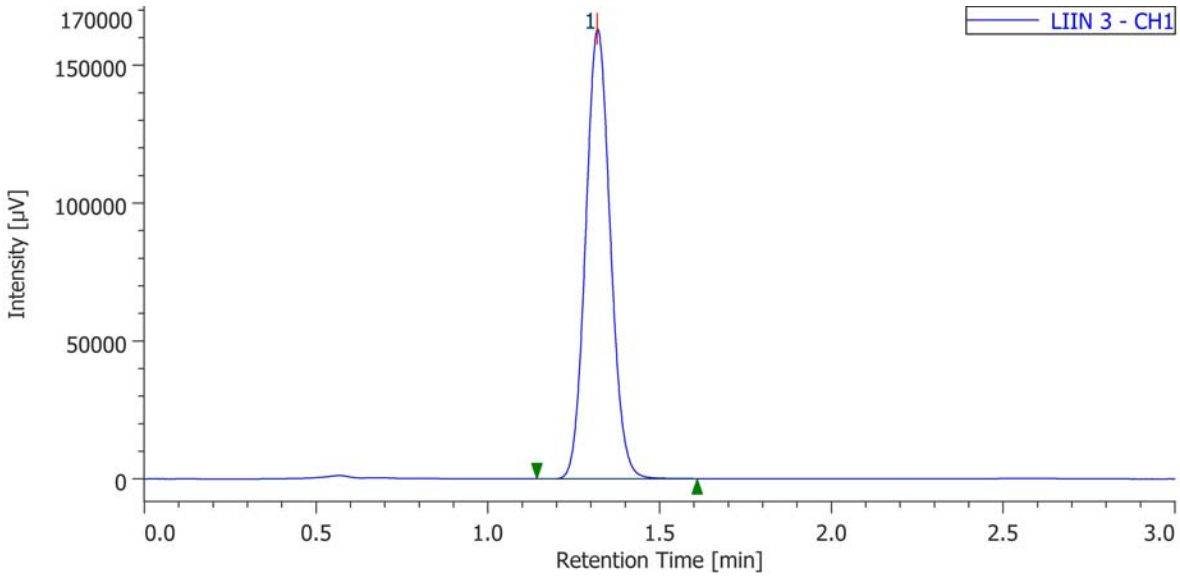

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:59:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:46:08
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.318	812647	163042	100.000	100.000	N/A	1625	N/A	1.090	

Creator QPackSA
Reviewer
Approver

Chromatogram

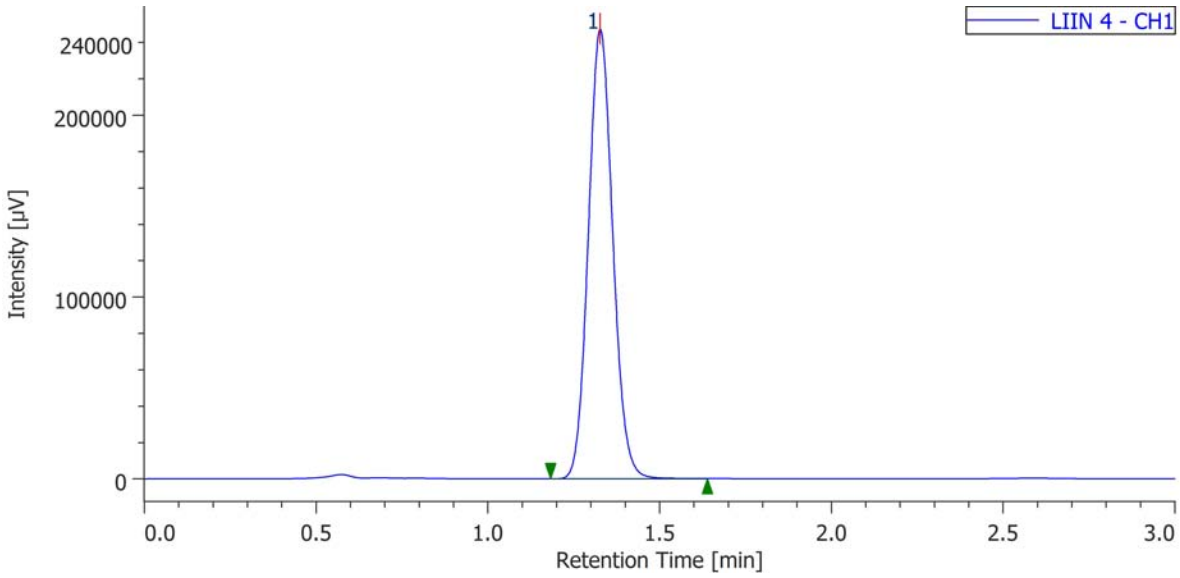

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:59:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:49:20
Volume	15.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.327	1220830	247295	100.000	100.000	N/A	1686	N/A	1.084	

Creator QPackSA
Reviewer
Approver

Chromatogram

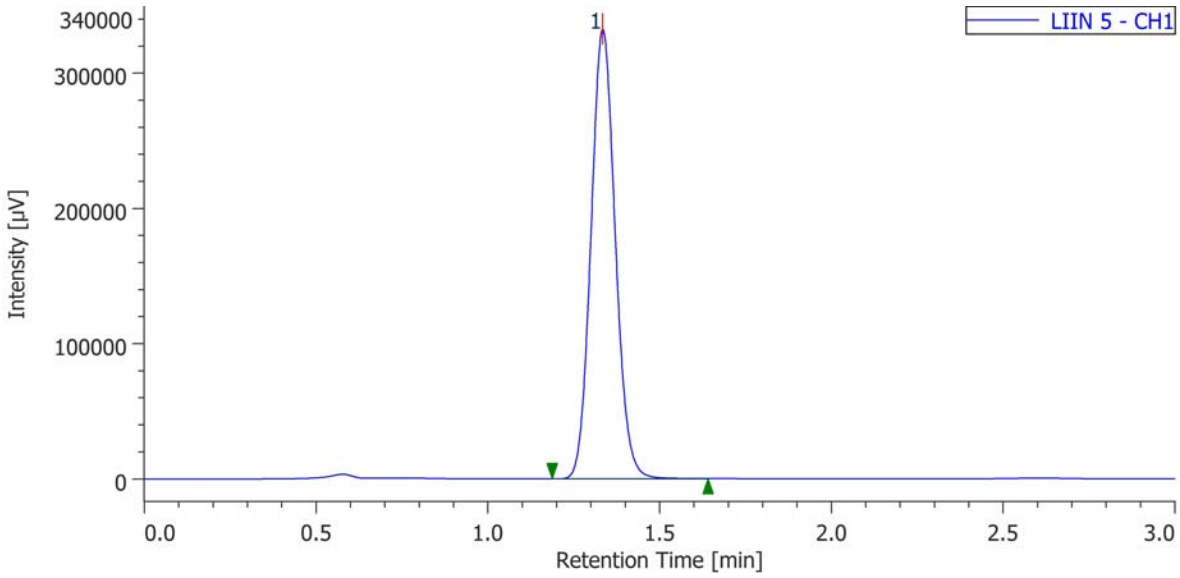

Chromatogram Information	
User Name	QPackSA
Date Modified	03/12/2025 15:59:13
Description	
HPLC System Name	BBA HPLC 03 UV
Injection Date	03/12/2025 15:52:32
Volume	20.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.333	1630325	332402	100.000	100.000	N/A	1729	N/A	1.096	

Creator QPackSA
Reviewer
Approver