

On Peak Spectra

Channel Information	
Chromatogram Name	EDUV_002-CH9
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

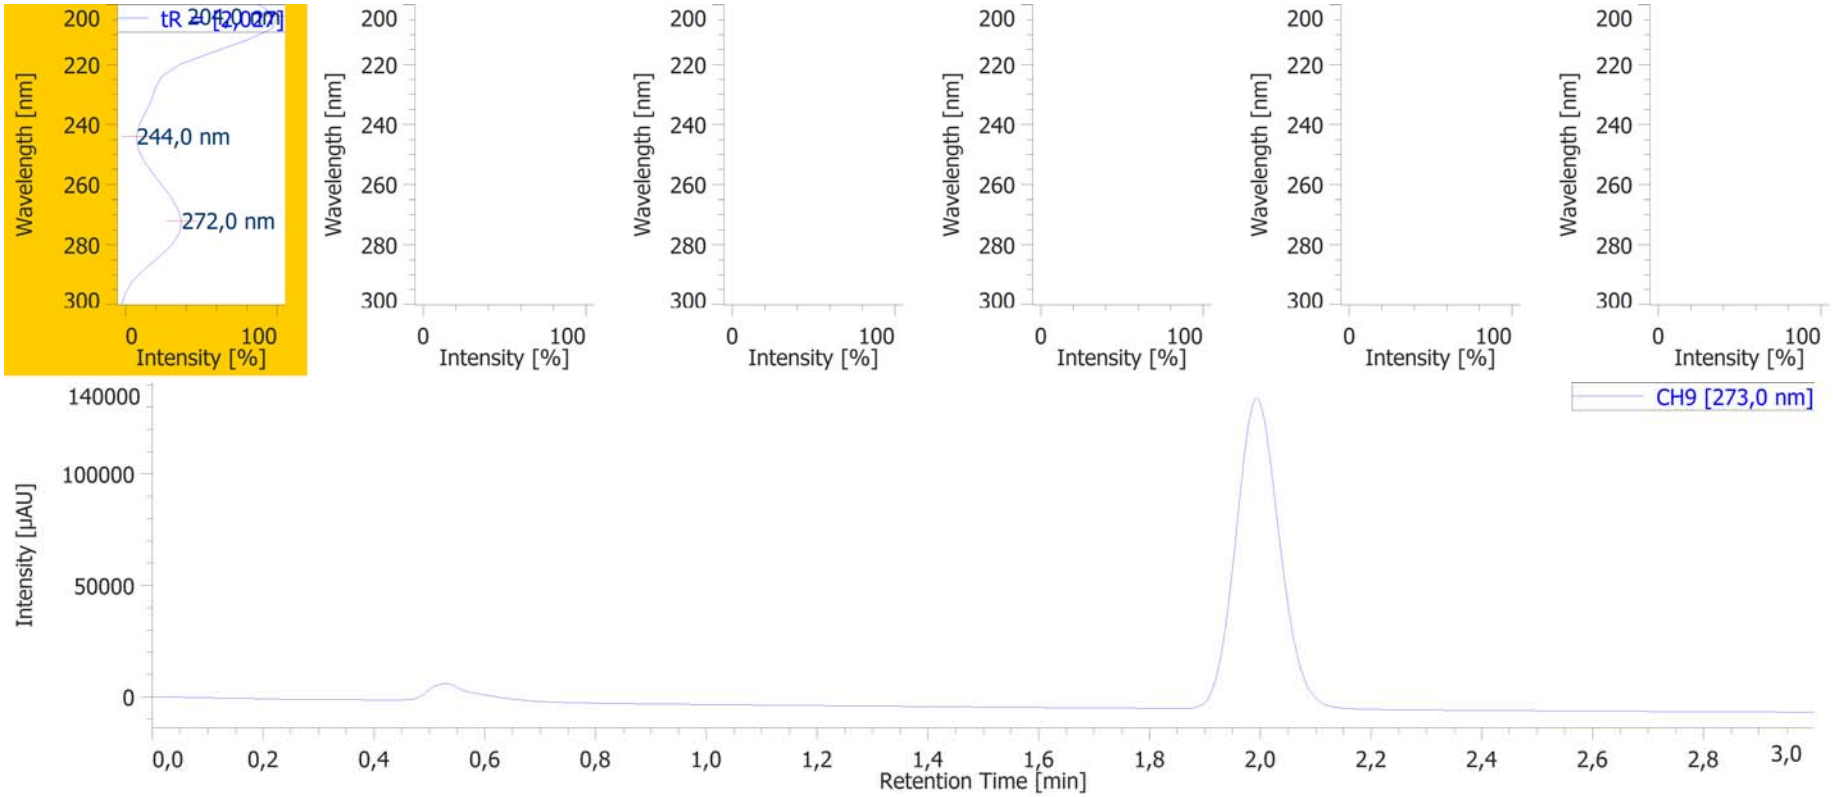

Chromatogram

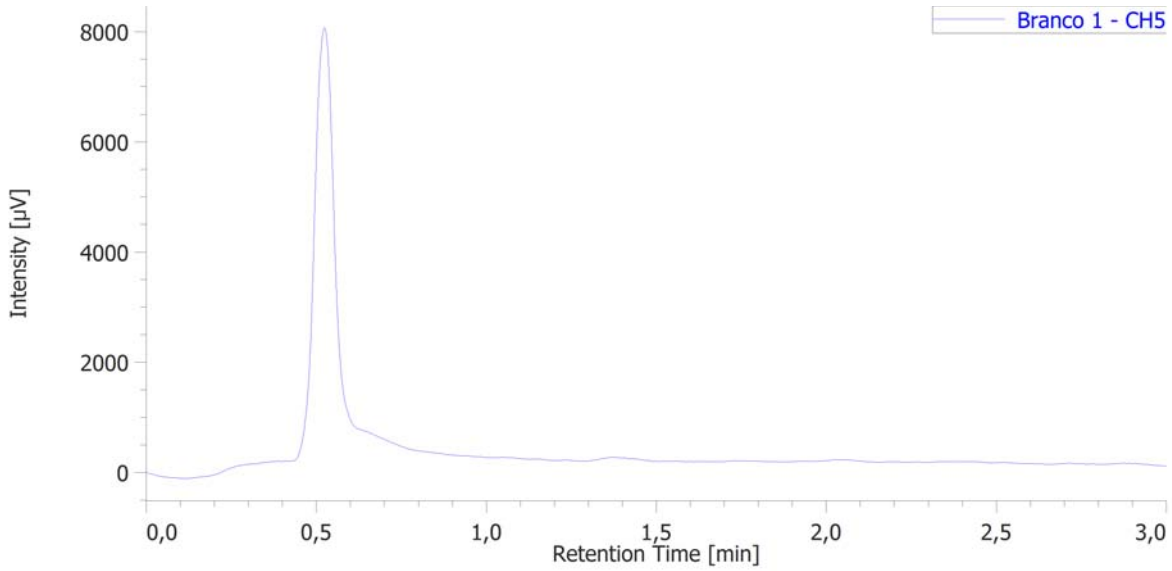


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:26
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:41:34
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

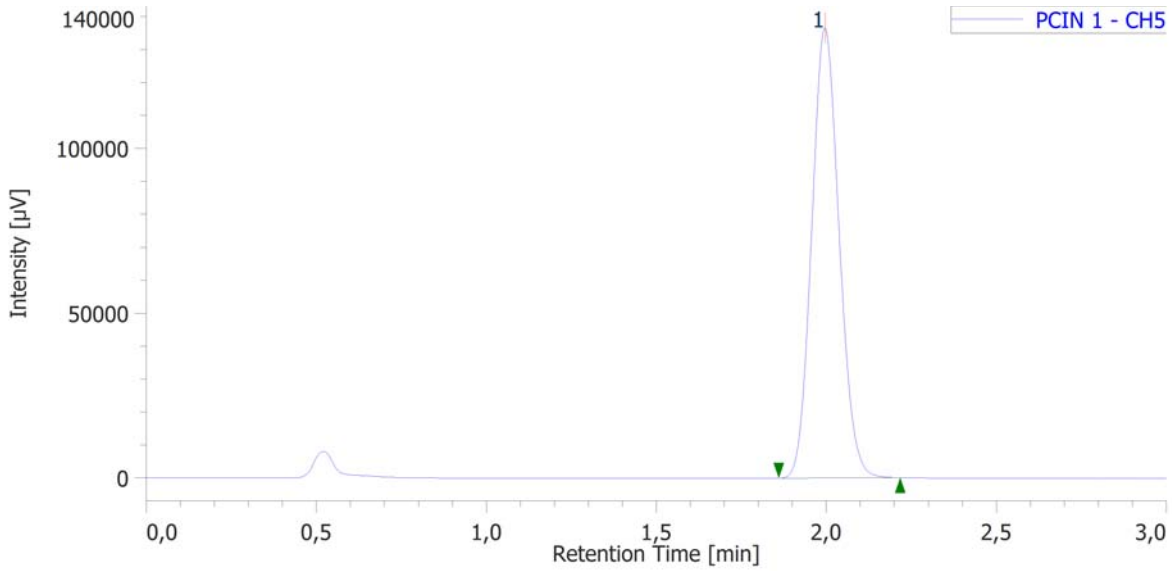

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:27
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:44:46
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,997	765869	136527	100,000	100,000	N/A	2924	N/A	1,085	

Creator Administrator
Reviewer
Approver

Chromatogram

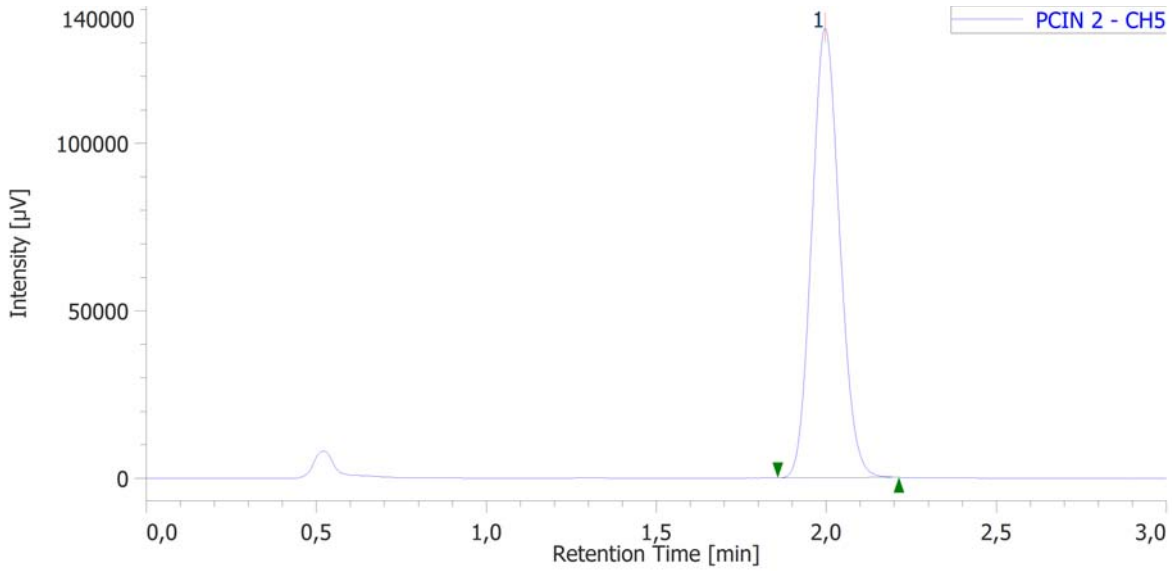

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:27
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:47:58
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,997	765423	134191	100,000	100,000	N/A	2820	N/A	1,098	

Creator Administrator
Reviewer
Approver

Chromatogram

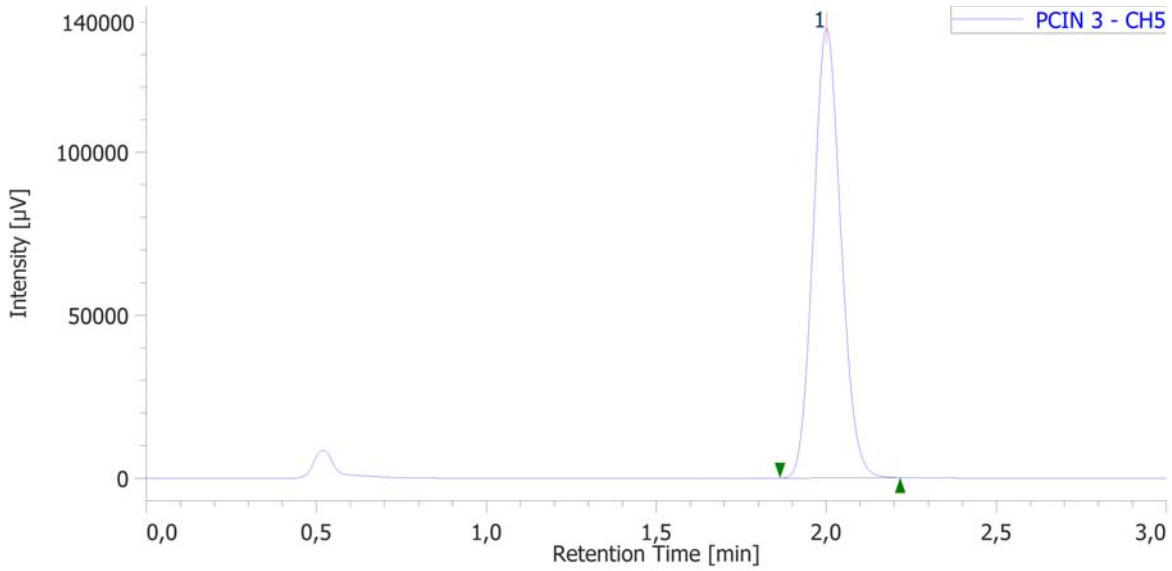

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:27
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:51:10
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,000	777554	138010	100,000	100,000	N/A	2907	N/A	1,108	

Creator Administrator
Reviewer
Approver

Chromatogram

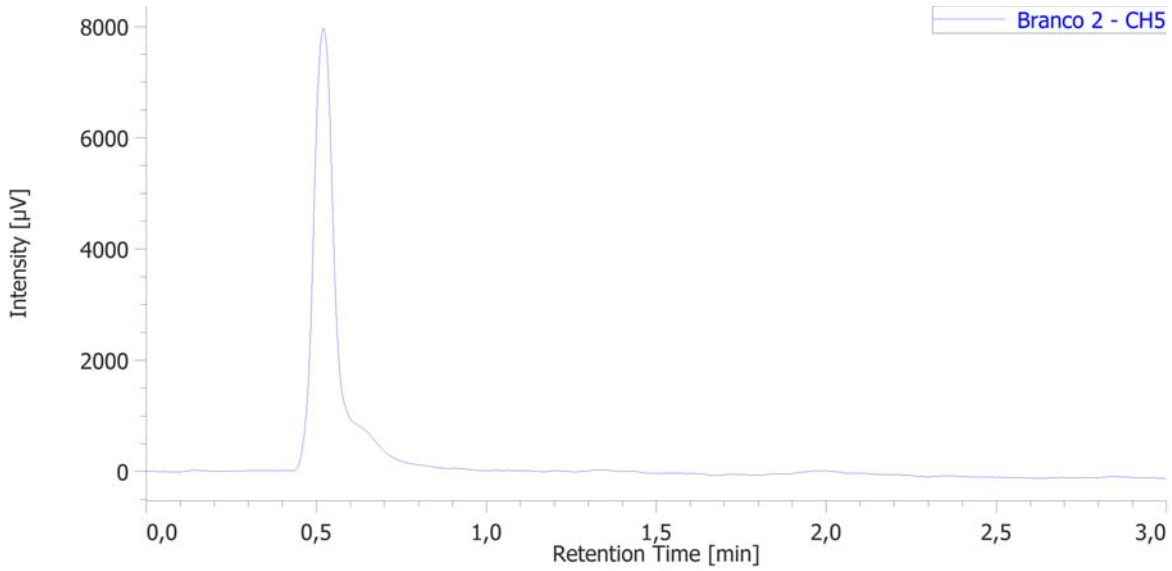


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:28
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:54:22
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

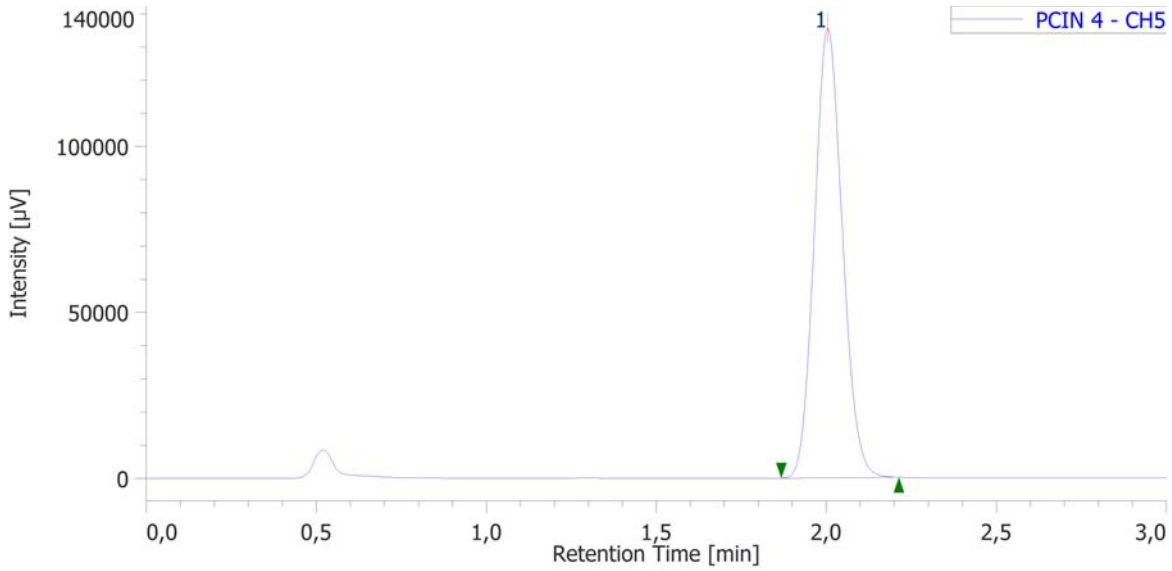

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:28
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 11:57:34
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,003	773562	135437	100,000	100,000	N/A	2834	N/A	1,114	

Creator Administrator
Reviewer
Approver

Chromatogram

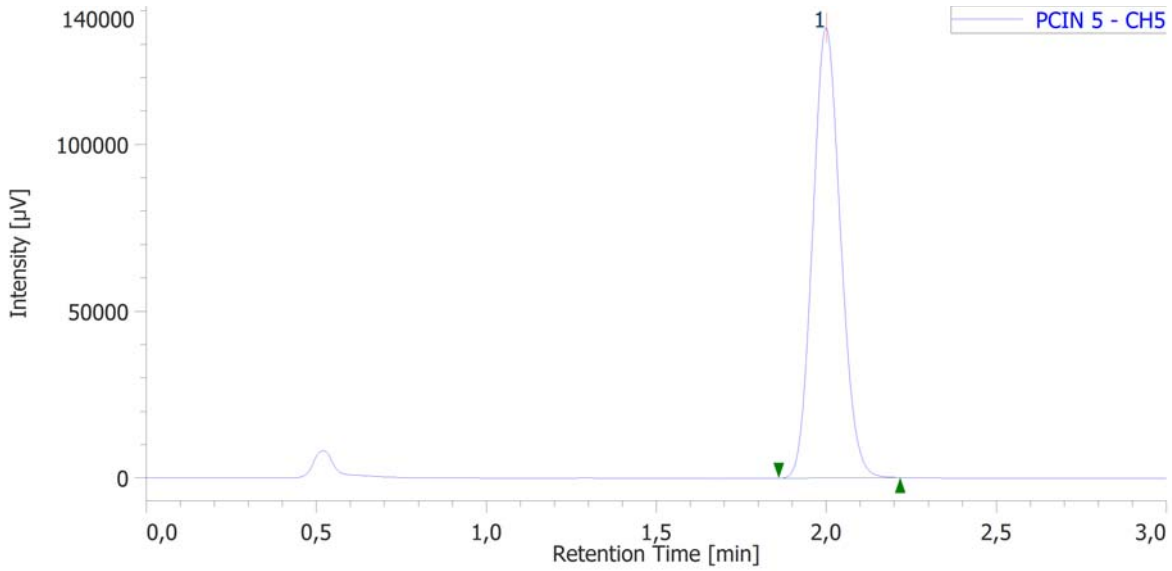

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:28
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 12:00:46
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,000	768989	134829	100,000	100,000	N/A	2833	N/A	1,090	

Creator Administrator
Reviewer
Approver

Chromatogram

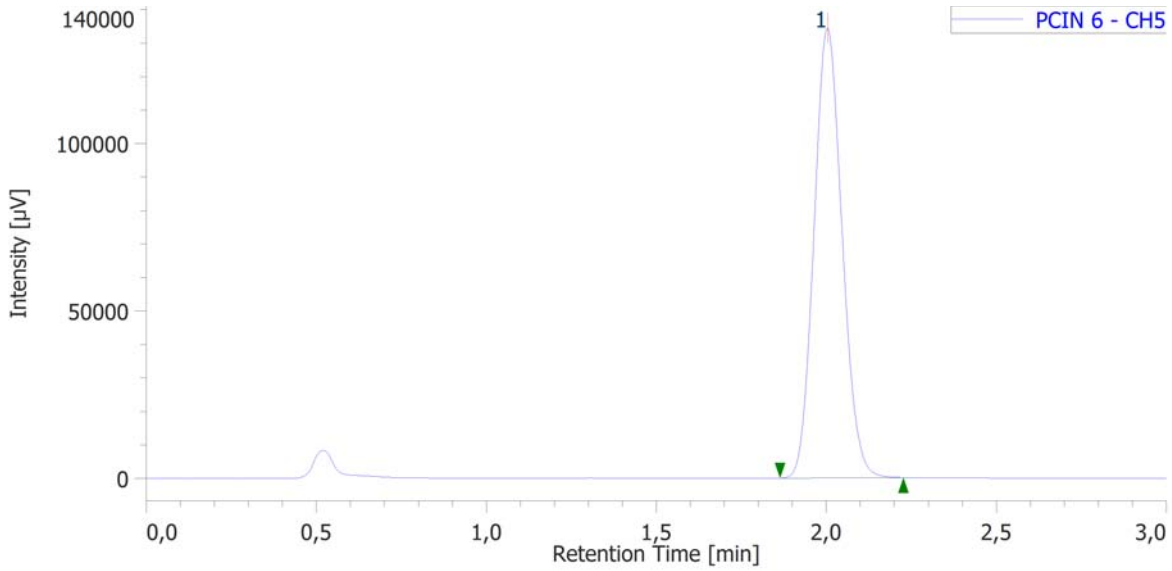

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:29
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 12:03:58
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,003	769311	134300	100,000	100,000	N/A	2817	N/A	1,102	

Creator Administrator
Reviewer
Approver

Chromatogram

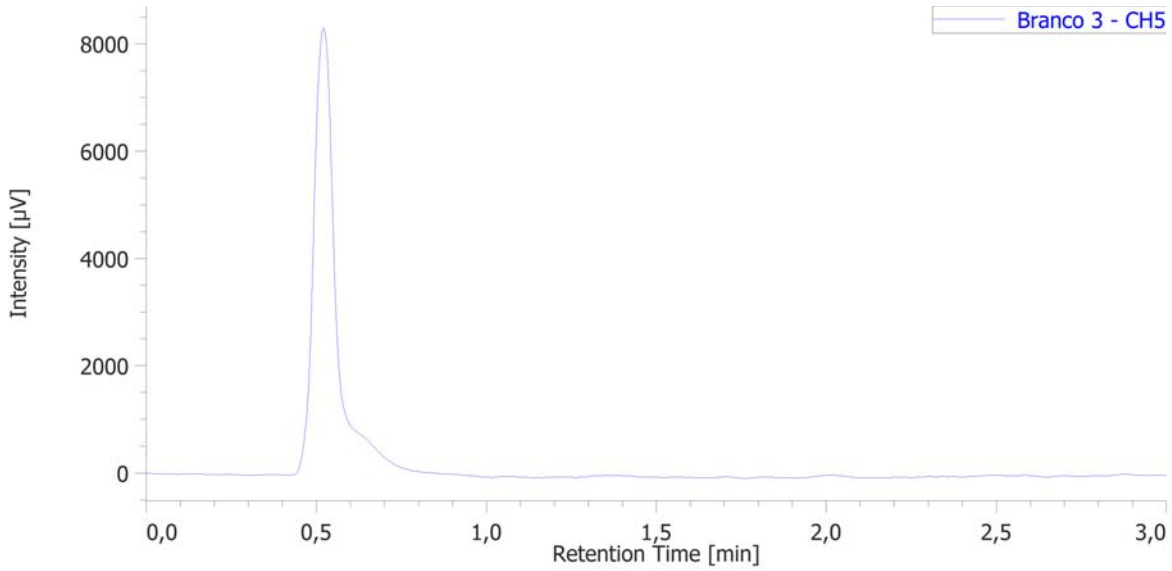


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 12:11:29
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 12:07:10
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

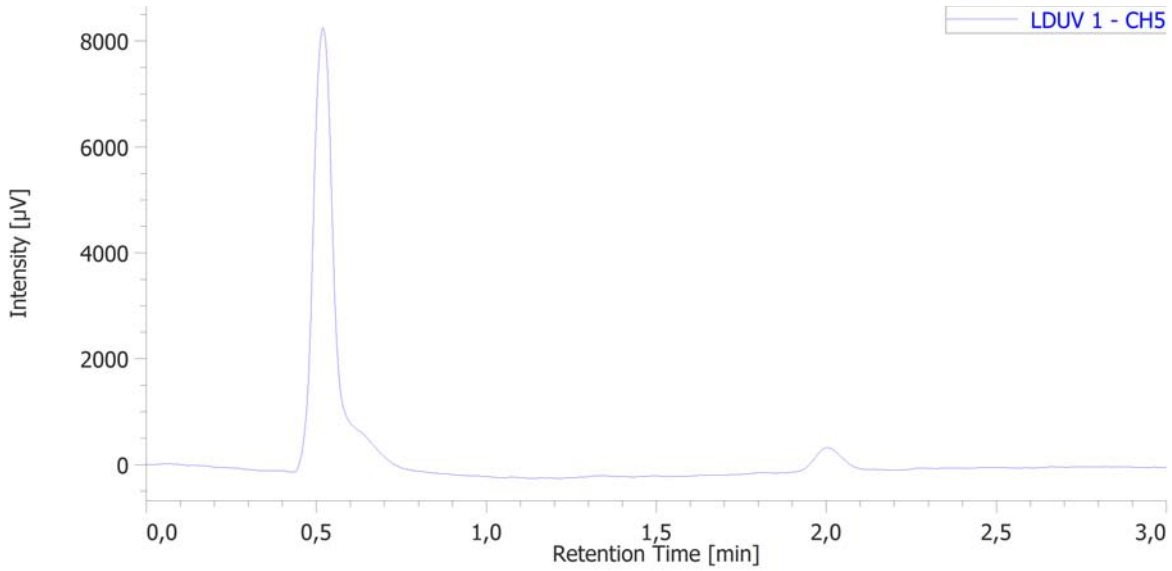


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 13:28:44
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:11:01
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

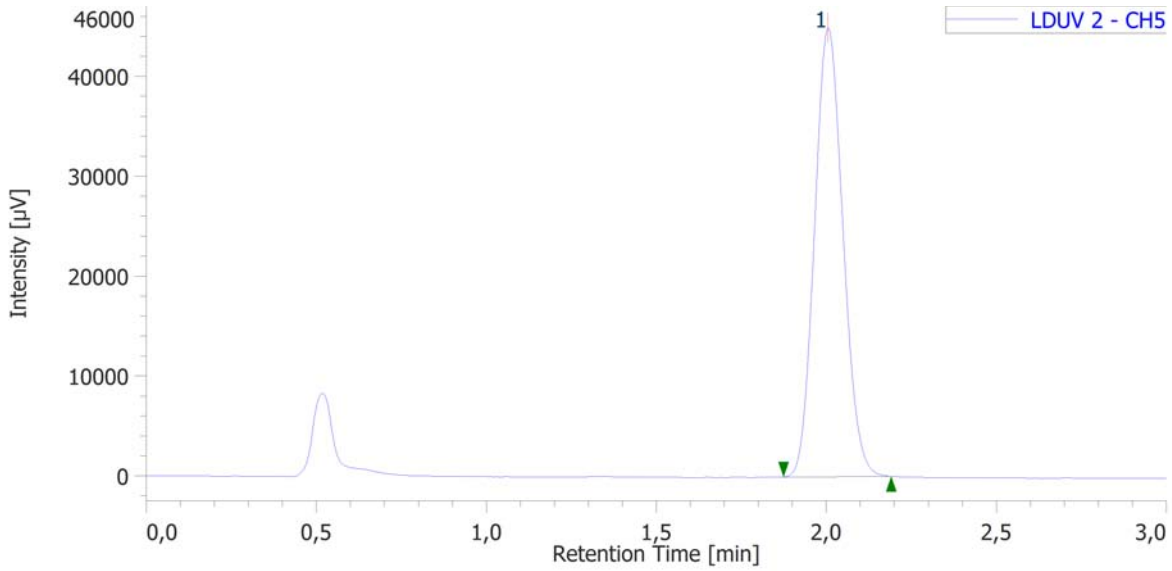

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 13:28:44
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:14:13
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,003	260902	44895	100,000	100,000	N/A	2713	N/A	1,129	

Creator Administrator
Reviewer
Approver

Chromatogram

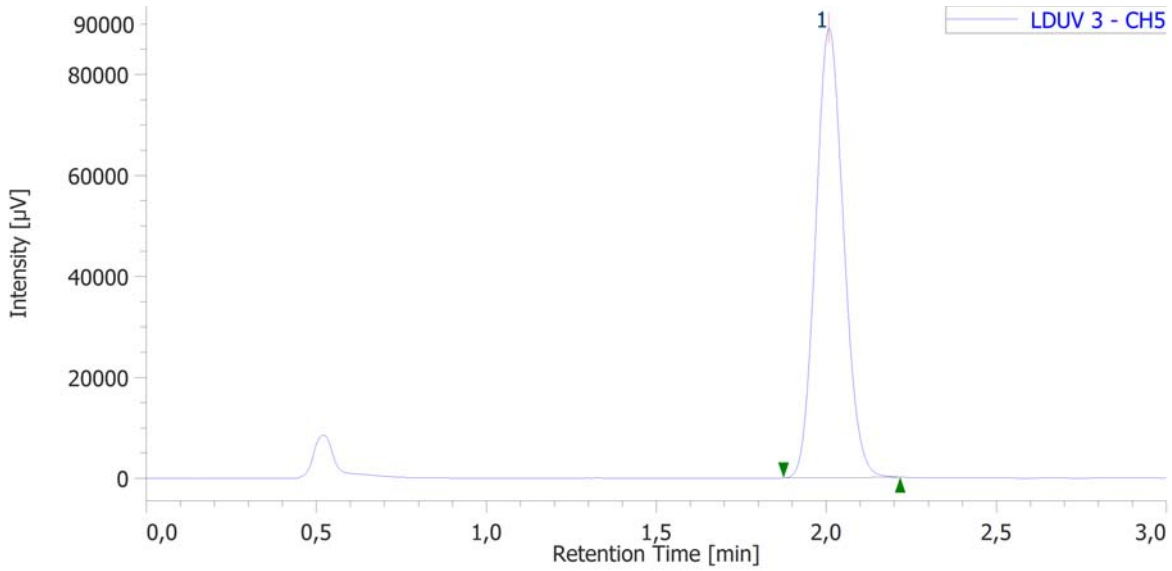

Chromatogram Information

User Name	Administrator
Date Modified	20/04/2018 13:28:45
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:17:25
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,007	508351	89029	100,000	100,000	N/A	2838	N/A	1,120	

Creator Administrator
Reviewer
Approver

Chromatogram

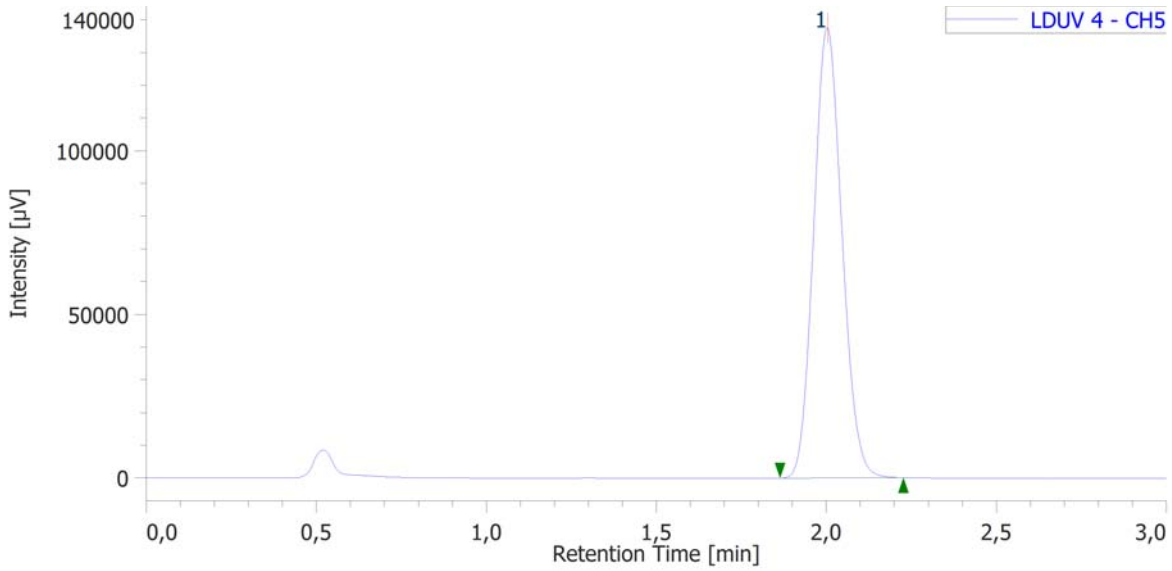

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 13:28:45
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:20:37
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,003	794148	137443	100,000	100,000	N/A	2767	N/A	1,095	

Creator Administrator
Reviewer
Approver

Chromatogram

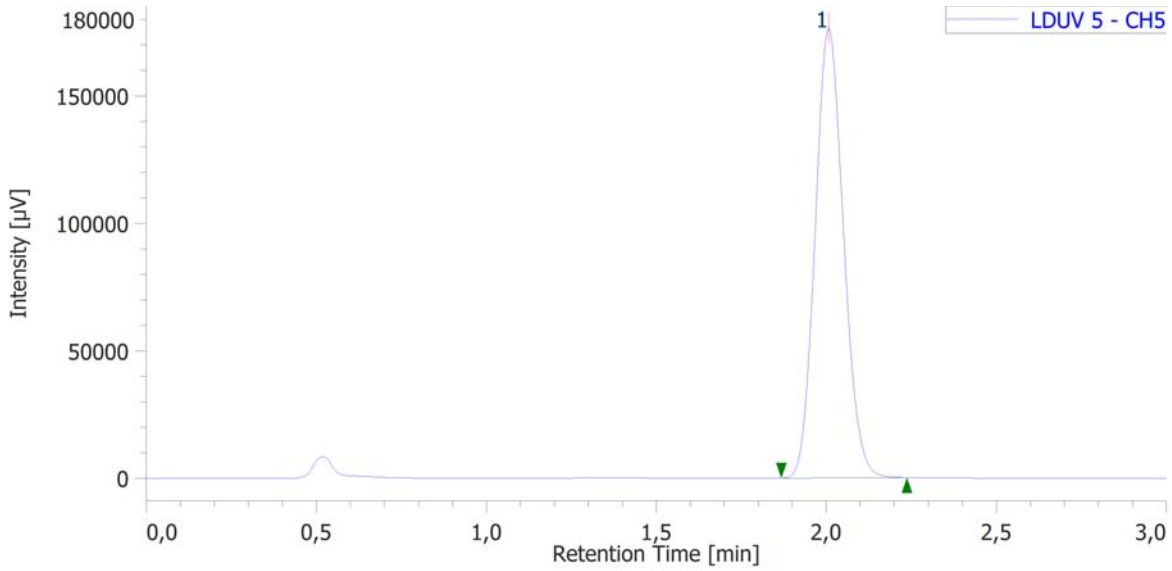

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 13:28:45
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:23:49
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,007	1021728	176340	100,000	100,000	N/A	2770	N/A	1,110	

Creator Administrator
Reviewer
Approver

Chromatogram

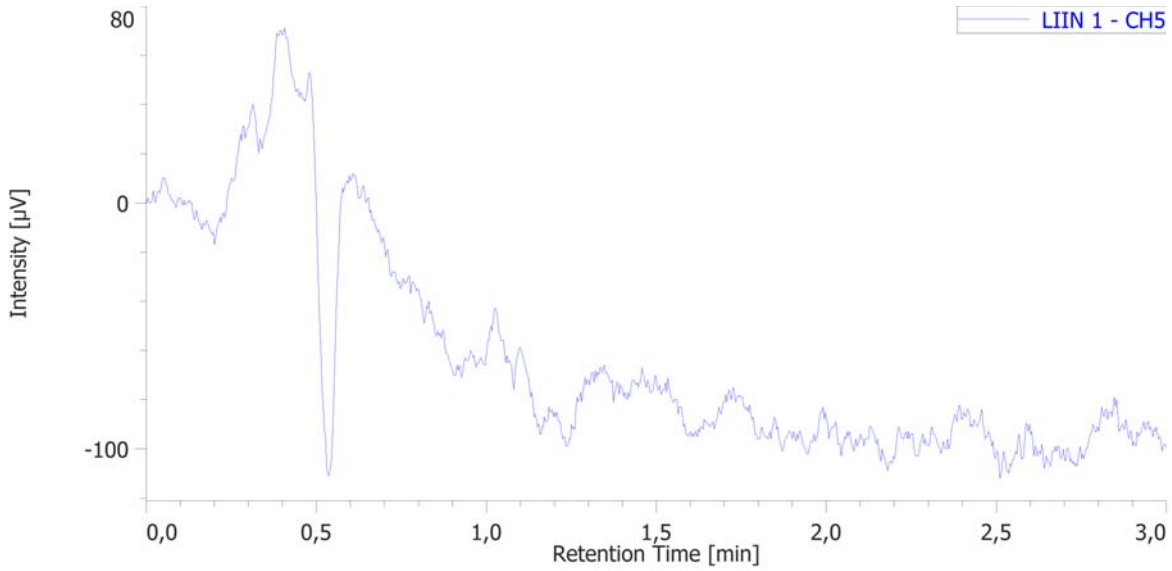


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:00:44
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:36:45
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

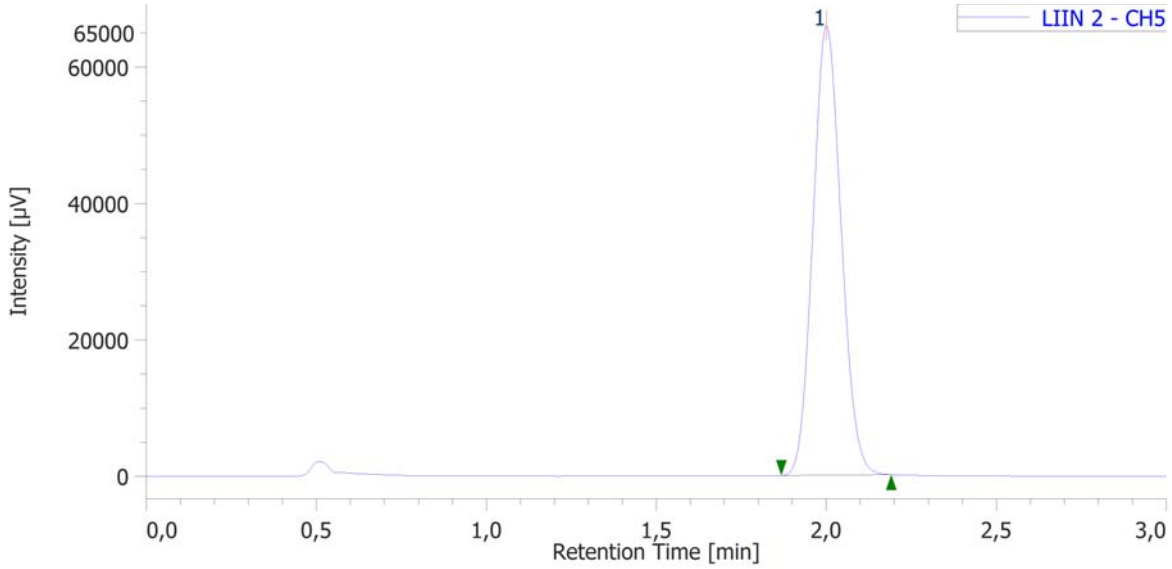

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:00:44
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:39:57
Volume	5,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,000	379841	65812	100,000	100,000	N/A	2738	N/A	1,098	

Creator Administrator
Reviewer
Approver

Chromatogram

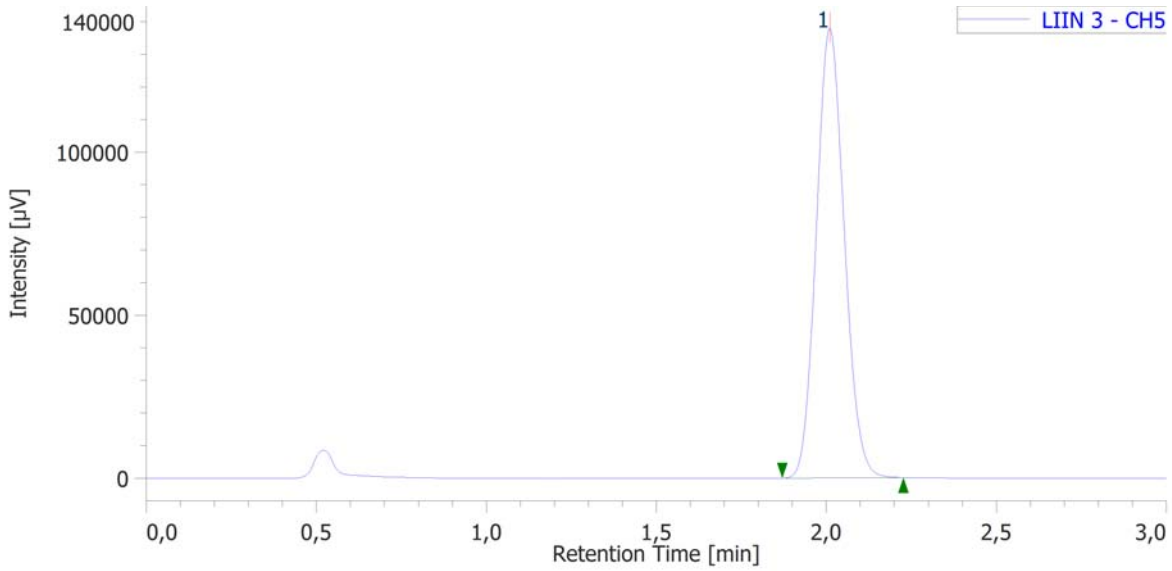

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:00:45
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:43:09
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,010	788015	137895	100,000	100,000	N/A	2850	N/A	1,097	

Creator Administrator
Reviewer
Approver

Chromatogram

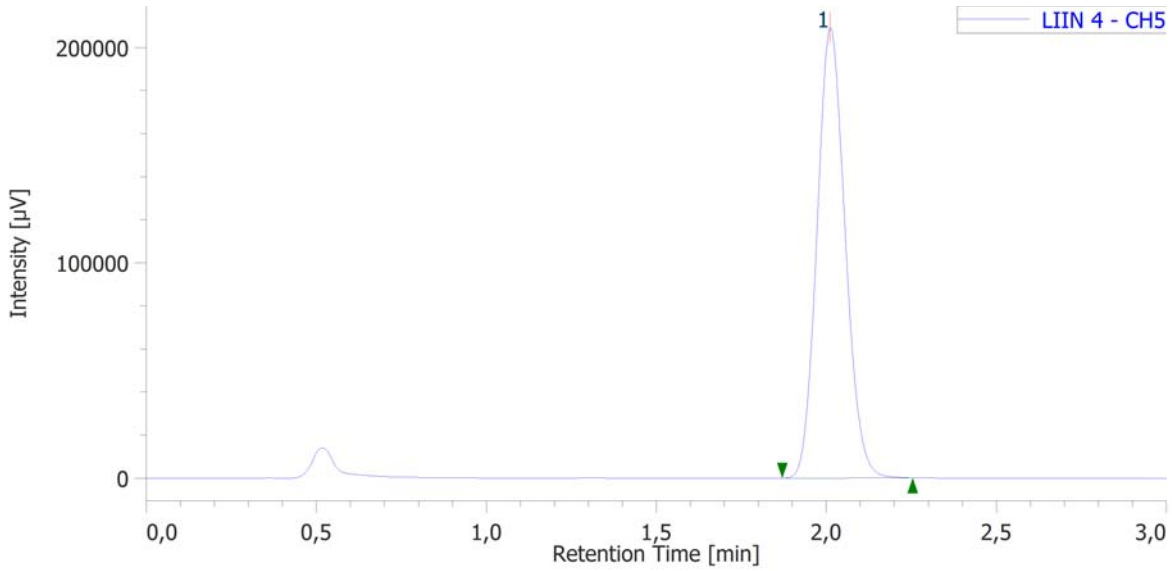

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:00:45
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:46:21
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,010	1203965	208897	100,000	100,000	N/A	2819	N/A	1,136	

Creator Administrator
Reviewer
Approver

Chromatogram

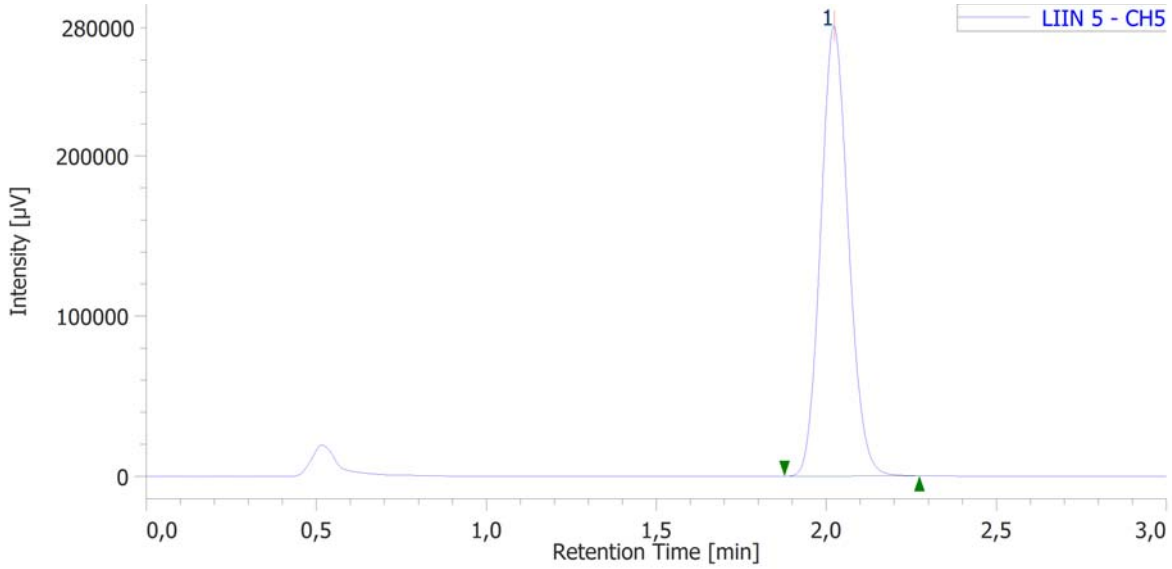

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:00:46
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 13:49:33
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,023	1591729	280809	100,000	100,000	N/A	2977	N/A	1,096	

Creator Administrator
Reviewer
Approver

Chromatogram

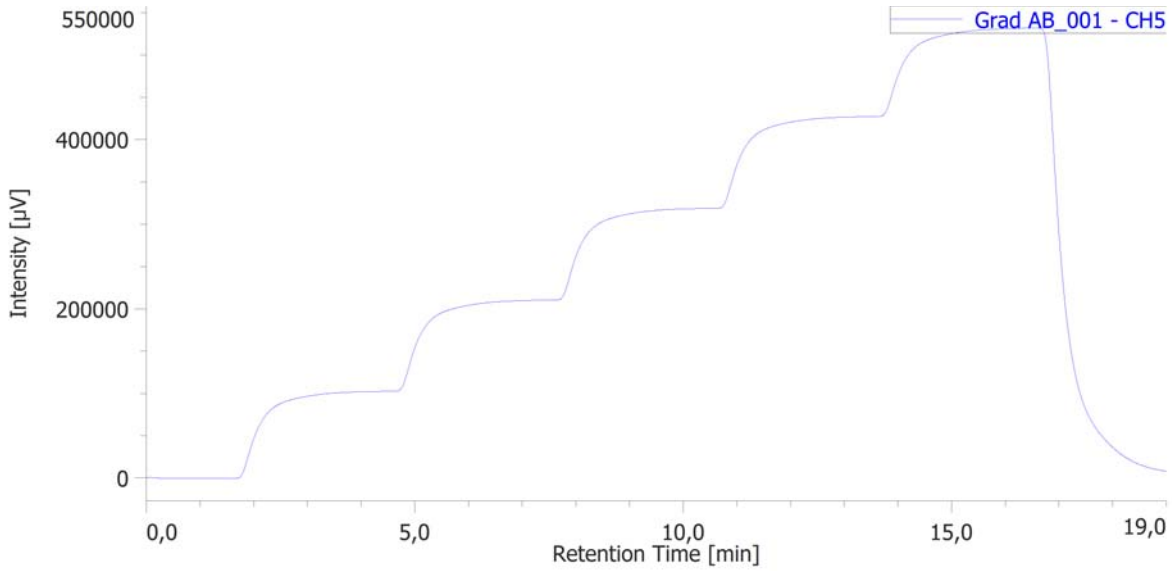


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:33:27
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 14:12:50
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação - Grad

Creator Administrator
Reviewer
Approver

Chromatogram

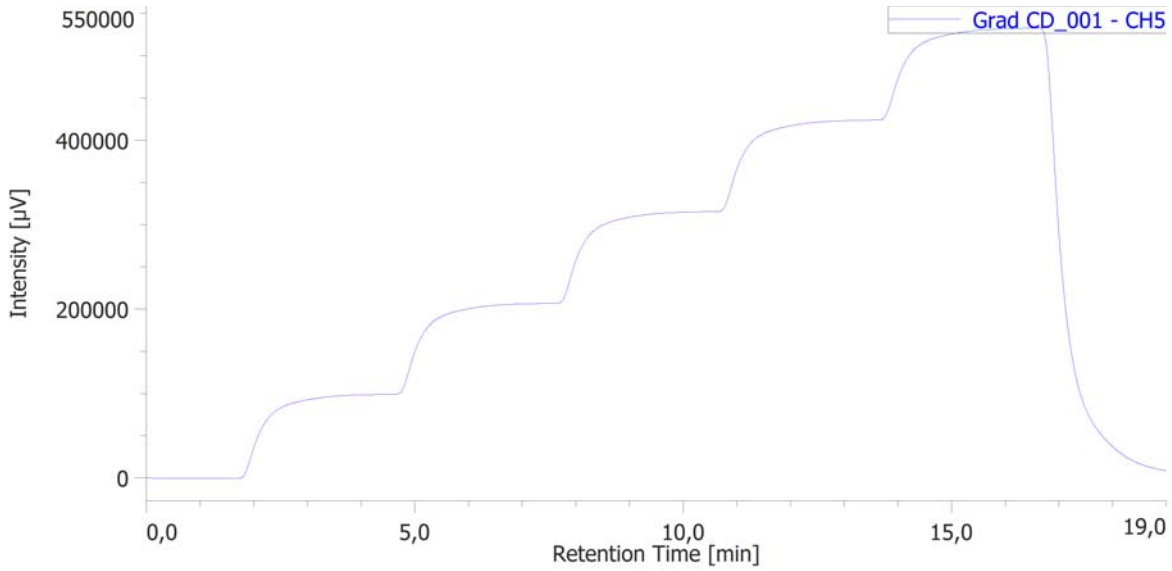

Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2018 14:57:01
Description	
HPLC System Name	01-HP-03
Injection Date	20/04/2018 14:37:06
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Qualificação - Grad

Creator Administrator
Reviewer
Approver