
Chromatogram

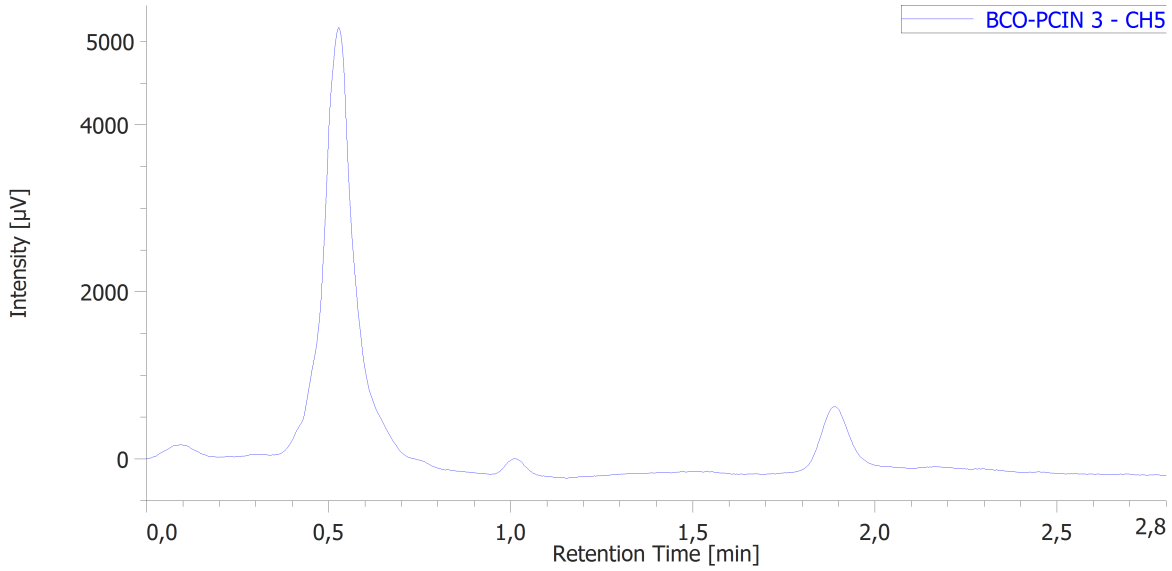


Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:32
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:35:44
Volume	10,00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BCO-PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

Creator	Administrator
Reviewer	
Approver	

Chromatogram

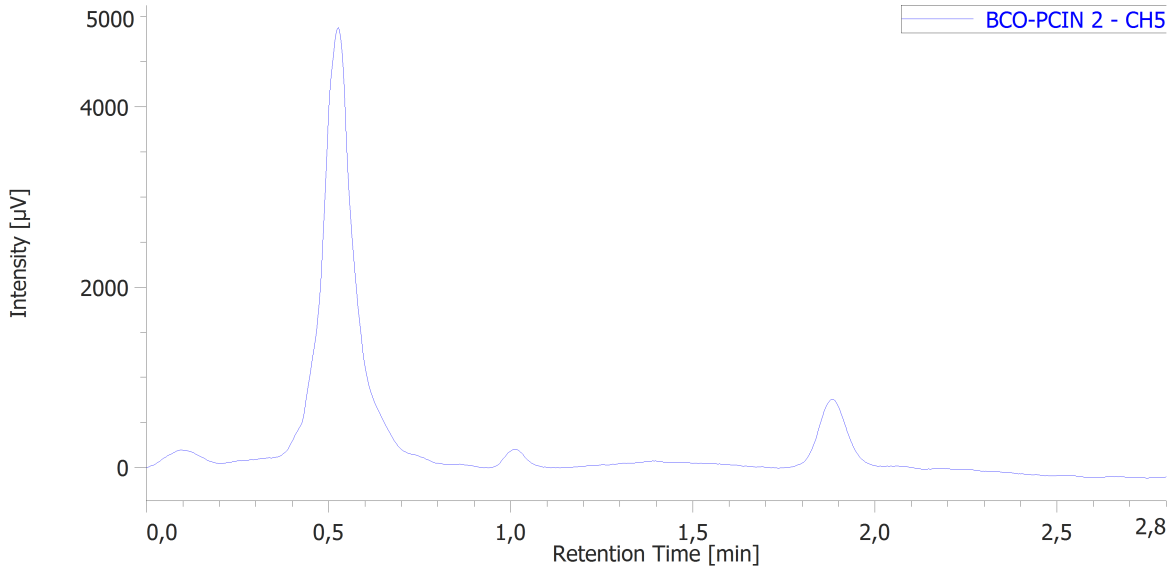


Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:29
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:23:44
Volume	10,00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BCO-PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

Creator	Administrator
Reviewer	
Approver	

Chromatogram

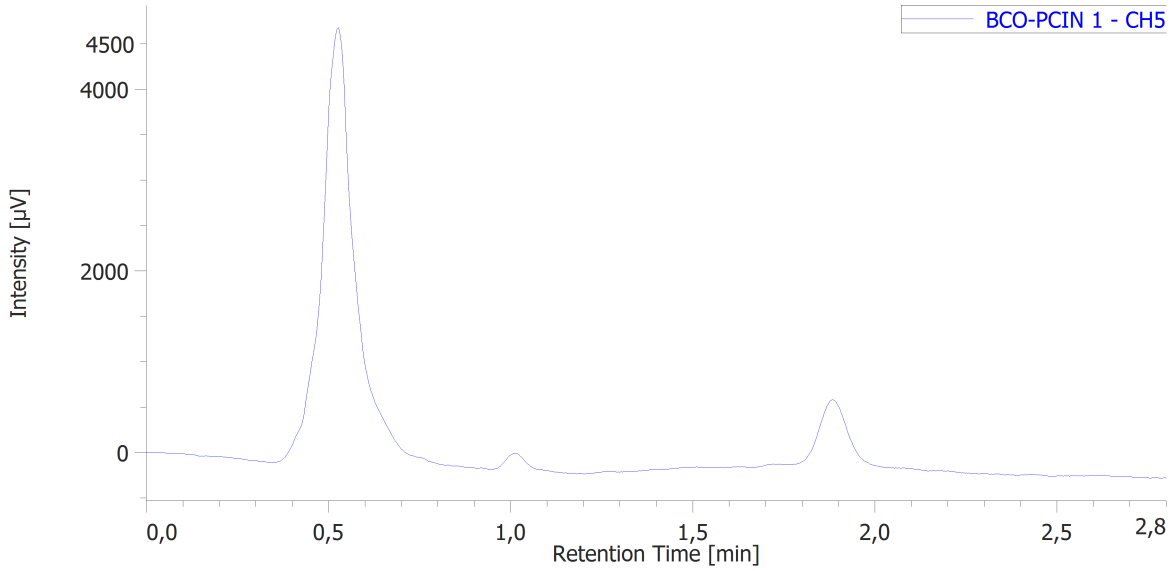

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:26
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:11:44
Volume	10,00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	BCO-PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA


Creator	Administrator
Reviewer	
Approver	

PDA


Sequence Name GRADIENTE CD_20042017 20/04/2017 12:18:38
Chromatogram Name GRADIENTE CD_002
Sample Name

Contour+Chrom+Spec

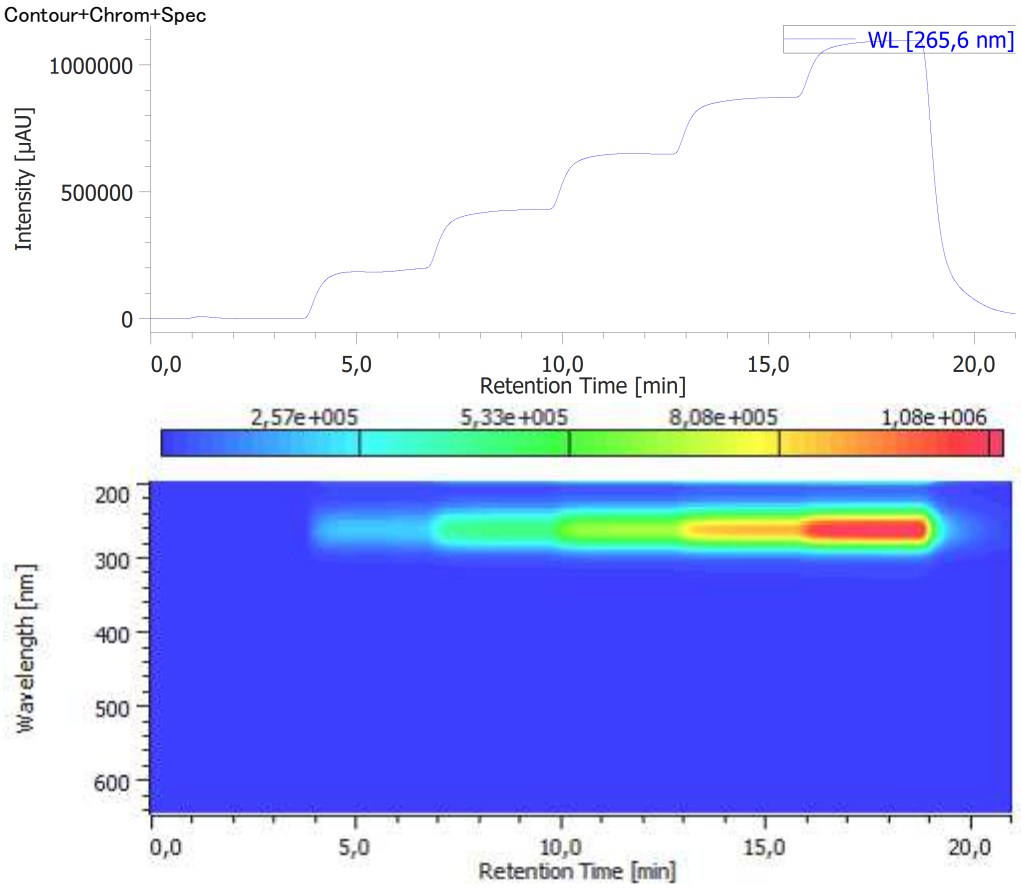

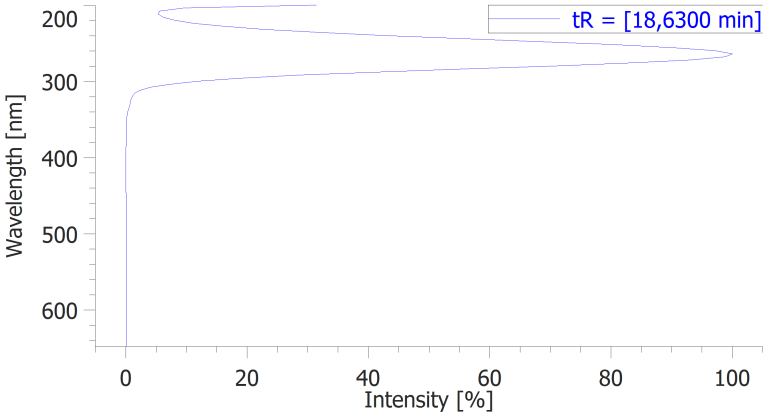

Chromatogram

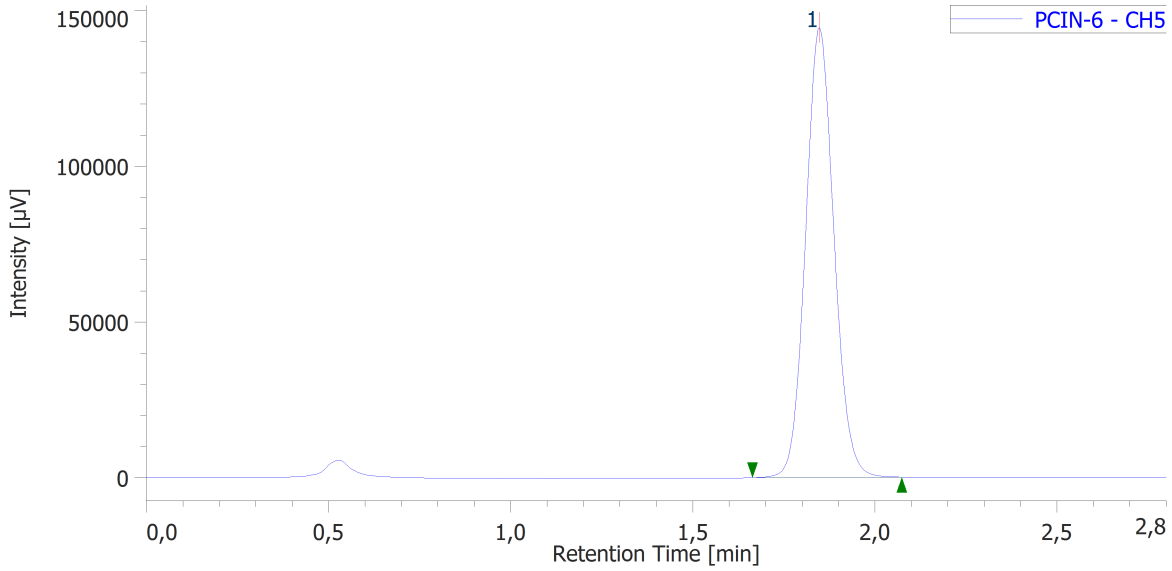

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:31
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:32:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,847	781676	144297	100,000	100,000	N/A	2748	N/A	1,090	

Creator Administrator
Reviewer
Approver

Chromatogram

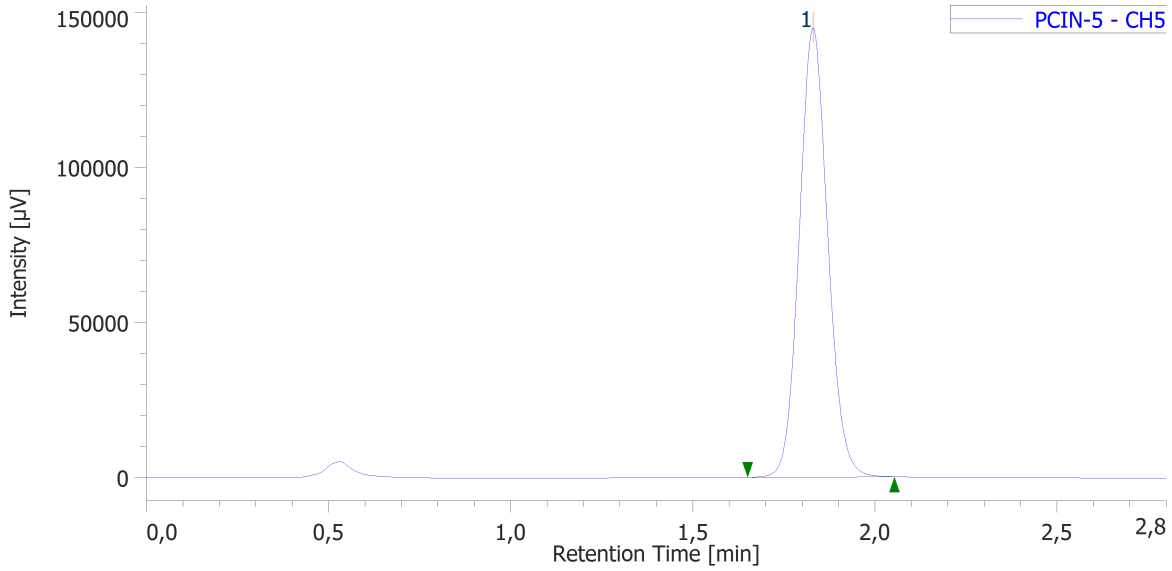

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:31
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:29:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,830	786107	144696	100,000	100,000	N/A	2681	N/A	1,088	

Creator Administrator
Reviewer
Approver

Chromatogram

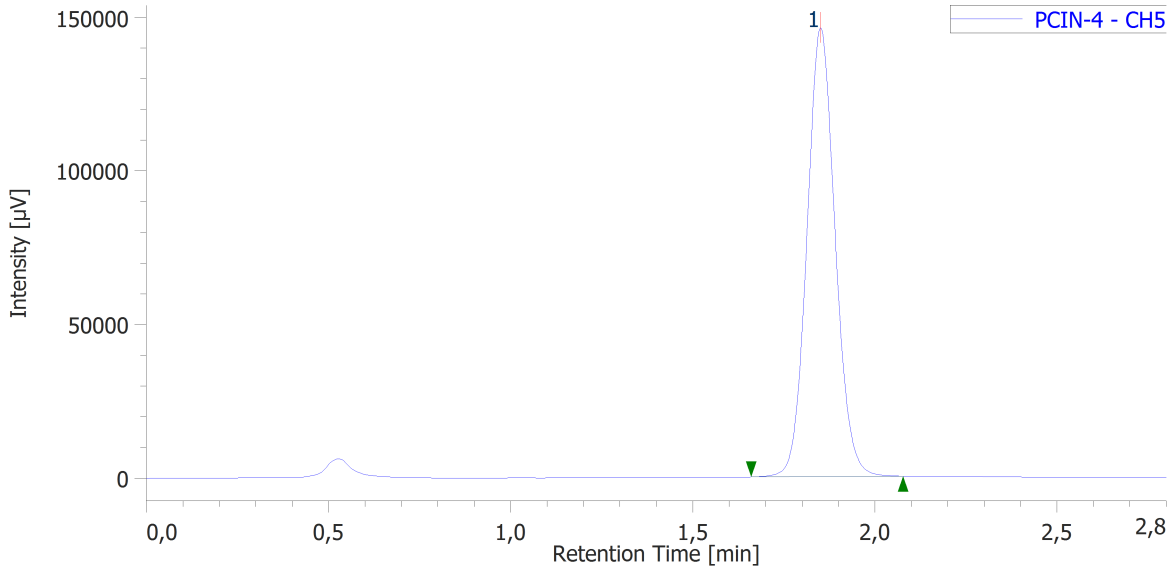

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:30
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:26:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,850	784677	145953	100,000	100,000	N/A	2808	N/A	1,088	

Creator Administrator
Reviewer
Approver

Chromatogram

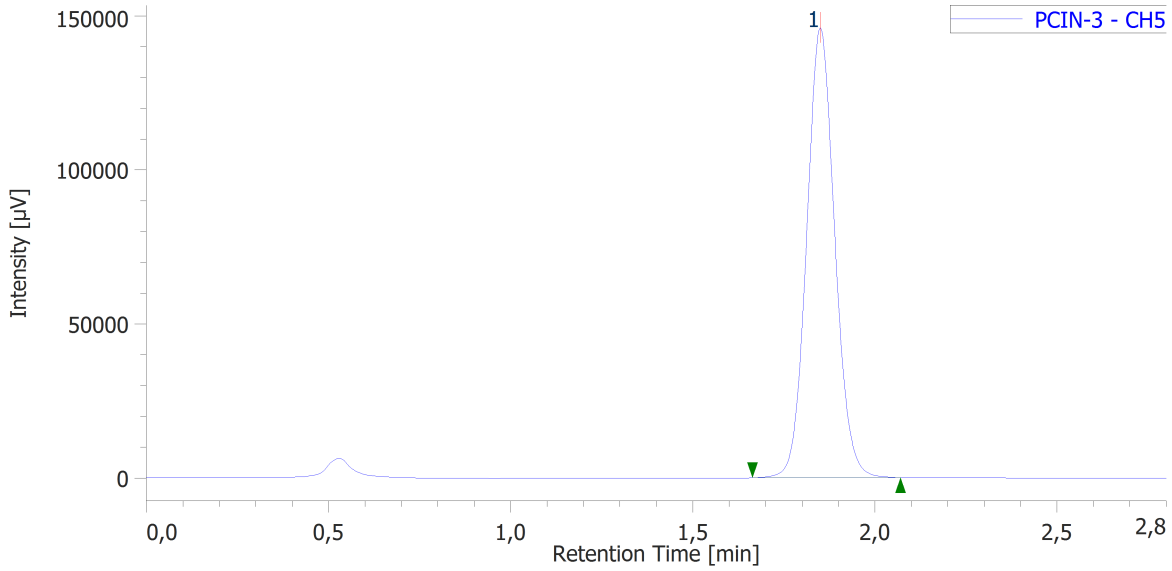

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:28
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:20:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,850	782339	145990	100,000	100,000	N/A	2828	N/A	1,072	

Creator Administrator
Reviewer
Approver

Chromatogram

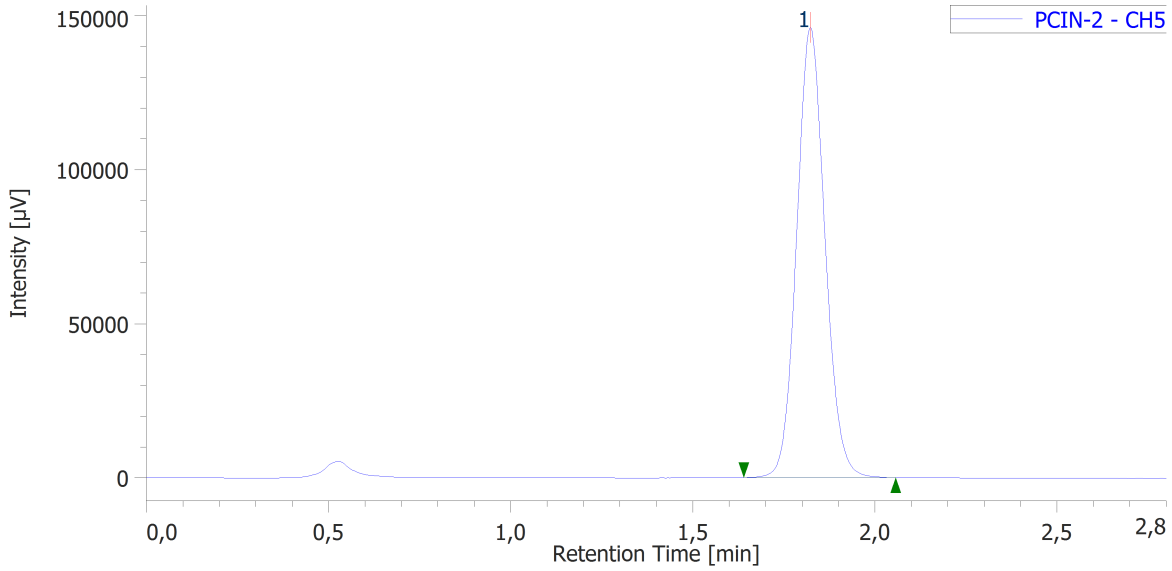

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:28
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:17:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,823	786632	145912	100,000	100,000	N/A	2709	N/A	1,076	

Creator Administrator
Reviewer
Approver

Chromatogram

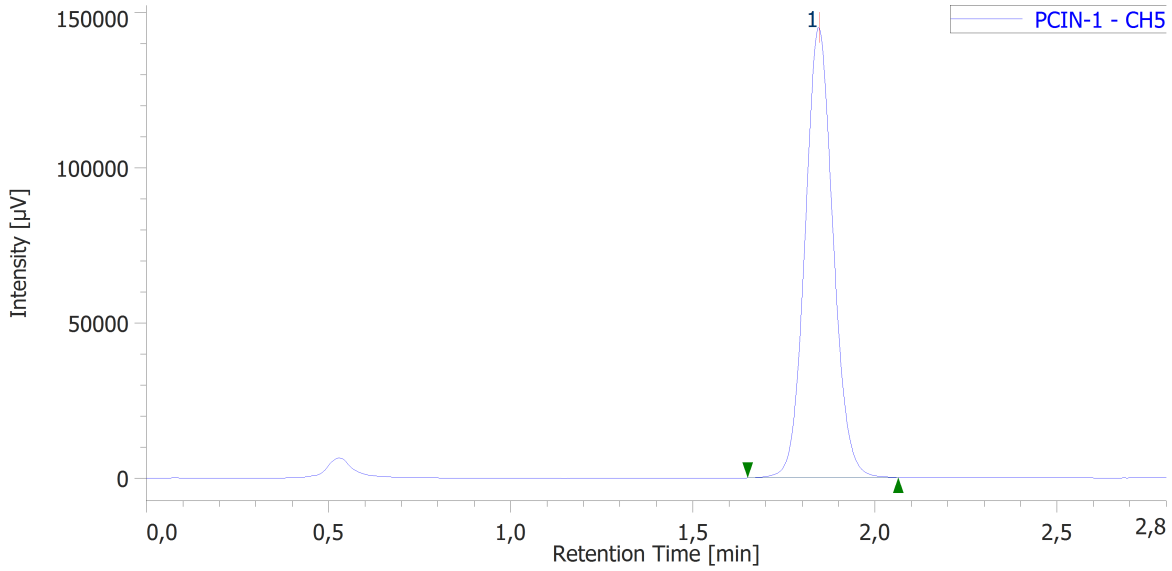

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 18:46:27
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 16:14:44
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	PCIN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN-1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,847	777092	145039	100,000	100,000	N/A	2823	N/A	1,057	

Creator Administrator
Reviewer
Approver

Chromatogram

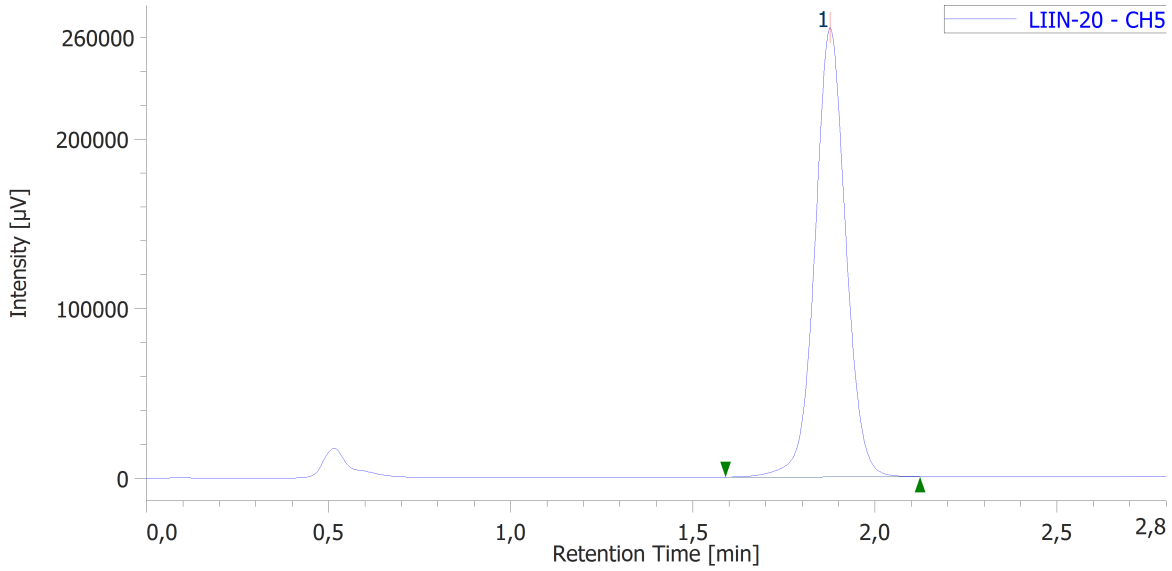

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:16:46
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:49:19
Volume	20,00 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LINN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN-20-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,877	1556668	264790	100,000	100,000	N/A	2497	N/A	1,031	

Creator Administrator
Reviewer
Approver

Chromatogram

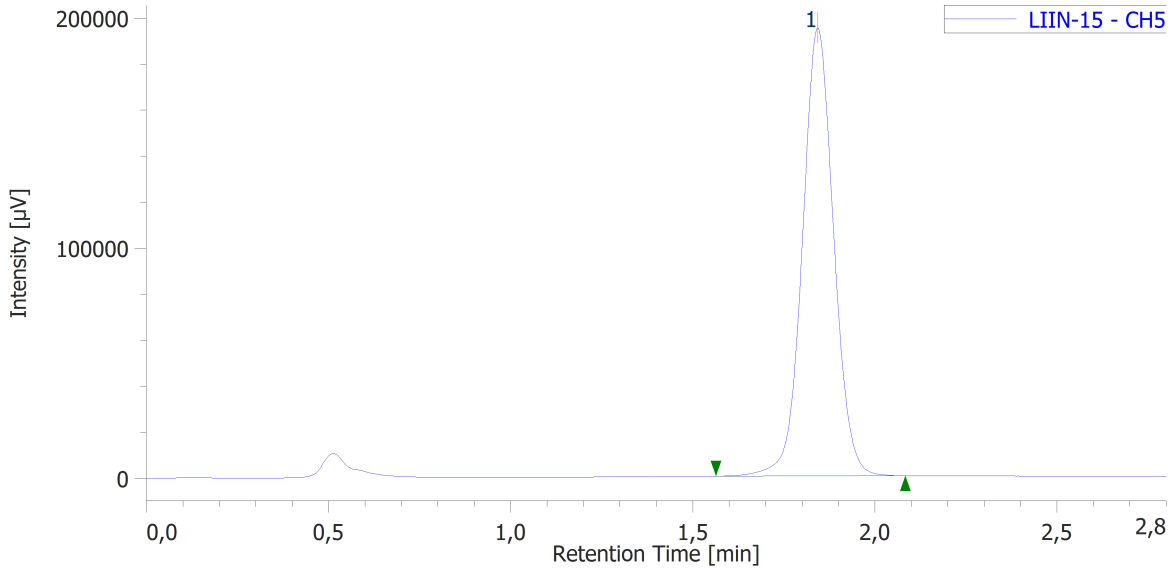

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:16:45
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:46:19
Volume	15,00 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LINN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN-15-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,843	1162059	194718	100,000	100,000	N/A	2312	N/A	1,030	

Creator Administrator
Reviewer
Approver

Chromatogram

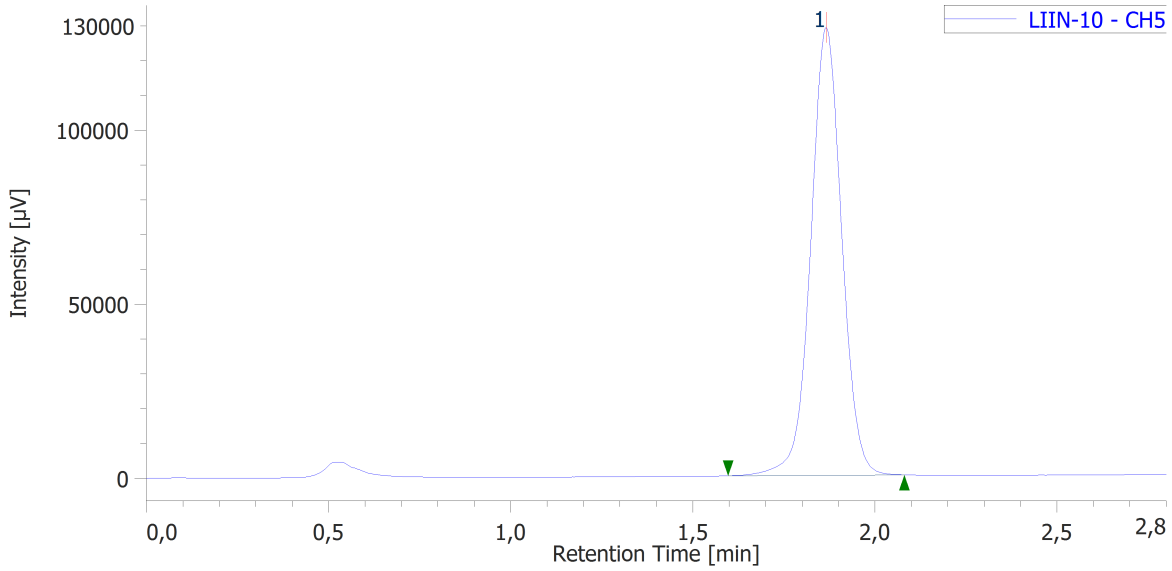

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:16:45
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:43:19
Volume	10,00 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LINN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN-10-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,867	761140	128528	100,000	100,000	N/A	2410	N/A	1,004	

Creator Administrator
Reviewer
Approver

Chromatogram

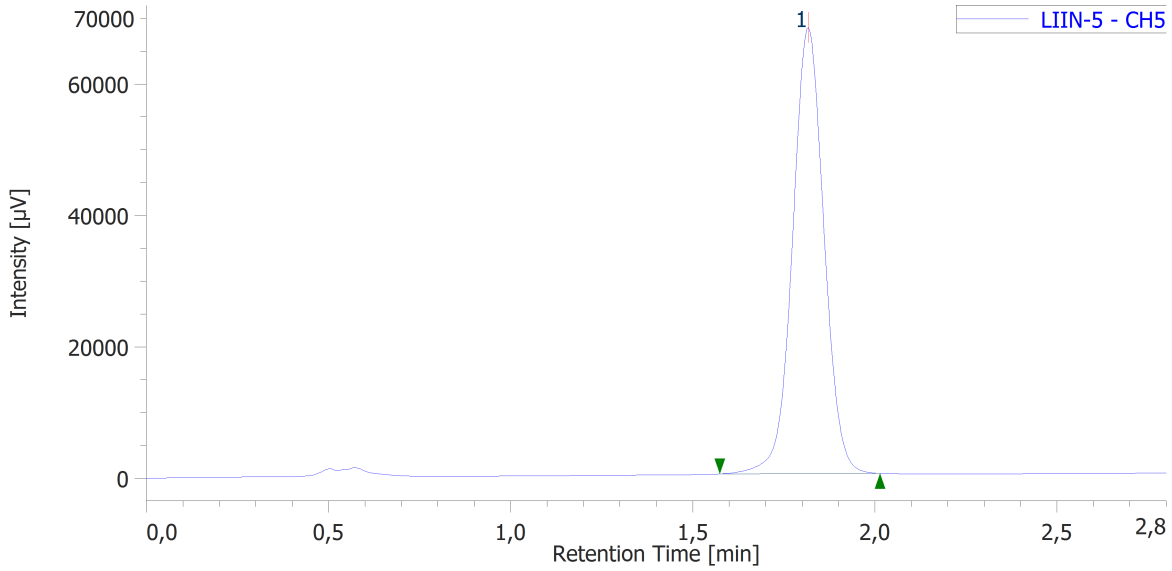

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:16:43
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:40:19
Volume	5,00 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LINN
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN-5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,817	407089	67830	100,000	100,000	N/A	2195	N/A	1,015	

Creator Administrator
Reviewer
Approver

Chromatogram

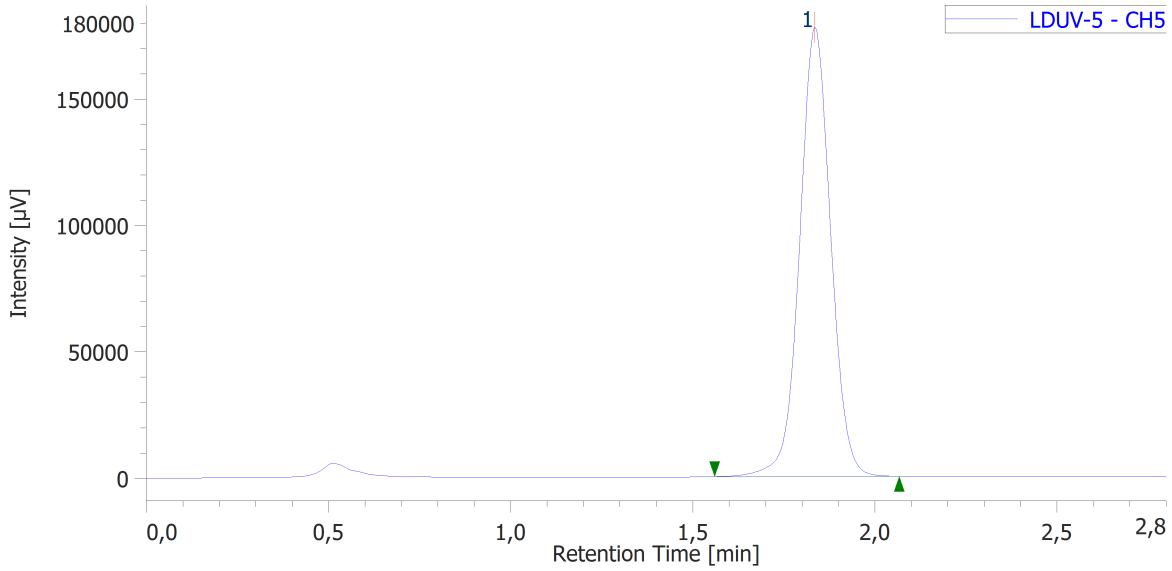

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:28:38
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:28:07
Volume	10,00 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LDUV
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV-5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,833	1053012	177464	100,000	100,000	N/A	2315	N/A	1,044	

Creator Administrator
Reviewer
Approver

Chromatogram

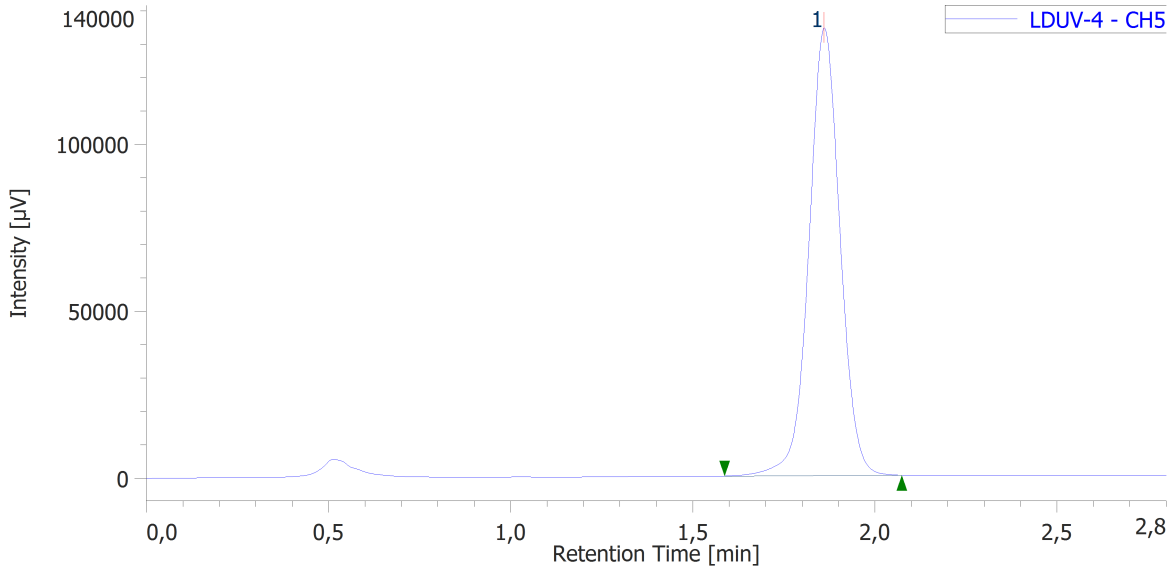

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:28:38
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:25:07
Volume	10,00 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LDUV
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV-4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,860	794125	134032	100,000	100,000	N/A	2398	N/A	1,022	

Creator Administrator
Reviewer
Approver

Chromatogram

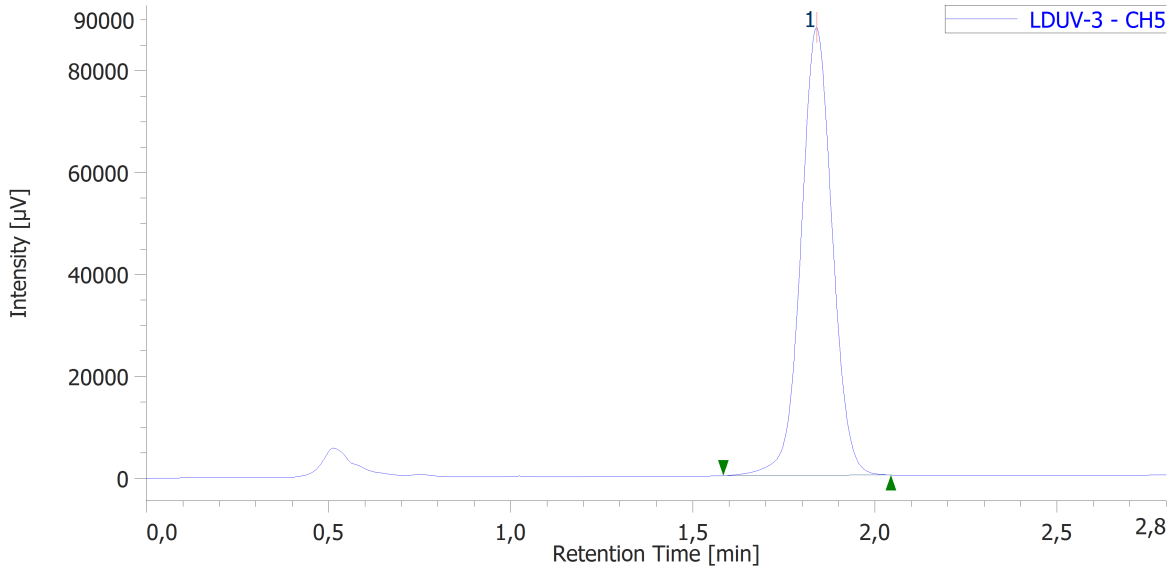

Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:28:37
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:22:07
Volume	10,00 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LDUV
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV-3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,840	524929	87819	100,000	100,000	N/A	2284	N/A	1,014	

Creator Administrator
Reviewer
Approver

Chromatogram

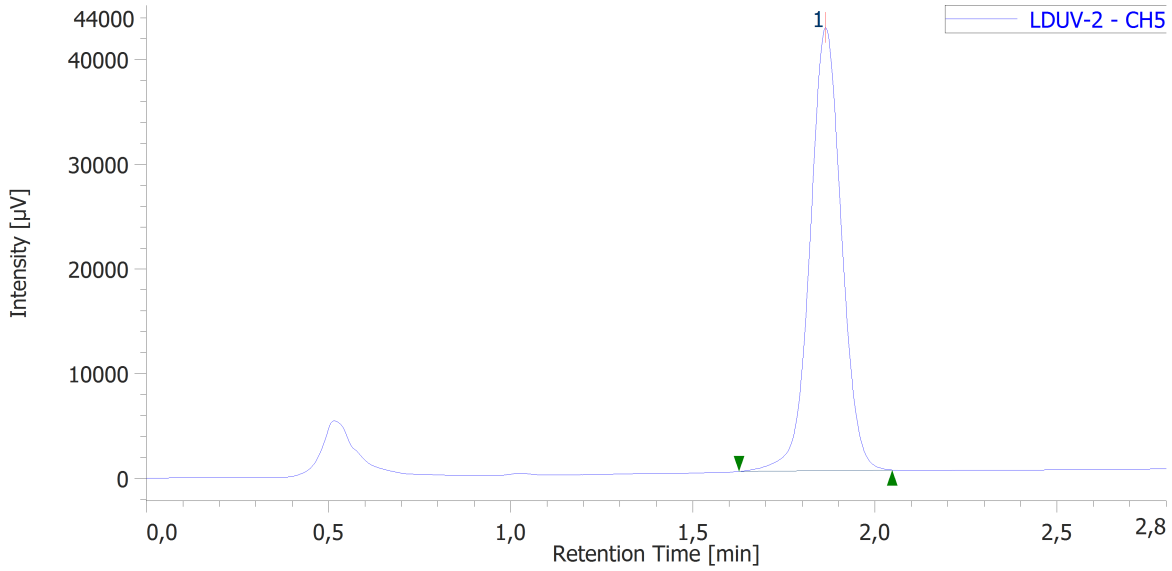

Chromatogram Information

User Name	Administrator
Date Modified	25/04/2017 19:28:37
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:19:07
Volume	10,00 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LDUV
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV-2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,863	252991	42295	100,000	100,000	N/A	2340	N/A	1,023	

Creator Administrator
Reviewer
Approver

Chromatogram

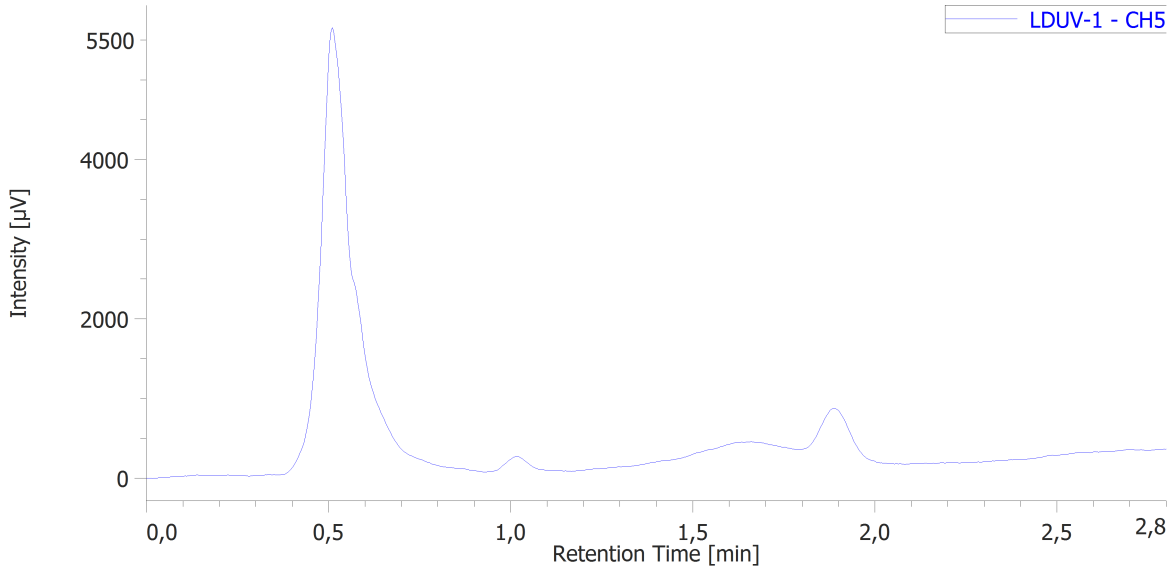


Chromatogram Information	
User Name	Administrator
Date Modified	25/04/2017 19:28:36
Description	
HPLC System Name	TRB
Injection Date	19/04/2017 17:16:07
Volume	10,00 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	2,8 [min]
Acquisition Sequence	LDUV
Control Method	QUALIFICAÇÃO 2017
Peak ID Table	Cafeina ID
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV-1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	CAFEINA

Creator	Administrator
Reviewer	
Approver	

Chromatogram

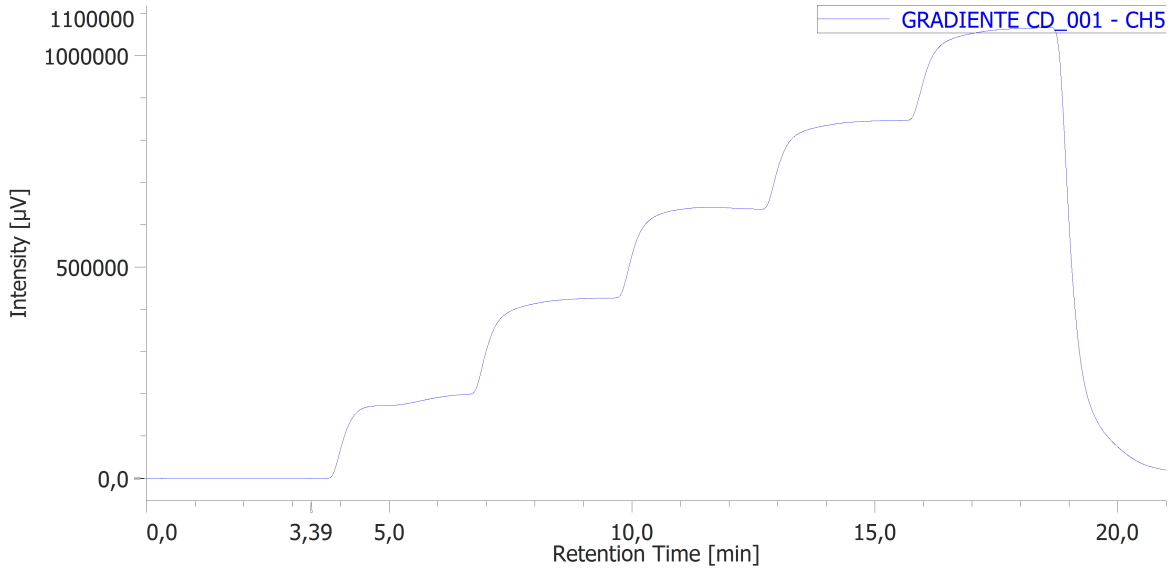


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2017 14:54:58
Description	
HPLC System Name	TRB
Injection Date	20/04/2017 14:33:56
Volume	0,00 [µL]
Sample #	–
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	GRAD CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRADIENTE CD_001-CH5
Sample Name	
Channel Name	265,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

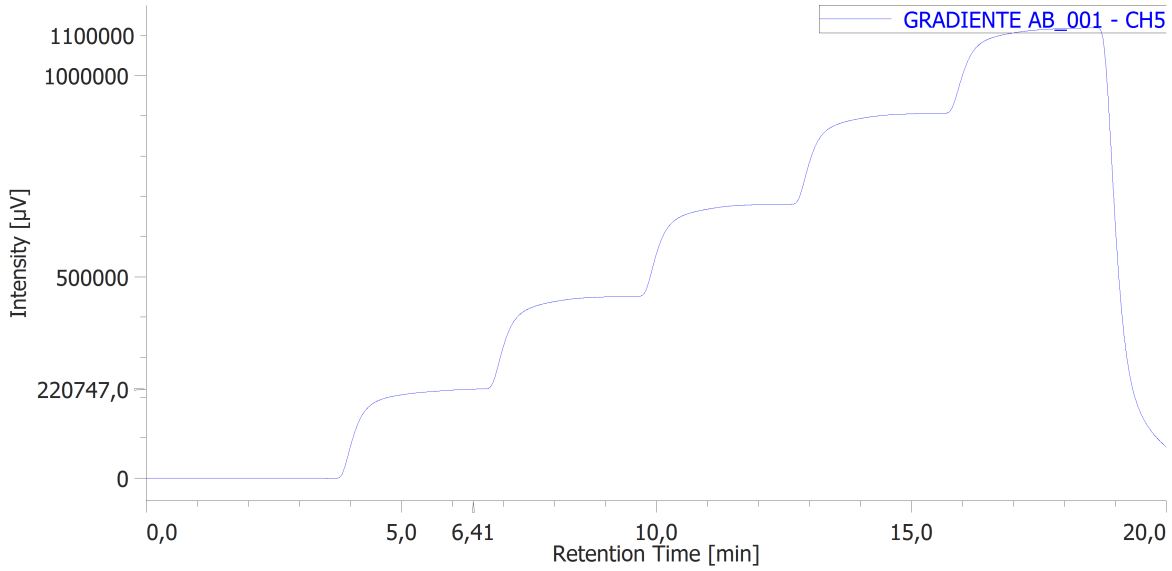


Chromatogram Information	
User Name	Administrator
Date Modified	20/04/2017 12:01:42
Description	
HPLC System Name	TRB
Injection Date	20/04/2017 11:41:40
Volume	0,00 [µL]
Sample #	–
Project Name	QUALIFICAÇÃO 2017
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	GRAD AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRADIENTE AB_001-CH5
Sample Name	
Channel Name	265,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Peak Find - EDUV PDA_1,8500.JWS

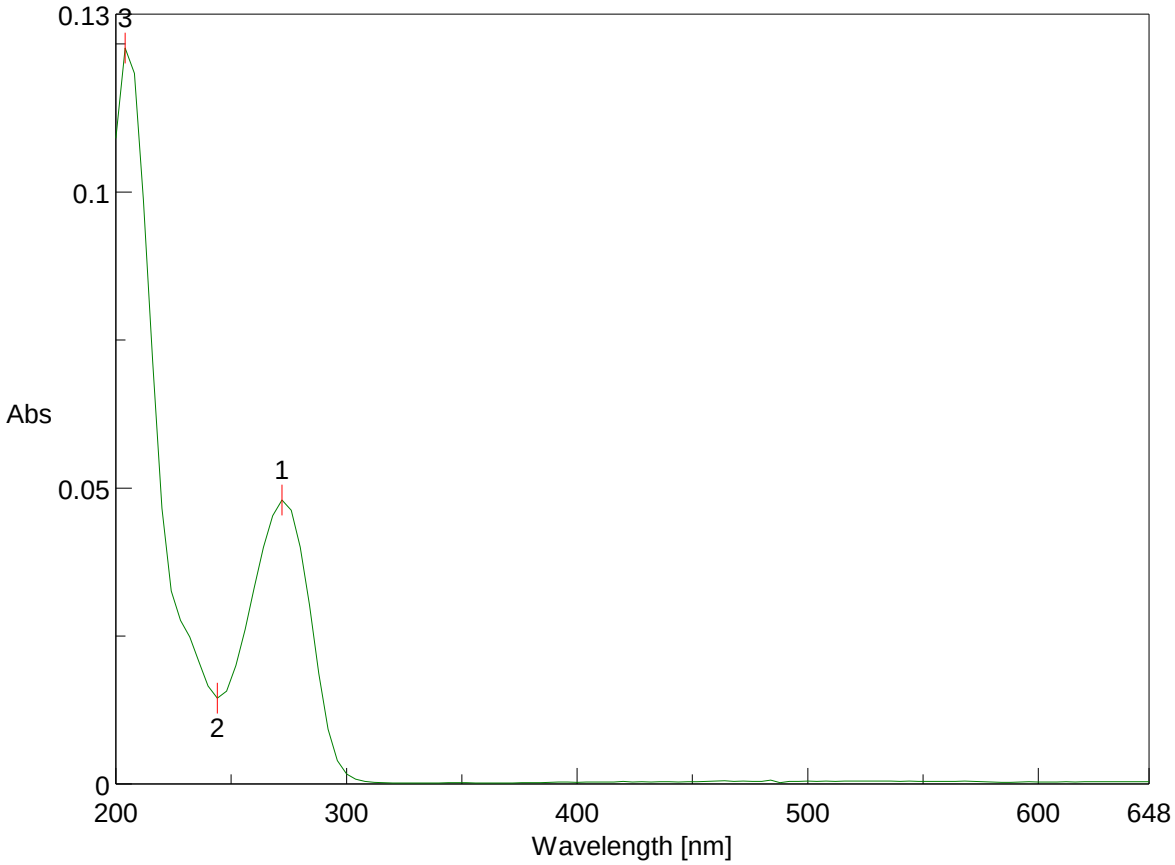

[Comments]

User	Administrator
Division	---
Company	Jasco Brasil
Creation date	19/04/2017 15:51

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113

[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A015061665
ROM version	V1.01.22

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.047946	2	244	0.014465
3	204	0.124252			