
Chromatogram

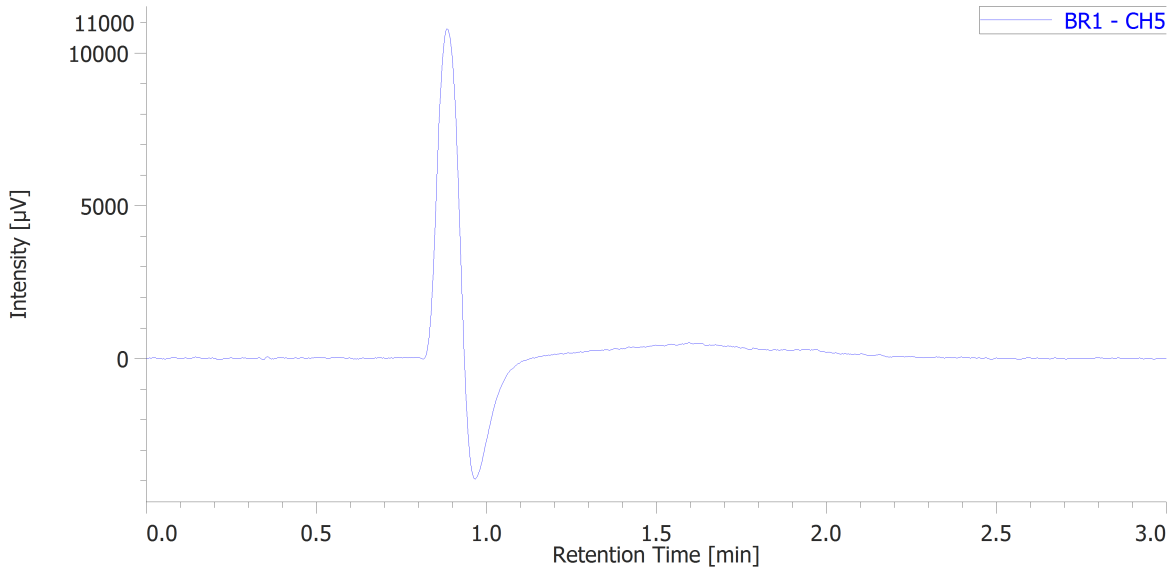


Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:30:58 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 3:40:02 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

Creator Administrator

Chromatogram

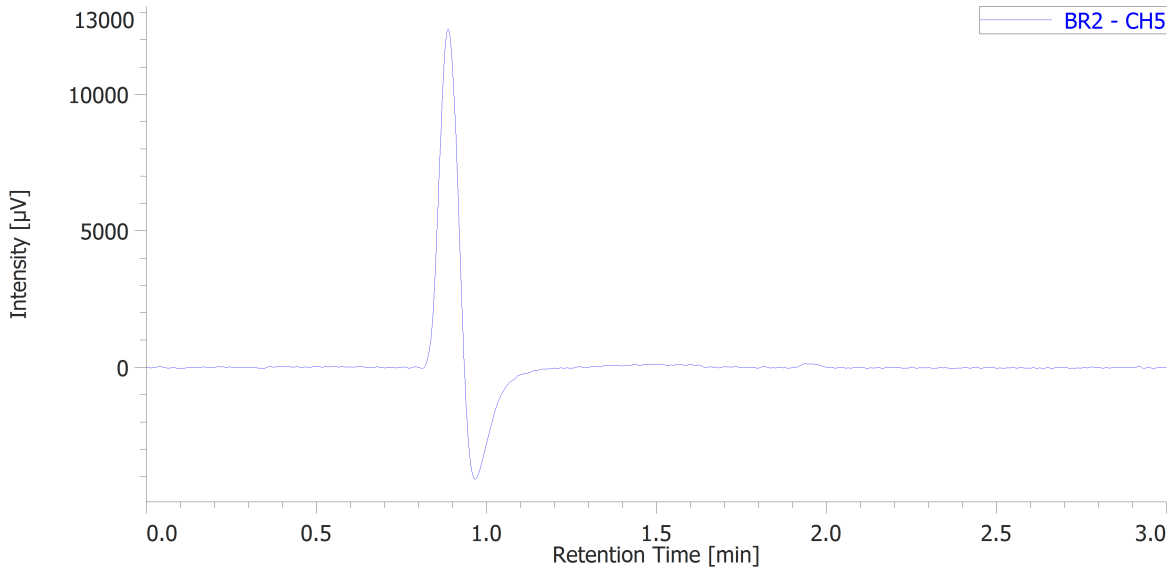


Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:05 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 3:56:04 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

Creator Administrator

Chromatogram

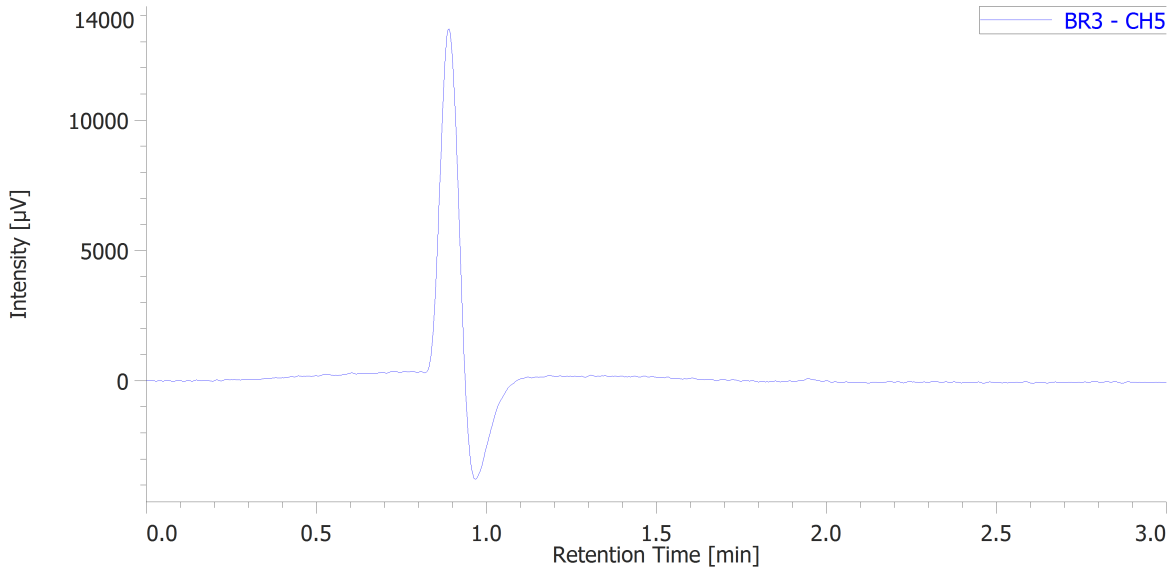


Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:08 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 4:11:54 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

Creator Administrator

Peak Find - EDUV_001 PDA_1.9733.JWS

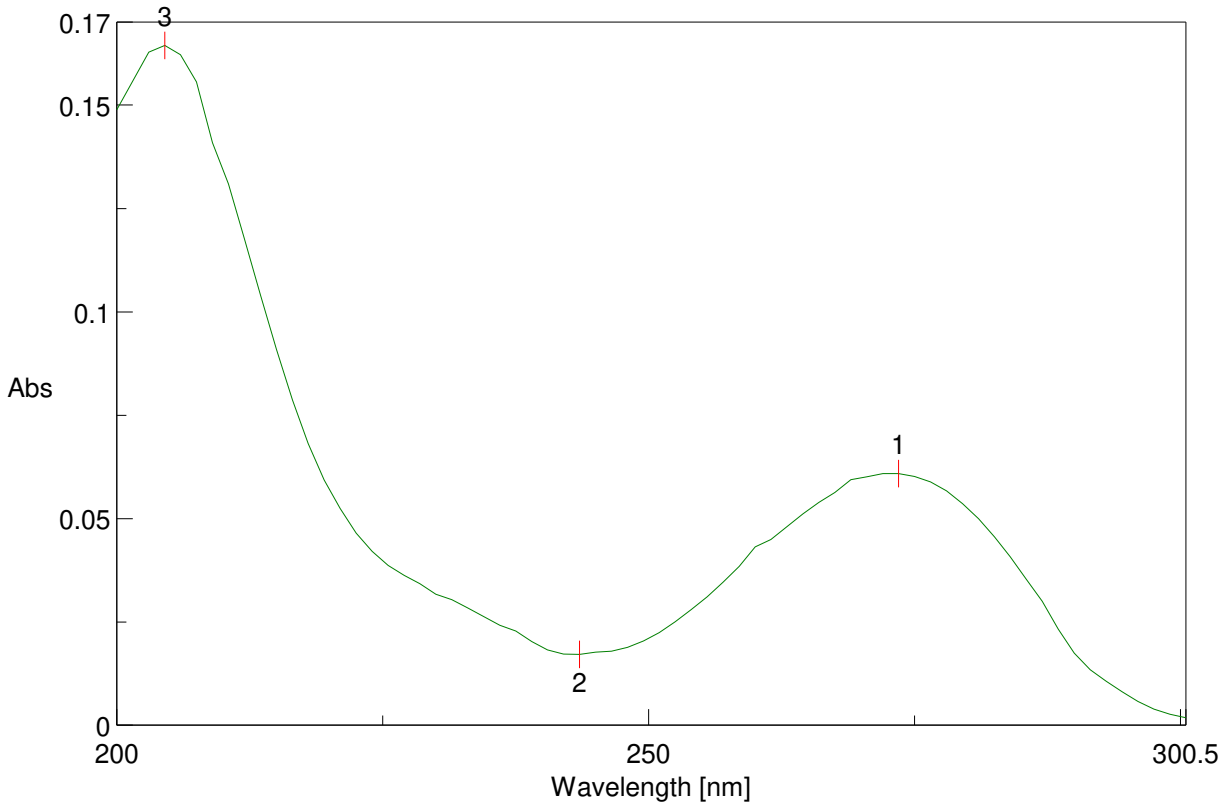

[Comments]

User	Administrator
Division	---
Company	Valer Laboratorios
Creation date	4/30/2018 1:54 PM

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300.5 nm
Data interval	1.5 nm
Data points	68


[Measurement Information]

Instrument Name	MD-2015
Model Name	MD-2015
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273.5	0.060784	2	243.5	0.017075
3	204.5	0.164333			

Chromatogram

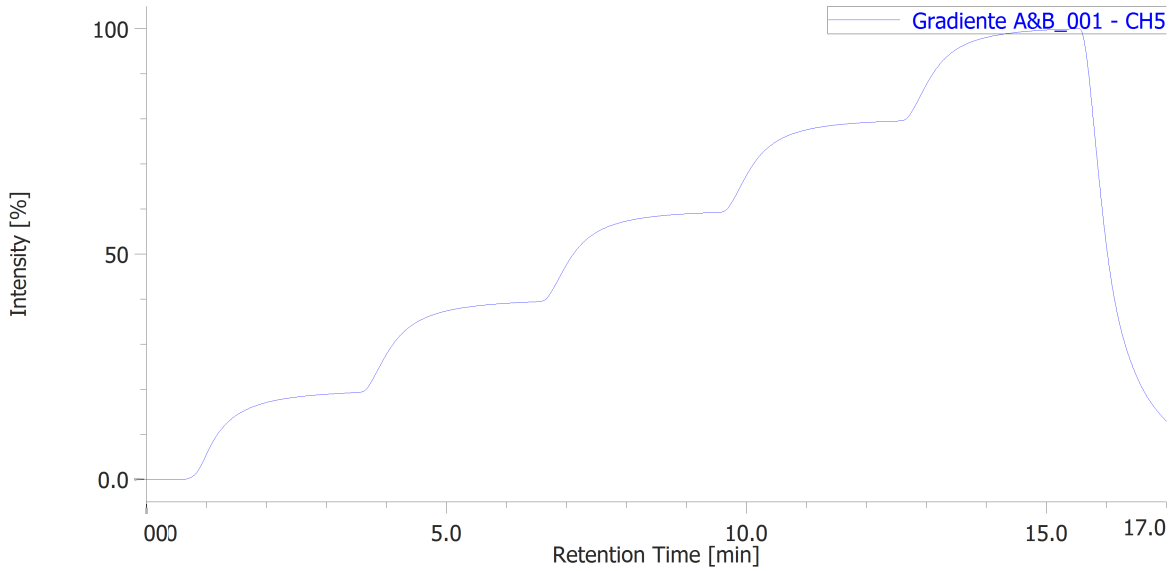


Chromatogram Information	
User Name	Administrator
Date Modified	5/1/2018 1:17:09 PM
Description	
HPLC System Name	HPL 02
Injection Date	5/1/2018 1:00:09 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	17.0 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente A&B_001-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	800 [msec]
Peak Method	

Creator Administrator

Chromatogram

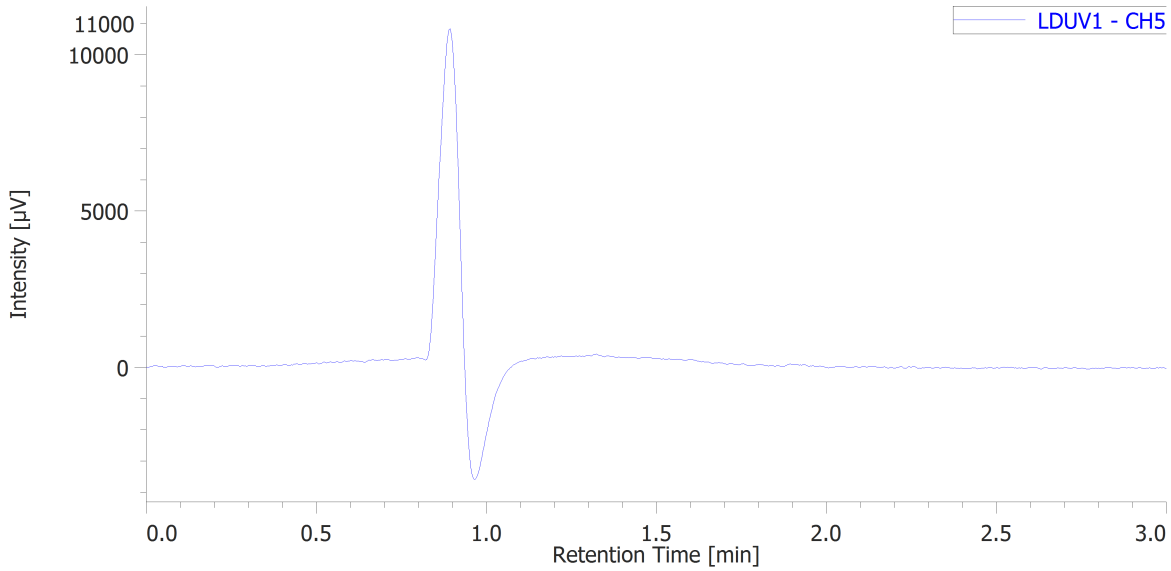


Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 5:52:39 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 5:30:53 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

Creator Administrator

Chromatogram

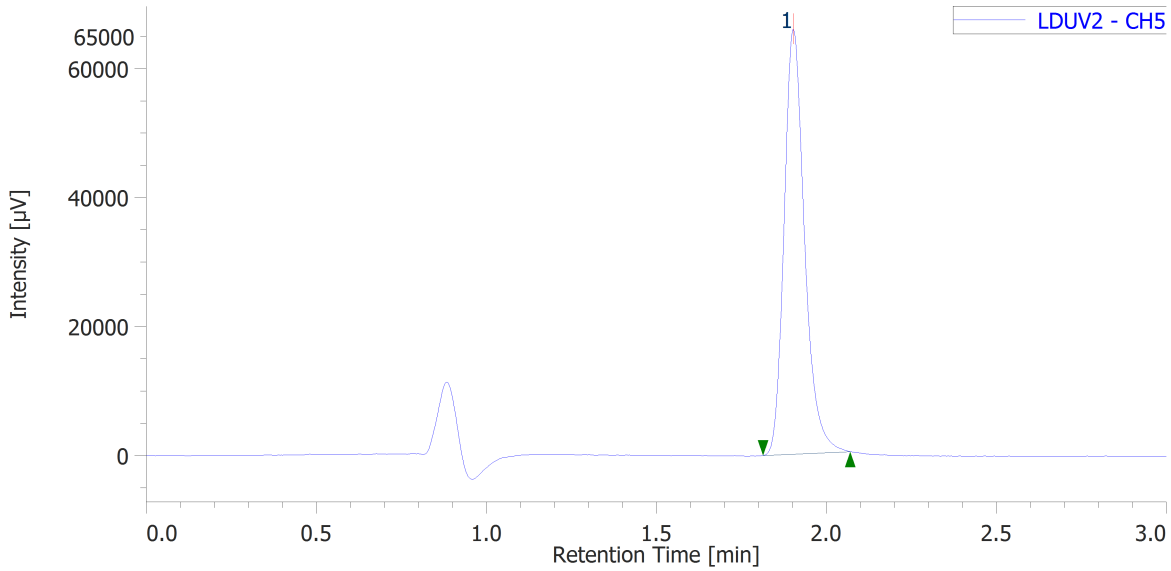

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 5:52:40 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 5:34:55 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.903	275505	65927	100.000	100.000	N/A	5149	N/A	1.245	

Creator Administrator

Chromatogram

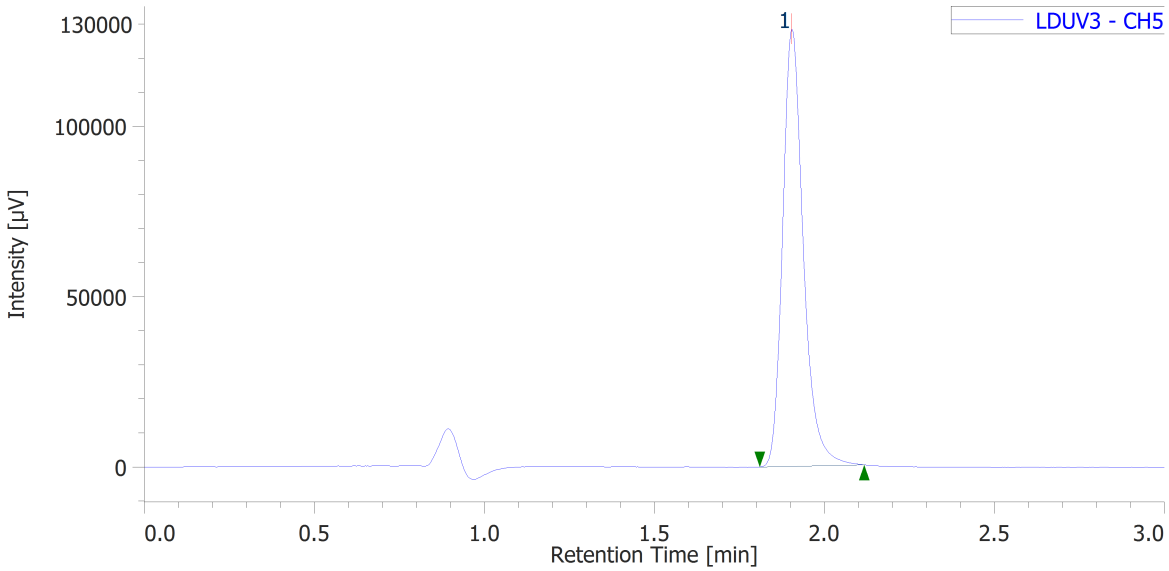

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 5:52:41 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 5:38:49 PM
Volume	10.00 [µL]
Sample #	3
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.903	542154	128370	100.000	100.000	N/A	5125	N/A	1.293	

Creator Administrator

Chromatogram

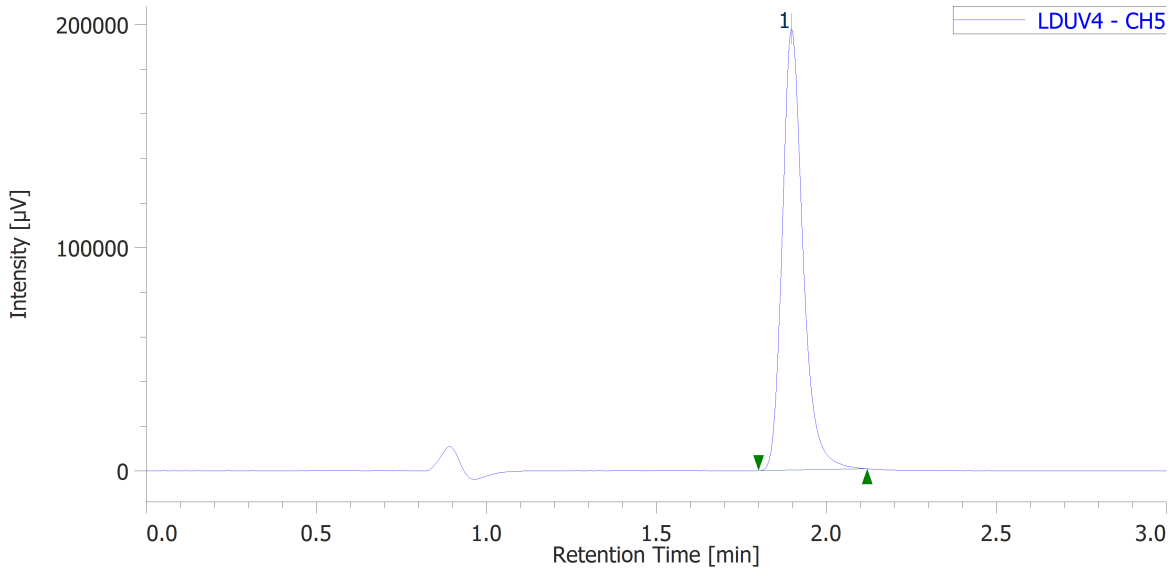

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 5:52:42 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 5:42:42 PM
Volume	10.00 [µL]
Sample #	4
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.897	834924	197764	100.000	100.000	N/A	5113	N/A	1.284	

Creator Administrator

Chromatogram

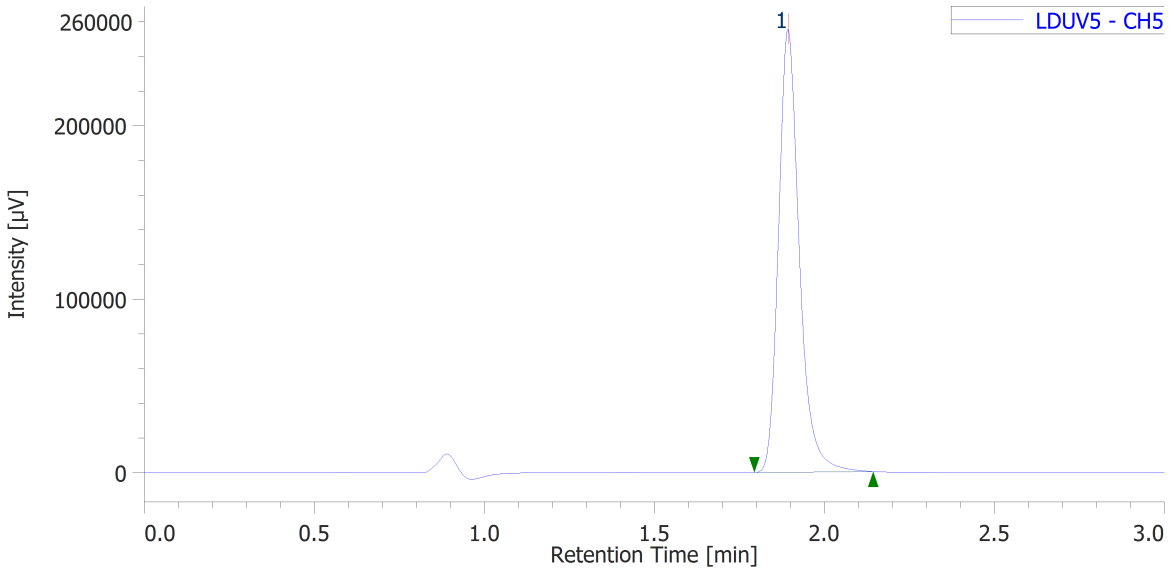

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 5:52:43 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 5:46:36 PM
Volume	10.00 [µL]
Sample #	5
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.893	1086923	255547	100.000	100.000	N/A	5049	N/A	1.245	

Creator Administrator

Chromatogram

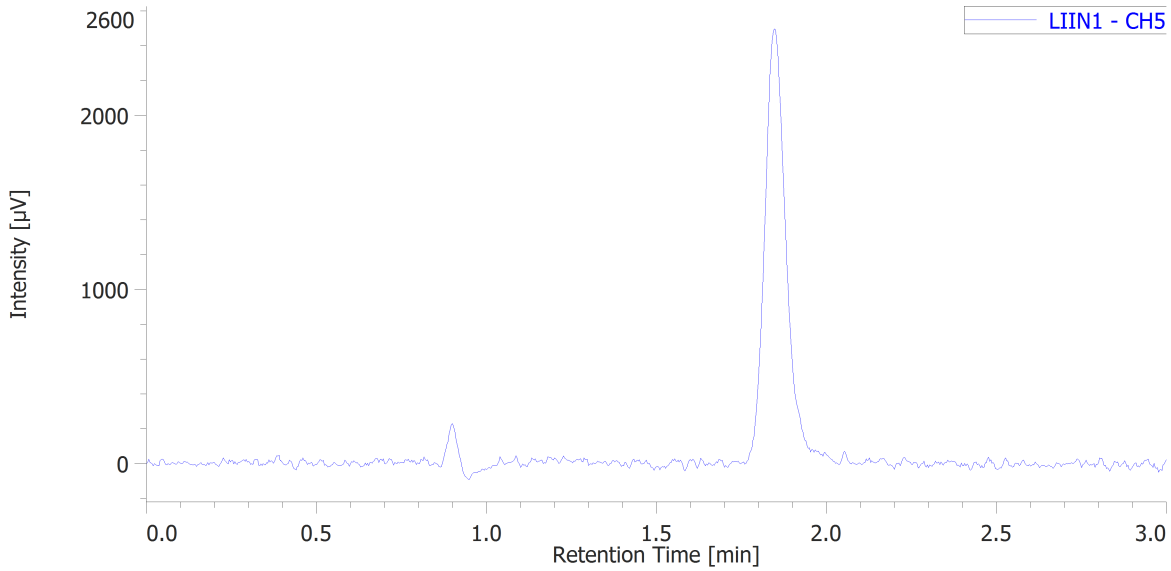


Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 6:38:41 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 6:17:50 PM
Volume	0.10 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

Creator Administrator

Chromatogram

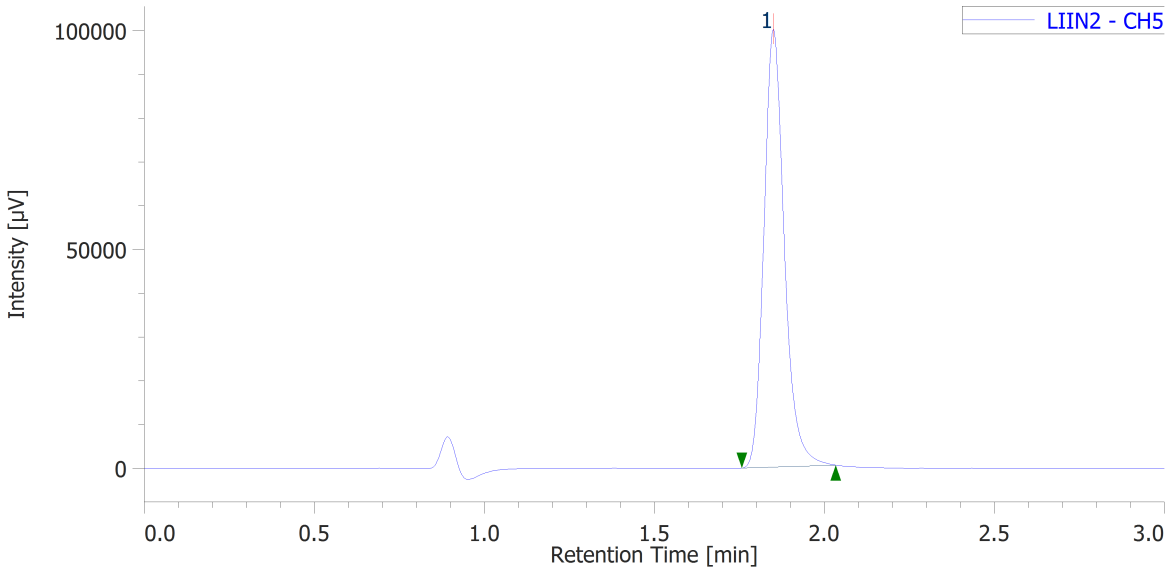

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 6:38:44 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 6:21:48 PM
Volume	5.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.850	416424	100077	100.000	100.000	N/A	4920	N/A	1.211	

Creator Administrator

Chromatogram

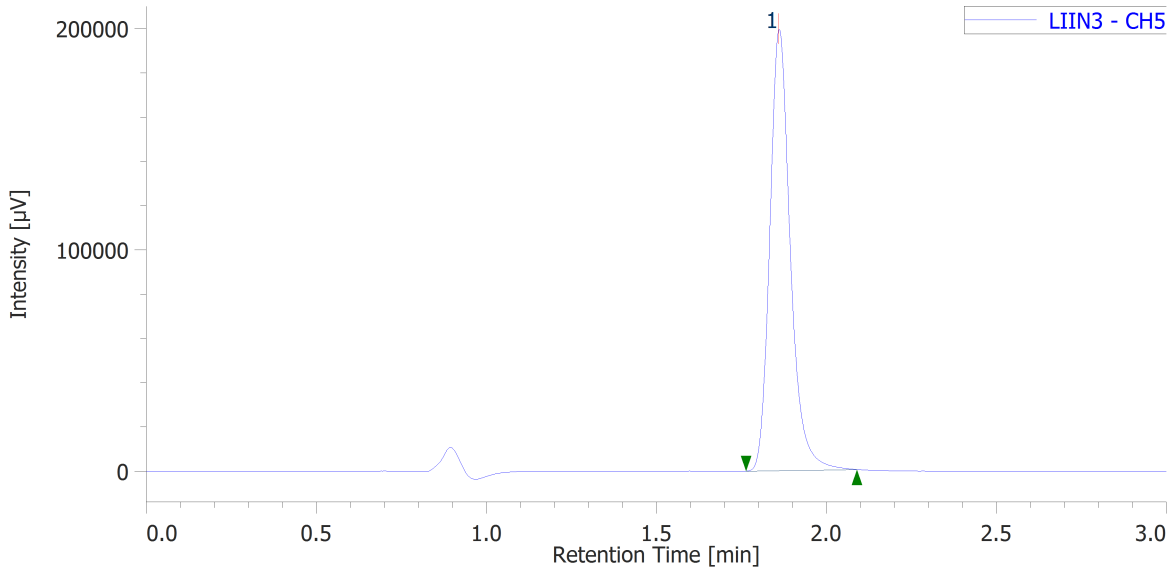

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 6:38:44 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 6:25:46 PM
Volume	10.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.860	836651	199580	100.000	100.000	N/A	4985	N/A	1.262	

Creator Administrator

Chromatogram

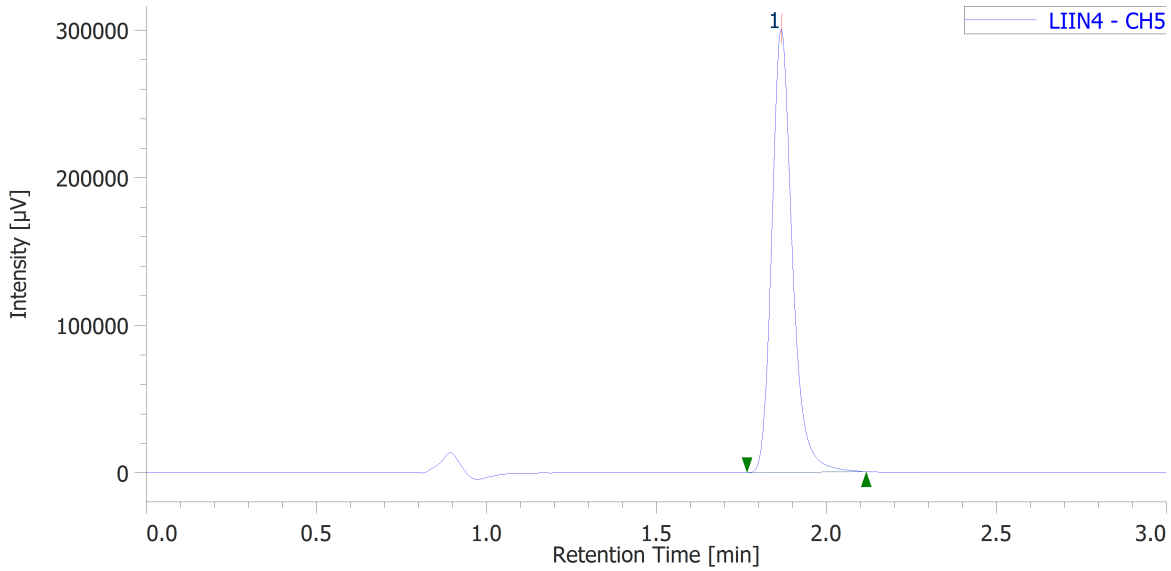

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 6:38:45 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 6:29:46 PM
Volume	15.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.867	1258054	300522	100.000	100.000	N/A	5055	N/A	1.248	

Creator Administrator

Chromatogram

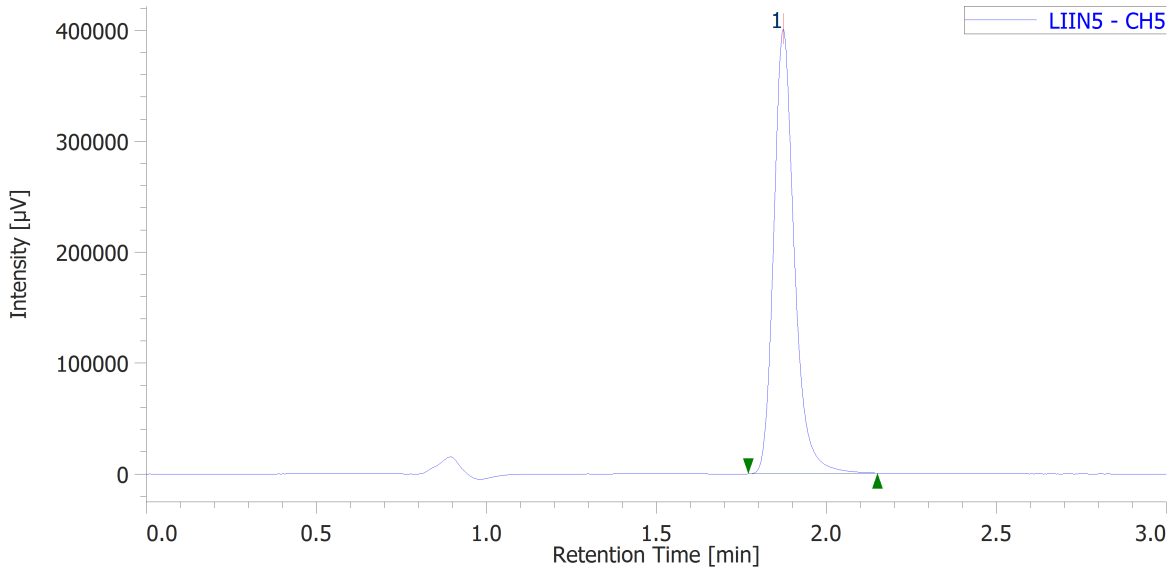

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 6:38:46 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 6:33:44 PM
Volume	20.00 [µL]
Sample #	1
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.873	1684064	401095	100.000	100.000	N/A	5087	N/A	1.230	

Creator Administrator

Chromatogram

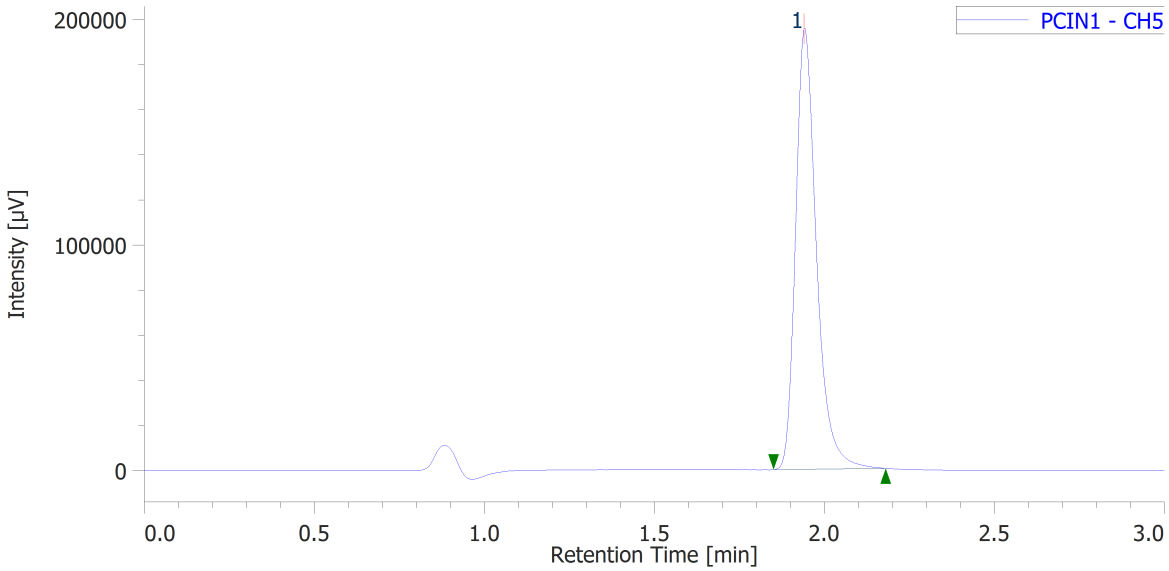

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:02 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 3:44:03 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN1-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.940	833094	195227	100.000	100.000	N/A	5256	N/A	1.379	

Creator Administrator

Chromatogram

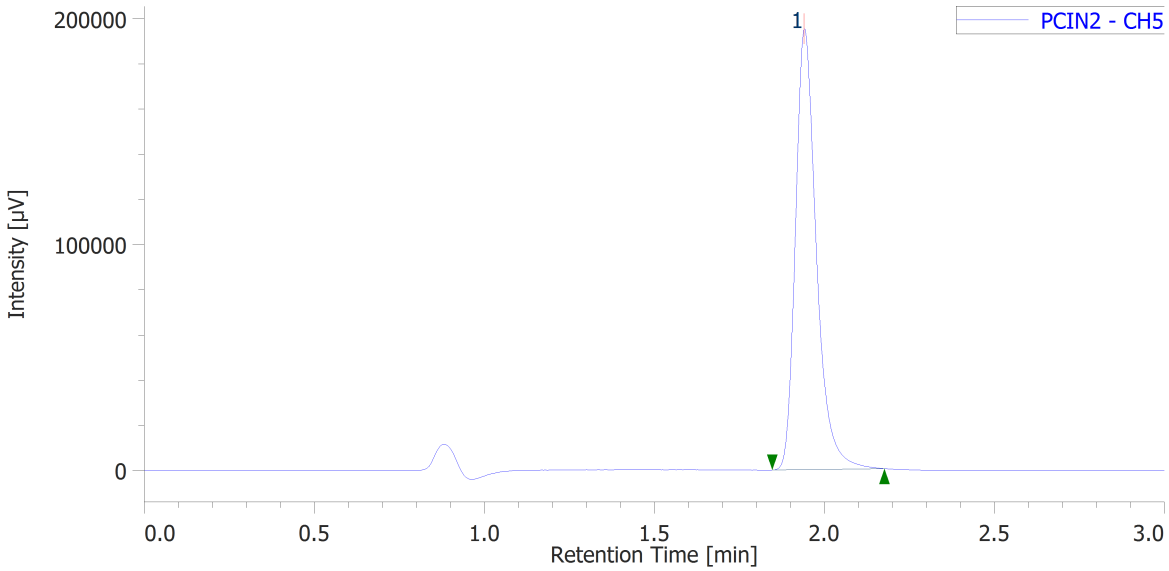

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:03 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 3:48:10 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN2-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.940	834402	195002	100.000	100.000	N/A	5219	N/A	1.369	

Creator Administrator

Chromatogram

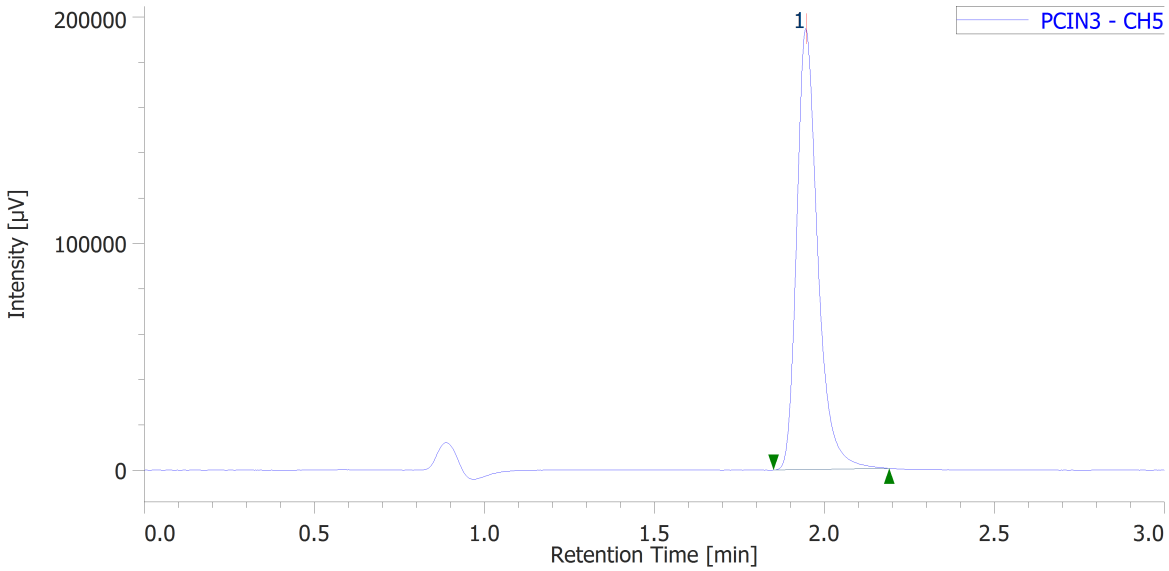

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:04 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 3:52:09 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN3-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.947	834587	194438	100.000	100.000	N/A	5244	N/A	1.301	

Creator Administrator

Chromatogram

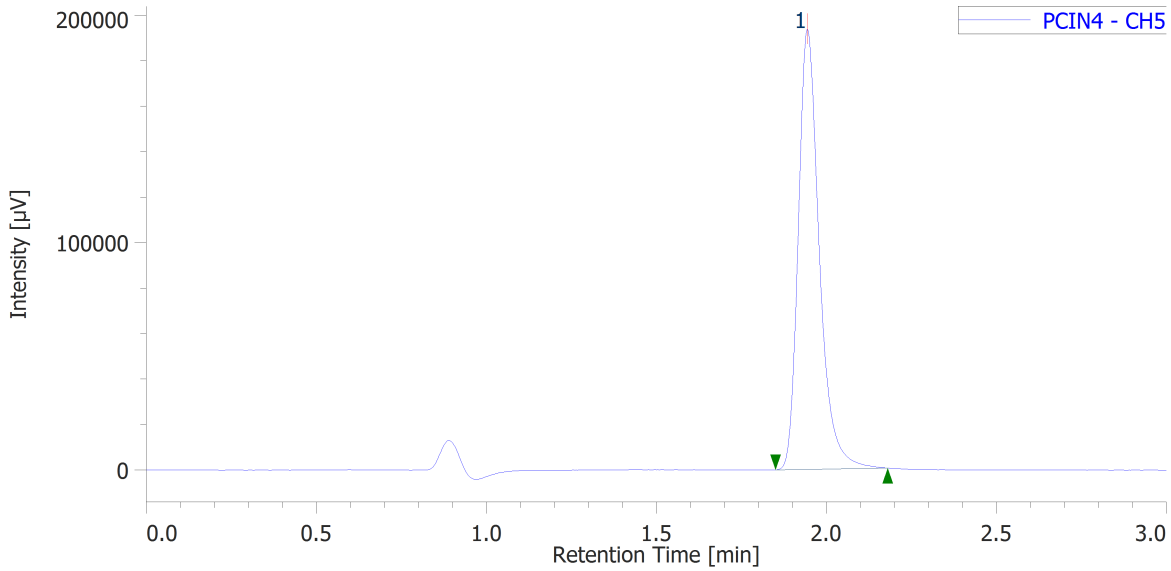

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:06 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 4:00:04 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN4-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.943	831149	193753	100.000	100.000	N/A	5211	N/A	1.345	

Creator Administrator

Chromatogram

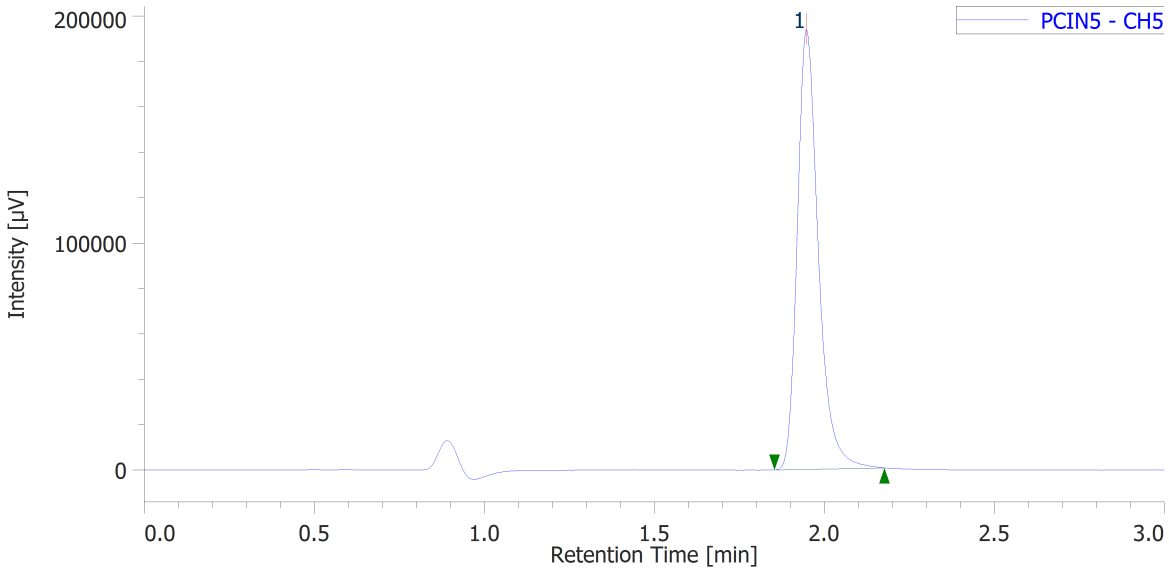

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:07 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 4:04:00 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN5-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.947	833304	194015	100.000	100.000	N/A	5198	N/A	1.330	

Creator Administrator

Chromatogram

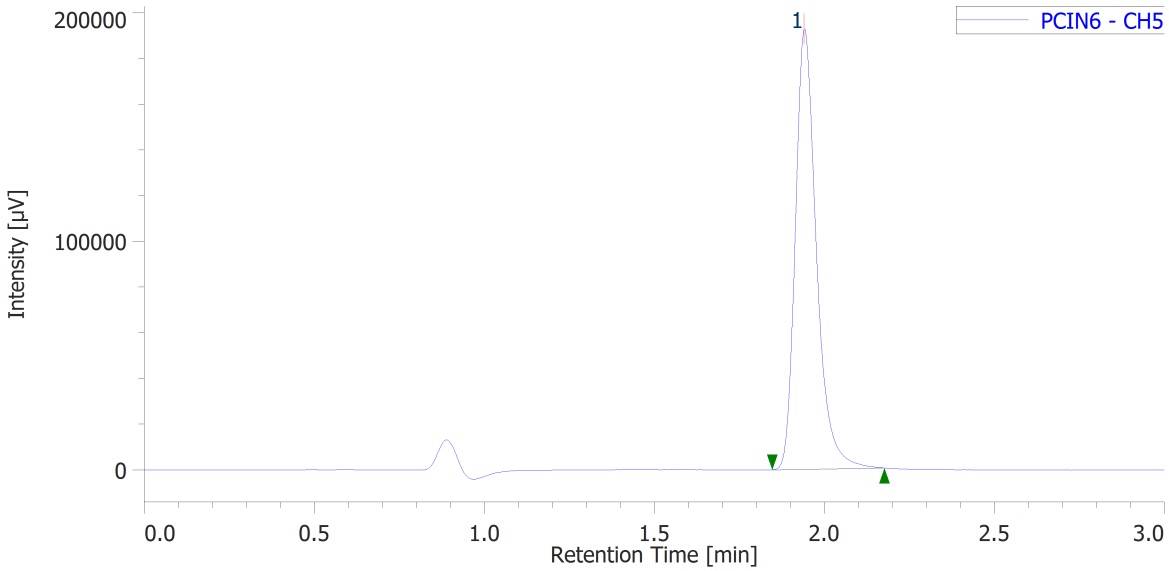

Chromatogram Information	
User Name	Administrator
Date Modified	4/30/2018 4:31:07 PM
Description	
HPLC System Name	HPL 02
Injection Date	4/30/2018 4:07:58 PM
Volume	10.00 [µL]
Sample #	2
Project Name	Teste Jasco
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN6-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	200 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1.940	830781	192696	100.000	100.000	N/A	5144	N/A	1.356	

Creator Administrator