
Peak Find - EDUV_001 PDA_tR1,75 D.jws

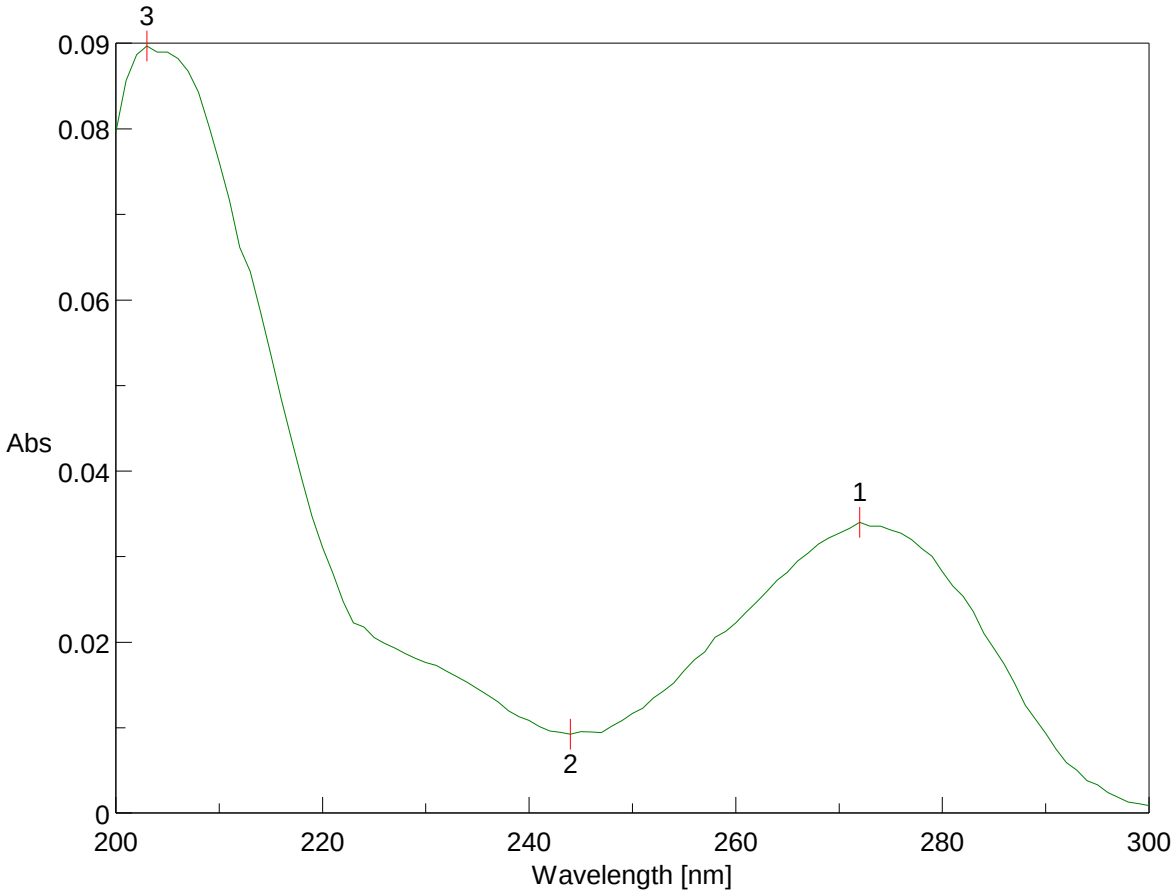

[Comments]

User	Administrator
Division	---
Company	SAUVET
Creation date	20/07/2021 15:45

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.03397	2	244	0.009192
3	203	0.089677			

Chromatogram

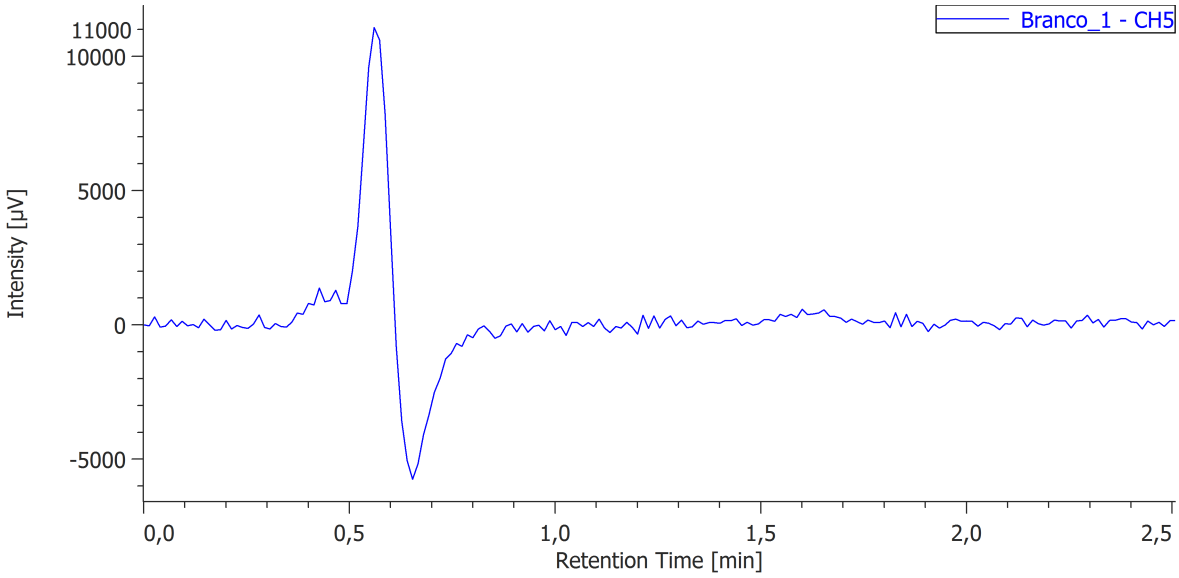


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 16:42:36
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

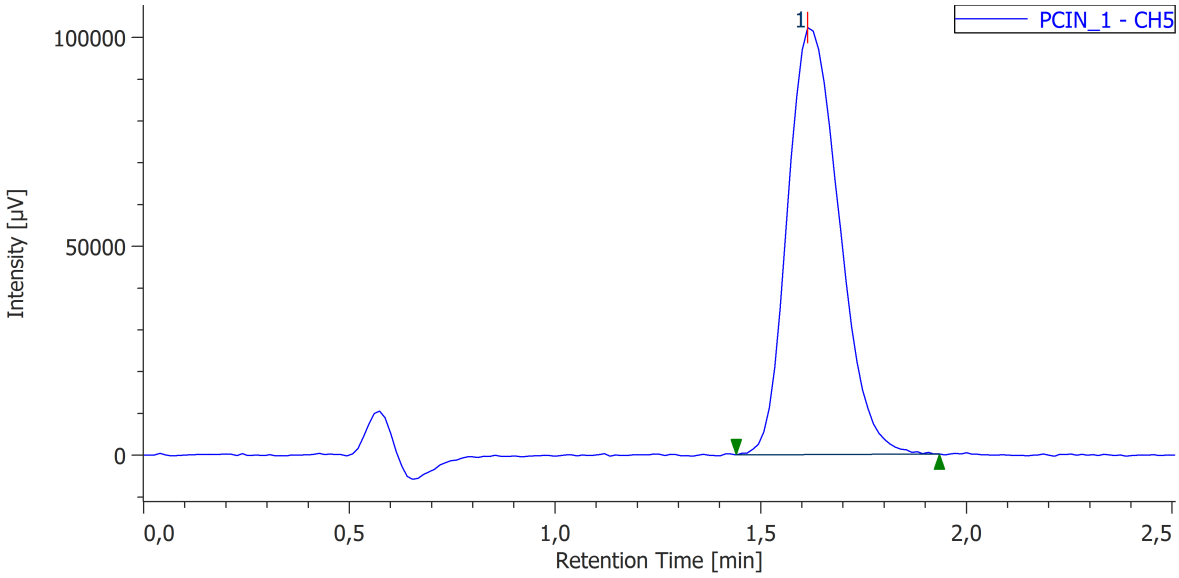


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 16:46:26
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	891797	102123	100,000	100,000	N/A	766	N/A	1,300	

Chromatogram

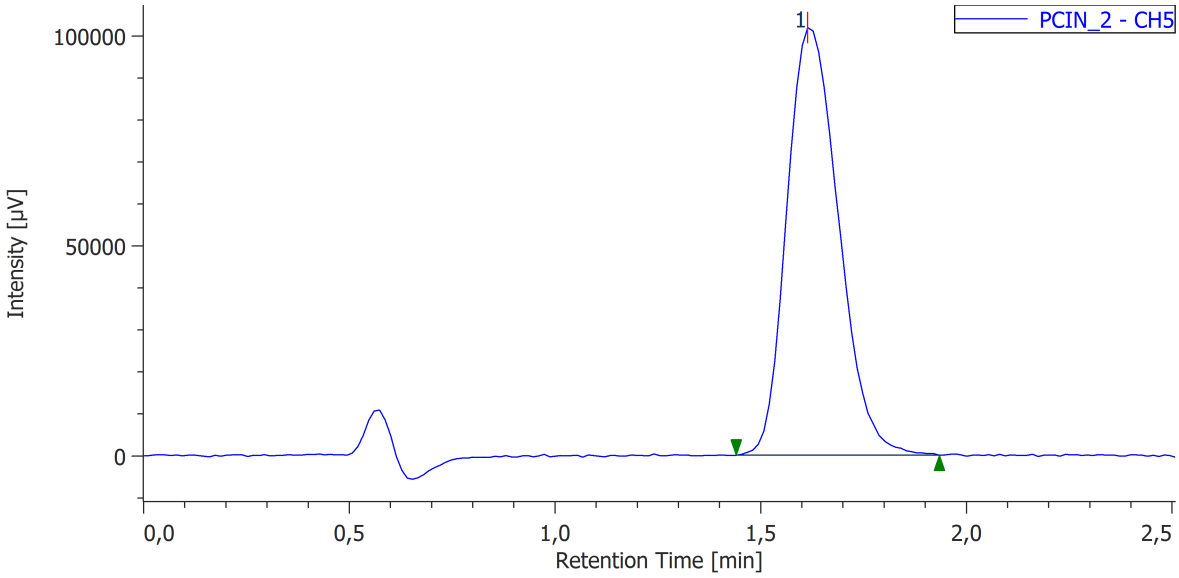


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 16:50:16
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	890888	101734	100,000	100,000	N/A	762	N/A	1,285	

Chromatogram

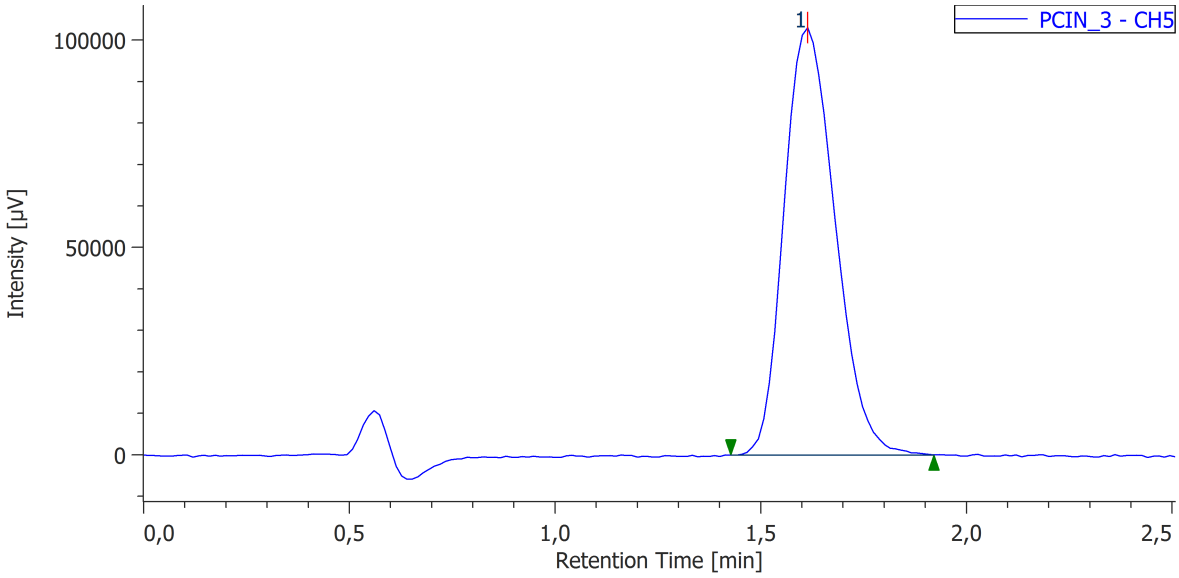


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 16:54:06
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	891210	103008	100,000	100,000	N/A	781	N/A	1,198	

Chromatogram

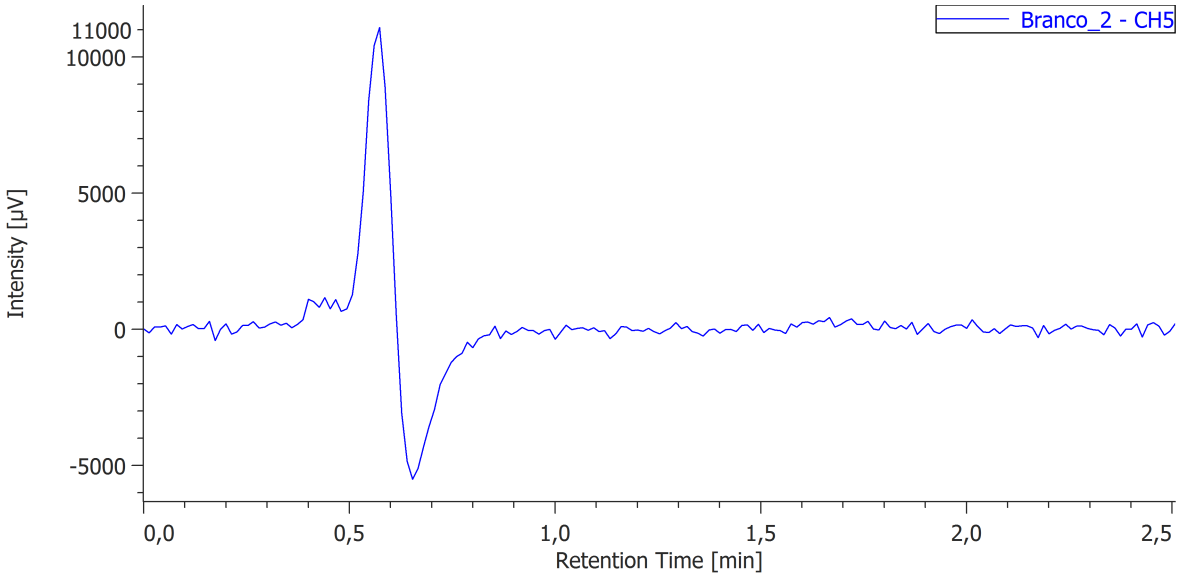


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 16:57:56
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

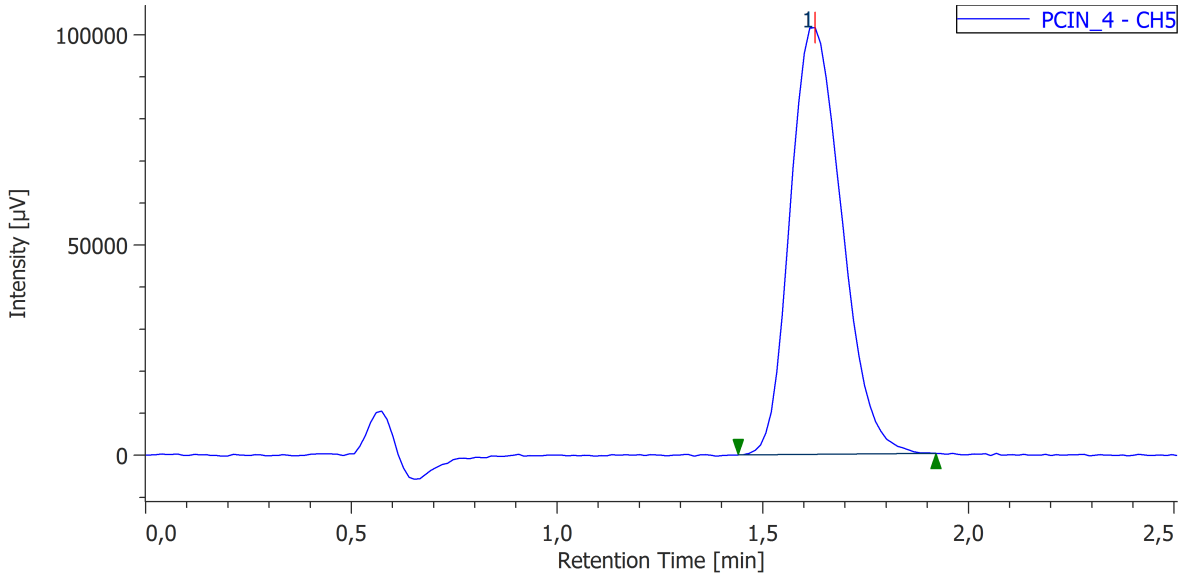


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:01:49
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,627	887016	101393	100,000	100,000	N/A	779	N/A	1,173	

Chromatogram

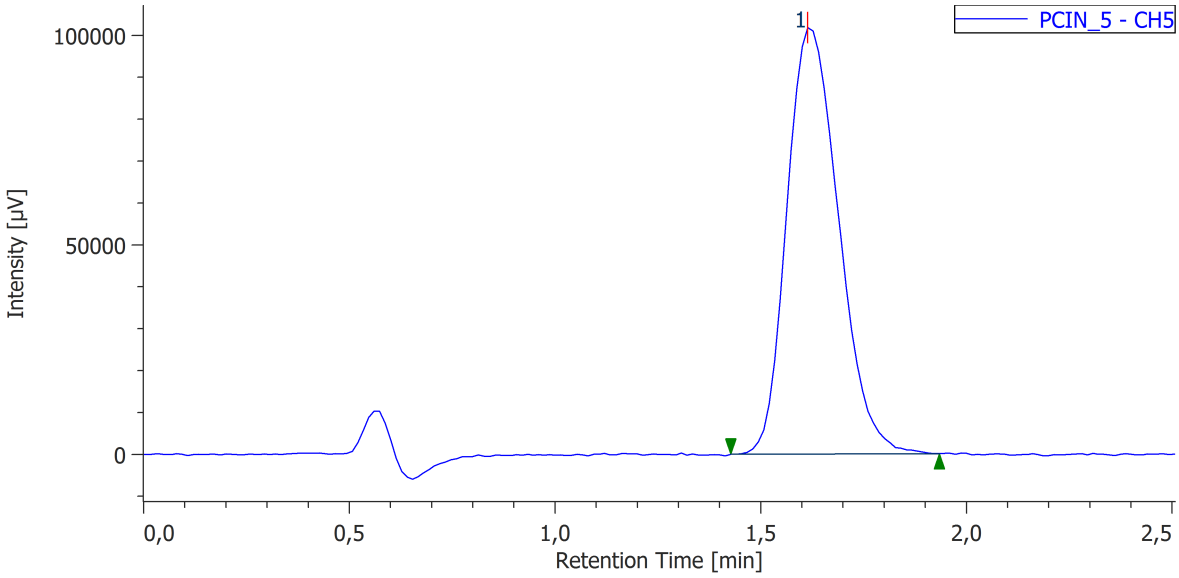


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:05:41
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	889942	101671	100,000	100,000	N/A	763	N/A	1,290	

Chromatogram

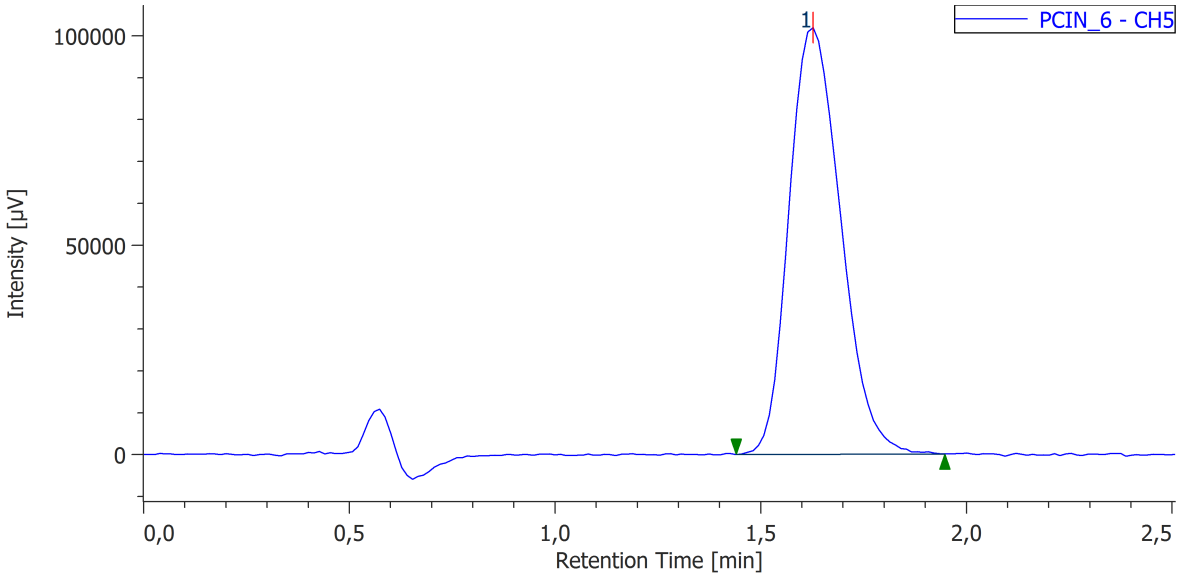


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:43
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:09:31
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN_6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,627	890760	101784	100,000	100,000	N/A	782	N/A	1,197	

Chromatogram

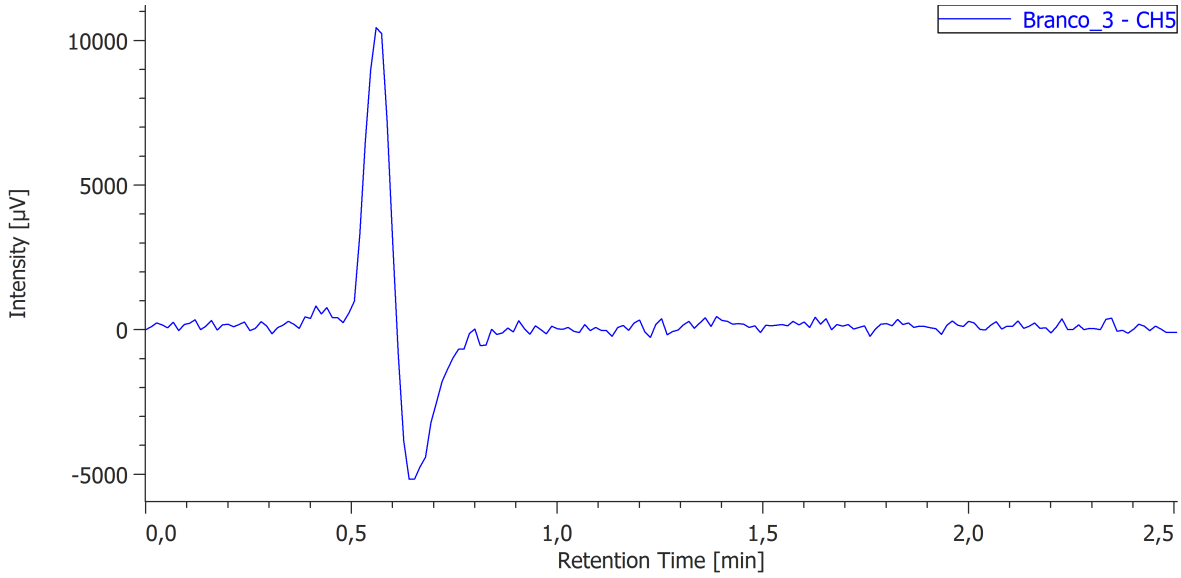


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:13:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

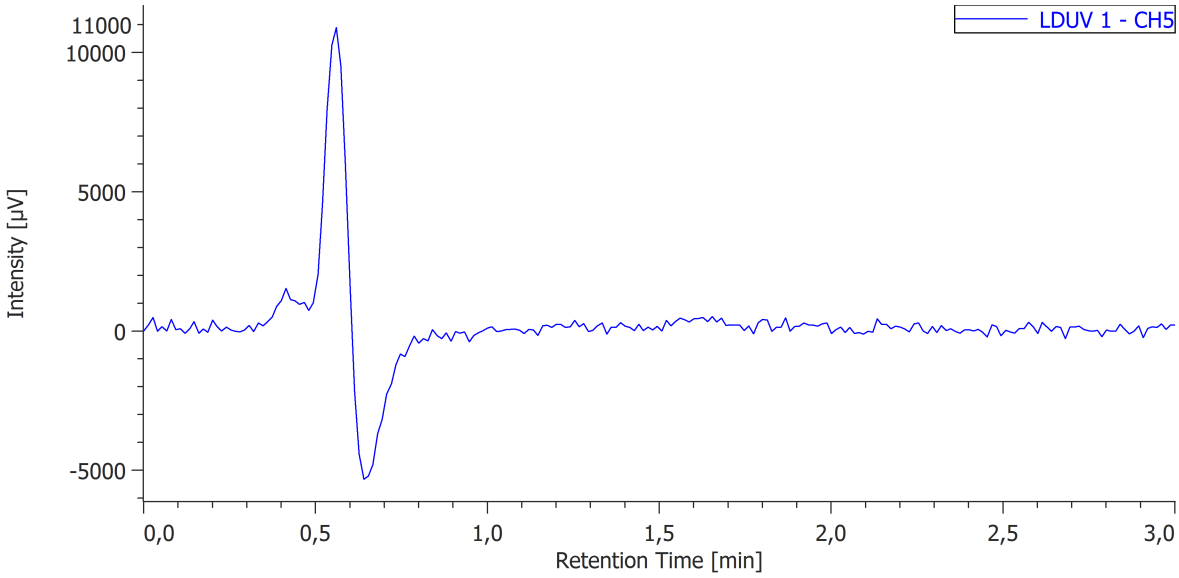


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:17:11
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

Chromatogram

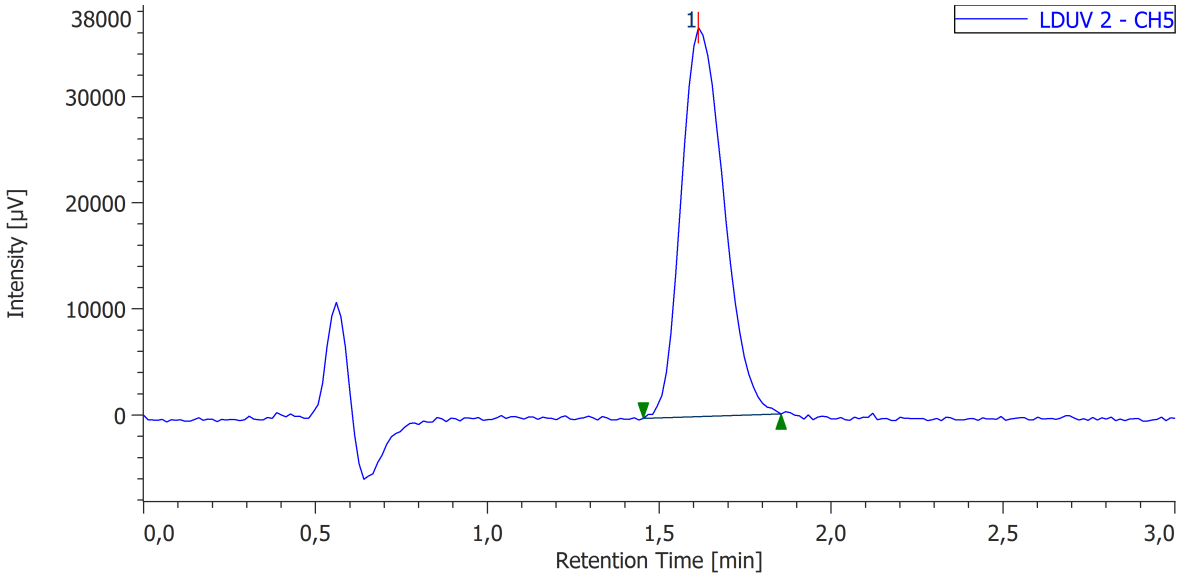


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:19:57
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:21:31
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	316621	36596	100,000	100,000	N/A	777	N/A	1,274	

Chromatogram

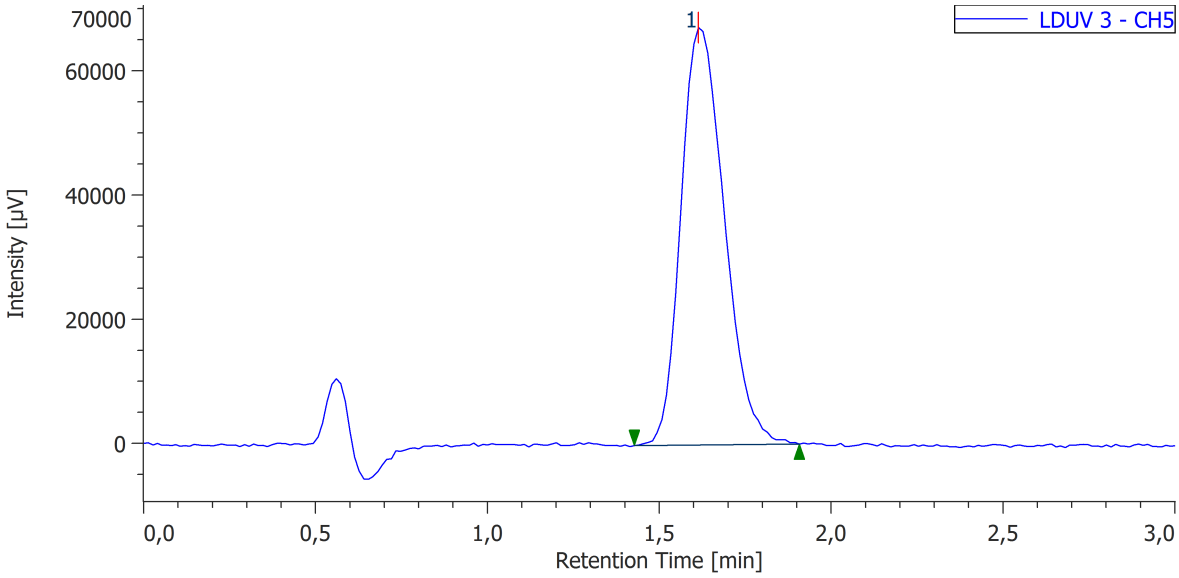


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:25:54
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	590060	67147	100,000	100,000	N/A	769	N/A	1,299	

Chromatogram

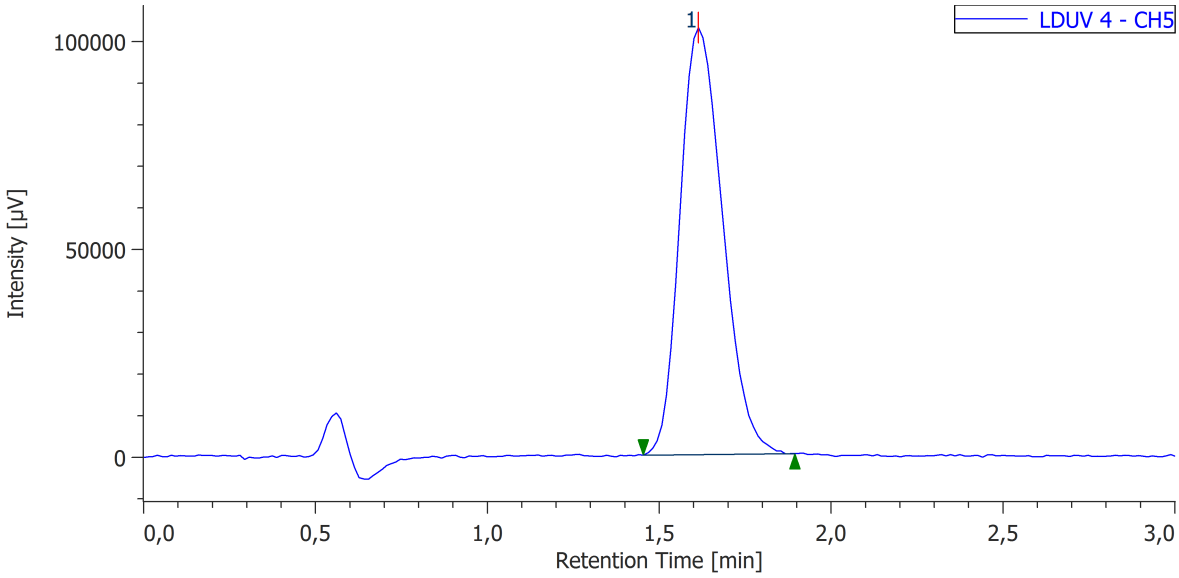


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:30:18
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	887108	102642	100,000	100,000	N/A	782	N/A	1,240	

Chromatogram

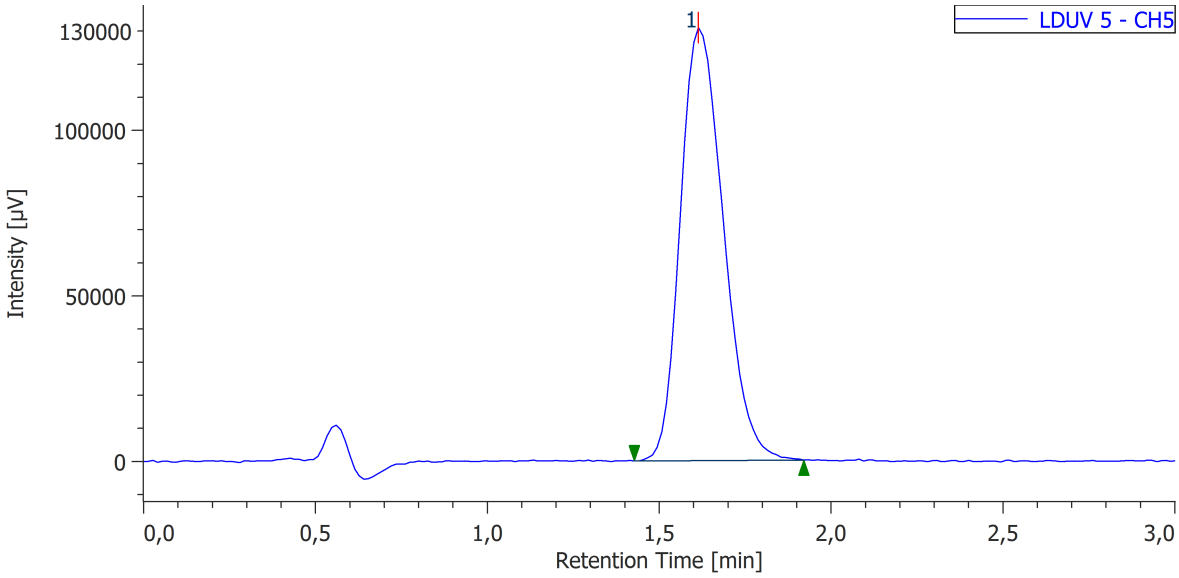


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:34:43
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	1137799	130703	100,000	100,000	N/A	778	N/A	1,257	

Chromatogram

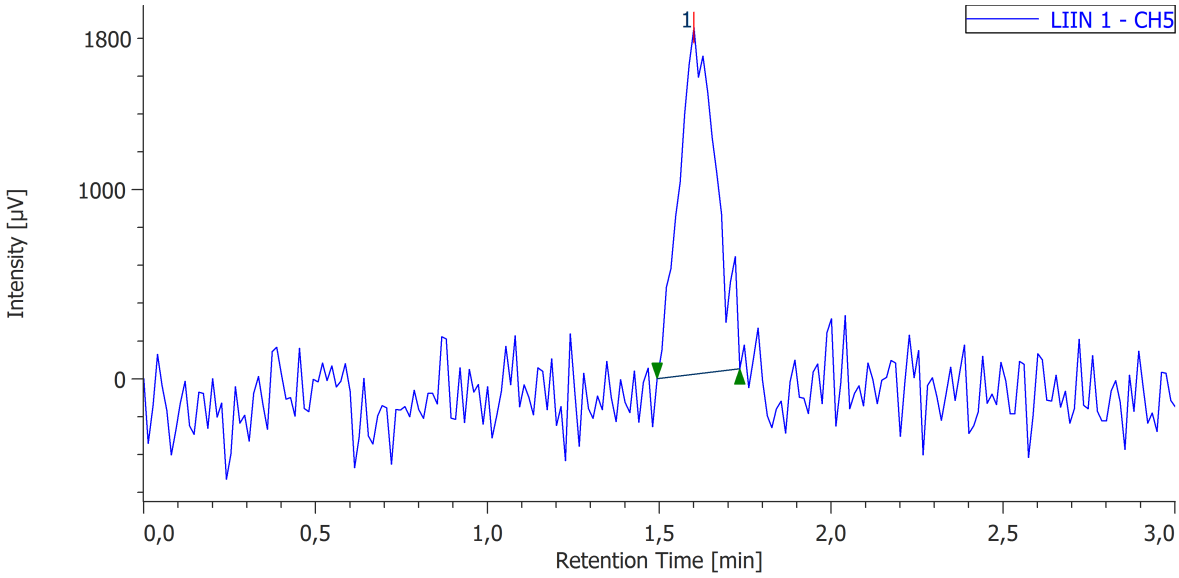


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:38:54
Volume	0,1 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,600	13663	1831	100,000	100,000	N/A	937	N/A	1,167	

Chromatogram

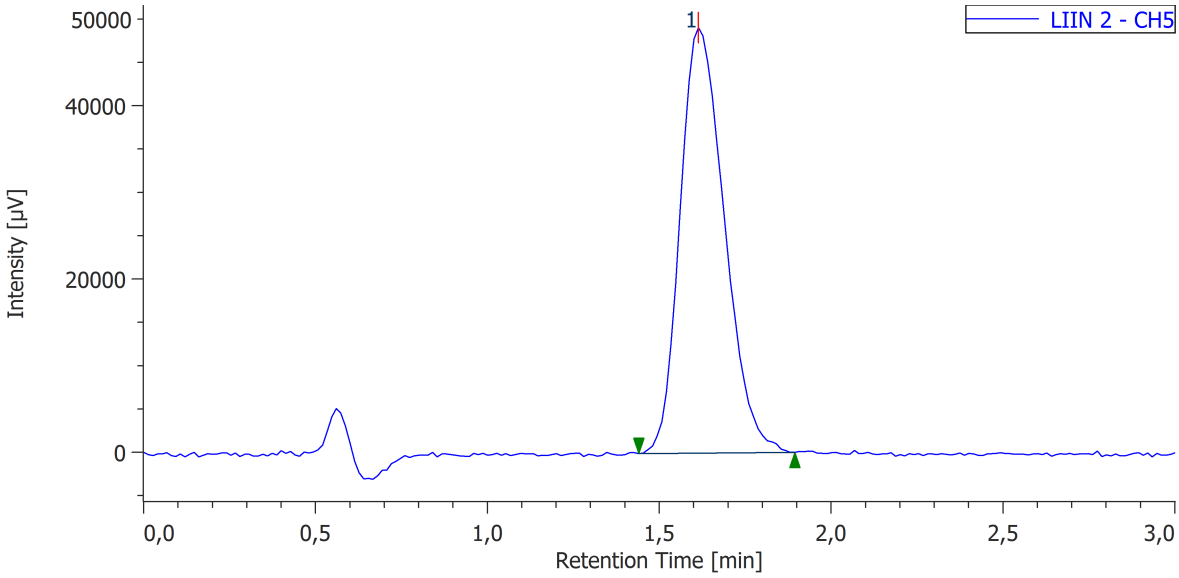


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:43:09
Volume	5,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,613	439780	49068	100,000	100,000	N/A	731	N/A	1,267	

Chromatogram

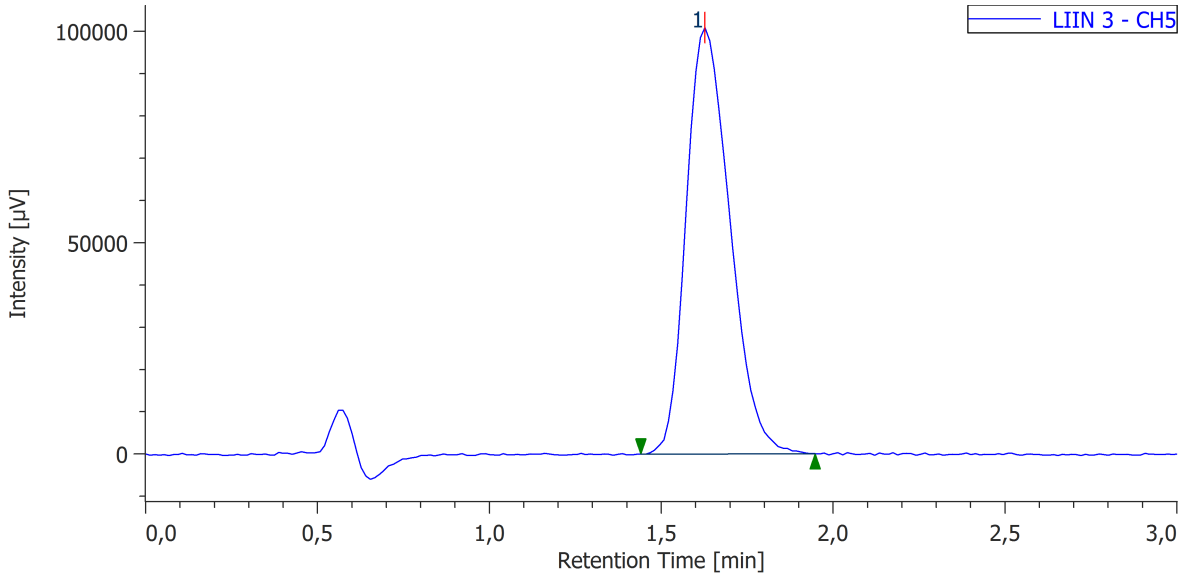


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:47:29
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,627	891650	100801	100,000	100,000	N/A	761	N/A	1,256	

Chromatogram

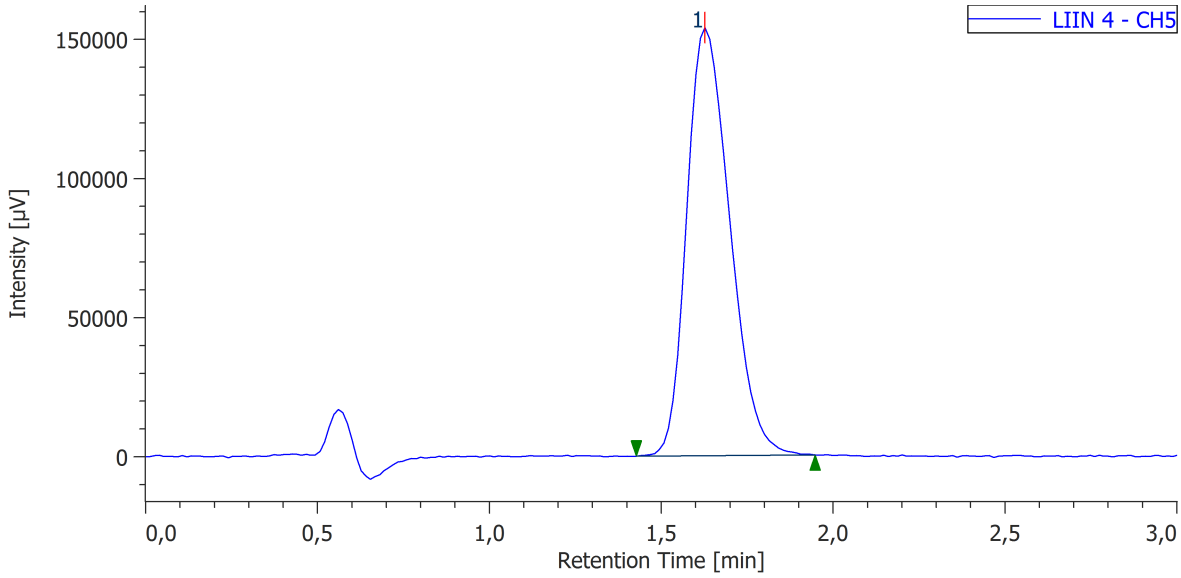


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:44
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:51:56
Volume	15,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,627	1338524	153718	100,000	100,000	N/A	790	N/A	1,269	

Chromatogram

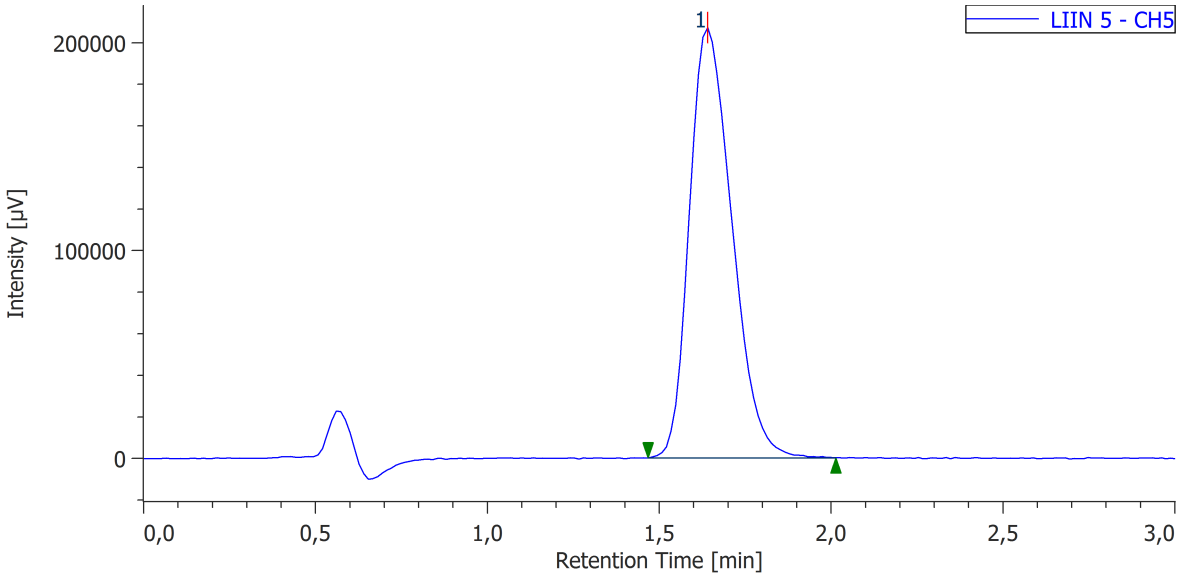


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 09:17:42
Description	
HPLC System Name	CQ 023
Injection Date	20/07/2021 17:56:30
Volume	20,0 [µL]
Sample #	11
Project Name	Qualificação 2020
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,640	1781493	206876	100,000	100,000	N/A	822	N/A	1,274	

Chromatogram

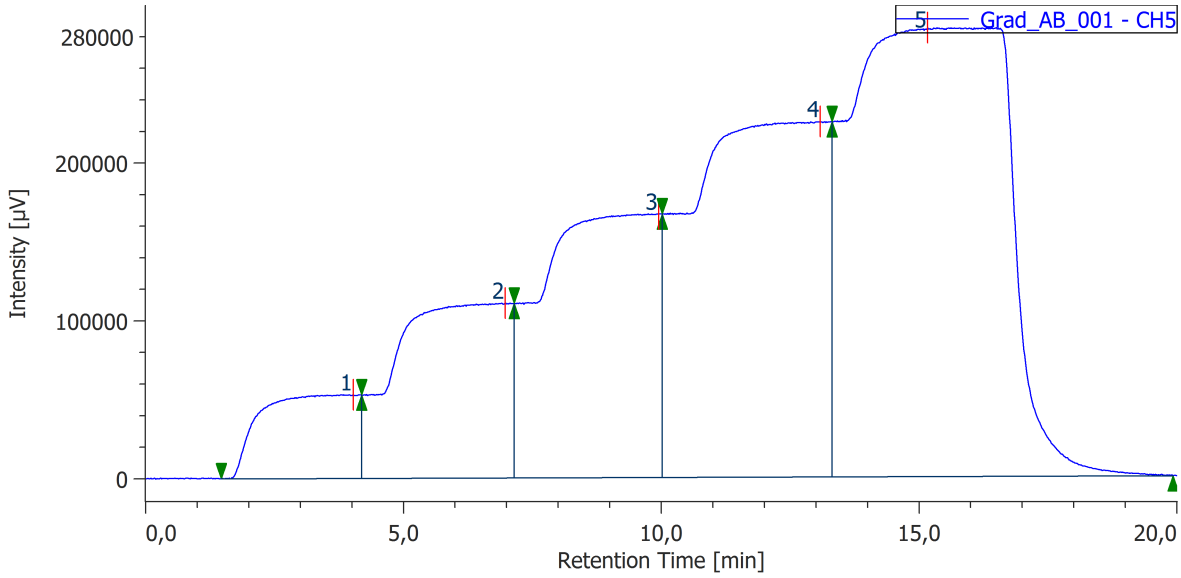


Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 11:35:09
Description	
HPLC System Name	CQ 023
Injection Date	21/07/2021 11:15:08
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação 2020
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad_AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	4,027	6769912	53105	4,487	6,322	N/A	N/A	N/A	N/A	
2	40 %	5	6,973	16833014	110685	11,158	13,178	N/A	N/A	N/A	N/A	
3	60 %	5	9,947	25846436	166864	17,132	19,866	N/A	N/A	N/A	N/A	
4	80 %	5	13,080	40982069	225147	27,165	26,805	N/A	N/A	N/A	N/A	
5	100 %	5	15,160	60432386	284143	40,058	33,829	N/A	N/A	N/A	N/A	

Chromatogram

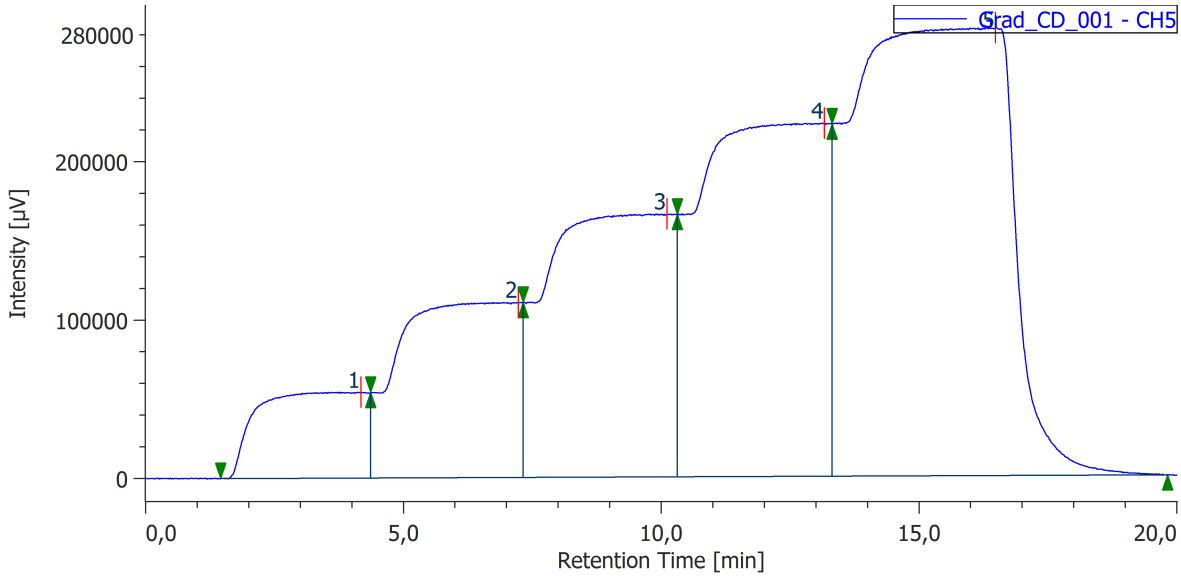

Chromatogram Information	
User Name	Administrator
Date Modified	21/07/2021 12:09:41
Description	
HPLC System Name	CQ 023
Injection Date	21/07/2021 11:47:27
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação 2020
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad_CD_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	4,173	7702536	54179	5,124	6,482	N/A	N/A	N/A	N/A	
2	40 %	5	7,227	17470228	110522	11,623	13,223	N/A	N/A	N/A	N/A	
3	60 %	5	10,107	27481630	165986	18,284	19,859	N/A	N/A	N/A	N/A	
4	80 %	5	13,160	37719370	222705	25,095	26,645	N/A	N/A	N/A	N/A	
5	100 %	5	16,480	59934453	282421	39,874	33,790	N/A	N/A	N/A	N/A	