
Peak Find - EDUV_003 UV_tR1,68 D.jws

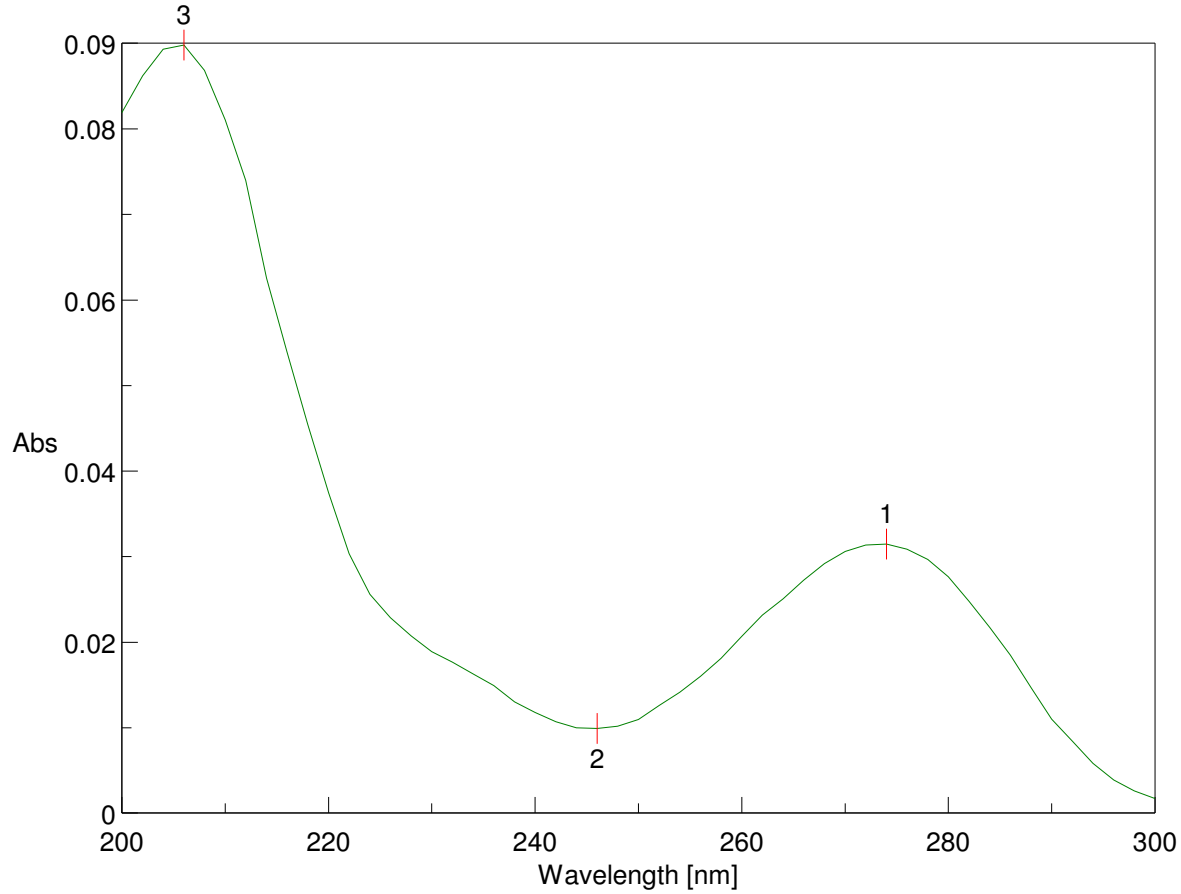

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	17/08/2021 13:27

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.031416	2	246	0.00986099
3	206	0.0897735			

Chromatogram

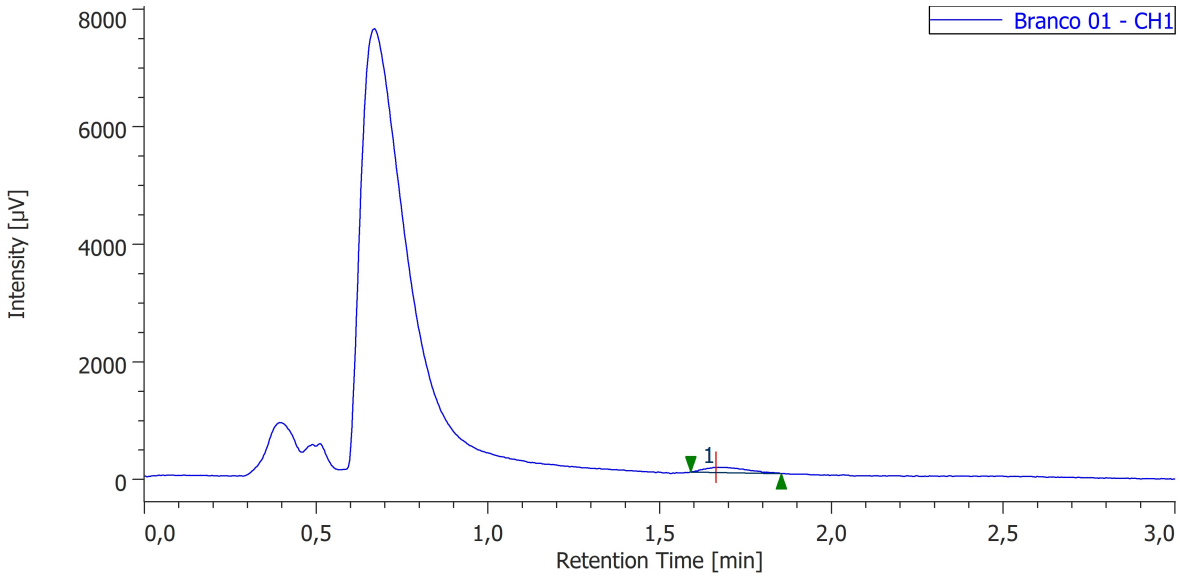


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:22:23
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:12:05
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	Branco 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	793	91	100,000	100,000	N/A	762	N/A	1,812	

Chromatogram

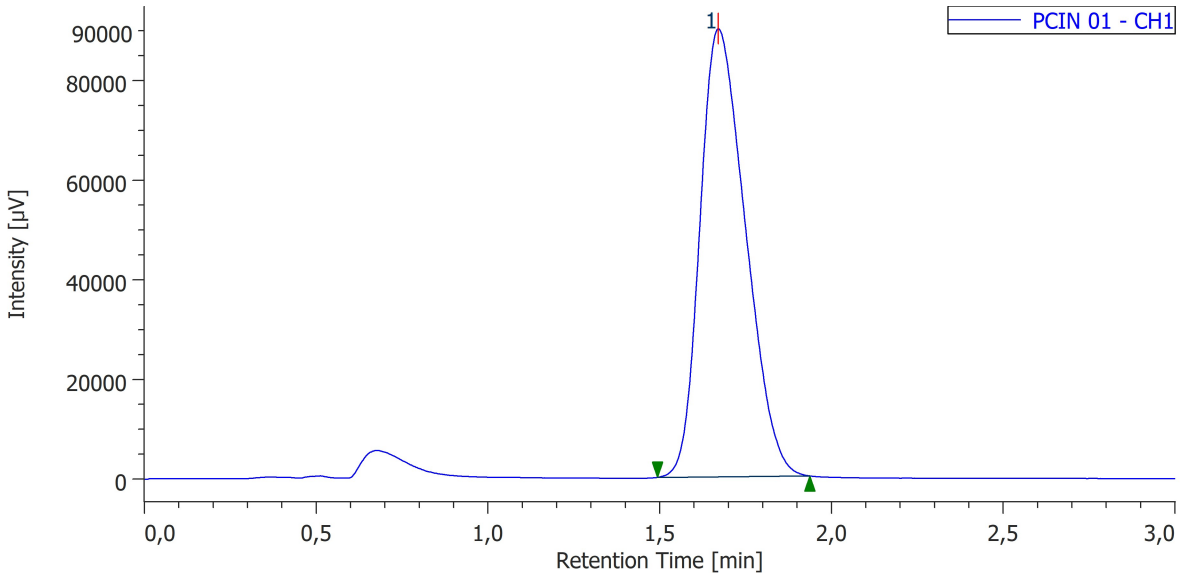


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:14
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:17:09
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	PCIN 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	828098	89919	100,000	100,000	N/A	728	N/A	1,309	

Chromatogram

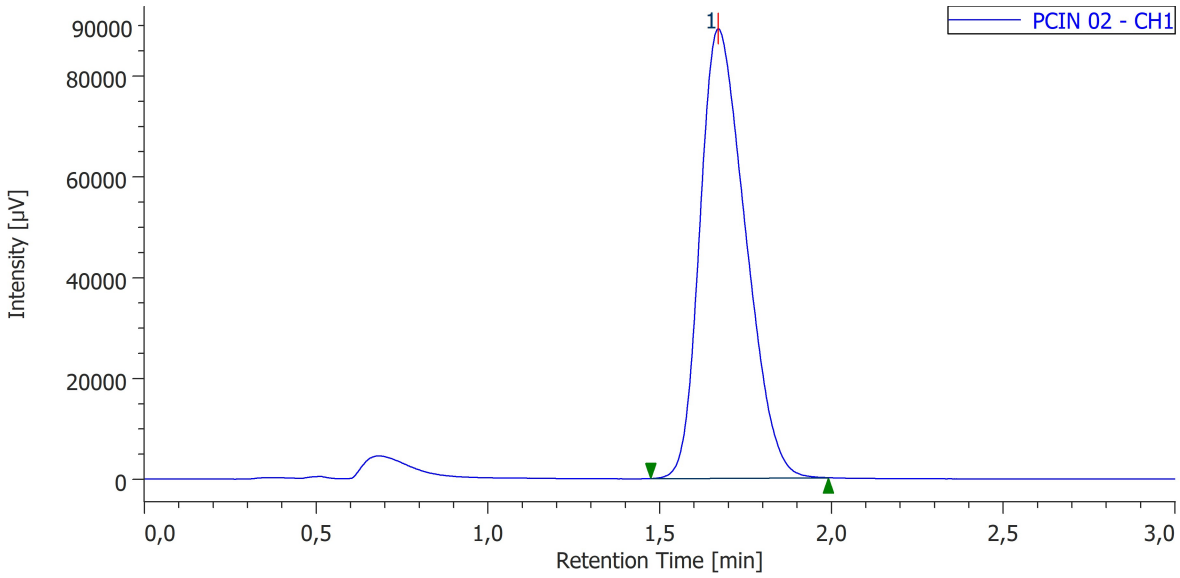


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:14
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:22:14
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	PCIN 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	820959	89167	100,000	100,000	N/A	735	N/A	1,317	

Chromatogram

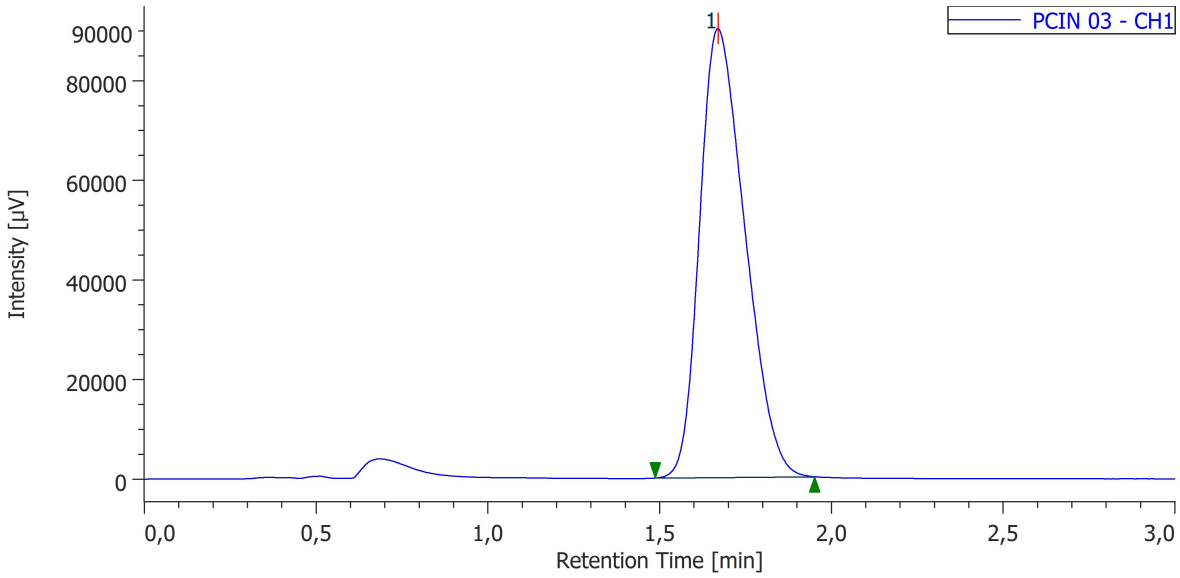


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:14
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:27:18
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	PCIN 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	825262	90096	100,000	100,000	N/A	741	N/A	1,309	

Chromatogram

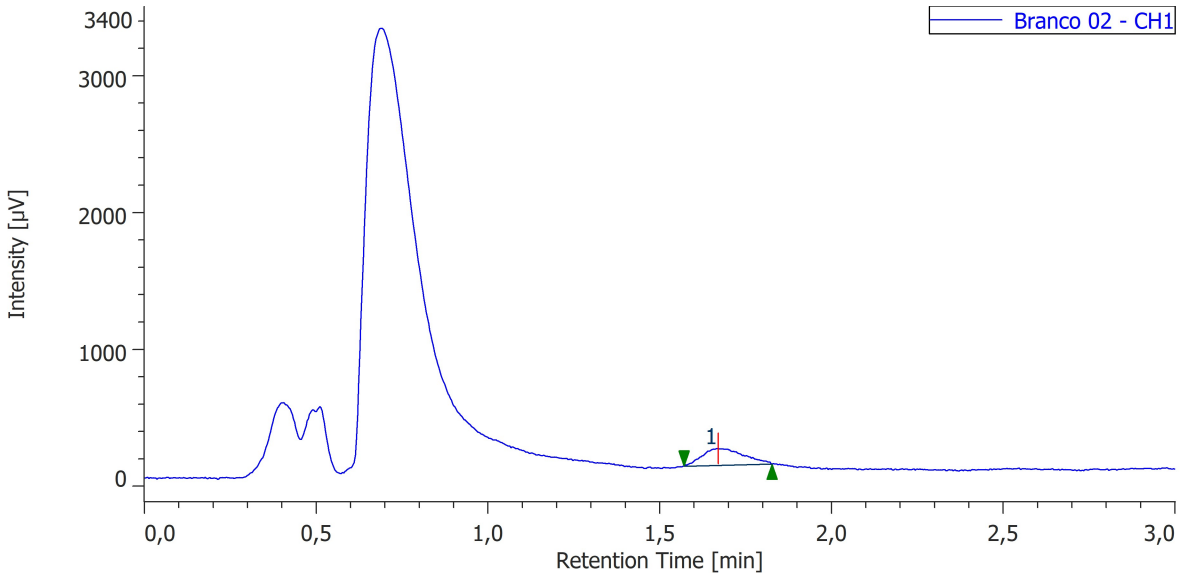


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:22:23
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:32:20
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	Branco 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	1031	123	100,000	100,000	N/A	796	N/A	1,282	

Chromatogram

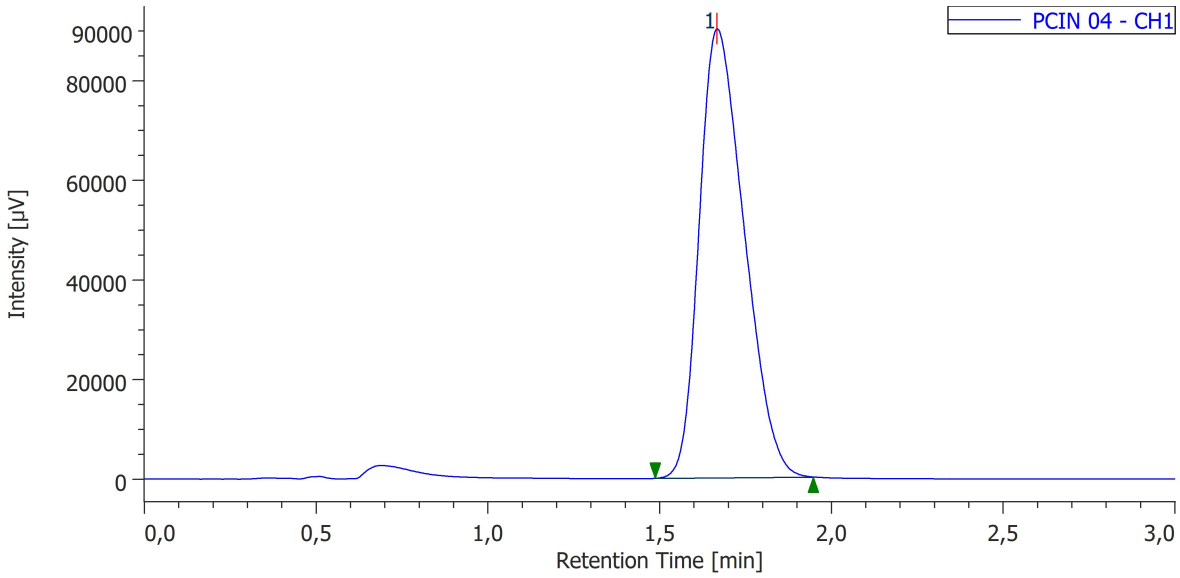


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:15
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:37:25
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	PCIN 04
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,667	820230	90124	100,000	100,000	N/A	746	N/A	1,336	

Chromatogram

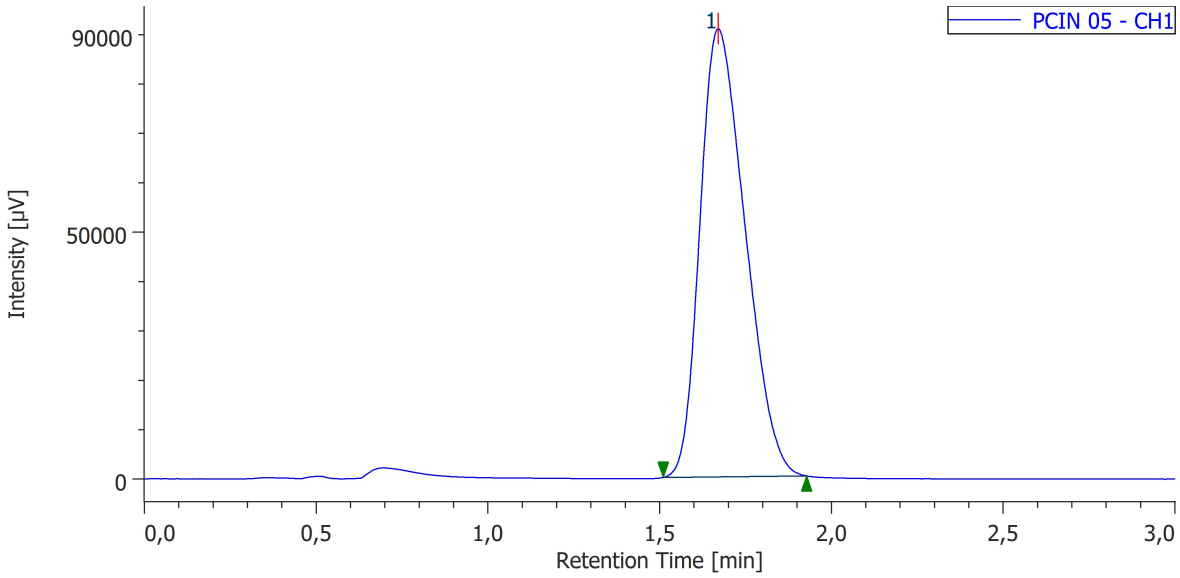


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:15
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:42:29
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	PCIN 05
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	828211	90702	100,000	100,000	N/A	738	N/A	1,323	

Chromatogram

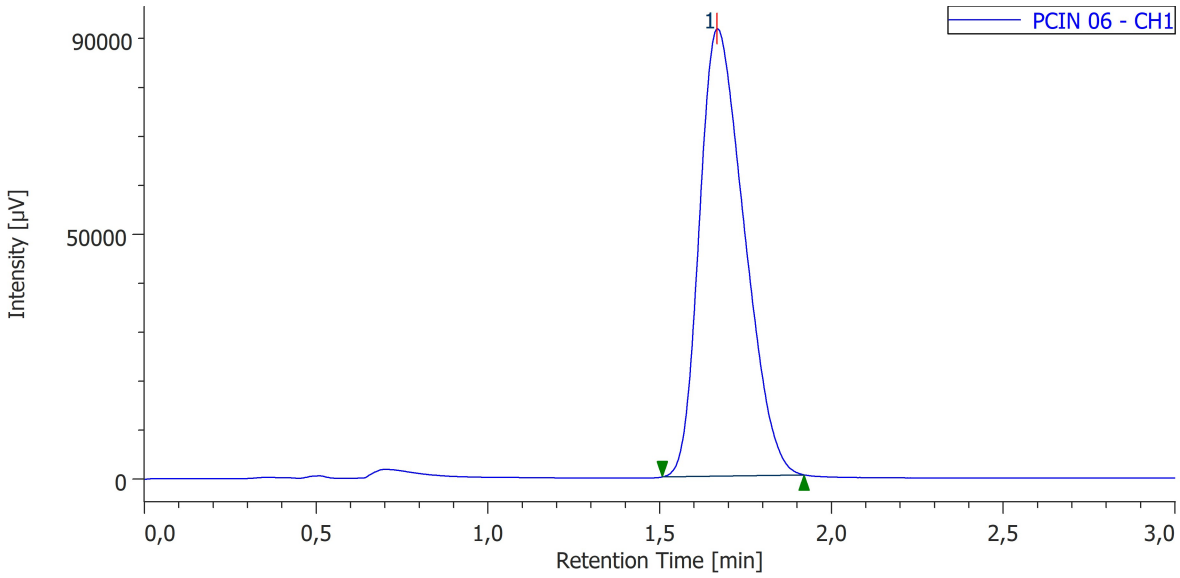


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:09:15
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:47:34
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	PCIN 06
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,667	828276	91382	100,000	100,000	N/A	748	N/A	1,341	

Chromatogram

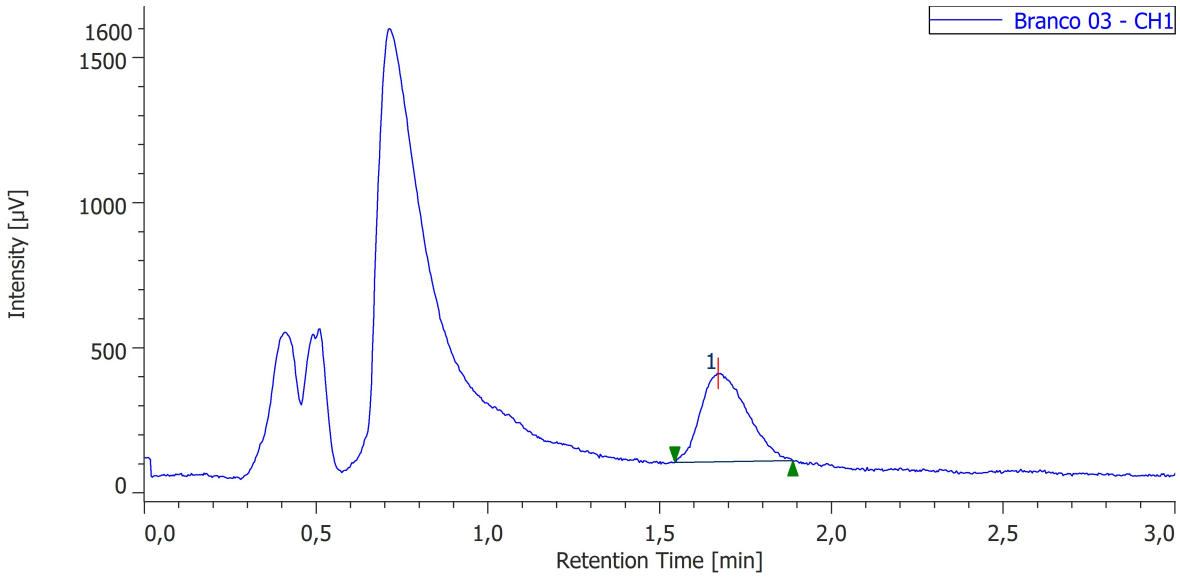


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:22:23
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 14:52:36
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	Branco 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	2858	305	100,000	100,000	N/A	683	N/A	1,306	

Chromatogram

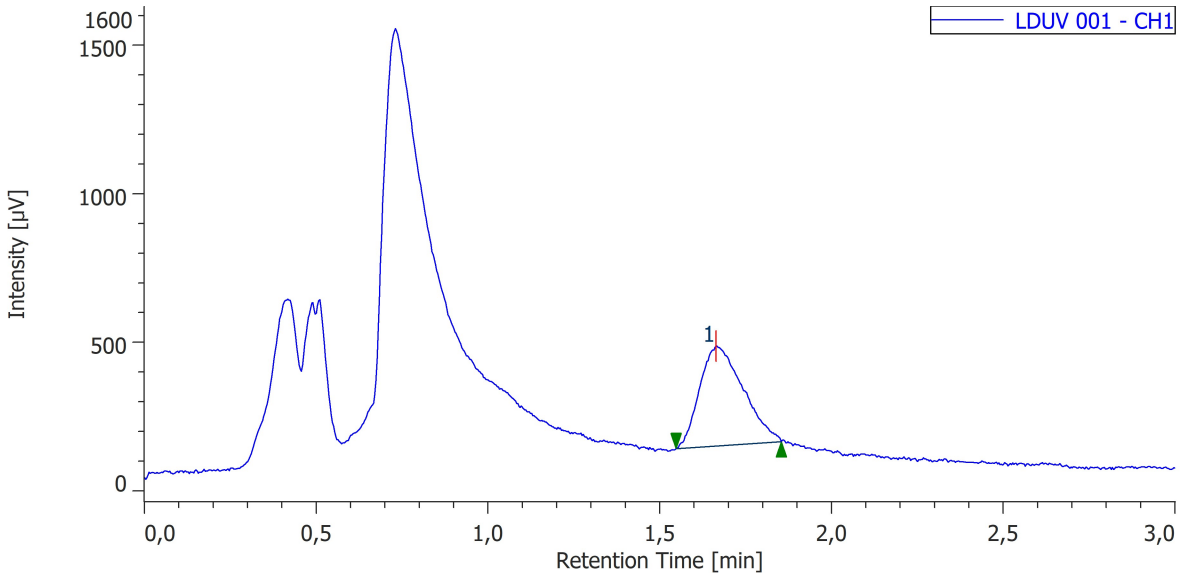


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:30:52
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:00:42
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH1
Sample Name	LDUV 001
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	2939	336	100,000	100,000	N/A	727	N/A	1,379	

Chromatogram

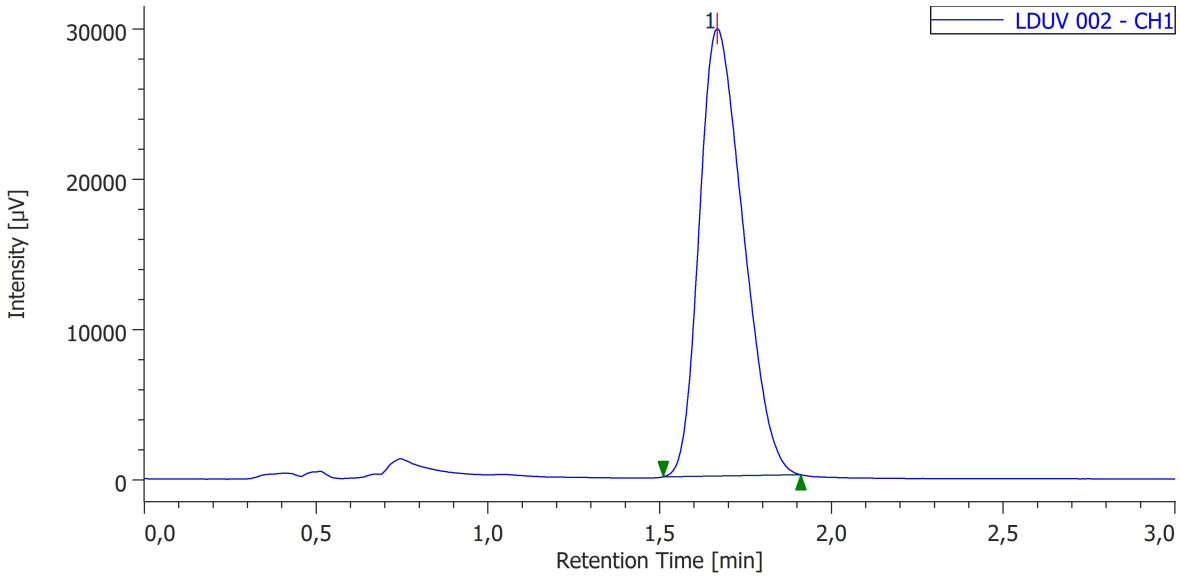


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:30:52
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:05:44
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH1
Sample Name	LDUV 002
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,667	263857	29744	100,000	100,000	N/A	781	N/A	1,311	

Chromatogram

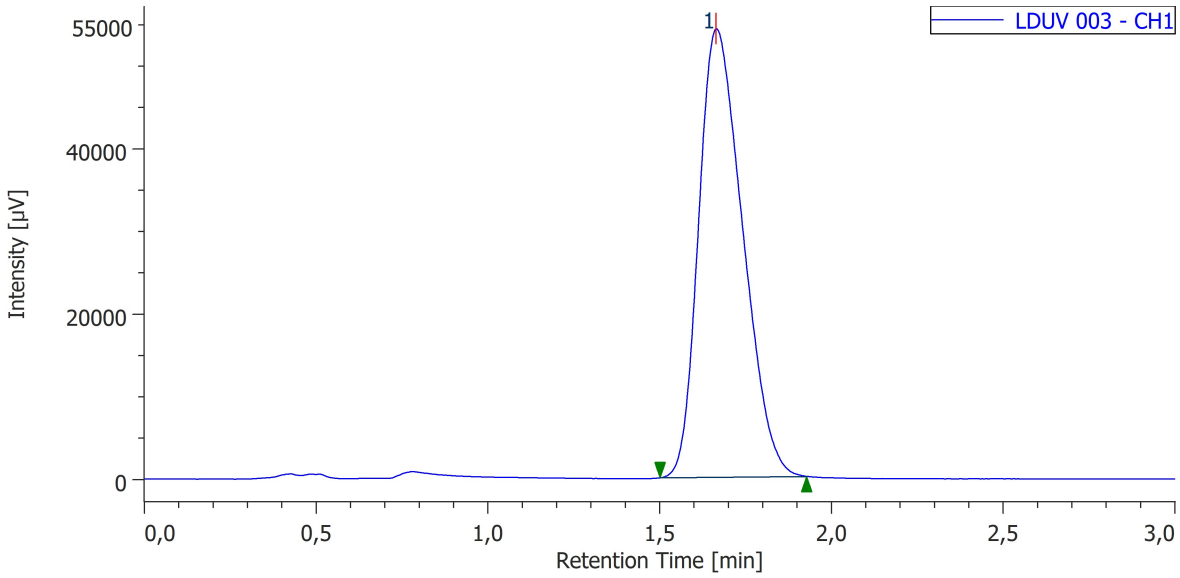


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:30:52
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:10:46
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH1
Sample Name	LDUV 003
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	482882	54234	100,000	100,000	N/A	773	N/A	1,330	

Chromatogram

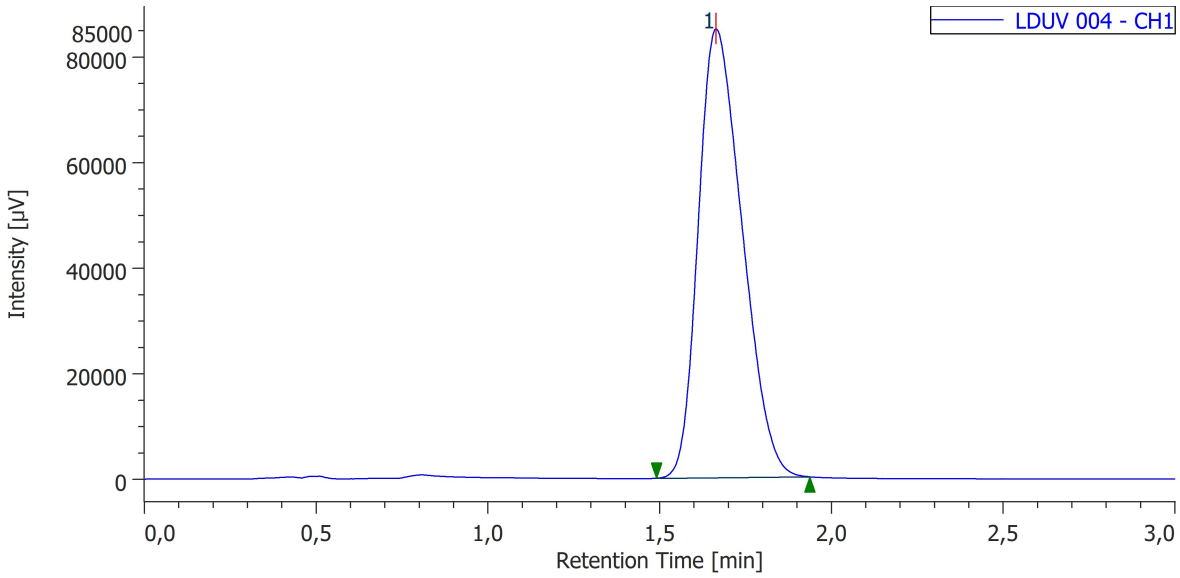


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:30:52
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:15:50
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH1
Sample Name	LDUV 004
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	754450	85029	100,000	100,000	N/A	777	N/A	1,315	

Chromatogram

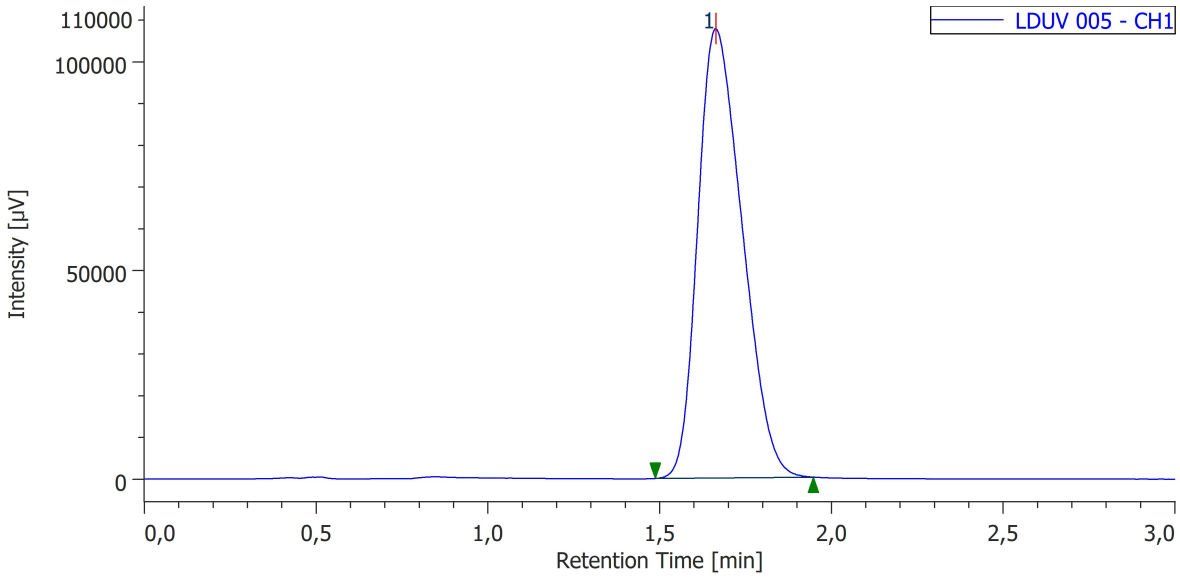


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:30:52
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:20:55
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH1
Sample Name	LDUV 005
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	966813	107616	100,000	100,000	N/A	754	N/A	1,301	

Chromatogram

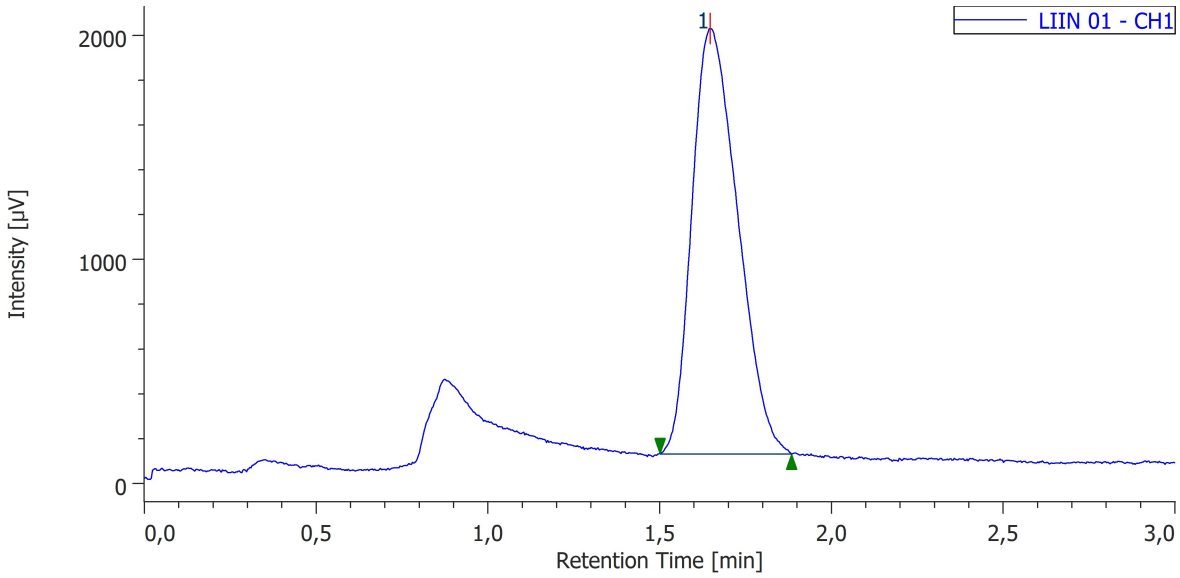


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:37:02
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:28:28
Volume	0,1 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	LIIN 01
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,647	17599	1897	100,000	100,000	N/A	687	N/A	1,315	

Chromatogram

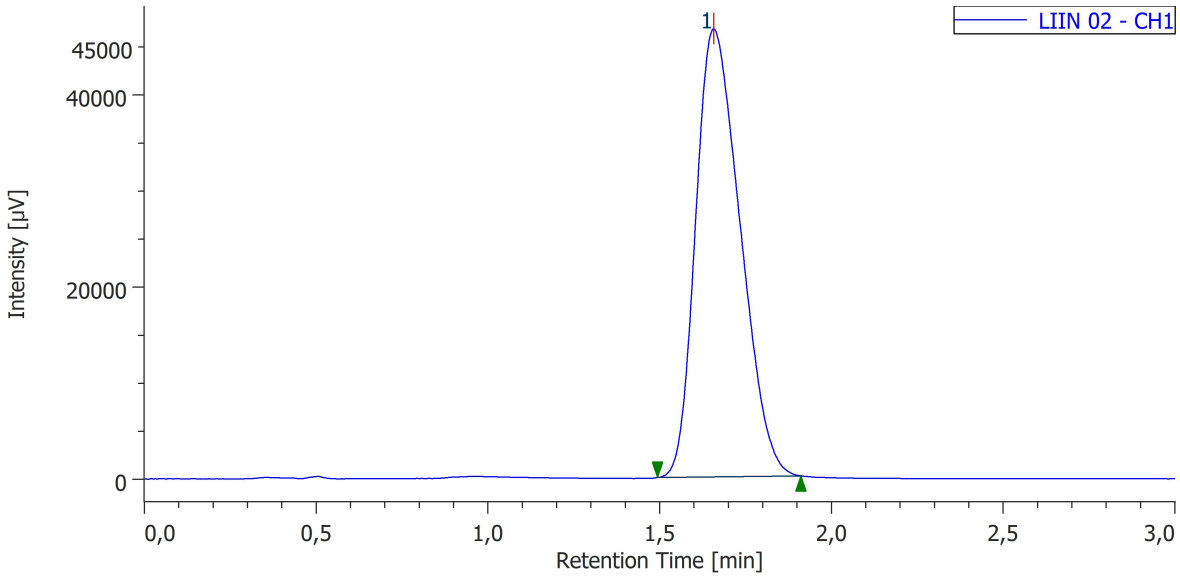


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:37:02
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:33:25
Volume	5,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	LIIN 02
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,657	420041	46624	100,000	100,000	N/A	739	N/A	1,308	

Chromatogram

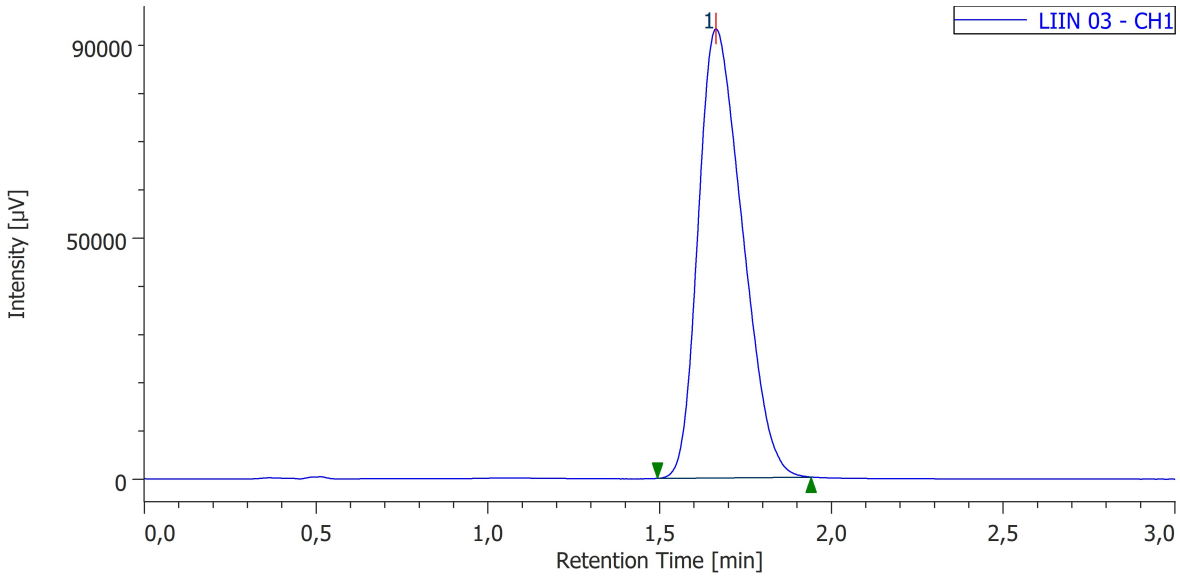


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:37:02
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:38:30
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	LIIN 03
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,663	830486	93095	100,000	100,000	N/A	766	N/A	1,325	

Chromatogram

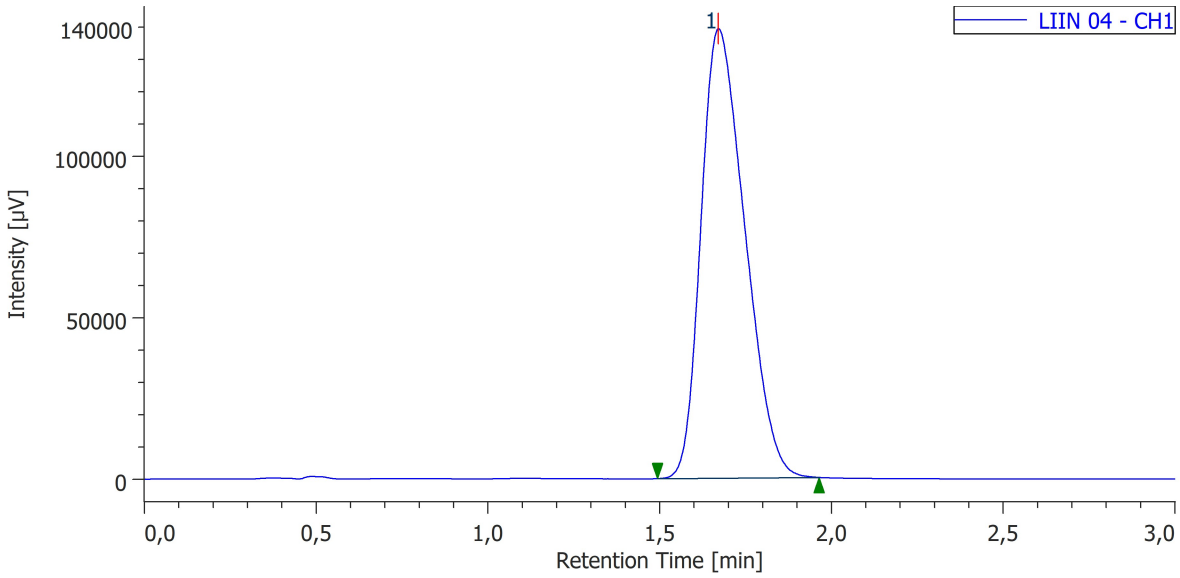


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:37:03
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:43:39
Volume	15,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	LIIN 04
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,670	1235730	139155	100,000	100,000	N/A	782	N/A	1,342	

Chromatogram

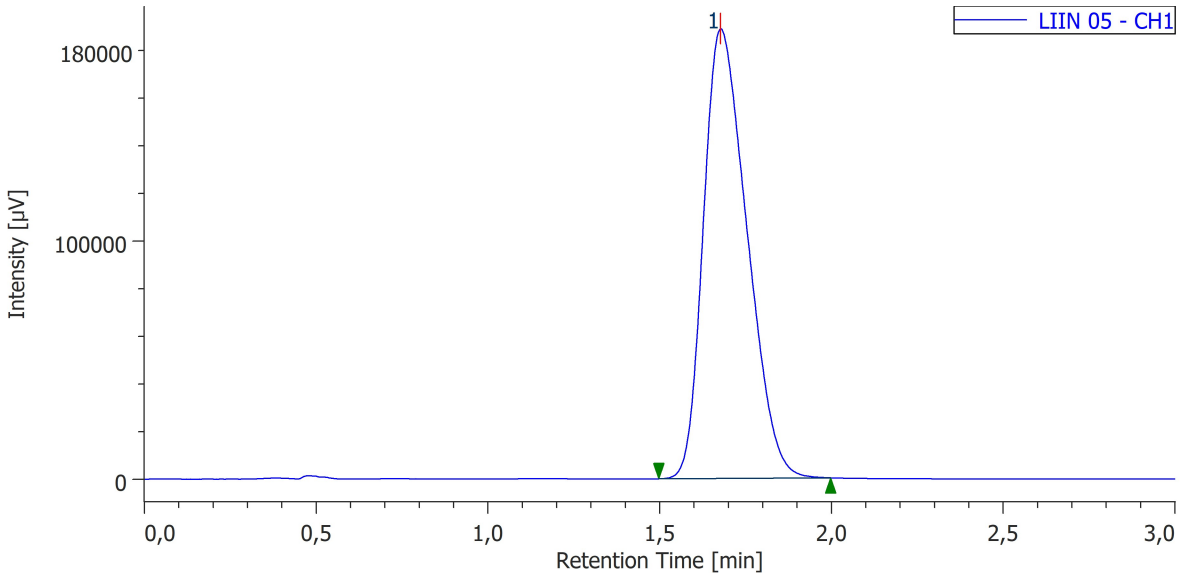


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 11:37:03
Description	
HPLC System Name	HPLC 0001
Injection Date	17/08/2021 15:48:53
Volume	20,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	LIIN 05
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,677	1660681	188687	100,000	100,000	N/A	804	N/A	1,342	

Chromatogram

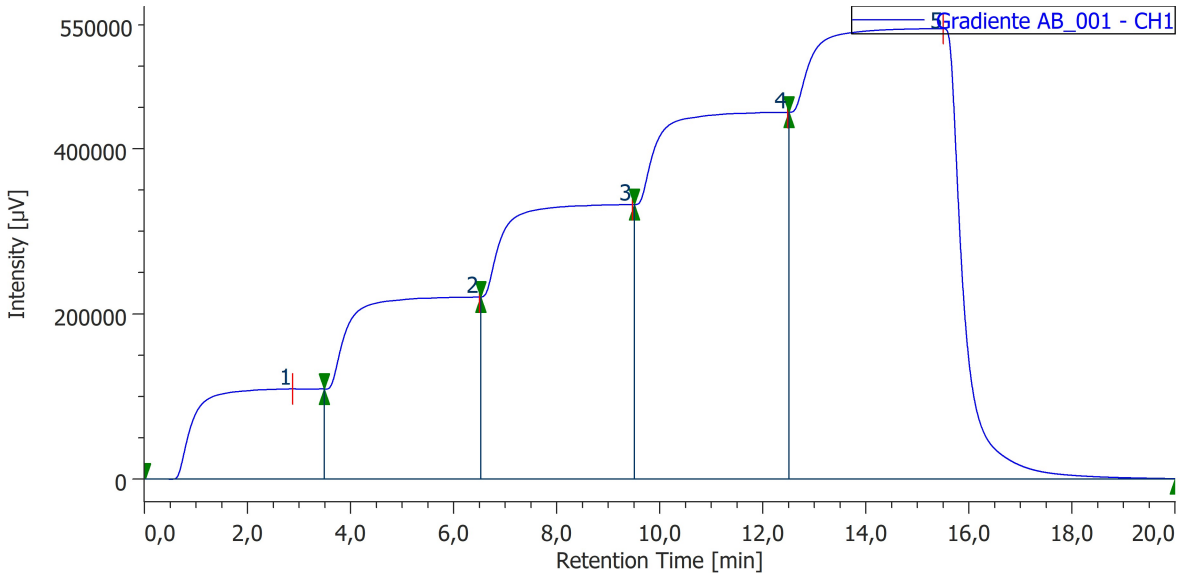


Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 09:42:48
Description	
HPLC System Name	HPLC 0001
Injection Date	18/08/2021 09:19:41
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 1
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Teste de Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	2,873	16619053	108869	5,597	6,604	N/A	N/A	N/A	N/A	
2	40%	1	6,500	37058255	219999	12,480	13,344	N/A	N/A	N/A	N/A	
3	60%	1	9,467	56486890	331756	19,023	20,123	N/A	N/A	N/A	N/A	
4	80%	1	12,483	76852034	443295	25,881	26,889	N/A	N/A	N/A	N/A	
5	100%	1	15,500	109923690	544698	37,019	33,040	N/A	N/A	N/A	N/A	

Chromatogram

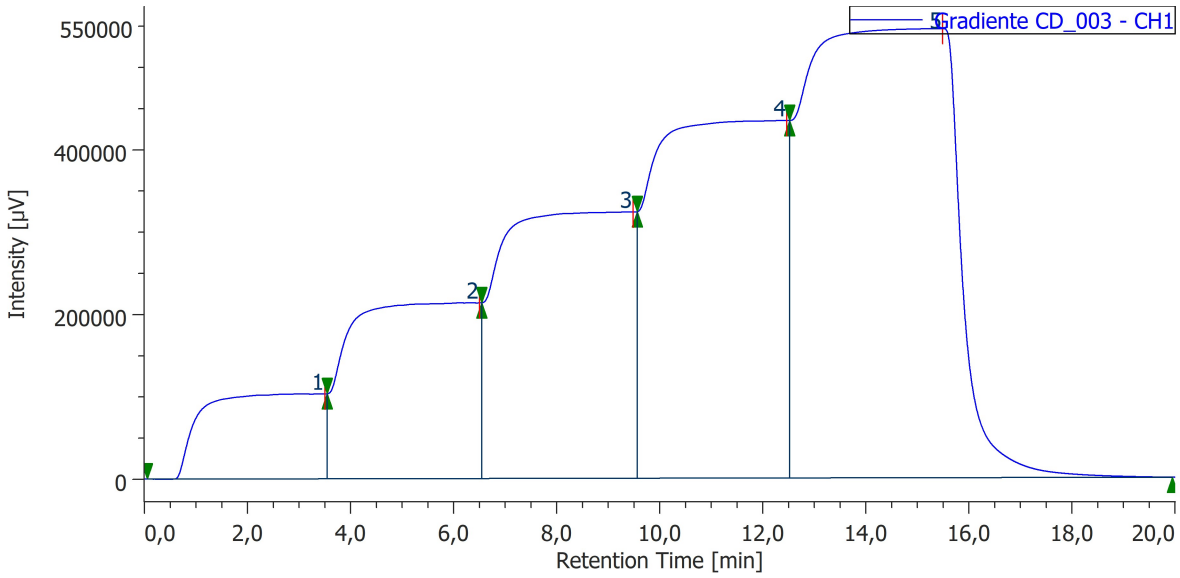

Chromatogram Information	
User Name	Administrator
Date Modified	18/08/2021 10:56:43
Description	
HPLC System Name	HPLC 0001
Injection Date	18/08/2021 10:34:42
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 1
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Teste de Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,500	15977998	103094	5,487	6,375	N/A	N/A	N/A	N/A	
2	40%	1	6,503	35765547	213021	12,282	13,172	N/A	N/A	N/A	N/A	
3	60%	1	9,483	55803609	322946	19,163	19,969	N/A	N/A	N/A	N/A	
4	80%	1	12,463	74448061	433450	25,565	26,801	N/A	N/A	N/A	N/A	
5	100%	1	15,487	109213365	544760	37,503	33,684	N/A	N/A	N/A	N/A	