
Chromatogram

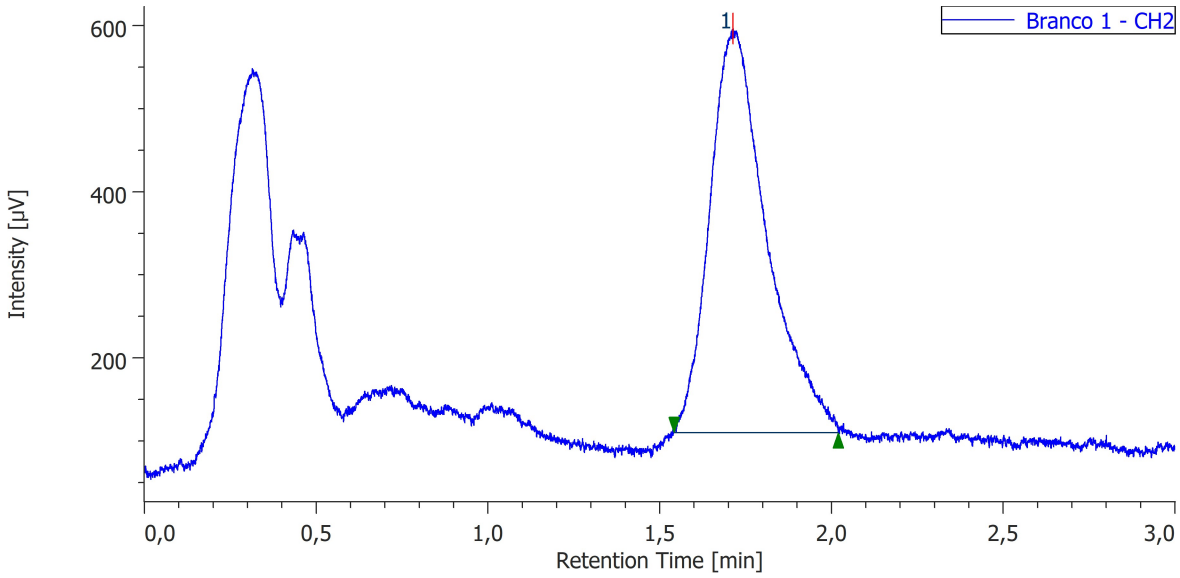


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:14:15
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,713	5599	486	100,000	100,000	N/A	564	N/A	1,436	

Chromatogram

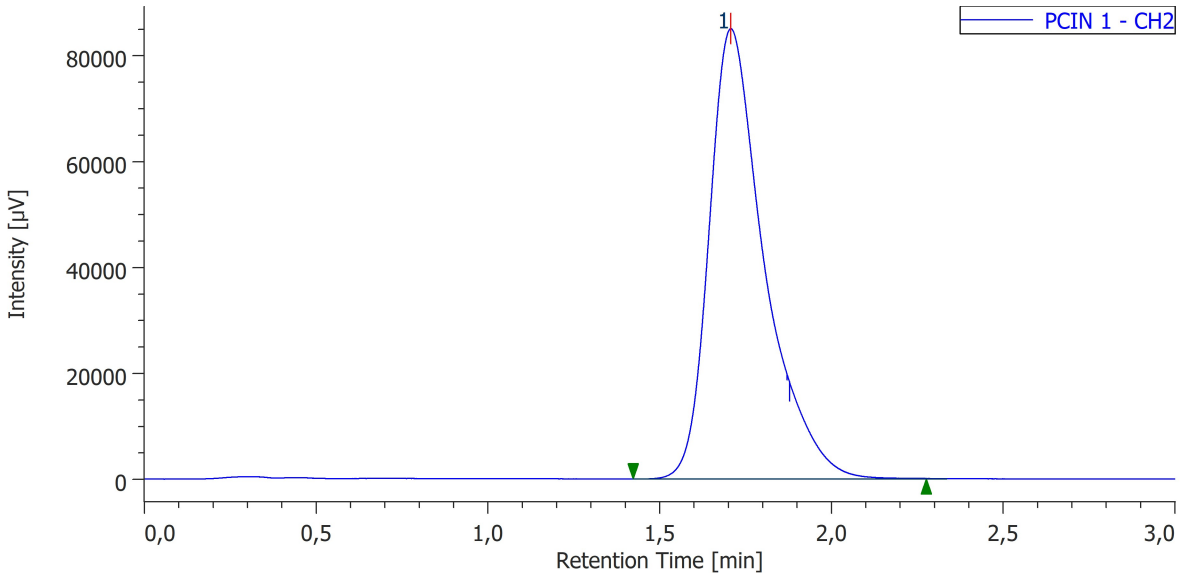


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:18:36
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,706	951381	84996	100,000	100,000	N/A	620	N/A	1,492	

Chromatogram

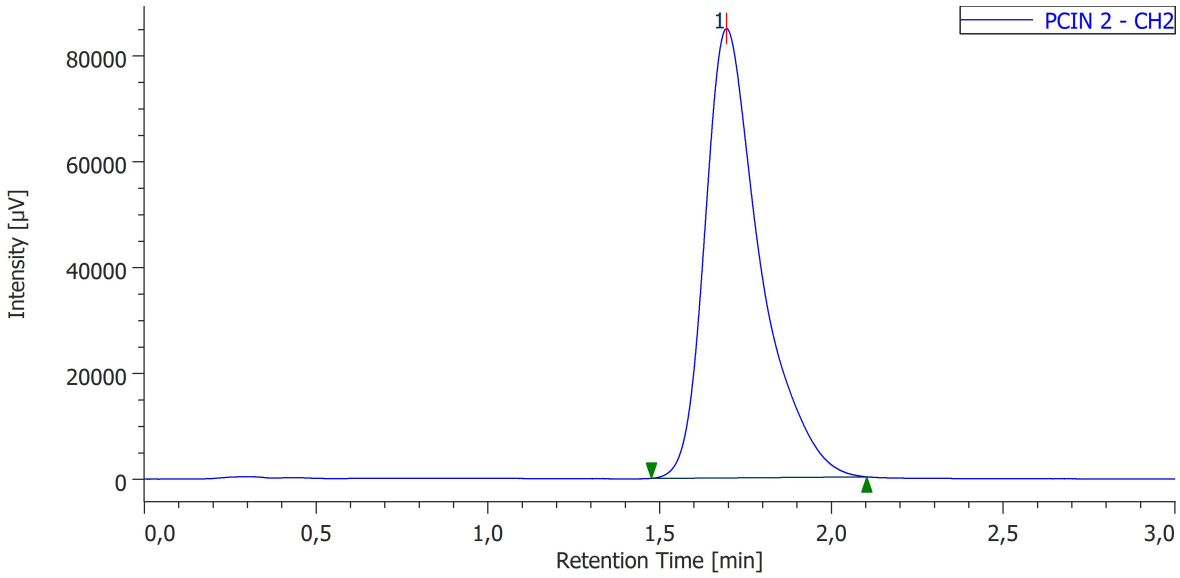


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:22:56
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,694	951638	84835	100,000	100,000	N/A	607	N/A	1,505	

Chromatogram

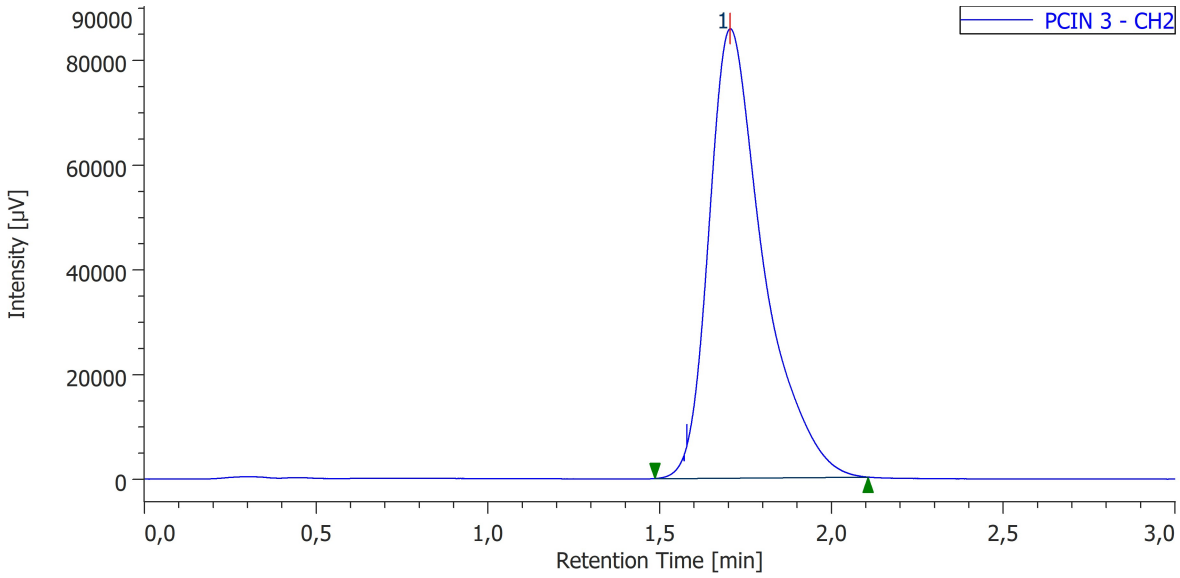

Chromatogram Information


User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:27:17
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,705	946696	85794	100,000	100,000	N/A	634	N/A	1,503	

Chromatogram

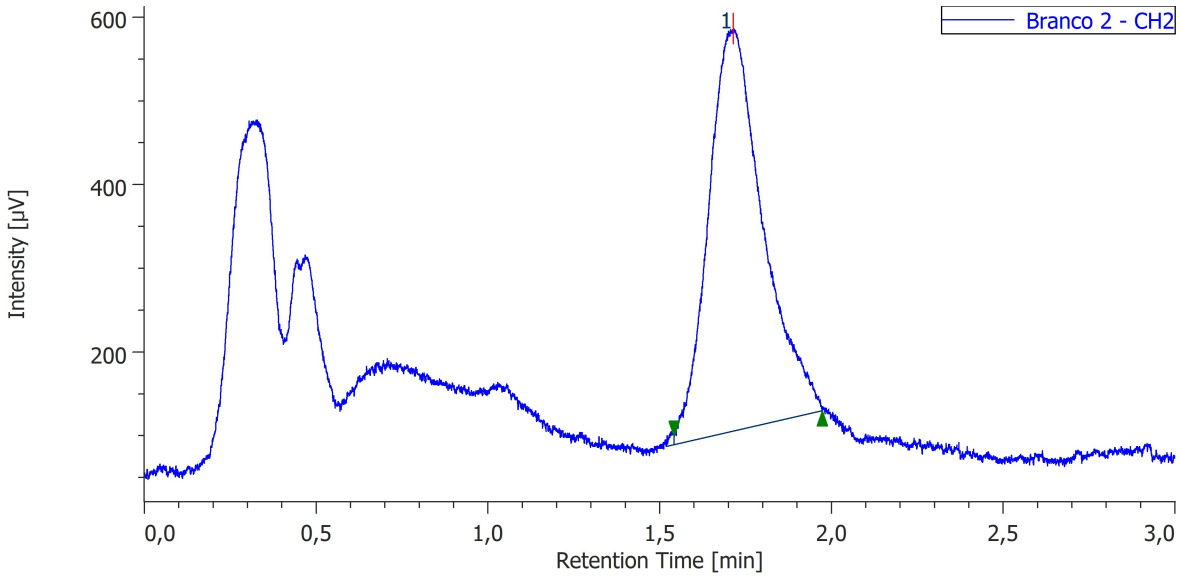


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:31:37
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,714	5311	480	100,000	100,000	N/A	622	N/A	1,220	

Chromatogram

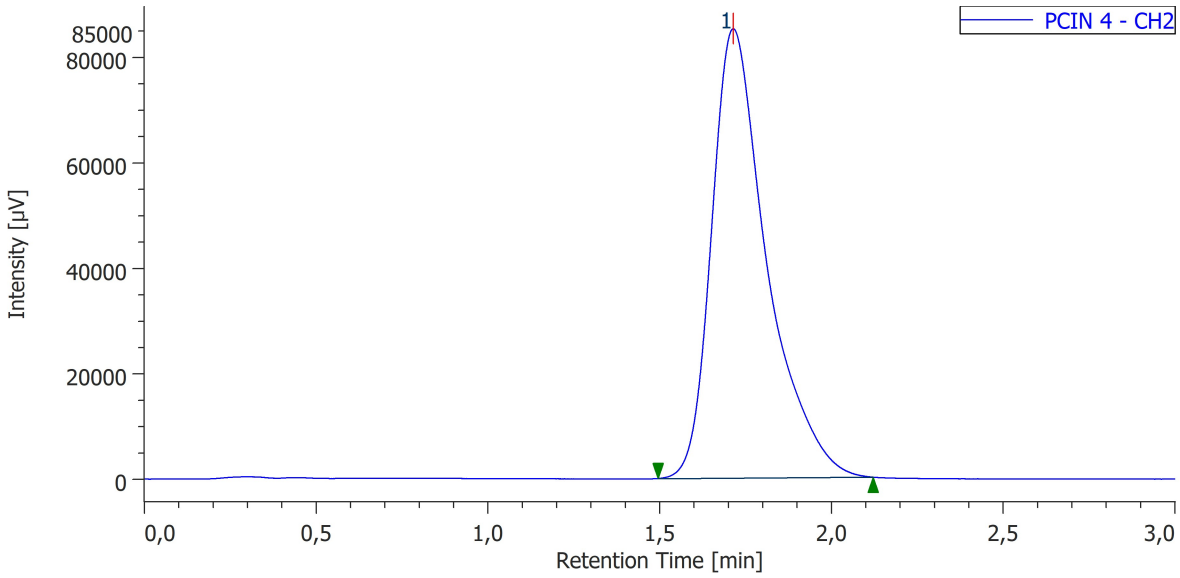

Chromatogram Information


User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:36:00
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,714	950331	85163	100,000	100,000	N/A	626	N/A	1,498	

Chromatogram

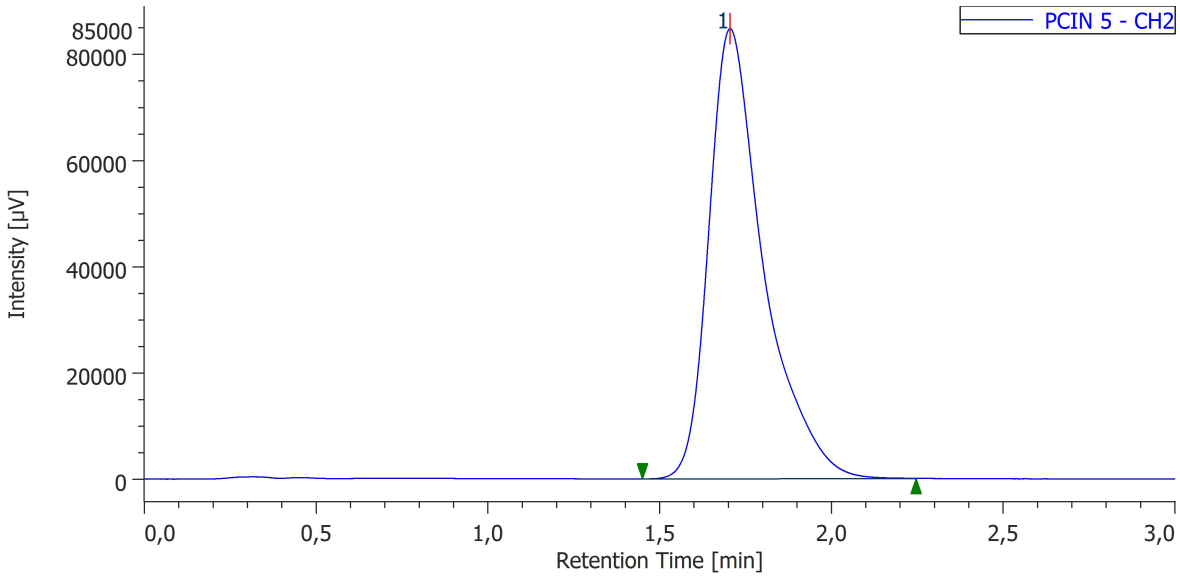

Chromatogram Information


User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:40:20
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,704	938587	84702	100,000	100,000	N/A	645	N/A	1,531	

Chromatogram

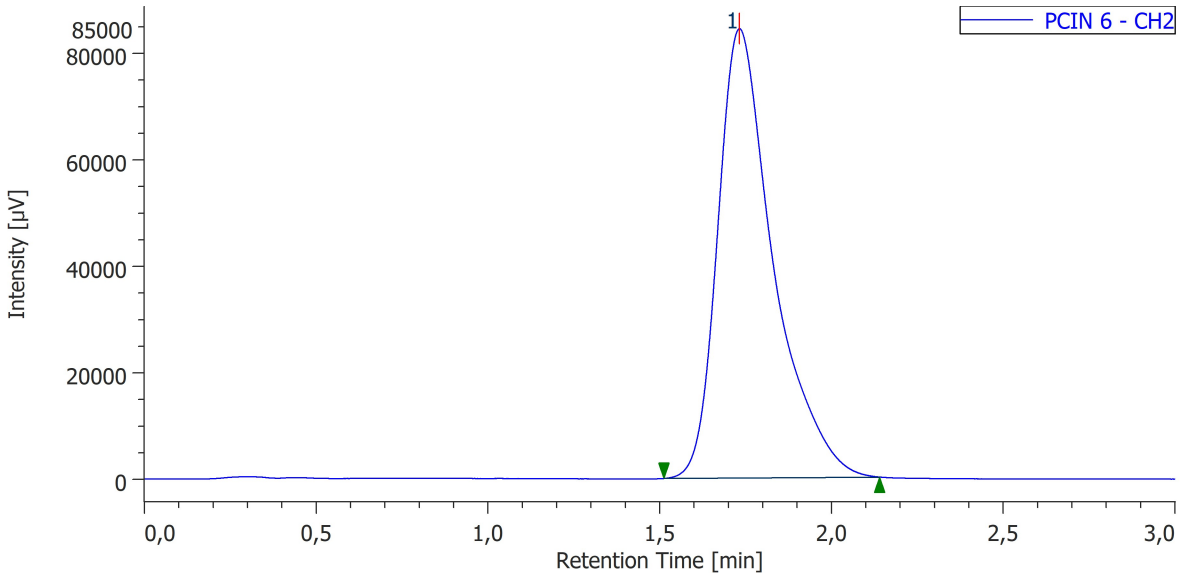

Chromatogram Information


User Name	Administrator
Date Modified	19/08/2021 12:11:14
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:44:41
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,731	946743	84364	100,000	100,000	N/A	633	N/A	1,511	

Chromatogram

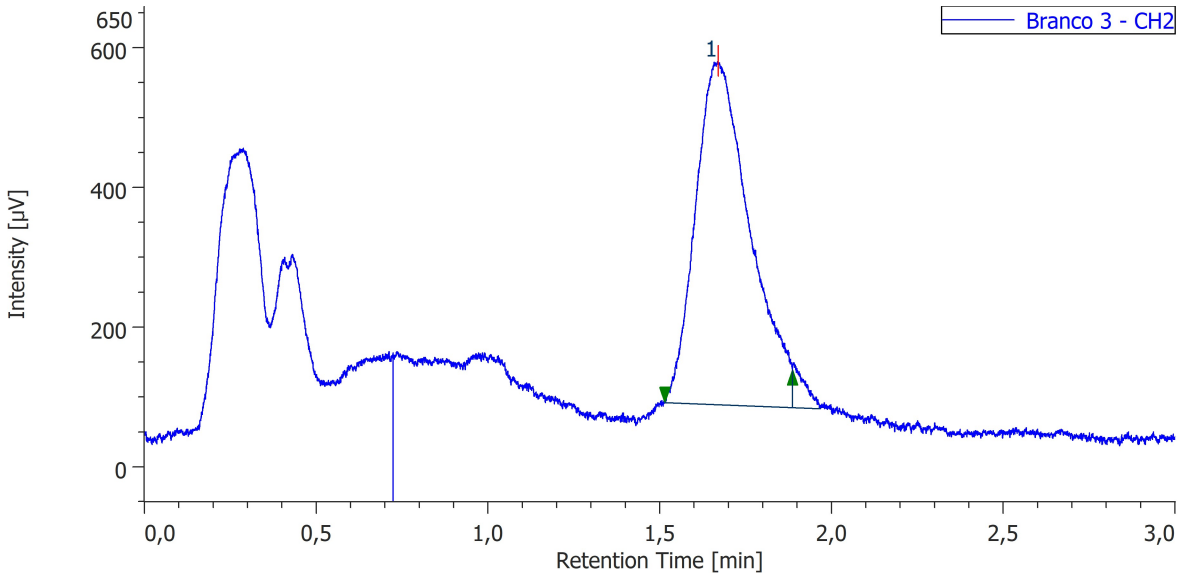


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:11:15
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:49:03
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,670	5388	492	100,000	100,000	N/A	558	N/A	N/A	

Chromatogram

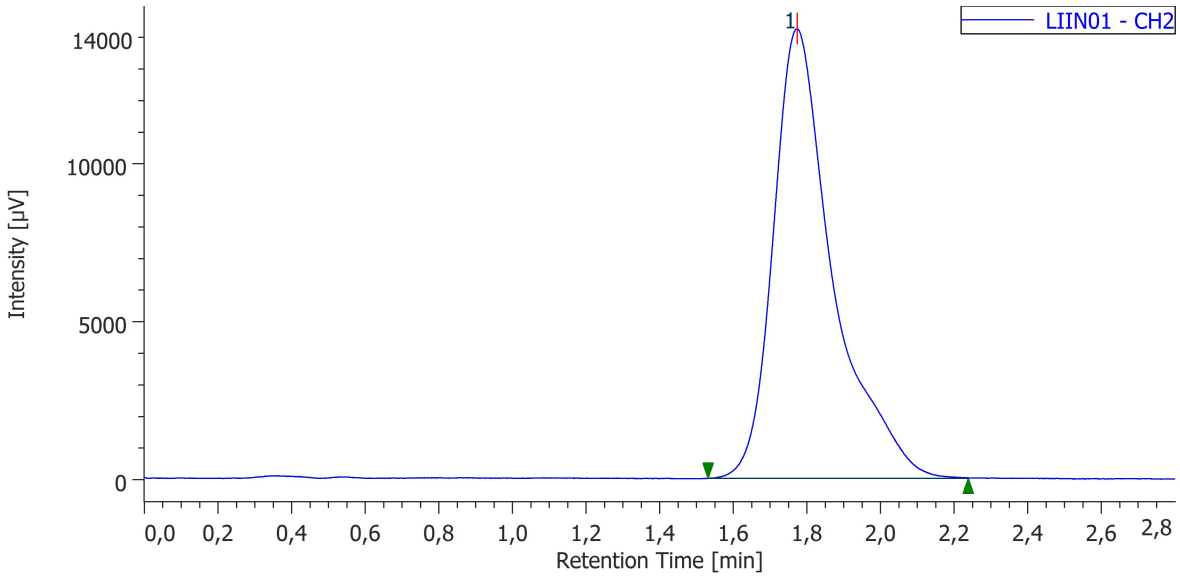


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:59:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 11:58:42
Volume	0,1 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN01-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,773	159967	14228	100,000	100,000	N/A	724	N/A	1,512	

Chromatogram

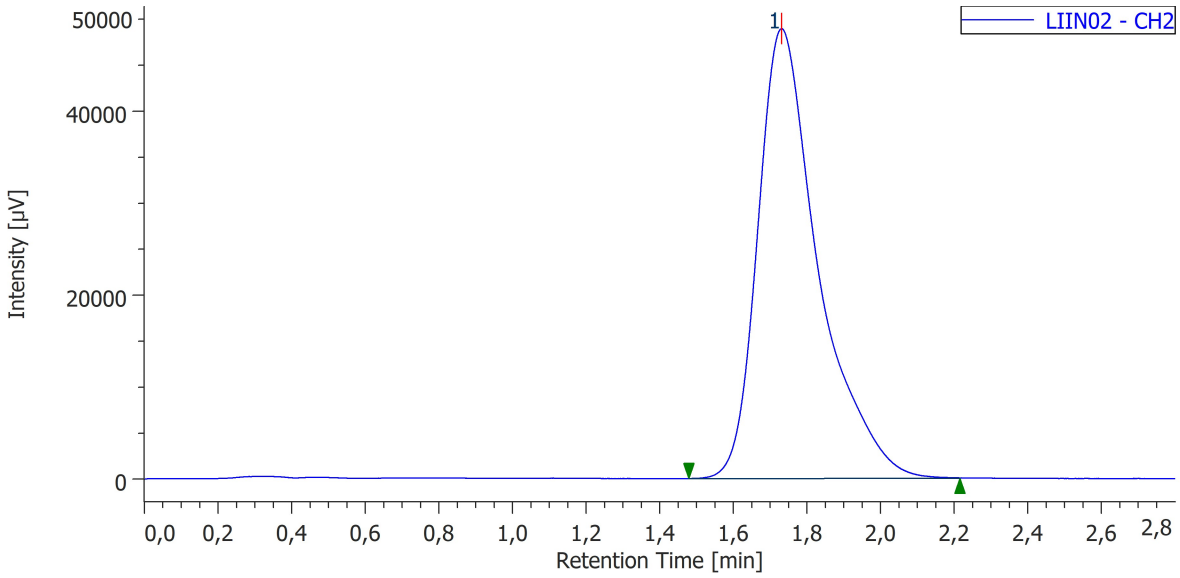


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:59:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 12:03:00
Volume	5,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN02-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,731	556289	48871	100,000	100,000	N/A	629	N/A	1,502	

Chromatogram

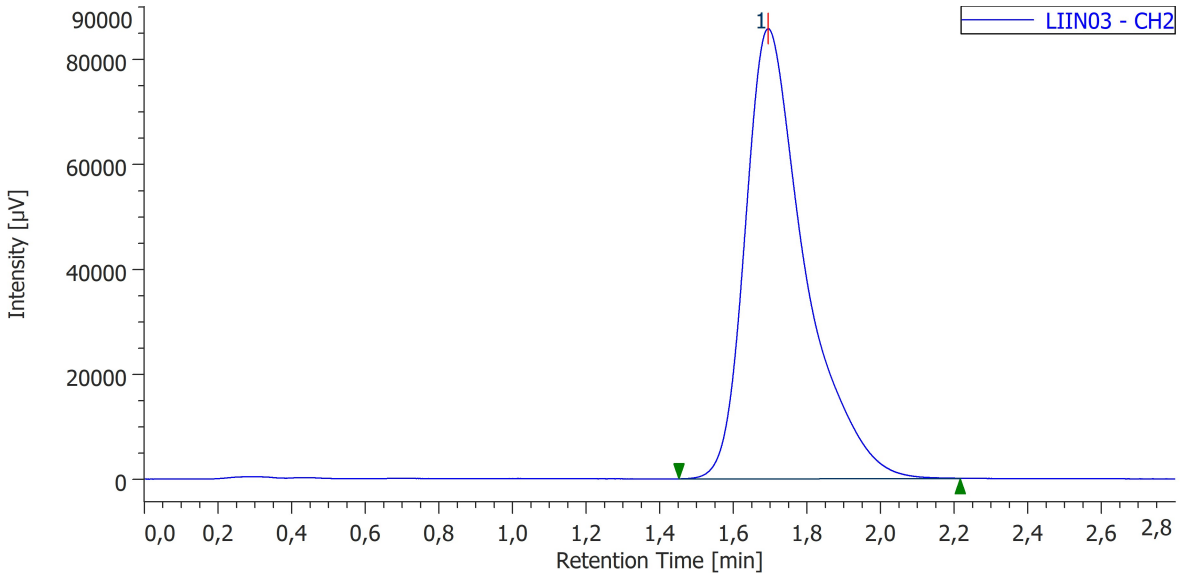


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:59:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 12:07:20
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN03-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,694	966296	85717	100,000	100,000	N/A	613	N/A	1,541	

Chromatogram

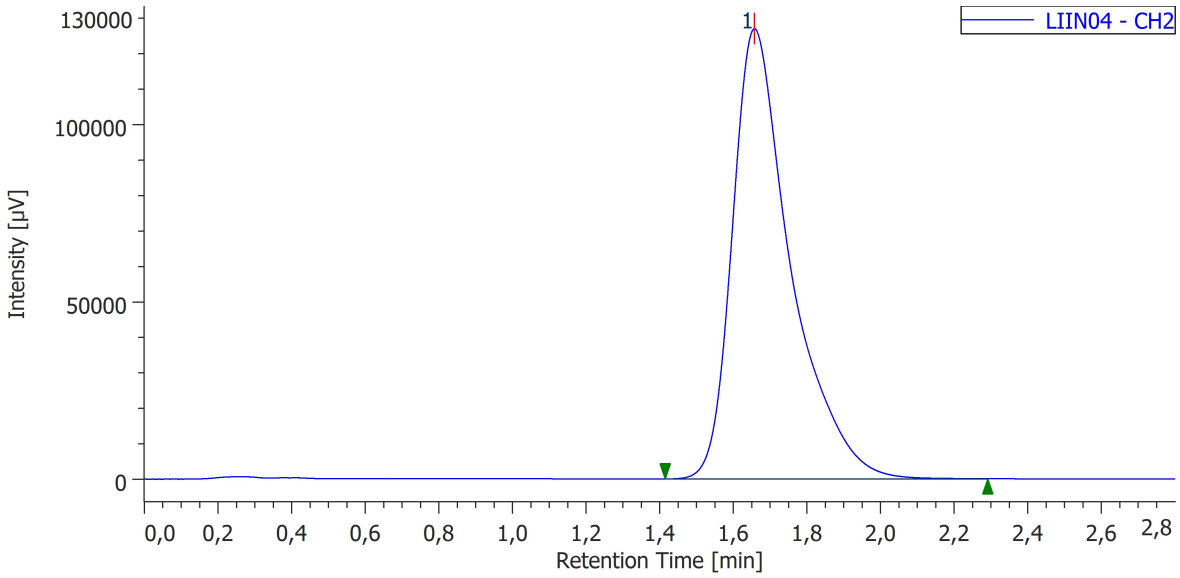


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:59:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 12:11:46
Volume	15,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN04-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,657	1399227	126926	100,000	100,000	N/A	615	N/A	1,560	

Chromatogram

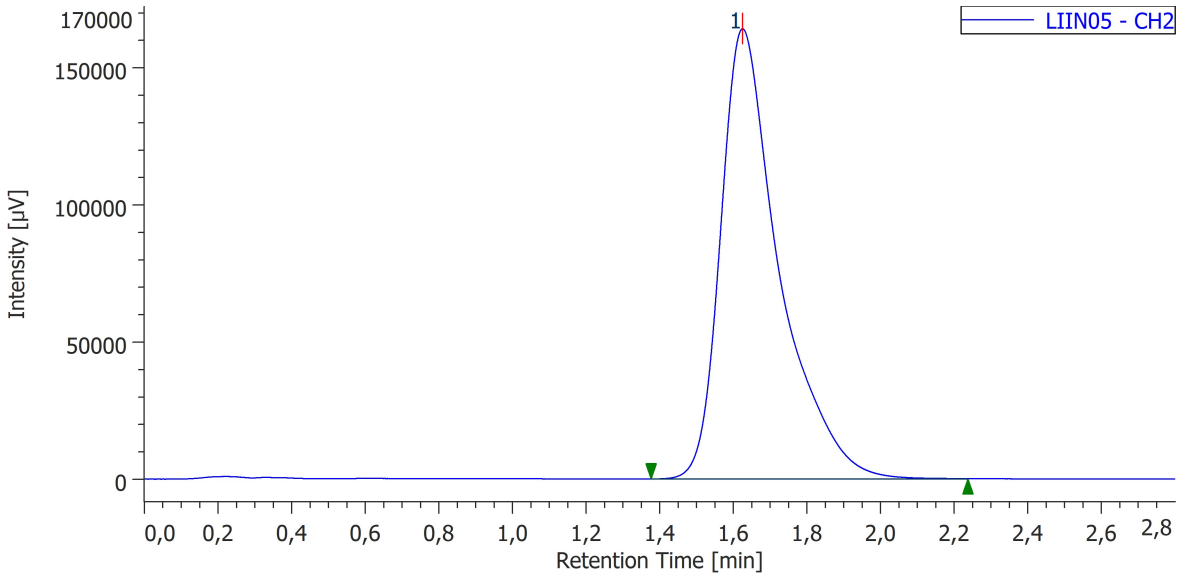


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 12:59:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 12:16:17
Volume	20,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 2
Acquisition Time	2,8 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Pd Cafeina01
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN05-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	Integração_Cafeina 09

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	2	1,625	1809312	164065	100,000	100,000	N/A	605	N/A	1,584	

Chromatogram

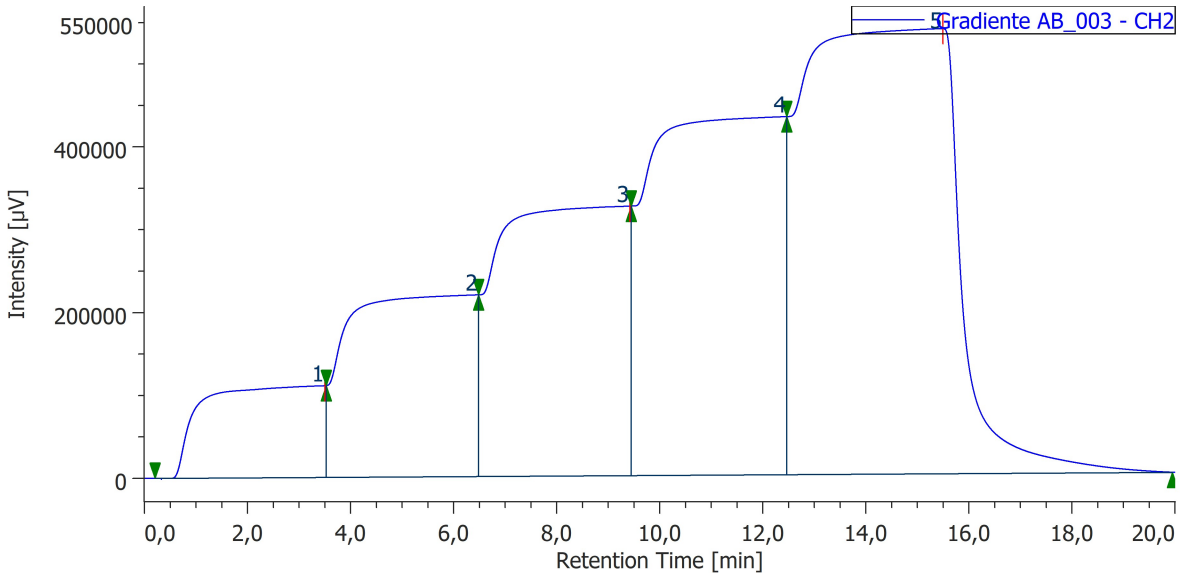


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 15:45:58
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 14:49:05
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 2
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_003-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	2	3,500	17123895	110456	5,832	6,805	N/A	N/A	N/A	N/A	
2	40%	2	6,485	36253935	219022	12,347	13,493	N/A	N/A	N/A	N/A	
3	60%	2	9,420	54860434	324977	18,684	20,020	N/A	N/A	N/A	N/A	
4	80%	2	12,464	75069723	431845	25,567	26,604	N/A	N/A	N/A	N/A	
5	100%	2	15,491	110313595	536935	37,570	33,078	N/A	N/A	N/A	N/A	

Chromatogram

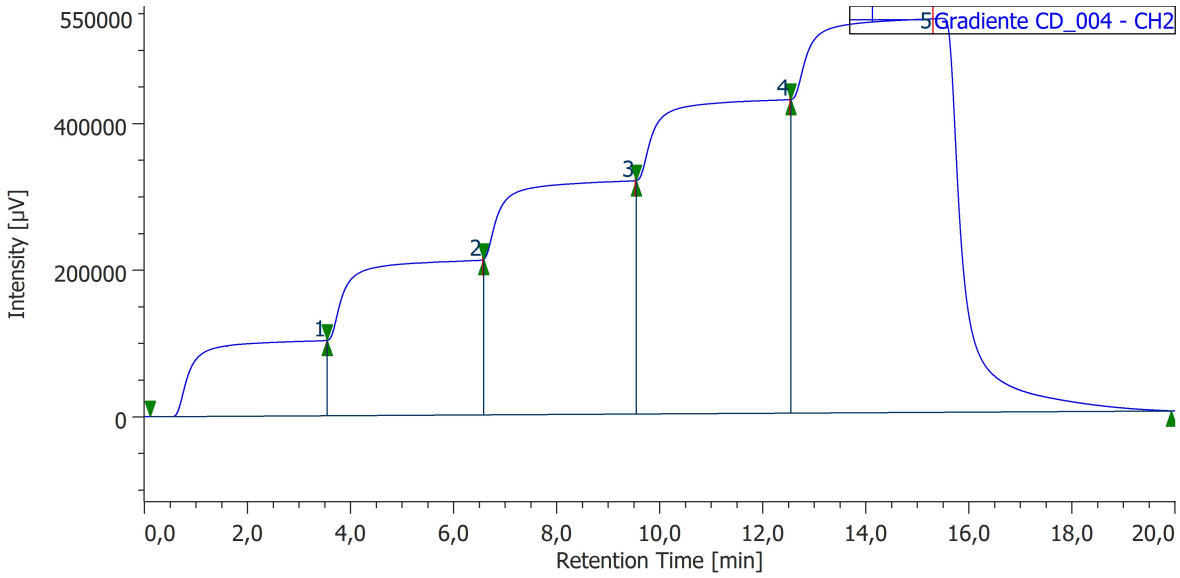


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 15:45:58
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 15:17:03
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 2
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_004-CH2
Sample Name	
Channel Name	
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	2	3,540	15952043	102724	5,534	6,438	N/A	N/A	N/A	N/A	
2	40%	2	6,560	35748419	211238	12,403	13,240	N/A	N/A	N/A	N/A	
3	60%	2	9,522	54025052	317853	18,744	19,922	N/A	N/A	N/A	N/A	
4	80%	2	12,521	74183173	427356	25,738	26,785	N/A	N/A	N/A	N/A	
5	100%	2	15,300	108320692	536327	37,581	33,615	N/A	N/A	N/A	N/A	

Chromatogram

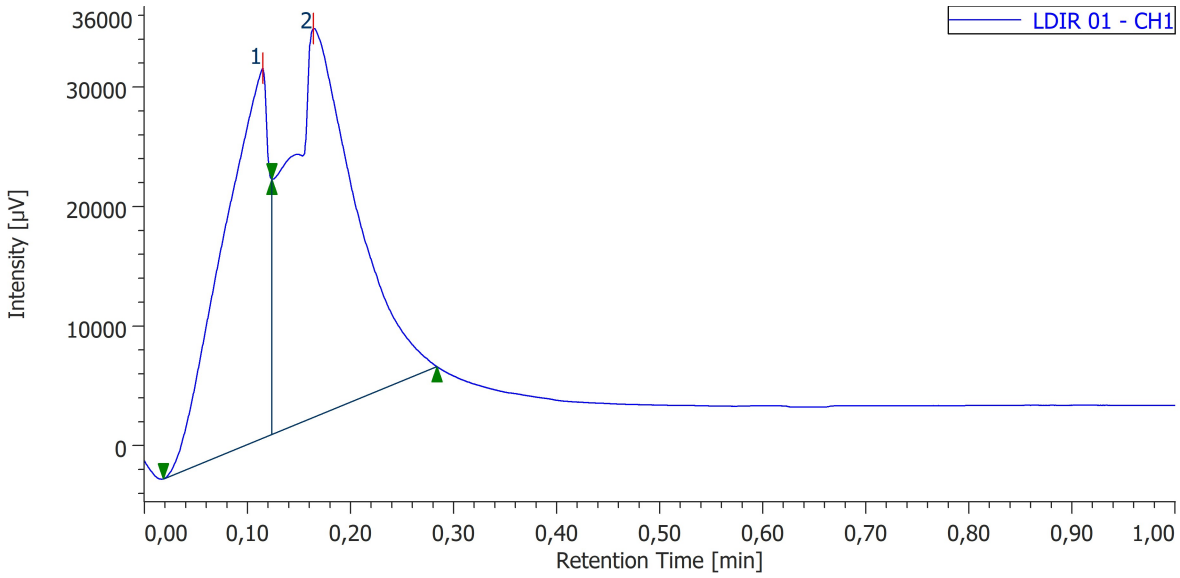


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 17:25:54
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 16:38:52
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	1,0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH1
Sample Name	
Channel Name	RI
Sampling Interval	20 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,115	95810	30930	39,342	48,766	N/A	N/A	N/A	N/A	
2	RI	1	0,164	147722	32495	60,658	51,234	N/A	N/A	N/A	N/A	

Chromatogram

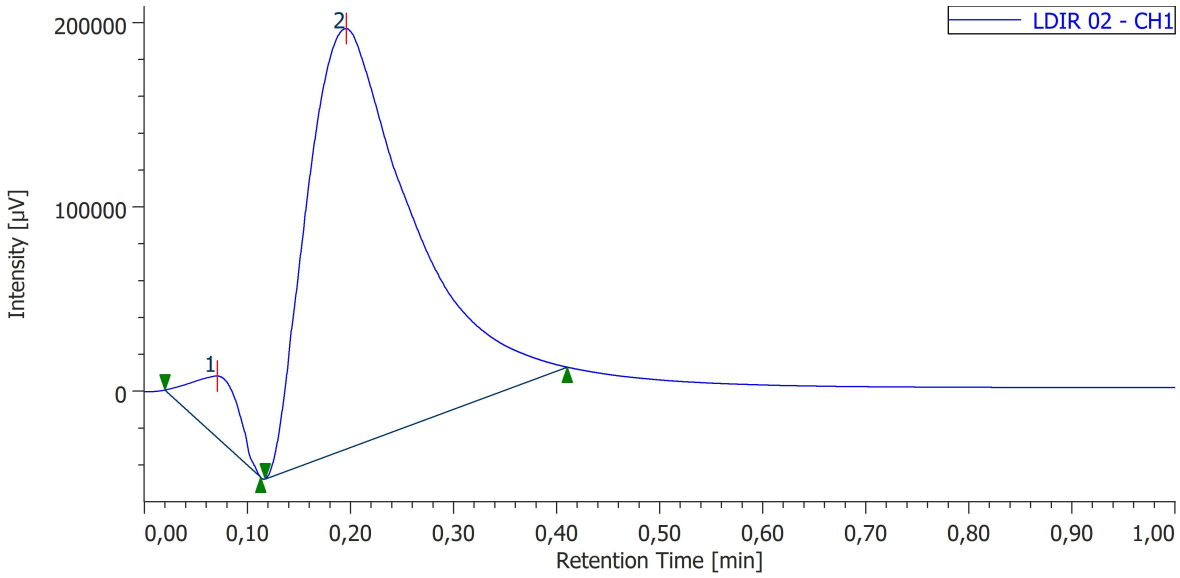


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 17:25:54
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 16:41:39
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	1,0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH1
Sample Name	
Channel Name	RI
Sampling Interval	20 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,071	104454	33454	6,043	12,803	N/A	10	0,924	0,898	
2	RI	1	0,196	1624078	227856	93,957	87,197	N/A	18	N/A	1,813	

Chromatogram

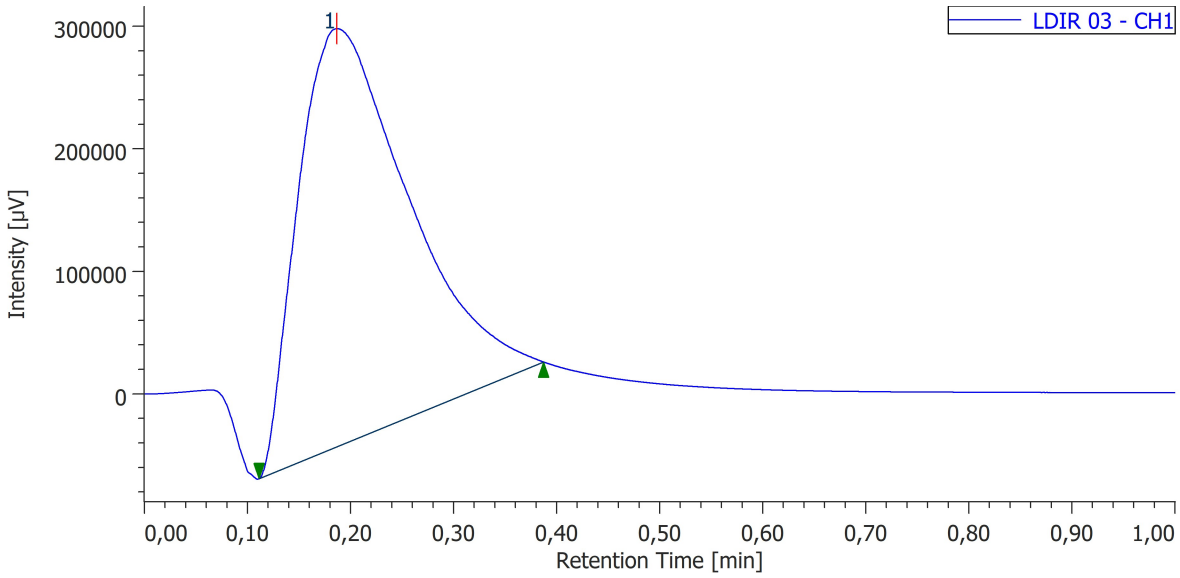


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 17:25:55
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 16:44:27
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação HPLC 2
Acquisition Time	1,0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH1
Sample Name	
Channel Name	RI
Sampling Interval	20 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,187	2539803	340971	100,000	100,000	N/A	14	N/A	1,803	

Chromatogram

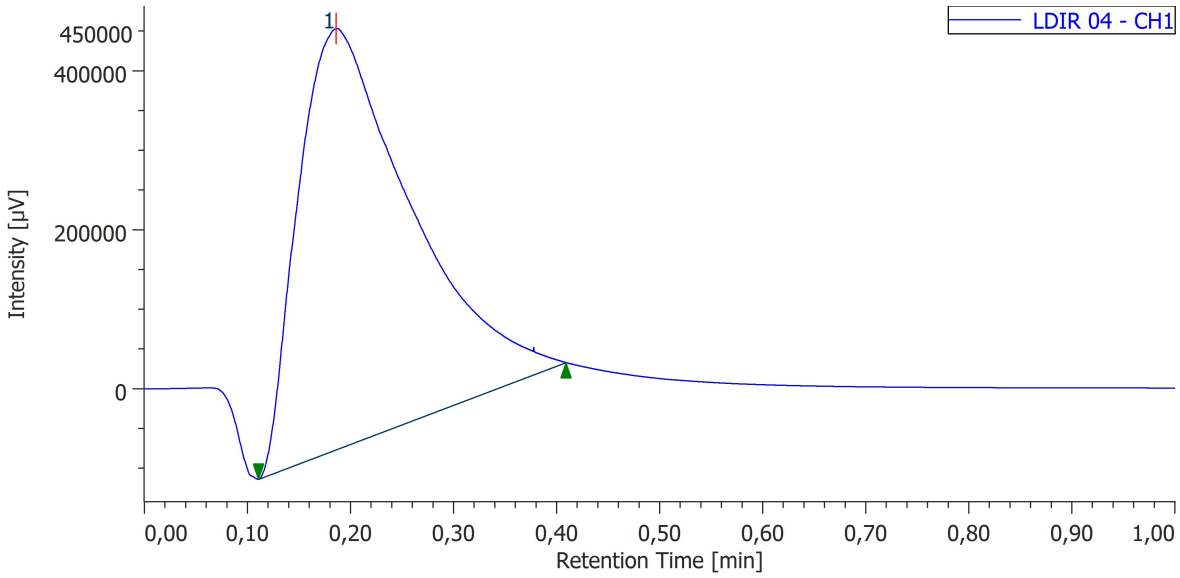


Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 17:25:55
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 16:47:14
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação HPLC 2
Acquisition Time	1,0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH1
Sample Name	
Channel Name	RI
Sampling Interval	20 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,186	4025113	529630	100,000	100,000	N/A	14	N/A	1,965	

Chromatogram

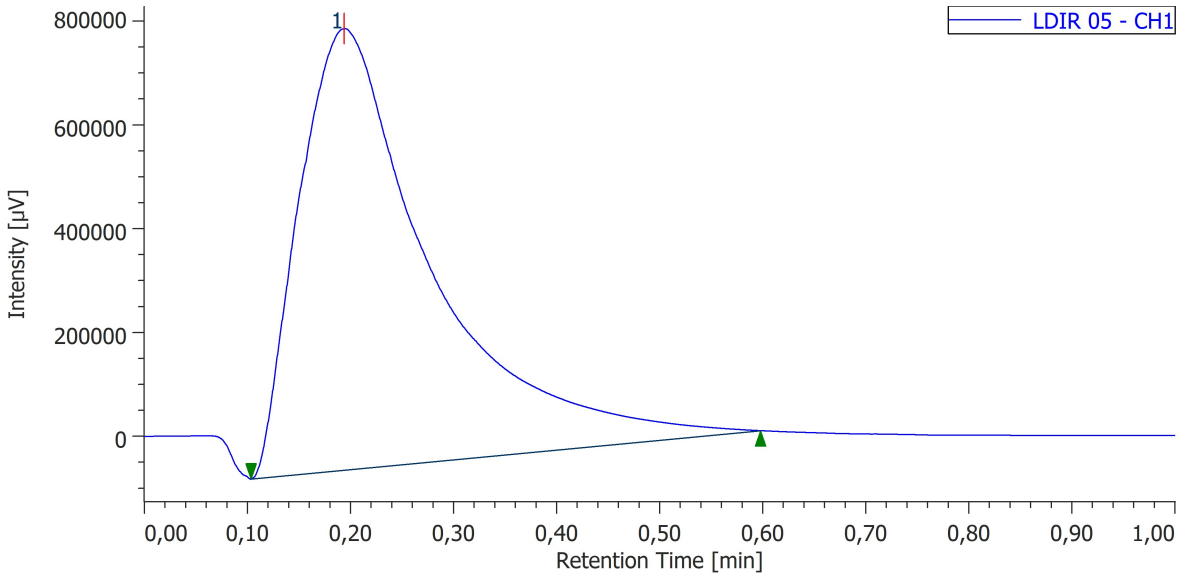

Chromatogram Information	
User Name	Administrator
Date Modified	19/08/2021 17:25:55
Description	
HPLC System Name	HPLC 002 RI
Injection Date	19/08/2021 16:50:02
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação HPLC 2
Acquisition Time	1,0 [min]
Acquisition Sequence	LDIR
Control Method	Qualificação
Peak ID Table	RI
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH1
Sample Name	
Channel Name	RI
Sampling Interval	20 [msec]
Peak Method	RI

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,194	7632639	850575	100,000	100,000	N/A	13	N/A	2,319	