
Peak Find - EDUV

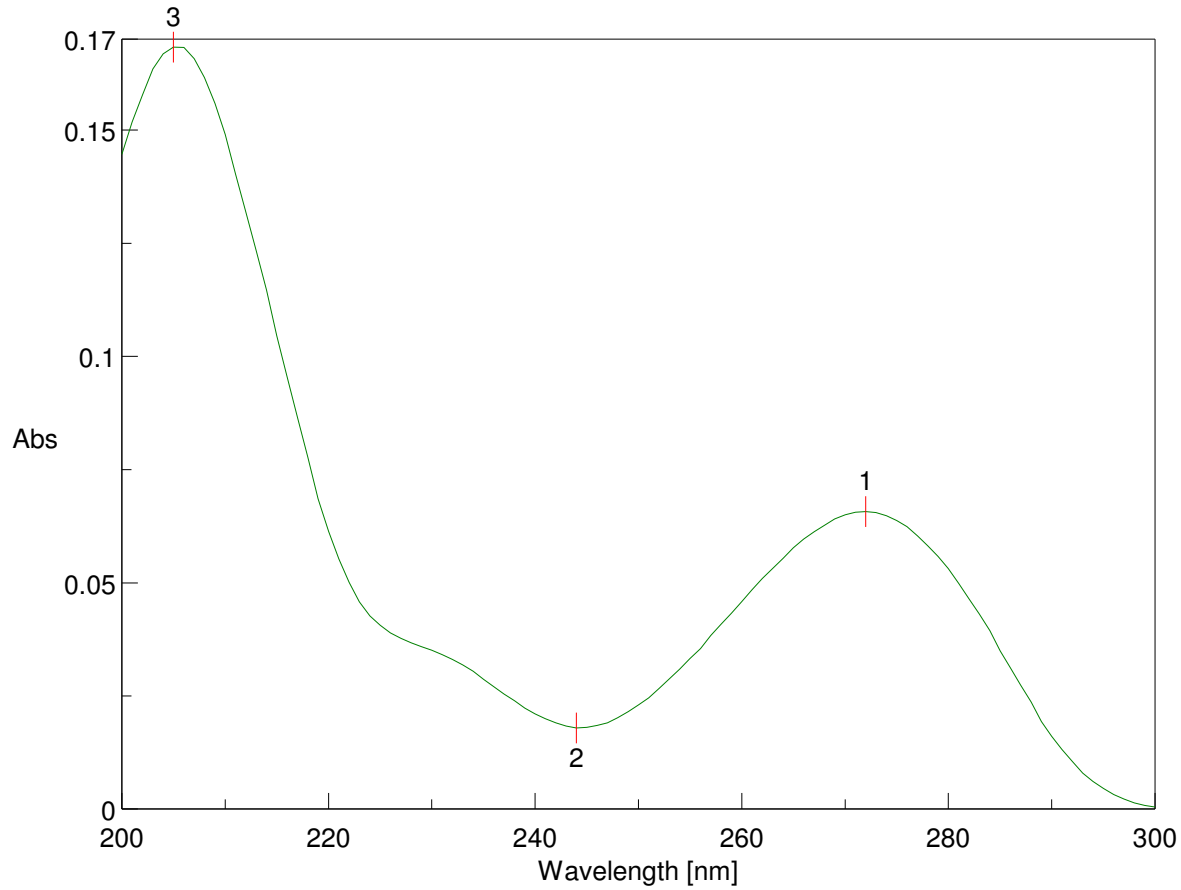

[Comments]

User	Beatriz
Division	---
Company	JP
Creation date	19/08/2021 16:43

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2018
Model Name	MD-2018
Serial No.	A023761331
ROM version	V1.05.01

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.065644	2	244	0.017864
3	205	0.168259			

Peak Find - EDUV-UV-4070

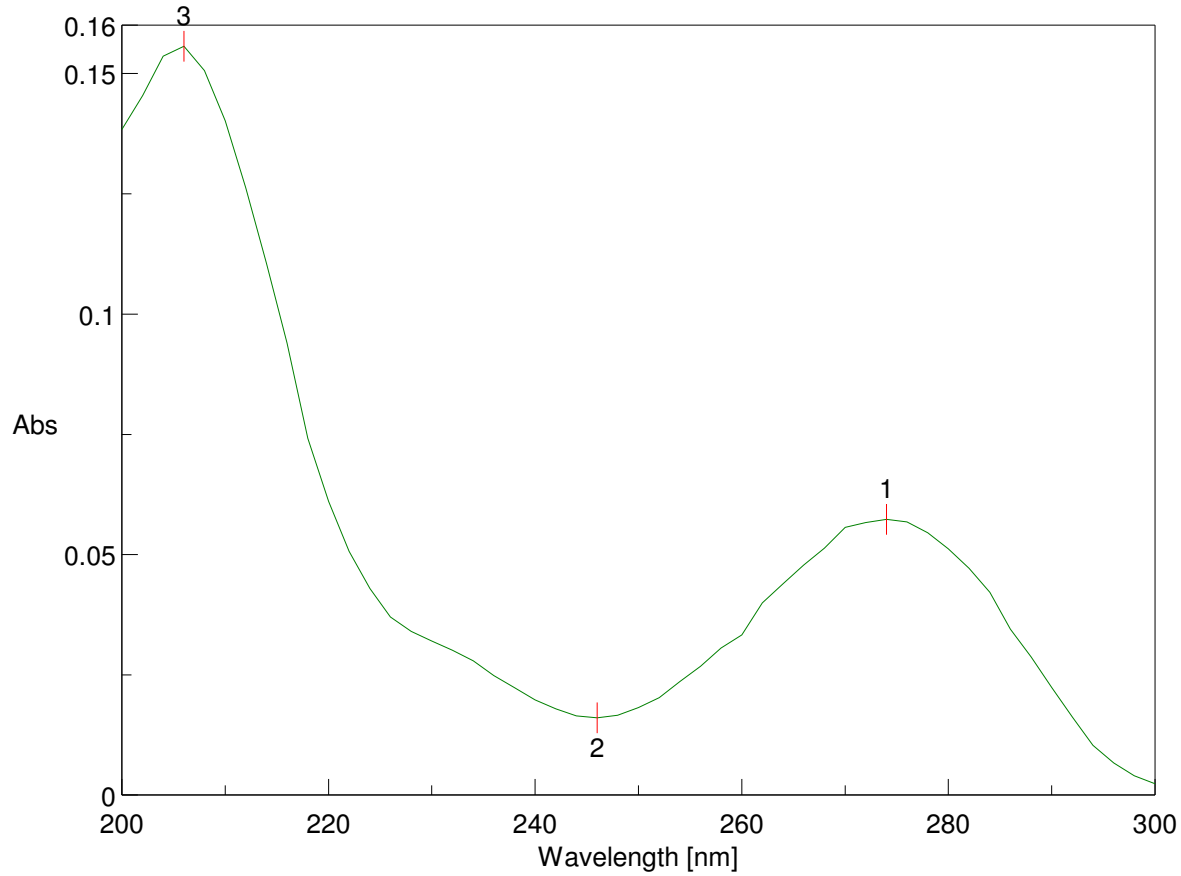

[Comments]

User	Beatriz
Division	---
Company	JP
Creation date	19/08/2021 16:49

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	900 nm
Data interval	2 nm
Data points	351


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	A010760888
ROM version	1.00.18

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0572895	2	246	0.0160589
3	206	0.155578			

Chromatogram

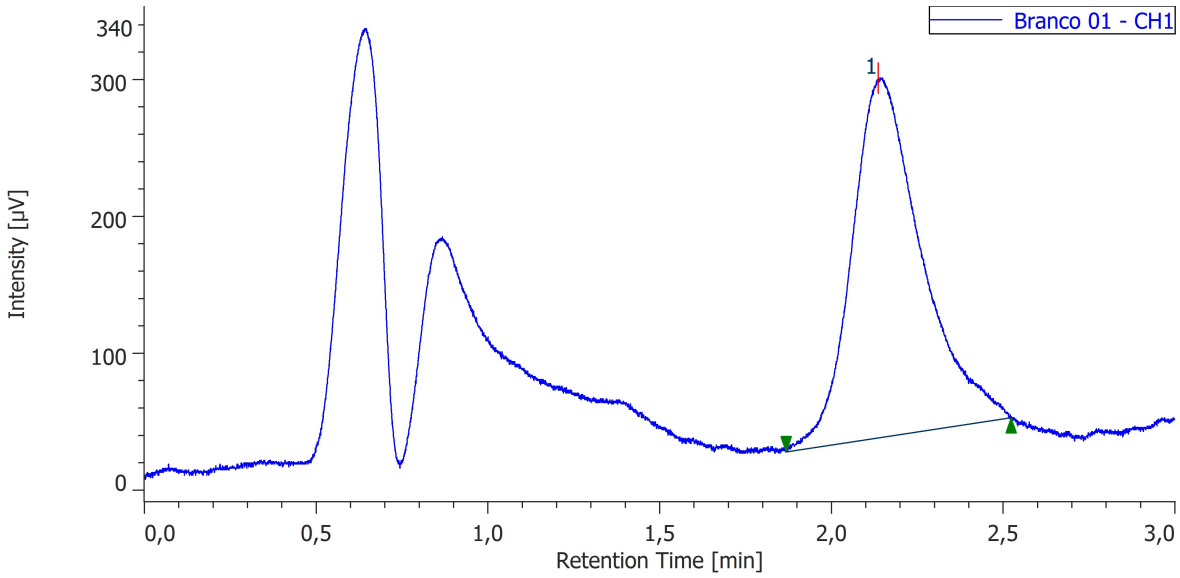


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:43:30
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:01:26
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,135	3696	263	100,000	100,000	N/A	589	N/A	1,371	

Chromatogram

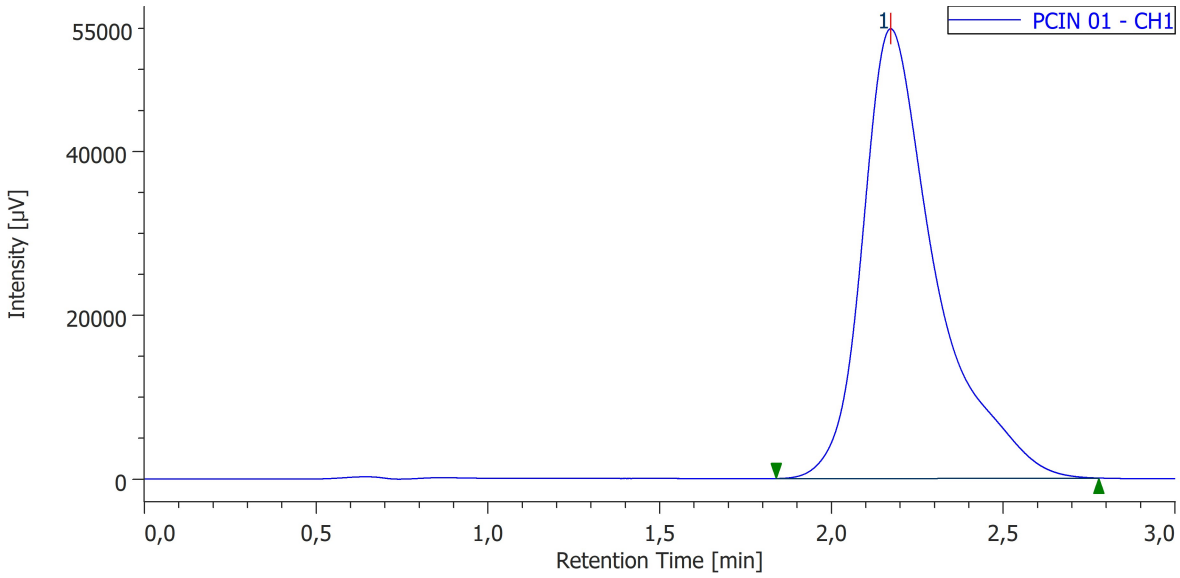


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:07:42
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:04:38
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,172	814769	54868	100,000	100,000	N/A	615	N/A	1,526	

Chromatogram

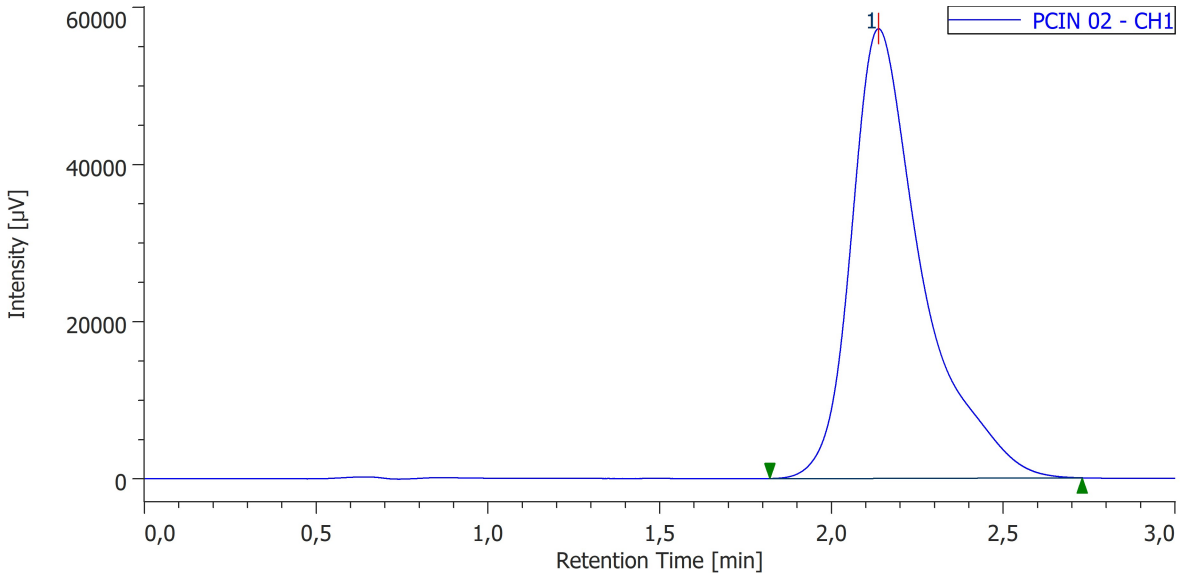


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:10:53
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:07:50
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,136	817631	57213	100,000	100,000	N/A	634	N/A	1,540	

Chromatogram

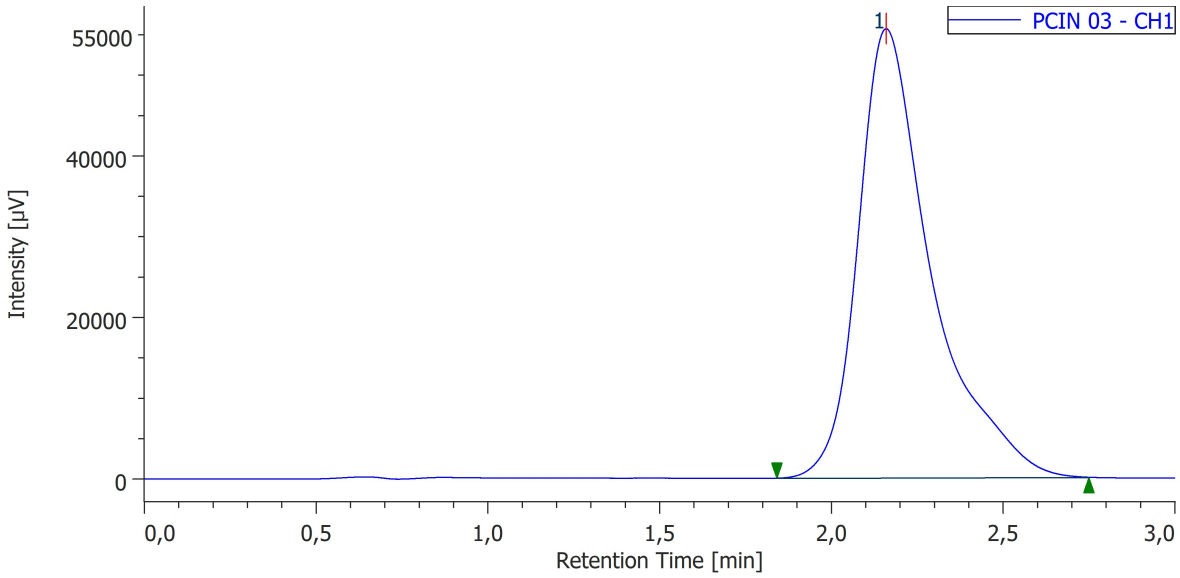


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:32:00
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:11:03
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,159	821510	55594	100,000	100,000	N/A	609	N/A	1,545	

Chromatogram

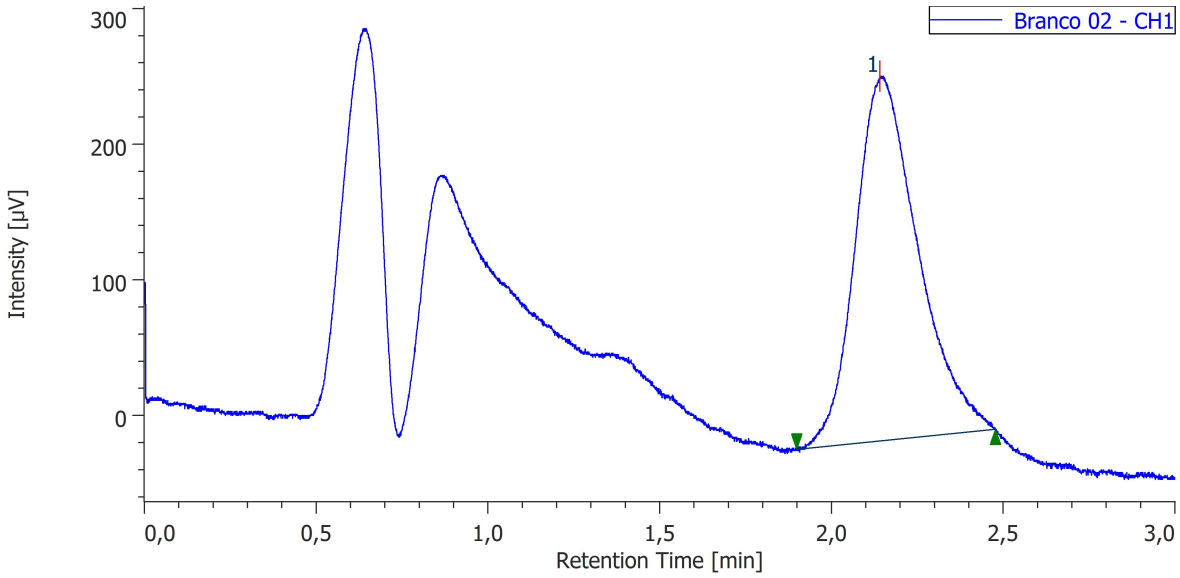


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:43:30
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:14:15
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,140	3397	269	100,000	100,000	N/A	693	N/A	1,337	

Chromatogram

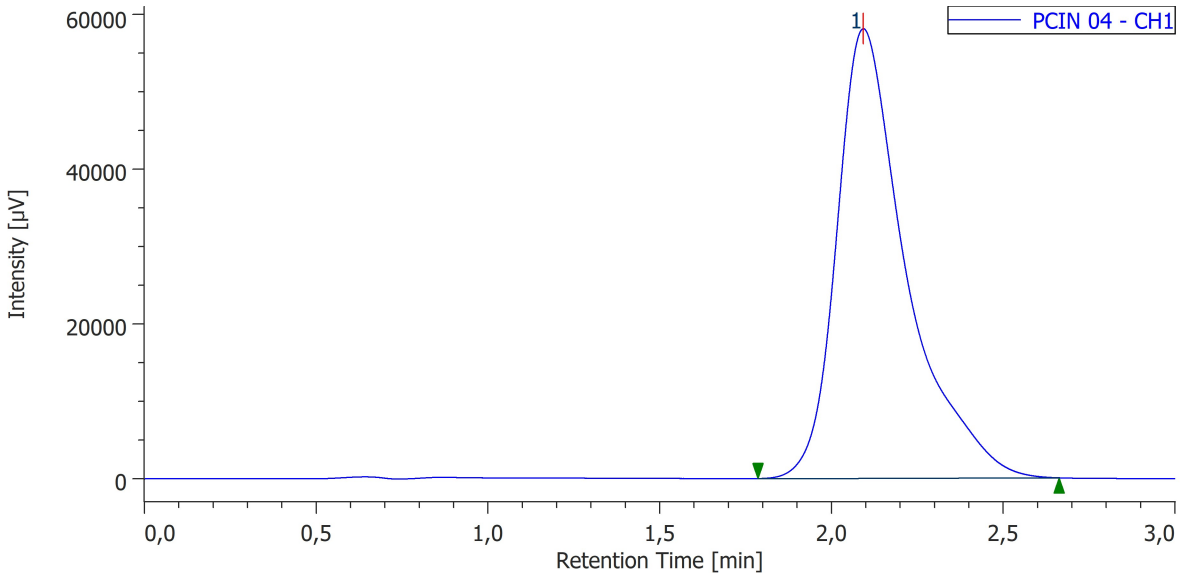


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:20:29
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:17:27
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,092	816519	58080	100,000	100,000	N/A	622	N/A	1,545	

Chromatogram

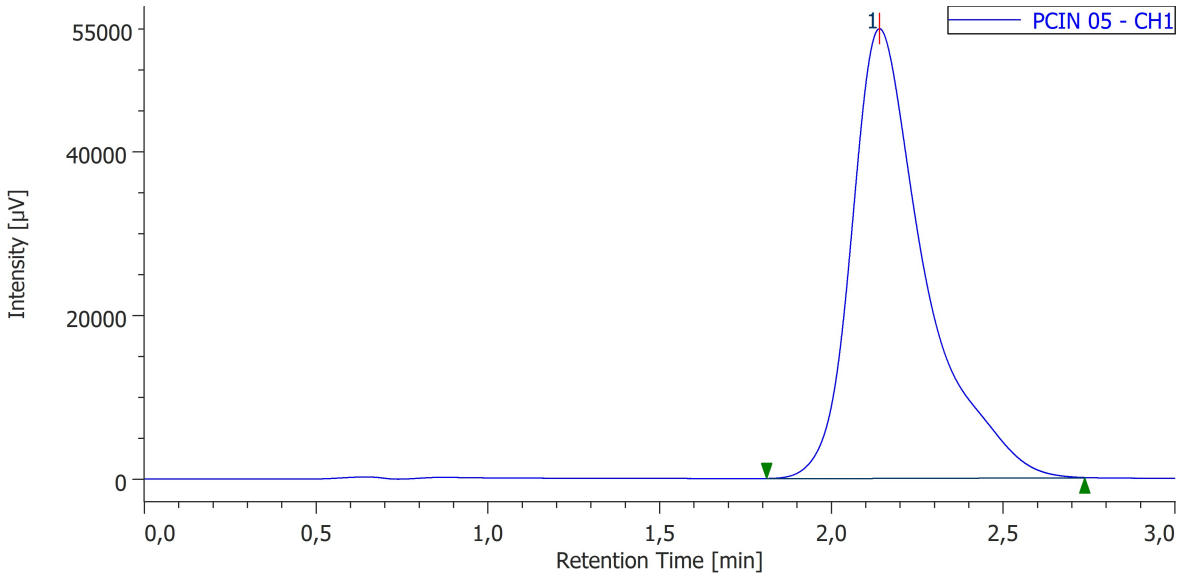


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:23:41
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:20:39
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,139	816845	54905	100,000	100,000	N/A	587	N/A	1,550	

Chromatogram

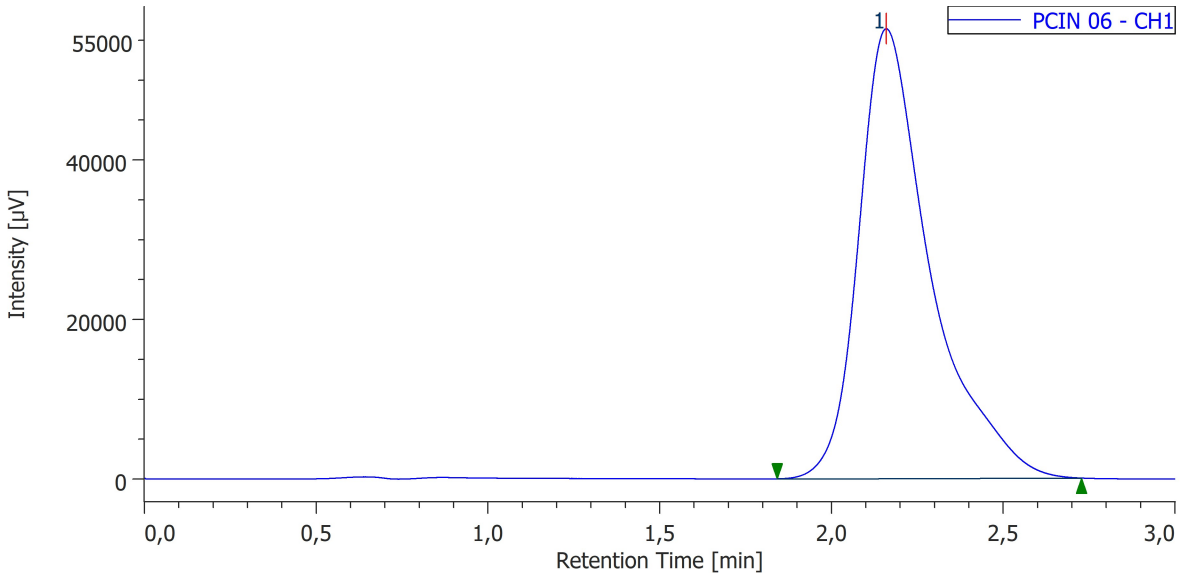


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:26:53
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:23:51
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,159	817273	56359	100,000	100,000	N/A	623	N/A	1,536	

Chromatogram

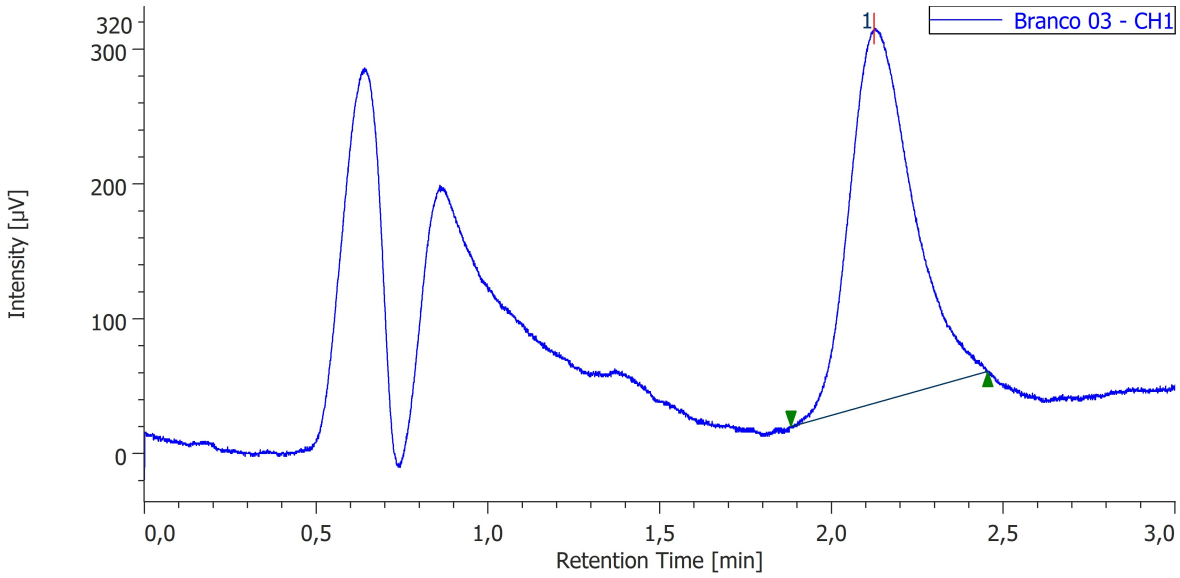


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:43:30
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:27:03
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,123	3534	278	100,000	100,000	N/A	684	N/A	1,389	

Chromatogram

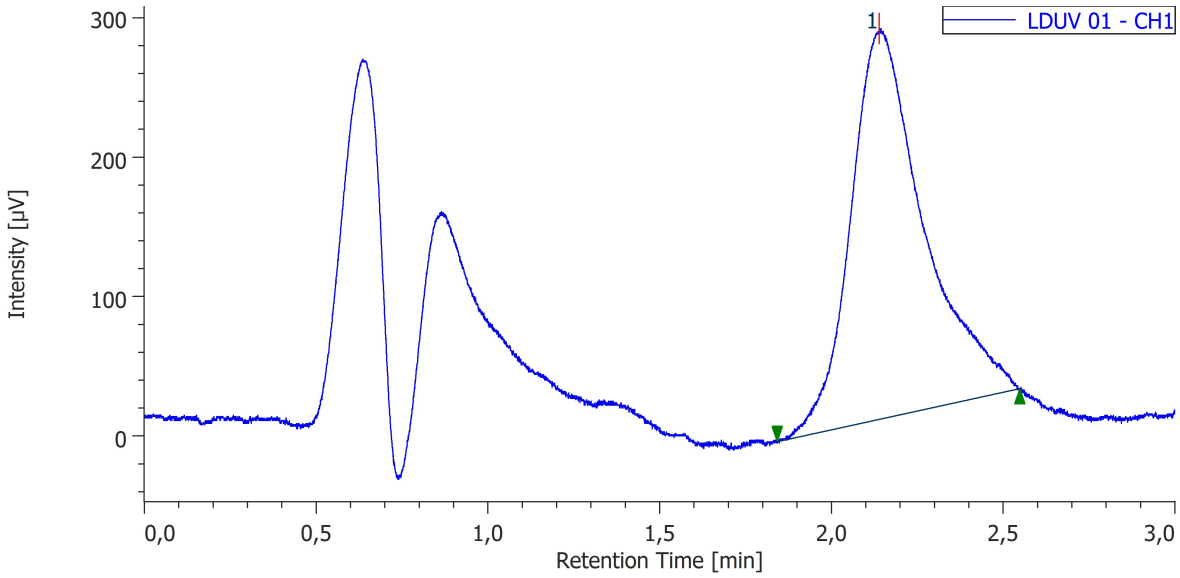


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:41:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:35:07
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,139	4117	280	100,000	100,000	N/A	586	N/A	1,386	

Chromatogram

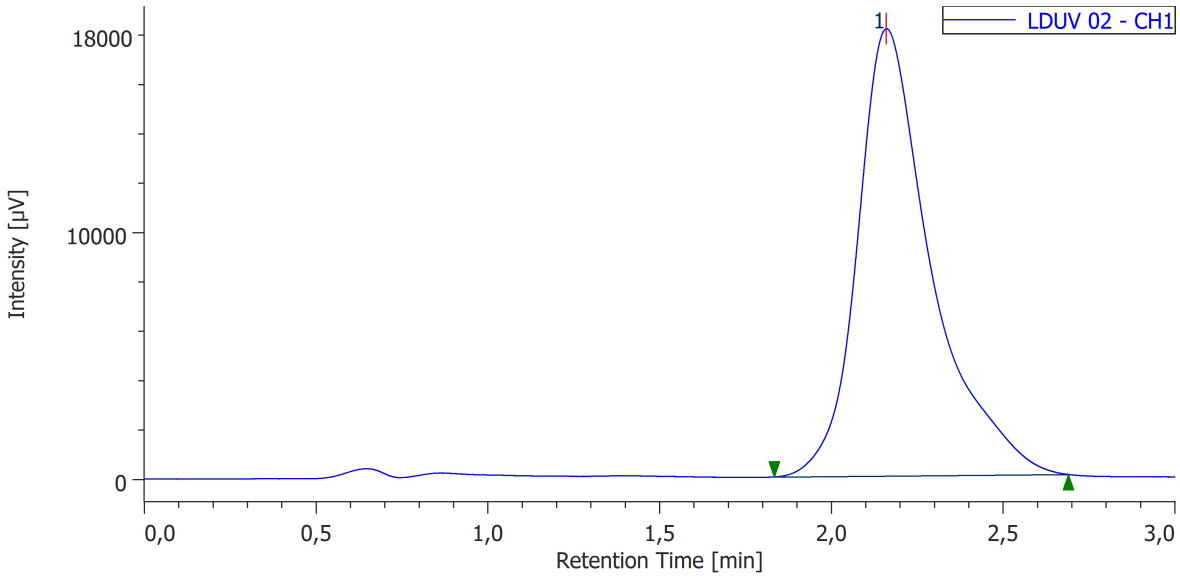


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:41:21
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:38:20
Volume	10,0 [µL]
Sample #	7
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,159	270906	18117	100,000	100,000	N/A	594	N/A	1,433	

Chromatogram

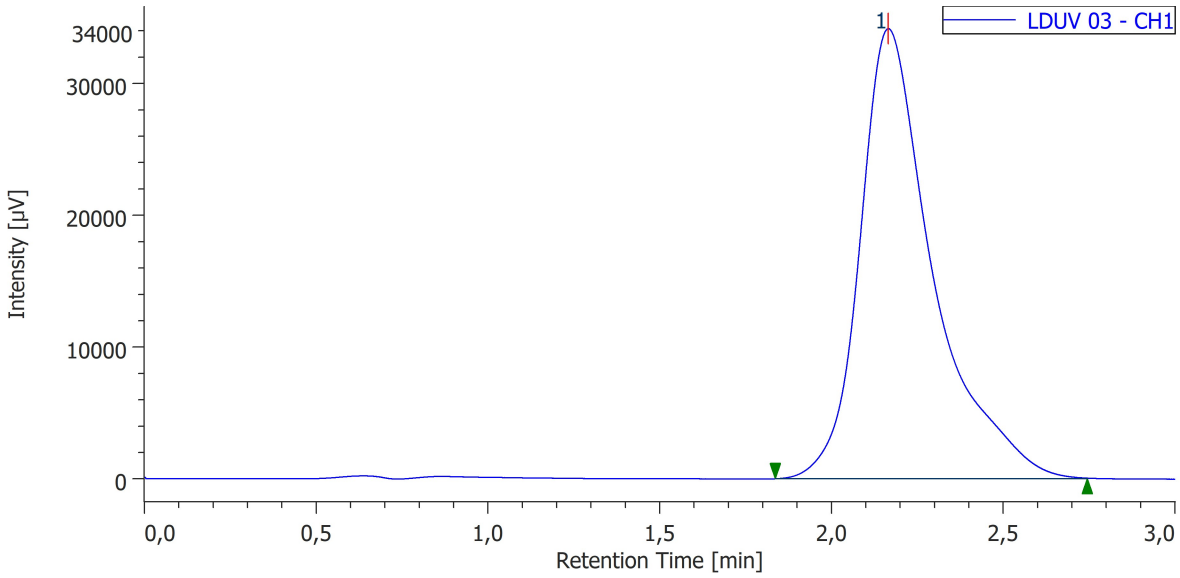


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:44:33
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:41:32
Volume	10,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,165	503481	34132	100,000	100,000	N/A	620	N/A	1,486	

Chromatogram

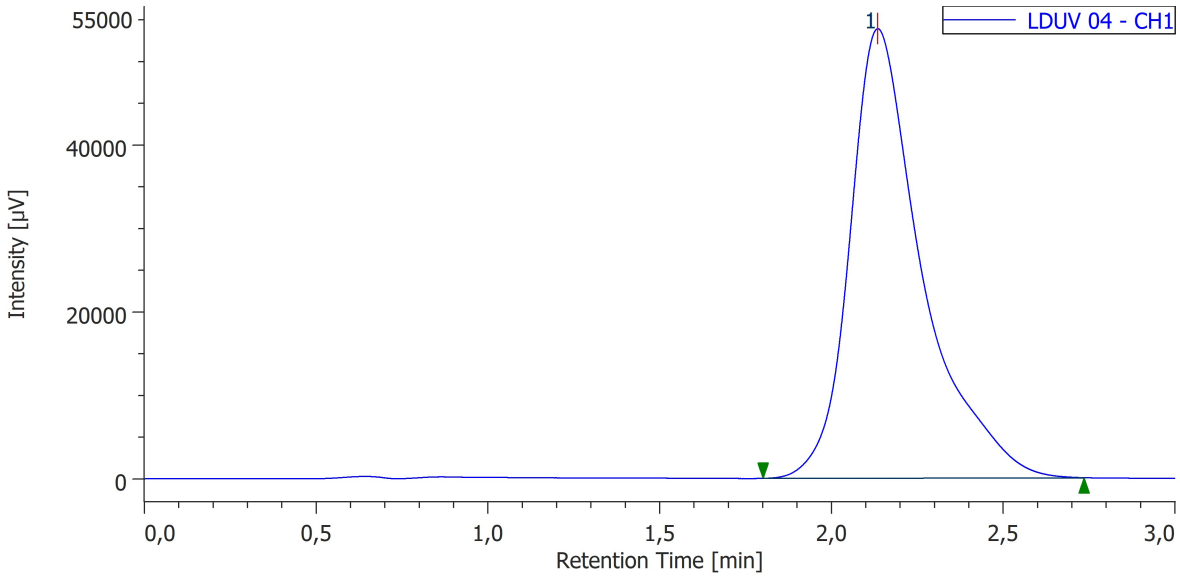


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:47:47
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:44:44
Volume	10,0 [µL]
Sample #	9
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,134	787611	53843	100,000	100,000	N/A	607	N/A	1,479	

Chromatogram

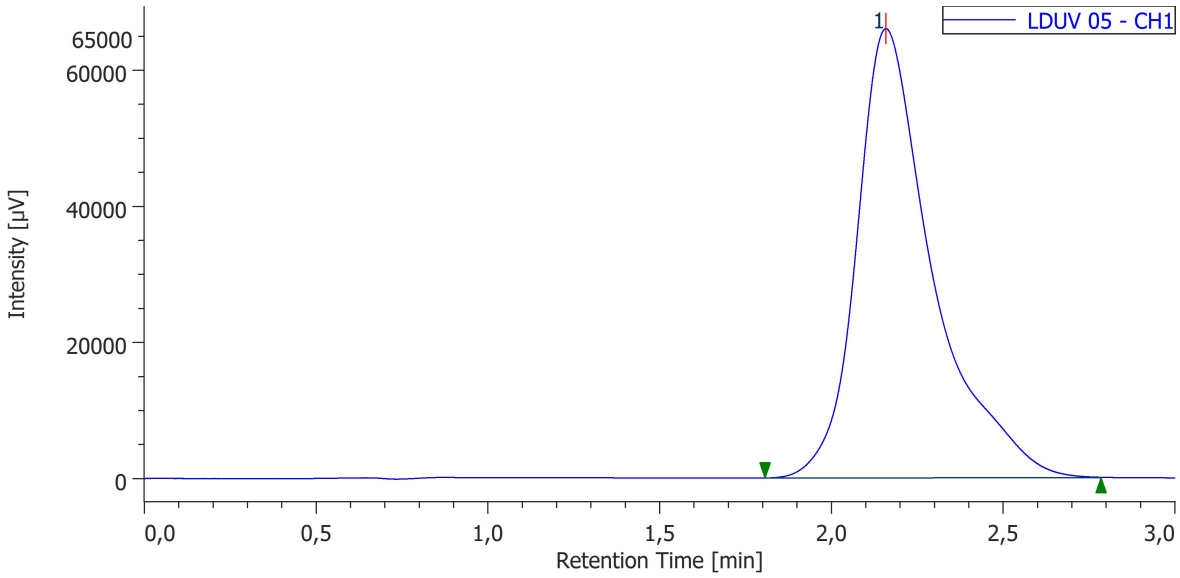


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 10:50:59
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:47:56
Volume	10,0 [µL]
Sample #	10
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,158	1013997	65973	100,000	100,000	N/A	571	N/A	1,485	

Chromatogram

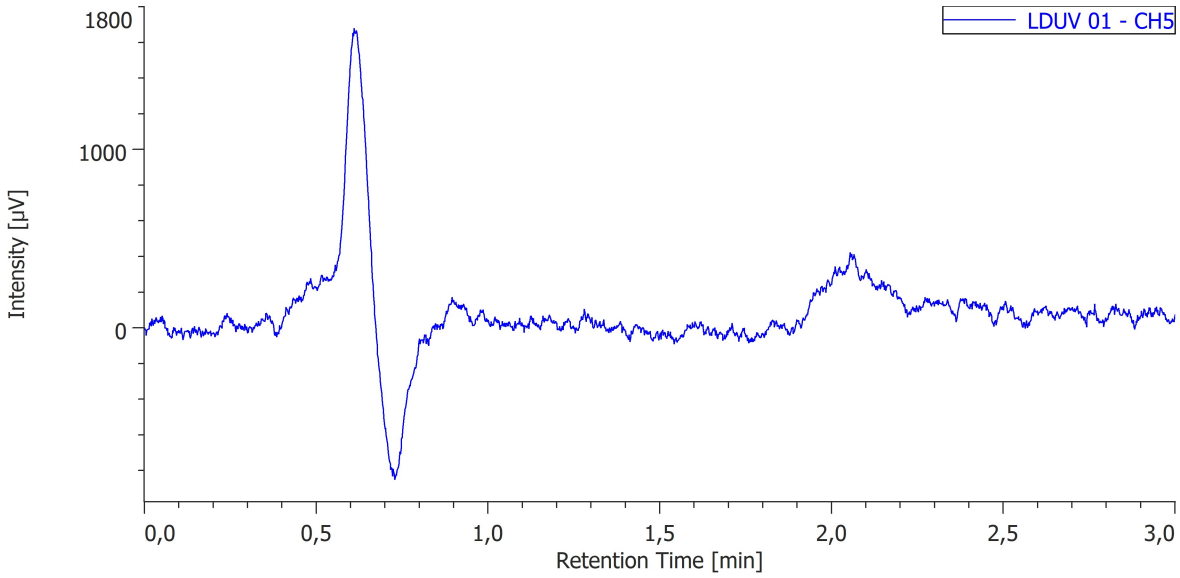


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:58:13
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:29:42
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Int_Cafeína

Chromatogram

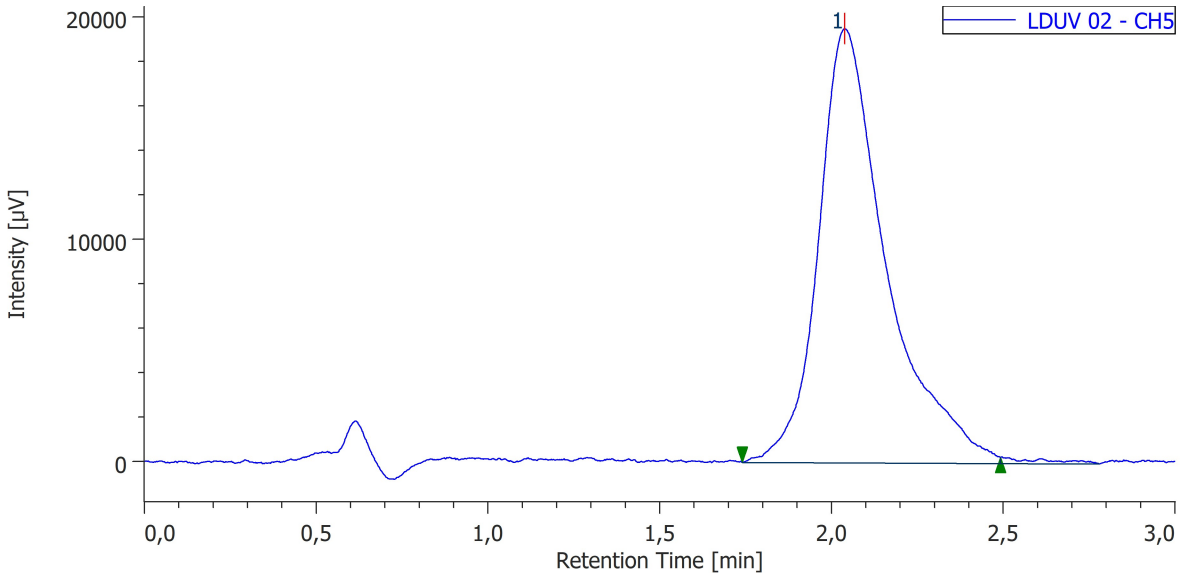


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:58:13
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:32:54
Volume	10,0 [µL]
Sample #	7
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,038	268087	19523	100,000	100,000	N/A	653	N/A	1,446	

Chromatogram

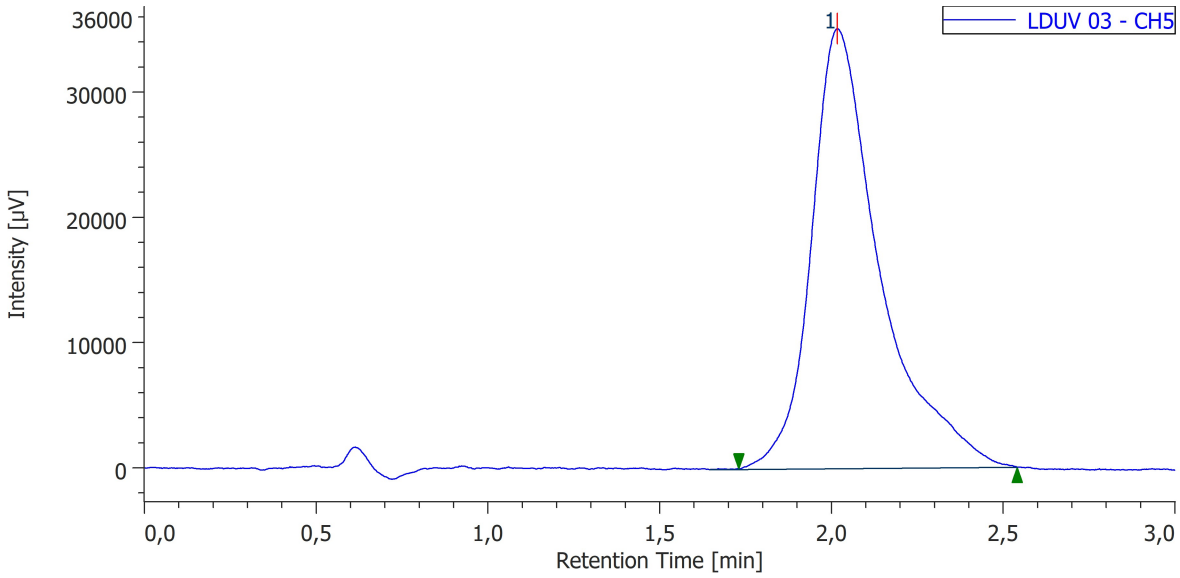


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:58:13
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:36:06
Volume	10,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,017	486954	35110	100,000	100,000	N/A	631	N/A	1,520	

Chromatogram

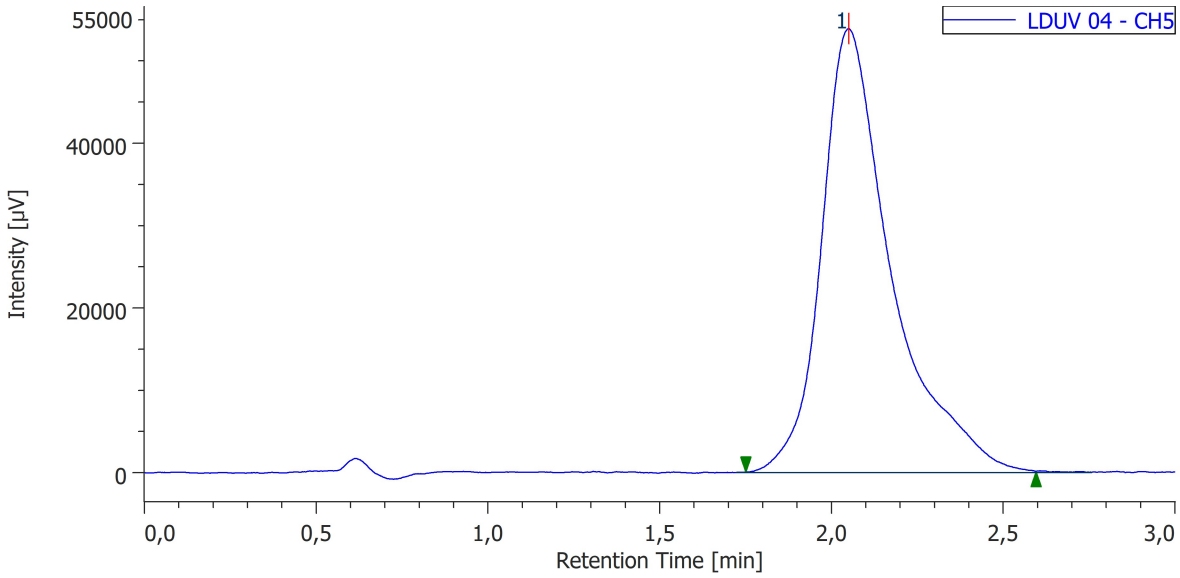


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:58:13
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:39:18
Volume	10,0 [µL]
Sample #	9
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,050	762457	53861	100,000	100,000	N/A	624	N/A	1,482	

Chromatogram

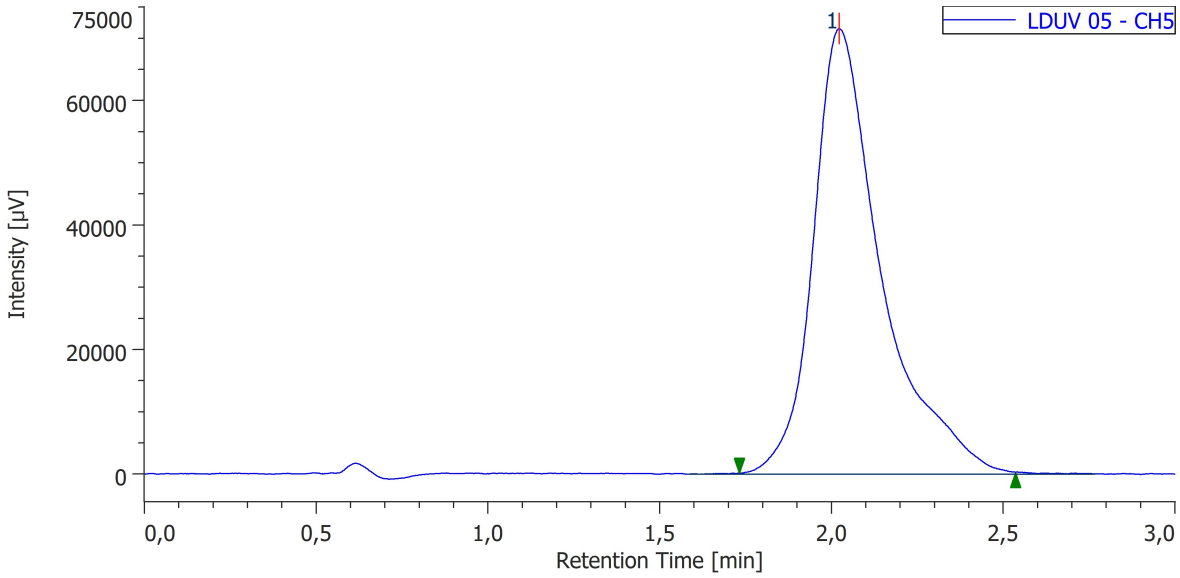


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:58:13
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:42:31
Volume	10,0 [µL]
Sample #	10
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	2,022	985827	71529	100,000	100,000	N/A	638	N/A	1,505	

Chromatogram

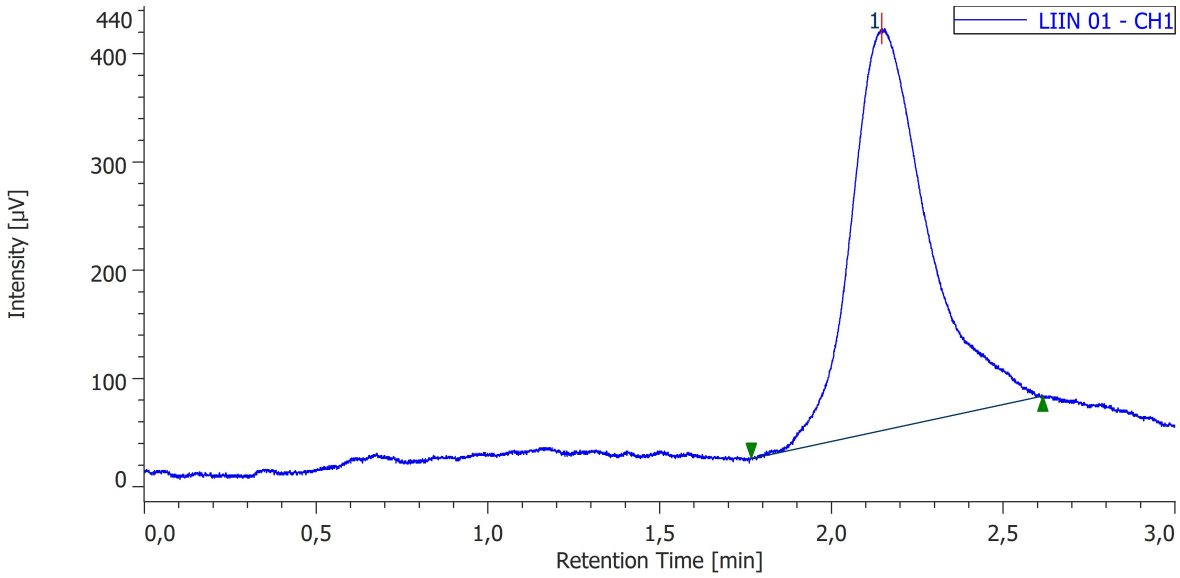


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:44:49
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:56:16
Volume	0,1 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,146	5739	371	100,000	100,000	N/A	529	N/A	1,336	

Chromatogram

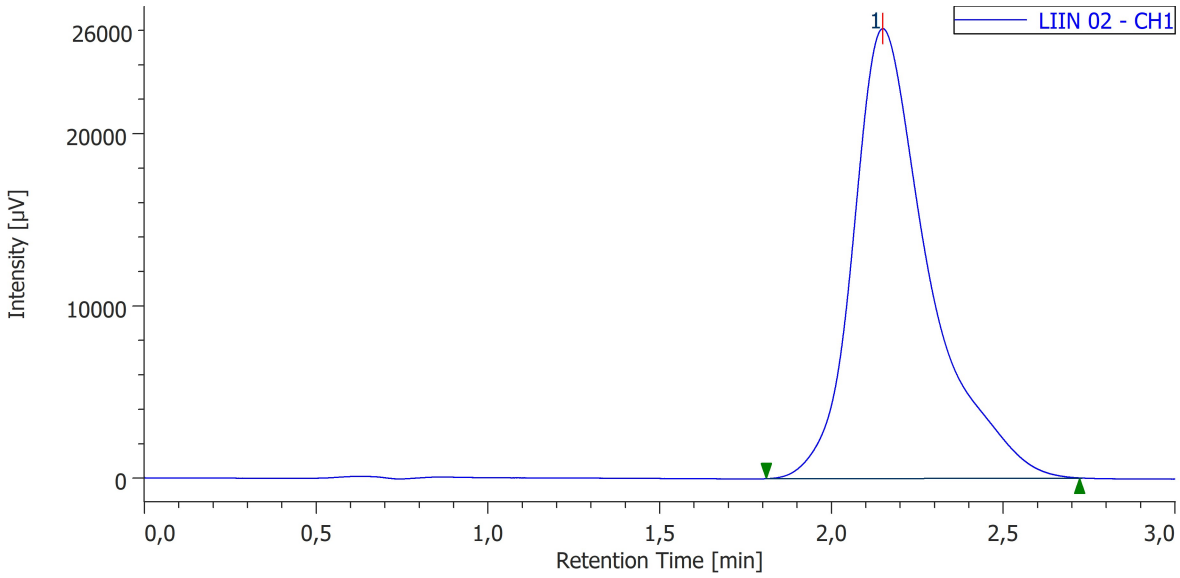


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:42:08
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 10:59:28
Volume	5,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,149	400001	26106	100,000	100,000	N/A	560	N/A	1,429	

Chromatogram

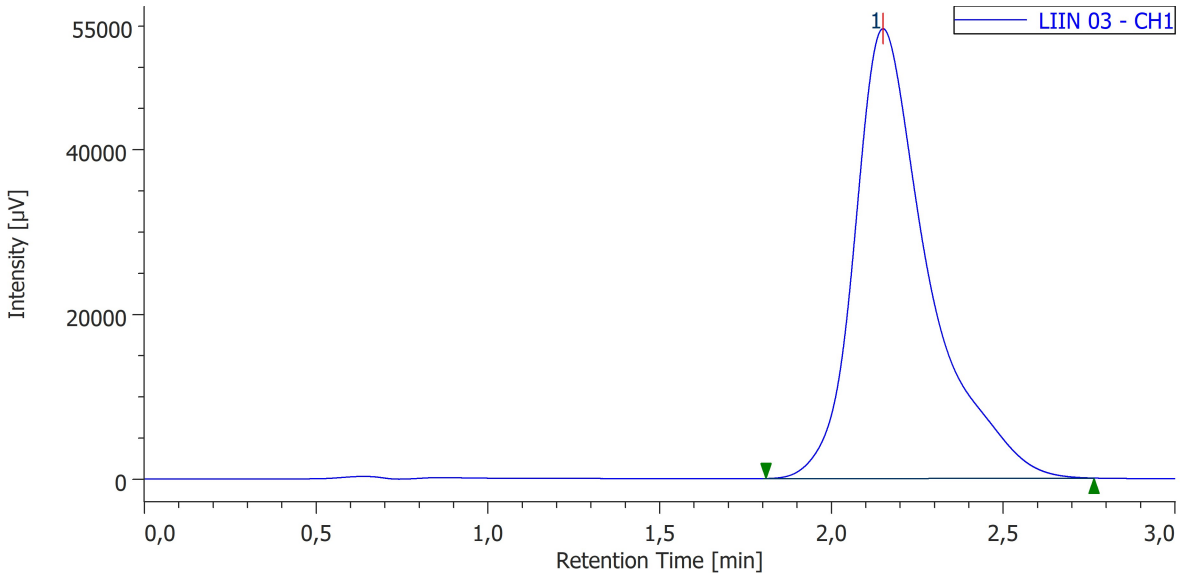


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:42:08
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:12:46
Volume	10,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,150	817745	54568	100,000	100,000	N/A	593	N/A	1,474	

Chromatogram

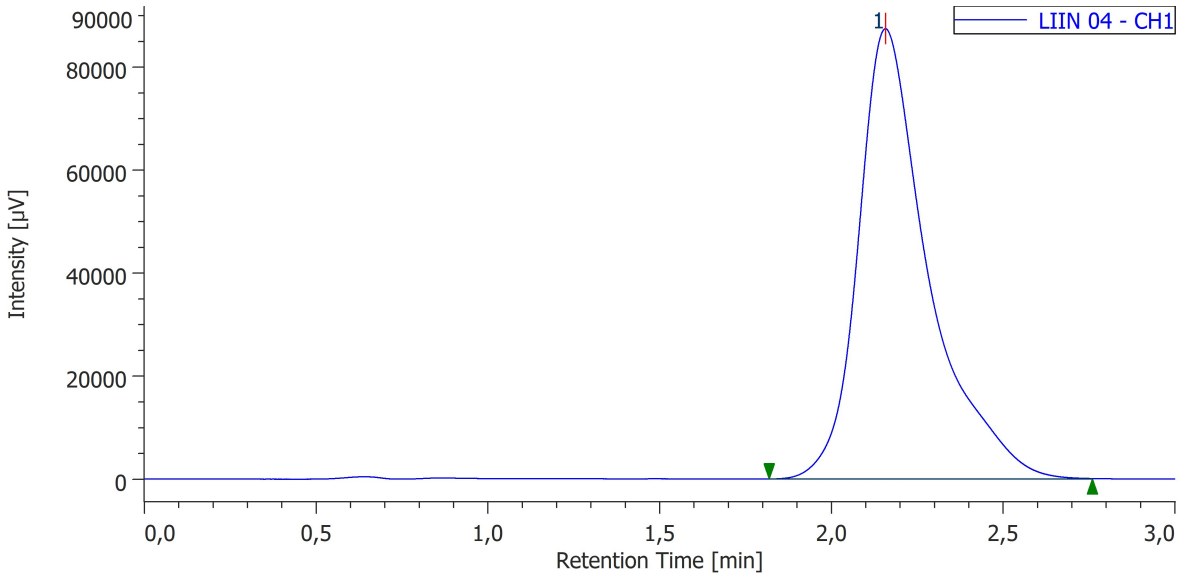

Chromatogram Information


User Name	Beatriz
Date Modified	20/08/2021 11:42:09
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:15:58
Volume	15,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,157	1237884	87392	100,000	100,000	N/A	669	N/A	1,476	

Chromatogram

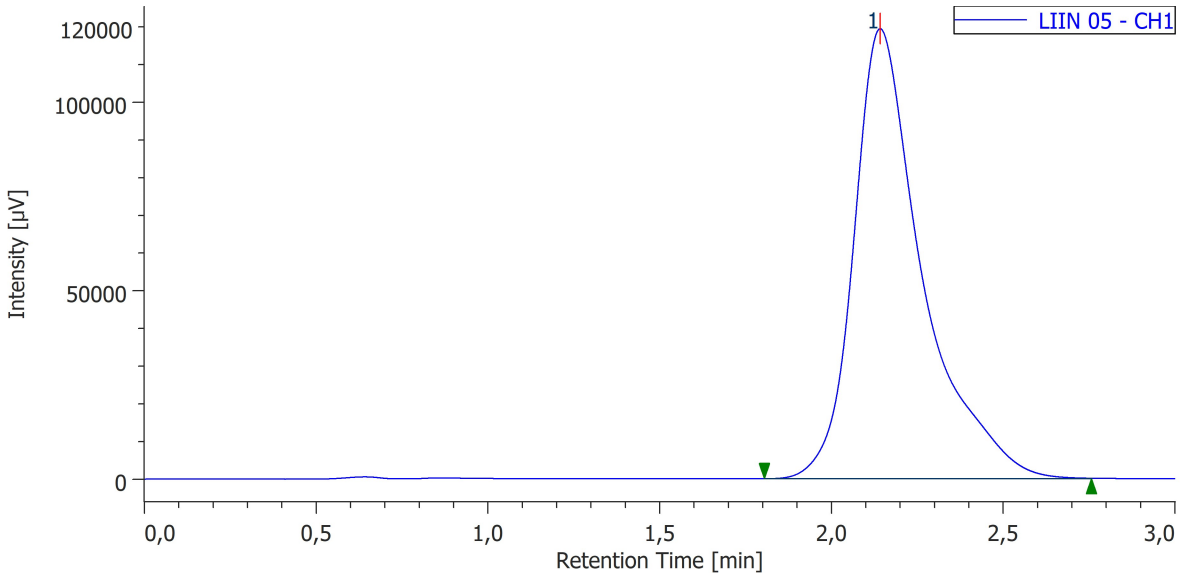


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 11:42:09
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 11:19:10
Volume	20,0 [µL]
Sample #	20
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	Int_Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	2,141	1653696	119341	100,000	100,000	N/A	695	N/A	1,503	

Chromatogram

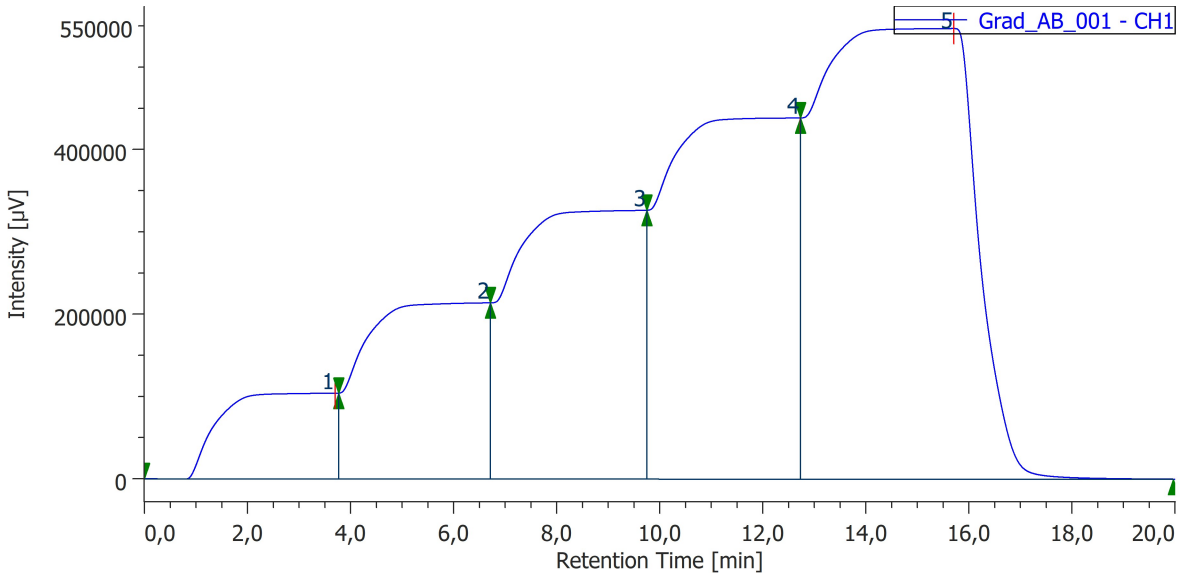


Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 12:51:44
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 12:12:22
Volume	0,0 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad_AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,700	15260699	103857	5,213	6,375	N/A	N/A	N/A	N/A	
2	40%	1	6,710	34162504	213733	11,670	13,120	N/A	N/A	N/A	N/A	
3	60%	1	9,747	55399705	326150	18,925	20,021	N/A	N/A	N/A	N/A	
4	80%	1	12,725	74685550	438356	25,513	26,909	N/A	N/A	N/A	N/A	
5	100%	1	15,705	113230787	546942	38,680	33,575	N/A	N/A	N/A	N/A	

Chromatogram

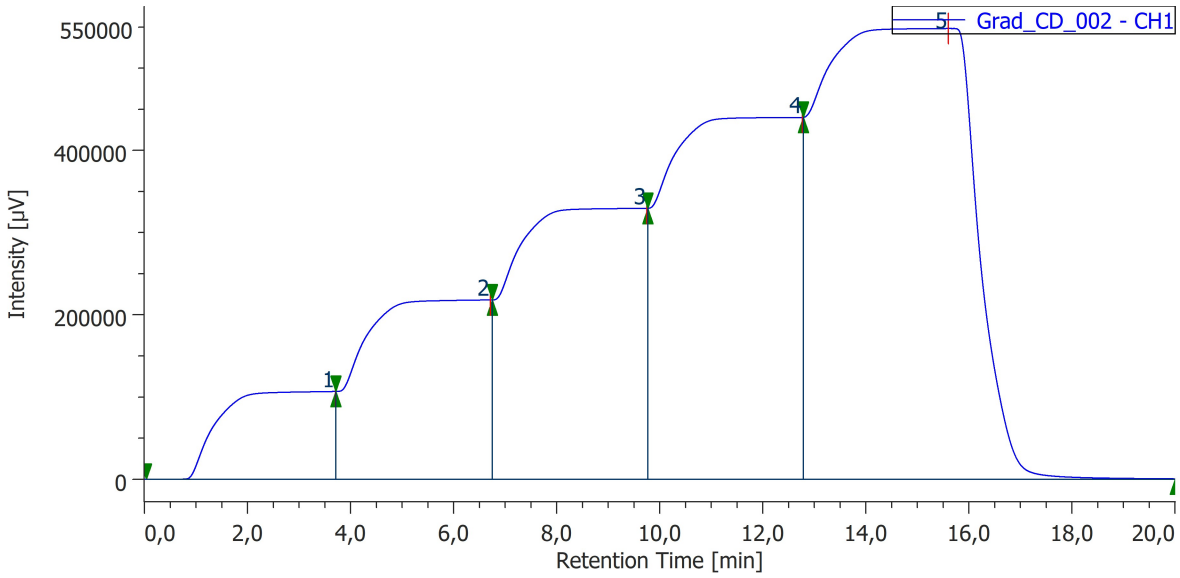

Chromatogram Information	
User Name	Beatriz
Date Modified	20/08/2021 13:08:25
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	20/08/2021 12:48:24
Volume	0,0 [µL]
Sample #	-
Project Name	JASCO
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad_CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	20 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,710	15222643	106509	5,160	6,495	N/A	N/A	N/A	N/A	
2	40%	1	6,710	35757968	217654	12,120	13,273	N/A	N/A	N/A	N/A	
3	60%	1	9,747	55954590	328882	18,966	20,056	N/A	N/A	N/A	N/A	
4	80%	1	12,765	76116754	439391	25,800	26,795	N/A	N/A	N/A	N/A	
5	100%	1	15,596	111975220	547404	37,954	33,382	N/A	N/A	N/A	N/A	