
Peak Find - EDUV UV-4070_002 UV_tR0,39 D

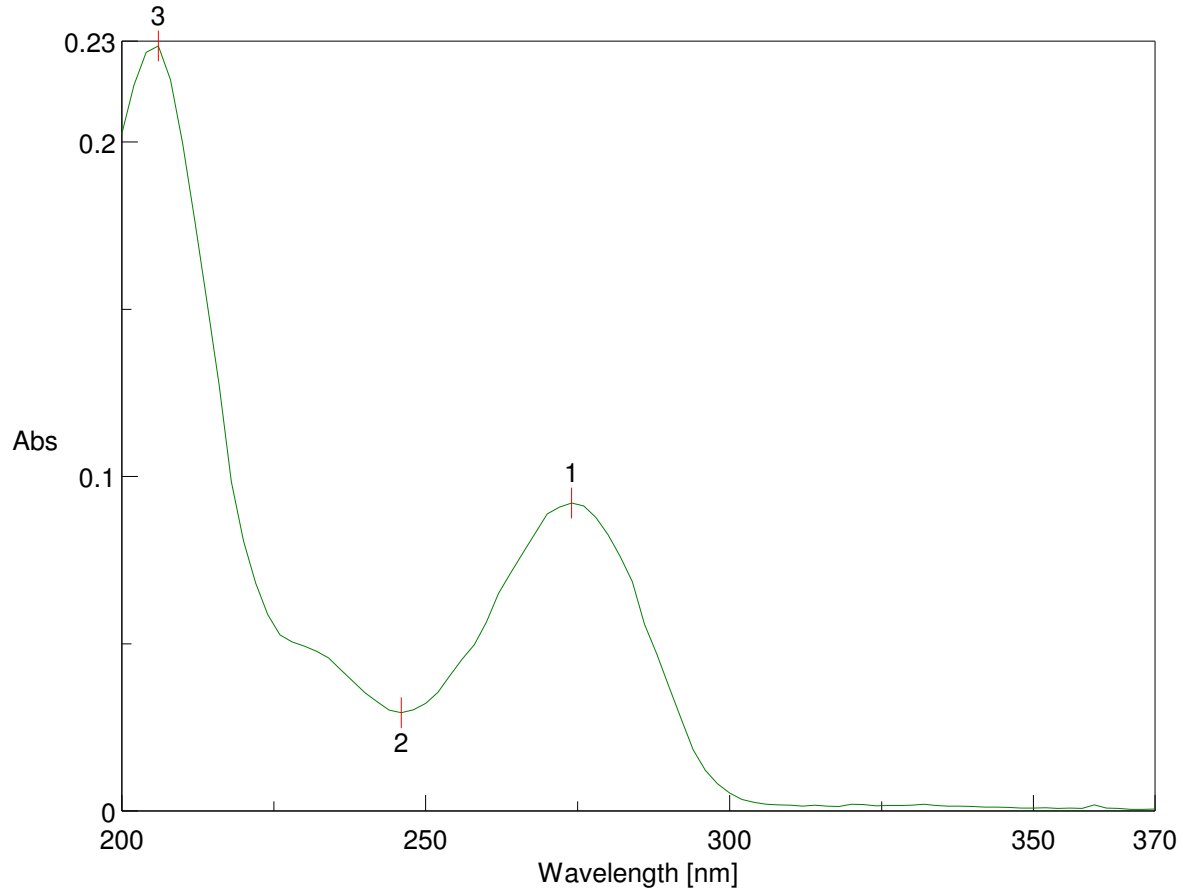

[Comments]

User	Giovana
Division	---
Company	JP
Creation date	27/08/2019 13:40

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	86


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	A010760888
ROM version	1.00.18

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.0919757	2	246	0.0293676
3	206	0.228519			

Peak Find - EDUV PDA_001 PDA_2,9533

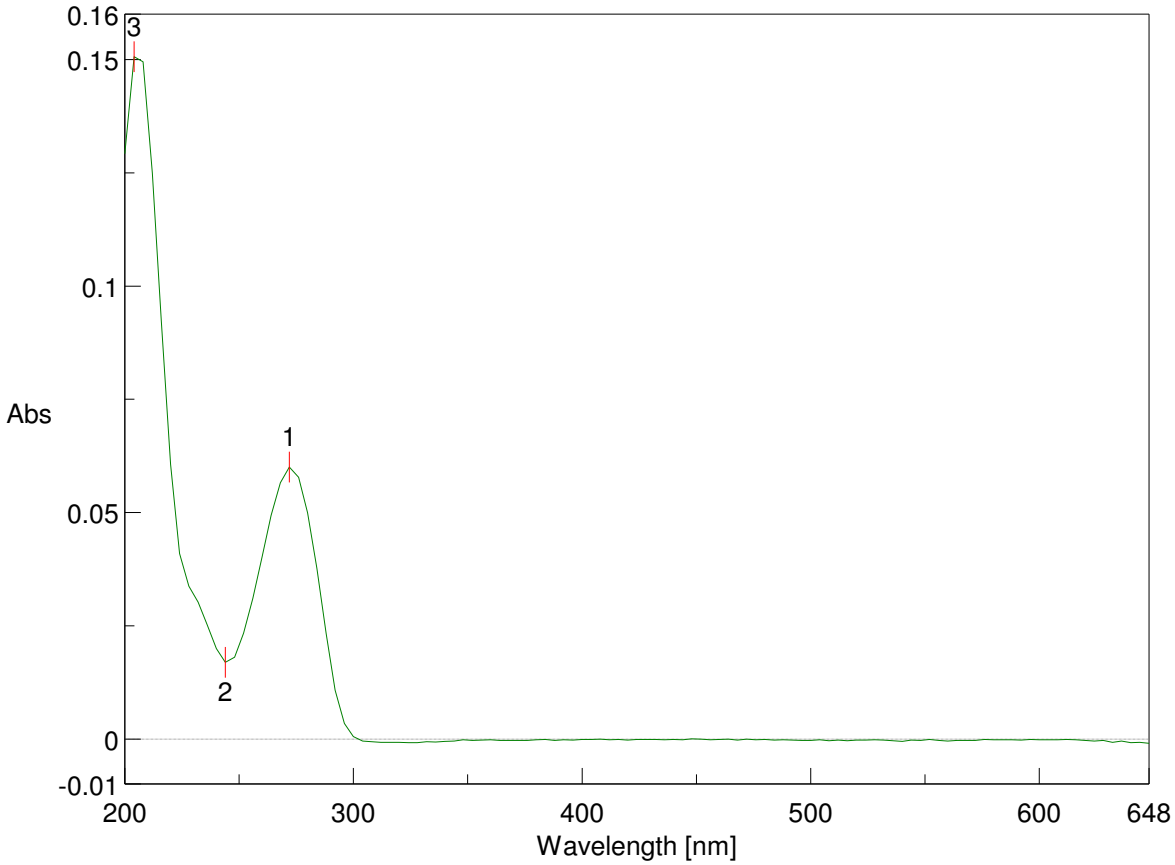

[Comments]

User	Giovana
Division	---
Company	JP
Creation date	27/08/2019 16:56

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113


[Measurement Information]

Instrument Name	MD-2018
Model Name	MD-2018
Serial No.	A023761331
ROM version	V1.05.01

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.059994	2	244	0.016888
3	204	0.150634			

Chromatogram

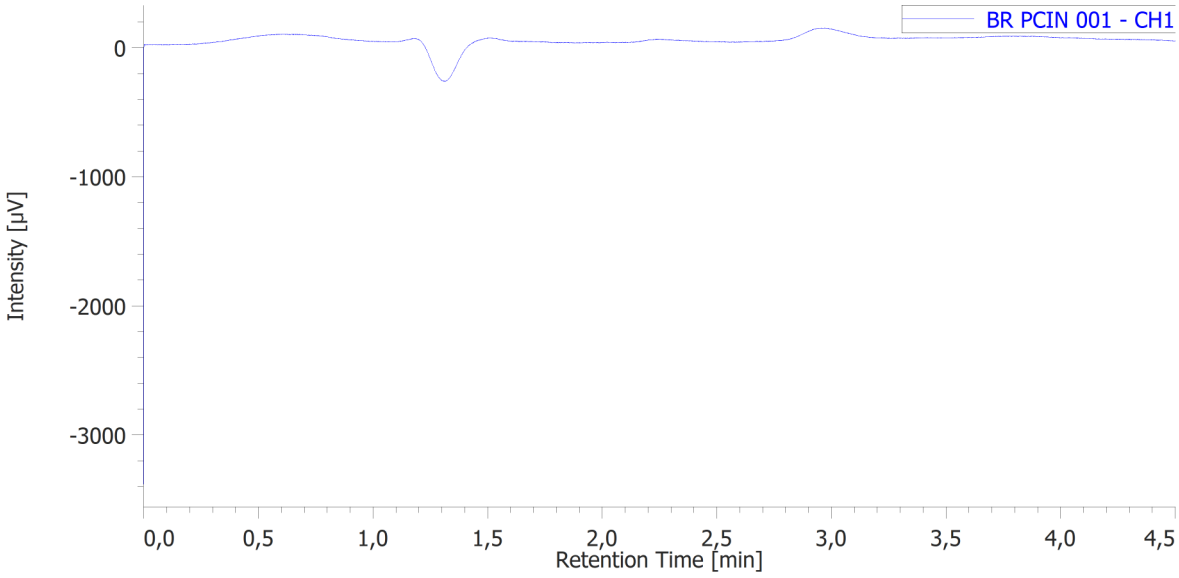


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 14:48:31
Volume	10.00 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

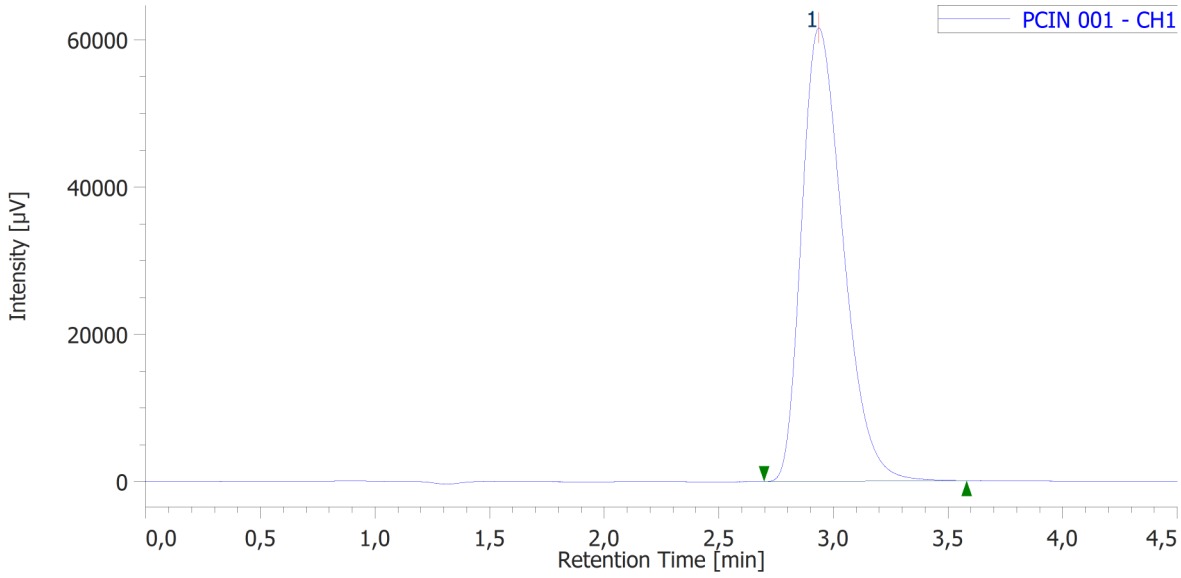


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 14:53:14
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.935	770970	61519	100.000	100.000	N/A	1269	N/A	1.361		N/A

Chromatogram

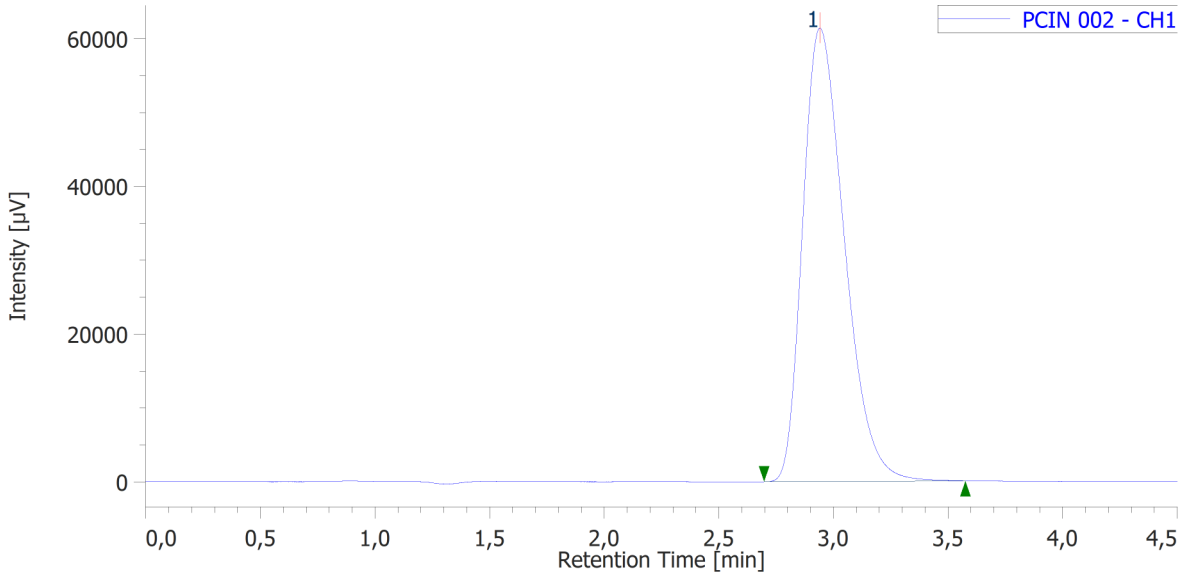


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 14:57:56
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.940	774987	61363	100.000	100.000	N/A	1254	N/A	1.368		N/A

Chromatogram

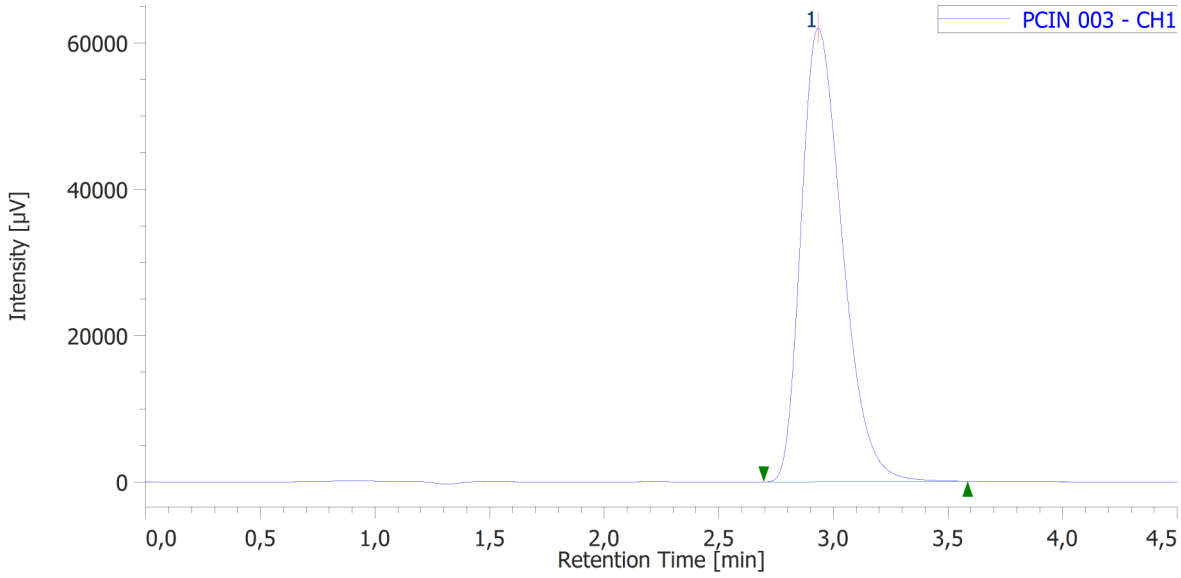

Chromatogram Information


User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:02:38
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.933	772855	61997	100.000	100.000	N/A	1283	N/A	1.360		N/A

Chromatogram

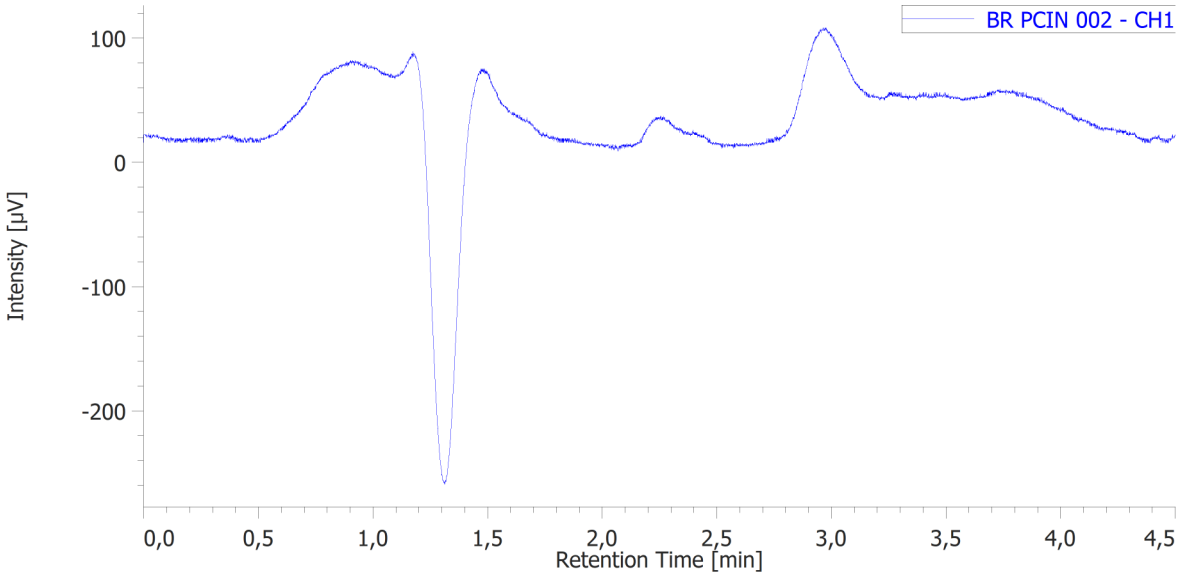


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:07:20
Volume	10.00 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

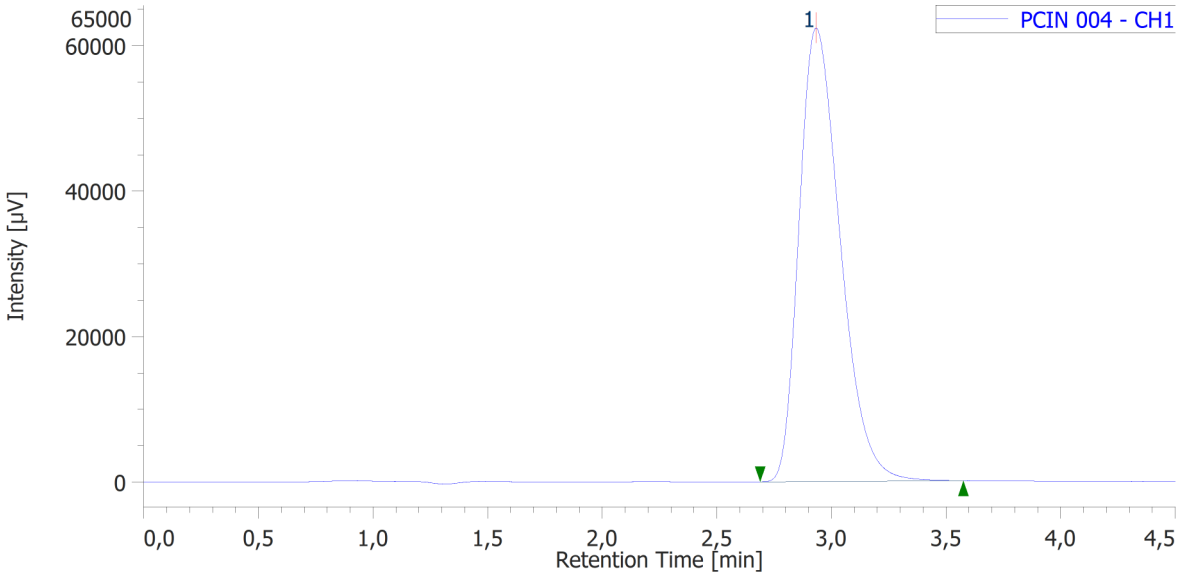


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:30
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:12:02
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.932	777498	62312	100.000	100.000	N/A	1281	N/A	1.365		N/A

Chromatogram

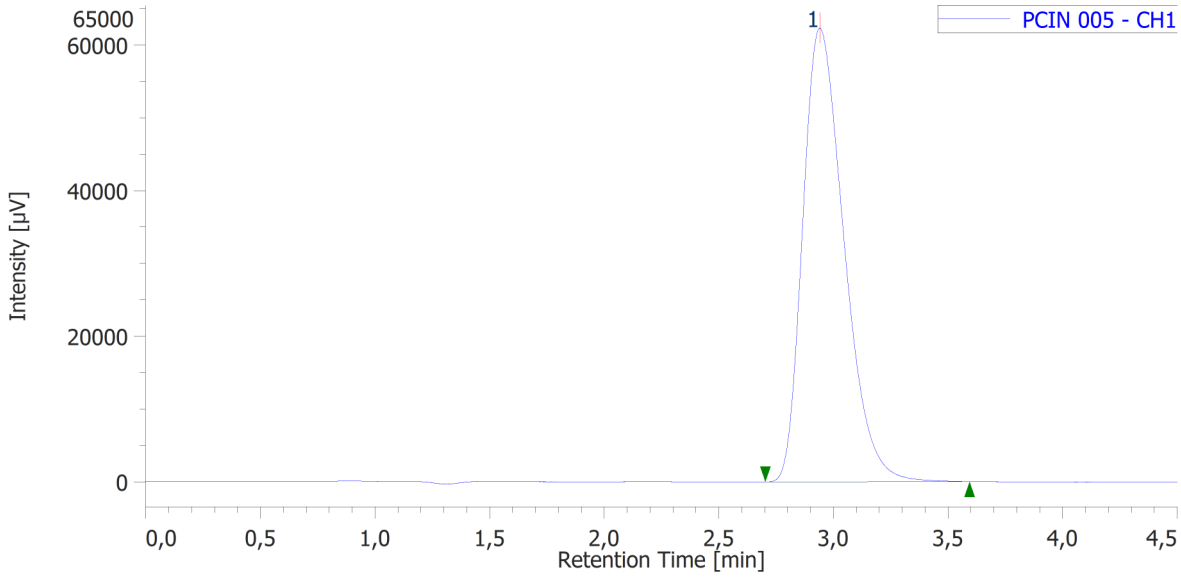

Chromatogram Information


User Name	Giovana
Date Modified	27/08/2019 15:26:31
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:16:44
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.939	778885	62321	100.000	100.000	N/A	1283	N/A	1.365		N/A

Chromatogram

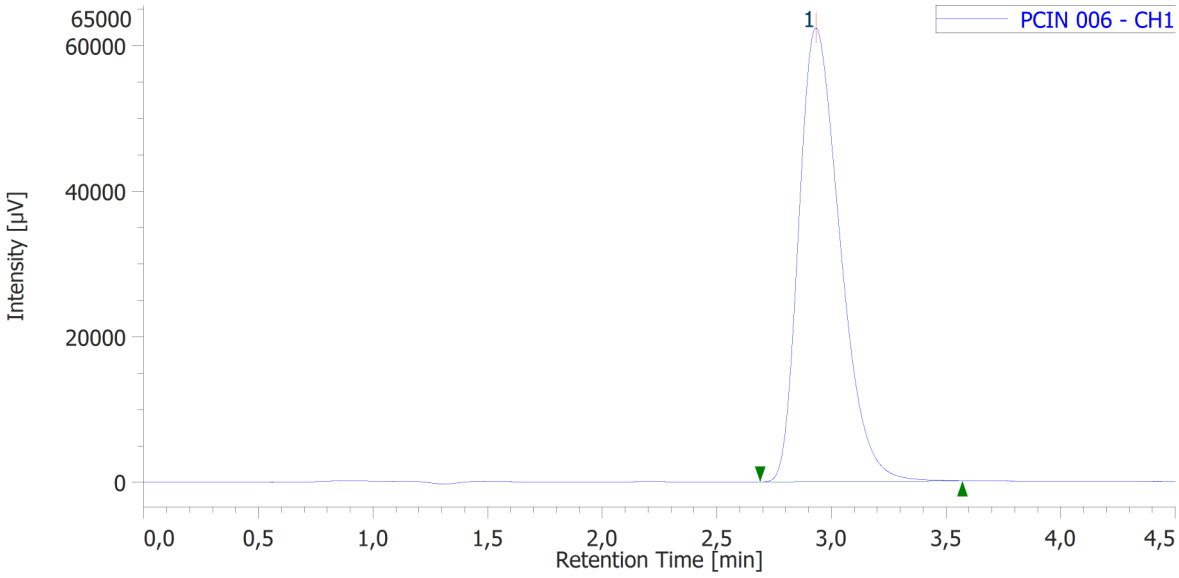


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:26:31
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:21:26
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.931	777917	62322	100.000	100.000	N/A	1278	N/A	1.363		N/A

Chromatogram

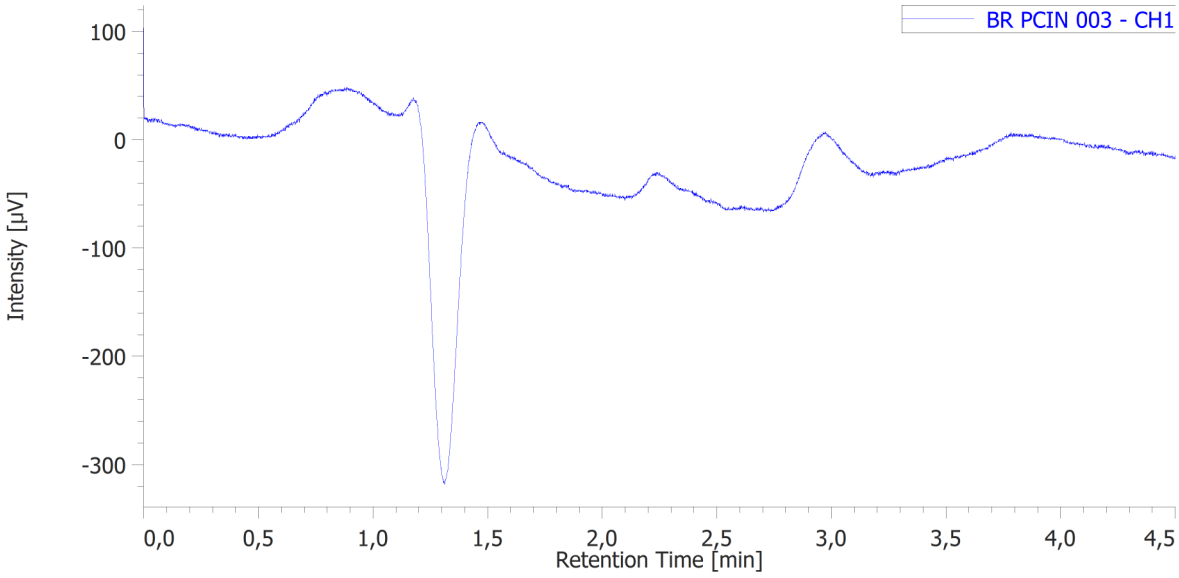


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:30:40
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:26:09
Volume	10.00 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

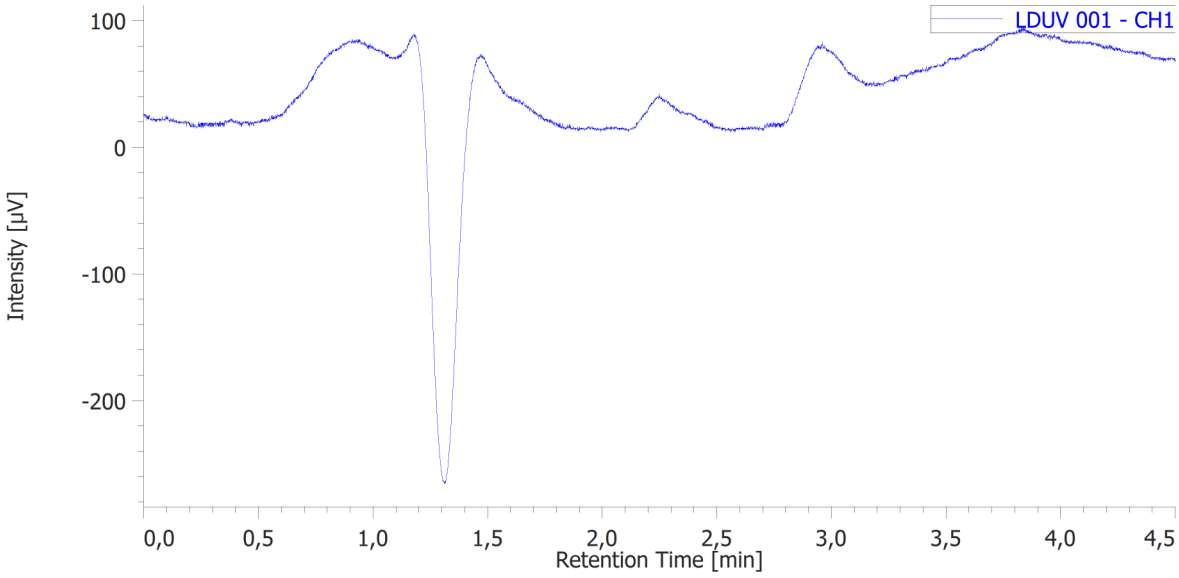


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:55:24
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:30:51
Volume	10.00 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

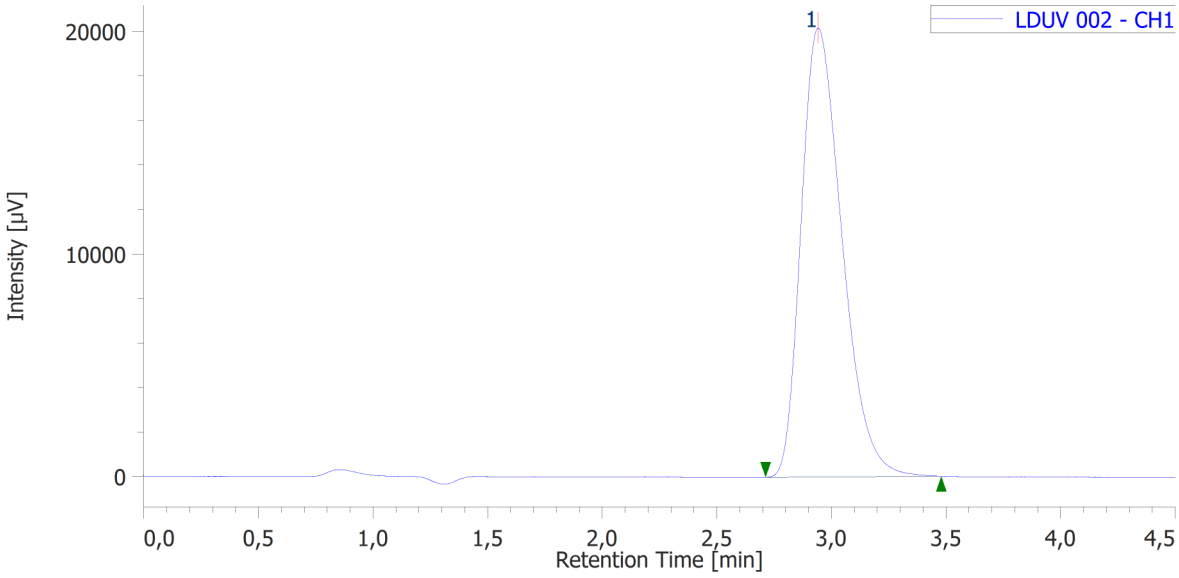


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:55:24
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:35:33
Volume	10.00 [µL]
Sample #	3
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.941	249752	20159	100.000	100.000	N/A	1307	N/A	1.352		N/A

Chromatogram

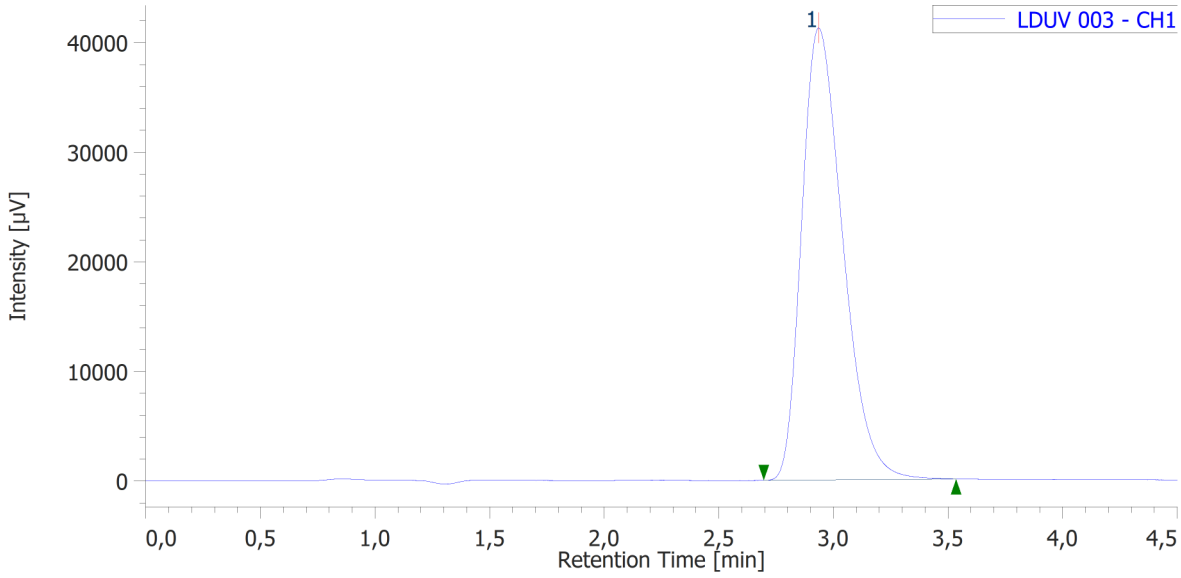


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:55:24
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:40:15
Volume	10.00 [µL]
Sample #	4
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.935	513878	41228	100.000	100.000	N/A	1287	N/A	1.365		N/A

Chromatogram

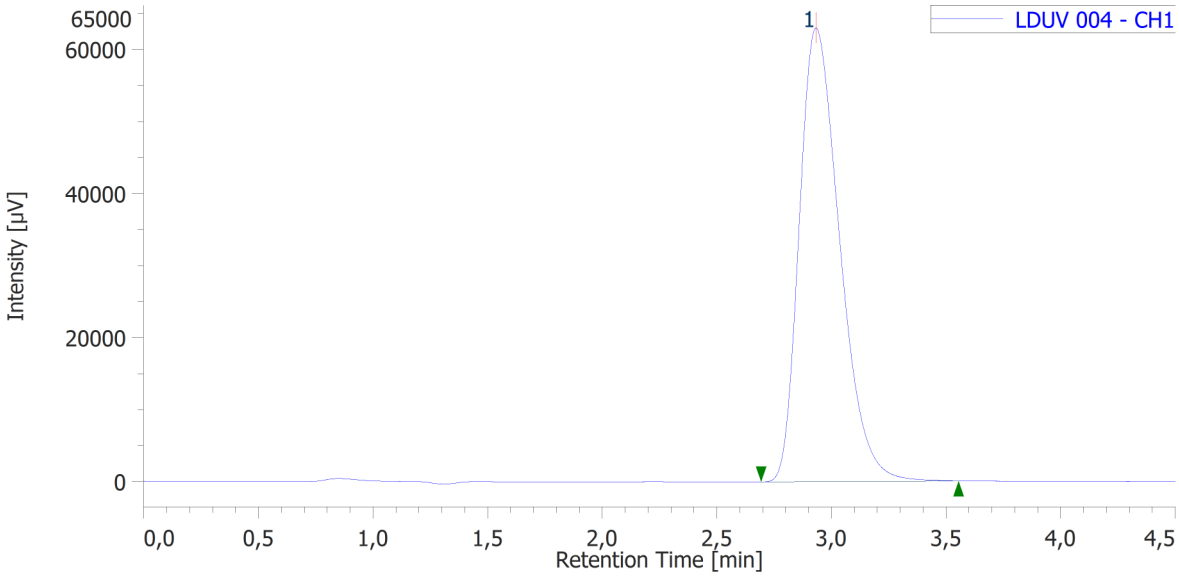


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:55:24
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:44:57
Volume	10.00 [µL]
Sample #	5
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.931	771042	62928	100.000	100.000	N/A	1330	N/A	1.365		N/A

Chromatogram

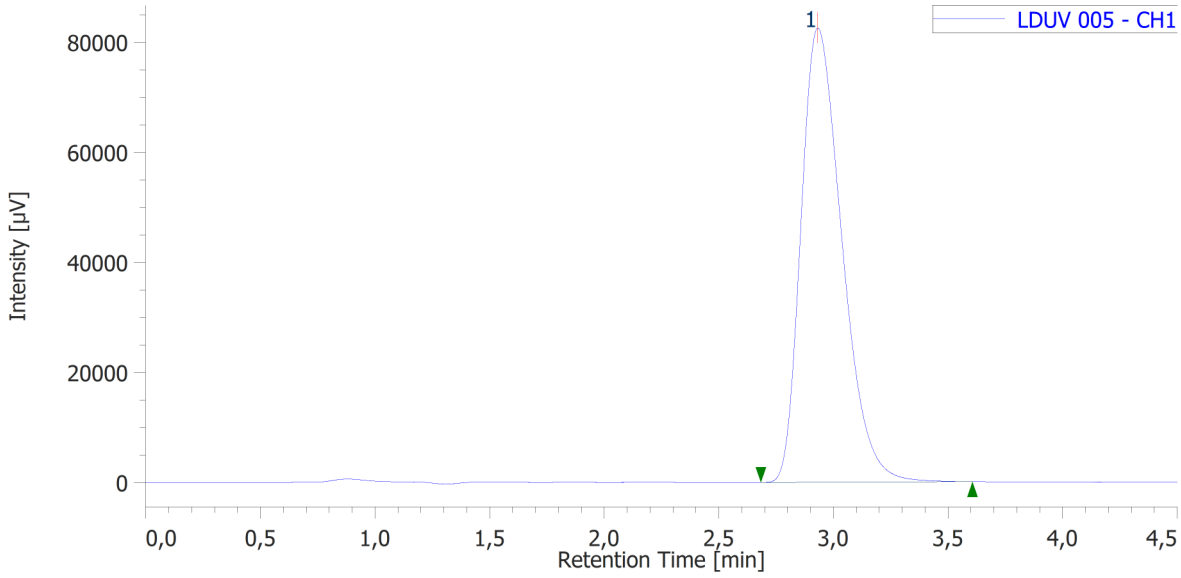


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:55:24
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:49:39
Volume	10,00 [µL]
Sample #	6
Project Name	HPLC 0003
Acquisition Time	4,5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2,931	1024576	82507	100,000	100,000	N/A	1293	N/A	1,373		N/A

Chromatogram

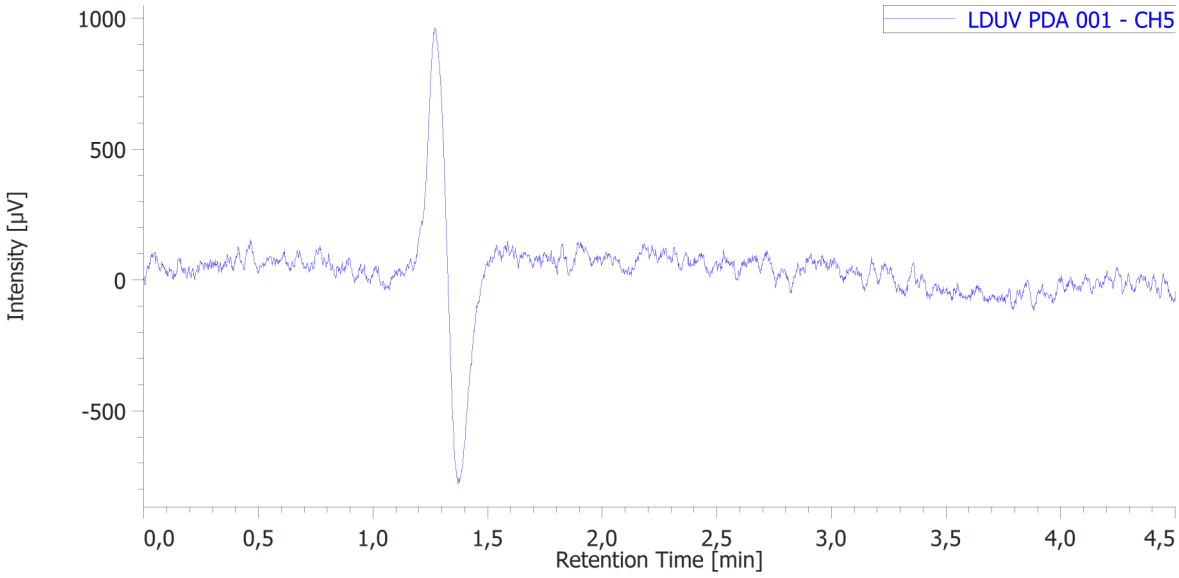


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 17:38:00
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 17:11:56
Volume	10.00 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019A
Control Method	Qualificação PDA 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV PDA 001-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

Chromatogram

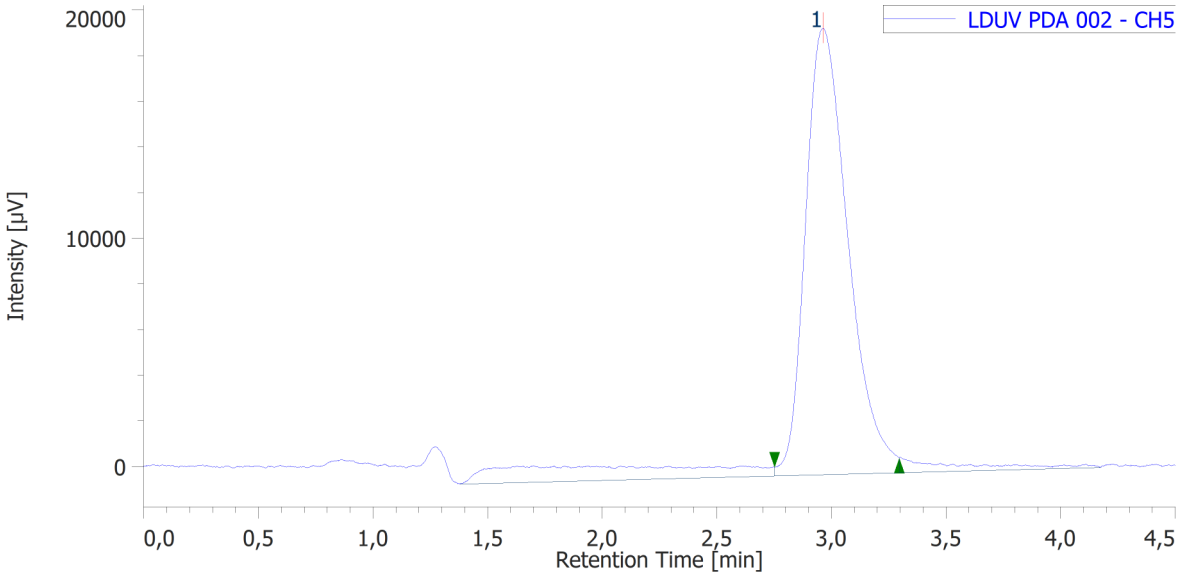


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 17:38:01
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 17:16:39
Volume	10.00 [µL]
Sample #	3
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019A
Control Method	Qualificação PDA 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV PDA 002-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	5	2.963	252393	19562	100.000	100.000	N/A	1250	N/A	1.406		N/A

Chromatogram

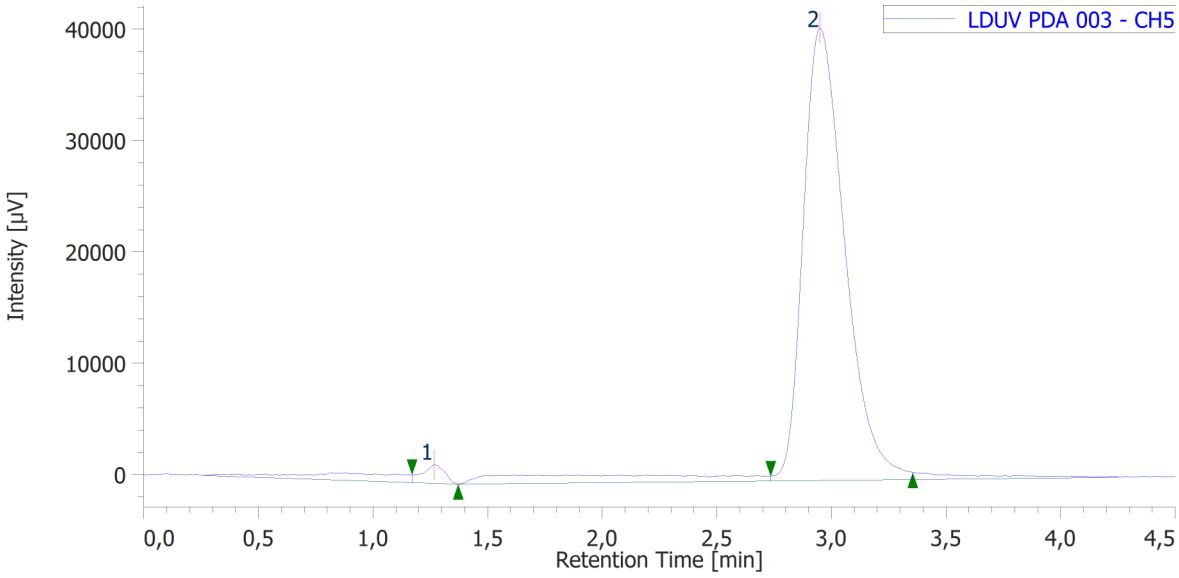


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 17:38:01
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 17:21:21
Volume	10,00 [µL]
Sample #	4
Project Name	HPLC 0003
Acquisition Time	4,5 [min]
Acquisition Sequence	Qualificação 2019A
Control Method	Qualificação PDA 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV PDA 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Unknown	5	1,265	11117	1670	2,131	3,950	N/A	803	6,696	N/A		N/A
2	Cafeína	5	2,950	510631	40600	97,869	96,050	N/A	1309	N/A	1,419		N/A

Chromatogram

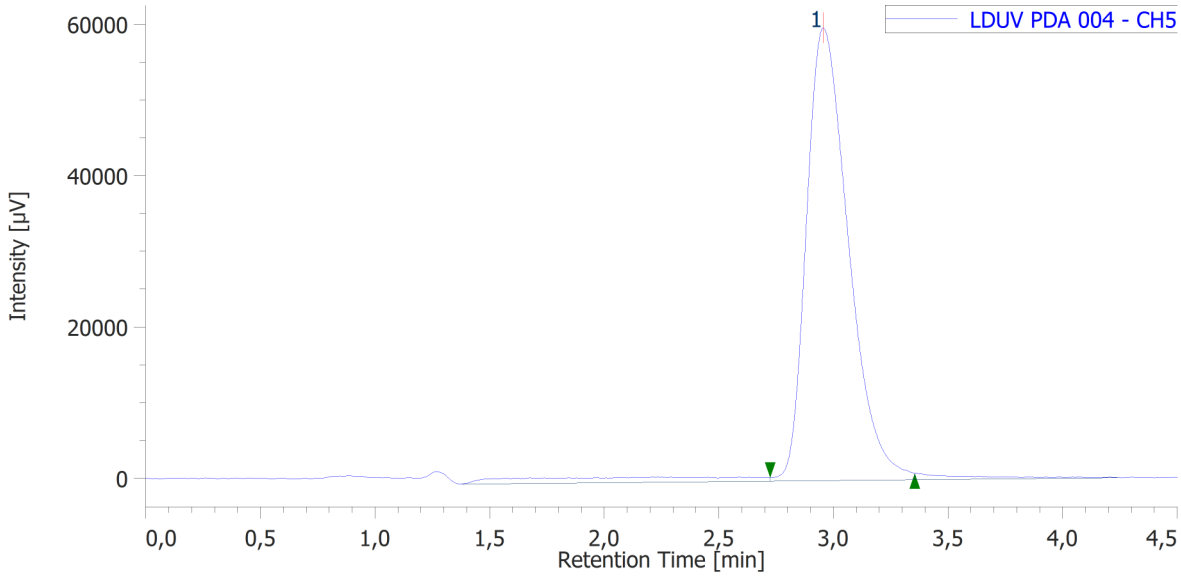

Chromatogram Information


User Name	Giovana
Date Modified	27/08/2019 17:38:01
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 17:26:03
Volume	10.00 [µL]
Sample #	5
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019A
Control Method	Qualificação PDA 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV PDA 004-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	5	2.953	762642	59795	100.000	100.000	N/A	1262	N/A	1.439		N/A

Chromatogram

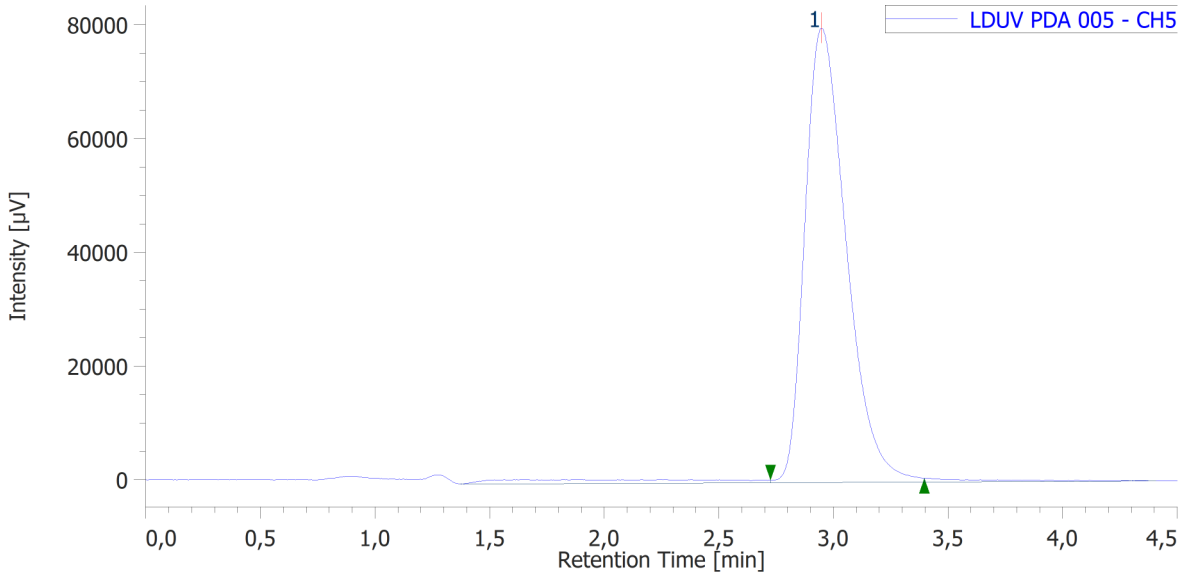


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 17:38:01
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 17:30:45
Volume	10.00 [µL]
Sample #	6
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019A
Control Method	Qualificação PDA 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV PDA 005-CH5
Sample Name	
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	5	2.947	1000953	79866	100.000	100.000	N/A	1302	N/A	1.431		N/A

Chromatogram

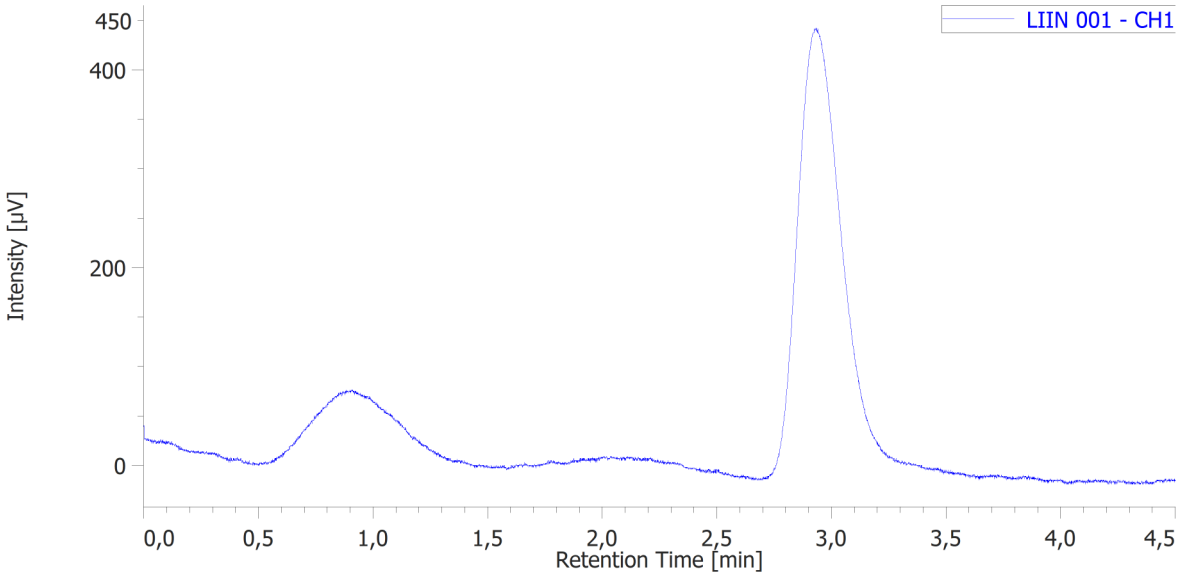


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 15:58:54
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:54:21
Volume	0.10 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 001-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	

Chromatogram

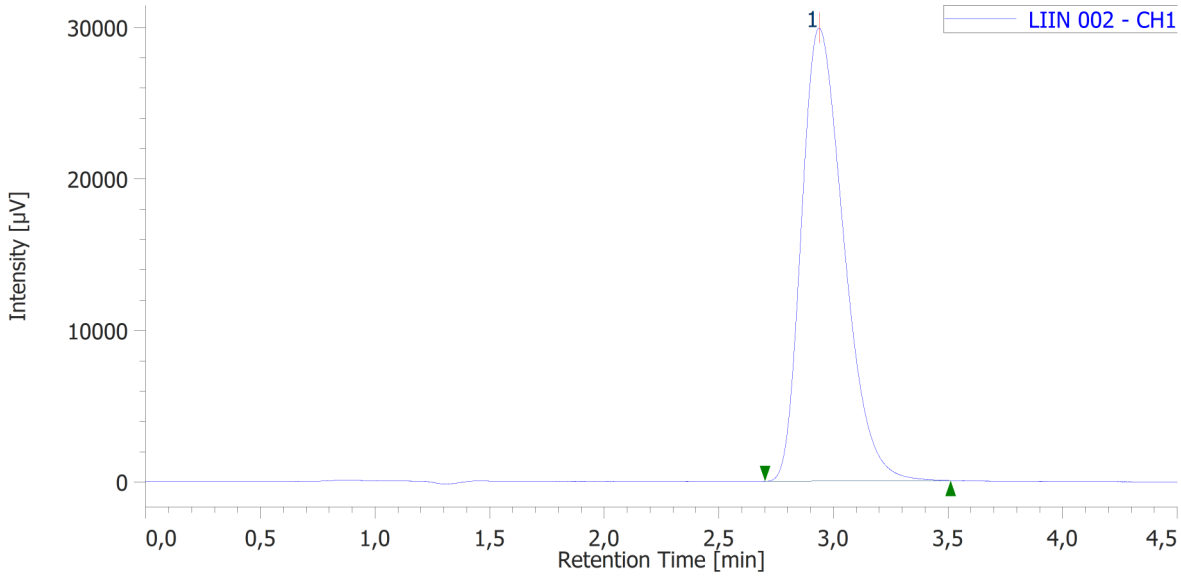


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 16:18:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 15:59:04
Volume	5,00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4,5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2,937	382752	29893	100,000	100,000	N/A	1216	N/A	1,349		N/A

Chromatogram

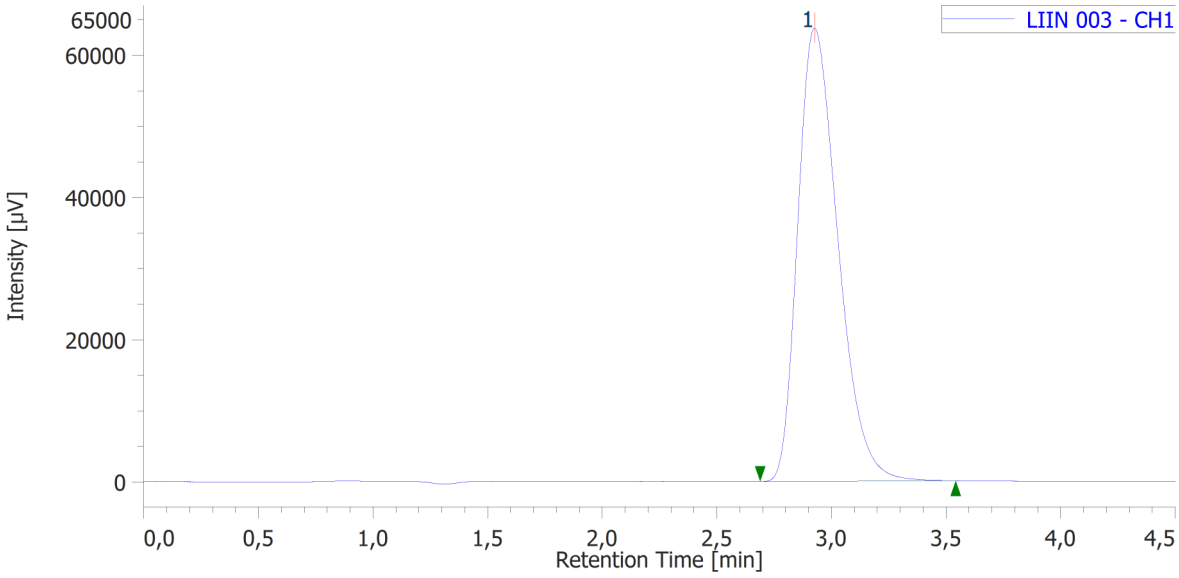


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 16:18:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 16:03:46
Volume	10.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 003-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.925	775734	63713	100.000	100.000	N/A	1343	N/A	1.358		N/A

Chromatogram

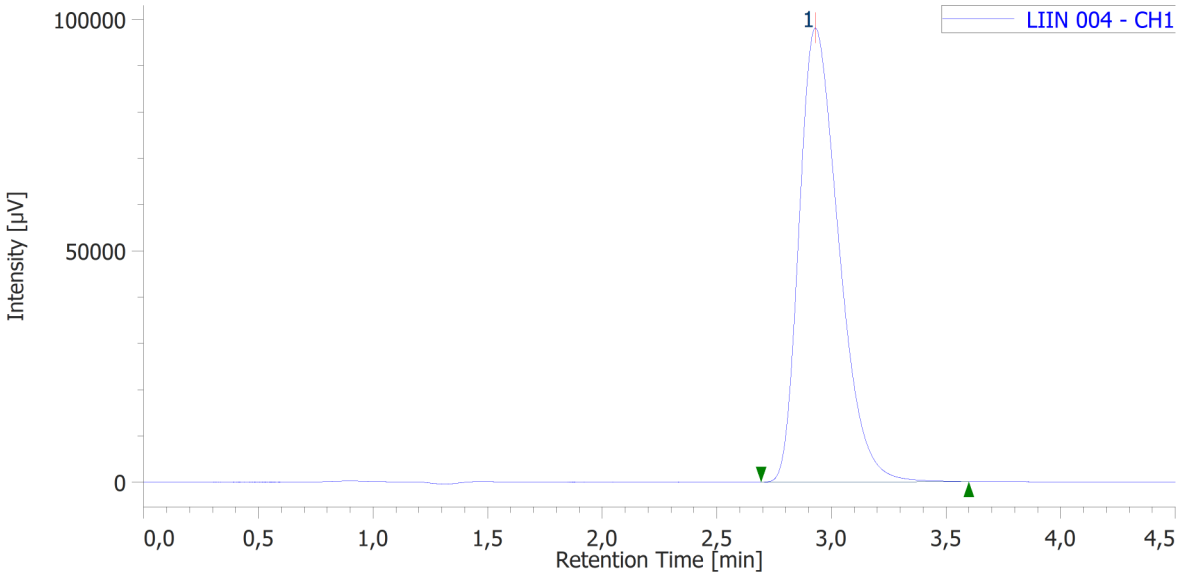


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 16:18:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 16:08:28
Volume	15,00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4,5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 004-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2,929	1175440	98052	100,000	100,000	N/A	1391	N/A	1,374		N/A

Chromatogram

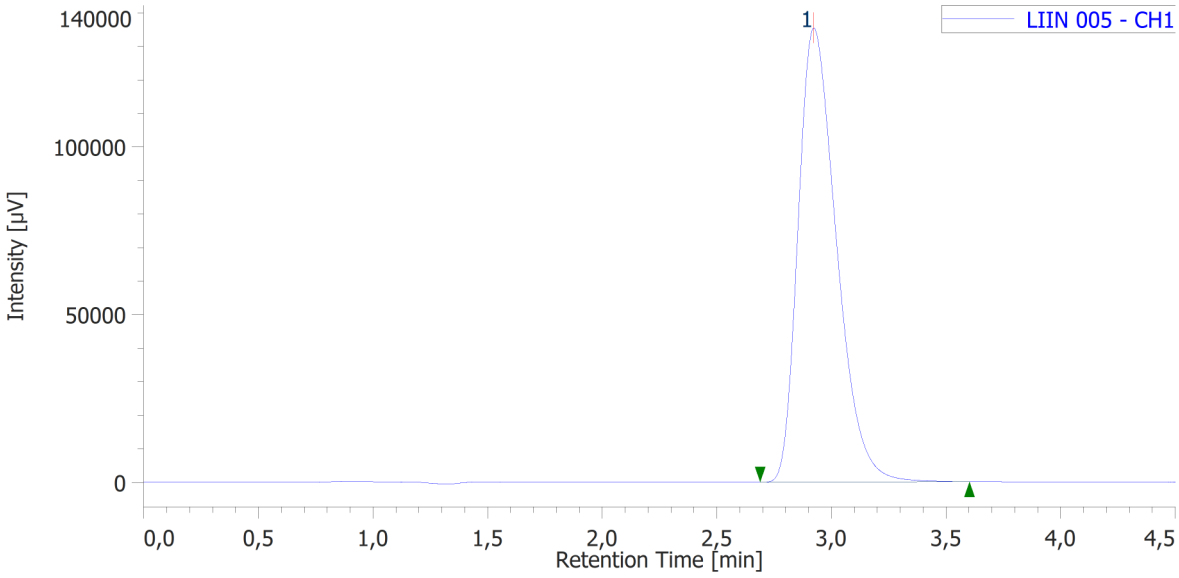


Chromatogram Information	
User Name	Giovana
Date Modified	27/08/2019 16:18:35
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	27/08/2019 16:13:10
Volume	20.00 [µL]
Sample #	2
Project Name	HPLC 0003
Acquisition Time	4.5 [min]
Acquisition Sequence	Qualificação 2019
Control Method	Qualificação UV 2019
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 005-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	1	2.922	1572203	135328	100.000	100.000	N/A	1477	N/A	1.383		N/A

Chromatogram

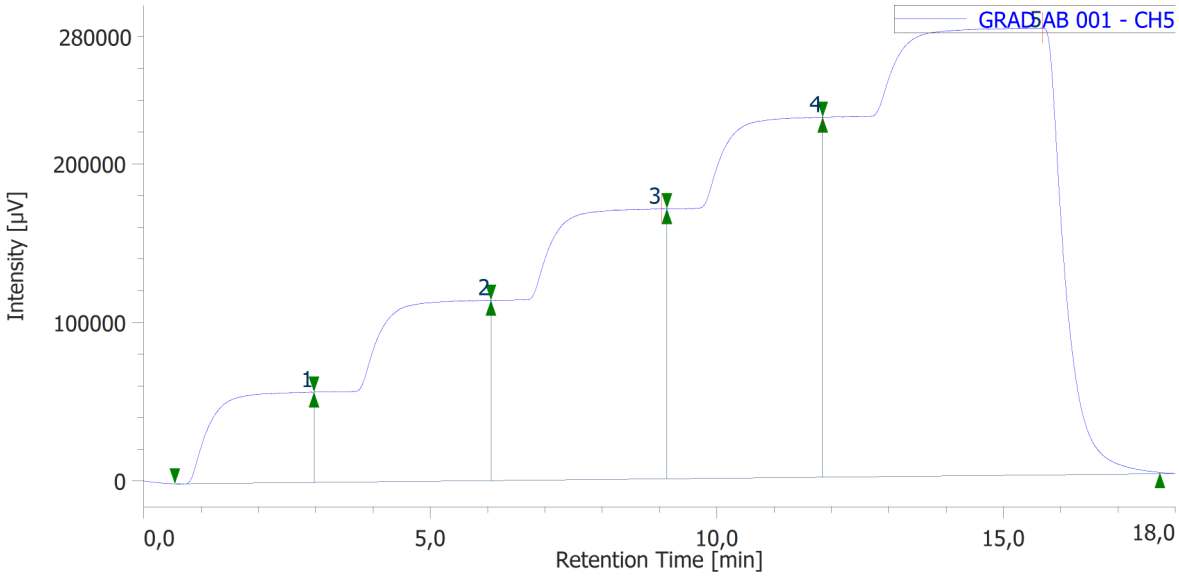


Chromatogram Information	
User Name	Giovana
Date Modified	28/08/2019 08:27:55
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 18:01:54
Volume	0,10 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	18,0 [min]
Acquisition Sequence	GRAD
Control Method	GRAD AB
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD AB 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Cafeína	5	2,967	6311178	56925	4,122	6,699	N/A	N/A	N/A	N/A		N/A
2	Unknown	5	6,055	17231063	113700	11,255	13,381	N/A	N/A	N/A	N/A		N/A
3	Unknown	5	9,037	27826006	170295	18,175	20,042	N/A	N/A	N/A	N/A		N/A
4	Unknown	5	11,838	33695747	227060	22,009	26,722	N/A	N/A	N/A	N/A		N/A
5	Unknown	5	15,678	68032891	281730	44,438	33,156	N/A	N/A	N/A	N/A		N/A

Chromatogram

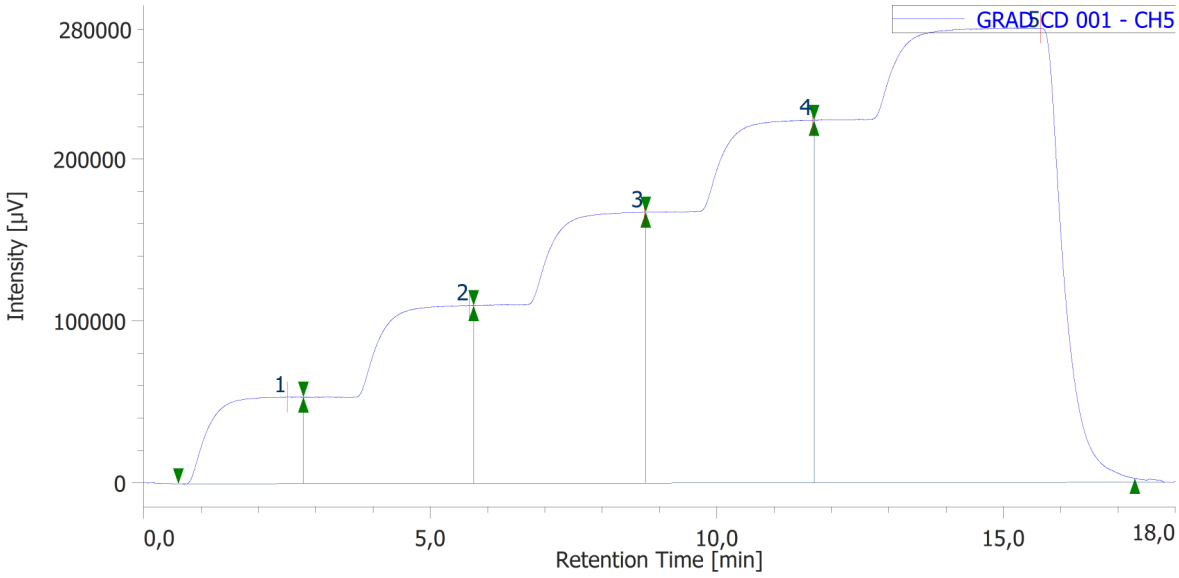

Chromatogram Information	
User Name	Giovana
Date Modified	28/08/2019 08:31:25
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	27/08/2019 18:20:06
Volume	0,10 [µL]
Sample #	1
Project Name	HPLC 0003
Acquisition Time	18,0 [min]
Acquisition Sequence	GRAD
Control Method	GRAD CD
Peak ID Table	Cafeína
Calibration Method	Curva Adenina
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD CD 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Corrected Quantity
1	Unknown	5	2,498	5405984	53431	3,598	6,400	N/A	N/A	N/A	N/A		N/A
2	Unknown	5	5,680	15130793	109902	10,070	13,165	N/A	N/A	N/A	N/A		N/A
3	Unknown	5	8,728	25518237	167237	16,982	20,033	N/A	N/A	N/A	N/A		N/A
4	Unknown	5	11,665	34894846	223884	23,222	26,819	N/A	N/A	N/A	N/A		N/A
5	Unknown	5	15,647	69313446	280355	46,128	33,583	N/A	N/A	N/A	N/A		N/A